



---

ALS Environmental  
ALS Group USA, Corp  
1317 South 13th Avenue  
Kelso, WA 98626  
T : +1 360 577 7222  
F : +1 360 636 1068  
[www.alsglobal.com](http://www.alsglobal.com)

December 04, 2020

**Analytical Report for Service Request No: K2010495**

Delaney Peterson  
Anchor QEA, LLC  
720 Olive Way, Suite 1900  
Seattle, WA 98101

**RE: GascoSiltronic: US Moorings**

Dear Delaney,

Enclosed are the results of the sample(s) submitted to our laboratory November 12, 2020  
For your reference, these analyses have been assigned our service request number **K2010495**.

Analyses were performed according to our laboratory's NELAP-approved quality assurance program. The test results meet requirements of the current NELAP standards, where applicable, and except as noted in the laboratory case narrative provided. For a specific list of NELAP-accredited analytes, refer to the certifications section at [www.alsglobal.com](http://www.alsglobal.com). All results are intended to be considered in their entirety, and ALS Group USA Corp. dba ALS Environmental (ALS) is not responsible for use of less than the complete report. Results apply only to the items submitted to the laboratory for analysis and individual items (samples) analyzed, as listed in the report.

Please contact me if you have any questions. My extension is 3376. You may also contact me via email at [Mark.Harris@alsglobal.com](mailto:Mark.Harris@alsglobal.com).

Respectfully submitted,

**ALS Group USA, Corp. dba ALS Environmental**

Mark Harris  
Project Manager



---

ALS Environmental  
ALS Group USA, Corp  
1317 South 13th Avenue  
Kelso, WA 98626  
T : +1 360 577 7222  
F : +1 360 636 1068  
[www.alsglobal.com](http://www.alsglobal.com)

## Table of Contents

Acronyms

Qualifiers

State Certifications, Accreditations, And Licenses

Case Narrative

Chain of Custody

Total Solids

Chlorinated Herbicides by GC

Raw Data

    Total Solids

    Chlorinated Herbicides by GC

## Acronyms

ASTM	American Society for Testing and Materials
A2LA	American Association for Laboratory Accreditation
CARB	California Air Resources Board
CAS Number	Chemical Abstract Service registry Number
CFC	Chlorofluorocarbon
CFU	Colony-Forming Unit
DEC	Department of Environmental Conservation
DEQ	Department of Environmental Quality
DHS	Department of Health Services
DOE	Department of Ecology
DOH	Department of Health
EPA	U. S. Environmental Protection Agency
ELAP	Environmental Laboratory Accreditation Program
GC	Gas Chromatography
GC/MS	Gas Chromatography/Mass Spectrometry
LOD	Limit of Detection
LOQ	Limit of Quantitation
LUFT	Leaking Underground Fuel Tank
M	Modified
MCL	Maximum Contaminant Level is the highest permissible concentration of a substance allowed in drinking water as established by the USEPA.
MDL	Method Detection Limit
MPN	Most Probable Number
MRL	Method Reporting Limit
NA	Not Applicable
NC	Not Calculated
NCASI	National Council of the Paper Industry for Air and Stream Improvement
ND	Not Detected
NIOSH	National Institute for Occupational Safety and Health
PQL	Practical Quantitation Limit
RCRA	Resource Conservation and Recovery Act
SIM	Selected Ion Monitoring
TPH	Total Petroleum Hydrocarbons
tr	Trace level is the concentration of an analyte that is less than the PQL but greater than or equal to the MDL.

### **Inorganic Data Qualifiers**

- \* The result is an outlier. See case narrative.
- # The control limit criteria is not applicable. See case narrative.
- B The analyte was found in the associated method blank at a level that is significant relative to the sample result as defined by the DOD or NELAC standards.
- E The result is an estimate amount because the value exceeded the instrument calibration range.
- J The result is an estimated value.
- U The analyte was analyzed for, but was not detected ("Non-detect") at or above the MRL/MDL.  
*DOD-QSM 4.2 definition* : Analyte was not detected and is reported as less than the LOD or as defined by the project. The detection limit is adjusted for dilution.
- i The MRL/MDL or LOQ/LOD is elevated due to a matrix interference.
- X See case narrative.
- Q See case narrative. One or more quality control criteria was outside the limits.
- H The holding time for this test is immediately following sample collection. The samples were analyzed as soon as possible after receipt by the laboratory.

### **Metals Data Qualifiers**

- # The control limit criteria is not applicable. See case narrative.
- J The result is an estimated value.
- E The percent difference for the serial dilution was greater than 10%, indicating a possible matrix interference in the sample.
- M The duplicate injection precision was not met.
- N The Matrix Spike sample recovery is not within control limits. See case narrative.
- S The reported value was determined by the Method of Standard Additions (MSA).
- U The analyte was analyzed for, but was not detected ("Non-detect") at or above the MRL/MDL.  
*DOD-QSM 4.2 definition* : Analyte was not detected and is reported as less than the LOD or as defined by the project. The detection limit is adjusted for dilution.
- W The post-digestion spike for furnace AA analysis is out of control limits, while sample absorbance is less than 50% of spike absorbance.  
  - i The MRL/MDL or LOQ/LOD is elevated due to a matrix interference.
- X See case narrative.
- + The correlation coefficient for the MSA is less than 0.995.
- Q See case narrative. One or more quality control criteria was outside the limits.

### **Organic Data Qualifiers**

- \* The result is an outlier. See case narrative.
- # The control limit criteria is not applicable. See case narrative.
- A A tentatively identified compound, a suspected aldol-condensation product.
- B The analyte was found in the associated method blank at a level that is significant relative to the sample result as defined by the DOD or NELAC standards.
- C The analyte was qualitatively confirmed using GC/MS techniques, pattern recognition, or by comparing to historical data.
- D The reported result is from a dilution.
- E The result is an estimated value.
- J The result is an estimated value.
- N The result is presumptive. The analyte was tentatively identified, but a confirmation analysis was not performed.
- P The GC or HPLC confirmation criteria was exceeded. The relative percent difference is greater than 40% between the two analytical results.
- U The analyte was analyzed for, but was not detected ("Non-detect") at or above the MRL/MDL.  
*DOD-QSM 4.2 definition* : Analyte was not detected and is reported as less than the LOD or as defined by the project. The detection limit is adjusted for dilution.  
  - i The MRL/MDL or LOQ/LOD is elevated due to a chromatographic interference.
- X See case narrative.
- Q See case narrative. One or more quality control criteria was outside the limits.

### **Additional Petroleum Hydrocarbon Specific Qualifiers**

- F The chromatographic fingerprint of the sample matches the elution pattern of the calibration standard.
- L The chromatographic fingerprint of the sample resembles a petroleum product, but the elution pattern indicates the presence of a greater amount of lighter molecular weight constituents than the calibration standard.
- H The chromatographic fingerprint of the sample resembles a petroleum product, but the elution pattern indicates the presence of a greater amount of heavier molecular weight constituents than the calibration standard.
- O The chromatographic fingerprint of the sample resembles an oil, but does not match the calibration standard.
- Y The chromatographic fingerprint of the sample resembles a petroleum product eluting in approximately the correct carbon range, but the elution pattern does not match the calibration standard.
- Z The chromatographic fingerprint does not resemble a petroleum product.



**ALS Group USA Corp. dba ALS Environmental (ALS) - Kelso  
State Certifications, Accreditations, and Licenses**

<b>Agency</b>	<b>Web Site</b>	<b>Number</b>
Alaska DEH	<a href="http://dec.alaska.gov/eh/lab/cs/csapproval.htm">http://dec.alaska.gov/eh/lab/cs/csapproval.htm</a>	UST-040
Arizona DHS	<a href="http://www.azdhs.gov/lab/license/env.htm">http://www.azdhs.gov/lab/license/env.htm</a>	AZ0339
Arkansas - DEQ	<a href="http://www.adeq.state.ar.us/techsvs/labcert.htm">http://www.adeq.state.ar.us/techsvs/labcert.htm</a>	88-0637
California DHS (ELAP)	<a href="http://www.cdph.ca.gov/certlic/labs/Pages/ELAP.aspx">http://www.cdph.ca.gov/certlic/labs/Pages/ELAP.aspx</a>	2795
DOD ELAP	<a href="http://www.denix.osd.mil/edqw/Accreditation/AccreditedLabs.cfm">http://www.denix.osd.mil/edqw/Accreditation/AccreditedLabs.cfm</a>	L16-58-R4
Florida DOH	<a href="http://www.doh.state.fl.us/lab/EnvLabCert/WaterCert.htm">http://www.doh.state.fl.us/lab/EnvLabCert/WaterCert.htm</a>	E87412
Hawaii DOH	<a href="http://health.hawaii.gov/">http://health.hawaii.gov/</a>	-
ISO 17025	<a href="http://www.pjllabs.com/">http://www.pjllabs.com/</a>	L16-57
Louisiana DEQ	<a href="http://www.deq.louisiana.gov/page/la-lab-accreditation">http://www.deq.louisiana.gov/page/la-lab-accreditation</a>	03016
Maine DHS	<a href="http://www.maine.gov/dhhs/">http://www.maine.gov/dhhs/</a>	WA01276
Minnesota DOH	<a href="http://www.health.state.mn.us/accreditation">http://www.health.state.mn.us/accreditation</a>	053-999-457
Nevada DEP	<a href="http://ndep.nv.gov/bsdw/labservice.htm">http://ndep.nv.gov/bsdw/labservice.htm</a>	WA01276
New Jersey DEP	<a href="http://www.nj.gov/dep/enforcement/oqa.html">http://www.nj.gov/dep/enforcement/oqa.html</a>	WA005
New York - DOH	<a href="https://www.wadsworth.org/regulatory/elap">https://www.wadsworth.org/regulatory/elap</a>	12060
North Carolina DEQ	<a href="https://deq.nc.gov/about/divisions/water-resources/water-resources-data/water-sciences-home-page/laboratory-certification-branch/non-field-lab-certification">https://deq.nc.gov/about/divisions/water-resources/water-resources-data/water-sciences-home-page/laboratory-certification-branch/non-field-lab-certification</a>	605
Oklahoma DEQ	<a href="http://www.deq.state.ok.us/CSDnew/labcert.htm">http://www.deq.state.ok.us/CSDnew/labcert.htm</a>	9801
Oregon – DEQ (NELAP)	<a href="http://public.health.oregon.gov/LaboratoryServices/EnvironmentalLaboratoryAccreditation/Pages/index.aspx">http://public.health.oregon.gov/LaboratoryServices/EnvironmentalLaboratoryAccreditation/Pages/index.aspx</a>	WA100010
South Carolina DHEC	<a href="http://www.scdhec.gov/environment/EnvironmentalLabCertification/">http://www.scdhec.gov/environment/EnvironmentalLabCertification/</a>	61002
Texas CEQ	<a href="http://www.tceq.texas.gov/field/qa/env_lab_accreditation.html">http://www.tceq.texas.gov/field/qa/env_lab_accreditation.html</a>	T104704427
Washington DOE	<a href="http://www.ecy.wa.gov/programs/eap/labs/lab-accreditation.html">http://www.ecy.wa.gov/programs/eap/labs/lab-accreditation.html</a>	C544
Wyoming (EPA Region 8)	<a href="https://www.epa.gov/region8-waterops/epa-region-8-certified-drinking-water">https://www.epa.gov/region8-waterops/epa-region-8-certified-drinking-water</a>	-
Kelso Laboratory Website	<a href="http://www.alsglobal.com">www.alsglobal.com</a>	NA

Analyses were performed according to our laboratory's NELAP-approved quality assurance program. A complete listing of specific NELAP-certified analytes, can be found in the certification section at [www.ALSGlobal.com](http://www.ALSGlobal.com) or at the accreditation bodies web site.

Please refer to the certification and/or accreditation body's web site if samples are submitted for compliance purposes. The states highlighted above, require the analysis be listed on the state certification if used for compliance purposes and if the method/analyte is offered by that state.



## Case Narrative

**ALS Environmental—Kelso Laboratory**  
1317 South 13th Avenue, Kelso, WA 98626  
Phone (360)577-7222 Fax (360)636-1068  
[www.alsglobal.com](http://www.alsglobal.com)

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Received:** 11/12/2020

### CASE NARRATIVE

All analyses were performed consistent with the quality assurance program of ALS Environmental. This report contains analytical results for samples for the Tier level IV requested by the client.


#### **Sample Receipt:**

Twelve sediment samples were received for analysis at ALS Environmental on 11/12/2020. Any discrepancies upon initial sample inspection are annotated on the sample receipt and preservation form included within this report. The samples were stored at minimum in accordance with the analytical method requirements.

#### **Semivoa GC:**

Method 8151A, 12/02/2020: The upper control criterion was exceeded for 2,4,5-TP in Continuing Calibration Verification (CCV) KQ2019199-05 and KQ2019199-07. The field samples analyzed in this sequence did not contain the analyte(s) in question. Since the apparent problem indicated a potential high bias, the data quality was not affected. No further corrective action was required.

A matrix spike (MS) and a duplicate matrix spike (DMS) were extracted in conjunction with sample USMPDI-006SC-D-12-14-201110. The percent recoveries for 2,4-D were not within project specified control limits following the analysis of the MS/DMS. The percent recovery for 2,4,5-TP was not within project specified control limits following the analysis of the DMS. The percent recoveries for both compounds were not within project specified control limits for the corresponding LCS. Since the percent recoveries for both compounds in all spikes were within in-house established QC limits, no corrective actions were taken.

Approved by 

Date 12/04/2020



# Chain of Custody

**ALS Environmental—Kelso Laboratory**  
1317 South 13th Avenue, Kelso, WA 98626  
Phone (360)577-7222 Fax (360)636-1068  
[www.alsglobal.com](http://www.alsglobal.com)

**ENVIRONMENTAL SAMPLE CHAIN OF CUSTODY**

**KJ010495**

**POC:** # Delaney Peterson (360-715-2707)  
1605 Cornwall Avenue, Bellingham, WA 98225

**Project:** GascoSiltronic: US Moorings  
**Client:** NW Natural

**COC ID:** ALS-20201110-153131  
**Sample Custodian:** CO  
**Lab:** ALS Environmental, Kelso, V

COC Sample Number	Field Sample ID	Sample Type	Matrix	Collected Date	Collected Time	Containers #	Lab QC*	Test Request	Method	TAT**	Preservative
001	USMPDI-003SC-B-00-02-201110	N	SE	11/10/2020	11:55	1	<input type="checkbox"/>	Herbicides Total Solids (ALS)	SW8151A SM2540G	30 30	4°C 4°C
002	USMPDI-003SC-B-02-04-201110	N	SE	11/10/2020	11:55	1	<input type="checkbox"/>	Herbicides Total Solids (ALS)	SW8151A SM2540G	30 30	4°C 4°C
003	USMPDI-003SC-B-04-06-201110	N	SE	11/10/2020	11:55	1	<input type="checkbox"/>	Herbicides Total Solids (ALS)	SW8151A SM2540G	30 30	4°C 4°C
004	USMPDI-003SC-B-06-08-201110	N	SE	11/10/2020	11:55	1	<input type="checkbox"/>	Herbicides Total Solids (ALS)	SW8151A SM2540G	30 30	4°C 4°C
005	USMPDI-006SC-D-00-02-201110	N	SE	11/10/2020	9:05	1	<input type="checkbox"/>	Herbicides Total Solids (ALS)	SW8151A SM2540G	30 30	4°C 4°C
006	USMPDI-006SC-D-02-04-201110	N	SE	11/10/2020	9:05	1	<input type="checkbox"/>	Herbicides Total Solids (ALS)	SW8151A SM2540G	30 30	4°C 4°C
007	USMPDI-006SC-D-04-06-201110	N	SE	11/10/2020	9:05	1	<input type="checkbox"/>	Herbicides	SW8151A	30	4°C

Comment:					
Relinquished By Signature	Received By Signature	Relinquished By Signature	Received By Signature	Relinquished By Signature	Received By Signature
Print Name Hayley Sharkey	Print Name BRIGING K	Print Name	Print Name	Print Name	Print Name
Company AQ	Company AV	Company	Company	Company	Company
Date/Time 11-11-20 07:45	Date/Time 11/12/20 10:15	Date/Time	Date/Time	Date/Time	Date/Time

\* Lab QC Requested for sample when box is checked \*\* TAT = Turn Around Time in DAYS # POC = Project Point of Contact

**ENVIRONMENTAL SAMPLE CHAIN OF CUSTODY**

1620 10495

**POC:** \* Delaney Peterson (360-715-2707)  
 1605 Cornwall Avenue, Bellingham, WA 98225

**Project:** GascoSiltronic: US Moorings  
**Client:** NW Natural

**COC ID:** ALS-20201110-153131  
**Sample Custodian:** CO  
**Lab:** ALS Environmental, Kelso, V

COC Sample Number	Field Sample ID	Sample Type	Matrix	Collected Date	Time	Containers #	Lab QC*	Test Request	Method	TAT**	Preservative
007	USMPDI-006SC-D-04-06-201110	N	SE	11/10/2020	9:05	1	<input type="checkbox"/>	Total Solids (ALS)	SM2540G	30	4°C
008	USMPDI-006SC-D-06-08-201110	N	SE	11/10/2020	9:05	1	<input type="checkbox"/>	Herbicides	SW8151A	30	4°C
								Total Solids (ALS)	SM2540G	30	4°C
009	USMPDI-006SC-D-08-10-201110	N	SE	11/10/2020	9:05	1	<input type="checkbox"/>	Herbicides	SW8151A	30	4°C
								Total Solids (ALS)	SM2540G	30	4°C
010	USMPDI-006SC-D-10-12-201110	N	SE	11/10/2020	9:05	1	<input type="checkbox"/>	Herbicides	SW8151A	30	4°C
								Total Solids (ALS)	SM2540G	30	4°C
011	USMPDI-006SC-D-12-14-201110	N	SE	11/10/2020	9:05	2	<input checked="" type="checkbox"/>	Herbicides	SW8151A	30	4°C
								Total Solids (ALS)	SM2540G	30	4°C
012	USMPDI-1006SC-D-10-12-201110	FD	SE	11/10/2020		1	<input type="checkbox"/>	Herbicides	SW8151A	30	4°C
								Total Solids (ALS)	SM2540G	30	4°C

**Comment:**

Relinquished By	Received By	Relinquished By	Received By	Relinquished By	Received By
Signature	Signature	Signature	Signature	Signature	Signature
Print Name	Print Name	Print Name	Print Name	Print Name	Print Name
Company	Company	Company	Company	Company	Company
Date/Time	Date/Time	Date/Time	Date/Time	Date/Time	Date/Time

\* Lab QC Requested for sample when box is checked \*\* TAT = Turn Around Time in DAYS # POC = Project Point of Contact

PM Mack

### Cooler Receipt and Preservation Form

Client Anchor GEN Service Request K20 10495  
Received: 11/2/20 Opened: 11/2/20 By: BR Unloaded: 11/2/20 By: BR

- 1. Samples were received via?  USPS  Fed Ex  UPS  DHL  PDX  Courier  Hand Delivered
  - 2. Samples were received in: (circle)  Cooler  Box  Envelope  Other  NA
  - 3. Were custody seals on coolers?  NA  Y  N If yes, how many and where? Front
  - If present, were custody seals intact?  NA  Y  N If present, were they signed and dated?  Y  N
  - 4. Was a Temperature Blank present in cooler?  NA  Y  N If yes, notate the temperature in the appropriate column below:  
    If no, take the temperature of a representative sample bottle contained within the cooler; notate in the column "Sample Temp":
  - 5. Were samples received within the method specified temperature ranges?  NA  Y  N  
    If no, were they received on ice and same day as collected? If not, notate the cooler # below and notify the PM.  NA  Y  N
- If applicable, tissue samples were received: Frozen Partially Thawed Thawed

Temp Blank	Sample Temp	IR Gun	Cooler #/COC ID / NA	Out of temp indicate with "X"	PM Notified If out of temp	Tracking Number NA	Filed
<u>4.0</u>		<u>11002</u>				<u>772057944711</u>	

- 6. Packing material:  Inserts  Baggies  Bubble Wrap  Gel Packs  Wet Ice  Dry Ice  Sleeves box
- 7. Were custody papers properly filled-out (ink, signed, etc.)?  NA  Y  N
- 8. Were samples received in good condition (unbroken)  NA  Y  N
- 9. Were all sample labels complete (ie, analysis, preservation, etc.)?  NA  Y  N
- 10. Did all sample labels and tags agree with custody papers?  NA  Y  N
- 11. Were appropriate bottles/containers and volumes received for the tests indicated?  NA  Y  N
- 12. Were the pH-preserved bottles (see SMO GEN SOP) received at the appropriate pH? Indicate in the table below  NA  Y  N
- 13. Were VOA vials received without headspace? Indicate in the table below.  NA  Y  N
- 14. Was C12/Res negative?  NA  Y  N

Sample ID on Bottle	Sample ID on COC	Identified by:

Sample ID	Bottle Count	Bottle Type	Head-space	Broke	pH	Reagent	Volume added	Reagent Lot Number	Initials	Time

Notes, Discrepancies, Resolutions: \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_



# Total Solids

**ALS Environmental—Kelso Laboratory**  
1317 South 13th Avenue, Kelso, WA 98626  
Phone (360)577-7222 Fax (360)636-1068  
[www.alsglobal.com](http://www.alsglobal.com)



**ALS Group USA, Corp.**  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment  
**Analysis Method:** SM 2540 G  
**Prep Method:** None

**Service Request:** K2010495  
**Date Collected:** 11/10/20  
**Date Received:** 11/12/20  
**Units:** Percent  
**Basis:** As Received

**Solids, Total**

Sample Name	Lab Code	Result	MRL	MDL	Dil.	Date Analyzed	Q
USMPDI-003SC-B-00-02-201110	K2010495-001	<b>60.0</b>	-	-	1	12/03/20 16:35	
USMPDI-003SC-B-02-04-201110	K2010495-002	<b>77.7</b>	-	-	1	12/03/20 16:35	
USMPDI-003SC-B-04-06-201110	K2010495-003	<b>77.3</b>	-	-	1	12/03/20 16:35	
USMPDI-003SC-B-06-08-201110	K2010495-004	<b>81.3</b>	-	-	1	12/03/20 16:35	
USMPDI-006SC-D-00-02-201110	K2010495-005	<b>58.8</b>	-	-	1	12/03/20 16:35	
USMPDI-006SC-D-02-04-201110	K2010495-006	<b>75.1</b>	-	-	1	12/03/20 16:35	
USMPDI-006SC-D-04-06-201110	K2010495-007	<b>80.7</b>	-	-	1	12/03/20 16:35	
USMPDI-006SC-D-06-08-201110	K2010495-008	<b>77.6</b>	-	-	1	12/03/20 16:35	
USMPDI-006SC-D-08-10-201110	K2010495-009	<b>76.2</b>	-	-	1	12/03/20 16:35	
USMPDI-006SC-D-10-12-201110	K2010495-010	<b>73.2</b>	-	-	1	12/03/20 16:35	
USMPDI-006SC-D-12-14-201110	K2010495-011	<b>72.3</b>	-	-	1	12/03/20 16:35	
USMPDI-1006SC-D-10-12-201110	K2010495-012	<b>72.9</b>	-	-	1	12/03/20 16:35	
Method Blank	K2010495-MB	ND U	-	-	1	12/03/20 16:35	

ALS Group USA, Corp.

dba ALS Environmental

QA/QC Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment  
**Analysis Method:** SM 2540 G  
**Prep Method:** None

**Service Request:** K2010495  
**Date Collected:** 11/10/20  
**Date Received:** 11/12/20

**Units:** Percent  
**Basis:** As Received

Replicate Sample Summary

Solids, Total

Sample Name:	Lab Code:	MRL	MDL	Sample Result	Duplicate Result	Average	RPD	RPD Limit	Date Analyzed
USMPDI-006SC-D-04-06-201110	K2010495-007DUP	-	-	80.7	80.6	80.7	<1	20	12/03/20
USMPDI-006SC-D-12-14-201110	K2010495-011DUP	-	-	72.3	72.6	72.5	<1	20	12/03/20

Results flagged with an asterisk (\*) indicate values outside control criteria.

Results flagged with a pound (#) indicate the control criteria is not applicable.

Percent recoveries and relative percent differences (RPD) are determined by the software using values in the calculation which have not been rounded.



# Chlorinated Herbicides by GC

**ALS Environmental—Kelso Laboratory**  
1317 South 13th Avenue, Kelso, WA 98626  
Phone (360)577-7222 Fax (360)636-1068  
[www.alsglobal.com](http://www.alsglobal.com)

ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 11:55  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-003SC-B-00-02-201110  
**Lab Code:** K2010495-001

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	83	4.0	1	12/02/20 08:59	11/13/20	
2,4-D	ND U	83	13	1	12/02/20 08:59	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	51	26 - 127	12/02/20 08:59	

ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 11:55  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-003SC-B-02-04-201110  
**Lab Code:** K2010495-002

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	64	3.1	1	12/02/20 18:54	11/13/20	
2,4-D	ND U	64	9.9	1	12/02/20 18:54	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	57	26 - 127	12/02/20 18:54	

**ALS Group USA, Corp.**  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 11:55  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-003SC-B-04-06-201110  
**Lab Code:** K2010495-003

**Units:** ug/Kg  
**Basis:** Dry

**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	64	3.1	1	12/02/20 19:17	11/13/20	
2,4-D	ND U	64	10	1	12/02/20 19:17	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	53	26 - 127	12/02/20 19:17	

**ALS Group USA, Corp.**  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 11:55  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-003SC-B-06-08-201110  
**Lab Code:** K2010495-004

**Units:** ug/Kg  
**Basis:** Dry

**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	61	3.0	1	12/02/20 19:40	11/13/20	
2,4-D	ND U	61	9.5	1	12/02/20 19:40	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	59	26 - 127	12/02/20 19:40	

ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-006SC-D-00-02-201110  
**Lab Code:** K2010495-005

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	84	4.1	1	12/02/20 20:03	11/13/20	
2,4-D	ND U	84	13	1	12/02/20 20:03	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	59	26 - 127	12/02/20 20:03	



ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-006SC-D-02-04-201110  
**Lab Code:** K2010495-006

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	66	3.2	1	12/02/20 20:26	11/13/20	
2,4-D	ND U	66	11	1	12/02/20 20:26	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	66	26 - 127	12/02/20 20:26	

ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-006SC-D-04-06-201110  
**Lab Code:** K2010495-007

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	62	3.0	1	12/02/20 20:49	11/13/20	
2,4-D	ND U	62	9.6	1	12/02/20 20:49	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	51	26 - 127	12/02/20 20:49	

ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-006SC-D-06-08-201110  
**Lab Code:** K2010495-008

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	64	3.1	1	12/02/20 21:12	11/13/20	
2,4-D	ND U	64	9.9	1	12/02/20 21:12	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	55	26 - 127	12/02/20 21:12	

ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-006SC-D-08-10-201110  
**Lab Code:** K2010495-009

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	65	3.2	1	12/02/20 22:20	11/13/20	
2,4-D	ND U	65	11	1	12/02/20 22:20	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	64	26 - 127	12/02/20 22:20	

ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-006SC-D-10-12-201110  
**Lab Code:** K2010495-010

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	68	3.3	1	12/02/20 22:43	11/13/20	
2,4-D	ND U	68	11	1	12/02/20 22:43	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	52	26 - 127	12/02/20 22:43	

ALS Group USA, Corp.  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-006SC-D-12-14-201110  
**Lab Code:** K2010495-011

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	69	3.4	1	12/02/20 23:06	11/13/20	
2,4-D	ND U	69	11	1	12/02/20 23:06	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	55	26 - 127	12/02/20 23:06	

**ALS Group USA, Corp.**  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20  
**Date Received:** 11/12/20 10:15

**Sample Name:** USMPDI-1006SC-D-10-12-201110  
**Lab Code:** K2010495-012

**Units:** ug/Kg  
**Basis:** Dry

**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	68	3.3	1	12/02/20 23:29	11/13/20	
2,4-D	ND U	68	11	1	12/02/20 23:29	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	59	26 - 127	12/02/20 23:29	

**ALS Group USA, Corp.**  
dba ALS Environmental

Analytical Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** NA  
**Date Received:** NA

**Sample Name:** Method Blank  
**Lab Code:** KQ2017965-04

**Units:** ug/Kg  
**Basis:** Dry

**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**Prep Method:** Method

Analyte Name	Result	MRL	MDL	Dil.	Date Analyzed	Date Extracted	Q
2,4,5-TP	ND U	50	2.4	1	12/02/20 05:33	11/13/20	
2,4-D	ND U	50	7.7	1	12/02/20 05:33	11/13/20	

Surrogate Name	% Rec	Control Limits	Date Analyzed	Q
DCAA	52	26 - 127	12/02/20 05:33	



ALS Group USA, Corp.  
dba ALS Environmental

Confirmation Results

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**SRM Matrix:** Sediment  
**Sample Name:** USMPDI-006SC-D-12-14-201110  
**Lab Code:** KQ2017965-01

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20

**Units:** ug/Kg  
**Basis:** Dry  
**Percent Solids:** 72.3

Chlorinated Herbicides by GC

**Analytical Method:** 8151A  
**Prep Method:** Method

	MDL	Primary Result	Confirmation Result	RPD	Q	Dilution Factor	Date Analyzed
2,4,5-TP	3.4	120	172	36		1	12/02/20 23:52
2,4-D	11	111	158	35		1	12/02/20 23:52

ALS Group USA, Corp.  
dba ALS Environmental

Confirmation Results

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**SRM Matrix:** Sediment  
**Sample Name:** USMPDI-006SC-D-12-14-201110  
**Lab Code:** KQ2017965-02

**Service Request:** K2010495  
**Date Collected:** 11/10/20 09:05  
**Date Received:** 11/12/20

**Units:** ug/Kg  
**Basis:** Dry  
**Percent Solids:** 72.3

Chlorinated Herbicides by GC

**Analytical Method:** 8151A  
**Prep Method:** Method

	MDL	Primary Result	Confirmation Result	RPD	Q	Dilution Factor	Date Analyzed
2,4,5-TP	3.4	113	160	34		1	12/03/20 00:15
2,4-D	11	106	145	31		1	12/03/20 00:15

ALS Group USA, Corp.  
dba ALS Environmental

Confirmation Results

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**SRM Matrix:** Sediment  
**Sample Name:** Lab Control Sample  
**Lab Code:** KQ2017965-03

**Service Request:** K2010495  
**Date Collected:** NA  
**Date Received:**

**Units:** ug/Kg  
**Basis:** Dry

Chlorinated Herbicides by GC

**Analytical Method:** 8151A  
**Prep Method:** Method

	<b>MDL</b>	<b>Primary Result</b>	<b>Confirmation Result</b>	<b>RPD</b>	<b>Q</b>	<b>Dilution Factor</b>	<b>Date Analyzed</b>
2,4,5-TP	2.4	81.5	114	33		1	12/02/20 05:56
2,4-D	7.7	76.6	106	32		1	12/02/20 05:56

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495

**SURROGATE RECOVERY SUMMARY**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**Extraction Method:** Method

<b>Sample Name</b>	<b>Lab Code</b>	<b>DCAA 26-127</b>
USMPDI-003SC-B-00-02-201110	K2010495-001	51
USMPDI-003SC-B-02-04-201110	K2010495-002	57
USMPDI-003SC-B-04-06-201110	K2010495-003	53
USMPDI-003SC-B-06-08-201110	K2010495-004	59
USMPDI-006SC-D-00-02-201110	K2010495-005	59
USMPDI-006SC-D-02-04-201110	K2010495-006	66
USMPDI-006SC-D-04-06-201110	K2010495-007	51
USMPDI-006SC-D-06-08-201110	K2010495-008	55
USMPDI-006SC-D-08-10-201110	K2010495-009	64
USMPDI-006SC-D-10-12-201110	K2010495-010	52
USMPDI-006SC-D-12-14-201110	K2010495-011	55
USMPDI-1006SC-D-10-12-201110	K2010495-012	59
Method Blank	KQ2017965-04	52
Lab Control Sample	KQ2017965-03	58
USMPDI-006SC-D-12-14-201110	KQ2017965-01	63
USMPDI-006SC-D-12-14-201110	KQ2017965-02	60

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Collected:** 11/10/20  
**Date Received:** 11/12/20  
**Date Analyzed:** 12/2/20  
**Date Extracted:** 11/13/20

**Duplicate Matrix Spike Summary  
Chlorinated Herbicides by GC**

**Sample Name:** USMPDI-006SC-D-12-14-201110  
**Lab Code:** K2010495-011  
**Analysis Method:** 8151A  
**Prep Method:** Method

**Units:** ug/Kg  
**Basis:** Dry

Analyte Name	Sample Result	Result	Matrix Spike KQ2017965-01		Result	Duplicate Matrix Spike KQ2017965-02		% Rec Limits	RPD	RPD Limit
			Spike Amount	% Rec		Spike Amount	% Rec			
2,4,5-TP	ND U	120	230	52	113	230	49	34-129	6	40
2,4-D	ND U	111	230	48	106	230	46	35-129	5	40

Results flagged with an asterisk (\*) indicate values outside control criteria.

Results flagged with a pound (#) indicate the control criteria is not applicable.

Percent recoveries and relative percent differences (RPD) are determined by the software using values in the calculation which have not been rounded.

Matrix Spike and Matrix Spike Duplicate Data is presented for information purposes only. The matrix may or may not be relevant to samples reported in this report. The laboratory evaluates system performance based on the LCS and LCSD control limits.

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20  
**Date Extracted:** 11/13/20

**Lab Control Sample Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**Prep Method:** Method

**Units:** ug/Kg  
**Basis:** Dry  
**Analysis Lot:** 705487

**Lab Control Sample**  
**KQ2017965-03**

<b>Analyte Name</b>	<b>Result</b>	<b>Spike Amount</b>	<b>% Rec</b>	<b>% Rec Limits</b>
2,4,5-TP	81.5	167	49	46-125
2,4-D	76.6	167	46	46-120

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 05:33  
**Date Extracted:** 11/13/20

**Method Blank Summary**  
**Chlorinated Herbicides by GC**

**Sample Name:** Method Blank  
**Lab Code:** KQ2017965-04

**Instrument ID:** K-GC-24  
**File ID:** J:\gc24\data\120120\12010033.D\

**Analysis Method:** 8151A  
**Prep Method:** Method

**Analysis Lot:** 705487,705654  
**Extraction Lot:** 369767

This Method Blank applies to the following analyses.

Sample Name	Lab Code	File ID	Date Analyzed
Lab Control Sample	KQ2017965-03	J:\gc24\data\120120\12010034.D\	12/02/20 05:56
USMPDI-003SC-B-00-02-201110	K2010495-001	J:\gc24\data\120120\12010042.D\	12/02/20 08:59
USMPDI-003SC-B-02-04-201110	K2010495-002	J:\gc24\data\120120\12010068.D\	12/02/20 18:54
USMPDI-003SC-B-04-06-201110	K2010495-003	J:\gc24\data\120120\12010069.D\	12/02/20 19:17
USMPDI-003SC-B-06-08-201110	K2010495-004	J:\gc24\data\120120\12010070.D\	12/02/20 19:40
USMPDI-006SC-D-00-02-201110	K2010495-005	J:\gc24\data\120120\12010071.D\	12/02/20 20:03
USMPDI-006SC-D-02-04-201110	K2010495-006	J:\gc24\data\120120\12010072.D\	12/02/20 20:26
USMPDI-006SC-D-04-06-201110	K2010495-007	J:\gc24\data\120120\12010073.D\	12/02/20 20:49
USMPDI-006SC-D-06-08-201110	K2010495-008	J:\gc24\data\120120\12010074.D\	12/02/20 21:12
USMPDI-006SC-D-08-10-201110	K2010495-009	J:\gc24\data\120120\12010077.D\	12/02/20 22:20
USMPDI-006SC-D-10-12-201110	K2010495-010	J:\gc24\data\120120\12010078.D\	12/02/20 22:43
USMPDI-006SC-D-12-14-201110	K2010495-011	J:\gc24\data\120120\12010079.D\	12/02/20 23:06
USMPDI-1006SC-D-10-12-201110	K2010495-012	J:\gc24\data\120120\12010080.D\	12/02/20 23:29
USMPDI-006SC-D-12-14-201110MS	KQ2017965-01	J:\gc24\data\120120\12010081.D\	12/02/20 23:52
USMPDI-006SC-D-12-14-201110DMS	KQ2017965-02	J:\gc24\data\120120\12010082.D\	12/03/20 00:15

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 05:56  
**Date Extracted:** 11/13/20

**Lab Control Sample Summary**  
**Chlorinated Herbicides by GC**

**Sample Name:** Lab Control Sample      **Instrument ID:** K-GC-24  
**Lab Code:** KQ2017965-03      **File ID:** J:\gc24\data\120120\12010034.D\  
**Analysis Method:** 8151A      **Analysis Lot:** 705487,705654  
**Prep Method:** Method      **Extraction Lot:** 369767

This Lab Control Sample applies to the following analyses.

Sample Name	Lab Code	File ID	Date Analyzed
Method Blank	KQ2017965-04	J:\gc24\data\120120\12010033.D\	12/02/20 05:33
USMPDI-003SC-B-00-02-201110	K2010495-001	J:\gc24\data\120120\12010042.D\	12/02/20 08:59
USMPDI-003SC-B-02-04-201110	K2010495-002	J:\gc24\data\120120\12010068.D\	12/02/20 18:54
USMPDI-003SC-B-04-06-201110	K2010495-003	J:\gc24\data\120120\12010069.D\	12/02/20 19:17
USMPDI-003SC-B-06-08-201110	K2010495-004	J:\gc24\data\120120\12010070.D\	12/02/20 19:40
USMPDI-006SC-D-00-02-201110	K2010495-005	J:\gc24\data\120120\12010071.D\	12/02/20 20:03
USMPDI-006SC-D-02-04-201110	K2010495-006	J:\gc24\data\120120\12010072.D\	12/02/20 20:26
USMPDI-006SC-D-04-06-201110	K2010495-007	J:\gc24\data\120120\12010073.D\	12/02/20 20:49
USMPDI-006SC-D-06-08-201110	K2010495-008	J:\gc24\data\120120\12010074.D\	12/02/20 21:12
USMPDI-006SC-D-08-10-201110	K2010495-009	J:\gc24\data\120120\12010077.D\	12/02/20 22:20
USMPDI-006SC-D-10-12-201110	K2010495-010	J:\gc24\data\120120\12010078.D\	12/02/20 22:43
USMPDI-006SC-D-12-14-201110	K2010495-011	J:\gc24\data\120120\12010079.D\	12/02/20 23:06
USMPDI-1006SC-D-10-12-201110	K2010495-012	J:\gc24\data\120120\12010080.D\	12/02/20 23:29
USMPDI-006SC-D-12-14-201110MS	KQ2017965-01	J:\gc24\data\120120\12010081.D\	12/02/20 23:52
USMPDI-006SC-D-12-14-201110DMS	KQ2017965-02	J:\gc24\data\120120\12010082.D\	12/03/20 00:15



ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

Client: Anchor QEA, LLC  
Project: GascoSiltronic: US Moorings

Service Request: K2010495  
Calibration Date: 10/21/2020

Initial Calibration Summary  
Chlorinated Herbicides by GC

Calibration ID: KC2000566  
Instrument ID: K-GC-24

Signal ID: RTX-CLP2

#	Lab Code	Sample Name	File Location	Acquisition Date
01	KC2000566-01	PENTA2-14K 10PPB	J:\gc24\data\102120\10210004.D	10/21/2020 13:46
02	KC2000566-02	PENTA2-14L 25PPB	J:\gc24\data\102120\10210005.D	10/21/2020 14:09
03	KC2000566-03	PENTA2-14M 75PPB	J:\gc24\data\102120\10210006.D	10/21/2020 14:33
04	KC2000566-04	PENTA2-14N 100PB	J:\gc24\data\102120\10210007.D	10/21/2020 14:57
05	KC2000566-05	PENTA2-15A 125PB	J:\gc24\data\102120\10210008.D	10/21/2020 15:21
06	KC2000566-06	PENTA2-15B 150PB	J:\gc24\data\102120\10210009.D	10/21/2020 15:44
07	KC2000566-07	PENTA2-15C 175PB	J:\gc24\data\102120\10210010.D	10/21/2020 16:08
08	KC2000566-08	PENTA2-15D 200PB	J:\gc24\data\102120\10210011.D	10/21/2020 16:32

Analyte

2,4,5-TP

#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.510	9.752E4	02	23.760	9.79E4	03	71.300	9.082E4	04	95.100	9.31E4
05	118.820	9.221E4	06	142.580	9.36E4	07	166.340	9.245E4	08	190.100	9.185E4

2,4-D

#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.400	2.488E4	02	23.510	2.377E4	03	70.500	2.075E4	04	94.000	2.056E4
05	117.540	2.029E4	06	141.050	2.025E4	07	164.560	1.991E4	08	188.060	1.951E4

DCAA

#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.020	2.115E4	02	22.550	2.015E4	03	67.600	1.798E4	04	90.200	1.794E4
05	112.730	1.738E4	06	135.280	1.732E4	07	157.830	1.694E4	08	180.370	1.67E4

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Calibration Date:** 10/21/2020

**Initial Calibration Summary  
Chlorinated Herbicides by GC**

**Calibration ID:** KC2000566  
**Instrument ID:** K-GC-24

**Signal ID:** RTX-CLP2

Analyte Name	Compound Type	Calibration Evaluation				Calibration Evaluation	
		Fit Type	Eval	Eval Result	Control Criteria	Average RRF	Minimum RRF
2,4,5-TP	TRG	Average RF	% RSD	2.8	20	9.368E4	
2,4-D	TRG	Average RF	% RSD	9.3	20	2.124E4	
DCAA	SURR	Average RF	% RSD	8.8	20	1.82E4	

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

Client: Anchor QEA, LLC  
Project: GascoSiltronic: US Moorings

Service Request: K2010495  
Calibration Date: 10/21/2020

Initial Calibration Summary  
Chlorinated Herbicides by GC

Calibration ID: KC2000566  
Instrument ID: K-GC-24

Signal ID: ZB-XLB-HT

#	Lab Code	Sample Name	File Location	Acquisition Date
01	KC2000566-01	PENTA2-14K 10PPB	J:\gc24\data\102120\10210004.D	10/21/2020 13:46
02	KC2000566-02	PENTA2-14L 25PPB	J:\gc24\data\102120\10210005.D	10/21/2020 14:09
03	KC2000566-03	PENTA2-14M 75PPB	J:\gc24\data\102120\10210006.D	10/21/2020 14:33
04	KC2000566-04	PENTA2-14N 100PB	J:\gc24\data\102120\10210007.D	10/21/2020 14:57
05	KC2000566-05	PENTA2-15A 125PB	J:\gc24\data\102120\10210008.D	10/21/2020 15:21
06	KC2000566-06	PENTA2-15B 150PB	J:\gc24\data\102120\10210009.D	10/21/2020 15:44
07	KC2000566-07	PENTA2-15C 175PB	J:\gc24\data\102120\10210010.D	10/21/2020 16:08
08	KC2000566-08	PENTA2-15D 200PB	J:\gc24\data\102120\10210011.D	10/21/2020 16:32

Analyte

2,4,5-TP

#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.510	2.358E5	02	23.760	2.178E5	03	71.300	1.953E5	04	95.100	1.956E5
05	118.820	1.949E5	06	142.580	1.947E5	07	166.340	1.946E5	08	190.100	1.952E5

2,4-D

#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.400	6.995E4	02	23.510	5.929E4	03	70.500	4.845E4	04	94.000	4.767E4
05	117.540	4.681E4	06	141.050	4.616E4	07	164.560	4.575E4	08	188.060	4.551E4

DCAA

#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.020	5.587E4	02	22.550	4.943E4	03	67.600	4.041E4	04	90.200	3.953E4
05	112.730	3.892E4	06	135.280	3.822E4	07	157.830	3.814E4	08	180.370	3.787E4

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Calibration Date:** 10/21/2020

**Initial Calibration Summary**  
**Chlorinated Herbicides by GC**

**Calibration ID:** KC2000566  
**Instrument ID:** K-GC-24

**Signal ID:** ZB-XLB-HT

Analyte Name	Compound Type	Calibration Evaluation				Calibration Evaluation	
		Fit Type	Eval	Eval Result	Control Criteria	Average RRF	Minimum RRF
2,4,5-TP	TRG	Average RF	% RSD	7.6	20	2.03E5	
2,4-D	TRG	Average RF	% RSD	17.2	20	5.12E4	
DCAA	SURR	Average RF	% RSD	15.8	20	4.23E4	

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Calibration Date:** 10/21/2020

**Initial Calibration Verification Summary**  
**Chlorinated Herbicides by GC**

**Calibration ID:** KC2000566  
**Instrument ID:** K-GC-24

**Signal ID:** RTX-CLP2

#	Lab Code	Sample Name	File Location	Acquisition Date
09	KC2000566-09	PENTA2-15E ICV 100 PPB	J:\gc24\data\102120\10210012.D	10/21/2020 16:56

Analyte Name	Expected	Result	Average RF	SSV RF	% D	Criteria	Curve Fit
2,4,5-TP	95.1	93.4	9.368E4	9.198E4	-1.819	±20	Average RF
2,4-D	94.0	90.4	2.124E4	2.043E4	-3.805	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Calibration Date:** 10/21/2020

**Initial Calibration Verification Summary**  
**Chlorinated Herbicides by GC**

**Calibration ID:** KC2000566  
**Instrument ID:** K-GC-24

**Signal ID:** ZB-XLB-HT

#	Lab Code	Sample Name	File Location	Acquisition Date
09	KC2000566-09	PENTA2-15E ICV 100 PPB	J:\gc24\data\102120\10210012.D	10/21/2020 16:56

Analyte Name	Expected	Result	Average RF	SSV RF	% D	Criteria	Curve Fit
2,4,5-TP	95.1	92.5	2.03E5	1.974E5	-2.734	±20	Average RF
2,4-D	94.0	83.6	5.12E4	4.556E4	-11.018	±20	Average RF

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 03:38

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010028.D\  
**Signal ID:** RTX-CLP2

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705487  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	81.3	9.368E4	8.013E4	-14.5	NA	±20	Average RF
2,4-D	94.0	75.3	2.124E4	1.702E4	-19.9	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	85.7	1.82E4	1.56E4	-14.3	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 03:38

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010028.D\  
**Signal ID:** ZB-XLB-HT

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705487  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	111	2.03E5	2.361E5	16.3	NA	±20	Average RF
2,4-D	94.0	99.1	5.12E4	5.4E4	5.5	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	111	4.23E4	4.715E4	11.5	NA	±20	Average RF



**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 08:13

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010040.D\  
**Signal ID:** RTX-CLP2

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705487  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	81.5	9.368E4	8.031E4	-14.3	NA	±20	Average RF
2,4-D	94.0	75.8	2.124E4	1.714E4	-19.3	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	85.3	1.82E4	1.553E4	-14.7	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 08:13

**Continuing Calibration Verification (CCV) Summary  
Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010040.D\  
**Signal ID:** ZB-XLB-HT

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705487  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	114	2.03E5	2.423E5	19.3	NA	±20	Average RF
2,4-D	94.0	101	5.12E4	5.514E4	7.7	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	114	4.23E4	4.829E4	14.2	NA	±20	Average RF

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 08:13

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010040.D\  
**Signal ID:** ZB-XLB-HT

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	114	2.03E5	2.423E5	19.3	NA	±20	Average RF
2,4-D	94.0	101	5.12E4	5.514E4	7.7	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	114	4.23E4	4.829E4	14.2	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 08:13

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010040.D\  
**Signal ID:** RTX-CLP2

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	81.5	9.368E4	8.031E4	-14.3	NA	±20	Average RF
2,4-D	94.0	75.8	2.124E4	1.714E4	-19.3	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	85.3	1.82E4	1.553E4	-14.7	NA	±20	Average RF

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 12:25

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010051.D\  
**Signal ID:** RTX-CLP2

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	81.6	9.368E4	8.04E4	-14.2	NA	±20	Average RF
2,4-D	94.0	75.4	2.124E4	1.703E4	-19.8	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	85.6	1.82E4	1.558E4	-14.4	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 12:25

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010051.D\  
**Signal ID:** ZB-XLB-HT

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	113	2.03E5	2.403E5	18.4	NA	±20	Average RF
2,4-D	94.0	100	5.12E4	5.465E4	6.7	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	113	4.23E4	4.762E4	12.6	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 17:00

**Continuing Calibration Verification (CCV) Summary  
Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010063.D\  
**Signal ID:** RTX-CLP2

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	81.3	9.368E4	8.011E4	-14.5	NA	±20	Average RF
2,4-D	94.0	75.1	2.124E4	1.697E4	-20.1	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	85.0	1.82E4	1.547E4	-15.0	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 17:00

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010063.D\  
**Signal ID:** ZB-XLB-HT

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	115	2.03E5	2.456E5	21.0*	NA	±20	Average RF
2,4-D	94.0	102	5.12E4	5.572E4	8.8	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	116	4.23E4	4.914E4	16.2	NA	±20	Average RF



**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 21:34

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010075.D\  
**Signal ID:** RTX-CLP2

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	82.2	9.368E4	8.101E4	-13.5	NA	±20	Average RF
2,4-D	94.0	75.7	2.124E4	1.71E4	-19.5	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	88.1	1.82E4	1.602E4	-11.9	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/02/20 21:34

**Continuing Calibration Verification (CCV) Summary  
Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010075.D\  
**Signal ID:** ZB-XLB-HT

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	116	2.03E5	2.467E5	21.5*	NA	±20	Average RF
2,4-D	94.0	103	5.12E4	5.634E4	10.0	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	116	4.23E4	4.917E4	16.3	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/03/20 00:38

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010083.D\  
**Signal ID:** RTX-CLP2

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	81.8	9.368E4	8.062E4	-13.9	NA	±20	Average RF
2,4-D	94.0	75.5	2.124E4	1.706E4	-19.7	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	87.8	1.82E4	1.598E4	-12.2	NA	±20	Average RF

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings

**Service Request:** K2010495  
**Date Analyzed:** 12/03/20 00:38

**Continuing Calibration Verification (CCV) Summary**  
**Chlorinated Herbicides by GC**

**Analysis Method:** 8151A  
**File ID:** J:\gc24\data\120120\12010083.D\  
**Signal ID:** ZB-XLB-HT

**Calibration Date:** 10/21/2020  
**Calibration ID:** KC2000566  
**Analysis Lot:** 705654  
**Units:** ppb

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
2,4,5-TP	95.1	114	2.03E5	2.431E5	19.7	NA	±20	Average RF
2,4-D	94.0	103	5.12E4	5.592E4	9.2	NA	±20	Average RF

Analyte Name	Expected	Result	Average RF	CCV RF	% D	% Drift	Criteria	Curve Fit
DCAA	100	115	4.23E4	4.869E4	15.1	NA	±20	Average RF

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

Client: Anchor QEA, LLC  
Project: GascoSiltronic: US Moorings

Service Request:K2010495

Analysis Run Log  
Chlorinated Herbicides by GC

Analysis Method: 8151A

Analysis Lot:705487  
Instrument ID:K-GC-24

Raw Data File	Sample Name	Lab Code	Date Analyzed	Time Analyzed	Q
J:\gc24\data\120120\12010027.D\	Continuing Calibration Blank	KQ2019138-02	12/2/2020	03:15:00	
J:\gc24\data\120120\12010028.D\	Continuing Calibration Verification	KQ2019138-01	12/2/2020	03:38:00	
J:\gc24\data\120120\12010029.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	04:01:00	
J:\gc24\data\120120\12010030.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	04:24:00	
J:\gc24\data\120120\12010031.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	04:47:00	
J:\gc24\data\120120\12010032.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	05:10:00	
J:\gc24\data\120120\12010033.D\	Method Blank	KQ2017965-04	12/2/2020	05:33:00	
J:\gc24\data\120120\12010034.D\	Lab Control Sample	KQ2017965-03	12/2/2020	05:56:00	
J:\gc24\data\120120\12010035.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	06:19:00	
J:\gc24\data\120120\12010036.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	06:42:00	
J:\gc24\data\120120\12010037.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	07:04:00	
J:\gc24\data\120120\12010038.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	07:27:00	
J:\gc24\data\120120\12010039.D\	Continuing Calibration Blank	KQ2019138-04	12/2/2020	07:50:00	
J:\gc24\data\120120\12010040.D\	Continuing Calibration Verification	KQ2019138-03	12/2/2020	08:13:00	

ALS Group USA, Corp.  
dba ALS Environmental

QA/QC Report

Client: Anchor QEA, LLC  
Project: GascoSiltronic: US Moorings

Service Request:K2010495

Analysis Run Log  
Chlorinated Herbicides by GC

Analysis Method: 8151A

Analysis Lot:705654

Instrument ID:K-GC-24

Raw Data File	Sample Name	Lab Code	Date Analyzed	Time Analyzed	Q
J:\gc24\data\120120\12010039.D\	Continuing Calibration Blank	KQ2019199-02	12/2/2020	07:50:00	
J:\gc24\data\120120\12010040.D\	Continuing Calibration Verification	KQ2019199-01	12/2/2020	08:13:00	
J:\gc24\data\120120\12010041.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	08:36:00	
J:\gc24\data\120120\12010042.D\	USMPDI-003SC-B-00-02-201110	K2010495-001	12/2/2020	08:59:00	
J:\gc24\data\120120\12010044.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	09:44:00	
J:\gc24\data\120120\12010045.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	10:07:00	
J:\gc24\data\120120\12010046.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	10:30:00	
J:\gc24\data\120120\12010047.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	10:53:00	
J:\gc24\data\120120\12010048.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	11:16:00	
J:\gc24\data\120120\12010049.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	11:39:00	
J:\gc24\data\120120\12010050.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	12:02:00	
J:\gc24\data\120120\12010051.D\	Continuing Calibration Verification	KQ2019199-03	12/2/2020	12:25:00	
J:\gc24\data\120120\12010052.D\	Continuing Calibration Blank	KQ2019199-04	12/2/2020	12:48:00	
J:\gc24\data\120120\12010053.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	13:11:00	
J:\gc24\data\120120\12010054.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	13:33:00	
J:\gc24\data\120120\12010055.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	13:56:00	
J:\gc24\data\120120\12010056.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	14:19:00	
J:\gc24\data\120120\12010057.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	14:42:00	
J:\gc24\data\120120\12010058.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	15:05:00	
J:\gc24\data\120120\12010059.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	15:28:00	
J:\gc24\data\120120\12010060.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	15:51:00	
J:\gc24\data\120120\12010061.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	16:14:00	
J:\gc24\data\120120\12010062.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	16:37:00	
J:\gc24\data\120120\12010063.D\	Continuing Calibration Verification	KQ2019199-05	12/2/2020	17:00:00	
J:\gc24\data\120120\12010064.D\	Continuing Calibration Blank	KQ2019199-06	12/2/2020	17:23:00	
J:\gc24\data\120120\12010065.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	17:46:00	
J:\gc24\data\120120\12010066.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	18:08:00	
J:\gc24\data\120120\12010067.D\	ZZZZZZZ	ZZZZZZZ	12/2/2020	18:31:00	
J:\gc24\data\120120\12010068.D\	USMPDI-003SC-B-02-04-201110	K2010495-002	12/2/2020	18:54:00	
J:\gc24\data\120120\12010069.D\	USMPDI-003SC-B-04-06-201110	K2010495-003	12/2/2020	19:17:00	
J:\gc24\data\120120\12010070.D\	USMPDI-003SC-B-06-08-201110	K2010495-004	12/2/2020	19:40:00	
J:\gc24\data\120120\12010071.D\	USMPDI-006SC-D-00-02-201110	K2010495-005	12/2/2020	20:03:00	
J:\gc24\data\120120\12010072.D\	USMPDI-006SC-D-02-04-201110	K2010495-006	12/2/2020	20:26:00	
J:\gc24\data\120120\12010073.D\	USMPDI-006SC-D-04-06-201110	K2010495-007	12/2/2020	20:49:00	
J:\gc24\data\120120\12010074.D\	USMPDI-006SC-D-06-08-201110	K2010495-008	12/2/2020	21:12:00	
J:\gc24\data\120120\12010075.D\	Continuing Calibration Verification	KQ2019199-07	12/2/2020	21:34:00	
J:\gc24\data\120120\12010076.D\	Continuing Calibration Blank	KQ2019199-08	12/2/2020	21:57:00	
J:\gc24\data\120120\12010077.D\	USMPDI-006SC-D-08-10-201110	K2010495-009	12/2/2020	22:20:00	
J:\gc24\data\120120\12010078.D\	USMPDI-006SC-D-10-12-201110	K2010495-010	12/2/2020	22:43:00	
J:\gc24\data\120120\12010079.D\	USMPDI-006SC-D-12-14-201110	K2010495-011	12/2/2020	23:06:00	
J:\gc24\data\120120\12010080.D\	USMPDI-1006SC-D-10-12-201110	K2010495-012	12/2/2020	23:29:00	
J:\gc24\data\120120\12010081.D\	USMPDI-006SC-D-12-14-201110 MS	KQ2017965-01	12/2/2020	23:52:00	
J:\gc24\data\120120\12010082.D\	USMPDI-006SC-D-12-14-201110 DMS	KQ2017965-02	12/3/2020	00:15:00	
J:\gc24\data\120120\12010083.D\	Continuing Calibration Verification	KQ2019199-09	12/3/2020	00:38:00	
J:\gc24\data\120120\12010084.D\	Continuing Calibration Blank	KQ2019199-10	12/3/2020	01:00:00	

ALS Group USA, Corp.  
dba ALS Environmental

Prep Summary Report

**Client:** Anchor QEA, LLC  
**Project:** GascoSiltronic: US Moorings  
**Sample Matrix:** Sediment

**Service Request:** K2010495

Chlorinated Herbicides by GC

**Prep Method:** Method  
**Analytical Method:** 8151A

**Extraction Lot:** 369767  
**Extraction Date:** 11/13/20 11:38

Sample Name	Lab Code	Date Collected	Date Received	Sample Amount	Final Amount	Percent Solids
USMPDI-003SC-B-00-02-201110	K2010495-001	11/10/20	11/12/20	30.032 g	50 mL	60.0
USMPDI-003SC-B-02-04-201110	K2010495-002	11/10/20	11/12/20	30.035 g	50 mL	77.7
USMPDI-003SC-B-04-06-201110	K2010495-003	11/10/20	11/12/20	30.139 g	50 mL	77.3
USMPDI-003SC-B-06-08-201110	K2010495-004	11/10/20	11/12/20	30.090 g	50 mL	81.3
USMPDI-006SC-D-00-02-201110	K2010495-005	11/10/20	11/12/20	30.258 g	50 mL	58.8
USMPDI-006SC-D-02-04-201110	K2010495-006	11/10/20	11/12/20	30.260 g	50 mL	75.1
USMPDI-006SC-D-04-06-201110	K2010495-007	11/10/20	11/12/20	30.024 g	50 mL	80.7
USMPDI-006SC-D-06-08-201110	K2010495-008	11/10/20	11/12/20	30.195 g	50 mL	77.6
USMPDI-006SC-D-08-10-201110	K2010495-009	11/10/20	11/12/20	30.150 g	50 mL	76.2
USMPDI-006SC-D-10-12-201110	K2010495-010	11/10/20	11/12/20	30.083 g	50 mL	73.2
USMPDI-006SC-D-12-14-201110	K2010495-011	11/10/20	11/12/20	30.008 g	50 mL	72.3
USMPDI-1006SC-D-10-12-201110	K2010495-012	11/10/20	11/12/20	30.132 g	50 mL	72.9
Matrix Spike	KQ2017965-01MS	11/10/20	11/12/20	30.092 g	50 mL	72.3
Duplicate Matrix Spike	KQ2017965-02DMS	11/10/20	11/12/20	30.054 g	50 mL	72.3
Lab Control Sample	KQ2017965-03LCS	NA	NA	30.00 g	50 mL	
Method Blank	KQ2017965-04MB	NA	NA	30.2970 g	50 mL	



## Raw Data

**ALS Environmental—Kelso Laboratory**  
1317 South 13th Avenue, Kelso, WA 98626  
Phone (360)577-7222 Fax (360)636-1068  
[www.alsglobal.com](http://www.alsglobal.com)





# Total Solids

**ALS Environmental—Kelso Laboratory**  
1317 South 13th Avenue, Kelso, WA 98626  
Phone (360)577-7222 Fax (360)636-1068  
[www.alsglobal.com](http://www.alsglobal.com)

# Analytical Results Summary

Instrument Name: K-Balance-41

Analyst: BNETLING

Analysis Lot: 705793

Method/Testcode: SM 2540 G/T/S

Lab Code	Target Analytes	QC	Parent Sample	Matrix	Raw Result	Sample Amt.	Final Result	Dil	MDL	PQL	% Rec	% RSD	Date Analyzed	QC? Tier
K2010495-001	Solids, Total	N/A		Sediment	60.00 Percent	27.7690 g	60.0 Percent	1					12/3/20 16:35:00	N IV
K2010495-002	Solids, Total	N/A		Sediment	77.70 Percent	26.0626 g	77.7 Percent	1					12/3/20 16:35:00	N IV
K2010495-003	Solids, Total	N/A		Sediment	77.30 Percent	26.266 g	77.3 Percent	1					12/3/20 16:35:00	N IV
K2010495-004	Solids, Total	N/A		Sediment	81.30 Percent	30.1708 g	81.3 Percent	1					12/3/20 16:35:00	N IV
K2010495-005	Solids, Total	N/A		Sediment	58.80 Percent	36.5374 g	58.8 Percent	1					12/3/20 16:35:00	N IV
K2010495-006	Solids, Total	N/A		Sediment	75.10 Percent	31.3029 g	75.1 Percent	1					12/3/20 16:35:00	N IV
K2010495-007	Solids, Total	N/A		Sediment	80.70 Percent	29.7549 g	80.7 Percent	1					12/3/20 16:35:00	N IV
K2010495-008	Solids, Total	N/A		Sediment	77.60 Percent	34.1139 g	77.6 Percent	1					12/3/20 16:35:00	N IV
K2010495-009	Solids, Total	N/A		Sediment	76.20 Percent	27.6363 g	76.2 Percent	1					12/3/20 16:35:00	N IV
K2010495-010	Solids, Total	N/A		Sediment	73.20 Percent	31.5741 g	73.2 Percent	1					12/3/20 16:35:00	N IV
K2010495-011	Solids, Total	N/A		Sediment	72.30 Percent	30.4872 g	72.3 Percent	1					12/3/20 16:35:00	Y IV
K2010495-012	Solids, Total	N/A		Sediment	72.90 Percent	26.2000 g	72.9 Percent	1					12/3/20 16:35:00	N IV
K2010728-021	Solids, Total	N/A		Sediment	79.70 Percent	25.7603 g	79.7 Percent	1					12/3/20 16:35:00	N IV
K2010728-022	Solids, Total	N/A		Sediment	74.00 Percent	25.6650 g	74.0 Percent	1					12/3/20 16:35:00	N IV
K2010728-023	Solids, Total	N/A		Sediment	74.80 Percent	33.7359 g	74.8 Percent	1					12/3/20 16:35:00	N IV
KQ2019286-01	Solids, Total	DUP	K2010495-007	Sediment	80.60 Percent	31.5001 g	80.6 Percent	1				<1	12/3/20 16:35:00	N IV
KQ2019286-02	Solids, Total	MB		Sediment	0.00 Percent	50.7176 g	0.0 Percent	1					12/3/20 16:35:00	N IV
KQ2019286-03	Solids, Total	DUP	K2010495-011	Sediment	72.60 Percent	29.8521 g	72.6 Percent	1				<1	12/3/20 16:35:00	N IV

Page 2

# indicates Final Result is not yet adjusted for Solids because it has not yet been determined.





**ALS Group USA, Corp.  
dba ALS Environmental**

Work Order #: K200495, 728


Method: SM 2540 G

Analysis: Total Solids / Volatile Solids

Run: 705793

Matrix: Soil/Solids

Oven Temp and Times				
Oven Temp	Time In	Date In	Time Out	Date Out
105	16:35	12/3/2020	8:35	12/4/2020
105	9:50	12/4/2020	11:00	12/4/2020
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/
/	/	/	/	/

Analyzed By:	BN	Date Analyzed:	12/3/2020
Reviewed By:		Date Reviewed:	12/4/20





# Chlorinated Herbicides by GC

**ALS Environmental—Kelso Laboratory**  
1317 South 13th Avenue, Kelso, WA 98626  
Phone (360)577-7222 Fax (360)636-1068  
[www.alsglobal.com](http://www.alsglobal.com)

# Preparation Information Benchsheet

Prep Run#: 369767

Team: Semivva GC/BGREER

Number of Copies to make: 2

Prep Workflow: OrgHerbs(14)

Prep Method: Method

Status: Prepped

Prep Date/Time: 11/13/20 11:38

#	Lab Code	Client ID	B#	Method /Test	pH	Matrix	Amt. Ext.	Final Vol	Sample Description
1	K2010456-020	USMPDI-057SC-B-04-06-201109	.01	8151A/HERB		Sediment	30.053g	50.00mL	JGRIMES K-Balance-49
2	K2010456-021	USMPDI-057SC-B-06-08-201109	.01	8151A/HERB		Sediment	30.076g	50.00mL	JGRIMES K-Balance-49
3	K2010456-023	USMPDI-057SC-B-10-12-201109	.01	8151A/HERB		Sediment	30.044g	50.00mL	JGRIMES K-Balance-49
4	K2010456-024	USMPDI-057SC-B-12-13-201109	.01	8151A/HERB		Sediment	30.238g	50.00mL	JGRIMES K-Balance-49
5	K2010456-025	USMPDI-1057SC-B-06-08-201109	.01	8151A/HERB		Sediment	30.297g	50.00mL	JGRIMES K-Balance-49
6	K2010495-001	USMPDI-003SC-B-00-02-201110	.01	8151A/HERB		Sediment	30.032g	50.00mL	JGRIMES K-Balance-49
7	K2010495-002	USMPDI-003SC-B-02-04-201110	.01	8151A/HERB		Sediment	30.035g	50.00mL	JGRIMES K-Balance-49
8	K2010495-003	USMPDI-003SC-B-04-06-201110	.01	8151A/HERB		Sediment	30.139g	50.00mL	JGRIMES K-Balance-49
9	K2010495-004	USMPDI-003SC-B-06-08-201110	.01	8151A/HERB		Sediment	30.090g	50.00mL	JGRIMES K-Balance-49
10	K2010495-005	USMPDI-006SC-D-00-02-201110	.01	8151A/HERB		Sediment	30.258g	50.00mL	JGRIMES K-Balance-49
11	K2010495-006	USMPDI-006SC-D-02-04-201110	.01	8151A/HERB		Sediment	30.260g	50.00mL	JGRIMES K-Balance-49
12	K2010495-007	USMPDI-006SC-D-04-06-201110	.01	8151A/HERB		Sediment	30.024g	50.00mL	JGRIMES K-Balance-49
13	K2010495-008	USMPDI-006SC-D-06-08-201110	.01	8151A/HERB		Sediment	30.195g	50.00mL	JGRIMES K-Balance-49
14	K2010495-009	USMPDI-006SC-D-08-10-201110	.01	8151A/HERB		Sediment	30.150g	50.00mL	JGRIMES K-Balance-49
15	K2010495-010	USMPDI-006SC-D-10-12-201110	.01	8151A/HERB		Sediment	30.083g	50.00mL	JGRIMES K-Balance-49
16	K2010495-011	USMPDI-006SC-D-12-14-201110	.02	8151A/HERB		Sediment	30.008g	50.00mL	JGRIMES K-Balance-49
17	K2010495-012	USMPDI-1006SC-D-10-12-201110	.01	8151A/HERB		Sediment	30.132g	50.00mL	JGRIMES K-Balance-49
18	KQ2017965-01	K2010495-011 MS	.02	8151A/HERB		Solid	30.092g	50.00mL	JGRIMES K-Balance-49
19	KQ2017965-02	K2010495-011 DMS	.02	8151A/HERB		Solid	30.054g	50.00mL	JGRIMES K-Balance-49
20	KQ2017965-03	LCS		8151A/HERB		Solid	30.00g	50.00mL	
21	KQ2017965-04	MB		8151A/HERB		Solid	30.2970g	50.00mL	

### Spiking Solutions

Name:	8151A 5ppm Herbicide surrogate	Inventory ID	213982	Logbook Ref:	Penta02-15M	Expires On:	05/22/2021
K2010456-020	1,000.00µL	K2010456-021	1,000.00µL	K2010456-024	1,000.00µL	K2010495-001	1,000.00µL
K2010495-002	1,000.00µL	K2010495-003	1,000.00µL	K2010495-004	1,000.00µL	K2010495-007	1,000.00µL
K2010495-008	1,000.00µL	K2010495-009	1,000.00µL	K2010495-010	1,000.00µL	K2010495-012	1,000.00µL
K2017965-02	1,000.00µL	KQ2017965-03	1,000.00µL	KQ2017965-04	1,000.00µL	KQ2017965-01	1,000.00µL
Name:	8151A 5-500ppm Herbicides matrix spike	Inventory ID	213989	Logbook Ref:	penta02-16B	Expires On:	05/22/2021
KQ2017965-01	1,000.00µL	KQ2017965-02	1,000.00µL	KQ2017965-03	1,000.00µL		



# Preparation Information Benchsheet

Prep Run#: 369767  
 Team: Semivoa GC/BGREER

Prep WorkFlow: OrgHerbs(14)  
 Prep Method: Method

Status: Prepped  
 Prep Date/Time: 11/13/20 11:38

## Preparation Steps

Step:	Weight	Step:	Extraction	Step:	Derivatization	Step:	Final Volume
Started:	11/13/20 11:38	Started:	11/24/20 15:05	Started:	11/30/20 09:25	Started:	11/30/20 09:55
Finished:	11/24/20 17:31	Finished:	11/24/20 15:35	Finished:	11/30/20 09:55	Finished:	11/30/20 11:45
By:	BGREER	By:	BGREER	By:	TNORRIS	By:	TNORRIS
Comments		Comments		Comments		Comments	

Comments: *White pulp 641-10-11*

Reviewed By: \_\_\_\_\_ Date: \_\_\_\_\_

Chain of Custody

Relinquished By: <u><i>Thom</i></u>	Date: <u><i>11/30/20</i></u>
Received By: _____	Date: _____
Extracts Examined Yes <input type="checkbox"/> No <input type="checkbox"/>	

# Preparation Information Benchsheet

Prep Run#: 369767

Team: Semivoa GC/BGREER

Number of Copies to make: 2

Prep Workflow: OrgHerbs(14)

Prep Method: Method

Status: Prepped

Prep Date/Time: 11/13/20 11:38

#	Lab Code	Client ID	B#	Method /Test	pH	Matrix	Amt. Ext.	Final Vol	Sample Description
1	K2010456-020	USMPDI-057SC-B-04-06-201109	.01	8151A/HERB		Sediment	30.053g	50.00mL	JGRIMES K-Balance-49
2	K2010456-021	USMPDI-057SC-B-06-08-201109	.01	8151A/HERB		Sediment	30.076g	50.00mL	JGRIMES K-Balance-49
3	K2010456-023	USMPDI-057SC-B-10-12-201109	.01	8151A/HERB		Sediment	30.044g	50.00mL	JGRIMES K-Balance-49
4	K2010456-024	USMPDI-057SC-B-12-13-5-201109	.01	8151A/HERB		Sediment	30.238g	50.00mL	JGRIMES K-Balance-49
5	K2010456-025	USMPDI-1057SC-B-06-08-201109	.01	8151A/HERB		Sediment	30.297g	50.00mL	JGRIMES K-Balance-49
6	K2010495-001	USMPDI-003SC-B-00-02-201110	.01	8151A/HERB		Sediment	30.032g	50.00mL	JGRIMES K-Balance-49
7	K2010495-002	USMPDI-003SC-B-02-04-201110	.01	8151A/HERB		Sediment	30.035g	50.00mL	JGRIMES K-Balance-49
8	K2010495-003	USMPDI-003SC-B-04-06-201110	.01	8151A/HERB		Sediment	30.139g	50.00mL	JGRIMES K-Balance-49
9	K2010495-004	USMPDI-003SC-B-06-08-201110	.01	8151A/HERB		Sediment	30.090g	50.00mL	JGRIMES K-Balance-49
10	K2010495-005	USMPDI-006SC-D-00-02-201110	.01	8151A/HERB		Sediment	30.258g	50.00mL	JGRIMES K-Balance-49
11	K2010495-006	USMPDI-006SC-D-02-04-201110	.01	8151A/HERB		Sediment	30.260g	50.00mL	JGRIMES K-Balance-49
12	K2010495-007	USMPDI-006SC-D-04-06-201110	.01	8151A/HERB		Sediment	30.024g	50.00mL	JGRIMES K-Balance-49
13	K2010495-008	USMPDI-006SC-D-06-08-201110	.01	8151A/HERB		Sediment	30.195g	50.00mL	JGRIMES K-Balance-49
14	K2010495-009	USMPDI-006SC-D-08-10-201110	.01	8151A/HERB		Sediment	30.150g	50.00mL	JGRIMES K-Balance-49
15	K2010495-010	USMPDI-006SC-D-10-12-201110	.01	8151A/HERB		Sediment	30.083g	50.00mL	JGRIMES K-Balance-49
16	K2010495-011	USMPDI-006SC-D-12-14-201110	.02	8151A/HERB		Sediment	30.008g	50.00mL	JGRIMES K-Balance-49
17	K2010495-012	USMPDI-1006SC-D-10-12-201110	.01	8151A/HERB		Sediment	30.132g	50.00mL	JGRIMES K-Balance-49
18	K2010495-011	MS	.02	8151A/HERB		Solid	30.092g	50.00mL	JGRIMES K-Balance-49
19	K2010495-02	K2010495-011 DMS	.02	8151A/HERB		Solid	30.054g	50.00mL	JGRIMES K-Balance-49
20	K2010495-03	LCS		8151A/HERB		Solid	30.00g	50.00mL	
21	K2010495-04	MB		8151A/HERB		Solid	30.2970g	50.00mL	

## Spiking Solutions

Name:	8151A 5ppm Herbicide surrogate	Inventory ID	213982	Logbook Ref:	Penta02-15M	Expires On:	05/22/2021
K2010456-020	1,000.00µL	K2010456-021	1,000.00µL	K2010456-024	1,000.00µL	K2010495-001	1,000.00µL
K2010495-002	1,000.00µL	K2010495-003	1,000.00µL	K2010495-004	1,000.00µL	K2010495-007	1,000.00µL
K2010495-008	1,000.00µL	K2010495-009	1,000.00µL	K2010495-010	1,000.00µL	K2010495-012	1,000.00µL
K2010495-02	1,000.00µL	K2010495-03	1,000.00µL	K2010495-04	1,000.00µL	K2010495-01	1,000.00µL
Name: 8151A 5-500ppm Herbicides matrix spike							
K2010495-01	1,000.00µL	K2010495-02	1,000.00µL	K2010495-03	1,000.00µL	Expires On: 05/22/2021	

# Preparation Information Benchsheet

Prep Run#: 369767  
 Team: Semivoa GC/BGREER

Prep WorkFlow: OrgHerbs(14)  
 Prep Method: Method

Status: Prepped  
 Prep Date/Time: 11/13/20 11:38

## Preparation Steps

Step:	Weight	Step:	Extraction	Step:	Derivatization	Step:	Final Volume
Started:	11/13/20 11:38	Started:	11/24/20 15:05	Started:	11/30/20 09:25	Started:	11/30/20 09:55
Finished:	11/24/20 17:31	Finished:	11/24/20 15:35	Finished:	11/30/20 09:55	Finished:	11/30/20 11:45
By:	BGREER	By:	BGREER	By:	TNORRIS	By:	TNORRIS
Comments		Comments		Comments		Comments	

Comments: \_\_\_\_\_

Reviewed By: [Signature] Date: 12-4-20

Chain of Custody

Relinquished By: <u>[Signature]</u>	Date: <u>11/30/20</u>	Extracts Examined Yes      No
Received By: <u>[Signature]</u>	Date: <u>11-30-20</u>	

# Preparation Information Benchsheet

Prep Run#: 369767

Team: Semivova GC/BGREER

Number of Copies to make: 2

Prep Workflow: OrgHerbS(14)

Prep Method: Method

Status: Draft

Prep Date/Time: 11/13/20 11:38 AM

#	Lab Code	Client ID	B#	Method / Test	Matrix	Amt. Ext.	pH	Int. Vol mL	Final Vol mL	Surr Amt mL	Spike Amt mL
1	K2010456-020	USMPDI-057SC-B-04-06-201109	.01	8151A / HERB	Sediment	9	N/A		888	1000	1000
2	K2010456-021	USMPDI-057SC-B-06-08-201109	.01	8151A / HERB	Sediment	X			888		
3	K2010456-023	USMPDI-057SC-B-10-12-201109	.01	8151A / HERB	Sediment	X			888		
4	K2010456-024	USMPDI-057SC-B-12-13.5-201109	.01	8151A / HERB	Sediment	X			888		
5	K2010456-025	USMPDI-107SC-B-06-08-201109	.01	8151A / HERB	Sediment	X			888		
6	K2010495-001	USMPDI-003SC-B-00-02-201110	.01	8151A / HERB	Sediment	X			888		
7	K2010495-002	USMPDI-003SC-B-02-04-201110	.01	8151A / HERB	Sediment	X			888		
8	K2010495-003	USMPDI-003SC-B-04-06-201110	.01	8151A / HERB	Sediment	X			888		
9	K2010495-004	USMPDI-003SC-B-06-08-201110	.01	8151A / HERB	Sediment	X			888		
10	K2010495-005	USMPDI-006SC-D-00-02-201110	.01	8151A / HERB	Sediment	X			888		
11	K2010495-006	USMPDI-006SC-D-02-04-201110	.01	8151A / HERB	Sediment	X			888		
12	K2010495-007	USMPDI-006SC-D-04-06-201110	.01	8151A / HERB	Sediment	X			888		
13	K2010495-008	USMPDI-006SC-D-06-08-201110	.01	8151A / HERB	Sediment	X			888		
14	K2010495-009	USMPDI-006SC-D-08-10-201110	.01	8151A / HERB	Sediment	X			888		
15	K2010495-010	USMPDI-006SC-D-10-12-201110	.01	8151A / HERB	Sediment	X			888		
16	K2010495-011	USMPDI-006SC-D-12-14-201110	.02	8151A / HERB	Sediment	X			888		
17	K2010495-012	USMPDI-1006SC-D-10-12-201110	.01	8151A / HERB	Sediment	X			888		
18	KQ2017965-01	K2010495-011 MS	.02	8151A / HERB	Solid	X			888		1000
19	KQ2017965-02	K2010495-011 DMS	.02	8151A / HERB	Solid	X			888		1000
20	KQ2017965-03	LCS		8151A / HERB	Solid	30.000			888		
21	KQ2017965-04	MB		8151A / HERB	Solid	30.297			888		

Comments: *See preprep sheet*

Surrogate ID: *Pentao2-15m 5ppm Ace xp: 5/12/21 1000µL* Spike ID: *Pentao2-16B 5-5ppm Ace xp: 5/12/21*

Witnessed By: *[Signature]*

Assisted By: *[Signature]*

# Pre-Prep Information Benchsheet

Prep Run #: 369767

Container Lot No: 090720-1BNU, 090720-1TW      Prep Due Date: Nov-18-2020

#	Lab Code	Bottle	Test Name	Weight	Sample Comments	Test Comments
1	K2010495-001	.01	HERB : 8151A/	30.032g		JGRIMES K-Balance-49
2	K2010495-002	.01	HERB : 8151A/	30.035g		JGRIMES K-Balance-49
3	K2010495-003	.01	HERB : 8151A/	30.139g		JGRIMES K-Balance-49
4	K2010495-004	.01	HERB : 8151A/	30.090g		JGRIMES K-Balance-49
5	K2010495-005	.01	HERB : 8151A/	30.258g		JGRIMES K-Balance-49
6	K2010495-006	.01	HERB : 8151A/	30.260g		JGRIMES K-Balance-49
7	K2010495-007	.01	HERB : 8151A/	30.024g		JGRIMES K-Balance-49
8	K2010495-008	.01	HERB : 8151A/	30.195g		JGRIMES K-Balance-49
9	K2010495-009	.01	HERB : 8151A/	30.150g		JGRIMES K-Balance-49
10	K2010495-010	.01	HERB : 8151A/	30.083g		JGRIMES K-Balance-49
11	K2010495-011	.02	HERB : 8151A/	30.008g		JGRIMES K-Balance-49
12	K2010495-011 MS	.02	HERB : 8151A/	30.092g		JGRIMES K-Balance-49
13	K2010495-011 DMS	.02	HERB : 8151A/	30.054g		JGRIMES K-Balance-49
14	K2010495-012	.01	HERB : 8151A/	30.132g		JGRIMES K-Balance-49

*Delivered to freezer*

Relinquished By: <i>JS</i>	Date/Time: <i>11/3/20</i>	Received By:	Date/Time:
----------------------------	---------------------------	--------------	------------

369767

Pre-Prep Information Benchsheet

Prep Run #: 369680 Container Lot No: 090720-1TW Prep Due Date: Nov-17-2020

#	Lab Code	Bottle	Test Name	Weight	Sample Comments	Test Comments
1	K2010456-021	.01	HERB : 8151A/	30.076g		JGRIMES K-Balance-49
2	<del>K2010456-022</del>	<del>.01</del>	<del>HERB : 8151A/</del>	<del>30.198g</del>		<del>JGRIMES K-Balance-49</del>
3	<del>K2010456-022</del>	<del>.01</del>	<del>HERB : 8151A/</del>	<del>30.095g</del>		<del>JGRIMES K-Balance-49</del>
4	<del>K2010456-022</del>	<del>.01</del>	<del>HERB : 8151A/</del>	<del>30.044g</del>		<del>JGRIMES K-Balance-49</del>
5	K2010456-023	.01	HERB : 8151A/	30.044g		JGRIMES K-Balance-49
6	K2010456-024	.01	HERB : 8151A/	30.238g		JGRIMES K-Balance-49
7	K2010456-025	.01	HERB : 8151A/	30.297g		JGRIMES K-Balance-49

Added to 369679 BG 11/21/20

Delivered to  
Freezer

Relinquished By: JB	Date/Time: 11-12-20 10:13	Received By:	Date/Time:
---------------------	---------------------------	--------------	------------

# Pre-Prep Information Benchsheet

Prep Run #: ~~369679~~

Container Lot No: 090720-1TTW

Prep Due Date: Nov-17-2020

#	Lab Code	Bottle	Test Name	Weight	Sample Comments	Test Comments
1	K2010456-001	.01	HERB : 8151A/	30.008g		JGRIMES K-Balance-49
2	K2010456-002	.01	HERB : 8151A/	30.012g		JGRIMES K-Balance-49
3	K2010456-003	.01	HERB : 8151A/	30.030g		JGRIMES K-Balance-49
4	K2010456-004	.01	HERB : 8151A/	30.003g		JGRIMES K-Balance-49
5	K2010456-005	.01	HERB : 8151A/	30.103g		JGRIMES K-Balance-49
6	K2010456-006	.01	HERB : 8151A/	30.010g		JGRIMES K-Balance-49
7	K2010456-007	.01	HERB : 8151A/	30.072g		JGRIMES K-Balance-49
8	K2010456-008	.01	HERB : 8151A/	30.076g		JGRIMES K-Balance-49
9	K2010456-009	.01	HERB : 8151A/	30.097g		JGRIMES K-Balance-49
10	K2010456-010	.01	HERB : 8151A/	30.066g		JGRIMES K-Balance-49
11	K2010456-011	.01	HERB : 8151A/	30.090g		JGRIMES K-Balance-49
12	K2010456-012	.01	HERB : 8151A/	30.080g		JGRIMES K-Balance-49
13	K2010456-013	.01	HERB : 8151A/	30.008g		JGRIMES K-Balance-49
14	K2010456-014	.01	HERB : 8151A/	30.141g		JGRIMES K-Balance-49
15	K2010456-015	.01	HERB : 8151A/	30.110g		JGRIMES K-Balance-49
16	K2010456-016	.01	HERB : 8151A/	30.142g		JGRIMES K-Balance-49
17	K2010456-017	.01	HERB : 8151A/	30.233g		JGRIMES K-Balance-49
18	K2010456-018	.01	HERB : 8151A/	30.104g		JGRIMES K-Balance-49
19	K2010456-019	.01	HERB : 8151A/	30.096g		JGRIMES K-Balance-49
20	<del>K2010456-020</del>	.01	HERB : 8151A/	30.055g		JGRIMES K-Balance-49

Added to 369767 RG 11/21/20  
 Delivered to freezer

Relinquished By: JG Date/Time: 11-12-20 10:13 Received By: \_\_\_\_\_ Date/Time: \_\_\_\_\_

**Additional Prep Information for EPA Method 8151A**

**Herbicides in Soil**

Service Request # K2010456/0495 Work Group # KQ2017965

Acidified Sulfate Lot # DZ03870 Matrix Sand Lot # 012418

Ethyl Ether Lot # DZ487 Hydrochloric Acid Lot # S8242

Wrist Action Shaker Start (time/date/initial): 15:05 11/24/20 QR/BG

Wrist Action Shaker Stop (time/date/initial): 15:35 11/24/20 QR/BG

N-Evap (time/date/initial) 0820 11/25/20 BG N-Evap Thermometer ID: X-SVM-004

Temp as measured: 20 °C Correction factor: 0.0 °C Adjusted temp: 20.0 °C

Saponification Start (time/date/initial): 0930 11/25/20 BG 37% KOH Lot # DZ03-80M

Saponification Stop (time/date/initial): 1035 11/25/20 BG

Extraction Start (time/date/initial): 1200 11/25/20 BG Sulfuric Acid Lot # DZ0397H

Extraction Stop (time/date/initial): 1315 11/25/20 BG

Derivatization Start (time/date/initial): 0955 11/30/20 TV Diazomethane Lot # DZ03 435

Derivatization Stop (time/date/initial): 0955 11/30/20 TV

Pipette (5 mL) Lot # 04420077

Solvent Exchange to Iso-Octane (time/date/initial): 0955 11/30/20 TV

Iso-Octane Lot # DY719-45 N-Evap Thermometer ID: X-SVM-000

Temp as measured: 20 °C Correction factor: 0 °C Adjusted temp: 20 °C

Pipette (1 mL) Lot # 02720076

Vial: red Vial Storage: \_\_\_\_\_

Archive Storage: Storilux

Additional Comments: completed 11/25 11/30/20 TV

Bench Sheet Review Check List	
<input checked="" type="checkbox"/>	Hold times met (if no, reason: _____)
<input checked="" type="checkbox"/>	Prep date, time, method, department, product code correct in stealth
<input checked="" type="checkbox"/>	Spike information and Q.C. correct (insufficient volume or mass recorded if no Q.C.)
<input checked="" type="checkbox"/>	Weights/Volumes and units correct on raw and final bench sheets
<input checked="" type="checkbox"/>	Sample IDs have been checked - bottle numbers appended if required
<input checked="" type="checkbox"/>	Names present for: started by, completed by, relinquished by, and witnessed by. Training circled.
<input checked="" type="checkbox"/>	Extract storage recorded
<input checked="" type="checkbox"/>	Additional prep sheet completely filled out ( NA or line out blanks)
<input checked="" type="checkbox"/>	All clean-ups have been noted on additional prep sheet
<input checked="" type="checkbox"/>	Signed service request with Form V, if applicable, has been attached



# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010042.D\  
**Lab ID:** K2010495-001  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 08:59:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery	X	
Continuing Calibration Recovery (Closing)	X	
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010042.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 08:59:00	<b>Vial:</b> 25
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-001	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-001.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.99	7.82	931530	3451302	51.193	81.595	51	82	51	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.26	10.10 <sup>-0.04</sup>	7177	102975	0.077	0.507	0.21U	1.4U	4.0 U	Y
2,4-D	9.34 <sup>+0.02</sup>	9.04 <sup>-0.03</sup>	2133	57569	0.100	1.124	0.28U	3.1U	13 U	Y

**Prep Amount:** 30.032 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 60.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010042.D Vial: 10  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 8:59 am Operator: UA  
 Sample : K2010495-001 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 15:10:03 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.988	7.822	931530	3451302	51.193m	81.595 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.338	9.042	2133	57569	0.100m	1.124 #
8) m 2,4,5-TP ...	10.258	10.095	7177	102975	0.077	0.507m#
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010042.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:59 am  
Sample : K2010495-001  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 15:10:03 2020  
Quant Results File: 102120\_8151.RES

Vial: 10  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010042.D Vial: 10  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 8:59 am Operator: UA  
 Sample : K2010495-001 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 14:32:11 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(2) 2,4-Dichlorophenylacetic Acid (s)

7.988min 53.226 ppb  
 response 968533

Manual Integration:

Before

12/02/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)



7.822min 81.595 ppb  
 response 3451302

(+) = Expected Retention Time

Data File : J:\gc24\data\120120\12010042.D Vial: 10  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:59 am Operator: UA  
Sample : K2010495-001 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 14:32:11 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(2) 2,4-Dichlorophenylacetic Acid (s)

7.988min 51.193 ppb m  
response 931530

Manual Integration:

After  
Baseline/Shoulder  
12/02/20



(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.822min 81.595 ppb  
response 3451302

Data File : J:\gc24\data\120120\12010042.D Vial: 10  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:59 am Operator: UA  
Sample : K2010495-001 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 14:32:11 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.338min 0.150 ppb  
response 3183



Manual Integration:  
Before  
12/02/20

(7) 2,4-D #2 (m)  
9.042min 1.124 ppb  
response 57569

Data File : J:\gc24\data\120120\12010042.D Vial: 10  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:59 am Operator: UA  
Sample : K2010495-001 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 14:32:11 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.338min 0.100 ppb m  
response 2133

(7) 2,4-D #2 (m)  
9.042min 1.124 ppb  
response 57569



Manual Integration:  
After  
Baseline/Shoulder  
12/02/20



Data File : J:\gc24\data\120120\12010042.D Vial: 10  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 8:59 am Operator: UA  
 Sample : K2010495-001 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 14:32:11 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
 10.258min 0.077 ppb  
 response 7177

(8) 2,4,5-TP (Silvex) #2 (m)  
 10.095min 0.507 ppb m  
 response 102975

Manual Integration:

After **Forgot to print "Before" chromatogram**  
 Baseline/Shoulder  
 12/02/20

(+) = Expected Retention Time

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010068.D\  
**Lab ID:** K2010495-002  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 18:54:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)		X
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010068.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 18:54:00	<b>Vial:</b> 3
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-002	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-002.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	1031038	4055729	56.661	95.885	57	96	57	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.12	9458	24242	0.101	0.119 <sup>ccv</sup>	0.22U	0.25U	3.1 U	Y
2,4-D	9.36 <sup>+0.06</sup>	9.03 <sup>-0.02</sup>	1957	46586	0.092	0.910	0.20U	1.9U	9.9 U	Y

**Prep Amount:** 30.035 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 77.70

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010068.D Vial: 11  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 6:54 pm Operator: UA  
 Sample : K2010495-002 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:00:26 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.978	7.811	1031038	4055729	56.661	95.885 #
Target Compounds						
1) m Dalapon	3.131	2.871	6894	89264	0.284	1.848 #
3) m Dicamba	8.201	7.911	13639	89658	0.195	0.605 #
4) m MCPP	8.304	8.095	51631	103812	1619.833	N.D. #
5) m MCPA	8.588	8.345	6243	84877	106.622	N.D. #
6) m Dichloroprop	8.951	8.748	18118	18754	0.972	0.450 #
7) m 2,4-D	9.361	9.031	1957	46586	0.092	0.910 #
8) m 2,4,5-TP ...	10.244	10.118	9458	24242	0.101	0.119 #
9) m 2,4,5-T	10.691	10.528	5110	21377	0.062	0.112 #
10) m 2,4-DB	11.321	11.168	42358	55009	4.129	1.896 #
11) m Dinoseb	11.638	11.318	66175	37746	1.070	0.276 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010068.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 6:54 pm  
Sample : K2010495-002  
Misc :

Vial: 11  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:00:26 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010069.D\  
**Lab ID:** K2010495-003  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 19:17:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)		X
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010069.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 19:17:00	<b>Vial:</b> 4
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-003	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-003.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	970929	3801322	53.358	89.870	53	90	53	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.08 <sup>-0.04</sup>	5075	56038	0.054	0.276 <sup>CCV</sup>	0.12U	0.59U	3.1 U	Y
2,4-D	9.37 <sup>+0.07</sup>	9.03 <sup>-0.02</sup>	2517	49944	0.119	0.975	0.26U	2.1U	10 U	Y

**Prep Amount:** 30.139 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 77.30

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010069.D Vial: 12  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 7:17 pm Operator: UA  
 Sample : K2010495-003 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:01:08 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.975	7.806	970929	3801322	53.358m	89.870m#
Target Compounds						
1) m Dalapon	3.135	2.876	58953	55143	2.430	1.141 #
3) m Dicamba	8.259	7.896	7536	60028	0.108	0.405 #
4) m MCPP	8.299	8.092	17093	68484	876.604	N.D. #
5) m MCPA	8.579	8.339	3588	68791	61.278	N.D. #
6) m Dichloroprop	8.945	8.766	14853	2359	0.797	0.057 #
7) m 2,4-D	9.365	9.026	2517	49944	0.119	0.975 #
8) m 2,4,5-TP ...	10.239	10.076f	5075	56038	0.054	0.276 #
9) m 2,4,5-T	10.732	10.516	15178	4404	0.184	0.023 #
10) m 2,4-DB	11.312	11.159	29301	18806	2.856	0.648 #
11) m Dinoseb	11.629	11.352	50423	231831	0.815	1.695 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data File : J:\gc24\data\120120\12010069.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:17 pm  
Sample : K2010495-003  
Misc :

Vial: 12  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:01:08 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010069.D Vial: 12  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:17 pm Operator: UA  
Sample : K2010495-003 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:00:46 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.975min 55.010 ppb

response 1001002

Manual Integration:

Before

12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.806min 91.244 ppb



response 3859412

(+) = Expected Retention Time

Data File : J:\gc24\data\120120\12010069.D Vial: 12  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:17 pm Operator: UA  
Sample : K2010495-003 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:00:46 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.975min 53.358 ppb m  
response 970929

Manual Integration:

After

Baseline/Shoulder

12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.806min 89.870 ppb m  
response 3801322

(+) = Expected Retention Time

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010070.D\  
**Lab ID:** K2010495-004  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 19:40:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)		X
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010070.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 19:40:00	<b>Vial:</b> 5
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-004	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-004.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	1068162	4240018	58.701	100.242	59	100	59	26 - 127 P	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.25 <sup>+0.01</sup>	10.09 <sup>-0.03</sup>	6921	107716	0.074	0.531 <sup>CCV</sup>	0.15U	1.1U	3.0 U	Y
2,4-D	9.28 <sup>-0.02</sup>	9.03 <sup>-0.02</sup>	9147	44777	0.431	0.875	0.88U	1.8U	9.5 U	Y

**Prep Amount:** 30.090 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 81.30

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010070.D Vial: 13  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 7:40 pm Operator: UA  
 Sample : K2010495-004 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:01:51 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.977	7.811	1068162	4240018	58.701m	100.242 #
Target Compounds						
1) m Dalapon	0.000	2.874	0	208140	N.D. d	4.308
3) m Dicamba	8.214	7.961	5373	23872	0.077	0.161 #
4) m MCPP	8.307	8.097	25005	77228	1046.864	N.D. #
5) m MCPA	8.550	8.344	2136	68671	36.480	N.D. #
6) m Dichloroprop	8.950	8.781	19759	2055	1.060	0.049 #
7) m 2,4-D	9.280	9.034	9147	44777	0.431	0.875 #
8) m 2,4,5-TP ...	10.250	10.087	6921	107716	0.074	0.531 #
9) m 2,4,5-T	10.694	10.527	2984	8225	0.036	0.043
10) m 2,4-DB	11.327	11.167	38030	29732	3.707	1.025 #
11) m Dinoseb	11.644	11.367	57135	336051	0.924	2.457 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010070.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:40 pm  
Sample : K2010495-004  
Misc :

Vial: 13  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:01:51 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010070.D Vial: 13  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:40 pm Operator: UA  
Sample : K2010495-004 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:01:23 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(2) 2,4-Dichlorophenylacetic Acid (s)

7.977min 60.517 ppb

response 1101203

Manual Integration:

Before

12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.811min 100.242 ppb



response 4240018



Data File : J:\gc24\data\120120\12010070.D Vial: 13  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:40 pm Operator: UA  
Sample : K2010495-004 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:01:23 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(2) 2,4-Dichlorophenylacetic Acid (s)

7.977min 58.701 ppb m

response 1068162

Manual Integration:

After

Baseline/Shoulder

12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.811min 100.242 ppb

response 4240018

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010071.D\  
**Lab ID:** K2010495-005  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 20:03:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)		X
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010071.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 20:03:00	<b>Vial:</b> 6
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-005	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-005.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.97 <sup>-0.01</sup>	7.81	1078598	3977158	59.275	94.027	59	94	59	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.23 <sup>-0.01</sup>	10.08 <sup>-0.04</sup>	6424	379996	0.069	1.872 <sup>CCV</sup>	0.19U	5.3J	4.1 U	Y
2,4-D	9.32 <sup>+0.02</sup>	9.09 <sup>+0.04</sup>	10063	41693	0.474	0.814	1.3U	2.3U	13 U	Y

**Prep Amount:** 30.258 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 58.80

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Data File : J:\gc24\data\120120\12010071.D Vial: 14  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 8:03 pm Operator: UA  
 Sample : K2010495-005 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:02:27 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.974	7.808	1078598	3977158	59.275m	94.027m#
Target Compounds						
1) m Dalapon	3.134	2.874	137736	269137	5.678	5.571
3) m Dicamba	8.228	7.921	10018	102456	0.144	0.691 #
4) m MCPP	8.301	8.091	50171	81074	1588.415	N.D. #
5) m MCPA	8.584	8.341	6003	84958	102.523	N.D. #
6) m Dichloroprop	8.948	8.768	9769	40811	0.524	0.978 #
7) m 2,4-D	9.324	9.088	10063	41693	0.474	0.814 #
8) m 2,4,5-TP ...	10.234	10.078f	6424	379996	0.069	1.872 #
9) m 2,4,5-T	10.674	10.521	21905	7543	0.265	0.039 #
10) m 2,4-DB	11.314	11.158	44538	55489	4.341	1.912 #
11) m Dinoseb	11.631	11.354	67004	618650	1.083	4.524 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010071.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:03 pm  
Sample : K2010495-005  
Misc :

Vial: 14  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:02:27 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010071.D Vial: 14  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:03 pm Operator: UA  
Sample : K2010495-005 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:02:05 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.974min 61.514 ppb

response 1119347

Manual Integration:

Before

12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.808min 94.872 ppb



response 4012870

(+) = Expected Retention Time

Data File : J:\gc24\data\120120\12010071.D Vial: 14  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:03 pm Operator: UA  
Sample : K2010495-005 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:02:05 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.974min 59.275 ppb m  
response 1078598

Manual Integration:

After  
Baseline/Shoulder  
12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.808min 94.027 ppb m  
response 3977158

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010072.D\  
**Lab ID:** K2010495-006  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 20:26:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)		X
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_



# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010072.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 20:26:00	<b>Vial:</b> 7
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-006	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-006.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	1201508	4586051	66.029	108.423	66	108	66	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.12	7289	43407	0.078	0.214 <sup>ccv</sup>	0.17U	0.47U	3.2 U	Y
2,4-D	9.28 <sup>-0.02</sup>	9.03 <sup>-0.02</sup>	18700	34920	0.880	0.682	1.9U	1.5U	11 U	Y

**Prep Amount:** 30.260 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 75.10

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010072.D Vial: 15  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 8:26 pm Operator: UA  
 Sample : K2010495-006 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:02:49 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.978	7.808	1201508	4586051	66.029	108.423 #
Target Compounds						
1) m Dalapon	3.135	2.875	4827	111076	0.199	2.299 #
3) m Dicamba	8.205	7.915	32370	96318	0.464	0.650 #
4) m MCPP	8.302	8.095	63470	85165	1874.599	N.D. #
5) m MCPA	8.548	8.345	24200	92544	413.304	N.D. #
6) m Dichloroprop	8.948	8.718	16964	17337	0.910	0.416 #
7) m 2,4-D	9.278	9.028	18700	34920	0.880	0.682
8) m 2,4,5-TP ...	10.238	10.115	7289	43407	0.078	0.214 #
9) m 2,4,5-T	10.678	10.522	14413	17346	0.175	0.091 #
10) m 2,4-DB	11.315	11.162	27297	39594	2.661	1.365 #
11) m Dinoseb	11.635	11.312	65381	51318	1.057	0.375 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010072.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:26 pm  
Sample : K2010495-006  
Misc :

Vial: 15  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:02:49 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2  
Signal #1 Info : 0.25 mm  
Signal #2 Phase: ZB-XLB-HT  
Signal #2 Info : 0.25 mm



# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010073.D\  
**Lab ID:** K2010495-007  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 20:49:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)		X
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010073.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 20:49:00	<b>Vial:</b> 8
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-007	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-007.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.82 <sup>+0.01</sup>	923900	3485387	50.773	82.401	51	82	51	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.25 <sup>+0.01</sup>	10.09 <sup>-0.03</sup>	9005	68475	0.096	0.337 <sup>CCV</sup>	0.20U	0.70U	3.0 U	Y
2,4-D	9.28 <sup>-0.02</sup>	9.03 <sup>-0.02</sup>	9333	33378	0.439	0.652	0.91U	1.3U	9.6 U	Y

**Prep Amount:** 30.024 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 80.70

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010073.D Vial: 16  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 8:49 pm Operator: UA  
 Sample : K2010495-007 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:03:11 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.983	7.816	923900	3485387	50.773	82.401 #
Target Compounds						
1) m Dalapon	3.136	2.876	31331	118853	1.292	2.460 #
3) m Dicamba	8.209	7.930	13999	44201	0.201	0.298 #
4) m MCPP	8.306	8.100	34107	98222	1242.731	N.D. #
5) m MCPA	8.586	8.346	7399	88561	126.365	N.D. #
6) m Dichloroprop	8.953	8.843f	15160	12695	0.813	0.304 #
7) m 2,4-D	9.283	9.033	9333	33378	0.439	0.652 #
8) m 2,4,5-TP ...	10.249	10.086	9005	68475	0.096	0.337 #
9) m 2,4,5-T	10.679	10.526	6618	9893	0.080	0.052 #
10) m 2,4-DB	11.323	11.163	23940	30673	2.333	1.057 #
11) m Dinoseb	11.639	11.363	54515	262972	0.881	1.923 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010073.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:49 pm  
Sample : K2010495-007  
Misc :

Vial: 16  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:03:11 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010074.D\  
**Lab ID:** K2010495-008  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 21:12:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)		X
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_



# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010074.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 21:12:00	<b>Vial:</b> 9
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-008	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-008.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	997864	3752079	54.838	88.706	55	89	55	26 - 127 P	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.11 <sup>-0.01</sup>	5576	20419	0.060	0.101 <sup>CCV</sup>	0.13U	0.22U	3.1 U	Y
2,4-D	9.27 <sup>-0.03</sup>	9.03 <sup>-0.02</sup>	8663	171738	0.408	3.354	0.87U	7.2U	9.9 U	Y

**Prep Amount:** 30.195 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 77.60

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010074.D Vial: 17  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 9:12 pm Operator: UA  
 Sample : K2010495-008 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:03:45 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.976	7.809	997864	3752079	54.838m	88.706 #
Target Compounds						
1) m Dalapon	3.139	2.873	26327	270703	1.085	5.603 #
3) m Dicamba	8.186	7.903	8990	20297	0.129	0.137
4) m MCPP	8.302	8.093	14805	17227	827.368	N.D. #
5) m MCPA	8.546	8.339	1221	72400	20.853	N.D. #
6) m Dichloroprop	8.949	8.753	14051	2400	0.753	0.058 #
7) m 2,4-D	9.272f	9.029	8663	171738	0.408	3.354 #
8) m 2,4,5-TP ...	10.242	10.109	5576	20419	0.060	0.101 #
9) m 2,4,5-T	10.736	10.516	13743	7513	0.167	0.039 #
10) m 2,4-DB	11.316	11.159	25717	37375	2.507	1.288 #
11) m Dinoseb	11.632	11.356	52573	279743	0.850	2.046 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010074.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 9:12 pm  
Sample : K2010495-008  
Misc :

Vial: 17  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:03:45 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010074.D Vial: 17  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 9:12 pm Operator: UA  
Sample : K2010495-008 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:03:30 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.976min 56.517 ppb

response 1028425

Manual Integration:

Before

12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)



7.809min 88.706 ppb

response 3752079

Data File : J:\gc24\data\120120\12010074.D Vial: 17  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 9:12 pm Operator: UA  
Sample : K2010495-008 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:03:30 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.976min 54.838 ppb m  
response 997864

Manual Integration:

After

Baseline/Shoulder

12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.809min 88.706 ppb  
response 3752079

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010077.D\  
**Lab ID:** K2010495-009  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 22:20:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)	X	
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010077.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 22:20:00	<b>Vial:</b> 15
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-009	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-009.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	1172870	4433170	64.455	104.808	64	105	64	26 - 127 P	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.11 <sup>-0.01</sup>	17979	37377	0.192	0.184 <sup>CCV</sup>	0.42U	0.40U	3.2 U	Y
2,4-D	9.27 <sup>-0.03</sup>	9.03 <sup>-0.03</sup>	6295	44572	0.296	0.871	0.64U	1.9U	11 U	Y

**Prep Amount:** 30.150 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 76.20

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Data File : J:\gc24\data\120120\12010077.D Vial: 18  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 10:20 pm Operator: UA  
 Sample : K2010495-009 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:04:28 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.978	7.811	1172870	4433170	64.455	104.808 #
Target Compounds						
1) m Dalapon	3.131	2.875	65479	428786	2.699	8.875 #
3) m Dicamba	8.208	7.921	6278	80553	0.090	0.543 #
4) m MCPP	8.301	8.095	62917	160564	1862.698	N.D. #
5) m MCPA	8.555	8.341	1637	100023	27.958	N.D. #
6) m Dichloroprop	8.948	8.748	17061	23433	0.915	0.562 #
7) m 2,4-D	9.275f	9.028	6295	44572	0.296	0.871 #
8) m 2,4,5-TP ...	10.245	10.115	17979	37377	0.192	0.184
9) m 2,4,5-T	10.681	10.525	11623	17155	0.141	0.090 #
10) m 2,4-DB	11.318	11.158	36384	16806	3.546	0.579 #
11) m Dinoseb	11.638	11.358	54724	344398	0.885	2.518 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data File : J:\gc24\data\120120\12010077.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 10:20 pm  
Sample : K2010495-009  
Misc :

Vial: 18  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:04:28 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010078.D\  
**Lab ID:** K2010495-010  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 22:43:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)	X	
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010078.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 22:43:00	<b>Vial:</b> 10
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-010	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-010.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.82 <sup>+0.01</sup>	948830	3638548	52.143	86.022	52	86	52	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.25 <sup>+0.01</sup>	10.12	6282	17433	0.067	0.086 <sup>CCV</sup>	0.15U	0.20U	3.3 U	Y
2,4-D	9.28 <sup>-0.02</sup>	9.04 <sup>-0.02</sup>	4791	60369	0.226	1.179	0.51U	2.7U	11 U	Y

**Prep Amount:** 30.083 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 73.20

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010078.D Vial: 19  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 10:43 pm Operator: UA  
 Sample : K2010495-010 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:05:03 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.984	7.818	948830	3638548	52.143m	86.022 #
Target Compounds						
1) m Dalapon	3.134	2.874	9447	640749	0.389	13.263 #
3) m Dicamba	8.214	7.918	14079	33610	0.202	0.227
4) m MCPP	8.311	8.104	22614	43604	995.411	N.D. #
5) m MCPA	8.584	8.348	2094	69472	35.763	N.D. #
6) m Dichloroprop	8.957	0.000	16882	0	0.905	N.D. #
7) m 2,4-D	9.277	9.038	4791	60369	0.226	1.179 #
8) m 2,4,5-TP ...	10.251	10.121	6282	17433	0.067	0.086 #
9) m 2,4,5-T	10.687	10.534	4049	8033	0.049	0.042
10) m 2,4-DB	11.324	11.168	28506	22905	2.779	0.789 #
11) m Dinoseb	11.644	11.321	47518	25044	0.768	0.183 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010078.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 10:43 pm  
Sample : K2010495-010  
Misc :

Vial: 19  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:05:03 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010078.D Vial: 19  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 10:43 pm Operator: UA  
 Sample : K2010495-010 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:04:48 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.984min 53.759 ppb  
 response 978228

Manual Integration:

Before

12/03/20



(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.818min 86.022 ppb  
 response 3638548

Data File : J:\gc24\data\120120\12010078.D Vial: 19  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 10:43 pm Operator: UA  
Sample : K2010495-010 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:04:48 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.984min 52.143 ppb m  
response 948830

Manual Integration:

After  
Baseline/Shoulder  
12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.818min 86.022 ppb  
response 3638548

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010079.D\  
**Lab ID:** K2010495-011  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 23:06:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)	X	
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_



# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010079.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 23:06:00	<b>Vial:</b> 16
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-011	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-011.02	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	992574	3903125	54.547	92.277	55	92	55	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.11 <sup>-0.01</sup>	5619	26663	0.060	0.131 <sup>CCV</sup>	0.14U	0.30U	3.4 U	Y
2,4-D	9.26 <sup>-0.04</sup>	9.03 <sup>-0.03</sup>	9653	67011	0.454	1.309	1.0U	3.0U	11 U	Y

**Prep Amount:** 30.008 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 72.30

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010079.D Vial: 20  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 11:06 pm Operator: UA  
 Sample : K2010495-011 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:05:34 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.975	7.809	992574	3903125	54.547m	92.277 #
Target Compounds						
1) m Dalapon	3.132	2.875	6702	473036	0.276	9.791 #
3) m Dicamba	8.195	7.912	10722	59561	0.154	0.402 #
4) m MCPP	8.302	8.092	18774	68782	912.778	N.D. #
5) m MCPA	8.555	8.339	3328	73581	56.838	N.D. #
6) m Dichloroprop	8.949	8.745	14960	16575	0.802	0.397 #
7) m 2,4-D	9.262f	9.025	9653	67011	0.454	1.309 #
8) m 2,4,5-TP ...	10.239	10.109	5619	26663	0.060	0.131 #
9) m 2,4,5-T	10.732	10.522	7842	9848	0.095	0.051 #
10) m 2,4-DB	11.315	11.159	39310	17770	3.832	0.612 #
11) m Dinoseb	11.632	11.312	56150	24946	0.908	0.182 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010079.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 11:06 pm  
Sample : K2010495-011  
Misc :

Vial: 20  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:05:34 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010079.D Vial: 20  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 11:06 pm Operator: UA  
 Sample : K2010495-011 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:05:19 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.975min 56.173 ppb  
 response 1022153

Manual Integration:

Before

12/03/20



(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.809min 92.277 ppb  
 response 3903125

Data File : J:\gc24\data\120120\12010079.D Vial: 20  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 11:06 pm Operator: UA  
Sample : K2010495-011 Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:05:19 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.975min 54.547 ppb m  
response 992574

Manual Integration:

After  
Baseline/Shoulder  
12/03/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.809min 92.277 ppb  
response 3903125

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010080.D\  
**Lab ID:** K2010495-012  
**RunType:** N/A  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 23:29:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Preparation Hold Time	X	
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)	X	
Lab Control Sample Recovery	X	
Method Blank	X	
Method Blank Surrogates	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010080.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 23:29:00	<b>Vial:</b> 17
<b>Run Type:</b> N/A	<b>Dilution:</b> 1
<b>Lab ID:</b> K2010495-012	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-012.01	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> K2010495
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.82 <sup>+0.01</sup>	1075539	4098623	59.107	96.899	59	97	59	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.25 <sup>+0.01</sup>	10.09 <sup>-0.03</sup>	8041	48272	0.086	0.238 <sup>CCV</sup>	0.20U	0.54U	3.3 U	Y
2,4-D	9.27 <sup>-0.03</sup>	9.04 <sup>-0.02</sup>	4803	44224	0.226	0.864	0.51U	2.0U	11 U	Y

**Prep Amount:** 30.132 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 72.90

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010080.D Vial: 21  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 11:29 pm Operator: UA  
 Sample : K2010495-012 Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:05:49 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.982	7.815	1075539	4098623	59.107	96.899 #
Target Compounds						
1) m Dalapon	3.132	2.875	7186	280810	0.296	5.812 #
3) m Dicamba	8.192	7.915	2217	63260	0.032	0.427 #
4) m MCPP	8.308	8.102	18840	59804	914.198	N.D. #
5) m MCPA	8.582	8.345	4471	67785	76.359	N.D. #
6) m Dichloroprop	8.955	0.000	11778	0	0.632	N.D. #
7) m 2,4-D	9.272f	9.035	4803	44224	0.226	0.864 #
8) m 2,4,5-TP ...	10.252	10.088	8041	48272	0.086	0.238 #
9) m 2,4,5-T	10.688	10.532	3440	7647	0.042	0.040
10) m 2,4-DB	11.252	11.165	30637	21037	2.986	0.725 #
11) m Dinoseb	11.642	11.322	44076	27084	0.712	0.198 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data File : J:\gc24\data\120120\12010080.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 11:29 pm  
Sample : K2010495-012  
Misc :

Vial: 21  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00



Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:05:49 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st  12/02/20  
2nd  12/02/20

**Data File:** J:\gc24\data\120120\12010033.D\  
**Lab ID:** KQ2017965-04  
**RunType:** MB  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 05:33:00  
**Batch ID:** 705487  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery	X	
Continuing Calibration Recovery (Closing)	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *SM* 12/02/20  
2nd *SM* 12/02/20

<b>Data File:</b> J:\gc24\data\120120\12010033.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 05:33:00	<b>Vial:</b> 14
<b>Run Type:</b> MB	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2017965-04	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705487	<b>Prep Lot:</b> 369767	<b>Report Group:</b> KQ2017965
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.99	7.82	943432	3400160	51.847	80.386	52	80	52	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.26	10.14	7339	6264	0.078	0.031	0.13U	0.051U	2.4 U	Y
2,4-D	9.27 <sup>-0.05</sup>	9.04 <sup>-0.03</sup>	3075	28512	0.145	0.557	0.24U	0.92U	7.7 U	Y

**Prep Amount:** 30.2970 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/3/20 17:17

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

# Quantitation Report

1st 12/02/20  
2nd 12/02/20

<b>Data File:</b> J:\gc24\data\120120\12010033.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 05:33:00	<b>Vial:</b> 14
<b>Run Type:</b> MB	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2017965-04	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705487	<b>Prep Lot:</b> 369767	<b>Report Group:</b> KQ2017965
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 18726

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
2,4-Dichlorophenylacetic Acid	7.99	7.82	943432	3400160	51.847	80.386	52	80	52	26 - 127 P	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-T	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	4.0 U	Y
2,4,5-TP (Silvex)	10.26	10.14	7339	6264	0.078	0.031	0.13U	0.051U	2.4 U	Y
2,4-D	9.27 <sup>-0.05</sup>	9.04 <sup>-0.03</sup>	3075	28512	0.145	0.557	0.24U	0.92U	7.7 U	Y
2,4-DB	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	5.4 U	Y
Dalapon	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	5.5 U	Y
Dicamba	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	4.3 U	Y
Dichlorprop	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	3.4 U	Y
Dinoseb	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	2.7 U	Y
MCPA	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	320 U	Y
MCPP	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	460 U	Y

<b>Prep Amount:</b> 30.2970 g	<b>Dilution:</b> 1
<b>Prep Final Amount:</b> 50.00 mL	<b>Basis Factor:</b> 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/2/20 13:00

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010033.D Vial: 3  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 5:33 am Operator: UA  
 Sample : KQ2017965-04MB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 11:13:08 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.991	7.825	943432	3400160	51.847m	80.386 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.274f	9.041	3075	28512	0.145	0.557 #
8) m 2,4,5-TP ...	10.261	10.138	7339	6264	0.078	0.031m#
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010033.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:33 am  
Sample : KQ2017965-04MB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 11:13:08 2020  
Quant Results File: 102120\_8151.RES

Vial: 3  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010033.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:33 am Operator: UA  
Sample : KQ2017965-04MB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:01 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.991min 53.762 ppb  
response 978281

Manual Integration:

Before

12/02/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)



7.825min 80.386 ppb  
response 3400160

(+) = Expected Retention Time

Data File : J:\gc24\data\120120\12010033.D Vial: 3  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 5:33 am Operator: UA  
 Sample : KQ2017965-04MB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 10:38:01 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.991min 51.847 ppb m  
 response 943432

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.825min 80.386 ppb  
 response 3400160

Manual Integration:



After  
 Baseline/Shoulder  
 12/02/20



Data File : J:\gc24\data\120120\12010033.D Vial: 3  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 5:33 am Operator: UA  
 Sample : KQ2017965-04MB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 10:38:01 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
 10.261min 0.078 ppb  
 response 7339



Manual Integration:  
 Before  
 12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)  
 10.138min 0.065 ppb  
 response 13111

Data File : J:\gc24\data\120120\12010033.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:33 am Operator: UA  
Sample : KQ2017965-04MB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:01 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.261min 0.078 ppb  
response 7339

(8) 2,4,5-TP (Silvex) #2 (m)  
10.138min 0.031 ppb m  
response 6264

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

# Validation Report

1st *[Signature]* 12/02/20  
2nd *[Signature]* 12/02/20

**Data File:** J:\gc24\data\120120\12010034.D\  
**Lab ID:** KQ2017965-03  
**RunType:** LCS  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 05:56:00  
**Batch ID:** 705487  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery	X	
Continuing Calibration Recovery (Closing)	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *SM* 12/02/20  
2nd *SM* 12/02/20

<b>Data File:</b> J:\gc24\data\120120\12010034.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 05:56:00	<b>Vial:</b> 13
<b>Run Type:</b> LCS	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2017965-03	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705487	<b>Prep Lot:</b> 369767	<b>Report Group:</b> KQ2017965
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.99	7.82	1057229	3815475	58.100	90.205	58	90	58	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.26	10.14	4580215	13936403	48.892	68.653	81.5	114	81.5	Y
2,4-D	9.32	9.07	976047	3261310	45.953	63.699	76.6	106	76.6	Y

**Prep Amount:** 30.00 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

?: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/3/20 17:17

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

# Quantitation Report

1st 12/02/20  
2nd 12/02/20

<b>Data File:</b> J:\gc24\data\120120\12010034.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 05:56:00	<b>Vial:</b> 13
<b>Run Type:</b> LCS	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2017965-03	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705487	<b>Prep Lot:</b> 369767	<b>Report Group:</b> KQ2017965
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 18726

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
2,4-Dichlorophenylacetic Acid	7.99	7.82	1057229	3815475	58.100	90.205	58	90	58	26 - 127 P	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-T	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	4.0 U	Y
2,4,5-TP (Silvex)	10.26	10.14	4580215	13936403	48.892	68.653	81.5	114	<b>81.5</b>	Y
2,4-D	9.32	9.07	976047	3261310	45.953	63.699	76.6	106	<b>76.6</b>	Y
2,4-DB	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	5.4 U	Y
Dalapon	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	5.5 U	Y
Dicamba	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	4.3 U	Y
Dichlorprop	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	3.4 U	Y
Dinoseb	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	2.7 U	Y
MCPA	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	320 U	Y
MCPP	0.00	0.00	0	0	0.000 <sup>CCV</sup>	0.000 <sup>CCV</sup>	0U	0U	460 U	Y

**Prep Amount:** 30.00 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/2/20 13:00

\\alprews001\starlims\LIMSRpts\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010034.D Vial: 4  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 5:56 am Operator: UA  
 Sample : KQ2017965-03LCS Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 11:22:09 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.989	7.823	1057229	3815475	58.100m	90.205 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.316	9.066	976047	3261310	45.953m	63.699m#
8) m 2,4,5-TP ...	10.256	10.136	4580215	13936403	48.892	68.653 #
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010034.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:56 am  
Sample : KQ2017965-03LCS  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 11:22:09 2020  
Quant Results File: 102120\_8151.RES

Vial: 4  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010034.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:56 am Operator: UA  
Sample : KQ2017965-03LCS Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:04 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.989min 58.804 ppb  
response 1070027

Manual Integration:

Before

12/02/20

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.823min 90.205 ppb  
response 3815475



(+) = Expected Retention Time



Data File : J:\gc24\data\120120\12010034.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:56 am Operator: UA  
Sample : KQ2017965-03LCS Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:04 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(2) 2,4-Dichlorophenylacetic Acid (s)

7.989min 58.100 ppb m  
response 1057229

(2) 2,4-Dichlorophenylacetic Acid #2 (s)

7.823min 90.205 ppb  
response 3815475



Manual Integration:

After  
Baseline/Shoulder  
12/02/20

Data File : J:\gc24\data\120120\12010034.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:56 am Operator: UA  
Sample : KQ2017965-03LCS Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:04 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.316min 46.133 ppb  
response 979875



Manual Integration:  
Before  
12/02/20

(7) 2,4-D #2 (m)  
9.066min 64.594 ppb  
response 3307125

Data File : J:\gc24\data\120120\12010034.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:56 am Operator: UA  
Sample : KQ2017965-03LCS Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:04 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.316min 45.953 ppb m  
response 976047



Manual Integration:  
Before  
12/02/20

(7) 2,4-D #2 (m)  
9.066min 64.594 ppb  
response 3307125

Data File : J:\gc24\data\120120\12010034.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:56 am Operator: UA  
Sample : KQ2017965-03LCS Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:04 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.316min 45.953 ppb m  
response 976047



(7) 2,4-D #2 (m)  
9.066min 64.594 ppb  
response 3307125

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

Data File : J:\gc24\data\120120\12010034.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:56 am Operator: UA  
Sample : KQ2017965-03LCS Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:04 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.316min 45.953 ppb m  
response 976047

(7) 2,4-D #2 (m)  
9.066min 63.699 ppb m  
response 3261310

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010081.D\  
**Lab ID:** KQ2017965-01  
**RunType:** MS  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 23:52:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010081.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 23:52:00	<b>Vial:</b> 42
<b>Run Type:</b> MS	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2017965-01	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-011.02	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> KQ2017965
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	1140607	4370013	62.682	103.315	63	103	63	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.12	4889718	15153311	52.195	74.648 <sup>CCV</sup>	120	172	120	Y
2,4-D	9.30	9.05 <sup>-0.01</sup>	1026830	3530138	48.344	68.950	111	158	111	Y

**Prep Amount:** 30.092 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 72.30

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010081.D Vial: 22  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 11:52 pm Operator: UA  
 Sample : KQ2017965-01MS Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:06:04 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.976	7.809	1140607	4370013	62.682	103.315 #
Target Compounds						
1) m Dalapon	3.119	2.873	1125773	4261153	46.407	88.199 #
3) m Dicamba	8.196	7.913	4152865	12421076	59.497	83.806 #
4) m MCPP	8.279	8.099	317127	1718736	7333.088	10460.091 #
5) m MCPA	8.543	8.343	371387	2160652	6342.801	9540.765 #
6) m Dichloroprop	8.943	8.743	1015952	3317955	54.481	79.538 #
7) m 2,4-D	9.296	9.049	1026830	3530138	48.344	68.950 #
8) m 2,4,5-TP ...	10.236	10.119	4889718	15153311	52.195	74.648 #
9) m 2,4,5-T	10.679	10.523	3640625	11438761	44.124	59.774 #
10) m 2,4-DB	11.259	11.156	641045	1530736	62.484	52.755 #
11) m Dinoseb	11.656	11.303	2593832	7374401	41.926	53.923 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data File : J:\gc24\data\120120\12010081.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 11:52 pm  
Sample : KQ2017965-01MS  
Misc :

Vial: 22  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:06:04 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010082.D\  
**Lab ID:** KQ2017965-02  
**RunType:** DMS  
**Matrix:** Sediment

**Date Acquired:** 12/3/20 00:15:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
Analytical Hold Time	X	
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)	X	
Surrogates	X	
Std MRL Unsupported by ICAL	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010082.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/3/20 00:15:00	<b>Vial:</b> 43
<b>Run Type:</b> DMS	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2017965-02	<b>Raw Units:</b> ppb

<b>Bottle ID:</b> K2010495-011.02	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b> 369767	<b>Report Group:</b> KQ2017965
<b>Analysis:</b> 8151A	<b>Prep Method:</b> Method	
	<b>Prep Date:</b> 11/13/20	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.98	7.81	1097197	4151425	60.297	98.147	60	98	60	26 - 127	P Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.12	4596513	14157274	49.065	69.741 <sup>CCV</sup>	113	160	113	Y
2,4-D	9.30	9.05 <sup>-0.01</sup>	974411	3227012	45.876	63.029	106	145	106	Y

**Prep Amount:** 30.054 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 72.30

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010082.D Vial: 23  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 03 Dec 2020 12:15 am Operator: UA  
 Sample : KQ2017965-02DMS Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:06:24 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.979	7.809	1097197	4151425	60.297	98.147 #
Target Compounds						
1) m Dalapon	3.119	2.872	882176	3719587	36.366	76.990 #
3) m Dicamba	8.196	7.912	3909718	11728573	56.013	79.133 #
4) m MCPP	8.282	8.099	294515	1624091	6846.496	9805.963 #
5) m MCPA	8.546	8.346	343406	2037132	5864.922	8887.929 #
6) m Dichloroprop	8.946	8.746	960937	3105826	51.531	74.453 #
7) m 2,4-D	9.299	9.052	974411	3227012	45.876	63.029 #
8) m 2,4,5-TP ...	10.239	10.119	4596513	14157274	49.065	69.741 #
9) m 2,4,5-T	10.682	10.526	3452084	10649796	41.839	55.651 #
10) m 2,4-DB	11.262	11.156	613245	1418805	59.774	48.898 #
11) m Dinoseb	11.659	11.306	2449174	7245428	39.588	52.980 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010082.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 03 Dec 2020 12:15 am  
Sample : KQ2017965-02DMS  
Misc :

Vial: 23  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:06:24 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st *K* 12/02/20  
2nd *SM* 12/02/20

**Data File:** J:\gc24\data\120120\12010027.D\  
**Lab ID:** KQ2019138-02  
**RunType:** CCB  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 03:15:00  
**Batch ID:** 705487  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery (Closing)	X	
Surrogates	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st 12/02/20  
2nd 12/02/20

<b>Data File:</b> J:\gc24\data\120120\12010027.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 03:15:00	<b>Vial:</b> 2
<b>Run Type:</b> CCB	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019138-02	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/9/20	<b>Receive Date:</b> 11/11/20

<b>Analysis Lot:</b> 705487	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019138
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	8.00	7.83	7004	35037	0.385	0.828				26 - 127	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.26	10.14	4112	12361	0.044	0.061	0.073U	0.10U	2.4 U	Y
2,4-D	9.29	9.05	2676	92888	0.126	1.814	0.21U	3.0U	7.7 U	Y

**Prep Amount:** 30.00 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/3/20 17:17

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010027.D Vial: 2  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 3:15 am Operator: UA  
 Sample : ~~PENTA2-14N-100PB~~\* CCB Inst : HP G1530A  
 Misc : \*CCB - Vials switched on instrument Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 10:42:42 2020 \*ES 12/2/2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	8.005	7.835	7004	35037	0.385	0.828 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.291	9.048	2676	92888	0.126	1.814 #
8) m 2,4,5-TP ...	10.261	10.141	4112	12361	0.044m	0.061 #
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data File : J:\gc24\data\120120\12010027.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 3:15 am  
Sample : PENTA2-14N 100PB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:42:42 2020  
Quant Results File: 102120\_8151.RES

Vial: 2  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010027.D Vial: 2  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 3:15 am Operator: UA  
Sample : ~~PENTA2-14N-100PB~~ Vials switched on instrument. This is a CCB. Inst : HP G1530A  
Misc : ES 12/2/2020 Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:37:43 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(8) 2,4,5-TP (Silvex) (m)

10.261min 0.076 ppb

response 7088

Manual Integration:

Before

12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)



10.141min 0.061 ppb

response 12361

Data File : J:\gc24\data\120120\12010027.D Vial: 2  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 3:15 am Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:37:43 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(8) 2,4,5-TP (Silvex) (m)

10.261min 0.044 ppb m  
response 4112

Manual Integration:

After



Baseline

12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)

10.141min 0.061 ppb  
response 12361

# Validation Report

1st  12/02/20  
2nd  12/02/20

**Data File:** J:\gc24\data\120120\12010039.D\  
**Lab ID:** KQ2019199-02  
**RunType:** CCB  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 07:50:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)	X	
Surrogates	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - RTX-CLP2	2,4,5-TP	-100		20	
	2,4-D	-100		20	
	DCAA	-100		20	
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	-100		20	
	2,4-D	-98		20	
	DCAA	-99		20	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st 12/02/20  
2nd 12/02/20

<b>Data File:</b> J:\gc24\data\120120\12010039.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 07:50:00	<b>Vial:</b> 18
<b>Run Type:</b> CCB	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-02	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/9/20	<b>Receive Date:</b> 11/11/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

### Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	8.01	7.83	6551	43865	0.360	1.037				26 - 127	Y

### Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.26	10.14	1911	5968	0.020	0.029	0.033U	0.048U	2.4 U	Y
2,4-D	9.36	9.04	1024	106038	0.048	2.071	0.080U	3.5U	7.7 U	Y

<b>Prep Amount:</b> 30.00 g	<b>Dilution:</b> 1
<b>Prep Final Amount:</b> 50.00 mL	<b>Basis Factor:</b> 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010039.D Vial: 2  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 7:50 am Operator: UA  
 Sample : ~~PENTA2-14N-100PB~~ \* .CCB Inst : HP G1530A  
 Misc : \*CCB - Vials switched on instrument Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P \*ES 12/2/2020  
 Quant Time: Dec 02 11:52:17 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	8.006	7.833	6551	43865	0.360	1.037 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.359	9.043	1024	106038	0.048	2.071 #
8) m 2,4,5-TP ...	10.263	10.139	1911	5968	0.020m	0.029 #
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010039.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:50 am  
Sample : PENTA2-14N 100PB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 11:52:17 2020  
Quant Results File: 102120\_8151.RES

Vial: 2  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010039.D Vial: 2  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:50 am Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:19 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.263min 0.245 ppb  
response 22907

Manual Integration:  
Before  
12/02/20



(8) 2,4,5-TP (Silvex) #2 (m)  
10.139min 0.029 ppb  
response 5968



Data File : J:\gc24\data\120120\12010039.D Vial: 2  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 7:50 am Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:19 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.263min 0.020 ppb m  
response 1911

(8) 2,4,5-TP (Silvex) #2 (m)  
10.139min 0.029 ppb  
response 5968

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010052.D\  
**Lab ID:** KQ2019199-04  
**RunType:** CCB  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 12:48:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery	X	
Continuing Calibration Recovery (Closing)		X
Surrogates	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010052.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 12:48:00	<b>Vial:</b> 20
<b>Run Type:</b> CCB	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-04	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/9/20	<b>Receive Date:</b> 11/11/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	8.00 <sup>+0.02</sup>	7.83 <sup>+0.01</sup>	6897	43968	0.379	1.039				26 - 127	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.25	10.13	5267	21690	0.056	0.107 <sup>CCV</sup>	0.093U	0.18U	2.4 U	Y
2,4-D	0.00	9.03 <sup>-0.03</sup>	0	123808	0.000	2.418	0U	4.0U	7.7 U	Y

**Prep Amount:** 30.00 g                      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL              **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010052.D Vial: 2  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 12:48 pm Operator: UA  
 Sample : IB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 16:55:42 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.997	7.827	6897	43968	0.379	1.039 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	0.000	9.034	0	123808	N.D. d	2.418
8) m 2,4,5-TP ...	10.250	10.130	5267	21690	0.056m	0.107 #
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010052.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 12:48 pm  
Sample : IB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 16:55:42 2020  
Quant Results File: 102120\_8151.RES

Vial: 2  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010052.D Vial: 2  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 12:48 pm Operator: UA  
Sample : IB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 16:54:10 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.250min 0.088 ppb  
response 8214



Manual Integration:  
Before  
12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)  
10.130min 0.107 ppb  
response 21690

Data File : J:\gc24\data\120120\12010052.D Vial: 2  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 12:48 pm Operator: UA  
Sample : IB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 16:54:10 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.250min 0.056 ppb m  
response 5267

(8) 2,4,5-TP (Silvex) #2 (m)  
10.130min 0.107 ppb  
response 21690

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010064.D\  
**Lab ID:** KQ2019199-06  
**RunType:** CCB  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 17:23:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)		X
Surrogates	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	21		20	CCV+ND
Continuing Calibration Recovery (Closing) - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_



# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010064.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 17:23:00	<b>Vial:</b> 22
<b>Run Type:</b> CCB	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-06	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/9/20	<b>Receive Date:</b> 11/11/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.99 <sup>+0.01</sup>	7.82 <sup>+0.01</sup>	8625	44840	0.474	1.060				26 - 127	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.24	10.12	6151	18001	0.066	0.089 <sup>CCV</sup>	0.11U	0.15U	2.4 U	Y
2,4-D	9.34 <sup>+0.04</sup>	9.03 <sup>-0.02</sup>	1150	138579	0.054	2.707	0.090U	4.5U	7.7 U	Y

**Prep Amount:** 30.00 g                      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL           **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Data File : J:\gc24\data\120120\12010064.D Vial: 2  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 5:23 pm Operator: UA  
 Sample : IB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 18:47:06 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.991	7.821	8625	44840	0.474	1.060 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.338	9.031	1150	138579	0.054	2.707 #
8) m 2,4,5-TP ...	10.244	10.124	6151	18001	0.066m	0.089 #
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010064.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:23 pm  
Sample : IB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:47:06 2020  
Quant Results File: 102120\_8151.RES

Vial: 2  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010064.D Vial: 2  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:23 pm Operator: UA  
Sample : IB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:46:03 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.244min 0.142 ppb  
response 13271



Manual Integration:  
Before  
12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)  
10.124min 0.089 ppb  
response 18001

Data File : J:\gc24\data\120120\12010064.D Vial: 2  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:23 pm Operator: UA  
Sample : IB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:46:03 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.244min 0.066 ppb m  
response 6151

(8) 2,4,5-TP (Silvex) #2 (m)  
10.124min 0.089 ppb  
response 18001

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010076.D\  
**Lab ID:** KQ2019199-08  
**RunType:** CCB  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 21:57:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery		X
Continuing Calibration Recovery (Closing)	X	
Surrogates	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

## Analyte Exceptions

Exception Categories	Analyte Name	Result	Low Limit	High Limit	Corrective Action
Continuing Calibration Recovery - ZB-XLB-HT	2,4,5-TP	22		20	CCV+ND

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010076.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 21:57:00	<b>Vial:</b> 12
<b>Run Type:</b> CCB	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-08	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	7.99 <sup>+0.01</sup>	7.82 <sup>+0.01</sup>	7460	44251	0.410	1.046				26 - 127	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.25 <sup>+0.01</sup>	10.12	13344	27831	0.142	0.137 <sup>CCV</sup>	0.24U	0.23U	2.4 U	Y
2,4-D	9.35 <sup>+0.05</sup>	9.03 <sup>-0.03</sup>	1188	143038	0.056	2.794	0.093U	4.7U	7.7 U	Y

**Prep Amount:** 30.00 g                      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL           **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010076.D Vial: 2  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 9:57 pm Operator: UA  
 Sample : IB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:04:17 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.993	7.823	7460	44251	0.410	1.046 #
Target Compounds						
1) m Dalapon	0.000	2.900f	0	87471	N.D. d	1.811
3) m Dicamba	8.203	7.917	7098	12287	0.102	0.083
4) m MCPP	0.000	8.113	0	9202	N.D.	N.D.
5) m MCPA	8.517f	8.360	22654	14064	386.900	N.D. #
6) m Dichloroprop	8.957	8.747	2928	4843	0.157	0.116 #
7) m 2,4-D	9.350	9.030	1188	143038	0.056	2.794 #
8) m 2,4,5-TP ...	10.247	10.123	13344	27831	0.142	0.137
9) m 2,4,5-T	10.693	10.537	4145	29505	0.050	0.154 #
10) m 2,4-DB	11.327	11.197	22847	20502	2.227	0.707 #
11) m Dinoseb	11.663	11.310	13204	31351	0.213	0.229
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data File : J:\gc24\data\120120\12010076.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 9:57 pm  
Sample : IB  
Misc :

Vial: 2  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:04:17 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010084.D\  
**Lab ID:** KQ2019199-10  
**RunType:** CCB  
**Matrix:** Sediment

**Date Acquired:** 12/3/20 01:00:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Continuing Calibration Recovery	X	
Surrogates	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010084.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/3/20 01:00:00	<b>Vial:</b> 14
<b>Run Type:</b> CCB	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-10	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	% Rec	% Rec Criteria	Rpt?
DCAA	8.00 <sup>+0.02</sup>	7.83 <sup>+0.02</sup>	7914	59829	0.435	1.414				26 - 127	Y

## Target Compounds

Final Conc.Units: ug/Kg

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Primary Conc	Rpt?
2,4,5-TP	10.26 <sup>+0.02</sup>	10.14 <sup>+0.02</sup>	12022	25632	0.128	0.126	0.21U	0.21U	2.4 U	Y
2,4-D	9.35 <sup>+0.05</sup>	9.04 <sup>-0.01</sup>	1164	149145	0.055	2.913	0.092U	4.9U	7.7 U	Y

**Prep Amount:** 30.00 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010084.D Vial: 2  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 03 Dec 2020 1:00 am Operator: UA  
 Sample : IB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:07:06 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	8.002	7.832	7914	59829	0.435	1.414 #
Target Compounds						
1) m Dalapon	0.000	2.902f	0	81563	N.D. d	1.688
3) m Dicamba	8.209	7.926	9502	16724	0.136	0.113
4) m MCPP	0.000	8.122	0	13253	N.D.	N.D.
5) m MCPA	8.525	8.372	7880	12794	134.580	N.D. #
6) m Dichloroprop	8.962	8.759	5986	11792	0.321	0.283
7) m 2,4-D	9.345	9.042	1164	149145	0.055	2.913 #
8) m 2,4,5-TP ...	10.259	10.139	12022	25632	0.128	0.126
9) m 2,4,5-T	10.709	10.556	11437	29648	0.139	0.155
10) m 2,4-DB	11.269	11.122	29616	13780	2.887	0.475 #
11) m Dinoseb	11.679	11.329	14215	33551	0.230	0.245
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010084.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 03 Dec 2020 1:00 am  
Sample : IB  
Misc :

Vial: 2  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00



Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:07:06 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st  12/02/20  
2nd  12/02/20

**Data File:** J:\gc24\data\120120\12010028.D\  
**Lab ID:** KQ2019138-01  
**RunType:** CCV  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 03:38:00  
**Batch ID:** 705487  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *SM* 12/02/20  
2nd *SM* 12/02/20

<b>Data File:</b> J:\gc24\data\120120\12010028.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 03:38:00	<b>Vial:</b> 1
<b>Run Type:</b> CCV	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019138-01	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/9/20	<b>Receive Date:</b> 11/11/20

<b>Analysis Lot:</b> 705487	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019138
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	Rpt?
DCAA	7.99	7.82	1559806	4715157	85.720	111.475			Y

## Target Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Rpt?
2,4,5-TP	10.26	10.14	7620185	22453949	81.342	110.612	81.3	111	Y
2,4-D	9.32	9.07	1599713	5076286	75.316	99.149	75.3	99.1	Y

**Prep Amount:** 30.00 g                      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL              **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/3/20 17:17

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010028.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 3:38 am Operator: UA  
 Sample : ~~IB~~\*PENTA2-14N 100 ppb Inst : HP G1530A  
 Misc : \*CCV - Vials switched on instrument Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P \*ES 12/2/2020  
 Quant Time: Dec 02 10:47:58 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.991	7.824	1559806	4715157	85.720	111.475 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.318	9.068	1599713	5076286	75.316	99.149 #
8) m 2,4,5-TP ...	10.258	10.138	7620185	22453949	81.342	110.612 #
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data File : J:\gc24\data\120120\12010028.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 3:38 am  
Sample : IB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:47:58 2020  
Quant Results File: 102120\_8151.RES



Vial: 1  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st  12/02/20  
2nd  12/02/20

**Data File:** J:\gc24\data\120120\12010040.D\  
**Lab ID:** KQ2019199-01  
**RunType:** CCV  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 08:13:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *SM* 12/02/20  
2nd *SM* 12/02/20

<b>Data File:</b> J:\gc24\data\120120\12010040.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 08:13:00	<b>Vial:</b> 1
<b>Run Type:</b> CCV	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-01	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/9/20	<b>Receive Date:</b> 11/11/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution		% Rec		Rpt?
					Conc 1	Conc 2	1	2	
DCAA	7.99	7.82	1552751	4828815	85.332	114.162			Y

## Target Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution		Final		Rpt?
					Conc 1	Conc 2	Conc 1	Conc 2	
2,4,5-TP	10.26	10.14	7637950	23040649	81.531	113.502	81.5	114	Y
2,4-D	9.32	9.07	1610845	5182812	75.840	101.230	75.8	101	Y

**Prep Amount:** 30.00 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010040.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 8:13 am Operator: UA  
 Sample : ~~TS~~ \*PENTA2-14N 100 ppb Inst : HP G1530A  
 Misc : \*CCV - Vials switched on instrument Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P \*ES 12/2/2020  
 Quant Time: Dec 02 11:56:14 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.988	7.822	1552751	4828815	85.332	114.162 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.315	9.065	1610845	5182812	75.840	101.230 #
8) m 2,4,5-TP ...	10.255	10.139	7637950	23040649	81.531m	113.502m#
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010040.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:13 am  
Sample : IB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 11:56:14 2020  
Quant Results File: 102120\_8151.RES

Vial: 1  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M


Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010040.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 8:13 am Operator: UA  
Sample : IB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 10:38:22 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)

10.255min 81.602 ppb

response 7644614

Manual Integration:

Before

12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)

10.139min 113.419 ppb



response 23023903

(+) = Expected Retention Time

Data File : J:\gc24\data\120120\12010040.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 8:13 am Operator: UA  
 Sample : IB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 10:38:22 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(8) 2,4,5-TP (Silvex) (m)  
 10.255min 81.531 ppb m  
 response 7637950

Manual Integration:  
 After  
 Baseline/Shoulder  
 12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)  
 10.139min 113.502 ppb m  
 response 23040649

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010051.D\  
**Lab ID:** KQ2019199-03  
**RunType:** CCV  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 12:25:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_



# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010051.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 12:25:00	<b>Vial:</b> 19
<b>Run Type:</b> CCV	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-03	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/9/20	<b>Receive Date:</b> 11/11/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution		% Rec		Rpt?
					Conc 1	Conc 2	1	2	
DCAA	7.98	7.82	1557669	4762359	85.602	112.591			Y

## Target Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution		Final		Rpt?
					Conc 1	Conc 2	Conc 1	Conc 2	
2,4,5-TP	10.25	10.13	7646510	22854297	81.623	112.584	81.6	113	Y
2,4-D	9.31	9.06	1600985	5136864	75.375	100.332	75.4	100	Y

**Prep Amount:** 30.00 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010051.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 12:25 pm Operator: UA  
 Sample : PENTA2-14N 100PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 14:42:54 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.984	7.817	1557669	4762359	85.602	112.591 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.310	9.061	1600985	5136864	75.375m	100.332 #
8) m 2,4,5-TP ...	10.250	10.131	7646510	22854297	81.623	112.584m#
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010051.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 12:25 pm  
Sample : PENTA2-14N 100PB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 14:42:54 2020  
Quant Results File: 102120\_8151.RES

Vial: 1  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2  
Signal #1 Info : 0.25 mm  
Signal #2 Phase: ZB-XLB-HT  
Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010051.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 12:25 pm Operator: UA  
 Sample : PENTA2-14N 100PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 14:32:38 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(7) 2,4-D (m)

9.310min 75.942 ppb

response 1613017

(7) 2,4-D #2 (m)

9.061min 100.332 ppb

response 5136864

Manual Integration:



Before

12/02/20

Data File : J:\gc24\data\120120\12010051.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 12:25 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 14:32:38 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.310min 75.375 ppb m  
response 1600985



(7) 2,4-D #2 (m)  
9.061min 100.332 ppb  
response 5136864

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

Data File : J:\gc24\data\120120\12010051.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 12:25 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 14:35:48 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)

10.250min 81.623 ppb

response 7646510

Manual Integration:

Before

12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)

10.131min 112.359 ppb



response 22808601

(+) = Expected Retention Time

Data File : J:\gc24\data\120120\12010051.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 12:25 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 14:35:48 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.250min 81.623 ppb  
response 7646510

(8) 2,4,5-TP (Silvex) #2 (m)  
10.131min 112.584 ppb m  
response 22854297

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010063.D\  
**Lab ID:** KQ2019199-05  
**RunType:** CCV  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 17:00:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_



# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010063.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 17:00:00	<b>Vial:</b> 21
<b>Run Type:</b> CCV	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-05	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/9/20	<b>Receive Date:</b> 11/11/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	Rpt?
DCAA	7.98	7.81	1546512	4914240	84.989	116.182			Y

## Target Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Rpt?
2,4,5-TP	10.24	10.12	7618798	23356475	81.327	115.058	81.3	115	Y
2,4-D	9.30	9.05	1594933	5237602	75.091	102.300	75.1	102	Y

**Prep Amount:** 30.00 g      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL      **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010063.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 5:00 pm Operator: UA  
 Sample : PENTA2-14N 100PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 18:23:48 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.978	7.811	1546512	4914240	84.989	116.182 #
Target Compounds						
1) m Dalapon	0.000	0.000	0	0	N.D. d	N.D. d
3) m Dicamba	0.000	0.000	0	0	N.D. d	N.D. d
4) m MCPP	0.000	0.000	0	0	N.D. d	N.D. d
5) m MCPA	0.000	0.000	0	0	N.D. d	N.D. d
6) m Dichloroprop	0.000	0.000	0	0	N.D. d	N.D. d
7) m 2,4-D	9.301	9.051	1594933	5237602	75.091m	102.300m#
8) m 2,4,5-TP ...	10.241	10.121	7618798	23356475	81.327m	115.058m#
9) m 2,4,5-T	0.000	0.000	0	0	N.D. d	N.D. d
10) m 2,4-DB	0.000	0.000	0	0	N.D. d	N.D. d
11) m Dinoseb	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010063.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 5:00 pm  
 Sample : PENTA2-14N 100PB  
 Misc :  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 18:23:48 2020  
 Quant Results File: 102120\_8151.RES

Vial: 1  
 Operator: UA  
 Inst : HP G1530A  
 Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\120120\12010063.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:00 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:19:12 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.301min 75.927 ppb  
response 1612690



Manual Integration:  
Before  
12/02/20

(7) 2,4-D #2 (m)  
9.051min 103.015 ppb  
response 5274224

Data File : J:\gc24\data\120120\12010063.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:00 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:19:12 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.301min 75.091 ppb m  
response 1594933



Manual Integration:  
Before  
12/02/20

(7) 2,4-D #2 (m)  
9.051min 103.015 ppb  
response 5274224

Data File : J:\gc24\data\120120\12010063.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:00 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:19:12 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.301min 75.091 ppb m  
response 1594933



Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

(7) 2,4-D #2 (m)  
9.051min 103.015 ppb  
response 5274224

Data File : J:\gc24\data\120120\12010063.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:00 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:19:12 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(7) 2,4-D (m)  
9.301min 75.091 ppb m  
response 1594933



(7) 2,4-D #2 (m)  
9.051min 102.300 ppb m  
response 5237602

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20

Data File : J:\gc24\data\120120\12010063.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:00 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:19:12 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.241min 81.507 ppb  
response 7635681

Manual Integration:  
Before  
12/02/20



(8) 2,4,5-TP (Silvex) #2 (m)  
10.121min 115.304 ppb  
response 23406509



Data File : J:\gc24\data\120120\12010063.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:00 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:19:12 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.241min 81.327 ppb m  
response 7618798



Manual Integration:  
Before  
12/02/20

(8) 2,4,5-TP (Silvex) #2 (m)  
10.121min 115.304 ppb  
response 23406509

Data File : J:\gc24\data\120120\12010063.D Vial: 1  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 5:00 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 02 18:19:12 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.241min 81.327 ppb m  
response 7618798

Manual Integration:  
After  
Baseline/Shoulder  
12/02/20



(8) 2,4,5-TP (Silvex) #2 (m)  
10.121min 115.304 ppb  
response 23406509

(+) = Expected Retention Time

Data File : J:\gc24\data\120120\12010063.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 5:00 pm Operator: UA  
 Sample : PENTA2-14N 100PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 02 18:21:20 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
 10.241min 81.327 ppb m  
 response 7618798

(8) 2,4,5-TP (Silvex) #2 (m)  
 10.121min 115.058 ppb m  
 response 23356475

Manual Integration:  
 After  
 Baseline/Shoulder  
 12/02/20

# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010075.D\  
**Lab ID:** KQ2019199-07  
**RunType:** CCV  
**Matrix:** Sediment

**Date Acquired:** 12/2/20 21:34:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_

# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010075.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/2/20 21:34:00	<b>Vial:</b> 11
<b>Run Type:</b> CCV	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-07	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	% Rec 1	% Rec 2	Rpt?
DCAA	7.98	7.81	1602226	4917376	88.051	116.256			Y

## Target Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution Conc 1	Solution Conc 2	Final Conc 1	Final Conc 2	Rpt?
2,4,5-TP	10.24	10.12	7704495	23461532	82.242	115.575	82.2	116	Y
2,4-D	9.30	9.06	1607321	5295769	75.674	103.436	75.7	103	Y

**Prep Amount:** 30.00 g                      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL              **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010075.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Dec 2020 9:34 pm Operator: UA  
 Sample : PENTA2-14N 100PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 09:31:12 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.980	7.814	1602226	4917376	88.051	116.256 #
Target Compounds						
1) m Dalapon	3.120	2.874	2271995	5640287	93.658	116.745
3) m Dicamba	8.200	7.917	6210167	18077877	88.971	121.972 #
4) m MCPP	8.284	8.104	417935	2229538	9502.392	13990.439 #
5) m MCPA	8.547	8.350	546014	2864305	9325.200	13259.761 #
6) m Dichloroprop	8.950	8.750	1581712	5018830	84.820	120.312 #
7) m 2,4-D	9.304	9.057	1607321	5295769	75.674	103.436 #
8) m 2,4,5-TP ...	10.244	10.124	7704495	23461532	82.242	115.575 #
9) m 2,4,5-T	10.687	10.527	5736895	16711670	69.530	87.328 #
10) m 2,4-DB	11.267	11.160	678246	2423097	66.110	83.509 #
11) m Dinoseb	11.664	11.310	4839569	14287752	78.226	104.476 #
-----						



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\120120\12010075.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Dec 2020 9:34 pm  
Sample : PENTA2-14N 100PB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 09:31:12 2020  
Quant Results File: 102120\_8151.RES

Vial: 1  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Validation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

**Data File:** J:\gc24\data\120120\12010083.D\  
**Lab ID:** KQ2019199-09  
**RunType:** CCV  
**Matrix:** Sediment

**Date Acquired:** 12/3/20 00:38:00  
**Batch ID:** 705654  
**Analysis Method:** 8151A/HERB

## Validations

Validation Categories	Pass	Fail
ICAL Analyte Recovery	X	
Second Source ICAL Verification	X	
Above Highest ICAL Level	X	
Analyte Coelutions	X	

Primary Review: \_\_\_\_\_

Secondary Review: \_\_\_\_\_



# Quantitation Report

1st *UA* 12/03/20  
2nd *SW* 12/03/20

<b>Data File:</b> J:\gc24\data\120120\12010083.D\	<b>Instrument:</b> K-GC-24
<b>Acqu Date:</b> 12/3/20 00:38:00	<b>Vial:</b> 13
<b>Run Type:</b> CCV	<b>Dilution:</b> 1
<b>Lab ID:</b> KQ2019199-09	<b>Raw Units:</b> ppb

<b>Bottle ID:</b>	<b>Tier:</b> IV	<b>Matrix:</b> Sediment
<b>Prod Code:</b> HERB	<b>Collect Date:</b> 11/10/20	<b>Receive Date:</b> 11/12/20

<b>Analysis Lot:</b> 705654	<b>Prep Lot:</b>	<b>Report Group:</b> KQ2019199
<b>Analysis:</b> 8151A	<b>Prep Method:</b>	
	<b>Prep Date:</b>	

<b>Title:</b> Chlorinated Herbicides by GC	<b>Calibration ID:</b> KC2000566
	<b>Report List ID:</b> 11736

## Surrogate Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution		% Rec		Rpt?
					Conc 1	Conc 2	1	2	
DCAA	7.98	7.81	1598105	4868528	87.824	115.101			Y

## Target Compounds

Parameter Name	RT 1	RT 2	Resp 1	Resp 2	Solution		Final		Rpt?
					Conc 1	Conc 2	Conc 1	Conc 2	
2,4,5-TP	10.24	10.12	7666893	23116522	81.840	113.876	81.8	114	Y
2,4-D	9.30	9.05	1603460	5256225	75.492	102.663	75.5	103	Y

**Prep Amount:** 30.00 g                      **Dilution:** 1  
**Prep Final Amount:** 50.00 mL              **Basis Factor:** 100.00

U: Undetected at or above MDL  
J: Analyte detected above MDL, but below MRL  
B: Hit above MRL also found in Method Blank  
E: Analyte concentration above high point of ICAL  
N: Presumptive evidence of compound

D: Result from dilution  
m: Manual integration performed  
d: Compound manually deleted  
NR: Analyte not reported from this analysis

\*: Result fails acceptance criteria  
#: Acceptance criteria not applicable  
?: Insufficient information to determine acceptance  
e: Result >= MRL, but MRL less than low point of ICAL  
c: check for co-elution

Printed: 12/4/20 17:20

\\alprews001\starlims\LIMSReps\QuantValidation.rpt

Data File : J:\gc24\data\120120\12010083.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 03 Dec 2020 12:38 am Operator: UA  
 Sample : PENTA2-14N 100PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Dec 03 10:06:42 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.976	7.813	1598105	4868528	87.824	115.101 #
Target Compounds						
1) m Dalapon	3.119	2.873	2254853	5626305	92.951	116.456 #
3) m Dicamba	8.199	7.913	6177811	17962272	88.507	121.192 #
4) m MCPP	8.282	8.099	417260	2234275	9487.867	14023.178 #
5) m MCPA	8.546	8.349	541456	2893281	9247.355	13412.907 #
6) m Dichloroprop	8.946	8.746	1578935	5020393	84.671	120.350 #
7) m 2,4-D	9.302	9.053	1603460	5256225	75.492	102.663 #
8) m 2,4,5-TP ...	10.239	10.123	7666893	23116522	81.840	113.876 #
9) m 2,4,5-T	10.686	10.526	5637749	16466101	68.328	86.045 #
10) m 2,4-DB	11.266	11.159	677109	2391066	65.999	82.406 #
11) m Dinoseb	11.659	11.306	4805669	14088958	77.678	103.022 #
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\120120\12010083.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 03 Dec 2020 12:38 am  
Sample : PENTA2-14N 100PB  
Misc :

Vial: 1  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Dec 03 10:06:42 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



# Injection Log

Directory: J:\gc24\data\102120

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	100	10210001.d	1.	CCV PRIMER		21 Oct 2020 12:34
2	100	10210002.d	1.	CCV PRIMER		21 Oct 2020 12:58
3	1	10210003.d	1.	IB		Unrecognized:Un
4	3	10210004.d	1.	PENTA2-14K 10PPB		Unrecognized:Un
5	4	10210005.d	1.	PENTA2-14L 25PPB		Unrecognized:Un
6	5	10210006.d	1.	PENTA2-14M 75PPB		Unrecognized:Un
7	6	10210007.d	1.	PENTA2-14N 100PB		Unrecognized:Un
8	7	10210008.d	1.	PENTA2-15A 125PB		Unrecognized:Un
9	8	10210009.d	1.	PENTA2-15B 150PB		Unrecognized:Un
10	9	10210010.d	1.	PENTA2-15C 175PB		Unrecognized:Un
11	10	10210011.d	1.	PENTA2-15D 200PB		Unrecognized:Un
12	11	10210012.d	1.	PENTA2-15E ICV 100 PPB		Unrecognized:Un

*ICAL: Kc2000566*

ALS-Kelso  
Initial Calibration Checklist GC

Method: 8151A Herb  
ICAL ID or Date: KC2000566  
Instrument: GC-24

Primary Secondary

- The new ICAL is saved with a unique ID.
- ICAL was performed continuously (i.e. not interrupted by maintenance event).
- All analytes in blank are  $< \frac{1}{2}$  MRL.
- ICAL contains minimum number of concentrations.
- No internal levels excluded for any analytes.
- Retention times updated using a midpoint of the calibration. Secondary reviewer double check peak IDs.
- Calibration files quantitated with new method.
- Check integrations. Primary reviewer must check all integrations electronically. Secondary reviewer will check low point and high point electronically.
- ICAL files added to calibration table.
- The average RF or COD meets method criteria for all analytes.
- ICV is quantitated against new ICAL.
- ICV meets method criteria.
- Linked in <sup>LIMS</sup>Stealth to an appropriate method. An appropriate method will be one that contains all analytes that were analyzed.
- All calibration reports included: ICAL SUMMARY, ICAL DETAILED, ICV SUMMARY.
- Enviroquant/Target responses match those in <sup>LIMS</sup>Stealth.
- All quant reports and manual integrations initialed and dated.

Data packet should be in the following order: Sequence log, Calibration Review, Stealth ICAL reports, and quant reports.

Primary: [Signature]

Date: 10-21-20

Secondary: [Signature]

Date: 10/22/20

Method Path : J:\gc24\Methods\  
 Method File : 102120\_8151.M  
 Title : 103118\_8151.m MJ215 CAL\_KC1800  
 Last Update : Wed Oct 21 17:31:59 2020  
 Response Via : Initial Calibration

Calibration Files

1 =10210004.D 2 =10210005.D =  
 4 =10210006.D 5 =10210007.D 6 =10210008.D

Compound	1	2	4	5	6	Avg	%RSD
1) m Dalapon	2.671	2.733	2.254	2.374	2.344	2.385	2.426 E4 7.29
2) s 2,4-Dichlorop...	2.115	2.015	1.798	1.794	1.738	1.732	1.820 E4 8.79
3) m Dicamba	7.596	7.540	6.777	6.892	6.778	6.830	6.980 E4 5.27
4) m MCPP	2.001	3.740	4.291	4.480	4.454	4.501	4.053 E1 21.41
5) m MCPA	4.567	6.110	6.022	6.133	6.030	6.046	5.855 E1 8.95
6) m Dichloroprop	2.275	2.117	1.795	1.815	1.755	1.752	1.865 E4 11.40
7) m 2,4-D	2.488	2.377	2.075	2.056	2.029	2.025	2.124 E4 9.25
8) m 2,4,5-TP (Sil...	9.752	9.790	9.082	9.310	9.221	9.360	9.368 E4 2.80
9) m 2,4,5-T	8.692	8.723	8.157	8.121	8.142	8.264	8.251 E4 3.64
10) m 2,4-DB	1.110	1.172	1.003	0.994	1.001	1.003	1.026 E4 7.40
11) m Dinoseb	6.933	6.670	6.137	6.031	5.965	6.030	6.187 E4 6.41


Signal #2 Calibration Files

1 =10210004.D 2 =10210005.D =  
 4 =10210006.D 5 =10210007.D 6 =10210008.D

Compound	1	2	4	5	6	Avg	%RSD
1) m Dalapon	5.105	5.207	4.698	4.631	4.838	4.664	4.831 E4 4.39
2) s 2,4-Dichlorop...	5.587	4.943	4.041	3.953	3.892	3.822	4.230 E4 15.77
3) m Dicamba	1.724	1.593	1.424	1.430	1.425	1.416	1.482 E5 7.71
4) m MCPP	3.248	2.629	1.847	1.727	1.645	1.574	1.963 E2 32.32
5) m MCPA	5.322	3.724	2.492	2.323	2.218	2.130	2.789 E2 41.64
6) m Dichloroprop	5.440	4.793	3.993	3.939	3.868	3.809	4.172 E4 14.71
7) m 2,4-D	6.995	5.929	4.845	4.767	4.681	4.616	5.120 E4 17.22
8) m 2,4,5-TP (Sil...	2.358	2.178	1.953	1.956	1.949	1.947	2.030 E5 7.62
9) m 2,4,5-T	2.241	2.074	1.833	1.848	1.821	1.835	1.914 E5 8.20
10) m 2,4-DB	3.572	3.225	2.779	2.756	2.726	2.732	2.902 E4 11.07
11) m Dinoseb	1.678	1.515	1.309	1.301	1.294	1.286	1.368 E5 10.83


(#) = Out of Range ### Number of calibration levels exceeded format ###

102120\_8151.M Wed Oct 21 17:48:58 2020









## Initial Calibration - Detailed Report

Calibration ID: KC2000566

Instrument ID: K-GC-24

Column Name: RTX-CLP2

#	Lab Code	Sample Name	File Location	Aquisition Date
01	KC2000566-01	PENTA2-14K 10PPB	J:\gc24\data\102120\10210004.D	10/21/2020 13:46
02	KC2000566-02	PENTA2-14L 25PPB	J:\gc24\data\102120\10210005.D	10/21/2020 14:09
03	KC2000566-03	PENTA2-14M 75PPB	J:\gc24\data\102120\10210006.D	10/21/2020 14:33
04	KC2000566-04	PENTA2-14N 100PB	J:\gc24\data\102120\10210007.D	10/21/2020 14:57
05	KC2000566-05	PENTA2-15A 125PB	J:\gc24\data\102120\10210008.D	10/21/2020 15:21
06	KC2000566-06	PENTA2-15B 150PB	J:\gc24\data\102120\10210009.D	10/21/2020 15:44
07	KC2000566-07	PENTA2-15C 175PB	J:\gc24\data\102120\10210010.D	10/21/2020 16:08
08	KC2000566-08	PENTA2-15D 200PB	J:\gc24\data\102120\10210011.D	10/21/2020 16:32

Analyte			Curve Fit			Weighting					
<b>2,4,5-T</b>			Average RF			RSD = 3.638			Average RF = 8.251E4		
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.480	8.692E4	02	23.700	8.723E4	03	71.100	8.157E4	04	94.800	8.121E4
05	118.490	8.142E4	06	142.190	8.264E4	07	165.890	7.962E4	08	189.590	7.946E4
<b>2,4,5-TP</b>			Average RF			RSD = 2.798			Average RF = 9.368E4		
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.510	9.752E4	02	23.760	9.79E4	03	71.300	9.082E4	04	95.100	9.31E4
05	118.820	9.221E4	06	142.580	9.36E4	07	166.340	9.245E4	08	190.100	9.185E4
<b>2,4-D</b>			Average RF			RSD = 9.253			Average RF = 2.124E4		
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.400	2.488E4	02	23.510	2.377E4	03	70.500	2.075E4	04	94.000	2.056E4
05	117.540	2.029E4	06	141.050	2.025E4	07	164.560	1.991E4	08	188.060	1.951E4
<b>2,4-DB</b>			Average RF			RSD = 7.4			Average RF = 1.026E4		
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.470	1.11E4	02	23.670	1.172E4	03	71.000	1.003E4	04	94.700	9.938E3
05	118.330	1.001E4	06	142.000	1.003E4	07	165.670	9.847E3	08	189.340	9.399E3
<b>Dalapon</b>			Average RF			RSD = 7.292			Average RF = 2.426E4		
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.110	2.671E4	02	22.770	2.733E4	03	68.300	2.254E4	04	91.100	2.374E4
05	113.830	2.344E4	06	136.600	2.385E4	07	159.360	2.357E4	08	182.130	2.287E4
<b>Dicamba</b>			Average RF			RSD = 5.272			Average RF = 6.98E4		
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.400	7.596E4	02	23.510	7.54E4	03	70.500	6.777E4	04	94.000	6.892E4
05	117.540	6.778E4	06	141.050	6.83E4	07	164.560	6.719E4	08	188.060	6.708E4
<b>Dichlorprop</b>			Average RF			RSD = 11.4			Average RF = 1.865E4		
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.440	2.275E4	02	23.590	2.117E4	03	70.800	1.795E4	04	94.400	1.815E4
05	117.960	1.755E4	06	141.550	1.752E4	07	165.140	1.724E4	08	188.730	1.684E4
<b>Dinoseb</b>			Average RF			RSD = 6.412			Average RF = 6.187E4		
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF
01	9.450	6.933E4	02	23.620	6.67E4	03	70.900	6.137E4	04	94.500	6.031E4
05	118.100	5.965E4	06	141.720	6.03E4	07	165.340	5.89E4	08	188.960	5.837E4

## Initial Calibration - Detailed Report

**Calibration ID:** KC2000566

**Instrument ID:** K-GC-24

**Column Name:** RTX-CLP2

### MCPA

**Average RF**

**RSD = 8.948**

**Average RF = 5.855E1**

#	Amount	RF
01	934.770	45.67
05	11683.01	60.3
0		

#	Amount	RF
02	2336.600	61.1
06	14019.61	60.46
0		

#	Amount	RF
03	7010.000	60.22
07	16356.21	59.76
0		

#	Amount	RF
04	9346.000	61.33
08	18692.82	59.57
0		

### MCPP

**Linear**

**1/X**

**R2 =**

**0.99984741644702**

**Y=46.47 X+-2.364E+04**

#	Amount	RF
01	938.770	20.01
05	11733.10	44.54
0		

#	Amount	RF
02	2346.620	37.4
06	14079.72	45.01
0		

#	Amount	RF
03	7040.000	42.91
07	16426.34	44.58
0		

#	Amount	RF
04	9386.000	44.8
08	18772.96	44.98
0		

### 2,4-Dichlorophenylacetic Acid

**Average RF**

**RSD = 8.791**

**Average RF = 1.82E4**

#	Amount	RF
01	9.020	2.115E4
05	112.730	1.738E4

#	Amount	RF
02	22.550	2.015E4
06	135.280	1.732E4

#	Amount	RF
03	67.600	1.798E4
07	157.830	1.694E4

#	Amount	RF
04	90.200	1.794E4
08	180.370	1.67E4

### Analyte

#### 2,4,5-T

#	Amount	Calculated		%D	#	Amount	Calculated		%D	#	Amount	Calculated		%D
		Conc	%D				Conc	%D				Conc	%D	
01	9.480	9.99	5.3	01	23.700	25.1	5.7	03	71.100	70.3	-1.1			
04	94.800	93.3	-1.6	05	118.490	117	-1.3	06	142.190	142	0.2			
07	165.890	160	-3.5	08	189.590	183	-3.7							

#### 2,4,5-TP

#	Amount	Calculated		%D	#	Amount	Calculated		%D	#	Amount	Calculated		%D
		Conc	%D				Conc	%D				Conc	%D	
01	9.510	9.90	4.1	01	23.760	24.8	4.5	03	71.300	69.1	-3.1			
04	95.100	94.5	-0.6	05	118.820	117	-1.6	06	142.580	142	-0.1			
07	166.340	164	-1.3	08	190.100	186	-2.0							

#### 2,4-D

#	Amount	Calculated		%D	#	Amount	Calculated		%D	#	Amount	Calculated		%D
		Conc	%D				Conc	%D				Conc	%D	
01	9.400	11.0	17.2	01	23.510	26.3	11.9	03	70.500	68.9	-2.3			
04	94.000	91.0	-3.2	05	117.540	112	-4.5	06	141.050	134	-4.7			
07	164.560	154	-6.3	08	188.060	173	-8.2							

#### 2,4-DB

#	Amount	Calculated		%D	#	Amount	Calculated		%D	#	Amount	Calculated		%D
		Conc	%D				Conc	%D				Conc	%D	
01	9.470	10.2	8.2	01	23.670	27.0	14.3	03	71.000	69.4	-2.3			
04	94.700	91.7	-3.1	05	118.330	116	-2.4	06	142.000	139	-2.3			
07	165.670	159	-4.0	08	189.340	173	-8.4							

#### Dalapon

#	Amount	Calculated		%D	#	Amount	Calculated		%D	#	Amount	Calculated		%D
		Conc	%D				Conc	%D				Conc	%D	
01	9.110	10.0	10.1	01	22.770	25.7	12.7	03	68.300	63.5	-7.1			
04	91.100	89.1	-2.1	05	113.830	110	-3.4	06	136.600	134	-1.7			
07	159.360	155	-2.8	08	182.130	172	-5.7							

#### Dicamba

## Initial Calibration - Detailed Report

**Calibration ID:** KC2000566

**Instrument ID:** K-GC-24

**Column Name:** RTX-CLP2

#	Amount	Calculated		#	Amount	Calculated		#	Amount	Calculated	
		Conc	%D			Conc	%D			Conc	%D
01	9.400	10.2	8.8	02	23.510	25.4	8.0	03	70.500	68.5	-2.9
04	94.000	92.8	-1.3	05	117.540	114	-2.9	06	141.050	138	-2.2
07	164.560	158	-3.7	08	188.060	181	-3.9				

### Dichlorprop

#	Amount	Calculated		#	Amount	Calculated		#	Amount	Calculated	
		Conc	%D			Conc	%D			Conc	%D
01	9.440	11.5	22.0	02	23.590	26.8	13.5	03	70.800	68.2	-3.7
04	94.400	91.9	-2.7	05	117.960	111	-5.9	06	141.550	133	-6.0
07	165.140	153	-7.6	08	188.730	170	-9.7				

### Dinoseb

#	Amount	Calculated		#	Amount	Calculated		#	Amount	Calculated	
		Conc	%D			Conc	%D			Conc	%D
01	9.450	10.6	12.1	02	23.620	25.5	7.8	03	70.900	70.3	-0.8
04	94.500	92.1	-2.5	05	118.100	114	-3.6	06	141.720	138	-2.5
07	165.340	157	-4.8	08	188.960	178	-5.6				

### MCPA

#	Amount	Calculated		#	Amount	Calculated		#	Amount	Calculated	
		Conc	%D			Conc	%D			Conc	%D
01	934.770	729	-22.0	02	2336.600	2440	4.4	03	7010.000	7210	2.8
04	9346.000	9790	4.7	05	11683.010	12000	3.0	06	14019.610	14500	3.3
07	16356.210	16700	2.1	08	18692.820	19000	1.7				

### MCPP

#	Amount	Calculated		#	Amount	Calculated		#	Amount	Calculated	
		Conc	%D			Conc	%D			Conc	%D
01	938.770	913	-2.8	02	2346.620	2400	2.2	03	7040.000	7010	-0.4
04	9386.000	9560	1.8	05	11733.100	11800	0.2	06	14079.720	14100	0.5
07	16426.340	16300	-1.0	08	18772.960	18700	-0.5				

### 2,4-Dichlorophenylacetic Acid

#	Amount	Calculated		#	Amount	Calculated		#	Amount	Calculated	
		Conc	%D			Conc	%D			Conc	%D
01	9.020	10.5	16.3	02	22.550	25.0	10.7	03	67.600	66.8	-1.2
04	90.200	88.9	-1.4	05	112.730	108	-4.5	06	135.280	129	-4.8
07	157.830	147	-6.9	08	180.370	166	-8.2				

**Calibration ID:** KC2000566

**Instrument ID:** K-GC-24

**Column Name:** ZB-XLB-HT

## Initial Calibration - Detailed Report

**Calibration ID:** KC2000566

**Instrument ID:** K-GC-24

**Column Name:** ZB-XLB-HT

#	Lab Code	Sample Name	File Location	Aquisition Date
01	KC2000566-01	PENTA2-14K 10PPB	J:\gc24\data\102120\10210004.D\10210004c.d	10/21/2020 13:46
02	KC2000566-02	PENTA2-14L 25PPB	J:\gc24\data\102120\10210005.D\10210005c.d	10/21/2020 14:09
03	KC2000566-03	PENTA2-14M 75PPB	J:\gc24\data\102120\10210006.D\10210006c.d	10/21/2020 14:33
04	KC2000566-04	PENTA2-14N 100PB	J:\gc24\data\102120\10210007.D\10210007c.d	10/21/2020 14:57
05	KC2000566-05	PENTA2-15A 125PB	J:\gc24\data\102120\10210008.D\10210008c.d	10/21/2020 15:21
06	KC2000566-06	PENTA2-15B 150PB	J:\gc24\data\102120\10210009.D\10210009c.d	10/21/2020 15:44
07	KC2000566-07	PENTA2-15C 175PB	J:\gc24\data\102120\10210010.D\10210010c.d	10/21/2020 16:08
08	KC2000566-08	PENTA2-15D 200PB	J:\gc24\data\102120\10210011.D\10210011c.d	10/21/2020 16:32

### Analyte

### Curve Fit

### Weighting

#### 2,4,5-T

#### Average RF

RSD = 8.204

Average RF = 1.914E5

#	Amount	RF
01	9.480	2.241E5
05	118.490	1.821E5

#	Amount	RF
02	23.700	2.074E5
06	142.190	1.835E5

#	Amount	RF
03	71.100	1.833E5
07	165.890	1.828E5

#	Amount	RF
04	94.800	1.848E5
08	189.590	1.83E5

#### 2,4,5-TP

#### Average RF

RSD = 7.62

Average RF = 2.03E5

#	Amount	RF
01	9.510	2.358E5
05	118.820	1.949E5

#	Amount	RF
02	23.760	2.178E5
06	142.580	1.947E5

#	Amount	RF
03	71.300	1.953E5
07	166.340	1.946E5

#	Amount	RF
04	95.100	1.956E5
08	190.100	1.952E5

#### 2,4-D

#### Average RF

RSD = 17.22

Average RF = 5.12E4

#	Amount	RF
01	9.400	6.995E4
05	117.540	4.681E4

#	Amount	RF
02	23.510	5.929E4
06	141.050	4.616E4

#	Amount	RF
03	70.500	4.845E4
07	164.560	4.575E4

#	Amount	RF
04	94.000	4.767E4
08	188.060	4.551E4

#### 2,4-DB

#### Average RF

RSD = 11.07

Average RF = 2.902E4

#	Amount	RF
01	9.470	3.572E4
05	118.330	2.726E4

#	Amount	RF
02	23.670	3.225E4
06	142.000	2.732E4

#	Amount	RF
03	71.000	2.779E4
07	165.670	2.706E4

#	Amount	RF
04	94.700	2.756E4
08	189.340	2.717E4

#### Dalapon

#### Average RF

RSD = 4.39

Average RF = 4.831E4

#	Amount	RF
01	9.110	5.105E4
05	113.830	4.838E4

#	Amount	RF
02	22.770	5.207E4
06	136.600	4.664E4

#	Amount	RF
03	68.300	4.698E4
07	159.360	4.774E4

#	Amount	RF
04	91.100	4.631E4
08	182.130	4.733E4

#### Dicamba

#### Average RF

RSD = 7.713

Average RF = 1.482E5

#	Amount	RF
01	9.400	1.724E5
05	117.540	1.425E5

#	Amount	RF
02	23.510	1.593E5
06	141.050	1.416E5

#	Amount	RF
03	70.500	1.424E5
07	164.560	1.42E5

#	Amount	RF
04	94.000	1.43E5
08	188.060	1.426E5

#### Dichlorprop

#### Average RF

RSD = 14.71

Average RF = 4.172E4

#	Amount	RF
01	9.440	5.44E4
05	117.960	3.868E4

#	Amount	RF
02	23.590	4.793E4
06	141.550	3.809E4

#	Amount	RF
03	70.800	3.993E4
07	165.140	3.779E4

#	Amount	RF
04	94.400	3.939E4
08	188.730	3.751E4

#### Dinoseb

#### Average RF

RSD = 10.83

Average RF = 1.368E5

#	Amount	RF
01	9.450	1.678E5
05	118.100	1.294E5

#	Amount	RF
02	23.620	1.515E5
06	141.720	1.286E5

#	Amount	RF
03	70.900	1.309E5
07	165.340	1.279E5

#	Amount	RF
04	94.500	1.301E5
08	188.960	1.278E5

## Initial Calibration - Detailed Report

<b>Calibration ID:</b> KC2000566	<b>Instrument ID:</b> K-GC-24
	<b>Column Name:</b> ZB-XLB-HT

<b>MCPA</b>			<b>Linear</b>			<b>1/X</b>			<b>R2 =</b> 0.9970434185726530			<b>Y=189.2 X+3.555E5</b>											
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF									
01	934.770	532.2	02	2336.600	372.4	03	7010.000	249.2	04	9346.000	232.3	05	11683.01	221.8	06	14019.61	213	07	16356.21	207.2	08	18692.82	203.3
	0			0			0			0			0			0							

<b>MCPP</b>			<b>Linear</b>			<b>1/X</b>			<b>R2 =</b> 0.9944121406118910			<b>Y=144.7 X+2.053E5</b>											
#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF	#	Amount	RF									
01	938.770	324.8	02	2346.620	262.9	03	7040.000	184.7	04	9386.000	172.7	05	11733.10	164.5	06	14079.72	157.4	07	16426.34	153.2	08	18772.96	150.1
	0			0			0			0			0			0							

<b>2,4-Dichlorophenylacetic Acid</b>				<b>Average RF</b>				<b>RSD = 15.77</b>				<b>Average RF = 4.23E4</b>			
#	Amount	RF	%D	#	Amount	RF	%D	#	Amount	RF	%D	#	Amount	RF	%D
01	9.020	5.587E4		02	22.550	4.943E4		03	67.600	4.041E4		04	90.200	3.953E4	
05	112.730	3.892E4		06	135.280	3.822E4		07	157.830	3.814E4		08	180.370	3.787E4	

**Analyte**

<b>2,4,5-T</b>											
#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.480	11.1	17.1	02	23.700	25.7	8.4	03	71.100	68.1	-4.2
04	94.800	91.6	-3.4	05	118.490	113	-4.8	06	142.190	136	-4.1
07	165.890	159	-4.5	08	189.590	181	-4.4				

<b>2,4,5-TP</b>											
#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.510	11.0	16.2	02	23.760	25.5	7.3	03	71.300	68.6	-3.8
04	95.100	91.6	-3.7	05	118.820	114	-4.0	06	142.580	137	-4.1
07	166.340	159	-4.2	08	190.100	183	-3.8				

<b>2,4-D</b>											
#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.400	12.8	36.6	02	23.510	27.2	15.8	03	70.500	66.7	-5.4
04	94.000	87.5	-6.9	05	117.540	107	-8.6	06	141.050	127	-9.8
07	164.560	147	-10.6	08	188.060	167	-11.1				

<b>2,4-DB</b>											
#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.470	11.7	23.1	02	23.670	26.3	11.2	03	71.000	68.0	-4.2
04	94.700	90.0	-5.0	05	118.330	111	-6.1	06	142.000	134	-5.8
07	165.670	154	-6.8	08	189.340	177	-6.4				

<b>Dalapon</b>											
#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.110	9.63	5.7	02	22.770	24.5	7.8	03	68.300	66.4	-2.8
04	91.100	87.3	-4.1	05	113.830	114	0.1	06	136.600	132	-3.5
07	159.360	157	-1.2	08	182.130	178	-2.0				

**Dicamba**

## Initial Calibration Verification Summary Report

<b>Calibration ID:</b>	KC2000566	<b>Instrument ID:</b>	K-GC-24
<b>Datafile ID:</b>	J:\gc24\data\102120\10210012.D	<b>Column Name:</b>	ZB-XLB-HT

Analyte	Lab Code	Type	Curve Fit	True Value	Calc Conc	Units	Result	Criteria
2,4,5-T	KC2000566-09	T	Average RF	94.80	98.768	ppb	4.2	<= 20
2,4,5-TP	KC2000566-09	T	Average RF	95.10	92.500	ppb	-2.7	<= 20
2,4-D	KC2000566-09	T	Average RF	94	83.643	ppb	-11.0	<= 20
2,4-DB	KC2000566-09	T	Average RF	94.70	95.240	ppb	0.6	<= 20
Dalapon	KC2000566-09	T	Average RF	91.10	95.982	ppb	5.4	<= 20
Dicamba	KC2000566-09	T	Average RF	94	96.106	ppb	2.2	<= 20
Dichlorprop	KC2000566-09	T	Average RF	94.40	85.597	ppb	-9.3	<= 20
Dinoseb	KC2000566-09	T	Average RF	94.50	94.362	ppb	-0.1	<= 20
MCPA	KC2000566-09	T	Linear	9346	10030.937	ppb	7.3	<= 20
MCPP	KC2000566-09	T	Linear	9386	10136.279	ppb	8.0	<= 20

<b>Calibration ID:</b>	KC2000566	<b>Instrument ID:</b>	K-GC-24
<b>Datafile ID:</b>	J:\gc24\data\102120\10210012.D	<b>Column Name:</b>	RTX-CLP2

Analyte	Lab Code	Type	Curve Fit	True Value	Calc Conc	Units	Result	Criteria
2,4,5-T	KC2000566-09	T	Average RF	94.80	98.209	ppb	3.6	<= 20
2,4,5-TP	KC2000566-09	T	Average RF	95.10	93.370	ppb	-1.8	<= 20
2,4-D	KC2000566-09	T	Average RF	94	90.423	ppb	-3.8	<= 20
2,4-DB	KC2000566-09	T	Average RF	94.70	93.935	ppb	-0.8	<= 20
Dalapon	KC2000566-09	T	Average RF	91.10	93.788	ppb	3.0	<= 20
Dicamba	KC2000566-09	T	Average RF	94	95.894	ppb	2.0	<= 20
Dichlorprop	KC2000566-09	T	Average RF	94.40	86.318	ppb	-8.6	<= 20
Dinoseb	KC2000566-09	T	Average RF	94.50	95.003	ppb	0.5	<= 20
MCPA	KC2000566-09	T	Average RF	9346	10069.096	ppb	7.7	<= 20
MCPP	KC2000566-09	T	Linear	9386	9672.717	ppb	3.1	<= 20

## Initial Calibration - Detailed Report

<b>Calibration ID:</b> KC2000566	<b>Instrument ID:</b> K-GC-24
	<b>Column Name:</b> ZB-XLB-HT

#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.400	10.9	16.3	02	23.510	25.3	7.5	03	70.500	67.7	-3.9
04	94.000	90.7	-3.5	05	117.540	113	-3.9	06	141.050	135	-4.5
07	164.560	158	-4.2	08	188.060	181	-3.8				

### Dichlorprop

#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.440	12.3	<b>30.4</b>	02	23.590	27.1	14.9	03	70.800	67.8	-4.3
04	94.400	89.1	-5.6	05	117.960	109	-7.3	06	141.550	129	-8.7
07	165.140	150	-9.4	08	188.730	170	-10.1				

### Dinoseb

#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.450	11.6	22.7	02	23.620	26.2	10.8	03	70.900	67.9	-4.2
04	94.500	89.9	-4.8	05	118.100	112	-5.4	06	141.720	133	-6.0
07	165.340	155	-6.5	08	188.960	177	-6.5				

### MCPA

#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	934.770	750	-19.7	02	2336.600	2720	16.4	03	7010.000	7350	4.9
04	9346.000	9600	2.7	05	11683.010	11800	1.1	06	14019.610	13900	-0.8
07	16356.210	16000	-2.0	08	18692.820	18200	-2.6				

### MCPP

#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	938.770	689	-26.6	02	2346.620	2840	21.2	03	7040.000	7570	7.5
04	9386.000	9780	4.2	05	11733.100	11900	1.6	06	14079.720	13900	-1.3
07	16426.340	16000	-2.8	08	18772.960	18100	-3.8				

### 2,4-Dichlorophenylacetic Acid

#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D	#	Amount	Calculated Conc	%D
01	9.020	11.9	<b>32.1</b>	02	22.550	26.4	16.9	03	67.600	64.6	-4.5
04	90.200	84.3	-6.5	05	112.730	104	-8.0	06	135.280	122	-9.7
07	157.830	142	-9.8	08	180.370	161	-10.5				



Data File : J:\gc24\data\102120\10210003.D Vial: 1  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 1:22 pm Operator: UA  
 Sample : IB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:46:26 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	8.009	7.829	7280	43923	0.400	1.038 #
Target Compounds						
1) m Dalapon	3.136	2.865	9965	74917	0.411	1.551 #
3) m Dicamba	8.209	7.905	29172	27129	0.418	0.183 #
4) m MCPP	0.000	8.082	0	2122	N.D.	N.D.
5) m MCPA	8.552	8.362	2704	44075	46.181	N.D. #
6) m Dichloroprop	8.939	8.758	23826	6916	1.278	0.166 #
7) m 2,4-D	9.349	0.000	6880	0	0.324	N.D. d#
8) m 2,4,5-TP ...	10.259	10.129	9196	34595	0.098	0.170 #
9) m 2,4,5-T	10.709	10.539	13577	43959	0.165	0.230 #
10) m 2,4-DB	0.000	11.139	0	3230	N.D. d	0.111
11) m Dinoseb	11.682	11.315	11024	25541	0.178	0.187
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\102120\10210003.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:22 pm  
Sample : IB  
Misc :

Vial: 1  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:46:26 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210004.D Vial: 3  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 1:46 pm Operator: UA  
 Sample : PENTA2-14K 10PPB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:30:40 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:28:50 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.997	7.820	190814	503954	10.736	12.487
Target Compounds						
1) m Dalapon	3.127	2.873	243340	465074	10.178	9.705
3) m Dicamba	8.217	7.920	714045	1620262	10.361m	11.193
4) m MCPP	8.300	8.106	18782	304912	432.162	1713.825 #
5) m MCPA	8.567	8.353	42691	497459	706.888	2049.337 #
6) m Dichloroprop	8.967	8.753	214760	513503	11.890	12.869
7) m 2,4-D	9.330	9.066	233900	657519	11.289	13.552
8) m 2,4,5-TP ...	10.263	10.130	927413	2242551	9.958m	11.308
9) m 2,4,5-T	10.710	10.536	823973	2124220	10.063	11.378
10) m 2,4-DB	11.290	11.173	105152	338252	10.371m	12.055
11) m Dinoseb	11.683	11.316	655169	1585317	10.776m	11.980
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\102120\10210004.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm  
Sample : PENTA2-14K 10PPB  
Misc :

Vial: 3  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:30:40 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210004.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm Operator: UA  
Sample : PENTA2-14K 10PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:29:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.290min 34.659 ppb  
response 351402



Manual Integration:  
Before  
10/21/20

(10) 2,4-DB #2 (m)  
11.173min 12.055 ppb  
response 338252

Data File : J:\gc24\data\102120\10210004.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm Operator: UA  
Sample : PENTA2-14K 10PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:29:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.290min 10.371 ppb m  
response 105152



Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(10) 2,4-DB #2 (m)  
11.173min 12.055 ppb  
response 338252

Data File : J:\gc24\data\102120\10210004.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm Operator: UA  
Sample : PENTA2-14K 10PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:29:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(11) Dinoseb (m)  
11.683min 11.414 ppb  
response 693954



Manual Integration:  
Before  
10/21/20

(11) Dinoseb #2 (m)  
11.316min 11.980 ppb  
response 1585317

Data File : J:\gc24\data\102120\10210004.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm Operator: UA  
Sample : PENTA2-14K 10PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:29:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(11) Dinoseb (m)  
11.683min 10.776 ppb m  
response 655169

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20



(11) Dinoseb #2 (m)  
11.316min 11.980 ppb  
response 1585317



Data File : J:\gc24\data\102120\10210004.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm Operator: UA  
Sample : PENTA2-14K 10PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:29:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(3) Dicamba (m)  
8.217min 12.005 ppb  
response 827399



Manual Integration:  
Before  
10/21/20

(3) Dicamba #2 (m)  
7.920min 11.193 ppb  
response 1620262

Data File : J:\gc24\data\102120\10210004.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm Operator: UA  
Sample : PENTA2-14K 10PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:29:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(3) Dicamba (m)  
8.217min 10.361 ppb m  
response 714045

(3) Dicamba #2 (m)  
7.920min 11.193 ppb  
response 1620262



Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(+) = Expected Retention Time

Data File : J:\gc24\data\102120\10210004.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm Operator: UA  
Sample : PENTA2-14K 10PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:29:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)

10.263min 10.244 ppb

response 954083

Manual Integration:

Before

10/21/20

(8) 2,4,5-TP (Silvex) #2 (m)



10.130min 11.308 ppb

response 2242551

Data File : J:\gc24\data\102120\10210004.D Vial: 3  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 1:46 pm Operator: UA  
Sample : PENTA2-14K 10PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:29:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:28:50 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(8) 2,4,5-TP (Silvex) (m)  
10.263min 9.958 ppb m  
response 927413

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(8) 2,4,5-TP (Silvex) #2 (m)  
10.130min 11.308 ppb  
response 2242551

Data File : J:\gc24\data\102120\10210005.D Vial: 4  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 2:09 pm Operator: UA  
 Sample : PENTA2-14L 25PPB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:28:28 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:26:33 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.994	7.817	454333	1114582	26.144	28.691
Target Compounds						
1) m Dalapon	3.128	2.874	622375	1185641	26.669m	25.104m
3) m Dicamba	8.214	7.917	1772679	3745342	26.131m	26.313
4) m MCPP	8.301	8.104	87770	616897	1973.683	3767.293 #
5) m MCPA	8.564	8.351	142776	870257	2368.770	3935.605 #
6) m Dichloroprop	8.968	8.751	499436	1130772	28.469	29.321
7) m 2,4-D	9.324	9.064	558866	1393959	27.651	29.833
8) m 2,4,5-TP ...	10.264	10.127	2326151	5175294	25.192	26.532
9) m 2,4,5-T	10.708	10.534	2067316	4914810	25.526m	26.821
10) m 2,4-DB	11.288	11.167	277452	763407	28.096m	27.903
11) m Dinoseb	11.684	11.314	1575526	3578948	26.340	27.716
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\102120\10210005.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm  
Sample : PENTA2-14L 25PPB  
Misc :

Vial: 4  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:28:28 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210005.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm Operator: UA  
Sample : PENTA2-14L 25PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:50 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.128min 26.760 ppb  
response 624496



Manual Integration:  
Before  
10/21/20

(1) Dalapon #2 (m)  
2.874min 42.153 ppb  
response 1990871

Data File : J:\gc24\data\102120\10210005.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm Operator: UA  
Sample : PENTA2-14L 25PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:50 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.128min 26.669 ppb m  
response 622375

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20



(1) Dalapon #2 (m)  
2.874min 25.104 ppb m  
response 1185641



Data File : J:\gc24\data\102120\10210005.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm Operator: UA  
Sample : PENTA2-14L 25PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:50 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.288min 50.935 ppb  
response 502979



Manual Integration:  
Before  
10/21/20

(10) 2,4-DB #2 (m)  
11.167min 27.903 ppb  
response 763407

Data File : J:\gc24\data\102120\10210005.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm Operator: UA  
Sample : PENTA2-14L 25PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:50 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.288min 28.096 ppb m  
response 277452



Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(10) 2,4-DB #2 (m)  
11.167min 27.903 ppb  
response 763407

Data File : J:\gc24\data\102120\10210005.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm Operator: UA  
Sample : PENTA2-14L 25PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:50 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(3) Dicamba (m)  
8.214min 26.882 ppb  
response 1823650



Manual Integration:  
Before  
10/21/20

(3) Dicamba #2 (m)  
7.917min 26.313 ppb  
response 3745342

Data File : J:\gc24\data\102120\10210005.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm Operator: UA  
Sample : PENTA2-14L 25PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:50 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(3) Dicamba (m)  
8.214min 26.131 ppb m  
response 1772679



(3) Dicamba #2 (m)  
7.917min 26.313 ppb  
response 3745342

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

Data File : J:\gc24\data\102120\10210005.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm Operator: UA  
Sample : PENTA2-14L 25PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:50 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(9) 2,4,5-T (m)  
10.708min 26.371 ppb  
response 2135780



Manual Integration:  
Before  
10/21/20

(9) 2,4,5-T #2 (m)  
10.534min 26.821 ppb  
response 4914810

Data File : J:\gc24\data\102120\10210005.D Vial: 4  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:09 pm Operator: UA  
Sample : PENTA2-14L 25PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:50 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:26:33 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(9) 2,4,5-T (m)  
10.708min 25.526 ppb m  
response 2067316

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(9) 2,4,5-T #2 (m)  
10.534min 26.821 ppb  
response 4914810

Data File : J:\gc24\data\102120\10210006.D Vial: 5  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 2:33 pm Operator: UA  
 Sample : PENTA2-14M 75PPB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:26:03 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:24:19 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.994	7.813	1215646	2731831	70.442	70.893
Target Compounds						
1) m Dalapon	3.127	2.873	1539560	3208933	65.523m	67.872m
3) m Dicamba	8.214	7.917	4777999	10040786	70.417	70.550
4) m MCPP	8.300	8.103	302116	1300529	6746.467	8151.025
5) m MCPA	8.564	8.350	422140	1746556	7002.375	8103.973
6) m Dichloroprop	8.964	8.750	1271081	2826954	72.793	73.826
7) m 2,4-D	9.324	9.057	1462698	3415664	72.757	73.646
8) m 2,4,5-TP ...	10.260	10.127	6475348	13928120	69.897	71.425
9) m 2,4,5-T	10.704	10.530	5799509	13030282	71.712	71.109
10) m 2,4-DB	11.284	11.163	711824	1973095	72.304m	72.345
11) m Dinoseb	11.680	11.313	4350886	9284027	73.117	72.100
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\102120\10210006.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:33 pm  
Sample : PENTA2-14M 75PPB  
Misc :

Vial: 5  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:26:03 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:24:19 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm







Data File : J:\gc24\data\102120\10210006.D Vial: 5  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:33 pm Operator: UA  
Sample : PENTA2-14M 75PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:24:40 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:24:19 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.127min 88.037 ppb  
response 2068544



Manual Integration:  
Before  
10/21/20

(1) Dalapon #2 (m)  
2.873min 84.167 ppb  
response 3979368

Data File : J:\gc24\data\102120\10210006.D Vial: 5  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 2:33 pm Operator: UA  
 Sample : PENTA2-14M 75PPB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:24:40 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:24:19 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
 3.127min 70.095 ppb m  
 response 1646979



(1) Dalapon #2 (m)  
 2.873min 67.872 ppb m  
 response 3208933

Manual Integration:  
 After  
 Baseline/Shoulder  
 10/21/20

Data File : J:\gc24\data\102120\10210006.D Vial: 5  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:33 pm Operator: UA  
Sample : PENTA2-14M 75PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:24:40 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:24:19 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.127min 65.523 ppb m  
response 1539560



Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(1) Dalapon #2 (m)  
2.873min 67.872 ppb m  
response 3208933

Data File : J:\gc24\data\102120\10210006.D Vial: 5  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:33 pm Operator: UA  
Sample : PENTA2-14M 75PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:24:40 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:24:19 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.284min 94.555 ppb  
response 930876



Manual Integration:  
Before  
10/21/20

(10) 2,4-DB #2 (m)  
11.163min 72.345 ppb  
response 1973095

Data File : J:\gc24\data\102120\10210006.D Vial: 5  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:33 pm Operator: UA  
Sample : PENTA2-14M 75PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:24:40 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:24:19 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.284min 72.304 ppb m  
response 711824

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(10) 2,4-DB #2 (m)  
11.163min 72.345 ppb  
response 1973095

Data File : J:\gc24\data\102120\10210007.D Vial: 6  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 2:57 pm Operator: UA  
 Sample : PENTA2-14N 100PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:16:06 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:14:34 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.997	7.817	1618486	3565715	90.200	90.200
Target Compounds						
1) m Dalapon	3.127	2.873	2162531	4219125	94.759m	90.872m
3) m Dicamba	8.217	7.917	6478443	13439517	94.000	94.000
4) m MCPP	8.300	8.107	420510	1620847	9386.000	9386.000
5) m MCPA	8.567	8.353	573212	2171147	9346.000	9346.000
6) m Dichloroprop	8.967	8.753	1713548	3718829	94.400	94.400
7) m 2,4-D	9.324	9.057	1932853	4480708	94.000	94.000
8) m 2,4,5-TP ...	10.264	10.130	8853387	18598859	95.100	95.100
9) m 2,4,5-T	10.704	10.530	7699095	17520598	94.800	95.204
10) m 2,4-DB	11.287	11.167	941169	2610405	93.789m	94.700
11) m Dinoseb	11.684	11.313	5699341	12298812	94.500	94.500
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\102120\10210007.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:57 pm  
Sample : PENTA2-14N 100PB  
Misc :

Vial: 6  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:16:06 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:14:34 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210007.D Vial: 6  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:57 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 16:16:14 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 16:16:08 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.127min 91.100 ppb  
response 2583448

(1) Dalapon #2 (m)  
2.873min 90.173 ppb m  
response 4587035



Manual Integration:  
After  
Baseline/Shoulder  
10/21/20



Data File : J:\gc24\data\102120\10210007.D Vial: 6  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:57 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:14:42 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:14:34 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.127min 94.759 ppb m  
response 2162531

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20



(1) Dalapon #2 (m)  
2.873min 90.872 ppb m  
response 4219125

(+) = Expected Retention Time

Data File : J:\gc24\data\102120\10210007.D Vial: 6  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:57 pm Operator: UA  
Sample : PENTA2-14N 100PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:14:42 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:14:34 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.287min 112.668 ppb  
response 1130621

Manual Integration:  
Before  
10/21/20



(10) 2,4-DB #2 (m)  
11.167min 94.700 ppb  
response 2610405

Data File : J:\gc24\data\102120\10210007.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 2:57 pm  
Sample : PENTA2-14N 100PB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:14:42 2020  
Quant Results File: 102120\_8151.RES

Vial: 6  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:14:34 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2  
Signal #1 Info : 0.25 mm  
Signal #2 Phase: ZB-XLB-HT  
Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.287min 93.789 ppb m  
response 941169

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(10) 2,4-DB #2 (m)  
11.167min 94.700 ppb  
response 2610405

Data File : J:\gc24\data\102120\10210008.D Vial: 7  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 3:21 pm Operator: UA  
 Sample : PENTA2-15A 125PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:24:02 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:22:48 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----							
System Monitoring Compounds							
2) s	2,4-Dichl...	7.993	7.813	1959232	4387572	113.731	114.146
Target Compounds							
1) m	Dalapon	3.127	2.873	2668589	5506745	113.511m	117.152m
3) m	Dicamba	8.213	7.916	7967267	16745862	117.390	117.694
4) m	MCPD	8.300	8.106	522627	1929619	11655.124	12187.501
5) m	MCPA	8.563	8.350	704455	2590948	11685.949	12109.753
6) m	Dichloroprop	8.963	8.750	2070717	4562901	118.745	119.464
7) m	2,4-D	9.320	9.056	2385344	5502448	118.932	118.917
8) m	2,4,5-TP ...	10.260	10.126	10956862	23161274	118.135	118.763
9) m	2,4,5-T	10.703	10.530	9647622	21578156	119.497	117.574
10) m	2,4-DB	11.283	11.166	1184989	3225586	120.887m	118.254
11) m	Dinoseb	11.680	11.313	7044640	15278779	118.457	118.795
-----							

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\102120\10210008.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:21 pm  
Sample : PENTA2-15A 125PB  
Misc :

Vial: 7  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:24:02 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:22:48 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210008.D Vial: 7  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:21 pm Operator: UA  
Sample : PENTA2-15A 125PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:22:59 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:22:48 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.127min 135.159 ppb  
response 3177545

Manual Integration:  
Before  
10/21/20



(1) Dalapon #2 (m)  
2.873min 131.218 ppb  
response 6167907

(+) = Expected Retention Time

Data File : J:\gc24\data\102120\10210008.D Vial: 7  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:21 pm Operator: UA  
Sample : PENTA2-15A 125PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:22:59 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:22:48 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.127min 113.511 ppb m  
response 2668589



Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(1) Dalapon #2 (m)  
2.873min 117.152 ppb m  
response 5506745

Data File : J:\gc24\data\102120\10210008.D Vial: 7  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:21 pm Operator: UA  
Sample : PENTA2-15A 125PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:22:59 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:22:48 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(10) 2,4-DB (m)  
11.283min 135.786 ppb  
response 1331036

Manual Integration:  
Before  
10/21/20



(10) 2,4-DB #2 (m)  
11.166min 118.254 ppb  
response 3225586



Data File : J:\gc24\data\102120\10210008.D Vial: 7  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:21 pm Operator: UA  
Sample : PENTA2-15A 125PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:22:59 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:22:48 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(10) 2,4-DB (m)  
11.283min 120.887 ppb m  
response 1184989

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(10) 2,4-DB #2 (m)  
11.166min 118.254 ppb  
response 3225586

Data File : J:\gc24\data\102120\10210009.D Vial: 8  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 3:44 pm Operator: UA  
 Sample : PENTA2-15B 150PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:22:31 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:20:52 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
System Monitoring Compounds						
2) s 2,4-Dichl...	7.993	7.813	2343632	5169864	136.302	134.240
Target Compounds						
1) m Dalapon	3.127	2.873	3258567	6370947	139.287m	135.187m
3) m Dicamba	8.213	7.916	9633232	19969572	142.235	140.119
4) m MCPP	8.297	8.103	633683	2215911	14149.230	13967.949
5) m MCPA	8.563	8.350	847585	2986150	14073.890	13936.089
6) m Dichloroprop	8.963	8.750	2480194	5391085	142.454	141.013
7) m 2,4-D	9.320	9.056	2855823	6510874	142.843	140.598
8) m 2,4,5-TP ...	10.260	10.126	13345050	27761527	144.324	142.275
9) m 2,4,5-T	10.703	10.530	11750806	26085006	146.702	142.112
10) m 2,4-DB	11.283	11.163	1423732	3879490	146.356m	142.303
11) m Dinoseb	11.680	11.310	8545635	18219499	144.368	141.640

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\102120\10210009.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:44 pm  
Sample : PENTA2-15B 150PB  
Misc :

Vial: 8  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:22:31 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:20:52 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210009.D Vial: 8  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:44 pm Operator: UA  
Sample : PENTA2-15B 150PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:21:21 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:20:52 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.127min 160.523 ppb  
response 3755373

Manual Integration:  
Before  
10/21/20



(1) Dalapon #2 (m)  
2.873min 151.774 ppb  
response 7152678

(+) = Expected Retention Time

Data File : J:\gc24\data\102120\10210009.D Vial: 8  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:44 pm Operator: UA  
Sample : PENTA2-15B 150PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:21:21 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:20:52 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(1) Dalapon (m)  
3.127min 139.287 ppb m  
response 3258567

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20



(1) Dalapon #2 (m)  
2.873min 135.187 ppb m  
response 6370947

(+) = Expected Retention Time

Data File : J:\gc24\data\102120\10210009.D Vial: 8  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:44 pm Operator: UA  
Sample : PENTA2-15B 150PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:21:21 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:20:52 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(10) 2,4-DB (m)  
11.283min 160.143 ppb  
response 1557848



Manual Integration:  
Before  
10/21/20

(10) 2,4-DB #2 (m)  
11.163min 142.303 ppb  
response 3879490

Data File : J:\gc24\data\102120\10210009.D Vial: 8  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 3:44 pm Operator: UA  
Sample : PENTA2-15B 150PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:21:21 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:20:52 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



QEdit

(10) 2,4-DB (m)  
11.283min 146.356 ppb m  
response 1423732

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(10) 2,4-DB #2 (m)  
11.163min 142.303 ppb  
response 3879490

Data File : J:\gc24\data\102120\10210010.D Vial: 9  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 4:08 pm Operator: UA  
 Sample : PENTA2-15C 175PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:20:38 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:19:22 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.993	7.813	2673899	6019072	154.374	155.532
Target Compounds						
1) m Dalapon	3.126	2.873	3756341	7607536	161.174m	162.479m
3) m Dicamba	8.213	7.916	11056277	23365839	162.598	163.645
4) m MCPP	8.300	8.106	732283	2515897	16313.328	15589.638
5) m MCPA	8.563	8.353	977526	3389231	16169.886	15560.846
6) m Dichloroprop	8.963	8.749	2846415	6241057	162.675	162.314
7) m 2,4-D	9.320	9.056	3276369	7528670	163.538	161.603
8) m 2,4,5-TP ...	10.260	10.129	15378740	32362961	166.306	165.616
9) m 2,4,5-T	10.703	10.529	13208642	30332986	164.413	164.939
10) m 2,4-DB	11.283	11.163	1631284	4482448	168.722m	163.801
11) m Dinoseb	11.683	11.313	9738174	21149943	164.104	163.966
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data File : J:\gc24\data\102120\10210010.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:08 pm  
Sample : PENTA2-15C 175PB  
Misc :

Vial: 9  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:20:38 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:19:22 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210010.D Vial: 9  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 4:08 pm Operator: UA  
 Sample : PENTA2-15C 175PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:19:31 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:19:22 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
 3.126min 186.524 ppb  
 response 4347148



Manual Integration:  
 Before  
 10/21/20

(1) Dalapon #2 (m)  
 2.873min 178.616 ppb  
 response 8363091

Data File : J:\gc24\data\102120\10210010.D Vial: 9  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:08 pm Operator: UA  
Sample : PENTA2-15C 175PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:19:31 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:19:22 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.126min 161.174 ppb m  
response 3756341



Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(1) Dalapon #2 (m)  
2.873min 162.479 ppb m  
response 7607536

Data File : J:\gc24\data\102120\10210010.D Vial: 9  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 4:08 pm Operator: UA  
 Sample : PENTA2-15C 175PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:19:31 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:19:22 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
 11.283min 180.728 ppb  
 response 1747369



Manual Integration:  
 Before  
 10/21/20

(10) 2,4-DB #2 (m)  
 11.163min 163.801 ppb  
 response 4482448

Data File : J:\gc24\data\102120\10210010.D Vial: 9  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:08 pm Operator: UA  
Sample : PENTA2-15C 175PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:19:31 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:19:22 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.283min 168.722 ppb m  
response 1631284

(10) 2,4-DB #2 (m)  
11.163min 163.801 ppb  
response 4482448

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

Data File : J:\gc24\data\102120\10210011.D Vial: 10  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 4:32 pm Operator: UA  
 Sample : PENTA2-15D 200PB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:19:09 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:16:23 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	7.991	7.814	3011902	6830371	167.857	172.784
Target Compounds						
1) m Dalapon	3.124	2.874	4166081	8620213	175.503m	186.129m
3) m Dicamba	8.214	7.914	12614321	26816087	183.029	187.560
4) m MCPP	8.298	8.104	844322	2817400	18845.702	16314.999
5) m MCPA	8.564	8.351	1113618	3800297	18157.111	16358.900
6) m Dichloroprop	8.964	8.751	3178809	7078599	175.122	179.686
7) m 2,4-D	9.321	9.057	3668350	8558209	178.402	179.541
8) m 2,4,5-TP ...	10.261	10.127	17460527	37116608	187.555	189.785
9) m 2,4,5-T	10.704	10.531	15065337	34693502	185.502	187.719
10) m 2,4-DB	11.288	11.167	1779525	5143484	179.055m	186.595
11) m Dinoseb	11.684	11.317	11030037	24155457	182.888	185.603
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data File : J:\gc24\data\102120\10210011.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:32 pm  
Sample : PENTA2-15D 200PB  
Misc :

Vial: 10  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:19:09 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:16:23 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210011.D Vial: 10  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:32 pm Operator: UA  
Sample : PENTA2-15D 200PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:17:43 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:16:23 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.124min 217.220 ppb  
response 5156366

Manual Integration:  
Before  
10/21/20



(1) Dalapon #2 (m)  
2.874min 208.116 ppb  
response 9638480



Data File : J:\gc24\data\102120\10210011.D Vial: 10  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:32 pm Operator: UA  
Sample : PENTA2-15D 200PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:17:43 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:16:23 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.124min 175.503 ppb m  
response 4166081



(1) Dalapon #2 (m)  
2.874min 186.129 ppb m  
response 8620213

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

Data File : J:\gc24\data\102120\10210011.D Vial: 10  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:32 pm Operator: UA  
Sample : PENTA2-15D 200PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:17:43 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:16:23 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.288min 194.607 ppb  
response 1934084



Manual Integration:  
Before  
10/21/20

(10) 2,4-DB #2 (m)  
11.167min 186.595 ppb  
response 5143484

Data File : J:\gc24\data\102120\10210011.D Vial: 10  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:32 pm Operator: UA  
Sample : PENTA2-15D 200PB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:17:43 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:16:23 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(10) 2,4-DB (m)  
11.288min 179.055 ppb m  
response 1779525

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(10) 2,4-DB #2 (m)  
11.167min 186.595 ppb  
response 5143484

Data File : J:\gc24\data\102120\10210012.D Vial: 11  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2020 4:56 pm Operator: UA  
 Sample : PENTA2-15E ICV 100 PPB Inst : HP G1530A  
 Misc : Multiplr: 1.00  
 Integration File signal 1: RTEINT.P  
 Integration File signal 2: RTEINT2.P  
 Quant Time: Oct 21 17:34:58 2020  
 Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
 Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
 QLast Update : Wed Oct 21 17:31:59 2020  
 Response via : Initial Calibration  
 DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
 Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
 Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

Compound	RT#1	RT#2	Resp#1	Resp#2	ppb	ppb
-----						
System Monitoring Compounds						
2) s 2,4-Dichl...	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
1) m Dalapon	3.124	2.874	2275140	4637166	93.788m	95.982m
3) m Dicamba	8.214	7.917	6693399	14244119	95.894	96.106
4) m MCPP	8.301	8.107	425850	1671884	9672.717	10136.278
5) m MCPA	8.564	8.354	589571	2253395	10069.096	10030.937
6) m Dichloroprop	8.967	8.754	1609647	3570683	86.318	85.597
7) m 2,4-D	9.324	9.064	1920602	4282415	90.423	83.643
8) m 2,4,5-TP ...	10.264	10.134	8747020	18777316	93.370	92.500
9) m 2,4,5-T	10.711	10.537	8103188	18900875	98.209	98.768
10) m 2,4-DB	11.291	11.174	963718	2763456	93.935	95.240
11) m Dinoseb	11.687	11.320	5877452	12904696	95.003	94.362
-----						



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data File : J:\gc24\data\102120\10210012.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:56 pm  
Sample : PENTA2-15E ICV 100 PPB  
Misc :  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:34:58 2020  
Quant Results File: 102120\_8151.RES

Vial: 11  
Operator: UA  
Inst : HP G1530A  
Multiplr: 1.00

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M



Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



Data File : J:\gc24\data\102120\10210012.D Vial: 11  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:56 pm Operator: UA  
Sample : PENTA2-15E ICV 100 PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:33:07 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

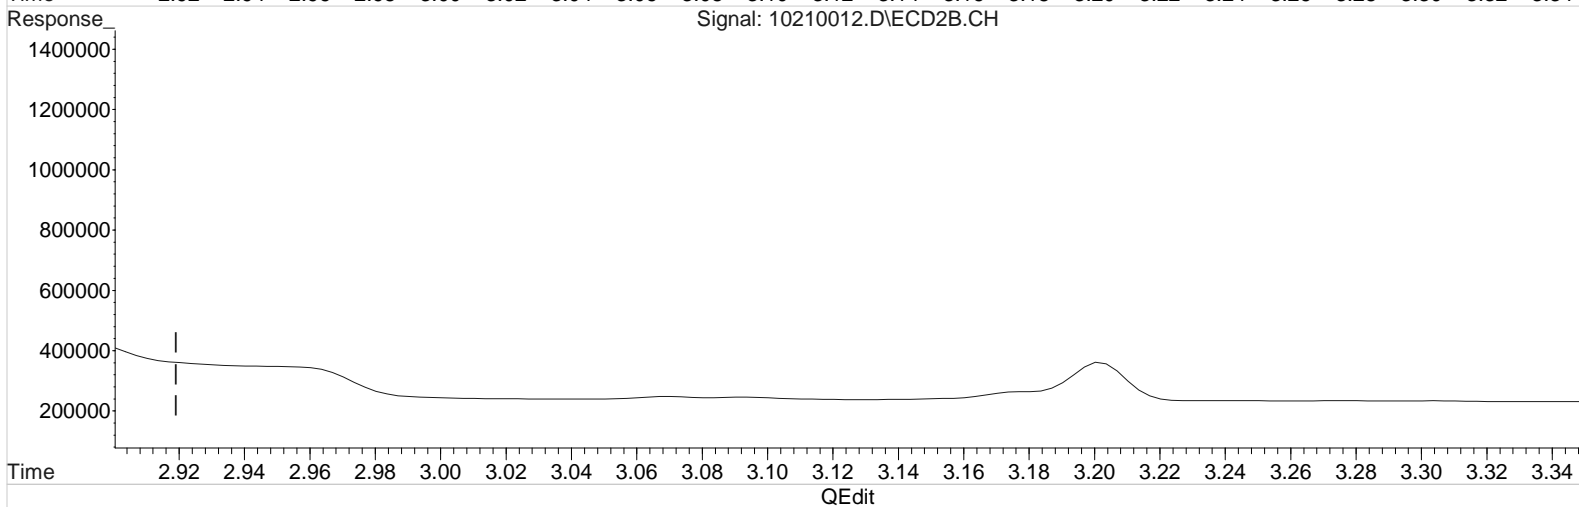

(1) Dalapon (m)  
3.124min 114.147 ppb  
response 2769027

Manual Integration:  
Before  
10/21/20



(1) Dalapon #2 (m)  
2.874min 131.747 ppb  
response 6365052

(+) = Expected Retention Time

Data File : J:\gc24\data\102120\10210012.D Vial: 11  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:56 pm Operator: UA  
Sample : PENTA2-15E ICV 100 PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:33:07 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm

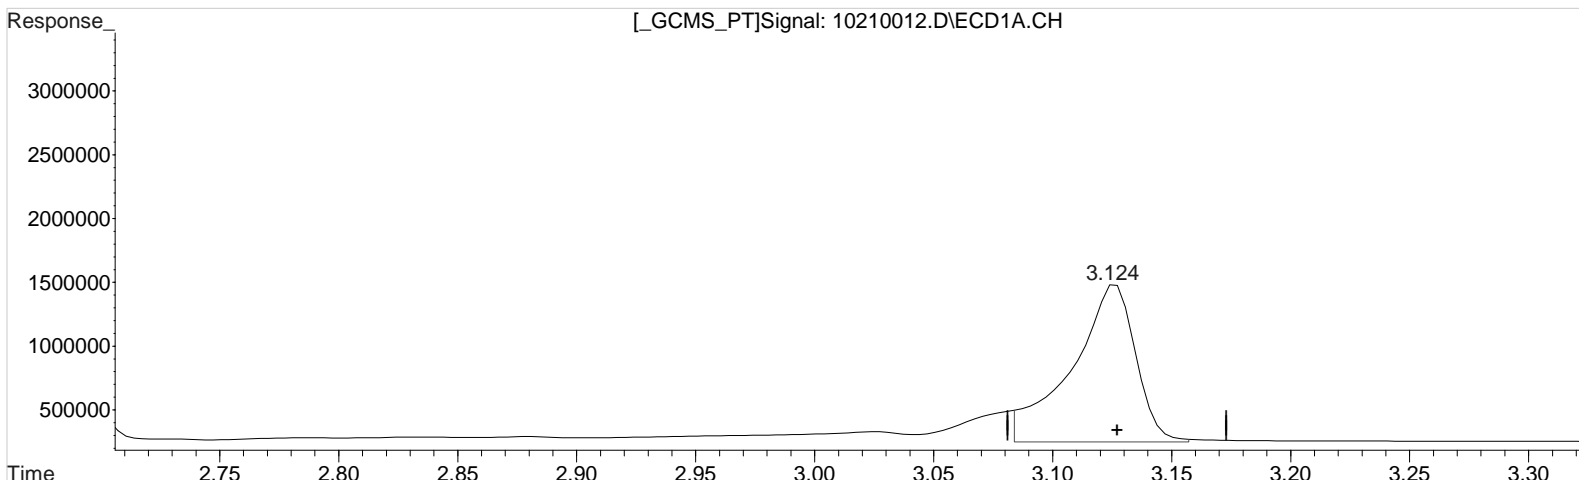

(1) Dalapon (m)  
3.124min 93.788 ppb m  
response 2275140



Manual Integration:  
Before  
10/21/20

(1) Dalapon #2 (m)  
2.874min 131.747 ppb  
response 6365052

Data File : J:\gc24\data\102120\10210012.D Vial: 11  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:56 pm Operator: UA  
Sample : PENTA2-15E ICV 100 PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:33:07 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.124min 93.788 ppb m  
response 2275140

(1) Dalapon #2 (m)  
2.874min 131.747 ppb  
response 6365052

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20



(+) = Expected Retention Time



Data File : J:\gc24\data\102120\10210012.D Vial: 11  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2020 4:56 pm Operator: UA  
Sample : PENTA2-15E ICV 100 PPB Inst : HP G1530A  
Misc : Multiplr: 1.00  
Integration File signal 1: RTEINT.P  
Integration File signal 2: RTEINT2.P  
Quant Time: Oct 21 17:33:07 2020  
Quant Results File: 102120\_8151.RES

Quant Method : J:\gc24\Methods\102120\_8151.M  
Quant Title : 103118\_8151.m MJ215 CAL\_KC1800  
QLast Update : Wed Oct 21 17:31:59 2020  
Response via : Initial Calibration  
DataAcq Meth:8151A-17.M

Volume Inj. : 2 uL  
Signal #1 Phase : RTX-CLP2 Signal #2 Phase: ZB-XLB-HT  
Signal #1 Info : 0.25 mm Signal #2 Info : 0.25 mm



(1) Dalapon (m)  
3.124min 93.788 ppb m  
response 2275140

Manual Integration:  
After  
Baseline/Shoulder  
10/21/20

(1) Dalapon #2 (m)  
2.874min 95.982 ppb m  
response 4637166

Sel	Run	Location	Method	Datafile	SeqTable	Calib:RF:RT	Sample Name
No	1	Vial 100	8151A-17	12010001	F:01:01		CCV PRIMER
No	2	Vial 100	8151A-17	12010002	F:02:01		PRIMER
No	3	Vial 2	8151A-17	12010003	F:03:01		PENTA2-14N 100PB
No	4	Vial 1	8151A-17	12010004	F:04:01		IB
No	5	Vial 51	8151A-17	12010005	F:05:01		KQ2018489-02MB
No	6	Vial 52	8151A-17	12010006	F:06:01		KQ2018489-01LCS
No	7	Vial 53	8151A-17	12010007	F:07:01		K2010456-001
No	8	Vial 54	8151A-17	12010008	F:08:01		K2010456-002
No	9	Vial 55	8151A-17	12010009	F:09:01		K2010456-003
No	10	Vial 56	8151A-17	12010010	F:10:01		K2010456-004
No	11	Vial 57	8151A-17	12010011	F:11:01		K2010456-005
No	12	Vial 58	8151A-17	12010012	F:12:01		K2010456-006
No	13	Vial 59	8151A-17	12010013	F:13:01		K2010456-007
No	14	Vial 60	8151A-17	12010014	F:14:01		K2010456-008
No	15	Vial 2	8151A-17	12010015	F:15:01		PENTA2-14N 100PB
No	16	Vial 1	8151A-17	12010016	F:16:01		IB
No	17	Vial 61	8151A-17	12010017	F:17:01		K2010456-009
No	18	Vial 62	8151A-17	12010018	F:18:01		K2010456-010
No	19	Vial 63	8151A-17	12010019	F:19:01		K2010456-011
No	20	Vial 64	8151A-17	12010020	F:20:01		K2010456-012
No	21	Vial 65	8151A-17	12010021	F:21:01		K2010456-016
No	22	Vial 66	8151A-17	12010022	F:22:01		K2010456-017
No	23	Vial 67	8151A-17	12010023	F:23:01		K2010456-018
No	24	Vial 68	8151A-17	12010024	F:24:01		K2010456-022
No	25	Vial 69	8151A-17	12010025	F:25:01		KQ2018489-03MS
No	26	Vial 70	8151A-17	12010026	F:26:01		KQ2018489-04DMS
No	27	Vial 2	8151A-17	12010027	F:27:01		PENTA2-14N 100PB
No	28	Vial 1	8151A-17	12010028	F:28:01		IB
No	29	Vial 71	8151A-17	12010029	F:29:01		K2010456-013 5X
No	30	Vial 72	8151A-17	12010030	F:30:01		K2010456-014 5X
No	31	Vial 73	8151A-17	12010031	F:31:01		K2010456-015 5X
No	32	Vial 74	8151A-17	12010032	F:32:01		K2010456-019 5X
No	33	Vial 3	8151A-17	12010033	F:33:01		KQ2017965-04MB
No	34	Vial 4	8151A-17	12010034	F:34:01		KQ2017965-03LCS
No	35	Vial 5	8151A-17	12010035	F:35:01		K2010456-020
No	36	Vial 6	8151A-17	12010036	F:36:01		K2010456-021
No	37	Vial 7	8151A-17	12010037	F:37:01		K2010456-023
No	38	Vial 8	8151A-17	12010038	F:38:01		K2010456-024
No	39	Vial 2	8151A-17	12010039	F:39:01		* <del>PENTA2-14N 100PB</del> IB
No	40	Vial 1	8151A-17	12010040	F:40:01		* <del>IB PENTA2-14N 100PB</del>
No	41	Vial 9	8151A-17	12010041	F:41:01		K2010456-025
No	42	Vial 10	8151A-17	12010042	F:42:01		K2010495-001
No	43	Vial 2	8151A-17	12010043	F:43:01		* <del>PENTA2-14N 100PB</del> Blank
No	44	Vial 51	8151A-17	12010044	F:44:01		KQ2018489-02MB
No	45	Vial 52	8151A-17	12010045	F:45:01		KQ2018489-01LCS
No	46	Vial 53	8151A-17	12010046	F:46:01		K2010456-001
No	47	Vial 54	8151A-17	12010047	F:47:01		K2010456-002
No	48	Vial 55	8151A-17	12010048	F:48:01		K2010456-003
No	49	Vial 56	8151A-17	12010049	F:49:01		K2010456-004
No	50	Vial 57	8151A-17	12010050	F:50:01		K2010456-005
No	51	Vial 1	8151A-17	12010051	F:51:01		PENTA2-14N 100PB ✓
No	52	Vial 2	8151A-17	12010052	F:52:01		IB
No	53	Vial 58	8151A-17	12010053	F:53:01		K2010456-006
No	54	Vial 59	8151A-17	12010054	F:54:01		K2010456-007
No	55	Vial 60	8151A-17	12010055	F:55:01		K2010456-008
No	56	Vial 61	8151A-17	12010056	F:56:01		K2010456-009
No	57	Vial 62	8151A-17	12010057	F:57:01		K2010456-010
No	58	Vial 63	8151A-17	12010058	F:58:01		K2010456-011
No	59	Vial 64	8151A-17	12010059	F:59:01		K2010456-012
No	60	Vial 65	8151A-17	12010060	F:60:01		K2010456-016
No	61	Vial 66	8151A-17	12010061	F:61:01		K2010456-017
No	62	Vial 67	8151A-17	12010062	F:62:01		K2010456-018
No	63	Vial 1	8151A-17	12010063	F:63:01		PENTA2-14N 100PB ✓
No	64	Vial 2	8151A-17	12010064	F:64:01		IB
No	65	Vial 68	8151A-17	12010065	F:65:01		K2010456-022

Run# 705654

RR

different Run

12/2/20

Seq	Run	Location	Method	Datafile	SeqTable	Calib:RF:RT	Sample Name
No	1	Vial 100	8151A-17	12010001	F:01:01		CCV PRIMER
No	2	Vial 100	8151A-17	12010002	F:02:01		PRIMER
No	3	Vial 2	8151A-17	12010003	F:03:01		PENTA2-14N 100PB
No	4	Vial 1	8151A-17	12010004	F:04:01		IB
No	5	Vial 51	8151A-17	12010005	F:05:01		KQ2018489-02MB
No	6	Vial 52	8151A-17	12010006	F:06:01		KQ2018489-01LCS
No	7	Vial 53	8151A-17	12010007	F:07:01		K2010456-001
No	8	Vial 54	8151A-17	12010008	F:08:01		K2010456-002
No	9	Vial 55	8151A-17	12010009	F:09:01		K2010456-003
No	10	Vial 56	8151A-17	12010010	F:10:01		K2010456-004
No	11	Vial 57	8151A-17	12010011	F:11:01		K2010456-005
No	12	Vial 58	8151A-17	12010012	F:12:01		K2010456-006
No	13	Vial 59	8151A-17	12010013	F:13:01		K2010456-007
No	14	Vial 60	8151A-17	12010014	F:14:01		K2010456-008
No	15	Vial 2	8151A-17	12010015	F:15:01		PENTA2-14N 100PB
No	16	Vial 1	8151A-17	12010016	F:16:01		IB
No	17	Vial 61	8151A-17	12010017	F:17:01		K2010456-009
No	18	Vial 62	8151A-17	12010018	F:18:01		K2010456-010
No	19	Vial 63	8151A-17	12010019	F:19:01		K2010456-011
No	20	Vial 64	8151A-17	12010020	F:20:01		K2010456-012
No	21	Vial 65	8151A-17	12010021	F:21:01		K2010456-016
No	22	Vial 66	8151A-17	12010022	F:22:01		K2010456-017
No	23	Vial 67	8151A-17	12010023	F:23:01		K2010456-018
No	24	Vial 68	8151A-17	12010024	F:24:01		K2010456-022
No	25	Vial 69	8151A-17	12010025	F:25:01		KQ2018489-03MS
No	26	Vial 70	8151A-17	12010026	F:26:01		KQ2018489-04DMS
No	27	Vial 2	8151A-17	12010027	F:27:01		PENTA2-14N 100PB
No	28	Vial 1	8151A-17	12010028	F:28:01		IB
No	29	Vial 71	8151A-17	12010029	F:29:01		K2010456-013 5X
No	30	Vial 72	8151A-17	12010030	F:30:01		K2010456-014 5X
No	31	Vial 73	8151A-17	12010031	F:31:01		K2010456-015 5X
No	32	Vial 74	8151A-17	12010032	F:32:01		K2010456-019 5X
No	33	Vial 3	8151A-17	12010033	F:33:01		KQ2017965-04MB
No	34	Vial 4	8151A-17	12010034	F:34:01		KQ2017965-03LCS
No	35	Vial 5	8151A-17	12010035	F:35:01		K2010456-020
No	36	Vial 6	8151A-17	12010036	F:36:01		K2010456-021
No	37	Vial 7	8151A-17	12010037	F:37:01		K2010456-023
No	38	Vial 8	8151A-17	12010038	F:38:01		K2010456-024
No	39	Vial 2	8151A-17	12010039	F:39:01		PENTA2-14N 100PB
No	40	Vial 1	8151A-17	12010040	F:40:01		IB
No	41	Vial 9	8151A-17	12010041	F:41:01		K2010456-025
No	42	Vial 10	8151A-17	12010042	F:42:01		K2010495-001
No	43	Vial 11	8151A-17	12010043	F:43:01		K2010495-002
No	44	Vial 12	8151A-17	12010044	F:44:01		K2010495-003
No	45	Vial 13	8151A-17	12010045	F:45:01		K2010495-004
No	46	Vial 14	8151A-17	12010046	F:46:01		K2010495-005
No	47	Vial 15	8151A-17	12010047	F:47:01		K2010495-006
No	48	Vial 16	8151A-17	12010048	F:48:01		K2010495-007
No	49	Vial 17	8151A-17	12010049	F:49:01		K2010495-008
No	50	Vial 18	8151A-17	12010050	F:50:01		K2010495-009
No	51	Vial 2	8151A-17	12010051	F:51:01		PENTA2-14N 100PB
No	52	Vial 1	8151A-17	12010052	F:52:01		IB
No	53	Vial 19	8151A-17	12010053	F:53:01		K2010495-010
No	54	Vial 20	8151A-17	12010054	F:54:01		K2010495-011
No	55	Vial 21	8151A-17	12010055	F:55:01		K2010495-012
No	56	Vial 22	8151A-17	12010056	F:56:01		KQ2017965-01MS
No	57	Vial 23	8151A-17	12010057	F:57:01		KQ2017965-02DMS
No	58	Vial 2	8151A-17	12010058	F:58:01		PENTA2-14N 100PB
No	59	Vial 1	8151A-17	12010059	F:59:01		IB
No	60	none	STANDBY	12010060	F:60:01		STANBY

Run #: 705487