



**Apex Laboratories, LLC**  
6700 SW Sandburg St. Tigard, Oregon 97223  
503.718.2323

**Level IV Data Package for  
Anchor QEA, LLC  
Gasco PreRD\_DG 2019 4c. Waste Characterization  
Apex Laboratories Work Order #:  
A9K0412**

***The information contained in this Data Package is intended solely for the purpose of validating client sample results submitted under the associated Chain of Custody(ies). An effort has been made to remove all traceable non-client data. Any incidental inclusion of non-client data is considered privileged and confidential information. The use of this information for any purpose other than data validation is strictly prohibited, and constitutes a breach of contract.***

**Table of Contents**  
**A9K0412**  
(page 1 of 2)

**Analytical Case Narrative**  
**Analytical Report**  
**Sample Receipt Documentation**  
(Work orders, Chain of Custody & Cooler Receipt Forms)  
**CLP-Like Forms**  
**Raw Data**

**TCLP Volatile Organic Compounds by EPA 1311/8260C**  
**Benchsheet & Analysis Sequence Data**  
Batch 9110813  
Sequence 9K19033 (A9K0412-01)

**Calibration Data**  
Sequence 9J24043 (Cal ID A9J2503) VOA-GCMS9

**TCLP Organochloride Pesticides by EPA 8081B**  
**Benchsheet & Analysis Sequence Data**  
Batch 9111243  
Sequence 9K27028 (A9K0412-01)

**Calibration Data**  
Sequence 9H23034 (Cal ID A9H2608) DualECD5R

**TCLP Semivolatile Organic Compounds by EPA 8270D**  
**Benchsheet & Analysis Sequence Data**  
Batch 9111242  
Sequence 9K27012 (A9K0412-01RE1)  
Sequence 9K26022 (QC Only)

**Calibration Data**  
Sequence 9I19035 (Cal ID A9I2405) SV-GCMS10

**TCLP Metals by EPA 6020A (ICPMS)**  
**Benchsheet Data and Analysis (Including Calibration)**  
Batch 9111213  
Sequence 9K26027

**Table of Contents**  
**A9K0412**  
(page 2 of 2)

**Metals IFA/IFB Metals Internal Standards Recovery Summary**

A19K340 IFA  
A19K341 IFB  
A9K0412 (I.S Tables)

**Total Solids by SM 2540G**

**Benchsheet Data**

Batch 9110857 (A9K0412-01)

**TCLP Extraction by EPA 1311**

**Benchsheet Data**

Batch 9111146 (A9K0412-01)  
Batch 9110920 (A9K0412-01) (ZHE)

**Balance Checksheets**

Extractions November 2019  
Extractions November 2019  
Dry Weight November 2019  
Wet Chem November 2019  
Metals November 2019  
Sample Rec. November 2019

## **Analytical Case Narrative**

## **Analytical Case Narrative**

Client: Anchor QEA, LLC  
Project: Gasco PreRD\_DG 2019 4c. Waste Characterization  
Apex Work Order Number: A9K0412

Date: 12/24/2019

This data package contains data associated with analysis of samples for the above referenced Apex work order numbers. The data package Table of Contents, along with the PDF bookmarks, allow for ease of navigation and location of items within the data deliverable.

The Sample Receipt Documentation section of this package contains sample receipt information, including sample temperature and condition of receipt documented on Cooler Receipt Form(s). Apex analyzed the samples by the methods indicated on the Chain of Custody. Any additional analyses requested are indicated on the Apex Work Order.

If any anomalies were encountered during analysis that could potentially impact data quality, sample results are qualified and/or a separate Case Narrative is included in the Analytical Report. Please refer to the Notes and Definition section of the Analytical Report(s) for Qualifier explanations, Conventions, and the Blank Policy.

Data represented in this package are in compliance with the referenced method(s), both technically and for completeness, for all conditions other than those stated above and/or noted by qualification of the reported data. The signature below verifies that the Laboratory Director or his designee has authorized release of this data package.



Estella Rieben,  
Quality Systems Manager  
Apex Laboratories, LLC

## **Analytical Report**



Apex Laboratories, LLC

6700 S.W. Sandburg Street  
Tigard, OR 97223  
503-718-2323  
EPA ID: OR01039

Wednesday, December 4, 2019

Ryan Barth  
Anchor QEA, LLC  
6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

RE: A9K0412 - Gasco PreRD DG 2019 - 4c. Waste Characterization - [none]

Thank you for using Apex Laboratories. We greatly appreciate your business and strive to provide the highest quality services to the environmental industry.

Enclosed are the results of analyses for work order A9K0412, which was received by the laboratory on 11/14/2019 at 1:40:00PM.

If you have any questions concerning this report or the services we offer, please feel free to contact me by email at: [dthomas@apex-labs.com](mailto:dthomas@apex-labs.com), or by phone at 503-718-2323.

Please note: All samples will be disposed of within 30 days of sample receipt, unless prior arrangements have been made.

---

Cooler Receipt Information

(See Cooler Receipt Form for details)

Cooler #1                      2.1 degC

---

This Final Report is the official version of the data results for this sample submission, unless superseded by a subsequent, labeled amended report.

All other deliverables derived from this data, including Electronic Data Deliverables (EDDs), CLP-like forms, client requested summary sheets, and all other products are considered secondary to this report.

---



---

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
Tigard, OR 97223  
503-718-2323  
**EPA ID: OR01039**

**Anchor QEA, LLC**

6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: **Gasco PreRD DG 2019 - 4c. Waste Characterization**

Project Number: [none]

Project Manager: **Ryan Barth**

**Report ID:**

**A9K0412 - 12 04 19 1401**

**ANALYTICAL REPORT FOR SAMPLES**

**SAMPLE INFORMATION**

Client Sample ID	Laboratory ID	Matrix	Date Sampled	Date Received
PDI-142RAB-C-00-30.4-191112	A9K0412-01	SO	11/12/19 15:40	11/14/19 13:40

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*

Darwin Thomas, Business Development Director

12/26/19 Anchor QEA, LLC - Gasco PreRD\_DG 2019 -4c. Waste Characterization Page 8 of 919





<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**ANALYTICAL SAMPLE RESULTS**

**TCLP Volatile Organic Compounds by EPA 1311/8260C**

Analyte	Sample Result	Detection Limit	Reporting Limit	Units	Dilution	Date Analyzed	Method Ref.	Notes
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01)</b>				<b>Matrix: SO</b>		<b>Batch: 9110813</b>		
Benzene	ND	0.00625	0.0125	mg/L	50	11/19/19 13:21	1311/8260C	
2-Butanone (MEK)	ND	0.250	0.500	mg/L	50	11/19/19 13:21	1311/8260C	
Carbon tetrachloride	ND	0.0250	0.0500	mg/L	50	11/19/19 13:21	1311/8260C	
Chlorobenzene	ND	0.0125	0.0250	mg/L	50	11/19/19 13:21	1311/8260C	
Chloroform	ND	0.0250	0.0500	mg/L	50	11/19/19 13:21	1311/8260C	
1,4-Dichlorobenzene	ND	0.0125	0.0250	mg/L	50	11/19/19 13:21	1311/8260C	
1,2-Dichloroethane (EDC)	ND	0.0125	0.0250	mg/L	50	11/19/19 13:21	1311/8260C	
1,1-Dichloroethene	ND	0.0125	0.0250	mg/L	50	11/19/19 13:21	1311/8260C	
Tetrachloroethene (PCE)	ND	0.0125	0.0250	mg/L	50	11/19/19 13:21	1311/8260C	
Trichloroethene (TCE)	ND	0.0125	0.0250	mg/L	50	11/19/19 13:21	1311/8260C	
Vinyl chloride	ND	0.0125	0.0250	mg/L	50	11/19/19 13:21	1311/8260C	
<i>Surrogate: 1,4-Difluorobenzene (Surr)</i>		<i>Recovery: 119 %</i>		<i>Limits: 80-120 %</i>		<i>1</i>	<i>11/19/19 13:21</i>	<i>1311/8260C</i>
<i>Toluene-d8 (Surr)</i>		<i>102 %</i>		<i>80-120 %</i>		<i>1</i>	<i>11/19/19 13:21</i>	<i>1311/8260C</i>
<i>4-Bromofluorobenzene (Surr)</i>		<i>101 %</i>		<i>80-120 %</i>		<i>1</i>	<i>11/19/19 13:21</i>	<i>1311/8260C</i>

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
 Tigard, OR 97223  
 503-718-2323  
 EPA ID: OR01039

<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**ANALYTICAL SAMPLE RESULTS**

**TCLP Organochlorine Pesticides by EPA 1311/8081B**

Analyte	Sample Result	Detection Limit	Reporting Limit	Units	Dilution	Date Analyzed	Method Ref.	Notes
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01)</b>				<b>Matrix: SO</b>		<b>Batch: 9111243</b>		
gamma-BHC (Lindane)	ND	0.0000750	0.000150	mg/L	1	11/27/19 15:24	1311/8081B	
Endrin	ND	0.0000750	0.000150	mg/L	1	11/27/19 15:24	1311/8081B	
Heptachlor	ND	0.0000750	0.000150	mg/L	1	11/27/19 15:24	1311/8081B	
Heptachlor epoxide	ND	0.0000750	0.000150	mg/L	1	11/27/19 15:24	1311/8081B	
Methoxychlor	ND	0.000200	0.000400	mg/L	1	11/27/19 15:24	1311/8081B	
Chlordane (Technical)	ND	0.000940	0.00188	mg/L	1	11/27/19 15:24	1311/8081B	
Toxaphene (Total)	ND	0.00250	0.00500	mg/L	1	11/27/19 15:24	1311/8081B	
<i>Surrogate: 2,4,5,6-TCMX (Surr)</i>		<i>Recovery: 72 %</i>		<i>Limits: 25-140 %</i>		<i>1</i>	<i>11/27/19 15:24</i>	<i>1311/8081B</i>
<i>Decachlorobiphenyl (Surr)</i>		<i>90 %</i>		<i>30-135 %</i>		<i>1</i>	<i>11/27/19 15:24</i>	<i>1311/8081B</i>

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**ANALYTICAL SAMPLE RESULTS**

**TCLP Semivolatile Organic Compounds by EPA 1311/8270D**

Analyte	Sample Result	Detection Limit	Reporting Limit	Units	Dilution	Date Analyzed	Method Ref.	Notes
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01RE1)</b>				<b>Matrix: SO</b>		<b>Batch: 9111242</b>		
2,4-Dinitrotoluene	ND	0.0100	0.0200	mg/L	10	11/27/19 15:20	1311/8270D	
Hexachlorobenzene	ND	0.0100	0.0200	mg/L	10	11/27/19 15:20	1311/8270D	
Hexachlorobutadiene	ND	0.0250	0.0500	mg/L	10	11/27/19 15:20	1311/8270D	
Hexachloroethane	ND	0.0250	0.0500	mg/L	10	11/27/19 15:20	1311/8270D	
2-Methylphenol	ND	0.0250	0.0500	mg/L	10	11/27/19 15:20	1311/8270D	
3+4-Methylphenol(s)	ND	0.0250	0.0500	mg/L	10	11/27/19 15:20	1311/8270D	
Nitrobenzene	ND	0.0250	0.0500	mg/L	10	11/27/19 15:20	1311/8270D	
Pentachlorophenol (PCP)	ND	0.0500	0.100	mg/L	10	11/27/19 15:20	1311/8270D	
Pyridine	ND	0.0500	0.100	mg/L	10	11/27/19 15:20	1311/8270D	
2,4,5-Trichlorophenol	ND	0.0250	0.0500	mg/L	10	11/27/19 15:20	1311/8270D	
2,4,6-Trichlorophenol	ND	0.0250	0.0500	mg/L	10	11/27/19 15:20	1311/8270D	
<i>Surrogate: Nitrobenzene-d5 (Surr)</i>		<i>Recovery: 75 %</i>		<i>Limits: 44-120 %</i>		<i>10</i>	<i>11/27/19 15:20</i>	<i>1311/8270D</i>
<i>2-Fluorobiphenyl (Surr)</i>		<i>91 %</i>		<i>44-120 %</i>		<i>10</i>	<i>11/27/19 15:20</i>	<i>1311/8270D</i>
<i>Phenol-d6 (Surr)</i>		<i>19 %</i>		<i>10-120 %</i>		<i>10</i>	<i>11/27/19 15:20</i>	<i>1311/8270D</i>
<i>p-Terphenyl-d14 (Surr)</i>		<i>107 %</i>		<i>50-133 %</i>		<i>10</i>	<i>11/27/19 15:20</i>	<i>1311/8270D</i>
<i>2-Fluorophenol (Surr)</i>		<i>40 %</i>		<i>19-120 %</i>		<i>10</i>	<i>11/27/19 15:20</i>	<i>1311/8270D</i>
<i>2,4,6-Tribromophenol (Surr)</i>		<i>89 %</i>		<i>43-140 %</i>		<i>10</i>	<i>11/27/19 15:20</i>	<i>1311/8270D</i>

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
 Tigard, OR 97223  
 503-718-2323  
 EPA ID: OR01039

<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**ANALYTICAL SAMPLE RESULTS**

**TCLP Metals by EPA 6020A (ICPMS)**

Analyte	Sample Result	Detection Limit	Reporting Limit	Units	Dilution	Date Analyzed	Method Ref.	Notes
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01)</b>				<b>Matrix: SO</b>				
Batch: 9111213								
Arsenic	ND	0.0500	0.100	mg/L	10	11/26/19 14:05	1311/6020A	
Barium	ND	2.50	5.00	mg/L	10	11/26/19 14:05	1311/6020A	
Cadmium	ND	0.0500	0.100	mg/L	10	11/26/19 14:05	1311/6020A	
Chromium	ND	0.0500	0.100	mg/L	10	11/26/19 14:05	1311/6020A	
Lead	ND	0.0250	0.0500	mg/L	10	11/26/19 14:05	1311/6020A	
Mercury	ND	0.00350	0.00700	mg/L	10	11/26/19 14:05	1311/6020A	
Selenium	ND	0.0500	0.100	mg/L	10	11/26/19 14:05	1311/6020A	
Silver	ND	0.0500	0.100	mg/L	10	11/26/19 14:05	1311/6020A	

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
 Tigard, OR 97223  
 503-718-2323  
 EPA ID: OR01039

<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**ANALYTICAL SAMPLE RESULTS**

**Solid and Moisture Determinations**

Analyte	Sample Result	Detection Limit	Reporting Limit	Units	Dilution	Date Analyzed	Method Ref.	Notes
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01)</b>				<b>Matrix: SO</b>				
Batch: 9110857								
<b>Total Solids</b>	<b>92.5</b>	1.00	1.00	% by Weight	1	11/16/19 11:44	SM 2540 G	

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
 Tigard, OR 97223  
 503-718-2323  
 EPA ID: OR01039

<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**ANALYTICAL SAMPLE RESULTS**

**TCLP Extraction by EPA 1311 (ZHE)**

Analyte	Sample Result	Detection Limit	Reporting Limit	Units	Dilution	Date Analyzed	Method Ref.	Notes
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01)</b>				<b>Matrix: SO</b>		<b>Batch: 9110920</b>		
TCLP ZHE Extraction	PREP	---		N/A	1	11/18/19 15:55	EPA 1311 ZHE	
TCLP Extraction	PREP	---		N/A	1	11/25/19 16:40	EPA 1311	
TCLP Extraction	PREP	---		N/A	1	11/25/19 16:40	EPA 1311	

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Anchor QEA, LLC**  
6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: **Gasco PreRD DG 2019 - 4c. Waste Characterization**  
Project Number: [none]  
Project Manager: **Ryan Barth**

**Report ID:**  
A9K0412 - 12 04 19 1401

**QUALITY CONTROL (QC) SAMPLE RESULTS**

**TCLP Volatile Organic Compounds by EPA 1311/8260C**

Analyte	Result	Detection Limit	Reporting Limit	Units	Dilution	Spike Amount	Source Result	% REC	% REC Limits	RPD	RPD Limit	Notes
<b>Batch 9110813 - EPA 1311/5030B TCLP Volatiles</b>						<b>Water</b>						
<b>Blank (9110813-BLK1)</b>						Prepared: 11/19/19 09:00 Analyzed: 11/19/19 12:00						<b>TCLP</b>
<b>1311/8260C</b>												
Benzene	ND	0.00625	0.0125	mg/L	50	---	---	---	---	---	---	
2-Butanone (MEK)	ND	0.250	0.500	mg/L	50	---	---	---	---	---	---	
Carbon tetrachloride	ND	0.0250	0.0500	mg/L	50	---	---	---	---	---	---	
Chlorobenzene	ND	0.0125	0.0250	mg/L	50	---	---	---	---	---	---	
Chloroform	ND	0.0250	0.0500	mg/L	50	---	---	---	---	---	---	
1,4-Dichlorobenzene	ND	0.0125	0.0250	mg/L	50	---	---	---	---	---	---	
1,2-Dichloroethane (EDC)	ND	0.0125	0.0250	mg/L	50	---	---	---	---	---	---	
1,1-Dichloroethene	ND	0.0125	0.0250	mg/L	50	---	---	---	---	---	---	
Tetrachloroethene (PCE)	ND	0.0125	0.0250	mg/L	50	---	---	---	---	---	---	
Trichloroethene (TCE)	ND	0.0125	0.0250	mg/L	50	---	---	---	---	---	---	
Vinyl chloride	ND	0.0125	0.0250	mg/L	50	---	---	---	---	---	---	
<i>Surr: 1,4-Difluorobenzene (Surr)</i>		<i>Recovery: 121 %</i>		<i>Limits: 80-120 %</i>		<i>Dilution: 1x</i>				<i>S-06</i>		
<i>Toluene-d8 (Surr)</i>		<i>103 %</i>		<i>80-120 %</i>		<i>"</i>						
<i>4-Bromofluorobenzene (Surr)</i>		<i>102 %</i>		<i>80-120 %</i>		<i>"</i>						

<b>LCS (9110813-BS1)</b>						Prepared: 11/19/19 09:00 Analyzed: 11/19/19 11:33						<b>TCLP</b>
<b>1311/8260C</b>												
Benzene	1.07	0.00625	0.0125	mg/L	50	1.00	---	107	80-120%	---	---	
2-Butanone (MEK)	1.94	0.250	0.500	mg/L	50	2.00	---	97	80-120%	---	---	
Carbon tetrachloride	1.20	0.0250	0.0500	mg/L	50	1.00	---	120	80-120%	---	---	
Chlorobenzene	1.03	0.0125	0.0250	mg/L	50	1.00	---	103	80-120%	---	---	
Chloroform	1.10	0.0250	0.0500	mg/L	50	1.00	---	110	80-120%	---	---	
1,4-Dichlorobenzene	1.00	0.0125	0.0250	mg/L	50	1.00	---	100	80-120%	---	---	
1,2-Dichloroethane (EDC)	0.962	0.0125	0.0250	mg/L	50	1.00	---	96	80-120%	---	---	
1,1-Dichloroethene	1.04	0.0125	0.0250	mg/L	50	1.00	---	104	80-120%	---	---	
Tetrachloroethene (PCE)	1.09	0.0125	0.0250	mg/L	50	1.00	---	109	80-120%	---	---	
Trichloroethene (TCE)	1.15	0.0125	0.0250	mg/L	50	1.00	---	115	80-120%	---	---	
Vinyl chloride	1.02	0.0125	0.0250	mg/L	50	1.00	---	102	80-120%	---	---	
<i>Surr: 1,4-Difluorobenzene (Surr)</i>		<i>Recovery: 107 %</i>		<i>Limits: 80-120 %</i>		<i>Dilution: 1x</i>						
<i>Toluene-d8 (Surr)</i>		<i>98 %</i>		<i>80-120 %</i>		<i>"</i>						
<i>4-Bromofluorobenzene (Surr)</i>		<i>98 %</i>		<i>80-120 %</i>		<i>"</i>						

**Duplicate (9110813-DUP1)** Prepared: 11/19/19 12:00 Analyzed: 11/19/19 12:54

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Anchor QEA, LLC**

6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: **Gasco PreRD DG 2019 - 4c. Waste Characterization**

Project Number: [none]  
Project Manager: Ryan Barth

**Report ID:**  
A9K0412 - 12 04 19 1401

**QUALITY CONTROL (QC) SAMPLE RESULTS**

**TCLP Volatile Organic Compounds by EPA 1311/8260C**

Analyte	Result	Detection Limit	Reporting Limit	Units	Dilution	Spike Amount	Source Result	% REC	% REC Limits	RPD	RPD Limit	Notes
<b>Batch 9110813 - EPA 1311/5030B TCLP Volatiles</b>												
<b>Water</b>												
<b>Duplicate (9110813-DUP1)</b>												
Prepared: 11/19/19 12:00 Analyzed: 11/19/19 12:54												
<b>QC Source Sample: Non-SDG (A9K0403-01)</b>												
Benzene	ND	0.00625	0.0125	mg/L	50	---	ND	---	---	---	30%	
2-Butanone (MEK)	ND	0.250	0.500	mg/L	50	---	ND	---	---	---	30%	
Carbon tetrachloride	ND	0.0250	0.0500	mg/L	50	---	ND	---	---	---	30%	
Chlorobenzene	ND	0.0125	0.0250	mg/L	50	---	ND	---	---	---	30%	
Chloroform	ND	0.0250	0.0500	mg/L	50	---	ND	---	---	---	30%	
1,4-Dichlorobenzene	ND	0.0125	0.0250	mg/L	50	---	ND	---	---	---	30%	
1,2-Dichloroethane (EDC)	ND	0.0125	0.0250	mg/L	50	---	ND	---	---	---	30%	
1,1-Dichloroethene	ND	0.0125	0.0250	mg/L	50	---	ND	---	---	---	30%	
Tetrachloroethene (PCE)	ND	0.0125	0.0250	mg/L	50	---	ND	---	---	---	30%	
Trichloroethene (TCE)	ND	0.0125	0.0250	mg/L	50	---	ND	---	---	---	30%	
Vinyl chloride	ND	0.0125	0.0250	mg/L	50	---	ND	---	---	---	30%	
Surr: 1,4-Difluorobenzene (Surr) Recovery: 121 % Limits: 80-120 % Dilution: 1x												S-06
Toluene-d8 (Surr) Recovery: 102 % Limits: 80-120 % Dilution: "												
4-Bromofluorobenzene (Surr) Recovery: 101 % Limits: 80-120 % Dilution: "												

<b>Matrix Spike (9110813-MS1)</b>												
Prepared: 11/19/19 12:00 Analyzed: 11/19/19 13:48												
<b>QC Source Sample: PDI-142RAB-C-00-30.4-191112 (A9K0412-01)</b>												
<b>1311/8260C</b>												
Benzene	1.18	0.00625	0.0125	mg/L	50	1.00	ND	118	70-130%	---	---	
2-Butanone (MEK)	2.06	0.250	0.500	mg/L	50	2.00	ND	103	70-130%	---	---	
Carbon tetrachloride	0.970	0.0250	0.0500	mg/L	50	1.00	ND	97	70-130%	---	---	
Chlorobenzene	1.08	0.0125	0.0250	mg/L	50	1.00	ND	108	70-130%	---	---	
Chloroform	1.01	0.0250	0.0500	mg/L	50	1.00	ND	101	70-130%	---	---	
1,4-Dichlorobenzene	1.01	0.0125	0.0250	mg/L	50	1.00	ND	101	70-130%	---	---	
1,2-Dichloroethane (EDC)	0.867	0.0125	0.0250	mg/L	50	1.00	ND	87	70-130%	---	---	
1,1-Dichloroethene	0.973	0.0125	0.0250	mg/L	50	1.00	ND	97	70-130%	---	---	
Tetrachloroethene (PCE)	1.15	0.0125	0.0250	mg/L	50	1.00	ND	115	70-130%	---	---	
Trichloroethene (TCE)	1.30	0.0125	0.0250	mg/L	50	1.00	ND	130	70-130%	---	---	
Vinyl chloride	1.08	0.0125	0.0250	mg/L	50	1.00	ND	108	70-130%	---	---	
Surr: 1,4-Difluorobenzene (Surr) Recovery: 119 % Limits: 80-120 % Dilution: 1x												
Toluene-d8 (Surr) Recovery: 99 % Limits: 80-120 % Dilution: "												
4-Bromofluorobenzene (Surr) Recovery: 97 % Limits: 80-120 % Dilution: "												

Apex Laboratories

The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.





<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**QUALITY CONTROL (QC) SAMPLE RESULTS**

**TCLP Organochlorine Pesticides by EPA 1311/8081B**

Analyte	Result	Detection Limit	Reporting Limit	Units	Dilution	Spike Amount	Source Result	% REC	% REC Limits	RPD	RPD Limit	Notes
<b>Batch 9111243 - EPA 1311/3510C (Neutral Ext.)</b>												
<b>Soil</b>												
<b>Blank (9111243-BLK1)</b>												
Prepared: 11/26/19 14:06 Analyzed: 11/27/19 14:32												
<b>1311/8081B</b>												
gamma-BHC (Lindane)	ND	0.0000750	0.000150	mg/L	1	---	---	---	---	---	---	
Endrin	ND	0.0000750	0.000150	mg/L	1	---	---	---	---	---	---	
Heptachlor	ND	0.0000750	0.000150	mg/L	1	---	---	---	---	---	---	
Heptachlor epoxide	ND	0.0000750	0.000150	mg/L	1	---	---	---	---	---	---	
Methoxychlor	ND	0.000200	0.000400	mg/L	1	---	---	---	---	---	---	
Chlordane (Technical)	ND	0.000940	0.00188	mg/L	1	---	---	---	---	---	---	
Toxaphene (Total)	ND	0.00250	0.00500	mg/L	1	---	---	---	---	---	---	
<i>Surr: 2,4,5,6-TCMX (Surr) Recovery: 77 % Limits: 25-140 % Dilution: 1x</i>												
<i>Decachlorobiphenyl (Surr) 95 % 30-135 % "</i>												
<b>LCS (9111243-BS1)</b>												
Prepared: 11/26/19 14:06 Analyzed: 11/27/19 14:49												
<b>1311/8081B</b>												
gamma-BHC (Lindane)	0.00226	0.0000750	0.000150	mg/L	1	0.00250	---	91	59-134%	---	---	
Endrin	0.00245	0.0000750	0.000150	mg/L	1	0.00250	---	98	60-138%	---	---	
Heptachlor	0.00208	0.0000750	0.000150	mg/L	1	0.00250	---	83	54-130%	---	---	
Heptachlor epoxide	0.00223	0.0000750	0.000150	mg/L	1	0.00250	---	89	61-133%	---	---	
Methoxychlor	0.00246	0.000200	0.000400	mg/L	1	0.00250	---	98	54-144%	---	---	
<i>Surr: 2,4,5,6-TCMX (Surr) Recovery: 79 % Limits: 25-140 % Dilution: 1x</i>												
<i>Decachlorobiphenyl (Surr) 94 % 30-135 % "</i>												
<b>LCS Dup (9111243-BSD1)</b>												
Prepared: 11/26/19 14:06 Analyzed: 11/27/19 15:07												
<b>1311/8081B</b>												
gamma-BHC (Lindane)	0.00214	0.0000750	0.000150	mg/L	1	0.00250	---	86	59-134%	6	30%	
Endrin	0.00232	0.0000750	0.000150	mg/L	1	0.00250	---	93	60-138%	6	30%	
Heptachlor	0.00191	0.0000750	0.000150	mg/L	1	0.00250	---	76	54-130%	9	30%	
Heptachlor epoxide	0.00211	0.0000750	0.000150	mg/L	1	0.00250	---	84	61-133%	6	30%	
Methoxychlor	0.00231	0.000200	0.000400	mg/L	1	0.00250	---	92	54-144%	6	30%	
<i>Surr: 2,4,5,6-TCMX (Surr) Recovery: 75 % Limits: 25-140 % Dilution: 1x</i>												
<i>Decachlorobiphenyl (Surr) 81 % 30-135 % "</i>												

Apex Laboratories

The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.



<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: Ryan Barth	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	---	--

**QUALITY CONTROL (QC) SAMPLE RESULTS**

**TCLP Semivolatile Organic Compounds by EPA 1311/8270D**

Analyte	Result	Detection Limit	Reporting Limit	Units	Dilution	Spike Amount	Source Result	% REC	% REC Limits	RPD	RPD Limit	Notes
<b>Batch 9111242 - EPA 1311/3510C (BNA Extraction) Soil</b>												
<b>Blank (9111242-BLK1)</b> Prepared: 11/26/19 14:05 Analyzed: 11/26/19 18:39												
<u>1311/8270D</u>												
2,4-Dinitrotoluene	ND	0.00100	0.00200	mg/L	1	---	---	---	---	---	---	
Hexachlorobenzene	ND	0.00100	0.00200	mg/L	1	---	---	---	---	---	---	
Hexachlorobutadiene	ND	0.00250	0.00500	mg/L	1	---	---	---	---	---	---	
Hexachloroethane	ND	0.00250	0.00500	mg/L	1	---	---	---	---	---	---	
2-Methylphenol	ND	0.00250	0.00500	mg/L	1	---	---	---	---	---	---	
3+4-Methylphenol(s)	ND	0.00250	0.00500	mg/L	1	---	---	---	---	---	---	
Nitrobenzene	ND	0.00250	0.00500	mg/L	1	---	---	---	---	---	---	
Pentachlorophenol (PCP)	ND	0.00500	0.0100	mg/L	1	---	---	---	---	---	---	
Pyridine	ND	0.00500	0.0100	mg/L	1	---	---	---	---	---	---	
2,4,5-Trichlorophenol	ND	0.00250	0.00500	mg/L	1	---	---	---	---	---	---	
2,4,6-Trichlorophenol	ND	0.00250	0.00500	mg/L	1	---	---	---	---	---	---	
<i>Surr: Nitrobenzene-d5 (Surr) Recovery: 56 % Limits: 44-120 % Dilution: 1x</i>												
<i>2-Fluorobiphenyl (Surr) 60 % 44-120 % "</i>												
<i>Phenol-d6 (Surr) 18 % 10-120 % "</i>												
<i>p-Terphenyl-d14 (Surr) 79 % 50-133 % "</i>												
<i>2-Fluorophenol (Surr) 34 % 19-120 % "</i>												
<i>2,4,6-Tribromophenol (Surr) 76 % 43-140 % "</i>												

<b>LCS (9111242-BS1)</b> Prepared: 11/26/19 14:05 Analyzed: 11/26/19 19:16												
<u>1311/8270D</u>												
2,4-Dinitrotoluene	0.0368	0.00400	0.00800	mg/L	4	0.0400	---	92	57-128%	---	---	
Hexachlorobenzene	0.0336	0.00400	0.00800	mg/L	4	0.0400	---	84	52-125%	---	---	
Hexachlorobutadiene	0.0313	0.0100	0.0200	mg/L	4	0.0400	---	78	22-124%	---	---	
Hexachloroethane	0.0314	0.0100	0.0200	mg/L	4	0.0400	---	78	21-120%	---	---	
2-Methylphenol	0.0275	0.0100	0.0200	mg/L	4	0.0400	---	69	30-120%	---	---	
3+4-Methylphenol(s)	0.0250	0.0100	0.0200	mg/L	4	0.0400	---	63	29-120%	---	---	
Nitrobenzene	0.0284	0.0100	0.0200	mg/L	4	0.0400	---	71	45-121%	---	---	
Pentachlorophenol (PCP)	0.0332	0.0200	0.0200	mg/L	4	0.0400	---	83	35-138%	---	---	
Pyridine	0.0139	0.000400	0.000400	mg/L	4	0.0400	---	35	5-120%	---	---	
2,4,5-Trichlorophenol	0.0384	0.0100	0.0200	mg/L	4	0.0400	---	96	53-123%	---	---	
2,4,6-Trichlorophenol	0.0370	0.0100	0.0200	mg/L	4	0.0400	---	92	50-125%	---	---	
<i>Surr: Nitrobenzene-d5 (Surr) Recovery: 73 % Limits: 44-120 % Dilution: 4x</i>												
<i>2-Fluorobiphenyl (Surr) 83 % 44-120 % "</i>												

Apex Laboratories

The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.



**Anchor QEA, LLC**  
6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: **Gasco PreRD DG 2019 - 4c. Waste Characterization**  
Project Number: [none]  
Project Manager: **Ryan Barth**

**Report ID:**  
A9K0412 - 12 04 19 1401

**QUALITY CONTROL (QC) SAMPLE RESULTS**

**TCLP Semivolatile Organic Compounds by EPA 1311/8270D**

Analyte	Result	Detection Limit	Reporting Limit	Units	Dilution	Spike Amount	Source Result	% REC	% REC Limits	RPD	RPD Limit	Notes
<b>Batch 9111242 - EPA 1311/3510C (BNA Extraction)</b>												
<b>Soil</b>												
<b>LCS (9111242-BS1)</b>												
Prepared: 11/26/19 14:05 Analyzed: 11/26/19 19:16												
<i>Surr: Phenol-d6 (Surr)</i>			Recovery: 27 %	Limits: 10-120 %		Dilution: 4x						
<i>p-Terphenyl-d14 (Surr)</i>			89 %	50-133 %		"						
<i>2-Fluorophenol (Surr)</i>			44 %	19-120 %		"						
<i>2,4,6-Tribromophenol (Surr)</i>			84 %	43-140 %		"						
<b>LCS Dup (9111242-BSD1)</b>												
Prepared: 11/26/19 14:05 Analyzed: 11/26/19 19:52												
<b>Q-19</b>												
<b>1311/8270D</b>												
2,4-Dinitrotoluene	0.0363	0.00400	0.00800	mg/L	4	0.0400	---	91	57-128%	1	30%	
Hexachlorobenzene	0.0340	0.00400	0.00800	mg/L	4	0.0400	---	85	52-125%	1	30%	
Hexachlorobutadiene	0.0305	0.0100	0.0200	mg/L	4	0.0400	---	76	22-124%	3	30%	
Hexachloroethane	0.0291	0.0100	0.0200	mg/L	4	0.0400	---	73	21-120%	8	30%	
2-Methylphenol	0.0264	0.0100	0.0200	mg/L	4	0.0400	---	66	30-120%	4	30%	
3+4-Methylphenol(s)	0.0240	0.0100	0.0200	mg/L	4	0.0400	---	60	29-120%	4	30%	
Nitrobenzene	0.0281	0.0100	0.0200	mg/L	4	0.0400	---	70	45-121%	1	30%	
Pentachlorophenol (PCP)	0.0337	0.0200	0.0200	mg/L	4	0.0400	---	84	35-138%	1	30%	
Pyridine	0.0125	0.000400	0.000400	mg/L	4	0.0400	---	31	5-120%	10	30%	
2,4,5-Trichlorophenol	0.0368	0.0100	0.0200	mg/L	4	0.0400	---	92	53-123%	4	30%	
2,4,6-Trichlorophenol	0.0369	0.0100	0.0200	mg/L	4	0.0400	---	92	50-125%	0.2	30%	
<i>Surr: Nitrobenzene-d5 (Surr)</i>			Recovery: 70 %	Limits: 44-120 %		Dilution: 4x						
<i>2-Fluorobiphenyl (Surr)</i>			81 %	44-120 %		"						
<i>Phenol-d6 (Surr)</i>			24 %	10-120 %		"						
<i>p-Terphenyl-d14 (Surr)</i>			91 %	50-133 %		"						
<i>2-Fluorophenol (Surr)</i>			41 %	19-120 %		"						
<i>2,4,6-Tribromophenol (Surr)</i>			83 %	43-140 %		"						

Apex Laboratories

The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.



<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**QUALITY CONTROL (QC) SAMPLE RESULTS**

**TCLP Metals by EPA 6020A (ICPMS)**

Analyte	Result	Detection Limit	Reporting Limit	Units	Dilution	Spike Amount	Source Result	% REC	% REC Limits	RPD	RPD Limit	Notes
<b>Batch 9111213 - EPA 1311/3015</b>												
<b>Soil</b>												
<b>Blank (9111213-BLK1)</b> Prepared: 11/26/19 09:55 Analyzed: 11/26/19 13:56												
<u>1311/6020A</u>												
Arsenic	ND	0.0500	0.100	mg/L	10	---	---	---	---	---	---	TCLPa
Barium	ND	2.50	5.00	mg/L	10	---	---	---	---	---	---	TCLPa
Cadmium	ND	0.0500	0.100	mg/L	10	---	---	---	---	---	---	TCLPa
Chromium	ND	0.0500	0.100	mg/L	10	---	---	---	---	---	---	TCLPa
Lead	ND	0.0250	0.0500	mg/L	10	---	---	---	---	---	---	TCLPa
Mercury	ND	0.00350	0.00700	mg/L	10	---	---	---	---	---	---	TCLPa
Selenium	ND	0.0500	0.100	mg/L	10	---	---	---	---	---	---	TCLPa
Silver	ND	0.0500	0.100	mg/L	10	---	---	---	---	---	---	TCLPa
<b>LCS (9111213-BS1)</b> Prepared: 11/26/19 09:55 Analyzed: 11/26/19 14:01												
<u>1311/6020A</u>												
Arsenic	5.09	0.0500	0.100	mg/L	10	5.00	---	102	80-120%	---	---	TCLPa
Barium	10.6	2.50	5.00	mg/L	10	10.0	---	106	80-120%	---	---	TCLPa
Cadmium	1.04	0.0500	0.100	mg/L	10	1.00	---	104	80-120%	---	---	TCLPa
Chromium	4.92	0.0500	0.100	mg/L	10	5.00	---	98	80-120%	---	---	TCLPa
Lead	5.13	0.0250	0.0500	mg/L	10	5.00	---	103	80-120%	---	---	TCLPa
Mercury	0.107	0.00350	0.00700	mg/L	10	0.100	---	107	80-120%	---	---	TCLPa
Selenium	1.00	0.0500	0.100	mg/L	10	1.00	---	100	80-120%	---	---	TCLPa
Silver	1.06	0.0500	0.100	mg/L	10	1.00	---	106	80-120%	---	---	TCLPa
<b>Matrix Spike (9111213-MS1)</b> Prepared: 11/26/19 09:55 Analyzed: 11/26/19 14:10												
<u>QC Source Sample: PDI-142RAB-C-00-30.4-191112 (A9K0412-01)</u>												
<u>1311/6020A</u>												
Arsenic	4.95	0.0500	0.100	mg/L	10	5.00	ND	99	50-150%	---	---	
Barium	10.5	2.50	5.00	mg/L	10	10.0	ND	105	50-150%	---	---	
Cadmium	1.01	0.0500	0.100	mg/L	10	1.00	ND	101	50-150%	---	---	
Chromium	4.77	0.0500	0.100	mg/L	10	5.00	ND	95	50-150%	---	---	
Lead	4.96	0.0250	0.0500	mg/L	10	5.00	ND	99	50-150%	---	---	
Mercury	0.102	0.00350	0.00700	mg/L	10	0.100	ND	102	50-150%	---	---	
Selenium	0.978	0.0500	0.100	mg/L	10	1.00	ND	98	50-150%	---	---	
Silver	1.03	0.0500	0.100	mg/L	10	1.00	ND	103	50-150%	---	---	

Apex Laboratories

The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
 Tigard, OR 97223  
 503-718-2323  
 EPA ID: OR01039

<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**QUALITY CONTROL (QC) SAMPLE RESULTS**

**Solid and Moisture Determinations**

Analyte	Result	Detection Limit	Reporting Limit	Units	Dilution	Spike Amount	Source Result	% REC	% REC Limits	RPD	RPD Limit	Notes
<b>Batch 9110857 - Total Solids (SM2540G/PSEP)</b>						<b>Sediment</b>						
<b>Duplicate (9110857-DUP1)</b>						Prepared: 11/15/19 11:24 Analyzed: 11/16/19 11:44						
<u>QC Source Sample: PDI-142RAB-C-00-30.4-191112 (A9K0412-01)</u>												
<u>SM 2540 G</u>												
Total Solids	92.3	1.00	1.00	% by Weight	1	---	92.5	---	---	0.2	10%	

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Anchor QEA, LLC**  
6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: **Gasco PreRD DG 2019 - 4c. Waste Characterization**  
Project Number: [none]  
Project Manager: **Ryan Barth**

**Report ID:**  
**A9K0412 - 12 04 19 1401**

**SAMPLE PREPARATION INFORMATION**

**TCLP Volatile Organic Compounds by EPA 1311/8260C**

Prep: EPA 1311/5030B TCLP Volatiles

Lab Number	Matrix	Method	Sampled	Prepared	Sample Initial/Final	Default Initial/Final	RL Prep Factor
Batch: 9110813							
A9K0412-01	SO	1311/8260C	11/12/19 15:40	11/19/19 12:00	5mL/5mL	5mL/5mL	1.00

**TCLP Organochlorine Pesticides by EPA 1311/8081B**

Prep: EPA 1311/3510C (Neutral Ext.)

Lab Number	Matrix	Method	Sampled	Prepared	Sample Initial/Final	Default Initial/Final	RL Prep Factor
Batch: 9111243							
A9K0412-01	SO	1311/8081B	11/12/19 15:40	11/26/19 14:06	200mL/5mL	200mL/5mL	1.00

**TCLP Semivolatile Organic Compounds by EPA 1311/8270D**

Prep: EPA 1311/3510C (BNA Extraction)

Lab Number	Matrix	Method	Sampled	Prepared	Sample Initial/Final	Default Initial/Final	RL Prep Factor
Batch: 9111242							
A9K0412-01RE1	SO	1311/8270D	11/12/19 15:40	11/26/19 14:05	200mL/2mL	200mL/2mL	1.00

**TCLP Metals by EPA 6020A (ICPMS)**

Prep: EPA 1311/3015

Lab Number	Matrix	Method	Sampled	Prepared	Sample Initial/Final	Default Initial/Final	RL Prep Factor
Batch: 9111213							
A9K0412-01	SO	1311/6020A	11/12/19 15:40	11/26/19 09:55	10mL/50mL	10mL/50mL	1.00

**Solid and Moisture Determinations**

Prep: Total Solids (SM2540G/PSEP)

Lab Number	Matrix	Method	Sampled	Prepared	Sample Initial/Final	Default Initial/Final	RL Prep Factor
Batch: 9110857							
A9K0412-01	SO	SM 2540 G	11/12/19 15:40	11/15/19 11:24			NA

**TCLP Extraction by EPA 1311**

Prep: EPA 1311 (TCLP)

Lab Number	Matrix	Method	Sampled	Prepared	Sample Initial/Final	Default Initial/Final	RL Prep Factor
Batch: 9111146							
A9K0412-01	SO	EPA 1311	11/12/19 15:40	11/25/19 16:40	100g/2000mL	100g/2000mL	NA

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
 Tigard, OR 97223  
 503-718-2323  
 EPA ID: OR01039

<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**SAMPLE PREPARATION INFORMATION**

**TCLP Extraction by EPA 1311**

Prep: EPA 1311 (TCLP)

Lab Number	Matrix	Method	Sampled	Prepared	Sample Initial/Final	Default Initial/Final	RL Prep Factor
------------	--------	--------	---------	----------	----------------------	-----------------------	----------------

Prep: EPA 1311 TCLP/ZHE

Lab Number	Matrix	Method	Sampled	Prepared	Sample Initial/Final	Default Initial/Final	RL Prep Factor
------------	--------	--------	---------	----------	----------------------	-----------------------	----------------

Batch: 9110920

A9K0412-01	SO	EPA 1311 ZHE	11/12/19 15:40	11/18/19 15:55	25g/500mL	25g/500mL	NA
------------	----	--------------	----------------	----------------	-----------	-----------	----

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
Tigard, OR 97223  
503-718-2323  
**EPA ID: OR01039**

**Anchor QEA, LLC**

6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: **Gasco PreRD DG 2019 - 4c. Waste Characterization**

Project Number: [none]

Project Manager: **Ryan Barth**

**Report ID:**

**A9K0412 - 12 04 19 1401**

**QUALIFIER DEFINITIONS**

**Client Sample and Quality Control (QC) Sample Qualifier Definitions:**

**Apex Laboratories**

- Q-19** Blank Spike Duplicate (BSD) sample analyzed in place of Matrix Spike/Duplicate samples due to limited sample amount available for analysis.
- S-06** Surrogate recovery is outside of established control limits.
- TCLP** This batch QC sample was prepared with TCLP or SPLP fluid from preparation batch 9110920.
- TCLPa** This batch QC sample was prepared with TCLP or SPLP fluid from preparation batch 9111146.

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*





Anchor QEA, LLC

6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Project Number: [none]

Project Manager: Ryan Barth

Report ID:

A9K0412 - 12 04 19 1401

**REPORTING NOTES AND CONVENTIONS:**

**Abbreviations:**

- DET Analyte DETECTED at or above the detection or reporting limit.
- ND Analyte NOT DETECTED at or above the detection or reporting limit.
- NR Result Not Reported
- RPD Relative Percent Difference. RPDs for Matrix Spikes and Matrix Spike Duplicates are based on concentration, not recovery.

**Detection Limits: Limit of Detection (LOD)**

Limits of Detection (LODs) are normally set at a level of one half the validated Limit of Quantitation (LOQ).  
If no value is listed ('-----'), then the data has not been evaluated below the Reporting Limit.

**Reporting Limits: Limit of Quantitation (LOQ)**

Validated Limits of Quantitation (LOQs) are reported as the Reporting Limits for all analyses where the LOQ, MRL, PQL or CRL are requested. The LOQ represents a level at or above the low point of the calibration curve, that has been validated according to Apex Laboratories' comprehensive LOQ policies and procedures.

**Reporting Conventions:**

- Basis: Results for soil samples are generally reported on a 100% dry weight basis.  
The Result Basis is listed following the units as "dry", "wet", or " " (blank) designation.
  - "dry" Sample results and Reporting Limits are reported on a dry weight basis. (i.e. "ug/kg dry")  
See Percent Solids section for details of dry weight analysis.
  - "wet" Sample results and Reporting Limits for this analysis are normally dry weight corrected, but have not been modified in this case.
  - " " Results without 'wet' or 'dry' designation are not normally dry weight corrected. These results are considered 'As Received'.

**QC Source:**

In cases where there is insufficient sample provided for Sample Duplicates and/or Matrix Spikes, a Lab Control Sample Duplicate (LCS Dup) may be analyzed to demonstrate accuracy and precision of the extraction batch.  
  
Non-Client Batch QC Samples (Duplicates and Matrix Spike/Duplicates) may not be included in this report. Please request a Full QC report if this data is required.

**Miscellaneous Notes:**

- " --- " QC results are not applicable. For example, % Recoveries for Blanks and Duplicates, % RPD for Blanks, Blank Spikes and Matrix Spikes, etc.
- " \*\*\* " Used to indicate a possible discrepancy with the Sample and Sample Duplicate results when the %RPD is not available. In this case, either the Sample or the Sample Duplicate has a reportable result for this analyte, while the other is Non Detect (ND).

**Blanks:**

Standard practice is to evaluate the results from Blank QC Samples down to a level equal to 1/2 the Reporting Limit (RL).  
-For Blank hits falling between 1/2 the RL and the RL (J flagged hits), the associated sample and QC data will receive a 'B-02' qualifier.  
-For Blank hits above the RL, the associated sample and QC data will receive a 'B' qualifier, per Apex Laboratories' Blank Policy.  
For further details, please request a copy of this document.

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Anchor QEA, LLC**

6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: **Gasco PreRD DG 2019 - 4c. Waste Characterization**

Project Number: [none]

Project Manager: **Ryan Barth**

**Report ID:**

**A9K0412 - 12 04 19 1401**

**REPORTING NOTES AND CONVENTIONS (Cont.):**

**Blanks (Cont.):**

Sample results flagged with a 'B' or 'B-02' qualifier are potentially biased high if the sample results are less than ten times the level found in the blank for inorganic analyses, or less than five times the level found in the blank for organic analyses.

'B' and 'B-02' qualifications are only applied to sample results detected above the Reporting Level.

**Preparation Notes:**

Mixed Matrix Samples:

Water Samples:

Water samples containing significant amounts of sediment are decanted or separated prior to extraction, and only the water portion analyzed, unless otherwise directed by the client.

Soil and Sediment Samples:

Soil and Sediment samples containing significant amounts of water are decanted prior to extraction, and only the solid portion analyzed, unless otherwise directed by the client.

**Sampling and Preservation Notes:**

Certain regulatory programs, such as National Pollutant Discharge Elimination System (NPDES), require that activities such as sample filtration (for dissolved metals, orthophosphate, hexavalent chromium, etc.) and testing of short hold analytes (pH, Dissolved Oxygen, etc.) be performed in the field (on-site) within a short time window. In addition, sample matrix spikes are required for some analyses, and sufficient volume must be provided, and billable site specific QC requested, if this is required. All regulatory permits should be reviewed to ensure that these requirements are being met.

Data users should be aware of which regulations pertain to the samples they submit for testing. If related sample collection activities are not approved for a particular regulatory program, results should be considered estimates. Apex Laboratories will qualify these analytes according to the most stringent requirements, however results for samples that are for non-regulatory purposes may be acceptable.

Samples that have been filtered and preserved at Apex Laboratories per client request are listed in the preparation section of the report with the date and time of filtration listed.

Apex Laboratories maintains detailed records on sample receipt, including client label verification, cooler temperature, sample preservation, hold time compliance and field filtration. Data is qualified as necessary, and the lack of qualification indicates compliance with required parameters.

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



**Apex Laboratories, LLC**

6700 S.W. Sandburg Street  
Tigard, OR 97223  
503-718-2323  
**EPA ID: OR01039**

<b><u>Anchor QEA, LLC</u></b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b><u>Gasco PreRD DG 2019 - 4c. Waste Characterization</u></b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
---	---	--

**LABORATORY ACCREDITATION INFORMATION**

**TNI Certification ID: OR100062 (Primary Accreditation) - EPA ID: OR01039**

All methods and analytes reported from work performed at Apex Laboratories are included on Apex Laboratories' ORELAP Scope of Certification, with the exception of any analyte(s) listed below:

**Apex Laboratories**

Matrix	Analysis	TNI_ID	Analyte	TNI_ID	Accreditation
--------	----------	--------	---------	--------	---------------

All reported analytes are included in Apex Laboratories' current ORELAP scope.

**Secondary Accreditations**

Apex Laboratories also maintains reciprocal accreditation with non-TNI states (Washington DOE), as well as other state specific accreditations not listed here.

**Subcontract Laboratory Accreditations**

Subcontracted data falls outside of Apex Laboratories' Scope of Accreditation. Please see the Subcontract Laboratory report for full details, or contact your Project Manager for more information.

**Field Testing Parameters**

Results for Field Tested data are provided by the client or sampler, and fall outside of Apex Laboratories' Scope of Accreditation.

Apex Laboratories

*The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.*



Anchor QEA, LLC

6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Project Number: [none]  
Project Manager: Ryan Barth

Report ID:

A9K0412 - 12 04 19 1401

**ENVIRONMENTAL SAMPLE CHAIN OF CUSTODY**

**Anchor QEA, LLC**  
 1301 3rd Avenue, Suite 2000, Seattle, WA 98101  
 POC: Delaney Peterson (360-715-2707) Project: Gasco PDI 1605 Cornwall Avenue, Bellingham, WA 98225 Client: NW Natural

COC ID: APEX-20191114-102611  
 Sample Custodian: SN  
 Lab: Apex

A9K0412

COC Sample Number	Field Sample ID	Sample Type	Matrix	Collected Date	Time	# Containers	Lab QC*	Test Request	Method	TAT**	Preservative
004	PDI-142RAB-10-20-181112	N	SO	11/12/2019	12:00	3	<input type="checkbox"/>	TOC Metals (QAPP 3) PCB Aroclors SVOCs (PAHs, BEHP, Phenols) Total solids (APEX) VOCs (QAPP 4c)	SM5310B SW6020A SW8082A SW8270D SM2540G SW8260C	30 30 30 30 30 30	4°C 4°C 4°C 4°C 4°C
005	PDI-142RAB-20-30-4-191112	N	SO	11/12/2019	14:35	3	<input type="checkbox"/>	Diesel Range Organics Total CN TOC Metals (QAPP 3) PCB Aroclors SVOCs (PAHs, BEHP, Phenols) Total solids (APEX) VOCs (QAPP 4c)	SW8015D D7511-12 SM5310B SW6020A SW8082A SW8270D SM2540G SW8260C	30 30 30 30 30 30 30 30	4°C 4°C 4°C 4°C 4°C
006	PDI-142RAB-05-30-4-181112	N	SO	11/12/2019	15:40	2	<input type="checkbox"/>	TCLP Metals TCLP Pesticides TCLP SVOCs TCLP VOCs Total solids (APEX)	SW6020A SW8081B SW8270D SW8260C SM2540G	30 30 30 30 30	
007	PDI-144RAB-05-10-181113	N	SO	11/13/2019	9:55	3	<input type="checkbox"/>				

Comment:

Requested By	Signature	Print Name	Company	Date/Time	Requested By	Signature	Print Name	Company	Date/Time
		Ryan Barth	Apex Lab	11/14/19 11:45			Ryan Barth	Apex Lab	11/14/19 13:40

Date Printed: 11/14/2019

\* Lab QC Requested for sample when box is checked \*\* TAT = Turn Around Time in DAYS # POC = Project Point of Contact

Page 2 of 4

Apex Laboratories

The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.



**Anchor QEA, LLC**

6720 SW Macadam Ave. Suite 125  
Portland, OR 97219

Project: **Gasco PreRD DG 2019 - 4c. Waste Characterization**

Project Number: [none]  
Project Manager: **Ryan Barth**

**Report ID:**

**A9K0412 - 12 04 19 1401**

**ANCHOR QEA**  
1021 3rd Avenue, Suite 2000, Seattle, WA 98101

**POC:** Delaney Peterson (360-715-2707)  
1605 Cornwell Avenue, Bellingham, WA 98225

**Project:** Gasco PDI  
**Client:** NW Natural

**ENVIRONMENTAL SAMPLE CHAIN OF CUSTODY**

**COC ID:** APEX-20191114-102611  
**Sample Custodian:** SN  
**Lab:** Apex

A9K0412

COC Sample Number	Field Sample ID	Sample Type	Matrix	Collected Date	Time	# Containers	Lab QC	Test Request	Method	TAT**	Preservative
009	PDI-144RAB-20-28-191113	N	SO	11/13/2019	12:00	3	<input type="checkbox"/>	PCB Aroclors SVOCs (PAHs, BEHP, Phenols) Total solids (APEX) VOCs (QAPP 4c)	SW8082A SW8270D SM2540G SW8260C	30 30 30 30	4°C 4°C
010	PDI-144RAB-20-28-191113	N	SO	11/13/2019	12:40	2	<input type="checkbox"/>	TCLP Metals TCLP Pesticides TCLP SVOCs TCLP VOCs Total solids (APEX)	SW6020A SW8081B SW8270D SW8260C SM2540G	30 30 30 30 30	

**Received By:** [Signature] **Received By:** [Signature]

**Print Name:** Sgha Norwood **Print Name:** M. Kollwitz

**Company:** Anchor QEA **Company:** Apex Labs

**Date/Time:** 11/14/19 @ 1145 **Date/Time:** 11-14-19 1340

**Date Printed:** 11/14/2019

\* Lab QC Requested for sample when box is checked \*\* TAT = Turn Around Time in DAYS # POC = Project Point of Contact

Apex Laboratories

The results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.

<b>Anchor QEA, LLC</b> 6720 SW Macadam Ave. Suite 125 Portland, OR 97219	Project: <b>Gasco PreRD DG 2019 - 4c. Waste Characterization</b> Project Number: [none] Project Manager: <b>Ryan Barth</b>	<b>Report ID:</b> A9K0412 - 12 04 19 1401
--	--	--

**APEX LABS COOLER RECEIPT FORM**

Client: Anchor QEA Element WO#: A9 120412  
 Project/Project #: Gasco PDI - Waste Characterization

**Delivery Info:**  
 Date/time received: 11-14-19 @ 1340 By: MK  
 Delivered by: Apex  Client  ESS  FedEx  UPS  Swift  Senvoy  SDS  Other

**Cooler Inspection** Date/time inspected: 11-14-19 @ 1445 By: MK  
 Chain of Custody included? Yes  No  Custody seals? Yes  No   
 Signed/dated by client? Yes  No   
 Signed/dated by Apex? Yes  No

	Cooler #1	Cooler #2	Cooler #3	Cooler #4	Cooler #5	Cooler #6	Cooler #7
Temperature (°C)	<u>2.1</u>						
Received on ice? (Y/N)	<u>Y</u>						
Temp. blanks? (Y/N)	<u>Y</u>						
Ice type: (Gel/Real/Other)	<u>Real</u>						
Condition:	<u>good</u>						

Cooler out of temp? (Y/N) Y Possible reason why: \_\_\_\_\_  
 If some coolers are in temp and some out, were green dots applied to out of temperature samples? Yes/No/NA NA  
 Out of temperature samples form initiated? Yes/No/NA NA  
**Samples Inspection:** Date/time inspected: 11/14/19 @ 1720 By: CB  
 All samples intact? Yes  No  Comments: \_\_\_\_\_

Bottle labels/COCs agree? Yes  No  Comments: PDI-142FAB-C-00-30.4-19112 time on conts. read 14:40


COC/container discrepancies form initiated? Yes  No  NA   
 Containers/volumes received appropriate for analysis? Yes  No  Comments: \_\_\_\_\_

Do VOA vials have visible headspace? Yes  No  NA   
 Comments: \_\_\_\_\_

Water samples: pH checked: Yes  No  NA  pH appropriate? Yes  No  NA   
 Comments: \_\_\_\_\_

**Additional information:**  
 \_\_\_\_\_  
 \_\_\_\_\_

Labeled by: CB Witness: MRP Cooler Inspected by: CB See Project Contact Form: Y



**Sample Receipt Documentation  
(Work orders, Chain of Custody & Cooler Receipt Forms)**

**A9K0412**

**Apex Laboratories**

<b>Client:</b> Anchor QEA, LLC	<b>Project Manager:</b> Darwin Thomas
<b>Project:</b> Gasco PreRD_DG 2019 - 4c. Waste Characterization	<b>Project Number:</b> [none]

<p><b>Report To:</b>                  Anchor QEA, LLC                  Ryan Barth                  6720 SW Macadam Ave. Suite 125                  Portland, OR 97219                  Phone: (503) 670-1108                  Fax: na</p>	<p><b>Invoice To:</b>                  Anchor QEA, LLC Seattle                  Accounts Payable                  1201 3rd Avenue, Suite 2600                  Seattle, WA 98101                  Phone : (206) 287-9130                  Fax: (206) 287-9131</p>
---	---

Date Due: 12/02/19 17:00 (10 day TAT)	
Received By: Mike Kachnik	Date Received: 11/14/19 13:40
Logged In By: Cameron L O'Brien	Date Logged In: 11/14/19 17:12

<b>Cooler #1 received at 2.1°C</b>									
Custody Seals	Yes	Containers Intact	Yes	COC/Labels Agree	Yes	PH Confirmed	No	Received On Ice	Yes
Temperature OK	Yes								

Analysis	Due	TAT	Expires	Comments
<b>A9K0412-01 PDI-142RAB-C-00-30.4-191112 [Soil] Sampled 11/12/19 15:40</b>				
<b>(GMT-08:00) Pacific Time (US &amp; Canada) 3 Containers</b>				
<b>Metals</b>				
Metals, TCLP 8	11/27/19 17:00	10	05/10/20 15:40	
TCLP Extraction - Metals	11/18/19 17:00	2	12/10/19 15:40	
TCLP Extraction - Organics	11/18/19 17:00	2	11/26/19 15:40	
<b>Project Mgmt</b>				
Data Package	01/15/20 17:00	10	02/19/20 15:40	
<b>Sample Control</b>				
Archive Samples - Frozen	11/15/19 17:00	1	11/13/19 15:40	3 months
<b>Semivols (ECD)</b>				
1311/8081B TCLP Pest Reg List	11/27/19 17:00	10	11/19/19 15:40	
<b>Semivols (Scan)</b>				
1311/8270D TCLP SVOC Reg List	11/27/19 17:00	10	11/19/19 15:40	
<b>Volatiles</b>				
1311/8260C TCLP/ZHE VOC Reg List	11/27/19 17:00	10	11/26/19 15:40	
TCLP/ZHE Extraction	11/26/19 17:00	2	11/26/19 15:40	
<b>Wet Chem</b>				
Solids, Total (SM 2540 G,B)	11/27/19 17:00	10	05/10/20 15:40	



**A9K0412**

**Apex Laboratories**

<b>Client:</b> Anchor QEA, LLC	<b>Project Manager:</b> Darwin Thomas
<b>Project:</b> Gasco PreRD_DG 2019 - 4c. Waste Characterization	<b>Project Number:</b> [none]

Analysis	Due	TAT	Expires	Comments
<b>A9K0412-02 PDI-144RAB-C-00-28.1-191113 [Soil] Sampled 11/13/19 12:40</b>				
<b>(GMT-08:00) Pacific Time (US &amp; Canada) 3 Containers</b>				
<b>Project Mgmt</b>				
Unresolved Login	11/15/19 17:00	1	02/20/20 12:40	cancelled all tests per client request 11/15; DWA
<b>Sample Control</b>				
Archive Samples - Frozen	11/15/19 17:00	1	11/14/19 12:40	
<b>Wet Chem</b>				
<del>Solids, Total (SM 2540-G,B)</del>	11/27/19 17:00	10	05/11/20 12:40	cancelled per client 11/15

<b>Analysis groups included in this work order</b>			
<i>Metals, TCLP &amp;</i>			
Ag (Silver) - 6020 - TCLP	As (Arsenic) - 6020 - TCLP	Ba (Barium) - 6020 - TCLP	Cd (Cadmium) - 6020 - TCLP
Cr (Chromium) - 6020 - TCLP	Hg (Mercury) - 6020 - TCLP	Pb (Lead) - 6020 - TCLP	Se (Selenium) - 6020 - TCLP



1201 3rd Avenue, Suite 2600, Seattle, WA 98101

# ENVIRONMENTAL SAMPLE CHAIN OF CUSTODY

*AK0112*

COC ID: APEX-20191114-102611  
Sample Custodian: SN  
Lab: Apex

POC: # Delaney Peterson (360-715-2707) Project: Gasco PDI  
1605 Cornwall Avenue, Bellingham, WA 98225 Client: NW Natural

COC Sample Number	Field Sample ID	Sample Type	Matrix	Collected Date	Time	Containers #	Lab QC*	Test Request	Method	TAT**	Preservative
004	PDI-142RAB-10-20-191112	N	SO	11/12/2019	12:00	3	<input type="checkbox"/>	TOC Metals (QAPP 3) PCB Aroclors SVOCs (PAHs, BEHP, Phenols) Total solids (APEX) VOCs (QAPP 4c)	SM5310B SW6020A SW6082A SW8270D SM2540G SW8260C	30 30 30 30 30 30	4°C 4°C 4°C 4°C
005	PDI-142RAB-20-30-4-191112	N	SO	11/12/2019	14:35	3	<input type="checkbox"/>	Diesel Range Organics Total CN TOC Metals (QAPP 3) PCB Aroclors SVOCs (PAHs, BEHP, Phenols) Total solids (APEX) VOCs (QAPP 4c)	SW8015D D7511-12 SM5310B SW6020A SW6082A SW8270D SM2540G SW8260C	30 30 30 30 30 30 30 30	4°C 4°C 4°C 4°C 4°C 4°C
006	PDI-142RAB-C-00-30-4-191112	N	SO	11/12/2019	15:40	2	<input type="checkbox"/>	TCLP Metals TCLP Pesticides TCLP SVOCs TCLP VOCs Total solids (APEX)	SW6020A SW8081B SW8270D SW8260C SM2540G	30 30 30 30 30	
007	PDI-144RAB-00-10-191113	N	SO	11/13/2019	9:55	3	<input type="checkbox"/>				

Comment:

Received By: Signature <i>[Signature]</i>	Relinquished By: Signature <i>[Signature]</i>
Print Name <i>Sasha Norwood</i>	Print Name <i>M. Kachnik</i>
Company <i>Anchor QEA</i>	Company <i>Apex Labs</i>
Date/Time <i>11/14/19 1145</i>	Date/Time <i>11-14-19 1340</i>

Date Printed: 11/14/2019

\* Lab QC Requested for sample when box is checked \*\* TAT = Turn Around Time in DAYS # POC = Project Point of Contact



1201 3rd Avenue, Suite 2600, Seattle, WA 98101

# ENVIRONMENTAL SAMPLE CHAIN OF CUSTODY

*AAK0412*

COC ID: APEX-20191114-102611  
 Sample Custodian: SN  
 Lab: Apex

POC: \* Delaney Peterson (360-715-2707) Project: Gasco PDI  
 1605 Cornwall Avenue, Bellingham, WA 98225 Client: NW Natural

COC Sample Number	Field Sample ID	Sample Type	Matrix	Collected Date	Collected Time	Containers #	Lab QC* <input type="checkbox"/>	Test Request	Method	TAT**	Preservative
009	PDI-144RAB-20-29-191113	N	SO	11/13/2019	12:00	3	<input type="checkbox"/>	PCB Aroclors SVOCs (PAHs, BEHP, Phenols) Total solids (APEX) VOCs (QAPP 4c)	SW8082A SW8270D SM2540G SW8260C	30 30 30 30	4°C 4°C
010	PDI-144RAB-C-00-28-191113	N	SO	11/13/2019	12:40	2	<input type="checkbox"/>	TCLP Metals TCLP Pesticides TCLP SVOCs TCLP VOCs Total solids (APEX)	SW6020A SW8081B SW8270D SW8260C SM2540G	30 30 30 30 30	

Comment:

Relinquished By	Relinquished By	Relinquished By	Relinquished By
Signature	Signature	Signature	Signature
<i>[Signature]</i>	<i>[Signature]</i>	<i>[Signature]</i>	<i>[Signature]</i>
Print Name Sasha Norwood	Print Name M. Kenanik	Print Name	Print Name
Company Anchor QEA	Company Apex Labs	Company	Company
Date/Time 11/14/19 @ 1145	Date/Time 11-14-19 1340	Date/Time	Date/Time

Date Printed: 11/14/2019 \* Lab QC Requested for sample when box is checked \*\* TAT = Turn Around Time in DAYS # POC = Project Point of Contact

**APEX LABS COOLER RECEIPT FORM**

Client: Anchor QEA Element WO#: A9 120412

Project/Project #: Gasco PDI - Waste Characterization

**Delivery Info:**

Date/time received: 11-14-19 @ 1300 By: MK

Delivered by: Apex  Client  ESS  FedEx  UPS  Swift  Senvoy  SDS  Other

**Cooler Inspection** Date/time inspected: 11-14-19 @ 1445 By: MK

Chain of Custody included? Yes  No  Custody seals? Yes  No

Signed/dated by client? Yes  No

Signed/dated by Apex? Yes  No

	Cooler #1	Cooler #2	Cooler #3	Cooler #4	Cooler #5	Cooler #6	Cooler #7
Temperature (°C)	<u>2.1</u>						
Received on ice? (Y/N)	<u>Y</u>						
Temp. blanks? (Y/N)	<u>Y</u>						
Ice type: (Gel/Real/Other)	<u>Real</u>						
Condition:	<u>good</u>						

Cooler out of temp? (Y/N) Possible reason why: (N)  
If some coolers are in temp and some out, were green dots applied to out of temperature samples? Yes/No/NA (NA)  
Out of temperature samples form initiated? Yes/No/NA (NA)

**Samples Inspection:** Date/time inspected: 11/14/19 @ 1720 By: CB

All samples intact? Yes  No  Comments: \_\_\_\_\_

Bottle labels/COCs agree? Yes  No  Comments: PDI-142FAB-C-00-304-19112 time on conts. read 14:40

COC/container discrepancies form initiated? Yes  No  NA

Containers/volumes received appropriate for analysis? Yes  No  Comments: \_\_\_\_\_

Do VOA vials have visible headspace? Yes  No  NA   
Comments: \_\_\_\_\_

Water samples: pH checked: Yes  No  NA  pH appropriate? Yes  No  NA   
Comments: \_\_\_\_\_

**Additional information:**  
\_\_\_\_\_  
\_\_\_\_\_

Labeled by: CB Witness: MRP Cooler Inspected by: CB See Project Contact Form: Y

## CLP-Like Forms

# Apex Laboratories

SDG: Gasco PreRD\_DG 2019  
CLASS: GCMS  
METHOD: 1311/8260C

**ANALYSES DATA PACKAGE COVER PAGE**

**1311/8260C**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

---

**Client Sample Id:**

PDI-142RAB-C-00-30.4-191112

**Lab Sample Id:**

A9K0412-01

**Matrix**

SO

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hardcopy data package and in computer-readable data submitted on diskette has been authorized by the Laboratory Manager or the Manager's designee, as verified by the following signatures.

Signature: \_\_\_\_\_



Name: \_\_\_\_\_

David G. Jack

Forms Created: \_\_\_\_\_

12/19/2019 1:07PM

Title: \_\_\_\_\_

Technical Manager

# METHOD DETECTION AND REPORTING LIMITS

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Charac

Batch Matrix: Water

Analyte	MDL	MRL	Units
Benzene	0.00625	0.0125	mg/L
2-Butanone (MEK)	0.250	0.500	mg/L
Carbon tetrachloride	0.0250	0.0500	mg/L
Chlorobenzene	0.0125	0.0250	mg/L
Chloroform	0.0250	0.0500	mg/L
1,4-Dichlorobenzene	0.0125	0.0250	mg/L
1,2-Dichloroethane (EDC)	0.0125	0.0250	mg/L
1,1-Dichloroethene	0.0125	0.0250	mg/L
Tetrachloroethene (PCE)	0.0125	0.0250	mg/L
Trichloroethene (TCE)	0.0125	0.0250	mg/L
Vinyl chloride	0.0125	0.0250	mg/L

Note: MDLs are listed only if the corresponding analyte was evaluated to the MDL in this report .



# ORGANIC ANALYSIS DATA SHEET

1311/8260C

PDI-142RAB-C-00-30.4-191112

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD_DG 2019</u>	
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD_DG 2019 - 4c. Waste Characterization</u>	
Matrix: <u>SO</u>	Laboratory ID: <u>A9K0412-01</u>	File ID: <u>VI19111811.D</u>
Sampled: <u>11/12/19 15:40</u>	Prepared: <u>11/19/19 12:00</u>	Analyzed: <u>11/19/19 13:21</u>
	Preparation: <u>EPA 1311/5030B TCLP Vola</u>	Initial/Final: <u>5 mL / 5 mL</u>

Batch: 9110813      Sequence: 9K19033      Calibration: A9J2503      Instrument: VOA-GCMS9

CAS NO.	COMPOUND	DILUTION	CONC. (mg/L)	Q
71-43-2	Benzene	50	0.00625	U
78-93-3	2-Butanone (MEK)	50	0.250	U
56-23-5	Carbon tetrachloride	50	0.0250	U
108-90-7	Chlorobenzene	50	0.0125	U
67-66-3	Chloroform	50	0.0250	U
106-46-7	1,4-Dichlorobenzene	50	0.0125	U
107-06-2	1,2-Dichloroethane (EDC)	50	0.0125	U
75-35-4	1,1-Dichloroethene	50	0.0125	U
127-18-4	Tetrachloroethene (PCE)	50	0.0125	U
79-01-6	Trichloroethene (TCE)	50	0.0125	U
75-01-4	Vinyl chloride	50	0.0125	U

SYSTEM MONITORING COMPOUND	ADDED (ng/mL)	CONC (ng/mL)	% REC	QC LIMITS	Q
1,4-Difluorobenzene (Surr)	50.0	59.7	119	80 - 120	
Toluene-d8 (Surr)	50.0	50.8	102	80 - 120	
4-Bromofluorobenzene (Surr)	50.0	50.7	101	80 - 120	

INTERNAL STANDARD	AREA	RT	REF AREA	REF RT	Q
Pentafluorobenzene (ISTD)	94988	6.211	103299	6.217	
Chlorobenzene-d5 (ISTD)	272456	9.91	301980	9.91	
1,4-Dichlorobenzene-d4 (ISTD)	122016	11.85	149066	11.85	

\* Values outside of QC limits

# PREPARATION BATCH SUMMARY

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Batch: 9110813 Batch Matrix: Water

Preparation: EPA 1311/5030B TCLP Volatiles

SAMPLE NAME	LAB SAMPLE ID	LAB FILE ID	DATE PREPARED	OBSERVATIONS
Blank	9110813-BLK1	VI19111808.D	11/19/19 09:00	
LCS	9110813-BS1	VI19111807.D	11/19/19 09:00	
PDI-142RAB-C-00-30.4-191112 (M	9110813-MS1	VI19111812.D	11/19/19 12:00	
PDI-142RAB-C-00-30.4-191112	A9K0412-01	VI19111811.D	11/19/19 12:00	

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# METHOD BLANK DATA SHEET

**1311/8260C**

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD_DG 2019</u>	
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD_DG 2019 - 4c. Waste Characterization</u>	
Matrix: <u>Water</u>	Laboratory ID: <u>9110813-BLK1</u>	File ID: <u>VI19111808.D</u>
Prepared: <u>11/19/19 09:00</u>	Preparation: <u>EPA 1311/5030B TCLP Vola</u>	Initial/Final: <u>5 mL / 5 mL</u>
Analyzed: <u>11/19/19 12:00</u>	Instrument: <u>VOA-GCMS9</u>	
Batch: <u>9110813</u>	Sequence: <u>9K19033</u>	Calibration: <u>A9J2503</u>

CAS NO.	COMPOUND	CONC. (mg/L)	Q
71-43-2	Benzene	0.00625	U
78-93-3	2-Butanone (MEK)	0.250	U
56-23-5	Carbon tetrachloride	0.0250	U
108-90-7	Chlorobenzene	0.0125	U
67-66-3	Chloroform	0.0250	U
106-46-7	1,4-Dichlorobenzene	0.0125	U
107-06-2	1,2-Dichloroethane (EDC)	0.0125	U
75-35-4	1,1-Dichloroethene	0.0125	U
127-18-4	Tetrachloroethene (PCE)	0.0125	U
79-01-6	Trichloroethene (TCE)	0.0125	U
75-01-4	Vinyl chloride	0.0125	U

SYSTEM MONITORING COMPOUND	ADDED (ng/mL)	CONC (ng/mL)	% REC	QC LIMITS	Q
1,4-Difluorobenzene (Surr)	50.0	60.3	121	80 - 120	*
Toluene-d8 (Surr)	50.0	51.4	103	80 - 120	
4-Bromofluorobenzene (Surr)	50.0	50.9	102	80 - 120	

INTERNAL STANDARD	AREA	RT	REF AREA	REF RT	Q
Pentafluorobenzene (ISTD)	94973	6.217	103299	6.217	
Chlorobenzene-d5 (ISTD)	274403	9.91	301980	9.91	
1,4-Dichlorobenzene-d4 (ISTD)	123791	11.85	149066	11.85	

# LCS / LCS DUPLICATE RECOVERY

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Matrix: Water

Batch: 9110813

Laboratory ID: 9110813-BS1

Preparation: EPA 1311/5030B TCLP Volatiles

Initial/Final: 5 mL / 5 mL

COMPOUND	SPIKE ADDED (mg/L)	LCS CONCENTRATION (mg/L)	LCS % REC. (*=Out)	QC LIMITS REC.
Benzene	1.00	1.07	107	80 - 120
2-Butanone (MEK)	2.00	1.94	97	80 - 120
Carbon tetrachloride	1.00	1.20	120	80 - 120
Chlorobenzene	1.00	1.03	103	80 - 120
Chloroform	1.00	1.10	110	80 - 120
1,4-Dichlorobenzene	1.00	1.00	100	80 - 120
1,2-Dichloroethane (EDC)	1.00	0.962	96	80 - 120
1,1-Dichloroethene	1.00	1.04	104	80 - 120
Tetrachloroethene (PCE)	1.00	1.09	109	80 - 120
Trichloroethene (TCE)	1.00	1.15	115	80 - 120
Vinyl chloride	1.00	1.02	102	80 - 120

\* = Values outside of QC limits

**MATRIX SPIKE / MATRIX SPIKE DUPLICATE RECOVERY**

**1311/8260C**

**PDI-142RAB-C-00-30.4-191112**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Matrix: Water

Batch: 9110813

Laboratory ID: 9110813-MS1

Preparation: EPA 1311/5030B TCLP Volatiles

Initial/Final: 5 mL / 5 mL

Source Sample Name: PDI-142RAB-C-00-30.4-191112

COMPOUND	SPIKE ADDED (mg/L)	SAMPLE CONCENTRATION (mg/L)	MS CONCENTRATION (mg/L)	MS % REC. (*=Out)	QC LIMITS REC.
Benzene	1.00	ND	1.18	118	70 - 130
2-Butanone (MEK)	2.00	ND	2.06	103	70 - 130
Carbon tetrachloride	1.00	ND	0.970	97	70 - 130
Chlorobenzene	1.00	ND	1.08	108	70 - 130
Chloroform	1.00	ND	1.01	101	70 - 130
1,4-Dichlorobenzene	1.00	ND	1.01	101	70 - 130
1,2-Dichloroethane (EDC)	1.00	ND	0.867	87	70 - 130
1,1-Dichloroethene	1.00	ND	0.973	97	70 - 130
Tetrachloroethene (PCE)	1.00	ND	1.15	115	70 - 130
Trichloroethene (TCE)	1.00	ND	1.30	130	70 - 130
Vinyl chloride	1.00	ND	1.08	108	70 - 130

# ANALYSIS BATCH (SEQUENCE) SUMMARY

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9J24043

Instrument: VOA-GCMS9

Matrix: Water

Calibration: A9J2503

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
MS Tune	9J24043-TUN1	VI19102415.D	10/24/19 15:01
Initial Cal Blank	9J24043-ICB1	VI19102416.D	10/24/19 15:28
Cal Standard	9J24043-CAL1	VI19102417.D	10/24/19 15:55
Cal Standard	9J24043-CAL2	VI19102418.D	10/24/19 16:21
Cal Standard	9J24043-CAL3	VI19102419.D	10/24/19 16:48
Cal Standard	9J24043-CAL4	VI19102420.D	10/24/19 17:15
Cal Standard	9J24043-CAL5	VI19102421.D	10/24/19 17:42
Cal Standard	9J24043-CAL6	VI19102422.D	10/24/19 18:09
Cal Standard	9J24043-CAL7	VI19102423.D	10/24/19 18:36
Cal Standard	9J24043-CAL8	VI19102424.D	10/24/19 19:03
Cal Standard	9J24043-CAL9	VI19102425.D	10/24/19 19:30
Cal Standard	9J24043-CALA	VI19102427.D	10/24/19 20:24
Cal Standard	9J24043-CALB	VI19102429.D	10/24/19 21:17
Initial Cal Check	9J24043-ICV1	VI19102432.D	10/24/19 22:38

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# ANALYSIS BATCH (SEQUENCE) SUMMARY

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9K19033

Instrument: VOA-GCMS9

Matrix: Water

Calibration: A9J2503

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
MS Tune	9K19033-TUN1	VI19111806.D	11/19/19 11:06
Calibration Check	9K19033-CCV1	VI19111807.D	11/19/19 11:33
Blank	9110813-BLK1	VI19111808.D	11/19/19 12:00
PDI-142RAB-C-00-30.4-191112	A9K0412-01	VI19111811.D	11/19/19 13:21
PDI-142RAB-C-00-30.4-191112 (MS	9110813-MS1	VI19111812.D	11/19/19 13:48

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# MASS SPECTROMETER INSTRUMENT PERFORMANCE CHECK

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Lab File ID: VI19102415.D

Injection Date: 10/24/19

Instrument ID: VOA-GCMS9

Injection Time: 15:01

Sequence: 9J24043

Lab Sample ID: 9J24043-TUN1

m/z	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE	
m/z 95	50 - 200% of m/z 174	117.89	PASS
m/z 96	5 - 9% of m/z 95	6.78	PASS
m/z 173	Less than 2% of m/z 174	0.39	PASS
m/z 174	50 - 200% of m/z 95	84.82	PASS
m/z 175	5 - 9% of m/z 174	7.17	PASS
m/z 176	95 - 105% of m/z 174	96.98	PASS
m/z 177	5 - 10% of m/z 176	6.50	PASS



# MASS SPECTROMETER INSTRUMENT PERFORMANCE CHECK

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Lab File ID: VI19111806.D

Injection Date: 11/19/19

Instrument ID: VOA-GCMS9

Injection Time: 11:06

Sequence: 9K19033

Lab Sample ID: 9K19033-TUN1

m/z	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE	
m/z 95	50 - 200% of m/z 174	111.52	PASS
m/z 96	5 - 9% of m/z 95	6.88	PASS
m/z 173	Less than 2% of m/z 174	0.38	PASS
m/z 174	50 - 200% of m/z 95	89.67	PASS
m/z 175	5 - 9% of m/z 174	6.90	PASS
m/z 176	95 - 105% of m/z 174	95.60	PASS
m/z 177	5 - 10% of m/z 176	6.44	PASS

# INITIAL CALIBRATION DATA (Summary)

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterizati

Calibration: A9J2503

Date: 10/25/19 11:16

Instrument: VOA-GCMS9

Compound	Mean RF	FIT	RF RSD	Mean RT	RT RSD	Linear r	Quad COD	LIMIT	Q
Benzene	3.820688	Ave	4.855288	6.122454	7.160173E-02				***
2-Butanone (MEK)	0.6946318	Ave	5.120943	5.8565	0.1061664				***
Carbon tetrachloride	0.958096	Ave	12.51546	5.66	5.110175E-02				***
Chlorobenzene	0.9385267	Ave	6.79626	9.928546	1.897513E-02				***
Chloroform	1.575216	Ave	8.981403	5.5286	0.067176				
1,4-Dichlorobenzene	1.407811	Ave	7.702776	10.78391	33.16626				***
1,2-Dichloroethane (EDC)	1.251571	Ave	4.756875	6.338556	5.089469E-02				***
1,1-Dichloroethene	1.185277	Ave	4.829149	3.232	0.1325109				
Tetrachloroethene (PCE)	0.3422483	Ave	13.47971	8.7972	4.042701E-02				***
Trichloroethene (TCE)	0.9844716	Ave	10.55293	6.743	6.329732E-02				***
Vinyl chloride	1.085853	Ave	7.669228	1.9992	0.2472262				***
1,4-Difluorobenzene (Surr)	3.158849	Ave	0.8371646	6.780727	4.460955E-02				***
Toluene-d8 (Surr)	1.312366	Ave	1.829616	8.297273	1.899629E-02				***
4-Bromofluorobenzene (Surr)	0.8078842	Ave	3.581628	10.974	1.572481E-02				***

Note: \*\* Quad COD may be incorrect if weighting (1/a) or (1/a<sup>2</sup>) used. Weighting not shown here. Please see instrument calibration printouts for validation.

# INITIAL CALIBRATION DATA

1311/8260C

Laboratory: Apex Laboratories  
 Client: Anchor QEA, LLC  
 Calibration: A9J2503

SDG: Gasco PreRD DG 2019  
 Project: Gasco PreRD DG 2019 - 4c. Waste Character  
 Instrument: VOA-GCMS9  
 Calibration Date: 10/25/19 11:16

Compound	Level 01		Level 02		Level 03		Level 04		Level 05		Level 06	
	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF
Benzene	0.1	3.949114	0.2	3.449838	0.4	3.773943	1	3.582293	2	4.047071	5	3.909918
2-Butanone (MEK)	0.2	θ	0.4	θ	0.8	θ	2	0.6247684	4	0.7043731	10	0.704351
Carbon tetrachloride	0.1	θ	0.2	θ	0.4	<del>0.6898245</del>	1	0.7716967	2	0.9028342	5	0.8969462
Chlorobenzene	0.1	0.7802924	0.2	0.8622852	0.4	0.9452326	1	0.9282586	2	0.9824385	5	0.9841268
Chloroform	0.1	θ	0.2	1.278444	0.4	1.442157	1	1.439553	2	1.642071	5	1.638231
1,4-Dichlorobenzene	0.1	1.113251	0.2	1.342384	0.4	1.453521	1	1.450559	2	1.531358	5	1.43969
1,2-Dichloroethane (EDC)	0.1	θ	0.2	θ	0.4	1.197705	1	1.130185	2	1.292084	5	1.293487
1,1-Dichloroethene	0.1	θ	0.2	θ	0.4	1.158637	1	1.066846	2	1.187607	5	1.199982
Tetrachloroethene (PCE)	0.1	θ	0.2	0.2203159	0.4	0.334186	1	0.3207882	2	0.363807	5	0.361185
Trichloroethene (TCE)	0.1	θ	0.2	0.8101892	0.4	0.8014466	1	0.9332747	2	1.032584	5	1.02153
Vinyl chloride	0.1	θ	0.2	0.8842388	0.4	1.079386	1	1.012987	2	1.13503	5	1.139807
1,4-Difluorobenzene (Surr)	50	3.139024	50	3.131529	50	3.145975	50	3.159536	50	3.133965	50	3.188163
Toluene-d8 (Surr)	50	1.320931	50	1.332765	50	1.345328	50	1.320856	50	1.326656	50	1.321953
4-Bromofluorobenzene (Surr)	50	0.831108	50	0.83824	50	0.8349678	50	0.8234743	50	0.8250562	50	0.8153522

## INITIAL CALIBRATION DATA (Continued)

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Character

Calibration: A9J2503

Instrument: VOA-GCMS9

Matrix:

Calibration Date: 10/25/19 11:16

Compound	Level 07		Level 08		Level 09		Level 10		Level 11		Level 12	
	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF
Benzene	10	3.713991	20	3.910312	50	3.758481	100	4.021864	200	3.910748		
2-Butanone (MEK)	20	0.6623274	40	0.7169769	100	0.7014442	200	0.7409522	400	0.7018611		
Carbon tetrachloride	10	0.8859942	20	0.9772165	50	0.9911705	100	1.10568	200	1.13323		
Chlorobenzene	10	0.964716	20	0.9849134	50	0.9397401	100	0.9805969	200	0.9711928		
Chloroform	10	1.606991	20	1.695617	50	1.617019	100	1.719147	200	1.672928		
1,4-Dichlorobenzene	10	1.4332	20	1.477561	50	1.40642	100	1.43615	200	1.401823		
1,2-Dichloroethane (EDC)	10	1.230146	20	1.306225	50	1.244865	100	1.313294	200	1.256151		
1,1-Dichloroethene	10	1.158212	20	1.202649	50	1.192087	100	1.279045	200	1.222424		
Tetrachloroethene (PCE)	10	0.3532076	20	0.3701403	50	0.3520966	100	0.3717106	200	0.3750457		
Trichloroethene (TCE)	10	0.9969135	20	1.053302	50	1.025866	100	1.095246	200	1.074364		
Vinyl chloride	10	1.069187	20	1.110172	50	1.15024	100	1.154176	200	1.123309		
1,4-Difluorobenzene (Surr)	50	3.124014	50	3.1575	50	3.200969	50	3.186536	50	3.180128		
Toluene-d8 (Surr)	50	1.327143	50	1.301918	50	1.292388	50	1.274013	50	1.27207		
4-Bromofluorobenzene (Surr)	50	0.8117213	50	0.7980421	50	0.7955945	50	0.7620051	50	0.7511646		

# SECOND-SOURCE CALIBRATION VERIFICATION

1311/8260C

Laboratory: Apex Laboratories SDG: Gasco PreRD DG 2019  
Client: Anchor QEA, LLC Project: Gasco PreRD\_DG 2019 - 4c. Waste Charac  
Instrument ID: VOA-GCMS9 Calibration: A9J2503  
Lab File ID: VI19102432.D  
Sequence: 9J24043 Inject Date: 10/24/19  
Lab Sample ID: 9J24043-ICV1 Inject Time: 22:38

ANALYTE	EXPECTED (ng/mL)	FOUND (ng/mL)	% DRIFT	QC LIMIT
Benzene	20.0	19.7	-1.6	70 - 130
2-Butanone (MEK)	40.0	37.9	-5.3	70 - 130
Carbon tetrachloride	20.0	20.7	3.5	70 - 130
Chlorobenzene	20.0	20.6	3.0	70 - 130
Chloroform	20.0	20.9	4.3	70 - 130
1,4-Dichlorobenzene	20.0	20.5	2.4	70 - 130
1,2-Dichloroethane (EDC)	20.0	20.2	0.8	70 - 130
1,1-Dichloroethene	20.0	19.7	-1.4	70 - 130
Tetrachloroethene (PCE)	20.0	20.9	4.4	70 - 130
Trichloroethene (TCE)	20.0	21.2	6.2	70 - 130
Vinyl chloride	20.0	22.1	10.6	70 - 130

# SURROGATE STANDARD RECOVERY AND RT SUMMARY

1311/8260C

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD DG 2019</u>
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD DG 2019 - 4c. Waste Characterization</u>
Sequence: <u>9J24043</u>	Instrument: <u>VOA-GCMS9</u>
Matrix: <u>Water</u>	Calibration: <u>A9J2503</u>

Surrogate Compound	Spike Level ng/mL	% Recovery	Recovery Limits	RT	Calibration Mean RT	RT Diff	RT Diff Limit	Q
<b>Initial Cal Check (9J24043-ICV1)</b>			Lab File ID: VI19102432.D		Analyzed: 10/24/19 22:38			
1,4-Difluorobenzene (Surr)	50.0	101	70 - 130	6.782	6.780727	0.0013	+/-1.0	
Toluene-d8 (Surr)	50.0	99	70 - 130	8.297	8.297273	-0.0003	+/-1.0	
4-Bromofluorobenzene (Surr)	50.0	99	70 - 130	10.974	10.974	0.0000	+/-1.0	

# SURROGATE STANDARD RECOVERY AND RT SUMMARY

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sequence: 9K19033

Instrument: VOA-GCMS9

Matrix: Water

Calibration: A9J2503

Surrogate Compound	Spike Level ng/mL	% Recovery	Recovery Limits	RT	Calibration Mean RT	RT Diff	RT Diff Limit	Q
<b>LCS (9110813-BS1 )</b>			Lab File ID: VI19111807.D		Analyzed: 11/19/19 11:33			
1,4-Difluorobenzene (Surr)	50.0	107	80 - 120	6.783	6.780727	0.0023	+/-1.0	
Toluene-d8 (Surr)	50.0	98	80 - 120	8.297	8.297273	-0.0003	+/-1.0	
4-Bromofluorobenzene (Surr)	50.0	98	80 - 120	10.974	10.974	0.0000	+/-1.0	
<b>Blank (9110813-BLK1 )</b>			Lab File ID: VI19111808.D		Analyzed: 11/19/19 12:00			
1,4-Difluorobenzene (Surr)	50.0	121	80 - 120	6.783	6.780727	0.0023	+/-1.0	*
Toluene-d8 (Surr)	50.0	103	80 - 120	8.297	8.297273	-0.0003	+/-1.0	
4-Bromofluorobenzene (Surr)	50.0	102	80 - 120	10.974	10.974	0.0000	+/-1.0	
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01 )</b>			Lab File ID: VI19111811.D		Analyzed: 11/19/19 13:21			
1,4-Difluorobenzene (Surr)	50.0	119	80 - 120	6.777	6.780727	-0.0037	+/-1.0	
Toluene-d8 (Surr)	50.0	102	80 - 120	8.297	8.297273	-0.0003	+/-1.0	
4-Bromofluorobenzene (Surr)	50.0	101	80 - 120	10.974	10.974	0.0000	+/-1.0	
<b>Matrix Spike (9110813-MS1 )</b>			Lab File ID: VI19111812.D		Analyzed: 11/19/19 13:48			
1,4-Difluorobenzene (Surr)	50.0	119	80 - 120	6.783	6.780727	0.0023	+/-1.0	
Toluene-d8 (Surr)	50.0	99	80 - 120	8.297	8.297273	-0.0003	+/-1.0	
4-Bromofluorobenzene (Surr)	50.0	97	80 - 120	10.974	10.974	0.0000	+/-1.0	

**INTERNAL STANDARD AREA AND RT SUMMARY**  
**1311/8260C**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sequence: 9K19033

Instrument: VOA-GCMS9

Matrix: Water

Calibration: A9J2503

Internal Standard	Response	RT	Reference Response	Reference RT	Area %	Area % Limits	RT Diff	RT Diff Limit	Q
<b>LCS (9110813-BS1 )</b>									
Lab File ID: VI19111807.D					Analyzed: 11/19/19 11:33				
Pentafluorobenzene (ISTD)	103299	6.217	103299	6.217	100	50 - 200	0.0000	+/-0.50	
Chlorobenzene-d5 (ISTD)	301980	9.91	301980	9.91	100	50 - 200	0.0000	+/-0.50	
1,4-Dichlorobenzene-d4 (ISTD)	149066	11.85	149066	11.85	100	50 - 200	0.0000	+/-0.50	
<b>Calibration Check (9K19033-CCV1 )</b>									
Lab File ID: VI19111807.D					Analyzed: 11/19/19 11:33				
Pentafluorobenzene (ISTD)	103299	6.217	112406	6.211	92	50 - 200	0.0060	+/-0.50	
Chlorobenzene-d5 (ISTD)	301980	9.91	307093	9.91	98	50 - 200	0.0000	+/-0.50	
1,4-Dichlorobenzene-d4 (ISTD)	149066	11.85	151591	11.85	98	50 - 200	0.0000	+/-0.50	
<b>Blank (9110813-BLK1 )</b>									
Lab File ID: VI19111808.D					Analyzed: 11/19/19 12:00				
Pentafluorobenzene (ISTD)	94973	6.217	103299	6.217	92	50 - 200	0.0000	+/-0.50	
Chlorobenzene-d5 (ISTD)	274403	9.91	301980	9.91	91	50 - 200	0.0000	+/-0.50	
1,4-Dichlorobenzene-d4 (ISTD)	123791	11.85	149066	11.85	83	50 - 200	0.0000	+/-0.50	
<b>Duplicate (9110813-DUP1 )</b>									
Lab File ID: VI19111810.D					Analyzed: 11/19/19 12:54				
Pentafluorobenzene (ISTD)	95376	6.217	103299	6.217	92	50 - 200	0.0000	+/-0.50	
Chlorobenzene-d5 (ISTD)	274368	9.91	301980	9.91	91	50 - 200	0.0000	+/-0.50	
1,4-Dichlorobenzene-d4 (ISTD)	122966	11.85	149066	11.85	82	50 - 200	0.0000	+/-0.50	
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01 )</b>									
Lab File ID: VI19111811.D					Analyzed: 11/19/19 13:21				
Pentafluorobenzene (ISTD)	94988	6.211	103299	6.217	92	50 - 200	-0.0060	+/-0.50	
Chlorobenzene-d5 (ISTD)	272456	9.91	301980	9.91	90	50 - 200	0.0000	+/-0.50	
1,4-Dichlorobenzene-d4 (ISTD)	122016	11.85	149066	11.85	82	50 - 200	0.0000	+/-0.50	
<b>Matrix Spike (9110813-MS1 )</b>									
Lab File ID: VI19111812.D					Analyzed: 11/19/19 13:48				
Pentafluorobenzene (ISTD)	103460	6.217	103299	6.217	100	50 - 200	0.0000	+/-0.50	
Chlorobenzene-d5 (ISTD)	305031	9.91	301980	9.91	101	50 - 200	0.0000	+/-0.50	
1,4-Dichlorobenzene-d4 (ISTD)	151550	11.85	149066	11.85	102	50 - 200	0.0000	+/-0.50	



# HOLDING TIME SUMMARY

1311/8260C

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sample Name	Date Collected	Date Received	Date Prepared	Days to Prep	Max Days to Prep	Date Analyzed	Days to Analysis	Max Days to Analysis	Q
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/19/19 12:00	6.85	14.00	11/19/19 13:21	6.90	14.00	

# Apex Laboratories

SDG: Gasco PreRD\_DG 2019

CLASS: GC

METHOD: 1311/8081B

**ANALYSES DATA PACKAGE COVER PAGE**

**1311/8081B**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

---

**Client Sample Id:**

PDI-142RAB-C-00-30.4-191112

**Lab Sample Id:**

A9K0412-01

**Matrix**

SO

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hardcopy data package and in computer-readable data submitted on diskette has been authorized by the Laboratory Manager or the Manager's designee, as verified by the following signatures.

Signature: \_\_\_\_\_



Name: \_\_\_\_\_

David G. Jack

Forms Created: \_\_\_\_\_

12/18/2019 12:23PM

Title: \_\_\_\_\_

Technical Manager

# METHOD DETECTION AND REPORTING LIMITS

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Charac

Batch Matrix: Soil

Analyte	MDL	MRL	Units
gamma-BHC (Lindane) [2C]	0.0000750	0.000150	mg/L
Endrin [2C]	0.0000750	0.000150	mg/L
Heptachlor [2C]	0.0000750	0.000150	mg/L
Heptachlor epoxide [2C]	0.0000750	0.000150	mg/L
Methoxychlor [2C]	0.000200	0.000400	mg/L
Chlordane (Technical) [2C]	0.000940	0.00188	mg/L
Toxaphene (Total) [2C]	0.00250	0.00500	mg/L

Note: MDLs are listed only if the corresponding analyte was evaluated to the MDL in this report .

**ORGANIC ANALYSIS DATA SHEET****1311/8081B****PDI-142RAB-C-00-30.4-191112**

Laboratory: Apex Laboratories SDG: Gasco PreRD\_DG 2019  
 Client: Anchor QEA, LLC Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization  
 Matrix: SO Laboratory ID: A9K0412-01 File ID: ECD5-11271913.D  
 Sampled: 11/12/19 15:40 Prepared: 11/26/19 14:06 Analyzed: 11/27/19 15:24  
 Preparation: EPA 1311/3510C (Neutral E) Initial/Final: 200 mL / 5 mL  
 Batch: 9111243 Sequence: 9K27028 Calibration: A9H2608 Instrument: DUALECD5

CAS NO.	COMPOUND	DILUTION	CONC. (mg/L)	Q
58-89-9	gamma-BHC (Lindane) [2C]	1	0.0000750	U
72-20-8	Endrin [2C]	1	0.0000750	U
76-44-8	Heptachlor [2C]	1	0.0000750	U
1024-57-3	Heptachlor epoxide [2C]	1	0.0000750	U
72-43-5	Methoxychlor [2C]	1	0.000200	U
12789-03-6	Chlordane (Technical) [2C]	1	0.000940	U
8001-35-2	Toxaphene (Total) [2C]	1	0.00250	U

SYSTEM MONITORING COMPOUND	ADDED (mg/L)	CONC (mg/L)	% REC	QC LIMITS	Q
2,4,5,6-TCMX (Surr) [2C]	0.00250	0.00181	72	25 - 140	
Decachlorobiphenyl (Surr) [2C]	0.00250	0.00225	90	30 - 135	

\* Values outside of QC limits

# PREPARATION BATCH SUMMARY

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Batch: 9111243 Batch Matrix: Soil

Preparation: EPA 1311/3510C (Neutral Ext.)

SAMPLE NAME	LAB SAMPLE ID	LAB FILE ID	DATE PREPARED	OBSERVATIONS
Blank	9111243-BLK1	ECD5-11271910.D	11/26/19 14:06	
LCS	9111243-BS1	ECD5-11271911.D	11/26/19 14:06	
LCS Dup	9111243-BSD1	ECD5-11271912.D	11/26/19 14:06	
PDI-142RAB-C-00-30.4-191112	A9K0412-01	ECD5-11271913.D	11/26/19 14:06	

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# METHOD BLANK DATA SHEET

**1311/8081B**

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD_DG 2019</u>		
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD_DG 2019 - 4c. Waste Characterization</u>		
Matrix: <u>Soil</u>	Laboratory ID: <u>9111243-BLK1</u>	File ID: <u>ECD5-11271910.D</u>	
Prepared: <u>11/26/19 14:06</u>	Preparation: <u>EPA 1311/3510C (Neutral E)</u>	Initial/Final: <u>200 mL / 5 mL</u>	
Analyzed: <u>11/27/19 14:32</u>	Instrument: <u>DUALECD5</u>		
Batch: <u>9111243</u>	Sequence: <u>9K27028</u>	Calibration: <u>A9H2608</u>	

CAS NO.	COMPOUND	CONC. (mg/L)	Q
58-89-9	gamma-BHC (Lindane) [2C]	0.0000750	U
72-20-8	Endrin [2C]	0.0000750	U
76-44-8	Heptachlor [2C]	0.0000750	U
1024-57-3	Heptachlor epoxide [2C]	0.0000750	U
72-43-5	Methoxychlor [2C]	0.000200	U
12789-03-6	Chlordane (Technical) [2C]	0.000940	U
8001-35-2	Toxaphene (Total) [2C]	0.00250	U

SYSTEM MONITORING COMPOUND	ADDED (mg/L)	CONC (mg/L)	% REC	QC LIMITS	Q
2,4,5,6-TCMX (Surr) [2C]	0.00250	0.00192	77	25 - 140	
Decachlorobiphenyl (Surr) [2C]	0.00250	0.00237	95	30 - 135	

# LCS / LCS DUPLICATE RECOVERY

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Matrix: Soil

Batch: 9111243

Laboratory ID: 9111243-BS1

Preparation: EPA 1311/3510C (Neutral Ext.)

Initial/Final: 200 mL / 5 mL

COMPOUND	SPIKE ADDED (mg/L)	LCS CONCENTRATION (mg/L)	LCS % REC. (*=Out)	QC LIMITS REC.
gamma-BHC (Lindane) [2C]	0.00250	0.00226	91	59 - 134
Endrin [2C]	0.00250	0.00245	98	60 - 138
Heptachlor [2C]	0.00250	0.00208	83	54 - 130
Heptachlor epoxide [2C]	0.00250	0.00223	89	61 - 133
Methoxychlor [2C]	0.00250	0.00246	98	54 - 144

\* = Values outside of QC limits



# LCS / LCS DUPLICATE RECOVERY

**1311/8081B**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Matrix: Soil

Batch: 9111243

Laboratory ID: 9111243-BSD1

Preparation: EPA 1311/3510C (Neutral Ext.)

Initial/Final: 200 mL / 5 mL

COMPOUND	SPIKE ADDED (mg/L)	LCSD CONCENTRATION (mg/L)	LCSD % REC. #	% RPD #	QC LIMITS	
					RPD	
gamma-BHC (Lindane) [2C]	0.00250	0.00214	86	6	30	59 - 134
Endrin [2C]	0.00250	0.00232	93	6	30	60 - 138
Heptachlor [2C]	0.00250	0.00191	76	9	30	54 - 130
Heptachlor epoxide [2C]	0.00250	0.00211	84	6	30	61 - 133
Methoxychlor [2C]	0.00250	0.00231	92	6	30	54 - 144

\* = Values outside of QC limits

# ANALYSIS BATCH (SEQUENCE) SUMMARY

**1311/8081B**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9H23034

Instrument: DUALECD5

Matrix: Soil

Calibration: A9H2608

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
Initial Cal Blank	9H23034-ICB1	ECD5-08231907.D	08/23/19 13:33
Cal Standard	9H23034-CAL1	ECD5-08231908.D	08/23/19 13:51
Cal Standard	9H23034-CAL2	ECD5-08231909.D	08/23/19 14:08
Cal Standard	9H23034-CAL3	ECD5-08231910.D	08/23/19 14:25
Cal Standard	9H23034-CAL4	ECD5-08231911.D	08/23/19 14:42
Cal Standard	9H23034-CAL5	ECD5-08231912.D	08/23/19 15:00
Cal Standard	9H23034-CAL6	ECD5-08231913.D	08/23/19 15:17
Cal Standard	9H23034-CAL7	ECD5-08231914.D	08/23/19 15:34
Cal Standard	9H23034-CAL8	ECD5-08231915.D	08/23/19 15:52
Initial Cal Check	9H23034-ICV1	ECD5-08231917.D	08/23/19 16:26
Cal Standard	9H23034-CALH	ECD5-08231928.D	08/23/19 19:36
Cal Standard	9H23034-CALI	ECD5-08231929.D	08/23/19 19:54
Cal Standard	9H23034-CALJ	ECD5-08231930.D	08/23/19 20:11
Cal Standard	9H23034-CALK	ECD5-08231931.D	08/23/19 20:28
Cal Standard	9H23034-CALL	ECD5-08231932.D	08/23/19 20:45
Cal Standard	9H23034-CALM	ECD5-08231933.D	08/23/19 21:02
Initial Cal Check	9H23034-ICV3	ECD5-08231935.D	08/23/19 21:37
Cal Standard	9H23034-CALN	ECD5-08231936.D	08/23/19 21:54
Cal Standard	9H23034-CALO	ECD5-08231937.D	08/23/19 22:11
Cal Standard	9H23034-CALP	ECD5-08231938.D	08/23/19 22:28
Cal Standard	9H23034-CALQ	ECD5-08231939.D	08/23/19 22:45
Cal Standard	9H23034-CALR	ECD5-08231940.D	08/23/19 23:03
Cal Standard	9H23034-CALS	ECD5-08231941.D	08/23/19 23:20
Initial Cal Check	9H23034-ICV4	ECD5-08231943.D	08/23/19 23:54

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# ANALYSIS BATCH (SEQUENCE) SUMMARY

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9K27028

Instrument: DUALECD5

Matrix: Soil

Calibration: A9H2608

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
Calibration Check	9K27028-CCV2	ECD5-11271908.D	11/27/19 13:58
Calibration Blank	9K27028-CCB1	ECD5-11271909.D	11/27/19 14:15
Blank	9111243-BLK1	ECD5-11271910.D	11/27/19 14:32
LCS	9111243-BS1	ECD5-11271911.D	11/27/19 14:49
LCS Dup	9111243-BSD1	ECD5-11271912.D	11/27/19 15:07
PDI-142RAB-C-00-30.4-191112	A9K0412-01	ECD5-11271913.D	11/27/19 15:24
Calibration Check	9K27028-CCV3	ECD5-11271914.D	11/27/19 15:41
Calibration Blank	9K27028-CCB2	ECD5-11271915.D	11/27/19 15:58

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# INITIAL CALIBRATION DATA

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Calibration: A9H2608

Instrument: DUALECD5

Calibration Date: 08/26/19 15:54

Compound	Level 01		Level 02		Level 03		Level 04		Level 05		Level 06	
	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF
gamma-BHC (Lindane)	1	207427	2	203013.5	5	204144.8	10	203485.9	25	195026.3	50	195720
gamma-BHC (Lindane) [2C]	1	352286	2	345461	5	348535.4	10	347673.3	25	340335.4	50	347621.4
Endrin	1	156412	2	149257.5	5	147790.6	10	147550.8	25	140356.2	50	139591.4
Endrin [2C]	1	222882	2	212444.5	5	218575.4	10	224448.3	25	213035.3	50	220307.6
Heptachlor	1	192066	2	184807.5	5	179818.2	10	181962.1	25	172572.2	50	174703.2
Heptachlor [2C]	1	309811	2	293382.5	5	301643.6	10	300591.5	25	291291.3	50	291902.8
Heptachlor epoxide	1	200503	2	196026	5	184724	10	186542.8	25	173771.4	50	177386
Heptachlor epoxide [2C]	1	310098	2	303120	5	291188.2	10	295930.1	25	282589.2	50	296755.8
Methoxychlor	1	59659	2	55733	5	54077.6	10	56170.6	25	55611.32	50	57213.66
Methoxychlor [2C]	1	95155	2	89037	5	82760.4	10	88306.9	25	86666.36	50	86923.98
2,4,5,6-TCMX (Surr)	1	176748	2	174986	5	166841.2	10	164444.7	25	160633.3	50	161429.6
2,4,5,6-TCMX (Surr) [2C]	1	300053	2	300383	5	287575.2	10	286585.4	25	282916.9	50	283935
Decachlorobiphenyl (Surr)	1	163865	2	154952	5	140210	10	133546.8	25	133705.4	50	133579.8
Decachlorobiphenyl (Surr) [2C]	1	191572	2	195003	5	174184.2	10	167872.8	25	166529.2	50	174613.8

# INITIAL CALIBRATION DATA (Continued)

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Character

Calibration: A9H2608

Instrument: DUALECD5

Matrix:

Calibration Date: 08/26/19 15:54

Compound	Level 07		Level 08		Level 09		Level 10		Level 11		Level 12	
	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF
gamma-BHC (Lindane)	100	195950.9	200	209448.6								
gamma-BHC (Lindane) [2C]	100	367889.9	200	403828.4								
Endrin	100	138127.1	200	157131.5								
Endrin [2C]	100	231024.1	200	263897.9								
Heptachlor	100	175515.3	200	188928.5								
Heptachlor [2C]	100	302778.2	200	356415.9								
Heptachlor epoxide	100	173184.4	200	181290.8								
Heptachlor epoxide [2C]	100	300455.1	200	326650.4								
Methoxychlor	100	58773.29	200	71355.7								
Methoxychlor [2C]	100	94449.87	200	118570.5								
2,4,5,6-TCMX (Surr)	100	158509.2	200	164212.7								
2,4,5,6-TCMX (Surr) [2C]	100	292563.3	200	312922.3								
Decachlorobiphenyl (Surr)	100	134054	200	134876.2								
Decachlorobiphenyl (Surr) [2C]	100	177840.7	200	190488.9								

# INITIAL CALIBRATION DATA (Continued)

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Character

Calibration: A9H2608

Instrument: DUALECD5

Matrix:

Calibration Date: 08/26/19 15:54

Compound	Level 13		Level 14		Level 15		Level 16		Level 17		Level 18	
	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF
Chlordane 1 (g)									50	20182.86	100	19788.97
Chlordane 2									50	25733.1	100	25195.2
Chlordane 3 (a)									50	5761.74	100	5481.96
Chlordane (Technical)									50	<del>407.3</del>	100	<del>49.38</del>
Chlordane 1 (g) [2C]									50	35094.14	100	33783.88
Chlordane 2 (a) [2C]									50	29448	100	29059.41
Chlordane 3 [2C]									50	8780.4	100	8744.65
Chlordane (Technical) [2C]									50	0	100	0

## SECOND-SOURCE CALIBRATION VERIFICATION

1311/8081B

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD DG 2019</u>
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD_DG 2019 - 4c. Waste Charac</u>
Instrument ID: <u>DUALECD5</u>	Calibration: <u>A9H2608</u>
Lab File ID: <u>ECD5-08231917.D</u>	
Sequence: <u>9H23034</u>	Inject Date: <u>08/23/19</u>
Lab Sample ID: <u>9H23034-ICV1</u>	Inject Time: <u>16:26</u>

ANALYTE	EXPECTED (ng/mL)	FOUND (ng/mL)	% DRIFT	QC LIMIT
gamma-BHC (Lindane)	50.0	51.4	2.8	70 - 130
gamma-BHC (Lindane) [2C]	50.0	52.7	5.5	70 - 130
Endrin	50.0	52.7	5.4	70 - 130
Endrin [2C]	50.0	53.1	6.3	70 - 130
Heptachlor	50.0	51.2	2.4	70 - 130
Heptachlor [2C]	50.0	52.3	4.6	70 - 130
Heptachlor epoxide	50.0	50.1	0.1	70 - 130
Heptachlor epoxide [2C]	50.0	51.4	2.7	70 - 130
Methoxychlor	50.0	55.4	10.7	70 - 130
Methoxychlor [2C]	50.0	56.3	12.5	70 - 130
2,4,5,6-TCMX (Surr)	50.0	49.5	-1.1	70 - 130
2,4,5,6-TCMX (Surr) [2C]	50.0	49.3	-1.4	70 - 130
Decachlorobiphenyl (Surr)	50.0	49.1	-1.8	70 - 130
Decachlorobiphenyl (Surr) [2C]	50.0	48.2	-3.6	70 - 130

# SECOND-SOURCE CALIBRATION VERIFICATION

1311/8081B

Laboratory: Apex Laboratories SDG: Gasco PreRD DG 2019  
Client: Anchor QEA, LLC Project: Gasco PreRD\_DG 2019 - 4c. Waste Charac  
Instrument ID: DUALECD5 Calibration: A9H2608  
Lab File ID: ECD5-08231935.D  
Sequence: 9H23034 Inject Date: 08/23/19  
Lab Sample ID: 9H23034-ICV3 Inject Time: 21:37

ANALYTE	EXPECTED (ng/mL)	FOUND (ng/mL)	% DRIFT	QC LIMIT
Chlordane 1 (g)	500	545	8.9	65 - 135
Chlordane 2	500	535	6.9	65 - 135
Chlordane 3 (a)	500	550	9.9	65 - 135
Chlordane (Technical)	500	543	8.6	65 - 135
Chlordane 1 (g) [2C]	500	549	9.8	65 - 135
Chlordane 2 (a) [2C]	500	536	7.3	65 - 135
Chlordane 3 [2C]	500	541	8.2	65 - 135
Chlordane (Technical) [2C]	500	542	8.4	65 - 135



## SECOND-SOURCE CALIBRATION VERIFICATION

**1311/8081B**

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD DG 2019</u>
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD_DG 2019 - 4c. Waste Charac</u>
Instrument ID: <u>DUALECD5</u>	Calibration: <u>A9H2608</u>
Lab File ID: <u>ECD5-08231943.D</u>	
Sequence: <u>9H23034</u>	Inject Date: <u>08/23/19</u>
Lab Sample ID: <u>9H23034-ICV4</u>	Inject Time: <u>23:54</u>

ANALYTE	EXPECTED (ng/mL)	FOUND (ng/mL)	% DRIFT	QC LIMIT
Toxaphene 1	500	476	-4.9	65 - 135
Toxaphene 2	500	474	-5.1	65 - 135
Toxaphene 3	500	487	-2.7	65 - 135
Toxaphene 4	500	485	-3.0	65 - 135
Toxaphene 5	500	495	-1.0	65 - 135
Toxaphene 6	500	489	-2.2	65 - 135
Toxaphene (Total)	500	484	-3.2	65 - 135
Toxaphene 1 [2C]	500	477	-4.5	65 - 135
Toxaphene 2 [2C]	500	492	-1.6	65 - 135
Toxaphene 3 [2C]	500	483	-3.4	65 - 135
Toxaphene 4 [2C]	500	484	-3.1	65 - 135
Toxaphene 5 [2C]	500	488	-2.3	65 - 135
Toxaphene 6 [2C]	500	498	-0.5	65 - 135
Toxaphene (Total) [2C]	500	487	-2.6	65 - 135

# CONTINUING CALIBRATION CHECK

**1311/8081B**

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Instrument ID: DUALECD5

Calibration: A9H2608

Lab File ID: ECD5-11271908.D

Calibration Date: 08/26/19 15:54

Sequence: 9K27028

Injection Date: 11/27/19

Lab Sample ID: 9K27028-CCV2

Injection Time: 13:58

COMPOUND	Curve Fit	Calculated Concentration (ng/mL) [L/Q Fits]			Response Factors [Ave RF]			Limit
		STD	CCV	% DIFF	ICAL	CCV	% Drift	
gamma-BHC (Lindane)	Ave	50.0	49.4		201777.1	199374.5	-1.2	20
gamma-BHC (Lindane) [2C]	Ave	50.0	48.4		356703.9	345123.6	-3.2	20
Endrin	Ave	50.0	50.3		147027.1	147939.5	0.6	20
Endrin [2C]	Ave	50.0	51.0		225826.9	230396.2	2.0	20
Heptachlor	Ave	50.0	49.0		181296.6	177753.2	-2.0	20
Heptachlor [2C]	Ave	50.0	47.3		305977.1	289243	-5.5	20
Heptachlor epoxide	Ave	50.0	48.2		184178.6	177687.2	-3.5	20
Heptachlor epoxide [2C]	Ave	50.0	47.3		300848.3	284722.4	-5.4	20
Methoxychlor	Ave	50.0	52.8		58574.27	61856.6	5.6	20
Methoxychlor [2C]	XXX	50.0	51.3	2.7				20

\*\* Quadratic Curve fit may be weighted (1/a or 1/a<sup>2</sup>).

\* = Values outside of QC limits

# CONTINUING CALIBRATION CHECK

**1311/8081B**

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Instrument ID: DUALECD5

Calibration: A9H2608

Lab File ID: ECD5-11271914.D

Calibration Date: 08/26/19 15:54

Sequence: 9K27028

Injection Date: 11/27/19

Lab Sample ID: 9K27028-CCV3

Injection Time: 15:41

COMPOUND	Curve Fit	Calculated Concentration (ng/mL) [L/Q Fits]			Response Factors [Ave RF]			Limit
		STD	CCV	% DIFF	ICAL	CCV	% Drift	
gamma-BHC (Lindane)	Ave	100	93.0		201777.1	187555.7	-7.0	20
gamma-BHC (Lindane) [2C]	Ave	100	96.9		356703.9	345527	-3.1	20
Endrin	Ave	100	95.7		147027.1	140633.1	-4.3	20
Endrin [2C]	Ave	100	98.7		225826.9	222910.7	-1.3	20
Heptachlor	Ave	100	92.1		181296.6	166908.4	-7.9	20
Heptachlor [2C]	Ave	100	95.5		305977.1	292224.6	-4.5	20
Heptachlor epoxide	Ave	100	91.6		184178.6	168772.2	-8.4	20
Heptachlor epoxide [2C]	Ave	100	94.3		300848.3	283652	-5.7	20
Methoxychlor	Ave	100	93.3		58574.27	54635.79	-6.7	20
Methoxychlor [2C]	XXX	100	91.3	-8.7				20

\*\* Quadratic Curve fit may be weighted (1/a or 1/a<sup>2</sup>).

\* = Values outside of QC limits

# SURROGATE STANDARD RECOVERY AND RT SUMMARY

1311/8081B

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD DG 2019</u>
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD DG 2019 - 4c. Waste Characterization</u>
Sequence: <u>9H23034</u>	Instrument: <u>DUALECD5</u>
Matrix: <u>Soil</u>	Calibration: <u>A9H2608</u>

Surrogate Compound	Spike Level ng/mL	% Recovery	Recovery Limits	RT	Calibration Mean RT	RT Diff	RT Diff Limit	Q
<b>Initial Cal Check (9H23034-ICV1 )</b>			Lab File ID: ECD5-08231917.D		Analyzed: 08/23/19 16:26			
2,4,5,6-TCMX (Surr)	50.0	99	70 - 130	5.395	5.39525	-0.0003	+/-1.0	
2,4,5,6-TCMX (Surr) [2C]	50.0	99	70 - 130	5.989	5.98975	-0.0008	+/-1.0	
Decachlorobiphenyl (Surr)	50.0	98	70 - 130	9.589	9.5925	-0.0035	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	50.0	96	70 - 130	10.539	10.54062	-0.0016	+/-1.0	

# SURROGATE STANDARD RECOVERY AND RT SUMMARY

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sequence: 9K27028

Instrument: DUALECD5

Matrix: Soil

Calibration: A9H2608

Surrogate Compound	Spike Level ng/mL	% Recovery	Recovery Limits	RT	Calibration Mean RT	RT Diff	RT Diff Limit	Q
<b>Calibration Check (9K27028-CCV2 )</b> Lab File ID: ECD5-11271908.D Analyzed: 11/27/19 13:58								
2,4,5,6-TCMX (Surr)	50.0	100	80 - 120	5.216	5.39525	-0.1793	+/-1.0	
2,4,5,6-TCMX (Surr) [2C]	50.0	98	80 - 120	5.807	5.98975	-0.1828	+/-1.0	
Decachlorobiphenyl (Surr)	50.0	93	80 - 120	9.401	9.5925	-0.1915	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	50.0	101	80 - 120	10.317	10.54062	-0.2236	+/-1.0	
<b>Calibration Blank (9K27028-CCB1 )</b> Lab File ID: ECD5-11271909.D Analyzed: 11/27/19 14:15								
2,4,5,6-TCMX (Surr) [2C]	100	92	25 - 140	5.806	5.98975	-0.1838	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	100	94	30 - 135	10.318	10.54062	-0.2226	+/-1.0	
<b>Blank (9111243-BLK1 )</b> Lab File ID: ECD5-11271910.D Analyzed: 11/27/19 14:32								
2,4,5,6-TCMX (Surr) [2C]	0.00250	77	25 - 140	5.805	5.98975	-0.1848	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	0.00250	95	30 - 135	10.317	10.54062	-0.2236	+/-1.0	
<b>LCS (9111243-BS1 )</b> Lab File ID: ECD5-11271911.D Analyzed: 11/27/19 14:49								
2,4,5,6-TCMX (Surr) [2C]	0.00250	79	25 - 140	5.805	5.98975	-0.1848	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	0.00250	94	30 - 135	10.315	10.54062	-0.2256	+/-1.0	
<b>LCS Dup (9111243-BSD1 )</b> Lab File ID: ECD5-11271912.D Analyzed: 11/27/19 15:07								
2,4,5,6-TCMX (Surr) [2C]	0.00250	75	25 - 140	5.804	5.98975	-0.1858	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	0.00250	81	30 - 135	10.316	10.54062	-0.2246	+/-1.0	
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01 )</b> Lab File ID: ECD5-11271913.D Analyzed: 11/27/19 15:24								
2,4,5,6-TCMX (Surr) [2C]	0.00250	72	25 - 140	5.803	5.98975	-0.1868	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	0.00250	90	30 - 135	10.314	10.54062	-0.2266	+/-1.0	
<b>Calibration Check (9K27028-CCV3 )</b> Lab File ID: ECD5-11271914.D Analyzed: 11/27/19 15:41								
2,4,5,6-TCMX (Surr)	100	98	80 - 120	5.214	5.39525	-0.1812	+/-1.0	
2,4,5,6-TCMX (Surr) [2C]	100	98	80 - 120	5.805	5.98975	-0.1848	+/-1.0	
Decachlorobiphenyl (Surr)	100	91	80 - 120	9.399	9.5925	-0.1935	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	100	105	80 - 120	10.315	10.54062	-0.2256	+/-1.0	
<b>Calibration Blank (9K27028-CCB2 )</b> Lab File ID: ECD5-11271915.D Analyzed: 11/27/19 15:58								
2,4,5,6-TCMX (Surr) [2C]	100	87	25 - 140	5.804	5.98975	-0.1858	+/-1.0	
Decachlorobiphenyl (Surr) [2C]	100	98	30 - 135	10.314	10.54062	-0.2266	+/-1.0	

# HOLDING TIME SUMMARY

1311/8081B

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sample Name	Date Collected	Date Received	Date Prepared	Days to Prep	Max Days to Prep	Date Analyzed	Days to Analysis	Max Days to Analysis	Q
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/26/19 14:06	13.93	7.00	11/27/19 15:24	1.05	40.00	*

# Apex Laboratories

SDG: Gasco PreRD\_DG 2019

CLASS: GCMS

METHOD: 1311/8270D

# ANALYSES DATA PACKAGE COVER PAGE

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

---

**Client Sample Id:**

PDI-142RAB-C-00-30.4-191112

**Lab Sample Id:**

A9K0412-01

**Matrix**

SO

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hardcopy data package and in computer-readable data submitted on diskette has been authorized by the Laboratory Manager or the Manager's designee, as verified by the following signatures.

Signature: \_\_\_\_\_



Name: \_\_\_\_\_

David G. Jack

Forms Created: \_\_\_\_\_

12/18/2019 12:23PM

Title: \_\_\_\_\_

Technical Manager



# METHOD DETECTION AND REPORTING LIMITS

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Charac

Batch Matrix: Soil

Analyte	MDL	MRL	Units
2,4-Dinitrotoluene	0.00100	0.00200	mg/L
Hexachlorobenzene	0.00100	0.00200	mg/L
Hexachlorobutadiene	0.00250	0.00500	mg/L
Hexachloroethane	0.00250	0.00500	mg/L
2-Methylphenol	0.00250	0.00500	mg/L
3+4-Methylphenol(s)	0.00250	0.00500	mg/L
Nitrobenzene	0.00250	0.00500	mg/L
Pentachlorophenol (PCP)	0.00500	0.0100	mg/L
Pyridine	0.00500	0.0100	mg/L
2,4,5-Trichlorophenol	0.00250	0.00500	mg/L
2,4,6-Trichlorophenol	0.00250	0.00500	mg/L

Note: MDLs are listed only if the corresponding analyte was evaluated to the MDL in this report .

# ORGANIC ANALYSIS DATA SHEET

1311/8270D

PDI-142RAB-C-00-30.4-191112

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD_DG 2019</u>	
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD_DG 2019 - 4c. Waste Characterization</u>	
Matrix: <u>SO</u>	Laboratory ID: <u>A9K0412-01RE1</u>	File ID: <u>J11271913.D</u>
Sampled: <u>11/12/19 15:40</u>	Prepared: <u>11/26/19 14:05</u>	Analyzed: <u>11/27/19 15:20</u>
	Preparation: <u>EPA 1311/3510C (BNA Extr</u>	Initial/Final: <u>200 mL / 2 mL</u>
Batch: <u>9111242</u>	Sequence: <u>9K27012</u>	Calibration: <u>A9I2405</u> Instrument: <u>SV-GCMS10</u>

CAS NO.	COMPOUND	DILUTION	CONC. (mg/L)	Q
121-14-2	2,4-Dinitrotoluene	10	0.0100	U
118-74-1	Hexachlorobenzene	10	0.0100	U
87-68-3	Hexachlorobutadiene	10	0.0250	U
67-72-1	Hexachloroethane	10	0.0250	U
95-48-7	2-Methylphenol	10	0.0250	U
NA	3+4-Methylphenol(s)	10	0.0250	U
98-95-3	Nitrobenzene	10	0.0250	U
87-86-5	Pentachlorophenol (PCP)	10	0.0500	U
110-86-1	Pyridine	10	0.0500	U
95-95-4	2,4,5-Trichlorophenol	10	0.0250	U
88-06-2	2,4,6-Trichlorophenol	10	0.0250	U

SYSTEM MONITORING COMPOUND	ADDED (mg/L)	CONC (mg/L)	% REC	QC LIMITS	Q
Nitrobenzene-d5 (Surr)	0.0250	0.0187	75	44 - 120	
2-Fluorobiphenyl (Surr)	0.0250	0.0228	91	44 - 120	
Phenol-d6 (Surr)	0.0250	0.00476	19	10 - 120	
p-Terphenyl-d14 (Surr)	0.0250	0.0268	107	50 - 133	
2-Fluorophenol (Surr)	0.0250	0.0100	40	19 - 120	
2,4,6-Tribromophenol (Surr)	0.0250	0.0221	89	43 - 140	

INTERNAL STANDARD	AREA	RT	REF AREA	REF RT	Q
1,4-Dichlorobenzene-d4 (ISTD)	387154	6.381	368375	6.381	
Naphthalene-d8 (ISTD)	1427888	7.648	1412968	7.648	
Acenaphthene-d10 (ISTD)	747611	9.424	751566	9.424	
Phenanthrene-d10 (ISTD)	1321721	10.932	1376916	10.938	
Chrysene-d12 (ISTD)	1317590	14.526	1352496	14.532	

\* Values outside of QC limits

# PREPARATION BATCH SUMMARY

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Batch: 9111242 Batch Matrix: Soil

Preparation: EPA 1311/3510C (BNA Extraction)

SAMPLE NAME	LAB SAMPLE ID	LAB FILE ID	DATE PREPARED	OBSERVATIONS
Blank	9111242-BLK1	J11261919.D	11/26/19 14:05	
LCS	9111242-BS1	J11261920.D	11/26/19 14:05	
LCS Dup	9111242-BSD1	J11261921.D	11/26/19 14:05	
PDI-142RAB-C-00-30.4-191112	A9K0412-01RE1	J11271913.D	11/26/19 14:05	

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# METHOD BLANK DATA SHEET

**1311/8270D**

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD_DG 2019</u>	
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD_DG 2019 - 4c. Waste Characterization</u>	
Matrix: <u>Soil</u>	Laboratory ID: <u>9111242-BLK1</u>	File ID: <u>J11261919.D</u>
Prepared: <u>11/26/19 14:05</u>	Preparation: <u>EPA 1311/3510C (BNA Extr</u>	Initial/Final: <u>200 mL / 2 mL</u>
Analyzed: <u>11/26/19 18:39</u>	Instrument: <u>SV-GCMS10</u>	
Batch: <u>9111242</u>	Sequence: <u>9K26022</u>	Calibration: <u>A9I2405</u>

CAS NO.	COMPOUND	CONC. (mg/L)	Q
121-14-2	2,4-Dinitrotoluene	0.00100	U
118-74-1	Hexachlorobenzene	0.00100	U
87-68-3	Hexachlorobutadiene	0.00250	U
67-72-1	Hexachloroethane	0.00250	U
95-48-7	2-Methylphenol	0.00250	U
NA	3+4-Methylphenol(s)	0.00250	U
98-95-3	Nitrobenzene	0.00250	U
87-86-5	Pentachlorophenol (PCP)	0.00500	U
110-86-1	Pyridine	0.00500	U
95-95-4	2,4,5-Trichlorophenol	0.00250	U
88-06-2	2,4,6-Trichlorophenol	0.00250	U

SYSTEM MONITORING COMPOUND	ADDED (mg/L)	CONC (mg/L)	% REC	QC LIMITS	Q
Nitrobenzene-d5 (Surr)	0.0250	0.0141	56	44 - 120	
2-Fluorobiphenyl (Surr)	0.0250	0.0150	60	44 - 120	
Phenol-d6 (Surr)	0.0250	0.00454	18	10 - 120	
p-Terphenyl-d14 (Surr)	0.0250	0.0196	79	50 - 133	
2-Fluorophenol (Surr)	0.0250	0.00855	34	19 - 120	
2,4,6-Tribromophenol (Surr)	0.0250	0.0190	76	43 - 140	

INTERNAL STANDARD	AREA	RT	REF AREA	REF RT	Q
1,4-Dichlorobenzene-d4 (ISTD)	447964	6.386	361048	6.38	
Naphthalene-d8 (ISTD)	1661730	7.648	1385010	7.648	
Acenaphthene-d10 (ISTD)	889317	9.424	748930	9.424	
Phenanthrene-d10 (ISTD)	1567268	10.938	1388573	10.937	
Chrysene-d12 (ISTD)	1665591	14.532	1350896	14.526	

# LCS / LCS DUPLICATE RECOVERY

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Matrix: Soil

Batch: 9111242

Laboratory ID: 9111242-BS1

Preparation: EPA 1311/3510C (BNA Extraction)

Initial/Final: 200 mL / 2 mL

COMPOUND	SPIKE ADDED (mg/L)	LCS CONCENTRATION (mg/L)	LCS % REC. (*=Out)	QC LIMITS REC.
2,4-Dinitrotoluene	0.0400	0.0368	92	57 - 128
Hexachlorobenzene	0.0400	0.0336	84	52 - 125
Hexachlorobutadiene	0.0400	0.0313	78	22 - 124
Hexachloroethane	0.0400	0.0314	78	21 - 120
2-Methylphenol	0.0400	0.0275	69	30 - 120
3+4-Methylphenol(s)	0.0400	0.0250	63	29 - 120
Nitrobenzene	0.0400	0.0284	71	45 - 121
Pentachlorophenol (PCP)	0.0400	0.0332	83	35 - 138
Pyridine	0.0400	0.0139	35	5 - 120
2,4,5-Trichlorophenol	0.0400	0.0384	96	53 - 123
2,4,6-Trichlorophenol	0.0400	0.0370	92	50 - 125

\* = Values outside of QC limits

# LCS / LCS DUPLICATE RECOVERY

**1311/8270D**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Matrix: Soil

Batch: 9111242

Laboratory ID: 9111242-BSD1

Preparation: EPA 1311/3510C (BNA Extraction)

Initial/Final: 200 mL / 2 mL

COMPOUND	SPIKE ADDED (mg/L)	LCSD CONCENTRATION (mg/L)	LCSD % REC. #	% RPD #	QC LIMITS	
					RPD	
2,4-Dinitrotoluene	0.0400	0.0363	91	1	30	57 - 128
Hexachlorobenzene	0.0400	0.0340	85	1	30	52 - 125
Hexachlorobutadiene	0.0400	0.0305	76	3	30	22 - 124
Hexachloroethane	0.0400	0.0291	73	8	30	21 - 120
2-Methylphenol	0.0400	0.0264	66	4	30	30 - 120
3+4-Methylphenol(s)	0.0400	0.0240	60	4	30	29 - 120
Nitrobenzene	0.0400	0.0281	70	1	30	45 - 121
Pentachlorophenol (PCP)	0.0400	0.0337	84	1	30	35 - 138
Pyridine	0.0400	0.0125	31	10	30	5 - 120
2,4,5-Trichlorophenol	0.0400	0.0368	92	4	30	53 - 123
2,4,6-Trichlorophenol	0.0400	0.0369	92	0.2	30	50 - 125

\* = Values outside of QC limits

# ANALYSIS BATCH (SEQUENCE) SUMMARY

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9I19035

Instrument: SV-GCMS10

Matrix: Soil

Calibration: A9I2405

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
MS Tune	9I19035-TUN1	J09191916.D	09/20/19 00:22
Initial Cal Blank	9I19035-ICB1	J09191917.D	09/20/19 00:49
Cal Standard	9I19035-CAL1	J09191918.D	09/20/19 01:24
Cal Standard	9I19035-CAL2	J09191919.D	09/20/19 01:59
Cal Standard	9I19035-CAL3	J09191920.D	09/20/19 02:34
Cal Standard	9I19035-CAL4	J09191921.D	09/20/19 03:09
Cal Standard	9I19035-CAL5	J09191922.D	09/20/19 03:44
Cal Standard	9I19035-CAL6	J09191923.D	09/20/19 04:19
Cal Standard	9I19035-CAL7	J09191924.D	09/20/19 04:54
Cal Standard	9I19035-CAL8	J09191925.D	09/20/19 05:29
Cal Standard	9I19035-CAL9	J09191926.D	09/20/19 06:04
Cal Standard	9I19035-CALA	J09191927.D	09/20/19 06:39
Initial Cal Check	9I19035-ICV1	J09191929.D	09/20/19 07:50

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# ANALYSIS BATCH (SEQUENCE) SUMMARY

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9K26022

Instrument: SV-GCMS10

Matrix: Soil

Calibration: A9I2405

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
MS Tune	9K26022-TUN2	J11261904.D	11/26/19 09:49
Calibration Check	9K26022-CCV2	J11261905.D	11/26/19 10:16
Calibration Blank	9K26022-CCB1	J11261906.D	11/26/19 10:52
Blank	9111242-BLK1	J11261919.D	11/26/19 18:39
LCS	9111242-BS1	J11261920.D	11/26/19 19:16
LCS Dup	9111242-BSD1	J11261921.D	11/26/19 19:52

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.



# ANALYSIS BATCH (SEQUENCE) SUMMARY

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9K27012

Instrument: SV-GCMS10

Matrix: Soil

Calibration: A9I2405

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
MS Tune	9K27012-TUN2	J11271904.D	11/27/19 10:07
Calibration Check	9K27012-CCV2	J11271905.D	11/27/19 10:34
Calibration Blank	9K27012-CCB1	J11271906.D	11/27/19 11:10
PDI-142RAB-C-00-30.4-191112	A9K0412-01RE1	J11271913.D	11/27/19 15:20

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# MASS SPECTROMETER INSTRUMENT PERFORMANCE CHECK

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Lab File ID: J09191916.D

Injection Date: 09/20/19

Instrument ID: SV-GCMS10

Injection Time: 00:22

Sequence: 9I19035

Lab Sample ID: 9I19035-TUN1

m/z	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE	
m/z 68	Less than 2% of m/z 69	1.61	PASS
m/z 69	Base peak, 100% relative abundance	100.00	PASS
m/z 70	Less than 2% of m/z 69	0.51	PASS
m/z 197	Less than 2% of m/z 198	0.00	PASS
m/z 198	Base peak, 100% relative abundance	100.00	PASS
m/z 199	5 - 9% of m/z 198	6.90	PASS
m/z 365	1 - 100% of m/z 198	3.17	PASS
m/z 441	Less than 150% of m/z 443	73.90	PASS
m/z 442	0.1 - 200% of m/z 198	95.52	PASS
m/z 443	15 - 24% of m/z 442	19.71	PASS

# MASS SPECTROMETER INSTRUMENT PERFORMANCE CHECK

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Lab File ID: J11261904.D

Injection Date: 11/26/19

Instrument ID: SV-GCMS10

Injection Time: 09:49

Sequence: 9K26022

Lab Sample ID: 9K26022-TUN2

m/z	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE	
m/z 68	Less than 2% of m/z 69	1.33	PASS
m/z 69	Base peak, 100% relative abundance	100.00	PASS
m/z 70	Less than 2% of m/z 69	0.56	PASS
m/z 197	Less than 2% of m/z 198	0.00	PASS
m/z 198	Base peak, 100% relative abundance	100.00	PASS
m/z 199	5 - 9% of m/z 198	7.11	PASS
m/z 365	1 - 100% of m/z 198	3.56	PASS
m/z 441	Less than 150% of m/z 443	76.36	PASS
m/z 442	0.1 - 200% of m/z 198	112.47	PASS
m/z 443	15 - 24% of m/z 442	20.09	PASS

# MASS SPECTROMETER INSTRUMENT PERFORMANCE CHECK

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Lab File ID: J11271904.D

Injection Date: 11/27/19

Instrument ID: SV-GCMS10

Injection Time: 10:07

Sequence: 9K27012

Lab Sample ID: 9K27012-TUN2

m/z	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE	
m/z 68	Less than 2% of m/z 69	1.30	PASS
m/z 69	Base peak, 100% relative abundance	100.00	PASS
m/z 70	Less than 2% of m/z 69	0.41	PASS
m/z 197	Less than 2% of m/z 198	0.00	PASS
m/z 198	Base peak, 100% relative abundance	100.00	PASS
m/z 199	5 - 9% of m/z 198	7.03	PASS
m/z 365	1 - 100% of m/z 198	3.42	PASS
m/z 441	Less than 150% of m/z 443	76.66	PASS
m/z 442	0.1 - 200% of m/z 198	109.59	PASS
m/z 443	15 - 24% of m/z 442	19.86	PASS

# INITIAL CALIBRATION DATA (Summary)

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Calibration: A9I2405

Date: 09/24/19 12:40

Instrument: SV-GCMS10

Compound	Mean RF	FIT	RF RSD	Mean RT	RT RSD	Linear r	Quad COD	LIMIT	Q
2,4-Dinitrotoluene	0.3649887	XXX	21.34667	9.806875	0.113925				
Hexachlorobenzene	0.2707358	Ave	10.60551	10.7482	4.451335E-02			20	
Hexachlorobutadiene	0.1891523	Ave	6.739156	7.9913	2.888985E-02			20	
Hexachloroethane	0.4806864	Ave	5.451873	7.077	2.898215E-02			20	
2-Methylphenol	1.03014	Ave	9.222719	6.8119	8.482721E-02			20	
3+4-Methylphenol(s)	1.277354	Ave	11.32459	6.961556	8.520401E-02			20	
Nitrobenzene	1.221036	Ave	7.439446	7.1363	0.1023456			20	
Pentachlorophenol (PCP)	0.1189653	XXX	26.10993	10.94237	3.850139E-02				
Pyridine	1.298764	Ave	10.27213	3.950556	0.8873878			20	
2,4,5-Trichlorophenol	0.3514615	XXX	18.51245	8.876	5.529415E-02				
2,4,6-Trichlorophenol	0.3575479	XXX	19.98563	8.842555	5.254443E-02				
Nitrobenzene-d5 (Surr)	1.205168	Ave	9.142619	7.1168	8.867008E-02			20	
2-Fluorobiphenyl (Surr)	1.565217	Ave	12.06569	8.927444	2.774874E-02			20	
Phenol-d6 (Surr)	1.553469	Ave	11.40827	6.2088	0.1181197			20	
p-Terphenyl-d14 (Surr)	0.9216776	Ave	6.530579	12.9267	5.442172E-02			20	
2-Fluorophenol (Surr)	1.213667	Ave	14.14738	5.3054	0.1655531			20	
2,4,6-Tribromophenol (Surr)	0.1092555	XXX	18.24175	10.42356	6.009604E-02				

Note: \*\* Quad COD may be incorrect if weighting (1/a) or (1/a<sup>2</sup>) used. Weighting not shown here. Please see instrument calibration printouts for validation.

# INITIAL CALIBRATION DATA

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Character

Calibration: A9I2405

Instrument: SV-GCMS10

Calibration Date: 09/24/19 12:40

Compound	Level 01		Level 02		Level 03		Level 04		Level 05		Level 06	
	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF
2,4-Dinitrotoluene	20	0.1603367	50	0.1627974	100	0.2214885	200	0.2765041	500	0.369336	1000	0.3982255
Hexachlorobenzene	20	0.3002082	50	0.2799895	100	0.2916868	200	0.277925	500	0.2949459	1000	0.2857907
Hexachlorobutadiene	20	0.1839228	50	0.199773	100	0.1954379	200	0.2004045	500	0.2006305	1000	0.1988902
Hexachloroethane	20	0.4342819	50	0.4549996	100	0.4516267	200	0.4715052	500	0.4944285	1000	0.4835438
2-Methylphenol	20	0.9295757	50	0.8796476	100	0.9810251	200	1.076563	500	1.154826	1000	1.147864
3+4-Methylphenol(s)	20	1.06531	50	1.132761	100	1.159969	200	1.345101	500	1.440506	1000	1.458462
Nitrobenzene	20	1.075593	50	1.183026	100	1.189288	200	1.30162	500	1.340887	1000	1.326686
Pentachlorophenol (PCP)	20	8.691609E-02	50	5.118127E-02	100	7.761508E-02	200	6.955638E-02	500	0.1080871	1000	0.1222728
Pyridine	20	0.7561372	50	1.052968	100	1.276558	200	1.345625	500	1.118092	1000	1.285171
2,4,5-Trichlorophenol	20	0.1901559	50	0.2373804	100	0.2701951	200	0.3011386	500	0.3811527	1000	0.3898394
2,4,6-Trichlorophenol	20	0.1746999	50	0.2365366	100	0.2572544	200	0.3068435	500	0.3835634	1000	0.4024493
Nitrobenzene-d5 (Surr)	20	0.9806475	50	1.085379	100	1.135054	200	1.209032	500	1.31341	1000	1.321832
2-Fluorobiphenyl (Surr)	20	1.476909	50	1.609929	100	1.734744	200	1.751334	500	1.739556	1000	1.652173
Phenol-d6 (Surr)	20	1.197274	50	1.304845	100	1.445522	200	1.602349	500	1.667059	1000	1.681755
p-Terphenyl-d14 (Surr)	20	0.8205178	50	0.9023018	100	0.9773009	200	0.9592621	500	0.994643	1000	0.9688955
2-Fluorophenol (Surr)	20	0.9398586	50	1.045277	100	0.9521188	200	1.216931	500	1.280008	1000	1.263499
2,4,6-Tribromophenol (Surr)	20	6.623006E-02	50	7.092577E-02	100	8.598271E-02	200	9.861561E-02	500	0.1200291	1000	0.122147

# INITIAL CALIBRATION DATA (Continued)

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Character

Calibration: A9I2405

Instrument: SV-GCMS10

Matrix:

Calibration Date: 09/24/19 12:40

Compound	Level 07		Level 08		Level 09		Level 10		Level 11		Level 12	
	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF	ng/mL	RF
2,4-Dinitrotoluene	2000	0.4391508	4000	0.4369418	6000	0.4126319	8000	0.3656313				
Hexachlorobenzene	2000	0.2793127	4000	0.2519446	6000	0.2310087	8000	0.2145459				
Hexachlorobutadiene	2000	0.1905242	4000	0.1849175	6000	0.1738819	8000	0.1631409				
Hexachloroethane	2000	0.5034331	4000	0.5096268	6000	0.5004542	8000	0.5029646				
2-Methylphenol	2000	1.116896	4000	1.057322	6000	1.00091	8000	0.9567711				
3+4-Methylphenol(s)	2000	1.400529	4000	1.304656	6000	1.18889	8000	<del>1.118737</del>				
Nitrobenzene	2000	1.280974	4000	1.234394	6000	1.165306	8000	1.112587				
Pentachlorophenol (PCP)	2000	0.1418302	4000	0.1484859	6000	0.1453844	8000	0.1384905				
Pyridine	2000	1.375861	4000	1.417463	6000	1.442542	8000	1.374592				
2,4,5-Trichlorophenol	2000	0.4178827	4000	0.4063886	6000	0.3928207	8000	0.3663551				
2,4,6-Trichlorophenol	2000	0.4232436	4000	0.4186057	6000	0.4009108	8000	0.3885235				
Nitrobenzene-d5 (Surr)	2000	1.281854	4000	1.28613	6000	1.24582	8000	1.192526				
2-Fluorobiphenyl (Surr)	2000	1.564374	4000	1.350787	6000	1.207146	8000	<del>1.092707</del>				
Phenol-d6 (Surr)	2000	1.673553	4000	1.705426	6000	1.658679	8000	1.598233				
p-Terphenyl-d14 (Surr)	2000	0.953339	4000	0.9235964	6000	0.8801238	8000	0.8367959				
2-Fluorophenol (Surr)	2000	1.332531	4000	1.380766	6000	1.371479	8000	1.354202				
2,4,6-Tribromophenol (Surr)	2000	0.1302975	4000	0.1246898	6000	0.1182398	8000	0.1123724				

## SECOND-SOURCE CALIBRATION VERIFICATION

1311/8270D

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD DG 2019</u>	
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD_DG 2019 - 4c. Waste Charac</u>	
Instrument ID: <u>SV-GCMS10</u>	Calibration: <u>A9I2405</u>	
Lab File ID: <u>J09191929.D</u>		
Sequence: <u>9I19035</u>	Inject Date: <u>09/20/19</u>	
Lab Sample ID: <u>9I19035-ICV1</u>	Inject Time: <u>07:50</u>	

ANALYTE	EXPECTED (ng/mL)	FOUND (ng/mL)	% DRIFT	QC LIMIT
2,4-Dinitrotoluene	1000	1050	4.8	70 - 130
Hexachlorobenzene	1000	1010	1.0	70 - 130
Hexachlorobutadiene	1000	1040	3.7	70 - 130
Hexachloroethane	1000	1040	4.1	70 - 130
2-Methylphenol	1000	1050	5.3	70 - 130
3+4-Methylphenol(s)	1000	1070	6.7	70 - 130
Nitrobenzene	1000	1060	5.8	70 - 130
Pentachlorophenol (PCP)	1000	976	-2.4	70 - 130
Pyridine	1000	896	-10.4	70 - 130
2,4,5-Trichlorophenol	1000	1050	4.8	70 - 130
2,4,6-Trichlorophenol	1000	1030	3.4	70 - 130
Nitrobenzene-d5 (Surr)	1000	1070	6.6	70 - 130
2-Fluorobiphenyl (Surr)	1000	1060	6.2	70 - 130
Phenol-d6 (Surr)	1000	1020	1.6	70 - 130
p-Terphenyl-d14 (Surr)	1000	1060	6.1	70 - 130
2-Fluorophenol (Surr)	1000	981	-1.9	70 - 130
2,4,6-Tribromophenol (Surr)	1000	1040	4.1	70 - 130



# CONTINUING CALIBRATION CHECK

**1311/8270D**

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Instrument ID: SV-GCMS10

Calibration: A9I2405

Lab File ID: J11261905.D

Calibration Date: 09/24/19 12:40

Sequence: 9K26022

Injection Date: 11/26/19

Lab Sample ID: 9K26022-CCV2

Injection Time: 10:16

COMPOUND	Curve Fit	Calculated Concentration (ng/mL) [L/Q Fits]			Response Factors [Ave RF]			Limit
		STD	CCV	% DIFF	ICAL	CCV	% Drift	
2,4-Dinitrotoluene	XXX	1000	1110	11.3				20
Hexachlorobenzene	Ave	1000	1020		0.2707358	0.2760474	2.0	20
Hexachlorobutadiene	Ave	1000	1080		0.1891523	0.2040592	7.9	20
Hexachloroethane	Ave	1000	1060		0.4806864	0.5087024	5.8	20
2-Methylphenol	Ave	1000	1020		1.03014	1.051367	2.1	20
3+4-Methylphenol(s)	Ave	1000	1040		1.277354	1.328959	4.0	20
Nitrobenzene	Ave	1000	925		1.221036	1.129324	-7.5	20
Pentachlorophenol (PCP)	XXX	1000	955	-4.5				20
Pyridine	Ave	1000	891		1.298764	1.157447	-10.9	20
2,4,5-Trichlorophenol	XXX	1000	1120	12.4				20
2,4,6-Trichlorophenol	XXX	1000	1140	14.2				20

\*\* Quadratic Curve fit may be weighted (1/a or 1/a<sup>2</sup>).

\* = Values outside of QC limits

# CONTINUING CALIBRATION CHECK

**1311/8270D**

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Instrument ID: SV-GCMS10

Calibration: A9I2405

Lab File ID: J11271905.D

Calibration Date: 09/24/19 12:40

Sequence: 9K27012

Injection Date: 11/27/19

Lab Sample ID: 9K27012-CCV2

Injection Time: 10:34

COMPOUND	Curve Fit	Calculated Concentration (ng/mL) [L/Q Fits]			Response Factors [Ave RF]			Limit
		STD	CCV	% DIFF	ICAL	CCV	% Drift	
2,4-Dinitrotoluene	XXX	1000	1120	11.6				20
Hexachlorobenzene	Ave	1000	1030		0.2707358	0.2776814	2.6	20
Hexachlorobutadiene	Ave	1000	1070		0.1891523	0.2026486	7.1	20
Hexachloroethane	Ave	1000	1100		0.4806864	0.5272671	9.7	20
2-Methylphenol	Ave	1000	1030		1.03014	1.056554	2.6	20
3+4-Methylphenol(s)	Ave	1000	1040		1.277354	1.330546	4.2	20
Nitrobenzene	Ave	1000	921		1.221036	1.125169	-7.9	20
Pentachlorophenol (PCP)	XXX	1000	961	-3.9				20
Pyridine	Ave	1000	885		1.298764	1.150013	-11.5	20
2,4,5-Trichlorophenol	XXX	1000	1140	13.6				20
2,4,6-Trichlorophenol	XXX	1000	1140	14.0				20

\*\* Quadratic Curve fit may be weighted (1/a or 1/a<sup>2</sup>).

\* = Values outside of QC limits

# SURROGATE STANDARD RECOVERY AND RT SUMMARY

1311/8270D

Laboratory: <u>Apex Laboratories</u>	SDG: <u>Gasco PreRD DG 2019</u>
Client: <u>Anchor QEA, LLC</u>	Project: <u>Gasco PreRD DG 2019 - 4c. Waste Characterization</u>
Sequence: <u>9I19035</u>	Instrument: <u>SV-GCMS10</u>
Matrix: <u>Soil</u>	Calibration: <u>A9I2405</u>

Surrogate Compound	Spike Level ng/mL	% Recovery	Recovery Limits	RT	Calibration Mean RT	RT Diff	RT Diff Limit	Q
<b>Initial Cal Check (9I19035-ICV1 )</b>			Lab File ID: J09191929.D		Analyzed: 09/20/19 07:50			
Nitrobenzene-d5 (Surr)	1000	107	70 - 130	7.113	7.1168	-0.0038	+/-1.0	
2-Fluorobiphenyl (Surr)	1000	106	70 - 130	8.927	8.927444	-0.0004	+/-1.0	
Phenol-d6 (Surr)	1000	102	70 - 130	6.209	6.2088	0.0002	+/-1.0	
p-Terphenyl-d14 (Surr)	1000	106	70 - 130	12.917	12.9267	-0.0097	+/-1.0	
2-Fluorophenol (Surr)	1000	98	70 - 130	5.316	5.3054	0.0106	+/-1.0	
2,4,6-Tribromophenol (Surr)	1000	104	70 - 130	10.419	10.42356	-0.0046	+/-1.0	

# SURROGATE STANDARD RECOVERY AND RT SUMMARY

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sequence: 9K26022

Instrument: SV-GCMS10

Matrix: Soil

Calibration: A9I2405

Surrogate Compound	Spike Level ng/mL	% Recovery	Recovery Limits	RT	Calibration Mean RT	RT Diff	RT Diff Limit	Q
<b>Calibration Check (9K26022-CCV2 )</b>			Lab File ID: J11261905.D		Analyzed: 11/26/19 10:16			
Nitrobenzene-d5 (Surr)	1000	95	80 - 120	6.926	7.1168	-0.1908	+/-1.0	
2-Fluorobiphenyl (Surr)	1000	103	80 - 120	8.739	8.927444	-0.1884	+/-1.0	
Phenol-d6 (Surr)	1000	96	80 - 120	6.033	6.2088	-0.1758	+/-1.0	
p-Terphenyl-d14 (Surr)	1000	109	80 - 120	12.665	12.9267	-0.2617	+/-1.0	
2-Fluorophenol (Surr)	1000	106	80 - 120	5.118	5.3054	-0.1874	+/-1.0	
2,4,6-Tribromophenol (Surr)	1000	97	80 - 120	10.226	10.42356	-0.1976	+/-1.0	
<b>Calibration Blank (9K26022-CCB1 )</b>			Lab File ID: J11261906.D		Analyzed: 11/26/19 10:52			
Nitrobenzene-d5 (Surr)			44 - 120	6.878	7.1168	-0.2388	+/-1.0	
2-Fluorobiphenyl (Surr)			44 - 120	0	8.927444	-8.9274	+/-1.0	
Phenol-d6 (Surr)			10 - 120	0	6.2088	-6.2088	+/-1.0	
p-Terphenyl-d14 (Surr)			50 - 133	12.671	12.9267	-0.2557	+/-1.0	
2-Fluorophenol (Surr)			19 - 120	0	5.3054	-5.3054	+/-1.0	
2,4,6-Tribromophenol (Surr)			43 - 140	0	10.42356	-10.4236	+/-1.0	
<b>Blank (9111242-BLK1 )</b>			Lab File ID: J11261919.D		Analyzed: 11/26/19 18:39			
Nitrobenzene-d5 (Surr)	0.0250	56	44 - 120	6.926	7.1168	-0.1908	+/-1.0	
2-Fluorobiphenyl (Surr)	0.0250	60	44 - 120	8.739	8.927444	-0.1884	+/-1.0	
Phenol-d6 (Surr)	0.0250	18	10 - 120	6.043	6.2088	-0.1658	+/-1.0	
p-Terphenyl-d14 (Surr)	0.0250	79	50 - 133	12.67	12.9267	-0.2567	+/-1.0	
2-Fluorophenol (Surr)	0.0250	34	19 - 120	5.134	5.3054	-0.1714	+/-1.0	
2,4,6-Tribromophenol (Surr)	0.0250	76	43 - 140	10.226	10.42356	-0.1976	+/-1.0	
<b>LCS (9111242-BS1 )</b>			Lab File ID: J11261920.D		Analyzed: 11/26/19 19:16			
Nitrobenzene-d5 (Surr)	0.0250	73	44 - 120	6.931	7.1168	-0.1858	+/-1.0	
2-Fluorobiphenyl (Surr)	0.0250	83	44 - 120	8.734	8.927444	-0.1934	+/-1.0	
Phenol-d6 (Surr)	0.0250	27	10 - 120	6.038	6.2088	-0.1708	+/-1.0	
p-Terphenyl-d14 (Surr)	0.0250	89	50 - 133	12.665	12.9267	-0.2617	+/-1.0	
2-Fluorophenol (Surr)	0.0250	44	19 - 120	5.134	5.3054	-0.1714	+/-1.0	
2,4,6-Tribromophenol (Surr)	0.0250	84	43 - 140	10.226	10.42356	-0.1976	+/-1.0	
<b>LCS Dup (9111242-BS1 )</b>			Lab File ID: J11261921.D		Analyzed: 11/26/19 19:52			
Nitrobenzene-d5 (Surr)	0.0250	70	44 - 120	6.926	7.1168	-0.1908	+/-1.0	
2-Fluorobiphenyl (Surr)	0.0250	81	44 - 120	8.734	8.927444	-0.1934	+/-1.0	
Phenol-d6 (Surr)	0.0250	24	10 - 120	6.038	6.2088	-0.1708	+/-1.0	
p-Terphenyl-d14 (Surr)	0.0250	91	50 - 133	12.665	12.9267	-0.2617	+/-1.0	
2-Fluorophenol (Surr)	0.0250	41	19 - 120	5.129	5.3054	-0.1764	+/-1.0	
2,4,6-Tribromophenol (Surr)	0.0250	83	43 - 140	10.226	10.42356	-0.1976	+/-1.0	

# SURROGATE STANDARD RECOVERY AND RT SUMMARY

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sequence: 9K27012

Instrument: SV-GCMS10

Matrix: Soil

Calibration: A9I2405

Surrogate Compound	Spike Level ng/mL	% Recovery	Recovery Limits	RT	Calibration Mean RT	RT Diff	RT Diff Limit	Q
<b>Calibration Check (9K27012-CCV2 )</b>			Lab File ID: J11271905.D		Analyzed: 11/27/19 10:34			
Nitrobenzene-d5 (Surr)	1000	93	80 - 120	6.926	7.1168	-0.1908	+/-1.0	
2-Fluorobiphenyl (Surr)	1000	103	80 - 120	8.734	8.927444	-0.1934	+/-1.0	
Phenol-d6 (Surr)	1000	95	80 - 120	6.038	6.2088	-0.1708	+/-1.0	
p-Terphenyl-d14 (Surr)	1000	107	80 - 120	12.665	12.9267	-0.2617	+/-1.0	
2-Fluorophenol (Surr)	1000	106	80 - 120	5.124	5.3054	-0.1814	+/-1.0	
2,4,6-Tribromophenol (Surr)	1000	100	80 - 120	10.226	10.42356	-0.1976	+/-1.0	
<b>Calibration Blank (9K27012-CCB1 )</b>			Lab File ID: J11271906.D		Analyzed: 11/27/19 11:10			
Nitrobenzene-d5 (Surr)			44 - 120	6.889	7.1168	-0.2278	+/-1.0	
2-Fluorobiphenyl (Surr)			44 - 120	0	8.927444	-8.9274	+/-1.0	
Phenol-d6 (Surr)			10 - 120	0	6.2088	-6.2088	+/-1.0	
p-Terphenyl-d14 (Surr)			50 - 133	0	12.9267	-12.9267	+/-1.0	
2-Fluorophenol (Surr)			19 - 120	0	5.3054	-5.3054	+/-1.0	
2,4,6-Tribromophenol (Surr)			43 - 140	0	10.42356	-10.4236	+/-1.0	
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01RE1 )</b>			Lab File ID: J11271913.D		Analyzed: 11/27/19 15:20			
Nitrobenzene-d5 (Surr)	0.0250	75	44 - 120	6.931	7.1168	-0.1858	+/-1.0	
2-Fluorobiphenyl (Surr)	0.0250	91	44 - 120	8.734	8.927444	-0.1934	+/-1.0	
Phenol-d6 (Surr)	0.0250	19	10 - 120	6.049	6.2088	-0.1598	+/-1.0	
p-Terphenyl-d14 (Surr)	0.0250	107	50 - 133	12.665	12.9267	-0.2617	+/-1.0	
2-Fluorophenol (Surr)	0.0250	40	19 - 120	5.118	5.3054	-0.1874	+/-1.0	
2,4,6-Tribromophenol (Surr)	0.0250	89	43 - 140	10.226	10.42356	-0.1976	+/-1.0	

**INTERNAL STANDARD AREA AND RT SUMMARY**  
**1311/8270D**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sequence: 9K27012

Instrument: SV-GCMS10

Matrix: Soil

Calibration: A9I2405

Internal Standard	Response	RT	Reference Response	Reference RT	Area %	Area % Limits	RT Diff	RT Diff Limit	Q
<b>Calibration Check (9K27012-CCV2 )</b>			Lab File ID: J11271905.D			Analyzed: 11/27/19 10:34			
1,4-Dichlorobenzene-d4 (ISTD)	368375	6.381	283511	6.568	130	50 - 200	-0.1870	+/-0.50	
Naphthalene-d8 (ISTD)	1412968	7.648	1143968	7.835	124	50 - 200	-0.1870	+/-0.50	
Acenaphthene-d10 (ISTD)	751566	9.424	583825	9.616	129	50 - 200	-0.1920	+/-0.50	
Phenanthrene-d10 (ISTD)	1376916	10.938	1065192	11.135	129	50 - 200	-0.1970	+/-0.50	
Chrysene-d12 (ISTD)	1352496	14.532	1048464	14.917	129	50 - 200	-0.3850	+/-0.50	
<b>Calibration Blank (9K27012-CCB1 )</b>			Lab File ID: J11271906.D			Analyzed: 11/27/19 11:10			
1,4-Dichlorobenzene-d4 (ISTD)	443001	6.386	368375	6.381	120	50 - 200	0.0050	+/-0.50	
Naphthalene-d8 (ISTD)	1732924	7.648	1412968	7.648	123	50 - 200	0.0000	+/-0.50	
Acenaphthene-d10 (ISTD)	917836	9.424	751566	9.424	122	50 - 200	0.0000	+/-0.50	
Phenanthrene-d10 (ISTD)	1633582	10.938	1376916	10.938	119	50 - 200	0.0000	+/-0.50	
Chrysene-d12 (ISTD)	1702493	14.532	1352496	14.532	126	50 - 200	0.0000	+/-0.50	
<b>PDI-142RAB-C-00-30.4-191112 (A9K0412-01RE1 )</b>			Lab File ID: J11271913.D			Analyzed: 11/27/19 15:20			
1,4-Dichlorobenzene-d4 (ISTD)	387154	6.381	368375	6.381	105	50 - 200	0.0000	+/-0.50	
Naphthalene-d8 (ISTD)	1427888	7.648	1412968	7.648	101	50 - 200	0.0000	+/-0.50	
Acenaphthene-d10 (ISTD)	747611	9.424	751566	9.424	99	50 - 200	0.0000	+/-0.50	
Phenanthrene-d10 (ISTD)	1321721	10.932	1376916	10.938	96	50 - 200	-0.0060	+/-0.50	
Chrysene-d12 (ISTD)	1317590	14.526	1352496	14.532	97	50 - 200	-0.0060	+/-0.50	

# HOLDING TIME SUMMARY

1311/8270D

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sample Name	Date Collected	Date Received	Date Prepared	Days to Prep	Max Days to Prep	Date Analyzed	Days to Analysis	Max Days to Analysis	Q
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/26/19 14:05	13.93	7.00	11/27/19 15:20	1.05	40.00	*

# Apex Laboratories

SDG: Gasco PreRD\_DG 2019

CLASS: METALS

METHOD: 1311/6020A



**ANALYSES DATA PACKAGE COVER PAGE**

**1311/6020A**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

---

**Client Sample Id:**

PDI-142RAB-C-00-30.4-191112

**Lab Sample Id:**

A9K0412-01

**Matrix**

SO

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hardcopy data package and in computer-readable data submitted on diskette has been authorized by the Laboratory Manager or the Manager's designee, as verified by the following signatures.

Signature: \_\_\_\_\_



Name: \_\_\_\_\_

David G. Jack

Forms Created: \_\_\_\_\_

12/18/2019 12:23PM

Title: \_\_\_\_\_

Technical Manager

# METHOD DETECTION AND REPORTING LIMITS

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Charac

Batch Matrix: Soil

Analyte	MDL	MRL	Units
Arsenic	0.0500	0.100	mg/L
Barium	2.50	5.00	mg/L
Cadmium	0.0500	0.100	mg/L
Chromium	0.0500	0.100	mg/L
Lead	0.0250	0.0500	mg/L
Mercury	0.00350	0.00700	mg/L
Selenium	0.0500	0.100	mg/L
Silver	0.0500	0.100	mg/L

Note: MDLs are listed only if the corresponding analyte was evaluated to the MDL in this report .

# INORGANIC ANALYSIS DATA SHEET

1311/6020A

PDI-142RAB-C-00-30.4-191112

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste

Matrix: SO

Laboratory ID: A9K0412-01

Characterization  
File ID: 9K26027-036

Sampled: 11/12/19 15:40

Prepared: 11/26/19 09:55

Analyzed: 11/26/19 14:05

Solids: N/A

Preparation: EPA 1311/3015

Initial/Final: 10 mL / 50 mL

Batch: 9111213

Sequence: 9K26027

Instrument: ICPMS5

CAS NO.	Analyte	Concentration (mg/L)	Dilution Factor	Q	Method
7440-38-2	Arsenic	0.0500	10	U	1311/6020A
7440-39-3	Barium	2.50	10	U	1311/6020A
7440-43-9	Cadmium	0.0500	10	U	1311/6020A
7440-47-3	Chromium	0.0500	10	U	1311/6020A
7439-92-1	Lead	0.0250	10	U	1311/6020A
7439-97-6	Mercury	0.00350	10	U	1311/6020A
7782-49-2	Selenium	0.0500	10	U	1311/6020A
7440-22-4	Silver	0.0500	10	U	1311/6020A

# PREPARATION BATCH SUMMARY

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Batch: 9111213 Batch Matrix: Soil

Preparation: EPA 1311/3015

SAMPLE NAME	LAB SAMPLE ID	LAB FILE ID	DATE PREPARED	OBSERVATIONS
Blank	9111213-BLK1	9K26027-034	11/26/19 09:55	
LCS	9111213-BS1	9K26027-035	11/26/19 09:55	
PDI-142RAB-C-00-30.4-191112 (M	9111213-MS1	9K26027-037	11/26/19 09:55	
PDI-142RAB-C-00-30.4-191112	A9K0412-01	9K26027-036	11/26/19 09:55	

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# METHOD BLANK DATA SHEET

1311/6020A

Laboratory: Apex Laboratories SDG: Gasco PreRD\_DG 2019  
Client: Anchor QEA, LLC Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization  
Matrix: Soil Laboratory ID: 9111213-BLK1 File ID: 9K26027-034  
Prepared: 11/26/19 09:55 Preparation: EPA 1311/3015 Initial/Final: 10 mL / 50 mL  
Analyzed: 11/26/19 13:56 Instrument: ICPMS5  
Batch: 9111213 Sequence: 9K26027 Calibration: UNASSIGNED

CAS NO.	COMPOUND	CONC. (mg/L)	Q
7440-38-2	Arsenic	0.0500	U
7440-39-3	Barium	2.50	U
7440-43-9	Cadmium	0.0500	U
7440-47-3	Chromium	0.0500	U
7439-92-1	Lead	0.0250	U
7439-97-6	Mercury	0.00350	U
7782-49-2	Selenium	0.0500	U
7440-22-4	Silver	0.0500	U

# LCS / LCS DUPLICATE RECOVERY

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Matrix: Soil

Batch: 9111213

Laboratory ID: 9111213-BS1

Preparation: EPA 1311/3015

Initial/Final: 10 mL / 50 mL

COMPOUND	SPIKE ADDED (mg/L)	LCS CONCENTRATION (mg/L)	LCS % REC. (*=Out)	QC LIMITS REC.
Arsenic	5.00	5.09	102	80 - 120
Barium	10.0	10.6	106	80 - 120
Cadmium	1.00	1.04	104	80 - 120
Chromium	5.00	4.92	98	80 - 120
Lead	5.00	5.13	103	80 - 120
Mercury	0.100	0.107	107	80 - 120
Selenium	1.00	1.00	100	80 - 120
Silver	1.00	1.06	106	80 - 120

\* = Values outside of QC limits

**MATRIX SPIKE / MATRIX SPIKE DUPLICATE RECOVERY****1311/6020A****PDI-142RAB-C-00-30.4-191112**Laboratory: Apex LaboratoriesSDG: Gasco PreRD\_DG 2019Client: Anchor QEA, LLCProject: Gasco PreRD\_DG 2019 - 4c. Waste CharacterizationMatrix: SoilBatch: 9111213Laboratory ID: 9111213-MS1Preparation: EPA 1311/3015Initial/Final: 10 mL / 50 mLSource Sample Name: PDI-142RAB-C-00-30.4-191112

COMPOUND	SPIKE ADDED (mg/L)	SAMPLE CONCENTRATION (mg/L)	MS CONCENTRATION (mg/L)	MS % REC. (*=Out)	QC LIMITS REC.
Arsenic	5.00	ND	4.95	99	50 - 150
Barium	10.0	ND	10.5	105	50 - 150
Cadmium	1.00	ND	1.01	101	50 - 150
Chromium	5.00	ND	4.77	95	50 - 150
Lead	5.00	ND	4.96	99	50 - 150
Mercury	0.100	ND	0.102	102	50 - 150
Selenium	1.00	ND	0.978	98	50 - 150
Silver	1.00	ND	1.03	103	50 - 150

# ANALYSIS BATCH (SEQUENCE) SUMMARY

**1311/6020A**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9K26027

Instrument: ICPMS5

Matrix: Soil

Calibration: UNASSIGNED

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
Initial Cal Check	9K26027-ICV1	9K26027-013	11/26/19 12:03
Initial Cal Blank	9K26027-ICB1	9K26027-014	11/26/19 12:08
Instrument RL Check	9K26027-CRL1	9K26027-015	11/26/19 12:12
Instrument RL Check	9K26027-CRL2	9K26027-016	11/26/19 12:17
Instrument RL Check	9K26027-CRL3	9K26027-017	11/26/19 12:22
Calibration Check	9K26027-CCV1	9K26027-031	11/26/19 13:42
Calibration Blank	9K26027-CCB1	9K26027-032	11/26/19 13:46
Blank	9111213-BLK1	9K26027-034	11/26/19 13:56
LCS	9111213-BS1	9K26027-035	11/26/19 14:01
PDI-142RAB-C-00-30.4-191112	A9K0412-01	9K26027-036	11/26/19 14:05
PDI-142RAB-C-00-30.4-191112 (MS	9111213-MS1	9K26027-037	11/26/19 14:10
Calibration Check	9K26027-CCV2	9K26027-043	11/26/19 14:40
Calibration Blank	9K26027-CCB2	9K26027-044	11/26/19 14:44
Instrument RL Check	9K26027-CRL4	9K26027-045	11/26/19 14:49
Instrument RL Check	9K26027-CRL5	9K26027-046	11/26/19 14:54
Instrument RL Check	9K26027-CRL6	9K26027-047	11/26/19 14:58
Calibration Check	9K26027-CCV3	9K26027-058	11/26/19 15:50
Calibration Blank	9K26027-CCB3	9K26027-059	11/26/19 15:54
Calibration Check	9K26027-CCV4	9K26027-070	11/26/19 16:46
Calibration Blank	9K26027-CCB4	9K26027-071	11/26/19 16:50
Calibration Check	9K26027-CCV5	9K26027-082	11/26/19 17:44
Calibration Blank	9K26027-CCB5	9K26027-083	11/26/19 17:49
Instrument RL Check	9K26027-CRL7	9K26027-084	11/26/19 17:54
Instrument RL Check	9K26027-CRL8	9K26027-085	11/26/19 17:58
Instrument RL Check	9K26027-CRL9	9K26027-086	11/26/19 18:03
Instrument RL Check	9K26027-CRLA	9K26027-087	11/26/19 18:08
Calibration Check	9K26027-CCV6	9K26027-098	11/26/19 18:59
Calibration Blank	9K26027-CCB6	9K26027-099	11/26/19 19:04
Calibration Check	9K26027-CCV7	9K26027-110	11/26/19 19:55
Calibration Blank	9K26027-CCB7	9K26027-111	11/26/19 20:00
Calibration Check	9K26027-CCV8	9K26027-120	11/26/19 20:42
Calibration Blank	9K26027-CCB8	9K26027-121	11/26/19 20:47
Instrument RL Check	9K26027-CRLB	9K26027-122	11/26/19 20:51



# ANALYSIS BATCH (SEQUENCE) SUMMARY

**1311/6020A**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9K26027

Instrument: ICPMS5

Matrix: Soil

Calibration: UNASSIGNED

Sample Name	Lab Sample ID	Lab File ID	Analysis Date/Time
Instrument RL Check	9K26027-CRLC	9K26027-123	11/26/19 20:56
Instrument RL Check	9K26027-CRLD	9K26027-124	11/26/19 21:01
Instrument RL Check	9K26027-CRLE	9K26027-125	11/26/19 21:05

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# INITIAL AND CONTINUING CALIBRATION CHECK

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Instrument ID: ICPMS5

Calibration: UNASSIGNED

Control Limit: +/- 10.00%

Sequence: 9K26027

Lab Sample ID	Analyte	True	Found	%R	Units	Method
9K26027-ICV1	Arsenic	100	96.8	97	ug/L	1311/6020A
	Barium	100	102	102	ug/L	1311/6020A
	Cadmium	100	98.1	98	ug/L	1311/6020A
	Chromium	100	96.1	96	ug/L	1311/6020A
	Lead	100	97.5	97	ug/L	1311/6020A
	Mercury	800	816	102	ng/L	1311/6020A
	Selenium	40.0	40.3	101	ug/L	1311/6020A
	Silver	40.0	40.2	101	ug/L	1311/6020A
	9K26027-CCV1	Arsenic	100	96.6	97	ug/L
Barium		100	102	102	ug/L	1311/6020A
Cadmium		100	98.6	99	ug/L	1311/6020A
Chromium		100	94.3	94	ug/L	1311/6020A
Lead		100	97.4	97	ug/L	1311/6020A
Mercury		800	821	103	ng/L	1311/6020A
Selenium		40.0	41.3	103	ug/L	1311/6020A
Silver		40.0	40.7	102	ug/L	1311/6020A
9K26027-CCV2		Arsenic	100	96.6	97	ug/L
	Barium	100	103	103	ug/L	1311/6020A
	Cadmium	100	98.0	98	ug/L	1311/6020A
	Chromium	100	94.7	95	ug/L	1311/6020A
	Lead	100	97.5	98	ug/L	1311/6020A
	Mercury	800	796	99	ng/L	1311/6020A
	Selenium	40.0	40.7	102	ug/L	1311/6020A
	Silver	40.0	40.3	101	ug/L	1311/6020A
	9K26027-CCV3	Arsenic	100	97.0	97	ug/L
Barium		100	103	103	ug/L	1311/6020A
Cadmium		100	97.4	97	ug/L	1311/6020A
Chromium		100	95.5	96	ug/L	1311/6020A
Lead		100	97.8	98	ug/L	1311/6020A
Mercury		800	824	103	ng/L	1311/6020A
Selenium		40.0	40.8	102	ug/L	1311/6020A
Silver		40.0	40.3	101	ug/L	1311/6020A
9K26027-CCV4		Arsenic	100	96.6	97	ug/L
	Barium	100	101	101	ug/L	1311/6020A
	Cadmium	100	99.6	100	ug/L	1311/6020A
	Chromium	100	95.9	96	ug/L	1311/6020A
	Lead	100	99.0	99	ug/L	1311/6020A
	Mercury	800	830	104	ng/L	1311/6020A
	Selenium	40.0	41.0	102	ug/L	1311/6020A
	Silver	40.0	40.8	102	ug/L	1311/6020A
	9K26027-CCV5	Arsenic	100	96.8	97	ug/L
Barium		100	102	102	ug/L	1311/6020A
Cadmium		100	99.6	100	ug/L	1311/6020A
Chromium		100	94.3	94	ug/L	1311/6020A
Lead		100	99.3	99	ug/L	1311/6020A
Mercury		800	849	106	ng/L	1311/6020A

# INITIAL AND CONTINUING CALIBRATION CHECK

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Instrument ID: ICPMS5

Calibration: UNASSIGNED

Control Limit: +/- 10.00%

Sequence: 9K26027

Lab Sample ID	Analyte	True	Found	%R	Units	Method
9K26027-CCV5	Selenium	40.0	40.6	101	ug/L	1311/6020A
	Silver	40.0	40.9	102	ug/L	1311/6020A
9K26027-CCV6	Arsenic	100	97.1	97	ug/L	1311/6020A
	Barium	100	102	102	ug/L	1311/6020A
	Cadmium	100	99.3	99	ug/L	1311/6020A
	Chromium	100	94.8	95	ug/L	1311/6020A
	Lead	100	98.0	98	ug/L	1311/6020A
	Mercury	800	822	103	ng/L	1311/6020A
	Selenium	40.0	41.2	103	ug/L	1311/6020A
	Silver	40.0	40.7	102	ug/L	1311/6020A
9K26027-CCV7	Arsenic	100	96.9	97	ug/L	1311/6020A
	Barium	100	101	101	ug/L	1311/6020A
	Cadmium	100	99.3	99	ug/L	1311/6020A
	Chromium	100	95.6	96	ug/L	1311/6020A
	Lead	100	99.3	99	ug/L	1311/6020A
	Mercury	800	829	104	ng/L	1311/6020A
	Selenium	40.0	41.1	103	ug/L	1311/6020A
	Silver	40.0	40.8	102	ug/L	1311/6020A
9K26027-CCV8	Arsenic	100	96.6	97	ug/L	1311/6020A
	Barium	100	101	101	ug/L	1311/6020A
	Cadmium	100	99.5	100	ug/L	1311/6020A
	Chromium	100	95.2	95	ug/L	1311/6020A
	Lead	100	99.6	100	ug/L	1311/6020A
	Mercury	800	813	102	ng/L	1311/6020A
	Selenium	40.0	41.0	102	ug/L	1311/6020A
	Silver	40.0	41.1	103	ug/L	1311/6020A

\* Values outside of QC limits

# INSTRUMENT BLANKS

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Instrument ID: ICPMS5

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sequence: 9K26027

Calibration: UNASSIGNED

Lab Sample ID	Analyte	Found	RL	Units	C	Method
9K26027-ICB1	Mercury	ND	70.0 (Inst)	ng/L		1311/6020A
	Lead	ND	0.500 (Inst)	ug/L		1311/6020A
	Silver	ND	1.00 (Inst)	ug/L		1311/6020A
	Arsenic	ND	1.00 (Inst)	ug/L		1311/6020A
	Barium	ND	50.0 (Inst)	ug/L		1311/6020A
	Cadmium	ND	1.00 (Inst)	ug/L		1311/6020A
	Chromium	ND	1.00 (Inst)	ug/L		1311/6020A
	Selenium	ND	1.00 (Inst)	ug/L		1311/6020A
	9K26027-CCB1	Mercury	ND	70.0 (Inst)	ng/L	
Lead		ND	0.500 (Inst)	ug/L		1311/6020A
Silver		ND	1.00 (Inst)	ug/L		1311/6020A
Arsenic		ND	1.00 (Inst)	ug/L		1311/6020A
Barium		ND	50.0 (Inst)	ug/L		1311/6020A
Cadmium		ND	1.00 (Inst)	ug/L		1311/6020A
Chromium		ND	1.00 (Inst)	ug/L		1311/6020A
Selenium		ND	1.00 (Inst)	ug/L		1311/6020A
9K26027-CCB2		Cadmium	ND	1.00 (Inst)	ug/L	
	Chromium	ND	1.00 (Inst)	ug/L		1311/6020A
	Selenium	ND	1.00 (Inst)	ug/L		1311/6020A
	Arsenic	ND	1.00 (Inst)	ug/L		1311/6020A
	Silver	ND	1.00 (Inst)	ug/L		1311/6020A
	Mercury	ND	70.0 (Inst)	ng/L		1311/6020A
	Barium	ND	50.0 (Inst)	ug/L		1311/6020A
	Lead	ND	0.500 (Inst)	ug/L		1311/6020A
	9K26027-CCB3	Cadmium	ND	1.00 (Inst)	ug/L	
Lead		ND	0.500 (Inst)	ug/L		1311/6020A
Silver		ND	1.00 (Inst)	ug/L		1311/6020A
Barium		ND	50.0 (Inst)	ug/L		1311/6020A
Chromium		ND	1.00 (Inst)	ug/L		1311/6020A
Selenium		ND	1.00 (Inst)	ug/L		1311/6020A
Arsenic		ND	1.00 (Inst)	ug/L		1311/6020A
Mercury		ND	70.0 (Inst)	ng/L		1311/6020A
9K26027-CCB4		Chromium	ND	1.00 (Inst)	ug/L	

# INSTRUMENT BLANKS

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Instrument ID: ICPMS5

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9K26027

Calibration: UNASSIGNED

Lab Sample ID	Analyte	Found	RL	Units	C	Method
9K26027-CCB4	Lead	ND	0.500 (Inst)	ug/L		1311/6020A
	Silver	ND	1.00 (Inst)	ug/L		1311/6020A
	Arsenic	ND	1.00 (Inst)	ug/L		1311/6020A
	Barium	ND	50.0 (Inst)	ug/L		1311/6020A
	Mercury	ND	70.0 (Inst)	ng/L		1311/6020A
	Selenium	ND	1.00 (Inst)	ug/L		1311/6020A
	Cadmium	ND	1.00 (Inst)	ug/L		1311/6020A
9K26027-CCB5	Mercury	ND	70.0 (Inst)	ng/L		1311/6020A
	Lead	ND	0.500 (Inst)	ug/L		1311/6020A
	Silver	ND	1.00 (Inst)	ug/L		1311/6020A
	Arsenic	ND	1.00 (Inst)	ug/L		1311/6020A
	Barium	ND	50.0 (Inst)	ug/L		1311/6020A
	Cadmium	ND	1.00 (Inst)	ug/L		1311/6020A
	Chromium	ND	1.00 (Inst)	ug/L		1311/6020A
	Selenium	ND	1.00 (Inst)	ug/L		1311/6020A
9K26027-CCB6	Mercury	ND	70.0 (Inst)	ng/L		1311/6020A
	Silver	ND	1.00 (Inst)	ug/L		1311/6020A
	Lead	ND	0.500 (Inst)	ug/L		1311/6020A
	Arsenic	ND	1.00 (Inst)	ug/L		1311/6020A
	Barium	ND	50.0 (Inst)	ug/L		1311/6020A
	Cadmium	ND	1.00 (Inst)	ug/L		1311/6020A
	Chromium	ND	1.00 (Inst)	ug/L		1311/6020A
	Selenium	ND	1.00 (Inst)	ug/L		1311/6020A
9K26027-CCB7	Mercury	ND	70.0 (Inst)	ng/L		1311/6020A
	Chromium	ND	1.00 (Inst)	ug/L		1311/6020A
	Selenium	ND	1.00 (Inst)	ug/L		1311/6020A
	Barium	ND	50.0 (Inst)	ug/L		1311/6020A
	Arsenic	ND	1.00 (Inst)	ug/L		1311/6020A
	Cadmium	ND	1.00 (Inst)	ug/L		1311/6020A
	Lead	ND	0.500 (Inst)	ug/L		1311/6020A
	Silver	ND	1.00 (Inst)	ug/L		1311/6020A
9K26027-CCB8	Mercury	ND	70.0 (Inst)	ng/L		1311/6020A
	Chromium	ND	1.00 (Inst)	ug/L		1311/6020A

# INSTRUMENT BLANKS

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Instrument ID: ICPMS5

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Sequence: 9K26027

Calibration: UNASSIGNED

Lab Sample ID	Analyte	Found	RL	Units	C	Method
9K26027-CCB8	Lead	ND	0.500 (Inst)	ug/L		1311/6020A
	Silver	ND	1.00 (Inst)	ug/L		1311/6020A
	Arsenic	ND	1.00 (Inst)	ug/L		1311/6020A
	Cadmium	ND	1.00 (Inst)	ug/L		1311/6020A
	Selenium	ND	1.00 (Inst)	ug/L		1311/6020A
	Barium	ND	50.0 (Inst)	ug/L		1311/6020A

(Inst) indicates on-Instrument Result and Reporting Level. Used for non-digested Instrument Blanks.

# CRDL STANDARD

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Instrument ID: ICPMS5

Calibration: UNASSIGNED

Sequence: 9K26027

Lab Sample ID	Analyte	True	Found	%R	Units	QC Limits
9K26027-CRL1	Arsenic	0.180	0.189	105	ug/L	70 - 130
	Barium	0.180	0.193	107	ug/L	70 - 130
	Cadmium	0.180	0.200	111	ug/L	70 - 130
	Chromium	0.180	0.185	103	ug/L	70 - 130
	Lead	0.180	0.215	120	ug/L	70 - 130
	Selenium	0.180	0.185	103	ug/L	70 - 130
	Silver	0.180	0.188	104	ug/L	70 - 130
9K26027-CRL2	Arsenic	0.900	0.909	101	ug/L	70 - 130
	Barium	0.900	0.925	103	ug/L	70 - 130
	Cadmium	0.900	0.911	101	ug/L	70 - 130
	Chromium	0.900	0.953	106	ug/L	70 - 130
	Lead	0.900	0.932	104	ug/L	70 - 130
	Mercury	36.0	40.1	111	ng/L	70 - 130
	Selenium	0.900	0.876	97	ug/L	70 - 130
	Silver	0.900	0.923	103	ug/L	70 - 130
9K26027-CRL3	Arsenic	1.80	1.89	105	ug/L	70 - 130
	Barium	1.80	1.89	105	ug/L	70 - 130
	Cadmium	1.80	1.89	105	ug/L	70 - 130
	Chromium	1.80	1.79	100	ug/L	70 - 130
	Lead	1.80	1.80	100	ug/L	70 - 130
	Mercury	72.0	75.7	105	ng/L	70 - 130
	Selenium	1.80	1.76	98	ug/L	70 - 130
	Silver	1.80	1.82	101	ug/L	70 - 130
9K26027-CRL4	Arsenic	0.180	0.161	90	ug/L	70 - 130
	Barium	0.180	0.173	96	ug/L	70 - 130
	Cadmium	0.180	0.213	119	ug/L	70 - 130
	Chromium	0.180	0.164	91	ug/L	70 - 130
	Lead	0.180	0.193	107	ug/L	70 - 130

# CRDL STANDARD

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Instrument ID: ICPMS5

Calibration: UNASSIGNED

Sequence: 9K26027

Lab Sample ID	Analyte	True	Found	%R	Units	QC Limits
9K26027-CRL4	Selenium	0.180	0.162	90	ug/L	70 - 130
	Silver	0.180	0.160	89	ug/L	70 - 130
9K26027-CRL5	Arsenic	0.900	0.836	93	ug/L	70 - 130
	Barium	0.900	0.960	107	ug/L	70 - 130
	Cadmium	0.900	0.927	103	ug/L	70 - 130
	Chromium	0.900	0.842	94	ug/L	70 - 130
	Lead	0.900	0.909	101	ug/L	70 - 130
	Mercury	36.0	34.6	96	ng/L	70 - 130
	Selenium	0.900	0.893	99	ug/L	70 - 130
	Silver	0.900	0.899	100	ug/L	70 - 130
9K26027-CRL6	Arsenic	1.80	1.82	101	ug/L	70 - 130
	Barium	1.80	1.86	103	ug/L	70 - 130
	Cadmium	1.80	1.82	101	ug/L	70 - 130
	Chromium	1.80	1.74	97	ug/L	70 - 130
	Lead	1.80	1.84	102	ug/L	70 - 130
	Mercury	72.0	85.1	118	ng/L	70 - 130
	Selenium	1.80	1.85	103	ug/L	70 - 130
	Silver	1.80	1.84	102	ug/L	70 - 130
9K26027-CRL7	Arsenic	0.180	0.164	91	ug/L	70 - 130
	Barium	0.180	0.180	100	ug/L	70 - 130
	Cadmium	0.180	0.194	108	ug/L	70 - 130
	Chromium	0.180	0.142	79	ug/L	70 - 130
	Lead	0.180	0.228	127	ug/L	70 - 130
	Mercury	7.20	8.74	121	ng/L	70 - 130
	Selenium	0.180	0.192	106	ug/L	70 - 130
	Silver	0.180	0.182	101	ug/L	70 - 130
9K26027-CRL8	Arsenic	0.900	0.877	97	ug/L	70 - 130
	Barium	0.900	0.901	100	ug/L	70 - 130



# CRDL STANDARD

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Instrument ID: ICPMS5

Calibration: UNASSIGNED

Sequence: 9K26027

Lab Sample ID	Analyte	True	Found	%R	Units	QC Limits
9K26027-CRL8	Cadmium	0.900	0.908	101	ug/L	70 - 130
	Chromium	0.900	0.846	94	ug/L	70 - 130
	Lead	0.900	0.962	107	ug/L	70 - 130
	Mercury	36.0	39.7	110	ng/L	70 - 130
	Selenium	0.900	0.965	107	ug/L	70 - 130
	Silver	0.900	0.895	99	ug/L	70 - 130
9K26027-CRL9	Arsenic	1.80	1.81	100	ug/L	70 - 130
	Barium	1.80	1.85	103	ug/L	70 - 130
	Cadmium	1.80	1.78	99	ug/L	70 - 130
	Chromium	1.80	1.73	96	ug/L	70 - 130
	Lead	1.80	1.87	104	ug/L	70 - 130
	Mercury	72.0	77.0	107	ng/L	70 - 130
	Selenium	1.80	1.81	101	ug/L	70 - 130
	Silver	1.80	1.80	100	ug/L	70 - 130
9K26027-CRLA	Arsenic	3.60	3.62	100	ug/L	70 - 130
	Barium	3.60	3.74	104	ug/L	70 - 130
	Cadmium	3.60	3.76	104	ug/L	70 - 130
	Chromium	3.60	3.45	96	ug/L	70 - 130
	Lead	3.60	3.70	103	ug/L	70 - 130
	Mercury	144	149	104	ng/L	70 - 130
	Selenium	3.60	3.57	99	ug/L	70 - 130
	Silver	3.60	3.61	100	ug/L	70 - 130
9K26027-CRLB	Arsenic	0.180	0.200	111	ug/L	70 - 130
	Barium	0.180	0.188	105	ug/L	70 - 130
	Cadmium	0.180	0.209	116	ug/L	70 - 130
	Chromium	0.180	0.152	85	ug/L	70 - 130
	Lead	0.180	0.199	110	ug/L	70 - 130
	Mercury	7.20	8.78	122	ng/L	70 - 130

# CRDL STANDARD

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Instrument ID: ICPMS5

Calibration: UNASSIGNED

Sequence: 9K26027

Lab Sample ID	Analyte	True	Found	%R	Units	QC Limits
9K26027-CRLB	Selenium	0.180	0.140	78	ug/L	70 - 130
	Silver	0.180	0.172	95	ug/L	70 - 130
9K26027-CRLC	Arsenic	0.900	0.948	105	ug/L	70 - 130
	Barium	0.900	0.949	105	ug/L	70 - 130
	Cadmium	0.900	0.946	105	ug/L	70 - 130
	Chromium	0.900	0.881	98	ug/L	70 - 130
	Lead	0.900	0.933	104	ug/L	70 - 130
	Mercury	36.0	40.0	111	ng/L	70 - 130
	Selenium	0.900	0.903	100	ug/L	70 - 130
	Silver	0.900	0.897	100	ug/L	70 - 130
9K26027-CRLD	Arsenic	1.80	1.83	101	ug/L	70 - 130
	Barium	1.80	1.87	104	ug/L	70 - 130
	Cadmium	1.80	1.92	106	ug/L	70 - 130
	Chromium	1.80	1.77	98	ug/L	70 - 130
	Lead	1.80	1.88	104	ug/L	70 - 130
	Mercury	72.0	76.5	106	ng/L	70 - 130
	Selenium	1.80	1.76	98	ug/L	70 - 130
	Silver	1.80	1.81	101	ug/L	70 - 130
9K26027-CRLE	Arsenic	3.60	3.68	102	ug/L	70 - 130
	Barium	3.60	3.72	103	ug/L	70 - 130
	Cadmium	3.60	3.74	104	ug/L	70 - 130
	Chromium	3.60	3.47	97	ug/L	70 - 130
	Lead	3.60	3.69	102	ug/L	70 - 130
	Mercury	144	147	102	ng/L	70 - 130
	Selenium	3.60	3.81	106	ug/L	70 - 130
	Silver	3.60	3.59	100	ug/L	70 - 130

\* Values outside of QC limits

# HOLDING TIME SUMMARY

1311/6020A

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sample Name	Date Collected	Date Received	Date Prepared	Days to Prep	Max Days to Prep	Date Analyzed	Days to Analysis	Max Days to Analysis	Q
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/26/19 09:55	13.76	28.00	11/26/19 14:05	13.93	28.00	
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/26/19 09:55	13.76	180.00	11/26/19 14:05	13.93	180.00	

# Apex Laboratories

SDG: Gasco PreRD\_DG 2019

CLASS: WET

METHOD: SM 2540 G

**ANALYSES DATA PACKAGE COVER PAGE**

**SM 2540 G**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

---

**Client Sample Id:**

PDI-142RAB-C-00-30.4-191112

**Lab Sample Id:**

A9K0412-01

**Matrix**

SO

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hardcopy data package and in computer-readable data submitted on diskette has been authorized by the Laboratory Manager or the Manager's designee, as verified by the following signatures.

Signature: \_\_\_\_\_



Name: \_\_\_\_\_

David G. Jack

Forms Created: \_\_\_\_\_

12/18/2019 12:23PM

Title: \_\_\_\_\_

Technical Manager

# METHOD DETECTION AND REPORTING LIMITS

## SM 2540 G

**Laboratory:** Apex Laboratories

**SDG:** Gasco PreRD\_DG 2019

**Client:** Anchor QEA, LLC

**Project:** Gasco PreRD\_DG 2019 - 4c. Waste Charac

**Batch Matrix:** Sediment

Analyte	MDL	MRL	Units
Total Solids	1.00	1.00	% by Weight

Note: MDLs are listed only if the corresponding analyte was evaluated to the MDL in this report .

# INORGANIC ANALYSIS DATA SHEET

SM 2540 G

PDI-142RAB-C-00-30.4-191112

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste  
Characterization

Matrix: SO

Laboratory ID: A9K0412-01

Sampled: 11/12/19 15:40

Prepared: 11/15/19 11:24

Analyzed: 11/16/19 11:44

Solids: N/A

Preparation: Total Solids (SM2540G/PSEP)

Initial/Final: 1 N/A / 1 N/A

Batch: 9110857

Calibration:

Instrument: Inst

CAS NO.	Analyte	Concentration (% by Weight)	Dilution Factor	Q	Method
TS	Total Solids	92.5	1		SM 2540 G

# PREPARATION BATCH SUMMARY

## SM 2540 G

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Batch: 9110857

Batch Matrix: Sediment

Preparation: Total Solids (SM2540G/PSEP)

SAMPLE NAME	LAB SAMPLE ID	LAB FILE ID	DATE PREPARED	OBSERVATIONS
PDI-142RAB-C-00-30.4-191112 (D)	9110857-DUP1		11/15/19 11:24	
PDI-142RAB-C-00-30.4-191112	A9K0412-01		11/15/19 11:24	

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.



# DUPLICATES

PDI-142RAB-C-00-30.4-191112

## SM 2540 G

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Charact

Matrix: Sediment

Laboratory ID: 9110857-DUP1

Batch: 9110857

Lab Source ID: A9K0412-01

Preparation: Total Solids (SM2540G/PSEP)

Initial/Final: 1 N/A / 1 N/A

Source Sample Name: PDI-142RAB-C-00-30.4-191112

% Solids:

ANALYTE	CONTROL LIMIT	SAMPLE CONCENTRATION (% by Weight)	C	DUPLICATE CONCENTRATION (% by Weight)	C	RPD %	Q	METHOD
Total Solids	10	92.5		92.3		0.2		SM 2540 G

\* Values outside of QC limits

# HOLDING TIME SUMMARY

## SM 2540 G

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sample Name	Date Collected	Date Received	Date Prepared	Days to Prep	Max Days to Prep	Date Analyzed	Days to Analysis	Max Days to Analysis	Q
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/15/19 11:24	2.82	180.00	11/16/19 11:44	1.01		

# Apex Laboratories

SDG: Gasco PreRD\_DG 2019

CLASS: GCMS

METHOD: EPA 1311 ZHE

**ANALYSES DATA PACKAGE COVER PAGE**

**EPA 1311 ZHE**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

---

**Client Sample Id:**

PDI-142RAB-C-00-30.4-191112

**Lab Sample Id:**

A9K0412-01

**Matrix**

SO

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hardcopy data package and in computer-readable data submitted on diskette has been authorized by the Laboratory Manager or the Manager's designee, as verified by the following signatures.

Signature: \_\_\_\_\_



Name: \_\_\_\_\_

David G. Jack

Forms Created: \_\_\_\_\_

12/18/2019 12:23PM

Title: \_\_\_\_\_

Technical Manager

# METHOD DETECTION AND REPORTING LIMITS

## EPA 1311 ZHE

**Laboratory:** Apex Laboratories

**SDG:** Gasco PreRD\_DG 2019

**Client:** Anchor QEA, LLC

**Project:** Gasco PreRD\_DG 2019 - 4c. Waste Charac

**Batch Matrix:** Solid

Analyte	MDL	MRL	Units
---------	-----	-----	-------

Note: MDLs are listed only if the corresponding analyte was evaluated to the MDL in this report .

# ORGANIC ANALYSIS DATA SHEET

## EPA 1311 ZHE

PDI-142RAB-C-00-30.4-191112

Laboratory: Apex Laboratories SDG: Gasco PreRD\_DG 2019  
Client: Anchor QEA, LLC Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization  
Matrix: SO Laboratory ID: A9K0412-01 File ID:  
Sampled: 11/12/19 15:40 Prepared: 11/18/19 15:55 Analyzed: 11/18/19 15:55  
Preparation: EPA 1311 TCLP/ZHE Initial/Final: 25 g / 500 mL

Batch: 9110920 Sequence: Calibration: Instrument: Inst

CAS NO.	COMPOUND	DILUTION	CONC. (N/A)	Q
NA	TCLP ZHE Extraction	1	PREP	

\* Values outside of QC limits

# PREPARATION BATCH SUMMARY

## EPA 1311 ZHE

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Batch: 9110920

Batch Matrix: Solid

Preparation: EPA 1311 TCLP/ZHE

SAMPLE NAME	LAB SAMPLE ID	LAB FILE ID	DATE PREPARED	OBSERVATIONS
PDI-142RAB-C-00-30.4-191112	A9K0412-01		11/18/19 15:55	

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# HOLDING TIME SUMMARY

## EPA 1311 ZHE

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sample Name	Date Collected	Date Received	Date Prepared	Days to Prep	Max Days to Prep	Date Analyzed	Days to Analysis	Max Days to Analysis	Q
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/18/19 15:55	6.01	14.00	11/18/19 15:55	0.00		



# Apex Laboratories

SDG: Gasco PreRD\_DG 2019

CLASS: METALS

METHOD: EPA 1311

**ANALYSES DATA PACKAGE COVER PAGE**

**EPA 1311**

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

---

**Client Sample Id:**

PDI-142RAB-C-00-30.4-191112

**Lab Sample Id:**

A9K0412-01

**Matrix**

SO

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hardcopy data package and in computer-readable data submitted on diskette has been authorized by the Laboratory Manager or the Manager's designee, as verified by the following signatures.

Signature: \_\_\_\_\_



Name: \_\_\_\_\_

David G. Jack

Forms Created: \_\_\_\_\_

12/18/2019 12:23PM

Title: \_\_\_\_\_

Technical Manager

# METHOD DETECTION AND REPORTING LIMITS

## EPA 1311

**Laboratory:** Apex Laboratories

**SDG:** Gasco PreRD\_DG 2019

**Client:** Anchor QEA, LLC

**Project:** Gasco PreRD\_DG 2019 - 4c. Waste Charac

**Batch Matrix:** Soil

Analyte	MDL	MRL	Units
---------	-----	-----	-------

Note: MDLs are listed only if the corresponding analyte was evaluated to the MDL in this report .

# INORGANIC ANALYSIS DATA SHEET

EPA 1311

PDI-142RAB-C-00-30.4-191112

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste  
Characterization

Matrix: SO

Laboratory ID: A9K0412-01

Sampled: 11/12/19 15:40

Prepared: 11/25/19 16:40

Analyzed: 11/25/19 16:40

Solids: N/A

Preparation: EPA 1311 (TCLP)

Initial/Final: 100 g / 2000 mL

Batch: 9111146

Calibration:

Instrument: Inst

CAS NO.	Analyte	Concentration (N/A)	Dilution Factor	Q	Method
TCLP	TCLP Extraction	PREP	1		EPA 1311
TCLP	TCLP Extraction	PREP	1		EPA 1311

# PREPARATION BATCH SUMMARY

## EPA 1311

Laboratory: Apex Laboratories

SDG: Gasco PreRD\_DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization

Batch: 9111146 Batch Matrix: Soil

Preparation: EPA 1311 (TCLP)

SAMPLE NAME	LAB SAMPLE ID	LAB FILE ID	DATE PREPARED	OBSERVATIONS
Blank	9111146-BLK1		11/25/19 16:40	
PDI-142RAB-C-00-30.4-191112	A9K0412-01		11/25/19 16:40	

Note: Client samples are listed only if they are included in this report.

Duplicates and Matrix Spike/Duplicates QC Samples are only listed if sourced from a sample included in this report.

# METHOD BLANK DATA SHEET

## EPA 1311

Laboratory: Apex Laboratories SDG: Gasco PreRD\_DG 2019  
Client: Anchor QEA, LLC Project: Gasco PreRD\_DG 2019 - 4c. Waste Characterization  
Matrix: Soil Laboratory ID: 9111146-BLK1 File ID:  
Prepared: 11/25/19 16:40 Preparation: EPA 1311 (TCLP) Initial/Final: 50 g / 1000 mL  
Analyzed: 11/25/19 16:40 Instrument: Inst  
Batch: 9111146 Sequence: Calibration:

CAS NO.	COMPOUND	CONC. (N/A)	Q
TCLP	TCLP Extraction	PREP	U

# HOLDING TIME SUMMARY

## EPA 1311

Laboratory: Apex Laboratories

SDG: Gasco PreRD DG 2019

Client: Anchor QEA, LLC

Project: Gasco PreRD DG 2019 - 4c. Waste Characterization

Sample Name	Date Collected	Date Received	Date Prepared	Days to Prep	Max Days to Prep	Date Analyzed	Days to Analysis	Max Days to Analysis	Q
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/25/19 16:40	13.04	14.00	11/25/19 16:40	0.00		
PDI-142RAB-C-00-30.4-191112	11/12/19 15:40	11/14/19 13:40	11/25/19 16:40	13.04	28.00	11/25/19 16:40	0.00		

**Raw Data**



**TCLP Volatile Organic Compounds by EPA 1311/8260C  
Benchsheet & Analysis Sequence Data**

Batch 9110813  
Sequence 9K19033 (A9K0412-01)

**PREPARATION BENCH SHEET**

**Apex Laboratories**



**BATCH #: 9110813 (Water)**

**Prep Method: EPA 1311/5030B TCLP Volatiles**

Lab Number	Cont.	Analysis	Prepared	Initial (mL)	Final (mL)	Spike ID	Source ID	ul Spike	ul Surr.	ClientID / Sample	Extraction Comments	pH*
9110813-BLK1		QC	11/19/19 09:00	5	5							
9110813-BS1		QC	11/19/19 09:00	5	5	A19K194		250			@50X	
A9K0403-01	A	1311/8260C TCLP/ZHE VOC	11/19/19 12:00	5	5					FC-111319-1219	MDL, ug/L	<del>✓</del>
9110813-DUPI		QC	11/19/19 12:00	5	5		A9K0403-01					<del>✓</del>
A9K0412-01	B	1311/8260C TCLP/ZHE VOC	11/19/19 12:00	5	5					PDI-142RAB-C-00-30.4-191112		<del>✓</del>
9110813-MS1		QC	11/19/19 12:00	5	5	A19K194	A9K0412-01	250			@50X	<del>✓</del>

\*pH <2 verified N/A 11/20/19 ml

**Standards/Reagents**

Reagent(s)			Analyte Spike(s)			Surrogate(s)		
Std ID	Exp. Date	Description	Std ID	Exp. Date	Description	Std ID	Exp. Date	Description
			A19K194	12/10/19	8260 Cal. Std. B VOCR+OXY Spike (20-40ug/r)			

GCMS9

Prepared By: 11/20/19 ml Date

Reviewed By: ML7 Date 11/20/19



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence: 9K19033  
Date: 11/19/19 10:00

Instrument: VOA-GCMS9  
Calibration: A9J2503

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
1	9K19033-IBL1	Water	QC	QC			A19I040	
2	9K19033-IBL2	Water	QC	QC			A19I040	
3	9K19033-TUN1	Water	QC	QC			A19I040	
4	9K19033-CCV1	Water	QC	QC			A19I040	
5	9110813-BS1	Water	QC	QC		9110813	A19I040	
6	9110813-BLK1	Water	QC	QC		9110813	A19I040	
7	A9K0403-01	Water	1311/8260C TCLP/ZHE VOC Reg List		11/20/19	9110813	A19I040	
8	9110813-DUP1	Water	QC	QC		9110813	A19I040	
9	A9K0412-01	Water	1311/8260C TCLP/ZHE VOC Reg List	Anchor QEA, LLC	11/27/19	9110813	A19I040	
10	9110813-MS1	Water	QC	QC		9110813	A19I040	
11	9K19033-IBL3	Water	QC	QC			A19I040	
12	9K19033-IBL4	Water	QC	QC			A19I040	

Data Entered By: 11/20/19 hnd



Comments:

Data Reviewed By: MK7 11/20/19

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111806.D  
 Acq On : 19 Nov 2019 11:06 am  
 Operator : TNL  
 Sample : 9K19033-TUN1  
 Misc : A19I039 5mL BFB (IS/SURR)  
 ALS Vial : 3 Sample Multiplier: 1

Integration File: RTEINT.P

Method : C:\msdchem\1\methods\VI191025W.M  
 Title : EPA 8260: Volatile Organic Compounds  
 Last Update : Fri Oct 25 08:32:21 2019





Spectrum Information: Average of 10.950 to 10.999 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
95	174	50	200	111.5	34329	PASS
96	95	5	9	6.9	2361	PASS
173	174	0.00	2	0.4	118	PASS
174	95	50	200	89.7	30783	PASS
175	174	5	9	6.9	2123	PASS
176	174	95	105	95.6	29429	PASS
177	176	5	10	6.4	1896	PASS

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111806.D  
 Acq On : 19 Nov 2019 11:06 am  
 Operator : TNL  
 Sample : 9K19033-TUN1  
 Misc : A19I039 5mL BFB (IS/SURR)  
 ALS Vial : 3 Sample Multiplier: 1

Integration File: RTEINT.P

Method : C:\msdchem\1\methods\VI191025W.M  
 Title : EPA 8260: Volatile Organic Compounds  
 Last Update : Fri Oct 25 08:32:21 2019



AutoFind: Scans 1543, 1544, 1545; Background Corrected with Scan 1536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
95	174	50	200	108.3	69251	PASS
96	95	5	9	6.7	4668	PASS
173	174	0.00	2	0.3	220	PASS
174	95	50	200	92.4	63957	PASS
175	174	5	9	6.9	4401	PASS
176	174	95	105	94.9	60699	FAIL*
177	176	5	10	6.5	3943	PASS

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111806.D  
 Acq On : 19 Nov 2019 11:06 am  
 Operator : TNL  
 Sample : 9K19033-TUN1  
 Misc : A19I039 5mL BFB (IS/SURR)  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 12:15:09 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene (I)	6.211	99	95143	50.00	ug/L	# 0.00
45) Chlorobenzene-d5 (I)	9.910	117	277774	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	123710	50.00	ug/L	0.00
System Monitoring Compounds						
32) Dibromofluoromethane (S)	5.712	111	104077	55.67	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.777	114	329989	54.90	ug/L	0.00
48) Toluene-d8 (S)	8.297	98	363896	49.91	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	102739	51.40	ug/L	0.00
Target Compounds						
3) Chloromethane	1.891	50	199	0.10	ug/L	# 47
5) Bromomethane	2.354	96	222	0.18	ug/L	# 33
14) Methylene Chloride	3.869	84	1176	Below Cal		83
15) Acetone	3.942	43	635	0.76	ug/L	83

*11/19/19 TNL*

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
Data File : VI19111806.D  
Acq On : 19 Nov 2019 11:06 am  
Operator : TNL  
Sample : 9K19033-TUN1  
Misc : A19I039 5mL BFB (IS/SURR)  
ALS Vial : 3 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 12:15:09 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration



Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111807.D  
 Acq On : 19 Nov 2019 11:33 am  
 Operator : TNL  
 Sample : 9110813-BS1@50  
 Misc : 50X 1mL/50mL 20/40PPB VOCRO A19K194  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 12:15:12 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

*11/19/19 TNL*

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I Pentafluorobenzene (I)	50.000	50.000	0.0	92	0.00
2 Dichlorodifluoromethane	20.000	19.564	2.2	92	0.01
3 P Chloromethane	20.000	18.468	7.7	92	0.00
4 C Vinyl Chloride	20.000	20.466	-2.3	92	0.00
5 Bromomethane	20.000	22.365	-11.8	107	0.01
6 Chloroethane	20.000	15.111	<u>24.4#</u>	78	0.01 <i>255</i>
7 Trichlorofluoromethane	20.000	21.142	-5.7	92	0.01
8 Ethanol	1250.000	1142.977	8.6	81	0.00
9 C 1,1-Dichloroethene	20.000	20.811	-4.1	94	0.00
10 Carbon Disulfide	20.000	21.612	-8.1	99	0.01
11 Freon 113	20.000	22.687	-13.4	101	0.01
12 Iodomethane	20.000	13.528	<i>NR</i> 32.4#	74	0.01
13 Acrolein	20.000	21.315	-6.6	96	0.01
14 Methylene Chloride	20.000	22.735	-13.7	102	0.00
15 Acetone	40.000	35.917	10.2	83	0.00
16 t-1,2-Dichloroethene	20.000	21.202	-6.0	91	0.01
17 n-Hexane	20.000	22.434	-12.2	99	0.00
18 Methyl-tert-butyl-ether	20.000	18.583	7.1	84	0.00
19 tert-Butanol (TBA)	1250.000	1118.507	10.5	73	0.00
20 Diisopropyl ether (DIPE)	5.000	4.044	19.1	70	0.00
21 P 1,1-Dichloroethane	20.000	20.365	-1.8	90	0.00
22 Acrylonitrile	20.000	21.722	-8.6	95	0.00
23 Ethyl-tert-butyl ether (ET)	5.000	3.990	<i>✓</i> 20.2#	69	0.00 <i>80%</i>
24 Vinyl Acetate	20.000	20.188	-0.9	90	0.00
25 c-1,2-Dichloroethene	20.000	20.267	-1.3	89	0.00
26 2,2-Dichloropropane	20.000	21.782	-8.9	98	0.00
27 Bromochloromethane	20.000	24.516	<u>-22.6#</u>	100	0.00 <i>056</i>
28 C Chloroform	20.000	21.965	-9.8	94	0.00
29 Carbon Tetrachloride	20.000	24.054	<i>✓</i> -20.3#	108	0.00 <i>120%</i>
30 Tetrahydrofuran	20.000	18.641	6.8	83	0.00
31 1,1,1-Trichloroethane	20.000	20.971	-4.9	93	0.00
32 S Dibromofluoromethane (S)	50.000	54.343	-8.7	101	0.00
33 1,1-Dichloropropene	20.000	20.712	-3.6	93	0.00
34 2-Butanone (MEK)	40.000	38.869	2.8	87	0.00
35 Benzene	20.000	21.324	-6.6	96	0.00
36 tert-Amyl methyl ether (TA)	5.000	4.117	17.7	73	0.00
37 1,2-Dichloroethane (EDC)	20.000	19.246	3.8	85	0.00
38 iso-Butyl Alcohol	500.000	472.239	5.6	81	0.00
39 S 1,4-Difluorobenzene (S)	50.000	53.747	-7.5	99	0.00
40 Trichloroethene (TCE)	20.000	23.098	-15.5	99	0.00
41 Tert-Amyl-Ethyl-Ether (TAEE)	5.000	3.714	<i>NR</i> 25.7#	63	0.00
42 Dibromomethane	20.000	22.655	-13.3	97	0.00
43 C 1,2-Dichloropropane	20.000	20.971	-4.9	93	0.00
44 Bromodichloromethane	20.000	22.521	-12.6	99	0.00
45 Chlorobenzene-d5 (I)	50.000	50.000	0.0	98	0.00
46 2-Chloroethyl Vinyl Ether	20.000	14.816	<i>NR</i> 25.9#	69	0.00
47 c-1,3-Dichloropropene	20.000	20.125	-0.6	93	0.00
48 S Toluene-d8 (S)	50.000	49.099	1.8	97	0.00
49 C Toluene	20.000	19.547	2.3	95	0.00
50 Tetrachloroethene (PCE)	20.000	21.754	-8.8	99	0.00



Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111807.D  
 Acq On : 19 Nov 2019 11:33 am  
 Operator : TNL  
 Sample : 9110813-BS1@50  
 Misc : 50X 1mL/50mL 20/40PPB VOCRO A19K194  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 12:15:12 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
51 4-Methyl-2-Pentanone (MIBK)	40.000	36.664	8.3	82	0.00
52 t-1,3-Dichloropropene	20.000	19.527	2.4	91	0.00
53 1,1,2-Trichloroethane	20.000	21.373	-6.9	97	0.00
54 Dibromochloromethane	20.000	26.526	-32.6#	114	0.00
55 1,3-Dichloropropane	20.000	20.037	-0.2	92	0.00
56 1,2-Dibromoethane (EDB)	20.000	20.360	-1.8	93	0.00
57 2-Hexanone	40.000	35.762	10.6	81	0.00
58 P Chlorobenzene	20.000	20.540	-2.7	96	0.00
59 C Ethylbenzene	20.000	19.601	2.0	93	0.00
60 1,1,1,2-Tetrachloroethane	20.000	23.250	-16.3	106	0.00
61 m,p-Xylenes (2)	40.000	39.187	2.0	90	0.00
62 o-Xylene	20.000	18.956	5.2	86	0.00
63 Styrene	20.000	19.814	0.9	90	0.00
64 P Bromoform	20.000	26.162	-30.8#	131	0.00
65 Isopropylbenzene	20.000	19.217	3.9	87	0.00
66 I 1,4-Dichlorobenzene-d4 (I)	50.000	50.000	0.0	98	0.00
67 S 4-Bromofluorobenzene (S)	50.000	49.054	1.9	98	0.00
68 Bromobenzene	20.000	20.626	-3.1	95	0.00
69 n-Propylbenzene	20.000	19.384	3.1	91	0.00
70 P 1,1,2,2-Tetrachloroethane	20.000	19.938	0.3	93	0.00
71 2-Chlorotoluene	20.000	19.491	2.5	91	0.00
72 1,3,5-Trimethylbenzene	20.000	19.610	2.0	89	0.00
73 1,2,3-Trichloropropane	20.000	19.856	0.7	93	0.00
74 t-1,4-Dichloro-2-butene	20.000	18.199	9.0	85	0.00
75 4-Chlorotoluene	20.000	19.104	4.5	90	0.00
76 tert-Butylbenzene	20.000	18.138	9.3	84	0.00
77 1,2,4-Trimethylbenzene	20.000	19.799	1.0	89	0.00
78 sec-Butylbenzene	20.000	19.305	3.5	89	0.00
79 4-Isopropyltoluene	20.000	20.027	-0.1	87	0.00
80 1,3-Dichlorobenzene	20.000	20.360	-1.8	95	0.00
81 1,4-Dichlorobenzene	20.000	20.069	-0.3	94	0.00
82 n-Butylbenzene	20.000	20.735	-3.7	89	0.00
83 1,2-Dichlorobenzene	20.000	19.931	0.3	93	0.00
84 1,2-Dibromo-3-Chloropropane	20.000	20.075	-0.4	97	0.00
85 Hexachlorobutadiene	20.000	20.069	-0.3	91	0.00
86 1,2,4-Trichlorobenzene	20.000	19.162	4.2	85	0.00
87 Naphthalene	20.000	17.588	12.1	78	0.00
88 1,2,3-Trichlorobenzene	20.000	19.793	1.0	88	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111807.D  
 Acq On : 19 Nov 2019 11:33 am  
 Operator : TNL  
 Sample : 9110813-BS1@50  
 Misc : 50X 1mL/50mL 20/40PPB VOCRO A19K194  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 12:15:12 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

*11/19/19 TNL*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	103299	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.910	117	301980	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	149066	50.00	ug/L		0.00
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.718	111	110300	54.34	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.783	114	350758	53.75	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	389168	49.10	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	118149	49.05	ug/L		0.00
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.685	85	33035	19.56	ug/L		99
3) Chloromethane	1.898	50	41354	18.47	ug/L		96
4) Vinyl Chloride	2.001	62	45913	20.47	ug/L		97
5) Bromomethane	2.366	96	29578	22.36	ug/L		96
6) Chloroethane	2.500	64	15580	<u>15.11</u>	ug/L		81 <i>Q55</i>
7) Trichlorofluoromethane	2.670	101	53707	21.14	ug/L		95
8) Ethanol	3.236	45	56739	1142.98	ug/L		89
9) 1,1-Dichloroethene	3.236	61	50962	20.81	ug/L		89
10) Carbon Disulfide	3.254	76	97657	21.61	ug/L		99
11) Freon 113	3.291	101	39945	22.69	ug/L		92
12) Iodomethane	3.394	142	8522	13.53	ug/L		94
13) Acrolein	3.625	56	10004	21.32	ug/L		79
14) Methylene Chloride	3.875	84	44432	22.73	ug/L		83
15) Acetone	3.942	43	32513	35.92	ug/L		87
16) t-1,2-Dichloroethene	4.045	61	50815	21.20	ug/L		84
17) n-Hexane	4.124	86	8186	22.43	ug/L		92
18) Methyl-tert-butyl-ether	4.167	73	103522	18.58	ug/L		91
19) tert-Butanol (TBA)	4.294	59	447328	1118.51	ug/L		98
20) Diisopropyl ether (DIPE)	4.568	45	24241	4.04	ug/L		93
21) 1,1-Dichloroethane	4.684	63	67791	20.36	ug/L		96
22) Acrylonitrile	4.751	53	21765	21.72	ug/L		99
23) Ethyl-tert-butyl ether...	4.939	59	22986	3.99	ug/L		96
24) Vinyl Acetate	4.958	43	81166	20.19	ug/L		96
25) c-1,2-Dichloroethene	5.243	61	52081	20.27	ug/L		86
26) 2,2-Dichloropropane	5.353	77	47316	21.78	ug/L		92
27) Bromochloromethane	5.450	130	30912	<u>24.52</u>	ug/L		90 <i>Q56</i>
28) Chloroform	5.529	83	71482	21.96	ug/L		94
29) Carbon Tetrachloride	5.663	117	47612	24.05	ug/L		92
30) Tetrahydrofuran	5.700	42	17756	18.64	ug/L		83
31) 1,1,1-Trichloroethane	5.736	97	57610	20.97	ug/L		98
33) 1,1-Dichloropropene	5.864	75	54639	20.71	ug/L		93
34) 2-Butanone (MEK)	5.852	43	55781	38.87	ug/L		98
35) Benzene	6.120	78	168321	21.32	ug/L		96
36) tert-Amyl methyl ether...	6.247	73	22051	4.12	ug/L		89
37) 1,2-Dichloroethane (EDC)	6.339	62	49765	19.25	ug/L		92
38) iso-Butyl Alcohol	6.375	43	67896	472.24	ug/L		97
40) Trichloroethene (TCE)	6.746	130	46979	23.10	ug/L		92
41) Tert-Amyl-Ethyl-Ether ...	6.996	59	14362	3.71	ug/L		78
42) Dibromomethane	7.196	93	28700	22.66	ug/L		95
43) 1,2-Dichloropropane	7.306	63	41290	20.97	ug/L		88
44) Bromodichloromethane	7.379	83	51125	22.52	ug/L		91
46) 2-Chloroethyl Vinyl Ether	8.024	63	22967	14.82	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	60085	20.12	ug/L		82

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111807.D  
 Acq On : 19 Nov 2019 11:33 am  
 Operator : TNL  
 Sample : 9110813-BS1@50  
 Misc : 50X 1mL/50mL 20/40PPB VOCRO A19K194  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Nov 19 12:15:12 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	173580	19.55	ug/L	98
50) Tetrachloroethene (PCE)	8.796	166	44966	21.75	ug/L	94
51) 4-Methyl-2-Pentanone (...)	8.796	43	98843	36.66	ug/L	91
52) t-1,3-Dichloropropene	8.833	75	51712	19.53	ug/L	97
53) 1,1,2-Trichloroethane	9.003	97	42075	21.37	ug/L	92
54) Dibromochloromethane	9.186	129	42215	26.53	ug/L	100
55) 1,3-Dichloropropane	9.289	76	68042	20.04	ug/L	86
56) 1,2-Dibromoethane (EDB)	9.423	107	43638	20.36	ug/L	95
57) 2-Hexanone	9.654	43	70645	35.76	ug/L	90
58) Chlorobenzene	9.928	112	116428	20.54	ug/L	97
59) Ethylbenzene	9.952	91	182539	19.60	ug/L	97
60) 1,1,1,2-Tetrachloroethane	9.989	131	38433	23.25	ug/L	95
61) m,p-Xylenes (2)	10.086	91	268736	39.19	ug/L	98
62) o-Xylene	10.463	91	128879	18.96	ug/L	99
63) Styrene	10.512	104	108274	19.81	ug/L	98
64) Bromoform	10.536	173	31234	26.16	ug/L	97
65) Isopropylbenzene	10.731	105	159395	19.22	ug/L	96
68) Bromobenzene	11.059	156	47654	20.63	ug/L	94
69) n-Propylbenzene	11.072	91	192025	19.38	ug/L	100
70) 1,1,2,2-Tetrachloroethane	11.138	85	38888	19.94	ug/L	94
71) 2-Chlorotoluene	11.205	126	41607	19.49	ug/L	89
72) 1,3,5-Trimethylbenzene	11.230	105	132754	19.61	ug/L	96
73) 1,2,3-Trichloropropane	11.248	110	18834	19.86	ug/L	93
74) t-1,4-Dichloro-2-butene	11.278	53	12352	18.20	ug/L	83
75) 4-Chlorotoluene	11.339	91	116487	19.10	ug/L	99
76) tert-Butylbenzene	11.479	91	68563	18.14	ug/L	99
77) 1,2,4-Trimethylbenzene	11.534	105	134842	19.80	ug/L	99
78) sec-Butylbenzene	11.619	105	161033	19.31	ug/L	98
79) 4-Isopropyltoluene	11.722	119	132167	20.03	ug/L	97
80) 1,3-Dichlorobenzene	11.796	146	81946	20.36	ug/L	99
81) 1,4-Dichlorobenzene	11.862	146	84232	20.07	ug/L	97
82) n-Butylbenzene	12.045	91	116294	20.74	ug/L	97
83) 1,2-Dichlorobenzene	12.179	146	77903	19.93	ug/L	99
84) 1,2-Dibromo-3-Chloropr...	12.799	157	13268	20.08	ug/L	89
85) Hexachlorobutadiene	13.304	223	10961	20.07	ug/L	97
86) 1,2,4-Trichlorobenzene	13.347	180	43165	19.16	ug/L	97
87) Naphthalene	13.627	128	125968	17.59	ug/L	98
88) 1,2,3-Trichlorobenzene	13.785	180	42333	19.79	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
Data File : VI19111807.D  
Acq On : 19 Nov 2019 11:33 am  
Operator : TNL  
Sample : 9110813-BS1@50  
Misc : 50X 1mL/50mL 20/40PPB VOCRO A19K194  
ALS Vial : 4 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 12:15:12 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111808.D  
 Acq On : 19 Nov 2019 12:00 pm  
 Operator : TNL  
 Sample : 9110813-BLK1@50  
 Misc : 50X 1mL/50mL TCLP/ZHE  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 14:51:19 2019  
 Quant Method : C:\msdchem\1\methods\VI190806W+.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene (I)	6.217	99	94973	50.00	ug/L	# 0.00
45) Chlorobenzene-d5 (I)	9.910	117	274403	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	123791	50.00	ug/L	0.00
<b>System Monitoring Compounds</b>						
32) Dibromofluoromethane (S)	5.712	111	102982	52.86	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.783	114	327916	60.27	ug/L	0.00 <i>ob</i>
48) Toluene-d8 (S)	8.297	98	363872	51.37	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	101414	50.93	ug/L	0.00
<b>Target Compounds</b>						
3) Chloromethane	1.898	50	238	0.11	ug/L	# 47
5) Bromomethane	2.366	96	288	0.19	ug/L	# 69
10) Carbon Disulfide	3.254	76	488	0.12	ug/L	# 78
14) Methylene Chloride	3.875	84	2019	Below Cal		# 93
15) Acetone	3.948	43	913	1.12	ug/L	# 44
28) Chloroform	5.529	83	470	0.14	ug/L	# 86
61) m,p-Xylenes (2)	10.092	91	280	0.10	ug/L	# 34
77) 1,2,4-Trimethylbenzene	11.534	105	177	0.11	ug/L	# 35
79) 4-Isopropyltoluene	11.729	119	154	0.14	ug/L	# 51
82) n-Butylbenzene	12.045	91	433	0.10	ug/L	# 68
86) 1,2,4-Trichlorobenzene	13.341	180	445	0.31	ug/L	# 67
87) Naphthalene	13.627	128	1138	0.65	ug/L	# 81
88) 1,2,3-Trichlorobenzene	13.785	180	490	0.35	ug/L	# 67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

*11/19/19*

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
Data File : VI19111808.D  
Acq On : 19 Nov 2019 12:00 pm  
Operator : TNL  
Sample : 9110813-BLK1@50  
Misc : 50X 1mL/50mL TCLP/ZHE  
ALS Vial : 5 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 14:51:19 2019  
Quant Method : C:\msdchem\1\methods\VI190806W+.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111811.D  
 Acq On : 19 Nov 2019 1:21 pm  
 Operator : TNL  
 Sample : A9K0412-01@50  
 Misc : 50X 1mL/50mL ZHE REG LIST  
 ALS Vial : 8 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 14:51:28 2019  
 Quant Method : C:\msdchem\1\methods\VI190806W+.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene (I)	6.211	99	94988	50.00	ug/L	# 0.00
45) Chlorobenzene-d5 (I)	9.910	117	272456	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	122016	50.00	ug/L	0.00
System Monitoring Compounds						
32) Dibromofluoromethane (S)	5.712	111	103419	53.08	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.777	114	325009	59.73	ug/L	-0.01
48) Toluene-d8 (S)	8.297	98	357185	50.78	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	99457	50.68	ug/L	0.00
Target Compounds						
5) Bromomethane	2.366	96	255	0.17	ug/L	Qvalue 78
6) Chloroethane	2.561	64	119	0.12	ug/L	# 36
14) Methylene Chloride	3.875	84	1180	Below Cal	#	82
15) Acetone	3.942	43	372	0.45	ug/L	# 44
87) Naphthalene	13.627	128	2037	0.86	ug/L	# 81


*11/19/19*

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
Data File : VI19111811.D  
Acq On : 19 Nov 2019 1:21 pm  
Operator : TNL  
Sample : A9K0412-01@50  
Misc : 50X 1mL/50mL ZHE REG LIST  
ALS Vial : 8 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 14:51:28 2019  
Quant Method : C:\msdchem\1\methods\VI190806W+.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration





Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111812.D  
 Acq On : 19 Nov 2019 1:48 pm  
 Operator : TNL  
 Sample : 9110813-MS1@50  
 Misc : 50X 1mL/50mL A19K194 (A9K0412-01)  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 14:51:31 2019  
 Quant Method : C:\msdchem\1\methods\VI190806W+.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (I)	6.217	99	103460	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.910	117	305031	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	151550	50.00	ug/L		0.00
System Monitoring Compounds							
32) Dibromofluoromethane (S)	5.718	111	110621	52.12	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.783	114	351443	59.30	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	388897	49.39	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	118037	48.42	ug/L		0.00
Target Compounds							
						Qvalue	
2) Dichlorodifluoromethane	1.685	85	33456	16.45	ug/L		97
3) Chloromethane	1.904	50	40619	16.96	ug/L		96
4) Vinyl Chloride	2.007	62	46235	21.64	ug/L		97
5) Bromomethane	2.366	96	27993	16.99	ug/L		96
6) Chloroethane	2.500	64	15203	14.02	ug/L		82
7) Trichlorofluoromethane	2.670	101	54373	15.95	ug/L		97
8) Ethanol	3.242	45	57962	1402.69	ug/L		86
9) 1,1-Dichloroethene	3.236	61	50789	19.45	ug/L		87
10) Carbon Disulfide	3.254	76	96360	22.49	ug/L		99
11) Freon 113	3.291	101	39978	23.47	ug/L		96
12) Iodomethane	3.394	142	10006	16.15	ug/L		95
13) Acrolein	3.625	56	9988	27.05	ug/L		72
14) Methylene Chloride	3.875	84	43618	21.22	ug/L		86
15) Acetone	3.948	43	32193	36.11	ug/L		87
16) t-1,2-Dichloroethene	4.045	61	51007	21.79	ug/L		86
17) n-Hexane	4.124	86	8014	27.94	ug/L		98
18) Methyl-tert-butyl-ether	4.173	73	102256	19.81	ug/L		93
19) tert-Butanol (TBA)	4.294	59	449962	1406.86	ug/L		96
20) Diisopropyl ether (DIPE)	4.568	45	24161	4.59	ug/L		96
21) 1,1-Dichloroethane	4.684	63	67985	20.61	ug/L		96
22) Acrylonitrile	4.751	53	21677	22.26	ug/L		95
23) Ethyl-tert-butyl ether...	4.945	59	22548	4.82	ug/L		95
24) Vinyl Acetate	4.957	43	80978	20.64	ug/L		96
25) c-1,2-Dichloroethene	5.243	61	51600	20.04	ug/L		85
26) 2,2-Dichloropropane	5.353	77	45076	19.59	ug/L		95
27) Bromochloromethane	5.450	130	30783	24.21	ug/L		90
28) Chloroform	5.529	83	71148	20.12	ug/L		97
29) Carbon Tetrachloride	5.663	117	47019	19.40	ug/L		96
30) Tetrahydrofuran	5.700	42	17577	20.55	ug/L		83
31) 1,1,1-Trichloroethane	5.736	97	56178	19.21	ug/L		98
33) 1,1-Dichloropropene	5.864	75	54236	23.15	ug/L		93
34) 2-Butanone (MEK)	5.858	43	55862	41.11	ug/L		90
35) Benzene	6.119	78	166638	23.65	ug/L		95
36) tert-Amyl methyl ether...	6.247	73	21775	4.64	ug/L		91
37) 1,2-Dichloroethane (EDC)	6.345	62	49882	17.34	ug/L		92
38) iso-Butyl Alcohol	6.375	43	70878	575.85	ug/L		97
40) Trichloroethene (TCE)	6.746	130	46771	26.05	ug/L		93
41) Tert-Amyl-Ethyl-Ether ...	7.002	59	14048	4.74	ug/L		79
42) Dibromomethane	7.196	93	28159	22.02	ug/L		95
43) 1,2-Dichloropropane	7.306	63	41153	21.51	ug/L		90
44) Bromodichloromethane	7.379	83	50602	19.70	ug/L		94
46) 2-Chloroethyl Vinyl Ether	8.024	63	22935	18.64	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	59401	20.57	ug/L		82

*11/19/19*

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
 Data File : VI19111812.D  
 Acq On : 19 Nov 2019 1:48 pm  
 Operator : TNL  
 Sample : 9110813-MS1@50  
 Misc : 50X 1mL/50mL A19K194 (A9K0412-01)  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Nov 19 14:51:31 2019  
 Quant Method : C:\msdchem\1\methods\VI190806W+.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	173776	20.36	ug/L	99
50) Tetrachloroethene (PCE)	8.796	166	44945	23.06	ug/L	94
51) 4-Methyl-2-Pentanone (...)	8.796	43	100017	36.99	ug/L	93
52) t-1,3-Dichloropropene	8.839	75	51510	17.92	ug/L	99
53) 1,1,2-Trichloroethane	9.003	97	41218	20.05	ug/L	94
54) Dibromochloromethane	9.186	129	40733	18.88	ug/L	96
55) 1,3-Dichloropropane	9.289	76	67243	19.56	ug/L	86
56) 1,2-Dibromoethane (EDB)	9.423	107	43974	20.83	ug/L	98
57) 2-Hexanone	9.654	43	71503	36.56	ug/L	86
58) Chlorobenzene	9.928	112	116471	21.55	ug/L	96
59) Ethylbenzene	9.952	91	182338	20.44	ug/L	97
60) 1,1,1,2-Tetrachloroethane	9.989	131	37922	20.26	ug/L	96
61) m,p-Xylenes (2)	10.086	91	269747	42.18	ug/L	98
62) o-Xylene	10.463	91	128775	20.35	ug/L	99
63) Styrene	10.512	104	108787	22.17	ug/L	99
64) Bromoform	10.536	173	30398	19.87	ug/L	97
65) Isopropylbenzene	10.731	105	161063	21.53	ug/L	98
68) Bromobenzene	11.059	156	47528	21.77	ug/L	92
69) n-Propylbenzene	11.071	91	193709	20.40	ug/L	99
70) 1,1,2,2-Tetrachloroethane	11.138	85	39553	19.98	ug/L	93
71) 2-Chlorotoluene	11.205	126	42108	22.35	ug/L	88
72) 1,3,5-Trimethylbenzene	11.230	105	133882	21.14	ug/L	97
73) 1,2,3-Trichloropropane	11.248	110	19343	20.01	ug/L	88
74) t-1,4-Dichloro-2-butene	11.278	53	12118	16.11	ug/L	80
75) 4-Chlorotoluene	11.339	91	117587	20.87	ug/L	99
76) tert-Butylbenzene	11.479	91	68421	19.62	ug/L	99
77) 1,2,4-Trimethylbenzene	11.534	105	136079	21.96	ug/L	97
78) sec-Butylbenzene	11.619	105	159898	21.08	ug/L	98
79) 4-Isopropyltoluene	11.722	119	130978	22.76	ug/L	97
80) 1,3-Dichlorobenzene	11.795	146	82534	21.52	ug/L	100
81) 1,4-Dichlorobenzene	11.862	146	85210	20.20	ug/L	96
82) n-Butylbenzene	12.045	91	114879	21.76	ug/L	99
83) 1,2-Dichlorobenzene	12.179	146	78159	21.22	ug/L	99
84) 1,2-Dibromo-3-Chloropr...	12.799	157	13224	22.94	ug/L	91
85) Hexachlorobutadiene	13.304	223	10544	20.62	ug/L	89
86) 1,2,4-Trichlorobenzene	13.341	180	43114	24.61	ug/L	96
87) Naphthalene	13.627	128	132926	23.52	ug/L	98
88) 1,2,3-Trichlorobenzene	13.785	180	42924	25.06	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-11\9K19033\  
Data File : VI19111812.D  
Acq On : 19 Nov 2019 1:48 pm  
Operator : TNL  
Sample : 9110813-MS1@50  
Misc : 50X 1mL/50mL A19K194 (A9K0412-01)  
ALS Vial : 9 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Nov 19 14:51:31 2019  
Quant Method : C:\msdchem\1\methods\VI190806W+.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



**TCLP Volatile Organic Compounds by EPA 1311/8260C  
Calibration Data**

Sequence 9J24043 (Cal ID A9J2503) VOA-GCMS9



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence: 9J24043

Instrument: VOA-GCMS9

Date: 10/24/19 14:12

Calibration: A9J2503

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
1	9J24043-IBL1	Water	QC	QC			A19I040	
2	9J24043-TUN1	Water	QC	QC			A19I040	
3	9J24043-ICB1	Water	QC	QC			A19I040	
4	9J24043-CAL1	Water	QC	QC			A19I040	A19J377
5	9J24043-CAL2	Water	QC	QC			A19I040	A19J378
6	9J24043-CAL3	Water	QC	QC			A19I040	A19J379
7	9J24043-CAL4	Water	QC	QC			A19I040	A19J380
8	9J24043-CAL5	Water	QC	QC			A19I040	A19J381
9	9J24043-CAL6	Water	QC	QC			A19I040	A19J382
10	9J24043-CAL7	Water	QC	QC			A19I040	A19J383
11	9J24043-CAL8	Water	QC	QC			A19I040	A19J384
12	9J24043-CAL9	Water	QC	QC			A19I040	A19J385
13	9J24043-IBL2	Water	QC	QC			A19I040	
14	9J24043-CALA	Water	QC	QC			A19I040	A19J386
15	9J24043-IBL3	Water	QC	QC			A19I040	
16	9J24043-CALB	Water	QC	QC			A19I040	A19J387
17	9J24043-IBL4	Water	QC	QC			A19I040	
18	9J24043-IBL5	Water	QC	QC			A19I040	
19	9J24043-ICV1	Water	QC	QC			A19I040	A19J131
20	9J24043-ICV2	Water	QC	QC			A19I040	A19E195
21	9J24043-IBL6	Water	QC	QC			A19I040	
22	9J24043-TUN2	Water	QC	QC			A19I040	
23	9J24043-IBL7	Water	QC	QC			A19I040	
24	9J24043-ICB2	Water	QC	QC			A19I040	
25	9J24043-CALC	Water	QC	QC			A19I040	A19J388
26	9J24043-CALD	Water	QC	QC			A19I040	A19J389
27	9J24043-CALE	Water	QC	QC			A19I040	A19J390
28	9J24043-CALF	Water	QC	QC			A19I040	A19J391
29	9J24043-CALH	Water	QC	QC			A19I040	A19J393
30	9J24043-CALI	Water	QC	QC			A19I040	A19J394
31	9J24043-CALJ	Water	QC	QC			A19I040	A19J395
32	9J24043-IBL8	Water	QC	QC			A19I040	
33	9J24043-IBL9	Water	QC	QC			A19I040	
34	9J24043-IBLA	Water	QC	QC			A19I040	
35	9J24043-IBLB	Water	QC	QC			A19I040	
36	9J24043-CALG	Water	QC	QC			A19I040	A19J392
37	9J24043-ICV3	Water	QC	QC			A19I040	A19G350

Data Entered By: *[Signature]* 10/25/19

Comments:

Data Reviewed By: *[Signature]* 10/28/19

Calibration Status Report VOA-GCMS9

Method Path : C:\msdchem\1\methods\  
 Method File : VI191025W.M  
 Title : EPA 8260: Volatile Organic Compounds  
 Last Update : Fri Oct 25 08:32:21 2019  
 Response Via : Initial Calibration

#	ID	Conc	ISTD Conc	Path\File
1	0.1	-1	50	C:\msdchem\1\data\2019-10\9J24043\VI19102417.D
2	0.2	0	50	C:\msdchem\1\data\2019-10\9J24043\VI19102418.D
3	0.5	0	50	C:\msdchem\1\data\2019-10\9J24043\VI19102419.D
4	1	1	50	C:\msdchem\1\data\2019-10\9J24043\VI19102420.D
5	2	2	50	C:\msdchem\1\data\2019-10\9J24043\VI19102421.D
6	5	5	50	C:\msdchem\1\data\2019-10\9J24043\VI19102422.D
7	10	10	50	C:\msdchem\1\data\2019-10\9J24043\VI19102423.D
8	20	20	50	C:\msdchem\1\data\2019-10\9J24043\VI19102424.D
9	50	50	50	C:\msdchem\1\data\2019-10\9J24043\VI19102425.D
10	100	100	50	C:\msdchem\1\data\2019-10\9J24043\VI19102427.D
11	200	200	50	C:\msdchem\1\data\2019-10\9J24043\VI19102429.D

#	ID	Update Time	Quant Time	Acquisition Time
1	0.1	Oct 25 08:32 2019	Oct 25 08:17 2019	24 Oct 2019 3:55 pm
2	0.2	Oct 25 08:32 2019	Oct 25 08:19 2019	24 Oct 2019 4:21 pm
3	0.5	Oct 25 08:32 2019	Oct 25 08:21 2019	24 Oct 2019 4:48 pm
4	1	Oct 25 08:32 2019	Oct 25 08:23 2019	24 Oct 2019 5:15 pm
5	2	Oct 25 08:32 2019	Oct 25 08:24 2019	24 Oct 2019 5:42 pm
6	5	Oct 25 08:32 2019	Oct 25 08:25 2019	24 Oct 2019 6:09 pm
7	10	Oct 25 08:32 2019	Oct 25 08:10 2019	24 Oct 2019 6:36 pm
8	20	Oct 25 08:32 2019	Oct 25 08:10 2019	24 Oct 2019 7:03 pm
9	50	Oct 25 08:32 2019	Oct 25 08:10 2019	24 Oct 2019 7:30 pm
10	100	Oct 25 08:32 2019	Oct 25 08:10 2019	24 Oct 2019 8:24 pm
11	200	Oct 25 08:32 2019	Oct 25 08:30 2019	24 Oct 2019 9:17 pm

VI191025W.M Fri Oct 25 09:01:36 2019

# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9J24043

### Analysis Included

8260C Full List  
8260C Additional Cpds  
8260C Iodomethane Add On  
8260C Oxygenates

### INSTRUMENT SEQUENCE LOG

<u>SampleID</u>	<u>SampleName</u>	<u>Matrix</u>	<u>STDID</u>	<u>ISTD ID</u>	<u>Analyzed</u>
9J24043-TUN1	MS Tune	Water		A19I040	10/24/2019 3:01:00PM
9J24043-ICB1	Initial Cal Blank	Water		A19I040	10/24/2019 3:28:00PM
9J24043-CAL1	Cal Standard	Water	A19J377	"	10/24/2019 3:55:00PM
9J24043-CAL2	Cal Standard	Water	A19J378	"	10/24/2019 4:21:00PM
9J24043-CAL3	Cal Standard	Water	A19J379	"	10/24/2019 4:48:00PM
9J24043-CAL4	Cal Standard	Water	A19J380	"	10/24/2019 5:15:00PM
9J24043-CAL5	Cal Standard	Water	A19J381	"	10/24/2019 5:42:00PM
9J24043-CAL6	Cal Standard	Water	A19J382	"	10/24/2019 6:09:00PM
9J24043-CAL7	Cal Standard	Water	A19J383	"	10/24/2019 6:36:00PM
9J24043-CAL8	Cal Standard	Water	A19J384	"	10/24/2019 7:03:00PM
9J24043-CAL9	Cal Standard	Water	A19J385	"	10/24/2019 7:30:00PM
9J24043-CALA	Cal Standard	Water	A19J386	"	10/24/2019 8:24:00PM
9J24043-CALB	Cal Standard	Water	A19J387	"	10/24/2019 9:17:00PM
9J24043-ICV1	Initial Cal Check	Water	A19J131	"	10/24/2019 10:38:00PM
9J24043-ICV2	Initial Cal Check	Water	A19E195	"	10/24/2019 11:05:00PM

### CALIBRATION STANDARD RECOVERIES

Calibration: **A9J2503**

Instrument: **VOA-GCMS9**

8260C Full List

Sequence: **9J24043**

Matrix: **Water**

<b>9J24043-CAL1</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CAL2</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CAL3</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CAL4</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CAL5</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CAL6</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CAL7</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CAL8</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CAL9</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CALA</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CALB</b>	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>

# CALIBRATION SEQUENCE REVIEW SHEET

**SEQUENCE: 9J24043**

Compounds listed above have recalculated recoveries outside 70-130% of the true values, and the calibration levels are above the reporting level. If no compounds are listed, all are OK. Please see the next section for quadratic fit compounds.

## Analytes With Quadratic Curve Fits

Qualifier   iMDL   iMRL   Spike Amt   %Difference   OK?   Raise MRL to ?  
 \_\_\_\_\_         \_\_\_\_\_

Analytes listed above have quadratic curve fits. If they are using a weighting option, they must be checked against the requested curve points to determine if the recalculated results are within limits (70-130 or as specified).

### ICV RECOVERIES

Calibration: **A9J2503**

Instrument: **VOA-GCMS9**

8260C Full List

Sequence: **9J24043**

Matrix: **Water**

9J24043-ICV1	Inst. MRL	ICV Level	Result	%Rec.	Qual
9J24043-ICV2	Inst. MRL	ICV Level	Result	%Rec.	Qual

Compounds listed above have Initial Calibration Verification standard recoveries outside 70-130% of the true values. If no compounds are listed, all have passing recoveries.



## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.N**

### Dichlorodifluoromethane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	562	0.627	1.67	
9J24043-CAL4	1	1583	0.682	1.68	
9J24043-CAL5	2	3731	0.842	1.69	
9J24043-CAL6	5	9010	0.812	1.68	
9J24043-CAL7	10	18118	0.770	1.68	
9J24043-CAL8	20	35982	0.800	1.67	
9J24043-CAL9	50	109425	0.946	1.68	
9J24043-CALA	100	212153	0.947	1.68	
9J24043-CALB	200	431143	0.929	1.69	
<b>AVE RF</b>	<b>0.817</b>	<b>RF RSD</b>	<b>13.92</b>	<b>AVE RT</b>	<b>1.68</b>

### Chloromethane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	479	2.063	4.90	
9J24043-CAL2	0.2	669	1.457	1.90	
9J24043-CAL3	0.4	1136	1.268	1.89	
9J24043-CAL4	1	2407	1.037	1.89	
9J24043-CAL5	2	4743	1.070	1.90	
9J24043-CAL6	5	11370	1.024	1.89	
9J24043-CAL7	10	22449	0.954	1.90	
9J24043-CAL8	20	45062	1.002	1.89	
9J24043-CAL9	50	118956	1.029	1.89	
9J24043-CALA	100	226754	1.012	1.90	
9J24043-CALB	200	456703	0.984	1.90	
<b>AVE RF</b>	<b>1.084</b>	<b>RF RSD</b>	<b>14.45</b>	<b>AVE RT</b>	<b>1.90</b>

### Vinyl chloride


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	406	0.884	2.01	
9J24043-CAL3	0.4	967	1.079	2.00	
9J24043-CAL4	1	2351	1.013	2.00	
9J24043-CAL5	2	5030	1.135	2.01	
9J24043-CAL6	5	12653	1.140	2.00	
9J24043-CAL7	10	25149	1.069	2.00	
9J24043-CAL8	20	49916	1.110	2.00	
9J24043-CAL9	50	133008	1.150	2.00	
9J24043-CALA	100	258510	1.154	2.00	
9J24043-CALB	200	521368	1.123	2.00	
<b>AVE RF</b>	<b>1.086</b>	<b>RF RSD</b>	<b>7.67</b>	<b>AVE RT</b>	<b>2.00</b>

### Methylene chloride

Curve Fit: **QUADRATIC: Weighting: (1/a), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	2024	8.716	0.00	
9J24043-CAL2	0.2	2201	4.794	0.00	
9J24043-CAL3	0.4	2646	2.954	0.00	
9J24043-CAL4	1	3939	1.697	0.00	
9J24043-CAL5	2	6151	1.388	0.00	
9J24043-CAL6	5	12549	1.130	3.87	
9J24043-CAL7	10	22701	0.965	3.87	
9J24043-CAL8	20	43598	0.970	3.87	
9J24043-CAL9	50	102541	0.887	3.87	
9J24043-CALA	100	209114	0.934	3.88	
9J24043-CALB	200	419637	0.904	3.88	
<b>AVE RF</b>	<b>2.304</b>	<b>RF RSD</b>	<b>106.11</b>	<b>AVE RT</b>	<b>2.11</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Bromomethane


Curve Fit: **AVERAGE RF**



				<u>Response</u>	
	<u>Standard Concentration</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	839	0.937	2.36	
9J24043-CAL4	1	1763	0.760	2.36	
9J24043-CAL5	2	3140	0.709	2.37	
9J24043-CAL6	5	7782	0.701	2.36	
9J24043-CAL7	10	14678	0.624	2.36	
9J24043-CAL8	20	27599	0.614	2.35	
9J24043-CAL9	50	66917	0.579	2.36	
9J24043-CALA	100	125242	0.559	2.37	
9J24043-CALB	200	267468	0.576	2.37	
<b>AVE RF</b>	<b>0.640</b>	<b>RF RSD</b>	<b>11.51</b>	<b>AVE RT</b>	<b>2.36</b>

### Chloroethane


Curve Fit: **AVERAGE RF**



				<u>Response</u>	
	<u>Standard Concentration</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	0	0.000	0.00	
9J24043-CAL5	2	2540	0.573	2.52	
9J24043-CAL6	5	5899	0.531	2.51	
9J24043-CAL7	10	11813	0.502	2.50	
9J24043-CAL8	20	19851	0.442	2.49	
9J24043-CAL9	50	51695	0.447	2.49	
9J24043-CALA	100	53786	0.240	2.51	
9J24043-CALB	200	53331	0.115	2.49	
<b>AVE RF</b>	<b>0.499</b>	<b>RF RSD</b>	<b>11.23</b>	<b>AVE RT</b>	<b>2.50</b>

### Trichlorofluoromethane


Curve Fit: **AVERAGE RF**



				<u>Response</u>	
	<u>Standard Concentration</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	958	1.069	2.66	
9J24043-CAL4	1	2784	1.200	2.66	
9J24043-CAL5	2	5667	1.279	2.68	
9J24043-CAL6	5	14236	1.282	2.66	
9J24043-CAL7	10	29038	1.235	2.66	
9J24043-CAL8	20	58162	1.294	2.66	
9J24043-CAL9	50	145579	1.259	2.66	
9J24043-CALA	100	279991	1.250	2.66	
9J24043-CALB	200	556445	1.199	2.66	
<b>AVE RF</b>	<b>1.230</b>	<b>RF RSD</b>	<b>5.62</b>	<b>AVE RT</b>	<b>2.66</b>

### 1,1-Dichloroethene

Curve Fit: **AVERAGE RF**



				<u>Response</u>	
	<u>Standard Concentration</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	1038	1.159	3.23	
9J24043-CAL4	1	2476	1.067	3.23	
9J24043-CAL5	2	5263	1.188	3.24	
9J24043-CAL6	5	13321	1.200	3.23	
9J24043-CAL7	10	27243	1.158	3.23	
9J24043-CAL8	20	54074	1.203	3.23	
9J24043-CAL9	50	137847	1.192	3.23	
9J24043-CALA	100	286478	1.279	3.24	
9J24043-CALB	200	567371	1.222	3.23	
<b>AVE RF</b>	<b>1.185</b>	<b>RF RSD</b>	<b>4.83</b>	<b>AVE RT</b>	<b>3.23</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Carbon disulfide


Curve Fit: **AVERAGE RF**



		Response			
Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	4573	1.970	3.25	
9J24043-CAL5	2	9757	2.202	3.26	
9J24043-CAL6	5	24060	2.167	3.25	
9J24043-CAL7	10	49011	2.084	3.25	
9J24043-CAL8	20	98898	2.200	3.24	
9J24043-CAL9	50	254448	2.200	3.25	
9J24043-CALA	100	531736	2.374	3.25	
9J24043-CALB	200	1067583	2.300	3.25	
<b>AVE RF</b>	<b>2.187</b>	<b>RF RSD</b>	<b>5.64</b>	<b>AVE RT</b>	<b>3.25</b>

### 1,1,2-Trichloro-1,2,2-trifluoroethane


Curve Fit: **AVERAGE RF**



		Response			
Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	1717	0.740	3.29	
9J24043-CAL5	2	3803	0.858	3.30	
9J24043-CAL6	5	9544	0.860	3.29	
9J24043-CAL7	10	19612	0.834	3.28	
9J24043-CAL8	20	39711	0.883	3.28	
9J24043-CAL9	50	97812	0.846	3.29	
9J24043-CALA	100	204168	0.912	3.29	
9J24043-CALB	200	411156	0.886	3.29	
<b>AVE RF</b>	<b>0.852</b>	<b>RF RSD</b>	<b>6.07</b>	<b>AVE RT</b>	<b>3.29</b>

### Acetone


Curve Fit: **AVERAGE RF**



		Response			
Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.2	0	0.000	0.00	
9J24043-CAL2	0.4	4468	1.272	3.95	
9J24043-CAL3	0.8	4646	0.902	3.95	
9J24043-CAL4	2	2840	0.633	3.95	
9J24043-CAL5	4	4523	0.510	3.95	
9J24043-CAL6	10	10355	0.466	3.94	
9J24043-CAL7	20	19796	0.421	3.94	
9J24043-CAL8	40	39380	0.438	3.94	
9J24043-CAL9	100	93945	0.406	3.94	
9J24043-CALA	200	188786	0.421	3.94	
9J24043-CALB	400	375022	0.404	3.94	
<b>AVE RF</b>	<b>0.438</b>	<b>RF RSD</b>	<b>8.73</b>	<b>AVE RT</b>	<b>3.94</b>

### trans-1,2-Dichloroethene

Curve Fit: **AVERAGE RF**



		Response			
Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	360	0.784	4.05	
9J24043-CAL3	0.4	963	1.075	4.04	
9J24043-CAL4	1	2657	1.145	4.04	
9J24043-CAL5	2	5503	1.242	4.05	
9J24043-CAL6	5	13685	1.233	4.04	
9J24043-CAL7	10	27372	1.164	4.04	
9J24043-CAL8	20	56066	1.247	4.03	
9J24043-CAL9	50	137318	1.188	4.04	
9J24043-CALA	100	285846	1.276	4.04	
9J24043-CALB	200	579277	1.248	4.04	
<b>AVE RF</b>	<b>1.160</b>	<b>RF RSD</b>	<b>12.54</b>	<b>AVE RT</b>	<b>4.04</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.N**

### n-Hexane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	357	0.154	4.12	
9J24043-CAL5	2	709	0.160	4.13	
9J24043-CAL6	5	1836	0.165	4.12	
9J24043-CAL7	10	4034	0.172	4.12	
9J24043-CAL8	20	8308	0.185	4.12	
9J24043-CAL9	50	21163	0.183	4.12	
9J24043-CALA	100	43920	0.196	4.12	
9J24043-CALB	200	92077	0.198	4.12	
<b>AVE RF</b>	<b>0.177</b>	<b>RF RSD</b>	<b>9.35</b>	<b>AVE RT</b>	<b>4.12</b>

### Methyl tert-butyl ether (MTBE)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	2309	2.577	4.17	
9J24043-CAL4	1	5789	2.494	4.17	
9J24043-CAL5	2	11957	2.698	4.17	
9J24043-CAL6	5	29908	2.694	4.17	
9J24043-CAL7	10	61557	2.617	4.17	
9J24043-CAL8	20	123669	2.750	4.17	
9J24043-CAL9	50	313020	2.707	4.17	
9J24043-CALA	100	646936	2.888	4.17	
9J24043-CALB	200	1318751	2.841	4.17	
<b>AVE RF</b>	<b>2.696</b>	<b>RF RSD</b>	<b>4.58</b>	<b>AVE RT</b>	<b>4.17</b>

### 1,1-Dichloroethane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	1323	1.477	4.68	
9J24043-CAL4	1	3672	1.582	4.68	
9J24043-CAL5	2	7227	1.631	4.69	
9J24043-CAL6	5	18307	1.649	4.68	
9J24043-CAL7	10	36999	1.573	4.68	
9J24043-CAL8	20	75120	1.671	4.68	
9J24043-CAL9	50	182910	1.582	4.68	
9J24043-CALA	100	379907	1.696	4.68	
9J24043-CALB	200	761535	1.641	4.68	
<b>AVE RF</b>	<b>1.611</b>	<b>RF RSD</b>	<b>4.09</b>	<b>AVE RT</b>	<b>4.68</b>

### Acrylonitrile

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	876	0.377	4.75	
9J24043-CAL5	2	1949	0.440	4.76	
9J24043-CAL6	5	5426	0.489	4.75	
9J24043-CAL7	10	11383	0.484	4.74	
9J24043-CAL8	20	22973	0.511	4.75	
9J24043-CAL9	50	58667	0.507	4.75	
9J24043-CALA	100	122564	0.547	4.75	
9J24043-CALB	200	243406	0.524	4.75	
<b>AVE RF</b>	<b>0.485</b>	<b>RF RSD</b>	<b>11.08</b>	<b>AVE RT</b>	<b>4.75</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### cis-1,2-Dichloroethene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	1008	1.125	5.24	
9J24043-CAL4	1	2744	1.182	5.24	
9J24043-CAL5	2	5568	1.256	5.25	
9J24043-CAL6	5	13959	1.257	5.24	
9J24043-CAL7	10	28723	1.221	5.24	
9J24043-CAL8	20	58359	1.298	5.24	
9J24043-CAL9	50	143124	1.238	5.24	
9J24043-CALA	100	297452	1.328	5.24	
9J24043-CALB	200	597836	1.288	5.24	
<b>AVE RF</b>	<b>1.244</b>	<b>RF RSD</b>	<b>4.98</b>	<b>AVE RT</b>	<b>5.24</b>

### 2,2-Dichloropropane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	853	0.952	5.35	
9J24043-CAL4	1	2316	0.998	5.35	
9J24043-CAL5	2	4776	1.078	5.35	
9J24043-CAL6	5	11793	1.062	5.35	
9J24043-CAL7	10	23663	1.006	5.35	
9J24043-CAL8	20	48254	1.073	5.35	
9J24043-CAL9	50	122658	1.061	5.35	
9J24043-CALA	100	252830	1.129	5.35	
9J24043-CALB	200	512393	1.104	5.35	
<b>AVE RF</b>	<b>1.051</b>	<b>RF RSD</b>	<b>5.31</b>	<b>AVE RT</b>	<b>5.35</b>

### Bromochloromethane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	391	0.436	5.44	
9J24043-CAL4	1	1188	0.512	5.45	
9J24043-CAL5	2	2679	0.605	5.46	
9J24043-CAL6	5	7172	0.646	5.44	
9J24043-CAL7	10	14961	0.636	5.45	
9J24043-CAL8	20	30935	0.688	5.44	
9J24043-CAL9	50	77572	0.671	5.44	
9J24043-CALA	100	151653	0.677	5.45	
9J24043-CALB	200	288672	0.622	5.45	
<b>AVE RF</b>	<b>0.610</b>	<b>RF RSD</b>	<b>13.73</b>	<b>AVE RT</b>	<b>5.45</b>

### Chloroform

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	587	1.278	5.53	
9J24043-CAL3	0.4	1292	1.442	5.53	
9J24043-CAL4	1	3341	1.440	5.53	
9J24043-CAL5	2	7277	1.642	5.54	
9J24043-CAL6	5	18186	1.638	5.53	
9J24043-CAL7	10	37799	1.607	5.53	
9J24043-CAL8	20	76239	1.696	5.52	
9J24043-CAL9	50	186984	1.617	5.52	
9J24043-CALA	100	385051	1.719	5.53	
9J24043-CALB	200	776466	1.673	5.53	
<b>AVE RF</b>	<b>1.575</b>	<b>RF RSD</b>	<b>8.98</b>	<b>AVE RT</b>	<b>5.53</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.N**

### Carbon tetrachloride


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	618	0.690	5.66	
9J24043-CAL4	1	1791	0.772	5.66	
9J24043-CAL5	2	4001	0.903	5.66	
9J24043-CAL6	5	9957	0.897	5.66	
9J24043-CAL7	10	20840	0.886	5.66	
9J24043-CAL8	20	43938	0.977	5.66	
9J24043-CAL9	50	114614	0.991	5.66	
9J24043-CALA	100	247648	1.106	5.66	
9J24043-CALB	200	525973	1.133	5.66	
<b>AVE RF</b>	<b>0.958</b>	<b>RF RSD</b>	<b>12.52</b>	<b>AVE RT</b>	<b>5.66</b>

### Tetrahydrofuran


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	945	0.407	5.71	
9J24043-CAL5	2	2045	0.461	5.71	
9J24043-CAL6	5	5112	0.460	5.71	
9J24043-CAL7	10	10375	0.441	5.70	
9J24043-CAL8	20	21330	0.474	5.70	
9J24043-CAL9	50	54072	0.468	5.69	
9J24043-CALA	100	111881	0.500	5.70	
9J24043-CALB	200	221252	0.477	5.69	
<b>AVE RF</b>	<b>0.461</b>	<b>RF RSD</b>	<b>5.94</b>	<b>AVE RT</b>	<b>5.70</b>

### 1,1,1-Trichloroethane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	1012	1.130	5.73	
9J24043-CAL4	1	2903	1.251	5.73	
9J24043-CAL5	2	5937	1.340	5.74	
9J24043-CAL6	5	14957	1.347	5.73	
9J24043-CAL7	10	30210	1.284	5.74	
9J24043-CAL8	20	62000	1.379	5.73	
9J24043-CAL9	50	156566	1.354	5.73	
9J24043-CALA	100	325398	1.453	5.74	
9J24043-CALB	200	663507	1.430	5.74	
<b>AVE RF</b>	<b>1.330</b>	<b>RF RSD</b>	<b>7.37</b>	<b>AVE RT</b>	<b>5.73</b>

### 2-Butanone (MEK)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.2	0	0.000	0.00	
9J24043-CAL2	0.4	0	0.000	0.00	
9J24043-CAL3	0.8	0	0.000	0.00	
9J24043-CAL4	2	2900	0.625	5.86	
9J24043-CAL5	4	6243	0.704	5.87	
9J24043-CAL6	10	15638	0.704	5.86	
9J24043-CAL7	20	31158	0.662	5.86	
9J24043-CAL8	40	64474	0.717	5.85	
9J24043-CAL9	100	162223	0.701	5.85	
9J24043-CALA	200	331914	0.741	5.85	
9J24043-CALB	400	651518	0.702	5.85	
<b>AVE RF</b>	<b>0.695</b>	<b>RF RSD</b>	<b>5.12</b>	<b>AVE RT</b>	<b>5.86</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### 1,1-Dichloropropene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	1049	1.171	5.87	
9J24043-CAL4	1	2749	1.184	5.86	
9J24043-CAL5	2	5724	1.292	5.87	
9J24043-CAL6	5	14423	1.299	5.86	
9J24043-CAL7	10	29295	1.245	5.86	
9J24043-CAL8	20	59019	1.313	5.86	
9J24043-CAL9	50	146998	1.271	5.86	
9J24043-CALA	100	308104	1.376	5.86	
9J24043-CALB	200	622283	1.341	5.86	
<b>AVE RF</b>	<b>1.277</b>	<b>RF RSD</b>	<b>5.30</b>	<b>AVE RT</b>	<b>5.86</b>

### Benzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	917	3.949	6.13	
9J24043-CAL2	0.2	1584	3.450	6.13	
9J24043-CAL3	0.4	3381	3.774	6.12	
9J24043-CAL4	1	8314	3.582	6.13	
9J24043-CAL5	2	17935	4.047	6.13	
9J24043-CAL6	5	43404	3.910	6.12	
9J24043-CAL7	10	87359	3.714	6.12	
9J24043-CAL8	20	175817	3.910	6.12	
9J24043-CAL9	50	434612	3.758	6.12	
9J24043-CALA	100	900809	4.022	6.12	
9J24043-CALB	200	1815119	3.911	6.12	
<b>AVE RF</b>	<b>3.821</b>	<b>RF RSD</b>	<b>4.86</b>	<b>AVE RT</b>	<b>6.12</b>

### Pentafluorobenzene (ISTD)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	116102	2322.040	6.22	
9J24043-CAL2	50	114788	2295.760	6.22	
9J24043-CAL3	50	111985	2239.700	6.21	
9J24043-CAL4	50	116043	2320.860	6.21	
9J24043-CAL5	50	110790	2215.800	6.22	
9J24043-CAL6	50	111010	2220.200	6.21	
9J24043-CAL7	50	117608	2352.160	6.22	
9J24043-CAL8	50	112406	2248.120	6.21	
9J24043-CAL9	50	115635	2312.700	6.21	
9J24043-CALA	50	111989	2239.780	6.22	
9J24043-CALB	50	116034	2320.680	6.22	
<b>AVE RF</b>	<b>2280.709</b>	<b>RF RSD</b>	<b>2.13</b>	<b>AVE RT</b>	<b>6.21</b>

### 1,2-Dichloroethane (EDC)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	1073	1.198	6.33	
9J24043-CAL4	1	2623	1.130	6.34	
9J24043-CAL5	2	5726	1.292	6.35	
9J24043-CAL6	5	14359	1.293	6.34	
9J24043-CAL7	10	28935	1.230	6.34	
9J24043-CAL8	20	58731	1.306	6.34	
9J24043-CAL9	50	143950	1.245	6.34	
9J24043-CALA	100	294149	1.313	6.34	
9J24043-CALB	200	583025	1.256	6.34	
<b>AVE RF</b>	<b>1.252</b>	<b>RF RSD</b>	<b>4.76</b>	<b>AVE RT</b>	<b>6.34</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Isobutyl alcohol


Curve Fit: **AVERAGE RF**



				<u>Response</u>	
<u>Standard</u>	<u>Concentration</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>	
9J24043-CAL1	2.5	0	0.000	0.00	
9J24043-CAL2	5	0	0.000	0.00	
9J24043-CAL3	10	1172	5.233	6.39	
9J24043-CAL4	25	3120	5.377	6.38	
9J24043-CAL5	50	7968	7.192	6.38	
9J24043-CAL6	125	20710	7.462	6.38	
9J24043-CAL7	250	39286	6.681	6.38	
9J24043-CAL8	500	83527	7.431	6.37	
9J24043-CAL9	1250	224878	0.078	6.37	
9J24043-CALA	2500	450055	8.037	6.38	
9J24043-CALB	5000	863259	7.440	6.38	
<b>AVE RF</b>	<b>6.959</b>	<b>RF RSD</b>	<b>14.51</b>	<b>AVE RT</b>	<b>6.38</b>

### Trichloroethene (TCE)


Curve Fit: **AVERAGE RF**



				<u>Response</u>	
<u>Standard</u>	<u>Concentration</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	372	0.810	6.75	
9J24043-CAL3	0.4	718	0.801	6.75	
9J24043-CAL4	1	2166	0.933	6.74	
9J24043-CAL5	2	4576	1.033	6.75	
9J24043-CAL6	5	11340	1.022	6.74	
9J24043-CAL7	10	23449	0.997	6.74	
9J24043-CAL8	20	47359	1.053	6.74	
9J24043-CAL9	50	118626	1.026	6.74	
9J24043-CALA	100	245311	1.095	6.75	
9J24043-CALB	200	498651	1.074	6.74	
<b>AVE RF</b>	<b>0.984</b>	<b>RF RSD</b>	<b>10.55</b>	<b>AVE RT</b>	<b>6.74</b>

### 1,4-Difluorobenzene (Surr)


Curve Fit: **AVERAGE RF**



				<u>Response</u>	
<u>Standard</u>	<u>Concentration</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>	
9J24043-CAL1	50	364447	3.139	6.78	
9J24043-CAL2	50	359462	3.132	6.78	
9J24043-CAL3	50	352302	3.146	6.78	
9J24043-CAL4	50	366642	3.160	6.78	
9J24043-CAL5	50	347212	3.134	6.78	
9J24043-CAL6	50	353918	3.188	6.78	
9J24043-CAL7	50	367409	3.124	6.78	
9J24043-CAL8	50	354922	3.158	6.78	
9J24043-CAL9	50	370144	3.201	6.78	
9J24043-CALA	50	356857	3.187	6.78	
9J24043-CALB	50	369003	3.180	6.78	
<b>AVE RF</b>	<b>3.159</b>	<b>RF RSD</b>	<b>0.84</b>	<b>AVE RT</b>	<b>6.78</b>

### Dibromomethane

Curve Fit: **AVERAGE RF**



				<u>Response</u>	
<u>Standard</u>	<u>Concentration</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	378	0.422	7.20	
9J24043-CAL4	1	1285	0.554	7.20	
9J24043-CAL5	2	2755	0.622	7.20	
9J24043-CAL6	5	7023	0.633	7.20	
9J24043-CAL7	10	14594	0.620	7.20	
9J24043-CAL8	20	29514	0.656	7.20	
9J24043-CAL9	50	74270	0.642	7.20	
9J24043-CALA	100	155032	0.692	7.20	
9J24043-CALB	200	314382	0.677	7.20	
<b>AVE RF</b>	<b>0.613</b>	<b>RF RSD</b>	<b>13.36</b>	<b>AVE RT</b>	<b>7.20</b>



## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### 1,2-Dichloropropane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	797	0.890	7.31	
9J24043-CAL4	1	1944	0.838	7.31	
9J24043-CAL5	2	4373	0.987	7.31	
9J24043-CAL6	5	10897	0.982	7.31	
9J24043-CAL7	10	21915	0.932	7.31	
9J24043-CAL8	20	44422	0.988	7.31	
9J24043-CAL9	50	109124	0.944	7.31	
9J24043-CALA	100	229327	1.024	7.31	
9J24043-CALB	200	461364	0.994	7.31	
<b>AVE RF</b>	<b>0.953</b>	<b>RF RSD</b>	<b>6.18</b>	<b>AVE RT</b>	<b>7.31</b>

### Bromodichloromethane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	800	0.893	7.38	
9J24043-CAL4	1	2259	0.973	7.38	
9J24043-CAL5	2	4681	1.056	7.39	
9J24043-CAL6	5	12021	1.083	7.38	
9J24043-CAL7	10	25055	1.065	7.38	
9J24043-CAL8	20	51693	1.150	7.38	
9J24043-CAL9	50	133532	1.155	7.38	
9J24043-CALA	100	282119	1.260	7.38	
9J24043-CALB	200	582259	1.255	7.38	
<b>AVE RF</b>	<b>1.099</b>	<b>RF RSD</b>	<b>11.01</b>	<b>AVE RT</b>	<b>7.38</b>

### cis-1,3-Dichloropropene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	1014	0.431	8.09	
9J24043-CAL4	1	2667	0.429	8.09	
9J24043-CAL5	2	5578	0.468	8.09	
9J24043-CAL6	5	14229	0.474	8.09	
9J24043-CAL7	10	30482	0.487	8.09	
9J24043-CAL8	20	64475	0.525	8.09	
9J24043-CAL9	50	166893	0.520	8.09	
9J24043-CALA	100	356393	0.559	8.09	
9J24043-CALB	200	736312	0.556	8.09	
<b>AVE RF</b>	<b>0.494</b>	<b>RF RSD</b>	<b>9.88</b>	<b>AVE RT</b>	<b>8.09</b>

### Toluene-d8 (Surr)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	406288	1.321	8.30	
9J24043-CAL2	50	403793	1.333	8.30	
9J24043-CAL3	50	396027	1.345	8.30	
9J24043-CAL4	50	410518	1.321	8.30	
9J24043-CAL5	50	395017	1.327	8.30	
9J24043-CAL6	50	397005	1.322	8.30	
9J24043-CAL7	50	415174	1.327	8.30	
9J24043-CAL8	50	399810	1.302	8.30	
9J24043-CAL9	50	415062	1.292	8.30	
9J24043-CALA	50	405945	1.274	8.30	
9J24043-CALB	50	420947	1.272	8.30	
<b>AVE RF</b>	<b>1.312</b>	<b>RF RSD</b>	<b>1.83</b>	<b>AVE RT</b>	<b>8.30</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Toluene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	978	1.590	8.36	
9J24043-CAL2	0.2	1744	1.439	8.35	
9J24043-CAL3	0.4	3505	1.488	8.36	
9J24043-CAL4	1	9040	1.454	8.35	
9J24043-CAL5	2	17851	1.499	8.36	
9J24043-CAL6	5	44272	1.474	8.36	
9J24043-CAL7	10	90400	1.445	8.36	
9J24043-CAL8	20	183309	1.492	8.36	
9J24043-CAL9	50	446611	1.391	8.36	
9J24043-CALA	100	931584	1.462	8.36	
9J24043-CALB	200	1905088	1.439	8.36	
<b>AVE RF</b>	<b>1.470</b>	<b>RF RSD</b>	<b>3.41</b>	<b>AVE RT</b>	<b>8.36</b>

### Tetrachloroethene (PCE)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	267	0.220	8.81	
9J24043-CAL3	0.4	787	0.334	8.80	
9J24043-CAL4	1	1994	0.321	8.80	
9J24043-CAL5	2	4333	0.364	8.80	
9J24043-CAL6	5	10847	0.361	8.80	
9J24043-CAL7	10	22099	0.353	8.80	
9J24043-CAL8	20	45467	0.370	8.80	
9J24043-CAL9	50	113079	0.352	8.80	
9J24043-CALA	100	236880	0.372	8.80	
9J24043-CALB	200	496433	0.375	8.80	
<b>AVE RF</b>	<b>0.342</b>	<b>RF RSD</b>	<b>13.48</b>	<b>AVE RT</b>	<b>8.80</b>

### 4-Methyl-2-pentanone (MiBK)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.2	0	0.000	0.00	
9J24043-CAL2	0.4	890	0.367	8.80	
9J24043-CAL3	0.8	1912	0.406	8.81	
9J24043-CAL4	2	5042	0.406	8.80	
9J24043-CAL5	4	11029	0.463	8.81	
9J24043-CAL6	10	28183	0.469	8.80	
9J24043-CAL7	20	58009	0.464	8.80	
9J24043-CAL8	40	120524	0.491	8.80	
9J24043-CAL9	100	304356	0.474	8.80	
9J24043-CALA	200	616767	0.484	8.80	
9J24043-CALB	400	1166981	0.441	8.80	
<b>AVE RF</b>	<b>0.446</b>	<b>RF RSD</b>	<b>9.09</b>	<b>AVE RT</b>	<b>8.80</b>

### trans-1,3-Dichloropropene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	610	0.259	8.84	
9J24043-CAL4	1	2122	0.341	8.84	
9J24043-CAL5	2	4500	0.378	8.84	
9J24043-CAL6	5	12130	0.404	8.84	
9J24043-CAL7	10	26302	0.420	8.84	
9J24043-CAL8	20	57085	0.465	8.83	
9J24043-CAL9	50	151987	0.473	8.83	
9J24043-CALA	100	327146	0.513	8.84	
9J24043-CALB	200	678927	0.513	8.84	
<b>AVE RF</b>	<b>0.438</b>	<b>RF RSD</b>	<b>14.34</b>	<b>AVE RT</b>	<b>8.84</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### 1,1,2-Trichloroethane


Curve Fit: **AVERAGE RF**



		Response			
Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	9.00	
9J24043-CAL2	0.2	288	0.238	9.01	
9J24043-CAL3	0.4	717	0.304	9.00	
9J24043-CAL4	1	1944	0.313	9.00	
9J24043-CAL5	2	4134	0.347	9.00	
9J24043-CAL6	5	10336	0.344	9.00	
9J24043-CAL7	10	21402	0.342	9.01	
9J24043-CAL8	20	43171	0.351	9.00	
9J24043-CAL9	50	107594	0.335	9.00	
9J24043-CALA	100	221018	0.347	9.01	
9J24043-CALB	200	447395	0.338	9.01	
<b>AVE RF</b>	<b>0.326</b>	<b>RF RSD</b>	<b>10.62</b>	<b>AVE RT</b>	<b>9.01</b>

### Dibromochloromethane


Curve Fit: **AVERAGE RF**



		Response			
Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	9.00	
9J24043-CAL2	0.2	0	0.000	9.00	
9J24043-CAL3	0.4	505	0.214	9.19	
9J24043-CAL4	1	1349	0.217	9.19	
9J24043-CAL5	2	3038	0.255	9.19	
9J24043-CAL6	5	8016	0.267	9.19	
9J24043-CAL7	10	17208	0.275	9.19	
9J24043-CAL8	20	36932	0.301	9.19	
9J24043-CAL9	50	101291	0.315	9.19	
9J24043-CALA	100	222919	0.350	9.19	
9J24043-CALB	200	473598	0.358	9.19	
<b>AVE RF</b>	<b>0.264</b>	<b>RF RSD</b>	<b>14.58</b>	<b>AVE RT</b>	<b>9.19</b>

### 1,3-Dichloropropane


Curve Fit: **AVERAGE RF**



		Response			
Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	9.00	
9J24043-CAL2	0.2	568	0.469	9.29	
9J24043-CAL3	0.4	1253	0.532	9.29	
9J24043-CAL4	1	3361	0.541	9.29	
9J24043-CAL5	2	6889	0.578	9.29	
9J24043-CAL6	5	17551	0.584	9.29	
9J24043-CAL7	10	36354	0.581	9.29	
9J24043-CAL8	20	73700	0.600	9.29	
9J24043-CAL9	50	183541	0.571	9.29	
9J24043-CALA	100	379039	0.595	9.29	
9J24043-CALB	200	755862	0.571	9.29	
<b>AVE RF</b>	<b>0.562</b>	<b>RF RSD</b>	<b>6.98</b>	<b>AVE RT</b>	<b>9.29</b>

### 1,2-Dibromoethane (EDB)

Curve Fit: **AVERAGE RF**



		Response			
Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	9.00	
9J24043-CAL2	0.2	279	0.230	9.42	
9J24043-CAL3	0.4	615	0.261	9.42	
9J24043-CAL4	1	1928	0.310	9.42	
9J24043-CAL5	2	4499	0.378	9.43	
9J24043-CAL6	5	11270	0.375	9.42	
9J24043-CAL7	10	22884	0.366	9.42	
9J24043-CAL8	20	46797	0.381	9.42	
9J24043-CAL9	50	117418	0.366	9.42	
9J24043-CALA	100	243688	0.382	9.42	
9J24043-CALB	200	496207	0.375	9.42	
<b>AVE RF</b>	<b>0.355</b>	<b>RF RSD</b>	<b>11.70</b>	<b>AVE RT</b>	<b>9.42</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.N**

### 2-Hexanone


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.2	0	0.000	0.00	
9J24043-CAL2	0.4	0	0.000	0.00	
9J24043-CAL3	0.8	1346	0.286	9.66	
9J24043-CAL4	2	3526	0.284	9.66	
9J24043-CAL5	4	7610	0.319	9.66	
9J24043-CAL6	10	19724	0.328	9.65	
9J24043-CAL7	20	41881	0.335	9.65	
9J24043-CAL8	40	87528	0.356	9.65	
9J24043-CAL9	100	224495	0.350	9.65	
9J24043-CALA	200	456833	0.358	9.65	
9J24043-CALB	400	866990	0.327	9.65	
<b>AVE RF</b>	<b>0.327</b>	<b>RF RSD</b>	<b>8.41</b>	<b>AVE RT</b>	<b>9.66</b>

### Chlorobenzene-d5 (ISTD)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	307577	6151.540	9.91	
9J24043-CAL2	50	302974	6059.480	9.92	
9J24043-CAL3	50	294372	5887.440	9.91	
9J24043-CAL4	50	310797	6215.940	9.91	
9J24043-CAL5	50	297754	5955.080	9.92	
9J24043-CAL6	50	300317	6006.340	9.91	
9J24043-CAL7	50	312833	6256.660	9.91	
9J24043-CAL8	50	307093	6141.860	9.91	
9J24043-CAL9	50	321159	6423.180	9.91	
9J24043-CALA	50	318635	6372.700	9.91	
9J24043-CALB	50	330915	6618.300	9.92	
<b>AVE RF</b>	<b>6189.865</b>	<b>RF RSD</b>	<b>3.53</b>	<b>AVE RT</b>	<b>9.91</b>

### Chlorobenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	480	0.780	9.93	
9J24043-CAL2	0.2	1045	0.862	9.93	
9J24043-CAL3	0.4	2226	0.945	9.93	
9J24043-CAL4	1	5770	0.928	9.93	
9J24043-CAL5	2	11701	0.982	9.93	
9J24043-CAL6	5	29555	0.984	9.93	
9J24043-CAL7	10	60359	0.965	9.93	
9J24043-CAL8	20	120984	0.985	9.93	
9J24043-CAL9	50	301806	0.940	9.93	
9J24043-CALA	100	624905	0.981	9.93	
9J24043-CALB	200	1285529	0.971	9.93	
<b>AVE RF</b>	<b>0.939</b>	<b>RF RSD</b>	<b>6.80</b>	<b>AVE RT</b>	<b>9.93</b>

### Ethylbenzene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	942	1.531	9.95	
9J24043-CAL2	0.2	1835	1.514	9.95	
9J24043-CAL3	0.4	3584	1.522	9.95	
9J24043-CAL4	1	8761	1.409	9.95	
9J24043-CAL5	2	19157	1.608	9.95	
9J24043-CAL6	5	46860	1.560	9.95	
9J24043-CAL7	10	96018	1.535	9.95	
9J24043-CAL8	20	195460	1.591	9.95	
9J24043-CAL9	50	486890	1.516	9.95	
9J24043-CALA	100	1015747	1.594	9.95	
9J24043-CALB	200	2091382	1.580	9.95	
<b>AVE RF</b>	<b>1.542</b>	<b>RF RSD</b>	<b>3.61</b>	<b>AVE RT</b>	<b>9.95</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### 1,1,1,2-Tetrachloroethane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	129	0.406	0.00	
9J24043-CAL3	0.4	470	0.200	9.99	
9J24043-CAL4	1	1476	0.237	9.99	
9J24043-CAL5	2	2985	0.251	9.99	
9J24043-CAL6	5	7981	0.266	9.99	
9J24043-CAL7	10	16995	0.272	9.99	
9J24043-CAL8	20	36336	0.296	9.99	
9J24043-CAL9	50	95075	0.296	9.99	
9J24043-CALA	100	206263	0.324	9.99	
9J24043-CALB	200	427244	0.323	9.99	
<b>AVE RF</b>	<b>0.274</b>	<b>RF RSD</b>	<b>14.90</b>	<b>AVE RT</b>	<b>9.99</b>

### Bromobenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	124	0.444	0.00	
9J24043-CAL2	0.2	432	0.800	11.06	
9J24043-CAL3	0.4	875	0.813	11.06	
9J24043-CAL4	1	2220	0.771	11.06	
9J24043-CAL5	2	4634	0.830	11.06	
9J24043-CAL6	5	11623	0.819	11.06	
9J24043-CAL7	10	24222	0.812	11.06	
9J24043-CAL8	20	50013	0.825	11.06	
9J24043-CAL9	50	126180	0.798	11.06	
9J24043-CALA	100	265287	0.813	11.06	
9J24043-CALB	200	542011	0.800	11.06	
<b>AVE RF</b>	<b>0.775</b>	<b>RF RSD</b>	<b>14.32</b>	<b>AVE RT</b>	<b>10.05</b>

### m,p-Xylene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.2	1368	1.112	10.09	
9J24043-CAL2	0.4	2470	1.019	10.09	
9J24043-CAL3	0.8	5197	1.103	10.09	
9J24043-CAL4	2	12789	1.029	10.09	
9J24043-CAL5	4	27092	1.137	10.09	
9J24043-CAL6	10	68847	1.146	10.09	
9J24043-CAL7	20	142004	1.135	10.09	
9J24043-CAL8	40	297066	1.209	10.09	
9J24043-CAL9	100	738497	1.150	10.09	
9J24043-CALA	200	1568164	1.230	10.09	
9J24043-CALB	400	3227914	1.219	10.09	
<b>AVE RF</b>	<b>1.135</b>	<b>RF RSD</b>	<b>6.12</b>	<b>AVE RT</b>	<b>10.09</b>

### o-Xylene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	585	0.951	10.47	
9J24043-CAL2	0.2	1221	1.008	10.47	
9J24043-CAL3	0.4	2605	1.106	10.47	
9J24043-CAL4	1	6630	1.067	10.46	
9J24043-CAL5	2	13605	1.142	10.47	
9J24043-CAL6	5	34456	1.147	10.46	
9J24043-CAL7	10	71417	1.141	10.46	
9J24043-CAL8	20	149422	1.216	10.46	
9J24043-CAL9	50	371768	1.158	10.46	
9J24043-CALA	100	785588	1.233	10.46	
9J24043-CALB	200	1606355	1.214	10.46	
<b>AVE RF</b>	<b>1.126</b>	<b>RF RSD</b>	<b>7.83</b>	<b>AVE RT</b>	<b>10.47</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Xylenes, total


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.3	1953	1.058	10.47	
9J24043-CAL2	0.6	3691	1.015	10.47	
9J24043-CAL3	1.2	7802	1.104	10.47	
9J24043-CAL4	3	19419	1.041	10.46	
9J24043-CAL5	6	40697	1.139	10.47	
9J24043-CAL6	15	103303	1.147	10.46	
9J24043-CAL7	30	213421	1.137	10.46	
9J24043-CAL8	60	446488	1.212	10.46	
9J24043-CAL9	150	1110265	1.152	10.46	
9J24043-CALA	300	2353752	1.231	10.46	
9J24043-CALB	600	4834269	1.217	10.46	
<b>AVE RF</b>	<b>1.132</b>	<b>RF RSD</b>	<b>6.38</b>	<b>AVE RT</b>	<b>10.47</b>

### Styrene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	754	0.622	10.52	
9J24043-CAL3	0.4	1656	0.703	10.52	
9J24043-CAL4	1	4878	0.785	10.52	
9J24043-CAL5	2	10363	0.870	10.52	
9J24043-CAL6	5	26739	0.890	10.51	
9J24043-CAL7	10	57022	0.911	10.51	
9J24043-CAL8	20	120205	0.979	10.51	
9J24043-CAL9	50	307044	0.956	10.51	
9J24043-CALA	100	653902	1.026	10.51	
9J24043-CALB	200	1353743	1.023	10.51	
<b>AVE RF</b>	<b>0.905</b>	<b>RF RSD</b>	<b>11.93</b>	<b>AVE RT</b>	<b>10.51</b>

### Bromoform


Curve Fit: **QUADRATIC: Weighting: (1/a), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	795	0.128	10.54	
9J24043-CAL5	2	1771	0.149	10.54	
9J24043-CAL6	5	4690	0.156	10.54	
9J24043-CAL7	10	10701	0.171	10.54	
9J24043-CAL8	20	23844	0.194	10.54	
9J24043-CAL9	50	71080	0.221	10.54	
9J24043-CALA	100	162527	0.255	10.54	
9J24043-CALB	200	361162	0.266	10.54	
<b>AVE RF</b>	<b>0.182</b>	<b>RF RSD</b>	<b>24.41</b>	<b>AVE RT</b>	<b>10.54</b>

### Isopropylbenzene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	1347	1.111	10.74	
9J24043-CAL3	0.4	3067	1.302	10.73	
9J24043-CAL4	1	7662	1.233	10.73	
9J24043-CAL5	2	16325	1.371	10.73	
9J24043-CAL6	5	41801	1.392	10.73	
9J24043-CAL7	10	86673	1.385	10.73	
9J24043-CAL8	20	182751	1.488	10.73	
9J24043-CAL9	50	458349	1.427	10.73	
9J24043-CALA	100	973691	1.528	10.73	
9J24043-CALB	200	1980670	1.496	10.73	
<b>AVE RF</b>	<b>1.373</b>	<b>RF RSD</b>	<b>9.37</b>	<b>AVE RT</b>	<b>10.73</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### 1,4-Dichlorobenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	311	1.113	0.00	
9J24043-CAL2	0.2	725	1.342	11.86	
9J24043-CAL3	0.4	1564	1.454	11.86	
9J24043-CAL4	1	4177	1.451	11.86	
9J24043-CAL5	2	8550	1.531	11.86	
9J24043-CAL6	5	20421	1.440	11.86	
9J24043-CAL7	10	42771	1.433	11.86	
9J24043-CAL8	20	89594	1.478	11.86	
9J24043-CAL9	50	222386	1.406	11.86	
9J24043-CALA	100	468883	1.436	11.86	
9J24043-CALB	200	949679	1.402	11.86	
<b>AVE RF</b>	<b>1.408</b>	<b>RF RSD</b>	<b>7.70</b>	<b>AVE RT</b>	<b>10.78</b>

### n-Butylbenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	379	1.357	0.00	
9J24043-CAL2	0.2	805	1.491	12.05	
9J24043-CAL3	0.4	1867	1.735	12.05	
9J24043-CAL4	1	4997	1.735	12.05	
9J24043-CAL5	2	10626	1.903	12.05	
9J24043-CAL6	5	28526	2.011	12.05	
9J24043-CAL7	10	59515	1.994	12.05	
9J24043-CAL8	20	130970	2.160	12.05	
9J24043-CAL9	50	325681	2.060	12.05	
9J24043-CALA	100	694929	2.129	12.05	
9J24043-CALB	200	1435776	2.119	12.05	
<b>AVE RF</b>	<b>1.881</b>	<b>RF RSD</b>	<b>14.34</b>	<b>AVE RT</b>	<b>10.95</b>

### 4-Bromofluorobenzene (Surr)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	116090	0.831	10.97	
9J24043-CAL2	50	113180	0.838	10.97	
9J24043-CAL3	50	112304	0.835	10.97	
9J24043-CAL4	50	118563	0.823	10.97	
9J24043-CAL5	50	115163	0.825	10.97	
9J24043-CAL6	50	115652	0.815	10.97	
9J24043-CAL7	50	121121	0.812	10.97	
9J24043-CAL8	50	120976	0.798	10.97	
9J24043-CAL9	50	125801	0.796	10.97	
9J24043-CALA	50	124392	0.762	10.97	
9J24043-CALB	50	127221	0.751	10.97	
<b>AVE RF</b>	<b>0.808</b>	<b>RF RSD</b>	<b>3.58</b>	<b>AVE RT</b>	<b>10.97</b>

### n-Propylbenzene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	873	3.125	11.08	
9J24043-CAL2	0.2	1649	3.053	11.08	
9J24043-CAL3	0.4	3544	3.294	11.08	
9J24043-CAL4	1	9160	3.181	11.08	
9J24043-CAL5	2	19292	3.455	11.08	
9J24043-CAL6	5	48000	3.384	11.07	
9J24043-CAL7	10	99009	3.318	11.07	
9J24043-CAL8	20	210703	3.475	11.07	
9J24043-CAL9	50	530991	3.358	11.07	
9J24043-CALA	100	1142995	3.501	11.07	
9J24043-CALB	200	2308779	3.408	11.07	
<b>AVE RF</b>	<b>3.323</b>	<b>RF RSD</b>	<b>4.44</b>	<b>AVE RT</b>	<b>11.07</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.N**

### 1,1,2,2-Tetrachloroethane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	305	0.565	11.14	
9J24043-CAL3	0.4	671	0.624	11.14	
9J24043-CAL4	1	1876	0.651	11.14	
9J24043-CAL5	2	4008	0.718	11.14	
9J24043-CAL6	5	9843	0.694	11.14	
9J24043-CAL7	10	20098	0.673	11.14	
9J24043-CAL8	20	41819	0.690	11.14	
9J24043-CAL9	50	106506	0.674	11.14	
9J24043-CALA	100	212550	0.651	11.14	
9J24043-CALB	200	408430	0.603	11.14	
<b>AVE RF</b>	<b>0.654</b>	<b>RF RSD</b>	<b>7.07</b>	<b>AVE RT</b>	<b>11.14</b>

### 2-Chlorotoluene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	719	0.668	11.21	
9J24043-CAL4	1	1910	0.663	11.21	
9J24043-CAL5	2	4172	0.747	11.21	
9J24043-CAL6	5	10150	0.716	11.21	
9J24043-CAL7	10	21625	0.725	11.21	
9J24043-CAL8	20	45664	0.753	11.21	
9J24043-CAL9	50	113724	0.719	11.21	
9J24043-CALA	100	238214	0.730	11.21	
9J24043-CALB	200	490093	0.723	11.21	
<b>AVE RF</b>	<b>0.716</b>	<b>RF RSD</b>	<b>4.34</b>	<b>AVE RT</b>	<b>11.21</b>

### 1,3,5-Trimethylbenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	556	1.990	11.23	
9J24043-CAL2	0.2	1127	2.087	11.23	
9J24043-CAL3	0.4	2289	2.127	11.23	
9J24043-CAL4	1	6197	2.152	11.23	
9J24043-CAL5	2	13089	2.344	11.23	
9J24043-CAL6	5	33314	2.349	11.23	
9J24043-CAL7	10	69892	2.342	11.23	
9J24043-CAL8	20	148694	2.452	11.23	
9J24043-CAL9	50	370702	2.344	11.23	
9J24043-CALA	100	783721	2.400	11.23	
9J24043-CALB	200	1618836	2.390	11.23	
<b>AVE RF</b>	<b>2.271</b>	<b>RF RSD</b>	<b>6.72</b>	<b>AVE RT</b>	<b>11.23</b>

### 1,2,3-Trichloropropane

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	271	0.252	11.25	
9J24043-CAL4	1	887	0.308	11.25	
9J24043-CAL5	2	1935	0.347	11.25	
9J24043-CAL6	5	4862	0.343	11.25	
9J24043-CAL7	10	10162	0.341	11.25	
9J24043-CAL8	20	20199	0.333	11.25	
9J24043-CAL9	50	51746	0.327	11.25	
9J24043-CALA	100	103994	0.319	11.25	
9J24043-CALB	200	199656	0.295	11.25	
<b>AVE RF</b>	<b>0.318</b>	<b>RF RSD</b>	<b>9.47</b>	<b>AVE RT</b>	<b>11.25</b>



## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.N**

### trans-1,4-Dichloro-2-butene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	531	0.184	11.29	
9J24043-CAL5	2	1313	0.235	11.28	
9J24043-CAL6	5	3293	0.232	11.28	
9J24043-CAL7	10	6985	0.234	11.28	
9J24043-CAL8	20	14515	0.239	11.28	
9J24043-CAL9	50	38431	0.243	11.28	
9J24043-CALA	100	76466	0.234	11.28	
9J24043-CALB	200	148266	0.219	11.28	
<b>AVE RF</b>	<b>0.228</b>	<b>RF RSD</b>	<b>8.27</b>	<b>AVE RT</b>	<b>11.28</b>

### 4-Chlorotoluene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	1020	1.889	11.34	
9J24043-CAL3	0.4	2178	2.024	11.34	
9J24043-CAL4	1	5461	1.896	11.34	
9J24043-CAL5	2	11718	2.099	11.34	
9J24043-CAL6	5	30239	2.132	11.34	
9J24043-CAL7	10	61742	2.069	11.34	
9J24043-CAL8	20	129933	2.143	11.34	
9J24043-CAL9	50	325043	2.056	11.33	
9J24043-CALA	100	688819	2.110	11.34	
9J24043-CALB	200	1379272	2.036	11.34	
<b>AVE RF</b>	<b>2.045</b>	<b>RF RSD</b>	<b>4.37</b>	<b>AVE RT</b>	<b>11.34</b>

### tert-Butylbenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	602	1.115	11.49	
9J24043-CAL3	0.4	1248	1.160	11.49	
9J24043-CAL4	1	3551	1.233	11.49	
9J24043-CAL5	2	7395	1.324	11.49	
9J24043-CAL6	5	18808	1.326	11.48	
9J24043-CAL7	10	38411	1.287	11.48	
9J24043-CAL8	20	81742	1.348	11.48	
9J24043-CAL9	50	202040	1.278	11.48	
9J24043-CALA	100	431117	1.320	11.48	
9J24043-CALB	200	872573	1.288	11.48	
<b>AVE RF</b>	<b>1.268</b>	<b>RF RSD</b>	<b>6.05</b>	<b>AVE RT</b>	<b>11.48</b>

### 1,2,4-Trimethylbenzene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	536	1.919	11.54	
9J24043-CAL2	0.2	1066	1.974	11.54	
9J24043-CAL3	0.4	2387	2.218	11.54	
9J24043-CAL4	1	6319	2.194	11.53	
9J24043-CAL5	2	12974	2.324	11.53	
9J24043-CAL6	5	34216	2.412	11.54	
9J24043-CAL7	10	70882	2.375	11.53	
9J24043-CAL8	20	151018	2.491	11.53	
9J24043-CAL9	50	374779	2.370	11.53	
9J24043-CALA	100	798406	2.445	11.53	
9J24043-CALB	200	1629601	2.405	11.53	
<b>AVE RF</b>	<b>2.284</b>	<b>RF RSD</b>	<b>8.30</b>	<b>AVE RT</b>	<b>11.54</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.N**

### sec-Butylbenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	1301	2.409	11.62	
9J24043-CAL3	0.4	2990	2.779	11.62	
9J24043-CAL4	1	7450	2.587	11.62	
9J24043-CAL5	2	15756	2.822	11.62	
9J24043-CAL6	5	40240	2.837	11.62	
9J24043-CAL7	10	83977	2.814	11.62	
9J24043-CAL8	20	180894	2.983	11.62	
9J24043-CAL9	50	451933	2.858	11.62	
9J24043-CALA	100	969880	2.971	11.62	
9J24043-CALB	200	1977513	2.919	11.62	
<b>AVE RF</b>	<b>2.798</b>	<b>RF RSD</b>	<b>6.31</b>	<b>AVE RT</b>	<b>11.62</b>

### 4-Isopropyltoluene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	481	1.722	11.73	
9J24043-CAL2	0.2	919	1.702	11.72	
9J24043-CAL3	0.4	2236	2.078	11.73	
9J24043-CAL4	1	6086	2.114	11.73	
9J24043-CAL5	2	12523	2.243	11.73	
9J24043-CAL6	5	33176	2.339	11.73	
9J24043-CAL7	10	68628	2.300	11.73	
9J24043-CAL8	20	151382	2.497	11.73	
9J24043-CAL9	50	378247	2.392	11.73	
9J24043-CALA	100	812481	2.489	11.73	
9J24043-CALB	200	1677679	2.476	11.73	
<b>AVE RF</b>	<b>2.214</b>	<b>RF RSD</b>	<b>12.88</b>	<b>AVE RT</b>	<b>11.73</b>

### 1,3-Dichlorobenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	629	1.165	11.80	
9J24043-CAL3	0.4	1412	1.312	11.80	
9J24043-CAL4	1	3650	1.268	11.80	
9J24043-CAL5	2	7718	1.382	11.80	
9J24043-CAL6	5	19712	1.390	11.80	
9J24043-CAL7	10	41299	1.384	11.80	
9J24043-CAL8	20	86247	1.422	11.80	
9J24043-CAL9	50	218694	1.383	11.80	
9J24043-CALA	100	461068	1.412	11.80	
9J24043-CALB	200	936572	1.382	11.80	
<b>AVE RF</b>	<b>1.350</b>	<b>RF RSD</b>	<b>5.93</b>	<b>AVE RT</b>	<b>11.80</b>

### 1,4-Dichlorobenzene-d4 (ISTD) Curve Fit:

**AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	139681	2793.620	11.85	
9J24043-CAL2	50	135021	2700.420	11.85	
9J24043-CAL3	50	134501	2690.020	11.85	
9J24043-CAL4	50	143979	2879.580	11.85	
9J24043-CAL5	50	139582	2791.640	11.85	
9J24043-CAL6	50	141843	2836.860	11.85	
9J24043-CAL7	50	149215	2984.300	11.85	
9J24043-CAL8	50	151591	3031.820	11.85	
9J24043-CAL9	50	158122	3162.440	11.85	
9J24043-CALA	50	163243	3264.860	11.85	
9J24043-CALB	50	169365	3387.300	11.85	
<b>AVE RF</b>	<b>2956.624</b>	<b>RF RSD</b>	<b>7.86</b>	<b>AVE RT</b>	<b>11.85</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### 1,2-Dichlorobenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	624	1.155	12.19	
9J24043-CAL3	0.4	1284	1.193	12.19	
9J24043-CAL4	1	3650	1.268	12.19	
9J24043-CAL5	2	7854	1.407	12.19	
9J24043-CAL6	5	19460	1.372	12.19	
9J24043-CAL7	10	40125	1.345	12.18	
9J24043-CAL8	20	83871	1.383	12.19	
9J24043-CAL9	50	211431	1.337	12.18	
9J24043-CALA	100	439251	1.345	12.19	
9J24043-CALB	200	884385	1.305	12.19	
<b>AVE RF</b>	<b>1.311</b>	<b>RF RSD</b>	<b>6.28</b>	<b>AVE RT</b>	<b>12.18</b>

### 1,2-Dibromo-3-chloropropane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	447	0.155	12.80	
9J24043-CAL5	2	1006	0.180	12.80	
9J24043-CAL6	5	2728	0.192	12.80	
9J24043-CAL7	10	6234	0.209	12.80	
9J24043-CAL8	20	13740	0.227	12.80	
9J24043-CAL9	50	38435	0.243	12.80	
9J24043-CALA	100	81625	0.250	12.80	
9J24043-CALB	200	169849	0.251	12.80	
<b>AVE RF</b>	<b>0.213</b>	<b>RF RSD</b>	<b>18.56</b>	<b>AVE RT</b>	<b>12.80</b>

### Hexachlorobutadiene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	443	0.154	13.31	
9J24043-CAL5	2	963	0.172	13.30	
9J24043-CAL6	5	2715	0.191	13.30	
9J24043-CAL7	10	5468	0.183	13.30	
9J24043-CAL8	20	12054	0.199	13.30	
9J24043-CAL9	50	29829	0.189	13.30	
9J24043-CALA	100	62008	0.190	13.30	
9J24043-CALB	200	126838	0.187	13.30	
<b>AVE RF</b>	<b>0.183</b>	<b>RF RSD</b>	<b>7.66</b>	<b>AVE RT</b>	<b>13.30</b>

### 1,2,4-Trichlorobenzene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	244	0.452	13.35	
9J24043-CAL3	0.4	615	0.572	13.35	
9J24043-CAL4	1	1833	0.637	13.35	
9J24043-CAL5	2	4043	0.724	13.34	
9J24043-CAL6	5	11114	0.784	13.35	
9J24043-CAL7	10	23133	0.775	13.35	
9J24043-CAL8	20	50962	0.840	13.35	
9J24043-CAL9	50	128379	0.812	13.34	
9J24043-CALA	100	268764	0.823	13.35	
9J24043-CALB	200	564943	0.834	13.35	
<b>AVE RF</b>	<b>0.756</b>	<b>RF RSD</b>	<b>12.49</b>	<b>AVE RT</b>	<b>13.35</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Full List**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Naphthalene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response	
			Factor	RT
9J24043-CAL1	0.1	0	0.000	0.00
9J24043-CAL2	0.2	924	1.714	13.63
9J24043-CAL3	0.4	2009	1.867	13.63
9J24043-CAL4	1	5345	1.856	13.63
9J24043-CAL5	2	12724	2.279	13.63
9J24043-CAL6	5	32892	2.319	13.63
9J24043-CAL7	10	72324	2.423	13.63
9J24043-CAL8	20	161860	2.669	13.63
9J24043-CAL9	50	425207	2.689	13.63
9J24043-CALA	100	899370	2.755	13.63
9J24043-CALB	200	1872418	2.764	13.63
<b>AVE RF</b>		<b>2.402</b>	<b>RF RSD</b>	<b>14.83</b>
			<b>AVE RT</b>	<b>13.63</b>

### 1,2,3-Trichlorobenzene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response	
			Factor	RT
9J24043-CAL1	0.1	0	0.000	0.00
9J24043-CAL2	0.2	261	0.483	13.79
9J24043-CAL3	0.4	687	0.638	13.78
9J24043-CAL4	1	1879	0.653	13.79
9J24043-CAL5	2	4073	0.729	13.79
9J24043-CAL6	5	10402	0.733	13.79
9J24043-CAL7	10	22293	0.747	13.79
9J24043-CAL8	20	48345	0.797	13.79
9J24043-CAL9	50	123175	0.779	13.79
9J24043-CALA	100	260549	0.798	13.79
9J24043-CALB	200	552458	0.815	13.79
<b>AVE RF</b>		<b>0.717</b>	<b>RF RSD</b>	<b>14.16</b>
			<b>AVE RT</b>	<b>13.79</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Additional Cpds**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Acrolein


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	420	0.181	3.63	
9J24043-CAL5	2	927	0.209	3.63	
9J24043-CAL6	5	2465	0.222	3.62	
9J24043-CAL7	10	4855	0.206	3.62	
9J24043-CAL8	20	10458	0.233	3.61	
9J24043-CAL9	50	28604	0.247	3.61	
9J24043-CALA	100	60054	0.268	3.63	
9J24043-CALB	200	116360	0.251	3.62	
<b>AVE RF</b>	<b>0.227</b>	<b>RF RSD</b>	<b>12.43</b>	<b>AVE RT</b>	<b>3.62</b>

### Vinyl acetate


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	3620	1.560	4.96	
9J24043-CAL5	2	7854	1.772	4.96	
9J24043-CAL6	5	20467	1.844	4.96	
9J24043-CAL7	10	42656	1.813	4.96	
9J24043-CAL8	20	90141	2.005	4.95	
9J24043-CAL9	50	246127	2.128	4.95	
9J24043-CALA	100	522592	2.333	4.96	
9J24043-CALB	200	980632	2.113	4.96	
<b>AVE RF</b>	<b>1.946</b>	<b>RF RSD</b>	<b>12.62</b>	<b>AVE RT</b>	<b>4.96</b>

### Pentafluorobenzene (ISTD)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	116102	2322.040	6.22	
9J24043-CAL2	50	114788	2295.760	6.22	
9J24043-CAL3	50	111985	2239.700	6.21	
9J24043-CAL4	50	116043	2320.860	6.21	
9J24043-CAL5	50	110790	2215.800	6.22	
9J24043-CAL6	50	111010	2220.200	6.21	
9J24043-CAL7	50	117608	2352.160	6.22	
9J24043-CAL8	50	112406	2248.120	6.21	
9J24043-CAL9	50	115635	2312.700	6.21	
9J24043-CALA	50	111989	2239.780	6.22	
9J24043-CALB	50	116034	2320.680	6.22	
<b>AVE RF</b>	<b>2280.709</b>	<b>RF RSD</b>	<b>2.13</b>	<b>AVE RT</b>	<b>6.21</b>

### 2-Chloroethyl vinyl ether

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	369	0.152	8.04	
9J24043-CAL4	1	1378	0.222	8.03	
9J24043-CAL5	2	2589	0.217	8.03	
9J24043-CAL6	5	7592	0.253	8.02	
9J24043-CAL7	10	15685	0.251	8.02	
9J24043-CAL8	20	33274	0.271	8.02	
9J24043-CAL9	50	88331	0.275	8.02	
9J24043-CALA	100	185987	0.292	8.02	
9J24043-CALB	200	361318	0.273	8.02	
<b>AVE RF</b>	<b>0.257</b>	<b>RF RSD</b>	<b>10.27</b>	<b>AVE RT</b>	<b>8.02</b>

**Element Calibration Review Sheet**

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Additional Cpds**

Instrument Cal ID: **VI191025W.M VI191025G.N**

**Chlorobenzene-d5 (ISTD)**

Curve Fit: **AVERAGE RF**



<u>Standard</u>	<u>Concentration</u>	<u>Response</u>	<u>Response Factor</u>	<u>RT</u>
9J24043-CAL1	50	307577	6151.540	9.91
9J24043-CAL2	50	302974	6059.480	9.92
9J24043-CAL3	50	294372	5887.440	9.91
9J24043-CAL4	50	310797	6215.940	9.91
9J24043-CAL5	50	297754	5955.080	9.92
9J24043-CAL6	50	300317	6006.340	9.91
9J24043-CAL7	50	312833	6256.660	9.91
9J24043-CAL8	50	307093	6141.860	9.91
9J24043-CAL9	50	321159	6423.180	9.91
9J24043-CALA	50	318635	6372.700	9.91
9J24043-CALB	50	330915	6618.300	9.92

**AVE RF 6189.865      RF RSD 3.53      AVE RT 9.91**

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Iodomethane Add On**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Iodomethane


Curve Fit: **QUADRATIC: Weighting: (1/a), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.1	0	0.000	0.00	
9J24043-CAL2	0.2	0	0.000	0.00	
9J24043-CAL3	0.4	0	0.000	0.00	
9J24043-CAL4	1	0	0.000	0.00	
9J24043-CAL5	2	0	0.000	0.00	
9J24043-CAL6	5	916	8.252	3.38	
9J24043-CAL7	10	3125	0.133	3.39	
9J24043-CAL8	20	11472	0.255	3.38	
9J24043-CAL9	50	57651	0.499	3.38	
9J24043-CALA	100	153366	0.685	3.39	
9J24043-CALB	200	348091	0.750	3.39	
<b>AVE RF</b>	<b>0.401</b>	<b>RF RSD</b>	<b>71.16</b>	<b>AVE RT</b>	<b>3.39</b>

### Pentafluorobenzene (ISTD)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	116102	2322.040	6.22	
9J24043-CAL2	50	114788	2295.760	6.22	
9J24043-CAL3	50	111985	2239.700	6.21	
9J24043-CAL4	50	116043	2320.860	6.21	
9J24043-CAL5	50	110790	2215.800	6.22	
9J24043-CAL6	50	111010	2220.200	6.21	
9J24043-CAL7	50	117608	2352.160	6.22	
9J24043-CAL8	50	112406	2248.120	6.21	
9J24043-CAL9	50	115635	2312.700	6.21	
9J24043-CALA	50	111989	2239.780	6.22	
9J24043-CALB	50	116034	2320.680	6.22	
<b>AVE RF</b>	<b>2280.709</b>	<b>RF RSD</b>	<b>2.13</b>	<b>AVE RT</b>	<b>6.21</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Oxygenates**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Ethanol

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9J24043-CAL1	6.25	0	0.000	0.00
9J24043-CAL2	12.5	0	0.000	0.00
9J24043-CAL3	25	1315	2.349	3.23
9J24043-CAL4	62.5	3446	2.376	3.24
9J24043-CAL5	125	7229	2.610	3.24
9J24043-CAL6	312	17243	2.489	3.23
9J24043-CAL7	625	34617	2.355	3.24
9J24043-CAL8	1250	70360	2.504	3.23
9J24043-CAL9	2500	131053	2.267	3.23
9J24043-CALA	5000	254643	2.274	3.24

**AVE RF 2.403      RF RSD 5.02      AVE RT 3.23**

### tert-Butanol (TBA)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9J24043-CAL1	6.25	2472	0.170	4.30
9J24043-CAL2	12.5	4690	0.163	4.30
9J24043-CAL3	25	10086	0.180	4.29
9J24043-CAL4	62.5	25977	0.179	4.30
9J24043-CAL5	125	58093	0.210	4.30
9J24043-CAL6	312	143817	0.208	4.29
9J24043-CAL7	625	292252	0.199	4.29
9J24043-CAL8	1250	614954	0.219	4.29
9J24043-CAL9	2500	1172838	0.203	4.29
9J24043-CALA	5000	2295578	0.205	4.29

**AVE RF 0.194      RF RSD 9.71      AVE RT 4.29**

### Diisopropyl ether (DIPE)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9J24043-CAL1	0.025	0	0.000	0.00
9J24043-CAL2	0.06	0	0.000	0.00
9J24043-CAL3	0.1	638	2.849	4.56
9J24043-CAL4	0.25	1604	2.764	4.56
9J24043-CAL5	0.5	3305	2.983	4.57
9J24043-CAL6	1.25	8576	3.090	4.57
9J24043-CAL7	2.5	17135	2.914	4.57
9J24043-CAL8	5	34871	3.102	4.56
9J24043-CAL9	10	63994	2.767	4.56
9J24043-CALA	20	122827	2.742	4.57

**AVE RF 2.901      RF RSD 5.01      AVE RT 4.57**

### Ethyl-tert-butyl ether (ETBE)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9J24043-CAL1	0.025	0	0.000	0.00
9J24043-CAL2	0.06	0	0.000	0.00
9J24043-CAL3	0.1	0	0.000	0.00
9J24043-CAL4	0.25	1449	2.497	4.94
9J24043-CAL5	0.5	3145	2.839	4.94
9J24043-CAL6	1.25	8071	2.908	4.94
9J24043-CAL7	2.5	16756	2.849	4.94
9J24043-CAL8	5	33471	2.978	4.94
9J24043-CAL9	10	63126	2.730	4.94
9J24043-CALA	20	121788	2.719	4.94

**AVE RF 2.789      RF RSD 5.66      AVE RT 4.94**



## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Oxygenates**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Pentafluorobenzene (ISTD)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	116102	2322.040	6.22	
9J24043-CAL2	50	114788	2295.760	6.22	
9J24043-CAL3	50	111985	2239.700	6.21	
9J24043-CAL4	50	116043	2320.860	6.21	
9J24043-CAL5	50	110790	2215.800	6.22	
9J24043-CAL6	50	111010	2220.200	6.21	
9J24043-CAL7	50	117608	2352.160	6.22	
9J24043-CAL8	50	112406	2248.120	6.21	
9J24043-CAL9	50	115635	2312.700	6.21	
9J24043-CALA	50	111989	2239.780	6.22	
9J24043-CALB	50	116034	2320.680	6.22	
<b>AVE RF</b>	<b>2280.709</b>	<b>RF RSD</b>	<b>2.13</b>	<b>AVE RT</b>	<b>6.21</b>

### tert-Amyl methyl ether (TAME)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.025	0	0.000	0.00	
9J24043-CAL2	0.05	0	0.000	0.00	
9J24043-CAL3	0.1	580	2.590	6.25	
9J24043-CAL4	0.25	1462	2.520	6.25	
9J24043-CAL5	0.5	2996	2.704	6.25	
9J24043-CAL6	1.25	7445	2.683	6.25	
9J24043-CAL7	2.5	15349	2.610	6.25	
9J24043-CAL8	5	30296	2.695	6.25	
9J24043-CAL9	10	56793	2.456	6.24	
9J24043-CALA	20	111127	2.481	6.25	
<b>AVE RF</b>	<b>2.592</b>	<b>RF RSD</b>	<b>3.80</b>	<b>AVE RT</b>	<b>6.25</b>

### 1,4-Difluorobenzene (Surr)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	364447	3.139	6.78	
9J24043-CAL2	50	359462	3.132	6.78	
9J24043-CAL3	50	352302	3.146	6.78	
9J24043-CAL4	50	366642	3.160	6.78	
9J24043-CAL5	50	347212	3.134	6.78	
9J24043-CAL6	50	353918	3.188	6.78	
9J24043-CAL7	50	367409	3.124	6.78	
9J24043-CAL8	50	354922	3.158	6.78	
9J24043-CAL9	50	370144	3.201	6.78	
9J24043-CALA	50	356857	3.187	6.78	
9J24043-CALB	50	369003	3.180	6.78	
<b>AVE RF</b>	<b>3.159</b>	<b>RF RSD</b>	<b>0.84</b>	<b>AVE RT</b>	<b>6.78</b>

### tert-Amyl ethyl ether (TAE)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	0.025	0	0.000	0.00	
9J24043-CAL2	0.05	0	0.000	0.00	
9J24043-CAL3	0.1	0	0.000	0.00	
9J24043-CAL4	0.25	950	1.637	7.00	
9J24043-CAL5	0.5	2147	1.938	7.00	
9J24043-CAL6	1.25	5331	1.921	7.00	
9J24043-CAL7	2.5	11032	1.876	7.00	
9J24043-CAL8	5	22696	2.019	7.00	
9J24043-CAL9	10	42660	1.845	7.00	
9J24043-CALA	20	83591	1.866	7.00	
<b>AVE RF</b>	<b>1.872</b>	<b>RF RSD</b>	<b>6.33</b>	<b>AVE RT</b>	<b>7.00</b>

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **8260C Oxygenates**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Toluene-d8 (Surr)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	406288	1.321	8.30	
9J24043-CAL2	50	403793	1.333	8.30	
9J24043-CAL3	50	396027	1.345	8.30	
9J24043-CAL4	50	410518	1.321	8.30	
9J24043-CAL5	50	395017	1.327	8.30	
9J24043-CAL6	50	397005	1.322	8.30	
9J24043-CAL7	50	415174	1.327	8.30	
9J24043-CAL8	50	399810	1.302	8.30	
9J24043-CAL9	50	415062	1.292	8.30	
9J24043-CALA	50	405945	1.274	8.30	
9J24043-CALB	50	420947	1.272	8.30	
<b>AVE RF</b>	<b>1.312</b>	<b>RF RSD</b>	<b>1.83</b>	<b>AVE RT</b>	<b>8.30</b>

### Chlorobenzene-d5 (ISTD)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	307577	6151.540	9.91	
9J24043-CAL2	50	302974	6059.480	9.92	
9J24043-CAL3	50	294372	5887.440	9.91	
9J24043-CAL4	50	310797	6215.940	9.91	
9J24043-CAL5	50	297754	5955.080	9.92	
9J24043-CAL6	50	300317	6006.340	9.91	
9J24043-CAL7	50	312833	6256.660	9.91	
9J24043-CAL8	50	307093	6141.860	9.91	
9J24043-CAL9	50	321159	6423.180	9.91	
9J24043-CALA	50	318635	6372.700	9.91	
9J24043-CALB	50	330915	6618.300	9.92	
<b>AVE RF</b>	<b>6189.865</b>	<b>RF RSD</b>	<b>3.53</b>	<b>AVE RT</b>	<b>9.91</b>

### 4-Bromofluorobenzene (Surr)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	116090	0.831	10.97	
9J24043-CAL2	50	113180	0.838	10.97	
9J24043-CAL3	50	112304	0.835	10.97	
9J24043-CAL4	50	118563	0.823	10.97	
9J24043-CAL5	50	115163	0.825	10.97	
9J24043-CAL6	50	115652	0.815	10.97	
9J24043-CAL7	50	121121	0.812	10.97	
9J24043-CAL8	50	120976	0.798	10.97	
9J24043-CAL9	50	125801	0.796	10.97	
9J24043-CALA	50	124392	0.762	10.97	
9J24043-CALB	50	127221	0.751	10.97	
<b>AVE RF</b>	<b>0.808</b>	<b>RF RSD</b>	<b>3.58</b>	<b>AVE RT</b>	<b>10.97</b>

### 1,4-Dichlorobenzene-d4 (ISTD)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9J24043-CAL1	50	139681	2793.620	11.85	
9J24043-CAL2	50	135021	2700.420	11.85	
9J24043-CAL3	50	134501	2690.020	11.85	
9J24043-CAL4	50	143979	2879.580	11.85	
9J24043-CAL5	50	139582	2791.640	11.85	
9J24043-CAL6	50	141843	2836.860	11.85	
9J24043-CAL7	50	149215	2984.300	11.85	
9J24043-CAL8	50	151591	3031.820	11.85	
9J24043-CAL9	50	158122	3162.440	11.85	
9J24043-CALA	50	163243	3264.860	11.85	
9J24043-CALB	50	169365	3387.300	11.85	
<b>AVE RF</b>	<b>2956.624</b>	<b>RF RSD</b>	<b>7.86</b>	<b>AVE RT</b>	<b>11.85</b>

## Response Factor Report VOA-GCMS9

Method Path : C:\msdchem\1\methods\  
 Method File : VI191025W.M  
 Title : EPA 8260: Volatile Organic Compounds  
 Last Update : Fri Oct 25 08:32:21 2019  
 Response Via : Initial Calibration

## Calibration Files

0.1 =VI19102417.D 0.2 =VI19102418.D 0.5 =VI19102419.D 1 =VI19102420.D 2 =VI19102421.D 5 =VI19102422.D  
 10 =VI19102423.D 20 =VI19102424.D 50 =VI19102425.D 100 =VI19102427.D 200 =VI19102429.D

Compound	0.1	0.2	0.5	1	2	5	10	20	50	100	200	Avg	%RSD
1) I Pentafluorobenzene...													
2) Dichlorodifluo...			0.627	0.682	0.842	0.812	0.770	0.800	0.946	0.947	0.929	0.817	13.92
3) P Chloromethane		1.457	1.268	1.037	1.070	1.024	0.954	1.002	1.029	1.012	0.984	1.084	14.45
4) C Vinyl Chloride		0.884	1.079	1.013	1.135	1.140	1.069	1.110	1.150	1.154	1.123	1.086	7.67
5) Bromomethane				0.760	0.709	0.701	0.624	0.614	0.579	0.559	0.576	0.640	11.51
6) Chloroethane					0.573	0.531	0.502	0.442	0.447			0.499	11.23
7) Trichlorofluor...			1.069	1.200	1.279	1.282	1.235	1.294	1.259	1.250	1.199	1.230	5.62
8) Ethanol			0.023	0.024	0.026	0.025	0.024	0.025	0.023	0.023		0.024	5.02
9) C 1,1-Dichloroet...			1.159	1.067	1.188	1.200	1.158	1.203	1.192	1.279	1.222	1.185	4.83
10) Carbon Disulfide				1.970	2.202	2.167	2.084	2.200	2.200	2.374	2.300	2.187	5.64
11) Freon 113				0.740	0.858	0.860	0.834	0.883	0.846	0.912	0.886	0.852	6.07
12) Iodomethane						0.083	0.133	0.255	0.499	0.685	0.750	0.401	71.16
13) Acrolein				0.181	0.209	0.222	0.206	0.233	0.247	0.268	0.251	0.227	12.43
14) Methylene Chlo...	8.716	4.794	2.954	1.697	1.388	1.130	0.965	0.970	0.887	0.934	0.904	2.304	106.11
15) Acetone					0.510	0.466	0.421	0.438	0.406	0.421	0.404	0.438	8.73
16) t-1,2-Dichloro...		0.784	1.075	1.145	1.242	1.233	1.164	1.247	1.188	1.276	1.248	1.160	12.54
17) n-Hexane				0.154	0.160	0.165	0.172	0.185	0.183	0.196	0.198	0.177	9.35
18) Methyl-tert-bu...			2.577	2.494	2.698	2.694	2.617	2.750	2.707	2.888	2.841	2.696	4.58
19) tert-Butanol ...	0.170	0.163	0.180	0.179	0.210	0.208	0.199	0.219	0.203	0.205		0.194	9.71
20) Diisopropyl et...			2.849	2.764	2.983	3.090	2.914	3.102	2.767	2.742		2.901	5.01
21) P 1,1-Dichloroet...			1.477	1.582	1.631	1.649	1.573	1.671	1.582	1.696	1.641	1.611	4.09
22) Acrylonitrile				0.377	0.440	0.489	0.484	0.511	0.507	0.547	0.524	0.485	11.08
23) Ethyl-tert-but...				2.497	2.839	2.908	2.849	2.978	2.730	2.719		2.789	5.66
24) Vinyl Acetate				1.560	1.772	1.844	1.813	2.005	2.128	2.333	2.113	1.946	12.62
25) c-1,2-Dichloro...			1.125	1.182	1.256	1.257	1.221	1.298	1.238	1.328	1.288	1.244	4.98
26) 2,2-Dichloropr...			0.952	0.998	1.078	1.062	1.006	1.073	1.061	1.129	1.104	1.051	5.31
27) Bromochloromet...			0.436	0.512	0.605	0.646	0.636	0.688	0.671	0.677	0.622	0.610	13.73
28) C Chloroform		1.278	1.442	1.440	1.642	1.638	1.607	1.696	1.617	1.719	1.673	1.575	8.98
29) Carbon Tetrach...				0.772	0.903	0.897	0.886	0.977	0.991	1.106	1.133	0.958	12.52
30) Tetrahydrofuran				0.407	0.461	0.460	0.441	0.474	0.468	0.500	0.477	0.461	5.94
31) 1,1,1-Trichlor...			1.130	1.251	1.340	1.347	1.284	1.379	1.354	1.453	1.430	1.330	7.37
32) S Dibromofluorom...	0.960	0.964	0.965	0.962	0.982	0.984	0.967	0.975	1.010	1.016	1.023	0.982	2.38
33) 1,1-Dichloropr...			1.171	1.184	1.292	1.299	1.245	1.313	1.271	1.376	1.341	1.277	5.30
34) 2-Butanone (MEK)				0.625	0.704	0.704	0.662	0.717	0.701	0.741	0.702	0.695	5.12
35) Benzene	3.949	3.450	3.774	3.582	4.047	3.910	3.714	3.910	3.758	4.022	3.911	3.821	4.86
36) tert-Amyl meth...			2.590	2.520	2.704	2.683	2.610	2.695	2.456	2.481		2.592	3.80
37) 1,2-Dichloroet...			1.198	1.130	1.292	1.293	1.230	1.306	1.245	1.313	1.256	1.252	4.76
38) iso-Butyl Alcohol			0.052	0.054	0.072	0.075	0.067	0.074	0.078	0.080	0.074	0.070	14.51
39) S 1,4-Difluorobe...	3.139	3.132	3.146	3.160	3.134	3.188	3.124	3.158	3.201	3.187	3.180	3.159	0.84
40) Trichloroethen...		0.810	0.801	0.933	1.033	1.022	0.997	1.053	1.026	1.095	1.074	0.984	10.55
41) Tert-Amyl-Ethy...				1.637	1.938	1.921	1.876	2.019	1.845	1.866		1.872	6.33

## Response Factor Report VOA-GCMS9

Method Path	C:\msdchem\1\methods\ Method File : VI191025W.M														
Title	EPA 8260: Volatile Organic Compounds														
42)	Dibromomethane	0.422	0.554	0.622	0.633	0.620	0.656	0.642	0.692	0.677	0.613	13.36	/		
43) C	1,2-Dichloropr...	0.890	0.838	0.987	0.982	0.932	0.988	0.944	1.024	0.994	0.953	6.18	/		
44)	Bromodichlorom...	0.893	0.973	1.056	1.083	1.065	1.150	1.155	1.260	1.255	1.099	11.01	/		
45)	Chlorobenzene-d5 (I)	-----ISTD-----													
46)	2-Chloroethyl ...		0.222	0.217	0.253	0.251	0.271	0.275	0.292	0.273	0.257	10.27	/		
47)	c-1,3-Dichloro...	0.431	0.429	0.468	0.474	0.487	0.525	0.520	0.559	0.556	0.494	9.88	/		
48) S	Toluene-d8 (S)	1.321	1.333	1.345	1.321	1.327	1.322	1.302	1.292	1.274	1.272	1.312	1.83	/	
49) C	Toluene	1.590	1.439	1.488	1.454	1.499	1.474	1.445	1.492	1.391	1.462	1.439	1.470	3.41	/
50)	Tetrachloroeth...	0.220	0.334	0.321	0.364	0.361	0.353	0.370	0.352	0.372	0.375	0.342	13.48	/	
51)	4-Methyl-2-Pen...	0.367	0.406	0.406	0.463	0.469	0.464	0.491	0.474	0.484	0.441	0.446	9.09	/	
52)	t-1,3-Dichloro...		0.341	0.378	0.404	0.420	0.465	0.473	0.513	0.513	0.438	14.34	/		
53)	1,1,2-Trichlor...	0.238	0.304	0.313	0.347	0.344	0.342	0.351	0.335	0.347	0.338	0.326	10.62	/	
54)	Dibromochlorom...		0.214	0.217	0.255	0.267	0.275	0.301	0.315		0.264	14.58	/		
55)	1,3-Dichloropr...	0.469	0.532	0.541	0.578	0.584	0.581	0.600	0.571	0.595	0.571	0.562	6.98	/	
56)	1,2-Dibromoeth...		0.261	0.310	0.378	0.375	0.366	0.381	0.366	0.382	0.375	0.355	11.70	/	
57)	2-Hexanone		0.286	0.284	0.319	0.328	0.335	0.356	0.350	0.358	0.327	0.327	8.41	/	
58) P	Chlorobenzene	0.780	0.862	0.945	0.928	0.982	0.984	0.965	0.985	0.940	0.981	0.971	0.939	6.80	/
59) C	Ethylbenzene	1.531	1.514	1.522	1.409	1.608	1.560	1.535	1.591	1.516	1.594	1.580	1.542	3.61	/
60)	1,1,1,2-Tetrac...		0.200	0.237	0.251	0.266	0.272	0.296	0.296	0.324	0.323	0.274	14.90	/	
61)	m,p-Xylenes (2)	1.112	1.019	1.103	1.029	1.137	1.146	1.135	1.209	1.150	1.230	1.219	1.135	6.12	/
62)	o-Xylene	0.951	1.008	1.106	1.067	1.142	1.147	1.141	1.216	1.158	1.233	1.214	1.126	7.83	/
63)	Styrene		0.703	0.785	0.870	0.890	0.911	0.979	0.956	1.026	1.023	0.905	11.93	/	
64) P	Bromoform			0.128	0.149	0.156	0.171	0.194	0.221	0.255		0.182	24.41	/	
65)	Isopropylbenzene	1.111	1.302	1.233	1.371	1.392	1.385	1.488	1.427	1.528	1.496	1.373	9.37	/	
66) I	1,4-Dichlorobenzen...	-----ISTD-----													
67) S	4-Bromofluorob...	0.831	0.838	0.835	0.823	0.825	0.815	0.812	0.798	0.796	0.762	0.751	0.808	3.58	/
68)	Bromobenzene	0.444	0.800	0.813	0.771	0.830	0.819	0.812	0.825	0.798	0.813	0.800	0.775	14.32	/
69)	n-Propylbenzene	3.125	3.053	3.294	3.181	3.455	3.384	3.318	3.475	3.358	3.501	3.408	3.323	4.44	/
70) P	1,1,1,2-Tetrac...		0.565	0.624	0.651	0.718	0.694	0.673	0.690	0.674	0.651	0.603	0.654	7.07	/
71)	2-Chlorotoluene		0.668	0.663	0.747	0.716	0.725	0.753	0.719	0.730	0.723	0.716	4.34	/	
72)	1,3,5-Trimethy...	1.990	2.087	2.127	2.152	2.344	2.349	2.342	2.452	2.344	2.400	2.390	2.271	6.72	/
73)	1,2,3-Trichlor...		0.252	0.308	0.347	0.343	0.341	0.333	0.327	0.319	0.295	0.318	9.47	/	
74)	t-1,4-Dichloro...			0.184	0.235	0.232	0.234	0.239	0.243	0.234	0.219	0.228	8.27	/	
75)	4-Chlorotoluene	1.889	2.024	1.896	2.099	2.132	2.069	2.143	2.056	2.110	2.036	2.045	4.37	/	
76)	tert-Butylbenzene	1.115	1.160	1.233	1.324	1.326	1.287	1.348	1.278	1.320	1.288	1.268	6.05	/	
77)	1,2,4-Trimethy...	1.919	1.974	2.218	2.194	2.324	2.412	2.375	2.491	2.370	2.445	2.405	2.284	8.30	/
78)	sec-Butylbenzene	2.409	2.779	2.587	2.822	2.837	2.814	2.983	2.858	2.971	2.919	2.798	6.32	/	
79)	4-Isopropyltol...	1.722	1.702	2.078	2.114	2.243	2.339	2.300	2.497	2.392	2.489	2.476	2.214	12.88	/
80)	1,3-Dichlorobe...	1.165	1.312	1.268	1.382	1.390	1.384	1.422	1.383	1.412	1.382	1.350	5.93	/	
81)	1,4-Dichlorobe...	1.113	1.342	1.454	1.451	1.531	1.440	1.433	1.478	1.406	1.436	1.402	1.408	7.70	/
82)	n-Butylbenzene	1.357	1.491	1.735	1.735	1.903	2.011	1.994	2.160	2.060	2.129	2.119	1.881	14.34	/
83)	1,2-Dichlorobe...	1.155	1.193	1.268	1.407	1.372	1.345	1.383	1.337	1.345	1.305	1.311	6.28	/	
84)	1,2-Dibromo-3-...			0.180	0.192	0.209	0.227	0.243	0.250	0.251	0.222	12.86	/		
85)	Hexachlorobuta...			0.154	0.172	0.191	0.183	0.199	0.189	0.190	0.187	0.183	7.66	/	
86)	1,2,4-Trichlor...		0.572	0.637	0.724	0.784	0.775	0.840	0.812	0.823	0.834	0.756	12.49	/	
87)	Naphthalene		1.867	1.856	2.279	2.319	2.423	2.669	2.689	2.755	2.764	2.402	14.83	/	
88)	1,2,3-Trichlor...	0.483	0.638	0.653	0.729	0.733	0.747	0.797	0.779	0.798	0.815	0.717	14.16	/	

(# ) = Out of Range

Compound List Report VOA-GCMS9

Method Path : C:\msdchem\1\methods\  
 Method File : VI191025W.M  
 Title : EPA 8260: Volatile Organic Compounds  
 Last Update : Fri Oct 25 08:32:21 2019  
 Response Via : Initial Calibration

Total Cpnds : 88

PK#	Compound Name	QIon	Exp_RT	Rel_RT	Cal	#Qual	A/H	ID
1 I	Pentafluorobenzene (I)	99	6.211	1.000	A	2	A	R
2	Dichlorodifluoromethane	85	1.673	0.269	A	2	A	R
3 P	Chloromethane	50	1.891	0.304	A	2	A	R
4 C	Vinyl Chloride	62	1.995	0.321	A	2	A	R
5	Bromomethane	96	2.353	0.379	A	2	A	R
6	Chloroethane	64	2.487	0.400	A	2	A	R
7	Trichlorofluoromethane	101	2.658	0.428	A	2	A	R
8	Ethanol	45	3.230	0.520	A	1	A	R
9 C	1,1-Dichloroethene	61	3.230	0.520	A	2	A	R
10	Carbon Disulfide	76	3.242	0.522	A	2	A	R
11	Freon 113	101	3.279	0.528	A	2	A	R
12	Iodomethane	142	3.382	0.545	Q/7	2	A	R
13	Acrolein	56	3.613	0.582	A	2	A	R
14	Methylene Chloride	84	3.868	0.623	Q/4	2	A	R
15	Acetone	43	3.935	0.634	A	1	A	R
16	t-1,2-Dichloroethene	61	4.033	0.649	A	2	A	R
17	n-Hexane	86	4.118	0.663	A	3	A	R
18	Methyl-tert-butyl-ether	73	4.167	0.671	A	3	A	R
19	tert-Butanol (TBA)	59	4.288	0.690	A	1	A	R
20	Diisopropyl ether (DIPE)	45	4.562	0.735	A	2	A	R
21 P	1,1-Dichloroethane	63	4.678	0.753	A	2	A	R
22	Acrylonitrile	53	4.745	0.764	A	2	A	R
23	Ethyl-tert-butyl ether (ETBE)	59	4.939	0.795	A	2	A	R
24	Vinyl Acetate	43	4.951	0.797	A	2	A	R
25	c-1,2-Dichloroethene	61	5.238	0.843	A	2	A	R
26	2,2-Dichloropropane	77	5.347	0.861	A	2	A	R
27	Bromochloromethane	130	5.444	0.877	A	2	A	R
28 C	Chloroform	83	5.523	0.889	A	2	A	R
29	Carbon Tetrachloride	117	5.657	0.911	A	2	A	R
30	Tetrahydrofuran	42	5.700	0.918	A	2	A	R
31	1,1,1-Trichloroethane	97	5.730	0.923	A	2	A	R
32 S	Dibromofluoromethane (S)	111	5.712	0.920	A	2	A	R
33	1,1-Dichloropropene	75	5.858	0.943	A	2	A	R
34	2-Butanone (MEK)	43	5.852	0.942	A	2	A	R
35	Benzene	78	6.120	0.985	A	2	A	R
36	tert-Amyl methyl ether (TAME)	73	6.247	1.006	A	2	A	R
37	1,2-Dichloroethane (EDC)	62	6.339	1.021	A	2	A	R
38	iso-Butyl Alcohol	43	6.369	1.025	A	2	A	R
39 S	1,4-Difluorobenzene (S)	114	6.777	1.091	A	2	A	R
40	Trichloroethene (TCE)	130	6.740	1.085	A	2	A	R
41	Tert-Amyl-Ethyl-Ether (TAEE)	59	6.996	1.126	A	2	A	R
42	Dibromomethane	93	7.196	1.159	A	2	A	R
43 C	1,2-Dichloropropane	63	7.306	1.176	A	2	A	R
44	Bromodichloromethane	83	7.379	1.188	A	2	A	R
45 I	Chlorobenzene-d5 (I)	117	9.910	1.000	A	2	A	R
46	2-Chloroethyl Vinyl Ether	63	8.017	0.809	A	2	A	R
47	c-1,3-Dichloropropene	75	8.091	0.816	A	2	A	R
48 S	Toluene-d8 (S)	98	8.298	0.837	A	2	A	R
49 C	Toluene	91	8.358	0.843	A	2	A	R
50	Tetrachloroethene (PCE)	166	8.796	0.888	A	2	A	R
51	4-Methyl-2-Pentanone (MIBK)	43	8.796	0.888	A	2	A	R
52	t-1,3-Dichloropropene	75	8.832	0.891	A	2	A	R
53	1,1,2-Trichloroethane	97	9.003	0.909	A	2	A	R
54	Dibromochloromethane	129	9.185	0.927	A	2	A	R
55	1,3-Dichloropropane	76	9.289	0.937	A	2	A	R

56		1,2-Dibromoethane (EDB)	107	9.423	0.951	A	2	A	R
57		2-Hexanone	43	9.654	0.974	A	2	A	R
58	P	Chlorobenzene	112	9.928	1.002	A	2	A	R
59	C	Ethylbenzene	91	9.952	1.004	A	2	A	R
60		1,1,1,2-Tetrachloroethane	131	9.988	1.008	A	2	A	R
61		m,p-Xylenes (2)	91	10.086	1.018	A	2	A	R
62		o-Xylene	91	10.463	1.056	A	2	A	R
63		Styrene	104	10.512	1.061	A	2	A	R
64	P	Bromoform	173	10.536	1.063	<del>Q</del>	2	A	R
65		Isopropylbenzene	105	10.731	1.083	A	2	A	R
66	I	1,4-Dichlorobenzene-d4 (I)	152	11.850	1.000	A	2	A	R
67	S	4-Bromofluorobenzene (S)	174	10.974	0.926	A	2	A	R
68		Bromobenzene	156	11.060	0.933	A	2	A	R
69		n-Propylbenzene	91	11.072	0.934	A	2	A	R
70	P	1,1,2,2-Tetrachloroethane	85	11.139	0.940	A	2	A	R
71		2-Chlorotoluene	126	11.206	0.946	A	2	A	R
72		1,3,5-Trimethylbenzene	105	11.229	0.948	A	2	A	R
73		1,2,3-Trichloropropane	110	11.248	0.949	A	2	A	R
74		t-1,4-Dichloro-2-butene	53	11.279	0.952	A	3	A	R
75		4-Chlorotoluene	91	11.339	0.957	A	2	A	R
76		tert-Butylbenzene	91	11.479	0.969	A	2	A	R
77		1,2,4-Trimethylbenzene	105	11.534	0.973	A	2	A	R
78		sec-Butylbenzene	105	11.619	0.980	A	2	A	R
79		4-Isopropyltoluene	119	11.728	0.990	A	2	A	R
80		1,3-Dichlorobenzene	146	11.796	0.995	A	2	A	R
81		1,4-Dichlorobenzene	146	11.863	1.001	A	2	A	R
82		n-Butylbenzene	91	12.045	1.016	A	2	A	R
83		1,2-Dichlorobenzene	146	12.185	1.028	A	2	A	R
84		1,2-Dibromo-3-Chloropropane	157	12.799	1.080	A	2	A	R
85		Hexachlorobutadiene	223	13.304	1.123	A	3	A	R
86		1,2,4-Trichlorobenzene	180	13.346	1.126	A	2	A	R
87		Naphthalene	128	13.626	1.150	A	2	A	R
88		1,2,3-Trichlorobenzene	180	13.784	1.163	A	2	A	R

Cal A = Average L = Linear LO = Linear w/origin Q = Quad QO = Quad w/origin

#Qual = number of qualifiers


A/H = Area or Height

ID R = R.T. B = R.T. & Q Q = Qvalue L = Largest A = All

-----  
 VI191025W.M Fri Oct 25 09:01:32 2019

Iodomethane




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\REQUANT\  
 Data File : VI19102421.D  
 Acq On : 24 Oct 2019 5:42 pm  
 Operator : MM  
 Sample : 9J24043-CAL5  
 Misc : 1X 5mL 2/4PPB VOCR  
 ALS Vial : 8 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:42:43 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration



(12) Iodomethane

3.400min (+ 0.018) 6.13 ug/L m

response 130


Ion	Exp%	Act%
141.90	100.00	100.00
126.90	34.80	0.00#
140.90	15.30	0.00#
0.00	0.00	0.00

*Handwritten notes:*  
 MM  
 10/25/19



Methylene Chloride

Response Ratio



$R = -2.46e-003 A^2 + 9.12e-001 A + 1.58e-002$

Coef of Det ( $r^2$ ) = 0.999 Curve Fit: Quadratic w(1/a)




Method Name: C:\msdchem\1\methods\VI191025W.M

Calibration Table Last Updated: Fri Oct 25 08:34:03 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\REQUANT\  
 Data File : VI19102418.D  
 Acq On : 24 Oct 2019 4:21 pm  
 Operator : MM  
 Sample : 9J24043-CAL2  
 Misc : 1X 5mL 0.2/0.4PPB VOCR  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:42:34 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration



TIC: VI19102418.D\data.ms

(14) Methylene Chloride

3.875min (+ 0.007) 0.18 ug/L


response 2201

*MM*

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	134.70	116.13
86.00	61.50	66.92
0.00	0.00	0.00

Bromoform

Response Ratio



$R = 3.82e-002 A^2 + 1.80e-001 A - 1.40e-003$

Coef of Det (r^2) = 1.000 Curve Fit: Quadratic w/(1/a)




Method Name: C:\msdchem\1\methods\VI191025W.M

Calibration Table Last Updated: Fri Oct 25 08:48:07 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\REQUANT\  
 Data File : VI19102419.D  
 Acq On : 24 Oct 2019 4:48 pm  
 Operator : MM  
 Sample : 9J24043-CAL3  
 Misc : 1X 5mL 0.4/0.8PPB VOCR  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:48:10 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration



(64) Bromoform (P)

10.542min (+ 0.006) 0.38 ug/L m

response -4

Ion	Exp%	Act%
172.90	100.00	100.00
174.90	49.20	0.00#
251.80	13.30	0.00
0.00	0.00	-0.00

*Handwritten signature and date:*  
 MM  
 10/25/19

Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102432.D  
 Acq On : 24 Oct 2019 10:38 pm  
 Operator : MM  
 Sample : 9J24043-ICV1  
 Misc : 1X 5mL 20/40PPB VOCR  
 ALS Vial : 19 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:53 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

*MM*  
*10/25/19*

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I Pentafluorobenzene (I)	50.000	50.000	0.0	103	0.00
2 Dichlorodifluoromethane	20.000	25.235	-26.2#	133	0.00
3 P Chloromethane	20.000	20.727	-3.6	115	0.00
4 C Vinyl Chloride	20.000	22.118	-10.6	111	0.00
5 Bromomethane	20.000	22.648	-13.2	122	0.00
6 Chloroethane	20.000	17.519	12.4	102	0.00
7 Trichlorofluoromethane	20.000	20.686	-3.4	101	0.00
8 Ethanol	<del>1250.000</del>	<del>37.145</del>	<del>97.0#</del>	<del>3</del>	<del>0.00</del>
9 C 1,1-Dichloroethene	20.000	19.721	1.4	100	0.00
10 Carbon Disulfide	20.000	18.350	8.2	94	0.00
11 Freon 113	20.000	19.089	4.6	95	0.00
12 Iodomethane	20.000	16.515	17.4	117	0.00
13 Acrolein	20.000	20.473	-2.4	103	0.00
14 Methylene Chloride	20.000	19.959	0.2	101	0.00
15 Acetone	40.000	37.600	6.0	97	0.00
16 t-1,2-Dichloroethene	20.000	20.982	-4.9	100	0.00
17 n-Hexane	20.000	19.272	3.6	95	0.00
18 Methyl-tert-butyl-ether	20.000	19.588	2.1	99	0.00
19 tert-Butanol (TBA)	<del>1250.000</del>	<del>28.139</del>	<del>97.7#</del>	<del>2</del>	<del>0.00</del>
20 Diisopropyl ether (DIPE)	<del>5.000</del>	<del>0.181</del>	<del>96.4#</del>	<del>3</del>	<del>0.00</del>
21 P 1,1-Dichloroethane	20.000	20.526	-2.6	102	0.00
22 Acrylonitrile	20.000	19.587	2.1	96	0.00
23 Ethyl-tert-butyl ether (ET)	<del>5.000</del>	<del>0.158</del>	<del>96.8#</del>	<del>3</del>	<del>0.00</del>
24 Vinyl Acetate	20.000	19.888	0.6	99	0.00
25 c-1,2-Dichloroethene	20.000	20.039	-0.2	99	0.00
26 2,2-Dichloropropane	20.000	17.720	11.4	89	0.00
27 Bromochloromethane	20.000	22.053	-10.3	101	0.00
28 C Chloroform	20.000	20.857	-4.3	100	0.00
29 Carbon Tetrachloride	20.000	20.695	-3.5	104	0.00
30 Tetrahydrofuran	20.000	19.026	4.9	95	0.00
31 1,1,1-Trichloroethane	20.000	19.935	0.3	99	0.00
32 S Dibromofluoromethane (S)	50.000	50.291	-0.6	104	0.00
33 1,1-Dichloropropene	20.000	19.605	2.0	98	0.00
34 2-Butanone (MEK)	40.000	37.882	5.3	94	0.00
35 Benzene	20.000	19.670	1.6	99	0.00
36 tert-Amyl methyl ether (TA)	<del>5.000</del>	<del>0.175</del>	<del>96.5#</del>	<del>3</del>	<del>0.01</del>
37 1,2-Dichloroethane (EDC)	20.000	20.160	-0.8	99	0.00
38 iso-Butyl Alcohol	500.000	519.105	-3.8	100	0.00
39 S 1,4-Difluorobenzene (S)	50.000	50.364	-0.7	104	0.00
40 Trichloroethene (TCE)	20.000	21.245	-6.2	102	0.00
41 Tert-Amyl-Ethyl-Ether (TAEE)	<del>5.000</del>	<del>0.144</del>	<del>97.1#</del>	<del>3</del>	<del>0.00</del>
42 Dibromomethane	20.000	21.130	-5.6	102	0.00
43 C 1,2-Dichloropropane	20.000	20.286	-1.4	101	0.00
44 Bromodichloromethane	20.000	20.751	-3.8	102	0.00
45 Chlorobenzene-d5 (I)	50.000	50.000	0.0	104	0.00
46 2-Chloroethyl Vinyl Ether	20.000	20.093	-0.5	99	0.00
47 c-1,3-Dichloropropene	20.000	19.890	0.5	98	0.00
48 S Toluene-d8 (S)	50.000	49.306	1.4	104	0.00
49 C Toluene	20.000	19.385	3.1	99	0.00
50 Tetrachloroethene (PCE)	20.000	20.889	-4.4	101	0.00

Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102432.D  
 Acq On : 24 Oct 2019 10:38 pm  
 Operator : MM  
 Sample : 9J24043-ICV1  
 Misc : 1X 5mL 20/40PPB VOCR  
 ALS Vial : 19 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:53 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
51	4-Methyl-2-Pentanone (MIBK)	40.000	41.038	-2.6	97	0.00
52	t-1,3-Dichloropropene	20.000	20.701	-3.5	102	0.00
53	1,1,2-Trichloroethane	20.000	21.234	-6.2	103	0.00
54	Dibromochloromethane	20.000	23.749	-18.7	108	0.00
55	1,3-Dichloropropane	20.000	20.475	-2.4	100	0.00
56	1,2-Dibromoethane (EDB)	20.000	20.657	-3.3	100	0.00
57	2-Hexanone	40.000	40.560	-1.4	97	0.00
58 P	Chlorobenzene	20.000	20.598	-3.0	102	0.00
59 C	Ethylbenzene	20.000	20.146	-0.7	102	0.00
60	1,1,1,2-Tetrachloroethane	20.000	21.774	-8.9	105	0.00
61	m,p-Xylenes (2)	40.000	40.933	-2.3	100	0.00
62	o-Xylene	20.000	20.989	-4.9	101	0.00
63	Styrene	20.000	20.857	-4.3	100	0.00
64 P	Bromoform	20.000	21.372	-6.9	111	0.00
65	Isopropylbenzene	20.000	20.931	-4.7	101	0.00
66 I	1,4-Dichlorobenzene-d4 (I)	50.000	50.000	0.0	104	0.00
67 S	4-Bromofluorobenzene (S)	50.000	49.582	0.8	105	0.00
68	Bromobenzene	20.000	20.988	-4.9	103	0.00
69	n-Propylbenzene	20.000	20.099	-0.5	100	0.00
70 P	1,1,2,2-Tetrachloroethane	20.000	20.344	-1.7	100	0.00
71	2-Chlorotoluene	20.000	19.935	0.3	99	0.00
72	1,3,5-Trimethylbenzene	20.000	20.663	-3.3	100	0.00
73	1,2,3-Trichloropropane	20.000	20.663	-3.3	103	0.00
74	t-1,4-Dichloro-2-butene	20.000	17.538	12.3	87	0.00
75	4-Chlorotoluene	20.000	20.563	-2.8	102	0.00
76	tert-Butylbenzene	20.000	20.366	-1.8	100	0.00
77	1,2,4-Trimethylbenzene	20.000	20.724	-3.6	99	0.00
78	sec-Butylbenzene	20.000	20.458	-2.3	100	0.00
79	4-Isopropyltoluene	20.000	21.662	-8.3	100	0.00
80	1,3-Dichlorobenzene	20.000	20.840	-4.2	103	0.00
81	1,4-Dichlorobenzene	20.000	20.477	-2.4	102	0.00
82	n-Butylbenzene	20.000	22.267	-11.3	101	0.00
83	1,2-Dichlorobenzene	20.000	20.819	-4.1	103	0.00
84	1,2-Dibromo-3-Chloropropane	20.000	20.036	-0.2	102	0.00
85	Hexachlorobutadiene	20.000	21.851	-9.3	105	0.00
86	1,2,4-Trichlorobenzene	20.000	22.259	-11.3	104	0.00
87	Naphthalene	20.000	21.916	-9.6	103	0.00
88	1,2,3-Trichlorobenzene	20.000	22.607	-13.0	106	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102433.D  
 Acq On : 24 Oct 2019 11:05 pm  
 Operator : MM  
 Sample : 9J24043-ICV2  
 Misc : 1X 5mL 5/1250PPB OXY  
 ALS Vial : 20 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*MM*  
*10/25/19*

Quant Time: Oct 25 08:52:56 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I Pentafluorobenzene (I)	50.000	50.000	0.0	99	0.00
2 Dichlorodifluoromethane	20.000	0.142	99.3#	1	0.00
3 P Chloromethane	20.000	0.423	97.9#	2	0.00
4 C Vinyl Chloride	20.000	0.200	99.0#	1	0.00
5 Bromomethane	20.000	0.740	96.3#	4	0.00
6 Chloroethane	20.000	0.736	96.3#	4	0.03
7 Trichlorofluoromethane	20.000	0.052	99.7#	0	0.01
8 Ethanol	1250.000	1059.187	15.3	80	0.00
9 C 1,1-Dichloroethene	20.000	0.161	99.2#	1	0.00
10 Carbon Disulfide	20.000	0.494	97.5#	2	0.01
11 Freon 113	20.000	0.000	100.0#	0	-3.28#
12 Iodomethane	20.000	6.269	68.7#	3	0.00
13 Acrolein	20.000	0.000	100.0#	0	-3.61#
14 Methylene Chloride	20.000	0.401	98.0#	6	0.00
15 Acetone	40.000	1.018	97.5#	3	0.01
16 t-1,2-Dichloroethene	20.000	0.302	98.5#	1	0.00
17 n-Hexane	20.000	0.000	100.0#	0	-4.12#
18 Methyl-tert-butyl-ether	20.000	0.085	99.6#	0	0.00
19 tert-Butanol (TBA)	1250.000	1179.792	5.6	83	0.00
20 Diisopropyl ether (DIPE)	5.000	4.407	11.9	82	0.00
21 P 1,1-Dichloroethane	20.000	0.254	98.7#	1	0.00
22 Acrylonitrile	20.000	0.000	100.0#	0	-4.74#
23 Ethyl-tert-butyl ether (ET)	5.000	4.402	12.0	82	0.00
24 Vinyl Acetate	20.000	0.689	96.6#	3	-0.02
25 c-1,2-Dichloroethene	20.000	0.236	98.8#	1	0.00
26 2,2-Dichloropropane	20.000	0.080	99.6#	0	0.01
27 Bromochloromethane	20.000	0.000	100.0#	0	-5.44#
28 C Chloroform	20.000	0.223	98.9#	1	0.00
29 Carbon Tetrachloride	20.000	0.000	100.0#	0	-5.66#
30 Tetrahydrofuran	20.000	0.000	100.0#	0	-5.70#
31 1,1,1-Trichloroethane	20.000	0.094	99.5#	0	0.00
32 S Dibromofluoromethane (S)	50.000	49.641	0.7	99	0.00
33 1,1-Dichloropropene	20.000	0.226	98.9#	1	0.00
34 2-Butanone (MEK)	40.000	0.000	100.0#	0	-5.85#
35 Benzene	20.000	0.266	98.7#	1	0.00
36 tert-Amyl methyl ether (TA)	5.000	4.185	16.3	80	0.00
37 1,2-Dichloroethane (EDC)	20.000	0.071	99.6#	0	0.01
38 iso-Butyl Alcohol	500.000	0.000	100.0#	0	-6.37#
39 S 1,4-Difluorobenzene (S)	50.000	50.455	-0.9	100	0.00
40 Trichloroethene (TCE)	20.000	0.257	98.7#	1	0.01
41 Tert-Amyl-Ethyl-Ether (TAEE)	5.000	4.278	14.4	78	0.00
42 Dibromomethane	20.000	0.000	100.0#	0	-7.20#
43 C 1,2-Dichloropropane	20.000	0.177	99.1#	1	0.00
44 Bromodichloromethane	20.000	0.108	99.5#	1	0.00
45 Chlorobenzene-d5 (I)	50.000	50.000	0.0	97	0.00
46 2-Chloroethyl Vinyl Ether	20.000	0.000	100.0#	0	-8.02#
47 c-1,3-Dichloropropene	20.000	0.143	99.3#	1	0.00
48 S Toluene-d8 (S)	50.000	50.620	-1.2	99	0.00
49 C Toluene	20.000	0.283	98.6#	1	0.00
50 Tetrachloroethene (PCE)	20.000	0.334	98.3#	1	0.00

Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102433.D  
 Acq On : 24 Oct 2019 11:05 pm  
 Operator : MM  
 Sample : 9J24043-ICV2  
 Misc : 1X 5mL 5/1250PPB OXY  
 ALS Vial : 20 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:56 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
51	4-Methyl-2-Pentanone (MIBK)	40.000	0.000	100.0#	0	-8.80#
52	t-1,3-Dichloropropene	20.000	0.080	99.6#	0	0.02
53	1,1,2-Trichloroethane	20.000	0.000	100.0#	0	-9.00#
54	Dibromochloromethane	20.000	0.000	100.0#	0	-9.19#
55	1,3-Dichloropropane	20.000	0.089	99.6#	0	0.00
56	1,2-Dibromoethane (EDB)	20.000	0.000	100.0#	0	-9.42#
57	2-Hexanone	40.000	0.000	100.0#	0	-9.65#
58 P	Chlorobenzene	20.000	0.297	98.5#	1	0.00
59 C	Ethylbenzene	20.000	0.274	98.6#	1	0.00
60	1,1,1,2-Tetrachloroethane	20.000	0.153	99.2#	1	0.00
61	m,p-Xylenes (2)	40.000	0.530	98.7#	1	0.00
62	o-Xylene	20.000	0.258	98.7#	1	0.00
63	Styrene	20.000	0.234	98.8#	1	0.00
64 P	Bromoform	20.000	0.000	100.0#	0	-10.54#
65	Isopropylbenzene	20.000	0.224	98.9#	1	0.00
66 I	1,4-Dichlorobenzene-d4 (I)	50.000	50.000	0.0	92	0.00
67 S	4-Bromofluorobenzene (S)	50.000	50.894	-1.8	94	0.00
68	Bromobenzene	20.000	0.267	98.7#	1	0.00
69	n-Propylbenzene	20.000	0.308	98.5#	1	0.00
70 P	1,1,2,2-Tetrachloroethane	20.000	0.000	100.0#	0	-11.14#
71	2-Chlorotoluene	20.000	0.261	98.7#	1	0.00
72	1,3,5-Trimethylbenzene	20.000	0.279	98.6#	1	0.00
73	1,2,3-Trichloropropane	20.000	0.000	100.0#	0	-11.25#
74	t-1,4-Dichloro-2-butene	20.000	0.000	100.0#	0	-11.28#
75	4-Chlorotoluene	20.000	0.357	98.2#	2	0.00
76	tert-Butylbenzene	20.000	0.243	98.8#	1	0.00
77	1,2,4-Trimethylbenzene	20.000	0.300	98.5#	1	0.00
78	sec-Butylbenzene	20.000	0.275	98.6#	1	0.00
79	4-Isopropyltoluene	20.000	0.295	98.5#	1	0.00
80	1,3-Dichlorobenzene	20.000	0.371	98.1#	2	0.00
81	1,4-Dichlorobenzene	20.000	0.404	98.0#	2	0.00
82	n-Butylbenzene	20.000	0.398	98.0#	2	0.00
83	1,2-Dichlorobenzene	20.000	0.272	98.6#	1	0.00
84	1,2-Dibromo-3-Chloropropane	20.000	0.000	100.0#	0	-12.80#
85	Hexachlorobutadiene	20.000	0.497	97.5#	2	0.00
86	1,2,4-Trichlorobenzene	20.000	0.570	97.2#	2	0.00
87	Naphthalene	20.000	0.356	98.2#	1	0.00
88	1,2,3-Trichlorobenzene	20.000	0.570	97.2#	2	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 6



Calibration Status Report VOA-GCMS9

Method Path : C:\msdchem\1\methods\  
 Method File : VI191025G.M  
 Title : NWTPH-Gx by GC/MS  
 Last Update : Fri Oct 25 10:31:05 2019  
 Response Via : Initial Calibration

#	ID	Conc	ISTD Conc	Path\File
1	50	50	50	C:\msdchem\1\data\2019-10\9J24043\VI19102439.D
2	100	100	50	C:\msdchem\1\data\2019-10\9J24043\VI19102440.D
3	250	250	50	C:\msdchem\1\data\2019-10\9J24043\VI19102441.D
4	500	500	50	C:\msdchem\1\data\2019-10\9J24043\VI19102442.D
5	1000	1000	50	C:\msdchem\1\data\2019-10\9J24043\VI19102452.D
6	2500	2500	50	C:\msdchem\1\data\2019-10\9J24043\VI19102444.D
7	5000	5000	50	C:\msdchem\1\data\2019-10\9J24043\VI19102445.D
8	10K	10000	50	C:\msdchem\1\data\2019-10\9J24043\VI19102446.D

#	ID	Update Time	Quant Time	Acquisition Time
1	50	Oct 25 09:04 2019	Oct 25 08:55 2019	25 Oct 2019 1:46 am
2	100	Oct 25 09:04 2019	Oct 25 08:55 2019	25 Oct 2019 2:13 am
3	250	Oct 25 09:04 2019	Oct 25 08:55 2019	25 Oct 2019 2:40 am
4	500	Oct 25 09:04 2019	Oct 25 08:55 2019	25 Oct 2019 3:07 am
5	1000	Oct 25 10:31 2019	Oct 25 10:30 2019	25 Oct 2019 10:13 am
6	2500	Oct 25 09:04 2019	Oct 25 08:55 2019	25 Oct 2019 4:00 am
7	5000	Oct 25 09:04 2019	Oct 25 08:55 2019	25 Oct 2019 4:27 am
8	10K	Oct 25 09:04 2019	Oct 25 08:55 2019	25 Oct 2019 4:54 am

VI191025G.M Fri Oct 25 10:41:17 2019

Method Path : C:\msdchem\1\methods\  
 Method File : VI191025G.M  
 Title : NWTPH-Gx by GC/MS  
 Last Update : Fri Oct 25 10:31:05 2019  
 Response Via : Initial Calibration

Calibration Files

50 =VI19102439.D 100 =VI19102440.D 250 =VI19102441.D 500 =VI19102442.D 1000=VI19102452.D 2500=VI19102444.D  
 5000=VI19102445.D 10K =VI19102446.D

Compound	50	100	250	500	1000	2500	5000	10K	Avg	%RSD
-----										
1) I Pentafluorobenzene...	-----ISTD-----									
2) S 1,4-Difluorobe...	1.634	1.635	1.620	1.616	1.606	1.628	1.624	1.644	1.626	0.73 /
3) S 4-Bromofluorob...	0.521	0.525	0.529	0.536	0.539	0.555	0.563	0.574	0.543	3.54 /
4) H NWTPH-Gx (TPH)	0.926	1.028	1.244	1.386	1.437	1.550	1.569	1.699	1.355	19.99 /
5) H TPHg (C5-C9)	3.091	2.191	1.950	1.925	1.927	1.943	1.882	1.984	2.112	19.26
6) H TPHg (C6-C10)	2.666	1.908	1.665	1.633	1.632	1.643	1.597	1.694	1.805	20.00 /
7) H CA-LUFT (C5-C12)	3.259	2.422	2.257	2.271	2.291	2.353	2.307	2.441	2.450	13.62 /
8) Benzene (NR)									0.000	-1.00
9) S Toluene-d8 (NR)									0.000	-1.00
10) Toluene (NR)									0.000	-1.00
11) S Chlorobenzene-...									0.000	-1.00
12) S 1,4-Dichlorobe...									0.000	-1.00
13) Naphthalene (NR)									0.000	-1.00

(#) = Out of Range

Compound List Report VOA-GCMS9

Method Path : C:\msdchem\1\methods\  
 Method File : VI191025G.M  
 Title : NWTPH-Gx by GC/MS  
 Last Update : Fri Oct 25 10:31:05 2019  
 Response Via : Initial Calibration

Total Cpnds : 13


PK#	Compound Name	QIon	Exp_RT	Rel_RT	Cal	#Qual	A/H	ID
1	I Pentafluorobenzene (IS)	168	6.217	1.000	A	2	A	B
2	S 1,4-Difluorobenzene (Sur)	114	6.783	1.091	A	2	A	B
3	S 4-Bromofluorobenzene (Sur)	174	10.974	1.765	A	2	A	B
4	H NWTPH-Gx (TPH)	TIC	9.890	1.591	Q	0	A	B
5	H TPHg (C5-C9)	TIC	9.890	1.591	Q	0	A	B
6	H TPHg (C6-C10)	TIC	9.890	1.591	Q	0	A	B
7	H CA-LUFT (C5-C12)	TIC	9.890	1.591	Q	0	A	B
8	Benzene (NR)	78	6.120	0.984	A	2	A	B
9	S Toluene-d8 (NR)	98	8.298	1.335	A	2	A	B
10	Toluene (NR)	91	8.358	1.344	A	2	A	B
11	S Chlorobenzene-d5 (NR)	117	9.916	1.595	A	2	A	B
12	S 1,4-Dichlorobenzene-d4 (NR)	150	11.850	1.906	A	2	A	B
13	Naphthalene (NR)	128	13.627	2.192	A	2	A	B

Cal A = Average L = Linear LO = Linear w/origin Q = Quad QO = Quad w/origin  
 #Qual = number of qualifiers  
 A/H = Area or Height  
 ID R = R.T. B = R.T. & Q Q = Qvalue L = Largest A = All

VI191025G.M Fri Oct 25 10:41:12 2019

NWTPH-Gx (TPH)



Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\REQUANT\  
 Data File : VI19102439.D  
 Acq On : 25 Oct 2019 1:46 am  
 Operator : MM  
 Sample : 9J24043-CALC  
 Misc : 1X 5mL 50PPB GX  
 ALS Vial : 26 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:32:52 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



(4) NWTPH-Gx (TPH) (H)


9.890min ( 0.000) 25.47 ug/L m

response 5099

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

TPHg (C5-C9)

Response Ratio





R = 6.91e-004 A\*A + 1.84e+000 A + 1.03e+000  
Coef of Det (r^2) = 1.000  
Curve Fit: Quadratic w(1/a)  
12/26/19 Anchor OEA, LLC - Gasco Per/D - DG 2019-4c Waste Characterization Page 214 of 919  
Method Name: C:\msdchem\1\methods\VI191025G.M  
Calibration Table Last Updated: Fri Oct 25 10:31:34 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\REQUANT\  
 Data File : VI19102439.D  
 Acq On : 25 Oct 2019 1:46 am  
 Operator : MM  
 Sample : 9J24043-CALC  
 Misc : 1X 5mL 50PPB GX  
 ALS Vial : 26 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:32:52 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



TIC: VI19102439.D\data.ms

(5) TPHg (C5-C9) (H)


9.890min ( 0.000) 19.12 ug/L m

response 362226

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

TPHg (C6-C10)

Response Ratio







Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\REQUANT\  
 Data File : VI19102439.D  
 Acq On : 25 Oct 2019 1:46 am  
 Operator : MM  
 Sample : 9J24043-CALC  
 Misc : 1X 5mL 50PPB GX  
 ALS Vial : 26 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:32:52 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPh-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



TIC: VI19102439.D\data.ms

(6) TPHg (C6-C10) (H)


9.890min ( 0.000) 12.28 ug/L m

response 278598

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

CA-LUFT (C5-C12)

Response Ratio



$R = 1.05e-003 A^2 + 2.22e+000 A + 7.45e-001$

Coef of Det (r^2) = 1.000 Curve Fit: Quadratic w(1/a)



Method Name: C:\msdchem\1\methods\VI191025G.M

Calibration Table Last Updated: Fri Oct 25 10:31:34 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\REQUANT\  
 Data File : VI19102439.D  
 Acq On : 25 Oct 2019 1:46 am  
 Operator : MM  
 Sample : 9J24043-CALC  
 Misc : 1X 5mL 50PPB GX  
 ALS Vial : 26 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:32:52 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



TIC: VI19102439.D\data.ms

(7) CA-LUFT (C5-C12) (H)

9.890min ( 0.000) 22.21 ug/L m

response 362637

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102453.D  
 Acq On : 25 Oct 2019 10:40 am  
 Operator : MM  
 Sample : 9J24043-ICV3  
 Misc : 1X 5mL 500PPB GX  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:55:48 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 15% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I Pentafluorobenzene (IS)	50.000	50.000	0.0	103	0.00
2 S 1,4-Difluorobenzene (Sur)	50.000	49.705	0.6	103	0.00
3 S 4-Bromofluorobenzene (Sur)	50.000	48.785	2.4	102	0.00
4 H NWTPH-Gx (TPH)	500.000	512.008	-2.4	108	0.00
5 H TPHg (C5-C9)	500.000	489.707	2.1	102	0.00
6 H TPHg (C6-C10)	500.000	503.040	-0.6	105	0.00
7 H CA-LUFT (C5-C12)	500.000	493.527	1.3	104	0.00
8 Benzene (NR)	-1.000	0.000	0.0	100	0.00
9 S Toluene-d8 (NR)	-1.000	0.000	0.0	102	0.00
10 Toluene (NR)	-1.000	0.000	0.0	103	0.00
11 S Chlorobenzene-d5 (NR)	-1.000	0.000	0.0	103	0.00
12 S 1,4-Dichlorobenzene-d4 (NR)	-1.000	0.000	0.0	100	0.00
13 Naphthalene (NR)	-1.000	0.000	0.0	114	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9J24043

## Analysis Included

8015D-Mod Gasoline (C6-C10) by GC/MS  
CA LUFT GRO  
NWTPH-Gx

### INSTRUMENT SEQUENCE LOG

<u>SampleID</u>	<u>SampleName</u>	<u>Matrix</u>	<u>STDID</u>	<u>ISTD_ID</u>	<u>Analyzed</u>
9J24043-TUN2	MS Tune	Water		A19I040	10/24/2019 11:59:00PM
9J24043-ICB2	Initial Cal Blank	Water		A19I040	10/25/2019 1:19:00AM
9J24043-CALC	Cal Standard	Water	A19J388	"	10/25/2019 1:46:00AM
9J24043-CALD	Cal Standard	Water	A19J389	"	10/25/2019 2:13:00AM
9J24043-CALE	Cal Standard	Water	A19J390	"	10/25/2019 2:40:00AM
9J24043-CALF	Cal Standard	Water	A19J391	"	10/25/2019 3:07:00AM
9J24043-CALH	Cal Standard	Water	A19J393	"	10/25/2019 4:00:00AM
9J24043-CALI	Cal Standard	Water	A19J394	"	10/25/2019 4:27:00AM
9J24043-CALJ	Cal Standard	Water	A19J395	"	10/25/2019 4:54:00AM
9J24043-CALG	Cal Standard	Water	A19J392	"	10/25/2019 10:13:00AM
9J24043-ICV3	Initial Cal Check	Water	A19G350	"	10/25/2019 10:40:00AM

### CALIBRATION STANDARD RECOVERIES

Calibration: **A9J2503**

Instrument: **VOA-GCMS9**

8015D-Mod Gasoline (C6-C10)

Sequence: **9J24043**

Matrix: **Water**

	<b>Inst. MRL</b>	<b>Recalc Res.</b>	<b>Cal Level</b>	<b>%Rec.</b>	<b>Qual</b>
<b>9J24043-CALC</b>					
<b>9J24043-CALD</b>					
<b>9J24043-CALE</b>					
<b>9J24043-CALF</b>					
<b>9J24043-CALG</b>					
<b>9J24043-CALH</b>					
<b>9J24043-CALI</b>					
<b>9J24043-CALJ</b>					

Compounds listed above have recalculated recoveries outside 70-130% of the true values, and the calibration levels are above the reporting level. If no compounds are listed, all are OK. Please see the next section for quadratic fit compounds.

**CALIBRATION SEQUENCE REVIEW SHEET**

**SEQUENCE: 9J24043**

**Analytes With Quadratic Curve Fits**

Qualifier   iMDL   iMRL   Spike Amt   %Difference   OK?   Raise MRL to ?  
\_\_\_\_\_         \_\_\_\_\_

Analytes listed above have quadratic curve fits. If they are using a weighting option, they must be checked against the requested curve points to determine if the recalculated results are within limits (70-130 or as specified).

**ICV RECOVERIES**

Calibration: **A9J2503**

Instrument: **VOA-GCMS9**

NWTPH-Gx

Sequence: **9J24043**

Matrix: **Water**

**9J24043-ICV3**

<b>Inst. MRL</b>	<b>ICV Level</b>	<b>Result</b>	<b>%Rec.</b>	<b>Qual</b>
------------------	------------------	---------------	--------------	-------------

Compounds listed above have Initial Calibration Verification standard recoveries outside 70-130% of the true values. If no compounds are listed, all have passing recoveries.

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **CA LUFT GRO**

Instrument Cal ID: **VI191025W.M VI191025G.N**

### Pentafluorobenzene (IS)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	209290	4185.800	6.22
9J24043-CALD	50	209478	4189.560	6.22
9J24043-CALE	50	220921	4418.420	6.22
9J24043-CALF	50	214780	4295.600	6.22
9J24043-CALG	50	234293	4685.860	6.22
9J24043-CALH	50	216435	4328.700	6.22
9J24043-CALI	50	233849	4676.980	6.22
9J24043-CALJ	50	234183	4683.660	6.22

**AVE RF 4433.073      RF RSD 4.95      AVE RT 6.22**

### 1,4-Difluorobenzene (Sur)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	341977	1.634	6.78
9J24043-CALD	50	342473	1.635	6.78
9J24043-CALE	50	357958	1.620	6.78
9J24043-CALF	50	347086	1.616	6.78
9J24043-CALG	50	376297	1.606	6.78
9J24043-CALH	50	352248	1.628	6.78
9J24043-CALI	50	379658	1.624	6.78
9J24043-CALJ	50	384961	1.644	6.78

**AVE RF 1.626      RF RSD 0.73      AVE RT 6.78**

### CA LUFT GRO (C5-C12)

Curve Fit: **QUADRATIC: Weighting: (1/a), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	681991	3.259	9.89
9J24043-CALD	100	1014687	2.422	9.89
9J24043-CALE	250	2493143	2.257	9.89
9J24043-CALF	500	4877141	2.271	9.89
9J24043-CALG	1000	1.073362E+07	2.291	9.89
9J24043-CALH	2500	2.54612E+07	2.353	9.89
9J24043-CALI	5000	5.393736E+07	2.307	9.89
9J24043-CALJ	10000	1.143412E+08	2.441	9.89

**AVE RF 2.450      RF RSD 13.62      AVE RT 9.89**

### 4-Bromofluorobenzene (Sur)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	109139	0.521	10.97
9J24043-CALD	50	110020	0.525	10.97
9J24043-CALE	50	116770	0.529	10.97
9J24043-CALF	50	115043	0.536	10.97
9J24043-CALG	50	126230	0.539	10.97
9J24043-CALH	50	120135	0.555	10.97
9J24043-CALI	50	131653	0.563	10.97
9J24043-CALJ	50	134509	0.574	10.97

**AVE RF 0.543      RF RSD 3.54      AVE RT 10.97**

## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**


Calibration Date: **10/25/2019**

Analysis: **NWTPH-Gx**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Pentafluorobenzene (IS)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	209290	4185.800	6.22
9J24043-CALD	50	209478	4189.560	6.22
9J24043-CALE	50	220921	4418.420	6.22
9J24043-CALF	50	214780	4295.600	6.22
9J24043-CALG	50	234293	4685.860	6.22
9J24043-CALH	50	216435	4328.700	6.22
9J24043-CALI	50	233849	4676.980	6.22
9J24043-CALJ	50	234183	4683.660	6.22

**AVE RF 4433.073      RF RSD 4.95      AVE RT 6.22**

### 1,4-Difluorobenzene (Sur)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	341977	1.634	6.78
9J24043-CALD	50	342473	1.635	6.78
9J24043-CALE	50	357958	1.620	6.78
9J24043-CALF	50	347086	1.616	6.78
9J24043-CALG	50	376297	1.606	6.78
9J24043-CALH	50	352248	1.628	6.78
9J24043-CALI	50	379658	1.624	6.78
9J24043-CALJ	50	384961	1.644	6.78

**AVE RF 1.626      RF RSD 0.73      AVE RT 6.78**

### Gasoline Range Organics

Curve Fit: **QUADRATIC: Weighting: (1/a), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	193702	0.926	9.89
9J24043-CALD	100	430822	1.028	9.89
9J24043-CALE	250	1374008	1.244	9.89
9J24043-CALF	500	2976997	1.386	9.89
9J24043-CALG	1000	6735895	1.437	9.89
9J24043-CALH	2500	1.67752E+07	1.550	9.89
9J24043-CALI	5000	3.669824E+07	1.569	9.89
9J24043-CALJ	10000	7.956248E+07	1.699	9.89

**AVE RF 1.355      RF RSD 19.99      AVE RT 9.89**

### 4-Bromofluorobenzene (Sur)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	109139	0.521	10.97
9J24043-CALD	50	110020	0.525	10.97
9J24043-CALE	50	116770	0.529	10.97
9J24043-CALF	50	115043	0.536	10.97
9J24043-CALG	50	126230	0.539	10.97
9J24043-CALH	50	120135	0.555	10.97
9J24043-CALI	50	131653	0.563	10.97
9J24043-CALJ	50	134509	0.574	10.97

**AVE RF 0.543      RF RSD 3.54      AVE RT 10.97**



## Element Calibration Review Sheet

Calibration ID: **A9J2503**

Instrument: **VOA-GCMS9**

Calibration Date: **10/25/2019**


Analysis: **8015D-Mod Gasoline (C6-C1)**

Instrument Cal ID: **VI191025W.M VI191025G.M**

### Pentafluorobenzene (IS)

Curve Fit: **AVERAGE RF**

8015D-Mod Gasoline (C6-C10) by GCMS - Pentafluorobenzene




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	209290	4185.800	6.22
9J24043-CALD	50	209478	4189.560	6.22
9J24043-CALE	50	220921	4418.420	6.22
9J24043-CALF	50	214780	4295.600	6.22
9J24043-CALG	50	234293	4685.860	6.22
9J24043-CALH	50	216435	4328.700	6.22
9J24043-CALI	50	233849	4676.980	6.22
9J24043-CALJ	50	234183	4683.660	6.22

**AVE RF 4433.073      RF RSD 4.95      AVE RT 6.22**

### 1,4-Difluorobenzene (Sur)

Curve Fit: **AVERAGE RF**

8015D-Mod Gasoline (C6-C10) by GCMS - 1,4-Difluorobenzene (S




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	341977	1.634	6.78
9J24043-CALD	50	342473	1.635	6.78
9J24043-CALE	50	357958	1.620	6.78
9J24043-CALF	50	347086	1.616	6.78
9J24043-CALG	50	376297	1.606	6.78
9J24043-CALH	50	352248	1.628	6.78
9J24043-CALI	50	379658	1.624	6.78
9J24043-CALJ	50	384961	1.644	6.78

**AVE RF 1.626      RF RSD 0.73      AVE RT 6.78**

### TPHg (C6-C10)

Curve Fit: **QUADRATIC: Weighting: (1/a), Origin: Ignore**

8015D-Mod Gasoline (C6-C10) by GCMS - TPHg (C6-C10)




Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	557886	2.666	9.89
9J24043-CALD	100	799328	1.908	9.89
9J24043-CALE	250	1839524	1.665	9.89
9J24043-CALF	500	3507779	1.633	9.89
9J24043-CALG	1000	7648071	1.632	9.89
9J24043-CALH	2500	1.778026E+07	1.643	9.89
9J24043-CALI	5000	3.735262E+07	1.597	9.89
9J24043-CALJ	10000	7.933946E+07	1.694	9.89

**AVE RF 1.805      RF RSD 20.00      AVE RT 9.89**

### 4-Bromofluorobenzene (Sur)

Curve Fit: **AVERAGE RF**

3015D-Mod Gasoline (C6-C10) by GCMS - 4-Bromofluorobenzene



Standard	Concentration	Response	Response Factor	RT
9J24043-CALC	50	109139	0.521	10.97
9J24043-CALD	50	110020	0.525	10.97
9J24043-CALE	50	116770	0.529	10.97
9J24043-CALF	50	115043	0.536	10.97
9J24043-CALG	50	126230	0.539	10.97
9J24043-CALH	50	120135	0.555	10.97
9J24043-CALI	50	131653	0.563	10.97
9J24043-CALJ	50	134509	0.574	10.97

**AVE RF 0.543      RF RSD 3.54      AVE RT 10.97**

# Injection Log

Directory: v:\data\2019-10\9J24043

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	Vi19102414.d	1.	9J24043-IBL1	1X 5mL DI	24 Oct 2019 14:34
2	2	Vi19102415.d	1.	9J24043-TUN1	A19I040 BFB (IS/...	24 Oct 2019 15:01
3	3	Vi19102416.d	1.	9J24043-ICB1	1X 5mL DI	24 Oct 2019 15:28
4	4	Vi19102417.d	1.	9J24043-CAL1	1X 5mL 0.1/0.2...	24 Oct 2019 15:55
5	5	Vi19102418.d	1.	9J24043-CAL2	1X 5mL 0.2/0.4...	24 Oct 2019 16:21
6	6	Vi19102419.d	1.	9J24043-CAL3	1X 5mL 0.4/0.8...	24 Oct 2019 16:48
7	7	Vi19102420.d	1.	9J24043-CAL4	1X 5mL 1/2PPB ...	24 Oct 2019 17:15
8	8	Vi19102421.d	1.	9J24043-CAL5	1X 5mL 2/4PPB ...	24 Oct 2019 17:42
9	9	Vi19102422.d	1.	9J24043-CAL6	1X 5mL 5/10PPB...	24 Oct 2019 18:09
10	10	Vi19102423.d	1.	9J24043-CAL7	1X 5mL 10/20PP...	24 Oct 2019 18:36
11	11	Vi19102424.d	1.	9J24043-CAL8	1X 5mL 20/40PP...	24 Oct 2019 19:03
12	12	Vi19102425.d	1.	9J24043-CAL9	1X 5mL 50/100P...	24 Oct 2019 19:30
13	13	Vi19102426.d	1.	9J24043-IBL2	1X 5mL DI	24 Oct 2019 19:57
14	14	Vi19102427.d	1.	9J24043-CALA	1X 5mL 100/200...	24 Oct 2019 20:24
15	15	Vi19102428.d	1.	9J24043-IBL3	1X 5mL DI	24 Oct 2019 20:51
16	16	Vi19102429.d	1.	9J24043-CALB	1X 5mL 200/400...	24 Oct 2019 21:17
17	17	Vi19102430.d	1.	9J24043-IBL4	1X 5mL DI	24 Oct 2019 21:44
18	18	Vi19102431.d	1.	9J24043-IBL5	1X 5mL DI	24 Oct 2019 22:11
19	19	Vi19102432.d	1.	9J24043-ICV1	1X 5mL 20/40PP...	24 Oct 2019 22:38
20	20	Vi19102433.d	1.	9J24043-ICV2	1X 5mL 5/1250P...	24 Oct 2019 23:05
21	21	Vi19102434.d	1.	9J24043-IBL6	1X 5mL DI	24 Oct 2019 23:32
22	22	Vi19102435.d	1.	9J24043-TUN2	A19I040 BFB (IS/...	24 Oct 2019 23:59
23	23	Vi19102436.d	1.	9J24043-RT1	A18A167 VPH RT STD	25 Oct 2019 00:26
24	24	Vi19102437.d	1.	9J24043-IBL7	1X 5mL DI	25 Oct 2019 00:52
25	25	Vi19102438.d	1.	9J24043-ICB2	1X 5mL DI	25 Oct 2019 01:19
26	26	Vi19102439.d	1.	9J24043-CALC	1X 5mL 50PPB GX	25 Oct 2019 01:46
27	27	Vi19102440.d	1.	9J24043-CALD	1X 5mL 100PPB GX	25 Oct 2019 02:13
28	28	Vi19102441.d	1.	9J24043-CALE	1X 5mL 250PPB GX	25 Oct 2019 02:40
29	29	Vi19102442.d	1.	9J24043-CALF	1X 5mL 500PPB GX	25 Oct 2019 03:07
30	30	Vi19102443.d	1.	9J24043-CALG	1X 5mL 1000PPB GX	25 Oct 2019 03:34
31	31	Vi19102444.d	1.	9J24043-CALH	1X 5mL 2500PPB GX	25 Oct 2019 04:00
32	32	Vi19102445.d	1.	9J24043-CALI	1X 5mL 5000PPB GX	25 Oct 2019 04:27
33	33	Vi19102446.d	1.	9J24043-CALJ	1X 5mL 10000PP...	25 Oct 2019 04:54
34	34	Vi19102447.d	1.	9J24043-IBL8	1X 5mL DI	25 Oct 2019 05:21
35	35	Vi19102448.d	1.	9J24043-IBL9	1X 5mL DI	25 Oct 2019 05:48
36	36	Vi19102449.d	1.	9J24043-ICV3	1X 5mL 500PPB GX	25 Oct 2019 06:15
37	37	Vi19102450.d	1.	9J24043-IBLA	1X 5mL DI	25 Oct 2019 06:42

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102414.D  
 Acq On : 24 Oct 2019 2:34 pm  
 Operator : MM  
 Sample : 9J24043-IBL1  
 Misc : 1X 5mL DI  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*NR*


Quant Time: Oct 25 08:52:04 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) Pentafluorobenzene (I)	6.217	99	116268	50.00	ug/L	# 0.00
45) Chlorobenzene-d5 (I)	9.909	117	306026	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	138672	50.00	ug/L	0.00
System Monitoring Compounds						
32) Dibromofluoromethane (S)	5.712	111	110907	48.55	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.783	114	362815	49.39	ug/L	0.00
48) Toluene-d8 (S)	8.297	98	408743	50.89	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	116096	51.81	ug/L	0.00
Target Compounds						
						Qvalue
6) Chloroethane	2.451	64	166	0.14	ug/L	# 58
14) Methylene Chloride	3.868	84	3943	0.99	ug/L	87
15) Acetone	3.948	43	891	0.87	ug/L	93
-----						

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102414.D  
Acq On : 24 Oct 2019 2:34 pm  
Operator : MM  
Sample : 9J24043-IBL1  
Misc : 1X 5mL DI  
ALS Vial : 1 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:04 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration





BFB

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102415.D  
Acq On : 24 Oct 2019 3:01 pm  
Operator : MM  
Sample : 9J24043-TUN1  
Misc : A19I040 BFB (IS/SURR)  
ALS Vial : 2 Sample Multiplier: 1

*MM*  
*10/25/19*

Integration File: RTEINT.P

Method : C:\msdchem\1\methods\VI191025W.M  
Title : EPA 8260: Volatile Organic Compounds  
Last Update : Fri Oct 25 08:32:21 2019



AutoFind: Scans 1543, 1544, 1545; Background Corrected with Scan 1536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
95	174	50	200	117.9	84595	PASS
96	95	5	9	6.8	5736	PASS
173	174	0.00	2	0.4	280	PASS
174	95	50	200	84.8	71757	PASS
175	174	5	9	7.2	5145	PASS
176	174	95	105	97.0	69587	PASS
177	176	5	10	6.5	4525	PASS

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102415.D  
 Acq On : 24 Oct 2019 3:01 pm  
 Operator : MM  
 Sample : 9J24043-TUN1  
 Misc : A19I040 BFB (IS/SURR)  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:12 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

*Handwritten:*  
 W  
 10/25/19


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene (I)	6.217	99	115135	50.00	ug/L	0.00
45) Chlorobenzene-d5 (I)	9.916	117	306446	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	141323	50.00	ug/L	0.00
System Monitoring Compounds						
32) Dibromofluoromethane (S)	5.718	111	110753	48.96	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.783	114	360182	49.52	ug/L	0.00
48) Toluene-d8 (S)	8.297	98	404469	50.29	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	115450	50.56	ug/L	0.00
Target Compounds						
3) Chloromethane	1.904	50	226	0.09	ug/L #	47
6) Chloroethane	2.463	64	432	0.38	ug/L #	36
14) Methylene Chloride	3.875	84	1793	Below Cal	#	76
15) Acetone	3.948	43	857	0.85	ug/L #	44
19) tert-Butanol (TBA)	4.307	59	115	0.26	ug/L	46

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102415.D  
Acq On : 24 Oct 2019 3:01 pm  
Operator : MM  
Sample : 9J24043-TUN1  
Misc : A19I040 BFB (IS/SURR)  
ALS Vial : 2 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:12 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102416.D  
 Acq On : 24 Oct 2019 3:28 pm  
 Operator : MM  
 Sample : 9J24043-ICB1  
 Misc : 1X 5mL DI  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*MM*  
*10/25/19*

Quant Time: Oct 25 08:52:24 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene (I)	6.217	99	109157	50.00	ug/L	# 0.00
45) Chlorobenzene-d5 (I)	9.916	117	292802	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	134268	50.00	ug/L	0.00
System Monitoring Compounds						
32) Dibromofluoromethane (S)	5.712	111	106415	49.62	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.782	114	343590	49.82	ug/L	0.00
48) Toluene-d8 (S)	8.297	98	387024	50.36	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	109949	50.68	ug/L	0.00
Target Compounds						
3) Chloromethane	1.897	50	228	0.10	ug/L	# 47
6) Chloroethane	2.530	64	212	0.19	ug/L	# 36
14) Methylene Chloride	3.868	84	1359	Below Cal		85
15) Acetone	3.948	43	763	0.80	ug/L	# 44

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102416.D  
Acq On : 24 Oct 2019 3:28 pm  
Operator : MM  
Sample : 9J24043-ICB1  
Misc : 1X 5mL DI  
ALS Vial : 3 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:24 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102417.D  
 Acq On : 24 Oct 2019 3:55 pm  
 Operator : MM  
 Sample : 9J24043-CAL1  
 Misc : 1X 5mL 0.1/0.2PPB VOCR  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:17:09 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*MM*  
*10/25/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	116102	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.909	117	307577	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	139681	50.00	ug/L		0.00
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	111441	46.79	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.783	114	364447	54.80	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	406288	51.17	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	116090	51.67	ug/L		0.00
<b>Target Compounds</b>							
							<b>Qvalue</b>
2) Dichlorodifluoromethane	0.000		0	N.D.			
3) Chloromethane	1.897	50	479	0.18	ug/L		91
4) Vinyl Chloride	0.000		0	N.D.	d		
5) Bromomethane	0.000		0	N.D.	d		
6) Chloroethane	0.000		0	N.D.	d		
7) Trichlorofluoromethane	0.000		0	N.D.	d		
8) Ethanol	0.000		0	N.D.	d		
9) 1,1-Dichloroethene	0.000		0	N.D.	d		
10) Carbon Disulfide	0.000		0	N.D.	d		
11) Freon 113	0.000		0	N.D.			
12) Iodomethane	0.000		0	N.D.			
13) Acrolein	0.000		0	N.D.			
14) Methylene Chloride	3.875	84	2024	Below	Cal		84
15) Acetone	0.000		0	N.D.	d		
16) t-1,2-Dichloroethene	0.000		0	N.D.			
17) n-Hexane	0.000		0	N.D.			
18) Methyl-tert-butyl-ether	0.000		0	N.D.	d		
19) tert-Butanol (TBA)	4.300	59	2472	6.89	ug/L		83
20) Diisopropyl ether (DIPE)	0.000		0	N.D.			
21) 1,1-Dichloroethane	0.000		0	N.D.	d		
22) Acrylonitrile	0.000		0	N.D.			
23) Ethyl-tert-butyl ether...	0.000		0	N.D.			
24) Vinyl Acetate	0.000		0	N.D.			
25) c-1,2-Dichloroethene	0.000		0	N.D.			
26) 2,2-Dichloropropane	0.000		0	N.D.			
27) Bromochloromethane	0.000		0	N.D.			
28) Chloroform	0.000		0	N.D.			
29) Carbon Tetrachloride	0.000		0	N.D.			
30) Tetrahydrofuran	0.000		0	N.D.			
31) 1,1,1-Trichloroethane	0.000		0	N.D.			
33) 1,1-Dichloropropene	0.000		0	N.D.			
34) 2-Butanone (MEK)	0.000		0	N.D.	d		
35) Benzene	6.132	78	917	0.12	ug/L		55
36) tert-Amyl methyl ether...	0.000		0	N.D.			
37) 1,2-Dichloroethane (EDC)	0.000		0	N.D.	d		
38) iso-Butyl Alcohol	0.000		0	N.D.			
40) Trichloroethene (TCE)	0.000		0	N.D.			
41) Tert-Amyl-Ethyl-Ether ...	0.000		0	N.D.			
42) Dibromomethane	0.000		0	N.D.			
43) 1,2-Dichloropropane	0.000		0	N.D.			
44) Bromodichloromethane	0.000		0	N.D.			
46) 2-Chloroethyl Vinyl Ether	0.000		0	N.D.			
47) c-1,3-Dichloropropene	0.000		0	N.D.			

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102417.D  
 Acq On : 24 Oct 2019 3:55 pm  
 Operator : MM  
 Sample : 9J24043-CAL1  
 Misc : 1X 5mL 0.1/0.2PPB VOCR  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:17:09 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	978	0.11	ug/L	85
50) Tetrachloroethene (PCE)	0.000		0	N.D.		
51) 4-Methyl-2-Pentanone (...)	0.000		0	N.D.	d	
52) t-1,3-Dichloropropene	0.000		0	N.D.		
53) 1,1,2-Trichloroethane	0.000		0	N.D.		
54) Dibromochloromethane	0.000		0	N.D.		
55) 1,3-Dichloropropane	0.000		0	N.D.	d	
56) 1,2-Dibromoethane (EDB)	0.000		0	N.D.		
57) 2-Hexanone	0.000		0	N.D.		
58) Chlorobenzene	9.934	112	480	0.09	ug/L #	35
59) Ethylbenzene	9.952	91	942	0.10	ug/L	91
60) 1,1,1,2-Tetrachloroethane	0.000		0	N.D.		
61) m,p-Xylenes (2)	10.086	91	1368	0.27	ug/L	84
62) o-Xylene	10.469	91	585	0.15	ug/L	89
63) Styrene	0.000		0	N.D.	d	
64) Bromoform	0.000		0	N.D.		
65) Isopropylbenzene	0.000		0	N.D.	d	
68) Bromobenzene	11.059	156	124	0.06	ug/L #	82
69) n-Propylbenzene	11.078	91	873	0.10	ug/L	58
70) 1,1,2,2-Tetrachloroethane	0.000		0	N.D.		
71) 2-Chlorotoluene	0.000		0	N.D.		
72) 1,3,5-Trimethylbenzene	11.230	105	556	0.10	ug/L	92
73) 1,2,3-Trichloropropane	0.000		0	N.D.		
74) t-1,4-Dichloro-2-butene	0.000		0	N.D.		
75) 4-Chlorotoluene	0.000		0	N.D.	d	
76) tert-Butylbenzene	0.000		0	N.D.	d	
77) 1,2,4-Trimethylbenzene	11.540	105	536	0.17	ug/L	80
78) sec-Butylbenzene	0.000		0	N.D.	d	
79) 4-Isopropyltoluene	11.728	119	481	0.20	ug/L	68
80) 1,3-Dichlorobenzene	0.000		0	N.D.	d	
81) 1,4-Dichlorobenzene	11.868	146	311	0.08	ug/L #	41
82) n-Butylbenzene	12.045	91	379	0.08	ug/L	81
83) 1,2-Dichlorobenzene	0.000		0	N.D.	d	
84) 1,2-Dibromo-3-Chloropr...	0.000		0	N.D.		
85) Hexachlorobutadiene	0.000		0	N.D.		
86) 1,2,4-Trichlorobenzene	0.000		0	N.D.		
87) Naphthalene	0.000		0	N.D.	d	
88) 1,2,3-Trichlorobenzene	0.000		0	N.D.		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102417.D  
 Acq On : 24 Oct 2019 3:55 pm  
 Operator : MM  
 Sample : 9J24043-CAL1  
 Misc : 1X 5mL 0.1/0.2PPB VOCR  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:12 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*MM*  
*10/25/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	116102	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.909	117	307577	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	139681	50.00	ug/L		0.00
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	111441	46.79	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.783	114	364447	54.80	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	406288	51.17	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	116090	51.67	ug/L		0.00
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	0.000		0	N.D.			
3) Chloromethane	1.897	50	479	0.18	ug/L	#	91
4) Vinyl Chloride	2.001	62	158	0.07	ug/L	#	50
5) Bromomethane	2.372	96	279	0.15	ug/L	#	64
6) Chloroethane	2.506	64	114	0.09	ug/L	#	61
7) Trichlorofluoromethane	2.676	101	188	0.05	ug/L	#	27
8) Ethanol	3.236	45	213	4.59	ug/L	#	29
9) 1,1-Dichloroethene	3.236	61	133	0.05	ug/L	#	28
10) Carbon Disulfide	3.254	76	531	0.11	ug/L		78
11) Freon 113	0.000		0	N.D.			
12) Iodomethane	0.000		0	N.D.			
13) Acrolein	0.000		0	N.D.			
14) Methylene Chloride	3.875	84	2024	Below Cal			84
15) Acetone	3.948	43	877	0.88	ug/L	#	44
16) t-1,2-Dichloroethene	0.000		0	N.D.			
17) n-Hexane	0.000		0	N.D.			
18) Methyl-tert-butyl-ether	4.167	73	444	0.08	ug/L		63
19) tert-Butanol (TBA)	4.300	59	2472	6.89	ug/L		83
20) Diisopropyl ether (DIPE)	0.000		0	N.D.			
21) 1,1-Dichloroethane	4.690	63	147	0.04	ug/L	#	48
22) Acrylonitrile	0.000		0	N.D.			
23) Ethyl-tert-butyl ether...	0.000		0	N.D.			
24) Vinyl Acetate	0.000		0	N.D.			
25) c-1,2-Dichloroethene	0.000		0	N.D.			
26) 2,2-Dichloropropane	0.000		0	N.D.			
27) Bromochloromethane	0.000		0	N.D.			
28) Chloroform	0.000		0	N.D.			
29) Carbon Tetrachloride	0.000		0	N.D.			
30) Tetrahydrofuran	0.000		0	N.D.			
31) 1,1,1-Trichloroethane	0.000		0	N.D.			
33) 1,1-Dichloropropene	0.000		0	N.D.			
34) 2-Butanone (MEK)	5.882	43	122	0.08	ug/L		52
35) Benzene	6.132	78	917	0.12	ug/L		55
36) tert-Amyl methyl ether...	0.000		0	N.D.			
37) 1,2-Dichloroethane (EDC)	6.345	62	176	0.05	ug/L		54
38) iso-Butyl Alcohol	0.000		0	N.D.			
40) Trichloroethene (TCE)	0.000		0	N.D.			
41) Tert-Amyl-Ethyl-Ether ...	0.000		0	N.D.			
42) Dibromomethane	0.000		0	N.D.			
43) 1,2-Dichloropropane	0.000		0	N.D.			
44) Bromodichloromethane	0.000		0	N.D.			
46) 2-Chloroethyl Vinyl Ether	0.000		0	N.D.			
47) c-1,3-Dichloropropene	0.000		0	N.D.			

*MM*

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102417.D  
 Acq On : 24 Oct 2019 3:55 pm  
 Operator : MM  
 Sample : 9J24043-CAL1  
 Misc : 1X 5mL 0.1/0.2PPB VOCR  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:10:12 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	978	0.11	ug/L	85
50) Tetrachloroethene (PCE)	0.000		0	N.D.		
51) 4-Methyl-2-Pentanone (...)	8.808	43	433	0.16	ug/L #	43
52) t-1,3-Dichloropropene	0.000		0	N.D.		
53) 1,1,2-Trichloroethane	0.000		0	N.D.		
54) Dibromochloromethane	0.000		0	N.D.		
55) 1,3-Dichloropropane	9.289	76	204	0.06	ug/L #	27
56) 1,2-Dibromoethane (EDB)	0.000		0	N.D.		
57) 2-Hexanone	0.000		0	N.D.		
58) Chlorobenzene	9.934	112	480	0.09	ug/L #	35
59) Ethylbenzene	9.952	91	942	0.10	ug/L	91
60) 1,1,1,2-Tetrachloroethane	0.000		0	N.D.		
61) m,p-Xylenes (2)	10.086	91	1368	0.27	ug/L	84
62) o-Xylene	10.469	91	585	0.15	ug/L	89
63) Styrene	10.524	104	329	0.22	ug/L #	42
64) Bromoform	0.000		0	N.D.		
65) Isopropylbenzene	10.731	105	805	0.22	ug/L	54
68) Bromobenzene	11.059	156	124	0.06	ug/L #	82
69) n-Propylbenzene	11.078	91	873	0.10	ug/L	58
70) 1,1,2,2-Tetrachloroethane	0.000		0	N.D.		
71) 2-Chlorotoluene	0.000		0	N.D.		
72) 1,3,5-Trimethylbenzene	11.230	105	556	0.10	ug/L	92
73) 1,2,3-Trichloropropane	0.000		0	N.D.		
74) t-1,4-Dichloro-2-butene	0.000		0	N.D.		
75) 4-Chlorotoluene	11.339	91	458	0.09	ug/L #	45
76) tert-Butylbenzene	11.485	91	177	0.06	ug/L #	74
77) 1,2,4-Trimethylbenzene	11.540	105	536	0.17	ug/L	80
78) sec-Butylbenzene	11.619	105	687	0.10	ug/L	59
79) 4-Isopropyltoluene	11.728	119	481	0.20	ug/L	68
80) 1,3-Dichlorobenzene	11.801	146	273	0.08	ug/L #	76
81) 1,4-Dichlorobenzene	11.868	146	311	0.08	ug/L #	41
82) n-Butylbenzene	12.045	91	379	0.08	ug/L	81
83) 1,2-Dichlorobenzene	12.185	146	241	0.07	ug/L #	25
84) 1,2-Dibromo-3-Chloropr...	0.000		0	N.D.		
85) Hexachlorobutadiene	0.000		0	N.D.		
86) 1,2,4-Trichlorobenzene	0.000		0	N.D.		
87) Naphthalene	13.633	128	452	0.48	ug/L	81
88) 1,2,3-Trichlorobenzene	0.000		0	N.D.		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102417.D  
Acq On : 24 Oct 2019 3:55 pm  
Operator : MM  
Sample : 9J24043-CAL1  
Misc : 1X 5mL 0.1/0.2PPB VOCR  
ALS Vial : 4 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:12 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102418.D  
 Acq On : 24 Oct 2019 4:21 pm  
 Operator : MM  
 Sample : 9J24043-CAL2  
 Misc : 1X 5mL 0.2/0.4PPB VOCR  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:19:21 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*Handwritten notes:*  
 all  
 10/25/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	Qvalue
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	114788	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.916	117	302974	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	135021	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.718	111	110610	46.98	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.783	114	359462	54.66	ug/L	0.00	
48) Toluene-d8 (S)	8.297	98	403793	51.63	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	113180	52.11	ug/L	0.00	
<b>Target Compounds</b>							
2) Dichlorodifluoromethane	0.000		0	N.D.	d		
3) Chloromethane	1.904	50	669	0.25	ug/L		89
4) Vinyl Chloride	2.007	62	406	0.17	ug/L		91
5) Bromomethane	0.000		0	N.D.	d		
6) Chloroethane	0.000		0	N.D.	d		
7) Trichlorofluoromethane	0.000		0	N.D.	d		
8) Ethanol	0.000		0	N.D.	d		
9) 1,1-Dichloroethene	0.000		0	N.D.	d		
10) Carbon Disulfide	0.000		0	N.D.	d		
11) Freon 113	0.000		0	N.D.	d		
12) Iodomethane	0.000		0	N.D.	d		
13) Acrolein	0.000		0	N.D.	d		
14) Methylene Chloride	3.875	84	2201	Below	Cal		87
15) Acetone	3.954	43	1168	1.18	ug/L		93
16) t-1,2-Dichloroethene	4.045	61	360	0.14	ug/L		74
17) n-Hexane	0.000		0	N.D.	d		
18) Methyl-tert-butyl-ether	0.000		0	N.D.	d		
19) tert-Butanol (TBA)	4.300	59	4690	13.22	ug/L		91
20) Diisopropyl ether (DIPE)	0.000		0	N.D.	d		
21) 1,1-Dichloroethane	0.000		0	N.D.	d		
22) Acrylonitrile	0.000		0	N.D.	d		
23) Ethyl-tert-butyl ether...	0.000		0	N.D.	d		
24) Vinyl Acetate	0.000		0	N.D.	d		
25) c-1,2-Dichloroethene	0.000		0	N.D.	d		
26) 2,2-Dichloropropane	0.000		0	N.D.	d		
27) Bromochloromethane	0.000		0	N.D.	d		
28) Chloroform	5.529	83	587	0.15	ug/L		74
29) Carbon Tetrachloride	0.000		0	N.D.	d		
30) Tetrahydrofuran	0.000		0	N.D.	d		
31) 1,1,1-Trichloroethane	0.000		0	N.D.	d		
33) 1,1-Dichloropropene	0.000		0	N.D.	d		
34) 2-Butanone (MEK)	0.000		0	N.D.	d		
35) Benzene	6.126	78	1584	0.20	ug/L		77
36) tert-Amyl methyl ether...	0.000		0	N.D.	d		
37) 1,2-Dichloroethane (EDC)	0.000		0	N.D.	d		
38) iso-Butyl Alcohol	0.000		0	N.D.	d		
40) Trichloroethene (TCE)	6.752	130	372	0.19	ug/L #		75
41) Tert-Amyl-Ethyl-Ether ...	0.000		0	N.D.	d		
42) Dibromomethane	0.000		0	N.D.	d		
43) 1,2-Dichloropropane	0.000		0	N.D.	d		
44) Bromodichloromethane	0.000		0	N.D.	d		
46) 2-Chloroethyl Vinyl Ether	0.000		0	N.D.	d		
47) c-1,3-Dichloropropene	0.000		0	N.D.	d		

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102418.D  
 Acq On : 24 Oct 2019 4:21 pm  
 Operator : MM  
 Sample : 9J24043-CAL2  
 Misc : 1X 5mL 0.2/0.4PPB VOCR  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:19:21 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.352	91	1744	0.21	ug/L	93
50) Tetrachloroethene (PCE)	8.808	166	267	0.14	ug/L #	25
51) 4-Methyl-2-Pentanone (...)	8.796	43	890	0.33	ug/L	85
52) t-1,3-Dichloropropene	0.000		0	N.D.	d	
53) 1,1,2-Trichloroethane	9.009	97	288	0.14	ug/L #	10
54) Dibromochloromethane	0.000		0	N.D.		
55) 1,3-Dichloropropane	9.289	76	568	0.17	ug/L	84
56) 1,2-Dibromoethane (EDB)	9.423	107	279	0.13	ug/L	84
57) 2-Hexanone	0.000		0	N.D.	d	
58) Chlorobenzene	9.928	112	1045	0.19	ug/L #	25
59) Ethylbenzene	9.952	91	1835	0.21	ug/L	93
60) 1,1,1,2-Tetrachloroethane	9.989	131	129	0.07	ug/L #	74
61) m,p-Xylenes (2)	10.086	91	2470	0.45	ug/L	93
62) o-Xylene	10.469	91	1221	0.26	ug/L	90
63) Styrene	10.518	104	754	0.31	ug/L	82
64) Bromoform	0.000		0	N.D.		
65) Isopropylbenzene	10.737	105	1347	0.29	ug/L	86
68) Bromobenzene	11.059	156	432	0.22	ug/L	89
69) n-Propylbenzene	11.078	91	1649	0.19	ug/L	94
70) 1,1,2,2-Tetrachloroethane	11.138	85	305	0.17	ug/L #	75
71) 2-Chlorotoluene	0.000		0	N.D.	d	
72) 1,3,5-Trimethylbenzene	11.230	105	1127	0.20	ug/L	79
73) 1,2,3-Trichloropropane	0.000		0	N.D.		
74) t-1,4-Dichloro-2-butene	0.000		0	N.D.		
75) 4-Chlorotoluene	11.339	91	1020	0.20	ug/L	80
76) tert-Butylbenzene	11.485	91	602	0.19	ug/L #	77
77) 1,2,4-Trimethylbenzene	11.540	105	1066	0.27	ug/L	83
78) sec-Butylbenzene	11.619	105	1301	0.19	ug/L	81
79) 4-Isopropyltoluene	11.722	119	919	0.29	ug/L	98
80) 1,3-Dichlorobenzene	11.802	146	629	0.18	ug/L	91
81) 1,4-Dichlorobenzene	11.862	146	725	0.19	ug/L #	31
82) n-Butylbenzene	12.045	91	805	0.17	ug/L	79
83) 1,2-Dichlorobenzene	12.185	146	624	0.19	ug/L	90
84) 1,2-Dibromo-3-Chloropr...	0.000		0	N.D.		
85) Hexachlorobutadiene	0.000		0	N.D.		
86) 1,2,4-Trichlorobenzene	13.347	180	244	0.16	ug/L	66
87) Naphthalene	13.627	128	924	0.58	ug/L	81
88) 1,2,3-Trichlorobenzene	13.791	180	261	0.17	ug/L	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102418.D  
 Acq On : 24 Oct 2019 4:21 pm  
 Operator : MM  
 Sample : 9J24043-CAL2  
 Misc : 1X 5mL 0.2/0.4PPB VOCR  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:16 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*MM*  
*10/25/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	114788	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.916	117	302974	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	135021	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.718	111	110610	46.98	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.783	114	359462	54.66	ug/L	0.00	
48) Toluene-d8 (S)	8.297	98	403793	51.63	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	113180	52.11	ug/L	0.00	
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.685	85	202	0.09	ug/L	#	49
3) Chloromethane	1.904	50	669	0.25	ug/L		89
4) Vinyl Chloride	2.007	62	406	0.17	ug/L		91
5) Bromomethane	2.366	96	403	0.22	ug/L	#	8
6) Chloroethane	2.512	64	534	0.44	ug/L	#	62
7) Trichlorofluoromethane	2.670	101	442	0.12	ug/L	#	76
8) Ethanol	3.242	45	573	12.50	ug/L	#	29
9) 1,1-Dichloroethene	3.236	61	354	0.12	ug/L	#	62
10) Carbon Disulfide	3.260	76	912	0.19	ug/L		78
11) Freon 113	3.297	101	119	0.06	ug/L	#	19
12) Iodomethane	0.000		0	N.D.			
13) Acrolein	0.000		0	N.D.			
14) Methylene Chloride	3.875	84	2201	Below Cal			87
15) Acetone	3.954	43	1168	1.18	ug/L		93
16) t-1,2-Dichloroethene	4.045	61	360	0.14	ug/L		74
17) n-Hexane	0.000		0	N.D.			
18) Methyl-tert-butyl-ether	4.167	73	1035	0.18	ug/L		63
19) tert-Butanol (TBA)	4.300	59	4690	13.22	ug/L		91
20) Diisopropyl ether (DIPE)	0.000		0	N.D.			
21) 1,1-Dichloroethane	4.690	63	650	0.18	ug/L	#	48
22) Acrylonitrile	0.000		0	N.D.			
23) Ethyl-tert-butyl ether...	0.000		0	N.D.			
24) Vinyl Acetate	4.982	43	476	0.11	ug/L		74
25) c-1,2-Dichloroethene	5.243	61	345	0.12	ug/L	#	70
26) 2,2-Dichloropropane	5.359	77	299	0.12	ug/L	#	30
27) Bromochloromethane	0.000		0	N.D.			
28) Chloroform	5.529	83	587	0.15	ug/L		74
29) Carbon Tetrachloride	5.675	117	123	0.05	ug/L	#	14
30) Tetrahydrofuran	0.000		0	N.D.			
31) 1,1,1-Trichloroethane	5.730	97	415	0.13	ug/L	#	25
33) 1,1-Dichloropropene	5.864	75	388	0.15	ug/L	#	43
34) 2-Butanone (MEK)	5.876	43	395	0.26	ug/L		52
35) Benzene	6.126	78	1584	0.20	ug/L		77
36) tert-Amyl methyl ether...	0.000		0	N.D.			
37) 1,2-Dichloroethane (EDC)	6.351	62	371	0.12	ug/L		54
38) iso-Butyl Alcohol	6.387	43	468	3.43	ug/L		89
40) Trichloroethene (TCE)	6.752	130	372	0.19	ug/L	#	75
41) Tert-Amyl-Ethyl-Ether ...	0.000		0	N.D.			
42) Dibromomethane	7.196	93	115	0.08	ug/L	#	2
43) 1,2-Dichloropropane	7.312	63	259	0.12	ug/L	#	35
44) Bromodichloromethane	7.379	83	222	0.08	ug/L	#	27
46) 2-Chloroethyl Vinyl Ether	0.000		0	N.D.			
47) c-1,3-Dichloropropene	8.097	75	326	0.11	ug/L	#	31

*Cal*

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102418.D  
 Acq On : 24 Oct 2019 4:21 pm  
 Operator : MM  
 Sample : 9J24043-CAL2  
 Misc : 1X 5mL 0.2/0.4PPB VOCR  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:10:16 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.352	91	1744	0.21	ug/L	93
50) Tetrachloroethene (PCE)	8.808	166	267	0.14	ug/L #	25
51) 4-Methyl-2-Pentanone (...)	8.796	43	890	0.33	ug/L	85
52) t-1,3-Dichloropropene	8.839	75	300	0.11	ug/L #	45
53) 1,1,2-Trichloroethane	9.009	97	288	0.14	ug/L #	10
54) Dibromochloromethane	0.000		0	N.D.		
55) 1,3-Dichloropropane	9.289	76	568	0.17	ug/L	84
56) 1,2-Dibromoethane (EDB)	9.423	107	279	0.13	ug/L	84
57) 2-Hexanone	9.666	43	516	0.27	ug/L #	35
58) Chlorobenzene	9.928	112	1045	0.19	ug/L #	25
59) Ethylbenzene	9.952	91	1835	0.21	ug/L	93
60) 1,1,1,2-Tetrachloroethane	9.989	131	129	0.07	ug/L #	74
61) m,p-Xylenes (2)	10.086	91	2470	0.45	ug/L	93
62) o-Xylene	10.469	91	1221	0.26	ug/L	90
63) Styrene	10.518	104	754	0.31	ug/L	82
64) Bromoform	0.000		0	N.D.		
65) Isopropylbenzene	10.737	105	1347	0.29	ug/L	86
68) Bromobenzene	11.059	156	432	0.22	ug/L	89
69) n-Propylbenzene	11.078	91	1649	0.19	ug/L	94
70) 1,1,2,2-Tetrachloroethane	11.138	85	305	0.17	ug/L #	75
71) 2-Chlorotoluene	11.211	126	229	0.14	ug/L #	88
72) 1,3,5-Trimethylbenzene	11.230	105	1127	0.20	ug/L	79
73) 1,2,3-Trichloropropane	0.000		0	N.D.		
74) t-1,4-Dichloro-2-butene	0.000		0	N.D.		
75) 4-Chlorotoluene	11.339	91	1020	0.20	ug/L	80
76) tert-Butylbenzene	11.485	91	602	0.19	ug/L #	77
77) 1,2,4-Trimethylbenzene	11.540	105	1066	0.27	ug/L	83
78) sec-Butylbenzene	11.619	105	1301	0.19	ug/L	81
79) 4-Isopropyltoluene	11.722	119	919	0.29	ug/L	98
80) 1,3-Dichlorobenzene	11.802	146	629	0.18	ug/L	91
81) 1,4-Dichlorobenzene	11.862	146	725	0.19	ug/L #	31
82) n-Butylbenzene	12.045	91	805	0.17	ug/L	79
83) 1,2-Dichlorobenzene	12.185	146	624	0.19	ug/L	90
84) 1,2-Dibromo-3-Chloropr...	0.000		0	N.D.		
85) Hexachlorobutadiene	0.000		0	N.D.		
86) 1,2,4-Trichlorobenzene	13.347	180	244	0.16	ug/L	66
87) Naphthalene	13.627	128	924	0.58	ug/L	81
88) 1,2,3-Trichlorobenzene	13.791	180	261	0.17	ug/L	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102418.D  
Acq On : 24 Oct 2019 4:21 pm  
Operator : MM  
Sample : 9J24043-CAL2  
Misc : 1X 5mL 0.2/0.4PPB VOCR  
ALS Vial : 5 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:16 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102419.D  
 Acq On : 24 Oct 2019 4:48 pm  
 Operator : MM  
 Sample : 9J24043-CAL3  
 Misc : 1X 5mL 0.4/0.8PPB VOCR  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:21:58 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*Handwritten notes:*  
 cal  
 10/25/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.211	99	111985	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.910	117	294372	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	134501	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	108083	47.05	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.777	114	352302	54.92	ug/L	-0.01	
48) Toluene-d8 (S)	8.297	98	396027	52.12	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	112304	51.91	ug/L	0.00	
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.672	85	562	0.26	ug/L		90
3) Chloromethane	1.891	50	1136	0.44	ug/L		91
4) Vinyl Chloride	1.995	62	967	0.42	ug/L		83
5) Bromomethane	2.360	96	839	0.47	ug/L		69
6) Chloroethane	0.000		0	N.D.	d		
7) Trichlorofluoromethane	2.664	101	958	0.26	ug/L		86
8) Ethanol	3.230	45	1315	29.40	ug/L		96
9) 1,1-Dichloroethene	3.230	61	1038	0.37	ug/L		87
10) Carbon Disulfide	0.000		0	N.D.	d		
11) Freon 113	0.000		0	N.D.	d		
12) Iodomethane	0.000		0	N.D.	d		
13) Acrolein	0.000		0	N.D.	d		
14) Methylene Chloride	3.869	84	2646	Below	Cal		89
15) Acetone	3.948	43	1616	1.67	ug/L		96
16) t-1,2-Dichloroethene	4.039	61	963	0.38	ug/L		98
17) n-Hexane	0.000		0	N.D.	d		
18) Methyl-tert-butyl-ether	4.167	73	2309	0.41	ug/L		94
19) tert-Butanol (TBA)	4.294	59	10086	29.13	ug/L		91
20) Diisopropyl ether (DIPE)	4.562	45	638	0.11	ug/L		76
21) 1,1-Dichloroethane	4.684	63	1323	0.37	ug/L		87
22) Acrylonitrile	0.000		0	N.D.	d		
23) Ethyl-tert-butyl ether...	0.000		0	N.D.	d		
24) Vinyl Acetate	0.000		0	N.D.	d		
25) c-1,2-Dichloroethene	5.244	61	1008	0.36	ug/L		91
26) 2,2-Dichloropropane	5.347	77	853	0.34	ug/L		76
27) Bromochloromethane	5.444	130	391	0.28	ug/L		94
28) Chloroform	5.529	83	1292	0.34	ug/L		95
29) Carbon Tetrachloride	5.651	117	618	0.24	ug/L		90
30) Tetrahydrofuran	0.000		0	N.D.	d		
31) 1,1,1-Trichloroethane	5.730	97	1012	0.32	ug/L		93
33) 1,1-Dichloropropene	5.870	75	1049	0.41	ug/L	#	43
34) 2-Butanone (MEK)	0.000		0	N.D.	d		
35) Benzene	6.120	78	3381	0.44	ug/L		99
36) tert-Amyl methyl ether...	6.247	73	580	0.11	ug/L	#	21
37) 1,2-Dichloroethane (EDC)	6.332	62	1073	0.34	ug/L		54
38) iso-Butyl Alcohol	6.387	43	1172	8.80	ug/L		84
40) Trichloroethene (TCE)	6.746	130	718	0.37	ug/L		74
41) Tert-Amyl-Ethyl-Ether ...	0.000		0	N.D.	d		
42) Dibromomethane	7.202	93	378	0.27	ug/L		86
43) 1,2-Dichloropropane	7.312	63	797	0.38	ug/L		95
44) Bromodichloromethane	7.379	83	800	0.29	ug/L		93
46) 2-Chloroethyl Vinyl Ether	8.036	63	359	1.00	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	1014	0.36	ug/L		89

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102419.D  
 Acq On : 24 Oct 2019 4:48 pm  
 Operator : MM  
 Sample : 9J24043-CAL3  
 Misc : 1X 5mL 0.4/0.8PPB VOCR  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:21:58 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	3505	0.43	ug/L	93
50) Tetrachloroethene (PCE)	8.796	166	787	0.42	ug/L	94
51) 4-Methyl-2-Pentanone (...)	8.808	43	1912	0.73	ug/L	91
52) t-1,3-Dichloropropene	8.839	75	610	0.22	ug/L #	45
53) 1,1,2-Trichloroethane	9.003	97	717	0.36	ug/L	82
54) Dibromochloromethane	9.186	129	505	0.24	ug/L	86
55) 1,3-Dichloropropane	9.289	76	1253	0.38	ug/L	95
56) 1,2-Dibromoethane (EDB)	9.423	107	615	0.30	ug/L	96
57) 2-Hexanone	9.660	43	1346	0.71	ug/L	91
58) Chlorobenzene	9.928	112	2226	0.43	ug/L #	64
59) Ethylbenzene	9.952	91	3584	0.42	ug/L	99
60) 1,1,1,2-Tetrachloroethane	9.989	131	470	0.26	ug/L #	66
61) m,p-Xylenes (2)	10.086	91	5197	0.91	ug/L	96
62) o-Xylene	10.469	91	2605	0.49	ug/L	93
63) Styrene	10.518	104	1656	0.51	ug/L	93
64) Bromoform	0.000		0	N.D.	d	
65) Isopropylbenzene	10.731	105	3067	0.54	ug/L	92
68) Bromobenzene	11.059	156	875	0.45	ug/L	92
69) n-Propylbenzene	11.078	91	3544	0.42	ug/L	99
70) 1,1,2,2-Tetrachloroethane	11.139	85	671	0.38	ug/L	87
71) 2-Chlorotoluene	11.205	126	719	0.43	ug/L	98
72) 1,3,5-Trimethylbenzene	11.230	105	2289	0.41	ug/L	92
73) 1,2,3-Trichloropropane	11.248	110	271	0.32	ug/L	91
74) t-1,4-Dichloro-2-butene	0.000		0	N.D.		
75) 4-Chlorotoluene	11.339	91	2178	0.44	ug/L	99
76) tert-Butylbenzene	11.485	91	1248	0.40	ug/L	99
77) 1,2,4-Trimethylbenzene	11.540	105	2387	0.51	ug/L	98
78) sec-Butylbenzene	11.619	105	2990	0.44	ug/L	97
79) 4-Isopropyltoluene	11.729	119	2236	0.56	ug/L	92
80) 1,3-Dichlorobenzene	11.802	146	1412	0.41	ug/L	95
81) 1,4-Dichlorobenzene	11.862	146	1564	0.42	ug/L #	54
82) n-Butylbenzene	12.045	91	1867	0.40	ug/L	85
83) 1,2-Dichlorobenzene	12.185	146	1284	0.39	ug/L	95
84) 1,2-Dibromo-3-Chloropr...	0.000		0	N.D.		
85) Hexachlorobutadiene	0.000		0	N.D.		
86) 1,2,4-Trichlorobenzene	13.347	180	615	0.40	ug/L	89
87) Naphthalene	13.633	128	2009	0.81	ug/L	81
88) 1,2,3-Trichlorobenzene	13.779	180	687	0.45	ug/L	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102419.D  
 Acq On : 24 Oct 2019 4:48 pm  
 Operator : MM  
 Sample : 9J24043-CAL3  
 Misc : 1X 5mL 0.4/0.8PPB VOCR  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:19 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*MM*  
*10/25/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.211	99	111985	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.910	117	294372	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	134501	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	108083	47.05	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.777	114	352302	54.92	ug/L	-0.01	
48) Toluene-d8 (S)	8.297	98	396027	52.12	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	112304	51.91	ug/L	0.00	
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.672	85	562	0.26	ug/L		90
3) Chloromethane	1.891	50	1136	0.44	ug/L		91
4) Vinyl Chloride	1.995	62	967	0.42	ug/L		83
5) Bromomethane	2.360	96	839	0.47	ug/L		69
6) Chloroethane	2.512	64	672	0.57	ug/L #		66
7) Trichlorofluoromethane	2.664	101	958	0.26	ug/L		86
8) Ethanol	3.230	45	1315	29.40	ug/L		96
9) 1,1-Dichloroethene	3.230	61	1038	0.37	ug/L		87
10) Carbon Disulfide	3.242	76	1798	0.39	ug/L		78
11) Freon 113	3.285	101	569	0.31	ug/L #		63
12) Iodomethane	0.000		0	N.D.			
13) Acrolein	0.000		0	N.D.			
14) Methylene Chloride	3.869	84	2646	Below Cal			89
15) Acetone	3.948	43	1616	1.67	ug/L		96
16) t-1,2-Dichloroethene	4.039	61	963	0.38	ug/L		98
17) n-Hexane	0.000		0	N.D.			
18) Methyl-tert-butyl-ether	4.167	73	2309	0.41	ug/L		94
19) tert-Butanol (TBA)	4.294	59	10086	29.13	ug/L		91
20) Diisopropyl ether (DIPE)	4.562	45	638	0.11	ug/L		76
21) 1,1-Dichloroethane	4.684	63	1323	0.37	ug/L		87
22) Acrylonitrile	4.751	53	129	0.12	ug/L #		15
23) Ethyl-tert-butyl ether...	4.945	59	438	0.09	ug/L #		38
24) Vinyl Acetate	4.964	43	1231	0.29	ug/L		74
25) c-1,2-Dichloroethene	5.244	61	1008	0.36	ug/L		91
26) 2,2-Dichloropropane	5.347	77	853	0.34	ug/L		76
27) Bromochloromethane	5.444	130	391	0.28	ug/L		94
28) Chloroform	5.529	83	1292	0.34	ug/L		95
29) Carbon Tetrachloride	5.651	117	618	0.24	ug/L		90
30) Tetrahydrofuran	5.712	42	281	0.30	ug/L #		62
31) 1,1,1-Trichloroethane	5.730	97	1012	0.32	ug/L		93
33) 1,1-Dichloropropene	5.870	75	1049	0.41	ug/L #		43
34) 2-Butanone (MEK)	5.864	43	1016	0.69	ug/L		52
35) Benzene	6.120	78	3381	0.44	ug/L		99
36) tert-Amyl methyl ether...	6.247	73	580	0.11	ug/L #		21
37) 1,2-Dichloroethane (EDC)	6.332	62	1073	0.34	ug/L		54
38) iso-Butyl Alcohol	6.387	43	1172	8.80	ug/L		84
40) Trichloroethene (TCE)	6.746	130	718	0.37	ug/L		74
41) Tert-Amyl-Ethyl-Ether ...	0.000		0	N.D.			
42) Dibromomethane	7.202	93	378	0.27	ug/L		86
43) 1,2-Dichloropropane	7.312	63	797	0.38	ug/L		95
44) Bromodichloromethane	7.379	83	800	0.29	ug/L		93
46) 2-Chloroethyl Vinyl Ether	8.036	63	359	1.00	ug/L #		100
47) c-1,3-Dichloropropene	8.091	75	1014	0.36	ug/L		89

*MM*

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102419.D  
 Acq On : 24 Oct 2019 4:48 pm  
 Operator : MM  
 Sample : 9J24043-CAL3  
 Misc : 1X 5mL 0.4/0.8PPB VOCR  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:10:19 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev (Min)
49) Toluene	8.358	91	3505	0.43	ug/L	93
50) Tetrachloroethene (PCE)	8.796	166	787	0.42	ug/L	94
51) 4-Methyl-2-Pentanone (...)	8.808	43	1912	0.73	ug/L	91
52) t-1,3-Dichloropropene	8.839	75	610	0.22	ug/L #	45
53) 1,1,2-Trichloroethane	9.003	97	717	0.36	ug/L	82
54) Dibromochloromethane	9.186	129	505	0.24	ug/L	86
55) 1,3-Dichloropropane	9.289	76	1253	0.38	ug/L	95
56) 1,2-Dibromoethane (EDB)	9.423	107	615	0.30	ug/L	96
57) 2-Hexanone	9.660	43	1346	0.71	ug/L	91
58) Chlorobenzene	9.928	112	2226	0.43	ug/L #	64
59) Ethylbenzene	9.952	91	3584	0.42	ug/L	99
60) 1,1,1,2-Tetrachloroethane	9.989	131	470	0.26	ug/L #	66
61) m,p-Xylenes (2)	10.086	91	5197	0.91	ug/L	96
62) o-Xylene	10.469	91	2605	0.49	ug/L	93
63) Styrene	10.518	104	1656	0.51	ug/L	93
64) Bromoform	10.542	173	215	0.15	ug/L #	36
65) Isopropylbenzene	10.731	105	3067	0.54	ug/L	92
68) Bromobenzene	11.059	156	875	0.45	ug/L	92
69) n-Propylbenzene	11.078	91	3544	0.42	ug/L	99
70) 1,1,2,2-Tetrachloroethane	11.139	85	671	0.38	ug/L	87
71) 2-Chlorotoluene	11.205	126	719	0.43	ug/L	98
72) 1,3,5-Trimethylbenzene	11.230	105	2289	0.41	ug/L	92
73) 1,2,3-Trichloropropane	11.248	110	271	0.32	ug/L	91
74) t-1,4-Dichloro-2-butene	0.000		0	N.D.		
75) 4-Chlorotoluene	11.339	91	2178	0.44	ug/L	99
76) tert-Butylbenzene	11.485	91	1248	0.40	ug/L	99
77) 1,2,4-Trimethylbenzene	11.540	105	2387	0.51	ug/L	98
78) sec-Butylbenzene	11.619	105	2990	0.44	ug/L	97
79) 4-Isopropyltoluene	11.729	119	2236	0.56	ug/L	92
80) 1,3-Dichlorobenzene	11.802	146	1412	0.41	ug/L	95
81) 1,4-Dichlorobenzene	11.862	146	1564	0.42	ug/L #	54
82) n-Butylbenzene	12.045	91	1867	0.40	ug/L	85
83) 1,2-Dichlorobenzene	12.185	146	1284	0.39	ug/L	95
84) 1,2-Dibromo-3-Chloropr...	0.000		0	N.D.		
85) Hexachlorobutadiene	0.000		0	N.D.		
86) 1,2,4-Trichlorobenzene	13.347	180	615	0.40	ug/L	89
87) Naphthalene	13.633	128	2009	0.81	ug/L	81
88) 1,2,3-Trichlorobenzene	13.779	180	687	0.45	ug/L	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102419.D  
Acq On : 24 Oct 2019 4:48 pm  
Operator : MM  
Sample : 9J24043-CAL3  
Misc : 1X 5mL 0.4/0.8PPB VOCR  
ALS Vial : 6 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:19 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration





Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102420.D  
 Acq On : 24 Oct 2019 5:15 pm  
 Operator : MM  
 Sample : 9J24043-CAL4  
 Misc : 1X 5mL 1/2PPB VOCR  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:23 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*Handwritten:*  
 10/25/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.211	99	116043	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.910	117	310797	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	143979	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	111608	46.89	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.783	114	366642	55.15	ug/L	0.00	
48) Toluene-d8 (S)	8.298	98	410518	51.17	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	118563	51.20	ug/L	0.00	
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.679	85	1583	0.69	ug/L		98
3) Chloromethane	1.892	50	2407	0.90	ug/L		90
4) Vinyl Chloride	1.995	62	2351	0.98	ug/L		95
5) Bromomethane	2.360	96	1763	0.95	ug/L	#	71
6) Chloroethane	<del>2.500</del>	<del>64</del>	<del>2425</del>	1.99	ug/L		75
7) Trichlorofluoromethane	2.664	101	2784	0.73	ug/L		90
8) Ethanol	3.236	45	3446	74.35	ug/L		88
9) 1,1-Dichloroethene	3.230	61	2476	0.85	ug/L		86
10) Carbon Disulfide	3.248	76	4573	0.95	ug/L		96
11) Freon 113	3.285	101	1717	0.90	ug/L		98
12) Iodomethane	0.000		0	N.D.			
13) Acrolein	3.625	56	420	1.01	ug/L		60
14) Methylene Chloride	3.869	84	3939	Below	Cal		91
15) Acetone	3.948	43	2940	2.94	ug/L		92
16) t-1,2-Dichloroethene	4.039	61	2657	1.01	ug/L		94
17) n-Hexane	4.124	86	357	1.11	ug/L	#	60
18) Methyl-tert-butyl-ether	4.167	73	5789	1.00	ug/L		81
19) tert-Butanol (TBA)	4.295	59	25977	72.41	ug/L		88
20) Diisopropyl ether (DIPE)	4.562	45	1604	0.27	ug/L		98
21) 1,1-Dichloroethane	4.684	63	3672	0.99	ug/L		94
22) Acrylonitrile	4.751	53	876	0.80	ug/L		79
23) Ethyl-tert-butyl ether...	4.939	59	1449	0.28	ug/L		83
24) Vinyl Acetate	4.964	43	3620	0.82	ug/L		88
25) c-1,2-Dichloroethene	5.244	61	2744	0.95	ug/L		83
26) 2,2-Dichloropropane	5.353	77	2316	0.90	ug/L		92
27) Bromochloromethane	5.450	130	1188	0.83	ug/L		88
28) Chloroform	5.530	83	3341	0.84	ug/L		98
29) Carbon Tetrachloride	5.663	117	1791	0.66	ug/L		91
30) Tetrahydrofuran	5.706	42	945	0.99	ug/L		87
31) 1,1,1-Trichloroethane	5.730	97	2903	0.89	ug/L		93
33) 1,1-Dichloropropene	5.864	75	2749	1.05	ug/L		93
34) 2-Butanone (MEK)	5.858	43	2900	1.90	ug/L		90
35) Benzene	6.126	78	8314	1.05	ug/L		96
36) tert-Amyl methyl ether...	6.247	73	1462	0.28	ug/L		60
37) 1,2-Dichloroethane (EDC)	6.339	62	2623	0.81	ug/L		91
38) iso-Butyl Alcohol	6.375	43	3120	22.60	ug/L		86
40) Trichloroethene (TCE)	6.740	130	2166	1.08	ug/L		94
41) Tert-Amyl-Ethyl-Ether ...	6.996	59	950	0.29	ug/L		74
42) Dibromomethane	7.196	93	1285	0.90	ug/L		96
43) 1,2-Dichloropropane	7.306	63	1944	0.91	ug/L		93
44) Bromodichloromethane	7.379	83	2259	0.78	ug/L		96
46) 2-Chloroethyl Vinyl Ether	8.030	63	1378	1.78	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	2667	0.91	ug/L		93

*Handwritten:*  
 Qdel

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102420.D  
 Acq On : 24 Oct 2019 5:15 pm  
 Operator : MM  
 Sample : 9J24043-CAL4  
 Misc : 1X 5mL 1/2PPB VOCR  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:23 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration




Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.352	91	9040	1.04	ug/L	99
50) Tetrachloroethene (PCE)	8.796	166	1994	1.00	ug/L	91
51) 4-Methyl-2-Pentanone (...)	8.802	43	5042	1.83	ug/L	93
52) t-1,3-Dichloropropene	8.839	75	2122	0.72	ug/L	95
53) 1,1,2-Trichloroethane	9.003	97	1944	0.93	ug/L	92
54) Dibromochloromethane	9.186	129	1349	0.61	ug/L	88
55) 1,3-Dichloropropane	9.289	76	3361	0.96	ug/L	93
56) 1,2-Dibromoethane (EDB)	9.423	107	1928	0.90	ug/L	93
57) 2-Hexanone	9.660	43	3526	1.77	ug/L	99
58) Chlorobenzene	9.928	112	5770	1.05	ug/L	93
59) Ethylbenzene	9.952	91	9335	1.03	ug/L	97
60) 1,1,1,2-Tetrachloroethane	9.989	131	1476	0.77	ug/L	91
61) m,p-Xylenes (2)	10.086	91	12789	2.05	ug/L	99
62) o-Xylene	10.463	91	6630	1.11	ug/L	97
63) Styrene	10.518	104	4878	1.15	ug/L	95
64) Bromoform	10.536	173	795	0.51	ug/L	91
65) Isopropylbenzene	10.731	105	7662	1.14	ug/L	98
68) Bromobenzene	11.059	156	2220	1.07	ug/L	88
69) n-Propylbenzene	11.078	91	9160	1.02	ug/L	99
70) 1,1,2,2-Tetrachloroethane	11.139	85	1876	1.00	ug/L	85
71) 2-Chlorotoluene	11.205	126	1910	1.07	ug/L	98
72) 1,3,5-Trimethylbenzene	11.230	105	6197	1.03	ug/L	90
73) 1,2,3-Trichloropropane	11.248	110	887	0.97	ug/L	97
74) t-1,4-Dichloro-2-butene	11.285	53	531	0.74	ug/L #	41
75) 4-Chlorotoluene	11.339	91	5461	1.02	ug/L	98
76) tert-Butylbenzene	11.485	91	3551	1.07	ug/L	94
77) 1,2,4-Trimethylbenzene	11.534	105	6319	1.16	ug/L	93
78) sec-Butylbenzene	11.619	105	7450	1.03	ug/L	98
79) 4-Isopropyltoluene	11.729	119	6086	1.25	ug/L	98
80) 1,3-Dichlorobenzene	11.796	146	3650	1.00	ug/L	96
81) 1,4-Dichlorobenzene	11.863	146	4177	1.04	ug/L	86
82) n-Butylbenzene	12.045	91	4997	1.00	ug/L	93
83) 1,2-Dichlorobenzene	12.185	146	3650	1.04	ug/L	97
84) 1,2-Dibromo-3-Chloropr...	12.799	157	447	0.82	ug/L #	69
85) Hexachlorobutadiene	13.310	223	443	0.91	ug/L	96
86) 1,2,4-Trichlorobenzene	13.347	180	1833	1.10	ug/L	94
87) Naphthalene	13.627	128	5345	1.42	ug/L	98
88) 1,2,3-Trichlorobenzene	13.785	180	1879	1.15	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102420.D  
 Acq On : 24 Oct 2019 5:15 pm  
 Operator : MM  
 Sample : 9J24043-CAL4  
 Misc : 1X 5mL 1/2PPB VOCR  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:23 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration



TIC: VI19102420.D\data.ms

(59) Ethylbenzene (C)

9.952min (+ 0.000) 1.03 ug/L

response 9335




*M.2*

Ion	Exp%	Act%
91.10	100.00	100.00
106.10	30.80	32.98
51.10	10.40	11.11
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102420.D  
 Acq On : 24 Oct 2019 5:15 pm  
 Operator : MM  
 Sample : 9J24043-CAL4  
 Misc : 1X 5mL 1/2PPB VOCR  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:23 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration



TIC: VI19102420.D\data.ms

(59) Ethylbenzene (C)




9.952min (+ 0.000)	0.96 ug/L	m
response	8761	
Ion	Exp%	Act%
91.10	100.00	100.00
106.10	30.80	32.98
51.10	10.40	11.11
0.00	0.00	0.00

*Handwritten signature/initials*

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102421.D  
 Acq On : 24 Oct 2019 5:42 pm  
 Operator : MM  
 Sample : 9J24043-CAL5  
 Misc : 1X 5mL 2/4PPB VOCR  
 ALS Vial : 8 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:26 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration



TIC: VI19102421.D\data.ms

(8) Ethanol

3.242min (+ 0.007) 157.83 ug/L

response 6984




*M.2.*

Ion	Exp%	Act%
45.00	100.00	100.00
46.00	47.50	36.12
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102421.D  
 Acq On : 24 Oct 2019 5:42 pm  
 Operator : MM  
 Sample : 9J24043-CAL5  
 Misc : 1X 5mL 2/4PPB VOCR  
 ALS Vial : 8 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:26 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration



TIC: VI19102421.D\data.ms

(8) Ethanol

3.242min (+ 0.007) 163.37 ug/L/m


response 7229

*Handwritten signature/initials*

Ion	Exp%	Act%
45.00	100.00	100.00
46.00	47.50	36.12
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102420.D  
Acq On : 24 Oct 2019 5:15 pm  
Operator : MM  
Sample : 9J24043-CAL4  
Misc : 1X 5mL 1/2PPB VOCR  
ALS Vial : 7 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:23 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102421.D  
 Acq On : 24 Oct 2019 5:42 pm  
 Operator : MM  
 Sample : 9J24043-CAL5  
 Misc : 1X 5mL 2/4PPB VOCR  
 ALS Vial : 8 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*MM*  
*10/25/19*

Quant Time: Oct 25 08:10:26 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	110790	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.916	117	297754	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	139582	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.718	111	108776	47.86	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.783	114	347212	54.71	ug/L	0.00	
48) Toluene-d8 (S)	8.297	98	395017	51.39	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	115163	51.29	ug/L	0.00	
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.691	85	3731	1.71	ug/L		97
3) Chloromethane	1.904	50	4743	1.85	ug/L		90
4) Vinyl Chloride	2.007	62	5030	2.20	ug/L		95
5) Bromomethane	2.372	96	3140	1.78	ug/L		93
6) Chloroethane	2.524	64	2540	2.19	ug/L		82
7) Trichlorofluoromethane	2.682	101	5667	1.55	ug/L		97
8) Ethanol	3.242	45	<del>6984</del> 729	157.83	ug/L		83
9) 1,1-Dichloroethene	3.242	61	5263	1.88	ug/L		96
10) Carbon Disulfide	3.260	76	9757	2.13	ug/L		99
11) Freon 113	3.297	101	3803	2.08	ug/L		95
12) Iodomethane	<del>3.400</del>	<del>142</del>	<del>130</del>	5.22	ug/L	#	47
13) Acrolein	3.625	56	927	2.34	ug/L		71
14) Methylene Chloride	3.881	84	6151	Below	Cal		89
15) Acetone	3.948	43	4523	4.74	ug/L		93
16) t-1,2-Dichloroethene	4.051	61	5503	2.20	ug/L		91
17) n-Hexane	4.130	86	709	2.31	ug/L	#	84
18) Methyl-tert-butyl-ether	4.173	73	11957	2.16	ug/L		93
19) tert-Butanol (TBA)	4.301	59	58093	169.62	ug/L		94
20) Diisopropyl ether (DIPE)	4.568	45	3305	0.59	ug/L		95
21) 1,1-Dichloroethane	4.690	63	7227	2.05	ug/L		100
22) Acrylonitrile	4.763	53	1949	1.87	ug/L		96
23) Ethyl-tert-butyl ether...	4.939	59	3145	0.63	ug/L		96
24) Vinyl Acetate	4.964	43	7854	1.87	ug/L		99
25) c-1,2-Dichloroethene	5.250	61	5568	2.02	ug/L		93
26) 2,2-Dichloropropane	5.353	77	4776	1.94	ug/L		95
27) Bromochloromethane	5.456	130	2679	1.97	ug/L		99
28) Chloroform	5.536	83	7277	1.92	ug/L		99
29) Carbon Tetrachloride	5.663	117	4001	1.54	ug/L		98
30) Tetrahydrofuran	5.706	42	2045	2.23	ug/L		88
31) 1,1,1-Trichloroethane	5.736	97	5937	1.90	ug/L		97
33) 1,1-Dichloropropene	5.870	75	5724	2.28	ug/L		95
34) 2-Butanone (MEK)	5.870	43	6243	4.29	ug/L		98
35) Benzene	6.126	78	17935	2.38	ug/L		94
36) tert-Amyl methyl ether...	6.247	73	2996	0.60	ug/L		72
37) 1,2-Dichloroethane (EDC)	6.345	62	5726	1.86	ug/L		98
38) iso-Butyl Alcohol	6.381	43	7968	60.45	ug/L		93
40) Trichloroethene (TCE)	6.746	130	4576	2.38	ug/L		95
41) Tert-Amyl-Ethyl-Ether ...	7.002	59	2147	0.68	ug/L		90
42) Dibromomethane	7.202	93	2755	2.01	ug/L		88
43) 1,2-Dichloropropane	7.312	63	4373	2.13	ug/L		93
44) Bromodichloromethane	7.385	83	4681	1.70	ug/L		94
46) 2-Chloroethyl Vinyl Ether	8.030	63	2589	2.82	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	5578	1.98	ug/L		90

*add*



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102421.D  
 Acq On : 24 Oct 2019 5:42 pm  
 Operator : MM  
 Sample : 9J24043-CAL5  
 Misc : 1X 5mL 2/4PPB VOCR  
 ALS Vial : 8 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:26 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	17851	2.14	ug/L	99
50) Tetrachloroethene (PCE)	8.796	166	4333	2.28	ug/L	92
51) 4-Methyl-2-Pentanone (...)	8.809	43	11029	4.18	ug/L	98
52) t-1,3-Dichloropropene	8.839	75	4500	1.60	ug/L	95
53) 1,1,2-Trichloroethane	9.003	97	4134	2.06	ug/L	93
54) Dibromochloromethane	9.192	129	3038	1.44	ug/L	91
55) 1,3-Dichloropropane	9.289	76	6889	2.05	ug/L	90
56) 1,2-Dibromoethane (EDB)	9.429	107	4499	2.18	ug/L	100
57) 2-Hexanone	9.660	43	7610	3.99	ug/L	92
58) Chlorobenzene	9.928	112	11701	2.22	ug/L	98
59) Ethylbenzene	9.952	91	19157	2.20	ug/L	95
60) 1,1,1,2-Tetrachloroethane	9.989	131	2985	1.63	ug/L	94
61) m,p-Xylenes (2)	10.086	91	27092	4.47	ug/L	98
62) o-Xylene	10.469	91	13605	2.31	ug/L	96
63) Styrene	10.518	104	10363	2.35	ug/L	98
64) Bromoform	10.536	173	1771	1.19	ug/L	90
65) Isopropylbenzene	10.731	105	16325	2.39	ug/L	97
68) Bromobenzene	11.059	156	4634	2.30	ug/L	83
69) n-Propylbenzene	11.078	91	19292	2.21	ug/L	99
70) 1,1,2,2-Tetrachloroethane	11.139	85	4008	2.20	ug/L	91
71) 2-Chlorotoluene	11.205	126	4172	2.40	ug/L	98
72) 1,3,5-Trimethylbenzene	11.230	105	13089	2.24	ug/L	97
73) 1,2,3-Trichloropropane	11.248	110	1935	2.17	ug/L	93
74) t-1,4-Dichloro-2-butene	11.278	53	1313	1.90	ug/L #	50
75) 4-Chlorotoluene	11.339	91	11718	2.26	ug/L	99
76) tert-Butylbenzene	11.485	91	7395	2.30	ug/L	98
77) 1,2,4-Trimethylbenzene	11.534	105	12974	2.38	ug/L	98
78) sec-Butylbenzene	11.619	105	15756	2.25	ug/L	99
79) 4-Isopropyltoluene	11.729	119	12523	2.53	ug/L	97
80) 1,3-Dichlorobenzene	11.802	146	7718	2.18	ug/L	97
81) 1,4-Dichlorobenzene	11.862	146	8550	2.20	ug/L	91
82) n-Butylbenzene	12.045	91	10626	2.18	ug/L	98
83) 1,2-Dichlorobenzene	12.185	146	7854	2.32	ug/L	97
84) 1,2-Dibromo-3-Chloropr...	12.799	157	1006	1.90	ug/L	77
85) Hexachlorobutadiene	13.304	223	963	2.05	ug/L	87
86) 1,2,4-Trichlorobenzene	13.341	180	4043	2.51	ug/L	89
87) Naphthalene	13.627	128	12724	2.92	ug/L	97
88) 1,2,3-Trichlorobenzene	13.785	180	4073	2.58	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102421.D  
Acq On : 24 Oct 2019 5:42 pm  
Operator : MM  
Sample : 9J24043-CAL5  
Misc : 1X 5mL 2/4PPB VOCR  
ALS Vial : 8 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:26 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102422.D  
 Acq On : 24 Oct 2019 6:09 pm  
 Operator : MM  
 Sample : 9J24043-CAL6  
 Misc : 1X 5mL 5/10PPB VOCR  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*MM*  
*10/25/19*




Quant Time: Oct 25 08:10:29 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (I)	6.211	99	111010	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.910	117	300317	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	141843	50.00	ug/L	0.00	
System Monitoring Compounds							
32) Dibromofluoromethane (S)	5.712	111	109232	47.97	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.777	114	353918	55.65	ug/L	-0.01	
48) Toluene-d8 (S)	8.297	98	397005	51.21	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	115652	50.69	ug/L	0.00	
Target Compounds							
							Qvalue
2) Dichlorodifluoromethane	1.679	85	9010	4.13	ug/L		98
3) Chloromethane	1.891	50	11370	4.42	ug/L		96
4) Vinyl Chloride	1.995	62	12653	5.52	ug/L		96
5) Bromomethane	2.360	96	7782	4.40	ug/L		97
6) Chloroethane	2.506	64	5899	5.07	ug/L		79
7) Trichlorofluoromethane	2.664	101	14236	3.89	ug/L		96
8) Ethanol	3.230	45	17243	388.90	ug/L		85
9) 1,1-Dichloroethene	3.230	61	13321	4.75	ug/L		93
10) Carbon Disulfide	3.248	76	24060	5.23	ug/L		98
11) Freon 113	3.291	101	9544	5.22	ug/L		91
12) Iodomethane	3.382	142	916	6.05	ug/L	#	79
13) Acrolein	3.619	56	2465	6.22	ug/L		88
14) Methylene Chloride	3.869	84	12549	2.62	ug/L		87
15) Acetone	3.942	43	10355	10.83	ug/L		98
16) t-1,2-Dichloroethene	4.039	61	13685	5.45	ug/L		96
17) n-Hexane	4.118	86	1836	5.97	ug/L		92
18) Methyl-tert-butyl-ether	4.167	73	29908	5.40	ug/L		93
19) tert-Butanol (TBA)	4.288	59	143817	419.08	ug/L		97
20) Diisopropyl ether (DIPE)	4.568	45	8576	1.52	ug/L		93
21) 1,1-Dichloroethane	4.684	63	18307	5.17	ug/L		95
22) Acrylonitrile	4.751	53	5426	5.19	ug/L		98
23) Ethyl-tert-butyl ether...	4.939	59	8071	1.61	ug/L		98
24) Vinyl Acetate	4.958	43	20467	4.86	ug/L		97
25) c-1,2-Dichloroethene	5.244	61	13959	5.05	ug/L		90
26) 2,2-Dichloropropane	5.353	77	11793	4.78	ug/L		98
27) Bromochloromethane	5.444	130	7172	5.26	ug/L		96
28) Chloroform	5.529	83	18186	4.79	ug/L		96
29) Carbon Tetrachloride	5.657	117	9957	3.83	ug/L		96
30) Tetrahydrofuran	5.706	42	5112	5.57	ug/L		83
31) 1,1,1-Trichloroethane	5.730	97	14957	4.77	ug/L		94
33) 1,1-Dichloropropene	5.864	75	14423	5.74	ug/L		94
34) 2-Butanone (MEK)	5.858	43	15638	10.72	ug/L		94
35) Benzene	6.120	78	43404	5.74	ug/L		97
36) tert-Amyl methyl ether...	6.247	73	7445	1.48	ug/L		89
37) 1,2-Dichloroethane (EDC)	6.339	62	14359	4.65	ug/L		90
38) iso-Butyl Alcohol	6.375	43	<del>18074</del> 26719	6.86	ug/L		98
40) Trichloroethene (TCE)	6.740	130	11340	5.89	ug/L		97
41) Tert-Amyl-Ethyl-Ether ...	6.996	59	5331	1.68	ug/L		83
42) Dibromomethane	7.196	93	7023	5.12	ug/L		97
43) 1,2-Dichloropropane	7.306	63	10897	5.31	ug/L		88
44) Bromodichloromethane	7.379	83	12021	4.36	ug/L		95
46) 2-Chloroethyl Vinyl Ether	8.024	63	7592	6.83	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	14229	5.00	ug/L		87

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102422.D  
 Acq On : 24 Oct 2019 6:09 pm  
 Operator : MM  
 Sample : 9J24043-CAL6  
 Misc : 1X 5mL 5/10PPB VOCR  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:29 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration



TIC: VI19102422.D\data.ms

(38) iso-Butyl Alcohol

6.375min (+ 0.000) 136.86 ug/L




response	18074		
Ion	Exp%	Act%	
43.10	100.00	100.00	
41.10	78.60	80.03	
74.10	11.20	9.63	
0.00	0.00	0.00	

*Handwritten signature/initials: A-2*

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102422.D  
 Acq On : 24 Oct 2019 6:09 pm  
 Operator : MM  
 Sample : 9J24043-CAL6  
 Misc : 1X 5mL 5/10PPB VOCR  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:29 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration



TIC: VI19102422.D\data.ms

(38) iso-Butyl Alcohol

6.375min (+ 0.000)	156.81 ug/L	m
response	20710	
Ion	Exp%	Act%
43.10	100.00	100.00
41.10	78.60	80.03
74.10	11.20	9.63
0.00	0.00	0.00

*MM*  
*10/25/19*

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102422.D  
 Acq On : 24 Oct 2019 6:09 pm  
 Operator : MM  
 Sample : 9J24043-CAL6  
 Misc : 1X 5mL 5/10PPB VOCR  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:10:29 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	44272	5.27	ug/L	100
50) Tetrachloroethene (PCE)	8.796	166	10847	5.65	ug/L	90
51) 4-Methyl-2-Pentanone (...)	8.796	43	28183	10.59	ug/L	97
52) t-1,3-Dichloropropene	8.839	75	12130	4.29	ug/L	98
53) 1,1,2-Trichloroethane	9.003	97	10336	5.11	ug/L	93
54) Dibromochloromethane	9.186	129	8016	3.77	ug/L	99
55) 1,3-Dichloropropane	9.289	76	17551	5.18	ug/L	88
56) 1,2-Dibromoethane (EDB)	9.423	107	11270	5.42	ug/L	98
57) 2-Hexanone	9.654	43	19724	10.24	ug/L	92
58) Chlorobenzene	9.928	112	29555	5.55	ug/L	97
59) Ethylbenzene	9.952	91	46860	5.34	ug/L	98
60) 1,1,1,2-Tetrachloroethane	9.989	131	7981	4.33	ug/L	94
61) m,p-Xylenes (2)	10.086	91	68847	11.15	ug/L	99
62) o-Xylene	10.463	91	34456	5.68	ug/L	99
63) Styrene	10.512	104	26739	5.76	ug/L	98
64) Bromoform	10.536	173	4690	3.11	ug/L	97
65) Isopropylbenzene	10.731	105	41801	5.88	ug/L	99
68) Bromobenzene	11.059	156	11623	5.69	ug/L	87
69) n-Propylbenzene	11.072	91	48000	5.40	ug/L	98
70) 1,1,2,2-Tetrachloroethane	11.139	85	9843	5.31	ug/L	96
71) 2-Chlorotoluene	11.205	126	10150	5.76	ug/L	90
72) 1,3,5-Trimethylbenzene	11.230	105	33314	5.62	ug/L	97
73) 1,2,3-Trichloropropane	11.248	110	4862	5.37	ug/L	96
74) t-1,4-Dichloro-2-butene	11.278	53	3293	4.68	ug/L #	57
75) 4-Chlorotoluene	11.339	91	30239	5.73	ug/L	95
76) tert-Butylbenzene	11.479	91	18808	5.76	ug/L	94
77) 1,2,4-Trimethylbenzene	11.540	105	34216	6.04	ug/L	97
78) sec-Butylbenzene	11.619	105	40240	5.67	ug/L	98
79) 4-Isopropyltoluene	11.729	119	33176	6.39	ug/L	99
80) 1,3-Dichlorobenzene	11.796	146	19712	5.49	ug/L	98
81) 1,4-Dichlorobenzene	11.862	146	20421	5.17	ug/L	94
82) n-Butylbenzene	12.045	91	28526	5.77	ug/L	98
83) 1,2-Dichlorobenzene	12.185	146	19460	5.65	ug/L	98
84) 1,2-Dibromo-3-Chloropr...	12.799	157	2728	5.06	ug/L	90
85) Hexachlorobutadiene	13.304	223	2715	5.67	ug/L	94
86) 1,2,4-Trichlorobenzene	13.347	180	11114	6.78	ug/L	93
87) Naphthalene	13.627	128	32892	6.76	ug/L	97
88) 1,2,3-Trichlorobenzene	13.785	180	10402	6.49	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102422.D  
Acq On : 24 Oct 2019 6:09 pm  
Operator : MM  
Sample : 9J24043-CAL6  
Misc : 1X 5mL 5/10PPB VOCR  
ALS Vial : 9 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:29 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102423.D  
 Acq On : 24 Oct 2019 6:36 pm  
 Operator : MM  
 Sample : 9J24043-CAL7  
 Misc : 1X 5mL 10/20PPB VOCR  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:32 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*MM*  
*10/25/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	117608	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.909	117	312833	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	149215	50.00	ug/L		0.00
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	113697	47.13	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.782	114	367409	54.53	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	415174	51.41	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	121121	50.47	ug/L		0.00
<b>Target Compounds</b>							
							<b>Qvalue</b>
2) Dichlorodifluoromethane	1.678	85	18118	7.84	ug/L		99
3) Chloromethane	1.897	50	22449	8.25	ug/L		98
4) Vinyl Chloride	2.001	62	25149	10.35	ug/L		96
5) Bromomethane	2.360	96	14678	7.84	ug/L		99
6) Chloroethane	2.500	64	11813	9.58	ug/L		80
7) Trichlorofluoromethane	2.664	101	29038	7.49	ug/L		94
8) Ethanol	3.236	45	34617	736.96	ug/L		86
9) 1,1-Dichloroethene	3.230	61	27243	9.18	ug/L		93
10) Carbon Disulfide	3.248	76	49011	10.06	ug/L		98
11) Freon 113	3.284	101	19612	10.13	ug/L		99
12) Iodomethane	3.388	142	3125	8.20	ug/L		93
13) Acrolein	3.619	56	4855	11.57	ug/L		76
14) Methylene Chloride	3.868	84	22701	7.47	ug/L		90
15) Acetone	3.941	43	19796	19.53	ug/L		95
16) t-1,2-Dichloroethene	4.039	61	27372	10.29	ug/L		93
17) n-Hexane	4.124	86	4034	12.37	ug/L		92
18) Methyl-tert-butyl-ether	4.167	73	61557	10.49	ug/L		95
19) tert-Butanol (TBA)	4.294	59	292252	803.84	ug/L		99
20) Diisopropyl ether (DIPE)	4.568	45	17135	2.87	ug/L		96
21) 1,1-Dichloroethane	4.684	63	36999	9.87	ug/L		97
22) Acrylonitrile	4.744	53	11383	10.28	ug/L		91
23) Ethyl-tert-butyl ether...	4.939	59	16756	3.15	ug/L		98
24) Vinyl Acetate	4.957	43	42656	9.56	ug/L		97
25) c-1,2-Dichloroethene	5.243	61	28723	9.81	ug/L		90
26) 2,2-Dichloropropane	5.353	77	23663	9.05	ug/L		99
27) Bromochloromethane	5.450	130	14961	10.35	ug/L		91
28) Chloroform	5.529	83	37799	9.40	ug/L		97
29) Carbon Tetrachloride	5.657	117	20840	7.56	ug/L		94
30) Tetrahydrofuran	5.700	42	10375	10.67	ug/L		83
31) 1,1,1-Trichloroethane	5.736	97	30210	9.09	ug/L		97
33) 1,1-Dichloropropene	5.864	75	29295	11.00	ug/L		95
34) 2-Butanone (MEK)	5.858	43	31158	20.17	ug/L		96
35) Benzene	6.119	78	87359	10.91	ug/L		96
36) tert-Amyl methyl ether...	6.247	73	15349	2.88	ug/L		94
37) 1,2-Dichloroethane (EDC)	6.338	62	28935	8.85	ug/L		92
38) iso-Butyl Alcohol	6.375	43	39286	280.78	ug/L		94
40) Trichloroethene (TCE)	6.740	130	23449	11.49	ug/L		96
41) Tert-Amyl-Ethyl-Ether ...	7.001	59	11032	3.28	ug/L		85
42) Dibromomethane	7.196	93	14594	10.04	ug/L		95
43) 1,2-Dichloropropane	7.312	63	21915	10.08	ug/L		94
44) Bromodichloromethane	7.379	83	25055	8.58	ug/L		99
46) 2-Chloroethyl Vinyl Ether	8.023	63	15685	12.76	ug/L	#	100
47) c-1,3-Dichloropropene	8.090	75	30482	10.29	ug/L		89



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102423.D  
 Acq On : 24 Oct 2019 6:36 pm  
 Operator : MM  
 Sample : 9J24043-CAL7  
 Misc : 1X 5mL 10/20PPB VOCR  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:10:32 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	90400	10.33	ug/L	100
50) Tetrachloroethene (PCE)	8.796	166	22099	11.06	ug/L	92
51) 4-Methyl-2-Pentanone (...)	8.802	43	58009	20.92	ug/L	92
52) t-1,3-Dichloropropene	8.839	75	26302	8.92	ug/L	96
53) 1,1,2-Trichloroethane	9.009	97	21402	10.15	ug/L	91
54) Dibromochloromethane	9.192	129	17208	7.78	ug/L	98
55) 1,3-Dichloropropane	9.289	76	36354	10.31	ug/L	92
56) 1,2-Dibromoethane (EDB)	9.423	107	22884	10.57	ug/L	92
57) 2-Hexanone	9.654	43	41881	20.88	ug/L	91
58) Chlorobenzene	9.928	112	60359	10.89	ug/L	98
59) Ethylbenzene	9.952	91	96018	10.49	ug/L	97
60) 1,1,1,2-Tetrachloroethane	9.988	131	16995	8.86	ug/L	94
61) m,p-Xylenes (2)	10.086	91	142004	21.90	ug/L	100
62) o-Xylene	10.463	91	71417	11.16	ug/L	99
63) Styrene	10.512	104	57022	11.55	ug/L	96
64) Bromoform	10.536	173	10701	6.82	ug/L	97
65) Isopropylbenzene	10.731	105	86673	11.50	ug/L	99
68) Bromobenzene	11.059	156	24222	11.27	ug/L	89
69) n-Propylbenzene	11.071	91	99009	10.59	ug/L	99
70) 1,1,2,2-Tetrachloroethane	11.138	85	20098	10.31	ug/L	97
71) 2-Chlorotoluene	11.205	126	21625	11.66	ug/L	93
72) 1,3,5-Trimethylbenzene	11.230	105	69892	11.21	ug/L	98
73) 1,2,3-Trichloropropane	11.248	110	10162	10.68	ug/L	92
74) t-1,4-Dichloro-2-butene	11.278	53	6985	9.43	ug/L #	66
75) 4-Chlorotoluene	11.339	91	61742	11.13	ug/L	98
76) tert-Butylbenzene	11.479	91	38411	11.19	ug/L	96
77) 1,2,4-Trimethylbenzene	11.534	105	70882	11.77	ug/L	98
78) sec-Butylbenzene	11.619	105	83977	11.24	ug/L	99
79) 4-Isopropyltoluene	11.728	119	68628	12.35	ug/L	98
80) 1,3-Dichlorobenzene	11.795	146	41299	10.93	ug/L	98
81) 1,4-Dichlorobenzene	11.862	146	42771	10.30	ug/L	96
82) n-Butylbenzene	12.045	91	59515	11.45	ug/L	98
83) 1,2-Dichlorobenzene	12.179	146	40125	11.07	ug/L	99
84) 1,2-Dibromo-3-Chloropr...	12.799	157	6234	10.99	ug/L	83
85) Hexachlorobutadiene	13.304	223	5468	10.86	ug/L	93
86) 1,2,4-Trichlorobenzene	13.347	180	23133	13.41	ug/L	99
87) Naphthalene	13.626	128	72324	13.49	ug/L	97
88) 1,2,3-Trichlorobenzene	13.785	180	22293	13.22	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102423.D  
Acq On : 24 Oct 2019 6:36 pm  
Operator : MM  
Sample : 9J24043-CAL7  
Misc : 1X 5mL 10/20PPB VOCR  
ALS Vial : 10 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:32 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102424.D  
 Acq On : 24 Oct 2019 7:03 pm  
 Operator : MM  
 Sample : 9J24043-CAL8  
 Misc : 1X 5mL 20/40PPB VOCR  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:35 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*Handwritten:*  
 10/25/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.211	99	112406	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.910	117	307093	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	151591	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	109549	47.51	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.777	114	354922	55.12	ug/L	-0.01	
48) Toluene-d8 (S)	8.298	98	399810	50.43	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	120976	49.61	ug/L	0.00	
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.673	85	35982	16.29	ug/L		98
3) Chloromethane	1.892	50	45062	17.32	ug/L		97
4) Vinyl Chloride	1.995	62	49916	21.50	ug/L		96
5) Bromomethane	2.354	96	27599	15.42	ug/L		98
6) Chloroethane	2.488	64	19851	16.84	ug/L		80
7) Trichlorofluoromethane	2.658	101	58162	15.70	ug/L		96
8) Ethanol	3.230	45	70360	1567.21	ug/L		87
9) 1,1-Dichloroethene	3.230	61	54074	19.06	ug/L		94
10) Carbon Disulfide	3.242	76	98898	21.25	ug/L		98
11) Freon 113	3.279	101	39711	21.45	ug/L		97
12) Iodomethane	3.382	142	11472	16.74	ug/L		96
13) Acrolein	3.613	56	10458	26.07	ug/L		77
14) Methylene Chloride	3.869	84	43598	19.20	ug/L		88
15) Acetone	3.936	43	39380	40.66	ug/L		94
16) t-1,2-Dichloroethene	4.033	61	56066	22.05	ug/L		94
17) n-Hexane	4.118	86	8308	26.66	ug/L		95
18) Methyl-tert-butyl-ether	4.167	73	123669	22.05	ug/L		95
19) tert-Butanol (TBA)	4.289	59	614954	1769.71	ug/L		97
20) Diisopropyl ether (DIPE)	4.562	45	34871	6.10	ug/L		94
21) 1,1-Dichloroethane	4.678	63	75120	20.96	ug/L		96
22) Acrylonitrile	4.745	53	22973	21.71	ug/L		97
23) Ethyl-tert-butyl ether...	4.939	59	33471	6.59	ug/L		98
24) Vinyl Acetate	4.952	43	90141	21.14	ug/L		97
25) c-1,2-Dichloroethene	5.238	61	58359	20.86	ug/L		92
26) 2,2-Dichloropropane	5.347	77	48254	19.80	ug/L		97
27) Bromochloromethane	5.444	130	30935	22.39	ug/L		93
28) Chloroform	5.523	83	76239	19.85	ug/L		97
29) Carbon Tetrachloride	5.657	117	43938	16.68	ug/L		92
30) Tetrahydrofuran	5.700	42	21330	22.95	ug/L		89
31) 1,1,1-Trichloroethane	5.730	97	62000	19.52	ug/L		96
33) 1,1-Dichloropropene	5.858	75	59019	23.19	ug/L		96
34) 2-Butanone (MEK)	5.852	43	64474	43.67	ug/L		98
35) Benzene	6.120	78	175817	22.96	ug/L		96
36) tert-Amyl methyl ether...	6.247	73	30296	5.94	ug/L		96
37) 1,2-Dichloroethane (EDC)	6.339	62	58731	18.79	ug/L		91
38) iso-Butyl Alcohol	6.369	43	83527	624.61	ug/L		94
40) Trichloroethene (TCE)	6.740	130	47359	24.28	ug/L		92
41) Tert-Amyl-Ethyl-Ether ...	6.996	59	22696	7.05	ug/L		83
42) Dibromomethane	7.196	93	29514	21.24	ug/L		94
43) 1,2-Dichloropropane	7.306	63	44422	21.38	ug/L		92
44) Bromodichloromethane	7.379	83	51693	18.52	ug/L		94
46) 2-Chloroethyl Vinyl Ether	8.018	63	33274	26.29	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	64475	22.18	ug/L		87

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102424.D  
 Acq On : 24 Oct 2019 7:03 pm  
 Operator : MM  
 Sample : 9J24043-CAL8  
 Misc : 1X 5mL 20/40PPB VOCR  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:10:35 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	183309	21.33	ug/L	100
50) Tetrachloroethene (PCE)	8.796	166	45467	23.17	ug/L	91
51) 4-Methyl-2-Pentanone (...)	8.796	43	120524	44.27	ug/L	94
52) t-1,3-Dichloropropene	8.833	75	57085	19.72	ug/L	96
53) 1,1,2-Trichloroethane	9.003	97	43171	20.86	ug/L	95
54) Dibromochloromethane	9.186	129	36932	17.00	ug/L	99
55) 1,3-Dichloropropane	9.289	76	73700	21.29	ug/L	92
56) 1,2-Dibromoethane (EDB)	9.423	107	46797	22.02	ug/L	95
57) 2-Hexanone	9.654	43	87528	44.45	ug/L	92
58) Chlorobenzene	9.928	112	120984	22.23	ug/L	99
59) Ethylbenzene	9.952	91	195460	21.76	ug/L	96
60) 1,1,1,2-Tetrachloroethane	9.989	131	36336	19.29	ug/L	96
61) m,p-Xylenes (2)	10.086	91	297066	46.05	ug/L	100
62) o-Xylene	10.463	91	149422	23.36	ug/L	99
63) Styrene	10.512	104	120205	24.26	ug/L	98
64) Bromoform	10.536	173	23844	15.48	ug/L	97
65) Isopropylbenzene	10.731	105	182751	24.16	ug/L	100
68) Bromobenzene	11.060	156	50013	22.90	ug/L	89
69) n-Propylbenzene	11.072	91	210703	22.19	ug/L	100
70) 1,1,2,2-Tetrachloroethane	11.139	85	41819	21.12	ug/L	95
71) 2-Chlorotoluene	11.206	126	45664	24.23	ug/L	95
72) 1,3,5-Trimethylbenzene	11.230	105	148694	23.48	ug/L	98
73) 1,2,3-Trichloropropane	11.248	110	20199	20.89	ug/L	96
74) t-1,4-Dichloro-2-butene	11.279	53	14515	19.29	ug/L #	73
75) 4-Chlorotoluene	11.339	91	129933	23.05	ug/L	99
76) tert-Butylbenzene	11.479	91	81742	23.44	ug/L	95
77) 1,2,4-Trimethylbenzene	11.534	105	151018	24.30	ug/L	97
78) sec-Butylbenzene	11.619	105	180894	23.84	ug/L	99
79) 4-Isopropyltoluene	11.729	119	151382	26.15	ug/L	97
80) 1,3-Dichlorobenzene	11.796	146	86247	22.48	ug/L	98
81) 1,4-Dichlorobenzene	11.863	146	89594	21.23	ug/L	97
82) n-Butylbenzene	12.045	91	130970	24.80	ug/L	97
83) 1,2-Dichlorobenzene	12.185	146	83871	22.77	ug/L	97
84) 1,2-Dibromo-3-Chloropr...	12.799	157	13740	23.83	ug/L	96
85) Hexachlorobutadiene	13.304	223	12054	23.57	ug/L	92
86) 1,2,4-Trichlorobenzene	13.347	180	50962	29.09	ug/L	98
87) Naphthalene	13.627	128	161860	28.24	ug/L	98
88) 1,2,3-Trichlorobenzene	13.785	180	48345	28.22	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102424.D  
Acq On : 24 Oct 2019 7:03 pm  
Operator : MM  
Sample : 9J24043-CAL8  
Misc : 1X 5mL 20/40PPB VOCR  
ALS Vial : 11 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:35 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102425.D  
 Acq On : 24 Oct 2019 7:30 pm  
 Operator : MM  
 Sample : 9J24043-CAL9  
 Misc : 1X 5mL 50/100PPB VOCR  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:38 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*Handwritten:*  
 W  
 10/25/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.211	99	115635	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.910	117	321159	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	158122	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	116809	49.24	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.777	114	370144	55.88	ug/L	-0.01	
48) Toluene-d8 (S)	8.298	98	415062	50.06	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	125801	49.46	ug/L	0.00	
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.679	85	109425	48.15	ug/L		99
3) Chloromethane	1.892	50	118956	44.44	ug/L		96
4) Vinyl Chloride	1.995	62	133008	55.69	ug/L		97
5) Bromomethane	2.360	96	66917	36.34	ug/L		96
6) Chloroethane	2.494	64	51695	42.64	ug/L		82
7) Trichlorofluoromethane	2.664	101	145579	38.20	ug/L		95
8) Ethanol	3.230	45	131053	2837.58	ug/L		88
9) 1,1-Dichloroethene	3.230	61	137847	47.23	ug/L		91
10) Carbon Disulfide	3.248	76	254448	53.14	ug/L		98
11) Freon 113	3.285	101	97812	51.37	ug/L		94
12) Iodomethane	3.382	142	57651	55.87	ug/L		92
13) Acrolein	3.613	56	28604	69.32	ug/L		78
14) Methylene Chloride	3.869	84	102541	48.75	ug/L		89
15) Acetone	3.936	43	93945	94.28	ug/L		97
16) t-1,2-Dichloroethene	4.039	61	137318	52.49	ug/L		92
17) n-Hexane	4.118	86	21163	66.01	ug/L	#	91
18) Methyl-tert-butyl-ether	4.167	73	313020	54.26	ug/L		94
19) tert-Butanol (TBA)	4.288	59	1172838	3280.93	ug/L		94
20) Diisopropyl ether (DIPE)	4.562	45	63994	10.88	ug/L		93
21) 1,1-Dichloroethane	4.684	63	182910	49.62	ug/L		96
22) Acrylonitrile	4.745	53	58667	53.90	ug/L		96
23) Ethyl-tert-butyl ether...	4.939	59	63126	12.08	ug/L		96
24) Vinyl Acetate	4.952	43	246127	56.12	ug/L		96
25) c-1,2-Dichloroethene	5.238	61	143124	49.74	ug/L		92
26) 2,2-Dichloropropane	5.347	77	122658	47.70	ug/L		96
27) Bromochloromethane	5.444	130	77572	54.59	ug/L		95
28) Chloroform	5.523	83	186984	47.32	ug/L		97
29) Carbon Tetrachloride	5.657	117	114614	42.30	ug/L		94
30) Tetrahydrofuran	5.694	42	54072	56.56	ug/L		88
31) 1,1,1-Trichloroethane	5.730	97	156566	47.91	ug/L		96
33) 1,1-Dichloropropene	5.858	75	146998	56.14	ug/L		96
34) 2-Butanone (MEK)	5.852	43	162223	106.80	ug/L		96
35) Benzene	6.120	78	434612	55.18	ug/L		96
36) tert-Amyl methyl ether...	6.241	73	56793	10.83	ug/L		98
37) 1,2-Dichloroethane (EDC)	6.339	62	143950	44.78	ug/L		92
38) iso-Butyl Alcohol	6.369	43	224878	1634.66	ug/L		92
40) Trichloroethene (TCE)	6.740	130	118626	59.12	ug/L		95
41) Tert-Amyl-Ethyl-Ether ...	6.996	59	42660	12.88	ug/L		84
42) Dibromomethane	7.196	93	74270	51.96	ug/L		96
43) 1,2-Dichloropropane	7.306	63	109124	51.04	ug/L		92
44) Bromodichloromethane	7.379	83	133532	46.50	ug/L		95
46) 2-Chloroethyl Vinyl Ether	8.018	63	88331	62.62	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	166893	54.89	ug/L		87

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102425.D  
 Acq On : 24 Oct 2019 7:30 pm  
 Operator : MM  
 Sample : 9J24043-CAL9  
 Misc : 1X 5mL 50/100PPB VOCR  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:10:38 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	446611	49.69	ug/L	99
50) Tetrachloroethene (PCE)	8.796	166	113079	55.11	ug/L	92
51) 4-Methyl-2-Pentanone (...)	8.796	43	304356	106.90	ug/L	94
52) t-1,3-Dichloropropene	8.833	75	151987	50.21	ug/L	97
53) 1,1,2-Trichloroethane	9.003	97	107594	49.71	ug/L	94
54) Dibromochloromethane	9.186	129	101291	44.59	ug/L	96
55) 1,3-Dichloropropane	9.289	76	183541	50.70	ug/L	91
56) 1,2-Dibromoethane (EDB)	9.423	107	117418	52.83	ug/L	95
57) 2-Hexanone	9.648	43	224495	109.02	ug/L	91
58) Chlorobenzene	9.928	112	301806	53.03	ug/L	98
59) Ethylbenzene	9.952	91	486890	51.84	ug/L	97
60) 1,1,1,2-Tetrachloroethane	9.989	131	95075	48.26	ug/L	97
61) m,p-Xylenes (2)	10.086	91	738497	106.14	ug/L	99
62) o-Xylene	10.463	91	371768	53.47	ug/L	99
63) Styrene	10.512	104	307044	56.78	ug/L	98
64) Bromoform	10.536	173	71080	44.14	ug/L	96
65) Isopropylbenzene	10.731	105	458349	55.46	ug/L	98
68) Bromobenzene	11.060	156	126180	55.39	ug/L	90
69) n-Propylbenzene	11.072	91	530991	53.60	ug/L	100
70) 1,1,2,2-Tetrachloroethane	11.139	85	106506	51.56	ug/L	94
71) 2-Chlorotoluene	11.206	126	113724	57.85	ug/L	93
72) 1,3,5-Trimethylbenzene	11.230	105	370702	56.11	ug/L	97
73) 1,2,3-Trichloropropane	11.248	110	51746	51.31	ug/L	92
74) t-1,4-Dichloro-2-butene	11.279	53	38431	48.98	ug/L	84
75) 4-Chlorotoluene	11.333	91	325043	55.29	ug/L	95
76) tert-Butylbenzene	11.479	91	202040	55.54	ug/L	97
77) 1,2,4-Trimethylbenzene	11.534	105	374779	56.03	ug/L	96
78) sec-Butylbenzene	11.619	105	451933	57.09	ug/L	98
79) 4-Isopropyltoluene	11.729	119	378247	59.61	ug/L	97
80) 1,3-Dichlorobenzene	11.796	146	218694	54.64	ug/L	99
81) 1,4-Dichlorobenzene	11.863	146	222386	50.52	ug/L	98
82) n-Butylbenzene	12.045	91	325681	59.11	ug/L	99
83) 1,2-Dichlorobenzene	12.179	146	211431	55.02	ug/L	98
84) 1,2-Dibromo-3-Chloropr...	12.799	157	38435	63.92	ug/L	93
85) Hexachlorobutadiene	13.304	223	29829	55.92	ug/L	96
86) 1,2,4-Trichlorobenzene	13.341	180	128379	70.24	ug/L	96
87) Naphthalene	13.627	128	425207	64.94	ug/L	98
88) 1,2,3-Trichlorobenzene	13.785	180	123175	68.94	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102425.D  
Acq On : 24 Oct 2019 7:30 pm  
Operator : MM  
Sample : 9J24043-CAL9  
Misc : 1X 5mL 50/100PPB VOCR  
ALS Vial : 12 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:38 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration





Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102426.D  
 Acq On : 24 Oct 2019 7:57 pm  
 Operator : MM  
 Sample : 9J24043-IBL2  
 Misc : 1X 5mL DI  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:52:40 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene (I)	6.217	99	112457	50.00	ug/L	# 0.00
45) Chlorobenzene-d5 (I)	9.910	117	299558	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	136435	50.00	ug/L	0.00
System Monitoring Compounds						
32) Dibromofluoromethane (S)	5.712	111	110045	49.80	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.783	114	354886	49.95	ug/L	0.00
48) Toluene-d8 (S)	8.298	98	401381	51.05	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	112112	50.86	ug/L	0.00
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.679	85	219	0.12	ug/L	# 49
3) Chloromethane	1.898	50	309	0.13	ug/L	# 47
5) Bromomethane	2.366	96	254	0.18	ug/L	# 43
6) Chloroethane	2.518	64	211	0.19	ug/L	# 36
10) Carbon Disulfide	3.248	76	1601	0.33	ug/L	78
15) Acetone	3.948	43	1040	1.06	ug/L	95
50) Tetrachloroethene (PCE)	8.803	166	260	0.13	ug/L	# 25
61) m,p-Xylenes (2)	10.092	91	1118	0.16	ug/L	95
69) n-Propylbenzene	11.072	91	1265	0.14	ug/L	91
72) 1,3,5-Trimethylbenzene	11.230	105	651	0.11	ug/L	81
75) 4-Chlorotoluene	11.339	91	738	0.13	ug/L	86
76) tert-Butylbenzene	11.485	91	323	0.09	ug/L	# 83
77) 1,2,4-Trimethylbenzene	11.540	105	743	0.12	ug/L	92
78) sec-Butylbenzene	11.625	105	1155	0.15	ug/L	94
79) 4-Isopropyltoluene	11.729	119	1010	0.17	ug/L	89
80) 1,3-Dichlorobenzene	11.802	146	590	0.16	ug/L	93
81) 1,4-Dichlorobenzene	11.863	146	797	0.21	ug/L	# 7
82) n-Butylbenzene	12.051	91	1166	0.23	ug/L	98
83) 1,2-Dichlorobenzene	12.185	146	421	0.12	ug/L	# 70
85) Hexachlorobutadiene	13.304	223	332	0.66	ug/L	# 72
86) 1,2,4-Trichlorobenzene	13.341	180	1230	0.60	ug/L	94
87) Naphthalene	13.627	128	3549	0.54	ug/L	93
88) 1,2,3-Trichlorobenzene	13.785	180	1510	0.77	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102426.D  
Acq On : 24 Oct 2019 7:57 pm  
Operator : MM  
Sample : 9J24043-IBL2  
Misc : 1X 5mL DI  
ALS Vial : 13 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:40 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102427.D  
 Acq On : 24 Oct 2019 8:24 pm  
 Operator : MM  
 Sample : 9J24043-CALA  
 Misc : 1X 5mL 100/200PPB VOCR  
 ALS Vial : 14 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:41 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*Handwritten:*  
 10/25/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	111989	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.909	117	318635	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	163243	50.00	ug/L		0.00
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.718	111	113819	49.55	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.783	114	356857	55.62	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	405945	49.35	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	124392	47.37	ug/L		0.00
<b>Target Compounds</b>							
						Qvalue	
2) Dichlorodifluoromethane	1.684	85	212153	96.39	ug/L		98
3) Chloromethane	1.897	50	226754	87.47	ug/L		96
4) Vinyl Chloride	2.001	62	258510	111.76	ug/L		98
5) Bromomethane	2.366	96	125242	70.23	ug/L		98
6) Chloroethane	2.506	64	53786	45.81	ug/L		81
7) Trichlorofluoromethane	2.664	101	279991	75.86	ug/L		97
8) Ethanol	3.242	45	254643	5693.08	ug/L		88
9) 1,1-Dichloroethene	3.236	61	286478	101.36	ug/L		92
10) Carbon Disulfide	3.254	76	531736	114.66	ug/L		98
11) Freon 113	3.291	101	204168	110.71	ug/L		97
12) Iodomethane	3.388	142	153366	122.76	ug/L		92
13) Acrolein	3.625	56	60054	150.27	ug/L		72
14) Methylene Chloride	3.875	84	209114	104.97	ug/L		88
15) Acetone	3.942	43	188786	195.63	ug/L		96
16) t-1,2-Dichloroethene	4.039	61	285846	112.82	ug/L		95
17) n-Hexane	4.124	86	43920	141.46	ug/L		93
18) Methyl-tert-butyl-ether	4.167	73	646936	115.78	ug/L		92
19) tert-Butanol (TBA)	4.294	59	2295578	6630.79	ug/L		91
20) Diisopropyl ether (DIPE)	4.568	45	122827	21.57	ug/L		93
21) 1,1-Dichloroethane	4.684	63	379907	106.41	ug/L		96
22) Acrylonitrile	4.751	53	122564	116.27	ug/L		98
23) Ethyl-tert-butyl ether...	4.939	59	121788	24.06	ug/L		98
24) Vinyl Acetate	4.957	43	522592	123.03	ug/L		95
25) c-1,2-Dichloroethene	5.243	61	297452	106.74	ug/L		91
26) 2,2-Dichloropropane	5.353	77	252830	101.52	ug/L		95
27) Bromochloromethane	5.450	130	151653	110.19	ug/L		94
28) Chloroform	5.529	83	385051	100.61	ug/L		97
29) Carbon Tetrachloride	5.663	117	247648	94.37	ug/L		94
30) Tetrahydrofuran	5.700	42	111881	120.85	ug/L		86
31) 1,1,1-Trichloroethane	5.736	97	325398	102.81	ug/L		96
33) 1,1-Dichloropropene	5.864	75	308104	121.49	ug/L		95
34) 2-Butanone (MEK)	5.852	43	331914	225.64	ug/L		97
35) Benzene	6.119	78	900809	118.09	ug/L		96
36) tert-Amyl methyl ether...	6.247	73	111127	21.87	ug/L		99
37) 1,2-Dichloroethane (EDC)	6.338	62	294149	94.48	ug/L		92
38) iso-Butyl Alcohol	6.375	43	450055	3378.00	ug/L		92
40) Trichloroethene (TCE)	6.746	130	245311	126.23	ug/L		94
41) Tert-Amyl-Ethyl-Ether ...	6.995	59	83591	26.07	ug/L		86
42) Dibromomethane	7.196	93	155032	111.99	ug/L		94
43) 1,2-Dichloropropane	7.312	63	229327	110.76	ug/L		90
44) Bromodichloromethane	7.379	83	282119	101.45	ug/L		92
46) 2-Chloroethyl Vinyl Ether	8.024	63	185987	122.70	ug/L	#	100
47) c-1,3-Dichloropropene	8.090	75	356393	118.14	ug/L		86

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102427.D  
 Acq On : 24 Oct 2019 8:24 pm  
 Operator : MM  
 Sample : 9J24043-CALA  
 Misc : 1X 5mL 100/200PPB VOCR  
 ALS Vial : 14 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:41 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	931584	104.48	ug/L	99
50) Tetrachloroethene (PCE)	8.796	166	236880	116.36	ug/L	92
51) 4-Methyl-2-Pentanone (...)	8.796	43	616767	218.34	ug/L	92
52) t-1,3-Dichloropropane	8.839	75	327146	108.93	ug/L	98
53) 1,1,2-Trichloroethane	9.009	97	221018	102.93	ug/L	92
54) Dibromochloromethane	9.186	129	222919	98.91	ug/L	98
55) 1,3-Dichloropropane	9.289	76	379039	105.53	ug/L	90
56) 1,2-Dibromoethane (EDB)	9.423	107	243688	110.52	ug/L	94
57) 2-Hexanone	9.654	43	456833	223.60	ug/L	90
58) Chlorobenzene	9.928	112	624905	110.67	ug/L	98
59) Ethylbenzene	9.952	91	1015747	109.00	ug/L	97
60) 1,1,1,2-Tetrachloroethane	9.989	131	206263	105.52	ug/L	96
61) m,p-Xylenes (2)	10.086	91	1568164	215.46	ug/L	98
62) o-Xylene	10.463	91	785588	106.87	ug/L	100
63) Styrene	10.512	104	653902	114.07	ug/L	98
64) Bromoform	10.536	173	162527	101.72	ug/L	98
65) Isopropylbenzene	10.731	105	973691	110.72	ug/L	98
68) Bromobenzene	11.059	156	265287	112.81	ug/L	91
69) n-Propylbenzene	11.071	91	1142995	111.76	ug/L	100
70) 1,1,2,2-Tetrachloroethane	11.138	85	212550	99.67	ug/L	94
71) 2-Chlorotoluene	11.205	126	238214	117.38	ug/L	96
72) 1,3,5-Trimethylbenzene	11.230	105	783721	114.91	ug/L	97
73) 1,2,3-Trichloropropane	11.248	110	103994	99.89	ug/L	91
74) t-1,4-Dichloro-2-butene	11.278	53	76466	94.39	ug/L	93
75) 4-Chlorotoluene	11.339	91	688819	113.48	ug/L	98
76) tert-Butylbenzene	11.479	91	431117	114.79	ug/L	98
77) 1,2,4-Trimethylbenzene	11.534	105	798406	110.07	ug/L	97
78) sec-Butylbenzene	11.619	105	969880	118.68	ug/L	98
79) 4-Isopropyltoluene	11.728	119	812481	115.11	ug/L	97
80) 1,3-Dichlorobenzene	11.795	146	461068	111.58	ug/L	98
81) 1,4-Dichlorobenzene	11.862	146	468883	103.17	ug/L	97
82) n-Butylbenzene	12.045	91	694929	122.18	ug/L	99
83) 1,2-Dichlorobenzene	12.185	146	439251	110.73	ug/L	98
84) 1,2-Dibromo-3-Chloropr...	12.799	157	81625	131.48	ug/L	92
85) Hexachlorobutadiene	13.304	223	62008	112.60	ug/L	96
86) 1,2,4-Trichlorobenzene	13.347	180	268764	142.44	ug/L	98
87) Naphthalene	13.627	128	899370	118.81	ug/L	98
88) 1,2,3-Trichlorobenzene	13.785	180	260549	141.24	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102427.D  
Acq On : 24 Oct 2019 8:24 pm  
Operator : MM  
Sample : 9J24043-CALA  
Misc : 1X 5mL 100/200PPB VOCR  
ALS Vial : 14 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:41 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102428.D  
 Acq On : 24 Oct 2019 8:51 pm  
 Operator : MM  
 Sample : 9J24043-IBL3  
 Misc : 1X 5mL DI  
 ALS Vial : 15 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:44 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	111004	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.916	117	296306	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	134814	50.00	ug/L		0.00
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.718	111	109567	50.24	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.783	114	354190	50.51	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	395820	50.89	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	112213	51.51	ug/L		0.00
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.685	85	460	0.25	ug/L	#	49
3) Chloromethane	1.904	50	377	0.16	ug/L	#	47
4) Vinyl Chloride	2.007	62	243	0.10	ug/L	#	50
5) Bromomethane	2.378	96	380	0.27	ug/L	#	63
6) Chloroethane	2.475	64	250	0.23	ug/L	#	36
7) Trichlorofluoromethane	2.676	101	332	0.12	ug/L	#	27
9) 1,1-Dichloroethene	3.242	61	244	0.09	ug/L	#	66
10) Carbon Disulfide	3.260	76	3074	0.63	ug/L		91
11) Freon 113	3.303	101	464	0.25	ug/L	#	64
12) Iodomethane	3.394	142	124	6.13	ug/L	#	47
14) Methylene Chloride	3.881	84	3969	1.09	ug/L	#	77
15) Acetone	3.948	43	1229	1.26	ug/L		100
16) t-1,2-Dichloroethene	4.045	61	638	0.25	ug/L		95
19) tert-Butanol (TBA)	4.307	59	387	0.90	ug/L		46
33) 1,1-Dichloropropene	5.870	75	460	0.16	ug/L	#	43
40) Trichloroethene (TCE)	6.752	130	288	0.13	ug/L	#	77
49) Toluene	8.352	91	913	0.10	ug/L		85
50) Tetrachloroethene (PCE)	8.796	166	577	0.28	ug/L	#	68
58) Chlorobenzene	9.928	112	773	0.14	ug/L	#	1
59) Ethylbenzene	9.958	91	1209	0.13	ug/L		91
61) m,p-Xylenes (2)	10.092	91	2162	0.32	ug/L		89
62) o-Xylene	10.469	91	668	0.10	ug/L		82
63) Styrene	10.524	104	495	0.09	ug/L	#	42
65) Isopropylbenzene	10.731	105	1275	0.16	ug/L		97
68) Bromobenzene	11.059	156	288	0.14	ug/L		83
69) n-Propylbenzene	11.078	91	2421	0.27	ug/L		95
71) 2-Chlorotoluene	11.211	126	168	0.09	ug/L	#	78
72) 1,3,5-Trimethylbenzene	11.230	105	1309	0.21	ug/L		93
75) 4-Chlorotoluene	11.345	91	1369	0.25	ug/L		91
76) tert-Butylbenzene	11.485	91	751	0.22	ug/L		89
77) 1,2,4-Trimethylbenzene	11.540	105	1395	0.23	ug/L		94
78) sec-Butylbenzene	11.619	105	2367	0.31	ug/L		93
79) 4-Isopropyltoluene	11.729	119	2004	0.34	ug/L		95
80) 1,3-Dichlorobenzene	11.795	146	1269	0.35	ug/L		90
81) 1,4-Dichlorobenzene	11.862	146	1515	0.40	ug/L	#	64
82) n-Butylbenzene	12.045	91	2454	0.48	ug/L		99
83) 1,2-Dichlorobenzene	12.185	146	829	0.23	ug/L		91
85) Hexachlorobutadiene	13.304	223	765	1.55	ug/L		89
86) 1,2,4-Trichlorobenzene	13.341	180	2446	1.20	ug/L		96
87) Naphthalene	13.627	128	6843	1.06	ug/L		97
88) 1,2,3-Trichlorobenzene	13.785	180	2978	1.54	ug/L		95

Quantitation Report (Not Reviewed)


Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102428.D  
Acq On : 24 Oct 2019 8:51 pm  
Operator : MM  
Sample : 9J24043-IBL3  
Misc : 1X 5mL DI  
ALS Vial : 15 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:44 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102428.D  
Acq On : 24 Oct 2019 8:51 pm  
Operator : MM  
Sample : 9J24043-IBL3  
Misc : 1X 5mL DI  
ALS Vial : 15 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:44 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration





Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102429.D  
 Acq On : 24 Oct 2019 9:17 pm  
 Operator : MM  
 Sample : 9J24043-CALB  
 Misc : 1X 5mL 200/400PPB VOCR  
 ALS Vial : 16 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:44 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration

*Handwritten:*  
 ✓  
 10/25/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	Qvalue
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	116034	50.00	ug/L	# 0.00	
45) Chlorobenzene-d5 (I)	9.916	117	330915	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	169365	50.00	ug/L	0.00	
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	118677	49.86	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.783	114	369003	55.51	ug/L	0.00	
48) Toluene-d8 (S)	8.297	98	420947	49.28	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	127221	46.70	ug/L	0.00	
<b>Target Compounds</b>							
2) Dichlorodifluoromethane	1.685	85	431143	189.06	ug/L		99
3) Chloromethane	1.897	50	456703	170.02	ug/L		96
4) Vinyl Chloride	2.001	62	521368	217.54	ug/L		97
5) Bromomethane	2.366	96	267468	144.76	ug/L		99
6) Chloroethane	2.494	64	53331	43.84	ug/L		86
7) Trichlorofluoromethane	2.658	101	556445	145.51	ug/L		96
8) Ethanol	3.248	45	3815	82.32	ug/L	#	1
9) 1,1-Dichloroethene	3.230	61	567371	193.74	ug/L		92
10) Carbon Disulfide	3.248	76	1067583	222.18	ug/L		98
11) Freon 113	3.285	101	411156	215.18	ug/L		96
12) Iodomethane	3.388	142	348091	216.50	ug/L		94
13) Acrolein	3.619	56	116360	281.01	ug/L		72
14) Methylene Chloride	3.875	84	419637	199.87	ug/L		87
15) Acetone	3.942	43	375022	375.07	ug/L		94
16) t-1,2-Dichloroethene	4.039	61	579277	220.67	ug/L		91
17) n-Hexane	4.124	86	92077	286.23	ug/L		96
18) Methyl-tert-butyl-ether	4.167	73	1318751	227.79	ug/L		93
19) tert-Butanol (TBA)	4.294	59	1885	5.26	ug/L	#	34
20) Diisopropyl ether (DIPE)	4.568	45	1263	0.21	ug/L		96
21) 1,1-Dichloroethane	4.684	63	761535	205.86	ug/L		97
22) Acrylonitrile	4.751	53	243406	222.86	ug/L		99
23) Ethyl-tert-butyl ether...	4.939	59	984	0.19	ug/L	#	1
24) Vinyl Acetate	4.957	43	980632	222.81	ug/L		94
25) c-1,2-Dichloroethene	5.243	61	597836	207.05	ug/L		89
26) 2,2-Dichloropropane	5.353	77	512393	198.56	ug/L		92
27) Bromochloromethane	5.450	130	288672	202.44	ug/L		91
28) Chloroform	5.529	83	776466	195.81	ug/L		96
29) Carbon Tetrachloride	5.663	117	525973	193.45	ug/L		95
30) Tetrahydrofuran	5.694	42	221252	230.66	ug/L		85
31) 1,1,1-Trichloroethane	5.736	97	663507	202.33	ug/L		95
33) 1,1-Dichloropropene	5.864	75	622283	236.82	ug/L		94
34) 2-Butanone (MEK)	5.852	43	651518	427.47	ug/L		95
35) Benzene	6.119	78	1815119	229.66	ug/L		96
36) tert-Amyl methyl ether	6.253	73	804	0.15	ug/L	#	44
37) 1,2-Dichloroethane (EDC)	6.338	62	583025	180.73	ug/L		92
38) iso-Butyl Alcohol	6.375	43	863259	6253.53	ug/L		90
40) Trichloroethene (TCE)	6.740	130	498651	247.64	ug/L		95
41) Tert-Amyl Ethyl Ether ...	7.002	59	794	0.24	ug/L		83
42) Dibromomethane	7.196	93	314382	219.17	ug/L		96
43) 1,2-Dichloropropane	7.312	63	461364	215.06	ug/L		91
44) Bromodichloromethane	7.379	83	582259	202.08	ug/L		93
46) 2-Chloroethyl Vinyl Ether	8.024	63	361318	207.89	ug/L	#	100
47) c-1,3-Dichloropropene	8.091	75	736312	235.01	ug/L		86

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102429.D  
 Acq On : 24 Oct 2019 9:17 pm  
 Operator : MM  
 Sample : 9J24043-CALB  
 Misc : 1X 5mL 200/400PPB VOCR  
 ALS Vial : 16 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:44 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Tue Aug 06 08:58:13 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	1905088	205.73	ug/L	100
50) Tetrachloroethene (PCE)	8.796	166	496433	234.81	ug/L	93
51) 4-Methyl-2-Pentanone (...)	8.796	43	1166981	397.79	ug/L	90
52) t-1,3-Dichloropropene	8.839	75	678927	217.67	ug/L	98
53) 1,1,2-Trichloroethane	9.009	97	447395	200.52	ug/L	91
54) Dibromochloromethane	9.186	129	473598	202.33	ug/L	98
55) 1,3-Dichloropropane	9.289	76	755862	202.63	ug/L	88
56) 1,2-Dibromoethane (EDB)	9.423	107	496207	216.69	ug/L	95
57) 2-Hexanone	9.654	43	866990	408.61	ug/L	89
58) Chlorobenzene	9.928	112	1285529	219.22	ug/L	98
59) Ethylbenzene	9.952	91	2091382	216.09	ug/L	96
60) 1,1,1,2-Tetrachloroethane	9.989	131	427244	210.45	ug/L	97
61) m,p-Xylenes (2)	10.086	91	3227914	393.99	ug/L	97
62) o-Xylene	10.463	91	1606355	191.75	ug/L	99
63) Styrene	10.512	104	1353743	206.36	ug/L	98
64) Bromoform	10.536	173	351162	211.63	ug/L	97
65) Isopropylbenzene	10.731	105	1980670	196.46	ug/L	98
68) Bromobenzene	11.059	156	542011	222.15	ug/L	92
69) n-Propylbenzene	11.071	91	2308779	217.60	ug/L	99
70) 1,1,2,2-Tetrachloroethane	11.138	85	408430	184.60	ug/L	94
71) 2-Chlorotoluene	11.205	126	490093	232.77	ug/L	92
72) 1,3,5-Trimethylbenzene	11.230	105	1618836	228.77	ug/L	97
73) 1,2,3-Trichloropropane	11.248	110	199656	184.85	ug/L	91
74) t-1,4-Dichloro-2-butene	11.278	53	148266	176.41	ug/L	93
75) 4-Chlorotoluene	11.339	91	1379272	219.02	ug/L	99
76) tert-Butylbenzene	11.479	91	872573	223.94	ug/L	99
77) 1,2,4-Trimethylbenzene	11.534	105	1629601	200.54	ug/L	97
78) sec-Butylbenzene	11.619	105	1977513	233.24	ug/L	98
79) 4-Isopropyltoluene	11.729	119	1677679	205.31	ug/L	96
80) 1,3-Dichlorobenzene	11.795	146	936572	218.47	ug/L	99
81) 1,4-Dichlorobenzene	11.862	146	949679	201.41	ug/L	97
82) n-Butylbenzene	12.045	91	1435776	243.31	ug/L	100
83) 1,2-Dichlorobenzene	12.185	146	884385	214.88	ug/L	98
84) 1,2-Dibromo-3-Chloropr...	12.799	157	169849	263.70	ug/L	91
85) Hexachlorobutadiene	13.304	223	126838	221.99	ug/L	96
86) 1,2,4-Trichlorobenzene	13.347	180	564943	288.60	ug/L	97
87) Naphthalene	13.627	128	1872418	204.22	ug/L	98
88) 1,2,3-Trichlorobenzene	13.785	180	552458	288.66	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102429.D  
Acq On : 24 Oct 2019 9:17 pm  
Operator : MM  
Sample : 9J24043-CALB  
Misc : 1X 5mL 200/400PPB VOCR  
ALS Vial : 16 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:10:44 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Tue Aug 06 08:58:13 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102430.D  
 Acq On : 24 Oct 2019 9:44 pm  
 Operator : MM  
 Sample : 9J24043-IBL4  
 Misc : 1X 5mL DI  
 ALS Vial : 17 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:47 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
-----							
Internal Standards							
1) Pentafluorobenzene (I)	6.217	99	114565	50.00	ug/L	0.00	
45) Chlorobenzene-d5 (I)	9.916	117	310520	50.00	ug/L	0.00	
66) 1,4-Dichlorobenzene-d4...	11.850	152	145083	50.00	ug/L	0.00	
System Monitoring Compounds							
32) Dibromofluoromethane (S)	5.718	111	112455	49.96	ug/L	0.00	
39) 1,4-Difluorobenzene (S)	6.783	114	365140	50.45	ug/L	0.00	
48) Toluene-d8 (S)	8.297	98	412521	50.61	ug/L	0.00	
67) 4-Bromofluorobenzene (S)	10.974	174	119053	50.79	ug/L	0.00	
Target Compounds							
							Qvalue
2) Dichlorodifluoromethane	1.685	85	901	0.48	ug/L		86
3) Chloromethane	1.904	50	702	0.28	ug/L		91
4) Vinyl Chloride	2.007	62	555	0.22	ug/L		76
5) Bromomethane	2.366	96	620	0.42	ug/L #		66
6) Chloroethane	2.475	64	119	0.10	ug/L #		36
7) Trichlorofluoromethane	2.682	101	785	0.28	ug/L		75
9) 1,1-Dichloroethene	3.242	61	667	0.25	ug/L #		68
10) Carbon Disulfide	3.254	76	6515	1.30	ug/L		94
11) Freon 113	3.291	101	931	0.48	ug/L		95
12) Iodomethane	3.394	142	137	6.13	ug/L #		47
14) Methylene Chloride	3.875	84	7612	2.78	ug/L		89
15) Acetone	3.954	43	1615	1.61	ug/L		99
16) t-1,2-Dichloroethene	4.045	61	1218	0.46	ug/L		78
17) n-Hexane	4.136	86	112	0.28	ug/L #		32
25) c-1,2-Dichloroethene	5.250	61	460	0.16	ug/L		83
33) 1,1-Dichloropropene	5.870	75	1080	0.37	ug/L		91
35) Benzene	6.132	78	1050	0.12	ug/L		55
40) Trichloroethene (TCE)	6.746	130	726	0.32	ug/L		83
49) Toluene	8.364	91	1892	0.21	ug/L		82
50) Tetrachloroethene (PCE)	8.802	166	1170	0.55	ug/L		97
52) t-1,3-Dichloropropene	8.851	75	248	0.09	ug/L #		45
58) Chlorobenzene	9.928	112	1487	0.26	ug/L #		41
59) Ethylbenzene	9.952	91	2481	0.26	ug/L		98
61) m,p-Xylenes (2)	10.086	91	3988	0.57	ug/L		87
62) o-Xylene	10.469	91	1347	0.19	ug/L		91
63) Styrene	10.518	104	1067	0.19	ug/L		84
65) Isopropylbenzene	10.731	105	2410	0.28	ug/L		98
68) Bromobenzene	11.059	156	607	0.27	ug/L #		77
69) n-Propylbenzene	11.078	91	4614	0.48	ug/L		96
71) 2-Chlorotoluene	11.205	126	614	0.30	ug/L		91
72) 1,3,5-Trimethylbenzene	11.230	105	2535	0.38	ug/L		94
75) 4-Chlorotoluene	11.339	91	2932	0.49	ug/L		94
76) tert-Butylbenzene	11.479	91	1522	0.41	ug/L #		74
77) 1,2,4-Trimethylbenzene	11.540	105	2816	0.42	ug/L		95
78) sec-Butylbenzene	11.619	105	4551	0.56	ug/L		94
79) 4-Isopropyltoluene	11.729	119	3934	0.61	ug/L		99
80) 1,3-Dichlorobenzene	11.802	146	2380	0.61	ug/L		96
81) 1,4-Dichlorobenzene	11.862	146	2728	0.67	ug/L #		77
82) n-Butylbenzene	12.045	91	4783	0.88	ug/L		94
83) 1,2-Dichlorobenzene	12.185	146	1646	0.43	ug/L		95
85) Hexachlorobutadiene	13.304	223	1948	3.66	ug/L		90
86) 1,2,4-Trichlorobenzene	13.347	180	4827	2.20	ug/L		92
87) Naphthalene	13.627	128	13602	1.95	ug/L		98

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102430.D  
Acq On : 24 Oct 2019 9:44 pm  
Operator : MM  
Sample : 9J24043-IBL4  
Misc : 1X 5mL DI  
ALS Vial : 17 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:52:47 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
88) 1,2,3-Trichlorobenzene	13.785	180	5992	2.88	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102430.D  
Acq On : 24 Oct 2019 9:44 pm  
Operator : MM  
Sample : 9J24043-IBL4  
Misc : 1X 5mL DI  
ALS Vial : 17 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:47 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102431.D  
 Acq On : 24 Oct 2019 10:11 pm  
 Operator : MM  
 Sample : 9J24043-IBL5  
 Misc : 1X 5mL DI  
 ALS Vial : 18 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:52:50 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene (I)	6.217	99	114296	50.00	ug/L	# 0.00
45) Chlorobenzene-d5 (I)	9.916	117	308297	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	139384	50.00	ug/L	0.00
<b>System Monitoring Compounds</b>						
32) Dibromofluoromethane (S)	5.718	111	112321	50.01	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.783	114	364393	50.46	ug/L	0.00
48) Toluene-d8 (S)	8.297	98	406006	50.17	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	117384	52.12	ug/L	0.00
<b>Target Compounds</b>						
						Qvalue
2) Dichlorodifluoromethane	1.691	85	321	0.17	ug/L	# 49
3) Chloromethane	1.904	50	302	0.12	ug/L	# 47
5) Bromomethane	2.378	96	484	0.33	ug/L	# 56
6) Chloroethane	2.500	64	259	0.23	ug/L	# 36
10) Carbon Disulfide	3.260	76	2655	0.53	ug/L	89
11) Freon 113	3.291	101	416	0.21	ug/L	# 74
14) Methylene Chloride	3.881	84	5891	1.96	ug/L	86
15) Acetone	3.954	43	3138	3.13	ug/L	97
16) t-1,2-Dichloroethene	4.039	61	402	0.15	ug/L	# 70
33) 1,1-Dichloropropene	5.870	75	357	0.12	ug/L	# 43
49) Toluene	8.358	91	884	0.10	ug/L	92
50) Tetrachloroethene (PCE)	8.802	166	422	0.20	ug/L	# 70
58) Chlorobenzene	9.928	112	577	0.10	ug/L	# 5
59) Ethylbenzene	9.952	91	980	0.10	ug/L	83
61) m,p-Xylenes (2)	10.086	91	1705	0.24	ug/L	86
65) Isopropylbenzene	10.737	105	735	0.09	ug/L	54
69) n-Propylbenzene	11.072	91	1706	0.18	ug/L	90
72) 1,3,5-Trimethylbenzene	11.230	105	901	0.14	ug/L	86
75) 4-Chlorotoluene	11.339	91	1026	0.18	ug/L	91
76) tert-Butylbenzene	11.479	91	379	0.11	ug/L	# 75
77) 1,2,4-Trimethylbenzene	11.540	105	984	0.15	ug/L	90
78) sec-Butylbenzene	11.625	105	1431	0.18	ug/L	80
79) 4-Isopropyltoluene	11.729	119	1483	0.24	ug/L	96
80) 1,3-Dichlorobenzene	11.802	146	846	0.22	ug/L	96
81) 1,4-Dichlorobenzene	11.862	146	1023	0.26	ug/L	# 40
82) n-Butylbenzene	12.051	91	1702	0.32	ug/L	91
83) 1,2-Dichlorobenzene	12.191	146	544	0.15	ug/L	# 66
85) Hexachlorobutadiene	13.304	223	353	0.69	ug/L	94
86) 1,2,4-Trichlorobenzene	13.347	180	1099	0.52	ug/L	84
87) Naphthalene	13.627	128	2260	0.34	ug/L	81
88) 1,2,3-Trichlorobenzene	13.785	180	993	0.50	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102431.D  
Acq On : 24 Oct 2019 10:11 pm  
Operator : MM  
Sample : 9J24043-IBL5  
Misc : 1X 5mL DI  
ALS Vial : 18 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:50 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration





Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102432.D  
 Acq On : 24 Oct 2019 10:38 pm  
 Operator : MM  
 Sample : 9J24043-ICV1  
 Misc : 1X 5mL 20/40PPB VOCR  
 ALS Vial : 19 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

VV  
10/25/19

Quant Time: Oct 25 08:52:53 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	115739	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.909	117	319865	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	157880	50.00	ug/L		0.00
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	114369	50.29	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.782	114	368262	50.36	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	413951	49.31	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	126483	49.58	ug/L		0.00
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.678	85	47743	25.24	ug/L		99
3) Chloromethane	1.891	50	52000	20.73	ug/L		96
4) Vinyl Chloride	1.995	62	55595	22.12	ug/L		97
5) Bromomethane	2.360	96	33560	22.65	ug/L		98
6) Chloroethane	2.494	64	20238	17.52	ug/L		79
7) Trichlorofluoromethane	2.658	101	58875	20.69	ug/L		97
8) Ethanol	3.236	45	2066	37.15	ug/L		95
9) 1,1-Dichloroethene	3.230	61	54108	19.72	ug/L		91
10) Carbon Disulfide	3.248	76	92901	18.35	ug/L		98
11) Freon 113	3.278	101	37659	19.09	ug/L		97
12) Iodomethane	3.382	142	13440	16.51	ug/L		90
13) Acrolein	3.619	56	10766	20.47	ug/L		64
14) Methylene Chloride	3.868	84	43934	19.96	ug/L		87
15) Acetone	3.935	43	38135	37.60	ug/L		96
16) t-1,2-Dichloroethene	4.039	61	56343	20.98	ug/L		89
17) n-Hexane	4.124	86	7879	19.27	ug/L	#	88
18) Methyl-tert-butyl-ether	4.167	73	122260	19.59	ug/L		93
19) tert-Butanol (TBA)	4.294	59	12609	28.14	ug/L		83
20) Diisopropyl ether (DIPE)	4.562	45	1214	0.18	ug/L		74
21) 1,1-Dichloroethane	4.684	63	76555	20.53	ug/L		97
22) Acrylonitrile	4.744	53	21989	19.59	ug/L		99
23) Ethyl-tert-butyl ether...	4.945	59	1021	0.16	ug/L		69
24) Vinyl Acetate	4.957	43	89589	19.89	ug/L		95
25) c-1,2-Dichloroethene	5.243	61	57695	20.04	ug/L		92
26) 2,2-Dichloropropane	5.347	77	43127	17.72	ug/L		97
27) Bromochloromethane	5.444	130	31156	22.05	ug/L		93
28) Chloroform	5.523	83	76051	20.86	ug/L		96
29) Carbon Tetrachloride	5.657	117	45898	20.70	ug/L		97
30) Tetrahydrofuran	5.700	42	20305	19.03	ug/L		86
31) 1,1,1-Trichloroethane	5.730	97	61359	19.94	ug/L		97
33) 1,1-Dichloropropene	5.858	75	57945	19.60	ug/L		96
34) 2-Butanone (MEK)	5.852	43	60911	37.88	ug/L		97
35) Benzene	6.119	78	173963	19.67	ug/L		97
36) tert-Amyl methyl ether...	6.259	73	1053	0.18	ug/L		74
37) 1,2-Dichloroethane (EDC)	6.338	62	58405	20.16	ug/L		94
38) iso-Butyl Alcohol	6.375	43	83622	519.10	ug/L		92
40) Trichloroethene (TCE)	6.740	130	48413	21.24	ug/L		94
41) Tert-Amyl-Ethyl-Ether ...	6.995	59	625	0.14	ug/L	#	64
42) Dibromomethane	7.196	93	29991	21.13	ug/L		96
43) 1,2-Dichloropropane	7.306	63	44751	20.29	ug/L		93
44) Bromodichloromethane	7.379	83	52780	20.75	ug/L		94
46) 2-Chloroethyl Vinyl Ether	8.023	63	32992	20.09	ug/L	#	100
47) c-1,3-Dichloropropene	8.090	75	62899	19.89	ug/L		88

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102432.D  
 Acq On : 24 Oct 2019 10:38 pm  
 Operator : MM  
 Sample : 9J24043-ICV1  
 Misc : 1X 5mL 20/40PPB VOCR  
 ALS Vial : 19 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:52:53 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
49) Toluene	8.358	91	182339	19.39	ug/L	100
50) Tetrachloroethene (PCE)	8.796	166	45736	20.89	ug/L	91
51) 4-Methyl-2-Pentanone (...)	8.796	43	117185	41.04	ug/L	94
52) t-1,3-Dichloropropene	8.839	75	58067	20.70	ug/L	99
53) 1,1,2-Trichloroethane	9.003	97	44277	21.23	ug/L	94
54) Dibromochloromethane	9.185	129	40034	23.75	ug/L	97
55) 1,3-Dichloropropane	9.289	76	73648	20.48	ug/L	92
56) 1,2-Dibromoethane (EDB)	9.423	107	46898	20.66	ug/L	94
57) 2-Hexanone	9.654	43	84867	40.56	ug/L	91
58) Chlorobenzene	9.928	112	123672	20.60	ug/L	98
59) Ethylbenzene	9.952	91	198723	20.15	ug/L	97
60) 1,1,1,2-Tetrachloroethane	9.988	131	38126	21.77	ug/L	95
61) m,p-Xylenes (2)	10.086	91	297332	40.93	ug/L	99
62) o-Xylene	10.463	91	151148	20.99	ug/L	99
63) Styrene	10.512	104	120728	20.86	ug/L	97
64) Bromoform	10.536	173	26445	21.37	ug/L	97
65) Isopropylbenzene	10.731	105	183894	20.93	ug/L	99
68) Bromobenzene	11.059	156	51357	20.99	ug/L	88
69) n-Propylbenzene	11.071	91	210884	20.10	ug/L	100
70) 1,1,2,2-Tetrachloroethane	11.138	85	42026	20.34	ug/L	94
71) 2-Chlorotoluene	11.205	126	45073	19.94	ug/L	95
72) 1,3,5-Trimethylbenzene	11.230	105	148155	20.66	ug/L	98
73) 1,2,3-Trichloropropane	11.248	110	20758	20.66	ug/L	90
74) t-1,4-Dichloro-2-butene	11.278	53	12607	17.54	ug/L #	74
75) 4-Chlorotoluene	11.339	91	132799	20.56	ug/L	98
76) tert-Butylbenzene	11.479	91	81539	20.37	ug/L	95
77) 1,2,4-Trimethylbenzene	11.534	105	149487	20.72	ug/L	97
78) sec-Butylbenzene	11.619	105	180737	20.46	ug/L	99
79) 4-Isopropyltoluene	11.728	119	151416	21.66	ug/L	97
80) 1,3-Dichlorobenzene	11.795	146	88840	20.84	ug/L	98
81) 1,4-Dichlorobenzene	11.862	146	91025	20.48	ug/L	97
82) n-Butylbenzene	12.045	91	132273	22.27	ug/L	99
83) 1,2-Dichlorobenzene	12.179	146	86186	20.82	ug/L	98
84) 1,2-Dibromo-3-Chloropr...	12.799	157	14025	20.04	ug/L	92
85) Hexachlorobutadiene	13.304	223	12640	21.85	ug/L	95
86) 1,2,4-Trichlorobenzene	13.347	180	53108	22.26	ug/L	97
87) Naphthalene	13.626	128	166250	21.92	ug/L	98
88) 1,2,3-Trichlorobenzene	13.785	180	51210	22.61	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102432.D  
Acq On : 24 Oct 2019 10:38 pm  
Operator : MM  
Sample : 9J24043-ICV1  
Misc : 1X 5mL 20/40PPB VOGR  
ALS Vial : 19 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:53 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102433.D  
 Acq On : 24 Oct 2019 11:05 pm  
 Operator : MM  
 Sample : 9J24043-ICV2  
 Misc : 1X 5mL 5/1250PPB OXY  
 ALS Vial : 20 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*Handwritten signature and date:*  
 10/25/19

Quant Time: Oct 25 08:52:56 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QI	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) Pentafluorobenzene (I)	6.217	99	111178	50.00	ug/L	#	0.00
45) Chlorobenzene-d5 (I)	9.910	117	298625	50.00	ug/L		0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	138840	50.00	ug/L		0.00
<b>System Monitoring Compounds</b>							
32) Dibromofluoromethane (S)	5.712	111	108440	49.64	ug/L		0.00
39) 1,4-Difluorobenzene (S)	6.783	114	354392	50.46	ug/L		0.00
48) Toluene-d8 (S)	8.297	98	396767	50.62	ug/L		0.00
67) 4-Bromofluorobenzene (S)	10.974	174	114172	50.89	ug/L		0.00
<b>Target Compounds</b>							
							Qvalue
2) Dichlorodifluoromethane	1.679	85	258	0.14	ug/L	#	49
3) Chloromethane	1.898	50	1019	0.42	ug/L		80
4) Vinyl Chloride	2.001	62	483	0.20	ug/L		73
5) Bromomethane	2.360	96	1054	0.74	ug/L		79
6) Chloroethane	2.512	64	817	0.74	ug/L	#	63
8) Ethanol	3.230	45	56590	1059.19	ug/L		85
9) 1,1-Dichloroethene	3.230	61	425	0.16	ug/L	#	74
10) Carbon Disulfide	3.254	76	2404	0.49	ug/L		78
12) Iodomethane	3.388	142	297	6.27	ug/L	#	47
14) Methylene Chloride	3.875	84	2571	0.40	ug/L		89
15) Acetone	3.948	43	992	1.02	ug/L		93
16) t-1,2-Dichloroethene	4.039	61	778	0.30	ug/L		95
18) Methyl-tert-butyl-ether	4.173	73	509	0.08	ug/L		63
19) tert-Butanol (TBA)	4.288	59	507827	1179.79	ug/L		99
20) Diisopropyl ether (DIPE)	4.562	45	28434	4.41	ug/L		96
21) 1,1-Dichloroethane	4.684	63	910	0.25	ug/L		91
23) Ethyl-tert-butyl ether...	4.939	59	27297	4.40	ug/L		98
24) Vinyl Acetate	4.933	43	2981	0.69	ug/L		63
25) c-1,2-Dichloroethene	5.244	61	653	0.24	ug/L		94
28) Chloroform	5.529	83	782	0.22	ug/L		86
31) 1,1,1-Trichloroethane	5.730	97	279	0.09	ug/L	#	25
33) 1,1-Dichloropropene	5.858	75	642	0.23	ug/L	#	43
35) Benzene	6.120	78	2264	0.27	ug/L		96
36) tert-Amyl methyl ether...	6.247	73	24122	4.18	ug/L		94
40) Trichloroethene (TCE)	6.752	130	563	0.26	ug/L		81
41) Tert-Amyl-Ethyl-Ether ...	6.996	59	17806	4.28	ug/L		82
43) 1,2-Dichloropropane	7.312	63	375	0.18	ug/L	#	35
44) Bromodichloromethane	7.379	83	264	0.11	ug/L		89
47) c-1,3-Dichloropropene	8.097	75	423	0.14	ug/L	#	31
49) Toluene	8.358	91	2481	0.28	ug/L		90
50) Tetrachloroethene (PCE)	8.796	166	682	0.33	ug/L		77
55) 1,3-Dichloropropane	9.289	76	299	0.09	ug/L	#	62
58) Chlorobenzene	9.928	112	1665	0.30	ug/L	#	53
59) Ethylbenzene	9.952	91	2525	0.27	ug/L		93
60) 1,1,1,2-Tetrachloroethane	9.989	131	250	0.15	ug/L	#	56
61) m,p-Xylenes (2)	10.086	91	3597	0.53	ug/L		99
62) o-Xylene	10.469	91	1736	0.26	ug/L		95
63) Styrene	10.518	104	1266	0.23	ug/L		98
65) Isopropylbenzene	10.731	105	1839	0.22	ug/L		96
68) Bromobenzene	11.066	156	575	0.27	ug/L	#	73
69) n-Propylbenzene	11.078	91	2840	0.31	ug/L		98
71) 2-Chlorotoluene	11.212	126	519	0.26	ug/L	#	70
72) 1,3,5-Trimethylbenzene	11.230	105	1758	0.28	ug/L		93

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102433.D  
 Acq On : 24 Oct 2019 11:05 pm  
 Operator : MM  
 Sample : 9J24043-ICV2  
 Misc : 1X 5mL 5/1250PPB OXY  
 ALS Vial : 20 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:52:56 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
75) 4-Chlorotoluene	11.339	91	2029	0.36	ug/L	92
76) tert-Butylbenzene	11.479	91	857	0.24	ug/L	90
77) 1,2,4-Trimethylbenzene	11.540	105	1902	0.30	ug/L	99
78) sec-Butylbenzene	11.619	105	2140	0.28	ug/L	96
79) 4-Isopropyltoluene	11.729	119	1814	0.30	ug/L	89
80) 1,3-Dichlorobenzene	11.802	146	1391	0.37	ug/L	91
81) 1,4-Dichlorobenzene	11.862	146	1580	0.40	ug/L #	77
82) n-Butylbenzene	12.051	91	2081	0.40	ug/L	97
83) 1,2-Dichlorobenzene	12.179	146	992	0.27	ug/L	94
85) Hexachlorobutadiene	13.304	223	253	0.50	ug/L	90
86) 1,2,4-Trichlorobenzene	13.347	180	1195	0.57	ug/L	98
87) Naphthalene	13.627	128	2373	0.36	ug/L	81
88) 1,2,3-Trichlorobenzene	13.785	180	1136	0.57	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102433.D  
Acq On : 24 Oct 2019 11:05 pm  
Operator : MM  
Sample : 9J24043-ICV2  
Misc : 1X 5mL 5/1250PPB OXY  
ALS Vial : 20 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:56 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102434.D  
 Acq On : 24 Oct 2019 11:32 pm  
 Operator : MM  
 Sample : 9J24043-IBL6  
 Misc : 1X 5mL DI  
 ALS Vial : 21 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 08:52:59 2019  
 Quant Method : C:\msdchem\1\methods\VI191025W.M  
 Quant Title : EPA 8260: Volatile Organic Compounds  
 QLast Update : Fri Oct 25 08:32:21 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene (I)	6.211	99	109647	50.00	ug/L	0.00
45) Chlorobenzene-d5 (I)	9.910	117	290801	50.00	ug/L	0.00
66) 1,4-Dichlorobenzene-d4...	11.850	152	129266	50.00	ug/L	0.00
System Monitoring Compounds						
32) Dibromofluoromethane (S)	5.712	111	106868	49.60	ug/L	0.00
39) 1,4-Difluorobenzene (S)	6.777	114	348077	50.25	ug/L	0.00
48) Toluene-d8 (S)	8.297	98	390388	51.15	ug/L	0.00
67) 4-Bromofluorobenzene (S)	10.974	174	109398	52.38	ug/L	0.00
Target Compounds						
						Qvalue
3) Chloromethane	1.891	50	233	0.10	ug/L	# 47
5) Bromomethane	2.360	96	288	0.21	ug/L	# 32
6) Chloroethane	2.500	64	219	0.20	ug/L	# 62
10) Carbon Disulfide	3.242	76	797	0.17	ug/L	78
14) Methylene Chloride	3.869	84	5477	1.87	ug/L	91
15) Acetone	3.942	43	1939	2.02	ug/L	95
19) tert-Butanol (TBA)	4.301	59	193	0.45	ug/L	46
61) m,p-Xylenes (2)	10.086	91	722	0.11	ug/L	86
79) 4-Isopropyltoluene	11.723	119	462	0.08	ug/L	51
81) 1,4-Dichlorobenzene	11.862	146	377	0.10	ug/L	# 1
82) n-Butylbenzene	12.045	91	599	0.12	ug/L	81
86) 1,2,4-Trichlorobenzene	13.341	180	337	0.17	ug/L	69
87) Naphthalene	13.633	128	630	0.10	ug/L	81
88) 1,2,3-Trichlorobenzene	13.785	180	159	0.09	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102434.D  
Acq On : 24 Oct 2019 11:32 pm  
Operator : MM  
Sample : 9J24043-IBL6  
Misc : 1X 5mL DI  
ALS Vial : 21 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:52:59 2019  
Quant Method : C:\msdchem\1\methods\VI191025W.M  
Quant Title : EPA 8260: Volatile Organic Compounds  
QLast Update : Fri Oct 25 08:32:21 2019  
Response via : Initial Calibration







Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102435.D  
 Acq On : 24 Oct 2019 11:59 pm  
 Operator : MM  
 Sample : 9J24043-TUN2  
 Misc : A19I040 BFB (IS/SURR)  
 ALS Vial : 22 Sample Multiplier: 1

*Handwritten:*  
 10/25/19

Integration File: APEXG.P

Method : C:\msdchem\1\methods\VI191025G.M  
 Title : NWTPH-Gx by GC/MS  
 Last Update : Fri Oct 25 10:31:05 2019



AutoFind: Scans 1543, 1544, 1545; Background Corrected with Scan 1536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
95	174	50	200	115.5	78893	PASS
96	95	5	9	6.6	5193	PASS
173	174	0.00	2	0.2	146	PASS
174	95	50	200	86.6	68315	PASS
175	174	5	9	7.2	4950	PASS
176	174	95	105	98.1	67045	PASS
177	176	5	10	6.4	4322	PASS

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102435.D  
 Acq On : 24 Oct 2019 11:59 pm  
 Operator : MM  
 Sample : 9J24043-TUN2  
 Misc : A19I040 BFB (IS/SURR)  
 ALS Vial : 22 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*Handwritten:*  
 d  
 10/25/19


Quant Time: Oct 25 10:34:47 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	210406	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	342441	50.05	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	110054	48.18	ug/L	0.00	
9) Toluene-d8 (NR)	8.298	98	383585	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	289628	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	210356	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	-629m	24.54	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	350597m	17.37	ug/L		
6) TPHg (C6-C10)	9.890	TIC	318995m	18.26	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	354669m	21.15	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102435.D  
Acq On : 24 Oct 2019 11:59 pm  
Operator : MM  
Sample : 9J24043-TUN2  
Misc : A19I040 BFB (IS/SURR)  
ALS Vial : 22 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M



Quant Time: Oct 25 10:34:47 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102436.D  
 Acq On : 25 Oct 2019 12:26 am  
 Operator : MM  
 Sample : 9J24043-RT1  
 Misc : A18A167 VPH RT STD  
 ALS Vial : 23 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:34:58 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



(4) NWTTPH-Gx (TPH) (H)

9.890min ( 0.000) 2930.43 ug/L m



response 19501721

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	1.04#
0.00	0.00	0.76#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102436.D  
 Acq On : 25 Oct 2019 12:26 am  
 Operator : MM  
 Sample : 9J24043-RT1  
 Misc : A18A167 VPH RT STD  
 ALS Vial : 23 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:34:58 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPh-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



(5) TPHg (C5-C9) (H)

9.890min ( 0.000) 973.75 ug/L m



response 8083029

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	2.52#
0.00	0.00	1.83#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102436.D  
 Acq On : 25 Oct 2019 12:26 am  
 Operator : MM  
 Sample : 9J24043-RT1  
 Misc : A18A167 VPH RT STD  
 ALS Vial : 23 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:34:58 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



(6) TPHg (C6-C10) (H)

9.890min ( 0.000) 1119.88 ug/L m



response 7845020

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	2.60#
0.00	0.00	1.88#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102436.D  
 Acq On : 25 Oct 2019 12:26 am  
 Operator : MM  
 Sample : 9J24043-RT1  
 Misc : A18A167 VPH RT STD  
 ALS Vial : 23 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:34:58 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



(7) CA-LUFT (C5-C12) (H)

9.890min ( 0.000) 1651.42 ug/L m

response 16435844

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	1.24#
0.00	0.00	0.90#
0.00	0.00	0.00

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102436.D  
 Acq On : 25 Oct 2019 12:26 am  
 Operator : MM  
 Sample : 9J24043-RT1  
 Misc : A18A167 VPH RT STD  
 ALS Vial : 23 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:34:58 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	218196	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	354554	49.97	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	120603	50.92	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	405063	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	307990	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	238057	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	19501721m	2930.43	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	8083029m	973.75	ug/L		
6) TPHg (C6-C10)	9.890	TIC	7845020m	1119.88	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	16435844m	1651.42	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102436.D  
Acq On : 25 Oct 2019 12:26 am  
Operator : MM  
Sample : 9J24043-RT1  
Misc : A18A167 VPH RT STD  
ALS Vial : 23 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:34:58 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWT PH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102437.D  
 Acq On : 25 Oct 2019 12:52 am  
 Operator : MM  
 Sample : 9J24043-IBL7  
 Misc : 1X 5mL DI  
 ALS Vial : 24 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 10:35:59 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene (IS)	6.217	168	210247	50.00	ug/L	0.00
System Monitoring Compounds						
2) 1,4-Difluorobenzene (Sur)	6.783	114	345936	50.60	ug/L	0.00
3) 4-Bromofluorobenzene (...)	10.974	174	111405	48.81	ug/L	0.00
9) Toluene-d8 (NR)	8.298	98	383628	0.00	ug/L	0.00
11) Chlorobenzene-d5 (NR)	9.910	117	292283	0.00	ug/L	0.00
12) 1,4-Dichlorobenzene-d4...	11.850	150	209732	0.00	ug/L	0.00
Target Compounds						
4) NWTPH-Gx (TPH)	9.890	TIC	24413m	28.59	ug/L	Qvalue
5) TPHg (C5-C9)	9.890	TIC	344892m	16.66	ug/L	
6) TPHg (C6-C10)	9.890	TIC	312692m	17.33	ug/L	
7) CA-LUFT (C5-C12)	9.890	TIC	358119m	21.55	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102437.D  
Acq On : 25 Oct 2019 12:52 am  
Operator : MM  
Sample : 9J24043-IBL7  
Misc : 1X 5mL DI  
ALS Vial : 24 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:35:59 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102438.D  
 Acq On : 25 Oct 2019 1:19 am  
 Operator : MM  
 Sample : 9J24043-ICB2  
 Misc : 1X 5mL DI  
 ALS Vial : 25 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*MM*  
*10/25/19*


Quant Time: Oct 25 10:36:04 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene (IS)	6.217	168	197519	50.00	ug/L	0.00
System Monitoring Compounds						
2) 1,4-Difluorobenzene (Sur)	6.783	114	324404	50.51	ug/L	0.00
3) 4-Bromofluorobenzene (...)	10.974	174	100113	46.69	ug/L	0.00
9) Toluene-d8 (NR)	8.298	98	365451	0.00	ug/L	0.00
11) Chlorobenzene-d5 (NR)	9.916	117	272946	0.00	ug/L	0.00
12) 1,4-Dichlorobenzene-d4...	11.850	150	191005	0.00	ug/L	0.00
Target Compounds						
4) NWTPH-Gx (TPH)	9.890	TIC	3183m	25.18	ug/L	Qvalue
5) TPHg (C5-C9)	9.890	TIC	344149m	19.44	ug/L	<i>MM</i>
6) TPHg (C6-C10)	9.890	TIC	310754m	20.11	ug/L	<i>MM</i>
7) CA-LUFT (C5-C12)	9.890	TIC	344897m	22.51	ug/L	<i>MM</i>

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102438.D  
Acq On : 25 Oct 2019 1:19 am  
Operator : MM  
Sample : 9J24043-ICB2  
Misc : 1X 5mL DI  
ALS Vial : 25 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:36:04 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102439.D  
 Acq On : 25 Oct 2019 1:46 am  
 Operator : MM  
 Sample : 9J24043-CALC  
 Misc : 1X 5mL 50PPB GX  
 ALS Vial : 26 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*Handwritten:*  
 ✓  
 10/25/19


Quant Time: Oct 25 08:55:14 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Tue Aug 06 09:35:12 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	209290	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.777	114	341977	48.13	ug/L	-0.01	
3) 4-Bromofluorobenzene (...)	10.974	174	109139	43.97	ug/L	0.00	
9) Toluene-d8 (NR)	8.298	98	385632	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	289080	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	203847	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	193702m	55.98	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	646954m	48.30	ug/L		
6) TPHg (C6-C10)	9.890	TIC	557886m	49.25	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	681991m	46.79	ug/L		
8) Benzene (NR)	6.120	78	3046	No	Calib		
10) Toluene (NR)	8.358	91	26962	No	Calib		
13) Naphthalene (NR)	13.633	128	1492	No	Calib		#

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102439.D  
Acq On : 25 Oct 2019 1:46 am  
Operator : MM  
Sample : 9J24043-CALC  
Misc : 1X 5mL 50PPB GX  
ALS Vial : 26 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:14 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Tue Aug 06 09:35:12 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102440.D  
 Acq On : 25 Oct 2019 2:13 am  
 Operator : MM  
 Sample : 9J24043-CALD  
 Misc : 1X 5mL 100PPB GX  
 ALS Vial : 27 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*W  
10/25/19*

Quant Time: Oct 25 08:55:16 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWT PH-Gx by GC/MS  
 QLast Update : Tue Aug 06 09:35:12 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	209478	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	342473	48.16	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	110020	44.29	ug/L	0.00	
9) Toluene-d8 (NR)	8.298	98	383736	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	289519	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	212572	0.00	ug/L	0.00	
Target Compounds							
4) NWT PH-Gx (TPH)	9.890	TIC	430822m	90.27	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	918071m	78.43	ug/L		
6) TPHg (C6-C10)	9.890	TIC	799328m	81.58	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	1014687m	77.57	ug/L		
8) Benzene (NR)	6.126	78	5908	No	Calib		
10) Toluene (NR)	8.358	91	53262	No	Calib		
13) Naphthalene (NR)	13.627	128	1678	No	Calib		#

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102440.D  
Acq On : 25 Oct 2019 2:13 am  
Operator : MM  
Sample : 9J24043-CALD  
Misc : 1X 5mL 100PPB GX  
ALS Vial : 27 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:16 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Tue Aug 06 09:35:12 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102441.D  
 Acq On : 25 Oct 2019 2:40 am  
 Operator : MM  
 Sample : 9J24043-CALE  
 Misc : 1X 5mL 250PPB GX  
 ALS Vial : 28 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*aw*  
*10/25/19*


Quant Time: Oct 25 08:55:19 2019  
 Quant Method : C:\msdchem\1\methods\VI-191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Tue Aug 06 09:35:12 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	220921	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.777	114	357958	47.73	ug/L	-0.01	
3) 4-Bromofluorobenzene (...)	10.974	174	116770	44.57	ug/L	0.00	
9) Toluene-d8 (NR)	8.298	98	404018	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	307058	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	223658	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	1374008m	216.41	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	2153713m	203.72	ug/L		
6) TPHg (C6-C10)	9.890	TIC	1839524m	208.44	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	2493143m	202.69	ug/L		
8) Benzene (NR)	6.120	78	15473	No	Calib		
10) Toluene (NR)	8.358	91	140638	No	Calib		
13) Naphthalene (NR)	13.627	128	3143	No	Calib		#

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102441.D  
Acq On : 25 Oct 2019 2:40 am  
Operator : MM  
Sample : 9J24043-CALE  
Misc : 1X 5mL 250PPB GX  
ALS Vial : 28 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:19 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Tue Aug 06 09:35:12 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102442.D  
 Acq On : 25 Oct 2019 3:07 am  
 Operator : MM  
 Sample : 9J24043-CALF  
 Misc : 1X 5mL 500PPB GX  
 ALS Vial : 29 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*MM*  
*10/25/19*


Quant Time: Oct 25 08:55:22 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWT PH-Gx by GC/MS  
 QLast Update : Tue Aug 06 09:35:12 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	214780	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	347086	47.60	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	115043	45.16	ug/L	0.00	
9) Toluene-d8 (NR)	8.298	98	395742	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	299444	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	223960	0.00	ug/L	0.00	
Target Compounds							
4) NWT PH-Gx (TPH)	9.890	TIC	2976997m	447.66	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	4135130m	425.95	ug/L		
6) TPHg (C6-C10)	9.890	TIC	3507779m	433.73	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	4877141m	424.71	ug/L		
8) Benzene (NR)	6.120	78	31187	No	Calib		
10) Toluene (NR)	8.358	91	281045	No	Calib		
13) Naphthalene (NR)	13.627	128	6060	No	Calib		#

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102442.D  
Acq On : 25 Oct 2019 3:07 am  
Operator : MM  
Sample : 9J24043-CALF  
Misc : 1X 5mL 500PPB GX  
ALS Vial : 29 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:22 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Tue Aug 06 09:35:12 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102443.D  
 Acq On : 25 Oct 2019 3:34 am  
 Operator : MM  
 Sample : 9J24043-CALG  
 Misc : 1X 5mL 1000PPB GX  
 ALS Vial : 30 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

*W*  
*10/25/19*


Quant Time: Oct 25 08:55:25 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWT PH-Gx by GC/MS  
 QLast Update : Tue Aug 06 09:35:12 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	211453	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	348407	48.54	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	115114	45.90	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	392439	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	298529	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	222551	0.00	ug/L	0.00	
Target Compounds							
4) NWT PH-Gx (TPH)	9.890	TIC	4888792m	727.40	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	5510904m	585.41	ug/L		
6) TPHg (C6-C10)	9.890	TIC	4867313m	622.06	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	6835714m	611.85	ug/L		
8) Benzene (NR)	6.119	78	58175	No Calib			
10) Toluene (NR)	8.358	91	520899	No Calib			
13) Naphthalene (NR)	13.627	128	12132	No Calib			

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102443.D  
Acq On : 25 Oct 2019 3:34 am  
Operator : MM  
Sample : 9J24043-CALG  
Misc : 1X 5mL 1000PPB GX  
ALS Vial : 30 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:25 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Tue Aug 06 09:35:12 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102444.D  
 Acq On : 25 Oct 2019 4:00 am  
 Operator : MM  
 Sample : 9J24043-CALH  
 Misc : 1X 5mL 2500PPB GX  
 ALS Vial : 31 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:28 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Tue Aug 06 09:35:12 2019  
 Response via : Initial Calibration

*MM*  
*10/25/19*


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	216435	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	352248	47.94	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	120135	46.80	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	398721	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	303642	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	237458	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	16775203m	2359.89	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	21028250m	2263.03	ug/L		
6) TPHg (C6-C10)	9.890	TIC	17780255m	2293.78	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	25461195m	2277.93	ug/L		
8) Benzene (NR)	6.119	78	158403	No	Calib		
10) Toluene (NR)	8.358	91	1477009	No	Calib		
13) Naphthalene (NR)	13.627	128	35052	No	Calib		

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102444.D  
Acq On : 25 Oct 2019 4:00 am  
Operator : MM  
Sample : 9J24043-CALH  
Misc : 1X 5mL 2500PPB GX  
ALS Vial : 31 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:28 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWT PH-Gx by GC/MS  
QLast Update : Tue Aug 06 09:35:12 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102445.D  
 Acq On : 25 Oct 2019 4:27 am  
 Operator : MM  
 Sample : 9J24043-CALI  
 Misc : 1X 5mL 5000PPB GX  
 ALS Vial : 32 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:31 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Tue Aug 06 09:35:12 2019  
 Response via : Initial Calibration


*W  
10/25/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	233849	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	379658	47.83	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	131653	47.47	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	428988	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	328511	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	265485	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	36698243m	4712.25	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	44004926m	4445.71	ug/L		
6) TPHg (C6-C10)	9.890	TIC	37352617m	4504.22	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	53937364m	4503.02	ug/L		
8) Benzene (NR)	6.119	78	331579	No	Calib		
10) Toluene (NR)	8.358	91	3164737	No	Calib		
13) Naphthalene (NR)	13.627	128	80787	No	Calib		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102445.D  
Acq On : 25 Oct 2019 4:27 am  
Operator : MM  
Sample : 9J24043-CALI  
Misc : 1X 5mL 5000PPB GX  
ALS Vial : 32 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:31 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Tue Aug 06 09:35:12 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102446.D  
 Acq On : 25 Oct 2019 4:54 am  
 Operator : MM  
 Sample : 9J24043-CALJ  
 Misc : 1X 5mL 10000PPB GX  
 ALS Vial : 33 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:34 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Tue Aug 06 09:35:12 2019  
 Response via : Initial Calibration


*W*  
*10/25/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	234183	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	384961	48.42	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	134509	48.43	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	441445	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	336849	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	271148	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	79562476m	9992.42	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	92937489m	9609.74	ug/L		
6) TPHg (C6-C10)	9.890	TIC	79339461m	9683.51	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	114341182m	9654.93	ug/L		
8) Benzene (NR)	6.126	78	681943	No	Calib		
10) Toluene (NR)	8.358	91	6524048	No	Calib		
13) Naphthalene (NR)	13.627	128	171453	No	Calib		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102446.D  
Acq On : 25 Oct 2019 4:54 am  
Operator : MM  
Sample : 9J24043-CALJ  
Misc : 1X 5mL 10000PPB GX  
ALS Vial : 33 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 08:55:34 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Tue Aug 06 09:35:12 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102447.D  
 Acq On : 25 Oct 2019 5:21 am  
 Operator : MM  
 Sample : 9J24043-IBL8  
 Misc : 1X 5mL DI  
 ALS Vial : 34 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 10:36:23 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	220300	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	358131	50.00	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	115759	48.41	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	401614	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	304304	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	217857	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	67010m	34.98	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	462754m	29.19	ug/L		
6) TPHg (C6-C10)	9.890	TIC	415778m	30.25	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	479273m	32.16	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102447.D  
Acq On : 25 Oct 2019 5:21 am  
Operator : MM  
Sample : 9J24043-IBL8  
Misc : 1X 5mL DI  
ALS Vial : 34 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:36:23 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102448.D  
 Acq On : 25 Oct 2019 5:48 am  
 Operator : MM  
 Sample : 9J24043-IBL9  
 Misc : 1X 5mL DI  
 ALS Vial : 35 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:36:26 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	224165	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	364141	49.96	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	116148	47.73	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	404017	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	307716	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	221768	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	6246m	25.58	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	423048m	23.38	ug/L		
6) TPHg (C6-C10)	9.890	TIC	367482m	22.24	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	414999m	24.87	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102448.D  
Acq On : 25 Oct 2019 5:48 am  
Operator : MM  
Sample : 9J24043-IBL9  
Misc : 1X 5mL DI  
ALS Vial : 35 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:36:26 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102449.D  
 Acq On : 25 Oct 2019 6:15 am  
 Operator : MM  
 Sample : NOT USED-ICV3  
 Misc : 1X 5mL 500PPB GX  
 ALS Vial : 36 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 10:36:29 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	210169	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	342543	50.13	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	111447	48.85	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	389625	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	294881	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	215811	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	3057398m	515.56	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	4012577m	490.15	ug/L		
6) TPHg (C6-C10)	9.890	TIC	3490261m	503.63	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	4796224m	494.15	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102449.D  
Acq On : 25 Oct 2019 6:15 am  
Operator : MM  
Sample : NOT USED-ICV3  
Misc : 1X 5mL 500PPB GX  
ALS Vial : 36 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:36:29 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102450.D  
 Acq On : 25 Oct 2019 6:42 am  
 Operator : MM  
 Sample : 9J24043-IBLA  
 Misc : 1X 5mL DI  
 ALS Vial : 37 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 10:36:32 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
-----							
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	220005	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	355641	49.72	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	113694	47.61	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	395183	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	297812	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	216661	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	1338m	24.84	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	395852m	20.99	ug/L		
6) TPHg (C6-C10)	9.890	TIC	356830m	21.68	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	380718m	22.16	ug/L		
-----							

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102450.D  
Acq On : 25 Oct 2019 6:42 am  
Operator : MM  
Sample : 9J24043-IBLA  
Misc : 1X 5mL DI  
ALS Vial : 37 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:36:32 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102451.D  
 Acq On : 25 Oct 2019 9:37 am  
 Operator : MM  
 Sample : 9J24043-IBLB  
 Misc : 1X 5mL DI  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M


Quant Time: Oct 25 10:36:35 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	220874	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	362775	50.51	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	117808	49.14	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	408461	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	309494	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	224643	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	516538m	104.07	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	1099818m	107.51	ug/L		
6) TPHg (C6-C10)	9.890	TIC	929473m	105.15	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	1204383m	105.77	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102451.D  
Acq On : 25 Oct 2019 9:37 am  
Operator : MM  
Sample : 9J24043-IBLB  
Misc : 1X 5mL DI  
ALS Vial : 2 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:36:35 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWT PH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102452.D  
 Acq On : 25 Oct 2019 10:13 am  
 Operator : MM  
 Sample : 9J24043-CALG  
 Misc : 1X 5mL 1000PPB GX  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:30:48 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 09:04:24 2019  
 Response via : Initial Calibration

*MM*  
*10/25/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	234293	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	376297	49.24	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	126230	49.57	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	425778	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.916	117	321320	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	240304	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	6735895m	1025.45	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	9031832m	1085.81	ug/L		
6) TPHg (C6-C10)	9.890	TIC	7648071m	1079.95	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	10733621m	1066.65	ug/L		
8) Benzene (NR)	6.126	78	64412	No	Calib		
10) Toluene (NR)	8.358	91	587525	No	Calib		
13) Naphthalene (NR)	13.627	128	13369	No	Calib		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

*Re-processed*  
*@*  
*10/25/19*



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102452.D  
Acq On : 25 Oct 2019 10:13 am  
Operator : MM  
Sample : 9J24043-CALG  
Misc : 1X 5mL 1000PPB GX  
ALS Vial : 3 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:30:48 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 09:04:24 2019  
Response via : Initial Calibration



Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102453.D  
 Acq On : 25 Oct 2019 10:40 am  
 Operator : MM  
 Sample : 9J24043-ICV3  
 Misc : 1X 5mL 500PPB GX  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:55:48 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) Pentafluorobenzene (IS)	6.217	168	221958	50.00	ug/L	0.00	
System Monitoring Compounds							
2) 1,4-Difluorobenzene (Sur)	6.783	114	358721	49.70	ug/L	0.00	
3) 4-Bromofluorobenzene (...)	10.974	174	117543	48.79	ug/L	0.00	
9) Toluene-d8 (NR)	8.297	98	403727	0.00	ug/L	0.00	
11) Chlorobenzene-d5 (NR)	9.910	117	307598	0.00	ug/L	0.00	
12) 1,4-Dichlorobenzene-d4...	11.850	150	224832	0.00	ug/L	0.00	
Target Compounds							
4) NWTPH-Gx (TPH)	9.890	TIC	3205343m	512.01	ug/L		Qvalue
5) TPHg (C5-C9)	9.890	TIC	4234043m	489.71	ug/L		
6) TPHg (C6-C10)	9.890	TIC	3681976m	503.04	ug/L		
7) CA-LUFT (C5-C12)	9.890	TIC	5059070m	493.53	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
 Data File : VI19102453.D  
 Acq On : 25 Oct 2019 10:40 am  
 Operator : MM  
 Sample : 9J24043-ICV3  
 Misc : 1X 5mL 500PPB GX  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:55:48 2019  
 Quant Method : C:\msdchem\1\methods\VI191025G.M  
 Quant Title : NWTPH-Gx by GC/MS  
 QLast Update : Fri Oct 25 10:31:05 2019  
 Response via : Initial Calibration



(4) NWTPH-Gx (TPH) (H)

9.890min ( 0.000) 512.01 ug/L m


response 3205343

Signal	Exp%	Act%
TIC	100.00	100.00
0.00	0.00	0.02#
0.00	0.00	0.01#
0.00	0.00	0.00

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-10\9J24043\  
Data File : VI19102453.D  
Acq On : 25 Oct 2019 10:40 am  
Operator : MM  
Sample : 9J24043-ICV3  
Misc : 1X 5mL 500PPB GX  
ALS Vial : 4 Sample Multiplier: 1  
DataAcq Meth:VI1611RUN.M

Quant Time: Oct 25 10:55:48 2019  
Quant Method : C:\msdchem\1\methods\VI191025G.M  
Quant Title : NWTPH-Gx by GC/MS  
QLast Update : Fri Oct 25 10:31:05 2019  
Response via : Initial Calibration



**TCLP Organochloride Pesticides by EPA 8081B  
Benchsheet & Analysis Sequence Data**

Batch 9111243  
Sequence 9K27028 (A9K0412-01)



**Apex Laboratories**  
**PREPARATION BENCH SHEET**

DEC 02 2019

BATCH #: 9111243 (Soil)

Prep Method: EPA 1311/3510C (Neutral Ext.)

#	Lab Number	Analysis	Prepared	Initial (mL)	Final (mL)	Spike ID	Source ID	ul Spike	ul Surr.	Sample ID	Extraction Comments	pH		
												<2	5	>11
	9111243-BLK1	QC	11/26/19 14:06	200	5				100					
	9111243-BSD1	QC	11/26/19 14:06	200	5	A19K227		100	100					
	9111243-BS1	QC	11/26/19 14:06	200	5	A19K227		100	100					
	A9K0412-01	A 1311/8081B TCLP Pest Reg List	11/26/19 14:06	200	5				100	PDI-142RAB-C-00-30.4-191112				

**Standards/Reagents**

Reagent(s)			Analyte Spike(s)			Surrogate(s)		
Std ID	Exp. Date	Description	Std ID	Exp. Date	Description	Std ID	Exp. Date	Description
A18K311	12/31/20	Glass Wool	A19K227	05/07/20	Mix AB Pesticide Matrix Spike	A19K052	04/17/20	8082 PCB Surrogate Spike
A19H411	08/31/21	n-Hexane Lot# 192712						
A19I263	03/18/20	DCM CHEM PROD. 194934						
A19K010	10/29/25	Sodium Sulfate Lot # 188777						

3x rinse

Witness: \_\_\_\_\_

Prepared By: \_\_\_\_\_ Date \_\_\_\_\_

Reviewed By: MJB Date: 11/27/19



**Apex Laboratories**  
**PREPARATION BENCH SHEET**

BATCH #: 9111243 (Soil)

Prep Method: EPA 1311/3510C (Neutral Ext.)

#	Lab Number	Analysis	Prepared	Initial (mL)	Final (mL)	Spike ID	Source ID	ul Spike	ul Surr.	Sample ID	Extraction Comments	pH			
												<2	2-11	>11	
	9111243-BLK1	QC	11/26/19 14:06	200	5				100						
	9111243-BSD1	QC	11/26/19 14:06	200	5	A19K227		100	100		X				
	9111243-BS1	QC	11/26/19 14:06	200	5	A19K227		100	100		X				
	A9K0412-01	A 1311/8081B TCLP Pest Reg List	11/26/19 14:06	200	5				100	PDI-142RAB-C-00-30.4-191112					

**Standards/Reagents**

Reagent(s)			Analyte Spike(s)			Surrogate(s)		
Std ID	Exp. Date	Description	Std ID	Exp. Date	Description	Std ID	Exp. Date	Description
A18K311	12/31/20	Glass Wool	A19K227	05/07/20	Mix AB Pesticide Matrix Spike	A19K052	04/17/20	8082 PCB Surrogate Spike
A19I263	03/18/20	DCM CHEM PROD. 194934						
A19K010	10/29/25	Sodium Sulfate Lot # 188777						
A19H411		n-Hexane						

3x rinse

Witness: CAS 11/26/19

X = NO BLK fluid added

2mL exchanged into 2mL of  
Hexane CWH  
11/26/19

CWH 11/26/19  
Prepared By: \_\_\_\_\_ Date

CWH 11/26/19  
Reviewed By: \_\_\_\_\_ Date



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence: **9K27028**

Instrument: **DUALECD5**

Date: **11/27/19 11:05**

Calibration: **A9H2608**

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
1	9K27028-BKD1	Soil	QC	QC				A19J201
2	9K27028-CCV1	Soil	QC	QC				A19K133
3	9K27028-BKD2	Soil	QC	QC				A19J201
4	9K27028-CCV2	Soil	QC	QC				A19K133
5	9K27028-CCB1	Soil	QC	QC				A19K026
6	9111243-BLK1	Soil	QC	QC		9111243		
7	9111243-BS1	Soil	QC	QC		9111243		
8	9111243-BSD1	Soil	QC	QC		9111243		
9	A9K0412-01	Soil	1311/8081B TCLP Pest Reg List	Anchor QEA, LLC	11/27/19	9111243		
10	9K27028-CCV3	Soil	QC	QC				A19K134
11	9K27028-CCB2	Soil	QC	QC				A19K026

Data Entered By: MJB 11/27/19

Comments:



Data Reviewed By: MV7 11/27/19



Quantitation Report (QT Reviewed)

Data Path : C:\msdchem\4\data\2019-11\9K27028\  
Data File : ECD5-11271904.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 12:24  
Operator : MJB  
Sample : 9K27028-BKD1  
Misc : A19J201  
ALS Vial : 2 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 12:42:56 2019  
Quant Method : C:\msdchem\4\methods\PestBreakdownCHK\_190823RT8.M  
Quant Title : Pesticides  
QLast Update : Thu Aug 21 11:53:22 2014  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271905.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 12:41  
 Operator : MJB  
 Sample : 9K27028-CCV1  
 Misc : A19K133, AB 50 ppb  
 ALS Vial : 3 (Sig #1); 0 (Sig #2) Sample Multiplier: 1  
 Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 14:17:31 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT8.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*Q-14*

*MJB  
11/27/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.226	5.816	8060097	13325730	48.562	45.423
22) S DCBP (S)	9.415	10.329	6016939	8622247	42.643	47.965
Target Compounds						
2) a-BHC	5.760	6.421	10122494	18011375	44.140	43.894
3) g-BHC	6.042	6.739	8087095	14629135	40.079	41.012
4) b-BHC	6.119	6.806	2910913	5573802	32.206	35.218
5) Heptachlor	6.451	7.108	6661618	11824322	36.744	38.644
6) d-BHC	6.267	7.057	6156033	13210435	31.298	37.459
7) Aldrin	6.690	7.371	8764497	15484918	44.389	47.011
8) Heptachlo...	7.149	7.809	7459335	12252092	40.501	40.725
9) trans-Chl...	7.245	7.947	7806384	12608561	42.221	40.241
10) cis-Chlor...	7.342	8.055	7461847	12857242	40.983	44.146
11) Endosulfa...	7.436	8.103	7402427	11227299	43.498	40.800
12) 4,4'-DDE	7.412	8.168	7549228	13149677	40.043	42.326
13) Dieldrin	7.608	8.303	8183774	13373676	42.628	43.971
14) Endrin	7.771	8.528	5514782	8349075	37.509	36.971
15) 4,4'-DDD	7.831	8.582	5335342	9566744	33.953	37.339
16) Endosulfa...	7.926	8.676	6042301	10419588	42.074	45.183
17) 4,4'-DDT	8.027	8.805	3721324	6037747	31.125	33.080
18) Endrin Al...	8.216	8.912	5102610	8672974	41.633	44.292
19) Endosulfa...	8.516	9.103	5694376	9142266	36.743	36.703
20) Methoxychlor	8.367	9.285	1795573	3042528	30.655	34.925
21) Endrin Ke...	8.707	9.497	6503883	10135812	39.002	39.391
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	6.330f	0	106471	N.D.	0.339 #
25) Oxychlorthane	7.085	7.772	33989	91831	0.207	0.335 #
26) 2,4'-DDE	7.149f	7.984	7459335	143301	58.157	0.676 #
27) trans-Non...	7.342	8.055	7461847	12857242	41.352	42.625
28) 2,4'-DDD	0.000	8.303f	0	13373676	N.D.	70.811 #
29) 2,4'-DDT	7.713	8.582f	25004	9566744	0.228	53.643 #
30) cis-Nonac...	7.831	8.582	5335342	9566744	25.698	28.519
31) Mirex	8.466	9.497	59350	10135812	0.473	54.472 #
32) Chlordane...	7.245	7.984	7806384	143301	396.472	3.960 #
33) Chlordane...	7.342	8.055f	7461847	12857242	297.708	423.436 #
34) Chlordane...	7.926f	8.724	6042301	108113	1045.178	12.058 #
35) Chlordane...	0.000	0.000	0	0	N.D.	N.D.
36) Toxaphene...	7.342	8.303	7461847	13373676	8331.232	5096.174
37) Toxaphene...	7.608	8.676f	8183774	10419588	5067.545	3166.061
38) Toxaphene...	7.926	8.676	6042301	10419588	1794.305	2055.828
39) Toxaphene...	0.000	8.754	0	98450	N.D.	11.791 #
40) Toxaphene...	8.367f	8.912	1795573	8672974	749.047	1861.010 #
41) Toxaphene...	8.466	9.285	59350	3042528	18.755	640.505 #
42) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
Data File : ECD5-11271905.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 12:41  
Operator : MJB  
Sample : 9K27028-CCV1  
Misc : A19K133, AB 50 ppb  
ALS Vial : 3 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 14:17:31 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT8.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Pesticide BKD

**Pesticide Breakdown Check (Validated 8/8/2013)**

Sequence: 9K27028 BKD2  
Data File: ECD5-11271907.D

First Column Area Counts		Percent Breakdown	
DDE	505149		
DDD	6455464		
DDT	109416167	<b>5.98</b>	<b>PASS</b>
Endrin	65409695	<b>14.83</b>	<b>PASS</b>
Endrin Aldehyde	3431975		
Endrin Ketone	7954086		

Second Column Area Counts		Percent Breakdown	
DDE	908095		
DDD	9573606		
DDT	163705443	<b>6.02</b>	<b>PASS</b>
Endrin	97916440	<b>13.83</b>	<b>PASS</b>
Endrin Aldehyde	4749737		
Endrin Ketone	10960509		

Breakdown must be less than 15% to accept sample data.

*MB*  
*11/27/19*

Data Path : C:\msdchem\4\data\2019-11\9K27028\  
 Data File : ECD5-11271907.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 13:40  
 Operator : MJB  
 Sample : 9K27028-BKD2  
 Misc : A19J201  
 ALS Vial : 2 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 14:05:45 2019  
 Quant Method : C:\msdchem\4\methods\PestBreakdownCHK\_190823RT9.M  
 Quant Title : Pesticides  
 QLast Update : Thu Aug 21 11:53:22 2014  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*RT update*

Compound	R.T.	Response	Conc Units
-----			
Target Compounds			
1) 4,4'-DDE	7.397	505149	NoCal ng/mL
2) Endrin	7.759	65409695	NoCal ng/mL
3) 4,4'-DDD	7.815	6455464	NoCal ng/mL
4) 4,4'-DDT	8.012	109416167	NoCal ng/mL
5) Endrin Aldehyde	8.202	3431975	NoCal ng/mL
6) Endrin Ketone	8.693	7954086	NoCal ng/mL
8) 4,4'-DDE [2C]	8.156	908095	NoCal ng/mL
9) Endrin [2C]	8.518	97916440	NoCal ng/mL
10) 4,4'-DDD [2C]	8.569	9573606	NoCal ng/mL
11) Endrin Aldehyde [2C]	8.901	4749737	NoCal ng/mL
12) 4,4'-DDT [2C]	8.794	163705443	NoCal ng/mL
13) Endrin Ketone [2C]	9.485	10960509	NoCal ng/mL
-----			

(f)=RT Delta > 1/2 Window

(m)=manual int.



*Replaced inlet liner & cut  
 ~ 7" off guard column.*

*MJB  
 11/27/19*

Quantitation Report (QT Reviewed)

Data Path : C:\msdchem\4\data\2019-11\9K27028\  
Data File : ECD5-11271907.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 13:40  
Operator : MJB  
Sample : 9K27028-BKD2  
Misc : A19J201  
ALS Vial : 2 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 14:05:45 2019  
Quant Method : C:\msdchem\4\methods\PestBreakdownCHK\_190823RT9.M  
Quant Title : Pesticides  
QLast Update : Thu Aug 21 11:53:22 2014  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271908.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 13:58  
 Operator : MJB  
 Sample : 9K27028-CCV2  
 Misc : A19K133, AB 50 ppb  
 ALS Vial : 3 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 14:24:50 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M *RT update*  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJP 11/27/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.216	5.807	8328148	14419781	50.177	49.153
22) S DCBP (S)	9.401	10.317	6553370	9087512	46.445	50.553
Target Compounds						
2) a-BHC	5.750	6.412	11714153	20837003	51.080	50.780
3) g-BHC	6.031	6.729	9968727	17256181	49.405	48.377
4) b-BHC	6.108	6.795	3938626	6971022	43.577	44.046
5) Heptachlor	6.440	7.098	8887661	14462151	49.023	47.265
6) d-BHC	6.254	7.047	8999104	16805371	45.753	47.652
7) Aldrin	6.678	7.360	9774664	17445923	49.506	52.964
8) Heptachlo...	7.138	7.798	8884360	14236118	48.238	47.320
9) trans-Chl...	7.233	7.937	9172647	14790032	49.611	47.203
10) cis-Chlor...	7.330	8.045	8747521	14114068	48.045	48.461
11) Endosulfa...	7.424	8.093	8373981	13076263	49.207	47.520
12) 4,4'-DDE	7.398	8.156	9308737	15415054	49.375	49.618
13) Dieldrin	7.596	8.293	9510262	14886490	49.538	48.945
14) Endrin	7.759	8.518	7396973	11519812	50.310	51.012
15) 4,4'-DDD	7.815	8.570	7348004	11896402	46.761	46.432
16) Endosulfa...	7.914	8.665	7237621	11862500	50.397	51.441
17) 4,4'-DDT	8.013	8.794	6050717	9265895	50.608	49.333
18) Endrin Al...	8.202	8.902	6158839	9695881	50.169	49.329
19) Endosulfa...	8.502	9.092	7012909	10913008	45.251	43.812
20) Methoxychlor	8.351	9.273	3092830	4615363	52.802	51.335
21) Endrin Ke...	8.694	9.486	7945103	12091700	47.644	46.992
23) Hexachlor...	3.024	3.568f	23068	5416	0.126	0.014 #
24) Hexachlor...	5.572f	6.320f	19217	16932	0.109	0.054 #
25) Oxychlorthane	7.074	7.762	39238	31354	0.238	0.114 #
26) 2,4'-DDE	7.138f	7.937	8884360	14790032	69.268	69.719
27) trans-Non...	7.330	8.045f	8747521	14114068	48.535	46.792
28) 2,4'-DDD	7.513	8.293f	21773	14886490	0.191	78.821 #
29) 2,4'-DDT	7.700	8.570f	27781	11896402	0.253	66.707 #
30) cis-Nonac...	7.815	8.570	7348004	11896402	35.392	35.464
31) Mirex	8.451	9.486	38681	12091700	0.309	64.984 #
32) Chlordane...	7.233	7.937	9172647	14790032	465.862	408.739
33) Chlordane...	7.330	8.045	8747521	14114068	349.003	464.828
34) Chlordane...	7.914f	8.707	7237621	82879	1251.941	9.244 #
35) Chlordane...	3.477	0.000	27163	0	NoCal	N.D.
36) Toxaphene...	7.330	8.293	8747521	14886490	9766.701	5672.647 #
37) Toxaphene...	7.596	8.665f	9510262	11862500	5888.931	3604.500
38) Toxaphene...	7.914	8.665	7237621	11862500	2149.263	2340.521
39) Toxaphene...	0.000	8.743	0	39773	N.D.	4.763 #
40) Toxaphene...	8.411f	8.902	17664	9695881	7.369	2080.501 #
41) Toxaphene...	8.451	9.273	38681	4615363	12.223	971.614 #
42) Toxaphene...	3.477	0.000	27163	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
Data File : ECD5-11271908.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 13:58  
Operator : MJB  
Sample : 9K27028-CCV2  
Misc : A19K133, AB 50 ppb  
ALS Vial : 3 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 14:24:50 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271909.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 14:15  
 Operator : MJB  
 Sample : 9K27028-CCB1  
 Misc : A19K026  
 ALS Vial : 5 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 14:31:25 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
11/27/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.215	5.806	15034283	26886105	90.581	91.647
22) S DCBP (S)	9.401	10.318	11969769	16895469	84.833	93.987
Target Compounds						
2) a-BHC	5.774f	0.000	3888	0	0.017	N.D. #
3) g-BHC	0.000	0.000	0	0	N.D.	N.D.
4) b-BHC	6.098	0.000	5927	0	0.066	N.D. #
5) Heptachlor	0.000	0.000	0	0	N.D.	N.D.
6) d-BHC	6.256	7.047	3651	5365	0.019	0.015
7) Aldrin	0.000	7.389f	0	19415	N.D.	0.059 #
8) Heptachlo...	0.000	0.000	0	0	N.D.	N.D.
9) trans-Chl...	7.219	0.000	18548	0	0.100	N.D. #
10) cis-Chlor...	7.317	0.000	3249	0	0.018	N.D. #
11) Endosulfa...	0.000	0.000	0	0	N.D.	N.D.
12) 4,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
13) Dieldrin	0.000	0.000	0	0	N.D.	N.D.
14) Endrin	0.000	8.526	0	6285	N.D.	0.028 #
15) 4,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
16) Endosulfa...	7.907	8.652	9621	10850	0.067	0.047
17) 4,4'-DDT	0.000	8.811	0	7967	N.D.	0.008 #
18) Endrin Al...	8.200	8.900	5301	6165	BelowCal	BelowCal
19) Endosulfa...	8.502	9.091	6818	8101	0.044	0.033
20) Methoxychlor	8.340	9.263	10573	1046	0.181	BelowCal #
21) Endrin Ke...	8.710	9.488	8250	14505	0.049	0.056
23) Hexachlor...	0.000	3.570f	0	3915	N.D.	0.010 #
24) Hexachlor...	5.594	0.000	16256	0	0.092	N.D. #
25) Oxychlorane	7.063	0.000	8660	0	0.053	N.D. #
26) 2,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
27) trans-Non...	7.317	0.000	3249	0	87346.682	N.D. #
28) 2,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
29) 2,4'-DDT	7.678f	8.526f	4828	6285	0.044	0.035
30) cis-Nonac...	0.000	0.000	0	0	N.D.	N.D.
31) Mirex	8.458	9.488	25232	14505	0.201	0.078 #
32) Chlordane...	7.219f	0.000	18548	0	0.942	N.D. #
33) Chlordane...	7.317f	0.000	3249	0	0.130	N.D. #
34) Chlordane...	7.882	8.708	5193	47484	0.898	5.296 #
35) Chlordane...	0.000	0.000	0	0	N.D.	N.D.
36) Toxaphene...	7.317	0.000	3249	0	3.627	N.D. #
37) Toxaphene...	0.000	8.652	0	10850	N.D.	3.297 #
38) Toxaphene...	7.907	8.652	9621	10850	2.857	2.141
39) Toxaphene...	0.000	8.736	0	8193	N.D.	0.981 #
40) Toxaphene...	0.000	8.900	0	6165	N.D.	1.323 #
41) Toxaphene...	8.458	9.263f	25232	1046	7.973	0.220 #
42) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
Data File : ECD5-11271909.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 14:15  
Operator : MJB  
Sample : 9K27028-CCB1  
Misc : A19K026  
ALS Vial : 5 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 14:31:25 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271910.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 14:32  
 Operator : MJB  
 Sample : 9111243-BLK1  
 Misc : 1x, 1311/8081B TCLP Pest Reg List  
 ALS Vial : 6 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 14:47:48 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
11/27/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.215	5.805	12201753	22541325	73.515	76.837
22) S DCBP (S)	9.400	10.317	12245801	17045900	86.789	94.824
Target Compounds						
2) a-BHC	5.752	0.000	45939	0	0.200	N.D. #
3) g-BHC	6.034	6.726	23418	27733	0.116	0.078
4) b-BHC	6.092	6.784	88268	24347	0.977	0.154 #
5) Heptachlor	6.439	7.100	27197	38136	0.150	0.125
6) d-BHC	6.231f	7.022f	23667	28370	0.120	0.080
7) Aldrin	6.676	7.387f	23329	48351	0.118	0.147
8) Heptachlo...	7.136	7.780	17524	54400	0.095	0.181 #
9) trans-Chl...	7.217	7.940	33815	64061	0.183	0.204
10) cis-Chlor...	7.313	8.007f	44925	22466	0.247	0.077 #
11) Endosulfa...	7.426	8.103	26733	33230	0.157	0.121
12) 4,4'-DDE	7.373f	8.131f	17251	13320	0.092	0.043 #
13) Dieldrin	7.593	8.283	14383	15941	0.075	0.052
14) Endrin	7.769	8.522	12456	9752	0.085	0.043 #
15) 4,4'-DDD	7.830	8.567	11221	19230	0.071	0.075
16) Endosulfa...	7.903	8.649	144852	185622	1.009	0.805
17) 4,4'-DDT	8.050f	8.813	7667	13219	0.064	0.039
18) Endrin Al...	8.187	8.883	50149	65424	BelowCal	BelowCal
19) Endosulfa...	8.501	9.089	4724	6762	0.030	0.027
20) Methoxychlor	8.345	9.281	9394	3763	0.160	BelowCal #
21) Endrin Ke...	8.685	9.488	12341	81928	0.074	0.318 #
23) Hexachlor...	3.021	3.564f	54346	29901	0.297	0.080 #
24) Hexachlor...	5.593	6.296	45129	83907	0.256	0.267
25) Oxychlorane	7.058f	7.723f	116519	60822	0.708	0.222 #
26) 2,4'-DDE	7.171	7.940	15497	64061	0.121	0.302 #
27) trans-Non...	7.313f	8.007	44925	22466	87346.450	0.074 #
28) 2,4'-DDD	7.522	8.354f	29507	17196	0.259	0.091 #
29) 2,4'-DDT	7.674f	8.567f	10528	19230	0.096	0.108
30) cis-Nonac...	7.830f	8.567	11221	19230	0.054	0.057
31) Mirex	8.455	9.488	23289	81928	0.186	0.440 #
32) Chlordane...	7.265f	7.940	33778	64061	1.716	1.770
33) Chlordane...	7.313f	0.000	44925	0	1.792	N.D. #
34) Chlordane...	7.903f	8.706	144852	51858	25.056	5.784 #
35) Chlordane...	3.489	3.429f	45721	37542	NoCal	NoCal
36) Toxaphene...	7.313	8.283	44925	15941	50.160	6.074 #
37) Toxaphene...	7.593	8.649	14383	185622	8.906	56.402 #
38) Toxaphene...	7.903	8.649	144852	185622	43.015	36.624
39) Toxaphene...	8.187f	8.737	50149	10070	15.477	1.206 #
40) Toxaphene...	8.345f	8.941f	9394	4819	3.919	1.034 #
41) Toxaphene...	8.455	9.281	23289	3763	7.359	0.792 #
42) Toxaphene...	3.489	3.484f	45721	1230109	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
Data File : ECD5-11271910.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 14:32  
Operator : MJB  
Sample : 9111243-BLK1  
Misc : 1x, 1311/8081B TCLP Pest Reg List  
ALS Vial : 6 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 14:47:48 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271911.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 14:49  
 Operator : MJB  
 Sample : 9111243-BS1  
 Misc : 1x, 1311/8081B TCLP Pest Reg List  
 ALS Vial : 7 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 15:06:00 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
11/27/19



	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds							
1)	S TCMX (S)	5.214	5.805	13051639	23064632	78.636	78.620
22)	S DCBP (S)	9.400	10.315	11505893	16962996	81.545	94.363
Target Compounds							
2)	a-BHC	5.748	6.411	20441007	38553841	89.134	93.956
3)	g-BHC	6.029	6.727	17918277	32316147	88.802	90.597
4)	b-BHC	6.105	6.793	7472796	13238048	82.679	83.644
5)	Heptachlor	6.438	7.096	15332657	25464473	84.572	83.223
6)	d-BHC	6.252	7.044	17148161	33154635	87.184	94.011
7)	Aldrin	6.677	7.358	14881158	26270197	75.368	79.753
8)	Heptachlo...	7.135	7.797	16118644	26873301	87.516	89.325
9)	trans-Chl...	7.231	7.935	15938639	26639491	86.205	85.022
10)	cis-Chlor...	7.328	8.043	15012262	24959897	82.453	85.700
11)	Endosulfa...	7.422	8.091	14992047	24572494	88.095	89.297
12)	4,4'-DDE	7.396	8.155	15088893	26034985	80.034	83.801
13)	Dieldrin	7.594	8.291	17346993	28880861	90.359	94.956
14)	Endrin	7.757	8.516	14103835	22171712	95.927	98.180
15)	4,4'-DDD	7.814	8.568	13030588	21870346	82.923	85.360
16)	Endosulfa...	7.912	8.663	14485094	24458936	100.863	106.064
17)	4,4'-DDT	8.011	8.792	11383763	17872825	95.214	88.985
18)	Endrin Al...	8.201	8.899	12180369	19323982	97.137	94.322
19)	Endosulfa...	8.500	9.090	14005263	22938866	90.370	92.092
20)	Methoxychlor	8.349	9.271	6156196	9650999	105.101	98.326
21)	Endrin Ke...	8.692	9.484	16227463	25631282	97.311	99.610
23)	Hexachlor...	3.017f	3.561f	78427	53145	0.429	0.141 #
24)	Hexachlor...	5.593	6.296	88053	103569	0.499	0.330
25)	Oxychlorane	7.061f	7.759	132710	44103	0.807	0.161 #
26)	2,4'-DDE	7.135f	7.935	16118644	26639491	125.671	125.576
27)	trans-Non...	7.328	8.043f	15012262	24959897	83.555	82.748
28)	2,4'-DDD	7.511	8.354f	35928	23501	0.315	0.124 #
29)	2,4'-DDT	7.698	8.568f	46543	21870346	0.424	122.633 #
30)	cis-Nonac...	7.814	8.568	13030588	21870346	62.763	65.197
31)	Mirex	8.448	9.484	67584	25631282	0.539	137.748 #
32)	Chlordane...	7.231	7.935	15938639	26639491	809.495	736.211
33)	Chlordane...	7.328	8.043	15012262	24959897	598.950	822.021
34)	Chlordane...	7.912f	8.705	14485094	94882	2505.586	10.583 #
35)	Chlordane...	3.487	3.428f	37990	64054	NoCal	NoCal
36)	Toxaphene...	7.328	8.291	15012262	28880861	16761.352	11005.343
37)	Toxaphene...	7.594	8.663f	17346993	24458936	10741.581	7432.011
38)	Toxaphene...	7.912	8.663	14485094	24458936	4301.452	4825.850
39)	Toxaphene...	0.000	8.741	0	72017	N.D.	8.625 #
40)	Toxaphene...	8.409f	8.899	43938	19323982	18.329	4146.459 #
41)	Toxaphene...	8.448	9.271	67584	9650999	21.356	2031.703 #
42)	Toxaphene...	3.487	3.484f	37990	1165153	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
Data File : ECD5-11271911.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 14:49  
Operator : MJB  
Sample : 9111243-BS1  
Misc : 1x, 1311/8081B TCLP Pest Reg List  
ALS Vial : 7 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 15:06:00 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271912.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 15:07  
 Operator : MJB  
 Sample : 9111243-BSD1  
 Misc : 1x, 1311/8081B TCLP Pest Reg List  
 ALS Vial : 8 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 15:20:33 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

QA



MJB 11/27/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.213	5.804	12400717	21881149	74.714	74.586
2) S DCBP (S)	9.400	10.316	10707986	14621308	75.890	81.337
Target Compounds						
2) a-BHC	5.747	6.410	19984565	36666237	87.144	89.356
3) g-BHC	6.029	6.726	16945032	30558913	83.979	85.670
4) b-BHC	6.105	6.793	7240742	12469504	80.111	78.788
5) Heptachlor	6.437	7.096	13935760	23317131	76.867	76.205
6) d-BHC	6.251	7.045	16550974	31841137	84.147	90.287
7) Aldrin	6.676	7.358	14050571	23921973	71.162	72.625
8) Heptachlo...	7.135	7.796	15180758	25385817	82.424	84.381
9) trans-Chl...	7.231	7.935	15150157	24721800	81.941	78.901
10) cis-Chlor...	7.328	8.043	14520187	24104868	79.750	82.764
11) Endosulfa...	7.422	8.091	15113450	23933562	88.809	86.975
12) 4,4'-DDE	7.396	8.154	13524004	23099373	71.734	74.352
13) Dieldrin	7.594	8.291	16715592	28045232	87.070	92.209
14) Endrin	7.756	8.516	13258181	20971706	90.175	92.866
15) 4,4'-DDD	7.814	8.568	12398141	20519162	78.898	80.086
16) Endosulfa...	7.912	8.663	14063077	23974221	97.924	103.962
17) 4,4'-DDT	8.011	8.792	9961741	15743480	83.320	79.607
18) Endrin Al...	8.201	8.900	11581037	19451431	92.584	94.891
19) Endosulfa...	8.500	9.090	13629953	22344370	87.948	89.705
20) Methoxychlor	8.349	9.271	5703259	8952840	97.368	92.226
21) Endrin Ke...	8.692	9.484	15717831	24802426	94.255	96.389
23) Hexachlor...	3.018	3.558f	58516	10306	0.320	0.027 #
24) Hexachlor...	5.591	6.295	54316	77084	0.308	0.245
25) Oxychlorthane	7.102f	7.759	77898	84195	0.473	0.307
26) 2,4'-DDE	7.135f	7.935	15180758	24721800	118.358	116.536
27) trans-Non...	7.328	8.043f	14520187	24104868	80.803	79.914
28) 2,4'-DDD	7.511	8.354f	38281	23722	0.335	0.126 #
29) 2,4'-DDT	7.698	8.568f	47138	20519162	0.430	115.057 #
30) cis-Nonac...	7.814	8.568	12398141	20519162	59.717	61.169
31) Mirex	8.449	9.484	78080	24802426	0.623	133.294 #
32) Chlordane...	7.231	7.935	15150157	24721800	769.449	683.214
33) Chlordane...	7.328	8.043	14520187	24104868	579.318	793.862
34) Chlordane...	7.912f	8.704	14063077	89550	2432.586	9.988 #
35) Chlordane...	3.461	3.427f	32823	20152	NoCal	NoCal
36) Toxaphene...	7.328	8.291	14520187	28045232	16211.945	10686.919
37) Toxaphene...	7.594	8.663f	16715592	23974221	10350.606	7284.728
38) Toxaphene...	7.912	8.663	14063077	23974221	4176.131	4730.214
39) Toxaphene...	0.000	8.741	0	94340	N.D.	11.298 #
40) Toxaphene...	8.409f	8.900	45088	19451431	18.809	4173.806 #
41) Toxaphene...	8.449	9.271	78080	8952840	24.673	1884.728 #
42) Toxaphene...	3.485	3.484f	32314	749421	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271912.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 15:07  
 Operator : MJB  
 Sample : 9111243-BSD1  
 Misc : 1x, 1311/8081B TCLP Pest Reg List  
 ALS Vial : 8 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 15:20:33 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271913.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 15:24  
 Operator : MJB  
 Sample : A9K0412-01  
 Misc : 1x, 1311/8081B TCLP Pest Reg List  
 ALS Vial : 9 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 15:43:18 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
11/27/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.212	5.803	11285309	21192030	67.994	72.237
22) S DCBP (S)	9.398	10.314	11497794	16162140	81.488	89.908
Target Compounds						
2) a-BHC	5.773f	6.400	653407	641880	2.849	1.564 #
3) g-BHC	6.031	6.709	7606	31400	0.038	0.088 #
4) b-BHC	6.119	6.784	21841	9989	0.242	0.063 #
5) Heptachlor	6.446	7.079	40794	65180	0.225	0.213
6) d-BHC	6.251	7.043	13929	25519	0.071	0.072
7) Aldrin	6.673	7.385f	5110	45497	0.026	0.138 #
8) Heptachlo...	0.000	7.778f	0	67133	N.D.	0.223 #
9) trans-Chl...	7.216	7.938	24538	46586	0.133	0.149
10) cis-Chlor...	7.343	0.000	11881	0	0.065	N.D. #
11) Endosulfa...	7.425	8.102	14025	33969	0.082	0.123 #
12) 4,4'-DDE	7.425f	8.156	14025	21703	0.074	0.070
13) Dieldrin	7.592	8.278	7512	293268	0.039	0.964 #
14) Endrin	7.767	8.520	185121	19118	1.259	0.085 #
15) 4,4'-DDD	7.827	8.564	23213	37802	0.148	0.148
16) Endosulfa...	7.902	8.647	106480	142648	0.741	0.619
17) 4,4'-DDT	8.009	8.776	11051	21092	0.092	0.085
18) Endrin Al...	8.187	8.882	41766	62550	BelowCal	BelowCal
19) Endosulfa...	8.499	9.088	19605	24426	0.127	0.098
20) Methoxychlor	8.347	9.291	15671	9832	0.268	BelowCal #
21) Endrin Ke...	8.688	9.486	14872	88775	0.089	0.345 #
23) Hexachlor...	3.019	0.000	48127	0	0.263	N.D. #
24) Hexachlor...	5.591f	6.294	26398	68367	0.150	0.218 #
25) Oxychlorane	0.000	7.718f	0	220210	N.D.	0.804 #
26) 2,4'-DDE	0.000	7.938	0	46586	N.D.	0.220 #
27) trans-Non...	7.343	7.992f	11881	105211	87346.634	0.349 #
28) 2,4'-DDD	7.520	8.352f	53752	32601	0.471	0.173 #
29) 2,4'-DDT	7.733	8.564	6334	37802	0.058	0.212 #
30) cis-Nonac...	7.827f	8.587	23213	21862	0.112	0.065 #
31) Mirex	8.454	9.486	28068	88775	0.224	0.477 #
32) Chlordane...	7.269f	7.938	56188	46586	3.311	1.287 #
33) Chlordane...	7.343	0.000	11881	0	0.474	N.D. #
34) Chlordane...	7.902	8.704	106480	74957	18.419	8.360 #
35) Chlordane...	3.490	3.426f	32815	18711	NoCal	NoCal
36) Toxaphene...	7.312	8.278	32065	293268	35.801	111.753 #
37) Toxaphene...	7.592	8.647	7512	142648	4.652	43.345 #
38) Toxaphene...	7.937	8.647f	11441	142648	3.398	28.145 #
39) Toxaphene...	8.187f	8.735	41766	17088	12.890	2.047 #
40) Toxaphene...	8.375	8.882f	10543	62550	4.398	13.422 #
41) Toxaphene...	8.454	9.291	28068	9832	8.869	2.070 #
42) Toxaphene...	3.490	3.482f	32815	910300	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
Data File : ECD5-11271913.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 15:24  
Operator : MJB  
Sample : A9K0412-01  
Misc : 1x, 1311/8081B TCLP Pest Reg List  
ALS Vial : 9 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 15:43:18 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271914.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 15:41  
 Operator : MJB  
 Sample : 9K27028-CCV3  
 Misc : A19K134, AB 100 ppb  
 ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 15:55:11 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
11/27/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.214	5.805	16340144	28867427	98.449	98.400
2) S DCBP (S)	9.399	10.315	12851206	18941563	91.080	105.370
Target Compounds						
2) a-BHC	5.748	6.410	22338652	41377723	97.409	100.838
3) g-BHC	6.029	6.727	18755571	34552695	92.952	96.867
4) b-BHC	6.105	6.793	7263218	12978238	80.360	82.003
5) Heptachlor	6.438	7.096	16690839	29222463	92.064	95.505
6) d-BHC	6.252	7.045	16695133	32257435	84.880	91.467
7) Aldrin	6.676	7.358	19302022	34738743	97.759	105.463
8) Heptachlo...	7.135	7.796	16877223	28365199	91.635	94.284
9) trans-Chl...	7.231	7.935	17640332	30978484	95.409	98.870
10) cis-Chlor...	7.328	8.043	17006667	28319859	93.407	97.237
11) Endosulfa...	7.422	8.090	15996126	26264163	93.995	95.445
12) 4,4'-DDE	7.397	8.154	16788327	29750058	89.049	95.759
13) Dieldrin	7.594	8.290	18177937	30581208	94.687	100.546
14) Endrin	7.757	8.515	14063310	22291067	95.651	98.709
15) 4,4'-DDD	7.815	8.568	13099714	22559553	83.363	88.050
16) Endosulfa...	7.912	8.662	13763393	23315553	95.838	101.106
17) 4,4'-DDT	8.012	8.792	11199300	17833085	93.671	88.812
18) Endrin Al...	8.201	8.899	11943864	19947264	95.344	97.099
19) Endosulfa...	8.500	9.090	13638168	22346916	88.001	89.715
20) Methoxychlor	8.350	9.271	5463579	8851233	93.276	91.329
21) Endrin Ke...	8.692	9.484	15623344	24477782	93.688	95.127
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	6.318f	0	100165	N.D.	0.319 #
25) Oxychlorane	7.072	7.759	85987	125193	0.523	0.457
26) 2,4'-DDE	7.135f	7.935	16877223	30978484	131.585	146.030
27) trans-Non...	7.328	8.043f	17006667	28319859	94.710	93.888
28) 2,4'-DDD	0.000	8.290f	0	30581208	N.D.	161.922 #
29) 2,4'-DDT	7.698	8.568f	63573	22559553	0.580	126.498 #
30) cis-Nonac...	7.815	8.568	13099714	22559553	63.096	67.252
31) Mirex	8.450	9.484	95371	24477782	0.761	131.549 #
32) Chlordane...	7.231	7.935	17640332	30978484	895.921	856.124
33) Chlordane...	7.328	8.043	17006667	28319859	678.522	932.677
34) Chlordane...	7.912f	8.740f	13763393	99443	2380.748	11.091 #
35) Chlordane...	0.000	3.469	0	5618	N.D.	NoCal
36) Toxaphene...	7.328	8.290	17006667	30581208	18988.127	11653.278
37) Toxaphene...	7.594	8.662f	18177937	23315553	11256.117	7084.587
38) Toxaphene...	7.912	8.662	13763393	23315553	4087.138	4600.256
39) Toxaphene...	0.000	8.740	0	99443	N.D.	11.910 #
40) Toxaphene...	8.350f	8.899	5463579	19947264	2279.205	4280.200 #
41) Toxaphene...	8.450	9.271	95371	8851233	30.137	1863.338 #
42) Toxaphene...	0.000	3.469	0	5618	N.D.	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
Data File : ECD5-11271914.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 15:41  
Operator : MJB  
Sample : 9K27028-CCV3  
Misc : A19K134, AB 100 ppb  
ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 15:55:11 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
 Data File : ECD5-11271915.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 Nov 2019 15:58  
 Operator : MJB  
 Sample : 9K27028-CCB2  
 Misc : A19K026  
 ALS Vial : 5 (Sig #1); 0 (Sig #2) Sample Multiplier: 1  
 Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Nov 27 16:12:31 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
 Quant Title : Instrument: DualECD5  
 Last Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
11/27/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.213	5.804	14777370	25453488	89.033	86.763
22) S DCBP (S)	9.400	10.314	11682448	17534308	82.796	97.541
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	0.000	0.000	0	0	N.D.	N.D.
4) b-BHC	6.100	0.000	5851	0	0.065	N.D. #
5) Heptachlor	0.000	0.000	0	0	N.D.	N.D.
6) d-BHC	6.255	7.046	8920	20356	0.045	0.058
7) Aldrin	0.000	7.388f	0	17990	N.D.	0.055 #
8) Heptachlo...	0.000	0.000	0	0	N.D.	N.D.
9) trans-Chl...	7.219	0.000	17803	0	0.096	N.D. #
10) cis-Chlor...	7.318	0.000	3995	0	0.022	N.D. #
11) Endosulfa...	0.000	0.000	0	0	N.D.	N.D.
12) 4,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
13) Dieldrin	0.000	0.000	0	0	N.D.	N.D.
14) Endrin	0.000	8.532	0	9792	N.D.	0.043 #
15) 4,4'-DDD	7.804	8.532f	4094	9792	0.026	0.038 #
16) Endosulfa...	7.909	8.655	11382	15597	0.079	0.068
17) 4,4'-DDT	0.000	8.809	0	10129	N.D.	0.021 #
18) Endrin Al...	8.200	8.897	12640	20819	BelowCal	BelowCal
19) Endosulfa...	8.501	9.089	16097	22893	0.104	0.092
20) Methoxychlor	8.349	0.000	20574	0	0.351	N.D. #
21) Endrin Ke...	8.709	9.485	17926	25689	0.107	0.100
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.591	0.000	17413	0	0.099	N.D. #
25) Oxychlorane	7.064	0.000	7806	0	0.047	N.D. #
26) 2,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
27) trans-Non...	7.318	0.000	3995	0	87346.678	N.D. #
28) 2,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
29) 2,4'-DDT	7.705	8.532	5003	9792	0.046	0.055
30) cis-Nonac...	7.804	0.000	4094	0	0.020	N.D. #
31) Mirex	8.456	9.485	29906	25689	0.239	0.138 #
32) Chlordane...	7.219f	0.000	17803	0	0.904	N.D. #
33) Chlordane...	7.318f	0.000	3995	0	0.159	N.D. #
34) Chlordane...	7.881	8.713	10949	25270	1.894	2.818 #
35) Chlordane...	0.000	0.000	0	0	N.D.	N.D.
36) Toxaphene...	7.318	0.000	3995	0	4.460	N.D. #
37) Toxaphene...	0.000	8.655f	0	15597	N.D.	4.739 #
38) Toxaphene...	7.909	8.655	11382	15597	3.380	3.077
39) Toxaphene...	0.000	8.736	0	20935	N.D.	2.507 #
40) Toxaphene...	8.349f	8.897	20574	20819	8.583	4.467 #
41) Toxaphene...	8.456	0.000	29906	0	9.450	N.D. #
42) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-11\9K27028\  
Data File : ECD5-11271915.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 27 Nov 2019 15:58  
Operator : MJB  
Sample : 9K27028-CCB2  
Misc : A19K026  
ALS Vial : 5 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Nov 27 16:12:31 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823RT9.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



**TCLP Organochloride Pesticides by EPA 8081B  
Calibration Data**

Sequence 9H23034 (Cal ID A9H2608) DualECD5R



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence: **9H23034**  
Date: **08/23/19 11:23**

Instrument: **DUALECD5**  
Calibration: **A9H2608**

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD.ID	STD.ID
1	9H23034-BKD1	Water	QC	QC				A19G138
2	9H23034-BKD2	Water	QC	QC				A19G138
3	9H23034-ICB1	Water	QC	QC				A19H348
4	9H23034-CAL1	Water	QC	QC				A19E245
5	9H23034-CAL2	Water	QC	QC				A19E246
6	9H23034-CAL3	Water	QC	QC				A19E247
7	9H23034-CAL4	Water	QC	QC				A19E249
8	9H23034-CAL5	Water	QC	QC				A19E250
9	9H23034-CAL6	Water	QC	QC				A19H383
10	9H23034-CAL7	Water	QC	QC				A19H384
11	9H23034-CAL8	Water	QC	QC				A19E244
12	9H23034-IBL1	Water	QC	QC				
13	9H23034-ICV1	Water	QC	QC				A19E106
14	9H23034-CAL9	Water	QC	QC				A19E272
15	9H23034-CALA	Water	QC	QC				A19E273
16	9H23034-CALB	Water	QC	QC				A19E274
17	9H23034-CALC	Water	QC	QC				A19E275
18	9H23034-CALD	Water	QC	QC				A19E276
19	9H23034-CALE	Water	QC	QC				A19E154
20	9H23034-CALF	Water	QC	QC				A19E155
21	9H23034-CALG	Water	QC	QC				A19E271
22	9H23034-IBL2	Water	QC	QC				
23	9H23034-ICV2	Water	QC	QC				A19E043
24	9H23034-CALH	Water	QC	QC				A19F232
25	9H23034-CALI	Water	QC	QC				A19F233
26	9H23034-CALJ	Water	QC	QC				A19F234
27	9H23034-CALK	Water	QC	QC				A19F235
28	9H23034-CALL	Water	QC	QC				A19F236
29	9H23034-CALM	Water	QC	QC				A19F231
30	9H23034-IBL3	Water	QC	QC				
31	9H23034-ICV3	Water	QC	QC				A19E108
32	9H23034-CALN	Water	QC	QC				A19D122
33	9H23034-CALO	Water	QC	QC				A19D123
34	9H23034-CALP	Water	QC	QC				A19D124
35	9H23034-CALQ	Water	QC	QC				A19D125
36	9H23034-CALR	Water	QC	QC				A19D126
37	9H23034-CALS	Water	QC	QC				A19D121
38	9H23034-IBL4	Water	QC	QC				
39	9H23034-ICV4	Water	QC	QC				A19D127

Data Entered By: MJB 8/26/19

Comments: ICAL

Data Reviewed By: MV 8/30/19



Calibration Status Report DUALECD5

Method Path : R:\methods\  
 Method File : ECD5\_QUANTPEST\_190823.M  
 Title : Instrument: DualECD5  
 Last Update : Mon Aug 26 11:48:23 2019  
 Response Via : Initial Calibration

*A9H2608*

*MJB  
8/26/19*

#	ID	Conc	ISTD Conc	Path\File
1	1	50	0	R:\data\2019-08\9H23034\ECD5-08231936.D
2	2	100	0	R:\data\2019-08\9H23034\ECD5-08231937.D
3	3	200	0	R:\data\2019-08\9H23034\ECD5-08231938.D
4	4	500	0	R:\data\2019-08\9H23034\ECD5-08231939.D
5	5	1000	0	R:\data\2019-08\9H23034\ECD5-08231940.D
6	6	2000	0	R:\data\2019-08\9H23034\ECD5-08231941.D
7	7	-1	0	R:\data\2019-08\9H23034\ECD5-08231924.D
8	8	-1	0	R:\data\2019-08\9H23034\ECD5-08231925.D

#	ID	Update Time	Quant Time	Acquisition Time
1	1	Aug 26 11:47 2019	Aug 26 11:37 2019	23 Aug 2019 21:54
2	2	Aug 26 11:47 2019	Aug 26 11:38 2019	23 Aug 2019 22:11
3	3	Aug 26 11:48 2019	Aug 26 11:39 2019	23 Aug 2019 22:28
4	4	Aug 26 11:48 2019	Aug 26 11:36 2019	23 Aug 2019 22:45
5	5	Aug 26 11:48 2019	Aug 26 11:40 2019	23 Aug 2019 23:03
6	6	Aug 26 11:48 2019	Aug 26 11:40 2019	23 Aug 2019 23:20
7	7	Aug 26 11:46 2019	Aug 26 11:26 2019	23 Aug 2019 18:27
8	8	Aug 26 11:46 2019	Aug 26 11:27 2019	23 Aug 2019 18:45

ECD5\_QUANTPEST\_190823.M Mon Aug 26 16:04:23 2019

Response Factor Report DUALECD5

Method Path : C:\msdchem\4\methods\  
 Method File : ECD5\_QUANTPEST\_190823.M  
 Title : Instrument: DualECD5  
 Last Update : Mon Aug 26 11:48:23 2019  
 Response Via : Initial Calibration

Calibration Files

1 =ECD5-08231936.D 2 =ECD5-08231937.D 3 =ECD5-08231938.D 4 =ECD5-08231939.D 5 =ECD5-08231940.D  
 6 =ECD5-08231941.D 7 =ECD5-08231924.D 8 =ECD5-08231925.D

Compound	1	2	3	4	5	6	7	8	Avg	%RSD
1) S TCMX (S)	1.767	1.750	1.668	1.644	1.606	1.614	1.585	1.642	1.660	E5 4.00
2) a-BHC	2.320	2.292	2.296	2.347	2.221	2.274	2.236	2.360	2.293	E5 2.14
3) g-BHC	2.074	2.030	2.041	2.035	1.950	1.957	1.960	2.094	2.018	E5 2.76
4) b-BHC	1.043	0.971	0.914	0.911	0.824	0.820	0.836	0.912	0.904	E5 8.59
5) Heptachlor	1.921	1.848	1.798	1.820	1.726	1.747	1.755	1.889	1.813	E5 3.86
6) d-BHC	1.998	1.935	2.008	2.006	1.867	1.922	1.948	2.051	1.967	E5 3.02
7) Aldrin	2.055	1.998	2.025	2.011	1.938	1.866	1.911	1.992	1.974	E5 3.23
8) Heptachlor Exp...	2.005	1.960	1.847	1.865	1.738	1.774	1.732	1.813	1.842	E5 5.42
9) trans-Chlordane	1.972	1.911	1.853	1.848	1.761	1.792	1.773	1.881	1.849	E5 3.93
10) cis-Chlordane	2.098	1.950	1.818	1.843	1.698	1.725	1.674	1.760	1.821	E5 7.86
11) Endosulfan I	1.852	1.787	1.723	1.709	1.645	1.597	1.609	1.693	1.702	E5 5.13
12) 4,4'-DDE	1.934	1.943	1.907	1.891	1.828	1.835	1.805	1.938	1.885	E5 2.92
13) Dieldrin	1.977	1.979	1.944	1.955	1.833	1.877	1.832	1.961	1.920	E5 3.25
14) Endrin	1.564	1.493	1.478	1.476	1.404	1.396	1.381	1.571	1.470	E5 4.98
15) 4,4'-DDD	1.650	1.573	1.581	1.566	1.491	1.545	1.544	1.622	1.571	E5 3.11
16) Endosulfan II	1.581	1.496	1.419	1.448	1.349	1.368	1.354	1.474	1.436	E5 5.61
17) 4,4'-DDT	1.139	1.091	1.106	1.147	1.170	1.241	1.218	1.454	1.196	E5 9.72
18) Endrin Aldehyde	2.413	1.641	1.367	1.375	1.248	1.245	1.236	1.331	1.482	E5 26.87
19) Endosulfan Sul...	1.761	1.611	1.538	1.554	1.458	1.484	1.437	1.556	1.550	E5 6.64
20) Methoxychlor	5.966	5.573	5.408	5.617	5.561	5.721	5.877	7.136	5.857	E4 9.33
21) Endrin Ketone	1.776	1.656	1.623	1.664	1.604	1.638	1.625	1.755	1.668	E5 3.80
22) S DCBP (S)	1.639	1.550	1.402	1.335	1.337	1.336	1.341	1.349	1.411	E5 8.33
23) Hexachlorobuta...	1.982	1.879	1.918	1.838	1.746	1.752	1.795	1.708	1.827	E5 5.17
24) Hexachlorobenzene	1.947	1.810	1.708	1.712	1.674	1.782	1.767	1.704	1.763	E5 4.96
25) Oxychlordane	1.768	1.697	1.639	1.592	1.553	1.677	1.636	1.602	1.645	E5 4.13
26) 2,4'-DDE	1.379	1.326	1.266	1.245	1.224	1.302	1.277	1.241	1.283	E5 4.01
27) trans-Nonachlor	2.368	2.076	1.866	1.818	1.756	1.916	1.835	1.751	1.923	E5 10.78
28) 2,4'-DDD	1.202	1.165	1.122	1.104	1.098	1.184	1.159	1.096	1.141	E5 3.65
29) 2,4'-DDT	1.071	1.021	1.074	1.052	1.092	1.137	1.177	1.151	1.097	E5 4.88
30) cis-Nonachlor	2.192	2.117	2.052	2.032	1.997	2.123	2.093	2.002	2.076	E5 3.25
31) Mirex	1.474	1.334	1.257	1.196	1.164	1.244	1.196	1.164	1.254	E5 8.39
32) Chlordane (1)	2.018	1.979	1.925	1.926	1.964	2.002			1.969	E4 1.96
33) Chlordane (2)	2.573	2.520	2.453	2.435	2.508	2.549			2.506	E4 2.14
34) Chlordane (3)	5.762	5.482	5.508	5.843	5.988	6.104			5.781	E3 4.34
35) Chlordane - AVE									0.000	-1.00
36) Toxaphene (1)	9.850	9.158	8.802	8.837	8.719	8.373			8.956	E2 5.64
37) Toxaphene (2)	1.766	1.661	1.588	1.639	1.556	1.479			1.615	E3 6.08
38) Toxaphene (3)	3.388	3.328	3.222	3.355	3.496	3.416			3.367	E3 2.72
39) Toxaphene (4)	3.286	3.203	3.162	3.299	3.287	3.204			3.240	E3 1.78
40) Toxaphene (5)	2.294	2.290	2.272	2.443	2.546	2.537			2.397	E3 5.33
41) Toxaphene (6)	3.063	3.026	2.990	3.247	3.407	3.255			3.165	E3 5.17
42) Toxaphene - AVE									0.000	-1.00

*MJB*  
*8/26/19*

Response Factor Report DUALECD5

Method Path : C:\msdchem\4\methods\  
 Method File : ECD5\_QUANTPEST\_190823.M  
 Title : Instrument: DualECD5

Signal #2 Calibration Files

1 =ECD5-08231936.D 2 =ECD5-08231937.D 3 =ECD5-08231938.D  
 4 =ECD5-08231939.D 5 =ECD5-08231940.D 6 =ECD5-08231941.D

Compound	1	2	3	4	5	6	Avg	%RSD
44) S TCMX (S) #2	3.001	3.004	2.876	2.866	2.829	2.839	2.926	3.129 2.934 E5 3.54
45) a-BHC #2	3.931	3.923	3.971	4.096	3.964	4.053	4.170	4.719 4.103 E5 6.41
46) g-BHC #2	3.523	3.455	3.485	3.477	3.403	3.476	3.679	4.038 3.567 E5 5.79
47) b-BHC #2	1.763	1.676	1.577	1.581	1.471	1.503	1.463	1.628 1.583 E5 6.60
48) Heptachlor #2	3.098	2.934	3.016	3.006	2.913	2.919	3.028	3.564 3.060 E5 6.98
49) d-BHC #2	3.491	3.346	3.435	3.614	3.299	3.462	3.518	4.049 3.527 E5 6.60
50) Aldrin #2	3.175	3.177	3.202	3.341	3.151	3.253	3.391	3.661 3.294 E5 5.19
51) Heptachlor Exp...	3.101	3.031	2.912	2.959	2.826	2.968	3.005	3.267 3.008 E5 4.40
52) trans-Chlordan...	3.641	3.222	3.004	3.003	2.863	2.936	3.074	3.322 3.133 E5 8.10
53) cis-Chlordane #2	2.994	2.898	2.870	2.860	2.774	2.800	2.904	3.199 2.912 E5 4.59
54) Endosulfan I #2	2.789	2.702	2.654	2.724	2.629	2.742	2.721	3.052 2.752 E5 4.77
55) 4,4'-DDE #2	2.985	2.990	2.976	3.050	3.000	3.111	3.250	3.492 3.107 E5 5.82
56) Dieldrin #2	2.967	2.919	2.925	2.899	2.934	3.087	3.100	3.502 3.042 E5 6.61
57) Endrin #2	2.229	2.124	2.186	2.244	2.130	2.203	2.310	2.639 2.258 E5 7.32
58) 4,4'-DDD #2	2.515	2.441	2.417	2.425	2.459	2.632	2.630	2.978 2.562 E5 7.37
59) Endosulfan II #2	2.322	2.311	2.193	2.244	2.179	2.307	2.302	2.592 2.306 E5 5.55
60) 4,4'-DDT #2	1.797	1.709	1.747	1.841	1.792	1.857	1.979	2.410 1.892 E5 11.88
61) Endrin Aldehyd...	3.486	2.388	2.092	2.125	1.939	2.042	2.050	2.254 2.297 E5 21.77
62) Endosulfan Sul...	2.658	2.494	2.352	2.425	2.392	2.430	2.448	2.730 2.491 E5 5.35
63) Methoxychlor #2	0.952	0.890	0.828	0.883	0.867	0.869	0.944	1.186 0.927 E5 12.09
64) Endrin Ketone #2	2.558	2.466	2.410	2.497	2.357	2.591	2.664	3.043 2.573 E5 8.31
65) S DCBP (S) #2	1.916	1.950	1.742	1.679	1.665	1.746	1.778	1.905 1.798 E5 6.18
66) Hexachlorobuta...	3.832	3.773	3.755	3.702	3.557	3.727	3.930	3.799 3.759 E5 2.87
67) Hexachlorobenz...	3.280	3.164	2.971	2.936	2.967	3.219	3.277	3.313 3.141 E5 5.04
68) Oxychlordane #2	2.791	2.705	2.651	2.539	2.481	2.835	2.973	2.937 2.739 E5 6.49
69) 2,4'-DDE #2	2.192	2.059	2.059	2.018	2.000	2.201	2.216	2.225 2.121 E5 4.52
70) trans-Nonachlo...	3.062	2.939	2.935	2.844	2.837	3.162	3.198	3.154 3.016 E5 4.84
71) 2,4'-DDD #2	1.920	1.868	1.797	1.779	1.756	1.985	2.012	1.992 1.889 E5 5.47
72) 2,4'-DDT #2	1.733	1.661	1.746	1.703	1.762	1.762	1.900	2.000 1.783 E5 6.24
73) cis-Nonachlor #2	3.327	3.124	3.174	3.148	3.288	3.544	3.607	3.623 3.354 E5 6.23
74) Mirex #2	2.098	1.941	1.791	1.723	1.655	1.820	1.936	1.921 1.861 E5 7.59
75) Chlordane (1) #2	3.509	3.378	3.376	3.566	3.797	4.085		3.618 E4 7.62
76) Chlordane (2) #2	2.945	2.906	2.942	2.962	3.149	3.314		3.036 E4 5.30
77) Chlordane (3) #2	8.780	8.745	8.659	8.543	9.359	9.709		8.966 E3 5.14
78) Chlordane - AV...								0.000 -1.00
79) Toxaphene (1) #2	2.737	2.675	2.545	2.618	2.655	2.515		2.624 E3 3.16
80) Toxaphene (2) #2	3.294	3.241	3.227	3.295	3.384	3.305		3.291 E3 1.70
81) Toxaphene (3) #2	5.097	4.944	4.978	4.950	5.168	5.273		5.068 E3 2.65
82) Toxaphene (4) #2	8.327	8.119	7.902	8.505	8.650	8.595		8.350 E3 3.51
83) Toxaphene (5) #2	4.664	4.522	4.477	4.681	4.900	4.718		4.660 E3 3.24
84) Toxaphene (6) #2	4.618	4.525	4.526	4.740	5.047	5.045		4.750 E3 5.10
85) Toxaphene - AV...								0.000 -1.00

*MJB*  
*6/26/19*

(#) = Out of Range

Compound List Report DUALECD5

Method Path : R:\methods\  
 Method File : ECD5\_QUANTPEST\_190823.M  
 Title : Instrument: DualECD5  
 Last Update : Mon Aug 26 11:48:23 2019  
 Response Via : Initial Calibration

Total Cpnds : 85

PK#	Compound Name	Exp_RT	Rel_RT	Cal	A/H	ID
1	S TCMX (S)	5.394	1.000	A	H	R
2	a-BHC	5.934	1.000	A	H	R
3	g-BHC	6.218	1.000	A	H	R
4	b-BHC	6.296	1.000	A	H	R
5	Heptachlor	6.632	1.000	A	H	R
6	d-BHC	6.446	1.000	A	H	R
7	Aldrin	6.873	1.000	A	H	R
8	Heptachlor Expoxide	7.332	1.000	A	H	R
9	trans-Chlordane	7.428	1.000	A	H	R
10	cis-Chlordane	7.524	1.000	A	H	R
11	Endosulfan I	7.621	1.000	A	H	R
12	4,4'-DDE	7.583	1.000	A	H	R
13	Dieldrin	7.792	1.000	A	H	R
14	Endrin	7.957	1.000	A	H	R
15	4,4'-DDD	8.003	1.000	A	H	R
16	Endosulfan II	8.114	1.000	A	H	R
17	4,4'-DDT	8.202	1.000	A	H	R
18	Endrin Aldehyde	8.403	1.000	<del>Q</del>	H	R
19	Endosulfan Sulfate	8.705	1.000	A	H	R
20	Methoxychlor	8.540	1.000	A	H	R
21	Endrin Ketone	8.899	1.000	A	H	R
22	S DCBP (S)	9.592	1.000	A	H	R
23	Hexachlorobutadiene	3.198	1.000	A	H	R
24	Hexachlorobenzene	5.774	1.000	A	H	R
25	Oxychlordane	7.261	1.000	A	H	R
26	2,4'-DDE	7.333	1.000	A	H	R
27	trans-Nonachlor	7.515	1.000	<del>Q</del>	H	R
28	2,4'-DDD	7.705	1.000	A	H	R
29	2,4'-DDT	7.887	1.000	A	H	R
30	cis-Nonachlor	7.985	1.000	A	H	R
31	Mirex	8.652	1.000	A	H	R
32	Chlordane (1)	7.427	1.000	A	H	R
33	Chlordane (2)	7.520	1.000	A	H	R
34	Chlordane (3)	8.067	1.000	A	H	R
35	Chlordane - AVE	3.447	1.000	A	H	R
36	Toxaphene (1)	7.502	1.000	A	H	R
37	Toxaphene (2)	7.794	1.000	A	H	R
38	Toxaphene (3)	8.105	1.000	A	H	R
39	Toxaphene (4)	8.346	1.000	A	H	R
40	Toxaphene (5)	8.574	1.000	A	H	R
41	Toxaphene (6)	8.640	1.000	A	H	R
42	Toxaphene - AVE	3.450	1.000	A	H	R
43	Signal #2	3.544	1.000	A	H	R
44	S TCMX (S) #2	5.988	1.000	A	H	R
45	a-BHC #2	6.595	1.000	A	H	R
46	g-BHC #2	6.914	1.000	A	H	R
47	b-BHC #2	6.978	1.000	A	H	R
48	Heptachlor #2	7.290	1.000	A	H	R
49	d-BHC #2	7.231	1.000	A	H	R
50	Aldrin #2	7.555	1.000	A	H	R
51	Heptachlor Expoxide #2	7.992	1.000	A	H	R
52	trans-Chlordane #2	8.131	1.000	A	H	R
53	cis-Chlordane #2	8.238	1.000	A	H	R
54	Endosulfan I #2	8.289	1.000	A	H	R
55	4,4'-DDE #2	8.343	1.000	A	H	R
56	Dieldrin #2	8.489	1.000	A	H	R

*MJB*  
*8/26/19*

57	Endrin #2	8.715	1.000	A	H	R
58	4,4'-DDD #2	8.758	1.000	A	H	R
59	Endosulfan II #2	8.863	1.000	A	H	R
60	4,4'-DDT #2	8.984	1.000	Q	H	R
61	Endrin Aldehyde #2	9.099	1.000	Q	H	R
62	Endosulfan Sulfate #2	9.289	1.000	A	H	R
63	Methoxychlor #2	9.463	1.000	Q	H	R
64	Endrin Ketone #2	9.687	1.000	A	H	R
65	S DCBP (S) #2	10.541	1.000	A	H	R
66	Hexachlorobutadiene #2	3.688	1.000	A	H	R
67	Hexachlorobenzene #2	6.454	1.000	A	H	R
68	Oxychlorane #2	7.920	1.000	A	H	R
69	2,4'-DDE #2	8.122	1.000	A	H	R
70	trans-Nonachlor #2	8.194	1.000	A	H	R
71	2,4'-DDD #2	8.495	1.000	A	H	R
72	2,4'-DDT #2	8.718	1.000	A	H	R
73	cis-Nonachlor #2	8.758	1.000	A	H	R
74	Mirex #2	9.679	1.000	A	H	R
75	Chlordane (1) #2	8.129	1.000	A	H	R
76	Chlordane (2) #2	8.236	1.000	A	H	R
77	Chlordane (3) #2	8.896	1.000	A	H	R
78	Chlordane - AVE #2	3.428	1.000	A	H	R
79	Toxaphene (1) #2	8.466	1.000	A	H	R
80	Toxaphene (2) #2	8.812	1.000	A	H	R
81	Toxaphene (3) #2	8.848	1.000	A	H	R
82	Toxaphene (4) #2	8.915	1.000	A	H	R
83	Toxaphene (5) #2	9.091	1.000	A	H	R
84	Toxaphene (6) #2	9.470	1.000	A	H	R
85	Toxaphene - AVE #2	3.434	1.000	A	H	R

Cal A = Average L = Linear LO = Linear w/origin Q = Quad QO = Quad w/origin

A/H = Area or Height

ID R = R.T. B = R.T. & Q Q = Qvalue L = Largest A = All

-----

ECD5\_QUANTPEST\_190823.M Mon Aug 26 16:04:34 2019

Calibration Report DUALECD5

Method Path : R:\methods\  
 Method File : ECD5\_QUANTPEST\_190823.M  
 Title : Instrument: DualECD5  
 Last Update : Mon Aug 26 11:48:23 2019  
 Response Via : Initial Calibration

Calibration Files

1 =ECD5-08231936 2 =ECD5-08231937 3 =ECD5-08231938 4 =ECD5-08231939 5 =ECD5-08231940  
 6 =ECD5-08231941 7 =ECD5-08231924 8 =ECD5-08231925

	Compound	Fit	Constant	Linear	Quad	RSD/Cf
1) S	TCMX (S)	Avg	-----	1.6598 e5	-----	0.0400
2)	a-BHC	Avg	-----	2.2933 e5	-----	0.0214
3)	g-BHC	Avg	-----	2.0178 e5	-----	0.0276
4)	b-BHC	Avg	-----	9.0384 e4	-----	0.0859
5)	Heptachlor	Avg	-----	1.8130 e5	-----	0.0386
6)	d-BHC	Avg	-----	1.9669 e5	-----	0.0302
7)	Aldrin	Avg	-----	1.9745 e5	-----	0.0323
8)	Heptachlor Expoxide	Avg	-----	1.8418 e5	-----	0.0542
9)	trans-Chlordane	Avg	-----	1.8489 e5	-----	0.0393
10)	cis-Chlordane	Avg	-----	1.8207 e5	-----	0.0786
11)	Endosulfan I	Avg	-----	1.7018 e5	-----	0.0513
12)	4,4'-DDE	Avg	-----	1.8853 e5	-----	0.0292
13)	Dieldrin	Avg	-----	1.9198 e5	-----	0.0325
14)	Endrin	Avg	-----	1.4703 e5	-----	0.0498
15)	4,4'-DDD	Avg	-----	1.5714 e5	-----	0.0311
16)	Endosulfan II	Avg	-----	1.4361 e5	-----	0.0561
17)	4,4'-DDT	Avg	-----	1.1956 e5	-----	0.0972
18)	Endrin Aldehyde	Quad	1.1904 e5	1.1635 e5	8.0472 e1	0.9966
19)	Endosulfan Sulfate	Avg	-----	1.5498 e5	-----	0.0664
20)	Methoxychlor	Avg	-----	5.8574 e4	-----	0.0933
21)	Endrin Ketone	Avg	-----	1.6676 e5	-----	0.0380
22) S	DCBP (S)	Avg	-----	1.4110 e5	-----	0.0833
23)	Hexachlorobutadiene	Avg	-----	1.8274 e5	-----	0.0517
24)	Hexachlorobenzene	Avg	-----	1.7629 e5	-----	0.0496
25)	Oxychlordane	Avg	-----	1.6454 e5	-----	0.0413
26)	2,4'-DDE	Avg	-----	1.2826 e5	-----	0.0401
27)	trans-Nonachlor	Quad	5.6661 e4	1.7916 e5	-2.0512	0.9987
28)	2,4'-DDD	Avg	-----	1.1413 e5	-----	0.0365
29)	2,4'-DDT	Avg	-----	1.0969 e5	-----	0.0488
30)	cis-Nonachlor	Avg	-----	2.0762 e5	-----	0.0325
31)	Mirex	Avg	-----	1.2537 e5	-----	0.0839
32)	Chlordane (1)	Avg	-----	1.9690 e4	-----	0.0196
33)	Chlordane (2)	Avg	-----	2.5064 e4	-----	0.0214
34)	Chlordane (3)	Avg	-----	5.7811 e3	-----	0.0434
35)	Chlordane - AVE	Avg	-----	-----	-----	0.0000
36)	Toxaphene (1)	Avg	-----	8.9565 e2	-----	0.0564
37)	Toxaphene (2)	Avg	-----	1.6149 e3	-----	0.0608
38)	Toxaphene (3)	Avg	-----	3.3675 e3	-----	0.0272
39)	Toxaphene (4)	Avg	-----	3.2402 e3	-----	0.0178
40)	Toxaphene (5)	Avg	-----	2.3971 e3	-----	0.0533
41)	Toxaphene (6)	Avg	-----	3.1646 e3	-----	0.0517
42)	Toxaphene - AVE	Avg	-----	-----	-----	0.0000

MJP  
5/26/19

Signal #2

	Compound	Fit	Constant	Linear	Quad	RSD/Cf
1) S	TCMX (S)	Avg	-----	2.9337 e5	-----	0.0354
2)	a-BHC	Avg	-----	4.1034 e5	-----	0.0641
3)	g-BHC	Avg	-----	3.5670 e5	-----	0.0579
4)	b-BHC	Avg	-----	1.5827 e5	-----	0.0660
5)	Heptachlor	Avg	-----	3.0598 e5	-----	0.0698
6)	d-BHC	Avg	-----	3.5267 e5	-----	0.0660
7)	Aldrin	Avg	-----	3.2939 e5	-----	0.0519

8)	Heptachlor Epoxide	Avg	-----	3.0085 e5	-----	0.0440
9)	trans-Chlordane	Avg	-----	3.1333 e5	-----	0.0810
10)	cis-Chlordane	Avg	-----	2.9125 e5	-----	0.0459
11)	Endosulfan I	Avg	-----	2.7518 e5	-----	0.0477
12)	4,4'-DDE	Avg	-----	3.1068 e5	-----	0.0582
13)	Dieldrin	Avg	-----	3.0415 e5	-----	0.0661
14)	Endrin	Avg	-----	2.2583 e5	-----	0.0732
15)	4,4'-DDD	Avg	-----	2.5621 e5	-----	0.0737
16)	Endosulfan II	Avg	-----	2.3061 e5	-----	0.0555
17)	4,4'-DDT	Quad	6.5669 e3	1.7140 e5	3.3014 e2	0.9992
18)	Endrin Aldehyde	Quad	1.5509 e5	1.8265 e5	2.1823 e2	0.9961
19)	Endosulfan Sulfate	Avg	-----	2.4909 e5	-----	0.0535
20)	Methoxychlor	Quad	1.4992 e4	8.0453 e4	1.7846 e2	0.9988
21)	Endrin Ketone	Avg	-----	2.5732 e5	-----	0.0831
22) S	DCBP (S)	Avg	-----	1.7976 e5	-----	0.0618
23)	Hexachlorobutadiene	Avg	-----	3.7593 e5	-----	0.0287
24)	Hexachlorobenzene	Avg	-----	3.1409 e5	-----	0.0504
25)	Oxychlordane	Avg	-----	2.7390 e5	-----	0.0649
26)	2,4'-DDE	Avg	-----	2.1214 e5	-----	0.0452
27)	trans-Nonachlor	Avg	-----	3.0164 e5	-----	0.0484
28)	2,4'-DDD	Avg	-----	1.8886 e5	-----	0.0547
29)	2,4'-DDT	Avg	-----	1.7834 e5	-----	0.0624
30)	cis-Nonachlor	Avg	-----	3.3545 e5	-----	0.0623
31)	Mirex	Avg	-----	1.8607 e5	-----	0.0759
32)	Chlordane (1)	Avg	-----	3.6185 e4	-----	0.0762
33)	Chlordane (2)	Avg	-----	3.0364 e4	-----	0.0530
34)	Chlordane (3)	Avg	-----	8.9659 e3	-----	0.0514
35)	Chlordane - AVE	Avg	-----	-----	-----	0.0000
36)	Toxaphene (1)	Avg	-----	2.6243 e3	-----	0.0316
37)	Toxaphene (2)	Avg	-----	3.2910 e3	-----	0.0170
38)	Toxaphene (3)	Avg	-----	5.0683 e3	-----	0.0265
39)	Toxaphene (4)	Avg	-----	8.3498 e3	-----	0.0351
40)	Toxaphene (5)	Avg	-----	4.6604 e3	-----	0.0324
41)	Toxaphene (6)	Avg	-----	4.7502 e3	-----	0.0510
42)	Toxaphene - AVE	Avg	-----	-----	-----	0.0000

-----

ECD5\_QUANTPEST\_190823.M Mon Aug 26 16:04:42 2019

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Chlordane (Technical)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9H23034-CALH	50	5365	107.300	3.45
9H23034-CALI	100	4938	49.380	3.45
9H23034-CALJ	200	4503	22.515	3.45
9H23034-CALK	500	4056	8.112	3.45
9H23034-CALL	1000	4825	4.825	3.45
9H23034-CALM	2000	4939	2.469	3.45

**AVE RF 0.000 RF RSD 0.00 AVE RT 0.00**

## Chlordane (Technical) [2C]

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9H23034-CALH	50	0	0.000	0.00
9H23034-CALI	100	0	0.000	0.00
9H23034-CALJ	200	0	0.000	0.00
9H23034-CALK	500	0	0.000	0.00
9H23034-CALL	1000	0	0.000	0.00
9H23034-CALM	2000	0	0.000	0.00

**AVE RF 0.000 RF RSD 0.00 AVE RT 0.00**

## Toxaphene (Total)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9H23034-CALN	50	4023	80.460	3.45
9H23034-CALO	100	3536	35.360	3.45
9H23034-CALP	200	3919	19.595	3.45
9H23034-CALQ	500	4132	8.264	3.45
9H23034-CALR	1000	2687	2.687	3.45
9H23034-CALS	2000	4166	2.083	3.45

**AVE RF 0.000 RF RSD 0.00 AVE RT 0.00**

## Toxaphene (Total) [2C]

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9H23034-CALN	50	0	0.000	0.00
9H23034-CALO	100	0	0.000	0.00
9H23034-CALP	200	0	0.000	0.00
9H23034-CALQ	500	0	0.000	0.00
9H23034-CALR	1000	0	0.000	0.00
9H23034-CALS	2000	0	0.000	0.00

**AVE RF 0.000 RF RSD 0.00 AVE RT 0.00**

## Hexachlorobutadiene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9H23034-CAL9	1	198207	198207.000	3.20
9H23034-CALA	2	375794	187897.000	3.20
9H23034-CALB	5	959211	191842.200	3.20
9H23034-CALC	10	1838187	183818.700	3.20
9H23034-CALD	25	4363988	174559.500	3.20
9H23034-CALE	50	8761747	175234.900	3.20
9H23034-CALF	100	795213E+07	179521.300	3.20
9H23034-CALG	200	416653E+07	170832.600	3.20

**AVE RF 3.200 RF RSD 5.17 AVE RT 3.20**



# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Hexachlorobutadiene [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	383198	383198.000	3.69	
9H23034-CALA	2	754548	377274.000	3.69	
9H23034-CALB	5	1877484	375496.800	3.69	
9H23034-CALC	10	3701532	370153.200	3.69	
9H23034-CALD	25	8892238	355689.500	3.69	
9H23034-CALE	50	863562E+07	372712.400	3.69	
9H23034-CALF	100	929888E+07	392988.800	3.69	
9H23034-CALG	200	598857E+07	379942.800	3.69	
<b>AVE RF</b>	<b>375931.900</b>	<b>RF RSD</b>	<b>2.87</b>	<b>AVE RT</b>	<b>3.69</b>

## 2,4,5,6-TCMX (Surr)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	176748	176748.000	5.40	
9H23034-CAL2	2	349972	174986.000	5.40	
9H23034-CAL3	5	834206	166841.200	5.40	
9H23034-CAL4	10	1644447	164444.700	5.40	
9H23034-CAL5	25	4015832	160633.300	5.39	
9H23034-CAL6	50	8071481	161429.600	5.39	
9H23034-CAL7	100	585092E+07	158509.200	5.40	
9H23034-CAL8	200	284254E+07	164212.700	5.39	
<b>AVE RF</b>	<b>165975.600</b>	<b>RF RSD</b>	<b>4.00</b>	<b>AVE RT</b>	<b>5.40</b>

## Hexachlorobenzene


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	194679	194679.000	5.78	
9H23034-CALA	2	362082	181041.000	5.78	
9H23034-CALB	5	853793	170758.600	5.78	
9H23034-CALC	10	1711884	171188.400	5.77	
9H23034-CALD	25	4184551	167382.000	5.77	
9H23034-CALE	50	8911624	178232.500	5.77	
9H23034-CALF	100	767002E+07	176700.200	5.78	
9H23034-CALG	200	407346E+07	170367.300	5.77	
<b>AVE RF</b>	<b>176293.600</b>	<b>RF RSD</b>	<b>4.96</b>	<b>AVE RT</b>	<b>5.77</b>

## alpha-BHC


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	231994	231994.000	5.94	
9H23034-CAL2	2	458365	229182.500	5.94	
9H23034-CAL3	5	1147932	229586.400	5.94	
9H23034-CAL4	10	2347065	234706.500	5.94	
9H23034-CAL5	25	5553096	222123.800	5.94	
9H23034-CAL6	50	136959E+07	227391.800	5.94	
9H23034-CAL7	100	236358E+07	223635.800	5.94	
9H23034-CAL8	200	720225E+07	236011.200	5.94	
<b>AVE RF</b>	<b>229329.000</b>	<b>RF RSD</b>	<b>2.14</b>	<b>AVE RT</b>	<b>5.94</b>

## 2,4,5,6-TCMX (Surr) [2C]

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	300053	300053.000	5.99	
9H23034-CAL2	2	600766	300383.000	5.99	
9H23034-CAL3	5	1437876	287575.200	5.99	
9H23034-CAL4	10	2865854	286585.400	5.99	
9H23034-CAL5	25	7072923	282916.900	5.99	
9H23034-CAL6	50	419675E+07	283935.000	5.99	
9H23034-CAL7	100	925633E+07	292563.300	5.99	
9H23034-CAL8	200	258445E+07	312922.300	5.99	
<b>AVE RF</b>	<b>293366.900</b>	<b>RF RSD</b>	<b>3.54</b>	<b>AVE RT</b>	<b>5.99</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## gamma-BHC (Lindane)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	207427	207427.000	6.22	
9H23034-CAL2	2	406027	203013.500	6.22	
9H23034-CAL3	5	1020724	204144.800	6.22	
9H23034-CAL4	10	2034859	203485.900	6.22	
9H23034-CAL5	25	4875657	195026.300	6.22	
9H23034-CAL6	50	9785999	195720.000	6.22	
9H23034-CAL7	100	959509E+07	195950.900	6.22	
9H23034-CAL8	200	188973E+07	209448.600	6.22	
<b>AVE RF</b>	<b>201777.100</b>	<b>RF RSD</b>	<b>2.76</b>	<b>AVE RT</b>	<b>6.22</b>

## beta-BHC


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	104326	104326.000	6.30	
9H23034-CAL2	2	194168	97084.000	6.30	
9H23034-CAL3	5	456954	91390.800	6.30	
9H23034-CAL4	10	910875	91087.500	6.30	
9H23034-CAL5	25	2060378	82415.120	6.30	
9H23034-CAL6	50	4100858	82017.160	6.30	
9H23034-CAL7	100	8355416	83554.160	6.30	
9H23034-CAL8	200	.82387E+07	91193.500	6.29	
<b>AVE RF</b>	<b>90383.530</b>	<b>RF RSD</b>	<b>8.59</b>	<b>AVE RT</b>	<b>6.30</b>

## delta-BHC


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	199840	199840.000	6.45	
9H23034-CAL2	2	386980	193490.000	6.45	
9H23034-CAL3	5	1004012	200802.400	6.45	
9H23034-CAL4	10	2006493	200649.300	6.45	
9H23034-CAL5	25	4667166	186686.600	6.45	
9H23034-CAL6	50	9610742	192214.800	6.45	
9H23034-CAL7	100	947558E+07	194755.800	6.45	
9H23034-CAL8	200	101659E+07	205083.000	6.45	
<b>AVE RF</b>	<b>196690.200</b>	<b>RF RSD</b>	<b>3.02</b>	<b>AVE RT</b>	<b>6.45</b>

## Hexachlorobenzene [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	328025	328025.000	6.45	
9H23034-CALA	2	632830	316415.000	6.45	
9H23034-CALB	5	1485583	297116.600	6.45	
9H23034-CALC	10	2936294	293629.400	6.45	
9H23034-CALD	25	7416324	296653.000	6.45	
9H23034-CALE	50	509416E+07	321883.200	6.45	
9H23034-CALF	100	276671E+07	327667.100	6.46	
9H23034-CALG	200	526197E+07	331309.800	6.45	
<b>AVE RF</b>	<b>314087.400</b>	<b>RF RSD</b>	<b>5.04</b>	<b>AVE RT</b>	<b>6.45</b>

## alpha-BHC [2C]

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	393119	393119.000	6.60	
9H23034-CAL2	2	784586	392293.000	6.60	
9H23034-CAL3	5	1985438	397087.600	6.60	
9H23034-CAL4	10	4095890	409589.000	6.60	
9H23034-CAL5	25	9910863	396434.500	6.60	
9H23034-CAL6	50	026582E+07	405316.400	6.60	
9H23034-CAL7	100	169921E+07	416992.100	6.60	
9H23034-CAL8	200	437675E+07	471883.800	6.60	
<b>AVE RF</b>	<b>419339.000</b>	<b>RF RSD</b>	<b>6.41</b>	<b>AVE RT</b>	<b>6.60</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Heptachlor


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	192066	192066.000	6.64	
9H23034-CAL2	2	369615	184807.500	6.64	
9H23034-CAL3	5	899091	179818.200	6.64	
9H23034-CAL4	10	1819621	181962.100	6.63	
9H23034-CAL5	25	4314306	172572.200	6.63	
9H23034-CAL6	50	8735158	174703.200	6.63	
9H23034-CAL7	100	755153E+07	175515.300	6.63	
9H23034-CAL8	200	1.77857E+07	188928.500	6.63	
<b>AVE RF</b>	<b>181296.600</b>	<b>RF RSD</b>	<b>3.86</b>	<b>AVE RT</b>	<b>6.63</b>

## Aldrin


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	205523	205523.000	6.88	
9H23034-CAL2	2	399550	199775.000	6.88	
9H23034-CAL3	5	1012733	202546.600	6.88	
9H23034-CAL4	10	2010802	201080.200	6.88	
9H23034-CAL5	25	4845355	193814.200	6.87	
9H23034-CAL6	50	9327672	186553.400	6.87	
9H23034-CAL7	100	910807E+07	191080.700	6.87	
9H23034-CAL8	200	1.98384E+07	199192.000	6.87	
<b>AVE RF</b>	<b>197445.600</b>	<b>RF RSD</b>	<b>3.23</b>	<b>AVE RT</b>	<b>6.87</b>

## gamma-BHC (Lindane) [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	352286	352286.000	6.92	
9H23034-CAL2	2	690922	345461.000	6.92	
9H23034-CAL3	5	1742677	348535.400	6.92	
9H23034-CAL4	10	3476733	347673.300	6.92	
9H23034-CAL5	25	8508386	340335.400	6.91	
9H23034-CAL6	50	738107E+07	347621.400	6.91	
9H23034-CAL7	100	578899E+07	367889.900	6.91	
9H23034-CAL8	200	076568E+07	403828.400	6.91	
<b>AVE RF</b>	<b>356703.900</b>	<b>RF RSD</b>	<b>5.79</b>	<b>AVE RT</b>	<b>6.91</b>

## beta-BHC [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	176262	176262.000	6.98	
9H23034-CAL2	2	335260	167630.000	6.98	
9H23034-CAL3	5	788630	157726.000	6.98	
9H23034-CAL4	10	1580847	158084.700	6.98	
9H23034-CAL5	25	3677155	147086.200	6.98	
9H23034-CAL6	50	7516011	150320.200	6.98	
9H23034-CAL7	100	462518E+07	146251.800	6.98	
9H23034-CAL8	200	255343E+07	162767.200	6.98	
<b>AVE RF</b>	<b>158266.000</b>	<b>RF RSD</b>	<b>6.60</b>	<b>AVE RT</b>	<b>6.98</b>

## delta-BHC [2C]

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	349123	349123.000	7.23	
9H23034-CAL2	2	669122	334561.000	7.23	
9H23034-CAL3	5	1717450	343490.000	7.23	
9H23034-CAL4	10	3613517	361351.700	7.23	
9H23034-CAL5	25	8247775	329911.000	7.23	
9H23034-CAL6	50	731126E+07	346225.200	7.23	
9H23034-CAL7	100	517663E+07	351766.300	7.23	
9H23034-CAL8	200	097975E+07	404898.800	7.23	
<b>AVE RF</b>	<b>352663.900</b>	<b>RF RSD</b>	<b>6.60</b>	<b>AVE RT</b>	<b>7.23</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Oxychlorthane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	176844	176844.000	7.26	
9H23034-CALA	2	339370	169685.000	7.26	
9H23034-CALB	5	819748	163949.600	7.26	
9H23034-CALC	10	1591613	159161.300	7.26	
9H23034-CALD	25	3881255	155250.200	7.26	
9H23034-CALE	50	8382873	167657.500	7.26	
9H23034-CALF	100	535922E+07	163592.200	7.26	
9H23034-CALG	200	203263E+07	160163.200	7.26	
<b>AVE RF</b>	<b>164537.900</b>	<b>RF RSD</b>	<b>4.13</b>	<b>AVE RT</b>	<b>7.26</b>

## Heptachlor [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	309811	309811.000	7.29	
9H23034-CAL2	2	586765	293382.500	7.29	
9H23034-CAL3	5	1508218	301643.600	7.29	
9H23034-CAL4	10	3005915	300591.500	7.29	
9H23034-CAL5	25	7282282	291291.300	7.29	
9H23034-CAL6	50	459514E+07	291902.800	7.29	
9H23034-CAL7	100	027782E+07	302778.200	7.29	
9H23034-CAL8	200	128318E+07	356415.900	7.29	
<b>AVE RF</b>	<b>305977.100</b>	<b>RF RSD</b>	<b>6.98</b>	<b>AVE RT</b>	<b>7.29</b>

## Heptachlor epoxide


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	200503	200503.000	7.34	
9H23034-CAL2	2	392052	196026.000	7.34	
9H23034-CAL3	5	923620	184724.000	7.34	
9H23034-CAL4	10	1865428	186542.800	7.34	
9H23034-CAL5	25	4344286	173771.400	7.33	
9H23034-CAL6	50	8869300	177386.000	7.33	
9H23034-CAL7	100	731844E+07	173184.400	7.33	
9H23034-CAL8	200	525817E+07	181290.800	7.33	
<b>AVE RF</b>	<b>184178.600</b>	<b>RF RSD</b>	<b>5.42</b>	<b>AVE RT</b>	<b>7.33</b>

## 2,4'-DDE


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	137947	137947.000	7.34	
9H23034-CALA	2	265212	132606.000	7.33	
9H23034-CALB	5	633168	126633.600	7.33	
9H23034-CALC	10	1245265	124526.500	7.33	
9H23034-CALD	25	3059421	122376.800	7.33	
9H23034-CALE	50	6510588	130211.800	7.33	
9H23034-CALF	100	276907E+07	127690.700	7.33	
9H23034-CALG	200	1.48192E+07	124096.000	7.33	
<b>AVE RF</b>	<b>128261.100</b>	<b>RF RSD</b>	<b>4.01</b>	<b>AVE RT</b>	<b>7.33</b>

## Chlordane 1 (g)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALH	50	1009143	20182.860	7.43	
9H23034-CALI	100	1978897	19788.970	7.43	
9H23034-CALJ	200	3849299	19246.490	7.43	
9H23034-CALK	500	9628671	19257.340	7.43	
9H23034-CALL	1000	964377E+07	19643.770	7.43	
9H23034-CALM	2000	1.00365E+07	20018.250	7.43	
<b>AVE RF</b>	<b>19669.410</b>	<b>RF RSD</b>	<b>1.96</b>	<b>AVE RT</b>	<b>7.43</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## trans-Chlordane


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	197202	197202.000	7.43	
9H23034-CAL2	2	382271	191135.500	7.43	
9H23034-CAL3	5	926577	185315.400	7.43	
9H23034-CAL4	10	1847996	184799.600	7.43	
9H23034-CAL5	25	4401456	176058.200	7.43	
9H23034-CAL6	50	8959305	179186.100	7.43	
9H23034-CAL7	100	773279E+07	177327.900	7.43	
9H23034-CAL8	200	762141E+07	188107.000	7.43	
<b>AVE RF</b>	<b>184891.500</b>	<b>RF RSD</b>	<b>3.93</b>	<b>AVE RT</b>	<b>7.43</b>

## Toxaphene 1


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	49250	985.000	7.51	
9H23034-CALO	100	91576	915.760	7.50	
9H23034-CALP	200	176047	880.235	7.50	
9H23034-CALQ	500	441826	883.652	7.50	
9H23034-CALR	1000	871889	871.889	7.50	
9H23034-CALS	2000	1674674	837.337	7.50	
<b>AVE RF</b>	<b>895.646</b>	<b>RF RSD</b>	<b>5.63</b>	<b>AVE RT</b>	<b>7.50</b>

## trans-Nonachlor


Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	236836	236836.000	7.52	
9H23034-CALA	2	415126	207563.000	7.52	
9H23034-CALB	5	933222	186644.400	7.52	
9H23034-CALC	10	1817552	181755.200	7.52	
9H23034-CALD	25	4391046	175641.800	7.52	
9H23034-CALE	50	9581794	191635.900	7.52	
9H23034-CALF	100	835125E+07	183512.500	7.52	
9H23034-CALG	200	502792E+07	175139.600	7.51	
<b>AVE RF</b>	<b>192341.100</b>	<b>RF RSD</b>	<b>10.78</b>	<b>AVE RT</b>	<b>7.52</b>

## Chlordane 2


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALH	50	1286655	25733.100	7.52	
9H23034-CALI	100	2519520	25195.200	7.52	
9H23034-CALJ	200	4906320	24531.600	7.52	
9H23034-CALK	500	217652E+07	24353.040	7.52	
9H23034-CALL	1000	508324E+07	25083.240	7.52	
9H23034-CALM	2000	097914E+07	25489.570	7.52	
<b>AVE RF</b>	<b>25064.290</b>	<b>RF RSD</b>	<b>2.14</b>	<b>AVE RT</b>	<b>7.52</b>

## cis-Chlordane

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	209780	209780.000	7.53	
9H23034-CAL2	2	389999	194999.500	7.53	
9H23034-CAL3	5	908795	181759.000	7.53	
9H23034-CAL4	10	1843346	184334.600	7.53	
9H23034-CAL5	25	4244413	169776.500	7.53	
9H23034-CAL6	50	8622674	172453.500	7.52	
9H23034-CAL7	100	574258E+07	167425.800	7.52	
9H23034-CAL8	200	520794E+07	176039.700	7.52	
<b>AVE RF</b>	<b>182071.900</b>	<b>RF RSD</b>	<b>7.66</b>	<b>AVE RT</b>	<b>7.53</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Aldrin [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	317466	317466.000	7.56	
9H23034-CAL2	2	635458	317729.000	7.56	
9H23034-CAL3	5	1600995	320199.000	7.56	
9H23034-CAL4	10	3341093	334109.300	7.56	
9H23034-CAL5	25	7878574	315143.000	7.56	
9H23034-CAL6	50	526442E+07	325288.400	7.56	
9H23034-CAL7	100	390642E+07	339064.200	7.56	
9H23034-CAL8	200	322818E+07	366140.900	7.55	
<b>AVE RF</b>	<b>329392.500</b>	<b>RF RSD</b>	<b>5.19</b>	<b>AVE RT</b>	<b>7.56</b>

## 4,4'-DDE


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	193435	193435.000	7.59	
9H23034-CAL2	2	388618	194309.000	7.59	
9H23034-CAL3	5	953351	190670.200	7.59	
9H23034-CAL4	10	1890931	189093.100	7.59	
9H23034-CAL5	25	4571066	182842.600	7.58	
9H23034-CAL6	50	9177389	183547.800	7.58	
9H23034-CAL7	100	805255E+07	180525.500	7.58	
9H23034-CAL8	200	876308E+07	193815.400	7.58	
<b>AVE RF</b>	<b>188529.800</b>	<b>RF RSD</b>	<b>2.92</b>	<b>AVE RT</b>	<b>7.58</b>

## Endosulfan I


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	185217	185217.000	7.63	
9H23034-CAL2	2	357368	178684.000	7.63	
9H23034-CAL3	5	861509	172301.800	7.62	
9H23034-CAL4	10	1709332	170933.200	7.62	
9H23034-CAL5	25	4111285	164451.400	7.62	
9H23034-CAL6	50	7984410	159688.200	7.62	
9H23034-CAL7	100	1.609E+07	160900.000	7.62	
9H23034-CAL8	200	385259E+07	169263.000	7.62	
<b>AVE RF</b>	<b>170179.800</b>	<b>RF RSD</b>	<b>5.13</b>	<b>AVE RT</b>	<b>7.62</b>

## 2,4'-DDD


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	120240	120240.000	7.71	
9H23034-CALA	2	233089	116544.500	7.71	
9H23034-CALB	5	560942	112188.400	7.71	
9H23034-CALC	10	1103587	110358.700	7.71	
9H23034-CALD	25	2745178	109807.100	7.71	
9H23034-CALE	50	5920095	118401.900	7.71	
9H23034-CALF	100	158755E+07	115875.500	7.71	
9H23034-CALG	200	191696E+07	109584.800	7.70	
<b>AVE RF</b>	<b>114125.100</b>	<b>RF RSD</b>	<b>3.65</b>	<b>AVE RT</b>	<b>7.71</b>

## Dieldrin

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	197721	197721.000	7.80	
9H23034-CAL2	2	395728	197864.000	7.80	
9H23034-CAL3	5	972009	194401.800	7.80	
9H23034-CAL4	10	1954890	195489.000	7.80	
9H23034-CAL5	25	4582306	183292.200	7.79	
9H23034-CAL6	50	9386664	187733.300	7.79	
9H23034-CAL7	100	832442E+07	183244.200	7.79	
9H23034-CAL8	200	921777E+07	196088.800	7.79	
<b>AVE RF</b>	<b>191979.300</b>	<b>RF RSD</b>	<b>3.25</b>	<b>AVE RT</b>	<b>7.79</b>

## Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

### Toxaphene 2


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9H23034-CALN	50	88321	1766.420	7.79
9H23034-CALO	100	166085	1660.850	7.80
9H23034-CALP	200	317587	1587.935	7.80
9H23034-CALQ	500	819454	1638.908	7.79
9H23034-CALR	1000	1556013	1556.013	7.79
9H23034-CALS	2000	2958997	1479.499	7.79
<b>AVE RF</b>		<b>1614.937</b>	<b>RF RSD</b>	<b>6.08</b>
			<b>AVE RT</b>	<b>7.79</b>

### 2,4'-DDT


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9H23034-CAL9	1	107110	107110.000	7.89
9H23034-CALA	2	204209	102104.500	7.89
9H23034-CALB	5	536967	107393.400	7.89
9H23034-CALC	10	1051565	105156.500	7.89
9H23034-CALD	25	2728794	109151.800	7.89
9H23034-CALE	50	5687323	113746.500	7.89
9H23034-CALF	100	177135E+07	117713.500	7.89
9H23034-CALG	200	302496E+07	115124.800	7.89
<b>AVE RF</b>		<b>109687.600</b>	<b>RF RSD</b>	<b>4.88</b>
			<b>AVE RT</b>	<b>7.89</b>

### Oxychlorane [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9H23034-CAL9	1	279143	279143.000	7.92
9H23034-CALA	2	541023	270511.500	7.92
9H23034-CALB	5	1325543	265108.600	7.92
9H23034-CALC	10	2538903	253890.300	7.92
9H23034-CALD	25	6202791	248111.600	7.92
9H23034-CALE	50	417254E+07	283450.800	7.92
9H23034-CALF	100	973215E+07	297321.500	7.92
9H23034-CALG	200	873698E+07	293684.900	7.92
<b>AVE RF</b>		<b>273902.800</b>	<b>RF RSD</b>	<b>6.49</b>
			<b>AVE RT</b>	<b>7.92</b>

### Endrin


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9H23034-CAL1	1	156412	156412.000	7.96
9H23034-CAL2	2	298515	149257.500	7.96
9H23034-CAL3	5	738953	147790.600	7.96
9H23034-CAL4	10	1475508	147550.800	7.96
9H23034-CAL5	25	3508904	140356.200	7.96
9H23034-CAL6	50	6979572	139591.400	7.96
9H23034-CAL7	100	381271E+07	138127.100	7.96
9H23034-CAL8	200	142631E+07	157131.500	7.96
<b>AVE RF</b>		<b>147027.100</b>	<b>RF RSD</b>	<b>4.98</b>
			<b>AVE RT</b>	<b>7.96</b>

### cis-Nonachlor

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9H23034-CAL9	1	219220	219220.000	7.99
9H23034-CALA	2	423442	211721.000	7.99
9H23034-CALB	5	1025899	205179.800	7.99
9H23034-CALC	10	2032010	203201.000	7.99
9H23034-CALD	25	4993110	199724.400	7.99
9H23034-CALE	50	061602E+07	212320.400	7.99
9H23034-CALF	100	093264E+07	209326.400	7.99
9H23034-CALG	200	004618E+07	200230.900	7.98
<b>AVE RF</b>		<b>206136.000</b>	<b>RF RSD</b>	<b>3.25</b>
			<b>AVE RT</b>	<b>7.99</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Heptachlor epoxide [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	310098	310098.000	7.99	
9H23034-CAL2	2	606240	303120.000	7.99	
9H23034-CAL3	5	1455941	291188.200	7.99	
9H23034-CAL4	10	2959301	295930.100	7.99	
9H23034-CAL5	25	7064729	282589.200	7.99	
9H23034-CAL6	50	483779E+07	296755.800	7.99	
9H23034-CAL7	100	004551E+07	300455.100	7.99	
9H23034-CAL8	200	533007E+07	326650.400	7.99	
<b>AVE RF</b>	<b>300848.300</b>	<b>RF RSD</b>	<b>4.40</b>	<b>AVE RT</b>	<b>7.99</b>

## 4,4'-DDD


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	164956	164956.000	8.01	
9H23034-CAL2	2	314622	157311.000	8.01	
9H23034-CAL3	5	790498	158099.600	8.01	
9H23034-CAL4	10	1565974	156597.400	8.01	
9H23034-CAL5	25	3727035	149081.400	8.00	
9H23034-CAL6	50	7726197	154523.900	8.00	
9H23034-CAL7	100	543715E+07	154371.500	8.00	
9H23034-CAL8	200	1.24368E+07	162184.000	8.00	
<b>AVE RF</b>	<b>157140.600</b>	<b>RF RSD</b>	<b>3.11</b>	<b>AVE RT</b>	<b>8.00</b>

## Chlordane 3 (a)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALH	50	288087	5761.740	8.07	
9H23034-CALI	100	548196	5481.960	8.07	
9H23034-CALJ	200	1101677	5508.385	8.07	
9H23034-CALK	500	2921278	5842.556	8.07	
9H23034-CALL	1000	5987927	5987.927	8.07	
9H23034-CALM	2000	220831E+07	6104.155	8.07	
<b>AVE RF</b>	<b>5781.121</b>	<b>RF RSD</b>	<b>4.34</b>	<b>AVE RT</b>	<b>8.07</b>

## Toxaphene 3


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	169381	3387.620	8.11	
9H23034-CALO	100	332842	3328.420	8.11	
9H23034-CALP	200	644464	3222.320	8.11	
9H23034-CALQ	500	1677481	3354.962	8.11	
9H23034-CALR	1000	3495877	3495.877	8.11	
9H23034-CALS	2000	6831460	3415.730	8.10	
<b>AVE RF</b>	<b>3367.488</b>	<b>RF RSD</b>	<b>2.72</b>	<b>AVE RT</b>	<b>8.11</b>

## Endosulfan II

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	158139	158139.000	8.12	
9H23034-CAL2	2	299106	149553.000	8.12	
9H23034-CAL3	5	709544	141908.800	8.12	
9H23034-CAL4	10	1448080	144808.000	8.12	
9H23034-CAL5	25	3371864	134874.600	8.12	
9H23034-CAL6	50	6840920	136818.400	8.11	
9H23034-CAL7	100	.35435E+07	135435.000	8.11	
9H23034-CAL8	200	947104E+07	147355.200	8.11	
<b>AVE RF</b>	<b>143611.500</b>	<b>RF RSD</b>	<b>5.61</b>	<b>AVE RT</b>	<b>8.12</b>



# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## 2,4'-DDE [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	219164	219164.000	8.12	
9H23034-CALA	2	411812	205906.000	8.12	
9H23034-CALB	5	1029687	205937.400	8.12	
9H23034-CALC	10	2018331	201833.100	8.12	
9H23034-CALD	25	4999232	199969.300	8.12	
9H23034-CALE	50	10064E+07	220128.000	8.12	
9H23034-CALF	100	21644E+07	221644.000	8.12	
9H23034-CALG	200	450459E+07	222523.000	8.12	
<b>AVE RF</b>	<b>212138.100</b>	<b>RF RSD</b>	<b>4.52</b>	<b>AVE RT</b>	<b>8.12</b>

## Chlordane 1 (g) [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALH	50	1754707	35094.140	8.13	
9H23034-CALI	100	3378388	33783.880	8.13	
9H23034-CALJ	200	6751197	33755.980	8.13	
9H23034-CALK	500	783043E+07	35660.860	8.13	
9H23034-CALL	1000	796674E+07	37966.740	8.13	
9H23034-CALM	2000	169171E+07	40845.860	8.13	
<b>AVE RF</b>	<b>36184.580</b>	<b>RF RSD</b>	<b>7.62</b>	<b>AVE RT</b>	<b>8.13</b>

## trans-Chlordane [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	364142	364142.000	8.14	
9H23034-CAL2	2	644454	322227.000	8.14	
9H23034-CAL3	5	1502119	300423.800	8.13	
9H23034-CAL4	10	3002782	300278.200	8.13	
9H23034-CAL5	25	7157480	286299.200	8.13	
9H23034-CAL6	50	467872E+07	293574.400	8.13	
9H23034-CAL7	100	074227E+07	307422.700	8.13	
9H23034-CAL8	200	644797E+07	332239.800	8.13	
<b>AVE RF</b>	<b>313325.900</b>	<b>RF RSD</b>	<b>8.10</b>	<b>AVE RT</b>	<b>8.13</b>

## trans-Nonachlor [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	306202	306202.000	8.20	
9H23034-CALA	2	587765	293882.500	8.19	
9H23034-CALB	5	1467723	293544.600	8.19	
9H23034-CALC	10	2844404	284440.400	8.19	
9H23034-CALD	25	7092288	283691.500	8.19	
9H23034-CALE	50	580771E+07	316154.200	8.19	
9H23034-CALF	100	197527E+07	319752.700	8.20	
9H23034-CALG	200	308364E+07	315418.200	8.19	
<b>AVE RF</b>	<b>301635.800</b>	<b>RF RSD</b>	<b>4.84</b>	<b>AVE RT</b>	<b>8.19</b>

## 4,4'-DDT

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	113897	113897.000	8.21	
9H23034-CAL2	2	218190	109095.000	8.20	
9H23034-CAL3	5	553009	110601.800	8.21	
9H23034-CAL4	10	1146556	114655.600	8.20	
9H23034-CAL5	25	2924467	116978.700	8.20	
9H23034-CAL6	50	6205369	124107.400	8.20	
9H23034-CAL7	100	217696E+07	121769.600	8.20	
9H23034-CAL8	200	907522E+07	145376.100	8.20	
<b>AVE RF</b>	<b>119566.100</b>	<b>RF RSD</b>	<b>9.72</b>	<b>AVE RT</b>	<b>8.20</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Chlordane 2 (a) [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALH	50	1472400	29448.000	8.24	
9H23034-CALI	100	2905941	29059.410	8.24	
9H23034-CALJ	200	5883615	29418.070	8.24	
9H23034-CALK	500	481227E+07	29624.540	8.24	
9H23034-CALL	1000	149368E+07	31493.680	8.24	
9H23034-CALM	2000	528139E+07	33140.700	8.24	
<b>AVE RF</b>	<b>30364.070</b>	<b>RF RSD</b>	<b>5.30</b>	<b>AVE RT</b>	<b>8.24</b>

## cis-Chlordane [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	299422	299422.000	8.24	
9H23034-CAL2	2	579667	289833.500	8.24	
9H23034-CAL3	5	1434855	286971.000	8.24	
9H23034-CAL4	10	2859573	285957.300	8.24	
9H23034-CAL5	25	6935857	277434.300	8.24	
9H23034-CAL6	50	400212E+07	280042.400	8.24	
9H23034-CAL7	100	904286E+07	290428.600	8.24	
9H23034-CAL8	200	397706E+07	319885.300	8.24	
<b>AVE RF</b>	<b>291246.800</b>	<b>RF RSD</b>	<b>4.59</b>	<b>AVE RT</b>	<b>8.24</b>

## Endosulfan I [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	278874	278874.000	8.29	
9H23034-CAL2	2	540442	270221.000	8.29	
9H23034-CAL3	5	1327191	265438.200	8.29	
9H23034-CAL4	10	2724272	272427.200	8.29	
9H23034-CAL5	25	6571512	262860.500	8.29	
9H23034-CAL6	50	371233E+07	274246.600	8.29	
9H23034-CAL7	100	721271E+07	272127.100	8.29	
9H23034-CAL8	200	104351E+07	305217.600	8.29	
<b>AVE RF</b>	<b>275176.500</b>	<b>RF RSD</b>	<b>4.77</b>	<b>AVE RT</b>	<b>8.29</b>

## 4,4'-DDE [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	298463	298463.000	8.35	
9H23034-CAL2	2	598066	299033.000	8.35	
9H23034-CAL3	5	1487999	297599.800	8.35	
9H23034-CAL4	10	3049792	304979.200	8.35	
9H23034-CAL5	25	7501047	300041.900	8.34	
9H23034-CAL6	50	555471E+07	311094.200	8.34	
9H23034-CAL7	100	1.24996E+07	324996.000	8.34	
9H23034-CAL8	200	984235E+07	349211.800	8.34	
<b>AVE RF</b>	<b>310677.400</b>	<b>RF RSD</b>	<b>5.82</b>	<b>AVE RT</b>	<b>8.34</b>

## Toxaphene 4

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	164317	3286.340	8.35	
9H23034-CALO	100	320313	3203.130	8.35	
9H23034-CALP	200	632351	3161.755	8.35	
9H23034-CALQ	500	1649569	3299.138	8.35	
9H23034-CALR	1000	3287014	3287.014	8.35	
9H23034-CALS	2000	6407070	3203.535	8.35	
<b>AVE RF</b>	<b>3240.132</b>	<b>RF RSD</b>	<b>1.82</b>	<b>AVE RT</b>	<b>8.35</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Endrin Aldehyde


Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	241285	241285.000	8.41	
9H23034-CAL2	2	328182	164091.000	8.41	
9H23034-CAL3	5	683393	136678.600	8.41	
9H23034-CAL4	10	1375129	137512.900	8.41	
9H23034-CAL5	25	3119767	124790.700	8.40	
9H23034-CAL6	50	6224451	124489.000	8.40	
9H23034-CAL7	100	236381E+07	123638.100	8.40	
9H23034-CAL8	200	562767E+07	133138.300	8.40	
<b>AVE RF</b>	<b>148203.000</b>	<b>RF RSD</b>	<b>26.87</b>	<b>AVE RT</b>	<b>8.41</b>

## Toxaphene 1 [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	136848	2736.960	8.47	
9H23034-CALO	100	267534	2675.340	8.47	
9H23034-CALP	200	508983	2544.915	8.47	
9H23034-CALQ	500	1308994	2617.988	8.47	
9H23034-CALR	1000	2654886	2654.886	8.47	
9H23034-CALS	2000	5030917	2515.458	8.47	
<b>AVE RF</b>	<b>2624.258</b>	<b>RF RSD</b>	<b>3.16</b>	<b>AVE RT</b>	<b>8.47</b>

## Dieldrin [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	296684	296684.000	8.49	
9H23034-CAL2	2	583812	291906.000	8.49	
9H23034-CAL3	5	1462538	292507.600	8.49	
9H23034-CAL4	10	2898866	289886.600	8.49	
9H23034-CAL5	25	7333890	293355.600	8.49	
9H23034-CAL6	50	543411E+07	308682.200	8.49	
9H23034-CAL7	100	100196E+07	310019.600	8.49	
9H23034-CAL8	200	003178E+07	350158.900	8.49	
<b>AVE RF</b>	<b>304150.100</b>	<b>RF RSD</b>	<b>6.61</b>	<b>AVE RT</b>	<b>8.49</b>

## 2,4'-DDD [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	192040	192040.000	8.50	
9H23034-CALA	2	373596	186798.000	8.50	
9H23034-CALB	5	898697	179739.400	8.50	
9H23034-CALC	10	1778790	177879.000	8.50	
9H23034-CALD	25	4389185	175567.400	8.50	
9H23034-CALE	50	9924934	198498.700	8.50	
9H23034-CALF	100	011892E+07	201189.200	8.50	
9H23034-CALG	200	198393E+07	199196.500	8.49	
<b>AVE RF</b>	<b>188863.500</b>	<b>RF RSD</b>	<b>5.47</b>	<b>AVE RT</b>	<b>8.50</b>

## Methoxychlor

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	59659	59659.000	8.54	
9H23034-CAL2	2	111466	55733.000	8.54	
9H23034-CAL3	5	270388	54077.600	8.54	
9H23034-CAL4	10	561706	56170.600	8.54	
9H23034-CAL5	25	1390283	55611.320	8.54	
9H23034-CAL6	50	2860683	57213.660	8.54	
9H23034-CAL7	100	5877329	58773.290	8.54	
9H23034-CAL8	200	427114E+07	71355.700	8.54	
<b>AVE RF</b>	<b>58574.290</b>	<b>RF RSD</b>	<b>9.93</b>	<b>AVE RT</b>	<b>8.54</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Toxaphene 5


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	114720	2294.400	8.57	
9H23034-CALO	100	228960	2289.600	8.57	
9H23034-CALP	200	454431	2272.155	8.57	
9H23034-CALQ	500	1221560	2443.120	8.57	
9H23034-CALR	1000	2546293	2546.293	8.57	
9H23034-CALS	2000	5074570	2537.285	8.57	
<b>AVE RF</b>	<b>2397.142</b>	<b>RF RSD</b>	<b>5.33</b>	<b>AVE RT</b>	<b>8.57</b>

## Toxaphene 6


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	153138	3062.760	8.64	
9H23034-CALO	100	302577	3025.770	8.64	
9H23034-CALP	200	597991	2989.955	8.64	
9H23034-CALQ	500	1623402	3246.804	8.64	
9H23034-CALR	1000	3406737	3406.737	8.64	
9H23034-CALS	2000	6510950	3255.475	8.64	
<b>AVE RF</b>	<b>3164.584</b>	<b>RF RSD</b>	<b>5.17</b>	<b>AVE RT</b>	<b>8.64</b>

## Mirex


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	147356	147356.000	8.66	
9H23034-CALA	2	266770	133385.000	8.66	
9H23034-CALB	5	628618	125723.600	8.65	
9H23034-CALC	10	1196365	119636.500	8.65	
9H23034-CALD	25	2910818	116432.700	8.65	
9H23034-CALE	50	6218341	124366.800	8.65	
9H23034-CALF	100	196075E+07	119607.500	8.65	
9H23034-CALG	200	2.3285E+07	116425.000	8.65	
<b>AVE RF</b>	<b>125366.600</b>	<b>RF RSD</b>	<b>8.39</b>	<b>AVE RT</b>	<b>8.65</b>

## Endosulfan sulfate


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	176097	176097.000	8.71	
9H23034-CAL2	2	322163	161081.500	8.71	
9H23034-CAL3	5	768798	153759.600	8.71	
9H23034-CAL4	10	1553540	155354.000	8.71	
9H23034-CAL5	25	3645411	145816.400	8.71	
9H23034-CAL6	50	7420576	148411.500	8.71	
9H23034-CAL7	100	436679E+07	143667.900	8.70	
9H23034-CAL8	200	112652E+07	155632.600	8.70	
<b>AVE RF</b>	<b>154977.600</b>	<b>RF RSD</b>	<b>6.64</b>	<b>AVE RT</b>	<b>8.71</b>

## Endrin [2C]

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	222882	222882.000	8.72	
9H23034-CAL2	2	424889	212444.500	8.72	
9H23034-CAL3	5	1092877	218575.400	8.72	
9H23034-CAL4	10	2244483	224448.300	8.72	
9H23034-CAL5	25	5325883	213035.300	8.72	
9H23034-CAL6	50	101538E+07	220307.600	8.72	
9H23034-CAL7	100	310241E+07	231024.100	8.72	
9H23034-CAL8	200	277958E+07	263897.900	8.72	
<b>AVE RF</b>	<b>225626.000</b>	<b>RF RSD</b>	<b>6.12</b>	<b>AVE RT</b>	<b>8.72</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## 2,4'-DDT [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	173338	173338.000	8.72	
9H23034-CALA	2	332170	166085.000	8.72	
9H23034-CALB	5	873074	174614.800	8.72	
9H23034-CALC	10	1702568	170256.800	8.72	
9H23034-CALD	25	4405554	176222.200	8.72	
9H23034-CALE	50	8810591	176211.800	8.72	
9H23034-CALF	100	899897E+07	189989.700	8.72	
9H23034-CALG	200	999923E+07	199996.200	8.72	
<b>AVE RF</b>	<b>178339.300</b>	<b>RF RSD</b>	<b>6.24</b>	<b>AVE RT</b>	<b>8.72</b>

## 4,4'-DDD [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	251549	251549.000	8.76	
9H23034-CAL2	2	488120	244060.000	8.76	
9H23034-CAL3	5	1208642	241728.400	8.76	
9H23034-CAL4	10	2425496	242549.600	8.76	
9H23034-CAL5	25	6146469	245858.800	8.76	
9H23034-CAL6	50	315945E+07	263189.000	8.76	
9H23034-CAL7	100	629748E+07	262974.800	8.76	
9H23034-CAL8	200	956027E+07	297801.400	8.76	
<b>AVE RF</b>	<b>256213.900</b>	<b>RF RSD</b>	<b>7.37</b>	<b>AVE RT</b>	<b>8.76</b>

## cis-Nonachlor [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	332745	332745.000	8.76	
9H23034-CALA	2	624783	312391.500	8.76	
9H23034-CALB	5	1587243	317448.600	8.76	
9H23034-CALC	10	3148054	314805.400	8.76	
9H23034-CALD	25	8219393	328775.700	8.76	
9H23034-CALE	50	772123E+07	354424.600	8.76	
9H23034-CALF	100	507264E+07	360726.400	8.76	
9H23034-CALG	200	245582E+07	362279.100	8.76	
<b>AVE RF</b>	<b>335449.500</b>	<b>RF RSD</b>	<b>6.23</b>	<b>AVE RT</b>	<b>8.76</b>

## Toxaphene 2 [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	164706	3294.120	8.81	
9H23034-CALO	100	324070	3240.700	8.81	
9H23034-CALP	200	645322	3226.610	8.81	
9H23034-CALQ	500	1647741	3295.482	8.81	
9H23034-CALR	1000	3384036	3384.036	8.81	
9H23034-CALS	2000	6610397	3305.198	8.81	
<b>AVE RF</b>	<b>3291.024</b>	<b>RF RSD</b>	<b>1.70</b>	<b>AVE RT</b>	<b>8.81</b>

## Toxaphene 3 [2C]

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	254833	5096.660	8.85	
9H23034-CALO	100	494430	4944.300	8.85	
9H23034-CALP	200	995555	4977.775	8.85	
9H23034-CALQ	500	2475022	4950.044	8.85	
9H23034-CALR	1000	5168269	5168.269	8.85	
9H23034-CALS	2000	054571E+07	5272.855	8.85	
<b>AVE RF</b>	<b>5088.319</b>	<b>RF RSD</b>	<b>2.65</b>	<b>AVE RT</b>	<b>8.85</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Endosulfan II [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	232156	232156.000	8.87	
9H23034-CAL2	2	462256	231128.000	8.86	
9H23034-CAL3	5	1096359	219271.800	8.87	
9H23034-CAL4	10	2243610	224361.000	8.86	
9H23034-CAL5	25	5447602	217904.100	8.86	
9H23034-CAL6	50	153453E+07	230690.600	8.86	
9H23034-CAL7	100	301637E+07	230163.700	8.86	
9H23034-CAL8	200	183489E+07	259174.400	8.86	
<b>AVE RF</b>	<b>230606.200</b>	<b>RF RSD</b>	<b>5.55</b>	<b>AVE RT</b>	<b>8.86</b>

## Chlordane 3 [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALH	50	439020	8780.400	8.90	
9H23034-CALI	100	874465	8744.650	8.90	
9H23034-CALJ	200	1731727	8658.635	8.90	
9H23034-CALK	500	4271709	8543.418	8.90	
9H23034-CALL	1000	9358900	9358.900	8.90	
9H23034-CALM	2000	941852E+07	9709.260	8.90	
<b>AVE RF</b>	<b>8965.877</b>	<b>RF RSD</b>	<b>5.14</b>	<b>AVE RT</b>	<b>8.90</b>

## Endrin ketone


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	177552	177552.000	8.90	
9H23034-CAL2	2	331269	165634.500	8.90	
9H23034-CAL3	5	811384	162276.800	8.90	
9H23034-CAL4	10	1664380	166438.000	8.90	
9H23034-CAL5	25	4008958	160358.300	8.90	
9H23034-CAL6	50	8190707	163814.100	8.90	
9H23034-CAL7	100	525194E+07	162519.400	8.90	
9H23034-CAL8	200	509472E+07	175473.600	8.90	
<b>AVE RF</b>	<b>166758.300</b>	<b>RF RSD</b>	<b>3.80</b>	<b>AVE RT</b>	<b>8.90</b>

## Toxaphene 4 [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CALN	50	416348	8326.960	8.92	
9H23034-CALO	100	811948	8119.480	8.92	
9H23034-CALP	200	1580436	7902.180	8.91	
9H23034-CALQ	500	4252640	8505.280	8.92	
9H23034-CALR	1000	8650068	8650.068	8.92	
9H23034-CALS	2000	719004E+07	8595.020	8.91	
<b>AVE RF</b>	<b>8349.831</b>	<b>RF RSD</b>	<b>3.51</b>	<b>AVE RT</b>	<b>8.91</b>

## 4,4'-DDT [2C]

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	179700	179700.000	8.99	
9H23034-CAL2	2	341782	170891.000	8.99	
9H23034-CAL3	5	873653	174730.600	8.99	
9H23034-CAL4	10	1841119	184111.900	8.99	
9H23034-CAL5	25	4480388	179215.500	8.98	
9H23034-CAL6	50	9285492	185709.800	8.99	
9H23034-CAL7	100	97895E+07	197895.000	8.98	
9H23034-CAL8	200	820344E+07	241017.200	8.98	
<b>AVE RF</b>	<b>189158.000</b>	<b>RF RSD</b>	<b>1.88</b>	<b>AVE RT</b>	<b>8.99</b>

# Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

## Toxaphene 5 [2C]

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9H23034-CALN	50	233185	4663.700	9.09
9H23034-CALO	100	452209	4522.090	9.09
9H23034-CALP	200	895397	4476.985	9.09
9H23034-CALQ	500	2340668	4681.336	9.09
9H23034-CALR	1000	4900430	4900.430	9.09
9H23034-CALS	2000	9435236	4717.618	9.09

**AVE RF 4660.360      RF RSD 3.24      AVE RT 9.09**

## Endrin Aldehyde [2C]

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9H23034-CAL1	1	348624	348624.000	9.10
9H23034-CAL2	2	477694	238847.000	9.10
9H23034-CAL3	5	1045869	209173.800	9.10
9H23034-CAL4	10	2125028	212502.800	9.10
9H23034-CAL5	25	4848504	193940.200	9.10
9H23034-CAL6	50	020903E+07	204180.600	9.10
9H23034-CAL7	100	050274E+07	205027.400	9.10
9H23034-CAL8	200	508454E+07	225422.700	9.10

**AVE RF 229714.800      RF RSD 21.77      AVE RT 9.10**

## Endosulfan sulfate [2C]

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9H23034-CAL1	1	265797	265797.000	9.29
9H23034-CAL2	2	498767	249383.500	9.29
9H23034-CAL3	5	1175908	235181.600	9.29
9H23034-CAL4	10	2424584	242458.400	9.29
9H23034-CAL5	25	5978906	239156.200	9.29
9H23034-CAL6	50	214929E+07	242985.800	9.29
9H23034-CAL7	100	447732E+07	244773.200	9.29
9H23034-CAL8	200	459279E+07	272964.000	9.29

**AVE RF 249087.500      RF RSD 5.35      AVE RT 9.29**

## Methoxychlor [2C]

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9H23034-CAL1	1	95155	95155.000	9.47
9H23034-CAL2	2	178074	89037.000	9.47
9H23034-CAL3	5	413802	82760.400	9.47
9H23034-CAL4	10	883069	88306.900	9.47
9H23034-CAL5	25	2166659	86666.360	9.46
9H23034-CAL6	50	4346199	86923.980	9.46
9H23034-CAL7	100	9444987	94449.870	9.46
9H23034-CAL8	200	1.37141E+07	118570.500	9.46

**AVE RF 92733.750      RF RSD 12.09      AVE RT 9.46**

## Toxaphene 6 [2C]

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9H23034-CALN	50	230922	4618.440	9.47
9H23034-CALO	100	452485	4524.850	9.47
9H23034-CALP	200	905244	4526.220	9.47
9H23034-CALQ	500	2369795	4739.590	9.47
9H23034-CALR	1000	5046645	5046.645	9.47
9H23034-CALS	2000	009095E+07	5045.475	9.47

**AVE RF 4756.200      RF RSD 5.10      AVE RT 9.47**

## Element Calibration Review Sheet

Calibration ID: **A9H2608**

Instrument: **DUALECD5**


Calibration Date: **08/26/2019**

Analysis: **8081B Pesticides + Add**

Instrument Cal ID: **ECD5\_QUANTPEST\_19082**

### Decachlorobiphenyl (Surr)


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	163865	163865.000	9.59	
9H23034-CAL2	2	309904	154952.000	9.59	
9H23034-CAL3	5	701050	140210.000	9.59	
9H23034-CAL4	10	1335468	133546.800	9.59	
9H23034-CAL5	25	3342634	133705.400	9.59	
9H23034-CAL6	50	6678990	133579.800	9.59	
9H23034-CAL7	100	.34054E+07	134054.000	9.59	
9H23034-CAL8	200	697523E+07	134876.200	9.59	
<b>AVE RF</b>	<b>141098.600</b>	<b>RF RSD</b>	<b>8.33</b>	<b>AVE RT</b>	<b>9.59</b>

### Mirex [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL9	1	209783	209783.000	9.68	
9H23034-CALA	2	388199	194099.500	9.68	
9H23034-CALB	5	895523	179104.600	9.68	
9H23034-CALC	10	1722960	172296.000	9.68	
9H23034-CALD	25	4138115	165524.600	9.68	
9H23034-CALE	50	9100959	182019.200	9.68	
9H23034-CALF	100	.93632E+07	193632.000	9.68	
9H23034-CALG	200	842553E+07	192127.600	9.68	
<b>AVE RF</b>	<b>186073.300</b>	<b>RF RSD</b>	<b>7.59</b>	<b>AVE RT</b>	<b>9.68</b>

### Endrin ketone [2C]


Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	255763	255763.000	9.69	
9H23034-CAL2	2	493110	246555.000	9.69	
9H23034-CAL3	5	1205004	241000.800	9.69	
9H23034-CAL4	10	2496985	249698.500	9.69	
9H23034-CAL5	25	5893691	235747.600	9.69	
9H23034-CAL6	50	295457E+07	259091.400	9.69	
9H23034-CAL7	100	563656E+07	266365.600	9.69	
9H23034-CAL8	200	086138E+07	304306.900	9.69	
<b>AVE RF</b>	<b>257316.100</b>	<b>RF RSD</b>	<b>8.31</b>	<b>AVE RT</b>	<b>9.69</b>

### Decachlorobiphenyl (Surr) [2C]

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT	
9H23034-CAL1	1	191572	191572.000	10.54	
9H23034-CAL2	2	390006	195003.000	10.54	
9H23034-CAL3	5	870921	174184.200	10.54	
9H23034-CAL4	10	1678728	167872.800	10.54	
9H23034-CAL5	25	4163229	166529.200	10.54	
9H23034-CAL6	50	8730692	174613.800	10.54	
9H23034-CAL7	100	778407E+07	177840.700	10.54	
9H23034-CAL8	200	809778E+07	190488.900	10.54	
<b>AVE RF</b>	<b>179763.100</b>	<b>RF RSD</b>	<b>6.18</b>	<b>AVE RT</b>	<b>10.54</b>



# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9H23034

## Analysis Included

1311/8081B TCLP Pest Reg List  
1311/8081B TCLP Pest Reg List +ADD  
1311/8081B TCLP Pesticides (All)  
1311/8081B TCLP Pesticides + Add (All)  
1312/8081B SPLP Pesticides  
608 Additional Only (QC)  
608 Pest (Chlordane)  
608 Pesticides  
608 Pesticides (DDT Only)  
608 Pesticides (SW)  
608 Pesticides (SW) Full List  
608 Pesticides (TTO)  
608 Pesticides + Adds  
608.3 Additional - DEVELOPMENT  
608.3 Chlordane - DEVELOPMENT  
608.3 PCBs - DEVELOPMENT  
608.3 Pesticides - DEVELOPMENT  
608.3 Pesticides + Adds - DEVELOPMENT  
608.3 Toxaphene - DEVELOPMENT  
8081B Pesticides  
8081B 2,4+4,4-DDx Only (+Add)  
8081B Chlordane  
8081B DDT Only  
8081B Pesticides + Add  
8081B RSET FW Sed (+Add) (2016)  
8081B RSET Sediment List (+Add)  
8081B RSET Sediment Marine (2016) (+Add)  
8081B Toxaphene

# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9H23034

## INSTRUMENT SEQUENCE LOG

SampleID	SampleName	Matrix	STDID	ISTD_ID	Analyzed
9H23034-ICB1	Initial Cal Blank	Water	A19H348		8/23/2019 1:33:00PM
9H23034-CAL1	Cal Standard	Water	A19E245	"	8/23/2019 1:51:00PM
9H23034-CAL2	Cal Standard	Water	A19E246	"	8/23/2019 2:08:00PM
9H23034-CAL3	Cal Standard	Water	A19E247	"	8/23/2019 2:25:00PM
9H23034-CAL4	Cal Standard	Water	A19E249	"	8/23/2019 2:42:00PM
9H23034-CAL5	Cal Standard	Water	A19E250	"	8/23/2019 3:00:00PM
9H23034-CAL6	Cal Standard	Water	A19H383	"	8/23/2019 3:17:00PM
9H23034-CAL7	Cal Standard	Water	A19H384	"	8/23/2019 3:34:00PM
9H23034-CAL8	Cal Standard	Water	A19E244	"	8/23/2019 3:52:00PM
9H23034-ICV1	Initial Cal Check	Water	A19E106	"	8/23/2019 4:26:00PM
9H23034-CAL9	Cal Standard	Water	A19E272	"	8/23/2019 4:44:00PM
9H23034-CALA	Cal Standard	Water	A19E273	"	8/23/2019 5:01:00PM
9H23034-CALB	Cal Standard	Water	A19E274	"	8/23/2019 5:18:00PM
9H23034-CALC	Cal Standard	Water	A19E275	"	8/23/2019 5:35:00PM
9H23034-CALD	Cal Standard	Water	A19E276	"	8/23/2019 5:53:00PM
9H23034-CALE	Cal Standard	Water	A19E154	"	8/23/2019 6:10:00PM
9H23034-CALF	Cal Standard	Water	A19E155	"	8/23/2019 6:27:00PM
9H23034-CALG	Cal Standard	Water	A19E271	"	8/23/2019 6:45:00PM
9H23034-ICV2	Initial Cal Check	Water	A19E043	"	8/23/2019 7:19:00PM
9H23034-CALH	Cal Standard	Water	A19F232	"	8/23/2019 7:36:00PM
9H23034-CALI	Cal Standard	Water	A19F233	"	8/23/2019 7:54:00PM
9H23034-CALJ	Cal Standard	Water	A19F234	"	8/23/2019 8:11:00PM
9H23034-CALK	Cal Standard	Water	A19F235	"	8/23/2019 8:28:00PM
9H23034-CALL	Cal Standard	Water	A19F236	"	8/23/2019 8:45:00PM
9H23034-CALM	Cal Standard	Water	A19F231	"	8/23/2019 9:02:00PM
9H23034-ICV3	Initial Cal Check	Water	A19E108	"	8/23/2019 9:37:00PM
9H23034-CALN	Cal Standard	Water	A19D122	"	8/23/2019 9:54:00PM
9H23034-CALO	Cal Standard	Water	A19D123	"	8/23/2019 10:11:00PM
9H23034-CALP	Cal Standard	Water	A19D124	"	8/23/2019 10:28:00PM
9H23034-CALQ	Cal Standard	Water	A19D125	"	8/23/2019 10:45:00PM
9H23034-CALR	Cal Standard	Water	A19D126	"	8/23/2019 11:03:00PM
9H23034-CALS	Cal Standard	Water	A19D121	"	8/23/2019 11:20:00PM
9H23034-ICV4	Initial Cal Check	Water	A19D127	"	8/23/2019 11:54:00PM

## CALIBRATION STANDARD RECOVERIES

Calibration: A9H2608

Instrument: DualECD5F

1311/8081B TCLP Pest Reg L

Sequence: 9H23034

Matrix: Water

SampleID	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CAL1					
9H23034-CAL2					
9H23034-CAL3					
9H23034-CAL4					
9H23034-CAL5					

# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9H23034

9H23034-CAL6	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CAL7	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CAL8	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CAL9	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALA	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALB	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALC	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALD	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALE	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALF	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALG	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALH	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALI	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALJ	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALK	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALL	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALM	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALN	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALO	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALP	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALQ	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALR	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9H23034-CALS	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual

Compounds listed above have recalculated recoveries outside 70-130% of the true values, and the calibration levels are above the reporting level. If no compounds are listed, all are OK. Please see the next section for quadratic fit compounds.

# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9H23034

## Analytes With Quadratic Curve Fits

Qualifier   iMDL   iMRL   Spike Amt   %Difference   OK?   Raise MRL to ?  
 \_\_\_\_\_         \_\_\_\_\_

Analytes listed above have quadratic curve fits. If they are using a weighting option, they must be checked against the requested curve points to determine if the recalculated results are within limits (70-130 or as specified).

### ICV RECOVERIES

Calibration: **A9H2608**

Instrument: **DualECD5F**

608 Pesticides (SW) Full List

Sequence: **9H23034**

Matrix: **Water**

9H23034-ICV1	Inst. MRL	ICV Level	Result	%Rec.	Qual
9H23034-ICV2	Inst. MRL	ICV Level	Result	%Rec.	Qual
9H23034-ICV3	Inst. MRL	ICV Level	Result	%Rec.	Qual
9H23034-ICV4	Inst. MRL	ICV Level	Result	%Rec.	Qual

Compounds listed above have Initial Calibration Verification standard recoveries outside 70-130% of the true values. If no compounds are listed, all have passing recoveries.

4,4'-DDT #2




R = 3.30e+002 A\*A + 1.71e+005 A + 6.57e+003  
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic w(1/a^2)  
Method Name: R:\methods\BCD5\_QUANTPEST\_190825.M  
Calibration Table Last Updated: Mon Aug 26 11:58:51 2019

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231908.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 13:51  
Operator : MJB  
Sample : 9H23034-CAL1  
Misc : A19E245, AB 1 ppb  
ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:59:55 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(17) 4,4'-DDT  
8.205min 0.953 ng/mL  
response 113897

MJB 8/26/19

(17) 4,4'-DDT #2  
8.971min -0.006 ng/mL (m)  
response 5621

Endrin Aldehyde




R = 8.05e+001 A\*A + 1.16e+005 A + 1.19e+005  
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic w/(1/a^2)  
Method Name: R:\methods\ECD5\_QUANTPEST\_190825.M  
Calibration Table Last Updated: Mon Aug 26 11:58:51 2019  
12/26/19 Anchor OEA, LLC Gasco PPRD DG 2019 -4c Waste Characterization Page 399 of 919

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231908.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 13:51  
Operator : MJB  
Sample : 9H23034-CAL1  
Misc : A19E245, AB 1 ppb  
ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:59:55 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped




(18) Endrin Aldehyde  
8.379min -0.993 ng/mL(m)  
response 3543

*MJB 8/26/19*

(18) Endrin Aldehyde #2  
9.101min 1.058 ng/mL  
response 348624



Endrin Aldehyde #2




R = 2.18e+002 A\*A + 1.83e+005 A + 1.55e+005  
Coef of Det (r<sup>2</sup>) = 0.996 Curve Fit: Quadratic w(1/a<sup>2</sup>)  
Method Name: R:\methods\BCD5\_QUANTRES1\_190823.M  
Calibration Table Last Updated: Mon Aug 26 11:58:51 2019

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231908.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 13:51  
 Operator : MJB  
 Sample : 9H23034-CAL1  
 Misc : A19E245, AB 1 ppb  
 ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:59:55 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(18) Endrin Aldehyde  
 8.379min -0.993 ng/mL m  
 response 3543

*MJB 8/26/19*

(18) Endrin Aldehyde #2  
 9.068min -0.831 ng/mL (m)  
 response 3374

Methoxychlor #2




R = 1.78e+002 A\*A + 8.05e+004 A + 1.50e+004  
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic w(1/a^2)  
Method Name: R:\methods\ECD5\_QUANTPEST\_190825.M  
Calibration Table Last Updated: Mon Aug 26 11:58:51 2019

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231908.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 13:51  
Operator : MJB  
Sample : 9H23034-CAL1  
Misc : A19E245, AB 1 ppb  
ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:59:55 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(20) Methoxychlor  
8.543min 1.019 ng/mL  
response 59659

MJB  
8/26/19

(20) Methoxychlor #2  
9.449min -0.161 ng/mL (m)  
response 2070

trans-Nonachlor



$R = -2.05e+000 A^2 + 1.79e+005 A + 5.67e+004$

Coef of Det ( $r^2$ ) = 0.999 Curve Fit: Quadratic w(1/a<sup>2</sup>)



Method Name: R:\methods\BCL5\_50\ANPRESI\_19023.M 12/26/19 Anchor QEA LLC - Gasco RefRD DG 2019 - 4c. Waste Characterization Page 405 of 919

Calibration Table Last Updated: Mon Aug 26 11:58:51 2019

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231918.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 16:44  
Operator : MJB  
Sample : 9H23034-CAL9  
Misc : A19E272, 9-42 1 ppb  
ALS Vial : 13 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:02:15 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(27) trans-Nonachlor  
7.498min 87346.675 ng/mL(m) *Q=01*  
response 4808 *MJB 8/26/19*

(27) trans-Nonachlor #2  
8.195min 1.015 ng/mL  
response 306202

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231907.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 13:33  
 Operator : MJB  
 Sample : 9H23034-ICB1  
 Misc : A19H348  
 ALS Vial : 3 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:02:44 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



MJB 8/26/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.398	5.992	15096765	27637017	90.958	94.206
22) S DCBP (S)	9.594	10.543	12462090	16576085	88.322	92.211
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.253f	0.000	6973	0	0.035	N.D. #
4) b-BHC	0.000	7.003f	0	10802	N.D.	0.068 #
5) Heptachlor	6.596f	0.000	8260	0	0.046	N.D. #
6) d-BHC	6.451	7.234	5541	7061	0.028	0.020
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	7.318	0.000	2356	0	0.013	N.D. #
9) trans-Chl...	0.000	8.140	0	104395	N.D.	0.333 #
10) cis-Chlor...	7.514	0.000	58774	0	0.323	N.D. #
11) Endosulfa...	0.000	0.000	0	0	N.D.	N.D.
12) 4,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
13) Dieldrin	0.000	0.000	0	0	N.D.	N.D.
14) Endrin	0.000	0.000	0	0	N.D.	N.D.
15) 4,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
16) Endosulfa...	8.119	0.000	3735	0	0.026	N.D. #
17) 4,4'-DDT	8.185	0.000	4049	0	0.034	N.D. #
18) Endrin Al...	8.408	9.102	14375	14948	BelowCal	BelowCal
19) Endosulfa...	8.709	9.292	12123	14809	0.078	0.059
20) Methoxychlor	8.542	0.000	4975	0	0.085	N.D. #
21) Endrin Ke...	8.903	9.690	4830	7943	0.029	0.031
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.779	0.000	21656	0	0.123	N.D. #
25) Oxychlorane	0.000	0.000	0	0	N.D.	N.D.
26) 2,4'-DDE	7.318	8.140	2356	104395	0.018	0.492 #
27) trans-Non...	7.514	0.000	58774	0	0.012	N.D. #
28) 2,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
29) 2,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
30) cis-Nonac...	0.000	0.000	0	0	N.D.	N.D.
31) Mirex	8.652	9.690	4544	7943	0.036	0.043
32) Chlordane...	0.000	8.140	0	104395	N.D.	2.885 #
33) Chlordane...	7.514	0.000	58774	0	2.345	N.D. #
34) Chlordane...	0.000	8.904	0	37260	N.D.	4.156 #
35) Chlordane...	3.445	0.000	6677	0	NoCal	N.D.
36) Toxaphene...	7.514	0.000	58774	0	65.621	N.D. #
37) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
38) Toxaphene...	8.119	0.000	3735	0	1.109	N.D. #
39) Toxaphene...	8.312f	8.904	24186	37260	7.464	4.462 #
40) Toxaphene...	8.542f	9.102	4975	14948	2.075	3.207 #
41) Toxaphene...	8.652	0.000	4544	0	1.436	N.D. #
42) Toxaphene...	3.445	0.000	6677	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231907.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 13:33  
Operator : MJB  
Sample : 9H23034-ICB1  
Misc : A19H348  
ALS Vial : 3 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:02:44 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231916.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 16:09  
 Operator : MJB  
 Sample : 9H23034-IBL1  
 Misc : Instrument Blank  
 ALS Vial : 1 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:02:50 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*Clean*



*MJB 8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
<b>System Monitoring Compounds</b>						
1) S TCMX (S)	0.000	5.984	0	7755	N.D.	0.026 #
22) S DCBP (S)	9.595	10.540	5550	5660	0.039	0.031
<b>Target Compounds</b>						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.249f	0.000	4370	0	0.022	N.D. #
4) b-BHC	0.000	7.003f	0	7432	N.D.	0.047 #
5) Heptachlor	6.602f	0.000	4945	0	0.027	N.D. #
6) d-BHC	6.450	7.233	6336	9226	0.032	0.026
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	0.000	0.000	0	0	N.D.	N.D.
9) trans-Chl...	0.000	8.142	0	99412	N.D.	0.317 #
10) cis-Chlor...	7.516	0.000	56525	0	0.310	N.D. #
11) Endosulfa...	0.000	0.000	0	0	N.D.	N.D.
12) 4,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
13) Dieldrin	0.000	0.000	0	0	N.D.	N.D.
14) Endrin	0.000	0.000	0	0	N.D.	N.D.
15) 4,4'-DDD	8.007	0.000	1177	0	0.007	N.D. #
16) Endosulfa...	8.117	8.865	3391	6280	0.024	0.027
17) 4,4'-DDT	8.226f	0.000	1460	0	0.012	N.D. #
18) Endrin Al...	8.407	9.100	21929	28697	BelowCal	BelowCal
19) Endosulfa...	8.707	9.291	12087	18257	0.078	0.073
20) Methoxychlor	8.544	0.000	4198	0	0.072	N.D. #
21) Endrin Ke...	8.901	9.686	4385	18734	0.026	0.073 #
23) Hexachlor...	0.000	3.689	0	2782	N.D.	0.007 #
24) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
25) Oxychlordane	0.000	0.000	0	0	N.D.	N.D.
26) 2,4'-DDE	0.000	8.142	0	99412	N.D. <i>Q-ent</i>	0.469 #
27) trans-Non...	7.516	0.000	56525	0	<del>0.7346.385</del>	N.D. #
28) 2,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
29) 2,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
30) cis-Nonac...	8.007f	0.000	1177	0	0.006	N.D. #
31) Mirex	0.000	9.686	0	18734	N.D.	0.101 #
32) Chlordane...	0.000	8.142	0	99412	N.D.	2.747 #
33) Chlordane...	7.516	0.000	56525	0	2.255	N.D. #
34) Chlordane...	8.065	8.904	2775	39801	0.480	4.439 #
35) Chlordane...	3.447	0.000	4520	0	NoCal	N.D.
36) Toxaphene...	7.516	0.000	56525	0	63.111	N.D. #
37) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
38) Toxaphene...	8.117	8.865	3391	6280	1.007	1.239
39) Toxaphene...	8.314f	8.904	23317	39801	7.196	4.767
40) Toxaphene...	8.583	9.100	2463	28697	1.028	6.158 #
41) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
42) Toxaphene...	3.447	0.000	4520	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231916.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 16:09  
Operator : MJB  
Sample : 9H23034-IBL1  
Misc : Instrument Blank  
ALS Vial : 1 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:02:50 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231917.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 16:26  
 Operator : MJB  
 Sample : 9H23034-ICV1  
 Misc : A19E106, AB 50 ppb  
 ALS Vial : 12 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:02:56 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.395	5.989	8209928	14467910	49.465	49.317
22) S DCBP (S)	9.589	10.539	6928381	8667079	49.103	48.214
Target Compounds						
2) a-BHC	5.935	6.596	11712240	21507667	51.072	52.414
3) g-BHC	6.218	6.913	10370774	18809716	51.397	52.732
4) b-BHC	6.296	6.977	4410789	7929442	48.801	50.102
5) Heptachlor	6.629	7.288	9286546	15998647	51.223	52.287
6) d-BHC	6.446	7.231	10162400	18561571	51.667	52.632
7) Aldrin	6.870	7.553	10415223	17743229	52.750	53.867
8) Heptachlo...	7.330	7.991	9218950	15454788	50.054	51.371
9) trans-Chl...	7.427	8.130	9449748	15882363	51.110	50.690
10) cis-Chlor...	7.523	8.238	8891439	15040020	48.835	51.640
11) Endosulfa...	7.620	8.288	8454858	14042285	49.682	51.030
12) 4,4'-DDE	7.583	8.343	9669653	16358741	51.290	52.655
13) Dieldrin	7.792	8.489	9566646	15751562	49.832	51.789
14) Endrin	7.957	8.715	7744641	11999227	52.675	53.135
15) 4,4'-DDD	8.003	8.758	8044313	14118585	51.192	55.105
16) Endosulfa...	8.114	8.862	7639079	12307624	53.193	53.371
17) 4,4'-DDT	8.201	8.984	6427421	10243965	53.759	54.092
18) Endrin Al...	8.403	9.098	7471981	12138603	60.652	61.144
19) Endosulfa...	8.704	9.289	8022310	12945664	51.764	51.972
20) Methoxychlor	8.537	9.463	3243218	5107379	55.369	56.272
21) Endrin Ke...	8.898	9.687	8897553	13958232	53.356	54.245
23) Hexachlor...	0.000	3.713f	0	6424	N.D.	0.017 #
24) Hexachlor...	5.778	6.482f	19713	11218	0.112	0.036 #
25) Oxychlordane	7.266	7.916	116203	18640	0.706	0.068 #
26) 2,4'-DDE	7.330	8.130	9218950	15882363	71.876	74.868
27) trans-Non...	7.523	8.193	8891439	52587	49.340	0.174 #
28) 2,4'-DDD	7.704	8.489	22276	15751562	0.195	83.402 #
29) 2,4'-DDT	7.889	8.715	44366	11999227	0.404	67.283 #
30) cis-Nonac...	8.003	8.758	8044313	14118585	38.746	42.089
31) Mirex	8.653	9.687	40409	13958232	0.322	75.015 #
32) Chlordane...	7.427	8.130	9449748	15882363	479.936	438.926
33) Chlordane...	7.523	8.238	8891439	15040020	354.745	495.323
34) Chlordane...	0.000	8.899	0	79876	N.D.	8.909 #
35) Chlordane...	3.446	0.000	5075	0	NoCal	N.D.
36) Toxaphene...	7.523f	8.489f	8891439	15751562	9927.388	6002.292
37) Toxaphene...	7.792	0.000	9566646	0	5923.845	N.D. #
38) Toxaphene...	8.114	8.862	7639079	12307624	2268.479	2428.346
39) Toxaphene...	8.324f	8.899	184731	79876	57.013	9.566 #
40) Toxaphene...	8.537f	9.098	3243218	12138603	1352.952	2604.650 #
41) Toxaphene...	8.653	9.463	40409	5107379	12.769	1075.192 #
42) Toxaphene...	3.446	0.000	5075	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231917.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 16:26  
Operator : MJB  
Sample : 9H23034-ICV1  
Misc : A19E106, AB 50 ppb  
ALS Vial : 12 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:02:56 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231926.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 19:02  
 Operator : MJB  
 Sample : 9H23034-IBL2  
 Misc : Instrument Blank  
 ALS Vial : 1 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:03:03 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



*Clean*  
*MJB*  
*8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
<b>System Monitoring Compounds</b>						
1) S TCMX (S)	0.000	5.979	0	6612	N.D.	0.023 #
22) S DCBP (S)	0.000	0.000	0	0	N.D.	N.D.
<b>Target Compounds</b>						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.246f	0.000	5266	0	0.026	N.D. #
4) b-BHC	0.000	0.000	0	0	N.D.	N.D.
5) Heptachlor	6.606f	0.000	2965	0	0.016	N.D. #
6) d-BHC	6.448	7.230	6262	8744	0.032	0.025
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	0.000	0.000	0	0	N.D.	N.D.
9) trans-Chl...	0.000	8.141	0	95737	N.D.	0.306 #
10) cis-Chlor...	7.516	0.000	51171	0	0.281	N.D. #
11) Endosulfa...	0.000	0.000	0	0	N.D.	N.D.
12) 4,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
13) Dieldrin	0.000	0.000	0	0	N.D.	N.D.
14) Endrin	0.000	0.000	0	0	N.D.	N.D.
15) 4,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
16) Endosulfa...	8.115	8.861	2908	5919	0.020	0.026
17) 4,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
18) Endrin Al...	8.404	9.098	11210	14199	BelowCal	BelowCal
19) Endosulfa...	8.705	9.288	9669	15528	0.062	0.062
20) Methoxychlor	8.535	0.000	2114	0	0.036	N.D. #
21) Endrin Ke...	8.899	9.685	4160	14028	0.025	0.055 #
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
25) Oxychlorthane	0.000	0.000	0	0	N.D.	N.D.
26) 2,4'-DDE	0.000	8.141	0	95737	N.D.	0.451 #
27) trans-Non...	7.516	0.000	51171	0	<del>87346.415</del>	N.D. #
28) 2,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
29) 2,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
30) cis-Nonac...	0.000	0.000	0	0	N.D.	N.D.
31) Mirex	8.653	9.685	1197	14028	0.010	0.075 #
32) Chlordane...	0.000	8.141	0	95737	N.D.	2.646 #
33) Chlordane...	7.516	0.000	51171	0	2.042	N.D. #
34) Chlordane...	8.051	8.903	2776	42860	0.480	4.780 #
35) Chlordane...	3.446	0.000	4206	0	NoCal	N.D.
36) Toxaphene...	7.516	0.000	51171	0	57.133	N.D. #
37) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
38) Toxaphene...	8.115	8.861	2908	5919	0.863	1.168
39) Toxaphene...	8.313f	8.903	23619	42860	7.290	5.133
40) Toxaphene...	8.535f	9.098	2114	14199	0.882	3.047 #
41) Toxaphene...	8.653	0.000	1197	0	0.378	N.D. #
42) Toxaphene...	3.446	0.000	4206	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231926.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 19:02  
Operator : MJB  
Sample : 9H23034-IBL2  
Misc : Instrument Blank  
ALS Vial : 1 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:03:03 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231927.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 19:19  
 Operator : MJB  
 Sample : 9H23034-ICV2  
 Misc : A19E043, 9-42 50 ppb  
 ALS Vial : 21 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:03:09 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*WPB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.367f	5.979	21795	7434	0.131	0.025 #
22) S DCBP (S)	9.593	0.000	5164	0	0.037	N.D. #
Target Compounds						
2) a-BHC	5.944	0.000	7626	0	0.033	N.D. #
3) g-BHC	6.193f	6.950f	4309	4488	0.021	0.013 #
4) b-BHC	6.276f	6.950f	4448	4488	0.049	0.028 #
5) Heptachlor	6.631	7.288	13910	18612	0.077	0.061
6) d-BHC	6.450	7.231	4193	7280	0.021	0.021
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	7.333	7.969f	6044730	30442	32.820	0.101 #
9) trans-Chl...	7.428	8.122	135885	10152421	0.735	32.402 #
10) cis-Chlor...	7.515	8.238	9079715	499411	49.869	1.715 #
11) Endosulfa...	7.623	8.313f	100346	33305	0.590	0.121 #
12) 4,4'-DDE	7.585	8.350	33793	99515	0.179	0.320 #
13) Dieldrin	7.801	8.494	35090	9221128	0.183	30.318 #
14) Endrin	7.985f	8.719	9530740	8396212	64.823	37.180 #
15) 4,4'-DDD	7.985	8.758	9530740	16410440	60.651	64.050
16) Endosulfa...	0.000	8.903f	0	43832	N.D.	0.190 #
17) 4,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
18) Endrin Al...	8.400	9.100	6045	8867	BelowCal	BelowCal
19) Endosulfa...	0.000	9.288	0	6758	N.D.	0.027 #
20) Methoxychlor	0.000	0.000	0	0	N.D.	N.D.
21) Endrin Ke...	8.897	9.678	3909	8640754	0.023	33.580 #
23) Hexachlor...	3.197	3.687	8657262	18235302	47.375	48.507
24) Hexachlor...	5.774	6.453	8419764	15057280	47.760	47.940
25) Oxychlordane	7.260	7.920	8060765	13729255	48.990	50.125
26) 2,4'-DDE	7.333	8.122	6044730	10152421	47.128	47.858
27) trans-Non...	7.515	8.194	9079715	15314695	50.392	50.772
28) 2,4'-DDD	7.704	8.494	5439144	9221128	47.659	48.824
29) 2,4'-DDT	7.888	8.719	5329154	8396212	48.585	47.080
30) cis-Nonac...	7.985	8.758	9530740	16410440	45.906	48.921
31) Mirex	8.652	9.678	5900124	8640754	47.063	46.437
32) Chlordane...	7.428	8.122	135885	10152421	6.901	280.573 #
33) Chlordane...	7.515	8.238	9079715	499411	362.257	16.447 #
34) Chlordane...	0.000	8.903	0	43832	N.D.	4.889 #
35) Chlordane...	3.444	3.433	15163	32758	NoCal	NoCal
36) Toxaphene...	7.515	8.494f	9079715	9221128	10137.600	3513.804 #
37) Toxaphene...	7.801	0.000	35090	0	21.729	N.D. #
38) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
39) Toxaphene...	8.313f	8.903	24546	43832	7.576	5.249
40) Toxaphene...	0.000	9.100	0	8867	N.D.	1.903 #
41) Toxaphene...	8.652	0.000	5900124	0	1864.424	N.D. #
42) Toxaphene...	3.444	3.433	15163	32758	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231927.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 19:19  
Operator : MJB  
Sample : 9H23034-ICV2  
Misc : A19E043, 9-42 50 ppb  
ALS Vial : 21 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:03:09 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231934.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 21:20  
 Operator : MJB  
 Sample : 9H23034-IBL3  
 Misc : Instrument Blank  
 ALS Vial : 1 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:03:15 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



*Ann*  
*MJB*  
*8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.976	0	5923	N.D.	0.020 #
22) S DCBP (S)	0.000	0.000	0	0	N.D.	N.D.
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.207	0.000	3774	0	0.019	N.D. #
4) b-BHC	0.000	0.000	0	0	N.D.	N.D.
5) Heptachlor	6.609f	0.000	2731	0	0.015	N.D. #
6) d-BHC	6.450	7.231	5497	6832	0.028	0.019
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	0.000	0.000	0	0	N.D.	N.D.
9) trans-Chl...	0.000	8.142	0	83130	N.D.	0.265 #
10) cis-Chlor...	7.519	0.000	51396	0	0.282	N.D. #
11) Endosulfa...	0.000	0.000	0	0	N.D.	N.D.
12) 4,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
13) Dieldrin	0.000	0.000	0	0	N.D.	N.D.
14) Endrin	0.000	0.000	0	0	N.D.	N.D.
15) 4,4'-DDD	8.023f	0.000	4578	0	0.029	N.D. #
16) Endosulfa...	8.116	8.861	1913	3871	0.013	0.017
17) 4,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
18) Endrin Al...	8.405	9.098	8970	10610	BelowCal	BelowCal
19) Endosulfa...	8.706	9.288	7044	10525	0.045	0.042
20) Methoxychlor	8.536	0.000	1701	0	0.029	N.D. #
21) Endrin Ke...	8.919f	9.686	4032	9735	0.024	0.038 #
23) Hexachlor...	0.000	3.679	0	2600	N.D.	0.007 #
24) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
25) Oxychlordane	0.000	0.000	0	0	N.D.	N.D.
26) 2,4'-DDE	0.000	8.142	0	83130	N.D. <i>Ret</i>	0.392 #
27) trans-Non...	7.519	0.000	51396	0	<del>87346.414</del>	N.D. #
28) 2,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
29) 2,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
30) cis-Nonac...	8.023f	0.000	4578	0	0.022	N.D. #
31) Mirex	0.000	9.686	0	9735	N.D.	0.052 #
32) Chlordane...	0.000	8.142	0	83130	N.D.	2.297 #
33) Chlordane...	7.519	0.000	51396	0	2.051	N.D. #
34) Chlordane...	0.000	8.904	0	38172	N.D.	4.258 #
35) Chlordane...	3.449	0.000	3828	0	NoCal	N.D.
36) Toxaphene...	7.519	0.000	51396	0	57.384	N.D. #
37) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
38) Toxaphene...	8.116	8.861	1913	3871	0.568	0.764
39) Toxaphene...	8.316f	8.904	21302	38172	6.574	4.572
40) Toxaphene...	8.536f	9.098	1701	10610	0.709	2.277 #
41) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
42) Toxaphene...	3.449	0.000	3828	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231934.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:20  
Operator : MJB  
Sample : 9H23034-IBL3  
Misc : Instrument Blank  
ALS Vial : 1 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:03:15 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231935.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 21:37  
 Operator : MJB  
 Sample : 9H23034-ICV3  
 Misc : A19F108, CHLOR 500 ppb  
 ALS Vial : 28 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:03:22 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB*  
*8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.975	0	8961	N.D.	0.031 #
22) S DCBP (S)	9.601	10.507f	18796	7616	0.133	0.042 #
Target Compounds						
2) a-BHC	5.934	6.622f	9141	348363	0.040	0.849 #
3) g-BHC	6.194f	6.923	92353	182619	0.458	0.512 #
4) b-BHC	6.323f	7.017f	112667	560662	1.247	3.543 #
5) Heptachlor	6.630	7.288	4625489	7814185	25.513	25.538 #
6) d-BHC	6.412f	7.222	337700	61064	1.717	0.173 #
7) Aldrin	6.874	7.557	83911	133681	0.425	0.406 #
8) Heptachlo...	7.336	8.010	771372	473989	4.188	1.576 #
9) trans-Chl...	7.427	8.130	10721056	19872286	57.986	63.424 #
10) cis-Chlor...	7.520	8.238	13401062	16289264	73.603	55.929 #
11) Endosulfa...	7.639	8.310f	285254	253033	1.676	0.920 #
12) 4,4'-DDE	7.578	8.333	311083	429833	1.650	1.384 #
13) Dieldrin	7.806	8.488	355046	1298858	1.849	4.270 #
14) Endrin	7.984f	8.713	1829350	383068	12.442	1.696 #
15) 4,4'-DDD	7.984	8.759	1829350	3046940	11.641	11.892 #
16) Endosulfa...	8.118	8.873	216170	351371	1.505	1.524 #
17) 4,4'-DDT	0.000	8.994	0	130946	N.D.	0.725 #
18) Endrin Al...	8.427f	9.128f	55387	802635	BelowCal	3.530 #
19) Endosulfa...	8.708	9.290	120383	34589	0.777	0.139 #
20) Methoxychlor	8.552	9.463	53824	27882	0.919	0.160 #
21) Endrin Ke...	8.894	9.687	19548	156351	0.117	0.608 #
23) Hexachlor...	3.198	3.688	5435	10087	0.030	0.027 #
24) Hexachlor...	5.768	6.431f	8591	38244	0.049	0.122 #
25) Oxychlordane	7.253	7.933	114695	258636	0.697	0.944 #
26) 2,4'-DDE	7.336	8.130	771372	19872286	6.014	93.676 #
27) trans-Non...	7.520	8.195	13401062	14312099	74.546	47.448 #
28) 2,4'-DDD	7.674f	8.488	831029	1298858	7.282	6.877 #
29) 2,4'-DDT	7.913f	8.713	254540	383068	2.321	2.148 #
30) cis-Nonac...	7.984	8.759	1829350	3046940	8.811	9.083 #
31) Mirex	8.643	9.687	16477	156351	0.131	0.840 #
32) Chlordane...	7.427	8.130	10721056	19872286	544.503	549.192 #
33) Chlordane...	7.520	8.238	13401062	16289264	534.667	536.465 #
34) Chlordane...	8.068	8.898	3177144	4850138	549.572	540.955 #
35) Chlordane...	3.448	0.000	3889	0	NoCal	N.D.
36) Toxaphene...	7.520	8.488f	13401062	1298858	14962.430	494.943 #
37) Toxaphene...	7.806	8.814	355046	496679	219.851	150.919 #
38) Toxaphene...	8.118	8.851	216170	383467	64.193	75.660 #
39) Toxaphene...	8.347	8.898	132572	4850138	40.915	580.866 #
40) Toxaphene...	8.552f	9.068f	53824	98957	22.453	21.234 #
41) Toxaphene...	8.643	9.463	16477	27882	5.207	5.870 #
42) Toxaphene...	3.448	0.000	3889	0	NoCal	N.D.

*B* *E*  
*542.91* *542.20*

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231935.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:37  
Operator : MJB  
Sample : 9H23034-ICV3  
Misc : A19F108, CHLOR 500 ppb  
ALS Vial : 28 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:03:22 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231942.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 23:37  
 Operator : MJB  
 Sample : 9H23034-IBL4  
 Misc : Instrument Blank  
 ALS Vial : 1 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:03:28 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



*MJB  
8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.983	0	6142	N.D.	0.021 #
22) S DCBP (S)	0.000	0.000	0	0	N.D.	N.D.
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.248f	0.000	4243	0	0.021	N.D. #
4) b-BHC	0.000	0.000	0	0	N.D.	N.D.
5) Heptachlor	0.000	0.000	0	0	N.D.	N.D.
6) d-BHC	6.450	7.232	5264	7410	0.027	0.021
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	7.334	0.000	1978	0	0.011	N.D. #
9) trans-Chl...	7.425	8.145	1693	72982	0.009	0.233 #
10) cis-Chlor...	7.522	0.000	38316	0	0.210	N.D. #
11) Endosulfa...	0.000	0.000	0	0	N.D.	N.D.
12) 4,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
13) Dieldrin	0.000	0.000	0	0	N.D.	N.D.
14) Endrin	0.000	0.000	0	0	N.D.	N.D.
15) 4,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
16) Endosulfa...	8.117	0.000	2505	0	0.017	N.D. #
17) 4,4'-DDT	8.194	0.000	767	0	0.006	N.D. #
18) Endrin Al...	8.406	9.100	10140	13686	BelowCal	BelowCal
19) Endosulfa...	8.707	9.290	7273	12897	0.047	0.052
20) Methoxychlor	8.540	0.000	2018	0	0.034	N.D. #
21) Endrin Ke...	8.901	9.687	3565	7207	0.021	0.028
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
25) Oxychlorane	0.000	0.000	0	0	N.D.	N.D.
26) 2,4'-DDE	7.334	8.145f	1978	72982	0.015	0.344 #
27) trans-Non...	7.522	0.000	38316	0	<del>87346.487</del>	N.D. #
28) 2,4'-DDD	0.000	0.000	0	0	N.D.	N.D.
29) 2,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
30) cis-Nonac...	0.000	0.000	0	0	N.D.	N.D.
31) Mirex	8.644	9.687	766	7207	0.006	0.039 #
32) Chlordane...	7.425	8.145	1693	72982	0.086	2.017 #
33) Chlordane...	7.522	0.000	38316	0	1.529	N.D. #
34) Chlordane...	8.049	8.906	2785	37528	0.482	4.186 #
35) Chlordane...	3.451	0.000	3890	0	NoCal	N.D.
36) Toxaphene...	7.522f	0.000	38316	0	42.781	N.D. #
37) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
38) Toxaphene...	8.117	0.000	2505	0	0.744	N.D. #
39) Toxaphene...	8.318f	8.906	18960	37528	5.852	4.495
40) Toxaphene...	8.540f	9.100	2018	13686	0.842	2.937 #
41) Toxaphene...	8.644	0.000	766	0	0.242	N.D. #
42) Toxaphene...	3.451	0.000	3890	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231942.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 23:37  
Operator : MJB  
Sample : 9H23034-IBL4  
Misc : Instrument Blank  
ALS Vial : 1 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:03:28 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231943.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 23:54  
 Operator : MJB  
 Sample : 9H23034-ICV4  
 Misc : A19D127, TOX 500 ppb  
 ALS Vial : 35 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 15:03:35 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.984	0	5611	N.D.	0.019 #
22) S DCBP (S)	9.591	10.521	22246	40017	0.158	0.223 #
Target Compounds						
2) a-BHC	5.949	6.596	3272	7415	0.014	0.018
3) g-BHC	6.247f	6.907	6246	18839	0.031	0.053 #
4) b-BHC	6.296	6.966	11447	24200	0.127	0.153
5) Heptachlor	6.631	7.293	23849	45477	0.132	0.149
6) d-BHC	6.434	7.233	11867	47325	0.060	0.134 #
7) Aldrin	6.871	7.582f	53004	119759	0.268	0.364
8) Heptachlo...	7.358f	7.984	250185	414973	1.358	1.379
9) trans-Chl...	7.445	8.135	315388	332556	1.706	1.061
10) cis-Chlor...	7.501f	8.220	426074	475646	2.340	1.633
11) Endosulfa...	7.629	8.295	511717	592244	3.007	2.152
12) 4,4'-DDE	7.551f	8.359	359885	753065	1.909	2.424
13) Dieldrin	7.794	8.506	766286	726725	3.992	2.389 #
14) Endrin	7.934f	8.711	607064	1341537	4.129	5.941 #
15) 4,4'-DDD	8.021	8.761	679517	912025	4.324	3.560
16) Endosulfa...	8.105	8.848	1638713	2447077	11.411	10.611
17) 4,4'-DDT	8.184	8.976	1416015	960593	11.844	5.508 #
18) Endrin Al...	8.392	9.091	1088580	2275708	8.285	11.454
19) Endosulfa...	8.709	9.291	549140	929201	3.543	3.730
20) Methoxychlor	8.543	9.470	549172	2364076	9.376	27.518 #
21) Endrin Ke...	8.893	9.712f	380224	458705	2.280	1.783
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.813f	6.462	3660	6563	0.021	0.021
25) Oxychlorane	7.265	7.936	334880	406205	2.035	1.483
26) 2,4'-DDE	7.358f	8.112	250185	466633	1.951	2.200
27) trans-Non...	7.501	8.205	426074	457454	2.062	1.517
28) 2,4'-DDD	7.712	8.506	575777	726725	5.045	3.848
29) 2,4'-DDT	7.898	8.711	911632	1341537	8.311	7.522
30) cis-Nonac...	7.982	8.761	1096031	912025	5.279	2.719 #
31) Mirex	8.641	9.712f	1546722	458705	12.338	2.465 #
32) Chlordane...	7.445	8.135	315388	332556	16.018	9.191 #
33) Chlordane...	7.501	8.220	426074	475646	16.999	15.665
34) Chlordane...	8.046f	8.915	705731	4045258	122.075	451.184 # A
35) Chlordane...	3.453	0.000	2732	0	NoCal	N.D. B
36) Toxaphene...	7.501	8.466	426074	1252556	475.717	477.299
37) Toxaphene...	7.794	8.813	766286	1618562	474.499	491.811
38) Toxaphene...	8.105	8.848	1638713	2447077	486.627	482.818
39) Toxaphene...	8.346	8.915	1570667	4045258	484.751	484.472
40) Toxaphene...	8.573	9.091	1186452	2275708	494.944	488.312
41) Toxaphene...	8.641	9.470	1546722	2364076	488.760	497.679
42) Toxaphene...	3.453	0.000	2732	0	NoCal	N.D.

484.22 487.07

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231943.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 23:54  
Operator : MJB  
Sample : 9H23034-ICV4  
Misc : A19D127, TOX 500 ppb  
ALS Vial : 35 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 15:03:35 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231908.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 13:51  
 Operator : MJB  
 Sample : 9H23034-CAL1  
 Misc : A19E245, AB 1 ppb  
 ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:59:55 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB 8/26/19


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.397	5.991	176748	300053	1.065	1.023
22) S DCBP (S)	9.593	10.541	163865	191572	1.161	1.066
Target Compounds						
2) a-BHC	5.937	6.597	231994	393119	1.012	0.958
3) g-BHC	6.221	6.915	207427	352286	1.028	0.988
4) b-BHC	6.300	6.980	104326	176262	1.154	1.114
5) Heptachlor	6.635	7.292	192066	309811	1.059	1.013
6) d-BHC	6.450	7.234	199840	349123	1.016	0.990
7) Aldrin	6.875	7.557	205523	317466	1.041	0.964
8) Heptachlo...	7.335	7.994	200503	310098	1.089	1.031
9) trans-Chl...	7.433	8.135	197202	364142	1.067	1.162
10) cis-Chlor...	7.528	8.241	209780	299422	1.152	1.028
11) Endosulfa...	7.625	8.291	185217	278874	1.088	1.013
12) 4,4'-DDE	7.586	8.346	193435	298463	1.026	0.961
13) Dieldrin	7.796	8.491	197721	296684	1.030	0.975
14) Endrin	7.961	8.718	156412	222882	1.064	0.987
15) 4,4'-DDD	8.007	8.760	164956	251549	1.050	0.982
16) Endosulfa...	8.118	8.865	158139	232156	1.101	1.007
17) 4,4'-DDT	8.205	8.986	113897	179700	0.953	1.008
18) Endrin Al...	8.407	9.101	241285	348624	1.050	1.058
19) Endosulfa...	8.708	9.292	176097	265797	1.136	1.067
20) Methoxychlor	8.543	9.466	59659	95155	1.019	0.994
21) Endrin Ke...	8.901	9.690	177552	255763	1.065	0.994
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
25) Oxychlorane	0.000	0.000	0	0	N.D.	N.D.
26) 2,4'-DDE	7.335	8.135	200503	364142	1.563	1.717
27) trans-Non...	7.528	0.000	209780	0	0.855	N.D. #
28) 2,4'-DDD	0.000	8.491	0	296684	N.D.	1.571 #
29) 2,4'-DDT	0.000	8.718	0	222882	N.D.	1.250 #
30) cis-Nonac...	8.007f	8.760	164956	251549	0.795	0.750
31) Mirex	0.000	9.690	0	255763	N.D.	1.375 #
32) Chlordane...	7.433	8.135	197202	364142	10.016	10.063
33) Chlordane...	7.528	8.241	209780	299422	8.370	9.861
34) Chlordane...	0.000	8.903	0	37787	N.D.	4.214 #
35) Chlordane...	3.445	0.000	4502	0	NoCal	N.D.
36) Toxaphene...	7.528f	8.491f	209780	296684	234.222	113.054 #
37) Toxaphene...	7.796	0.000	197721	0	122.432	N.D. #
38) Toxaphene...	8.118	8.865	158139	232156	46.960	45.805
39) Toxaphene...	8.312f	8.903	20859	37787	6.438	4.525
40) Toxaphene...	8.543f	9.101	59659	348624	24.888	74.806 #
41) Toxaphene...	0.000	9.466	0	95155	N.D.	20.032 #
42) Toxaphene...	3.445	0.000	4502	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231908.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 13:51  
Operator : MJB  
Sample : 9H23034-CAL1  
Misc : A19E245, AB 1 ppb  
ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:59:55 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231909.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 14:08  
 Operator : MJB  
 Sample : 9H23034-CAL2  
 Misc : A19E246, AB 2 ppb  
 ALS Vial : 5 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:00:13 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



MJB  
8/26/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.396	5.990	349972	600766	2.109	2.048
22) S DCBP (S)	9.593	10.542	309904	390006	2.196	2.170
Target Compounds						
2) a-BHC	5.936	6.597	458365	784586	1.999	1.912
3) g-BHC	6.220	6.915	406027	690922	2.012	1.937
4) b-BHC	6.300	6.980	194168	335260	2.148	2.118
5) Heptachlor	6.635	7.291	369615	586765	2.039	1.918
6) d-BHC	6.450	7.233	386980	669122	1.967	1.897
7) Aldrin	6.875	7.556	399550	635458	2.024	1.929
8) Heptachlo...	7.335	7.993	392052	606240	2.129	2.015
9) trans-Chl...	7.432	8.135	382271	644454	2.068	2.057
10) cis-Chlor...	7.527	8.241	389999	579667	2.142	1.990
11) Endosulfa...	7.625	8.291	357368	540442	2.100	1.964
12) 4,4'-DDE	7.586	8.345	388618	598066	2.061	1.925
13) Dieldrin	7.796	8.491	395728	583812	2.061	1.919
14) Endrin	7.960	8.718	298515	424889	2.030	1.881
15) 4,4'-DDD	8.006	8.760	314622	488120	2.002	1.905
16) Endosulfa...	8.118	8.864	299106	462256	2.083	2.005
17) 4,4'-DDT	8.204	8.986	218190	341782	1.825	1.948
18) Endrin Al...	8.407	9.101	328182	477694	1.795	1.763
19) Endosulfa...	8.707	9.291	322163	498767	2.079	2.002
20) Methoxychlor	8.542	9.465	111466	178074	1.903	2.018
21) Endrin Ke...	8.901	9.689	331269	493110	1.987	1.916
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
25) Oxychlordane	7.271	0.000	4709	0	0.029	N.D. #
26) 2,4'-DDE	7.335	8.135	392052	644454	3.057	3.038
27) trans-Non...	7.527	0.000	389999	0	1.861	N.D. #
28) 2,4'-DDD	0.000	8.491	0	583812	N.D.	3.091 #
29) 2,4'-DDT	0.000	8.718	0	424889	N.D.	2.382 #
30) cis-Nonac...	8.006f	8.760	314622	488120	1.515	1.455
31) Mirex	8.657	9.689	1737	493110	0.014	2.650 #
32) Chlordane...	7.432	8.135	382271	644454	19.415	17.810
33) Chlordane...	7.527	8.241	389999	579667	15.560	19.091
34) Chlordane...	8.065	8.903	2900	40429	0.502	4.509 #
35) Chlordane...	3.445	0.000	4897	0	NoCal	N.D.
36) Toxaphene...	7.527f	8.491f	389999	583812	435.438	222.468 #
37) Toxaphene...	7.796	0.000	395728	0	245.042	N.D. #
38) Toxaphene...	8.118	8.864	299106	462256	88.822	91.205
39) Toxaphene...	8.312f	8.903	21365	40429	6.594	4.842
40) Toxaphene...	8.582	9.101	2314	477694	0.965	102.502 #
41) Toxaphene...	8.657	9.465	1737	178074	0.549	37.488 #
42) Toxaphene...	3.445	0.000	4897	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231909.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 14:08  
Operator : MJB  
Sample : 9H23034-CAL2  
Misc : A19E246, AB 2 ppb  
ALS Vial : 5 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:00:13 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231910.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 14:25  
 Operator : MJB  
 Sample : 9H23034-CAL3  
 Misc : A19E247, AB 5 ppb  
 ALS Vial : 6 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:00:25 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.396	5.990	834206	1437876	5.026	4.901
22) S DCBP (S)	9.594	10.542	701050	870921	4.969	4.845
Target Compounds						
2) a-BHC	5.937	6.597	1147932	1985438	5.006	4.839
3) g-BHC	6.220	6.915	1020724	1742677	5.059	4.885
4) b-BHC	6.300	6.980	456954	788630	5.056	4.983
5) Heptachlor	6.635	7.291	899091	1508218	4.959	4.929
6) d-BHC	6.449	7.233	1004012	1717450	5.105	4.870
7) Aldrin	6.875	7.556	1012733	1600995	5.129	4.860
8) Heptachlo...	7.335	7.994	923620	1455941	5.015	4.839
9) trans-Chl...	7.432	8.134	926577	1502119	5.011	4.794
10) cis-Chlor...	7.528	8.241	908795	1434855	4.991	4.927
11) Endosulfa...	7.624	8.290	861509	1327191	5.062	4.823
12) 4,4'-DDE	7.586	8.345	953351	1487999	5.057	4.790
13) Dieldrin	7.796	8.491	972009	1462538	5.063	4.809
14) Endrin	7.960	8.718	738953	1092877	5.026	4.839
15) 4,4'-DDD	8.007	8.759	790498	1208642	5.031	4.717
16) Endosulfa...	8.118	8.865	709544	1096359	4.941	4.754
17) 4,4'-DDT	8.205	8.986	553009	873653	4.625	5.010
18) Endrin Al...	8.407	9.101	683393	1045869	4.834	4.849
19) Endosulfa...	8.708	9.291	768798	1175908	4.961	4.721
20) Methoxychlor	8.542	9.466	270388	413802	4.616	4.904
21) Endrin Ke...	8.901	9.689	811384	1205004	4.866	4.683
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.782	0.000	4389	0	0.025	N.D. #
25) Oxychlordane	7.271	0.000	11672	0	0.071	N.D. #
26) 2,4'-DDE	7.335	8.134	923620	1502119	7.201	7.081
27) trans-Non...	7.528	0.000	908795	0	4.756	N.D. #
28) 2,4'-DDD	0.000	8.491	0	1462538	N.D.	7.744 #
29) 2,4'-DDT	7.894	8.718	3329	1092877	0.030	6.128 #
30) cis-Nonac...	8.007f	8.759	790498	1208642	3.808	3.603
31) Mirex	8.645	9.689	4292	1205004	0.034	6.476 #
32) Chlordane...	7.432	8.134	926577	1502119	47.059	41.513
33) Chlordane...	7.528	8.241	908795	1434855	36.259	47.255
34) Chlordane...	8.063	8.903	7555	42265	1.307	4.714 #
35) Chlordane...	3.446	0.000	4904	0	NoCal	N.D.
36) Toxaphene...	7.528f	8.491f	908795	1462538	1014.680	557.315 #
37) Toxaphene...	7.796	0.000	972009	0	601.886	N.D. #
38) Toxaphene...	8.118	8.865	709544	1096359	210.704	216.316
39) Toxaphene...	8.328	8.903	27348	42265	8.440	5.062 #
40) Toxaphene...	8.542f	9.101	270388	1045869	112.796	224.418 #
41) Toxaphene...	8.645	9.466	4292	413802	1.356	87.113 #
42) Toxaphene...	3.446	0.000	4904	0	NoCal	N.D.

MJB  
8/26/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231910.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 14:25  
Operator : MJB  
Sample : 9H23034-CAL3  
Misc : A19E247, AB 5 ppb  
ALS Vial : 6 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:00:25 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231911.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 14:42  
 Operator : MJB  
 Sample : 9H23034-CAL4  
 Misc : A19E249, AB 10 ppb  
 ALS Vial : 7 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:00:36 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



*MJB 8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.396	5.990	1644447	2865854	9.908	9.769
22) S DCBP (S)	9.593	10.541	1335468	1678728	9.465	9.339
Target Compounds						
2) a-BHC	5.936	6.597	2347065	4095890	10.234	9.982
3) g-BHC	6.220	6.915	2034859	3476733	10.085	9.747
4) b-BHC	6.299	6.980	910875	1580847	10.078	9.989
5) Heptachlor	6.634	7.291	1819621	3005915	10.037	9.824
6) d-BHC	6.449	7.234	2006493	3613517	10.201	10.246
7) Aldrin	6.875	7.556	2010802	3341093	10.184	10.143
8) Heptachlo...	7.335	7.994	1865428	2959301	10.128	9.837
9) trans-Chl...	7.431	8.134	1847996	3002782	9.995	9.584
10) cis-Chlor...	7.527	8.241	1843346	2859573	10.124	9.818
11) Endosulfa...	7.623	8.291	1709332	2724272	10.044	9.900
12) 4,4'-DDE	7.585	8.346	1890931	3049792	10.030	9.817
13) Dieldrin	7.795	8.491	1954890	2898866	10.183	9.531
14) Endrin	7.960	8.718	1475508	2244483	10.036	9.939
15) 4,4'-DDD	8.006	8.760	1565974	2425496	9.965	9.467
16) Endosulfa...	8.117	8.864	1448080	2243610	10.083	9.729
17) 4,4'-DDT	8.204	8.987	1146556	1841119	9.590	10.491
18) Endrin Al...	8.406	9.101	1375129	2125028	10.716	10.650
19) Endosulfa...	8.707	9.292	1553540	2424584	10.024	9.734
20) Methoxychlor	8.542	9.465	561706	883069	9.590	10.543
21) Endrin Ke...	8.900	9.689	1664380	2496985	9.981	9.704
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.781	0.000	6414	0	0.036	N.D. #
25) Oxychlorane	7.271	0.000	23125	0	0.141	N.D. #
26) 2,4'-DDE	7.335	8.134	1865428	3002782	14.544	14.155
27) trans-Non...	7.527	0.000	1843346	0	9.974	N.D. #
28) 2,4'-DDD	0.000	8.491	0	2898866	N.D.	15.349 #
29) 2,4'-DDT	7.893	8.718	6940	2244483	0.063	12.585 #
30) cis-Nonac...	8.006f	8.760	1565974	2425496	7.543	7.231
31) Mirex	8.644	9.689	9584	2496985	0.076	13.419 #
32) Chlordane...	7.431	8.134	1847996	3002782	93.856	82.985
33) Chlordane...	7.527	8.241	1843346	2859573	73.545	94.176
34) Chlordane...	8.062	8.903	15147	46214	2.620	5.154 #
35) Chlordane...	3.446	0.000	4445	0	NoCal	N.D.
36) Toxaphene...	7.527f	8.491f	1843346	2898866	2058.116	1104.642 #
37) Toxaphene...	7.795	0.000	1954890	0	1210.504	N.D. #
38) Toxaphene...	8.117	8.864	1448080	2243610	430.018	442.674
39) Toxaphene...	8.328	8.903	47046	46214	14.520	5.535 #
40) Toxaphene...	8.542f	9.101	561706	2125028	234.323	455.980 #
41) Toxaphene...	8.644	9.465	9584	883069	3.029	185.901 #
42) Toxaphene...	3.446	0.000	4445	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231911.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 14:42  
Operator : MJB  
Sample : 9H23034-CAL4  
Misc : A19E249, AB 10 ppb  
ALS Vial : 7 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:00:36 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231912.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 15:00  
 Operator : MJB  
 Sample : 9H23034-CAL5  
 Misc : A19E250, AB 25 ppb  
 ALS Vial : 8 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:01:01 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.394	5.989	4015832	7072923	24.195	24.109
22) S DCBP (S)	9.592	10.539	3342634	4163229	23.690	23.160
Target Compounds						
2) a-BHC	5.935	6.596	5553096	9910863	24.215	24.153
3) g-BHC	6.218	6.913	4875657	8508386	24.164	23.853
4) b-BHC	6.297	6.978	2060378	3677155	22.796	23.234
5) Heptachlor	6.633	7.289	4314306	7282282	23.797	23.800
6) d-BHC	6.447	7.232	4667166	8247775	23.729	23.387
7) Aldrin	6.873	7.555	4845355	7878574	24.540	23.919
8) Heptachlo...	7.332	7.992	4344286	7064729	23.587	23.483
9) trans-Chl...	7.429	8.131	4401456	7157480	23.806	22.844
10) cis-Chlor...	7.525	8.239	4244413	6935857	23.312	23.814
11) Endosulfa...	7.621	8.288	4111285	6571512	24.158	23.881
12) 4,4'-DDE	7.583	8.343	4571066	7501047	24.246	24.144
13) Dieldrin	7.792	8.489	4582306	7333890	23.869	24.113
14) Endrin	7.957	8.716	3508904	5325883	23.866	23.584
15) 4,4'-DDD	8.004	8.758	3727035	6146469	23.718	23.990
16) Endosulfa...	8.115	8.862	3371864	5447602	23.479	23.623
17) 4,4'-DDT	8.202	8.984	2924467	4480388	24.460	24.907
18) Endrin Al...	8.404	9.099	3119767	4848504	25.346	24.953
19) Endosulfa...	8.705	9.289	3645411	5978906	23.522	24.003
20) Methoxychlor	8.540	9.463	1390283	2166659	23.735	25.322
21) Endrin Ke...	8.899	9.688	4008958	5893691	24.041	22.904
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.779	0.000	7817	0	0.044	N.D. #
25) Oxychlordane	7.269	0.000	51278	0	0.312	N.D. #
26) 2,4'-DDE	7.332	8.131	4344286	7157480	33.871	33.740
27) trans-Non...	7.525	8.192	4244413	24831	23.380	0.082 #
28) 2,4'-DDD	0.000	8.489	0	7333890	N.D.	38.832 #
29) 2,4'-DDT	7.891	8.716	15573	5325883	0.142	29.864 #
30) cis-Nonac...	8.004	8.758	3727035	6146469	17.952	18.323
31) Mirex	8.651	9.688	18145	5893691	0.145	31.674 #
32) Chlordane...	7.429	8.131	4401456	7157480	223.542	197.805
33) Chlordane...	7.525	8.239	4244413	6935857	169.341	228.423
34) Chlordane...	8.059	8.901	33094	57884	5.724	6.456
35) Chlordane...	3.446	0.000	4689	0	NoCal	N.D.
36) Toxaphene...	7.525f	8.489f	4244413	7333890	4738.933	2794.653 #
37) Toxaphene...	7.792	0.000	4582306	0	2837.449	N.D. #
38) Toxaphene...	8.115	8.862	3371864	5447602	1001.299	1074.835
39) Toxaphene...	8.326f	8.901	104762	57884	32.332	6.932 #
40) Toxaphene...	8.540f	9.099	1390283	4848504	579.975	1040.371 #
41) Toxaphene...	8.651	9.463	18145	2166659	5.734	456.119 #
42) Toxaphene...	3.446	0.000	4689	0	NoCal	N.D.

NB  
(2611)

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231912.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 15:00  
Operator : MJB  
Sample : 9H23034-CAL5  
Misc : A19E250, AB 25 ppb  
ALS Vial : 8 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:01:01 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231913.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 15:17  
 Operator : MJB  
 Sample : 9H23034-CAL6  
 Misc : A19H383, AB 50 ppb  
 ALS Vial : 9 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:01:12 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB 8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.394	5.989	8071481	14196745	48.631	48.392
22) S DCBP (S)	9.592	10.541	6678990	8730692	47.336	48.568
Target Compounds						
2) a-BHC	5.935	6.596	11369592	20265817	49.578	49.388
3) g-BHC	6.218	6.914	9785999	17381069	48.499	48.727
4) b-BHC	6.296	6.978	4100858	7516011	45.372	47.490
5) Heptachlor	6.632	7.290	8735158	14595143	48.182	47.700
6) d-BHC	6.447	7.232	9610742	17311258	48.862	49.087
7) Aldrin	6.873	7.555	9327672	16264416	47.242	49.377
8) Heptachlo...	7.332	7.992	8869300	14837794	48.156	49.320
9) trans-Chl...	7.428	8.131	8959305	14678719	48.457	46.848
10) cis-Chlor...	7.524	8.238	8622674	14002116	47.359	48.076
11) Endosulfa...	7.621	8.289	7984410	13712329	46.917	49.831
12) 4,4'-DDE	7.583	8.344	9177389	15554706	48.679	50.067
13) Dieldrin	7.792	8.489	9386664	15434113	48.894	50.745
14) Endrin	7.957	8.716	6979572	11015379	47.471	48.778
15) 4,4'-DDD	8.004	8.758	7726197	13159451	49.167	51.361
16) Endosulfa...	8.114	8.863	6840920	11534525	47.635	50.018
17) 4,4'-DDT	8.202	8.985	6205369	9285492	51.902	49.430
18) Endrin Al...	8.404	9.099	6224451	10209034	50.697	51.836
19) Endosulfa...	8.705	9.289	7420576	12149289	47.882	48.775
20) Methoxychlor	8.540	9.464	2860683	4346199	48.839	48.597
21) Endrin Ke...	8.899	9.687	8190707	12954568	49.117	50.345
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.777	6.487f	17034	6623	0.097	0.021 #
25) Oxychlordane	7.268	7.916	93115	13858	0.566	0.051 #
26) 2,4'-DDE	7.332	8.131	8869300	14678719	69.150	69.194
27) trans-Non...	7.524	8.193	8622674	44541	47.838	0.148 #
28) 2,4'-DDD	7.705	8.489	15706	15434113	0.138	81.721 #
29) 2,4'-DDT	7.890	8.716	32276	11015379	0.294	61.766 #
30) cis-Nonac...	8.004	8.758	7726197	13159451	37.214	39.229
31) Mirex	8.653	9.687	33100	12954568	0.264	69.621 #
32) Chlordane...	7.428	8.131	8959305	14678719	455.027	405.662
33) Chlordane...	7.524	8.238	8622674	14002116	344.022	461.141
34) Chlordane...	8.059	8.901	56505	76664	9.774	8.551
35) Chlordane...	3.445	0.000	3954	0	NoCal	N.D.
36) Toxaphene...	7.524f	8.489f	8622674	15434113	9627.309	5881.324
37) Toxaphene...	7.792	8.823	9386664	45987	5812.397	13.973 #
38) Toxaphene...	8.114	8.863	6840920	11534525	2031.460	2275.810
39) Toxaphene...	8.325f	8.901	190344	76664	58.746	9.182 #
40) Toxaphene...	8.540f	9.099	2860683	10209034	1193.372	2190.611 #
41) Toxaphene...	8.653	9.464	33100	4346199	10.460	914.950 #
42) Toxaphene...	3.445	0.000	3954	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231913.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 15:17  
Operator : MJB  
Sample : 9H23034-CAL6  
Misc : A19H383, AB 50 ppb  
ALS Vial : 9 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:01:12 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231914.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 15:34  
 Operator : MJB  
 Sample : 9H23034-CAL7  
 Misc : A19H382, AB 100 ppb  
 ALS Vial : 10 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:01:22 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.395	5.989	15850922	29256334	95.502	99.726
22) S DCBP (S)	9.592	10.540	13405396	17784069	95.007	98.931
Target Compounds						
2) a-BHC	5.935	6.596	22363584	41699210	97.517	101.621
3) g-BHC	6.218	6.914	19595093	36788994	97.113	103.136
4) b-BHC	6.296	6.977	8355416	14625175	92.444	92.409
5) Heptachlor	6.632	7.289	17551528	30277818	96.811	98.955
6) d-BHC	6.446	7.232	19475580	35176633	99.016	99.745
7) Aldrin	6.872	7.555	19108074	33906422	96.776	102.936
8) Heptachlo...	7.331	7.991	17318444	30045511	94.031	99.869
9) trans-Chl...	7.427	8.131	17732791	30742272	95.909	98.116
10) cis-Chlor...	7.523	8.238	16742584	29042863	91.956	99.719
11) Endosulfa...	7.619	8.288	16089996	27212707	94.547	98.892
12) 4,4'-DDE	7.582	8.344	18052552	32499603	95.754	104.609
13) Dieldrin	7.791	8.488	18324422	31001958	95.450	101.930
14) Endrin	7.957	8.715	13812708	23102413	93.947	102.301
15) 4,4'-DDD	8.003	8.758	15437146	26297484	98.238	102.639
16) Endosulfa...	8.113	8.861	13543500	23016371	94.307	99.808
17) 4,4'-DDT	8.201	8.984	12176961	19789501	101.848	97.215
18) Endrin Al...	8.403	9.098	12363806	20502737	98.526	99.562
19) Endosulfa...	8.704	9.289	14366789	24477320	92.702	98.268
20) Methoxychlor	8.539	9.463	5877329	9444987	100.340	96.538
21) Endrin Ke...	8.898	9.687	16251943	26636559	97.458	103.517
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.777	0.000	29252	0	0.166	N.D. #
25) Oxychlorane	7.267	7.915	165864	25145	1.008	0.092 #
26) 2,4'-DDE	7.331	8.131	17318444	30742272	135.025	144.916
27) trans-Non...	7.523	8.192	16742584	77338	93.233	0.256 #
28) 2,4'-DDD	7.704	8.488	32176	31001958	0.282	164.150 #
29) 2,4'-DDT	7.889	8.715	66298	23102413	0.604	129.542 #
30) cis-Nonac...	8.003	8.758	15437146	26297484	74.355	78.395
31) Mirex	8.651	9.687	63592	26636559	0.507	143.151 #
32) Chlordane...	7.427	8.131	17732791	30742272	900.616	849.596
33) Chlordane...	7.523	8.238	16742584	29042863	667.985	956.488 #
34) Chlordane...	8.059	8.899	102306	115089	17.697	12.836
35) Chlordane...	3.447	0.000	5362	0	NoCal	N.D.
36) Toxaphene...	7.523f	8.488f	16742584	31001958	18693.275	11813.609
37) Toxaphene...	7.791	0.000	18324422	0	11346.823	N.D. #
38) Toxaphene...	8.113	8.861	13543500	23016371	4021.839	4541.226
39) Toxaphene...	8.324f	8.899	362066	115089	111.744	13.783 #
40) Toxaphene...	8.598f	9.098	51910	20502737	21.655	4399.391 #
41) Toxaphene...	8.651	9.463	63592	9444987	20.095	1988.334 #
42) Toxaphene...	3.447	0.000	5362	0	NoCal	N.D.

MJB  
6/26/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231914.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 15:34  
Operator : MJB  
Sample : 9H23034-CAL7  
Misc : A19H382, AB 100 ppb  
ALS Vial : 10 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:01:22 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231915.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 15:52  
 Operator : MJB  
 Sample : 9H23034-CAL8  
 Misc : A19E244, AB 200 ppb  
 ALS Vial : 11 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:01:32 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*10/6/2019*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.394	5.990	32842535	62584449	197.876	213.332
22) S DCBP (S)	9.591	10.539	26975231	38097779	191.180	211.933
Target Compounds						
2) a-BHC	5.935	6.597	47202252	94376748	205.828	229.997
3) g-BHC	6.218	6.914	41889726	80765680	207.604	226.422
4) b-BHC	6.294	6.977	18238696	32553433	201.792	205.688
5) Heptachlor	6.630	7.289	37785699	71283176	208.419	232.969
6) d-BHC	6.445	7.232	41016592	80979751	208.534	229.622
7) Aldrin	6.870	7.554	39838403	73228186	201.769	222.313
8) Heptachlo...	7.330	7.991	36258170	65330070	196.864	217.153
9) trans-Chl...	7.425	8.130	37621413	66447972	203.478	212.073
10) cis-Chlor...	7.521	8.238	35207945	63977063	193.375	219.666
11) Endosulfa...	7.618	8.288	33852593	61043507	198.922	221.834
12) 4,4'-DDE	7.581	8.344	38763081	69842351	205.607	224.807
13) Dieldrin	7.791	8.489	39217772	70031781	204.281	230.254
14) Endrin	7.955	8.715	31426311	52779585	213.745	233.717
15) 4,4'-DDD	8.002	8.758	32436804	59560270	206.419	232.463
16) Endosulfa...	8.112	8.862	29471042	51834888	205.214	224.777
17) 4,4'-DDT	8.200	8.984	29075222	48203441	243.185	202.337
18) Endrin Al...	8.402	9.098	26627672	45084544	200.132	198.781
19) Endosulfa...	8.704	9.289	31126520	54592794	200.845	219.171
20) Methoxychlor	8.537	9.463	14271143	23714100	243.642	203.084
21) Endrin Ke...	8.898	9.688	35094718	60861376	210.452	236.524
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.776	0.000	55469	0	0.315	N.D. #
25) Oxychlordane	7.265	7.915	336226	30124	2.043	0.110 #
26) 2,4'-DDE	7.330	8.130	36258170	66447972	282.690	313.230
27) trans-Non...	7.521	8.191	35207945	140624	196.641	0.466 #
28) 2,4'-DDD	7.703	8.489	57049	70031781	0.500	370.806 #
29) 2,4'-DDT	7.886	8.715	129876	52779585	1.184	295.950 #
30) cis-Nonac...	8.002	8.758	32436804	59560270	156.235	177.554
31) Mirex	8.651	9.688	103310	60861376	0.824	327.083 #
32) Chlordane...	7.425	8.130	37621413	66447972	1910.724	1836.362
33) Chlordane...	7.521	8.238	35207945	63977063	1404.705	2106.999 #
34) Chlordane...	8.058	8.862f	183720	51834888	31.779	5781.350 #
35) Chlordane...	3.445	0.000	4872	0	NoCal	N.D.
36) Toxaphene...	7.521	8.489f	35207945	70031781	39310.050	26686.316
37) Toxaphene...	7.791	0.000	39217772	0	24284.375	N.D. #
38) Toxaphene...	8.112	8.862	29471042	51834888	8751.637	10227.240
39) Toxaphene...	8.322f	8.943f	634260	207653	195.750	24.869 #
40) Toxaphene...	8.537f	9.098	14271143	45084544	5953.399	9674.052 #
41) Toxaphene...	8.651	9.463	103310	23714100	32.646	4992.230 #
42) Toxaphene...	3.445	0.000	4872	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231915.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 15:52  
Operator : MJB  
Sample : 9H23034-CAL8  
Misc : A19E244, AB 200 ppb  
ALS Vial : 11 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:01:32 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231918.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 16:44  
 Operator : MJB  
 Sample : 9H23034-CAL9  
 Misc : A19E272, 9-42 1 ppb  
 ALS Vial : 13 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:02:15 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



MJB 8/26/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.984	0	6576	N.D.	0.022 #
22) S DCBP (S)	9.593	10.540	2255	5805	0.016	0.032 #
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.249f	0.000	4648	0	0.023	N.D. #
4) b-BHC	0.000	7.002f	0	7162	N.D.	0.045 #
5) Heptachlor	6.601f	0.000	3572	0	0.020	N.D. #
6) d-BHC	6.449	7.232	5321	8483	0.027	0.024
7) Aldrin	0.000	7.577f	0	8990	N.D.	0.027 #
8) Heptachlo...	7.335	0.000	137947	0	0.749	N.D. #
9) trans-Chl...	7.420	8.123	5532	219164	0.030	0.699 #
10) cis-Chlor...	7.518	0.000	236836	0	1.301	N.D. #
11) Endosulfa...	7.582f	0.000	5522	0	0.032	N.D. #
12) 4,4'-DDE	7.582	0.000	5522	0	0.029	N.D. #
13) Dieldrin	7.755f	8.495	4087	192040	0.021	0.631 #
14) Endrin	7.987f	8.719	219220	173338	1.491	0.768 #
15) 4,4'-DDD	7.987	8.759	219220	332745	1.395	1.299 #
16) Endosulfa...	8.116	8.903f	2586	40443	0.018	0.175 #
17) 4,4'-DDT	8.202	0.000	1027	0	0.009	N.D. #
18) Endrin Al...	8.404	9.099	13122	17799	BelowCal	BelowCal
19) Endosulfa...	8.706	9.290	8041	12118	0.052	0.049
20) Methoxychlor	8.548	0.000	665	0	0.011	N.D. #
21) Endrin Ke...	8.900	9.680	3962	209783	0.024	0.815 #
23) Hexachlor...	3.198	3.687	198207	383198	1.085	1.019
24) Hexachlor...	5.775	6.453	194679	328025	1.104	1.044
25) Oxychlorane	7.263	7.922	176844	279143	1.075	1.019
26) 2,4'-DDE	7.335	8.123	137947	219164	1.076	1.033
27) trans-Non...	7.518	8.195	236836	306202	1.006	1.015
28) 2,4'-DDD	7.707	8.495	120240	192040	1.054	1.017
29) 2,4'-DDT	7.890	8.719	107110	173338	0.977	0.972
30) cis-Nonac...	7.987	8.759	219220	332745	1.056	0.992
31) Mirex	8.655	9.680	147356	209783	1.175	1.127
32) Chlordane...	7.420	8.123	5532	219164	0.281	6.057 #
33) Chlordane...	7.518	0.000	236836	0	9.449	N.D. #
34) Chlordane...	0.000	8.903	0	40443	N.D.	4.511 #
35) Chlordane...	3.444	0.000	4642	0	NoCal	N.D.
36) Toxaphene...	7.518	8.495f	236836	192040	264.430	73.179 #
37) Toxaphene...	7.755f	0.000	4087	0	2.531	N.D. #
38) Toxaphene...	8.116	0.000	2586	0	0.768	N.D. #
39) Toxaphene...	8.312f	8.903	22217	40443	6.857	4.844
40) Toxaphene...	8.548f	9.099	665	17799	0.277	3.819 #
41) Toxaphene...	8.655	0.000	147356	0	46.564	N.D. #
42) Toxaphene...	3.444	0.000	4642	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231918.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 16:44  
Operator : MJB  
Sample : 9H23034-CAL9  
Misc : A19E272, 9-42 1 ppb  
ALS Vial : 13 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:02:15 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231919.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 17:01  
 Operator : MJB  
 Sample : 9H23034-CALA  
 Misc : A19E273, 9-42 2 ppb  
 ALS Vial : 14 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:02:30 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.394	5.986	6323	13044	0.038	0.044
22) S DCBP (S)	9.592	10.539	6116	7474	0.043	0.042
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.248f	0.000	3811	0	0.019	N.D. #
4) b-BHC	0.000	0.000	0	0	N.D.	N.D.
5) Heptachlor	6.631	0.000	3915	0	0.022	N.D. #
6) d-BHC	6.449	7.231	6839	9605	0.035	0.027
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	7.334	0.000	265212	0	1.440	N.D. #
9) trans-Chl...	7.429	8.123	4955	411812	0.027	1.314 #
10) cis-Chlor...	7.518	0.000	415126	0	2.280	N.D. #
11) Endosulfa...	7.582f	0.000	3811	0	0.022	N.D. #
12) 4,4'-DDE	7.582	0.000	3811	0	0.020	N.D. #
13) Dieldrin	7.754f	8.495	8020	373596	0.042	1.228 #
14) Endrin	7.986f	8.718	423442	332170	2.880	1.471 #
15) 4,4'-DDD	7.986	8.758	423442	624783	2.695	2.439
16) Endosulfa...	8.116	8.862	3733	5461	0.026	0.024
17) 4,4'-DDT	8.200	0.000	1311	0	0.011	N.D. #
18) Endrin Al...	8.405	9.099	11160	14424	BelowCal	BelowCal
19) Endosulfa...	8.705	9.289	10006	14488	0.065	0.058
20) Methoxychlor	0.000	0.000	0	0	N.D.	N.D.
21) Endrin Ke...	8.899	9.680	5404	388199	0.032	1.509 #
23) Hexachlor...	3.198	3.687	375794	754548	2.056	2.007
24) Hexachlor...	5.775	6.453	362082	632830	2.054	2.015
25) Oxychlordane	7.262	7.921	339370	541023	2.063	1.975
26) 2,4'-DDE	7.334	8.123	265212	411812	2.068	1.941
27) trans-Non...	7.518	8.194	415126	587765	2.001	1.949
28) 2,4'-DDD	7.707	8.495	233089	373596	2.042	1.978
29) 2,4'-DDT	7.889	8.718	204209	332170	1.862	1.863
30) cis-Nonac...	7.986	8.758	423442	624783	2.040	1.863
31) Mirex	8.655	9.680	266770	388199	2.128	2.086
32) Chlordane...	7.429	8.123	4955	411812	0.252	11.381 #
33) Chlordane...	7.518	0.000	415126	0	16.562	N.D. #
34) Chlordane...	0.000	8.903	0	41985	N.D.	4.683 #
35) Chlordane...	3.444	0.000	5015	0	NoCal	N.D.
36) Toxaphene...	7.518	8.495f	415126	373596	463.493	142.363 #
37) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
38) Toxaphene...	8.116	8.862	3733	5461	1.108	1.077
39) Toxaphene...	8.312f	8.903	22876	41985	7.060	5.028
40) Toxaphene...	0.000	9.099	0	14424	N.D.	3.095 #
41) Toxaphene...	8.655	0.000	266770	0	84.299	N.D. #
42) Toxaphene...	3.444	0.000	5015	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231919.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 17:01  
Operator : MJB  
Sample : 9H23034-CALA  
Misc : A19E273, 9-42 2 ppb  
ALS Vial : 14 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:02:30 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231920.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 17:18  
 Operator : MJB  
 Sample : 9H23034-CALB  
 Misc : A19E274, 9-42 5 ppb  
 ALS Vial : 15 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:02:42 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



MJB  
8/26/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.368f	5.982	4403	6341	0.027	0.022
22) S DCBP (S)	9.592	10.539	7940	5412	0.056	0.030 #
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.247f	0.000	5412	0	0.027	N.D. #
4) b-BHC	0.000	0.000	0	0	N.D.	N.D.
5) Heptachlor	6.631	7.289	4685	5276	0.026	0.017
6) d-BHC	6.449	7.232	7597	11663	0.039	0.033
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	7.334	7.991	633168	6408	3.438	0.021 #
9) trans-Chl...	7.429	8.123	9886	1029687	0.053	3.286 #
10) cis-Chlor...	7.518	8.236	933222	8550	5.126	0.029 #
11) Endosulfa...	0.000	0.000	0	0	N.D.	N.D.
12) 4,4'-DDE	0.000	0.000	0	0	N.D.	N.D.
13) Dieldrin	7.799	8.495	5522	898697	0.029	2.955 #
14) Endrin	7.986f	8.719	1025899	873074	6.978	3.866 #
15) 4,4'-DDD	7.986	8.759	1025899	1587243	6.529	6.195
16) Endosulfa...	8.116	8.862	3810	5519	0.027	0.024
17) 4,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
18) Endrin Al...	8.404	9.098	10319	12495	BelowCal	BelowCal
19) Endosulfa...	8.705	9.289	10733	14179	0.069	0.057
20) Methoxychlor	8.550	0.000	617	0	0.011	N.D. #
21) Endrin Ke...	8.899	9.679	5632	895523	0.034	3.480 #
23) Hexachlor...	3.198	3.687	959211	1877484	5.249	4.994
24) Hexachlor...	5.775	6.453	853793	1485583	4.843	4.730
25) Oxychlordane	7.262	7.921	819748	1325543	4.982	4.839
26) 2,4'-DDE	7.334	8.123	633168	1029687	4.937	4.854
27) trans-Non...	7.518	8.194	933222	1467723	4.893	4.866
28) 2,4'-DDD	7.705	8.495	560942	898697	4.915	4.758
29) 2,4'-DDT	7.889	8.719	536967	873074	4.895	4.896
30) cis-Nonac...	7.986	8.759	1025899	1587243	4.941	4.732
31) Mirex	8.654	9.679	628618	895523	5.014	4.813
32) Chlordane...	7.429	8.123	9886	1029687	0.502	28.457 #
33) Chlordane...	7.518	8.236	933222	8550	37.233	0.282 #
34) Chlordane...	0.000	8.903	0	41570	N.D.	4.636 #
35) Chlordane...	3.443	3.434	5083	3848	NoCal	NoCal
36) Toxaphene...	7.518	8.495f	933222	898697	1041.953	342.457 #
37) Toxaphene...	7.799	0.000	5522	0	3.419	N.D. #
38) Toxaphene...	8.116	8.862	3810	5519	1.131	1.089
39) Toxaphene...	8.312f	8.903	22738	41570	7.017	4.979
40) Toxaphene...	8.550f	9.098	617	12495	0.257	2.681 #
41) Toxaphene...	8.654	0.000	628618	0	198.642	N.D. #
42) Toxaphene...	3.443	3.434	5083	3848	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231920.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 17:18  
Operator : MJB  
Sample : 9H23034-CALB  
Misc : A19E274, 9-42 5 ppb  
ALS Vial : 15 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:02:42 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231921.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 17:35  
 Operator : MJB  
 Sample : 9H23034-CALC  
 Misc : A19E275, 9-42 10 ppb  
 ALS Vial : 16 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:02:55 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB 8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.367f	5.983	5244	8048	0.032	0.027
22) S DCBP (S)	9.591	10.539	8426	10511	0.060	0.058
Target Compounds						
2) a-BHC	5.934	6.594	5268	9085	0.023	0.022
3) g-BHC	6.219	6.912	5161	7308	0.026	0.020
4) b-BHC	6.300	6.978	6085	7741	0.067	0.049
5) Heptachlor	6.631	7.288	8267	12275	0.046	0.040
6) d-BHC	6.449	7.232	14325	24245	0.073	0.069
7) Aldrin	6.872	7.553	3901	5863	0.020	0.018
8) Heptachlo...	7.333	7.990	1245265	15714	6.761	0.052 #
9) trans-Chl...	7.428	8.122	20597	2018331	0.111	6.442 #
10) cis-Chlor...	7.516	8.236	1817552	21137	9.983	0.073 #
11) Endosulfa...	7.620	8.289	8045	10794	0.047	0.039
12) 4,4'-DDE	7.582	8.342	11334	7910	0.060	0.025 #
13) Dieldrin	7.797	8.495	12142	1778790	0.063	5.848 #
14) Endrin	7.986f	8.719	2032010	1702568	13.821	7.539 #
15) 4,4'-DDD	7.986	8.759	2032010	3148054	12.931	12.287
16) Endosulfa...	8.115	8.863	8267	13466	0.058	0.058
17) 4,4'-DDT	8.202	0.000	2833	0	0.024	N.D. #
18) Endrin Al...	8.404	9.098	18899	26666	BelowCal	BelowCal
19) Endosulfa...	8.705	9.289	20232	26713	0.131	0.107
20) Methoxychlor	8.543	0.000	1294	0	0.022	N.D. #
21) Endrin Ke...	8.899	9.679	11108	1722960	0.067	6.696 #
23) Hexachlor...	3.198	3.687	1838187	3701532	10.059	9.846
24) Hexachlor...	5.774	6.453	1711884	2936294	9.710	9.349
25) Oxychlorane	7.261	7.921	1591613	2538903	9.673	9.269
26) 2,4'-DDE	7.333	8.122	1245265	2018331	9.709	9.514
27) trans-Non...	7.516	8.194	1817552	2844404	9.830	9.430
28) 2,4'-DDD	7.705	8.495	1103587	1778790	9.670	9.418
29) 2,4'-DDT	7.888	8.719	1051565	1702568	9.587	9.547
30) cis-Nonac...	7.986	8.759	2032010	3148054	9.787	9.385
31) Mirex	8.654	9.679	1196365	1722960	9.543	9.260
32) Chlordane...	7.428	8.122	20597	2018331	1.046	55.779 #
33) Chlordane...	7.516	8.236	1817552	21137	72.516	0.696 #
34) Chlordane...	0.000	8.903	0	42511	N.D.	4.741 #
35) Chlordane...	3.445	3.433	6229	7261	NoCal	NoCal
36) Toxaphene...	7.516	8.495f	1817552	1778790	2029.316	677.826 #
37) Toxaphene...	7.797	0.000	12142	0	7.518	N.D. #
38) Toxaphene...	8.115	8.863	8267	13466	2.455	2.657
39) Toxaphene...	8.312f	8.903	23581	42511	7.278	5.091
40) Toxaphene...	8.582	9.098	560	26666	0.234	5.722 #
41) Toxaphene...	8.654	0.000	1196365	0	378.048	N.D. #
42) Toxaphene...	3.445	3.433	6229	7261	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231921.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 17:35  
Operator : MJB  
Sample : 9H23034-CALC  
Misc : A19E275, 9-42 10 ppb  
ALS Vial : 16 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:02:55 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231922.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 17:53  
 Operator : MJB  
 Sample : 9H23034-CALD  
 Misc : A19E276, 9-42 25 ppb  
 ALS Vial : 17 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:03:06 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.367f	5.981	10828	6833	0.065	0.023 #
22) S DCBP (S)	9.592	10.539	20297	20262	0.144	0.113
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.248f	0.000	5786	0	0.029	N.D. #
4) b-BHC	0.000	0.000	0	0	N.D.	N.D.
5) Heptachlor	6.632	7.288	9958	12977	0.055	0.042
6) d-BHC	6.450	7.231	5090	7876	0.026	0.022
7) Aldrin	0.000	0.000	0	0	N.D.	N.D.
8) Heptachlo...	7.333	7.989	3059421	19960	16.611	0.066 #
9) trans-Chl...	7.428	8.122	36083	4999232	0.195	15.955 #
10) cis-Chlor...	7.516	8.235	4391046	27018	24.117	0.093 #
11) Endosulfa...	7.604	8.299	11350	9999	0.067	0.036 #
12) 4,4'-DDE	7.604f	0.000	11350	0	0.060	N.D. #
13) Dieldrin	7.800	8.495	19961	4389185	0.104	14.431 #
14) Endrin	7.986f	8.719	4993110	4405554	33.960	19.509 #
15) 4,4'-DDD	7.986	8.759	4993110	8219393	31.775	32.080
16) Endosulfa...	0.000	8.862	0	7977	N.D.	0.035 #
17) 4,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
18) Endrin Al...	8.404	9.098	7779	9076	BelowCal	BelowCal
19) Endosulfa...	0.000	9.289	0	11382	N.D.	0.046 #
20) Methoxychlor	0.000	0.000	0	0	N.D.	N.D.
21) Endrin Ke...	8.899	9.679	4709	4138115	0.028	16.082 #
23) Hexachlor...	3.198	3.687	4363988	8892238	23.881	23.654
24) Hexachlor...	5.774	6.453	4184551	7416324	23.736	23.612
25) Oxychlordane	7.261	7.920	3881255	6202791	23.589	22.646
26) 2,4'-DDE	7.333	8.122	3059421	4999232	23.853	23.566
27) trans-Non...	7.516	8.194	4391046	7092288	24.199	23.513
28) 2,4'-DDD	7.705	8.495	2745178	4389185	24.054	23.240
29) 2,4'-DDT	7.888	8.719	2728794	4405554	24.878	24.703
30) cis-Nonac...	7.986	8.759	4993110	8219393	24.050	24.503
31) Mirex	8.654	9.679	2910818	4138115	23.218	22.239
32) Chlordane...	7.428	8.122	36083	4999232	1.833	138.159 #
33) Chlordane...	7.516	8.235	4391046	27018	175.191	0.890 #
34) Chlordane...	0.000	8.903	0	43328	N.D.	4.833 #
35) Chlordane...	3.444	3.433	9286	16581	NoCal	NoCal
36) Toxaphene...	7.516	8.495f	4391046	4389185	4902.650	1672.543 #
37) Toxaphene...	7.800	0.000	19961	0	12.360	N.D. #
38) Toxaphene...	0.000	8.862	0	7977	N.D.	1.574 #
39) Toxaphene...	8.313f	8.903	24731	43328	7.633	5.189
40) Toxaphene...	8.607f	9.098	797	9076	0.332	1.947 #
41) Toxaphene...	8.654	0.000	2910818	0	919.811	N.D. #
42) Toxaphene...	3.444	3.433	9286	16581	NoCal	NoCal



MJB 8/26/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231922.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 17:53  
Operator : MJB  
Sample : 9H23034-CALD  
Misc : A19E276, 9-42 25 ppb  
ALS Vial : 17 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:03:06 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231923.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 18:10  
 Operator : MJB  
 Sample : 9H23034-CALE  
 Misc : A19E154, 9-42 50 ppb  
 ALS Vial : 18 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:03:18 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.367f	5.981	19019	8441	0.115	0.029 #
22) S DCBP (S)	9.591	10.538	35203	39503	0.249	0.220
Target Compounds						
2) a-BHC	5.949	0.000	5252	0	0.023	N.D. #
3) g-BHC	6.196f	6.951f	4084	3735	0.020	0.010 #
4) b-BHC	0.000	6.951f	0	3735	N.D.	0.024 #
5) Heptachlor	6.632	7.289	17900	26152	0.099	0.085
6) d-BHC	6.450	7.232	4458	7173	0.023	0.020
7) Aldrin	0.000	7.520f	0	4998	N.D.	0.015 #
8) Heptachlo...	7.333	7.989	6510588	39220	35.349	0.130 #
9) trans-Chl...	7.428	8.122	71663	11006400	0.388	35.128 #
10) cis-Chlor...	7.516	8.236	9581794	53379	52.627	0.183 #
11) Endosulfa...	7.604	8.299	22096	24918	0.130	0.091
12) 4,4'-DDE	7.604f	8.314f	22096	29928	0.117	0.096
13) Dieldrin	7.798	8.495	33203	9924934	0.173	32.632 #
14) Endrin	7.985f	8.718	10616019	8810591	72.204	39.015 #
15) 4,4'-DDD	7.985	8.758	10616019	17721229	67.557	69.166
16) Endosulfa...	0.000	8.862	0	12791	N.D.	0.055 #
17) 4,4'-DDT	0.000	0.000	0	0	N.D.	N.D.
18) Endrin Al...	8.409	9.099	5626	7468	BelowCal	BelowCal
19) Endosulfa...	0.000	9.289	0	9409	N.D.	0.038 #
20) Methoxychlor	0.000	0.000	0	0	N.D.	N.D.
21) Endrin Ke...	8.898	9.679	5162	9100959	0.031	35.369 #
23) Hexachlor...	3.198	3.688	8761747	18635615	47.947	49.572 #
24) Hexachlor...	5.774	6.454	8911624	16094159	50.550	51.241
25) Oxychlorane	7.261	7.920	8382873	14172543	50.948	51.743
26) 2,4'-DDE	7.333	8.122	6510588	11006400	50.760	51.883
27) trans-Non...	7.516	8.194	9581794	15807712	53.197	52.407
28) 2,4'-DDD	7.705	8.495	5920095	9924934	51.874	52.551
29) 2,4'-DDT	7.888	8.718	5687323	8810591	51.850	49.404
30) cis-Nonac...	7.985	8.758	10616019	17721229	51.133	52.828
31) Mirex	8.652	9.679	6218341	9100959	49.601	48.911
32) Chlordane...	7.428	8.122	71663	11006400	3.640	304.174 #
33) Chlordane...	7.516	8.236	9581794	53379	382.289	1.758 #
34) Chlordane...	0.000	8.903	0	43859	N.D.	4.892 #
35) Chlordane...	3.445	3.433	16729	32384	NoCal	NoCal
36) Toxaphene...	7.516	8.495f	9581794	9924934	10698.176	3781.996 #
37) Toxaphene...	7.798	0.000	33203	0	20.560	N.D. #
38) Toxaphene...	0.000	8.862	0	12791	N.D.	2.524 #
39) Toxaphene...	8.314f	8.903	24262	43859	7.488	5.253
40) Toxaphene...	8.605f	9.099	1073	7468	0.448	1.603 #
41) Toxaphene...	8.652	0.000	6218341	0	1964.980	N.D. #
42) Toxaphene...	3.445	3.433	16729	32384	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231923.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 18:10  
Operator : MJB  
Sample : 9H23034-CALE  
Misc : A19E154, 9-42 50 ppb  
ALS Vial : 18 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:03:18 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231924.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 18:27  
 Operator : MJB  
 Sample : 9H23034-CALF  
 Misc : A19E155, 9-42 100 ppb  
 ALS Vial : 19 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:03:29 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



MJB  
8/26/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.368f	5.981	33988	9402	0.205	0.032 #
22) S DCBP (S)	9.592	10.540	62236	73549	0.441	0.409
Target Compounds						
2) a-BHC	5.950	0.000	8055	0	0.035	N.D. #
3) g-BHC	6.198	6.952f	8435	9250	0.042	0.026
4) b-BHC	6.301	6.979	5312	6852	0.059	0.043
5) Heptachlor	6.634	7.290	29320	42832	0.162	0.140
6) d-BHC	6.451	7.234	4881	8440	0.025	0.024
7) Aldrin	0.000	7.521f	0	8525	N.D.	0.026 #
8) Heptachlo...	7.334	7.990	12769067	71027	69.330	0.236 #
9) trans-Chl...	7.428	8.123	131019	22164400	0.709	70.739 #
10) cis-Chlor...	7.516	8.237	18351251	88947	100.792	0.305 #
11) Endosulfa...	7.604	8.299	36455	42308	0.214	0.154
12) 4,4'-DDE	7.604f	8.315f	36455	43813	0.193	0.141
13) Dieldrin	7.798	8.496	56666	20118925	0.295	66.148 #
14) Endrin	7.986f	8.721	20932641	18998968	142.373	84.131 #
15) 4,4'-DDD	7.986	8.760	20932641	36072644	133.210	140.791
16) Endosulfa...	8.115	8.863	14279	23343	0.099	0.101
17) 4,4'-DDT	8.202	8.985	6473	9074	0.054	0.015 #
18) Endrin Al...	8.415	9.101	7567	8073	BelowCal	BelowCal
19) Endosulfa...	0.000	9.290	0	9186	N.D.	0.037 #
20) Methoxychlor	0.000	0.000	0	0	N.D.	N.D.
21) Endrin Ke...	8.898	9.680	6812	19363200	0.041	75.251 #
23) Hexachlor...	3.199	3.690	17952134	39298885	98.239	104.537
24) Hexachlor...	5.776	6.455	17670025	32766708	100.231	104.324
25) Oxychlorane	7.261	7.922	16359215	29732149	99.425	108.550
26) 2,4'-DDE	7.334	8.123	12769067	22164400	99.555	104.481
27) trans-Non...	7.516	8.195	18351251	31975271	102.232	106.006
28) 2,4'-DDD	7.705	8.496	11587554	20118925	101.534	106.526
29) 2,4'-DDT	7.888	8.721	11771354	18998968	107.317	106.533
30) cis-Nonac...	7.986	8.760	20932641	36072644	100.824	107.535
31) Mirex	8.653	9.680	11960753	19363200	95.406	104.062
32) Chlordane...	7.428	8.123	131019	22164400	6.654	612.537 #
33) Chlordane...	7.516	8.237	18351251	88947	732.167	2.929 #
34) Chlordane...	0.000	8.905	0	44814	N.D.	4.998 #
35) Chlordane...	3.443	3.434	27193	63535	NoCal	NoCal
36) Toxaphene...	7.516	8.496f	18351251	20118925	20489.369	7666.519 #
37) Toxaphene...	7.798	0.000	56666	0	35.089	N.D. #
38) Toxaphene...	8.115	8.863	14279	23343	4.240	4.606
39) Toxaphene...	8.316f	8.905	25592	44814	7.898	5.367
40) Toxaphene...	8.604f	9.101	1951	8073	0.814	1.732 #
41) Toxaphene...	8.653	0.000	11960753	0	3779.567	N.D. #
42) Toxaphene...	3.443	3.434	27193	63535	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231924.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 18:27  
Operator : MJB  
Sample : 9H23034-CALF  
Misc : A19E155, 9-42 100 ppb  
ALS Vial : 19 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:03:29 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231925.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 18:45  
 Operator : MJB  
 Sample : 9H23034-CALG  
 Misc : A19E271, 9-42 200 ppb  
 ALS Vial : 20 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:03:40 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
6/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.367f	5.980	60549	10992	0.365	0.037 #
22) S DCBP (S)	9.590	10.538	118766	140925	0.842	0.784
Target Compounds						
2) a-BHC	5.933	6.593	27118	40902	0.118	0.100
3) g-BHC	6.218	6.912	21255	30993	0.105	0.087
4) b-BHC	6.299	6.977	25058	44238	0.277	0.280
5) Heptachlor	6.630	7.287	63252	104459	0.349	0.341
6) d-BHC	6.448	7.231	43545	78794	0.221	0.223
7) Aldrin	6.870	7.552	17012	29944	0.086	0.091
8) Heptachlo...	7.331	7.988	24819199	162906	134.756	0.541 #
9) trans-Chl...	7.425	8.122	250239	44504592	1.353	142.039 #
10) cis-Chlor...	7.514	8.235	35027918	188111	192.386	0.646 #
11) Endosulfa...	7.581f	8.289	74592	84898	0.438	0.309
12) 4,4'-DDE	7.581	8.341	74592	59877	0.396	0.193 #
13) Dieldrin	7.794	8.494	114089	39839303	0.594	130.986 #
14) Endrin	7.984f	8.719	40046185	39999231	272.373	177.123
15) 4,4'-DDD	7.984	8.759	40046185	72455823	254.843	282.794
16) Endosulfa...	8.113	8.861	50946	84198	0.355	0.365
17) 4,4'-DDT	8.201	8.983	28640	48189	0.240	0.243
18) Endrin Al...	8.404	9.098	39025	57504	BelowCal	BelowCal
19) Endosulfa...	0.000	9.289	0	61418	N.D.	0.247 #
20) Methoxychlor	8.541	9.464	9687	26335	0.165	0.141
21) Endrin Ke...	8.898	9.679	37586	38425530	0.225	149.332 #
23) Hexachlor...	3.199	3.689	34166533	75988565	186.969	202.134
24) Hexachlor...	5.774	6.454	34073459	66261966	193.277	210.967
25) Oxychlorane	7.258	7.920	32032634	58736982	194.683	214.445
26) 2,4'-DDE	7.331	8.122	24819199	44504592	193.505	209.791
27) trans-Non...	7.514	8.194	35027918	63083636	195.632	209.138
28) 2,4'-DDD	7.703	8.494	21916962	39839303	192.043	210.942
29) 2,4'-DDT	7.887	8.719	23024956	39999231	209.914	224.287
30) cis-Nonac...	7.984	8.759	40046185	72455823	192.886	215.996
31) Mirex	8.652	9.679	23284997	38425530	185.735	206.507
32) Chlordane...	7.425	8.122	250239	44504592	12.709	1229.933 #
33) Chlordane...	7.514	8.235	35027918	188111	1397.523	6.195 #
34) Chlordane...	0.000	8.902	0	52051	N.D.	5.805 #
35) Chlordane...	3.438	3.433	48985	106773	NoCal	NoCal
36) Toxaphene...	7.514	8.494f	35027918	39839303	39109.048	15181.168 #
37) Toxaphene...	7.794	0.000	114089	0	70.646	N.D. #
38) Toxaphene...	8.113	8.861	50946	84198	15.129	16.613
39) Toxaphene...	8.313f	8.902	28693	52051	8.856	6.234
40) Toxaphene...	8.602f	9.098	3169	57504	1.322	12.339 #
41) Toxaphene...	8.652	9.464	23284997	26335	7357.999	5.544 #
42) Toxaphene...	3.438	3.433	48985	106773	NoCal	NoCal

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231925.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 18:45  
Operator : MJB  
Sample : 9H23034-CALG  
Misc : A19E271, 9-42 200 ppb  
ALS Vial : 20 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:03:40 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231928.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 19:36  
 Operator : MJB  
 Sample : 9H23034-CALH  
 Misc : A19F232, CHLOR 50 ppb  
 ALS Vial : 22 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:04:22 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

WB 8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D.	N.D.
22) S DCBP (S)	9.606	0.000	5901	0	0.042	N.D. #
Target Compounds						
2) a-BHC	0.000	6.622f	0	41997	N.D.	0.102 #
3) g-BHC	6.194f	6.924	13212	19652	0.065	0.055
4) b-BHC	6.323f	7.016f	10976	62438	0.121	0.395 #
5) Heptachlor	6.632	7.288	412192	714454	2.274	2.335
6) d-BHC	6.412f	0.000	34416	0	0.175	N.D. #
7) Aldrin	6.877	7.558	6150	10093	0.031	0.031
8) Heptachlo...	7.337	8.010	84467	51183	0.459	0.170 #
9) trans-Chl...	7.429	8.131	1009143	1754707	5.458	5.600
10) cis-Chlor...	7.521	8.237	1286655	1472400	7.067	5.056
11) Endosulfa...	7.640	8.308	29794	24027	0.175	0.087 #
12) 4,4'-DDE	7.579	8.333	33953	45018	0.180	0.145
13) Dieldrin	7.807	8.488	35520	119533	0.185	0.393 #
14) Endrin	7.986f	8.714	182097	37218	1.239	0.165 #
15) 4,4'-DDD	7.986	8.759	182097	301826	1.159	1.178
16) Endosulfa...	8.118	8.873	19535	32870	0.136	0.143
17) 4,4'-DDT	0.000	8.994	0	11155	N.D.	0.027 #
18) Endrin Al...	8.368f	9.128f	14946	80647	BelowCal	BelowCal
19) Endosulfa...	8.708	9.316f	13079	6249	0.084	0.025 #
20) Methoxychlor	8.553	0.000	3815	0	0.065	N.D. #
21) Endrin Ke...	8.899	9.686	2603	18155	0.016	0.071 #
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
25) Oxychlordane	7.256	7.934	11579	24468	0.070	0.089
26) 2,4'-DDE	7.337	8.131	84467	1754707	0.659	8.272 #
27) trans-Non...	7.521	8.194	1286655	1274306	6.866	4.225
28) 2,4'-DDD	7.675f	8.488	83034	119533	0.728	0.633
29) 2,4'-DDT	7.914f	8.714	22312	37218	0.203	0.209
30) cis-Nonac...	7.986	8.759	182097	301826	0.877	0.900
31) Mirex	0.000	9.686	0	18155	N.D.	0.098 #
32) Chlordane...	7.429	8.131	1009143	1754707	51.253	48.493
33) Chlordane...	7.521	8.237	1286655	1472400	51.334	48.492
34) Chlordane...	8.068	8.897	288087	439020	49.832	48.966
35) Chlordane...	3.446	0.000	5365	0	NoCal	N.D.
36) Toxaphene...	7.521	8.488f	1286655	119533	1436.564	45.549 #
37) Toxaphene...	7.807	8.814	35520	51904	21.995	15.771
38) Toxaphene...	8.118	8.851	19535	35575	5.801	7.019
39) Toxaphene...	8.348	8.897	14389	439020	4.441	52.578 #
40) Toxaphene...	8.553f	9.128f	3815	80647	1.591	17.305 #
41) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
42) Toxaphene...	3.446	0.000	5365	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231928.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 19:36  
Operator : MJB  
Sample : 9H23034-CALH  
Misc : A19F232, CHLOR 50 ppb  
ALS Vial : 22 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:04:22 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231929.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 19:54  
 Operator : MJB  
 Sample : 9H23034-CALI  
 Misc : A19F233, CHLOR 100 ppb  
 ALS Vial : 23 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:04:32 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



*MB  
8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.984	0	5943	N.D.	0.020 #
22) S DCBP (S)	9.606	0.000	7472	0	0.053	N.D. #
Target Compounds						
2) a-BHC	0.000	6.622f	0	77932	N.D.	0.190 #
3) g-BHC	6.194f	6.923	23514	36662	0.117	0.103
4) b-BHC	6.323f	7.016f	21053	115009	0.233	0.727 #
5) Heptachlor	6.632	7.288	802906	1372147	4.429	4.484
6) d-BHC	6.412f	0.000	63497	0	0.323	N.D. #
7) Aldrin	6.877	7.558	12864	20481	0.065	0.062
8) Heptachlo...	7.338	8.010	155514	93915	0.844	0.312 #
9) trans-Chl...	7.429	8.130	1978897	3378388	10.703	10.782
10) cis-Chlor...	7.521	8.238	2519520	2905941	13.838	9.978
11) Endosulfa...	7.641f	8.309f	56850	48968	0.334	0.178 #
12) 4,4'-DDE	7.579	8.334	63125	84256	0.335	0.271
13) Dieldrin	7.807	8.488	69910	230931	0.364	0.759 #
14) Endrin	7.986f	8.713	344068	89428	2.340	0.396 #
15) 4,4'-DDD	7.986	8.760	344068	593441	2.190	2.316
16) Endosulfa...	8.118	8.873	39271	74727	0.273	0.324
17) 4,4'-DDT	0.000	8.995	0	22043	N.D.	0.090 #
18) Endrin Al...	8.428f	9.128f	7592	153472	BelowCal	BelowCal
19) Endosulfa...	8.709	9.317f	21141	11695	0.136	0.047 #
20) Methoxychlor	8.553	0.000	6889	0	0.118	N.D. #
21) Endrin Ke...	8.897	9.687	3240	29883	0.019	0.116 #
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	6.430f	0	7921	N.D.	0.025 #
25) Oxychlordane	7.255	7.934	24127	50634	0.147	0.185
26) 2,4'-DDE	7.338	8.130	155514	3378388	1.212	15.925 #
27) trans-Non...	7.521	8.195	2519520	2542319	13.749	8.428
28) 2,4'-DDD	7.676f	8.488	159771	230931	1.400	1.223
29) 2,4'-DDT	7.914f	8.713	44472	89428	0.405	0.501
30) cis-Nonac...	7.986	8.760	344068	593441	1.657	1.769
31) Mirex	0.000	9.687	0	29883	N.D.	0.161 #
32) Chlordane...	7.429	8.130	1978897	3378388	100.505	93.365
33) Chlordane...	7.521	8.238	2519520	2905941	100.522	95.703
34) Chlordane...	8.068	8.898	548196	874465	94.825	97.533
35) Chlordane...	3.446	0.000	4938	0	NoCal	N.D.
36) Toxaphene...	7.521	8.488f	2519520	230931	2813.072	87.999 #
37) Toxaphene...	7.807	8.815	69910	108014	43.289	32.821
38) Toxaphene...	8.118	8.851	39271	84269	11.662	16.627 #
39) Toxaphene...	8.349	8.898	25383	874465	7.834	104.728 #
40) Toxaphene...	8.553f	9.068f	6889	13931	2.874	2.989
41) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
42) Toxaphene...	3.446	0.000	4938	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231929.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 19:54  
Operator : MJB  
Sample : 9H23034-CALI  
Misc : A19F233, CHLOR 100 ppb  
ALS Vial : 23 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:04:32 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231930.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 20:11  
 Operator : MJB  
 Sample : 9H23034-CALJ  
 Misc : A19F234, CHLOR 200 ppb  
 ALS Vial : 24 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:04:43 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D.	N.D.
22) S DCBP (S)	9.605	0.000	9631	0	0.068	N.D. #
Target Compounds						
2) a-BHC	0.000	6.623f	0	141009	N.D.	0.344 #
3) g-BHC	6.197f	6.925	44236	70355	0.219	0.197
4) b-BHC	6.269f	0.000	45994	0	0.509	N.D. #
5) Heptachlor	6.633	7.290	1604459	2790294	8.850	9.119
6) d-BHC	6.414f	7.222	125171	21783	0.636	0.062 #
7) Aldrin	6.878	7.559	27966	42088	0.142	0.128
8) Heptachlo...	7.339	8.011	296306	184421	1.609	0.613 #
9) trans-Chl...	7.429	8.131	3849299	6751197	20.819	21.547
10) cis-Chlor...	7.522	8.239	4906320	5883615	26.947	20.201
11) Endosulfa...	7.641f	8.311f	111658	101195	0.656	0.368 #
12) 4,4'-DDE	7.579	8.334	119469	162236	0.634	0.522
13) Dieldrin	7.808	8.488	135995	479651	0.708	1.577 #
14) Endrin	7.986f	8.714	662867	142098	4.508	0.629 #
15) 4,4'-DDD	7.986	8.759	662867	1113368	4.218	4.345
16) Endosulfa...	8.119	8.852	78177	142714	0.544	0.619
17) 4,4'-DDT	0.000	8.995	0	47222	N.D.	0.237 #
18) Endrin Al...	8.429f	9.129f	17160	296262	BelowCal	0.772
19) Endosulfa...	8.709	9.317f	39967	28714	0.258	0.115 #
20) Methoxychlor	8.528	9.426f	15895	10981	0.271	BelowCal #
21) Endrin Ke...	8.895	9.688	5405	57534	0.032	0.224 #
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.768	6.432f	3592	14719	0.020	0.047 #
25) Oxychlordane	7.256	7.935	46857	97946	0.285	0.358
26) 2,4'-DDE	7.339	8.131	296306	6751197	2.310	31.825 #
27) trans-Non...	7.522	8.196	4906320	5159253	27.077	17.104
28) 2,4'-DDD	7.676f	8.488	310109	479651	2.717	2.540
29) 2,4'-DDT	7.915f	8.714	90205	142098	0.822	0.797
30) cis-Nonac...	7.986	8.759	662867	1113368	3.193	3.319
31) Mirex	8.690f	9.688	25315	57534	0.202	0.309 #
32) Chlordane...	7.429	8.131	3849299	6751197	195.499	186.577
33) Chlordane...	7.522	8.239	4906320	5883615	195.749	193.769
34) Chlordane...	8.069	8.898	1101677	1731727	190.565	193.146
35) Chlordane...	3.448	0.000	4503	0	NoCal	N.D.
36) Toxaphene...	7.522f	8.488f	4906320	479651	5477.960	182.776 #
37) Toxaphene...	7.808	8.815	135995	186597	84.211	56.699
38) Toxaphene...	8.119	8.852	78177	142714	23.215	28.158
39) Toxaphene...	8.349	8.898	48611	1731727	15.003	207.397 #
40) Toxaphene...	8.553f	9.069f	15795	32796	6.589	7.037
41) Toxaphene...	0.000	0.000	0	0	N.D.	N.D.
42) Toxaphene...	3.448	0.000	4503	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231930.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 20:11  
Operator : MJB  
Sample : 9H23034-CALJ  
Misc : A19F234, CHLOR 200 ppb  
ALS Vial : 24 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:04:43 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231931.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 20:28  
 Operator : MJB  
 Sample : 9H23034-CALK  
 Misc : A19F235, CHLOR 500 ppb  
 ALS Vial : 25 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:04:52 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
6/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.982	0	9372	N.D.	0.032 #
22) S DCBP (S)	9.605	10.512f	13871	6664	0.098	0.037 #
Target Compounds						
2) a-BHC	0.000	6.621f	0	314411	N.D.	0.766 #
3) g-BHC	6.194f	6.923	92958	161395	0.461	0.452
4) b-BHC	6.322f	7.016f	105835	520011	1.171	3.286 #
5) Heptachlor	6.631	7.288	4107971	7192687	22.659	23.507
6) d-BHC	6.412f	7.219	305503	51612	1.553	0.146 #
7) Aldrin	6.876	7.558	67201	101902	0.340	0.309
8) Heptachlo...	7.336	8.009	709786	434942	3.854	1.446 #
9) trans-Chl...	7.427	8.129	9628671	17830433	52.077	56.907
10) cis-Chlor...	7.520	8.237	12176524	14812273	66.878	50.858
11) Endosulfa...	7.639	8.308	267451	260205	1.572	0.946
12) 4,4'-DDE	7.577	8.332	288716	403680	1.531	1.299
13) Dieldrin	7.806	8.487	320749	1311343	1.671	4.312 #
14) Endrin	7.984f	8.712	1680286	346653	11.428	1.535 #
15) 4,4'-DDD	7.984	8.758	1680286	2798638	10.693	10.923
16) Endosulfa...	8.118	8.872	194466	323054	1.354	1.401
17) 4,4'-DDT	0.000	8.994	0	120742	N.D.	0.665 #
18) Endrin Al...	8.427f	9.127f	45775	749534	BelowCal	3.242
19) Endosulfa...	8.708	9.316f	99125	76741	0.640	0.308 #
20) Methoxychlor	8.552	9.462	44336	19918	0.757	0.061 #
21) Endrin Ke...	8.892	9.686	12903	140715	0.077	0.547 #
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.767	6.430f	6475	34351	0.037	0.109 #
25) Oxychlordane	7.283f	7.933	1963331	230983	11.932	0.843 #
26) 2,4'-DDE	7.336	8.129	709786	17830433	5.534	84.051 #
27) trans-Non...	7.520	8.194	12176524	13173616	67.700	43.674
28) 2,4'-DDD	7.674f	8.487	765105	1311343	6.704	6.943
29) 2,4'-DDT	7.913f	8.712	230360	346653	2.100	1.944
30) cis-Nonac...	7.984	8.758	1680286	2798638	8.093	8.343
31) Mirex	8.645	9.686	12290	140715	0.098	0.756 #
32) Chlordane...	7.427	8.129	9628671	17830433	489.023	492.763
33) Chlordane...	7.520	8.237	12176524	14812273	485.812	487.822
34) Chlordane...	8.067	8.896	2921278	4271709	505.313	476.441
35) Chlordane...	3.447	0.000	4056	0	NoCal	N.D.
36) Toxaphene...	7.520	8.487f	12176524	1311343	13595.220	499.701 #
37) Toxaphene...	7.806	8.813	320749	462807	198.614	140.627
38) Toxaphene...	8.118	8.850	194466	348421	57.748	68.745
39) Toxaphene...	8.348	8.896	120098	4271709	37.065	511.592 #
40) Toxaphene...	8.552f	9.067f	44336	90716	18.495	19.465
41) Toxaphene...	8.645	9.462	12290	19918	3.884	4.193
42) Toxaphene...	3.447	0.000	4056	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231931.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 20:28  
Operator : MJB  
Sample : 9H23034-CALK  
Misc : A19F235, CHLOR 500 ppb  
ALS Vial : 25 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:04:52 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231932.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 20:45  
 Operator : MJB  
 Sample : 9H23034-CALL  
 Misc : A19F236, CHLOR 1000 ppb  
 ALS Vial : 26 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:05:04 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB*  
*8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
-----						
System Monitoring Compounds						
1) S TCMX (S)	5.393	5.980	6433	11040	0.039	0.038
22) S DCBP (S)	9.604	10.553	33011	8716	0.234	0.048 #
Target Compounds						
2) a-BHC	0.000	6.622f	0	610263	N.D.	1.487 #
3) g-BHC	6.194f	6.923	179715	319626	0.891	0.896
4) b-BHC	6.322f	7.016f	206312	1070369	2.283	6.763 #
5) Heptachlor	6.631	7.288	8491782	15019038	46.839	49.085
6) d-BHC	6.411f	7.241	615917	64884	3.131	0.184 #
7) Aldrin	6.875	7.558	134371	205192	0.681	0.623
8) Heptachlo...	7.335	8.009	1431988	873449	7.775	2.903 #
9) trans-Chl...	7.426	8.130	19643766	37966746	106.245	121.173
10) cis-Chlor...	7.519	8.237	25083239	31493677	137.766	108.134
11) Endosulfa...	7.638	8.309f	523226	508009	3.075	1.846
12) 4,4'-DDE	7.576	8.332	564335	775935	2.993	2.498
13) Dieldrin	7.805	8.487	632206	2703774	3.293	8.890 #
14) Endrin	7.985f	8.713	3305895	704023	22.485	3.118 #
15) 4,4'-DDD	7.985	8.758	3305895	5865563	21.038	22.893
16) Endosulfa...	8.118	8.872	392448	653843	2.733	2.835
17) 4,4'-DDT	8.241f	8.994	1019486	242495	8.527	1.373 #
18) Endrin Al...	8.427f	9.128f	96085	1500188	BelowCal	7.301
19) Endosulfa...	8.708	9.269	190049	57556	1.226	0.231 #
20) Methoxychlor	8.552	9.462	93194	45695	1.591	0.381 #
21) Endrin Ke...	8.891	9.687	25043	266287	0.150	1.035 #
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.767	6.430f	12323	65416	0.070	0.208 #
25) Oxychlordane	7.252	7.933	207847	466300	1.263	1.702
26) 2,4'-DDE	7.335	8.130	1431988	37966746	11.165	178.972 #
27) trans-Non...	7.519	8.194	25083239	27721467	139.911	91.904
28) 2,4'-DDD	7.673f	8.487	1536407	2703774	13.462	14.316
29) 2,4'-DDT	7.912f	8.713	462112	704023	4.213	3.948
30) cis-Nonac...	7.985	8.758	3305895	5865563	15.923	17.486
31) Mirex	8.645	9.687	28961	266287	0.231	1.431 #
32) Chlordane...	7.426	8.130	19643766	37966746	997.671	1049.252
33) Chlordane...	7.519	8.237	25083239	31493677	1000.756	1037.202
34) Chlordane...	8.067	8.897	5987927	9358900	1035.773	1043.835
35) Chlordane...	3.447	0.000	4825	0	NoCal	N.D.
36) Toxaphene...	7.519	8.487f	25083239	2703774	28005.706	1030.300 #
37) Toxaphene...	7.805	8.814	632206	927954	391.474	281.965
38) Toxaphene...	8.118	8.850	392448	706508	116.540	139.397
39) Toxaphene...	8.348	8.897	233440	9358900	72.046	1120.849 #
40) Toxaphene...	8.552f	9.067f	93194	183092	38.877	39.287
41) Toxaphene...	8.645	9.462	28961	45695	9.152	9.620
42) Toxaphene...	3.447	0.000	4825	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231932.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 20:45  
Operator : MJB  
Sample : 9H23034-CALL  
Misc : A19F236, CHLOR 1000 ppb  
ALS Vial : 26 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:05:04 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231933.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 21:02  
 Operator : MJB  
 Sample : 9H23034-CALM  
 Misc : A19F231, CHLOR 2000 ppb  
 ALS Vial : 27 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:05:14 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB*  
*8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.393	5.971	11655	15748	0.070	0.054
22) S DCBP (S)	9.604	10.552	57777	17575	0.409	0.098 #
Target Compounds						
2) a-BHC	0.000	6.621f	0	1174704	N.D.	2.863 #
3) g-BHC	6.193f	6.922	334417	594314	1.657	1.666
4) b-BHC	6.321f	7.016f	403109	2092681	4.460	13.223 #
5) Heptachlor	6.630	7.288	16898199	31950039	93.207	104.420
6) d-BHC	6.411f	7.240	1241284	122584	6.311	0.348 #
7) Aldrin	6.874	7.557	258489	381283	1.309	1.158
8) Heptachlo...	7.335	8.008	2829322	1755780	15.362	5.836 #
9) trans-Chl...	7.426	8.130	40036500	81691713	216.541	260.724
10) cis-Chlor...	7.519	8.238	50979142	66281388	279.996	227.578
11) Endosulfa...	7.638	8.308	1047673	1022624	6.156	3.716
12) 4,4'-DDE	7.576	8.332	1098754	1565142	5.828	5.038
13) Dieldrin	7.805	8.486	1246658	5614133	6.494	18.458 #
14) Endrin	7.984f	8.692f	6820662	2823722	46.391	12.504 #
15) 4,4'-DDD	7.984	8.759	6820662	12014776	43.405	46.894
16) Endosulfa...	8.118	8.872	787524	1320218	5.484	5.725
17) 4,4'-DDT	8.242f	8.993	2107649	483614	17.628	2.768 #
18) Endrin Al...	8.427f	9.128f	193793	3090717	0.642	15.775 #
19) Endosulfa...	8.709	9.268f	400484	128754	2.584	0.517 #
20) Methoxychlor	8.552	9.462	195767	96597	3.342	1.012 #
21) Endrin Ke...	8.892	9.686	57711	528113	0.346	2.052 #
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.766	6.430f	22503	117032	0.128	0.373 #
25) Oxychlorane	7.252	7.932	378689	930396	2.302	3.397 #
26) 2,4'-DDE	7.335	8.130	2829322	81691713	22.059	385.087 #
27) trans-Non...	7.519	8.194	50979142	59315099	285.157	196.645
28) 2,4'-DDD	7.673f	8.486	3134690	5614133	27.467	29.726
29) 2,4'-DDT	7.912f	8.692f	956476	2823722	8.720	15.833 #
30) cis-Nonac...	7.984	8.759	6820662	12014776	32.852	35.817
31) Mirex	8.645	9.686	70178	528113	0.560	2.838 #
32) Chlordane...	7.426	8.130	40036500	81691713	2033.382	2257.639
33) Chlordane...	7.519	8.238	50979142	66281388	2033.935	2182.889
34) Chlordane...	8.067	8.897	12208306	19418517	2111.754	2165.824
35) Chlordane...	3.449	0.000	4939	0	NoCal	N.D.
36) Toxaphene...	7.519	8.486f	50979142	5614133	56918.762	2139.322 #
37) Toxaphene...	7.805	8.814	1246658	1872513	771.954	568.976
38) Toxaphene...	8.118	8.850	787524	1450920	233.861	286.273
39) Toxaphene...	8.368f	8.897	565943	19418517	174.666	2325.617 #
40) Toxaphene...	8.552f	9.067f	195767	367185	81.667	78.789
41) Toxaphene...	8.645	9.462	70178	96597	22.176	20.335
42) Toxaphene...	3.449	0.000	4939	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231933.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:02  
Operator : MJB  
Sample : 9H23034-CALM  
Misc : A19F231, CHLOR 2000 ppb  
ALS Vial : 27 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:05:14 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231936.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 21:54  
 Operator : MJB  
 Sample : 9H23034-CALN  
 Misc : A19D122, TOX 50 ppb  
 ALS Vial : 29 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:06:20 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB  
8/26/19*


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.984	0	6201	N.D.	0.021 #
22) S DCBP (S)	0.000	0.000	0	0	N.D.	N.D.
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D.	N.D.
3) g-BHC	6.249f	0.000	4430	0	0.022	N.D. #
4) b-BHC	6.297	0.000	3017	0	0.033	N.D. #
5) Heptachlor	6.627	0.000	4370	0	0.024	N.D. #
6) d-BHC	6.469f	0.000	2958	0	0.015	N.D. #
7) Aldrin	6.871	7.582f	4859	11806	0.025	0.036 #
8) Heptachlo...	7.336	7.985	13601	46078	0.074	0.153 #
9) trans-Chl...	7.446	8.142	34060	99117	0.184	0.316 #
10) cis-Chlor...	7.518	8.221	69068	59106	0.379	0.203 #
11) Endosulfa...	7.629	8.294	55946	68659	0.329	0.250
12) 4,4'-DDE	7.550f	8.359	47125	82546	0.250	0.266
13) Dieldrin	7.794	8.505	88321	82204	0.460	0.270 #
14) Endrin	7.934f	8.709	54457	133121	0.370	0.589 #
15) 4,4'-DDD	8.020	8.762	70973	90688	0.452	0.354
16) Endosulfa...	8.105	8.847	169381	254833	1.179	1.105
17) 4,4'-DDT	8.180f	8.977	146997	96725	1.229	0.525 #
18) Endrin Al...	8.392	9.091	108459	233185	BelowCal	0.427
19) Endosulfa...	8.708	9.291	48053	90329	0.310	0.363
20) Methoxychlor	8.573f	9.470	114720	230922	1.959	2.668
21) Endrin Ke...	8.894	9.711f	33550	36259	0.201	0.141
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	0.000	6.487f	0	8846	N.D.	0.028 #
25) Oxychlordane	7.265	7.935	38772	48452	0.236	0.177
26) 2,4'-DDE	7.336	8.112	13601	53529	0.106	0.252 #
27) trans-Non...	7.518	8.204	69068	54722	0.069	0.181 #
28) 2,4'-DDD	7.713	8.505	60294	82204	0.528	0.435
29) 2,4'-DDT	7.899	8.709	96979	133121	0.884	0.746
30) cis-Nonac...	7.981	8.762	116026	90688	0.559	0.270 #
31) Mirex	8.641	9.711f	153138	36259	1.222	0.195 #
32) Chlordane...	7.446	8.142	34060	99117	1.730	2.739 #
33) Chlordane...	7.518	8.221	69068	59106	2.756	1.947
34) Chlordane...	8.047f	8.915	69875	416348	12.087	46.437 #
35) Chlordane...	3.449	0.000	4023	0	NoCal	N.D.
36) Toxaphene...	7.506	8.466	49110	136848	54.832m	52.147
37) Toxaphene...	7.794	8.813	88321	164706	54.690	50.047
38) Toxaphene...	8.105	8.847	169381	254833	50.299	50.280
39) Toxaphene...	8.346	8.915	164317	416348	50.713	49.863
40) Toxaphene...	8.573	9.091	114720	233185	47.857	50.036
41) Toxaphene...	8.641	9.470	153138	230922	48.391	48.613
42) Toxaphene...	3.449	0.000	4023	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231936.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:54  
Operator : MJB  
Sample : 9H23034-CALN  
Misc : A19D122, TOX 50 ppb  
ALS Vial : 29 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:05:49 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(36) Toxaphene (1)  
7.506min 54.832 ng/mL  
response 49110


*MJB 8/26/19*

(36) Toxaphene (1) #2  
8.466min 52.147 ng/mL  
response 136848

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231936.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:54  
Operator : MJB  
Sample : 9H23034-CALN  
Misc : A19D122, TOX 50 ppb  
ALS Vial : 29 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:05:49 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(36) Toxaphene (1)  
7.518min 77.175 ng/mL  
response 69068



*MJB*  
*8/26/19*

(36) Toxaphene (1) #2  
8.466min 52.147 ng/mL  
response 136848

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231936.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:54  
Operator : MJB  
Sample : 9H23034-CALN  
Misc : A19D122, TOX 50 ppb  
ALS Vial : 29 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:06:20 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231937.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 22:11  
 Operator : MJB  
 Sample : 9H23034-CALO  
 Misc : A19D123, TOX 100 ppb  
 ALS Vial : 30 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:07:08 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.985	0	6562	N.D.	0.022 #
2) S DCBP (S)	9.592	0.000	4802	0	0.034	N.D. #
Target Compounds						
2) a-BHC	5.952	0.000	2451	0	0.011	N.D. #
3) g-BHC	6.250f	0.000	4208	0	0.021	N.D. #
4) b-BHC	6.297	6.965	3419	5803	0.038	0.037
5) Heptachlor	6.629	7.259f	5698	7338	0.031	0.024
6) d-BHC	6.470f	7.259f	3844	7338	0.020	0.021
7) Aldrin	6.872	7.582f	9196	24729	0.047	0.075 #
8) Heptachlo...	7.359f	7.984	53934	87078	0.293	0.289
9) trans-Chl...	7.445	8.141	66985	117380	0.362	0.375
10) cis-Chlor...	7.517	8.220	93146	107177	0.512	0.368
11) Endosulfa...	7.629	8.295	104883	129689	0.616	0.471
12) 4,4'-DDE	7.551f	8.359	82562	155356	0.438	0.500
13) Dieldrin	7.795	8.506	166085	156611	0.865	0.515 #
14) Endrin	7.934f	8.710	115324	262153	0.784	1.161 #
15) 4,4'-DDD	8.021	8.762	139852	178338	0.890	0.696
16) Endosulfa...	8.106	8.848	332842	494430	2.318	2.144
17) 4,4'-DDT	8.182f	8.977	285351	192921	2.387	1.085 #
18) Endrin Al...	8.393	9.091	215405	452209	0.828	1.624 #
19) Endosulfa...	8.710	9.291	103697	183737	0.669	0.738
20) Methoxychlor	8.543	9.471	105544	452485	1.802	5.374 #
21) Endrin Ke...	8.894	9.712f	71764	83930	0.430	0.326
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.811f	6.488f	2684	8988	0.015	0.029 #
25) Oxychlorane	7.266	7.935	73507	87358	0.447	0.319
26) 2,4'-DDE	7.359f	8.112	53934	99205	0.420	0.468
27) trans-Non...	7.517	8.204	93146	102328	0.204	0.339 #
28) 2,4'-DDD	7.713	8.506	118203	156611	1.036	0.829
29) 2,4'-DDT	7.899	8.710	187872	262153	1.713	1.470
30) cis-Nonac...	7.982	8.762	219963	178338	1.059	0.532 #
31) Mirex	8.641	9.712f	302577	83930	2.414	0.451 #
32) Chlordane...	7.410	8.141	46689	117380	2.371	3.244
33) Chlordane...	7.517	8.220	93146	107177	3.716	3.530
34) Chlordane...	8.047f	8.915	142490	811948	24.647	90.560 #
35) Chlordane...	3.450	0.000	3536	0	NoCal	N.D.
36) Toxaphene...	7.501	8.466	91358	267534	102.002m	101.946
37) Toxaphene...	7.795	8.813	166085	324070	102.843	98.471
38) Toxaphene...	8.106	8.848	332842	494430	98.840	97.553
39) Toxaphene...	8.346	8.915	320313	811948	98.857	97.241
40) Toxaphene...	8.574	9.091	228960	452209	95.514	97.033
41) Toxaphene...	8.641	9.471	302577	452485	95.614	95.256
42) Toxaphene...	3.450	0.000	3536	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231937.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:11  
Operator : MJB  
Sample : 9H23034-CALO  
Misc : A19D123, TOX 100 ppb  
ALS Vial : 30 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:06:39 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(36) Toxaphene (1)  
7.501min 102.002 ng/mL (m)  
response 91358


(36) Toxaphene (1) #2  
8.466min 101.946 ng/mL  
response 267534

~~MJB 8/26/19~~  
6/26/19  
MJB 8/26/19

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231937.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:11  
Operator : MJB  
Sample : 9H23034-CALO  
Misc : A19D123, TOX 100 ppb  
ALS Vial : 30 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:06:39 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



~~(36) Toxaphene (1)  
7.517min 103.998 ng/mL  
response 93146~~



*MJB 8/26/19*

(36) Toxaphene (1) #2  
8.466min 101.946 ng/mL  
response 267534

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231937.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:11  
Operator : MJB  
Sample : 9H23034-CALO  
Misc : A19D123, TOX 100 ppb  
ALS Vial : 30 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:07:08 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231938.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 22:28  
 Operator : MJB  
 Sample : 9H23034-CALP  
 Misc : A19D124, TOX 200 ppb  
 ALS Vial : 31 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:07:22 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.984	0	6031	N.D.	0.021 #
22) S DCBP (S)	9.591	10.521	8317	11024	0.059	0.061
Target Compounds						
2) a-BHC	5.950	0.000	2445	0	0.011	N.D. #
3) g-BHC	6.249f	6.906	4762	8484	0.024	0.024
4) b-BHC	6.297	6.965	5553	11866	0.061	0.075
5) Heptachlor	6.630	7.292	9834	18991	0.054	0.062
6) d-BHC	6.469f	7.232	7279	22404	0.037	0.064 #
7) Aldrin	6.872	7.582f	20475	52234	0.104	0.159 #
8) Heptachlo...	7.336	7.984	58943	180203	0.320	0.599 #
9) trans-Chl...	7.445	8.139	130754	171469	0.707	0.547
10) cis-Chlor...	7.502f	8.220	176047	207038	0.967	0.711
11) Endosulfa...	7.629	8.294	203563	255143	1.196	0.927
12) 4,4'-DDE	7.551f	8.358	153844	307212	0.816	0.989
13) Dieldrin	7.795	8.506	317587	302159	1.654	0.993
14) Endrin	7.934f	8.709	233827	517355	1.590	2.291 #
15) 4,4'-DDD	8.021	8.761	271844	361076	1.730	1.409
16) Endosulfa...	8.105	8.847	644464	995555	4.488	4.317
17) 4,4'-DDT	8.182f	8.976	572615	378347	4.789	2.160 #
18) Endrin Al...	8.392	9.090	423151	895397	2.609	4.034 #
19) Endosulfa...	8.709	9.290	207483	368442	1.339	1.479
20) Methoxychlor	8.543	9.469	215126	905244	3.673	10.806 #
21) Endrin Ke...	8.893	9.711f	142657	173912	0.855	0.676
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.811f	6.487f	2563	8587	0.015	0.027 #
25) Oxychlorthane	7.266	7.935	140581	179085	0.854	0.654
26) 2,4'-DDE	7.336	8.112	58943	198883	0.460	0.938 #
27) trans-Non...	7.502	8.205	176047	199265	0.666	0.661
28) 2,4'-DDD	7.713	8.506	232393	302159	2.036	1.600
29) 2,4'-DDT	7.899	8.709	356627	517355	3.251	2.901
30) cis-Nonac...	7.982	8.761	437778	361076	2.109	1.076 #
31) Mirex	8.640	9.711f	597991	173912	4.770	0.935 #
32) Chlordane...	7.445	8.139	130754	171469	6.641	4.739
33) Chlordane...	7.502	8.220	176047	207038	7.024	6.819
34) Chlordane...	8.047f	8.914	280898	1580436	48.589	176.272 #
35) Chlordane...	3.451	0.000	3919	0	NoCal	N.D.
36) Toxaphene...	7.502	8.466	176047	508983	196.559	193.953
37) Toxaphene...	7.795	8.812	317587	645322	196.656	196.085
38) Toxaphene...	8.105	8.847	644464	995555	191.378	196.427
39) Toxaphene...	8.346	8.914	632351	1580436	195.161	189.278
40) Toxaphene...	8.574	9.090	454431	895397	189.572	192.130
41) Toxaphene...	8.640	9.469	597991	905244	188.964	190.570
42) Toxaphene...	3.451	0.000	3919	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231938.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:28  
Operator : MJB  
Sample : 9H23034-CALP  
Misc : A19D124, TOX 200 ppb  
ALS Vial : 31 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:07:22 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231939.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 22:45  
 Operator : MJB  
 Sample : 9H23034-CALQ  
 Misc : A19D125, TOX 500 ppb  
 ALS Vial : 32 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:07:35 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	5.984	0	5601	N.D.	0.019 #
22) S DCBP (S)	9.591	10.521	21035	39647	0.149	0.221 #
Target Compounds						
2) a-BHC	5.938	6.598	3646	8422	0.016	0.021
3) g-BHC	6.246f	6.908	6276	21315	0.031	0.060 #
4) b-BHC	6.296	6.966	12656	26420	0.140	0.167
5) Heptachlor	6.631	7.291	26275	48687	0.145	0.159
6) d-BHC	6.434	7.233	12949	50866	0.066	0.144 #
7) Aldrin	6.871	7.582f	54986	128738	0.278	0.391 #
8) Heptachlo...	7.337	7.985	148782	431601	0.808	1.435 #
9) trans-Chl...	7.445	8.136	326510	348418	1.766	1.112
10) cis-Chlor...	7.502f	8.220	441826	492762	2.427	1.692
11) Endosulfa...	7.629	8.295	523361	619890	3.075	2.253
12) 4,4'-DDE	7.551f	8.358	370244	790371	1.964	2.544
13) Dieldrin	7.794	8.506	819454	752423	4.268	2.474 #
14) Endrin	7.934f	8.711	624315	1366705	4.246	6.052 #
15) 4,4'-DDD	8.021	8.761	715456	940917	4.553	3.672
16) Endosulfa...	8.105	8.848	1677481	2475022	11.681	10.733
17) 4,4'-DDT	8.182f	8.977	1480674	1000646	12.384	5.736 #
18) Endrin Al...	8.392	9.091	1117641	2340668	8.532	11.800
19) Endosulfa...	8.709	9.290	555797	952729	3.586	3.825
20) Methoxychlor	8.574f	9.470	1221560	2369795	20.855	27.582
21) Endrin Ke...	8.894	9.711f	386326	477017	2.317	1.854
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.814f	6.461	4241	6767	0.024	0.022
25) Oxychlorane	7.265	7.936	350487	422818	2.130	1.544
26) 2,4'-DDE	7.337	8.112	148782	485681	1.160	2.289 #
27) trans-Non...	7.502	8.205	441826	487255	2.150	1.615
28) 2,4'-DDD	7.713	8.506	583556	752423	5.113	3.984
29) 2,4'-DDT	7.899	8.711	935213	1366705	8.526	7.664
30) cis-Nonac...	7.981	8.761	1117997	940917	5.385	2.805 #
31) Mirex	8.640	9.711f	1623402	477017	12.949	2.564 #
32) Chlordane...	7.408	8.136	238293	348418	12.102	9.629
33) Chlordane...	7.502	8.220	441826	492762	17.628	16.228
34) Chlordane...	8.046f	8.915	731630	4252640	126.555	474.314 #
35) Chlordane...	3.450	0.000	4132	0	NoCal	N.D.
36) Toxaphene...	7.502	8.466	441826	1308994	493.303	498.805
37) Toxaphene...	7.794	8.812	819454	1647741	507.421	500.677
38) Toxaphene...	8.105	8.848	1677481	2475022	498.140	488.332
39) Toxaphene...	8.346	8.915	1649569	4252640	509.102	509.308
40) Toxaphene...	8.574	9.091	1221560	2340668	509.590	502.251
41) Toxaphene...	8.640	9.470	1623402	2369795	512.991	498.883
42) Toxaphene...	3.450	0.000	4132	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231939.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:45  
Operator : MJB  
Sample : 9H23034-CALQ  
Misc : A19D125, TOX 500 ppb  
ALS Vial : 32 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:07:35 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231940.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 23:03  
 Operator : MJB  
 Sample : 9H23034-CALR  
 Misc : A19D126, TOX 1000 ppb  
 ALS Vial : 33 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:07:46 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.415f	5.982	2381	5264	0.014	0.018
22) S DCBP (S)	9.591	10.522	47060	86882	0.334	0.483 #
Target Compounds						
2) a-BHC	5.937	6.597	7133	14957	0.031	0.036
3) g-BHC	6.231	6.907	12268	49388	0.061	0.138 #
4) b-BHC	6.296	6.967	24041	58985	0.266	0.373 #
5) Heptachlor	6.632	7.293	48435	95609	0.267	0.312
6) d-BHC	6.434	7.233	28416	100471	0.144	0.285 #
7) Aldrin	6.871	7.551	108360	147580	0.549	0.448
8) Heptachlo...	7.336	7.985	294905	840940	1.601	2.795 #
9) trans-Chl...	7.445	8.111f	659823	964498	3.569	3.078
10) cis-Chlor...	7.501f	8.220	871889	947518	4.789	3.253
11) Endosulfa...	7.628	8.295	1038833	1226540	6.104	4.457
12) 4,4'-DDE	7.550f	8.358	746675	1543581	3.961	4.968
13) Dieldrin	7.793	8.506	1556013	1462579	8.105	4.809 #
14) Endrin	7.933f	8.711	1312768	2786774	8.929	12.340
15) 4,4'-DDD	8.020	8.762	1452045	1895471	9.240	7.398
16) Endosulfa...	8.105	8.848	3495877	5168269	24.343	22.412
17) 4,4'-DDT	8.183	8.977	2996314	2028436	25.061	11.540 #
18) Endrin Al...	8.391	9.091	2338006	4900430	18.826	25.221
19) Endosulfa...	8.709	9.291	1188299	2002950	7.668	8.041
20) Methoxychlor	8.543	9.470	1177404	5046645	20.101	55.668 #
21) Endrin Ke...	8.893	9.712f	829327	990858	4.973	3.851
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.745f	6.463	2404	9221	0.014	0.029 #
25) Oxychlordane	7.265	7.936	684836	845822	4.162	3.088
26) 2,4'-DDE	7.336	8.111	294905	964498	2.299	4.547 #
27) trans-Non...	7.501	8.204	871889	963521	4.550	3.194
28) 2,4'-DDD	7.712	8.506	1203385	1462579	10.544	7.744
29) 2,4'-DDT	7.898	8.711	1885482	2786774	17.190	15.626
30) cis-Nonac...	7.981	8.762	2207076	1895471	10.631	5.651 #
31) Mirex	8.640	9.712f	3406737	990858	27.174	5.325 #
32) Chlordane...	7.445	8.111	659823	964498	33.511	26.655
33) Chlordane...	7.501	8.220	871889	947518	34.786	31.205
34) Chlordane...	8.045f	8.915	1508434	8650068	260.924	964.776 #
35) Chlordane...	3.451	0.000	2687	0	NoCal	N.D.
36) Toxaphene...	7.501	8.467	871889	2654886	973.473	1011.671
37) Toxaphene...	7.793	8.813	1556013	3384036	963.512	1028.262
38) Toxaphene...	8.105	8.848	3495877	5168269	1038.126	1019.721
39) Toxaphene...	8.345	8.915	3287014	8650068	1014.463	1035.957
40) Toxaphene...	8.573	9.091	2546293	4900430	1062.220	1051.514
41) Toxaphene...	8.640	9.470	3406737	5046645	1076.520	1062.406
42) Toxaphene...	3.451	0.000	2687	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231940.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 23:03  
Operator : MJB  
Sample : 9H23034-CALR  
Misc : A19D126, TOX 1000 ppb  
ALS Vial : 33 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:07:46 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\REQUANT\  
 Data File : ECD5-08231941.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 23:20  
 Operator : MJB  
 Sample : 9H23034-CALS  
 Misc : A19D121, TOX 2000 ppb  
 ALS Vial : 34 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 12:07:58 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:48:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MB  
8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.416f	5.979	3411	9459	0.021	0.032 #
22) S DCBP (S)	9.591	10.521	106938	194794	0.758	1.084 #
Target Compounds						
2) a-BHC	5.935	6.596	13246	39719	0.058	0.097 #
3) g-BHC	6.231	6.908	20790	85564	0.103	0.240 #
4) b-BHC	6.295	6.967	35592	107682	0.394	0.680 #
5) Heptachlor	6.633	7.293	79787	161818	0.440	0.529
6) d-BHC	6.433	7.233	46116	159995	0.234	0.454 #
7) Aldrin	6.871	7.581f	182635	424827	0.925	1.290
8) Heptachlo...	7.357f	7.984	952857	1568607	5.174	5.214
9) trans-Chl...	7.444	8.111f	1223688	1798529	6.618	5.740
10) cis-Chlor...	7.500f	8.218f	1674674	1710240	9.198	5.872
11) Endosulfa...	7.627	8.294	1999949	2341198	11.752	8.508
12) 4,4'-DDE	7.549f	8.357	1335034	2938735	7.081	9.459
13) Dieldrin	7.792	8.505	2958997	2895788	15.413	9.521
14) Endrin	7.981f	8.711	4441487	5651216	30.209	25.025
15) 4,4'-DDD	8.020	8.761	2883315	3832878	18.349	14.960
16) Endosulfa...	8.104	8.848	6831460	10545708	47.569	45.730
17) 4,4'-DDT	8.183	8.977	5897786	4051156	49.329	22.612 #
18) Endrin Al...	8.391	9.091	4718611	9435236	38.506	48.051
19) Endosulfa...	8.708	9.291	2483005	4046643	16.022	16.246
20) Methoxychlor	8.542	9.471	2322878	10090951	39.657	102.111 #
21) Endrin Ke...	8.893	9.712f	1725359	2080010	10.346	8.083
23) Hexachlor...	0.000	0.000	0	0	N.D.	N.D.
24) Hexachlor...	5.744f	6.462	3614	25550	0.021	0.081 #
25) Oxychlordane	7.264	7.935	1262060	1485955	7.670	5.425
26) 2,4'-DDE	7.357f	8.111	952857	1798529	7.429	8.478
27) trans-Non...	7.500	8.204	1674674	1791431	9.032	5.939
28) 2,4'-DDD	7.712	8.505	2255144	2895788	19.760	15.333
29) 2,4'-DDT	7.898	8.711	3633258	5651216	33.124	31.688
30) cis-Nonac...	7.981	8.761	4441487	3832878	21.393	11.426 #
31) Mirex	8.640	9.712f	6510950	2080010	51.935	11.178 #
32) Chlordane...	7.444	8.111	1223688	1798529	62.149	49.704
33) Chlordane...	7.500	8.218	1674674	1710240	66.815	56.324
34) Chlordane...	8.044f	8.914	2935856	17190037	507.835	1917.273 #
35) Chlordane...	3.452	0.000	4166	0	NoCal	N.D.
36) Toxaphene...	7.500	8.466	1674674	5030917	1869.791	1917.082
37) Toxaphene...	7.792	8.813	2958997	6610397	1832.266	2008.613
38) Toxaphene...	8.104	8.848	6831460	10545708	2028.651	2080.712
39) Toxaphene...	8.345	8.914	6407070	17190037	1977.398	2058.728
40) Toxaphene...	8.572	9.091	5074570	9435236	2116.925	2024.573
41) Toxaphene...	8.640	9.471	6510950	10090951	2057.443	2124.320
42) Toxaphene...	3.452	0.000	4166	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : R:\data\2019-08\9H23034\REQUANT\  
Data File : ECD5-08231941.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 23:20  
Operator : MJB  
Sample : 9H23034-CALS  
Misc : A19D121, TOX 2000 ppb  
ALS Vial : 34 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 12:07:58 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:48:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Sequence Name: C:\msdchem\4\sequence\9H23034.s

Comment: Pesticides

Operator: MJB

Data Path: C:\MSDCHEM\4\DATA\2019-08\9H23034\

Instrument Control Pre-Seq Cmd:

Data Analysis Pre-Seq Cmd:

Instrument Control Post-Seq Cmd:

Data Analysis Post-Seq Cmd:

Method Sections To Run            Sequence Barcode Options  
(X) Full Method                    (X) On Mismatch, Inject Anyway  
( ) Reprocessing Only            ( ) On Mismatch, Don't Inject  
                                      ( ) Barcode Disabled

-----

Line		Sample Name/Misc Info
1)	Sample	100 CONDITIONING RUN
	Datafile	ECD5-08231901
	Method	ECD5_AQUPEST_160111
2)	Sample	100 CONDITIONING RUN
	Datafile	ECD5-08231902
	Method	ECD5_AQUPEST_160111
3)	Sample	1 Hexane
	Datafile	ECD5-08231903
	Method	ECD5_AQUPEST_160111
4)	Sample	2 9H23034-BKD1
	Datafile	ECD5-08231904
	Method	ECD5_AQUPEST_160111
5)	Sample	1 Hexane
	Datafile	ECD5-08231905
	Method	ECD5_AQUPEST_160111
6)	Sample	2 9H23034-BKD2
	Datafile	ECD5-08231906
	Method	ECD5_AQUPEST_160111
7)	Sample	3 9H23034-ICB1
	Datafile	ECD5-08231907
	Method	ECD5_AQUPEST_160111
8)	Sample	4 9H23034-CAL1
	Datafile	ECD5-08231908
	Method	ECD5_AQUPEST_160111
9)	Sample	5 9H23034-CAL2
	Datafile	ECD5-08231909
	Method	ECD5_AQUPEST_160111
10)	Sample	6 9H23034-CAL3
	Datafile	ECD5-08231910
	Method	ECD5_AQUPEST_160111
11)	Sample	7 9H23034-CAL4
	Datafile	ECD5-08231911
	Method	ECD5_AQUPEST_160111
12)	Sample	8 9H23034-CAL5
	Datafile	ECD5-08231912
	Method	ECD5_AQUPEST_160111
13)	Sample	9 9H23034-CAL6
	Datafile	ECD5-08231913
	Method	ECD5_AQUPEST_160111
14)	Sample	10 9H23034-CAL7
	Datafile	ECD5-08231914
	Method	ECD5_AQUPEST_160111
15)	Sample	11 9H23034-CAL8
	Datafile	ECD5-08231915
	Method	ECD5_AQUPEST_160111
16)	Sample	1 9H23034-IBL1
	Datafile	ECD5-08231916
	Method	ECD5_AQUPEST_160111
17)	Sample	12 9H23034-ICV1
	Datafile	ECD5-08231917
	Method	ECD5_AQUPEST_160111
18)	Sample	13 9H23034-CAL9
	Datafile	ECD5-08231918
	Method	ECD5_AQUPEST_160111
19)	Sample	14 9H23034-CALA
	Datafile	ECD5-08231919
	Method	ECD5_AQUPEST_160111
20)	Sample	15 9H23034-CALB

MJB 8/26/19

	Datafile		ECD5-08231920
	Method		ECD5_AQUPEST_160111
21)	Sample	16	9H23034-CALC
	Datafile		ECD5-08231921
	Method		ECD5_AQUPEST_160111
22)	Sample	17	9H23034-CALD
	Datafile		ECD5-08231922
	Method		ECD5_AQUPEST_160111
23)	Sample	18	9H23034-CALE
	Datafile		ECD5-08231923
	Method		ECD5_AQUPEST_160111
24)	Sample	19	9H23034-CALF
	Datafile		ECD5-08231924
	Method		ECD5_AQUPEST_160111
25)	Sample	20	9H23034-CALG
	Datafile		ECD5-08231925
	Method		ECD5_AQUPEST_160111
26)	Sample	1	9H23034-IBL2
	Datafile		ECD5-08231926
	Method		ECD5_AQUPEST_160111
27)	Sample	21	9H23034-ICV2
	Datafile		ECD5-08231927
	Method		ECD5_AQUPEST_160111
28)	Sample	22	9H23034-CALH
	Datafile		ECD5-08231928
	Method		ECD5_AQUPEST_160111
29)	Sample	23	9H23034-CALI
	Datafile		ECD5-08231929
	Method		ECD5_AQUPEST_160111
30)	Sample	24	9H23034-CALJ
	Datafile		ECD5-08231930
	Method		ECD5_AQUPEST_160111
31)	Sample	25	9H23034-CALK
	Datafile		ECD5-08231931
	Method		ECD5_AQUPEST_160111
32)	Sample	26	9H23034-CALL
	Datafile		ECD5-08231932
	Method		ECD5_AQUPEST_160111
33)	Sample	27	9H23034-CALM
	Datafile		ECD5-08231933
	Method		ECD5_AQUPEST_160111
34)	Sample	1	9H23034-IBL3
	Datafile		ECD5-08231934
	Method		ECD5_AQUPEST_160111
35)	Sample	28	9H23034-ICV3
	Datafile		ECD5-08231935
	Method		ECD5_AQUPEST_160111
36)	Sample	29	9H23034-CALN
	Datafile		ECD5-08231936
	Method		ECD5_AQUPEST_160111
37)	Sample	30	9H23034-CALO
	Datafile		ECD5-08231937
	Method		ECD5_AQUPEST_160111
38)	Sample	31	9H23034-CALP
	Datafile		ECD5-08231938
	Method		ECD5_AQUPEST_160111
39)	Sample	32	9H23034-CALQ
	Datafile		ECD5-08231939
	Method		ECD5_AQUPEST_160111
40)	Sample	33	9H23034-CALR
	Datafile		ECD5-08231940
	Method		ECD5_AQUPEST_160111
41)	Sample	34	9H23034-CALS
	Datafile		ECD5-08231941
	Method		ECD5_AQUPEST_160111
42)	Sample	1	9H23034-IBL4
	Datafile		ECD5-08231942
	Method		ECD5_AQUPEST_160111
43)	Sample	35	9H23034-ICV4
	Datafile		ECD5-08231943
	Method		ECD5_AQUPEST_160111

Quantitation Report (QT Reviewed)

Data Path : C:\msdchem\4\data\2019-08\9H23034\  
 Data File : ECD5-08231904.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 12:24  
 Operator : MJB  
 Sample : 9H23034-BKD1  
 Misc : A19G138  
 ALS Vial : 2 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 23 12:40:24 2019  
 Quant Method : C:\msdchem\4\methods\PestBreakdownCHK\_190823.M  
 Quant Title : Pesticides  
 QLast Update : Thu Aug 21 11:53:22 2014  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Compound	R.T.	Response	Conc	Units
-----				
Target Compounds				
1) 4,4'-DDE	7.587	1120444	NoCal	ng/mL
2) Endrin	7.960	63253664	NoCal	ng/mL
3) 4,4'-DDD	8.007	6621952	NoCal	ng/mL
4) 4,4'-DDT	8.205	107029729	NoCal	ng/mL
5) Endrin Aldehyde	8.407	4202397	NoCal	ng/mL
6) Endrin Ketone	8.901	6297738	NoCal	ng/mL
8) 4,4'-DDE [2C]	8.347	1706439	NoCal	ng/mL
9) Endrin [2C]	8.719	95742281	NoCal	ng/mL
10) 4,4'-DDD [2C]	8.761	11347306	NoCal	ng/mL
11) Endrin Aldehyde [2C]	9.102	6529476	NoCal	ng/mL
12) 4,4'-DDT [2C]	8.988	167003448	NoCal	ng/mL
13) Endrin Ketone [2C]	9.690	10363842	NoCal	ng/mL
-----				

(f)=RT Delta > 1/2 Window



(m)=manual int.

*Break down the High MJB 8/26/19*  
*passing, but not maintenance performed*  
*MJB 8/26/19*

Quantitation Report (QT Reviewed)

Data Path : C:\msdchem\4\data\2019-08\9H23034\  
Data File : ECD5-08231904.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 12:24  
Operator : MJB  
Sample : 9H23034-BKD1  
Misc : A19G138  
ALS Vial : 2 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 23 12:40:24 2019  
Quant Method : C:\msdchem\4\methods\PestBreakdownCHK\_190823.M  
Quant Title : Pesticides  
QLast Update : Thu Aug 21 11:53:22 2014  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





Pesticide BKD

**Pesticide Breakdown Check (Validated 8/8/2013)**

Sequence: 9H23034 BKD2  
Data File: ECD5-08231906.D

First Column Area Counts		Percent Breakdown	
DDE	734891		
DDD	4530463		
DDT	125149199	<b>4.04</b>	<b>PASS</b>
Endrin	70846235	<b>8.91</b>	<b>PASS</b>
Endrin Aldehyde	2399187		
Endrin Ketone	4532548		

Second Column Area Counts		Percent Breakdown	
DDE	977816		
DDD	7819328		
DDT	188765825	<b>4.45</b>	<b>PASS</b>
Endrin	109289125	<b>8.73</b>	<b>PASS</b>
Endrin Aldehyde	3703608		
Endrin Ketone	6751447		

Breakdown must be less than 15% to accept sample data.

*MB 8/26/13*

Quantitation Report (QT Reviewed)

Data Path : C:\msdchem\4\data\2019-08\9H23034\  
 Data File : ECD5-08231906.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 13:16  
 Operator : MJB  
 Sample : 9H23034-BKD2  
 Misc : A19G138  
 ALS Vial : 2 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 23 13:30:06 2019  
 Quant Method : C:\msdchem\4\methods\PestBreakdownCHK\_190823.M  
 Quant Title : Pesticides  
 QLast Update : Thu Aug 21 11:53:22 2014  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Compound	R.T.	Response	Conc	Units
-----				
Target Compounds				
1) 4,4'-DDE	7.586	734891	NoCal	ng/mL
2) Endrin	7.960	70846235	NoCal	ng/mL
3) 4,4'-DDD	8.007	4530463	NoCal	ng/mL
4) 4,4'-DDT	8.205	125149199	NoCal	ng/mL
5) Endrin Aldehyde	8.407	2399187	NoCal	ng/mL
6) Endrin Ketone	8.902	4532548	NoCal	ng/mL
8) 4,4'-DDE [2C]	8.345	977816	NoCal	ng/mL
9) Endrin [2C]	8.718	109289125	NoCal	ng/mL
10) 4,4'-DDD [2C]	8.760	7819328	NoCal	ng/mL
11) Endrin Aldehyde [2C]	9.101	3703608	NoCal	ng/mL
12) 4,4'-DDT [2C]	8.988	188765825	NoCal	ng/mL
13) Endrin Ketone [2C]	9.690	6751447	NoCal	ng/mL

(f)=RT Delta > 1/2 Window



(m)=manual int.

*Swabbed in 1st w/  
Hexane.*

*MJP 8/26/19*

Data Path : C:\msdchem\4\data\2019-08\9H23034\  
Data File : ECD5-08231906.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 13:16  
Operator : MJB  
Sample : 9H23034-BKD2  
Misc : A19G138  
ALS Vial : 2 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 23 13:30:06 2019  
Quant Method : C:\msdchem\4\methods\PestBreakdownCHK\_190823.M  
Quant Title : Pesticides  
QLast Update : Thu Aug 21 11:53:22 2014  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231908.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 13:51  
 Operator : MJB  
 Sample : 9H23034-CAL1  
 Misc : A19E245, AB 1 ppb  
 ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:15:45 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 10:58:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*WJ  
8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.397	5.991	176748	300053	1.633	1.607
22) S DCBP (S)	9.593	10.541	163865	191572	1.202	1.206
Target Compounds						
2) a-BHC	5.937	6.597	231994	393119	1.665	1.296
3) g-BHC	6.221	6.915	207427	352286	1.380	1.170
4) b-BHC	6.300	6.980	104326	176262	1.760	1.450
5) Heptachlor	6.635	7.292	192066	309811	1.183	1.054
6) d-BHC	6.450	7.234	199840	349123	1.893	1.474
7) Aldrin	6.875	7.557	205523	317466	1.221	1.096
8) Heptachlo...	7.335	7.994	200503	310098	1.276	1.175
9) trans-Chl...	7.433	8.135	197202	364142	1.276	1.384
10) cis-Chlor...	7.528	8.241	209780	299422	1.367	1.179
11) Endosulfa...	7.625	8.291	185217	278874	1.245	1.173
12) 4,4'-DDE	7.586	8.346	193435	298463	1.647	1.374
13) Dieldrin	7.796	8.491	197721	296684	1.194	1.095
14) Endrin	7.961	8.718	156412	222882	1.190	1.096
15) 4,4'-DDD	8.007	8.760	164956	251549	1.683	1.281
16) Endosulfa...	8.118	8.865	158139	232156	1.378	1.183
17) 4,4'-DDT	8.205	8.986	113897	179700	1.686	1.607
18) Endrin Al...	8.407	9.101	241285	348624	2.337	2.034
19) Endosulfa...	8.708	9.292	176097	265797	1.418	1.337
20) Methoxychlor	8.543	9.466	59659	95155	1.698	1.611
21) Endrin Ke...	8.901	9.690	177552	255763	1.293	1.268
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlorane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231908.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 13:51  
Operator : MJB  
Sample : 9H23034-CAL1  
Misc : A19E245, AB 1 ppb  
ALS Vial : 4 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:15:45 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 10:58:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231909.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 14:08  
 Operator : MJB  
 Sample : 9H23034-CAL2  
 Misc : A19E246, AB 2 ppb  
 ALS Vial : 5 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:16:21 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 10:58:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.396	5.990	349972	600766	3.233	3.230
22) S DCBP (S)	9.593	10.542	309904	390006	2.547	2.456
Target Compounds						
2) a-BHC	5.936	6.597	458365	784586	3.177	2.540
3) g-BHC	6.220	6.915	406027	690922	2.702	2.295
4) b-BHC	6.300	6.980	194168	335260	3.275	2.757
5) Heptachlor	6.635	7.291	369615	586765	2.276	1.995
6) d-BHC	6.450	7.233	386980	669122	3.575	2.783
7) Aldrin	6.875	7.556	399550	635458	2.375	2.194
8) Heptachlo...	7.335	7.993	392052	606240	2.495	2.296
9) trans-Chl...	7.432	8.135	382271	644454	2.473	2.449
10) cis-Chlor...	7.527	8.241	389999	579667	2.541	2.282
11) Endosulfa...	7.625	8.291	357368	540442	2.402	2.273
12) 4,4'-DDE	7.586	8.345	388618	598066	3.268	2.709
13) Dieldrin	7.796	8.491	395728	583812	2.390	2.154
14) Endrin	7.960	8.718	298515	424889	2.271	2.149
15) 4,4'-DDD	8.006	8.760	314622	488120	3.236	2.486
16) Endosulfa...	8.118	8.864	299106	462256	2.607	2.355
17) 4,4'-DDT	8.204	8.986	218190	341782	3.052	2.875
18) Endrin Al...	8.407	9.101	328182	477694	3.179	2.786
19) Endosulfa...	8.707	9.291	322163	498767	2.595	2.558
20) Methoxychlor	8.542	9.465	111466	178074	3.136	2.980
21) Endrin Ke...	8.901	9.689	331269	493110	2.413	2.461
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

MJB  
8/26/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231909.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 14:08  
Operator : MJB  
Sample : 9H23034-CAL2  
Misc : A19E246, AB 2 ppb  
ALS Vial : 5 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:16:21 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 10:58:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231910.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 14:25  
 Operator : MJB  
 Sample : 9H23034-CAL3  
 Misc : A19E247, AB 5 ppb  
 ALS Vial : 6 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:16:57 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Mon Aug 26 10:58:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.396	5.990	834206	1437876	7.707	7.700
22) S DCBP (S)	9.594	10.542	701050	870921	6.146	5.485
Target Compounds						
2) a-BHC	5.937	6.597	1147932	1985438	7.742	6.328
3) g-BHC	6.220	6.915	1020724	1742677	6.792	5.790
4) b-BHC	6.300	6.980	456954	788630	7.708	6.486
5) Heptachlor	6.635	7.291	899091	1508218	5.537	5.129
6) d-BHC	6.449	7.233	1004012	1717450	9.061	7.030
7) Aldrin	6.875	7.556	1012733	1600995	6.019	5.528
8) Heptachlo...	7.335	7.994	923620	1455941	5.877	5.514
9) trans-Chl...	7.432	8.134	926577	1502119	5.993	5.707
10) cis-Chlor...	7.528	8.241	908795	1434855	5.922	5.649
11) Endosulfa...	7.624	8.290	861509	1327191	5.790	5.583
12) 4,4'-DDE	7.586	8.345	953351	1487999	7.901	6.642
13) Dieldrin	7.796	8.491	972009	1462538	5.870	5.397
14) Endrin	7.960	8.718	738953	1092877	5.622	5.608
15) 4,4'-DDD	8.007	8.759	790498	1208642	8.130	6.156
16) Endosulfa...	8.118	8.865	709544	1096359	6.185	5.586
17) 4,4'-DDT	8.205	8.986	553009	873653	7.371	6.957
18) Endrin Al...	8.407	9.101	683393	1045869	6.620	6.101
19) Endosulfa...	8.708	9.291	768798	1175908	6.192	6.083
20) Methoxychlor	8.542	9.466	270388	413802	7.493	6.808
21) Endrin Ke...	8.901	9.689	811384	1205004	5.910	6.014
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlorane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231910.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 14:25  
Operator : MJB  
Sample : 9H23034-CAL3  
Misc : A19E247, AB 5 ppb  
ALS Vial : 6 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:16:57 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 10:58:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231911.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 14:42  
 Operator : MJB  
 Sample : 9H23034-CAL4  
 Misc : A19E249, AB 10 ppb  
 ALS Vial : 7 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:19:05 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 10:58:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB*  
*8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.396	5.990	1644447	2865854	15.193	15.177
22) S DCBP (S)	9.593	10.541	1335468	1678728	11.976	10.572
Target Compounds						
2) a-BHC	5.936	6.597	2347065	4095890	15.530	12.883
3) g-BHC	6.220	6.915	2034859	3476733	13.541	11.551
4) b-BHC	6.299	6.980	910875	1580847	15.365	13.002
5) Heptachlor	6.634	7.291	1819621	3005915	11.206	10.223
6) d-BHC	6.449	7.234	2006493	3613517	17.784	14.564
7) Aldrin	6.875	7.556	2010802	3341093	11.950	11.536
8) Heptachlo...	7.335	7.994	1865428	2959301	11.869	11.208
9) trans-Chl...	7.431	8.134	1847996	3002782	11.953	11.409
10) cis-Chlor...	7.527	8.241	1843346	2859573	12.012	11.257
11) Endosulfa...	7.623	8.291	1709332	2724272	11.438	11.460
12) 4,4'-DDE	7.585	8.346	1890931	3049792	15.482	13.444
13) Dieldrin	7.795	8.491	1954890	2898866	11.805	10.697
14) Endrin	7.960	8.718	1475508	2244483	11.225	11.476
15) 4,4'-DDD	8.006	8.760	1565974	2425496	15.969	12.353
16) Endosulfa...	8.117	8.864	1448080	2243610	12.623	11.432
17) 4,4'-DDT	8.204	8.987	1146556	1841119	14.788	14.109
18) Endrin Al...	8.406	9.101	1375129	2125028	13.321	12.396
19) Endosulfa...	8.707	9.292	1553540	2424584	12.512	12.489
20) Methoxychlor	8.542	9.465	561706	883069	15.275	14.167
21) Endrin Ke...	8.900	9.689	1664380	2496985	12.124	12.365
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlorthane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231911.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 14:42  
Operator : MJB  
Sample : 9H23034-CAL4  
Misc : A19E249, AB 10 ppb  
ALS Vial : 7 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:19:05 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 10:58:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231912.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 15:00  
 Operator : MJB  
 Sample : 9H23034-CAL5  
 Misc : A19E250, AB 25 ppb  
 ALS Vial : 8 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:19:37 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Mon Aug 26 10:58:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.394	5.989	4015832	7072923	37.101	36.221
22) S DCBP (S)	9.592	10.539	3342634	4163229	30.365	26.219
Target Compounds						
2) a-BHC	5.935	6.596	5553096	9910863	35.515	30.324
3) g-BHC	6.218	6.913	4875657	8508386	32.445	28.267
4) b-BHC	6.297	6.978	2060378	3677155	34.755	30.244
5) Heptachlor	6.633	7.289	4314306	7282282	26.568	24.766
6) d-BHC	6.447	7.232	4667166	8247775	39.910	32.244
7) Aldrin	6.873	7.555	4845355	7878574	28.797	27.203
8) Heptachlo...	7.332	7.992	4344286	7064729	27.642	26.758
9) trans-Chl...	7.429	8.131	4401456	7157480	28.469	27.194
10) cis-Chlor...	7.525	8.239	4244413	6935857	27.657	27.304
11) Endosulfa...	7.621	8.288	4111285	6571512	27.630	27.643
12) 4,4'-DDE	7.583	8.343	4571066	7501047	36.397	32.167
13) Dieldrin	7.792	8.489	4582306	7333890	27.672	27.063
14) Endrin	7.957	8.716	3508904	5325883	26.694	26.642
15) 4,4'-DDD	8.004	8.758	3727035	6146469	37.001	31.304
16) Endosulfa...	8.115	8.862	3371864	5447602	29.393	27.758
17) 4,4'-DDT	8.202	8.984	2924467	4480388	35.460	32.123
18) Endrin Al...	8.404	9.099	3119767	4848504	30.221	28.282
19) Endosulfa...	8.705	9.289	3645411	5978906	29.360	30.102
20) Methoxychlor	8.540	9.463	1390283	2166659	36.145	32.800
21) Endrin Ke...	8.899	9.688	4008958	5893691	29.202	28.514
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231912.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 15:00  
Operator : MJB  
Sample : 9H23034-CAL5  
Misc : A19E250, AB 25 ppb  
ALS Vial : 8 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:19:37 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 10:58:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231913.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 15:17  
 Operator : MJB  
 Sample : 9H23034-CAL6  
 Misc : A19H383, AB 50 ppb  
 ALS Vial : 9 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 10:58:12 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Wed Aug 07 17:49:44 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.394	5.989	8071481	14196745	74.571	69.077
22) S DCBP (S)	9.592	10.541	6678990	8730692	60.740	54.984
Target Compounds						
2) a-BHC	5.935	6.596	11369592	20265817	69.154	59.445
3) g-BHC	6.218	6.914	9785999	17381069	65.120	57.745
4) b-BHC	6.296	6.978	4100858	7516011	69.174	61.818
5) Heptachlor	6.632	7.290	8735158	14595143	53.793	49.636
6) d-BHC	6.447	7.232	9610742	17311258	77.761	64.308
7) Aldrin	6.873	7.555	9327672	16264416	55.436	56.158
8) Heptachlo...	7.332	7.992	8869300	14837794	56.484	56.198
9) trans-Chl...	7.428	8.131	8959305	14678719	57.950	55.771
10) cis-Chlor...	7.524	8.238	8622674	14002116	56.187	55.122
11) Endosulfa...	7.621	8.289	7984410	13712329	53.659	57.680
12) 4,4'-DDE	7.583	8.344	9177389	15554706	70.089	63.904
13) Dieldrin	7.792	8.489	9386664	15434113	56.685	56.955
14) Endrin	7.957	8.716	6979572	11015379	53.097	52.880
15) 4,4'-DDD	8.004	8.758	7726197	13159451	73.239	67.021
16) Endosulfa...	8.114	8.863	6840920	11534525	59.632	58.774
17) 4,4'-DDT	8.202	8.985	6205369	9285492	69.085	60.834
18) Endrin Al...	8.404	9.099	6224451	10209034	60.296	59.551
19) Endosulfa...	8.705	9.289	7420576	12149289	59.766	58.797
20) Methoxychlor	8.540	9.464	2860683	4346199	69.570	60.726
21) Endrin Ke...	8.899	9.687	8190707	12954568	59.663	59.905
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231913.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 15:17  
Operator : MJB  
Sample : 9H23034-CAL6  
Misc : A19H383, AB 50 ppb  
ALS Vial : 9 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 10:58:12 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Wed Aug 07 17:49:44 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231914.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 15:34  
 Operator : MJB  
 Sample : 9H23034-CAL7  
 Misc : A19H382, AB 100 ppb  
 ALS Vial : 10 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:20:14 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Mon Aug 26 10:58:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB 8/26/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.395	5.989	15850922	29256334	146.444	130.224
22) S DCBP (S)	9.592	10.540	13405396	17784069	121.277	111.999
Target Compounds						
2) a-BHC	5.935	6.596	22363584	41699210	125.842	113.668
3) g-BHC	6.218	6.914	19595093	36788994	130.394	122.224
4) b-BHC	6.296	6.977	8355416	14625175	140.940	120.290
5) Heptachlor	6.632	7.289	17551528	30277818	108.086	102.970
6) d-BHC	6.446	7.232	19475580	35176633	144.149	120.302
7) Aldrin	6.872	7.555	19108074	33906422	113.562	117.072
8) Heptachlo...	7.331	7.991	17318444	30045511	110.195	113.798
9) trans-Chl...	7.427	8.131	17732791	30742272	114.698	116.803
10) cis-Chlor...	7.523	8.238	16742584	29042863	109.098	114.333
11) Endosulfa...	7.619	8.288	16089996	27212707	108.133	114.469
12) 4,4'-DDE	7.582	8.344	18052552	32499603	128.779	123.812
13) Dieldrin	7.791	8.488	18324422	31001958	110.659	114.403
14) Endrin	7.957	8.715	13812708	23102413	105.080	102.828
15) 4,4'-DDD	8.003	8.758	15437146	26297484	135.694	133.933
16) Endosulfa...	8.113	8.861	13543500	23016371	118.059	117.279
17) 4,4'-DDT	8.201	8.984	12176961	19789501	120.685	112.516
18) Endrin Al...	8.403	9.098	12363806	20502737	119.767	119.596
19) Endosulfa...	8.704	9.289	14366789	24477320	115.711	110.592
20) Methoxychlor	8.539	9.463	5877329	9444987	128.396	114.860
21) Endrin Ke...	8.898	9.687	16251943	26636559	118.383	114.357
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlorane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231914.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 15:34  
Operator : MJB  
Sample : 9H23034-CAL7  
Misc : A19H382, AB 100 ppb  
ALS Vial : 10 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:20:14 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 10:58:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231915.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 15:52  
 Operator : MJB  
 Sample : 9H23034-CAL8  
 Misc : A19E244, AB 200 ppb  
 ALS Vial : 11 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:20:45 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 10:58:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB*  
*8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	5.394	5.990	32842535	62584449	303.426	241.228
22) S DCBP (S)	9.591	10.539	26975231	38097779	240.687	239.829
Target Compounds						
2) a-BHC	5.935	6.597	47202252	94376748	232.879	224.790
3) g-BHC	6.218	6.914	41889726	80765680	278.753	268.327
4) b-BHC	6.294	6.977	18238696	32553433	307.652	267.747
5) Heptachlor	6.630	7.289	37785699	71283176	232.692	242.422
6) d-BHC	6.445	7.232	41016592	80979751	263.399	237.546
7) Aldrin	6.870	7.554	39838403	73228186	236.765	252.843
8) Heptachlo...	7.330	7.991	36258170	65330070	230.706	247.439
9) trans-Chl...	7.425	8.130	37621413	66447972	243.340	252.464
10) cis-Chlor...	7.521	8.238	35207945	63977063	229.421	251.859
11) Endosulfa...	7.618	8.288	33852593	61043507	227.507	256.777
12) 4,4'-DDE	7.581	8.344	38763081	69842351	244.719	234.608
13) Dieldrin	7.791	8.489	39217772	70031781	236.831	258.430
14) Endrin	7.955	8.715	31426311	52779585	239.075	204.455
15) 4,4'-DDD	8.002	8.758	32436804	59560270	251.258	303.340
16) Endosulfa...	8.112	8.862	29471042	51834888	256.899	264.124
17) 4,4'-DDT	8.200	8.984	29075222	48203441	232.877	216.675
18) Endrin Al...	8.402	9.098	26627672	45084544	257.940	262.986
19) Endosulfa...	8.704	9.289	31126520	54592794	250.696	216.937
20) Methoxychlor	8.537	9.463	14271143	23714100	255.612	227.264
21) Endrin Ke...	8.898	9.688	35094718	60861376	255.639	227.431
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlorthane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231915.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 15:52  
Operator : MJB  
Sample : 9H23034-CAL8  
Misc : A19E244, AB 200 ppb  
ALS Vial : 11 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:20:45 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 10:58:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231918.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 16:44  
 Operator : MJB  
 Sample : 9H23034-CAL9  
 Misc : A19E272, 9-42 1 ppb  
 ALS Vial : 13 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:23:34 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	3.198	3.687	198207	383198	1.330	1.219
24) Hexachlor...	5.775	6.453	194679	328025	1.585	1.463
25) Oxychlordane	7.263	7.922	176844	279143	1.364	1.326
26) 2,4'-DDE	7.335	8.123	137947	219164	1.468	1.405
27) trans-Non...	7.518	8.195	236836	306202	1.652	1.333
28) 2,4'-DDD	7.707	8.495	120240	192040	1.439	1.409
29) 2,4'-DDT	7.890	8.719	107110	173338	1.500	1.372
30) cis-Nonac...	7.987	8.759	219220	332745	1.362	1.310
31) Mirex	8.655	9.680	147356	209783	1.505	1.458
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231918.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 16:44  
Operator : MJB  
Sample : 9H23034-CAL9  
Misc : A19E272, 9-42 1 ppb  
ALS Vial : 13 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:23:34 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231919.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 17:01  
 Operator : MJB  
 Sample : 9H23034-CALA  
 Misc : A19E273, 9-42 2 ppb  
 ALS Vial : 14 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:24:10 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB 8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	3.198	3.687	375794	754548	2.521	2.400
24) Hexachlor...	5.775	6.453	362082	632830	2.948	2.823
25) Oxychlordane	7.262	7.921	339370	541023	2.617	2.571
26) 2,4'-DDE	7.334	8.123	265212	411812	2.822	2.639
27) trans-Non...	7.518	8.194	415126	587765	2.896	2.559
28) 2,4'-DDD	7.707	8.495	233089	373596	2.789	2.741
29) 2,4'-DDT	7.889	8.718	204209	332170	2.725	2.614
30) cis-Nonac...	7.986	8.758	423442	624783	2.632	2.460
31) Mirex	8.655	9.680	266770	388199	2.725	2.697
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231919.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 17:01  
Operator : MJB  
Sample : 9H23034-CALA  
Misc : A19E273, 9-42 2 ppb  
ALS Vial : 14 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:24:10 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231920.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 17:18  
 Operator : MJB  
 Sample : 9H23034-CALB  
 Misc : A19E274, 9-42 5 ppb  
 ALS Vial : 15 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:24:43 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	3.198	3.687	959211	1877484	6.435	5.971
24) Hexachlor...	5.775	6.453	853793	1485583	6.951	6.626
25) Oxychlordane	7.262	7.921	819748	1325543	6.321	6.298
26) 2,4'-DDE	7.334	8.123	633168	1029687	6.738	6.600
27) trans-Non...	7.518	8.194	933222	1467723	6.510	6.390
28) 2,4'-DDD	7.705	8.495	560942	898697	6.711	6.593
29) 2,4'-DDT	7.889	8.719	536967	873074	6.892	6.802
30) cis-Nonac...	7.986	8.759	1025899	1587243	6.376	6.249
31) Mirex	8.654	9.679	628618	895523	6.422	6.222
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231920.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 17:18  
Operator : MJB  
Sample : 9H23034-CALB  
Misc : A19E274, 9-42 5 ppb  
ALS Vial : 15 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:24:43 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231921.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 17:35  
 Operator : MJB  
 Sample : 9H23034-CALC  
 Misc : A19E275, 9-42 10 ppb  
 ALS Vial : 16 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:25:17 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB 8/26/19


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	3.198	3.687	1838187	3701532	12.333	11.773
24) Hexachlor...	5.774	6.453	1711884	2936294	13.936	13.097
25) Oxychlordane	7.261	7.921	1591613	2538903	12.272	12.063
26) 2,4'-DDE	7.333	8.122	1245265	2018331	13.252	12.936
27) trans-Non...	7.516	8.194	1817552	2844404	12.679	12.384
28) 2,4'-DDD	7.705	8.495	1103587	1778790	13.203	13.050
29) 2,4'-DDT	7.888	8.719	1051565	1702568	13.249	13.099
30) cis-Nonac...	7.986	8.759	2032010	3148054	12.629	12.394
31) Mirex	8.654	9.679	1196365	1722960	12.222	11.971
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231921.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 17:35  
Operator : MJB  
Sample : 9H23034-CALC  
Misc : A19E275, 9-42 10 ppb  
ALS Vial : 16 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:25:17 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231922.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 17:53  
 Operator : MJB  
 Sample : 9H23034-CALD  
 Misc : A19E276, 9-42 25 ppb  
 ALS Vial : 17 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:25:49 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	3.198	3.687	4363988	8892238	29.278	28.282
24) Hexachlor...	5.774	6.453	4184551	7416324	34.066	33.080
25) Oxychlordane	7.261	7.920	3881255	6202791	29.926	29.471
26) 2,4'-DDE	7.333	8.122	3059421	4999232	32.558	32.042
27) trans-Non...	7.516	8.194	4391046	7092288	30.631	30.877
28) 2,4'-DDD	7.705	8.495	2745178	4389185	32.844	32.200
29) 2,4'-DDT	7.888	8.719	2728794	4405554	33.278	32.676
30) cis-Nonac...	7.986	8.759	4993110	8219393	31.032	32.361
31) Mirex	8.654	9.679	2910818	4138115	29.738	28.753
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231922.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 17:53  
Operator : MJB  
Sample : 9H23034-CALD  
Misc : A19E276, 9-42 25 ppb  
ALS Vial : 17 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:25:49 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231923.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 18:10  
 Operator : MJB  
 Sample : 9H23034-CALE  
 Misc : A19E154, 9-42 50 ppb  
 ALS Vial : 18 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:22:32 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 10:58:24 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	3.198	3.688	8761747	18635615	58.783	59.271
24) Hexachlor...	5.774	6.454	8911624	16094159	72.549	71.786
25) Oxychlordane	7.261	7.920	8382873	14172543	64.636	67.337
26) 2,4'-DDE	7.333	8.122	6510588	11006400	69.284	70.544
27) trans-Non...	7.516	8.194	9581794	15807712	66.841	68.821
28) 2,4'-DDD	7.705	8.495	5920095	9924934	70.829	72.811
29) 2,4'-DDT	7.888	8.718	5687323	8810591	66.398	62.033
30) cis-Nonac...	7.985	8.758	10616019	17721229	65.978	69.771
31) Mirex	8.652	9.679	6218341	9100959	67.528	63.235
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231923.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 18:10  
Operator : MJB  
Sample : 9H23034-CALE  
Misc : A19E154, 9-42 50 ppb  
ALS Vial : 18 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:22:32 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 10:58:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231924.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 18:27  
 Operator : MJB  
 Sample : 9H23034-CALF  
 Misc : A19E155, 9-42 100 ppb  
 ALS Vial : 19 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:26:27 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB 8/26/19

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	3.199	3.690	17952134	39298885	120.443	124.991
24) Hexachlor...	5.776	6.455	17670025	32766708	143.851	146.152
25) Oxychlordane	7.261	7.922	16359215	29732149	126.137	141.263
26) 2,4'-DDE	7.334	8.123	12769067	22164400	135.886	142.059
27) trans-Non...	7.516	8.195	18351251	31975271	128.015	139.210
28) 2,4'-DDD	7.705	8.496	11587554	20118925	138.635	147.597
29) 2,4'-DDT	7.888	8.721	11771354	18998968	127.689	121.350
30) cis-Nonac...	7.986	8.760	20932641	36072644	130.096	142.024
31) Mirex	8.653	9.680	11960753	19363200	122.194	134.540
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231924.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 18:27  
Operator : MJB  
Sample : 9H23034-CALF  
Misc : A19E155, 9-42 100 ppb  
ALS Vial : 19 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:26:27 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231925.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 18:45  
 Operator : MJB  
 Sample : 9H23034-CALG  
 Misc : A19E271, 9-42 200 ppb  
 ALS Vial : 20 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:27:05 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB*  
*8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	3.199	3.689	34166533	75988565	229.227	241.683
24) Hexachlor...	5.774	6.454	34073459	66261966	277.392	295.553
25) Oxychlordane	7.258	7.920	32032634	58736982	246.986	279.071
26) 2,4'-DDE	7.331	8.122	24819199	44504592	264.121	285.245
27) trans-Non...	7.514	8.194	35027918	63083636	244.348	274.645
28) 2,4'-DDD	7.703	8.494	21916962	39839303	262.217	292.269
29) 2,4'-DDT	7.887	8.719	23024956	39999231	224.761	221.024
30) cis-Nonac...	7.984	8.759	40046185	72455823	248.887	285.271
31) Mirex	8.652	9.679	23284997	38425530	237.885	266.989
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231925.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 18:45  
Operator : MJB  
Sample : 9H23034-CALG  
Misc : A19E271, 9-42 200 ppb  
ALS Vial : 20 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:27:05 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231928.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 19:36  
 Operator : MJB  
 Sample : 9H23034-CALH  
 Misc : A19F232, CHLOR 50 ppb  
 ALS Vial : 22 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:31:56 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:29:20 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJP 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	7.429	8.131	1009143	1754707	65.443	66.784
33) Chlordane...	7.521	8.237	1286655	1472400	62.192	67.669
34) Chlordane...	8.068	8.897	288087	439020	60.282	67.059
35) Chlordane...	3.446	0.000	5365	0	NoCal	N.D.
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231928.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 19:36  
Operator : MJB  
Sample : 9H23034-CALH  
Misc : A19F232, CHLOR 50 ppb  
ALS Vial : 22 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:31:56 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:29:20 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231929.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 19:54  
 Operator : MJB  
 Sample : 9H23034-CALI  
 Misc : A19F233, CHLOR 100 ppb  
 ALS Vial : 23 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:32:31 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:29:20 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	7.429	8.130	1978897	3378388	128.331	127.866
33) Chlordane...	7.521	8.238	2519520	2905941	121.784	133.934
34) Chlordane...	8.068	8.898	548196	874465	114.710	133.920
35) Chlordane...	3.446	0.000	4938	0	NoCal	N.D.
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231929.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 19:54  
Operator : MJB  
Sample : 9H23034-CALI  
Misc : A19F233, CHLOR 100 ppb  
ALS Vial : 23 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:32:31 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:29:20 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231930.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 20:11  
 Operator : MJB  
 Sample : 9H23034-CALJ  
 Misc : A19F234, CHLOR 200 ppb  
 ALS Vial : 24 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:33:08 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:29:20 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	7.429	8.131	3849299	6751197	249.627	251.318
33) Chlordane...	7.522	8.239	4906320	5883615	237.153	267.927
34) Chlordane...	8.069	8.898	1101677	1731727	230.526	261.800
35) Chlordane...	3.448	0.000	4503	0	NoCal	N.D.
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231930.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 20:11  
Operator : MJB  
Sample : 9H23034-CALJ  
Misc : A19F234, CHLOR 200 ppb  
ALS Vial : 24 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:33:08 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:29:20 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231931.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 20:28  
 Operator : MJB  
 Sample : 9H23034-CALK  
 Misc : A19F235, CHLOR 500 ppb  
 ALS Vial : 25 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:28:33 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
4/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	7.427	8.129	9628671	17830433	624.419	629.093
33) Chlordane...	7.520	8.237	12176524	14812273	588.567	644.287
34) Chlordane...	8.067	8.896	2921278	4271709	611.277	615.748
35) Chlordane...	3.447	0.000	4056	0	NoCal	N.D.
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231931.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 20:28  
Operator : MJB  
Sample : 9H23034-CALK  
Misc : A19F235, CHLOR 500 ppb  
ALS Vial : 25 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:28:33 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231932.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 20:45  
 Operator : MJB  
 Sample : 9H23034-CALL  
 Misc : A19F236, CHLOR 1000 ppb  
 ALS Vial : 26 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:33:36 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:22:42 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	7.426	8.130	19643766	37966746	1273.898	1234.450
33) Chlordane...	7.519	8.237	25083239	31493677	1212.428	1269.749
34) Chlordane...	8.067	8.897	5987927	9358900	1252.974	1240.988
35) Chlordane...	3.447	0.000	4825	0	NoCal	N.D.
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231932.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 20:45  
Operator : MJB  
Sample : 9H23034-CALL  
Misc : A19F236, CHLOR 1000 ppb  
ALS Vial : 26 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:33:36 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:22:42 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231933.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 21:02  
 Operator : MJB  
 Sample : 9H23034-CALM  
 Misc : A19F231, CHLOR 2000 ppb  
 ALS Vial : 27 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:34:12 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:29:20 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB 8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	7.426	8.130	40036500	81691713	2596.366	2326.014
33) Chlordane...	7.519	8.238	50979142	66281388	2464.138	2365.956
34) Chlordane...	8.067	8.897	12208306	19418517	2554.588	2271.661
35) Chlordane...	3.449	0.000	4939	0	NoCal	N.D.
36) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
37) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
38) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
39) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
40) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
41) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d
42) Toxaphene...	0.000	0.000	0	0	N.D. d	N.D. d

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231933.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:02  
Operator : MJB  
Sample : 9H23034-CALM  
Misc : A19F231, CHLOR 2000 ppb  
ALS Vial : 27 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:34:12 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:29:20 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231936.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 21:54  
 Operator : MJB  
 Sample : 9H23034-CALN  
 Misc : A19D122, TOX 50 ppb  
 ALS Vial : 29 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:37:48 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:36:51 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	7.506	8.466	49250	136848	69.167m	65.864
37) Toxaphene...	7.794	8.813	88321	164706	67.251	67.260
38) Toxaphene...	8.105	8.847	169381	254833	62.397	67.028
39) Toxaphene...	8.346	8.915	164317	416348	64.716	65.275
40) Toxaphene...	8.573	9.091	114720	233185	60.554	65.984
41) Toxaphene...	8.641	9.470	153138	230922	57.297	70.513
42) Toxaphene...	3.449	0.000	4023	0	NoCal	N.D.


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.



Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231936.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:54  
Operator : MJB  
Sample : 9H23034-CALN  
Misc : A19D122, TOX 50 ppb  
ALS Vial : 29 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:37:09 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(36) Toxaphene (1)  
7.506min 69.167 ng/mL(m)  
response 49250


*MJB 8/26/19*

(36) Toxaphene (1) #2  
8.466min 65.864 ng/mL  
response 136848

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231936.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:54  
Operator : MJB  
Sample : 9H23034-CALN  
Misc : A19D122, TOX 50 ppb  
ALS Vial : 29 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:37:09 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped





~~(36) Toxaphene (1)  
7.518min 96.999 ng/mL  
response 69068~~

*MJB 6/26/19*

(36) Toxaphene (1) #2  
8.466min 65.864 ng/mL  
response 136848

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231936.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 21:54  
Operator : MJB  
Sample : 9H23034-CALN  
Misc : A19D122, TOX 50 ppb  
ALS Vial : 29 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:37:48 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231937.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 22:11  
 Operator : MJB  
 Sample : 9H23034-CALO  
 Misc : A19D123, TOX 100 ppb  
 ALS Vial : 30 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:38:53 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:36:51 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	7.501	8.466	91576	267534	128.609m	128.761
37) Toxaphene...	7.795	8.813	166085	324070	126.462	132.338
38) Toxaphene...	8.106	8.848	332842	494430	122.613	130.048
39) Toxaphene...	8.346	8.915	320313	811948	126.154	127.297
40) Toxaphene...	8.574	9.091	228960	452209	120.854	127.962
41) Toxaphene...	8.641	9.471	302577	452485	113.210	135.226
42) Toxaphene...	3.450	0.000	3536	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231937.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:11  
Operator : MJB  
Sample : 9H23034-CALO  
Misc : A19D123, TOX 100 ppb  
ALS Vial : 30 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:38:11 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(36) Toxaphene (1)

7.501min 128.609 ng/mL m  
response 91576

*MJB 8/26/19*


(36) Toxaphene (1) #2

8.466min 128.761 ng/mL  
response 267534

Quantitation Report (Qedit)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231937.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:11  
Operator : MJB  
Sample : 9H23034-CALO  
Misc : A19D123, TOX 100 ppb  
ALS Vial : 30 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:38:11 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



(36) Toxaphene (1)  
7.517min 130.814 ng/mL  
response 93146



*MJB 8/26/19*

(36) Toxaphene (1) #2  
8.466min 128.761 ng/mL  
response 267534

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231937.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:11  
Operator : MJB  
Sample : 9H23034-CALO  
Misc : A19D123, TOX 100 ppb  
ALS Vial : 30 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:38:53 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231938.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 22:28  
 Operator : MJB  
 Sample : 9H23034-CALP  
 Misc : A19D124, TOX 200 ppb  
 ALS Vial : 31 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:39:29 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:36:51 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlorthane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	7.502	8.466	176047	508983	247.240	244.968
37) Toxaphene...	7.795	8.812	317587	645322	241.821	263.525
38) Toxaphene...	8.105	8.847	644464	995555	237.409	261.857
39) Toxaphene...	8.346	8.914	632351	1580436	249.049	247.779
40) Toxaphene...	8.574	9.090	454431	895397	239.867	253.371
41) Toxaphene...	8.640	9.469	597991	905244	223.740	263.952
42) Toxaphene...	3.451	0.000	3919	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.



Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231938.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:28  
Operator : MJB  
Sample : 9H23034-CALP  
Misc : A19D124, TOX 200 ppb  
ALS Vial : 31 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:39:29 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231939.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 22:45  
 Operator : MJB  
 Sample : 9H23034-CALQ  
 Misc : A19D125, TOX 500 ppb  
 ALS Vial : 32 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:36:29 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualeCD5  
 QLast Update : Mon Aug 26 11:29:20 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

MJB  
8/26/19



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	7.502	8.466	441826	1308994	620.497	630.004
37) Toxaphene...	7.794	8.812	819454	1647741	623.958	672.874
38) Toxaphene...	8.105	8.848	1677481	2475022	617.954	650.997
39) Toxaphene...	8.346	8.915	1649569	4252640	649.677	666.725
40) Toxaphene...	8.574	9.091	1221560	2340668	644.788	662.340
41) Toxaphene...	8.640	9.470	1623402	2369795	607.400	652.719
42) Toxaphene...	3.450	0.000	4132	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231939.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 22:45  
Operator : MJB  
Sample : 9H23034-CALQ  
Misc : A19D125, TOX 500 ppb  
ALS Vial : 32 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:36:29 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:29:20 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

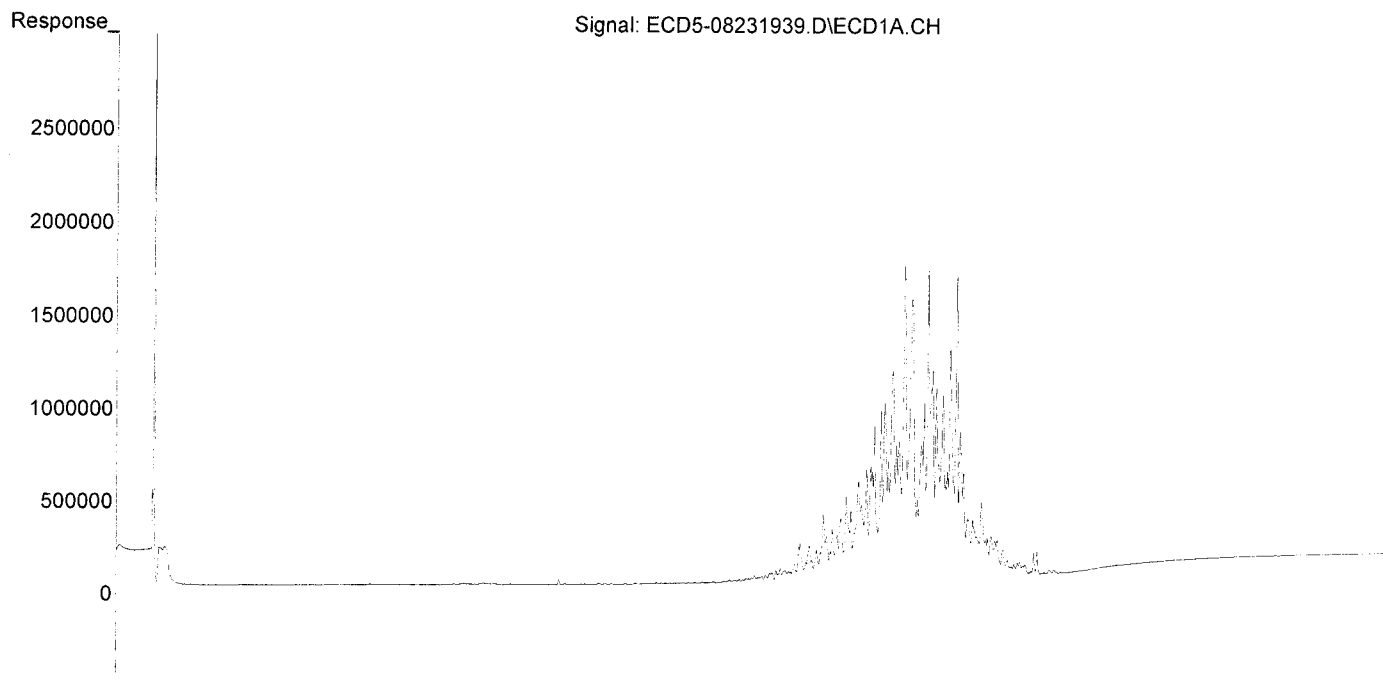

Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231940.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 23:03  
 Operator : MJB  
 Sample : 9H23034-CALR  
 Misc : A19D126, TOX 1000 ppb  
 ALS Vial : 33 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:40:10 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:36:51 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB*  
*4/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	7.501	8.467	871889	2654886	1224.474	1277.768
37) Toxaphene...	7.793	8.813	1556013	3384036	1184.797	1381.910
38) Toxaphene...	8.105	8.848	3495877	5168269	1287.817	1359.392
39) Toxaphene...	8.345	8.915	3287014	8650068	1294.579	1356.150
40) Toxaphene...	8.573	9.091	2546293	4900430	1344.035	1386.677
41) Toxaphene...	8.640	9.470	3406737	5046645	1274.639	1281.306
42) Toxaphene...	3.451	0.000	2687	0	NoCal	N.D.

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231940.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 23:03  
Operator : MJB  
Sample : 9H23034-CALR  
Misc : A19D126, TOX 1000 ppb  
ALS Vial : 33 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:40:10 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



Data Path : R:\data\2019-08\9H23034\  
 Data File : ECD5-08231941.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 23 Aug 2019 23:20  
 Operator : MJB  
 Sample : 9H23034-CALS  
 Misc : A19D121, TOX 2000 ppb  
 ALS Vial : 34 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
 Integration File signal 2: PEST2.e  
 Quant Time: Aug 26 11:40:44 2019  
 Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
 Quant Title : Instrument: DualECD5  
 QLast Update : Mon Aug 26 11:36:51 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

*MJB 8/26/19*



Compound	RT#1	RT#2	Resp#1	Resp#2	ng/mL	ng/mL
-----						
System Monitoring Compounds						
1) S TCMX (S)	0.000	0.000	0	0	N.D. d	N.D. d
22) S DCBP (S)	0.000	0.000	0	0	N.D. d	N.D. d
Target Compounds						
2) a-BHC	0.000	0.000	0	0	N.D. d	N.D. d
3) g-BHC	0.000	0.000	0	0	N.D. d	N.D. d
4) b-BHC	0.000	0.000	0	0	N.D. d	N.D. d
5) Heptachlor	0.000	0.000	0	0	N.D. d	N.D. d
6) d-BHC	0.000	0.000	0	0	N.D. d	N.D. d
7) Aldrin	0.000	0.000	0	0	N.D. d	N.D. d
8) Heptachlo...	0.000	0.000	0	0	N.D. d	N.D. d
9) trans-Chl...	0.000	0.000	0	0	N.D. d	N.D. d
10) cis-Chlor...	0.000	0.000	0	0	N.D. d	N.D. d
11) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
12) 4,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
13) Dieldrin	0.000	0.000	0	0	N.D. d	N.D. d
14) Endrin	0.000	0.000	0	0	N.D. d	N.D. d
15) 4,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
16) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
17) 4,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
18) Endrin Al...	0.000	0.000	0	0	N.D. d	N.D. d
19) Endosulfa...	0.000	0.000	0	0	N.D. d	N.D. d
20) Methoxychlor	0.000	0.000	0	0	N.D. d	N.D. d
21) Endrin Ke...	0.000	0.000	0	0	N.D. d	N.D. d
23) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
24) Hexachlor...	0.000	0.000	0	0	N.D. d	N.D. d
25) Oxychlordane	0.000	0.000	0	0	N.D. d	N.D. d
26) 2,4'-DDE	0.000	0.000	0	0	N.D. d	N.D. d
27) trans-Non...	0.000	0.000	0	0	N.D. d	N.D. d
28) 2,4'-DDD	0.000	0.000	0	0	N.D. d	N.D. d
29) 2,4'-DDT	0.000	0.000	0	0	N.D. d	N.D. d
30) cis-Nonac...	0.000	0.000	0	0	N.D. d	N.D. d
31) Mirex	0.000	0.000	0	0	N.D. d	N.D. d
32) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
33) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
34) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
35) Chlordane...	0.000	0.000	0	0	N.D. d	N.D. d
36) Toxaphene...	7.500	8.466	1674674	5030917	2351.899	2421.326
37) Toxaphene...	7.792	8.813	2958997	6610397	2253.073	2699.433
38) Toxaphene...	8.104	8.848	6831460	10545708	2516.585	2773.802
39) Toxaphene...	8.345	8.914	6407070	17190037	2523.403	2695.039
40) Toxaphene...	8.572	9.091	5074570	9435236	2678.561	2669.893
41) Toxaphene...	8.640	9.471	6510950	10090951	2436.088	2281.169
42) Toxaphene...	3.452	0.000	4166	0	NoCal	N.D.
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 40% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : R:\data\2019-08\9H23034\  
Data File : ECD5-08231941.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 23 Aug 2019 23:20  
Operator : MJB  
Sample : 9H23034-CALS  
Misc : A19D121, TOX 2000 ppb  
ALS Vial : 34 (Sig #1); 0 (Sig #2) Sample Multiplier: 1

Integration File signal 1: PEST1.e  
Integration File signal 2: PEST2.e  
Quant Time: Aug 26 11:40:44 2019  
Quant Method : R:\methods\ECD5\_QUANTPEST\_190823.M  
Quant Title : Instrument: DualECD5  
QLast Update : Mon Aug 26 11:36:51 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped



**TCLP Semivolatile Organic Compounds by EPA 8270D  
Benchsheet & Analysis Sequence Data**

Batch 9111242  
Sequence 9K27012 (A9K0412-01RE1)





**Apex Laboratories**  
**PREPARATION BENCH SHEET**

DEC 03 2019

BATCH #: 9111242 (Soil)

Prep Method: EPA 1311/3510C (BNA Extraction)

#	Lab Number	Analysis	Prepared	Initial (mL)	Final (mL)	Spike ID	Source ID	ul Spike	ul Surr.	Sample ID	Extraction Comments	pH		
												<2	Other	>11
	9111242-BLK1	QC	11/26/19 14:05	200	2				100					
	9111242-BSD1	QC	11/26/19 14:05	200	2	A19K302		100	100					
	9111242-BS1	QC	11/26/19 14:05	200	2	A19K302		100	100					
	A9K0412-01	A 1311/8270D TCLP SVOC Reg List	11/26/19 14:05	200	2				100	PDI-142RAB-C-00-30.4-191112				
	A9K0412-01RE1	A 1311/8270D TCLP SVOC Reg List	11/26/19 14:05	200	2				100	PDI-142RAB-C-00-30.4-191112	Added 11/27/2019 by ams			

**Standards/Reagents**

Reagent(s)			Analyte Spike(s)			Surrogate(s)		
Std ID	Exp. Date	Description	Std ID	Exp. Date	Description	Std ID	Exp. Date	Description
A18K311	12/31/20	Glass Wool	A19K302	05/19/20	8270D PAH+/Phenols (JSCS) Spike @ 80 PPM	A19J495	04/28/20	PAH Soil and Water Surr. (50ppm)
A19H399	08/23/21	Conc. HCl - Omnitrace						
A19I263	03/18/20	DCM CHEM PROD. 194934						
A19I297	03/22/20	6N Sodium Hydroxide						
A19K010	10/29/25	Sodium Sulfate Lot # 188777						

3x rinse

Witness: \_\_\_\_\_

Bottle Check: \_\_\_\_\_

Prepared By: \_\_\_\_\_ Date \_\_\_\_\_


  
 Reviewed By: \_\_\_\_\_ Date: 12/2/19



**Apex Laboratories**  
**PREPARATION BENCH SHEET**

BATCH #: 9111242 (Soil)

Prep Method: EPA 1311/3510C (BNA Extraction)

#	Lab Number	Analysis	Prepared	Initial (mL)	Final (mL)	Spike ID	Source ID	ul Spike	ul Surr.	Sample ID	Extraction Comments	pH			
												<2	Other	>11	
	9111242-BLK1	QC	11/26/19 14:05	200	2				100						
	9111242-BSD1	QC	11/26/19 14:05	200	2	A19K302		100	100		*				
	9111242-BS1	QC	11/26/19 14:05	200	2	A19K302		100	100		*				
	A9K0412-01	A 1311/8270D TCLP SVOC Reg List	11/26/19 14:05	200	2				100	PDI-142RAB-C-00-30.4-191112					

**Standards/Reagents**

Reagent(s)			Analyte Spike(s)			Surrogate(s)		
Std ID	Exp. Date	Description	Std ID	Exp. Date	Description	Std ID	Exp. Date	Description
A18K311	12/31/20	Glass Wool	A19K302	05/19/20	8270D PAH+/Phenols (JSCS) Spike @ 80 PPM	A19J495	04/28/20	PAH Soil and Water Surr. (50ppm)
A19H399	08/23/21	Conc. HCl - Omnitrace						
A19I263	03/18/20	DCM CHEM PROD. 194934						
A19I297	03/22/20	6N Sodium Hydroxide						
A19K010	10/29/25	Sodium Sulfate Lot # 188777						

3x rinse ✓

Witness: cah 11/26/19

Bottle Check: N/A cah 11/26/19

\* = No BLK fluid added

cah 11/26/19  
Prepared By: Date

cah 11/26/19  
Reviewed By: Date



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence: **9K27012**

Instrument: **SV-GCMS10**

Date: **11/27/19 08:06**

Calibration: **A9I2405**

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
1	9K27012-TUN1	Water	QC	QC			A19I086	A19K329
2	9K27012-CCV1	Water	QC	QC			A19I086	A19G243
3	9K27012-IBL1	Water	QC	QC			A19I086	
4	9K27012-TUN2	Water	QC	QC			A19I086	A19K329
5	9K27012-CCV2	Water	QC	QC			A19I086	A19G243
6	9K27012-CCB1	Water	QC	QC			A19I086	
7	A9K0590-03RE3	Soil	8270D LL Full List		12/04/19	9111140	A19I086	
8	"	Soil	8270D LL PAH/PHTH/Phenols	(QC Source)		9111140	A19I086	
9	9111140-DUP7	Soil	QC	QC		9111140	A19I086	
10	A9K0590-05RE2	Soil	8270D LL Full List		12/04/19	9111140	A19I086	
11	"	Soil	8270D LL PAH/PHTH/Phenols	(QC Source)		9111140	A19I086	
12	9111140-DUP8	Soil	QC	QC		9111140	A19I086	
13	9111140-MS4	Soil	QC	QC		9111140	A19I086	
14	A9K0590-01RE2	Soil	8270D LL Full List		12/04/19	9111140	A19I086	
15	A9K0412-01RE1	Soil	1311/8270D TCLP SVOC Reg List	Anchor QEA, LLC	11/27/19	9111242	A19I086	
16	A9K0656-04	Soil	8270D LL PAH/PHTH/Phenols		12/09/19	9111249	A19I086	
17	A9K0598-06	Soil	8270D LL PAH/PHTH/Phenols		12/05/19	9111140	A19I086	
18	A9K0656-04RE1	Soil	8270D LL PAH/PHTH/Phenols		12/09/19	9111249	A19I086	
19	9111296-BLK1	Soil	QC	QC		9111296	A19I086	
20	9111296-BS1	Soil	QC	QC		9111296	A19I086	
21	9111296-BSD1	Soil	QC	QC		9111296	A19I086	
22	A9K0715-03	Soil	1311/8270D TCLP Full List SVOC		12/02/19	9111296	A19I086	
23	A9K0715-03RE1	Soil	1311/8270D TCLP Full List SVOC		12/02/19	9111296	A19I086	
24	A9K0749-02	Water	625 PAH/PCP/HCB (SW)		12/10/19	9111159	A19I086	
25	A9K0763-01	Water	625 PAH/PCP/HCB (SW)		12/10/19	9111159	A19I086	
26	9K27012-IBL2	Water	QC	QC			A19I086	

Data Entered By:

*AMS 12/2/19*

Comments:

Data Reviewed By:



*PK 12/2/19*

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271901.D  
 Acq On : 27 Nov 2019 8:13 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-TUN1  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1

*AMS*  
*12/2/19*  
*Q-14*

Integration File: rteint.p

Method : T:\methods\DFTPP.M  
 Title : 8270 DFTPP Tune Method  
 Last Update : Mon Nov 11 08:41:49 2019



AutoFind: Scans 1454, 1455, 1456; Background Corrected with Scan 1449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	1784	PASS
69	198	0.01	100	20.4	119959	PASS
70	69	0.00	2	0.6	667	PASS
197	198	0.00	2	0.1	678	PASS
198	198	100	100	100.0	589312	PASS
199	198	5	9	6.9	40587	PASS
365	198	1	100	3.5	20693	PASS
441	443	0.01	150	76.2	100147	PASS
442	198	0.10	200	112.8	664875	PASS
443	442	15	24	19.8	131352	PASS

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271901.D  
 Acq On : 27 Nov 2019 8:13 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-TUN1  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Dec 02 08:54:01 2019  
 Quant Method : T:\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Mon Nov 11 08:41:49 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.412	150	163060	2.00	ug/mL	0.00
2) Naphthalene-d8	7.675	136	427405	2.00	ug/mL	0.00
3) Acenaphthene-d10	9.456	162	218302	2.00	ug/mL	0.00
5) Phenanthrene-d10	10.970	188	378161	2.00	ug/mL	0.00
11) Chrysene-d12	14.569	240	299210	2.00	ug/mL	-0.01
12) Perylene-d12	16.869	264	284989	2.00	ug/mL	#-0.04
-----						
Target Compounds						
4) Pentachlorophenol	10.788	266	826830	40.11	ug/mL	82
6) DFTPP	11.274	442	795301	26.05	ug/mL#	69
7) Benzidine	12.398	184	2773770	20.62	ug/mL	98
8) 4,4-DDE	12.644	TIC	44524	No Calib		
9) 4,4-DDD	13.125	TIC	384193	No Calib		
10) 4,4-DDT	13.649	TIC	9601229	24.76	ug/mL	94
-----						

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : T:\data\2019-11\9K27012\  
Data File : J11271901.D  
Acq On : 27 Nov 2019 8:13 am  
Operator : JK/ AMS/ DTH  
Sample : 9K27012-TUN1  
Misc : 1x, A19K329 DFTPP@45  
ALS Vial : 1 Sample Multiplier: 1  
DataAcq Meth:DFTPP.M

Quant Time: Dec 02 08:54:01 2019  
Quant Method : T:\methods\DFTPP.M  
Quant Title : 8270 DFTPP Tune Method  
QLast Update : Mon Nov 11 08:41:49 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271902.D  
 Acq On : 27 Nov 2019 8:41 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV1  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

AMS  
12/2/19 Q-14

Quant Time: Dec 02 08:54:12 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) 1,4-Dichlorobenzene-d4...	6.380	152	359541	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1401695	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	742081	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.937	188	1378339	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.537	240	1330036	2000.00	ng/ml	0.01	
86) Perylene-d12 (ISTD)	17.982	264	1301618	2000.00	ng/ml	0.02	
94) Dibenz(a,h)Anthracene-d...	20.372	292	1110267	2000.00	ng/ml	0.02	
System Monitoring Compounds							
4) 2-Fluorophenol (Surr)	5.118	112	230678	1057.28	ng/ml	-0.03	
5) Phenol-d6 (Surr)	6.038	99	271733	973.02	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	206529	953.27	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	608361	1047.53	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	83935	1010.23	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.670	244	653059	1065.47	ng/ml	0.00	
Target Compounds							
							Qvalue
2) N-Nitrosodimethylamine	3.695	74	118317	863.93	ng/ml		89
3) Pyridine	3.711	79	203065m	869.73	ng/ml		
6) Phenol	6.049	94	286731	933.74	ng/ml		97
7) Aniline	6.065	93	176195	665.04	ng/ml		86
8) Bis(2-chloroethyl) ether	6.124	93	253807	915.82	ng/ml		96
9) 2-Chlorophenol	6.182	128	266067	1045.12	ng/ml		97
10) 1,3-Dichlorobenzene	6.327	146	292615	1022.59	ng/ml		98
11) 1,4-Dichlorobenzene	6.396	146	286679	1019.34	ng/ml		98
12) Benzyl alcohol	6.519	108	146411	971.34	ng/ml		95
13) 1,2-Dichlorobenzene	6.552	146	285608	1029.75	ng/ml		96
14) 2-Methylphenol	6.637	107	192485	1039.40	ng/ml		99
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	185918	760.18	ng/ml		84
16) N-Nitrosodi-n-propylamine	6.782	70	146324	909.40	ng/ml		93
17) 3+4-Methylphenol	6.787	107	241175	1050.27	ng/ml		97
18) Hexachloroethane	6.883	201	90167	1043.44	ng/ml		93
20) Nitrobenzene	6.947	77	204793	932.97	ng/ml		88
22) Isophorone	7.183	82	419493	938.73	ng/ml		98
23) 2-Nitrophenol	7.263	139	149017	1122.15	ng/ml		89
24) 2,4-Dimethylphenol	7.311	122	220196	1171.68	ng/ml		98
25) Bis(2-chloroethoxy) me...	7.397	93	267761	985.61	ng/ml		99
26) Benzoic acid	7.418	105	198787	2476.25	ng/ml		93
27) 2,4-Dichlorophenol	7.509	162	224773	1069.51	ng/ml		97
28) 1,2,4-Trichlorobenzene	7.589	180	267027	1088.47	ng/ml		98
29) Naphthalene	7.669	128	764179	1036.35	ng/ml		99
30) 4-Chloroaniline	7.728	127	157423	681.07	ng/ml		97
31) Hexachlorobutadiene	7.798	225	138264	1042.97	ng/ml		98
32) 4-Chloro-3-methylphenol	8.215	107	199338	1071.75	ng/ml		92
33) 2-Methylnaphthalene	8.365	142	544344	1056.56	ng/ml		98
34) 1-Methylnaphthalene	8.466	142	519781	1042.17	ng/ml		98
36) Hexachlorocyclopentadiene	8.536	237	130770	1139.58	ng/ml		98
37) 2,4,6-Trichlorophenol	8.654	196	165785	1151.77	ng/ml		97
38) 2,4,5-Trichlorophenol	8.696	198	162948	1148.04	ng/ml		99
39) 1,1'-Biphenyl	8.835	154	652854	1023.56	ng/ml		98
41) 2-Chloronaphthalene	8.857	162	504095	1094.31	ng/ml		96
42) 2-Nitroaniline	8.964	138	158636	1148.77	ng/ml		84
43) 2,6-Dimethylnaphthalene	8.996	156	485779	1038.17	ng/ml		98

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271902.D  
 Acq On : 27 Nov 2019 8:41 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV1  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:54:12 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	75554	1286.62	ng/ml	85
45) Dimethyl phthalate	9.146	163	577694	1077.97	ng/ml	99
46) 1,3-Dinitrobenzene	9.172	168	87861	1182.53	ng/ml	86
47) 2,6-Dinitrotoluene	9.204	165	132676	1098.85	ng/ml	90
48) 1,2-Dinitrobenzene	9.263	168	61472	1132.23	ng/ml	76
49) Acenaphthylene	9.279	152	796950	1056.45	ng/ml	99
50) 3-Nitroaniline	9.381	138	94899	1016.96	ng/ml	85
51) Acenaphthene	9.456	153	494790	998.84	ng/ml	99
52) 2,4-Dinitrophenol	9.483	184	36583	1220.83	ng/ml	90
53) 4-Nitrophenol	9.563	139	75160	1030.23	ng/ml	91
54) 2,4-Dinitrotoluene	9.616	165	169430	1121.53	ng/ml	86
55) Dibenzofuran	9.632	168	707759	1071.82	ng/ml	97
56) 2,3,5,6-Tetrachlorophenol	9.718	232	128229	1124.02	ng/ml	98
57) 2,3,4,6-Tetrachlorophenol	9.766	232	135388	1085.24	ng/ml	96
58) Diethyl phthalate	9.862	149	534657	1083.81	ng/ml	99
59) 2,3,5-Trimethylnaphtha...	9.846	170	464842	1105.46	ng/ml	93
60) Fluorene	9.980	166	532739	1025.17	ng/ml	98
61) 4-Chlorophenyl phenyl ...	9.980	204	266543	1052.11	ng/ml	92
62) 4-Nitroaniline	10.001	138	90780	1138.35	ng/ml	92
63) 4,6-Dinitro-2-methylph...	10.033	198	66484	1216.78	ng/ml	87
65) N-Nitrosodiphenylamine	10.098	169	462145	1087.43	ng/ml	99
66) Azobenzene (1,2-DPH)	10.140	77	382193	888.67	ng/ml	88
68) 4-Bromophenyl phenyl e...	10.477	248	165402	1063.47	ng/ml	94
69) Hexachlorobenzene	10.552	284	190209	1019.43	ng/ml	98
70) Pentachlorophenol (PCP)	10.750	266	84922	916.51	ng/ml	99
71) Phenanthrene	10.959	178	771690	997.98	ng/ml	99
72) Anthracene	11.012	178	780809	1050.49	ng/ml	99
73) Carbazole	11.178	167	639585	1146.32	ng/ml	99
74) Di-n-butyl phthalate	11.531	149	877001	1075.89	ng/ml	99
75) Fluoranthene	12.200	202	864344	1090.62	ng/ml	98
76) Benzidine	12.355	184	247416	1337.22	ng/ml	98
77) Pyrene	12.472	202	873997	1083.67	ng/ml	99
80) Butyl benzyl phthalate	13.425	149	382570	1117.84	ng/ml	92
81) Bis(2-ethylhexyl) adipate	13.590	129	333566	1081.32	ng/ml	99
82) 3,3-Dichlorobenzidine	14.500	252	208030	1978.01	ng/ml	98
83) Benz(a)anthracene	14.510	228	763258	1027.83	ng/ml	96
84) Chrysene	14.591	228	730621	1049.89	ng/ml	99
85) Bis(2-ethylhexyl) phth...	14.692	149	554772	1159.57	ng/ml	97
87) Di-n-octyl phthalate	16.345	149	896232	1186.72	ng/ml	98
88) Benzo(b)fluoranthene	17.067	252	768417	1069.81	ng/ml	98
89) Benzo(k)fluoranthene	17.131	252	761692	1053.52	ng/ml	99
90) Benzo(b+k)fluoranthene	17.131	252	1552936	2106.21	ng/ml	99
91) Benzo(e)pyrene	17.709	252	748511	1118.85	ng/ml	98
92) Benzo(a)pyrene	17.832	252	717846	1100.52	ng/ml	97
93) Perylene	18.035	252	627557	1069.07	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.362	276	658648	1003.21	ng/ml	97
96) Dibenz(a,h)anthracene	20.437	278	638517	1059.26	ng/ml	99
97) Benzo(g,h,i)perylene	20.897	276	685335	1086.75	ng/ml	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271902.D  
 Acq On : 27 Nov 2019 8:41 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV1  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:54:12 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10





Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271904.D  
 Acq On : 27 Nov 2019 10:07 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-TUN2  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1

*Replaced  
liner*

*AMS  
11/27/19 ✓*

Integration File: rteint.p

Method : T:\methods\DFTPP.M  
 Title : 8270 DFTPP Tune Method  
 Last Update : Mon Nov 11 08:41:49 2019



AutoFind: Scans 1453, 1454, 1455; Background Corrected with Scan 1448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.3	1539	PASS
69	198	0.01	100	20.7	118824	PASS
70	69	0.00	2	0.4	487	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	572800	PASS
199	198	5	9	7.0	40251	PASS
365	198	1	100	3.4	19576	PASS
441	443	0.01	150	76.7	95541	PASS
442	198	0.10	200	109.6	627733	PASS
443	442	15	24	19.9	124637	PASS

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271904.D  
 Acq On : 27 Nov 2019 10:07 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-TUN2  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Dec 02 08:54:39 2019  
 Quant Method : T:\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Mon Nov 11 08:41:49 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10




Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	6.413	150	142179	2.00	ug/mL	0.00
2) Naphthalene-d8	7.675	136	420053	2.00	ug/mL	0.00
3) Acenaphthene-d10	9.451	162	222042	2.00	ug/mL	0.00
5) Phenanthrene-d10	10.964	188	366550	2.00	ug/mL	0.00
11) Chrysene-d12	14.564	240	285430	2.00	ug/mL	-0.02
12) Perylene-d12	16.949	264	346	2.00	ug/mL	# 0.04
<b>Target Compounds</b>						
4) Pentachlorophenol	10.782	266	714504	34.08	ug/mL	82
6) DFTPP	11.269	442	763066	25.79	ug/mL	72
7) Benzidine	12.392	184	3212213	24.63	ug/mL	97
8) 4,4-DDE	12.633	TIC	43631	No Calib		
9) 4,4-DDD	13.114	TIC	19998	No Calib		
10) 4,4-DDT	13.639	TIC	9663676	25.71	ug/mL	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271904.D  
 Acq On : 27 Nov 2019 10:07 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-TUN2  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Dec 02 08:54:39 2019  
 Quant Method : T:\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Mon Nov 11 08:41:49 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J11271904.D\data.ms

(4) Pentachlorophenol

10.782min (-0.005) 34.08 ug/mL




response 714504

Ion	Exp%	Act%
265.90	100.00	100.00
164.90	50.60	36.17
201.90	25.80	21.35
129.90	27.30	15.27

Quantitation Report (Qedit)

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271904.D  
 Acq On : 27 Nov 2019 10:07 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-TUN2  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Dec 02 08:54:39 2019  
 Quant Method : T:\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Mon Nov 11 08:41:49 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J11271904.D\data.ms

(7) Benzidine

12.392min (-0.011) 24.63 ug/mL

response 3212213

Ion	Exp%	Act%
184.10	100.00	100.00
156.10	8.50	7.09
92.10	8.20	7.29
0.00	0.00	0.00

# DDT Breakdown Check (Validated 5/1/2013)


From:  
9K27012-TUN2  
SV-GCMS10

First Column Area Counts	Percent Breakdown
DDE 43631	
DDD 19998	
<b>DDT 9663676</b>	<b>0.65 PASS</b>

Breakdown must be less than 20% to accept sample data.

Data Path : T:\data\2019-11\9K27012\  
Data File : J11271904.D  
Acq On : 27 Nov 2019 10:07 am  
Operator : JK/ AMS/ DTH  
Sample : 9K27012-TUN2  
Misc : 1x, A19K329 DFTPP@45  
ALS Vial : 1 Sample Multiplier: 1  
DataAcq Meth:DFTPP.M

Quant Time: Dec 02 08:54:39 2019  
Quant Method : T:\methods\DFTPP.M  
Quant Title : 8270 DFTPP Tune Method  
QLast Update : Mon Nov 11 08:41:49 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10



Evaluate Continuing Calibration Report

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271905.D  
 Acq On : 27 Nov 2019 10:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

*AMS*  
*2/2 1/19*

Quant Time: Dec 02 08:56:13 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4 (IST	2000.000	2000.000	0.0	130	-0.01
2 TG	N-Nitrosodimethylamine	1000.000	898.038	10.2	120	-0.03
3 TG	Pyridine	1000.000	885.468	11.5	116	-0.03
4 S	2-Fluorophenol (Surr)	1000.000	1057.885	-5.8	132	-0.03
5 S	Phenol-d6 (Surr)	1000.000	953.791	4.6	114	0.00
6 T	Phenol	1000.000	915.600	8.4	110	-0.01
7 T	Aniline	1000.000	622.719	37.7#	89	-0.02
8 T	Bis(2-chloroethyl) ether	1000.000	891.223	10.9	106	-0.01
9 T	2-Chlorophenol	1000.000	1031.934	-3.2	126	-0.01
10 T	1,3-Dichlorobenzene	1000.000	1025.176	-2.5	130	-0.02
11 T	1,4-Dichlorobenzene	1000.000	1012.946	-1.3	127	-0.02
12 T	Benzyl alcohol	1000.000	949.972	5.0	117	0.00
13 T	1,2-Dichlorobenzene	1000.000	1020.577	-2.1	128	-0.01
14 T	2-Methylphenol	1000.000	1025.641	-2.6	120	0.00
15 T	2,2'-Oxybis(1-Chloropropane	1000.000	751.300	24.9#	92	0.00
16 T	N-Nitrosodi-n-propylamine	1000.000	874.570	12.5	106	0.00
17 T	3+4-Methylphenol	1000.000	1041.643	-4.2	119	0.00
18 T	Hexachloroethane	1000.000	1096.904	-9.7	142	-0.01
19 S	Nitrobenzene-d5 (Surr)	1000.000	934.295	6.6	111	-0.01
20 T	Nitrobenzene	1000.000	921.487	7.9	110	0.00
21 I	Naphthalene-d8 (ISTD)	2000.000	2000.000	0.0	124	0.00
22 T	Isophorone	1000.000	922.545	7.7	110	0.00
23 T	2-Nitrophenol	1000.000	1093.259	-9.3	127	0.00
24 T	2,4-Dimethylphenol	1000.000	1128.703	-12.9	130	0.00
25 T	Bis(2-chloroethoxy) methane	1000.000	980.827	1.9	114	0.00
26 T	Benzoic acid	2000.000	1926.472	3.7	133	0.00
27 T	2,4-Dichlorophenol	1000.000	1064.321	-6.4	130	0.00
28 T	1,2,4-Trichlorobenzene	1000.000	1085.515	-8.6	130	0.00
29 T	Naphthalene	1000.000	1038.708	-3.9	121	0.00
30 T	4-Chloroaniline	1000.000	639.616	36.0#	75	-0.01
31 T	Hexachlorobutadiene	1000.000	1071.351	-7.1	126	0.00
32 T	4-Chloro-3-methylphenol	1000.000	1051.294	-5.1	121	0.00
33 T	2-Methylnaphthalene	1000.000	1065.228	-6.5	122	0.00
34 T	1-Methylnaphthalene	1000.000	1039.273	-3.9	121	0.00
35 I	Acenaphthene-d10 (ISTD)	2000.000	2000.000	0.0	129	0.00
36 T	Hexachlorocyclopentadiene	1000.000	1307.595	-30.8#	152	0.00
37 T	2,4,6-Trichlorophenol	1000.000	1140.406	-14.0	141	0.00
38 T	2,4,5-Trichlorophenol	1000.000	1135.982	-13.6	143	0.00
39 T	1,1'-Biphenyl	1000.000	1027.211	-2.7	124	0.00
40 S	2-Fluorobiphenyl (Surr)	1000.000	1026.210	-2.6	125	0.00
41 T	2-Chloronaphthalene	1000.000	1095.792	-9.6	132	0.00
42 T	2-Nitroaniline	1000.000	1136.967	-13.7	140	0.00
43 T	2,6-Dimethylnaphthalene	1000.000	1027.556	-2.8	125	0.00
44 T	1,4-Dinitrobenzene	1000.000	1294.196	-29.4#	174	0.00
45 T	Dimethyl phthalate	1000.000	1042.577	-4.3	126	0.00
46 T	1,3-Dinitrobenzene	1000.000	1161.530	-16.2	152	0.00
47 T	2,6-Dinitrotoluene	1000.000	1085.364	-8.5	136	0.00
48 T	1,2-Dinitrobenzene	1000.000	1136.163	-13.6	138	0.00



Evaluate Continuing Calibration Report

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271905.D  
 Acq On : 27 Nov 2019 10:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:56:13 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area	Dev(min)
49 T Acenaphthylene	1000.000	1031.393	-3.1	124	0.00
50 T 3-Nitroaniline	1000.000	940.978	5.9	118	0.00
51 T Acenaphthene	1000.000	991.067	0.9	124	0.00
52 T 2,4-Dinitrophenol	1000.000	1017.274	-1.7	159	0.00
53 T 4-Nitrophenol	1000.000	929.876	7.0	115	0.00
54 T 2,4-Dinitrotoluene	1000.000	1115.679	-11.6	147	0.00
55 T Dibenzofuran	1000.000	1056.744	-5.7	128	0.00
56 T 2,3,5,6-Tetrachlorophenol	1000.000	1083.166	-8.3	136	0.00
57 T 2,3,4,6-Tetrachlorophenol	1000.000	1092.894	-9.3	137	0.00
58 T Diethyl phthalate	1000.000	1065.121	-6.5	125	0.00
59 T 2,3,5-Trimethylnaphthalene	1000.000	1088.491	-8.8	130	0.00
60 T Fluorene	1000.000	1022.783	-2.3	126	0.00
61 T 4-Chlorophenyl phenyl ether	1000.000	1058.796	-5.9	130	0.00
62 T 4-Nitroaniline	1000.000	1216.265	-21.6#	156	0.00
63 T 4,6-Dinitro-2-methylphenol	1000.000	1163.608	-16.4	164	0.00
64 I Phenanthrene-d10 (ISTD)	2000.000	2000.000	0.0	129	0.00
65 T N-Nitrosodiphenylamine	1000.000	1076.160	-7.6	130	0.00
66 T Azobenzene (1,2-DPH)	1000.000	882.035	11.8	107	0.00
67 S 2,4,6-Tribromophenol (Surr)	1000.000	1002.705	-0.3	128	0.00
68 T 4-Bromophenyl phenyl ether	1000.000	1055.092	-5.5	130	0.00
69 T Hexachlorobenzene	1000.000	1025.655	-2.6	126	0.00
70 T Pentachlorophenol (PCP)	1000.000	960.972	3.9	137	0.00
71 T Phenanthrene	1000.000	1007.430	-0.7	127	0.00
72 T Anthracene	1000.000	1064.559	-6.5	130	0.00
73 T Carbazole	1000.000	1166.828	-16.7	141	0.00
74 T Di-n-butyl phthalate	1000.000	1081.324	-8.1	129	0.00
75 T Fluoranthene	1000.000	1108.753	-10.9	131	0.00
76 T Benzidine	2000.000	1413.879	29.3#	87	0.00
77 T Pyrene	1000.000	1094.507	-9.5	129	0.00
78 I Chrysene-d12 (ISTD)	2000.000	2000.000	0.0	129	0.00
79 S Terphenyl-d14 (Surr)	1000.000	1069.739	-7.0	131	0.00
80 T Butyl benzyl phthalate	1000.000	1102.043	-10.2	137	0.00
81 T Bis(2-ethylhexyl) adipate	1000.000	1069.472	-6.9	135	0.00
82 T 3,3-Dichlorobenzidine	2000.000	1933.069	3.3	119	0.02
83 T Benz(a)anthracene	1000.000	1037.184	-3.7	136	0.01
84 T Chrysene	1000.000	1052.991	-5.3	134	0.00
85 T Bis(2-ethylhexyl) phthalate	1000.000	1132.224	-13.2	141	0.00
86 I Perylene-d12 (ISTD)	2000.000	2000.000	0.0	128	0.00
87 T Di-n-octyl phthalate	1000.000	1121.039	-12.1	146	0.00
88 T Benzo(b)fluoranthene	1000.000	1093.702	-9.4	139	0.01
89 T Benzo(k)fluoranthene	1000.000	1054.402	-5.4	134	0.00
90 T Benzo(b+k)fluoranthene	2000.000	2133.804	-6.7	136	0.00
91 T Benzo(e)pyrene	1000.000	1137.856	-13.8	135	0.00
92 T Benzo(a)pyrene	1000.000	1109.025	-10.9	138	0.01
93 T Perylene	1000.000	1091.327	-9.1	137	0.01
94 I Dibenz(a,h)Anthrcene-d14 (I	2000.000	2000.000	0.0	130	0.01

Evaluate Continuing Calibration Report

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271905.D  
 Acq On : 27 Nov 2019 10:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:56:13 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
95 T Indeno(1,2,3-cd)pyrene	1000.000	1023.715	-2.4	137	0.02
96 T Dibenz(a,h)anthracene	1000.000	1082.243	-8.2	138	0.01
97 T Benzo(g,h,i)perylene	1000.000	1133.836	-13.4	138	0.02

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271905.D  
 Acq On : 27 Nov 2019 10:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:56:13 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA.8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) 1,4-Dichlorobenzene-d4...	6.381	152	368375	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1412968	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	751566	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1376916	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.532	240	1352496	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.971	264	1331887	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.362	292	1152858	2000.00	ng/ml	0.01	
System Monitoring Compounds							
4) 2-Fluorophenol (Surr)	5.124	112	236482	1057.88	ng/ml	-0.03	
5) Phenol-d6 (Surr)	6.038	99	272908	953.79	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	207392	934.30	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	603598	1026.21	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	83213	1002.70	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	666750	1069.74	ng/ml	0.00	
Target Compounds							
							Qvalue
2) N-Nitrosodimethylamine	3.712	74	126010	898.04	ng/ml		89
3) Pyridine	3.728	79	211818m	885.47	ng/ml		
6) Phenol	6.049	94	288069	915.60	ng/ml		96
7) Aniline	6.065	93	169035	622.72	ng/ml		81
8) Bis(2-chloroethyl) ether	6.124	93	253059	891.22	ng/ml		99
9) 2-Chlorophenol	6.183	128	269165	1031.93	ng/ml		96
10) 1,3-Dichlorobenzene	6.327	146	300562	1025.18	ng/ml		98
11) 1,4-Dichlorobenzene	6.397	146	291881	1012.95	ng/ml		98
12) Benzyl alcohol	6.525	108	146589	949.97	ng/ml		92
13) 1,2-Dichlorobenzene	6.552	146	290019	1020.58	ng/ml		97
14) 2-Methylphenol	6.637	107	194604	1025.64	ng/ml		99
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	188262	751.30	ng/ml		83
16) N-Nitrosodi-n-propylamine	6.782	70	144177	874.57	ng/ml		91
17) 3+4-Methylphenol	6.787	107	245070	1041.64	ng/ml		95
18) Hexachloroethane	6.883	201	97116	1096.90	ng/ml		95
20) Nitrobenzene	6.948	77	207242	921.49	ng/ml		89
22) Isophorone	7.183	82	415575	922.55	ng/ml		98
23) 2-Nitrophenol	7.263	139	146185	1093.26	ng/ml		89
24) 2,4-Dimethylphenol	7.311	122	213825	1128.70	ng/ml		96
25) Bis(2-chloroethoxy) me...	7.397	93	268604	980.83	ng/ml		99
26) Benzoic acid	7.407	105	132481	1926.47	ng/ml		94
27) 2,4-Dichlorophenol	7.509	162	225469	1064.32	ng/ml		97
28) 1,2,4-Trichlorobenzene	7.589	180	268444	1085.51	ng/ml		100
29) Naphthalene	7.670	128	772074	1038.71	ng/ml		99
30) 4-Chloroaniline	7.728	127	149016	639.62	ng/ml		96
31) Hexachlorobutadiene	7.798	225	143168	1071.35	ng/ml		99
32) 4-Chloro-3-methylphenol	8.215	107	197106	1051.29	ng/ml		92
33) 2-Methylnaphthalene	8.365	142	553223	1065.23	ng/ml		99
34) 1-Methylnaphthalene	8.467	142	522506	1039.27	ng/ml		99
36) Hexachlorocyclopentadiene	8.536	237	151968	1307.60	ng/ml		100
37) 2,4,6-Trichlorophenol	8.654	196	166204	1140.41	ng/ml		100
38) 2,4,5-Trichlorophenol	8.691	198	163264	1135.98	ng/ml		98
39) 1,1'-Biphenyl	8.836	154	663560	1027.21	ng/ml		99
41) 2-Chloronaphthalene	8.857	162	511229	1095.79	ng/ml		95
42) 2-Nitroaniline	8.964	138	158938	1136.97	ng/ml		82
43) 2,6-Dimethylnaphthalene	8.996	156	486958	1027.56	ng/ml		97

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271905.D  
 Acq On : 27 Nov 2019 10:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Dec 02 08:56:13 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	77023	1294.20	ng/ml	79
45) Dimethyl phthalate	9.146	163	565870	1042.58	ng/ml	99
46) 1,3-Dinitrobenzene	9.173	168	87293	1161.53	ng/ml	87
47) 2,6-Dinitrotoluene	9.205	165	132696	1085.36	ng/ml	88
48) 1,2-Dinitrobenzene	9.258	168	62474	1136.16	ng/ml	83
49) Acenaphthylene	9.280	152	787992	1031.39	ng/ml	98
50) 3-Nitroaniline	9.381	138	90147	940.98	ng/ml	89
51) Acenaphthene	9.456	153	497213	991.07	ng/ml	100
52) 2,4-Dinitrophenol	9.483	184	28656	1017.27	ng/ml	92
53) 4-Nitrophenol	9.558	139	67693	929.88	ng/ml	93
54) 2,4-Dinitrotoluene	9.617	165	170667	1115.68	ng/ml	82
55) Dibenzofuran	9.633	168	706724	1056.74	ng/ml	98
56) 2,3,5,6-Tetrachlorophenol	9.718	232	124938	1083.17	ng/ml	97
57) 2,3,4,6-Tetrachlorophenol	9.761	232	138109	1092.89	ng/ml	98
58) Diethyl phthalate	9.863	149	532153	1065.12	ng/ml	97
59) 2,3,5-Trimethylnaphtha...	9.846	170	463556	1088.49	ng/ml	91
60) Fluorene	9.980	166	538292	1022.78	ng/ml	99
61) 4-Chlorophenyl phenyl ...	9.980	204	271664	1058.80	ng/ml	91
62) 4-Nitroaniline	10.002	138	98233	1216.27	ng/ml	88
63) 4,6-Dinitro-2-methylph...	10.034	198	63770	1163.61	ng/ml	87
65) N-Nitrosodiphenylamine	10.098	169	456883	1076.16	ng/ml	100
66) Azobenzene (1,2-DPH)	10.141	77	378950	882.04	ng/ml	85
68) 4-Bromophenyl phenyl e...	10.478	248	163929	1055.09	ng/ml	95
69) Hexachlorobenzene	10.553	284	191172	1025.65	ng/ml	98
70) Pentachlorophenol (PCP)	10.750	266	89311	960.97	ng/ml	96
71) Phenanthrene	10.959	178	778196	1007.43	ng/ml	99
72) Anthracene	11.012	178	790453	1064.56	ng/ml	100
73) Carbazole	11.173	167	646561	1166.83	ng/ml	100
74) Di-n-butyl phthalate	11.526	149	880522	1081.32	ng/ml	99
75) Fluoranthene	12.195	202	877808	1108.75	ng/ml	98
76) Benzidine	12.350	184	262912	1413.88	ng/ml	97
77) Pyrene	12.467	202	881826	1094.51	ng/ml	98
80) Butyl benzyl phthalate	13.419	149	383262	1102.04	ng/ml	92
81) Bis(2-ethylhexyl) adipate	13.585	129	335481	1069.47	ng/ml	99
82) 3,3-Dichlorobenzidine	14.489	252	207508	1933.07	ng/ml	93
83) Benz(a)anthracene	14.511	228	783209	1037.18	ng/ml	97
84) Chrysene	14.585	228	745153	1052.99	ng/ml	99
85) Bis(2-ethylhexyl) phth...	14.687	149	550836	1132.22	ng/ml	97
87) Di-n-octyl phthalate	16.334	149	862989	1121.04	ng/ml	98
88) Benzo(b)fluoranthene	17.062	252	804146	1093.70	ng/ml	99
89) Benzo(k)fluoranthene	17.126	252	780042	1054.40	ng/ml	99
90) Benzo(b+k)fluoranthene	17.126	252	1609897	2133.80	ng/ml	99
91) Benzo(e)pyrene	17.709	252	778927	1137.86	ng/ml	99
92) Benzo(a)pyrene	17.827	252	740269	1109.02	ng/ml	98
93) Perylene	18.030	252	655518	1091.33	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.362	276	697896	1023.71	ng/ml	97
96) Dibenz(a,h)anthracene	20.426	278	677395	1082.24	ng/ml	97
97) Benzo(g,h,i)perylene	20.891	276	742457	1133.84	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271905.D  
 Acq On : 27 Nov 2019 10:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:56:13 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271906.D  
 Acq On : 27 Nov 2019 11:10 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

AMS  
12/2/19

Quant Time: Dec 02 08:56:42 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.386	152	443001	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.648	136	1732924	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	917836	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1633582	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.532	240	1702493	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.976	264	1710175	2000.00	ng/ml	0.01	
94) Dibenz(a,h)Anthrcene-d...	20.367	292	1426780	2000.00	ng/ml	0.02	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	0.000	112	0	0.00	ng/ml		
5) Phenol-d6 (Surr)	0.000	99	0	0.00	ng/ml		
19) Nitrobenzene-d5 (Surr)	6.889	82	50	0.19	ng/ml	-0.05	
40) 2-Fluorobiphenyl (Surr)	0.000	172	0	0.00	ng/ml		
67) 2,4,6-Tribromophenol (...)	0.000	330	0	0.00	ng/ml		
79) Terphenyl-d14 (Surr)	0.000	244	0	0.00	ng/ml		
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	0.000		0	N.D.			Qvalue
3) Pyridine	3.781	79	632	N.D.			
6) Phenol	0.000		0	N.D.			
7) Aniline	6.140	93	80	N.D.			
8) Bis(2-chloroethyl) ether	6.140	93	80	N.D.			
9) 2-Chlorophenol	0.000		0	N.D.			
10) 1,3-Dichlorobenzene	0.000		0	N.D.			
11) 1,4-Dichlorobenzene	0.000		0	N.D.			
12) Benzyl alcohol	0.000		0	N.D.			
13) 1,2-Dichlorobenzene	0.000		0	N.D.			
14) 2-Methylphenol	6.664	107	63	N.D.			
15) 2,2'-Oxybis(1-Chloropr...	0.000		0	N.D.			
16) N-Nitrosodi-n-propylamine	6.776	70	82	N.D.			
17) 3+4-Methylphenol	6.728	107	73	N.D.			
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	6.958	77	53	N.D.			
22) Isophorone	7.167	82	103	N.D.			
23) 2-Nitrophenol	0.000		0	N.D.			
24) 2,4-Dimethylphenol	0.000		0	N.D.			
25) Bis(2-chloroethoxy) me...	7.349	93	56	N.D.			
26) Benzoic acid	7.429	105	73	806.55	ng/ml#	25	
27) 2,4-Dichlorophenol	0.000		0	N.D.			
28) 1,2,4-Trichlorobenzene	0.000		0	N.D.			
29) Naphthalene	7.670	128	123	N.D.			
30) 4-Chloroaniline	0.000		0	N.D.			
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	8.253	107	99	N.D.			
33) 2-Methylnaphthalene	0.000		0	N.D.			
34) 1-Methylnaphthalene	0.000		0	N.D.			
36) Hexachlorocyclopentadiene	0.000		0	N.D.			
37) 2,4,6-Trichlorophenol	0.000		0	N.D.			
38) 2,4,5-Trichlorophenol	0.000		0	N.D.			
39) 1,1'-Biphenyl	0.000		0	N.D.			
41) 2-Chloronaphthalene	0.000		0	N.D.			
42) 2-Nitroaniline	0.000		0	N.D.			
43) 2,6-Dimethylnaphthalene	9.156	156	81	N.D.			

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271906.D  
 Acq On : 27 Nov 2019 11:10 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K27012-CCB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Dec 02 08:56:42 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	0.000		0		N.D.	
45) Dimethyl phthalate	9.156	163	231		N.D.	
46) 1,3-Dinitrobenzene	0.000		0		N.D.	
47) 2,6-Dinitrotoluene	0.000		0		N.D.	
48) 1,2-Dinitrobenzene	0.000		0		N.D.	
49) Acenaphthylene	0.000		0		N.D.	
50) 3-Nitroaniline	9.424	138	99	30.40	ng/ml#	1
51) Acenaphthene	9.424	153	209		N.D.	
52) 2,4-Dinitrophenol	0.000		0		N.D.	
53) 4-Nitrophenol	0.000		0		N.D.	
54) 2,4-Dinitrotoluene	9.622	165	162	54.56	ng/ml#	27
55) Dibenzofuran	0.000		0		N.D.	
56) 2,3,5,6-Tetrachlorophenol	0.000		0		N.D.	
57) 2,3,4,6-Tetrachlorophenol	0.000		0		N.D.	
58) Diethyl phthalate	9.873	149	66		N.D.	
59) 2,3,5-Trimethylnaphtha...	9.953	170	218		N.D.	
60) Fluorene	0.000		0		N.D.	
61) 4-Chlorophenyl phenyl ...	0.000		0		N.D.	
62) 4-Nitroaniline	0.000		0		N.D.	
63) 4,6-Dinitro-2-methylph...	0.000		0		N.D.	
65) N-Nitrosodiphenylamine	0.000		0		N.D.	
66) Azobenzene (1,2-DPH)	10.146	77	102		N.D.	
68) 4-Bromophenyl phenyl e...	0.000		0		N.D.	
69) Hexachlorobenzene	0.000		0		N.D.	
70) Pentachlorophenol (PCP)	10.697	266	86	77.32	ng/ml#	1
71) Phenanthrene	10.938	178	704		N.D.	
72) Anthracene	11.066	178	55		N.D.	
73) Carbazole	0.000		0		N.D.	
74) Di-n-butyl phthalate	11.531	149	415		N.D.	
75) Fluoranthene	12.200	202	80		N.D.	
76) Benzidine	12.382	184	157	123.65	ng/ml	67
77) Pyrene	0.000		0		N.D.	
80) Butyl benzyl phthalate	0.000		0		N.D.	
81) Bis(2-ethylhexyl) adipate	13.585	129	9301	23.55	ng/ml	88
82) 3,3-Dichlorobenzidine	14.543	252	83		Below Cal #	1
83) Benz(a)anthracene	14.532	228	4092	4.30	ng/ml	75
84) Chrysene	14.532	228	4039	4.53	ng/ml	74
85) Bis(2-ethylhexyl) phth...	14.676	149	608		N.D.	
87) Di-n-octyl phthalate	16.340	149	57	58.00	ng/ml#	42
88) Benzo(b)fluoranthene	17.062	252	58	8.02	ng/ml	57
89) Benzo(k)fluoranthene	17.062	252	58	8.54	ng/ml	57
90) Benzo(b+k)fluoranthene	17.062	252	58	15.80	ng/ml	57
91) Benzo(e)pyrene	0.000		0		N.D.	
92) Benzo(a)pyrene	0.000		0		N.D.	
93) Perylene	17.976	252	5976	7.75	ng/ml	78
95) Indeno(1,2,3-cd)pyrene	20.362	276	334		N.D.	
96) Dibenz(a,h)anthracene	20.426	278	53		N.D.	
97) Benzo(g,h,i)perylene	0.000		0		N.D.	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K27012\  
Data File : J11271906.D  
Acq On : 27 Nov 2019 11:10 am  
Operator : JK/ AMS/ DTH  
Sample : 9K27012-CCB1  
Misc : 1x, DCM + ISTD  
ALS Vial : 3 Sample Multiplier: 1  
DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:56:42 2019  
Quant Method : T:\methods\SV10\_091919R4.M  
Quant Title : EPA 8270D: Semivolatile Organics  
QLast Update : Fri Oct 25 11:15:50 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10





Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271913.D  
 Acq On : 27 Nov 2019 3:20 pm  
 Operator : JK/ AMS/ DTH  
 Sample : A9K0412-01RE1@10  
 Misc : 10x, 8270D TCLP REG LIST  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

AMS Roy  
 12/2/19

Quant Time: Dec 02 08:57:50 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	Qvalue
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.381	152	387154	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1427888	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	747611	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.932	188	1321721	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.526	240	1317590	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.971	264	1315281	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.357	292	1103753	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.118	112	23591	100.41	ng/ml	-0.03	
5) Phenol-d6 (Surr)	6.049	99	14317	47.61	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.931	82	43556	186.70	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.734	172	133484	228.14	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	16203	221.43	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	162799	268.12	ng/ml	0.00	
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	3.712	74	66	N.D.			
3) Pyridine	3.728	79	731m	2.91	ng/ml#		
6) Phenol	6.060	94	1505	4.55	ng/ml		87
7) Aniline	6.049	93	87	N.D.			
8) Bis(2-chloroethyl) ether	6.102	93	363	N.D.			
9) 2-Chlorophenol	6.199	128	610	N.D.			
10) 1,3-Dichlorobenzene	6.391	146	148	N.D.			
11) 1,4-Dichlorobenzene	6.391	146	148	N.D.			
12) Benzyl alcohol	0.000		0	N.D.			
13) 1,2-Dichlorobenzene	0.000		0	N.D.			
14) 2-Methylphenol	6.659	107	347	N.D.			
15) 2,2'-Oxybis(1-Chloropr...	6.643	45	314	N.D.			
16) N-Nitrosodi-n-propylamine	6.792	70	289	N.D.			
17) 3+4-Methylphenol	6.782	107	88	N.D.			
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	6.926	77	306	N.D.			
22) Isophorone	7.199	82	324	N.D.			
23) 2-Nitrophenol	7.279	139	190	43.65	ng/ml		66
24) 2,4-Dimethylphenol	7.317	122	110	N.D.			
25) Bis(2-chloroethoxy) me...	7.418	93	110	N.D.			
26) Benzoic acid	7.402	105	128	807.13	ng/ml#		25
27) 2,4-Dichlorophenol	7.547	162	269	26.13	ng/ml#		59
28) 1,2,4-Trichlorobenzene	0.000		0	N.D.			
29) Naphthalene	7.664	128	37529	49.96	ng/ml		97
30) 4-Chloroaniline	7.670	127	4936	33.43	ng/ml#		40
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	8.242	107	928	4.90	ng/ml		84
33) 2-Methylnaphthalene	8.365	142	34607	65.94	ng/ml		98
34) 1-Methylnaphthalene	8.466	142	20532	40.41	ng/ml		96
36) Hexachlorocyclopentadiene	8.541	237	51	N.D.			
37) 2,4,6-Trichlorophenol	8.664	196	431	26.67	ng/ml#		10
38) 2,4,5-Trichlorophenol	8.664	198	458	25.90	ng/ml#		50
39) 1,1'-Biphenyl	8.836	154	13102	20.39	ng/ml		96
41) 2-Chloronaphthalene	8.846	162	186	N.D.			
42) 2-Nitroaniline	8.975	138	56	30.86	ng/ml#		27
43) 2,6-Dimethylnaphthalene	9.001	156	13799	29.27	ng/ml		88

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271913.D  
 Acq On : 27 Nov 2019 3:20 pm  
 Operator : JK/ AMS/ DTH  
 Sample : A9K0412-01RE1@10  
 Misc : 10x, 8270D TCLP REG LIST  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Dec 02 08:57:50 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.108	168	373	72.63	ng/ml	70
45) Dimethyl phthalate	9.156	163	200	N.D.		
46) 1,3-Dinitrobenzene	9.108	168	373	62.70	ng/ml#	1
47) 2,6-Dinitrotoluene	9.194	165	154	26.30	ng/ml#	1
48) 1,2-Dinitrobenzene	0.000		0	N.D.		
49) Acenaphthylene	9.279	152	4827	6.35	ng/ml	86
50) 3-Nitroaniline	9.419	138	150	30.99	ng/ml#	1
51) Acenaphthene	9.456	153	85409	171.14	ng/ml	98
52) 2,4-Dinitrophenol	0.000		0	N.D.		
53) 4-Nitrophenol	9.536	139	349	78.44	ng/ml#	34
54) 2,4-Dinitrotoluene	9.627	165	531	57.03	ng/ml	69
55) Dibenzofuran	9.627	168	4833	7.26	ng/ml	91
56) 2,3,5,6-Tetrachlorophenol	0.000		0	N.D.		
57) 2,3,4,6-Tetrachlorophenol	0.000		0	N.D.		
58) Diethyl phthalate	9.857	149	537	N.D.		
59) 2,3,5-Trimethylnaphtha...	9.846	170	4855	11.46	ng/ml	79
60) Fluorene	9.980	166	31840	60.82	ng/ml	98
61) 4-Chlorophenyl phenyl ...	10.007	204	57	N.D.		
62) 4-Nitroaniline	9.975	138	403	5.02	ng/ml#	37
63) 4,6-Dinitro-2-methylph...	0.000		0	N.D.		
65) N-Nitrosodiphenylamine	10.109	169	2038	5.00	ng/ml#	1
66) Azobenzene (1,2-DPH)	10.125	77	654	N.D.		
68) 4-Bromophenyl phenyl e...	0.000		0	N.D.		
69) Hexachlorobenzene	0.000		0	N.D.		
70) Pentachlorophenol (PCP)	10.750	266	81	77.43	ng/ml#	18
71) Phenanthrene	10.959	178	146461	197.52	ng/ml	99
72) Anthracene	11.007	178	19839	27.83	ng/ml	97
73) Carbazole	11.178	167	9151	18.44	ng/ml	98
74) Di-n-butyl phthalate	11.526	149	2399	3.07	ng/ml	94
75) Fluoranthene	12.194	202	38408	50.54	ng/ml	98
76) Benzidine	12.323	184	77	123.39	ng/ml#	29
77) Pyrene	12.467	202	47758	61.75	ng/ml	98
80) Butyl benzyl phthalate	13.425	149	283	30.18	ng/ml	82
81) Bis(2-ethylhexyl) adipate	13.585	129	5217	17.07	ng/ml	92
82) 3,3-Dichlorobenzidine	14.543	252	50	Below Cal	#	1
83) Benz(a)anthracene	14.526	228	5365	7.29	ng/ml	65
84) Chrysene	14.575	228	1842	2.67	ng/ml	90
85) Bis(2-ethylhexyl) phth...	14.687	149	4329	9.13	ng/ml	84
87) Di-n-octyl phthalate	16.313	149	179	58.17	ng/ml#	9
88) Benzo(b)fluoranthene	17.046	252	255	8.31	ng/ml	82
89) Benzo(k)fluoranthene	17.115	252	137	8.66	ng/ml#	40
90) Benzo(b+k)fluoranthene	17.115	252	137	15.92	ng/ml#	40
91) Benzo(e)pyrene	17.709	252	175	N.D.		
92) Benzo(a)pyrene	17.816	252	465	10.54	ng/ml	46
93) Perylene	17.966	252	4332	7.30	ng/ml	68
95) Indeno(1,2,3-cd)pyrene	20.351	276	568	N.D.		
96) Dibenz(a,h)anthracene	20.421	278	81	N.D.		
97) Benzo(g,h,i)perylene	20.897	276	184	N.D.		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271913.D  
 Acq On : 27 Nov 2019 3:20 pm  
 Operator : JK/ AMS/ DTH  
 Sample : A9K0412-01RE1@10  
 Misc : 10x, 8270D TCLP REG LIST  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:57:50 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271917.D  
 Acq On : 27 Nov 2019 5:46 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BLK1  
 Misc : 1x, 8270D TCLP REG LIST  
 ALS Vial : 14 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

AMS  
12/2/19

Quant Time: Dec 02 08:58:10 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.380	152	394080	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.643	136	1457012	2000.00	ng/ml	-0.01	
35) Acenaphthene-d10 (ISTD)	9.424	162	767866	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.932	188	1355867	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.526	240	1379735	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.971	264	1341737	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthracene-d...	20.362	292	1150043	2000.00	ng/ml	0.01	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.129	112	216574	905.63	ng/ml	-0.02	
5) Phenol-d6 (Surr)	6.043	99	142916	466.90	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	414993	1747.59	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	1001180	1666.03	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	178651	2176.35	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.670	244	1503530	2364.65	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.728	74	241	N.D.			
3) Pyridine	3.776	79	689m	2.69	ng/ml#		
6) Phenol	6.054	94	3927	11.67	ng/ml#		45
7) Aniline	6.054	93	104	N.D.			
8) Bis(2-chloroethyl) ether	6.108	93	1918	6.31	ng/ml#		47
9) 2-Chlorophenol	6.193	128	287	N.D.			
10) 1,3-Dichlorobenzene	6.327	146	97	N.D.			
11) 1,4-Dichlorobenzene	6.397	146	142	N.D.			
12) Benzyl alcohol	6.536	108	550	27.76	ng/ml		80
13) 1,2-Dichlorobenzene	6.546	146	121	N.D.			
14) 2-Methylphenol	6.643	107	826	4.07	ng/ml#		43
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	182	N.D.			
16) N-Nitrosodi-n-propylamine	6.771	70	334	N.D.			
17) 3+4-Methylphenol	6.792	107	922	3.66	ng/ml#		1
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	6.931	77	1782	7.41	ng/ml#		39
22) Isophorone	7.183	82	1296	2.79	ng/ml		79
23) 2-Nitrophenol	7.274	139	296	44.37	ng/ml		70
24) 2,4-Dimethylphenol	7.327	122	399	N.D.			
25) Bis(2-chloroethoxy) me...	7.391	93	376	N.D.			
26) Benzoic acid	7.397	105	4681	845.56	ng/ml		73
27) 2,4-Dichlorophenol	0.000		0	N.D.			
28) 1,2,4-Trichlorobenzene	7.589	180	77	N.D.			
29) Naphthalene	7.664	128	9009	11.75	ng/ml		92
30) 4-Chloroaniline	7.723	127	149	13.85	ng/ml#		48
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	8.188	107	126	N.D.			
33) 2-Methylnaphthalene	8.365	142	2866	5.35	ng/ml		99
34) 1-Methylnaphthalene	8.466	142	2243	4.33	ng/ml		81
36) Hexachlorocyclopentadiene	0.000		0	N.D.			
37) 2,4,6-Trichlorophenol	8.670	196	230	25.27	ng/ml#		63
38) 2,4,5-Trichlorophenol	8.664	198	115	23.53	ng/ml		75
39) 1,1'-Biphenyl	8.835	154	3209	4.86	ng/ml		88
41) 2-Chloronaphthalene	8.857	162	221	N.D.			
42) 2-Nitroaniline	8.959	138	115	31.26	ng/ml#		52
43) 2,6-Dimethylnaphthalene	9.007	156	1604	3.31	ng/ml#		71

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271917.D  
 Acq On : 27 Nov 2019 5:46 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BLK1  
 Misc : 1x, 8270D TCLP REG LIST  
 ALS Vial : 14 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Dec 02 08:58:10 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.119	168	91	67.79	ng/ml#	15
45) Dimethyl phthalate	9.140	163	892	N.D.		
46) 1,3-Dinitrobenzene	9.156	168	63	58.67	ng/ml#	1
47) 2,6-Dinitrotoluene	9.194	165	990	32.77	ng/ml	70
48) 1,2-Dinitrobenzene	0.000		0	N.D.		
49) Acenaphthylene	9.279	152	1291	N.D.		
50) 3-Nitroaniline	9.370	138	234	31.66	ng/ml#	32
51) Acenaphthene	9.456	153	1622	3.16	ng/ml	91
52) 2,4-Dinitrophenol	0.000		0	N.D.		
53) 4-Nitrophenol	9.536	139	359	78.45	ng/ml#	8
54) 2,4-Dinitrotoluene	9.611	165	262	55.32	ng/ml#	72
55) Dibenzofuran	9.632	168	983	N.D.		
56) 2,3,5,6-Tetrachlorophenol	0.000		0	N.D.		
57) 2,3,4,6-Tetrachlorophenol	9.830	232	99	29.14	ng/ml#	1
58) Diethyl phthalate	9.857	149	3923	7.69	ng/ml	94
59) 2,3,5-Trimethylnaphtha...	9.841	170	1109	2.55	ng/ml#	49
60) Fluorene	9.980	166	2014	3.75	ng/ml	97
61) 4-Chlorophenyl phenyl ...	9.975	204	131	N.D.		
62) 4-Nitroaniline	10.002	138	91	N.D.		
63) 4,6-Dinitro-2-methylph...	0.000		0	N.D.		
65) N-Nitrosodiphenylamine	10.092	169	211	N.D.		
66) Azobenzene (1,2-DPH)	10.146	77	2771	6.55	ng/ml#	1
68) 4-Bromophenyl phenyl e...	10.472	248	88	N.D.		
69) Hexachlorobenzene	10.547	284	54	N.D.		
70) Pentachlorophenol (PCP)	10.766	266	186	78.47	ng/ml#	42
71) Phenanthrene	10.959	178	12163	15.99	ng/ml	83
72) Anthracene	11.007	178	1917	2.62	ng/ml	88
73) Carbazole	11.178	167	873	6.79	ng/ml	60
74) Di-n-butyl phthalate	11.526	149	17269	21.54	ng/ml	99
75) Fluoranthene	12.194	202	10727	13.76	ng/ml	97
76) Benzidine	12.344	184	57	123.28	ng/ml#	1
77) Pyrene	12.467	202	13893	17.51	ng/ml	99
80) Butyl benzyl phthalate	13.419	149	1951	34.82	ng/ml	82
81) Bis(2-ethylhexyl) adipate	13.580	129	21202	66.25	ng/ml	97
82) 3,3-Dichlorobenzidine	0.000		0	N.D.		
83) Benz(a)anthracene	14.521	228	6933	9.00	ng/ml	73
84) Chrysene	14.580	228	5024	6.96	ng/ml	93
85) Bis(2-ethylhexyl) phth...	14.682	149	29595	59.63	ng/ml	94
87) Di-n-octyl phthalate	16.334	149	101	58.06	ng/ml#	1
88) Benzo(b)fluoranthene	17.056	252	4367	13.87	ng/ml	94
89) Benzo(k)fluoranthene	17.121	252	1376	10.26	ng/ml	75
90) Benzo(b+k)fluoranthene	17.056	252	6227	23.82	ng/ml	94
91) Benzo(e)pyrene	17.704	252	3317	4.81	ng/ml	98
92) Benzo(a)pyrene	17.821	252	3735	15.35	ng/ml	96
93) Perylene	18.019	252	916	N.D.		
95) Indeno(1,2,3-cd)pyrene	20.340	276	4011	5.90	ng/ml	39
96) Dibenz(a,h)anthracene	20.405	278	673	N.D.		
97) Benzo(g,h,i)perylene	20.881	276	3701	5.67	ng/ml	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271917.D  
 Acq On : 27 Nov 2019 5:46 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BLK1  
 Misc : 1x, 8270D TCLP REG LIST  
 ALS Vial : 14 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:58:10 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271918.D  
 Acq On : 27 Nov 2019 6:22 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BS104  
 Misc : 4x, 8270D TCLP REG LIST  
 ALS Vial : 15 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

*AMS*  
*12/2/19*

Quant Time: Dec 02 08:58:15 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.380	152	397173	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1440071	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	754563	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1381861	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.543	240	1353668	2000.00	ng/ml	0.02	
86) Perylene-d12 (ISTD)	17.982	264	1400909	2000.00	ng/ml	0.02	
94) Dibenz(a,h)Anthracene-d...	20.373	292	1201078	2000.00	ng/ml	0.02	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.129	112	65176	270.42	ng/ml	-0.02	
5) Phenol-d6 (Surr)	6.044	99	49734	161.21	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	110087	459.98	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	300703	509.21	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	48750	593.62	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.671	244	415010	665.27	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.733	74	66715	440.98	ng/ml		92
3) Pyridine	3.760	79	76564m	296.86	ng/ml		
6) Phenol	6.054	94	96891	285.63	ng/ml		97
7) Aniline	6.065	93	83742	286.13	ng/ml		97
8) Bis(2-chloroethyl) ether	6.124	93	204249	667.17	ng/ml		99
9) 2-Chlorophenol	6.183	128	211497	752.05	ng/ml		96
10) 1,3-Dichlorobenzene	6.327	146	179830	568.90	ng/ml		98
11) 1,4-Dichlorobenzene	6.397	146	175414	564.62	ng/ml		98
12) Benzyl alcohol	6.525	108	104832	640.44	ng/ml		94
13) 1,2-Dichlorobenzene	6.552	146	181400	592.06	ng/ml		98
14) 2-Methylphenol	6.637	107	141744	692.88	ng/ml		97
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	155403	575.20	ng/ml		84
16) N-Nitrosodi-n-propylamine	6.782	70	137340	772.69	ng/ml		93
17) 3+4-Methylphenol	6.787	107	164984	650.40	ng/ml		95
18) Hexachloroethane	6.883	201	57270	599.95	ng/ml		93
20) Nitrobenzene	6.947	77	172098	709.74	ng/ml		89
22) Isophorone	7.183	82	399524	870.22	ng/ml		98
23) 2-Nitrophenol	7.263	139	153485	1124.88	ng/ml		88
24) 2,4-Dimethylphenol	7.311	122	182084	943.06	ng/ml		96
25) Bis(2-chloroethoxy) me...	7.397	93	249066	892.37	ng/ml		99
26) Benzoic acid	7.391	105	62906	1336.39	ng/ml		91
27) 2,4-Dichlorophenol	7.509	162	202563	939.82	ng/ml		97
28) 1,2,4-Trichlorobenzene	7.589	180	171765	681.50	ng/ml		96
29) Naphthalene	7.670	128	569197	751.36	ng/ml		100
30) 4-Chloroaniline	7.728	127	141359	595.51	ng/ml		97
31) Hexachlorobutadiene	7.798	225	81976	601.90	ng/ml		97
32) 4-Chloro-3-methylphenol	8.215	107	182846	956.88	ng/ml		92
33) 2-Methylnaphthalene	8.365	142	422199	797.64	ng/ml		99
34) 1-Methylnaphthalene	8.466	142	401245	783.06	ng/ml		98
36) Hexachlorocyclopentadiene	8.536	237	92247	790.58	ng/ml		100
37) 2,4,6-Trichlorophenol	8.654	196	154176	1055.84	ng/ml		99
38) 2,4,5-Trichlorophenol	8.696	198	154020	1068.74	ng/ml		96
39) 1,1'-Biphenyl	8.836	154	1331	N.D.			
41) 2-Chloronaphthalene	8.857	162	413419	882.62	ng/ml		97
42) 2-Nitroaniline	8.959	138	156309	1114.73	ng/ml		88
43) 2,6-Dimethylnaphthalene	9.001	156	325	N.D.			

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271918.D  
 Acq On : 27 Nov 2019 6:22 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BS1@4  
 Misc : 4x, 8270D TCLP REG LIST  
 ALS Vial : 15 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:58:15 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	75791	1271.10	ng/ml	77
45) Dimethyl phthalate	9.146	163	568734	1043.69	ng/ml	99
46) 1,3-Dinitrobenzene	9.172	168	83870	1114.84	ng/ml	88
47) 2,6-Dinitrotoluene	9.205	165	128813	1050.02	ng/ml	91
48) 1,2-Dinitrobenzene	9.258	168	57365	1039.11	ng/ml	83
49) Acenaphthylene	9.279	152	702000	915.19	ng/ml	99
50) 3-Nitroaniline	9.376	138	92086	960.72	ng/ml	84
51) Acenaphthene	9.456	153	428944	851.59	ng/ml	98
52) 2,4-Dinitrophenol	9.483	184	40811	1305.14	ng/ml	87
53) 4-Nitrophenol	9.563	139	25067	400.75	ng/ml	93
54) 2,4-Dinitrotoluene	9.616	165	161541	1054.23	ng/ml	81
55) Dibenzofuran	9.632	168	637588	949.58	ng/ml	96
56) 2,3,5,6-Tetrachlorophenol	9.718	232	121220	1048.34	ng/ml	95
57) 2,3,4,6-Tetrachlorophenol	9.761	232	127771	1009.11	ng/ml	98
58) Diethyl phthalate	9.862	149	536901	1070.36	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	9.836	170	113	N.D.		
60) Fluorene	9.980	166	499777	945.83	ng/ml	98
61) 4-Chlorophenyl phenyl ...	9.980	204	249715	969.39	ng/ml	91
62) 4-Nitroaniline	10.002	138	95166	1173.61	ng/ml	90
63) 4,6-Dinitro-2-methylph...	10.034	198	77296	1359.45	ng/ml	87
65) N-Nitrosodiphenylamine	10.098	169	428604	1005.94	ng/ml	99
66) Azobenzene (1,2-DPH)	10.141	77	362440	840.59	ng/ml	85
68) 4-Bromophenyl phenyl e...	10.478	248	151474	971.44	ng/ml	95
69) Hexachlorobenzene	10.552	284	177332	948.00	ng/ml	99
70) Pentachlorophenol (PCP)	10.750	266	82843	893.79	ng/ml	98
71) Phenanthrene	10.959	178	736917	950.58	ng/ml	99
72) Anthracene	11.012	178	744713	999.37	ng/ml	99
73) Carbazole	11.173	167	665288	1212.02	ng/ml	100
74) Di-n-butyl phthalate	11.531	149	880661	1077.62	ng/ml	99
75) Fluoranthene	12.200	202	849500	1069.16	ng/ml	97
76) Benzidine	12.355	184	63092	433.88	ng/ml	95
77) Pyrene	12.473	202	857296	1060.25	ng/ml	99
80) Butyl benzyl phthalate	13.425	149	381342	1095.88	ng/ml	87
81) Bis(2-ethylhexyl) adipate	13.590	129	337238	1074.14	ng/ml	99
82) 3,3-Dichlorobenzidine	14.489	252	315854	3159.10	ng/ml	97
83) Benz(a)anthracene	14.516	228	796923	1054.43	ng/ml	97
84) Chrysene	14.591	228	734532	1037.08	ng/ml	98
85) Bis(2-ethylhexyl) phth...	14.692	149	551876	1133.38	ng/ml	99
87) Di-n-octyl phthalate	16.345	149	892063	1102.95	ng/ml	99
88) Benzo(b)fluoranthene	17.072	252	784985	1016.31	ng/ml	98
89) Benzo(k)fluoranthene	17.131	252	782188	1004.23	ng/ml	98
90) Benzo(b+k)fluoranthene	17.072	252	1594050	2008.90	ng/ml	98
91) Benzo(e)pyrene	17.709	252	288	N.D.		
92) Benzo(a)pyrene	17.832	252	696851	993.60	ng/ml	97
93) Perylene	18.035	252	1223	N.D.		
95) Indeno(1,2,3-cd)pyrene	20.362	276	697241	981.69	ng/ml	100
96) Dibenz(a,h)anthracene	20.437	278	667686	1023.91	ng/ml	98
97) Benzo(g,h,i)perylene	20.902	276	742971	1089.07	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271918.D  
 Acq On : 27 Nov 2019 6:22 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BS1@4  
 Misc : 4x, 8270D TCLP REG LIST  
 ALS Vial : 15 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:58:15 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271919.D  
 Acq On : 27 Nov 2019 6:57 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BSD1@4  
 Misc : 4x, 8270D TCLP REG LIST  
 ALS Vial : 16 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

*AMS*  
*12/2/19*  
*Q-19*

Quant Time: Dec 02 08:58:21 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.386	152	395328	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.648	136	1442068	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	750392	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1353081	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.537	240	1174680	2000.00	ng/ml	0.01	
86) Perylene-d12 (ISTD)	17.982	264	1125325	2000.00	ng/ml	0.02	
94) Dibenz(a,h)Anthrcene-d...	20.373	292	934790	2000.00	ng/ml	0.02	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.124	112	66137	275.69	ng/ml	-0.03	
5) Phenol-d6 (Surr)	6.044	99	55291	180.06	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.931	82	112466	472.11	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.739	172	317332	540.36	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	46167	574.84	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.671	244	363465	671.42	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.706	74	62811m	417.12	ng/ml		
3) Pyridine	3.728	79	71907m	280.10	ng/ml		
6) Phenol	6.054	94	102248	302.83	ng/ml		97
7) Aniline	6.065	93	76856	263.83	ng/ml		90
8) Bis(2-chloroethyl) ether	6.124	93	216329	709.92	ng/ml		99
9) 2-Chlorophenol	6.183	128	211430	755.32	ng/ml		97
10) 1,3-Dichlorobenzene	6.332	146	201478	640.36	ng/ml		97
11) 1,4-Dichlorobenzene	6.402	146	198600	642.23	ng/ml		96
12) Benzyl alcohol	6.525	108	109700	671.83	ng/ml		95
13) 1,2-Dichlorobenzene	6.552	146	202301	663.36	ng/ml		97
14) 2-Methylphenol	6.637	107	144553	709.91	ng/ml		99
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	159140	591.78	ng/ml		83
16) N-Nitrosodi-n-propylamine	6.782	70	137854	779.20	ng/ml		91
17) 3+4-Methylphenol	6.792	107	167404	663.02	ng/ml		98
18) Hexachloroethane	6.883	201	62589	658.73	ng/ml		95
20) Nitrobenzene	6.947	77	178099	737.91	ng/ml		88
22) Isophorone	7.183	82	396335	862.08	ng/ml		99
23) 2-Nitrophenol	7.268	139	150311	1101.09	ng/ml		85
24) 2,4-Dimethylphenol	7.311	122	178578	923.63	ng/ml		96
25) Bis(2-chloroethoxy) me...	7.397	93	247039	883.88	ng/ml		99
26) Benzoic acid	7.391	105	51623	1241.78	ng/ml		92
27) 2,4-Dichlorophenol	7.514	162	197907	917.32	ng/ml		95
28) 1,2,4-Trichlorobenzene	7.595	180	192615	763.17	ng/ml		98
29) Naphthalene	7.670	128	611179	805.66	ng/ml		99
30) 4-Chloroaniline	7.734	127	136426	574.06	ng/ml		96
31) Hexachlorobutadiene	7.803	225	94495	692.85	ng/ml		98
32) 4-Chloro-3-methylphenol	8.215	107	178060	930.54	ng/ml		94
33) 2-Methylnaphthalene	8.365	142	452102	852.95	ng/ml		99
34) 1-Methylnaphthalene	8.466	142	424437	827.18	ng/ml		99
36) Hexachlorocyclopentadiene	8.536	237	98626	849.95	ng/ml		97
37) 2,4,6-Trichlorophenol	8.654	196	149523	1030.36	ng/ml		99
38) 2,4,5-Trichlorophenol	8.696	198	147346	1028.96	ng/ml		98
39) 1,1'-Biphenyl	8.841	154	1716	2.66	ng/ml		97
41) 2-Chloronaphthalene	8.857	162	427591	917.95	ng/ml		97
42) 2-Nitroaniline	8.964	138	144507	1039.66	ng/ml		83
43) 2,6-Dimethylnaphthalene	9.012	156	235	N.D.			

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271919.D  
 Acq On : 27 Nov 2019 6:57 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BSD1@4  
 Misc : 4x, 8270D TCLP REG LIST  
 ALS Vial : 16 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Dec 02 08:58:21 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	68479	1166.47	ng/ml	82
45) Dimethyl phthalate	9.146	163	558558	1030.71	ng/ml	99
46) 1,3-Dinitrobenzene	9.173	168	79914	1071.30	ng/ml	89
47) 2,6-Dinitrotoluene	9.205	165	126627	1038.15	ng/ml	90
48) 1,2-Dinitrobenzene	9.258	168	56732	1033.35	ng/ml	83
49) Acenaphthylene	9.279	152	716676	939.52	ng/ml	99
50) 3-Nitroaniline	9.381	138	85092	880.46	ng/ml	84
51) Acenaphthene	9.456	153	454556	907.46	ng/ml	99
52) 2,4-Dinitrophenol	9.483	184	33659	1141.06	ng/ml	87
53) 4-Nitrophenol	9.563	139	21189	352.60	ng/ml	92
54) 2,4-Dinitrotoluene	9.616	165	154087	1012.93	ng/ml	84
55) Dibenzofuran	9.633	168	635490	951.72	ng/ml	97
56) 2,3,5,6-Tetrachlorophenol	9.718	232	116241	1012.52	ng/ml	97
57) 2,3,4,6-Tetrachlorophenol	9.761	232	120527	958.55	ng/ml	98
58) Diethyl phthalate	9.863	149	518523	1039.46	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	9.852	170	119	N.D.		
60) Fluorene	9.980	166	503975	959.08	ng/ml	99
61) 4-Chlorophenyl phenyl ...	9.980	204	244758	955.42	ng/ml	93
62) 4-Nitroaniline	10.002	138	85128	1055.66	ng/ml	95
63) 4,6-Dinitro-2-methylph...	10.034	198	67248	1217.07	ng/ml	89
65) N-Nitrosodiphenylamine	10.098	169	412201	988.02	ng/ml	99
66) Azobenzene (1,2-DPH)	10.141	77	349050	826.75	ng/ml	87
68) 4-Bromophenyl phenyl e...	10.478	248	150154	983.46	ng/ml	96
69) Hexachlorobenzene	10.552	284	172196	940.12	ng/ml	98
70) Pentachlorophenol (PCP)	10.750	266	73578	817.64	ng/ml	98
71) Phenanthrene	10.959	178	706810	931.13	ng/ml	99
72) Anthracene	11.012	178	711486	975.09	ng/ml	99
73) Carbazole	11.173	167	604593	1084.90	ng/ml	98
74) Di-n-butyl phthalate	11.531	149	796097	994.87	ng/ml	99
75) Fluoranthene	12.200	202	777553	999.42	ng/ml	98
76) Benzidine	12.355	184	70621	478.26	ng/ml	99
77) Pyrene	12.467	202	790784	998.80	ng/ml	99
80) Butyl benzyl phthalate	13.425	149	319250	1059.03	ng/ml	90
81) Bis(2-ethylhexyl) adipate	13.591	129	272403	999.84	ng/ml	99
82) 3,3-Dichlorobenzidine	14.494	252	215544	2388.85	ng/ml	99
83) Benz(a)anthracene	14.510	228	666604	1016.40	ng/ml	97
84) Chrysene	14.591	228	626259	1018.94	ng/ml	98
85) Bis(2-ethylhexyl) phth...	14.692	149	478081	1131.43	ng/ml	98
87) Di-n-octyl phthalate	16.345	149	690638	1065.61	ng/ml	97
88) Benzo(b)fluoranthene	17.072	252	630715	1016.55	ng/ml	98
89) Benzo(k)fluoranthene	17.137	252	636425	1017.45	ng/ml	97
90) Benzo(b+k)fluoranthene	17.137	252	1291071	2025.49	ng/ml	97
91) Benzo(e)pyrene	17.704	252	1111	N.D.		
92) Benzo(a)pyrene	17.832	252	552727	981.23	ng/ml	99
93) Perylene	18.062	252	1225	N.D.		
95) Indeno(1,2,3-cd)pyrene	20.362	276	549172	993.48	ng/ml	99
96) Dibenz(a,h)anthracene	20.437	278	524558	1033.57	ng/ml	98
97) Benzo(g,h,i)perylene	20.902	276	581673	1095.52	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K27012\  
 Data File : J11271919.D  
 Acq On : 27 Nov 2019 6:57 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111296-BSD1@4  
 Misc : 4x, 8270D TCLP REG LIST  
 ALS Vial : 16 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Dec 02 08:58:21 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



**TCLP Semivolatile Organic Compounds by EPA 8270D  
Benchsheet & Analysis Sequence Data**

Sequence 9K26022 (QC Only)



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence: **9K26022**

Instrument: **SV-GCMS10**

Date: **11/26/19 07:56**

Calibration: **A9I2405**

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
1	9K26022-TUN1	Water	QC	QC			A19I086	A19K329
2	9K26022-CCV1	Water	QC	QC			A19I086	A19G243
3	9K26022-IBL1	Water	QC	QC			A19I086	
4	9K26022-TUN2	Water	QC	QC			A19I086	A19K329
5	9K26022-CCV2	Water	QC	QC			A19I086	A19G243
6	9K26022-CCB1	Water	QC	QC			A19I086	
7	9111196-BLK1	Water	QC	QC		9111196	A19I086	
8	9111196-BS1	Water	QC	QC		9111196	A19I086	
9	9111196-BSD1	Water	QC	QC		9111196	A19I086	
10	A9K0666-01RE1	Soil	8270D LL Full List		11/26/19	9111140	A19I086	
11	A9K0330-01RE1	Soil	1311/8270D TCLP SVOC Reg List	Anchor QEA, LLC	11/25/19	9111111	A19I086	
12	A9K0692-05RE1	Soil	8270D LL PAH/PHTH/Phenols	Anchor QEA, LLC	12/06/19	9111141	A19I086	
13	A9K0692-06RE2	Soil	8270D LL PAH/PHTH/Phenols	Anchor QEA, LLC	12/06/19	9111141	A19I086	
14	9111141-MS2	Soil	QC	QC		9111141	A19I086	
15	9111141-MSD2	Soil	QC	QC		9111141	A19I086	
16	A9K0692-07RE1	Soil	8270D LL PAH/PHTH/Phenols	Anchor QEA, LLC	12/06/19	9111141	A19I086	
17	A9K0692-08RE1	Soil	8270D LL PAH/PHTH/Phenols	Anchor QEA, LLC	12/06/19	9111141	A19I086	
18	A9K0692-11RE1	Soil	8270D LL PAH/PHTH/Phenols	Anchor QEA, LLC	12/06/19	9111141	A19I086	
19	9111242-BLK1	Soil	QC	QC		9111242	A19I086	
20	9111242-BS1	Soil	QC	QC		9111242	A19I086	
21	9111242-BSD1	Soil	QC	QC		9111242	A19I086	
22	A9K0412-01	Soil	1311/8270D TCLP SVOC Reg List	Anchor QEA, LLC	11/27/19	9111242	A19I086	
23	A9K0656-06	Soil	8270D LL Full List	(QC Source)		9111249	A19I086	
24	"	Soil	8270D LL PAH/PHTH/Phenols	"	12/09/19	9111249	A19I086	
25	A9K0808-13	Soil	8270D LL PAH/PHTH/Phenols		12/02/19	9111249	A19I086	
26	A9K0769-01	Water	625 LL Full List (All Compounds)		12/03/19	9111196	A19I086	
27	A9K0764-01	Water	625 LL Full List (All Compounds)		12/03/19	9111159	A19I086	
28	A9K0764-02	Water	625 LL Full List (All Compounds)		12/03/19	9111159	A19I086	
29	A9K0765-01	Water	625 LL Full List (All Compounds)		12/03/19	9111159	A19I086	
30	A9K0767-01	Water	625 LL Full List (All Compounds)		12/03/19	9111159	A19I086	
31	A9K0768-01	Water	625 LL Full List (All Compounds)		12/03/19	9111159	A19I086	
32	9K26022-IBL2	Water	QC	QC			A19I086	

Data Entered By:

*AMS 11/27/19*

Comments:

Data Reviewed By:

*AMS 11/27/19*



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence: **9K26022**

Instrument: **SV-GCMS10**

Date: **11/26/19 07:56**

Calibration: **A9I2405**

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
1	9K26022-TUN1	Water	QC	QC			A19I086	A19K329
2	9K26022-CCV1	Water	QC	QC			A19I086	A19G243
3	9K26022-IBL1	Water	QC	QC			A19I086	
4	9K26022-TUN2	Water	QC	QC			A19I086	A19K329
5	9K26022-CCV2	Water	QC	QC			A19I086	A19G243
6	9K26022-CCB1	Water	QC	QC			A19I086	
7	9111196-BLK1	Water	QC	QC		9111196	A19I086	
8	9111196-BS1	Water	QC	QC		9111196	A19I086	
9	9111196-BSD1	Water	QC	QC		9111196	A19I086	
10	A9K0666-01RE1	Soil	8270D LL Full List		11/26/19	9111140	A19I086	
11	A9K0330-01RE1	Soil	1311/8270D TCLP SVOC Reg List	Anchor QEA, LLC	11/25/19	9111111	A19I086	

*Partial*

Data Entered By: *AMS 11/26/19*

Comments:



Data Reviewed By: *JD 11/26/19*

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261901.D  
 Acq On : 26 Nov 2019 8:03 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-TUN1  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1

*AMS Q14*  
*11/26/19*

Integration File: rteint.p

Method : T:\methods\DFTPP.M  
 Title : 8270 DFTPP Tune Method  
 Last Update : Mon Nov 11 08:41:49 2019



AutoFind: Scans 1454, 1455, 1456; Background Corrected with Scan 1449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	1609	PASS
69	198	0.01	100	19.2	103285	PASS
70	69	0.00	2	0.6	589	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	537963	PASS
199	198	5	9	6.9	37056	PASS
365	198	1	100	3.7	19845	PASS
441	443	0.01	150	77.2	99659	PASS
442	198	0.10	200	122.1	656725	PASS
443	442	15	24	19.7	129139	PASS



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261901.D  
 Acq On : 26 Nov 2019 8:03 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-TUN1  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M


Quant Time: Nov 26 12:45:29 2019  
 Quant Method : T:\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Mon Nov 11 08:41:49 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.413	150	151907	2.00	ug/mL	0.00
2) Naphthalene-d8	7.675	136	417377	2.00	ug/mL	0.00
3) Acenaphthene-d10	9.451	162	209283	2.00	ug/mL	0.00
5) Phenanthrene-d10	10.964	188	368353	2.00	ug/mL	0.00
11) Chrysene-d12	14.564	240	278948	2.00	ug/mL	-0.02
12) Perylene-d12	16.842	264	269993	2.00	ug/mL	#-0.07
Target Compounds						
4) Pentachlorophenol	10.782	266	798437	40.40	ug/mL	85
6) DFTPP	11.269	442	748623	25.17	ug/mL	83
7) Benzidine	12.392	184	2933900	22.39	ug/mL	97
8) 4,4-DDE	12.638	TIC	40828	No Calib		
9) 4,4-DDD	13.120	TIC	497051	No Calib		
10) 4,4-DDT	13.644	TIC	8965831	23.74	ug/mL	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
Data File : J11261901.D  
Acq On : 26 Nov 2019 8:03 am  
Operator : JK/ AMS/ DTH  
Sample : 9K26022-TUN1  
Misc : 1x, A19K329 DFTPP@45  
ALS Vial : 1 Sample Multiplier: 1  
DataAcq Meth:DFTPP.M

Quant Time: Nov 26 12:45:29 2019  
Quant Method : T:\methods\DFTPP.M  
Quant Title : 8270 DFTPP Tune Method  
QLast Update : Mon Nov 11 08:41:49 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261902.D  
 Acq On : 26 Nov 2019 8:31 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV1  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

AMS  
11/26/19 Q-14

Quant Time: Nov 26 12:45:46 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) 1,4-Dichlorobenzene-d4...	6.380	152	375653	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1386656	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	735483	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.932	188	1396742	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.532	240	1317715	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.971	264	1300844	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthracene-d...	20.362	292	1110306	2000.00	ng/ml	0.01	
System Monitoring Compounds							
4) 2-Fluorophenol (Surr)	5.118	112	235015	1030.95	ng/ml	-0.03	
5) Phenol-d6 (Surr)	6.038	99	266242	912.47	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	202401	894.15	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	605736	1052.36	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	82737	983.16	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	661804	1089.83	ng/ml	0.00	
Target Compounds							
							Qvalue
2) N-Nitrosodimethylamine	3.701	74	124043m	866.89	ng/ml		
3) Pyridine	3.717	79	205152m	840.99	ng/ml		
6) Phenol	6.049	94	285860	890.98	ng/ml		98
7) Aniline	6.065	93	146005	527.46	ng/ml		92
8) Bis(2-chloroethyl) ether	6.124	93	295019	1018.87	ng/ml		97
9) 2-Chlorophenol	6.183	128	268664	1010.06	ng/ml		97
10) 1,3-Dichlorobenzene	6.327	146	303399	1014.80	ng/ml		98
11) 1,4-Dichlorobenzene	6.396	146	295937	1007.12	ng/ml		99
12) Benzyl alcohol	6.520	108	144213	917.65	ng/ml		95
13) 1,2-Dichlorobenzene	6.552	146	293073	1011.34	ng/ml		98
14) 2-Methylphenol	6.637	107	189930	981.61	ng/ml		98
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	185393	725.52	ng/ml		80
16) N-Nitrosodi-n-propylamine	6.782	70	141801	843.49	ng/ml		91
17) 3+4-Methylphenol	6.787	107	242984	1012.77	ng/ml		97
18) Hexachloroethane	6.883	201	105180	1164.97	ng/ml		93
20) Nitrobenzene	6.947	77	200629	874.80	ng/ml		92
22) Isophorone	7.183	82	414039	936.58	ng/ml		98
23) 2-Nitrophenol	7.263	139	175036	1323.76	ng/ml		91
24) 2,4-Dimethylphenol	7.311	122	218322	1174.31	ng/ml		96
25) Bis(2-chloroethoxy) me...	7.397	93	265383	987.45	ng/ml		99
26) Benzoic acid	7.413	105	196184	2472.42	ng/ml		94
27) 2,4-Dichlorophenol	7.509	162	223930	1076.97	ng/ml		96
28) 1,2,4-Trichlorobenzene	7.589	180	266794	1099.31	ng/ml		99
29) Naphthalene	7.669	128	755556	1035.77	ng/ml		100
30) 4-Chloroaniline	7.728	127	174605	763.79	ng/ml		97
31) Hexachlorobutadiene	7.798	225	141788	1081.16	ng/ml		98
32) 4-Chloro-3-methylphenol	8.215	107	196461	1067.74	ng/ml		91
33) 2-Methylnaphthalene	8.365	142	547082	1073.39	ng/ml		98
34) 1-Methylnaphthalene	8.466	142	517474	1048.80	ng/ml		98
36) Hexachlorocyclopentadiene	8.536	237	144244	1268.27	ng/ml		95
37) 2,4,6-Trichlorophenol	8.654	196	165182	1157.73	ng/ml		97
38) 2,4,5-Trichlorophenol	8.691	198	160864	1143.61	ng/ml		99
39) 1,1'-Biphenyl	8.835	154	633467	1002.07	ng/ml		98
41) 2-Chloronaphthalene	8.857	162	499631	1094.35	ng/ml		97
42) 2-Nitroaniline	8.958	138	161452	1178.28	ng/ml		87
43) 2,6-Dimethylnaphthalene	8.996	156	482865	1041.20	ng/ml		97

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261902.D  
 Acq On : 26 Nov 2019 8:31 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV1  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Nov 26 12:45:46 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	75405	1294.66	ng/ml	76
45) Dimethyl phthalate	9.146	163	566999	1067.50	ng/ml	98
46) 1,3-Dinitrobenzene	9.172	168	86707	1177.80	ng/ml	87
47) 2,6-Dinitrotoluene	9.205	165	130369	1089.58	ng/ml	88
48) 1,2-Dinitrobenzene	9.258	168	61093	1135.34	ng/ml	81
49) Acenaphthylene	9.279	152	789520	1055.99	ng/ml	100
50) 3-Nitroaniline	9.376	138	100432	1103.67	ng/ml	88
51) Acenaphthene	9.456	153	491869	1001.85	ng/ml	99
52) 2,4-Dinitrophenol	9.483	184	44632	1418.72	ng/ml	88
53) 4-Nitrophenol	9.558	139	78893	1083.29	ng/ml	92
54) 2,4-Dinitrotoluene	9.616	165	170877	1140.53	ng/ml	82
55) Dibenzofuran	9.632	168	703328	1074.66	ng/ml	97
56) 2,3,5,6-Tetrachlorophenol	9.718	232	131889	1164.63	ng/ml	96
57) 2,3,4,6-Tetrachlorophenol	9.761	232	138919	1122.62	ng/ml	98
58) Diethyl phthalate	9.862	149	528033	1079.99	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	9.846	170	457749	1098.36	ng/ml	94
60) Fluorene	9.980	166	538936	1046.40	ng/ml	97
61) 4-Chlorophenyl phenyl ...	9.975	204	275085	1095.57	ng/ml	95
62) 4-Nitroaniline	9.996	138	106043	1341.67	ng/ml	92
63) 4,6-Dinitro-2-methylph...	10.028	198	72051	1309.99	ng/ml	96
65) N-Nitrosodiphenylamine	10.098	169	461764	1072.22	ng/ml	100
66) Azobenzene (1,2-DPH)	10.141	77	383878	880.82	ng/ml	85
68) 4-Bromophenyl phenyl e...	10.477	248	163215	1035.59	ng/ml	95
69) Hexachlorobenzene	10.552	284	190684	1008.52	ng/ml	96
70) Pentachlorophenol (PCP)	10.750	266	90227	957.35	ng/ml	99
71) Phenanthrene	10.959	178	782758	998.95	ng/ml	99
72) Anthracene	11.012	178	787242	1045.19	ng/ml	99
73) Carbazole	11.173	167	656644	1168.90	ng/ml	99
74) Di-n-butyl phthalate	11.526	149	878243	1063.22	ng/ml	99
75) Fluoranthene	12.194	202	870456	1083.86	ng/ml	98
76) Benzidine	12.350	184	325614	1695.82	ng/ml	96
77) Pyrene	12.467	202	874172	1069.61	ng/ml	99
80) Butyl benzyl phthalate	13.425	149	389511	1147.29	ng/ml	88
81) Bis(2-ethylhexyl) adipate	13.585	129	335565	1097.98	ng/ml	99
82) 3,3-Dichlorobenzidine	14.484	252	219284	2129.14	ng/ml	98
83) Benz(a)anthracene	14.505	228	777756	1057.15	ng/ml	98
84) Chrysene	14.585	228	735623	1066.96	ng/ml	97
85) Bis(2-ethylhexyl) phth...	14.687	149	537116	1133.16	ng/ml	98
87) Di-n-octyl phthalate	16.334	149	887370	1176.37	ng/ml	98
88) Benzo(b)fluoranthene	17.056	252	782625	1089.90	ng/ml	98
89) Benzo(k)fluoranthene	17.126	252	758777	1050.04	ng/ml	99
90) Benzo(b+k)fluoranthene	17.126	252	1569485	2129.89	ng/ml	99
91) Benzo(e)pyrene	17.709	252	745778	1115.43	ng/ml	99
92) Benzo(a)pyrene	17.827	252	723436	1109.66	ng/ml	99
93) Perylene	18.030	252	630156	1074.14	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.351	276	663411	1010.42	ng/ml	99
96) Dibenz(a,h)anthracene	20.426	278	653462	1084.02	ng/ml	99
97) Benzo(g,h,i)perylene	20.891	276	696906	1105.06	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261902.D  
 Acq On : 26 Nov 2019 8:31 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV1  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:45:46 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10





Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261904.D  
 Acq On : 26 Nov 2019 9:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-TUN2  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1

*AMS*  
*11/26/19*

Integration File: rteint.p

Method : T:\methods\DFTPP.M  
 Title : 8270 DFTPP Tune Method  
 Last Update : Mon Nov 11 08:41:49 2019



AutoFind: Scans 1453, 1454, 1455; Background Corrected with Scan 1448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.3	1505	PASS
69	198	0.01	100	19.5	113411	PASS
70	69	0.00	2	0.6	635	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	582251	PASS
199	198	5	9	7.1	41381	PASS
365	198	1	100	3.6	20731	PASS
441	443	0.01	150	76.4	100467	PASS
442	198	0.10	200	112.5	654869	PASS
443	442	15	24	20.1	131573	PASS

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261904.D  
 Acq On : 26 Nov 2019 9:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-TUN2  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Nov 26 12:46:19 2019  
 Quant Method : T:\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Mon Nov 11 08:41:49 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10




Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.413	150	157228	2.00	ug/mL	0.00
2) Naphthalene-d8	7.675	136	422577	2.00	ug/mL	0.00
3) Acenaphthene-d10	9.451	162	221217	2.00	ug/mL	0.00
5) Phenanthrene-d10	10.964	188	375451	2.00	ug/mL	0.00
11) Chrysene-d12	14.559	240	298671	2.00	ug/mL	-0.02
12) Perylene-d12	16.971	264	441	2.00	ug/mL	# 0.06
-----						
Target Compounds						
4) Pentachlorophenol	10.782	266	751961	36.00	ug/mL	81
6) DFTPP	11.269	442	757802	25.00	ug/mL#	68
7) Benzidine	12.392	184	3187313	23.86	ug/mL	96
8) 4,4-DDE	12.633	TIC	38705	No Calib		
9) 4,4-DDD	13.114	TIC	19179	No Calib		
10) 4,4-DDT	13.633	TIC	9750678	25.33	ug/mL	94
-----						

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261904.D  
 Acq On : 26 Nov 2019 9:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-TUN2  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Nov 26 12:46:19 2019  
 Quant Method : T:\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Mon Nov 11 08:41:49 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J11261904.D\data.ms

(4) Pentachlorophenol

10.782min (-0.005) 36.00 ug/mL

response 751961




Ion	Exp%	Act%
265.90	100.00	100.00
164.90	50.60	35.84
201.90	25.80	21.81
129.90	27.30	14.99



Quantitation Report (Qedit)

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261904.D  
 Acq On : 26 Nov 2019 9:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-TUN2  
 Misc : 1x, A19K329 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Nov 26 12:46:19 2019  
 Quant Method : T:\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Mon Nov 11 08:41:49 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J11261904.D\data.ms

(7) Benzidine

12.392min (-0.011) 23.86 ug/mL

response 3187313 ✓

Ion	Exp%	Act%
184.10	100.00	100.00
156.10	8.50	6.95
92.10	8.20	7.23
0.00	0.00	0.00

### DDT Breakdown Check (Validated 5/1/2013)


From:  
9K26022-TUN2  
SV-GCMS10

First Column Area Counts	Percent Breakdown	
DDE	38705	
DDD	19179	✓
<b>DDT</b>	<b>9750678</b>	<b>0.59</b> <b>PASS</b>

Breakdown must be less than 20% to accept sample data.

Data Path : T:\data\2019-11\9K26022\  
Data File : J11261904.D  
Acq On : 26 Nov 2019 9:49 am  
Operator : JK/ AMS/ DTH  
Sample : 9K26022-TUN2  
Misc : 1x, A19K329 DFTPP@45  
ALS Vial : 1 Sample Multiplier: 1  
DataAcq Meth:DFTPP.M

Quant Time: Nov 26 12:46:19 2019  
Quant Method : T:\methods\DFTPP.M  
Quant Title : 8270 DFTPP Tune Method  
QLast Update : Mon Nov 11 08:41:49 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10



Evaluate Continuing Calibration Report

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261905.D  
 Acq On : 26 Nov 2019 10:16 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:47:30 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*AMS*  
*11/26/19*

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4 (IST	2000.000	2000.000	0.0	127	-0.01
2 TG	N-Nitrosodimethylamine	1000.000	896.063	10.4	118	-0.04
3 TG	Pyridine	1000.000	891.192	10.9	115	-0.04
4 S	2-Fluorophenol (Surr)	1000.000	1055.222	-5.5	129	-0.03
5 S	Phenol-d6(Surr)	1000.000	964.140	3.6	113	-0.01
6 T	Phenol	1000.000	925.740	7.4	109	-0.01
7 T	Aniline	1000.000	731.584	26.8#	103	-0.02
8 T	Bis(2-chloroethyl) ether	1000.000	938.145	6.2	110	-0.01
9 T	2-Chlorophenol	1000.000	1038.329	-3.8	124	-0.01
10 T	1,3-Dichlorobenzene	1000.000	1007.512	-0.8	126	-0.02
11 T	1,4-Dichlorobenzene	1000.000	1009.007	-0.9	124	-0.02
12 T	Benzyl alcohol	1000.000	991.731	0.8	120	-0.01
13 T	1,2-Dichlorobenzene	1000.000	1029.009	-2.9	126	-0.01
14 T	2-Methylphenol	1000.000	1020.606	-2.1	117	0.00
15 T	2,2'-Oxybis(1-Chloropropane	1000.000	759.409	24.1#	91	0.00
16 T	N-Nitrosodi-n-propylamine	1000.000	894.905	10.5	106	0.00
17 T	3+4-Methylphenol	1000.000	1040.400	-4.0	116	0.00
18 T	Hexachloroethane	1000.000	1058.283	-5.8	134	-0.01
19 S	Nitrobenzene-d5 (Surr)	1000.000	945.386	5.5	110	-0.01
20 T	Nitrobenzene	1000.000	924.889	7.5	108	0.00
21 I	Naphthalene-d8 (ISTD)	2000.000	2000.000	0.0	121	0.00
22 T	Isophorone	1000.000	944.606	5.5	110	0.00
23 T	2-Nitrophenol	1000.000	1384.332	-38.4#	159	0.00
24 T	2,4-Dimethylphenol	1000.000	1144.621	-14.5	129	0.00
25 T	Bis(2-chloroethoxy) methane	1000.000	996.383	0.4	113	0.00
26 T	Benzoic acid	2000.000	2177.133	-8.9	161	0.00
27 T	2,4-Dichlorophenol	1000.000	1068.359	-6.8	128	0.00
28 T	1,2,4-Trichlorobenzene	1000.000	1106.334	-10.6	130	0.00
29 T	Naphthalene	1000.000	1043.544	-4.4	119	0.00
30 T	4-Chloroaniline	1000.000	623.978	37.6#	71	-0.01
31 T	Hexachlorobutadiene	1000.000	1078.809	-7.9	124	0.00
32 T	4-Chloro-3-methylphenol	1000.000	1058.004	-5.8	120	0.00
33 T	2-Methylnaphthalene	1000.000	1085.228	-8.5	122	0.00
34 T	1-Methylnaphthalene	1000.000	1058.247	-5.8	121	0.00
35 I	Acenaphthene-d10 (ISTD)	2000.000	2000.000	0.0	128	0.00
36 T	Hexachlorocyclopentadiene	1000.000	1341.331	-34.1#	156	0.00
37 T	2,4,6-Trichlorophenol	1000.000	1141.902	-14.2	141	0.00
38 T	2,4,5-Trichlorophenol	1000.000	1124.327	-12.4	141	0.00
39 T	1,1'-Biphenyl	1000.000	1013.743	-1.4	122	0.00
40 S	2-Fluorobiphenyl (Surr)	1000.000	1032.017	-3.2	125	0.00
41 T	2-Chloronaphthalene	1000.000	1085.274	-8.5	130	0.00
42 T	2-Nitroaniline	1000.000	1167.582	-16.8	143	0.00
43 T	2,6-Dimethylnaphthalene	1000.000	1039.868	-4.0	126	0.00
44 T	1,4-Dinitrobenzene	1000.000	1304.479	-30.4#	175	0.00
45 T	Dimethyl phthalate	1000.000	1061.552	-6.2	128	0.00
46 T	1,3-Dinitrobenzene	1000.000	1180.361	-18.0	154	0.00
47 T	2,6-Dinitrotoluene	1000.000	1067.520	-6.8	134	0.00
48 T	1,2-Dinitrobenzene	1000.000	1133.756	-13.4	137	0.00

Evaluate Continuing Calibration Report

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261905.D  
 Acq On : 26 Nov 2019 10:16 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:47:30 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T Acenaphthylene	1000.000	1043.647	-4.4	125	0.00
50 T 3-Nitroaniline	1000.000	1067.764	-6.8	131	0.00
51 T Acenaphthene	1000.000	986.632	1.3	123	0.00
52 T 2,4-Dinitrophenol	1000.000	1369.966	-37.0#	240	0.00
53 T 4-Nitrophenol	1000.000	1036.598	-3.7	130	0.00
54 T 2,4-Dinitrotoluene	1000.000	1113.389	-11.3	146	0.00
55 T Dibenzofuran	1000.000	1055.805	-5.6	128	0.00
56 T 2,3,5,6-Tetrachlorophenol	1000.000	1122.718	-12.3	141	0.00
57 T 2,3,4,6-Tetrachlorophenol	1000.000	1095.548	-9.6	136	0.00
58 T Diethyl phthalate	1000.000	1065.658	-6.6	124	0.00
59 T 2,3,5-Trimethylnaphthalene	1000.000	1099.346	-9.9	131	0.00
60 T Fluorene	1000.000	1041.745	-4.2	128	0.00
61 T 4-Chlorophenyl phenyl ether	1000.000	1060.133	-6.0	129	0.00
62 T 4-Nitroaniline	1000.000	1297.395	-29.7#	165	0.00
63 T 4,6-Dinitro-2-methylphenol	1000.000	1295.448	-29.5#	186	0.00
64 I Phenanthrene-d10 (ISTD)	2000.000	2000.000	0.0	130	0.00
65 T N-Nitrosodiphenylamine	1000.000	1080.166	-8.0	132	0.00
66 T Azobenzene (1,2-DPH)	1000.000	897.614	10.2	109	0.00
67 S 2,4,6-Tribromophenol (Surr)	1000.000	972.857	2.7	125	0.00
68 T 4-Bromophenyl phenyl ether	1000.000	1073.251	-7.3	134	0.00
69 T Hexachlorobenzene	1000.000	1019.619	-2.0	126	0.00
70 T Pentachlorophenol (PCP)	1000.000	955.071	4.5	137	0.00
71 T Phenanthrene	1000.000	1015.637	-1.6	130	0.00
72 T Anthracene	1000.000	1056.953	-5.7	130	0.00
73 T Carbazole	1000.000	1190.358	-19.0	144	0.00
74 T Di-n-butyl phthalate	1000.000	1056.986	-5.7	127	0.00
75 T Fluoranthene	1000.000	1098.614	-9.9	131	0.00
76 T Benzidine	2000.000	1743.316	12.8	110	0.00
77 T Pyrene	1000.000	1091.411	-9.1	130	0.00
78 I Chrysene-d12 (ISTD)	2000.000	2000.000	0.0	129	0.00
79 S Terphenyl-d14 (Surr)	1000.000	1087.739	-8.8	133	0.00
80 T Butyl benzyl phthalate	1000.000	1068.454	-6.8	133	0.00
81 T Bis(2-ethylhexyl) adipate	1000.000	1065.354	-6.5	135	0.00
82 T 3,3-Dichlorobenzidine	2000.000	1954.743	2.3	120	0.02
83 T Benz(a)anthracene	1000.000	1031.248	-3.1	135	0.00
84 T Chrysene	1000.000	1047.201	-4.7	133	0.00
85 T Bis(2-ethylhexyl) phthalate	1000.000	1089.073	-8.9	136	0.00
86 I Perylene-d12 (ISTD)	2000.000	2000.000	0.0	127	0.00
87 T Di-n-octyl phthalate	1000.000	1042.228	-4.2	134	0.00
88 T Benzo(b)fluoranthene	1000.000	1082.008	-8.2	137	0.00
89 T Benzo(k)fluoranthene	1000.000	1066.077	-6.6	135	0.00
90 T Benzo(b+k)fluoranthene	2000.000	2131.342	-6.6	136	0.00
91 T Benzo(e)pyrene	1000.000	1134.863	-13.5	134	0.00
92 T Benzo(a)pyrene	1000.000	1109.126	-10.9	138	0.00
93 T Perylene	1000.000	1111.583	-11.2	140	0.00
94 I Dibenz(a,h)Anthrcene-d14 (I	2000.000	2000.000	0.0	128	0.01

Evaluate Continuing Calibration Report

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261905.D  
 Acq On : 26 Nov 2019 10:16 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:47:30 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 20% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
95 T	Indeno(1,2,3-cd)pyrene	1000.000	1025.951	-2.6	135	0.00
96 T	Dibenz(a,h)anthracene	1000.000	1083.055	-8.3	136	0.01
97 T	Benzo(g,h,i)perylene	1000.000	1127.037	-12.7	135	0.01

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261905.D  
 Acq On : 26 Nov 2019 10:16 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:47:30 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) 1,4-Dichlorobenzene-d4...	6.380	152	361048	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1385010	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	748930	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.937	188	1388573	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.526	240	1350896	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.971	264	1328057	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.362	292	1134512	2000.00	ng/ml	0.01	
System Monitoring Compounds							
4) 2-Fluorophenol (Surr)	5.118	112	231195	1055.22	ng/ml	-0.03	
5) Phenol-d6 (Surr)	6.033	99	270382	964.14	ng/ml	-0.01	
19) Nitrobenzene-d5 (Surr)	6.926	82	205680	945.39	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.739	172	604885	1032.02	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	81376	972.86	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	677167	1087.74	ng/ml	0.00	
Target Compounds							
							Qvalue
2) N-Nitrosodimethylamine	3.701	74	123232m	896.06	ng/ml		
3) Pyridine	3.711	79	208947m	891.19	ng/ml		
6) Phenol	6.049	94	285466	925.74	ng/ml		94
7) Aniline	6.065	93	194636	731.58	ng/ml		96
8) Bis(2-chloroethyl) ether	6.124	93	261084	938.15	ng/ml		97
9) 2-Chlorophenol	6.183	128	265446	1038.33	ng/ml		97
10) 1,3-Dichlorobenzene	6.327	146	289508	1007.51	ng/ml		98
11) 1,4-Dichlorobenzene	6.396	146	284963	1009.01	ng/ml		97
12) Benzyl alcohol	6.519	108	150225	991.73	ng/ml		92
13) 1,2-Dichlorobenzene	6.552	146	286599	1029.01	ng/ml		97
14) 2-Methylphenol	6.637	107	189797	1020.61	ng/ml		99
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	186509	759.41	ng/ml		85
16) N-Nitrosodi-n-propylamine	6.782	70	144595	894.90	ng/ml		91
17) 3+4-Methylphenol	6.787	107	239909	1040.40	ng/ml		97
18) Hexachloroethane	6.883	201	91833	1058.28	ng/ml		94
20) Nitrobenzene	6.947	77	203870	924.89	ng/ml		89
22) Isophorone	7.183	82	417093	944.61	ng/ml		97
23) 2-Nitrophenol	7.263	139	183121	1384.33	ng/ml		92
24) 2,4-Dimethylphenol	7.311	122	212550	1144.62	ng/ml		94
25) Bis(2-chloroethoxy) me...	7.397	93	267465	996.38	ng/ml		99
26) Benzoic acid	7.407	105	159975	2177.13	ng/ml		96
27) 2,4-Dichlorophenol	7.509	162	221856	1068.36	ng/ml		96
28) 1,2,4-Trichlorobenzene	7.589	180	268179	1106.33	ng/ml		99
29) Naphthalene	7.669	128	760321	1043.54	ng/ml		100
30) 4-Chloroaniline	7.728	127	142485	623.98	ng/ml		96
31) Hexachlorobutadiene	7.803	225	141312	1078.81	ng/ml		99
32) 4-Chloro-3-methylphenol	8.215	107	194439	1058.00	ng/ml		90
33) 2-Methylnaphthalene	8.365	142	552458	1085.23	ng/ml		99
34) 1-Methylnaphthalene	8.466	142	521518	1058.25	ng/ml		99
36) Hexachlorocyclopentadiene	8.536	237	155342	1341.33	ng/ml		98
37) 2,4,6-Trichlorophenol	8.654	196	165844	1141.90	ng/ml		98
38) 2,4,5-Trichlorophenol	8.691	198	160989	1124.33	ng/ml		99
39) 1,1'-Biphenyl	8.835	154	652563	1013.74	ng/ml		98
41) 2-Chloronaphthalene	8.857	162	504546	1085.27	ng/ml		96
42) 2-Nitroaniline	8.958	138	162843	1167.58	ng/ml		89
43) 2,6-Dimethylnaphthalene	8.996	156	491064	1039.87	ng/ml		98

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261905.D  
 Acq On : 26 Nov 2019 10:16 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:47:30 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	77434	1304.48	ng/ml	77
45) Dimethyl phthalate	9.146	163	574148	1061.55	ng/ml	99
46) 1,3-Dinitrobenzene	9.172	168	88498	1180.36	ng/ml	86
47) 2,6-Dinitrotoluene	9.204	165	130020	1067.52	ng/ml	89
48) 1,2-Dinitrobenzene	9.258	168	62123	1133.76	ng/ml	82
49) Acenaphthylene	9.279	152	794557	1043.65	ng/ml	99
50) 3-Nitroaniline	9.376	138	99617	1067.76	ng/ml	88
51) Acenaphthene	9.456	153	493252	986.63	ng/ml	99
52) 2,4-Dinitrophenol	9.483	184	43311	1369.97	ng/ml	88
53) 4-Nitrophenol	9.557	139	76390	1036.60	ng/ml	91
54) 2,4-Dinitrotoluene	9.616	165	169706	1113.39	ng/ml	81
55) Dibenzofuran	9.632	168	703620	1055.81	ng/ml	97
56) 2,3,5,6-Tetrachlorophenol	9.718	232	129256	1122.72	ng/ml	96
57) 2,3,4,6-Tetrachlorophenol	9.761	232	137967	1095.55	ng/ml	95
58) Diethyl phthalate	9.862	149	530554	1065.66	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	9.846	170	466537	1099.35	ng/ml	91
60) Fluorene	9.980	166	546349	1041.75	ng/ml	98
61) 4-Chlorophenyl phenyl ...	9.975	204	271053	1060.13	ng/ml	96
62) 4-Nitroaniline	9.996	138	104418	1297.39	ng/ml	91
63) 4,6-Dinitro-2-methylph...	10.028	198	72386	1295.45	ng/ml	94
65) N-Nitrosodiphenylamine	10.098	169	462466	1080.17	ng/ml	99
66) Azobenzene (1,2-DPH)	10.135	77	388908	897.61	ng/ml	93
68) 4-Bromophenyl phenyl e...	10.472	248	168162	1073.25	ng/ml	95
69) Hexachlorobenzene	10.552	284	191656	1019.62	ng/ml	97
70) Pentachlorophenol (PCP)	10.750	266	89468	955.07	ng/ml	98
71) Phenanthrene	10.959	178	791178	1015.64	ng/ml	100
72) Anthracene	11.012	178	791449	1056.95	ng/ml	99
73) Carbazole	11.173	167	660701	1190.36	ng/ml	99
74) Di-n-butyl phthalate	11.526	149	867990	1056.99	ng/ml	99
75) Fluoranthene	12.194	202	877144	1098.61	ng/ml	99
76) Benzidine	12.349	184	333599	1743.32	ng/ml	96
77) Pyrene	12.467	202	886776	1091.41	ng/ml	98
80) Butyl benzyl phthalate	13.419	149	370571	1068.45	ng/ml	90
81) Bis(2-ethylhexyl) adipate	13.585	129	333794	1065.35	ng/ml	100
82) 3,3-Dichlorobenzidine	14.489	252	209207	1954.74	ng/ml	95
83) Benz(a)anthracene	14.505	228	777805	1031.25	ng/ml	98
84) Chrysene	14.585	228	740179	1047.20	ng/ml	100
85) Bis(2-ethylhexyl) phth...	14.687	149	529216	1089.07	ng/ml	98
87) Di-n-octyl phthalate	16.329	149	795912	1042.23	ng/ml	98
88) Benzo(b)fluoranthene	17.056	252	793115	1082.01	ng/ml	98
89) Benzo(k)fluoranthene	17.126	252	786228	1066.08	ng/ml	99
90) Benzo(b+k)fluoranthene	17.126	252	1603413	2131.34	ng/ml	99
91) Benzo(e)pyrene	17.703	252	774644	1134.86	ng/ml	99
92) Benzo(a)pyrene	17.821	252	738208	1109.13	ng/ml	99
93) Perylene	18.024	252	665765	1111.58	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.351	276	688290	1025.95	ng/ml	99
96) Dibenz(a,h)anthracene	20.426	278	667115	1083.05	ng/ml	98
97) Benzo(g,h,i)perylene	20.886	276	726261	1127.04	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261905.D  
 Acq On : 26 Nov 2019 10:16 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCV2  
 Misc : 1x, A19G243@1000  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:47:30 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261906.D  
 Acq On : 26 Nov 2019 10:52 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

AMS  
 11/26/19

Quant Time: Nov 26 12:47:53 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.381	152	419057	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1631497	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	883506	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.932	188	1617278	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.521	240	1667447	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.966	264	1651056	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthracene-d...	20.357	292	1416154	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	0.000	112	0	0.00	ng/ml		
5) Phenol-d6 (Surr)	0.000	99	0	0.00	ng/ml		
19) Nitrobenzene-d5 (Surr)	6.878	82	80	0.32	ng/ml	-0.06	
40) 2-Fluorobiphenyl (Surr)	0.000	172	0	0.00	ng/ml		
67) 2,4,6-Tribromophenol (...)	0.000	330	0	0.00	ng/ml		
79) Terphenyl-d14 (Surr)	12.671	244	171	0.22	ng/ml	0.00	
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	0.000		0	N.D.			Qvalue
3) Pyridine	3.685	79	810m	2.98	ng/ml#		
6) Phenol	6.118	94	130	N.D.			
7) Aniline	6.065	93	66	N.D.			
8) Bis(2-chloroethyl) ether	6.065	93	66	N.D.			
9) 2-Chlorophenol	6.225	128	59	N.D.			
10) 1,3-Dichlorobenzene	0.000		0	N.D.			
11) 1,4-Dichlorobenzene	0.000		0	N.D.			
12) Benzyl alcohol	0.000		0	N.D.			
13) 1,2-Dichlorobenzene	0.000		0	N.D.			
14) 2-Methylphenol	0.000		0	N.D.			
15) 2,2'-Oxybis(1-Chloropr...	0.000		0	N.D.			
16) N-Nitrosodi-n-propylamine	6.760	70	106	N.D.			
17) 3+4-Methylphenol	6.798	107	78	N.D.			
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	6.910	77	121	N.D.			
22) Isophorone	7.156	82	85	N.D.			
23) 2-Nitrophenol	0.000		0	N.D.			
24) 2,4-Dimethylphenol	0.000		0	N.D.			
25) Bis(2-chloroethoxy) me...	7.450	93	64	N.D.			
26) Benzoic acid	7.391	105	54	806.44	ng/ml#	8	
27) 2,4-Dichlorophenol	0.000		0	N.D.			
28) 1,2,4-Trichlorobenzene	0.000		0	N.D.			
29) Naphthalene	7.670	128	162	N.D.			
30) 4-Chloroaniline	0.000		0	N.D.			
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	0.000		0	N.D.			
33) 2-Methylnaphthalene	0.000		0	N.D.			
34) 1-Methylnaphthalene	0.000		0	N.D.			
36) Hexachlorocyclopentadiene	0.000		0	N.D.			
37) 2,4,6-Trichlorophenol	0.000		0	N.D.			
38) 2,4,5-Trichlorophenol	0.000		0	N.D.			
39) 1,1'-Biphenyl	0.000		0	N.D.			
41) 2-Chloronaphthalene	0.000		0	N.D.			
42) 2-Nitroaniline	0.000		0	N.D.			
43) 2,6-Dimethylnaphthalene	0.000		0	N.D.			

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261906.D  
 Acq On : 26 Nov 2019 10:52 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9K26022-CCB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Nov 26 12:47:53 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	0.000		0	N.D.		
45) Dimethyl phthalate	9.156	163	156	N.D.		
46) 1,3-Dinitrobenzene	0.000		0	N.D.		
47) 2,6-Dinitrotoluene	9.156	165	146	26.06	ng/ml#	51
48) 1,2-Dinitrobenzene	0.000		0	N.D.		
49) Acenaphthylene	0.000		0	N.D.		
50) 3-Nitroaniline	9.424	138	95	30.40	ng/ml#	1
51) Acenaphthene	9.424	153	297	N.D.		
52) 2,4-Dinitrophenol	0.000		0	N.D.		
53) 4-Nitrophenol	0.000		0	N.D.		
54) 2,4-Dinitrotoluene	9.606	165	108	54.31	ng/ml#	27
55) Dibenzofuran	0.000		0	N.D.		
56) 2,3,5,6-Tetrachlorophenol	0.000		0	N.D.		
57) 2,3,4,6-Tetrachlorophenol	0.000		0	N.D.		
58) Diethyl phthalate	9.863	149	71	N.D.		
59) 2,3,5-Trimethylnaphtha...	9.948	170	174	N.D.		
60) Fluorene	0.000		0	N.D.		
61) 4-Chlorophenyl phenyl ...	0.000		0	N.D.		
62) 4-Nitroaniline	0.000		0	N.D.		
63) 4,6-Dinitro-2-methylph...	0.000		0	N.D.		
65) N-Nitrosodiphenylamine	0.000		0	N.D.		
66) Azobenzene (1,2-DPH)	10.151	77	68	N.D.		
68) 4-Bromophenyl phenyl e...	0.000		0	N.D.		
69) Hexachlorobenzene	0.000		0	N.D.		
70) Pentachlorophenol (PCP)	10.702	266	97	77.42	ng/ml#	1
71) Phenanthrene	10.938	178	911	N.D.		
72) Anthracene	11.012	178	50	N.D.		
73) Carbazole	0.000		0	N.D.		
74) Di-n-butyl phthalate	11.531	149	196	N.D.		
75) Fluoranthene	12.195	202	162	N.D.		
76) Benzidine	12.371	184	73	123.30	ng/ml	67
77) Pyrene	12.467	202	280	N.D.		
80) Butyl benzyl phthalate	13.435	149	90	29.56	ng/ml#	1
81) Bis(2-ethylhexyl) adipate	13.580	129	19630	50.76	ng/ml	93
82) 3,3-Dichlorobenzidine	0.000		0	N.D.		
83) Benz(a)anthracene	14.527	228	3661	3.93	ng/ml	68
84) Chrysene	14.580	228	271	N.D.		
85) Bis(2-ethylhexyl) phth...	14.682	149	749	N.D.		
87) Di-n-octyl phthalate	16.324	149	85	58.03	ng/ml#	1
88) Benzo(b)fluoranthene	17.051	252	263	8.25	ng/ml	57
89) Benzo(k)fluoranthene	17.051	252	222	8.71	ng/ml	57
90) Benzo(b+k)fluoranthene	17.051	252	263	16.01	ng/ml	57
91) Benzo(e)pyrene	17.623	252	84	N.D.		
92) Benzo(a)pyrene	0.000		0	N.D.		
93) Perylene	17.966	252	5355	7.19	ng/ml	71
95) Indeno(1,2,3-cd)pyrene	20.362	276	886	N.D.		
96) Dibenz(a,h)anthracene	20.405	278	208	N.D.		
97) Benzo(g,h,i)perylene	20.870	276	164	N.D.		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
Data File : J11261906.D  
Acq On : 26 Nov 2019 10:52 am  
Operator : JK/ AMS/ DTH  
Sample : 9K26022-CCB1  
Misc : 1x, DCM + ISTD  
ALS Vial : 3 Sample Multiplier: 1  
DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:47:53 2019  
Quant Method : T:\methods\SV10\_091919R4.M  
Quant Title : EPA 8270D: Semivolatile Organics  
QLast Update : Fri Oct 25 11:15:50 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261907.D  
 Acq On : 26 Nov 2019 11:28 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9111196-BLK1  
 Misc : 1x, 625 B(a)P Only  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:48:06 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

AMS  
11/26/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) 1,4-Dichlorobenzene-d4...	6.386	152	453367	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.648	136	1636282	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	884708	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.932	188	1572664	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.526	240	1633391	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.971	264	1588995	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.357	292	1351282	2000.00	ng/ml	0.00	
System Monitoring Compounds							
4) 2-Fluorophenol (Surr)	5.129	112	120761	438.94	ng/ml	-0.02	
5) Phenol-d6 (Surr)	6.044	99	71703	203.62	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	180523	660.79	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	419162	605.39	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	69033	733.47	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	632333	840.05	ng/ml	0.00	
Target Compounds							
2) N-Nitrosodimethylamine	0.000		0	N.D.			Qvalue
3) Pyridine	3.754	79	955m	3.24	ng/ml#		
6) Phenol	6.054	94	2086	5.39	ng/ml#		48
7) Aniline	6.076	93	67	N.D.			
8) Bis(2-chloroethyl) ether	6.113	93	444	N.D.			
9) 2-Chlorophenol	6.183	128	222	N.D.			
10) 1,3-Dichlorobenzene	6.332	146	64	N.D.			
11) 1,4-Dichlorobenzene	6.402	146	191	N.D.			
12) Benzyl alcohol	6.536	108	158	25.30	ng/ml#		54
13) 1,2-Dichlorobenzene	0.000		0	N.D.			
14) 2-Methylphenol	6.648	107	148	N.D.			
15) 2,2'-Oxybis(1-Chloropr...	0.000		0	N.D.			
16) N-Nitrosodi-n-propylamine	6.787	70	72	N.D.			
17) 3+4-Methylphenol	6.808	107	67	N.D.			
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	6.931	77	781	2.82	ng/ml#		30
22) Isophorone	7.188	82	207	N.D.			
23) 2-Nitrophenol	7.279	139	51	42.61	ng/ml#		42
24) 2,4-Dimethylphenol	0.000		0	N.D.			
25) Bis(2-chloroethoxy) me...	7.418	93	162	N.D.			
26) Benzoic acid	7.391	105	281	808.15	ng/ml#		42
27) 2,4-Dichlorophenol	0.000		0	N.D.			
28) 1,2,4-Trichlorobenzene	7.589	180	66	N.D.			
29) Naphthalene	7.664	128	2328	2.70	ng/ml		94
30) 4-Chloroaniline	7.664	127	247	14.14	ng/ml#		27
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	8.236	107	300	N.D.			
33) 2-Methylnaphthalene	8.365	142	418	N.D.			
34) 1-Methylnaphthalene	8.466	142	312	N.D.			
36) Hexachlorocyclopentadiene	0.000		0	N.D.			
37) 2,4,6-Trichlorophenol	0.000		0	N.D.			
38) 2,4,5-Trichlorophenol	0.000		0	N.D.			
39) 1,1'-Biphenyl	8.836	154	629	N.D.			
41) 2-Chloronaphthalene	8.862	162	122	N.D.			
42) 2-Nitroaniline	0.000		0	N.D.			
43) 2,6-Dimethylnaphthalene	8.996	156	78	N.D.			

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261907.D  
 Acq On : 26 Nov 2019 11:28 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9111196-BLK1  
 Misc : 1x, 625 B(a)P Only  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Nov 26 12:48:06 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	0.000		0		N.D.	
45) Dimethyl phthalate	9.140	163	248		N.D.	
46) 1,3-Dinitrobenzene	0.000		0		N.D.	
47) 2,6-Dinitrotoluene	9.199	165	87	25.66	ng/ml#	62
48) 1,2-Dinitrobenzene	0.000		0		N.D.	
49) Acenaphthylene	9.279	152	259		N.D.	
50) 3-Nitroaniline	9.419	138	87	30.34	ng/ml#	1
51) Acenaphthene	9.456	153	397		N.D.	
52) 2,4-Dinitrophenol	0.000		0		N.D.	
53) 4-Nitrophenol	0.000		0		N.D.	
54) 2,4-Dinitrotoluene	9.606	165	148	54.52	ng/ml#	27
55) Dibenzofuran	9.632	168	218		N.D.	
56) 2,3,5,6-Tetrachlorophenol	0.000		0		N.D.	
57) 2,3,4,6-Tetrachlorophenol	0.000		0		N.D.	
58) Diethyl phthalate	9.857	149	472		N.D.	
59) 2,3,5-Trimethylnaphtha...	9.873	170	55		N.D.	
60) Fluorene	9.980	166	316		N.D.	
61) 4-Chlorophenyl phenyl ...	9.975	204	63		N.D.	
62) 4-Nitroaniline	0.000		0		N.D.	
63) 4,6-Dinitro-2-methylph...	0.000		0		N.D.	
65) N-Nitrosodiphenylamine	10.103	169	115		N.D.	
66) Azobenzene (1,2-DPH)	10.146	77	488		N.D.	
68) 4-Bromophenyl phenyl e...	0.000		0		N.D.	
69) Hexachlorobenzene	10.547	284	51		N.D.	
70) Pentachlorophenol (PCP)	10.756	266	140	77.81	ng/ml#	37
71) Phenanthrene	10.959	178	1915		N.D.	
72) Anthracene	11.002	178	472		N.D.	
73) Carbazole	11.189	167	233	5.87	ng/ml	60
74) Di-n-butyl phthalate	11.526	149	1155		N.D.	
75) Fluoranthene	12.200	202	991		N.D.	
76) Benzidine	12.360	184	72	123.30	ng/ml	67
77) Pyrene	12.467	202	919		N.D.	
80) Butyl benzyl phthalate	13.419	149	116	29.63	ng/ml#	27
81) Bis(2-ethylhexyl) adipate	13.580	129	14247	37.61	ng/ml	95
82) 3,3-Dichlorobenzidine	0.000		0		N.D.	
83) Benz(a)anthracene	14.526	228	4051	4.44	ng/ml	63
84) Chrysene	14.569	228	525		N.D.	
85) Bis(2-ethylhexyl) phth...	14.682	149	4456	7.58	ng/ml	83
87) Di-n-octyl phthalate	16.340	149	53	58.00	ng/ml	54
88) Benzo(b)fluoranthene	17.046	252	57	8.02	ng/ml	57
89) Benzo(k)fluoranthene	17.105	252	202	8.70	ng/ml	57
90) Benzo(b+k)fluoranthene	17.105	252	420	16.20	ng/ml	57
91) Benzo(e)pyrene	17.704	252	183		N.D.	
92) Benzo(a)pyrene	17.816	252	234	10.13	ng/ml	59
93) Perylene	17.976	252	5353	7.47	ng/ml	74
95) Indeno(1,2,3-cd)pyrene	20.340	276	211		N.D.	
96) Dibenz(a,h)anthracene	20.415	278	77		N.D.	
97) Benzo(g,h,i)perylene	20.881	276	125		N.D.	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261907.D  
 Acq On : 26 Nov 2019 11:28 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9111196-BLK1  
 Misc : 1x, 625 B(a)P Only  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:48:06 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261908.D  
 Acq On : 26 Nov 2019 12:04 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111196-BS1  
 Misc : 1x, 625 B(a)P Only  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

*AMS*  
*11/26/19*

Quant Time: Nov 26 12:48:25 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.380	152	440697	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1581967	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	854856	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1584035	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.532	240	1544885	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.976	264	1618769	2000.00	ng/ml	0.01	
94) Dibenz(a,h)Anthrcene-d...	20.367	292	1398958	2000.00	ng/ml	0.02	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.118	112	114242	427.19	ng/ml	-0.03	
5) Phenol-d6 (Surr)	6.038	99	83348	243.49	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	176246	663.68	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	456580	682.46	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	74570	785.16	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	587095	824.64	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.695	74	63418m	377.79	ng/ml		
3) Pyridine	3.706	79	671	N.D.			
6) Phenol	6.049	94	145532	386.65	ng/ml	95	
7) Aniline	6.049	93	3790	11.67	ng/ml#	1	
8) Bis(2-chloroethyl) ether	6.124	93	316858	932.78	ng/ml	98	
9) 2-Chlorophenol	6.183	128	341507	1094.42	ng/ml	96	
10) 1,3-Dichlorobenzene	6.327	146	203210	579.37	ng/ml	98	
11) 1,4-Dichlorobenzene	6.397	146	201987	585.94	ng/ml	98	
12) Benzyl alcohol	6.520	108	121588	668.14	ng/ml	93	
13) 1,2-Dichlorobenzene	6.552	146	212583	625.31	ng/ml	97	
14) 2-Methylphenol	6.637	107	226750	998.94	ng/ml	98	
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	242938	810.39	ng/ml	88	
16) N-Nitrosodi-n-propylamine	6.782	70	206379	1046.44	ng/ml	92	
17) 3+4-Methylphenol	6.787	107	259278	921.18	ng/ml	98	
18) Hexachloroethane	6.883	201	56334	531.86	ng/ml	96	
20) Nitrobenzene	6.947	77	277889	1032.84	ng/ml	92	
22) Isophorone	7.183	82	601382	1192.40	ng/ml	97	
23) 2-Nitrophenol	7.268	139	203996	1351.30	ng/ml	84	✓
24) 2,4-Dimethylphenol	7.311	122	297155	1401.00	ng/ml	93	
25) Bis(2-chloroethoxy) me...	7.397	93	380792	1241.95	ng/ml	99	
26) Benzoic acid	7.402	105	101370	1578.94	ng/ml	95	
27) 2,4-Dichlorophenol	7.509	162	315363	1327.43	ng/ml	97	
28) 1,2,4-Trichlorobenzene	7.589	180	194692	703.18	ng/ml	99	
29) Naphthalene	7.670	128	734394	882.47	ng/ml	99	
30) 4-Chloroaniline	7.723	127	14378	66.36	ng/ml	98	
31) Hexachlorobutadiene	7.798	225	82151	549.08	ng/ml	99	
32) 4-Chloro-3-methylphenol	8.210	107	277177	1320.43	ng/ml	95	
33) 2-Methylnaphthalene	8.365	142	520831	895.72	ng/ml	98	
34) 1-Methylnaphthalene	8.466	142	516712	917.96	ng/ml	98	
36) Hexachlorocyclopentadiene	8.536	237	94243	712.93	ng/ml	96	
37) 2,4,6-Trichlorophenol	8.654	196	241706	1449.63	ng/ml	99	
38) 2,4,5-Trichlorophenol	8.691	198	240506	1464.75	ng/ml	97	
39) 1,1'-Biphenyl	8.841	154	1958	2.66	ng/ml	95	
41) 2-Chloronaphthalene	8.857	162	542073	1021.51	ng/ml	96	
42) 2-Nitroaniline	8.959	138	237774	1477.85	ng/ml	88	
43) 2,6-Dimethylnaphthalene	9.001	156	445	N.D.			



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261908.D  
 Acq On : 26 Nov 2019 12:04 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111196-BS1  
 Misc : 1x, 625 B(a)P Only  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Nov 26 12:48:25 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	119421	1707.37	ng/ml	79
45) Dimethyl phthalate	9.146	163	835530	1353.40	ng/ml	99
46) 1,3-Dinitrobenzene	9.172	168	131241	1508.54	ng/ml	87
47) 2,6-Dinitrotoluene	9.205	165	196599	1409.02	ng/ml	90
48) 1,2-Dinitrobenzene	9.263	168	91124	1456.96	ng/ml	75
49) Acenaphthylene	9.279	152	977465	1124.81	ng/ml	99
50) 3-Nitroaniline	9.376	138	96554	876.38	ng/ml	92
51) Acenaphthene	9.456	153	600805	1052.85	ng/ml	100
52) 2,4-Dinitrophenol	9.483	184	79433	1936.31	ng/ml	86
53) 4-Nitrophenol	9.558	139	41476	546.69	ng/ml	94
54) 2,4-Dinitrotoluene	9.616	165	252352	1439.14	ng/ml	81
55) Dibenzofuran	9.632	168	908358	1194.13	ng/ml	98
56) 2,3,5,6-Tetrachlorophenol	9.718	232	194966	1466.84	ng/ml	95
57) 2,3,4,6-Tetrachlorophenol	9.761	232	198197	1372.30	ng/ml	97
58) Diethyl phthalate	9.862	149	796563	1401.70	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	9.857	170	438	N.D.		
60) Fluorene	9.980	166	709913	1185.89	ng/ml	98
61) 4-Chlorophenyl phenyl ...	9.975	204	353265	1210.47	ng/ml	94
62) 4-Nitroaniline	9.996	138	141380	1538.98	ng/ml	93
63) 4,6-Dinitro-2-methylph...	10.034	198	132670	1925.38	ng/ml	87
65) N-Nitrosodiphenylamine	10.098	169	650600	1332.08	ng/ml	99
66) Azobenzene (1,2-DPH)	10.141	77	533415	1079.22	ng/ml	85
68) 4-Bromophenyl phenyl e...	10.478	248	235917	1319.89	ng/ml	95
69) Hexachlorobenzene	10.552	284	271535	1266.33	ng/ml	98
70) Pentachlorophenol (PCP)	10.750	266	145287	1328.79	ng/ml	98
71) Phenanthrene	10.959	178	1098032	1235.62	ng/ml	99
72) Anthracene	11.012	178	1118430	1309.32	ng/ml	99
73) Carbazole	11.173	167	998568	Below Cal		99
74) Di-n-butyl phthalate	11.526	149	1299187	1386.85	ng/ml	99
75) Fluoranthene	12.194	202	1280065	1405.43	ng/ml	98
76) Benzidine	12.355	184	180	123.77	ng/ml	58
77) Pyrene	12.467	202	1323834	1428.27	ng/ml	99
80) Butyl benzyl phthalate	13.419	149	578717	1437.85	ng/ml	89
81) Bis(2-ethylhexyl) adipate	13.585	129	514622	1436.25	ng/ml	98
82) 3,3-Dichlorobenzidine	14.484	252	510574	4718.31	ng/ml	99
83) Benz(a)anthracene	14.510	228	1208420	1400.99	ng/ml	97
84) Chrysene	14.591	228	1116908	1381.77	ng/ml	99
85) Bis(2-ethylhexyl) phth...	14.687	149	825401	1485.30	ng/ml	97
87) Di-n-octyl phthalate	16.334	149	1348767	1419.79	ng/ml	98
88) Benzo(b)fluoranthene	17.067	252	1215957	1355.62	ng/ml	96
89) Benzo(k)fluoranthene	17.137	252	1191432	1333.06	ng/ml	98
90) Benzo(b+k)fluoranthene	17.067	252	2443889	2665.35	ng/ml	96
91) Benzo(e)pyrene	17.709	252	281	N.D.		
92) Benzo(a)pyrene	17.832	252	1083239	1333.17	ng/ml	98
93) Perylene	18.062	252	1444	N.D.		
95) Indeno(1,2,3-cd)pyrene	20.357	276	1069379	1292.68	ng/ml	98
96) Dibenz(a,h)anthracene	20.431	278	1040548	1369.99	ng/ml	99
97) Benzo(g,h,i)perylene	20.897	276	1150216	1447.54	ng/ml	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
Data File : J11261908.D  
Acq On : 26 Nov 2019 12:04 pm  
Operator : JK/ AMS/ DTH  
Sample : 9111196-BS1  
Misc : 1x, 625 B(a)P Only  
ALS Vial : 5 Sample Multiplier: 1  
DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 12:48:25 2019  
Quant Method : T:\methods\SV10\_091919R4.M  
Quant Title : EPA 8270D: Semivolatile Organics  
QLast Update : Fri Oct 25 11:15:50 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261909.D  
 Acq On : 26 Nov 2019 12:39 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111196-BSD1  
 Misc : 1x, 625 B(a)P Only  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Q-19

Quant Time: Nov 26 13:50:33 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

AMS  
11/26/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.381	152	445620	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1583440	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	855938	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1587190	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.532	240	1507447	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.971	264	1549284	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthracene-d...	20.367	292	1336841	2000.00	ng/ml	0.02	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.118	112	115679	427.78	ng/ml	-0.03	
5) Phenol-d6 (Surr)	6.038	99	85611	247.34	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	184541	687.24	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	505214	754.20	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	76122	799.54	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	577310	831.03	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.696	74	71297m	420.04	ng/ml		
3) Pyridine	3.738	79	481	N.D.			
6) Phenol	6.049	94	153287	402.75	ng/ml	92	
7) Aniline	6.070	93	1790	5.45	ng/ml#	1	
8) Bis(2-chloroethyl) ether	6.124	93	334698	974.41	ng/ml	97	
9) 2-Chlorophenol	6.183	128	364453	1155.05	ng/ml	97	
10) 1,3-Dichlorobenzene	6.327	146	315122	888.52	ng/ml	98	
11) 1,4-Dichlorobenzene	6.397	146	309752	888.63	ng/ml	99	
12) Benzyl alcohol	6.520	108	128634	697.70	ng/ml	93	
13) 1,2-Dichlorobenzene	6.552	146	310283	902.62	ng/ml	97	
14) 2-Methylphenol	6.637	107	231692	1009.44	ng/ml	98	
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	257293	848.80	ng/ml	82	
16) N-Nitrosodi-n-propylamine	6.782	70	213924	1072.71	ng/ml	92	
17) 3+4-Methylphenol	6.787	107	270357	949.93	ng/ml	95	
18) Hexachloroethane	6.883	201	100417	937.59	ng/ml	95	
20) Nitrobenzene	6.948	77	294959	1084.17	ng/ml	88	
22) Isophorone	7.183	82	620252	1228.68	ng/ml	98	
23) 2-Nitrophenol	7.268	139	216898	1432.50	ng/ml	86	
24) 2,4-Dimethylphenol	7.311	122	304281	1433.27	ng/ml	96	
25) Bis(2-chloroethoxy) me...	7.397	93	386150	1258.25	ng/ml	99	
26) Benzoic acid	7.402	105	107435	1623.44	ng/ml	94	
27) 2,4-Dichlorophenol	7.509	162	327378	1376.57	ng/ml	97	
28) 1,2,4-Trichlorobenzene	7.595	180	291182	1050.70	ng/ml	98	
29) Naphthalene	7.670	128	923409	1108.56	ng/ml	99	
30) 4-Chloroaniline	7.728	127	18698	82.28	ng/ml	92	
31) Hexachlorobutadiene	7.803	225	140794	940.16	ng/ml	99	
32) 4-Chloro-3-methylphenol	8.215	107	277680	1321.60	ng/ml	88	
33) 2-Methylnaphthalene	8.365	142	678803	1166.32	ng/ml	99	
34) 1-Methylnaphthalene	8.467	142	647390	1149.04	ng/ml	99	
36) Hexachlorocyclopentadiene	8.536	237	164018	1239.19	ng/ml	98	
37) 2,4,6-Trichlorophenol	8.654	196	251020	1502.38	ng/ml	98	
38) 2,4,5-Trichlorophenol	8.691	198	241443	1468.54	ng/ml	98	
39) 1,1'-Biphenyl	8.836	154	2109	2.87	ng/ml	97	
41) 2-Chloronaphthalene	8.857	162	675011	1270.42	ng/ml	96	
42) 2-Nitroaniline	8.959	138	244645	1516.87	ng/ml	87	
43) 2,6-Dimethylnaphthalene	9.007	156	376	N.D.			

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261909.D  
 Acq On : 26 Nov 2019 12:39 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111196-BSD1  
 Misc : 1x, 625 B(a)P Only  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Nov 26 13:50:33 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	122938	1750.16	ng/ml	80
45) Dimethyl phthalate	9.151	163	864826	1399.09	ng/ml	99
46) 1,3-Dinitrobenzene	9.173	168	134804	1545.17	ng/ml	87
47) 2,6-Dinitrotoluene	9.205	165	203067	1453.14	ng/ml	91
48) 1,2-Dinitrobenzene	9.263	168	90263	1441.37	ng/ml	79
49) Acenaphthylene	9.280	152	1091596	1254.55	ng/ml	98
50) 3-Nitroaniline	9.376	138	112241	1048.98	ng/ml	88
51) Acenaphthene	9.456	153	679553	1189.35	ng/ml	99
52) 2,4-Dinitrophenol	9.483	184	82957	1996.81	ng/ml	87
53) 4-Nitrophenol	9.558	139	44251	576.69	ng/ml	92
54) 2,4-Dinitrotoluene	9.616	165	259142	1475.18	ng/ml	82
55) Dibenzofuran	9.633	168	991374	1301.61	ng/ml	99
56) 2,3,5,6-Tetrachlorophenol	9.718	232	203448	1526.25	ng/ml	95
57) 2,3,4,6-Tetrachlorophenol	9.761	232	206574	1427.51	ng/ml	95
58) Diethyl phthalate	9.863	149	809417	1422.52	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	9.857	170	346	N.D.		
60) Fluorene	9.980	166	750341	1251.84	ng/ml	97
61) 4-Chlorophenyl phenyl ...	9.975	204	384202	1314.81	ng/ml	95
62) 4-Nitroaniline	9.996	138	143803	1563.38	ng/ml	90
63) 4,6-Dinitro-2-methylph...	10.034	198	138910	1999.21	ng/ml	88
65) N-Nitrosodiphenylamine	10.098	169	669320	1367.68	ng/ml	99
66) Azobenzene (1,2-DPH)	10.141	77	558118	1126.96	ng/ml	84
68) 4-Bromophenyl phenyl e...	10.478	248	250518	1398.79	ng/ml	95
69) Hexachlorobenzene	10.553	284	288767	1344.01	ng/ml	98
70) Pentachlorophenol (PCP)	10.750	266	153024	1393.16	ng/ml	97
71) Phenanthrene	10.959	178	1137119	1277.06	ng/ml	99
72) Anthracene	11.012	178	1148091	1341.37	ng/ml	99
73) Carbazole	11.173	167	1014545	Below Cal		99
74) Di-n-butyl phthalate	11.526	149	1319961	1406.23	ng/ml	99
75) Fluoranthene	12.195	202	1300677	1425.22	ng/ml	99
76) Benzidine	12.355	184	58	123.24	ng/ml	67
77) Pyrene	12.467	202	1338267	1440.98	ng/ml	99
80) Butyl benzyl phthalate	13.419	149	583861	1484.31	ng/ml	91
81) Bis(2-ethylhexyl) adipate	13.585	129	513803	1469.58	ng/ml	99
82) 3,3-Dichlorobenzidine	14.478	252	574839	5567.89	ng/ml	97
83) Benz(a)anthracene	14.505	228	1217302	1446.34	ng/ml	97
84) Chrysene	14.585	228	1139043	1444.15	ng/ml	98
85) Bis(2-ethylhexyl) phth...	14.687	149	841066	1551.08	ng/ml	97
87) Di-n-octyl phthalate	16.334	149	1354718	1485.95	ng/ml	98
88) Benzo(b)fluoranthene	17.062	252	1214466	1413.61	ng/ml	97
89) Benzo(k)fluoranthene	17.126	252	1177491	1377.98	ng/ml	98
90) Benzo(b+k)fluoranthene	17.062	252	2430049	2769.35	ng/ml	97
91) Benzo(e)pyrene	17.693	252	262	N.D.		
92) Benzo(a)pyrene	17.827	252	1077706	1385.44	ng/ml	99
93) Perylene	18.030	252	1236	N.D.		
95) Indeno(1,2,3-cd)pyrene	20.362	276	1057636	1337.89	ng/ml	98
96) Dibenz(a,h)anthracene	20.437	278	1026799	1414.70	ng/ml	99
97) Benzo(g,h,i)perylene	20.897	276	1145867	1509.07	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261909.D  
 Acq On : 26 Nov 2019 12:39 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111196-BSD1  
 Misc : 1x, 625 B(a)P Only  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 26 13:50:33 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261919.D  
 Acq On : 26 Nov 2019 6:39 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BLK1  
 Misc : 1x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 16 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

AMS  
 11/27/19

Quant Time: Nov 27 08:34:02 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.386	152	447964	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.648	136	1661730	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	889317	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1567268	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.532	240	1665591	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.976	264	1619205	2000.00	ng/ml	0.01	
94) Dibenz(a,h)Anthracene-d...	20.362	292	1403400	2000.00	ng/ml	0.01	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.134	112	232455	855.12	ng/ml	-0.02	
5) Phenol-d6 (Surr)	6.043	99	158099	454.37	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	380617	1410.03	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.739	172	1042662	1498.11	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	180742	1904.03	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.670	244	1507233	1963.65	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.658	74	422	N.D.			
3) Pyridine	3.722	79	647	N.D.			
6) Phenol	6.054	94	19564	51.13	ng/ml		91
7) Aniline	6.060	93	610	N.D.			
8) Bis(2-chloroethyl) ether	6.150	93	214	N.D.			
9) 2-Chlorophenol	6.193	128	272	N.D.			
10) 1,3-Dichlorobenzene	6.332	146	84	N.D.			
11) 1,4-Dichlorobenzene	6.402	146	292	N.D.			
12) Benzyl alcohol	6.536	108	364	26.39	ng/ml#		81
13) 1,2-Dichlorobenzene	6.557	146	168	N.D.			
14) 2-Methylphenol	6.643	107	618	2.68	ng/ml		79
15) 2,2'-Oxybis(1-Chloropr...	6.669	45	258	N.D.			
16) N-Nitrosodi-n-propylamine	6.776	70	432	N.D.			
17) 3+4-Methylphenol	6.792	107	322	N.D.			
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	6.953	77	174	N.D.			
22) Isophorone	7.188	82	646	N.D.			
23) 2-Nitrophenol	7.274	139	191	43.47	ng/ml#		65
24) 2,4-Dimethylphenol	7.327	122	678	3.04	ng/ml#		55
25) Bis(2-chloroethoxy) me...	7.397	93	228	N.D.			
26) Benzoic acid	7.402	105	5946	850.06	ng/ml		80
27) 2,4-Dichlorophenol	7.493	162	56	25.13	ng/ml#		1
28) 1,2,4-Trichlorobenzene	0.000		0	N.D.			
29) Naphthalene	7.669	128	13757	15.74	ng/ml		95
30) 4-Chloroaniline	7.739	127	155	13.80	ng/ml#		16
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	8.220	107	984	4.46	ng/ml		42
33) 2-Methylnaphthalene	8.365	142	6241	10.22	ng/ml		95
34) 1-Methylnaphthalene	8.466	142	3515	5.94	ng/ml		93
36) Hexachlorocyclopentadiene	0.000		0	N.D.			
37) 2,4,6-Trichlorophenol	8.573	196	59	24.08	ng/ml#		13
38) 2,4,5-Trichlorophenol	8.659	198	106	23.38	ng/ml#		66
39) 1,1'-Biphenyl	8.835	154	5077	6.64	ng/ml		91
41) 2-Chloronaphthalene	8.862	162	354	N.D.			
42) 2-Nitroaniline	8.948	138	163	31.44	ng/ml#		71
43) 2,6-Dimethylnaphthalene	9.007	156	4152	7.40	ng/ml		86

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261919.D  
 Acq On : 26 Nov 2019 6:39 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BLK1  
 Misc : 1x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 16 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Nov 27 08:34:02 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.071	168	125	68.07	ng/ml#	32
45) Dimethyl phthalate	9.140	163	754	N.D.		
46) 1,3-Dinitrobenzene	9.188	168	161	59.63	ng/ml#	1
47) 2,6-Dinitrotoluene	9.199	165	855	30.81	ng/ml#	54
48) 1,2-Dinitrobenzene	9.269	168	64	N.D.		
49) Acenaphthylene	9.274	152	1354	N.D.		
50) 3-Nitroaniline	9.392	138	89	30.35	ng/ml#	47
51) Acenaphthene	9.456	153	2084	3.51	ng/ml	93
52) 2,4-Dinitrophenol	9.408	184	60	229.21	ng/ml#	1
53) 4-Nitrophenol	9.552	139	213	76.16	ng/ml#	1
54) 2,4-Dinitrotoluene	9.606	165	2949	69.08	ng/ml#	54
55) Dibenzofuran	9.632	168	1379	N.D.		
56) 2,3,5,6-Tetrachlorophenol	9.718	232	52	35.90	ng/ml#	1
57) 2,3,4,6-Tetrachlorophenol	9.766	232	164	29.46	ng/ml#	1
58) Diethyl phthalate	9.857	149	4249	7.19	ng/ml	96
59) 2,3,5-Trimethylnaphtha...	9.841	170	2544	5.05	ng/ml	85
60) Fluorene	9.980	166	3801	6.10	ng/ml#	84
61) 4-Chlorophenyl phenyl ...	9.980	204	233	N.D.		
62) 4-Nitroaniline	10.007	138	87	N.D.		
63) 4,6-Dinitro-2-methylph...	9.991	198	67	159.67	ng/ml#	1
65) N-Nitrosodiphenylamine	10.108	169	1813	3.75	ng/ml#	1
66) Azobenzene (1,2-DPH)	10.151	77	3164	6.47	ng/ml#	1
68) 4-Bromophenyl phenyl e...	10.494	248	75	N.D.		
69) Hexachlorobenzene	0.000		0	N.D.		
70) Pentachlorophenol (PCP)	10.756	266	173	78.10	ng/ml#	29
71) Phenanthrene	10.959	178	12352	14.05	ng/ml	71
72) Anthracene	11.007	178	1077	N.D.		
73) Carbazole	11.173	167	1129	6.93	ng/ml#	1
74) Di-n-butyl phthalate	11.526	149	24464	26.39	ng/ml	98
75) Fluoranthene	12.200	202	5744	6.37	ng/ml	81
76) Benzidine	12.344	184	90	123.38	ng/ml#	1
77) Pyrene	12.467	202	8513	9.28	ng/ml	97
80) Butyl benzyl phthalate	13.414	149	2188	34.43	ng/ml	88
81) Bis(2-ethylhexyl) adipate	13.585	129	8341	21.59	ng/ml	95
82) 3,3-Dichlorobenzidine	14.500	252	52	Below Cal	#	1
83) Benz(a)anthracene	14.532	228	5742	6.17	ng/ml	70
84) Chrysene	14.585	228	1756	N.D.		
85) Bis(2-ethylhexyl) phth...	14.687	149	63675	106.28	ng/ml	95
87) Di-n-octyl phthalate	16.350	149	163	58.11	ng/ml#	1
88) Benzo(b)fluoranthene	17.072	252	1579	9.73	ng/ml	74
89) Benzo(k)fluoranthene	17.104	252	506	9.02	ng/ml	71
90) Benzo(b+k)fluoranthene	17.072	252	2381	18.30	ng/ml	74
91) Benzo(e)pyrene	17.704	252	899	N.D.		
92) Benzo(a)pyrene	17.811	252	1521	11.70	ng/ml#	1
93) Perylene	17.976	252	6093	8.34	ng/ml	69
95) Indeno(1,2,3-cd)pyrene	20.351	276	1740	N.D.		
96) Dibenz(a,h)anthracene	20.431	278	198	N.D.		
97) Benzo(g,h,i)perylene	20.875	276	1465	N.D.		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261919.D  
 Acq On : 26 Nov 2019 6:39 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BLK1  
 Misc : 1x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 16 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 27 08:34:02 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10





Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261920.D  
 Acq On : 26 Nov 2019 7:16 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BS104  
 Misc : 4x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 17 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 27 08:34:08 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

AMS  
11/27/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							
1) 1,4-Dichlorobenzene-d4...	6.386	152	438453	2000.00	ng/ml	0.00	
2) Naphthalene-d8 (ISTD)	7.648	136	1664129	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	892444	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1630686	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.532	240	1668578	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.976	264	1655049	2000.00	ng/ml	0.01	
94) Dibenz(a,h)Anthracene-d...	20.367	292	1438024	2000.00	ng/ml	0.02	
System Monitoring Compounds							
4) 2-Fluorophenol (Surr)	5.134	112	73222	275.20	ng/ml	-0.02	
5) Phenol-d6 (Surr)	6.038	99	57263	168.14	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.931	82	119835	453.57	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.734	172	361536	517.64	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	50876	527.51	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	427706	556.22	ng/ml	0.00	
Target Compounds							
2) N-Nitrosodimethylamine	3.738	74	75630	452.85	ng/ml		Qvalue 93
3) Pyridine	3.760	79	98624m	346.39	ng/ml		
6) Phenol	6.054	94	114280	305.17	ng/ml		98
7) Aniline	6.065	93	120141	371.86	ng/ml		99
8) Bis(2-chloroethyl) ether	6.124	93	226904	671.39	ng/ml		99
9) 2-Chlorophenol	6.188	128	227361	732.35	ng/ml		97
10) 1,3-Dichlorobenzene	6.332	146	252965	724.92	ng/ml		96
11) 1,4-Dichlorobenzene	6.402	146	244978	714.29	ng/ml		97
12) Benzyl alcohol	6.525	108	116195	642.91	ng/ml		94
13) 1,2-Dichlorobenzene	6.552	146	245565	726.03	ng/ml		99
14) 2-Methylphenol	6.637	107	155240	687.41	ng/ml		97
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	172086	576.98	ng/ml		84
16) N-Nitrosodi-n-propylamine	6.782	70	135880	692.50	ng/ml		92
17) 3+4-Methylphenol	6.787	107	175254	625.84	ng/ml		95
18) Hexachloroethane	6.889	201	82709	784.87	ng/ml		89
20) Nitrobenzene	6.948	77	189838	709.19	ng/ml		92
22) Isophorone	7.183	82	410488	773.72	ng/ml		99
23) 2-Nitrophenol	7.268	139	162758	1035.96	ng/ml		85
24) 2,4-Dimethylphenol	7.311	122	186092	834.05	ng/ml		94
25) Bis(2-chloroethoxy) me...	7.397	93	255789	793.06	ng/ml		99
26) Benzoic acid	7.391	105	73867	1344.83	ng/ml		93
27) 2,4-Dichlorophenol	7.509	162	208694	839.65	ng/ml		96
28) 1,2,4-Trichlorobenzene	7.589	180	237365	814.97	ng/ml		99
29) Naphthalene	7.670	128	696227	795.30	ng/ml		99
30) 4-Chloroaniline	7.728	127	128637	470.12	ng/ml		97
31) Hexachlorobutadiene	7.803	225	123224	782.94	ng/ml		96
32) 4-Chloro-3-methylphenol	8.215	107	184850	837.12	ng/ml		91
33) 2-Methylnaphthalene	8.365	142	520719	851.32	ng/ml		99
34) 1-Methylnaphthalene	8.467	142	488973	825.79	ng/ml		99
36) Hexachlorocyclopentadiene	8.536	237	116774	846.16	ng/ml		97
37) 2,4,6-Trichlorophenol	8.654	196	159120	924.86	ng/ml		98
38) 2,4,5-Trichlorophenol	8.691	198	163448	961.23	ng/ml		99
39) 1,1'-Biphenyl	8.836	154	1858	N.D.			
41) 2-Chloronaphthalene	8.857	162	482520	870.99	ng/ml		97
42) 2-Nitroaniline	8.959	138	160560	974.28	ng/ml		90
43) 2,6-Dimethylnaphthalene	8.996	156	237	N.D.			

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261920.D  
 Acq On : 26 Nov 2019 7:16 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BS104  
 Misc : 4x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 17 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Nov 27 08:34:08 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	75470	1089.61	ng/ml	82
45) Dimethyl phthalate	9.146	163	582552	903.88	ng/ml	99
46) 1,3-Dinitrobenzene	9.173	168	85556	971.62	ng/ml	86
47) 2,6-Dinitrotoluene	9.205	165	131629	909.82	ng/ml	87
48) 1,2-Dinitrobenzene	9.258	168	59900	917.39	ng/ml	87
49) Acenaphthylene	9.280	152	763654	841.75	ng/ml	99
50) 3-Nitroaniline	9.376	138	97529	843.37	ng/ml	90
51) Acenaphthene	9.456	153	472568	793.25	ng/ml	100
52) 2,4-Dinitrophenol	9.483	184	42678	1194.48	ng/ml	88
53) 4-Nitrophenol	9.558	139	30214	406.86	ng/ml	94
54) 2,4-Dinitrotoluene	9.611	165	165691	920.11	ng/ml	88
55) Dibenzofuran	9.633	168	679281	855.37	ng/ml	98
56) 2,3,5,6-Tetrachlorophenol	9.718	232	129703	952.74	ng/ml	93
57) 2,3,4,6-Tetrachlorophenol	9.761	232	132732	889.56	ng/ml	98
58) Diethyl phthalate	9.863	149	551367	929.37	ng/ml	97
59) 2,3,5-Trimethylnaphtha...	9.825	170	143	N.D.		
60) Fluorene	9.980	166	526684	842.76	ng/ml	99
61) 4-Chlorophenyl phenyl ...	9.980	204	260142	853.84	ng/ml	93
62) 4-Nitroaniline	9.996	138	108492	1131.24	ng/ml	96
63) 4,6-Dinitro-2-methylph...	10.034	198	78445	1197.84	ng/ml	86
65) N-Nitrosodiphenylamine	10.098	169	447237	889.50	ng/ml	99
66) Azobenzene (1,2-DPH)	10.141	77	372825	732.73	ng/ml	83
68) 4-Bromophenyl phenyl e...	10.478	248	161849	879.59	ng/ml	95
69) Hexachlorobenzene	10.553	284	185331	839.58	ng/ml	98
70) Pentachlorophenol (PCP)	10.750	266	90236	830.73	ng/ml	99
71) Phenanthrene	10.959	178	747957	817.60	ng/ml	99
72) Anthracene	11.012	178	772510	878.49	ng/ml	99
73) Carbazole	11.173	167	684311	993.67	ng/ml	98
74) Di-n-butyl phthalate	11.526	149	905115	938.55	ng/ml	99
75) Fluoranthene	12.195	202	870298	928.20	ng/ml	99
76) Benzidine	12.350	184	87551	488.43	ng/ml	97
77) Pyrene	12.467	202	895103	938.09	ng/ml	100
80) Butyl benzyl phthalate	13.419	149	394882	928.35	ng/ml	91
81) Bis(2-ethylhexyl) adipate	13.585	129	355350	918.22	ng/ml	98
82) 3,3-Dichlorobenzidine	14.484	252	282672	2174.56	ng/ml	95
83) Benz(a)anthracene	14.505	228	824732	885.28	ng/ml	97
84) Chrysene	14.585	228	764962	876.21	ng/ml	98
85) Bis(2-ethylhexyl) phth...	14.687	149	572981	954.64	ng/ml	99
87) Di-n-octyl phthalate	16.334	149	927112	978.70	ng/ml	99
88) Benzo(b)fluoranthene	17.062	252	803002	882.11	ng/ml	98
89) Benzo(k)fluoranthene	17.126	252	814006	882.69	ng/ml	99
90) Benzo(b+k)fluoranthene	17.126	252	1644258	1754.68	ng/ml	99
91) Benzo(e)pyrene	17.704	252	685	N.D.		
92) Benzo(a)pyrene	17.827	252	719644	869.80	ng/ml	97
93) Perylene	17.976	252	12430	16.65	ng/ml	74
95) Indeno(1,2,3-cd)pyrene	20.357	276	704753	828.77	ng/ml	100
96) Dibenz(a,h)anthracene	20.431	278	674668	864.14	ng/ml	100
97) Benzo(g,h,i)perylene	20.897	276	733720	898.29	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261920.D  
 Acq On : 26 Nov 2019 7:16 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BS1@4  
 Misc : 4x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 17 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 27 08:34:08 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261921.D  
 Acq On : 26 Nov 2019 7:52 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BSD1@4  
 Misc : 4x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 18 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

*Q-19*  
*AMS*  
*11/27/19*

Quant Time: Nov 27 08:34:14 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.386	152	423520	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.648	136	1639490	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	885845	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.937	188	1614446	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.537	240	1638936	2000.00	ng/ml	0.01	
86) Perylene-d12 (ISTD)	17.976	264	1637848	2000.00	ng/ml	0.01	
94) Dibenz(a,h)Anthrcene-d...	20.367	292	1412595	2000.00	ng/ml	0.02	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.129	112	65383	254.40	ng/ml	-0.02	
5) Phenol-d6 (Surr)	6.038	99	48817	148.40	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	6.926	82	111266	435.98	ng/ml	-0.01	
40) 2-Fluorobiphenyl (Surr)	8.734	172	352909	509.05	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.226	330	49605	519.85	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.665	244	427776	566.38	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.738	74	61565m	381.63	ng/ml		
3) Pyridine	3.760	79	85952m	312.52	ng/ml		
6) Phenol	6.054	94	100336	277.38	ng/ml		98
7) Aniline	6.065	93	97096	311.12	ng/ml		98
8) Bis(2-chloroethyl) ether	6.124	93	218778	670.17	ng/ml		99
9) 2-Chlorophenol	6.183	128	210454	701.79	ng/ml		99
10) 1,3-Dichlorobenzene	6.332	146	231586	687.06	ng/ml		97
11) 1,4-Dichlorobenzene	6.402	146	229423	692.52	ng/ml		98
12) Benzyl alcohol	6.525	108	108722	623.67	ng/ml		94
13) 1,2-Dichlorobenzene	6.552	146	235173	719.82	ng/ml		98
14) 2-Methylphenol	6.637	107	144037	660.29	ng/ml		99
15) 2,2'-Oxybis(1-Chloropr...	6.653	45	164819	572.10	ng/ml		85
16) N-Nitrosodi-n-propylamine	6.782	70	135844	716.73	ng/ml		91
17) 3+4-Methylphenol	6.787	107	162438	600.53	ng/ml		95
18) Hexachloroethane	6.889	201	73950	726.49	ng/ml		88
20) Nitrobenzene	6.947	77	181509	701.98	ng/ml		89
22) Isophorone	7.183	82	396356	758.31	ng/ml		99
23) 2-Nitrophenol	7.268	139	155469	1005.80	ng/ml		86
24) 2,4-Dimethylphenol	7.311	122	175774	799.65	ng/ml		95
25) Bis(2-chloroethoxy) me...	7.397	93	245314	772.02	ng/ml		99
26) Benzoic acid	7.391	105	63500	1277.04	ng/ml		95
27) 2,4-Dichlorophenol	7.509	162	203317	830.50	ng/ml		96
28) 1,2,4-Trichlorobenzene	7.595	180	224859	783.64	ng/ml		99
29) Naphthalene	7.669	128	668272	774.84	ng/ml		100
30) 4-Chloroaniline	7.728	127	139031	515.10	ng/ml		94
31) Hexachlorobutadiene	7.803	225	118135	761.88	ng/ml		98
32) 4-Chloro-3-methylphenol	8.215	107	178972	822.68	ng/ml		91
33) 2-Methylnaphthalene	8.365	142	496184	823.40	ng/ml		99
34) 1-Methylnaphthalene	8.466	142	469675	805.12	ng/ml		99
36) Hexachlorocyclopentadiene	8.536	237	110048	803.36	ng/ml		97
37) 2,4,6-Trichlorophenol	8.654	196	157548	922.61	ng/ml		99
38) 2,4,5-Trichlorophenol	8.691	198	155263	920.85	ng/ml		99
39) 1,1'-Biphenyl	8.835	154	1842	N.D.			
41) 2-Chloronaphthalene	8.857	162	465483	846.50	ng/ml		96
42) 2-Nitroaniline	8.958	138	155269	950.33	ng/ml		88
43) 2,6-Dimethylnaphthalene	9.007	156	370	N.D.			

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261921.D  
 Acq On : 26 Nov 2019 7:52 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BSD1@4  
 Misc : 4x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 18 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Nov 27 08:34:14 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.092	168	74050	1078.39	ng/ml	80
45) Dimethyl phthalate	9.146	163	566054	884.83	ng/ml	98
46) 1,3-Dinitrobenzene	9.172	168	85475	977.47	ng/ml	87
47) 2,6-Dinitrotoluene	9.204	165	127901	891.07	ng/ml	89
48) 1,2-Dinitrobenzene	9.258	168	57574	888.34	ng/ml	86
49) Acenaphthylene	9.279	152	745520	827.89	ng/ml	100
50) 3-Nitroaniline	9.376	138	101181	887.97	ng/ml	92
51) Acenaphthene	9.456	153	469701	794.31	ng/ml	98
52) 2,4-Dinitrophenol	9.483	184	44090	1229.24	ng/ml	88
53) 4-Nitrophenol	9.563	139	26735	371.41	ng/ml	90
54) 2,4-Dinitrotoluene	9.611	165	162055	907.29	ng/ml	88
55) Dibenzofuran	9.632	168	671035	851.28	ng/ml	96
56) 2,3,5,6-Tetrachlorophenol	9.718	232	128103	948.22	ng/ml	95
57) 2,3,4,6-Tetrachlorophenol	9.761	232	131756	889.59	ng/ml	98
58) Diethyl phthalate	9.862	149	544030	923.84	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	9.852	170	158	N.D.		
60) Fluorene	9.980	166	511460	824.49	ng/ml	98
61) 4-Chlorophenyl phenyl ...	9.975	204	258851	855.93	ng/ml	96
62) 4-Nitroaniline	9.996	138	106427	1117.97	ng/ml	92
63) 4,6-Dinitro-2-methylph...	10.028	198	80914	1236.33	ng/ml	94
65) N-Nitrosodiphenylamine	10.098	169	433377	870.61	ng/ml	100
66) Azobenzene (1,2-DPH)	10.135	77	365878	726.31	ng/ml	94
68) 4-Bromophenyl phenyl e...	10.477	248	156012	856.40	ng/ml	97
69) Hexachlorobenzene	10.552	284	185915	850.70	ng/ml	97
70) Pentachlorophenol (PCP)	10.750	266	90717	842.41	ng/ml	96
71) Phenanthrene	10.959	178	745932	823.59	ng/ml	99
72) Anthracene	11.012	178	762018	875.27	ng/ml	99
73) Carbazole	11.173	167	681320	1001.37	ng/ml	99
74) Di-n-butyl phthalate	11.526	149	890878	933.08	ng/ml	99
75) Fluoranthene	12.194	202	874146	941.68	ng/ml	99
76) Benzidine	12.350	184	140310	713.56	ng/ml	96
77) Pyrene	12.467	202	901744	954.56	ng/ml	99
80) Butyl benzyl phthalate	13.419	149	397127	949.42	ng/ml	90
81) Bis(2-ethylhexyl) adipate	13.585	129	349495	919.43	ng/ml	97
82) 3,3-Dichlorobenzidine	14.489	252	259085	2003.22	ng/ml	98
83) Benz(a)anthracene	14.505	228	838113	915.91	ng/ml	97
84) Chrysene	14.591	228	759454	885.63	ng/ml	99
85) Bis(2-ethylhexyl) phth...	14.687	149	577206	979.07	ng/ml	98
87) Di-n-octyl phthalate	16.334	149	917376	978.61	ng/ml	98
88) Benzo(b)fluoranthene	17.062	252	808399	897.10	ng/ml	100
89) Benzo(k)fluoranthene	17.126	252	797484	873.73	ng/ml	99
90) Benzo(b+k)fluoranthene	17.126	252	1630967	1758.76	ng/ml	99
91) Benzo(e)pyrene	17.693	252	810	N.D.		
92) Benzo(a)pyrene	17.821	252	727303	888.08	ng/ml	98
93) Perylene	17.971	252	13783	18.66	ng/ml	73
95) Indeno(1,2,3-cd)pyrene	20.351	276	710812	850.94	ng/ml	100
96) Dibenz(a,h)anthracene	20.431	278	690298	900.07	ng/ml	99
97) Benzo(g,h,i)perylene	20.891	276	750806	935.76	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261921.D  
 Acq On : 26 Nov 2019 7:52 pm  
 Operator : JK/ AMS/ DTH  
 Sample : 9111242-BSD1@4  
 Misc : 4x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 18 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 27 08:34:14 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 Last Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261922.D  
 Acq On : 26 Nov 2019 8:27 pm  
 Operator : JK/ AMS/ DTH  
 Sample : A9K0412-01@50  
 Misc : 50x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 19 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

*RRI*  
*AMS*  
*11/27/19*

Quant Time: Nov 27 08:34:19 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.381	152	408104	2000.00	ng/ml	-0.01	
21) Naphthalene-d8 (ISTD)	7.648	136	1648670	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.424	162	892217	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	10.938	188	1578416	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.527	240	1633311	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	17.971	264	1581008	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.362	292	1341695	2000.00	ng/ml	0.01	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.129	112	3475	14.03	ng/ml	-0.02	
5) Phenol-d6 (Surr)	6.054	99	1489	4.70	ng/ml	0.01	
19) Nitrobenzene-d5 (Surr)	6.937	82	6857	27.88	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.739	172	24208	34.67	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.237	330	2162	46.07	ng/ml	0.01	
79) Terphenyl-d14 (Surr)	12.665	244	29986	39.84	ng/ml	0.00	
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	0.000		0	N.D.			Qvalue
3) Pyridine	3.824	79	736m	2.78	ng/ml#		
6) Phenol	6.070	94	52	N.D.			
7) Aniline	6.065	93	69	N.D.			
8) Bis(2-chloroethyl) ether	6.065	93	69	N.D.			
9) 2-Chlorophenol	0.000		0	N.D.			
10) 1,3-Dichlorobenzene	0.000		0	N.D.			
11) 1,4-Dichlorobenzene	0.000		0	N.D.			
12) Benzyl alcohol	0.000		0	N.D.			
13) 1,2-Dichlorobenzene	0.000		0	N.D.			
14) 2-Methylphenol	0.000		0	N.D.			
15) 2,2'-Oxybis(1-Chloropr...	6.648	45	66	N.D.			
16) N-Nitrosodi-n-propylamine	6.739	70	70	N.D.			
17) 3+4-Methylphenol	6.760	107	63	N.D.			
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	6.926	77	225	N.D.			
22) Isophorone	7.178	82	168	N.D.			
23) 2-Nitrophenol	0.000		0	N.D.			
24) 2,4-Dimethylphenol	0.000		0	N.D.			
25) Bis(2-chloroethoxy) me...	7.402	93	73	N.D.			
26) Benzoic acid	7.424	105	99	806.77	ng/ml#		23
27) 2,4-Dichlorophenol	0.000		0	N.D.			
28) 1,2,4-Trichlorobenzene	0.000		0	N.D.			
29) Naphthalene	7.664	128	7290	8.41	ng/ml		96
30) 4-Chloroaniline	7.771	127	84	13.55	ng/ml#		46
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	0.000		0	N.D.			
33) 2-Methylnaphthalene	8.370	142	6529	10.77	ng/ml		94
34) 1-Methylnaphthalene	8.467	142	4344	7.41	ng/ml		88
36) Hexachlorocyclopentadiene	0.000		0	N.D.			
37) 2,4,6-Trichlorophenol	0.000		0	N.D.			
38) 2,4,5-Trichlorophenol	8.729	198	50	23.05	ng/ml#		9
39) 1,1'-Biphenyl	8.841	154	2217	2.89	ng/ml		96
41) 2-Chloronaphthalene	8.911	162	261	N.D.			
42) 2-Nitroaniline	0.000		0	N.D.			
43) 2,6-Dimethylnaphthalene	9.007	156	2608	4.64	ng/ml		73

Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261922.D  
 Acq On : 26 Nov 2019 8:27 pm  
 Operator : JK/ AMS/ DTH  
 Sample : A9K0412-01@50  
 Misc : 50x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 19 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 27 08:34:19 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	0.000		0		N.D.	
45) Dimethyl phthalate	9.157	163	162		N.D.	
46) 1,3-Dinitrobenzene	0.000		0		N.D.	
47) 2,6-Dinitrotoluene	9.151	165	58	25.46	ng/ml#	49
48) 1,2-Dinitrobenzene	0.000		0		N.D.	
49) Acenaphthylene	9.280	152	996		N.D.	
50) 3-Nitroaniline	9.424	138	150	30.78	ng/ml#	1
51) Acenaphthene	9.456	153	17403	29.22	ng/ml	96
52) 2,4-Dinitrophenol	0.000		0		N.D.	
53) 4-Nitrophenol	9.542	139	125	75.15	ng/ml#	1
54) 2,4-Dinitrotoluene	9.595	165	281	55.20	ng/ml#	27
55) Dibenzofuran	9.633	168	1144		N.D.	
56) 2,3,5,6-Tetrachlorophenol	0.000		0		N.D.	
57) 2,3,4,6-Tetrachlorophenol	0.000		0		N.D.	
58) Diethyl phthalate	9.857	149	172		N.D.	
59) 2,3,5-Trimethylnaphtha...	9.847	170	488		N.D.	
60) Fluorene	9.980	166	6219	9.95	ng/ml	88
61) 4-Chlorophenyl phenyl ...	0.000		0		N.D.	
62) 4-Nitroaniline	9.980	138	54		N.D.	
63) 4,6-Dinitro-2-methylph...	0.000		0		N.D.	
65) N-Nitrosodiphenylamine	10.103	169	266		N.D.	
66) Azobenzene (1,2-DPH)	10.151	77	221		N.D.	
68) 4-Bromophenyl phenyl e...	0.000		0		N.D.	
69) Hexachlorobenzene	0.000		0		N.D.	
70) Pentachlorophenol (PCP)	10.697	266	123	77.66	ng/ml#	33
71) Phenanthrene	10.959	178	29306	33.10	ng/ml	98
72) Anthracene	11.007	178	3637	4.27	ng/ml	95
73) Carbazole	11.178	167	1745	7.64	ng/ml	89
74) Di-n-butyl phthalate	11.526	149	598		N.D.	
75) Fluoranthene	12.195	202	7223	7.96	ng/ml	92
76) Benzidine	0.000		0		N.D.	
77) Pyrene	12.467	202	8306	8.99	ng/ml	98
80) Butyl benzyl phthalate	0.000		0		N.D.	
81) Bis(2-ethylhexyl) adipate	13.585	129	11362	29.99	ng/ml	99
82) 3,3-Dichlorobenzidine	0.000		0		N.D.	
83) Benz(a)anthracene	14.532	228	3967	4.35	ng/ml	66
84) Chrysene	14.585	228	527		N.D.	
85) Bis(2-ethylhexyl) phth...	14.687	149	635		N.D.	
87) Di-n-octyl phthalate	16.292	149	223	58.17	ng/ml	59
88) Benzo(b)fluoranthene	17.078	252	64	8.03	ng/ml	57
89) Benzo(k)fluoranthene	17.078	252	64	8.55	ng/ml	57
90) Benzo(b+k)fluoranthene	17.078	252	64	15.81	ng/ml	57
91) Benzo(e)pyrene	17.709	252	68		N.D.	
92) Benzo(a)pyrene	17.821	252	63	9.92	ng/ml	59
93) Perylene	17.971	252	4823	6.76	ng/ml	66
95) Indeno(1,2,3-cd)pyrene	20.351	276	582		N.D.	
96) Dibenz(a,h)anthracene	20.415	278	63		N.D.	
97) Benzo(g,h,i)perylene	0.000		0		N.D.	

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : T:\data\2019-11\9K26022\  
 Data File : J11261922.D  
 Acq On : 26 Nov 2019 8:27 pm  
 Operator : JK/ AMS/ DTH  
 Sample : A9K0412-01@50  
 Misc : 50x, 8270D TCLP SVOC REG LIST  
 ALS Vial : 19 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Nov 27 08:34:19 2019  
 Quant Method : T:\methods\SV10\_091919R4.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Oct 25 11:15:50 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



**TCLP Semivolatile Organic Compounds by EPA 8270D  
Calibration Data**

Sequence 9119035 (Cal ID A9I2405) SV-GCMS10



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence: **9I19035**

Instrument: **SV-GCMS10**

Date: **09/19/19 17:44**

Calibration: **A9I2405**

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
1	9I19035-IBL1	Water	QC	QC			A19I086	
2	9I19035-TUN1	Water	QC	QC			A19I086	A19I165
3	9I19035-ICB1	Water	QC	QC			A19I086	
4	9I19035-CAL1	Water	QC	QC			A19I086	A19G238
5	9I19035-CAL2	Water	QC	QC			A19I086	A19G239
6	9I19035-CAL3	Water	QC	QC			A19I086	A19G240
7	9I19035-CAL4	Water	QC	QC			A19I086	A19G241
8	9I19035-CAL5	Water	QC	QC			A19I086	A19G242
9	9I19035-CAL6	Water	QC	QC			A19I086	A19G243
10	9I19035-CAL7	Water	QC	QC			A19I086	A19G244
11	9I19035-CAL8	Water	QC	QC			A19I086	A19G245
12	9I19035-CAL9	Water	QC	QC			A19I086	A19G246
13	9I19035-CALA	Water	QC	QC			A19I086	A19G247
14	9I19035-IBL2	Water	QC	QC			A19I086	
15	9I19035-ICV1	Water	QC	QC			A19I086	A19I254
16	9I19035-IBL3	Water	QC	QC			A19I086	

Data Entered By: JD 9/24/19

Comments:

Data Reviewed By: MVF 9/26/19

Calibration Status Report SV-GCMS10

Method Path : C:\msdchem\1\methods\  
 Method File : SV10\_091919.M  
 Title : EPA 8270D: Semivolatile Organics  
 Last Update : Fri Sep 20 10:41:03 2019  
 Response Via : Initial Calibration

*A9I 2405*  
*Old 9/23/19*

#	ID	Conc	ISTD Conc	Path\File
1	20	20	2000	C:\msdchem\1\data\2019-09\9I19035\J09191918.D
2	50	50	2000	C:\msdchem\1\data\2019-09\9I19035\J09191919.D
3	100	100	2000	C:\msdchem\1\data\2019-09\9I19035\J09191920.D
4	200	200	2000	C:\msdchem\1\data\2019-09\9I19035\J09191921.D
5	500	500	2000	C:\msdchem\1\data\2019-09\9I19035\J09191922.D
6	1000	1000	2000	C:\msdchem\1\data\2019-09\9I19035\J09191923.D
7	2000	2000	2000	C:\msdchem\1\data\2019-09\9I19035\J09191924.D
8	4000	4000	2000	C:\msdchem\1\data\2019-09\9I19035\J09191925.D
9	6000	6000	2000	C:\msdchem\1\data\2019-09\9I19035\J09191926.D
10	8000	8000	2000	C:\msdchem\1\data\2019-09\9I19035\J09191927.D

#	ID	Update Time	Quant Time	Acquisition Time
1	20	Sep 20 10:40 2019	Sep 20 10:14 2019	20 Sep 2019 1:24 am
2	50	Sep 20 10:40 2019	Sep 20 10:17 2019	20 Sep 2019 1:59 am
3	100	Sep 20 10:40 2019	Sep 20 10:18 2019	20 Sep 2019 2:34 am
4	200	Sep 20 10:40 2019	Sep 20 10:21 2019	20 Sep 2019 3:09 am
5	500	Sep 20 10:40 2019	Sep 20 10:22 2019	20 Sep 2019 3:44 am
6	1000	Sep 20 10:40 2019	Sep 20 09:46 2019	20 Sep 2019 4:19 am
7	2000	Sep 20 10:40 2019	Sep 20 09:46 2019	20 Sep 2019 4:54 am
8	4000	Sep 20 10:40 2019	Sep 20 10:28 2019	20 Sep 2019 5:29 am
9	6000	Sep 20 10:40 2019	Sep 20 10:29 2019	20 Sep 2019 6:04 am
10	8000	Sep 20 10:41 2019	Sep 20 10:30 2019	20 Sep 2019 6:39 am

SV10\_091919.M Fri Sep 20 14:11:04 2019

Compound List Report SV-GCMS10

Method Path : C:\msdchem\1\methods\  
 Method File : SV10\_091919.M  
 Title : EPA 8270D: Semivolatile Organics  
 Last Update : Fri Sep 20 10:41:03 2019  
 Response Via : Initial Calibration

*9/20/19*

Total Cpnds : 97

PK#	Compound Name	QIon	Exp_RT	Rel_RT	Cal	#Qual	A/H	ID
1	I 1,4-Dichlorobenzene-d4 (ISTD)	152	6.568	1.000	A	2	A	R
2	T N-Nitrosodimethylamine	74	3.883	0.591	A	2	A	A
3	T Pyridine	79	3.904	0.594	A	2	A	A
4	S 2-Fluorophenol (Surr)	112	5.289	0.805	A	1	A	R
5	S Phenol-d6 (Surr)	99	6.204	0.945	A	2	A	R
6	T Phenol	94	6.215	0.946	A	2	A	R
7	T Aniline	93	6.241	0.950	A	2	A	R
8	T Bis(2-chloroethyl) ether	93	6.305	0.960	A	2	A	R
9	T 2-Chlorophenol	128	6.364	0.969	A	2	A	R
10	T 1,3-Dichlorobenzene	146	6.514	0.992	A	2	A	R
11	T 1,4-Dichlorobenzene	146	6.584	1.002	A	2	A	R
12	T Benzyl alcohol	108	6.701	1.020	-Q	2	A	R
13	T 1,2-Dichlorobenzene	146	6.739	1.026	A	2	A	R
14	T 2-Methylphenol	107	6.808	1.037	A	2	A	R
15	T 2,2'-Oxybis(1-Chloropropane)	45	6.835	1.041	A	2	A	R
16	T N-Nitrosodi-n-propylamine	70	6.963	1.060	A	2	A	R
17	T 3+4-Methylphenol	107	6.958	1.059	A	3	A	R
18	T Hexachloroethane	201	7.076	1.077	A	2	A	R
19	S Nitrobenzene-d5 (Surr)	82	7.113	1.083	A	2	A	R
20	T Nitrobenzene	77	7.129	1.085	A	2	A	R
21	I Naphthalene-d8 (ISTD)	136	7.835	1.000	A	1	A	R
22	T Isophorone	82	7.370	0.941	A	2	A	R
23	T 2-Nitrophenol	139	7.450	0.951	-Q	2	A	R
24	T 2,4-Dimethylphenol	122	7.487	0.956	A	2	A	R
25	T Bis(2-chloroethoxy) methane	93	7.579	0.967	A	2	A	R
26	T Benzoic acid	105	7.578	0.967	-Q	2	A	R
27	T 2,4-Dichlorophenol	162	7.690	0.981	-Q	2	A	R
28	T 1,2,4-Trichlorobenzene	180	7.782	0.993	A	2	A	R
29	T Naphthalene	128	7.857	1.003	A	1	A	R
30	T 4-Chloroaniline	127	7.904	1.009	-Q	2	A	R
31	T Hexachlorobutadiene	225	7.990	1.020	A	2	A	R
32	T 4-Chloro-3-methylphenol	107	8.386	1.070	A	2	A	R
33	T 2-Methylnaphthalene	142	8.557	1.092	A	2	A	R
34	T 1-Methylnaphthalene	142	8.659	1.105	A	2	A	R
35	I Acenaphthene-d10 (ISTD)	162	9.616	1.000	A	2	A	R
36	T Hexachlorocyclopentadiene	237	8.728	0.908	A	2	A	R
37	T 2,4,6-Trichlorophenol	196	8.840	0.919	-Q	2	A	R
38	T 2,4,5-Trichlorophenol	198	8.872	0.923	-Q	2	A	R
39	T 1,1'-Biphenyl	154	9.028	0.939	A	2	A	R
40	S 2-Fluorobiphenyl (Surr)	172	8.926	0.928	A	2	A	R
41	T 2-Chloronaphthalene	162	9.049	0.941	A	2	A	R
42	T 2-Nitroaniline	138	9.145	0.951	-Q	2	A	R
43	T 2,6-Dimethylnaphthalene	156	9.188	0.955	A	2	A	R
44	T 1,4-Dinitrobenzene	168	9.274	0.964	-Q	2	A	R
45	T Dimethyl phthalate	163	9.333	0.971	A	2	A	R
46	T 1,3-Dinitrobenzene	168	9.354	0.973	-Q	2	A	R
47	T 2,6-Dinitrotoluene	165	9.391	0.977	-Q	2	A	R
48	T 1,2-Dinitrobenzene	168	9.445	0.982	A	2	A	R
49	T Acenaphthylene	152	9.471	0.985	A	2	A	R
50	T 3-Nitroaniline	138	9.562	0.994	-Q	2	A	R
51	T Acenaphthene	153	9.648	1.003	A	2	A	R
52	T 2,4-Dinitrophenol	184	9.664	1.005	-Q	2	A	R
53	T 4-Nitrophenol	139	9.723	1.011	-Q	2	A	R
54	T 2,4-Dinitrotoluene	165	9.798	1.019	-Q	2	A	R

55	T	Dibenzofuran	168	9.825	1.022	A	2	A	R
56	T	2,3,5,6-Tetrachlorophenol	232	9.905	1.030	Q 1/a <sup>2</sup>	2	A	R
57	T	2,3,4,6-Tetrachlorophenol	232	9.947	1.034	Q 1/a <sup>2</sup>	2	A	R
58	T	Diethyl phthalate	149	10.050	1.045	A	2	A	R
59	T	2,3,5-Trimethylnaphthalene	170	10.039	1.044	A	2	A	R
60	T	Fluorene	166	10.172	1.058	A	2	A	R
61	T	4-Chlorophenyl phenyl ether	204	10.167	1.057	A	2	A	R
62	T	4-Nitroaniline	138	10.183	1.059	A	2	A	R
63	T	4,6-Dinitro-2-methylphenol	198	10.215	1.062	Q 1/a <sup>2</sup>	2	A	R
64	I	Phenanthrene-d10 (ISTD)	188	11.135	1.000	A	2	A	R
65	T	N-Nitrosodiphenylamine	169	10.284	0.924	A	2	A	R
66	T	Azobenzene (1,2-DPH)	77	10.327	0.927	A	2	A	R
67	S	2,4,6-Tribromophenol (Surr)	330	10.418	0.936	Q 1/a <sup>2</sup>	2	A	R
68	T	4-Bromophenyl phenyl ether	248	10.670	0.958	A	2	A	R
69	T	Hexachlorobenzene	284	10.745	0.965	A	2	A	R
70	T	Pentachlorophenol (PCP)	266	10.942	0.983	Q 1/a	2	A	R
71	T	Phenanthrene	178	11.156	1.002	A	2	A	R
72	T	Anthracene	178	11.210	1.007	A 1/a <sup>2</sup>	2	A	R
73	T	Carbazole	167	11.365	1.021	Q 1/a <sup>2</sup>	2	A	R
74	T	Di-n-butyl phthalate	149	11.718	1.052	A	2	A	R
75	T	Fluoranthene	202	12.424	1.116	A 1/a <sup>2</sup>	2	A	R
76	T	Benzidine	184	12.579	1.130	Q 1/a <sup>2</sup>	2	A	R
77	T	Pyrene	202	12.713	1.142	A	2	A	R
78	I	Chrysene-d12 (ISTD)	240	14.917	1.000	A	2	A	R
79	S	Terphenyl-d14 (Surr)	244	12.922	0.866	A	2	A	R
80	T	Butyl benzyl phthalate	149	13.734	0.921	Q 1/a <sup>2</sup>	2	A	R
81	T	Bis(2-ethylhexyl) adipate	129	13.911	0.933	A	2	A	R
82	T	3,3-Dichlorobenzidine	252	14.863	0.996	Q 1/a <sup>2</sup>	2	A	R
83	T	Benz(a)anthracene	228	14.890	0.998	A	2	A	R
84	T	Chrysene	228	14.976	1.004	A	2	A	R
85	T	Bis(2-ethylhexyl) phthalate	149	15.071	1.010	A	2	A	R
86	I	Perylene-d12 (ISTD)	264	18.399	1.000	A 1/a <sup>2</sup>	2	A	R
87	T	Di-n-octyl phthalate	149	16.746	0.910	Q 1/a <sup>2</sup>	2	A	R
88	T	Benzo(b)fluoranthene	252	17.478	0.950	Q 1/a <sup>2</sup>	2	A	R
89	T	Benzo(k)fluoranthene	252	17.548	0.954	Q 1/a <sup>2</sup>	2	A	R
90	T	Benzo(b+k)fluoranthene	252	17.548	0.954	Q 1/a <sup>2</sup>	2	A	R
91	T	Benzo(e)pyrene	252	18.137	0.986	A 1/a <sup>2</sup>	2	A	R
92	T	Benzo(a)pyrene	252	18.254	0.992	Q 1/a <sup>2</sup>	2	A	R
93	T	Perylene	252	18.458	1.003	A	2	A	B
94	I	Dibenz(a,h)Anthracene-d14 (I...	292	20.795	1.000	A	1	A	B
95	T	Indeno(1,2,3-cd)pyrene	276	20.790	1.000	A	1	A	R
96	T	Dibenz(a,h)anthracene	278	20.865	1.003	A	2	A	R
97	T	Benzo(g,h,i)perylene	276	21.325	1.025	A	2	A	R

Cal A = Average L = Linear LO = Linear w/origin Q = Quad QO = Quad w/origin  
#Qual = number of qualifiers  
A/H = Area or Height  
ID R = R.T. B = R.T. & Q Q = Qvalue L = Largest A = All

SV10\_091919.M Fri Sep 20 12:56:52 2019

Response Factor Report SV-GCMS10

Method Path : C:\msdchem\1\methods\  
 Method File : SV10\_091919.M  
 Title : EPA 8270D: Semivolatile Organics  
 Last Update : Fri Sep 20 10:41:03 2019  
 Response Via : Initial Calibration

*9/23/19*

Calibration Files

20 =J09191918.D 50 =J09191919.D 100 =J09191920.D 200 =J09191921.D 500 =J09191922.D 1000=J09191923.D 2000=J09191924.D  
 4000=J09191925.D 6000=J09191926.D 8000=J09191927.D

Compound	20	50	100	200	500	1000	2000	4000	6000	8000	Avg	%RSD
-----ISTD-----												3.51
1) I 1,4-Dichlorobenzen...												
2) TG N-Nitrosodimet...	0.759	0.758	0.808	0.697	0.702	0.739	0.762	0.786	0.804	0.804	0.762	5.28 J
3) TG Pyridine		1.053	1.277	1.346	1.118	1.285	1.376	1.417	1.443	1.375	1.299	10.27 J
4) S 2-Fluorophenol...	0.940	1.045	0.952	1.217	1.280	1.263	1.333	1.381	1.371	1.354	1.214	14.15 J
5) S Phenol-d6 (Surr)	1.197	1.305	1.446	1.602	1.667	1.682	1.674	1.705	1.659	1.598	1.553	11.41 J
6) T Phenol	1.542	1.562	1.608	1.797	1.827	1.843	1.776	1.794	1.708	1.625	1.708	6.71 J
7) T Aniline		1.505	1.592	1.714	1.671	1.336	1.129	1.375	1.569	1.374	1.474	12.65 J
8) T Bis(2-chloroet...	1.409	1.401	1.477	1.489	1.547	1.678	1.759	1.573			1.542	8.18 J
9) T 2-Chlorophenol	1.231	1.299	1.339	1.474	1.520	1.505	1.485	1.475	1.445	1.389	1.416	6.89 J
10) T 1,3-Dichlorobe...	1.526	1.590	1.641	1.679	1.688	1.625	1.631	1.578	1.503	1.457	1.592	4.80 J
11) T 1,4-Dichlorobe...	1.540	1.656	1.606	1.633	1.652	1.622	1.590	1.515	1.433	1.397	1.564	5.83 J
12) T Benzyl alcohol		0.475	0.613	0.639	0.793	0.881	0.917	0.951	0.916	0.866	0.783	21.39 J
13) T 1,2-Dichlorobe...	1.431	1.680	1.634	1.675	1.672	1.602	1.552	1.481	1.383	1.318	1.543	8.56 J
14) T 2-Methylphenol	0.930	0.880	0.981	1.077	1.155	1.148	1.117	1.057	1.001	0.957	1.030	9.22 J
15) T 2,2'-Oxybis(1-...	1.500	1.454	1.504	1.552	1.511	1.442	1.285	1.209	1.125	1.024	1.360	13.68 J
16) T N-Nitrosodi-n-...	0.922	0.898	0.938	0.991	0.999	0.963	0.901	0.825	0.768	0.745	0.895	9.91 J
17) T 3+4-Methylphenol	1.065	1.133	1.160	1.345	1.441	1.458	1.401	1.305	1.189		1.277	11.32 J
18) T Hexachloroethane	0.434	0.455	0.452	0.472	0.494	0.484	0.503	0.510	0.500	0.503	0.481	5.45 J
19) S Nitrobenzene-d...	0.981	1.085	1.135	1.209	1.313	1.322	1.282	1.286	1.246	1.193	1.205	9.14 J
20) T Nitrobenzene	1.076	1.183	1.189	1.302	1.341	1.327	1.281	1.234	1.165	1.113	1.221	7.44 J
-----ISTD-----												4.83
21) I Naphthalene-d8 (ISTD)												
22) T Isophorone	0.569	0.605	0.640	0.652	0.683	0.661	0.671	0.637	0.632	0.627	0.638	5.17 J
23) T 2-Nitrophenol			0.122	0.135	0.180	0.201	0.189	0.201	0.201	0.195	0.178	17.69 J
24) T 2,4-Dimethylph...		0.198	0.249	0.265	0.283	0.287	0.304	0.287	0.284	0.256	0.268	11.73 J
25) T Bis(2-chloroet...	0.388	0.385	0.394	0.408	0.432	0.413	0.411	0.376	0.348	0.321	0.388	8.46 J
26) T Benzoic acid				0.037	0.087	0.142	0.188	0.195	0.216	0.144		48.51 J
27) T 2,4-Dichloroph...		0.170	0.214	0.252	0.295	0.303	0.320	0.305	0.287	0.272	0.269	18.30 J
28) T 1,2,4-Trichlor...	0.357	0.371	0.359	0.374	0.372	0.362	0.355	0.336	0.317	0.297	0.350	7.29 J
29) T Naphthalene	1.146	1.151	1.167	1.173	1.186	1.117	1.076	0.925	0.826	0.754	1.052	15.05 J
30) T 4-Chloroaniline	0.125	0.244	0.255	0.320	0.351	0.349	0.340	0.277	0.276	0.276	0.281	23.94 J
31) T Hexachlorobuta...	0.184	0.200	0.195	0.200	0.201	0.199	0.191	0.185	0.174	0.163	0.189	6.74 J
32) T 4-Chloro-3-met...			0.197	0.220	0.278	0.284	0.309	0.291	0.278	0.266	0.265	14.24 J
33) T 2-Methylnaphth...	0.706	0.774	0.776	0.819	0.833	0.793	0.783	0.679	0.620	0.570	0.735	12.00 J
34) T 1-Methylnaphth...	0.737	0.770	0.777	0.793	0.804	0.752	0.740	0.635	0.577	0.532	0.712	13.43 J
-----ISTD-----												3.37
35) I Acenaphthene-d10 (...)												
36) T Hexachlorocycl...		0.218	0.261	0.286	0.327	0.342	0.363	0.328	0.338	0.320	0.309	14.82 J
37) T 2,4,6-Trichlor...		0.237	0.257	0.307	0.384	0.402	0.423	0.419	0.401	0.389	0.358	19.99 J
38) T 2,4,5-Trichlor...		0.237	0.270	0.301	0.381	0.390	0.418	0.406	0.393	0.366	0.351	18.51 J
39) T 1,1'-Biphenyl	1.593	1.862	1.891	1.926	1.923	1.827	1.723	1.451	1.275		1.719	13.51 J

Response Factor Report SV-GCMS10

Method Path : C:\msdchem\1\methods\

Method File : SV10\_091919.M

Title : EPA 8270D: Semivolatile Organics

40)	S	2-Fluorobiphen...	1.477	1.610	1.735	1.751	1.740	1.652	1.564	1.351	1.207	✓	1.565	12.07	J
41)	T	2-Chloronaphth...	1.194	1.263	1.356	1.408	1.432	1.325	1.296	1.154	1.045	0.943	1.242	12.73	J
42)	T	2-Nitroaniline	✓	0.177	0.224	0.264	0.357	0.389	0.424	0.415	0.416	0.398	0.340	27.55	J
43)	T	2,6-Dimethylna...	1.108	1.335	1.410	1.426	1.405	1.336	1.263	1.089	0.979	✓	1.261	12.95	J
44)	T	1,4-Dinitroben...	✓		0.065	0.084	0.127	0.151	0.184	0.203	0.205	0.206	0.153	36.62	J
45)	T	Dimethyl phtha...	1.435	1.460	1.596	1.570	1.600	1.540	1.481	1.346	1.249	1.166	1.444	10.30	J
46)	T	1,3-Dinitroben...	✓		0.099	0.125	0.180	0.196	0.220	0.228	0.229	0.221	0.187	26.72	J
47)	T	2,6-Dinitrotol...	✓	0.189	0.212	0.275	0.327	0.334	0.344	0.334	0.324	0.306	0.294	19.32	J
48)	T	1,2-Dinitroben...	✓			0.119	0.146	0.155	0.160	0.159	0.150	0.136	0.146	10.12	J
49)	T	Acenaphthylene	1.944	2.090	2.211	2.226	2.309	2.184	2.067	1.748	1.519	✓	2.033	12.60	J
50)	T	3-Nitroaniline	✓	0.137	0.196	0.256	0.282	0.261	0.196	✓			0.221	24.71	J
51)	T	Acenaphthene	1.387	1.465	1.444	1.458	1.436	1.370	1.314	1.127	1.013	✓	1.335	12.00	J
52)	T	2,4-Dinitrophenol	✓			0.013	0.029	0.062	0.100	0.137	0.153	✓	0.082	69.44	J
53)	T	4-Nitrophenol	✓		0.068	0.095	0.164	0.201	0.242	0.257	0.263	✓	0.184	42.54	J
54)	T	2,4-Dinitrotol...	✓		0.221	0.277	0.369	0.398	0.439	0.437	0.413	0.366	0.365	21.35	J
55)	T	Dibenzofuran	1.822	1.907	2.037	2.018	1.983	1.887	1.852	1.604	1.422	1.264	1.780	14.79	J
56)	T	2,3,5,6-Tetrac...	✓	0.109	0.184	0.216	0.296	0.315	0.344	0.342	0.335	0.322	0.274	30.66	J
57)	T	2,3,4,6-Tetrac...	✓	0.163	0.236	0.262	0.323	0.347	0.364	0.355	0.339	0.326	0.302	22.30	J
58)	T	Diethyl phthalate	1.254	1.388	1.556	1.505	1.488	1.460	1.384	1.206	1.077	0.976	1.330	14.62	J
59)	T	2,3,5-Trimethy...	1.191	1.238	1.255	1.278	1.274	1.217	1.168	1.004	0.895	0.813	1.133	14.83	J
60)	T	Fluorene	1.423	1.444	1.592	1.562	1.562	1.460	1.385	1.151	1.025	✓	1.401	13.79	J
61)	T	4-Chlorophenyl...	0.710	0.743	0.775	0.749	0.750	0.718	0.704	0.618	0.558	0.502	0.683	13.46	J
62)	T	4-Nitroaniline	✓		0.181	0.210	0.234	0.216	0.220	0.221	0.217	0.220	0.215	7.13	J
63)	T	4,6-Dinitro-2-...	✓			0.041	0.091	0.133	0.174	0.203	0.212	0.212	0.152	43.85	J
64)	I	Phenanthrene-d10 (...)	-----ISTD-----											4.15	
65)	T	N-Nitrosodiphe...	0.518	0.605	0.660	0.703	0.703	0.658	0.604	0.483	✓		0.617	13.21	J
66)	T	Azobenzene (1,...	0.596	0.640	0.676	0.698	0.710	0.667	0.627	0.537	0.465	✓	0.624	12.85	J
67)	S	2,4,6-Tribromo...	✓	0.071	0.086	0.099	0.120	0.122	0.130	0.125	0.118	0.112	0.109	18.24	J
68)	T	4-Bromophenyl ...	0.208	0.233	0.237	0.239	0.238	0.236	0.235	0.223	0.211	0.198	0.226	6.56	J
69)	T	Hexachlorobenzene	0.300	0.280	0.292	0.278	0.295	0.286	0.279	0.252	0.231	0.215	0.271	10.61	J
70)	T	Pentachlorophe...	✓		0.078	0.070	0.108	0.122	0.142	0.148	0.145	0.138	0.119	26.11	J
71)	T	Phenanthrene	1.195	1.197	1.225	1.228	1.225	1.146	1.091	0.940	0.851	✓	1.122	12.26	J
72)	T	Anthracene	0.995	1.126	1.166	1.205	1.196	1.143	1.088	0.944	0.844	✓	1.079	11.55	J
73)	T	Carbazole	0.798	0.900	0.979	1.011	1.002	0.861	0.592				0.878	16.89	J
74)	T	Di-n-butyl pht...	✓	1.071	1.257	1.259	1.318	1.283	1.235	1.082	0.958	✓	1.183	10.85	J
75)	T	Fluoranthene	1.065	1.146	1.256	1.262	1.316	1.257	1.229	1.088	0.992	0.891	1.150	12.02	J
76)	T	Benzidine	✓		0.114	0.197	0.271	0.284	0.275	0.307	0.320	0.323	0.261	27.45	J
77)	T	Pyrene	1.099	1.203	1.242	1.308	1.336	1.283	1.225	1.094	0.997	0.915	1.170	11.89	J
78)	I	Chrysene-d12 (ISTD)	-----ISTD-----											4.74	
79)	S	Terphenyl-d14 ...	0.821	0.902	0.977	0.959	0.995	0.969	0.953	0.924	0.880	0.837	0.922	6.53	J
80)	T	Butyl benzyl p...	✓	0.243	0.334	0.380	0.487	0.533	0.570	0.590	0.580	0.569	0.476	26.60	J
81)	T	Bis(2-ethylhex...	✓			0.336	0.441	0.473	0.506	0.520	0.488	0.482	0.464	13.26	J
82)	T	3,3-Dichlorobe...	✓			0.241	0.193	0.167	0.129	0.122	0.119	0.117	0.155	30.50	J
83)	T	Benz(a)anthracene	1.161	1.070	1.154	1.114	1.143	1.102	1.125	1.115	1.107	1.076	1.117	2.72	J
84)	T	Chrysene	0.995	1.051	1.094	1.080	1.094	1.062	1.054	1.041	1.009	0.985	1.046	3.74	J
85)	T	Bis(2-ethylhex...	✓			0.521	0.706	0.743	0.776	0.790	0.763	0.737	0.719	12.78	J
86)	I	Perylene-d12 (ISTD)	-----ISTD-----											4.02	
87)	T	Di-n-octyl pht...	✓		0.597	0.694	0.979	1.136	1.337	1.352	1.295	1.229	1.077	27.27	J



Response Factor Report SV-GCMS10

Method Path : C:\msdchem\1\methods\  
 Method File : SV10\_091919.M  
 Title : EPA 8270D: Semivolatile Organics

88)	T	Benzo(b)fluora...	0.716	0.795	1.016	1.038	1.109	1.109	1.178	1.183	1.177	1.128	1.045	15.65	✓
89)	T	Benzo(k)fluora...	0.705	0.864	1.038	1.065	1.120	1.117	1.168	1.078	0.973	0.854	0.998	14.77	✓
90)	T	Benzo(b+k)fluo...	0.734	0.871	1.068	1.079	1.136	1.134	1.191	1.148	1.113	1.060	1.053	13.45	✓
91)	T	Benzo(e)pyrene	0.747	0.896	1.032	1.039	1.102	1.105	1.133	1.110	1.089	1.027	1.028	11.67	✓
92)	T	Benzo(a)pyrene	0.574	0.677	0.889	0.917	1.028	1.027	1.091	1.049	1.010	0.968	0.923	18.38	✓
93)	T	Perylene	0.801	0.900	0.892	0.920	0.951	0.914	0.954	0.913	0.908	0.867	0.902	4.87	✓
94)	I	Dibenz(a,h)Anthrce...	-----ISTD-----											6.05	
95)	T	Indeno(1,2,3-c...	1.102	1.169	1.176	1.156	1.171	1.152	1.205	1.224	1.230	1.241	1.183	3.60	✓
96)	T	Dibenz(a,h)ant...	0.958	1.019	1.091	1.097	1.135	1.105	1.145	1.152	1.103	1.054	1.086	5.57	✓
97)	T	Benzo(g,h,i)pe...	0.850	0.944	1.107	1.165	1.222	1.214	1.250	1.243	1.204	1.158	1.136	11.87	✓

(#) = Out of Range

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### N-Nitrosodimethylamine

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2214	0.759	3.97
9I19035-CAL2	50	5516	0.758	3.95
9I19035-CAL3	100	11734	0.808	3.95
9I19035-CAL4	200	19941	0.697	3.92
9I19035-CAL5	500	52485	0.702	3.93
9I19035-CAL6	1000	104763	0.739	3.88
9I19035-CAL7	2000	217151	0.762	3.94
9I19035-CAL8	4000	480484	0.786	3.93
9I19035-CAL9	6000	674636	0.804	3.88
9I19035-CALA	8000	866525	0.804	3.96

**AVE RF 0.762      RF RSD 5.28      AVE RT 3.93**

### Pyridine

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2206	0.766	4.06
9I19035-CAL2	50	7667	1.053	4.00
9I19035-CAL3	100	18548	1.277	3.99
9I19035-CAL4	200	38499	1.346	3.95
9I19035-CAL5	500	83583	1.118	3.96
9I19035-CAL6	1000	182180	1.285	3.90
9I19035-CAL7	2000	392152	1.376	3.96
9I19035-CAL8	4000	866960	1.417	3.94
9I19035-CAL9	6000	1210013	1.443	3.89
9I19035-CALA	8000	1480958	1.375	3.96

**AVE RF 1.299      RF RSD 10.27      AVE RT 3.95**

### 2-Fluorophenol (Surr)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2742	0.940	5.32
9I19035-CAL2	50	7611	1.045	5.31
9I19035-CAL3	100	13834	0.952	5.31
9I19035-CAL4	200	34817	1.217	5.30
9I19035-CAL5	500	95687	1.280	5.31
9I19035-CAL6	1000	179108	1.263	5.29
9I19035-CAL7	2000	379802	1.333	5.31
9I19035-CAL8	4000	844515	1.381	5.31
9I19035-CAL9	6000	1150405	1.371	5.30
9I19035-CALA	8000	1458990	1.354	5.32

**AVE RF 1.214      RF RSD 14.15      AVE RT 5.31**

### Phenol-d6 (Surr)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	3493	1.197	6.20
9I19035-CAL2	50	9501	1.305	6.20
9I19035-CAL3	100	21003	1.446	6.20
9I19035-CAL4	200	45844	1.602	6.20
9I19035-CAL5	500	124621	1.667	6.20
9I19035-CAL6	1000	238398	1.682	6.20
9I19035-CAL7	2000	477001	1.674	6.21
9I19035-CAL8	4000	1043086	1.705	6.22
9I19035-CAL9	6000	1391310	1.659	6.22
9I19035-CALA	8000	1721904	1.598	6.23

**AVE RF 1.553      RF RSD 11.41      AVE RT 6.21**

## Element Calibration Review Sheet

Calibration ID: **A912405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A912405**

### Phenol

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4498	1.542	6.22
9I19035-CAL2	50	11373	1.562	6.22
9I19035-CAL3	100	23364	1.608	6.22
9I19035-CAL4	200	51417	1.797	6.22
9I19035-CAL5	500	136576	1.827	6.22
9I19035-CAL6	1000	261231	1.843	6.22
9I19035-CAL7	2000	506313	1.776	6.22
9I19035-CAL8	4000	1097096	1.794	6.23
9I19035-CAL9	6000	1432862	1.708	6.23
9I19035-CALA	8000	1750392	1.625	6.25

**AVE RF 1.708      RF RSD 6.71      AVE RT 6.22**

### Aniline

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2038	0.699	6.26
9I19035-CAL2	50	10955	1.505	6.25
9I19035-CAL3	100	23125	1.592	6.25
9I19035-CAL4	200	49031	1.714	6.25
9I19035-CAL5	500	124901	1.671	6.25
9I19035-CAL6	1000	189393	1.336	6.24
9I19035-CAL7	2000	321662	1.129	6.25
9I19035-CAL8	4000	840844	1.375	6.25
9I19035-CAL9	6000	1316393	1.569	6.25
9I19035-CALA	8000	1480736	1.374	6.26

**AVE RF 1.474      RF RSD 12.65      AVE RT 6.25**

### Bis(2-Chloroethyl) ether

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4110	1.409	6.31
9I19035-CAL2	50	10198	1.401	6.31
9I19035-CAL3	100	21464	1.477	6.31
9I19035-CAL4	200	42595	1.489	6.31
9I19035-CAL5	500	115667	1.547	6.31
9I19035-CAL6	1000	237931	1.678	6.31
9I19035-CAL7	2000	501220	1.759	6.31
9I19035-CAL8	4000	962255	1.573	6.32
9I19035-CAL9	6000	1158478	1.381	6.32
9I19035-CALA	8000	1435010	1.332	6.32

**AVE RF 1.542      RF RSD 8.18      AVE RT 6.31**

### 2-Chlorophenol

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	3591	1.231	6.37
9I19035-CAL2	50	9461	1.299	6.36
9I19035-CAL3	100	19462	1.339	6.37
9I19035-CAL4	200	42160	1.474	6.36
9I19035-CAL5	500	113634	1.520	6.37
9I19035-CAL6	1000	213396	1.505	6.36
9I19035-CAL7	2000	423147	1.485	6.37
9I19035-CAL8	4000	902056	1.475	6.37
9I19035-CAL9	6000	1211719	1.445	6.37
9I19035-CALA	8000	1496104	1.389	6.38

**AVE RF 1.416      RF RSD 6.89      AVE RT 6.37**

## Element Calibration Review Sheet

Calibration ID: **A912405**

Instrument: **SV-GCMS10**


Calibration Date: **09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A912405**

### 1,3-Dichlorobenzene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9119035-CAL1	20	4452	1.526	6.52
9119035-CAL2	50	11576	1.590	6.52
9119035-CAL3	100	23840	1.641	6.52
9119035-CAL4	200	48050	1.679	6.51
9119035-CAL5	500	126152	1.688	6.51
9119035-CAL6	1000	230358	1.625	6.51
9119035-CAL7	2000	464902	1.631	6.52
9119035-CAL8	4000	965051	1.578	6.52
9119035-CAL9	6000	1260484	1.503	6.52
9119035-CALA	8000	1570022	1.457	6.53

**AVE RF 1.592      RF RSD 4.80      AVE RT 6.52**

### 1,4-Dichlorobenzene-d4 (ISTD)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9119035-CAL1	2000	291746	145.873	6.57
9119035-CAL2	2000	291253	145.626	6.57
9119035-CAL3	2000	290594	145.297	6.57
9119035-CAL4	2000	286105	143.053	6.57
9119035-CAL5	2000	299020	149.510	6.57
9119035-CAL6	2000	283511	141.755	6.57
9119035-CAL7	2000	285023	142.511	6.57
9119035-CAL8	2000	305814	152.907	6.57
9119035-CAL9	2000	279602	139.801	6.57
9119035-CALA	2000	269345	134.673	6.58

**AVE RF 144.101      RF RSD 3.51      AVE RT 6.57**

### 1,4-Dichlorobenzene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9119035-CAL1	20	4492	1.540	6.59
9119035-CAL2	50	12059	1.656	6.59
9119035-CAL3	100	23338	1.606	6.59
9119035-CAL4	200	46724	1.633	6.58
9119035-CAL5	500	123497	1.652	6.59
9119035-CAL6	1000	229877	1.622	6.58
9119035-CAL7	2000	453326	1.590	6.59
9119035-CAL8	4000	926647	1.515	6.59
9119035-CAL9	6000	1202300	1.433	6.59
9119035-CALA	8000	1504749	1.397	6.59

**AVE RF 1.564      RF RSD 5.83      AVE RT 6.59**

### Benzyl alcohol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT
9119035-CAL1	20	4506	0.546	6.72
9119035-CAL2	50	3460	0.475	6.71
9119035-CAL3	100	8907	0.613	6.71
9119035-CAL4	200	18281	0.639	6.70
9119035-CAL5	500	59263	0.793	6.70
9119035-CAL6	1000	124850	0.881	6.70
9119035-CAL7	2000	261354	0.917	6.71
9119035-CAL8	4000	581465	0.951	6.71
9119035-CAL9	6000	768204	0.916	6.71
9119035-CALA	8000	932774	0.866	6.72

**AVE RF 0.783      RF RSD 21.39      AVE RT 6.71**

## Element Calibration Review Sheet

Calibration ID: **A912405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A912405**

### 1,2-Dichlorobenzene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4176	1.431	6.74
9I19035-CAL2	50	12229	1.680	6.74
9I19035-CAL3	100	23746	1.634	6.74
9I19035-CAL4	200	47924	1.675	6.74
9I19035-CAL5	500	124976	1.672	6.74
9I19035-CAL6	1000	227139	1.602	6.74
9I19035-CAL7	2000	442316	1.552	6.74
9I19035-CAL8	4000	906070	1.481	6.74
9I19035-CAL9	6000	1159865	1.383	6.74
9I19035-CALA	8000	1419977	1.318	6.74

**AVE RF 1.543      RF RSD 8.56      AVE RT 6.74**

### 2-Methylphenol

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2712	0.930	6.81
9I19035-CAL2	50	6405	0.880	6.81
9I19035-CAL3	100	14254	0.981	6.81
9I19035-CAL4	200	30801	1.077	6.81
9I19035-CAL5	500	86329	1.155	6.81
9I19035-CAL6	1000	162716	1.148	6.81
9I19035-CAL7	2000	318341	1.117	6.81
9I19035-CAL8	4000	646688	1.057	6.81
9I19035-CAL9	6000	839569	1.001	6.82
9I19035-CALA	8000	1030806	0.957	6.82

**AVE RF 1.030      RF RSD 9.22      AVE RT 6.81**

### 2,2'-Oxybis(1-Chloropropane)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4376	1.500	6.84
9I19035-CAL2	50	10585	1.454	6.84
9I19035-CAL3	100	21848	1.504	6.84
9I19035-CAL4	200	44401	1.552	6.84
9I19035-CAL5	500	112933	1.511	6.84
9I19035-CAL6	1000	204366	1.442	6.84
9I19035-CAL7	2000	366117	1.285	6.84
9I19035-CAL8	4000	739481	1.209	6.84
9I19035-CAL9	6000	943818	1.125	6.84
9I19035-CALA	8000	1103589	1.024	6.85

**AVE RF 1.360      RF RSD 13.68      AVE RT 6.84**

### 3+4-Methylphenol(s)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	3108	1.065	6.96
9I19035-CAL2	50	8248	1.133	6.96
9I19035-CAL3	100	16854	1.160	6.96
9I19035-CAL4	200	38484	1.345	6.96
9I19035-CAL5	500	107685	1.441	6.96
9I19035-CAL6	1000	206745	1.458	6.96
9I19035-CAL7	2000	399183	1.401	6.96
9I19035-CAL8	4000	797964	1.305	6.97
9I19035-CAL9	6000	997248	1.189	6.97
9I19035-CALA	8000	1205305	1.119	6.99

**AVE RF 1.277      RF RSD 11.32      AVE RT 6.96**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**


Calibration Date: **09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### N-Nitroso-di-n-propylamine

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2691	0.922	6.96
9I19035-CAL2	50	6538	0.898	6.96
9I19035-CAL3	100	13631	0.938	6.96
9I19035-CAL4	200	28365	0.991	6.96
9I19035-CAL5	500	74700	0.999	6.96
9I19035-CAL6	1000	136460	0.963	6.96
9I19035-CAL7	2000	256713	0.901	6.97
9I19035-CAL8	4000	504346	0.825	6.98
9I19035-CAL9	6000	644101	0.768	6.99
9I19035-CALA	8000	803148	0.745	7.00

**AVE RF 0.895      RF RSD 9.91      AVE RT 6.97**

### Hexachloroethane

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	1267	0.434	7.08
9I19035-CAL2	50	3313	0.455	7.08
9I19035-CAL3	100	6562	0.452	7.08
9I19035-CAL4	200	13490	0.472	7.08
9I19035-CAL5	500	36961	0.494	7.08
9I19035-CAL6	1000	68545	0.484	7.08
9I19035-CAL7	2000	143490	0.503	7.08
9I19035-CAL8	4000	311702	0.510	7.08
9I19035-CAL9	6000	419784	0.500	7.08
9I19035-CALA	8000	541884	0.503	7.08

**AVE RF 0.481      RF RSD 5.45      AVE RT 7.08**

### Nitrobenzene-d5 (Surr)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2861	0.981	7.11
9I19035-CAL2	50	7903	1.085	7.11
9I19035-CAL3	100	16492	1.135	7.11
9I19035-CAL4	200	34591	1.209	7.11
9I19035-CAL5	500	98184	1.313	7.11
9I19035-CAL6	1000	187377	1.322	7.11
9I19035-CAL7	2000	365358	1.282	7.11
9I19035-CAL8	4000	786633	1.286	7.12
9I19035-CAL9	6000	1045001	1.246	7.12
9I19035-CALA	8000	1284804	1.193	7.13

**AVE RF 1.205      RF RSD 9.14      AVE RT 7.12**

### Nitrobenzene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	3138	1.076	7.14
9I19035-CAL2	50	8614	1.183	7.14
9I19035-CAL3	100	17280	1.189	7.14
9I19035-CAL4	200	37240	1.302	7.13
9I19035-CAL5	500	100238	1.341	7.13
9I19035-CAL6	1000	188065	1.327	7.13
9I19035-CAL7	2000	365107	1.281	7.14
9I19035-CAL8	4000	754990	1.234	7.14
9I19035-CAL9	6000	977466	1.165	7.15
9I19035-CALA	8000	1198679	1.113	7.15

**AVE RF 1.221      RF RSD 7.44      AVE RT 7.14**

## Element Calibration Review Sheet

Calibration ID: **A912405**

Instrument: **SV-GCMS10**


Calibration Date: **09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A912405**

### Isophorone

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	6954	0.569	7.37
9I19035-CAL2	50	18082	0.605	7.37
9I19035-CAL3	100	37997	0.640	7.37
9I19035-CAL4	200	78525	0.652	7.37
9I19035-CAL5	500	207804	0.683	7.37
9I19035-CAL6	1000	377941	0.661	7.37
9I19035-CAL7	2000	734609	0.671	7.38
9I19035-CAL8	4000	1524753	0.637	7.38
9I19035-CAL9	6000	2075603	0.632	7.39
9I19035-CALA	8000	2693969	0.627	7.40

**AVE RF 0.638      RF RSD 5.17      AVE RT 7.38**

### 2-Nitrophenol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4053	0.086	7.46
9I19035-CAL2	50	3400	0.114	7.46
9I19035-CAL3	100	7240	0.122	7.45
9I19035-CAL4	200	16298	0.135	7.45
9I19035-CAL5	500	54694	0.180	7.45
9I19035-CAL6	1000	114845	0.201	7.45
9I19035-CAL7	2000	207149	0.189	7.46
9I19035-CAL8	4000	481353	0.201	7.46
9I19035-CAL9	6000	659170	0.201	7.46
9I19035-CALA	8000	838038	0.195	7.46

**AVE RF 0.178      RF RSD 17.69      AVE RT 7.45**

### 2,4-Dimethylphenol

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2375	0.194	7.49
9I19035-CAL2	50	5922	0.198	7.49
9I19035-CAL3	100	14806	0.249	7.49
9I19035-CAL4	200	31880	0.265	7.49
9I19035-CAL5	500	86093	0.283	7.49
9I19035-CAL6	1000	164250	0.287	7.49
9I19035-CAL7	2000	333523	0.304	7.49
9I19035-CAL8	4000	686286	0.287	7.50
9I19035-CAL9	6000	932922	0.284	7.50
9I19035-CALA	8000	1099526	0.256	7.51

**AVE RF 0.268      RF RSD 11.73      AVE RT 7.49**

### Bis(2-Chloroethoxy) methane

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4738	0.388	7.58
9I19035-CAL2	50	11523	0.385	7.58
9I19035-CAL3	100	23395	0.394	7.58
9I19035-CAL4	200	49149	0.408	7.58
9I19035-CAL5	500	131344	0.432	7.58
9I19035-CAL6	1000	236290	0.413	7.58
9I19035-CAL7	2000	449978	0.411	7.58
9I19035-CAL8	4000	900203	0.376	7.59
9I19035-CAL9	6000	1142883	0.348	7.59
9I19035-CALA	8000	1380842	0.321	7.60

**AVE RF 0.388      RF RSD 8.46      AVE RT 7.58**

## Element Calibration Review Sheet

Calibration ID: **A912405**

Instrument: **SV-GCMS10**


Calibration Date: **09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A912405**

### Benzoic acid

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Factor	RT
9119035-CAL1	40	229	9.372	7.55
9119035-CAL2	100	200	3.345	7.57
9119035-CAL3	200	2086	0.018	7.54
9119035-CAL4	400	3335	1.386	7.54
9119035-CAL5	1000	22389	0.037	7.55
9119035-CAL6	2000	99342	8.684	7.58
9119035-CAL7	4000	311714	0.142	7.61
9119035-CAL8	8000	902544	0.188	7.67
9119035-CAL9	12000	1277463	0.195	7.69
9119035-CALA	16000	1853462	0.216	7.73

**AVE RF 0.144      RF RSD 48.51      AVE RT 7.64**

### 2,4-Dichlorophenol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Factor	RT
9119035-CAL1	20	1603	0.131	7.69
9119035-CAL2	50	5068	0.170	7.69
9119035-CAL3	100	12689	0.214	7.69
9119035-CAL4	200	30346	0.252	7.69
9119035-CAL5	500	89833	0.295	7.69
9119035-CAL6	1000	173249	0.303	7.69
9119035-CAL7	2000	350635	0.320	7.69
9119035-CAL8	4000	731346	0.305	7.70
9119035-CAL9	6000	943067	0.287	7.70
9119035-CALA	8000	1167761	0.272	7.71

**AVE RF 0.269      RF RSD 18.30      AVE RT 7.70**

### 1,2,4-Trichlorobenzene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Factor	RT
9119035-CAL1	20	4361	0.357	7.78
9119035-CAL2	50	11103	0.371	7.78
9119035-CAL3	100	21292	0.359	7.78
9119035-CAL4	200	45007	0.374	7.78
9119035-CAL5	500	113367	0.372	7.78
9119035-CAL6	1000	206953	0.362	7.78
9119035-CAL7	2000	388384	0.355	7.78
9119035-CAL8	4000	805154	0.336	7.78
9119035-CAL9	6000	1041502	0.317	7.79
9119035-CALA	8000	1277566	0.297	7.79

**AVE RF 0.350      RF RSD 7.29      AVE RT 7.78**

### Naphthalene-d8 (ISTD)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Factor	RT
9119035-CAL1	2000	1221708	610.854	7.84
9119035-CAL2	2000	1195757	597.878	7.84
9119035-CAL3	2000	1186873	593.437	7.84
9119035-CAL4	2000	1204364	602.182	7.84
9119035-CAL5	2000	1217422	608.711	7.84
9119035-CAL6	2000	1143968	571.984	7.84
9119035-CAL7	2000	1095362	547.681	7.84
9119035-CAL8	2000	1197569	598.784	7.84
9119035-CAL9	2000	1094080	547.040	7.84
9119035-CALA	2000	1074761	537.381	7.85

**AVE RF 581.593      RF RSD 4.83      AVE RT 7.84**



# Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

## Naphthalene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	14004	1.146	7.86
9I19035-CAL2	50	34402	1.151	7.86
9I19035-CAL3	100	69263	1.167	7.86
9I19035-CAL4	200	141239	1.173	7.86
9I19035-CAL5	500	361018	1.186	7.86
9I19035-CAL6	1000	638989	1.117	7.86
9I19035-CAL7	2000	1178988	1.076	7.86
9I19035-CAL8	4000	2214900	0.925	7.86
9I19035-CAL9	6000	2711030	0.826	7.87
9I19035-CALA	8000	3240737	0.754	7.87

**AVE RF 1.052 RF RSD 15.05 AVE RT 7.86**

## 4-Chloroaniline

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	1531	0.125	7.91
9I19035-CAL2	50	7306	0.244	7.91
9I19035-CAL3	100	15139	0.255	7.91
9I19035-CAL4	200	38526	0.320	7.91
9I19035-CAL5	500	106945	0.351	7.91
9I19035-CAL6	1000	199585	0.349	7.91
9I19035-CAL7	2000	372183	0.340	7.92
9I19035-CAL8	4000	663200	0.277	7.93
9I19035-CAL9	6000	906180	0.276	7.93
9I19035-CALA	8000	1186251	0.276	7.93

**AVE RF 0.281 RF RSD 23.94 AVE RT 7.91**

## Hexachlorobutadiene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2247	0.184	7.99
9I19035-CAL2	50	5972	0.200	7.99
9I19035-CAL3	100	11598	0.195	7.99
9I19035-CAL4	200	24136	0.200	7.99
9I19035-CAL5	500	61063	0.201	7.99
9I19035-CAL6	1000	113762	0.199	7.99
9I19035-CAL7	2000	208693	0.191	7.99
9I19035-CAL8	4000	442903	0.185	7.99
9I19035-CAL9	6000	570722	0.174	8.00
9I19035-CALA	8000	701350	0.163	8.00

**AVE RF 0.189 RF RSD 6.74 AVE RT 7.99**

## 4-Chloro-3-methylphenol

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4917	0.157	8.39
9I19035-CAL2	50	5241	0.174	8.39
9I19035-CAL3	100	11698	0.197	8.39
9I19035-CAL4	200	26469	0.220	8.39
9I19035-CAL5	500	84667	0.278	8.39
9I19035-CAL6	1000	162469	0.284	8.39
9I19035-CAL7	2000	338452	0.309	8.39
9I19035-CAL8	4000	698064	0.291	8.39
9I19035-CAL9	6000	912303	0.278	8.40
9I19035-CALA	8000	1141605	0.266	8.40

**AVE RF 0.265 RF RSD 14.24 AVE RT 8.39**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### 2-Methylnaphthalene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	8620	0.706	8.55
9I19035-CAL2	50	23135	0.774	8.56
9I19035-CAL3	100	46039	0.776	8.56
9I19035-CAL4	200	98607	0.819	8.56
9I19035-CAL5	500	253485	0.833	8.56
9I19035-CAL6	1000	453493	0.793	8.56
9I19035-CAL7	2000	857631	0.783	8.56
9I19035-CAL8	4000	1625949	0.679	8.56
9I19035-CAL9	6000	2034929	0.620	8.56
9I19035-CALA	8000	2448839	0.570	8.56

**AVE RF 0.735      RF RSD 12.00      AVE RT 8.56**

### 1-Methylnaphthalene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	9000	0.737	8.65
9I19035-CAL2	50	23006	0.770	8.65
9I19035-CAL3	100	46134	0.777	8.66
9I19035-CAL4	200	95459	0.793	8.65
9I19035-CAL5	500	244797	0.804	8.66
9I19035-CAL6	1000	430139	0.752	8.66
9I19035-CAL7	2000	810434	0.740	8.66
9I19035-CAL8	4000	1521185	0.635	8.66
9I19035-CAL9	6000	1893325	0.577	8.66
9I19035-CALA	8000	2286875	0.532	8.66

**AVE RF 0.712      RF RSD 13.43      AVE RT 8.66**

### Hexachlorocyclopentadiene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4303	0.203	8.72
9I19035-CAL2	50	3356	0.218	8.72
9I19035-CAL3	100	8031	0.261	8.72
9I19035-CAL4	200	17504	0.286	8.73
9I19035-CAL5	500	51180	0.327	8.72
9I19035-CAL6	1000	99801	0.342	8.73
9I19035-CAL7	2000	213088	0.363	8.72
9I19035-CAL8	4000	417829	0.328	8.73
9I19035-CAL9	6000	601203	0.338	8.73
9I19035-CALA	8000	759063	0.320	8.73

**AVE RF 0.309      RF RSD 14.82      AVE RT 8.73**

### 2,4,6-Trichlorophenol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4119	0.175	8.84
9I19035-CAL2	50	3644	0.237	8.84
9I19035-CAL3	100	7912	0.257	8.84
9I19035-CAL4	200	18771	0.307	8.84
9I19035-CAL5	500	59985	0.384	8.84
9I19035-CAL6	1000	117480	0.402	8.84
9I19035-CAL7	2000	248218	0.423	8.84
9I19035-CAL8	4000	532499	0.419	8.85
9I19035-CAL9	6000	713503	0.401	8.85
9I19035-CALA	8000	922776	0.389	8.85

**AVE RF 0.358      RF RSD 19.99      AVE RT 8.84**

# Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

## 2,4,5-Trichlorophenol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4248	0.190	8.87
9I19035-CAL2	50	3657	0.237	8.87
9I19035-CAL3	100	8310	0.270	8.87
9I19035-CAL4	200	18422	0.301	8.87
9I19035-CAL5	500	59608	0.381	8.87
9I19035-CAL6	1000	113799	0.390	8.87
9I19035-CAL7	2000	245074	0.418	8.87
9I19035-CAL8	4000	516958	0.406	8.88
9I19035-CAL9	6000	699105	0.393	8.88
9I19035-CALA	8000	870124	0.366	8.88

**AVE RF 0.351      RF RSD 18.51      AVE RT 8.88**

## 2-Fluorobiphenyl (Surr)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	9460	1.477	8.93
9I19035-CAL2	50	24802	1.610	8.93
9I19035-CAL3	100	53353	1.735	8.93
9I19035-CAL4	200	107137	1.751	8.93
9I19035-CAL5	500	272047	1.740	8.93
9I19035-CAL6	1000	482290	1.652	8.93
9I19035-CAL7	2000	917452	1.564	8.93
9I19035-CAL8	4000	1718307	1.351	8.93
9I19035-CAL9	6000	2148364	1.207	8.93
9I19035-CALA	8000	2595274	1.093	8.94

**AVE RF 1.565      RF RSD 12.07      AVE RT 8.93**

## 1,1'-Biphenyl

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	10205	1.593	9.03
9I19035-CAL2	50	28683	1.862	9.03
9I19035-CAL3	100	58168	1.891	9.03
9I19035-CAL4	200	117826	1.926	9.03
9I19035-CAL5	500	300735	1.923	9.03
9I19035-CAL6	1000	533233	1.827	9.03
9I19035-CAL7	2000	1010736	1.723	9.03
9I19035-CAL8	4000	1845876	1.451	9.03
9I19035-CAL9	6000	2268485	1.275	9.04
9I19035-CALA	8000	2706900	1.140	9.04

**AVE RF 1.719      RF RSD 13.51      AVE RT 9.03**

## 2-Chloronaphthalene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	7646	1.194	9.05
9I19035-CAL2	50	19450	1.263	9.05
9I19035-CAL3	100	41705	1.356	9.05
9I19035-CAL4	200	86117	1.408	9.05
9I19035-CAL5	500	223930	1.432	9.05
9I19035-CAL6	1000	386877	1.325	9.05
9I19035-CAL7	2000	759926	1.296	9.05
9I19035-CAL8	4000	1467799	1.154	9.06
9I19035-CAL9	6000	1860060	1.045	9.06
9I19035-CALA	8000	2240055	0.943	9.06

**AVE RF 1.242      RF RSD 12.73      AVE RT 9.05**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### 2-Nitroaniline

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	939	0.147	9.15
9I19035-CAL2	50	2728	0.177	9.15
9I19035-CAL3	100	6877	0.224	9.15
9I19035-CAL4	200	16161	0.264	9.15
9I19035-CAL5	500	55795	0.357	9.15
9I19035-CAL6	1000	113482	0.389	9.15
9I19035-CAL7	2000	248865	0.424	9.15
9I19035-CAL8	4000	528406	0.415	9.16
9I19035-CAL9	6000	739914	0.416	9.16
9I19035-CALA	8000	944974	0.398	9.17

**AVE RF 0.340      RF RSD 27.55      AVE RT 9.15**

### 2,6-Dimethylnaphthalene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	7097	1.108	9.19
9I19035-CAL2	50	20566	1.335	9.19
9I19035-CAL3	100	43362	1.410	9.19
9I19035-CAL4	200	87215	1.426	9.19
9I19035-CAL5	500	219677	1.405	9.19
9I19035-CAL6	1000	389863	1.336	9.19
9I19035-CAL7	2000	740663	1.263	9.19
9I19035-CAL8	4000	1385514	1.089	9.19
9I19035-CAL9	6000	1742370	0.979	9.20
9I19035-CALA	8000	2089018	0.880	9.20

**AVE RF 1.261      RF RSD 12.95      AVE RT 9.19**

### 1,4-Dinitrobenzene

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	381	5.948	9.27
9I19035-CAL2	50	915	5.939	9.27
9I19035-CAL3	100	2006	0.065	9.27
9I19035-CAL4	200	5164	8.441	9.27
9I19035-CAL5	500	19841	0.127	9.27
9I19035-CAL6	1000	44207	0.151	9.27
9I19035-CAL7	2000	108019	0.184	9.28
9I19035-CAL8	4000	258106	0.203	9.29
9I19035-CAL9	6000	365105	0.205	9.29
9I19035-CALA	8000	488295	0.206	9.30

**AVE RF 0.153      RF RSD 36.62      AVE RT 9.28**

### Dimethylphthalate

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	9190	1.435	9.33
9I19035-CAL2	50	22486	1.460	9.33
9I19035-CAL3	100	49089	1.596	9.33
9I19035-CAL4	200	96043	1.570	9.33
9I19035-CAL5	500	250192	1.600	9.33
9I19035-CAL6	1000	449574	1.540	9.33
9I19035-CAL7	2000	868820	1.481	9.34
9I19035-CAL8	4000	1712764	1.346	9.35
9I19035-CAL9	6000	2223667	1.249	9.35
9I19035-CALA	8000	2768841	1.166	9.36

**AVE RF 1.444      RF RSD 10.30      AVE RT 9.34**

# Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

## 1,3-Dinitrobenzene

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	417	6.510	9.35
9I19035-CAL2	50	1390	9.023	9.35
9I19035-CAL3	100	3033	9.862	9.35
9I19035-CAL4	200	7621	0.125	9.35
9I19035-CAL5	500	28132	0.180	9.35
9I19035-CAL6	1000	57342	0.196	9.35
9I19035-CAL7	2000	128986	0.220	9.36
9I19035-CAL8	4000	289563	0.228	9.37
9I19035-CAL9	6000	407082	0.229	9.38
9I19035-CALA	8000	525829	0.221	9.39

**AVE RF 0.187 RF RSD 26.72 AVE RT 9.36**

## 2,6-Dinitrotoluene

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	1042	0.163	9.39
9I19035-CAL2	50	2915	0.189	9.39
9I19035-CAL3	100	6526	0.212	9.39
9I19035-CAL4	200	16812	0.275	9.39
9I19035-CAL5	500	51160	0.327	9.39
9I19035-CAL6	1000	97373	0.334	9.39
9I19035-CAL7	2000	201552	0.344	9.39
9I19035-CAL8	4000	424265	0.334	9.40
9I19035-CAL9	6000	575872	0.324	9.41
9I19035-CALA	8000	727325	0.306	9.41

**AVE RF 0.294 RF RSD 19.32 AVE RT 9.39**

## 1,2-Dinitrobenzene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	304	4.746	9.44
9I19035-CAL2	50	1349	8.757	9.44
9I19035-CAL3	100	2742	8.915	9.45
9I19035-CAL4	200	7269	0.119	9.44
9I19035-CAL5	500	22807	0.146	9.45
9I19035-CAL6	1000	45222	0.155	9.45
9I19035-CAL7	2000	94079	0.160	9.45
9I19035-CAL8	4000	202294	0.159	9.47
9I19035-CAL9	6000	266233	0.150	9.47
9I19035-CALA	8000	322227	0.136	9.48

**AVE RF 0.146 RF RSD 10.12 AVE RT 9.46**

## Acenaphthylene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	12450	1.944	9.47
9I19035-CAL2	50	32192	2.090	9.47
9I19035-CAL3	100	68008	2.211	9.47
9I19035-CAL4	200	136163	2.226	9.47
9I19035-CAL5	500	361152	2.309	9.47
9I19035-CAL6	1000	637470	2.184	9.47
9I19035-CAL7	2000	1211941	2.067	9.48
9I19035-CAL8	4000	2224222	1.748	9.48
9I19035-CAL9	6000	2704211	1.519	9.48
9I19035-CALA	8000	3146686	1.325	9.49

**AVE RF 2.033 RF RSD 12.60 AVE RT 9.48**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### 3-Nitroaniline

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	592	9.242	9.56
9I19035-CAL2	50	2106	0.137	9.56
9I19035-CAL3	100	6036	0.196	9.56
9I19035-CAL4	200	15637	0.256	9.56
9I19035-CAL5	500	44178	0.282	9.56
9I19035-CAL6	1000	76212	0.261	9.56
9I19035-CAL7	2000	114743	0.196	9.56
9I19035-CAL8	4000	123246	9.686	9.57
9I19035-CAL9	6000	180797	0.102	0.00
9I19035-CALA	8000	174843	7.362	0.00

**AVE RF 0.221      RF RSD 24.71      AVE RT 9.56**

### Acenaphthene-d10 (ISTD)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	2000	640527	320.263	9.62
9I19035-CAL2	2000	616226	308.113	9.62
9I19035-CAL3	2000	615111	307.555	9.62
9I19035-CAL4	2000	611745	305.873	9.62
9I19035-CAL5	2000	625555	312.778	9.62
9I19035-CAL6	2000	583825	291.913	9.62
9I19035-CAL7	2000	586466	293.233	9.62
9I19035-CAL8	2000	636039	318.020	9.62
9I19035-CAL9	2000	593235	296.618	9.62
9I19035-CALA	2000	593771	296.885	9.63

**AVE RF 305.125      RF RSD 3.32      AVE RT 9.62**

### Acenaphthene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	8885	1.387	9.65
9I19035-CAL2	50	22572	1.465	9.65
9I19035-CAL3	100	44425	1.444	9.65
9I19035-CAL4	200	89211	1.458	9.65
9I19035-CAL5	500	224540	1.436	9.65
9I19035-CAL6	1000	399993	1.370	9.65
9I19035-CAL7	2000	770675	1.314	9.65
9I19035-CAL8	4000	1433796	1.127	9.66
9I19035-CAL9	6000	1803278	1.013	9.66
9I19035-CALA	8000	2204696	0.928	9.66

**AVE RF 1.335      RF RSD 12.00      AVE RT 9.65**

### 2,4-Dinitrophenol

Curve Fit: **QUADRATIC: Weighting: (1/a), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	0	0.000	0.00
9I19035-CAL2	50	0	0.000	0.00
9I19035-CAL3	100	169	5.495	9.67
9I19035-CAL4	200	796	1.301	9.67
9I19035-CAL5	500	4568	2.921	9.67
9I19035-CAL6	1000	18042	6.181	9.66
9I19035-CAL7	2000	58400	9.958	9.67
9I19035-CAL8	4000	174238	0.137	9.68
9I19035-CAL9	6000	272053	0.153	9.68
9I19035-CALA	8000	388560	0.164	9.69

**AVE RF 8.224      RF RSD 69.44      AVE RT 9.67**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### 4-Nitrophenol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	420	1.873	9.72
9I19035-CAL2	50	699	4.537	9.72
9I19035-CAL3	100	2106	6.848	9.72
9I19035-CAL4	200	5790	9.465	9.72
9I19035-CAL5	500	25654	0.164	9.72
9I19035-CAL6	1000	58727	0.201	9.72
9I19035-CAL7	2000	141903	0.242	9.73
9I19035-CAL8	4000	326661	0.257	9.74
9I19035-CAL9	6000	467183	0.263	9.75
9I19035-CALA	8000	610739	0.267	9.76

**AVE RF 0.184      RF RSD 42.54      AVE RT 9.73**

### 2,4-Dinitrotoluene

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4027	0.160	9.80
9I19035-CAL2	50	2508	0.163	9.80
9I19035-CAL3	100	6812	0.221	9.80
9I19035-CAL4	200	16915	0.277	9.80
9I19035-CAL5	500	57760	0.369	9.80
9I19035-CAL6	1000	116247	0.398	9.80
9I19035-CAL7	2000	257547	0.439	9.80
9I19035-CAL8	4000	555824	0.437	9.81
9I19035-CAL9	6000	734363	0.413	9.82
9I19035-CALA	8000	868405	0.366	9.83

**AVE RF 0.365      RF RSD 21.35      AVE RT 9.81**

### Dibenzofuran

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	11668	1.822	9.83
9I19035-CAL2	50	29377	1.907	9.83
9I19035-CAL3	100	62656	2.037	9.83
9I19035-CAL4	200	123476	2.018	9.83
9I19035-CAL5	500	310051	1.983	9.83
9I19035-CAL6	1000	550893	1.887	9.83
9I19035-CAL7	2000	1086183	1.852	9.83
9I19035-CAL8	4000	2040744	1.604	9.83
9I19035-CAL9	6000	2531005	1.422	9.84
9I19035-CALA	8000	3003141	1.264	9.84

**AVE RF 1.780      RF RSD 14.79      AVE RT 9.83**

### 2,3,5,6-Tetrachlorophenol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	774	0.121	9.94
9I19035-CAL2	50	1678	0.109	9.91
9I19035-CAL3	100	5673	0.184	9.91
9I19035-CAL4	200	13193	0.216	9.91
9I19035-CAL5	500	46260	0.296	9.91
9I19035-CAL6	1000	91879	0.315	9.91
9I19035-CAL7	2000	201504	0.344	9.91
9I19035-CAL8	4000	434819	0.342	9.91
9I19035-CAL9	6000	597064	0.335	9.92
9I19035-CALA	8000	763806	0.322	9.92

**AVE RF 0.274      RF RSD 30.66      AVE RT 9.91**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### 2,3,4,6-Tetrachlorophenol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	856	0.134	9.95
9I19035-CAL2	50	2513	0.163	9.95
9I19035-CAL3	100	7263	0.236	9.95
9I19035-CAL4	200	16040	0.262	9.95
9I19035-CAL5	500	50476	0.323	9.95
9I19035-CAL6	1000	101167	0.347	9.95
9I19035-CAL7	2000	213539	0.364	9.95
9I19035-CAL8	4000	451267	0.355	9.96
9I19035-CAL9	6000	603345	0.339	9.96
9I19035-CALA	8000	773723	0.326	9.96

**AVE RF 0.302      RF RSD 22.30      AVE RT 9.95**

### 2,3,5-Trimethylnaphthalene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	7629	1.191	10.03
9I19035-CAL2	50	19066	1.238	10.03
9I19035-CAL3	100	38608	1.255	10.03
9I19035-CAL4	200	78195	1.278	10.04
9I19035-CAL5	500	199252	1.274	10.03
9I19035-CAL6	1000	355247	1.217	10.04
9I19035-CAL7	2000	685050	1.168	10.04
9I19035-CAL8	4000	1276533	1.004	10.04
9I19035-CAL9	6000	1592300	0.895	10.05
9I19035-CALA	8000	1931750	0.813	10.05

**AVE RF 1.133      RF RSD 14.83      AVE RT 10.04**

### Diethylphthalate

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	8035	1.254	10.04
9I19035-CAL2	50	21378	1.388	10.04
9I19035-CAL3	100	47870	1.556	10.04
9I19035-CAL4	200	92047	1.505	10.04
9I19035-CAL5	500	232776	1.488	10.04
9I19035-CAL6	1000	426259	1.460	10.05
9I19035-CAL7	2000	811497	1.384	10.06
9I19035-CAL8	4000	1534521	1.206	10.06
9I19035-CAL9	6000	1916805	1.077	10.07
9I19035-CALA	8000	2319061	0.976	10.07

**AVE RF 1.330      RF RSD 14.62      AVE RT 10.05**

### 4-Chlorophenyl phenyl ether

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	4548	0.710	10.17
9I19035-CAL2	50	11449	0.743	10.17
9I19035-CAL3	100	23837	0.775	10.17
9I19035-CAL4	200	45790	0.749	10.17
9I19035-CAL5	500	117369	0.750	10.17
9I19035-CAL6	1000	209713	0.718	10.17
9I19035-CAL7	2000	412942	0.704	10.17
9I19035-CAL8	4000	786385	0.618	10.17
9I19035-CAL9	6000	992417	0.558	10.18
9I19035-CALA	8000	1192807	0.502	10.18

**AVE RF 0.683      RF RSD 13.46      AVE RT 10.17**



## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**


Calibration Date: **09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### Fluorene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	9113	1.423	10.17
9I19035-CAL2	50	22247	1.444	10.17
9I19035-CAL3	100	48968	1.592	10.17
9I19035-CAL4	200	95574	1.562	10.17
9I19035-CAL5	500	244304	1.562	10.17
9I19035-CAL6	1000	426158	1.460	10.17
9I19035-CAL7	2000	812478	1.385	10.18
9I19035-CAL8	4000	1464263	1.151	10.18
9I19035-CAL9	6000	1824399	1.025	10.19
9I19035-CALA	8000	2171368	0.914	10.19

**AVE RF 1.401      RF RSD 13.79      AVE RT 10.18**

### 4-Nitroaniline

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	719	0.112	10.18
9I19035-CAL2	50	2192	0.142	10.18
9I19035-CAL3	100	5563	0.181	10.18
9I19035-CAL4	200	12832	0.210	10.18
9I19035-CAL5	500	36541	0.234	10.18
9I19035-CAL6	1000	63138	0.216	10.18
9I19035-CAL7	2000	129234	0.220	10.19
9I19035-CAL8	4000	281600	0.221	10.20
9I19035-CAL9	6000	385746	0.217	10.21
9I19035-CALA	8000	523369	0.220	10.21

**AVE RF 0.215      RF RSD 7.13      AVE RT 10.19**

### 4,6-Dinitro-2-methylphenol

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	0	0.000	0.00
9I19035-CAL2	50	206	1.337	10.22
9I19035-CAL3	100	761	0.025	10.24
9I19035-CAL4	200	2504	4.093	10.22
9I19035-CAL5	500	14208	9.085	10.22
9I19035-CAL6	1000	38878	0.133	10.22
9I19035-CAL7	2000	101854	0.174	10.22
9I19035-CAL8	4000	258196	0.203	10.23
9I19035-CAL9	6000	377769	0.212	10.24
9I19035-CALA	8000	504056	0.212	10.24

**AVE RF 0.152      RF RSD 43.85      AVE RT 10.23**

### N-Nitrosodiphenylamine

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	5957	0.518	10.29
9I19035-CAL2	50	16461	0.605	10.29
9I19035-CAL3	100	36899	0.660	10.29
9I19035-CAL4	200	77183	0.703	10.29
9I19035-CAL5	500	197334	0.703	10.29
9I19035-CAL6	1000	350586	0.658	10.29
9I19035-CAL7	2000	659355	0.604	10.29
9I19035-CAL8	4000	1182676	0.483	10.30
9I19035-CAL9	6000	1560352	0.455	10.30
9I19035-CALA	8000	1760214	0.377	10.34

**AVE RF 0.617      RF RSD 13.21      AVE RT 10.29**

# Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

## Azobenzene (1,2-DPH)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	6853	0.596	10.33
9I19035-CAL2	50	17404	0.640	10.33
9I19035-CAL3	100	37821	0.676	10.33
9I19035-CAL4	200	76676	0.698	10.33
9I19035-CAL5	500	199437	0.710	10.33
9I19035-CAL6	1000	355316	0.667	10.33
9I19035-CAL7	2000	684303	0.627	10.33
9I19035-CAL8	4000	1316342	0.537	10.34
9I19035-CAL9	6000	1601806	0.465	10.34
9I19035-CALA	8000	1950077	0.418	10.34

**AVE RF 0.624 RF RSD 12.85 AVE RT 10.33**

## 2,4,6-Tribromophenol (Surr)

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	762	6.623	10.41
9I19035-CAL2	50	1929	7.093	10.42
9I19035-CAL3	100	4809	8.598	10.42
9I19035-CAL4	200	10829	9.862	10.42
9I19035-CAL5	500	33701	0.120	10.42
9I19035-CAL6	1000	65055	0.122	10.42
9I19035-CAL7	2000	142266	0.130	10.42
9I19035-CAL8	4000	305471	0.125	10.43
9I19035-CAL9	6000	407389	0.118	10.43
9I19035-CALA	8000	524653	0.112	10.44

**AVE RF 0.109 RF RSD 18.24 AVE RT 10.42**

## 4-Bromophenyl phenyl ether

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2390	0.208	10.67
9I19035-CAL2	50	6326	0.233	10.67
9I19035-CAL3	100	13242	0.237	10.67
9I19035-CAL4	200	26212	0.239	10.67
9I19035-CAL5	500	66857	0.238	10.67
9I19035-CAL6	1000	125621	0.236	10.67
9I19035-CAL7	2000	256334	0.235	10.67
9I19035-CAL8	4000	546207	0.223	10.68
9I19035-CAL9	6000	726568	0.211	10.68
9I19035-CALA	8000	926306	0.198	10.68

**AVE RF 0.226 RF RSD 6.56 AVE RT 10.67**

## Hexachlorobenzene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	3454	0.300	10.75
9I19035-CAL2	50	7615	0.280	10.75
9I19035-CAL3	100	16314	0.292	10.75
9I19035-CAL4	200	30519	0.278	10.75
9I19035-CAL5	500	82813	0.295	10.75
9I19035-CAL6	1000	152211	0.286	10.75
9I19035-CAL7	2000	304969	0.279	10.75
9I19035-CAL8	4000	617226	0.252	10.75
9I19035-CAL9	6000	795928	0.231	10.76
9I19035-CALA	8000	1001688	0.215	10.76

**AVE RF 0.271 RF RSD 10.61 AVE RT 10.75**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### Pentachlorophenol (PCP)

Curve Fit: **QUADRATIC: Weighting: (1/a), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	1000	8.692	10.94
9I19035-CAL2	50	1392	5.118	10.94
9I19035-CAL3	100	4341	7.762	10.94
9I19035-CAL4	200	7638	6.956	10.94
9I19035-CAL5	500	30348	0.108	10.94
9I19035-CAL6	1000	65122	0.122	10.94
9I19035-CAL7	2000	154858	0.142	10.94
9I19035-CAL8	4000	363768	0.148	10.94
9I19035-CAL9	6000	500914	0.145	10.95
9I19035-CALA	8000	646595	0.138	10.95

**AVE RF 0.119      RF RSD 26.11      AVE RT 10.94**

### Phenanthrene-d10 (ISTD)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	2000	1150535	575.268	11.13
9I19035-CAL2	2000	1087898	543.949	11.13
9I19035-CAL3	2000	1118597	559.298	11.13
9I19035-CAL4	2000	1098102	549.051	11.13
9I19035-CAL5	2000	1123094	561.547	11.13
9I19035-CAL6	2000	1065192	532.596	11.14
9I19035-CAL7	2000	1091855	545.928	11.14
9I19035-CAL8	2000	1224924	612.462	11.14
9I19035-CAL9	2000	1148482	574.241	11.14
9I19035-CALA	2000	1167219	583.609	11.14

**AVE RF 563.795      RF RSD 4.15      AVE RT 11.13**

### Phenanthrene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	13749	1.195	11.16
9I19035-CAL2	50	32566	1.197	11.16
9I19035-CAL3	100	68493	1.225	11.15
9I19035-CAL4	200	134878	1.228	11.15
9I19035-CAL5	500	343840	1.225	11.16
9I19035-CAL6	1000	610421	1.146	11.16
9I19035-CAL7	2000	1191270	1.091	11.16
9I19035-CAL8	4000	2302690	0.940	11.16
9I19035-CAL9	6000	2932288	0.851	11.17
9I19035-CALA	8000	3584429	0.768	11.17

**AVE RF 1.122      RF RSD 12.26      AVE RT 11.16**

### Anthracene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	11450	0.995	11.21
9I19035-CAL2	50	30636	1.126	11.21
9I19035-CAL3	100	65192	1.166	11.21
9I19035-CAL4	200	132343	1.205	11.21
9I19035-CAL5	500	335865	1.196	11.21
9I19035-CAL6	1000	608748	1.143	11.21
9I19035-CAL7	2000	1187408	1.088	11.21
9I19035-CAL8	4000	2312152	0.944	11.22
9I19035-CAL9	6000	2907155	0.844	11.22
9I19035-CALA	8000	3477728	0.745	11.22

**AVE RF 1.079      RF RSD 11.55      AVE RT 11.21**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### Carbazole

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	9186	0.798	11.37
9I19035-CAL2	50	24489	0.900	11.37
9I19035-CAL3	100	54742	0.979	11.37
9I19035-CAL4	200	110985	1.011	11.37
9I19035-CAL5	500	281210	1.002	11.37
9I19035-CAL6	1000	458747	0.861	11.37
9I19035-CAL7	2000	646631	0.592	11.37
9I19035-CAL8	4000	858655	0.350	11.37
9I19035-CAL9	6000	1156567	0.336	11.37
9I19035-CALA	8000	1166062	0.250	11.37

**AVE RF 0.878      RF RSD 16.89      AVE RT 11.37**

### Di-n-butylphthalate

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	11697	1.017	11.72
9I19035-CAL2	50	29117	1.071	11.72
9I19035-CAL3	100	70280	1.257	11.72
9I19035-CAL4	200	138215	1.259	11.72
9I19035-CAL5	500	369981	1.318	11.72
9I19035-CAL6	1000	683398	1.283	11.72
9I19035-CAL7	2000	1348435	1.235	11.72
9I19035-CAL8	4000	2651399	1.082	11.72
9I19035-CAL9	6000	3301933	0.958	11.73
9I19035-CALA	8000	4037361	0.865	11.72

**AVE RF 1.183      RF RSD 10.85      AVE RT 11.72**

### Fluoranthene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	12248	1.065	12.43
9I19035-CAL2	50	31166	1.146	12.42
9I19035-CAL3	100	70234	1.256	12.42
9I19035-CAL4	200	138551	1.262	12.42
9I19035-CAL5	500	369455	1.316	12.43
9I19035-CAL6	1000	669325	1.257	12.42
9I19035-CAL7	2000	1341415	1.229	12.43
9I19035-CAL8	4000	2665095	1.088	12.44
9I19035-CAL9	6000	3417993	0.992	12.44
9I19035-CALA	8000	4158773	0.891	12.44

**AVE RF 1.150      RF RSD 12.02      AVE RT 12.43**

### Benzidine

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	40	3398	0.148	12.58
9I19035-CAL2	100	5652	0.104	12.58
9I19035-CAL3	200	12748	0.114	12.58
9I19035-CAL4	400	43242	0.197	12.58
9I19035-CAL5	1000	152022	0.271	12.58
9I19035-CAL6	2000	302104	0.284	12.58
9I19035-CAL7	4000	601547	0.275	12.59
9I19035-CAL8	8000	1506619	0.307	12.60
9I19035-CAL9	12000	2204013	0.320	12.60
9I19035-CALA	16000	3017555	0.323	12.60

**AVE RF 0.261      RF RSD 27.45      AVE RT 12.59**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### Pyrene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	12641	1.099	12.71
9I19035-CAL2	50	32717	1.203	12.71
9I19035-CAL3	100	69474	1.242	12.71
9I19035-CAL4	200	143586	1.308	12.71
9I19035-CAL5	500	375136	1.336	12.71
9I19035-CAL6	1000	683508	1.283	12.71
9I19035-CAL7	2000	1337637	1.225	12.72
9I19035-CAL8	4000	2681088	1.094	12.73
9I19035-CAL9	6000	3436590	0.997	12.74
9I19035-CALA	8000	4271888	0.915	12.73

**AVE RF 1.170      RF RSD 11.89      AVE RT 12.72**

### 3,3'-Dichlorobenzidine

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	40	3617	0.166	0.00
9I19035-CAL2	100	11318	0.203	0.00
9I19035-CAL3	200	24584	0.249	14.85
9I19035-CAL4	400	53778	0.241	14.86
9I19035-CAL5	1000	110907	0.193	14.86
9I19035-CAL6	2000	174855	0.167	14.86
9I19035-CAL7	4000	281736	0.129	14.86
9I19035-CAL8	8000	555604	0.122	14.88
9I19035-CAL9	12000	730056	0.119	14.89
9I19035-CALA	16000	945543	0.117	0.00

**AVE RF 0.155      RF RSD 30.50      AVE RT 12.74**

### p-Terphenyl-d14 (Surr)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	9512	0.821	12.92
9I19035-CAL2	50	25113	0.902	12.92
9I19035-CAL3	100	54871	0.977	12.92
9I19035-CAL4	200	107135	0.959	12.92
9I19035-CAL5	500	285146	0.995	12.92
9I19035-CAL6	1000	507926	0.969	12.92
9I19035-CAL7	2000	1038865	0.953	12.93
9I19035-CAL8	4000	2102593	0.924	12.94
9I19035-CAL9	6000	2699067	0.880	12.94
9I19035-CALA	8000	3392009	0.837	12.93

**AVE RF 0.922      RF RSD 6.53      AVE RT 12.93**

### Butyl benzyl phthalate

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2535	0.249	13.73
9I19035-CAL2	50	6765	0.243	13.74
9I19035-CAL3	100	18774	0.334	13.74
9I19035-CAL4	200	42397	0.380	13.74
9I19035-CAL5	500	139695	0.487	13.74
9I19035-CAL6	1000	279356	0.533	13.74
9I19035-CAL7	2000	621242	0.570	13.74
9I19035-CAL8	4000	1344154	0.590	13.75
9I19035-CAL9	6000	1779167	0.580	13.76
9I19035-CALA	8000	2308181	0.569	13.75

**AVE RF 0.476      RF RSD 26.60      AVE RT 13.74**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### Bis(2-Ethylhexyl) adipate

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2762	0.238	13.91
9I19035-CAL2	50	6924	0.249	13.91
9I19035-CAL3	100	18358	0.327	13.91
9I19035-CAL4	200	37581	0.336	13.91
9I19035-CAL5	500	126449	0.441	13.91
9I19035-CAL6	1000	247877	0.473	13.91
9I19035-CAL7	2000	551677	0.506	13.92
9I19035-CAL8	4000	1183408	0.520	13.92
9I19035-CAL9	6000	1497303	0.488	13.93
9I19035-CALA	8000	1955106	0.482	13.92

**AVE RF 0.464      RF RSD 13.26      AVE RT 13.92**

### Benz(a)anthracene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	13459	1.161	14.89
9I19035-CAL2	50	29779	1.070	14.89
9I19035-CAL3	100	64818	1.154	14.89
9I19035-CAL4	200	124472	1.114	14.89
9I19035-CAL5	500	327557	1.143	14.89
9I19035-CAL6	1000	577553	1.102	14.89
9I19035-CAL7	2000	1225586	1.125	14.90
9I19035-CAL8	4000	2538581	1.115	14.91
9I19035-CAL9	6000	3394067	1.107	14.92
9I19035-CALA	8000	4360504	1.076	14.91

**AVE RF 1.117      RF RSD 2.72      AVE RT 14.90**

### Chrysene-d12 (ISTD)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	2000	1159268	579.634	14.91
9I19035-CAL2	2000	1113286	556.643	14.91
9I19035-CAL3	2000	1122909	561.454	14.91
9I19035-CAL4	2000	1116848	558.424	14.91
9I19035-CAL5	2000	1146727	573.363	14.92
9I19035-CAL6	2000	1048464	524.232	14.92
9I19035-CAL7	2000	1089712	544.856	14.92
9I19035-CAL8	2000	1138264	569.132	14.94
9I19035-CAL9	2000	1022230	511.115	14.94
9I19035-CALA	2000	1013392	506.696	14.93

**AVE RF 548.555      RF RSD 4.74      AVE RT 14.92**

### Chrysene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	11530	0.995	14.97
9I19035-CAL2	50	29254	1.051	14.96
9I19035-CAL3	100	61418	1.094	14.97
9I19035-CAL4	200	120574	1.080	14.97
9I19035-CAL5	500	313539	1.094	14.97
9I19035-CAL6	1000	556735	1.062	14.98
9I19035-CAL7	2000	1148470	1.054	14.98
9I19035-CAL8	4000	2370714	1.041	15.00
9I19035-CAL9	6000	3095456	1.009	15.01
9I19035-CALA	8000	3992263	0.985	15.00

**AVE RF 1.046      RF RSD 3.74      AVE RT 14.98**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**


Calibration Date: **09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### Bis(2-ethylhexyl)phthalate

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	2659	0.229	15.08
9I19035-CAL2	50	8694	0.342	15.07
9I19035-CAL3	100	26668	0.475	15.07
9I19035-CAL4	200	58143	0.521	15.07
9I19035-CAL5	500	202494	0.706	15.08
9I19035-CAL6	1000	389483	0.743	15.07
9I19035-CAL7	2000	846014	0.776	15.08
9I19035-CAL8	4000	1799096	0.790	15.09
9I19035-CAL9	6000	2338505	0.763	15.09
9I19035-CALA	8000	2986931	0.737	15.08

**AVE RF 0.719      RF RSD 12.78      AVE RT 15.08**

### Di-n-octyl phthalate

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	3334	0.288	16.74
9I19035-CAL2	50	9864	0.359	16.74
9I19035-CAL3	100	33665	0.597	16.74
9I19035-CAL4	200	75567	0.694	16.74
9I19035-CAL5	500	281414	0.979	16.75
9I19035-CAL6	1000	592055	1.136	16.75
9I19035-CAL7	2000	1439135	1.337	16.75
9I19035-CAL8	4000	3203842	1.352	16.76
9I19035-CAL9	6000	4149203	1.295	16.77
9I19035-CALA	8000	5450180	1.229	16.75

**AVE RF 1.077      RF RSD 27.27      AVE RT 16.75**

### Benzo(b)fluoranthene

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	8297	0.716	17.46
9I19035-CAL2	50	21819	0.795	17.47
9I19035-CAL3	100	57260	1.016	17.47
9I19035-CAL4	200	113080	1.038	17.48
9I19035-CAL5	500	318669	1.109	17.48
9I19035-CAL6	1000	578435	1.109	17.48
9I19035-CAL7	2000	1267321	1.178	17.49
9I19035-CAL8	4000	2803227	1.183	17.52
9I19035-CAL9	6000	3768759	1.177	17.52
9I19035-CALA	8000	5003892	1.128	17.52

**AVE RF 1.045      RF RSD 15.65      AVE RT 17.49**

### Benzo(b+k)fluoranthene(s)

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	40	17019	0.734	17.46
9I19035-CAL2	100	47809	0.871	17.47
9I19035-CAL3	200	120376	1.068	17.54
9I19035-CAL4	400	234995	1.079	17.48
9I19035-CAL5	1000	653019	1.136	17.54
9I19035-CAL6	2000	1182652	1.134	17.55
9I19035-CAL7	4000	2563432	1.191	17.55
9I19035-CAL8	8000	5439284	1.148	17.59
9I19035-CAL9	12000	7129046	1.113	17.60
9I19035-CALA	16000	9407940	1.060	17.59

**AVE RF 1.053      RF RSD 13.45      AVE RT 17.54**

## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### Benzo(k)fluoranthene

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response	
			Factor	RT
9I19035-CAL1	20	8174	0.705	17.54
9I19035-CAL2	50	23687	0.864	17.54
9I19035-CAL3	100	58523	1.038	17.54
9I19035-CAL4	200	115987	1.065	17.54
9I19035-CAL5	500	321918	1.120	17.54
9I19035-CAL6	1000	582389	1.117	17.55
9I19035-CAL7	2000	1256906	1.168	17.55
9I19035-CAL8	4000	2555733	1.078	17.59
9I19035-CAL9	6000	3115398	0.973	17.60
9I19035-CALA	8000	3789489	0.854	17.59

**AVE RF 0.998      RF RSD 14.77      AVE RT 17.56**

### Benzo(e)pyrene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response	
			Factor	RT
9I19035-CAL1	20	8657	0.747	18.13
9I19035-CAL2	50	24570	0.896	18.12
9I19035-CAL3	100	58165	1.032	18.12
9I19035-CAL4	200	113143	1.039	18.13
9I19035-CAL5	500	316818	1.102	18.13
9I19035-CAL6	1000	576088	1.105	18.14
9I19035-CAL7	2000	1218818	1.133	18.14
9I19035-CAL8	4000	2630004	1.110	18.17
9I19035-CAL9	6000	3489142	1.089	18.19
9I19035-CALA	8000	4556103	1.027	18.17

**AVE RF 1.028      RF RSD 11.67      AVE RT 18.14**

### Benzo(a)pyrene

Curve Fit: **QUADRATIC: Weighting: (1/a^2), Origin: Ignore**




Standard	Concentration	Response	Response	
			Factor	RT
9I19035-CAL1	20	6648	0.574	18.24
9I19035-CAL2	50	18583	0.677	18.24
9I19035-CAL3	100	50114	0.889	18.24
9I19035-CAL4	200	99882	0.917	18.24
9I19035-CAL5	500	295305	1.028	18.25
9I19035-CAL6	1000	535317	1.027	18.25
9I19035-CAL7	2000	1174506	1.091	18.26
9I19035-CAL8	4000	2485829	1.049	18.29
9I19035-CAL9	6000	3235783	1.010	18.31
9I19035-CALA	8000	4292201	0.968	18.30

**AVE RF 0.923      RF RSD 18.38      AVE RT 18.26**

### Perylene-d12 (ISTD)

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response	
			Factor	RT
9I19035-CAL1	2000	1158997	579.498	18.39
9I19035-CAL2	2000	1097209	548.604	18.39
9I19035-CAL3	2000	1127380	563.690	18.39
9I19035-CAL4	2000	1089238	544.619	18.40
9I19035-CAL5	2000	1149483	574.742	18.40
9I19035-CAL6	2000	1042709	521.354	18.40
9I19035-CAL7	2000	1076142	538.071	18.40
9I19035-CAL8	2000	1185024	592.512	18.42
9I19035-CAL9	2000	1067597	533.798	18.43
9I19035-CALA	2000	1108960	554.480	18.41

**AVE RF 555.137      RF RSD 4.02      AVE RT 18.40**



## Element Calibration Review Sheet

Calibration ID: **A9I2405**

Instrument: **SV-GCMS10**


Calibration Date: **09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A9I2405**

### Perylene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	9278	0.801	18.45
9I19035-CAL2	50	24689	0.900	18.45
9I19035-CAL3	100	50289	0.892	18.45
9I19035-CAL4	200	100217	0.920	18.45
9I19035-CAL5	500	273199	0.951	18.45
9I19035-CAL6	1000	476752	0.914	18.46
9I19035-CAL7	2000	1026574	0.954	18.47
9I19035-CAL8	4000	2164033	0.913	18.50
9I19035-CAL9	6000	2908580	0.908	18.51
9I19035-CALA	8000	3844220	0.867	18.50

**AVE RF 0.902      RF RSD 4.87      AVE RT 18.47**

### Indeno(1,2,3-cd)pyrene

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	10072	1.102	20.77
9I19035-CAL2	50	25006	1.169	20.78
9I19035-CAL3	100	52504	1.176	20.78
9I19035-CAL4	200	100411	1.156	20.78
9I19035-CAL5	500	279363	1.171	20.78
9I19035-CAL6	1000	510691	1.152	20.79
9I19035-CAL7	2000	1143875	1.205	20.80
9I19035-CAL8	4000	2539375	1.224	20.84
9I19035-CAL9	6000	3489319	1.230	20.85
9I19035-CALA	8000	4879339	1.241	20.84

**AVE RF 1.183      RF RSD 3.60      AVE RT 20.80**

### Dibenz(a,h)anthracene-d14 (ISTD)

Curve Fit: **AVERAGE RF**




Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	2000	913932	456.966	20.80
9I19035-CAL2	2000	855339	427.669	20.79
9I19035-CAL3	2000	892958	446.479	20.79
9I19035-CAL4	2000	868590	434.295	20.80
9I19035-CAL5	2000	954508	477.254	20.80
9I19035-CAL6	2000	886236	443.118	20.80
9I19035-CAL7	2000	949148	474.574	20.80
9I19035-CAL8	2000	1037191	518.596	20.83
9I19035-CAL9	2000	945822	472.911	20.84
9I19035-CALA	2000	982889	491.444	20.82

**AVE RF 464.331      RF RSD 6.05      AVE RT 20.80**

### Dibenz(a,h)anthracene

Curve Fit: **AVERAGE RF**



Standard	Concentration	Response	Response Factor	RT
9I19035-CAL1	20	8754	0.958	20.85
9I19035-CAL2	50	21791	1.019	20.85
9I19035-CAL3	100	48705	1.091	20.85
9I19035-CAL4	200	95316	1.097	20.85
9I19035-CAL5	500	270778	1.135	20.86
9I19035-CAL6	1000	489557	1.105	20.87
9I19035-CAL7	2000	1087002	1.145	20.88
9I19035-CAL8	4000	2389624	1.152	20.90
9I19035-CAL9	6000	3129173	1.103	20.91
9I19035-CALA	8000	4143300	1.054	20.90

**AVE RF 1.086      RF RSD 5.57      AVE RT 20.87**

# Element Calibration Review Sheet

Calibration ID: **A912405**

Instrument: **SV-GCMS10**

Calibration Date:


**09/24/2019**

Analysis: **8270D LL Full List**

Instrument Cal ID: **A912405**

## Benzo(g,h,i)perylene

Curve Fit: **AVERAGE RF**



<u>Standard</u>	<u>Concentration</u>	<u>Response</u>	<u>Response</u>	<u>Factor</u>	<u>RT</u>
9I19035-CAL1	20	7772		0.850	21.32
9I19035-CAL2	50	20181		0.944	21.31
9I19035-CAL3	100	49447		1.107	21.31
9I19035-CAL4	200	101188		1.165	21.32
9I19035-CAL5	500	291609		1.222	21.33
9I19035-CAL6	1000	538150		1.214	21.33
9I19035-CAL7	2000	1186793		1.250	21.34
9I19035-CAL8	4000	2579448		1.243	21.38
9I19035-CAL9	6000	3417702		1.204	21.39
9I19035-CALA	8000	4554601		1.158	21.38


AVE RF **1.136**

RF RSD **11.87**

AVE RT **21.34**

Benzyl alcohol




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms


(12) Benzyl alcohol (T)

6.766min (+ 0.065) 26.03 ng/ml m

response 193

Ion	Exp%	Act%
108.10	100.00	100.00
79.10	108.60	31.35#
77.00	68.40	50.40
0.00	0.00	0.00

2-Nitrophenol





R = 1.05e-003 A\*A + 1.96e-001 A - 4.15e-003  
Coef of Det (r^2) = 0.997  
Method Name: C:\msdchem\1\methods\SV10\_091919.M  
Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(23) 2-Nitrophenol (T)


7.466min (+ 0.016) 43.56 ng/ml m

response 151

Ion	Exp%	Act%
139.00	100.00	100.00
109.00	25.20	53.85
65.00	38.40	58.82
0.00	0.00	0.00

Benzoic acid




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(26) Benzoic acid (T)

7.552min (-0.026) 807.68 ng/ml m ✓


response 164

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	63.41
77.00	72.00	38.05#
0.00	0.00	0.00



2,4-Dichlorophenol




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms


(27) 2,4-Dichlorophenol (T)

7.723min (+ 0.033) 25.85 ng/ml m

response	177	
Ion	Exp%	Act%
162.00	100.00	100.00
164.00	64.50	62.20
98.00	33.60	0.00#
0.00	0.00	0.00

4-Chloroaniline




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(30) 4-Chloroaniline (T)


7.932min (+ 0.028) 14.02 ng/ml m

response 160

Ion	Exp%	Act%
127.00	100.00	100.00
129.00	33.00	0.00#
65.00	23.50	18.01
0.00	0.00	0.00

2,4,6-Trichlorophenol




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms


(37) 2,4,6-Trichlorophenol (T)

8.830min (-0.010) 24.69 ng/ml m

response	119
Ion	Exp% Act%
195.90	100.00 100.00
197.90	94.40 61.61#
199.90	29.80 21.67
0.00	0.00 0.00

2,4,5-Trichlorophenol


Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



(38) 2,4,5-Trichlorophenol (T)

8.905min (+ 0.033) 23.67 ng/ml m


response 113 ✓

Ion	Exp%	Act%
197.90	100.00	100.00
195.90	103.40	26.40#
199.90	32.90	21.60
0.00	0.00	0.00



2-Nitroaniline

Response Ratio



$R = 1.23e-002 A * A + 3.75e-001 A - 5.72e-003$

Coef of Det (r^2) = 0.9999  
12/28/19 Anchor QEA, LLC Gasco Field DG 2010-4a (2) Waste Characterization Page 681 of 919




Method Name: C:\msdchem\1\methods\SV10\_091919.M

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(42) 2-Nitroaniline (T)


9.151min (+ 0.006) 31.75 ng/ml m

response 155

Ion	Exp%	Act%
138.00	100.00	100.00
65.10	69.90	48.28
92.00	55.20	48.97
0.00	0.00	0.00

1,4-Dinitrobenzene




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms


(44) 1,4-Dinitrobenzene (T)

9.269min (-0.005) 68.86 ng/ml m ✓

response	130
Ion	Exp% Act%
168.00	100.00 100.00
75.00	102.70 80.36
92.10	34.10 55.06
0.00	0.00 0.00

1,3-Dinitrobenzene


Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



(46) 1,3-Dinitrobenzene (T)


9.354min (+ 0.000) 60.01 ng/ml m

response 141

Ion	Exp%	Act%
168.00	100.00	100.00
64.00	23.30	14.38
152.10	9.60	34.76
0.00	0.00	0.00

2,6-Dinitrotoluene




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(47) 2,6-Dinitrotoluene (T)


9.392min (+ 0.001) 26.03 ng/ml m ✓

response 103

Ion	Exp%	Act%
165.00	100.00	100.00
89.00	46.30	43.52
63.00	36.80	34.46
0.00	0.00	0.00



3-Nitroaniline






R = -1.10e-001 A\*A + 3.17e-001 A - 4.68e-003  
Coef of Det (r^2) = 0.996  
12/28/19 Anchor GEA, LEC Gasco Prep DG 2010-48 Waste Characterization Page 689 of 919  
Method Name: C:\msdchem\1\methods\SV10\_091919.M  
Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10




TIC: J09191918.D\data.ms

(50) 3-Nitroaniline (T)

9.552min (-0.010) 30.87 ng/ml m

response	116
Ion	Exp% Act%
138.00	100.00 100.00
92.00	100.10 107.34
108.10	10.00 24.31
0.00	0.00 0.00

2,4-Dinitrophenol






R = 2.65e-002 A\*A + 8.01e-002 A - 9.46e-003  
Coef of Det (r^2) = 0.996  
Method Name: C:\msdchem\1\methods\SV10\_091919.M  
Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 12:58:40 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(52) 2,4-Dinitrophenol (T)


11.157min (+ 1.493) 233.65 ng/ml m

response 166

Ion	Exp%	Act%
184.00	100.00	100.00
91.00	42.80	6.68#
79.00	26.10	17.15
0.00	0.00	0.00

4-Nitrophenol

Response Ratio



$R = 2.73e-002 A^2 + 1.97e-001 A - 7.29e-003$

Coef of Det (r^2) = 0.991 Curve Fit: Quadratic w(1/a^2)




Method Name: C:\msdchem\1\methods\SV10\_091919.M 12/26/19 Anchor DEA, LLC, Gasco Field, DG 2019-4C Waste Characterization Page 693 of 919

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(53) 4-Nitrophenol (T)


9.723min (+ 0.000) 75.63 ng/ml ✓

response 120

Ion	Exp%	Act%
139.00	100.00	100.00
109.00	58.50	72.04
81.10	23.90	27.42
0.00	0.00	0.00

2,4-Dinitrotoluene

Response Ratio



$R = -9.39e-003 A^2 + 4.33e-001 A - 1.16e-002$

Coef of Det (r^2) = 0.995  
12/26/19 Anchor QEA, LLC Gasco Field DG 2019-4C Waste Characterization Page 695 of 919




Method Name: C:\msdchem\1\methods\SV10\_091919.M

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(54) 2,4-Dinitrotoluene (T)

9.809min (+ 0.011) 54.53 ng/ml m


response 109

Ion	Exp%	Act%
165.00	100.00	100.00
89.00	61.80	135.76#
63.00	32.90	55.76
0.00	0.00	0.00



2,3,5,6-Tetrachlorophenol

Response Ratio






R = 6.93e-003 A\*A + 3.13e-001 A - 5.57e-003  
Coef of Det (r^2) = 0.994 Curve Fit: Quadratic w(1/a^2)  
Method Name: C:\msdchem\1\methods\SV10\_091919.M  
12/26/19 Anchor DEA LLC Gasco Field DG 2019-48 Waste Characterization Page 697 of 919  
Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms


(56) 2,3,5,6-Tetrachlorophenol (T)

9.900min (-0.005) 37.40 ng/ml m

response	188	
Ion	Exp%	Act%
231.90	100.00	100.00
233.90	48.30	24.72
130.90	40.60	55.10
0.00	0.00	0.00

2,3,4,6-Tetrachlorophenol




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(57) 2,3,4,6-Tetrachlorophenol (T)


9.959min (+ 0.012) 29.40 ng/ml m

response 112

Ion	Exp%	Act%
231.90	100.00	100.00
130.90	45.50	28.97
229.90	77.80	98.74
0.00	0.00	0.00

4,6-Dinitro-2-methylphenol




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms


(63) 4,6-Dinitro-2-methylphenol (T)

8.894min (-1.321) 161.35 ng/ml m

response	134	
Ion	Exp%	Act%
198.10	100.00	100.00
105.00	40.70	9.00#
77.00	20.00	37.37
0.00	0.00	0.00

2,4,6-Tribromophenol (Surr)

Response Ratio



$R = -1.82e-003 A^2 + 1.24e-001 A - 1.50e-003$

Coef of Det (r^2) = 0.996 Curve Fitting Quadratic (1/a^2)




Method Name: C:\msdchem\1\methods\SV10\_091919.M

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(67) 2,4,6-Tribromophenol (Surr) (S)


10.424min (+ 0.006) 26.15 ng/ml m

response	151	
Ion	Exp%	Act%
329.80	100.00	100.00
331.80	97.00	81.25
140.90	32.90	37.90
0.00	0.00	0.00



Pentachlorophenol (PCP)

Response Ratio



$R = -1.05e-003 A^2 + 1.47e-001 A - 5.64e-003$

Coef of Det (r^2) = 0.998  
Curve Fitting Quadratic w/1/a  
12/20/19 Anchor QEA, LLC - Gasco Field DG 2019-4c Waste Characterization Page 705 of 919




Method Name: C:\msdchem\1\methods\SV10\_091919.M

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(70) Pentachlorophenol (PCP) (T)


10.959min (+ 0.017) 77.97 ng/ml m

response 116 ✓

Ion	Exp%	Act%
265.80	100.00	100.00
263.90	63.30	32.28#
267.80	64.70	0.00#
0.00	0.00	0.00

Carbazole

Response Ratio



$R = -4.70e-001 A^2 + 1.08e+000 A - 3.03e-003$

Coef of Det (r^2) = 0.998  
12/26/19 Anchor QEX, LLC - Gasco Field DG 2019-4c Waste Characterization Page 707 of 919




Method Name: C:\msdchem\1\methods\SV10\_091919.M

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(73) Carbazole (T)


11.392min (+ 0.027) 5.78 ng/ml m

response 115

Ion	Exp%	Act%
167.10	100.00	100.00
139.10	12.90	18.22
166.10	20.90	15.42
0.00	0.00	0.00

Benzidine

Response Ratio



$R = 4.30e-003 A^2 + 2.93e-001 A - 1.80e-002$

Coef of Det ( $r^2$ ) = 0.9999 Curve Fit: Quadratic w/1/a<sup>2</sup>




Method Name: C:\msdchem\1\methods\SV10\_091919.M 12/26/19 Anchor QEA, LLC - Gasco PrefD, DG, 2019-4c. Waste Characterization Page 709 of 919

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(76) Benzidine (T)


12.654min (+ 0.075) 123.93 ng/ml m

response 158

Ion	Exp%	Act%
184.10	100.00	100.00
185.10	15.50	0.00
92.10	9.10	70.99#
0.00	0.00	0.00

Butyl benzyl phthalate

Response Ratio



$R = 2.13e-002 A^2 + 5.16e-001 A - 7.58e-003$

Coef of Det (r^2) = 0.995 Curve Fitting Quadratic (1/a^2)




Method Name: C:\msdchem\1\methods\SV10\_091919.M

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(80) Butyl benzyl phthalate (T)

13.740min (+ 0.006) 29.98 ng/ml m


response 188

Ion	Exp%	Act%
149.00	100.00	100.00
91.10	64.60	66.02
206.10	20.40	16.13
0.00	0.00	0.00



3,3-Dichlorobenzidine




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



(82) 3,3-Dichlorobenzidine (T)


14.853min (-0.010) -1.00 ng/ml m

response 3954

Ion	Exp%	Act%
252.00	100.00	100.00
254.00	66.30	62.09
126.00	12.00	11.91
0.00	0.00	0.00

Di-n-octyl phthalate




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10




TIC: J09191918.D\data.ms

(87) Di-n-octyl phthalate (T)

16.762min (+ 0.016)	58.11 ng/ml m	✓
response	117	
Ion	Exp%	Act%
149.00	100.00	100.00
150.00	9.90	19.81
43.10	5.60	52.08#
0.00	0.00	0.00

Benzo (b) fluoranthene




Response Ratio



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(88) Benzo(b)fluoranthene (T)

17.442min (-0.036) 8.23 ng/ml m




response 176

Ion	Exp%	Act%
252.10	100.00	100.00
126.00	16.50	12.07
253.10	21.90	8.37
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(89) Benzo(k)fluoranthene (T)


17.602min (+ 0.054) 8.71 ng/ml m

response 154

Ion	Exp%	Act%
252.10	100.00	100.00
126.10	16.90	0.00
253.10	22.00	0.00
0.00	0.00	0.00

Benzo (b+k) fluoranthene

Response Ratio








Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(90) Benzo(b+k)fluoranthene (T)


17.666min (+ 0.118) 15.95 ng/ml m

response 140

Ion	Exp%	Act%
252.10	100.00	100.00
126.10	16.90	0.00
253.10	22.00	0.00
0.00	0.00	0.00

Benzo (a) pyrene

Response Ratio



$R = 4.44e-004 A^2 + 1.01e+000 A - 4.97e-003$

Coef of Det ( $r^2$ ) = 0.995 Curve Fit: Quadratic w(1/a^2)




Method Name: C:\msdchem\1\methods\SV10\_091919.M

Calibration Table Last Updated: Fri Sep 20 13:01:57 2019

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\REQUANT\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 13:02:03 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(92) Benzo(a)pyrene (T)

18.324min (+ 0.070) 10.04 ng/ml m ✓

response 116

Ion	Exp%	Act%
252.10	100.00	100.00
113.00	9.90	0.00
253.10	22.50	0.00
0.00	0.00	0.00

# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9I19035

Analysis Included  
8270D LL Full List

## INSTRUMENT SEQUENCE LOG

<u>SampleID</u>	<u>SampleName</u>	<u>Matrix</u>	<u>STDID</u>	<u>ISTD_ID</u>	<u>Analyzed</u>
9I19035-TUN1	MS Tune	Soil	A19I165	A19I086	9/20/2019 12:22:00AM
9I19035-ICB1	Initial Cal Blank	Soil		A19I086	9/20/2019 12:49:00AM
9I19035-CAL1	Cal Standard	Soil	A19G238	"	9/20/2019 1:24:00AM
9I19035-CAL2	Cal Standard	Soil	A19G239	"	9/20/2019 1:59:00AM
9I19035-CAL3	Cal Standard	Soil	A19G240	"	9/20/2019 2:34:00AM
9I19035-CAL4	Cal Standard	Soil	A19G241	"	9/20/2019 3:09:00AM
9I19035-CAL5	Cal Standard	Soil	A19G242	"	9/20/2019 3:44:00AM
9I19035-CAL6	Cal Standard	Soil	A19G243	"	9/20/2019 4:19:00AM
9I19035-CAL7	Cal Standard	Soil	A19G244	"	9/20/2019 4:54:00AM
9I19035-CAL8	Cal Standard	Soil	A19G245	"	9/20/2019 5:29:00AM
9I19035-CAL9	Cal Standard	Soil	A19G246	"	9/20/2019 6:04:00AM
9I19035-CALA	Cal Standard	Soil	A19G247	"	9/20/2019 6:39:00AM
9I19035-ICV1	Initial Cal Check	Soil	A19I254	"	9/20/2019 7:50:00AM

## CALIBRATION STANDARD RECOVERIES

Calibration: **A9I2405**      Instrument: **SV-GCMS10**

8270D LL Full List      Sequence: **9I19035**      Matrix: **Soil**

SampleID	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9I19035-CAL1					
9I19035-CAL2					
9I19035-CAL3					
9I19035-CAL4					
9I19035-CAL5					
9I19035-CAL6					
9I19035-CAL7					
9I19035-CAL8					
9I19035-CAL9					
9I19035-CALA					

Compounds listed above have recalculated recoveries outside 70-130% of the true values, and the calibration levels are above the reporting level. If no compounds are listed, all are OK. Please see the next section for quadratic fit compounds.

# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9I19035

## Analytes With Quadratic Curve Fits

<u>Qualifier</u>	<u>iMDL</u>	<u>iMRL</u>	<u>Spike Amt</u>	<u>%Difference</u>	<u>OK?</u>	<u>Raise MRL to ?</u>
_____				_____	<input type="checkbox"/>	<input type="checkbox"/>

Analytes listed above have quadratic curve fits. If they are using a weighting option, they must be checked against the requested curve points to determine if the recalculated results are within limits (70-130 or as specified).

## ICV RECOVERIES

Calibration: **A9I2405**                      Instrument: **SV-GCMS10**

8270D LL Full List

Sequence: **9I19035**

Matrix: **Soil**

**9I19035-ICV1**

**Inst. MRL**

**ICV Level**

**Result**

**%Rec.**

**Qual**

Compounds listed above have Initial Calibration Verification standard recoveries outside 70-130% of the true values. If no compounds are listed, all have passing recoveries.

# CALIBRATION SEQUENCE REVIEW SHEET

SEQUENCE: 9I19035

## Analysis Included

8270D LL Full List

### INSTRUMENT SEQUENCE LOG

<u>SampleID</u>	<u>SampleName</u>	<u>Matrix</u>	<u>STDID</u>	<u>ISTD_ID</u>	<u>Analyzed</u>
9I19035-TUN1	MS Tune	Water	A19I165	A19I086	9/20/2019 12:22:00AM
9I19035-ICB1	Initial Cal Blank	Water		A19I086	9/20/2019 12:49:00AM
9I19035-CAL1	Cal Standard	Water	A19G238	"	9/20/2019 1:24:00AM
9I19035-CAL2	Cal Standard	Water	A19G239	"	9/20/2019 1:59:00AM
9I19035-CAL3	Cal Standard	Water	A19G240	"	9/20/2019 2:34:00AM
9I19035-CAL4	Cal Standard	Water	A19G241	"	9/20/2019 3:09:00AM
9I19035-CAL5	Cal Standard	Water	A19G242	"	9/20/2019 3:44:00AM
9I19035-CAL6	Cal Standard	Water	A19G243	"	9/20/2019 4:19:00AM
9I19035-CAL7	Cal Standard	Water	A19G244	"	9/20/2019 4:54:00AM
9I19035-CAL8	Cal Standard	Water	A19G245	"	9/20/2019 5:29:00AM
9I19035-CAL9	Cal Standard	Water	A19G246	"	9/20/2019 6:04:00AM
9I19035-CALA	Cal Standard	Water	A19G247	"	9/20/2019 6:39:00AM
9I19035-ICV1	Initial Cal Check	Water	A19I254	"	9/20/2019 7:50:00AM

### CALIBRATION STANDARD RECOVERIES

Calibration: A9I2405

Instrument: SV-GCMS10

8270D LL Full List

Sequence: 9I19035

Matrix: Water

	Inst. MRL	Recalc Res.	Cal Level	%Rec.	Qual
9I19035-CAL1					
9I19035-CAL2					
9I19035-CAL3					
9I19035-CAL4					
9I19035-CAL5					
9I19035-CAL6					
9I19035-CAL7					
9I19035-CAL8					
9I19035-CAL9					
9I19035-CALA					

Compounds listed above have recalculated recoveries outside 70-130% of the true values, and the calibration levels are above the reporting level. If no compounds are listed, all are OK. Please see the next section for quadratic fit compounds.

**CALIBRATION SEQUENCE REVIEW SHEET**

**SEQUENCE: 9I19035**

**Analytes With Quadratic Curve Fits**

Qualifier   iMDL   iMRL   Spike Amt   %Difference   OK?   Raise MRL to ?  
\_\_\_\_\_         \_\_\_\_\_

Analytes listed above have quadratic curve fits. If they are using a weighting option, they must be checked against the requested curve points to determine if the recalculated results are within limits (70-130 or as specified).

**ICV RECOVERIES**

Calibration: **A9I2405**   Instrument: **SV-GCMS10**

**8270D LL Full List**

Sequence: **9I19035**

Matrix: **Water**

**9I19035-ICV1**

**Inst. MRL**

**ICV Level**

**Result**

**%Rec.**

**Qual**

Compounds listed above have Initial Calibration Verification standard recoveries outside 70-130% of the true values. If no compounds are listed, all have passing recoveries.

Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 14:32:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*Handwritten signature and date: JJA 9/23/19*

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 30% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev (min)
1 I 1,4-Dichlorobenzene-d4 (ISTD)	2000.000	2000.000	0.0	106	0.00
2 TG N-Nitrosodimethylamine	1000.000	1045.350	-4.5	114	0.09
3 TG Pyridine	1000.000	896.190	10.4	96	0.10
4 S 2-Fluorophenol (Surr)	1000.000	981.272	1.9	100	0.03
5 S Phenol-d6 (Surr)	1000.000	1015.692	-1.6	99	0.00
6 T Phenol	1000.000	989.661	1.0	97	0.01
7 T Aniline	1000.000	836.204	16.4	97	0.02
8 T Bis(2-chloroethyl) ether	1000.000	1091.651	-9.2	106	0.00
9 T 2-Chlorophenol	1000.000	1008.898	-0.9	100	0.00
10 T 1,3-Dichlorobenzene	1000.000	1009.723	-1.0	105	0.00
11 T 1,4-Dichlorobenzene	1000.000	1002.987	-0.3	102	0.00
12 T Benzyl alcohol	1000.000	910.785	8.9	91	0.00
13 T 1,2-Dichlorobenzene	1000.000	1024.110	-2.4	104	0.00
14 T 2-Methylphenol	1000.000	1052.523	-5.3	100	0.00
15 T 2,2'-Oxybis(1-Chloropropane	1000.000	970.278	3.0	97	0.00
16 T N-Nitrosodi-n-propylamine	1000.000	1043.262	-4.3	102	0.00
17 T 3+4-Methylphenol	1000.000	1067.423	-6.7	99	0.00
18 T Hexachloroethane	1000.000	1040.964	-4.1	109	0.00
19 S Nitrobenzene-d5 (Surr)	1000.000	1065.680	-6.6	103	0.00
20 T Nitrobenzene	1000.000	1058.009	-5.8	103	0.00
21 I Naphthalene-d8 (ISTD)	2000.000	2000.000	0.0	102	0.00
22 T Isophorone	1000.000	1048.414	-4.8	103	0.00
23 T 2-Nitrophenol	1000.000	968.550	3.1	93	0.00
24 T 2,4-Dimethylphenol	1000.000	967.663	3.2	92	0.00
25 T Bis(2-chloroethoxy) methane	1000.000	1057.133	-5.7	101	0.00
26 T Benzoic acid	2000.000	1974.824	1.3	115	0.00
27 T 2,4-Dichlorophenol	1000.000	968.833	3.1	98	0.00
28 T 1,2,4-Trichlorobenzene	1000.000	999.393	0.1	99	0.00
29 T Naphthalene	1000.000	1048.170	-4.8	101	0.00
30 T 4-Chloroaniline	1000.000	939.273	6.1	90	0.00
31 T Hexachlorobutadiene	1000.000	1037.179	-3.7	101	0.00
32 T 4-Chloro-3-methylphenol	1000.000	1056.418	-5.6	101	0.00
33 T 2-Methylnaphthalene	1000.000	1097.134	-9.7	104	0.00
34 T 1-Methylnaphthalene	1000.000	1073.196	-7.3	104	0.00
35 I Acenaphthene-d10 (ISTD)	2000.000	2000.000	0.0	105	0.00
36 T Hexachlorocyclopentadiene	1000.000	1072.195	-7.2	102	0.00
37 T 2,4,6-Trichlorophenol	1000.000	1033.651	-3.4	105	0.00
38 T 2,4,5-Trichlorophenol	1000.000	1048.469	-4.8	108	0.00
39 T 1,1'-Biphenyl	1000.000	1032.434	-3.2	102	0.00
40 S 2-Fluorobiphenyl (Surr)	1000.000	1062.096	-6.2	106	0.00
41 T 2-Chloronaphthalene	1000.000	1056.535	-5.7	104	0.00
42 T 2-Nitroaniline	1000.000	1106.583	-10.7	111	0.00
43 T 2,6-Dimethylnaphthalene	1000.000	1034.190	-3.4	103	0.00
44 T 1,4-Dinitrobenzene	1000.000	1114.508	-11.5	121	0.00
45 T Dimethyl phthalate	1000.000	1061.398	-6.1	105	0.00
46 T 1,3-Dinitrobenzene	1000.000	1081.705	-8.2	115	0.00
47 T 2,6-Dinitrotoluene	1000.000	1043.999	-4.4	107	0.00
48 T 1,2-Dinitrobenzene	1000.000	1063.484	-6.3	106	0.00



Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 14:32:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 30% Max. Rel. Area : 200%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T Acenaphthylene	1000.000	1059.382	-5.9	104	0.00
50 T 3-Nitroaniline	1000.000	1060.772	-6.1	107	0.00
51 T Acenaphthene	1000.000	1001.616	-0.2	103	0.00
52 T 2,4-Dinitrophenol	1000.000	972.001	2.8	122	0.00
53 T 4-Nitrophenol	1000.000	1106.887	-10.7	115	0.00
54 T 2,4-Dinitrotoluene	1000.000	1048.405	-4.8	113	0.00
55 T Dibenzofuran	1000.000	1071.222	-7.1	106	0.00
56 T 2,3,5,6-Tetrachlorophenol	1000.000	1077.305	-7.7	111	0.00
57 T 2,3,4,6-Tetrachlorophenol	1000.000	1013.999	-1.4	103	0.00
58 T Diethyl phthalate	1000.000	1087.436	-8.7	104	0.00
59 T 2,3,5-Trimethylnaphthalene	1000.000	1037.334	-3.7	102	0.00
60 T Fluorene	1000.000	1045.897	-4.6	106	0.00
61 T 4-Chlorophenyl phenyl ether	1000.000	1051.565	-5.2	105	0.00
62 T 4-Nitroaniline	1000.000	1080.738	-8.1	113	0.00
63 T 4,6-Dinitro-2-methylphenol	1000.000	1157.716	-15.8	133	0.00
64 I Phenanthrene-d10 (ISTD)	2000.000	2000.000	0.0	108	0.00
65 T N-Nitrosodiphenylamine	1000.000	1064.375	-6.4	108	0.00
66 T Azobenzene (1,2-DPH)	1000.000	1037.259	-3.7	105	0.00
67 S 2,4,6-Tribromophenol (Surr)	1000.000	1040.672	-4.1	111	0.00
68 T 4-Bromophenyl phenyl ether	1000.000	1032.582	-3.3	107	0.00
69 T Hexachlorobenzene	1000.000	1010.042	-1.0	104	0.00
70 T Pentachlorophenol (PCP)	1000.000	975.756	2.4	117	0.00
71 T Phenanthrene	1000.000	1015.497	-1.5	108	0.00
72 T Anthracene	1000.000	1058.253	-5.8	108	0.00
73 T Carbazole	1000.000	964.910	3.5	103	0.00
74 T Di-n-butyl phthalate	1000.000	1057.534	-5.8	106	0.00
75 T Fluoranthene	1000.000	1088.446	-8.8	108	0.00
76 T Benzidine	2000.000	1842.776	7.9	97	0.00
77 T Pyrene	1000.000	1070.616	-7.1	106	0.00
78 I Chrysene-d12 (ISTD)	2000.000	2000.000	0.0	109	-0.01
79 S Terphenyl-d14 (Surr)	1000.000	1060.782	-6.1	110	0.00
80 T Butyl benzyl phthalate	1000.000	1003.995	-0.4	105	0.00
81 T Bis(2-ethylhexyl) adipate	1000.000	1058.578	-5.9	113	-0.01
82 T 3,3-Dichlorobenzidine	2000.000	2062.773	-3.1	106	-0.01
83 T Benz(a)anthracene	1000.000	1029.118	-2.9	114	-0.01
84 T Chrysene	1000.000	1009.528	-1.0	108	-0.01
85 T Bis(2-ethylhexyl) phthalate	1000.000	1039.182	-3.9	110	0.00
86 I Perylene-d12 (ISTD)	2000.000	2000.000	0.0	111	-0.01
87 T Di-n-octyl phthalate	1000.000	1013.796	-1.4	114	-0.02
88 T Benzo(b)fluoranthene	1000.000	1008.508	-0.9	112	-0.02
89 T Benzo(k)fluoranthene	1000.000	992.118	0.8	110	-0.02
90 T Benzo(b+k)fluoranthene	2000.000	1987.636	0.6	111	-0.02
91 T Benzo(e)pyrene	1000.000	1042.799	-4.3	108	-0.02
92 T Benzo(a)pyrene	1000.000	971.420	2.9	105	-0.02
93 T Perylene	1000.000	1215.264	-21.5	134	-0.02
94 I Dibenz(a,h)Anthrcene-d14 (I	2000.000	2000.000	0.0	113	-0.02

Evaluate Continuing Calibration Report

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 14:32:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 30% Max. Rel. Area : 200%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
95 T	Indeno(1,2,3-cd)pyrene	1000.000	973.509	2.6	113	-0.02
96 T	Dibenz(a,h)anthracene	1000.000	1019.307	-1.9	113	-0.02
97 T	Benzo(g,h,i)perylene	1000.000	1054.879	-5.5	111	-0.02

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191916.D  
 Acq On : 20 Sep 2019 12:22 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-TUN1  
 Misc : 1x, A19I165 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Sep 20 09:40:00 2019  
 Quant Method : C:\msdchem\1\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Thu Sep 19 15:09:10 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*JK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	6.600	150	134967	2.00	ug/mL	0.00
2) Naphthalene-d8	7.867	136	357596	2.00	ug/mL	0.00
3) Acenaphthene-d10	9.648	162	174398	2.00	ug/mL	0.00
5) Phenanthrene-d10	11.162	188	269663	2.00	ug/mL	0.00
11) Chrysene-d12	14.885	240	230198	2.00	ug/mL	0.00
12) Perylene-d12	17.126	264	213465	2.00	ug/mL	#-0.03
<b>Target Compounds</b>						
4) Pentachlorophenol	10.975	266	684363	41.56	ug/mL	84
6) DFTPP	11.456	442	746382	34.29	ug/mL	85
7) Benzidine	12.628	184	2478643	25.84	ug/mL	98
8) 4,4-DDE	12.890	TIC	40067	No Calib		
9) 4,4-DDD	13.403	TIC	23267	No Calib		
10) 4,4-DDT	13.975	TIC	9144669	33.07	ug/mL	95



(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191916.D  
 Acq On : 20 Sep 2019 12:22 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-TUN1  
 Misc : 1x, A19I165 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : C:\msdchem\1\methods\DFTPP.M  
 Title : 8270 DFTPP Tune Method  
 Last Update : Thu Sep 19 15:09:10 2019

*Handwritten signature*






AutoFind: Scans 1488, 1489, 1490; Background Corrected with Scan 1483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	1920	PASS
69	198	0.01	100	21.3	118967	PASS
70	69	0.00	2	0.5	611	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	557760	PASS
199	198	5	9	6.9	38464	PASS
365	198	1	100	3.2	17707	PASS
441	443	0.01	150	73.9	77592	PASS
442	198	0.10	200	95.5	532779	PASS
443	442	15	24	19.7	104995	PASS

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191916.D  
 Acq On : 20 Sep 2019 12:22 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-TUN1  
 Misc : 1x, A19I165 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Sep 20 09:40:00 2019  
 Quant Method : C:\msdchem\1\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Thu Sep 19 15:09:10 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



(4) Pentachlorophenol

10.975min (+ 0.005) 41.56 ug/mL




Ion	Exp%	Act%
265.90	100.00	100.00
164.90	50.60	38.07
201.90	25.80	22.85
129.90	27.30	16.90

*Handwritten signature and date: 9/20/19*

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191916.D  
 Acq On : 20 Sep 2019 12:22 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-TUN1  
 Misc : 1x, A19I165 DFTPP@45  
 ALS Vial : 1 Sample Multiplier: 1  
 DataAcq Meth:DFTPP.M

Quant Time: Sep 20 09:40:00 2019  
 Quant Method : C:\msdchem\1\methods\DFTPP.M  
 Quant Title : 8270 DFTPP Tune Method  
 QLast Update : Thu Sep 19 15:09:10 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191916.D\data.ms

(7) Benzidine

12.628min (+ 0.005) 25.84 ug/mL

response 2478643

Ion	Exp%	Act%
184.10	100.00	100.00
156.10	8.50	7.27
92.10	8.20	8.38
0.00	0.00	0.00

*JK 9/20/19*

## DDT Breakdown Check (Validated 5/1/2013)

From:  
9119035-TUN1  
SV-GCMS10


First Column Area Counts	Percent Breakdown
DDE 40067	
DDD 23267	
DDT 9144669	0.69 PASS

Breakdown must be less than 20% to accept sample data.

*gd 9/20/19*

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
Data File : J09191916.D  
Acq On : 20 Sep 2019 12:22 am  
Operator : JK/ AMS/ DTH  
Sample : 9I19035-TUN1  
Misc : 1x, A19I165 DFTPP@45  
ALS Vial : 1 Sample Multiplier: 1  
DataAcq Meth:DFTPP.M

Quant Time: Sep 20 09:40:00 2019  
Quant Method : C:\msdchem\1\methods\DFTPP.M  
Quant Title : 8270 DFTPP Tune Method  
QLast Update : Thu Sep 19 15:09:10 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10





Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191917.D  
 Acq On : 20 Sep 2019 12:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:06 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*Handwritten:* 9/20/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.568	152	263426	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.835	136	1245077	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.616	162	634026	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.130	188	1140103	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.912	240	1131801	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	18.399	264	1099318	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.790	292	879454	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.402	112	67	0.37	ng/ml	0.11	
5) Phenol-d6(Surr)	0.000	99	0	0.00	ng/ml		
19) Nitrobenzene-d5 (Surr)	7.129	82	88	0.42	ng/ml	0.02	
40) 2-Fluorobiphenyl (Surr)	0.000	172	0	0.00	ng/ml		
67) 2,4,6-Tribromophenol (...)	0.000	330	0	0.00	ng/ml		
79) Terphenyl-d14 (Surr)	0.000	244	0	0.00	ng/ml		
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	0.000		0	N.D.			Qvalue
3) Pyridine	3.947	79	261	N.D.			
6) Phenol	6.215	94	79	N.D.			
7) Aniline	6.284	93	59	N.D.			
8) Bis(2-chloroethyl) ether	6.306	93	72	N.D.			
9) 2-Chlorophenol	0.000		0	N.D.			
10) 1,3-Dichlorobenzene	0.000		0	N.D.			
11) 1,4-Dichlorobenzene	0.000		0	N.D.			
12) Benzyl alcohol	6.744	108	78	N.D.			
13) 1,2-Dichlorobenzene	0.000		0	N.D.			
14) 2-Methylphenol	6.819	107	109	N.D.			
15) 2,2'-Oxybis(1-Chloropr...	6.814	45	64	N.D.			
16) N-Nitrosodi-n-propylamine	7.028	70	172	N.D.			
17) 3+4-Methylphenol	0.000		0	N.D.			
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	7.086	77	108	N.D.			
22) Isophorone	7.370	82	96	N.D.			
23) 2-Nitrophenol	0.000		0	N.D.			
24) 2,4-Dimethylphenol	0.000		0	N.D.			
25) Bis(2-chloroethoxy) me...	0.000		0	N.D.			
26) Benzoic acid	7.563	105	152	305.02	ng/ml#	28	
27) 2,4-Dichlorophenol	0.000		0	N.D.			
28) 1,2,4-Trichlorobenzene	0.000		0	N.D.			
29) Naphthalene	0.000		0	N.D.			
30) 4-Chloroaniline	0.000		0	N.D.			
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	8.392	107	91	N.D.			
33) 2-Methylnaphthalene	8.557	142	100	N.D.			
34) 1-Methylnaphthalene	8.659	142	61	N.D.			
36) Hexachlorocyclopentadiene	0.000		0	N.D.			
37) 2,4,6-Trichlorophenol	0.000		0	N.D.			
38) 2,4,5-Trichlorophenol	0.000		0	N.D.			
39) 1,1'-Biphenyl	0.000		0	N.D.			
41) 2-Chloronaphthalene	0.000		0	N.D.			
42) 2-Nitroaniline	0.000		0	N.D.			
43) 2,6-Dimethylnaphthalene	0.000		0	N.D.			

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191917.D  
 Acq On : 20 Sep 2019 12:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Sep 20 09:46:06 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	0.000		0	N.D.		
45) Dimethyl phthalate	9.344	163	194	N.D.		
46) 1,3-Dinitrobenzene	0.000		0	N.D.		
47) 2,6-Dinitrotoluene	0.000		0	N.D.		
48) 1,2-Dinitrobenzene	0.000		0	N.D.		
49) Acenaphthylene	9.483	152	84	N.D.		
50) 3-Nitroaniline	0.000		0	N.D.		
51) Acenaphthene	9.648	153	78	N.D.		
52) 2,4-Dinitrophenol	0.000		0	N.D.		
53) 4-Nitrophenol	0.000		0	N.D.		
54) 2,4-Dinitrotoluene	9.777	165	228	N.D.		
55) Dibenzofuran	0.000		0	N.D.		
56) 2,3,5,6-Tetrachlorophenol	0.000		0	N.D.		
57) 2,3,4,6-Tetrachlorophenol	0.000		0	N.D.		
58) Diethyl phthalate	10.039	149	103	N.D.		
59) 2,3,5-Trimethylnaphtha...	10.146	170	164	N.D.		
60) Fluorene	0.000		0	N.D.		
61) 4-Chlorophenyl phenyl ...	0.000		0	N.D.		
62) 4-Nitroaniline	0.000		0	N.D.		
63) 4,6-Dinitro-2-methylph...	0.000		0	N.D.		
65) N-Nitrosodiphenylamine	0.000		0	N.D.		
66) Azobenzene (1,2-DPH)	10.338	77	165	N.D.		
68) 4-Bromophenyl phenyl e...	0.000		0	N.D.		
69) Hexachlorobenzene	0.000		0	N.D.		
70) Pentachlorophenol (PCP)	10.938	266	325	35.51	ng/ml	76
71) Phenanthrene	11.135	178	418	N.D.		
72) Anthracene	11.135	178	418	N.D.		
73) Carbazole	11.381	167	91	N.D.		
74) Di-n-butyl phthalate	11.718	149	81	N.D.		
75) Fluoranthene	12.414	202	105	N.D.		
76) Benzidine	12.580	184	2179	68.20	ng/ml	91
77) Pyrene	12.724	202	64	N.D.		
80) Butyl benzyl phthalate	0.000		0	N.D.		
81) Bis(2-ethylhexyl) adipate	13.906	129	791	N.D.		
82) 3,3-Dichlorobenzidine	14.863	252	271	Below Cal	#	25
83) Benz(a)anthracene	14.912	228	2854	4.30	ng/ml	67
84) Chrysene	14.912	228	2826	4.52	ng/ml	66
85) Bis(2-ethylhexyl) phth...	15.067	149	83	N.D.		
87) Di-n-octyl phthalate	16.735	149	81	30.90	ng/ml#	1
88) Benzo(b)fluoranthene	17.468	252	54	N.D.		
89) Benzo(k)fluoranthene	17.538	252	89	N.D.		
90) Benzo(b+k)fluoranthene	17.538	252	89	N.D.		
91) Benzo(e)pyrene	0.000		0	N.D.		
92) Benzo(a)pyrene	0.000		0	N.D.		
93) Perylene	18.399	252	3568	6.28	ng/ml	70
95) Indeno(1,2,3-cd)pyrene	20.790	276	464	N.D.		
96) Dibenz(a,h)anthracene	20.790	278	242	N.D.		
97) Benzo(g,h,i)perylene	0.000		0	N.D.		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191917.D  
 Acq On : 20 Sep 2019 12:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:06 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191917.D  
 Acq On : 20 Sep 2019 12:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

*Final Request*

*Ad 9/23/19*

Quant Time: Sep 20 14:22:39 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.568	152	263426	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.835	136	1245077	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.616	162	634026	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.130	188	1140103	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.912	240	1131801	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	18.399	264	1099318	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.790	292	879454	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.402	112	67	0.42	ng/ml	0.11	
5) Phenol-d6 (Surr)	0.000	99	0	0.00	ng/ml		
19) Nitrobenzene-d5 (Surr)	7.129	82	88	0.55	ng/ml	0.02	
40) 2-Fluorobiphenyl (Surr)	0.000	172	0	0.00	ng/ml		
67) 2,4,6-Tribromophenol (...)	0.000	330	0	0.00	ng/ml		
79) Terphenyl-d14 (Surr)	0.000	244	0	0.00	ng/ml		
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	0.000		0	N.D.			Qvalue
3) Pyridine	3.947	79	261	N.D.			
6) Phenol	6.215	94	79	N.D.			
7) Aniline	6.284	93	59	N.D.			
8) Bis(2-chloroethyl) ether	6.306	93	72	N.D.			
9) 2-Chlorophenol	0.000		0	N.D.			
10) 1,3-Dichlorobenzene	0.000		0	N.D.			
11) 1,4-Dichlorobenzene	0.000		0	N.D.			
12) Benzyl alcohol	6.744	108	78	25.17	ng/ml#	41	
13) 1,2-Dichlorobenzene	0.000		0	N.D.			
14) 2-Methylphenol	6.819	107	109	N.D.			
15) 2,2'-Oxybis(1-Chloropr...	6.814	45	64	N.D.			
16) N-Nitrosodi-n-propylamine	7.028	70	172	N.D.			
17) 3+4-Methylphenol	0.000		0	N.D.			
18) Hexachloroethane	0.000		0	N.D.			
20) Nitrobenzene	7.086	77	108	N.D.			
22) Isophorone	7.370	82	96	N.D.			
23) 2-Nitrophenol	0.000		0	N.D.			
24) 2,4-Dimethylphenol	0.000		0	N.D.			
25) Bis(2-chloroethoxy) me...	0.000		0	N.D.			
26) Benzoic acid	7.563	105	152	807.53	ng/ml#	28	
27) 2,4-Dichlorophenol	0.000		0	N.D.			
28) 1,2,4-Trichlorobenzene	0.000		0	N.D.			
29) Naphthalene	0.000		0	N.D.			
30) 4-Chloroaniline	0.000		0	N.D.			
31) Hexachlorobutadiene	0.000		0	N.D.			
32) 4-Chloro-3-methylphenol	8.392	107	91	N.D.			
33) 2-Methylnaphthalene	8.557	142	100	N.D.			
34) 1-Methylnaphthalene	8.659	142	61	N.D.			
36) Hexachlorocyclopentadiene	0.000		0	N.D.			
37) 2,4,6-Trichlorophenol	0.000		0	N.D.			
38) 2,4,5-Trichlorophenol	0.000		0	N.D.			
39) 1,1'-Biphenyl	0.000		0	N.D.			
41) 2-Chloronaphthalene	0.000		0	N.D.			
42) 2-Nitroaniline	0.000		0	N.D.			
43) 2,6-Dimethylnaphthalene	0.000		0	N.D.			

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191917.D  
 Acq On : 20 Sep 2019 12:49 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICB1  
 Misc : 1x, DCM + ISTD  
 ALS Vial : 2 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Sep 20 14:22:39 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	0.000		0		N.D.	
45) Dimethyl phthalate	9.344	163	194		N.D.	
46) 1,3-Dinitrobenzene	0.000		0		N.D.	
47) 2,6-Dinitrotoluene	0.000		0		N.D.	
48) 1,2-Dinitrobenzene	0.000		0		N.D.	
49) Acenaphthylene	9.483	152	84		N.D.	
50) 3-Nitroaniline	0.000		0		N.D.	
51) Acenaphthene	9.648	153	78		N.D.	
52) 2,4-Dinitrophenol	0.000		0		N.D.	
53) 4-Nitrophenol	0.000		0		N.D.	
54) 2,4-Dinitrotoluene	9.777	165	228	55.41	ng/ml#	54
55) Dibenzofuran	0.000		0		N.D.	
56) 2,3,5,6-Tetrachlorophenol	0.000		0		N.D.	
57) 2,3,4,6-Tetrachlorophenol	0.000		0		N.D.	
58) Diethyl phthalate	10.039	149	103		N.D.	
59) 2,3,5-Trimethylnaphtha...	10.146	170	164		N.D.	
60) Fluorene	0.000		0		N.D.	
61) 4-Chlorophenyl phenyl ...	0.000		0		N.D.	
62) 4-Nitroaniline	0.000		0		N.D.	
63) 4,6-Dinitro-2-methylph...	0.000		0		N.D.	
65) N-Nitrosodiphenylamine	0.000		0		N.D.	
66) Azobenzene (1,2-DPH)	10.338	77	165		N.D.	
68) 4-Bromophenyl phenyl e...	0.000		0		N.D.	
69) Hexachlorobenzene	0.000		0		N.D.	
70) Pentachlorophenol (PCP)	10.938	266	325	80.48	ng/ml	76
71) Phenanthrene	11.135	178	418		N.D.	
72) Anthracene	11.135	178	418		N.D.	
73) Carbazole	11.381	167	91	5.75	ng/ml	60
74) Di-n-butyl phthalate	11.718	149	81		N.D.	
75) Fluoranthene	12.414	202	105		N.D.	
76) Benzidine	12.580	184	2179	136.03	ng/ml	91
77) Pyrene	12.724	202	64		N.D.	
80) Butyl benzyl phthalate	0.000		0		N.D.	
81) Bis(2-ethylhexyl) adipate	13.906	129	791	3.01	ng/ml	88
82) 3,3-Dichlorobenzidine	14.863	252	271	Below Cal	#	25
83) Benz(a)anthracene	14.912	228	2854	4.52	ng/ml	67
84) Chrysene	14.912	228	2826	4.77	ng/ml	66
85) Bis(2-ethylhexyl) phth...	15.067	149	83		N.D.	
87) Di-n-octyl phthalate	16.735	149	81	58.06	ng/ml#	1
88) Benzo(b)fluoranthene	17.468	252	54	8.05	ng/ml	57
89) Benzo(k)fluoranthene	17.538	252	89	8.62	ng/ml	57
90) Benzo(b+k)fluoranthene	17.538	252	89	15.88	ng/ml	57
91) Benzo(e)pyrene	0.000		0		N.D.	
92) Benzo(a)pyrene	0.000		0		N.D.	
93) Perylene	18.399	252	3568	7.20	ng/ml	70
95) Indeno(1,2,3-cd)pyrene	20.790	276	464		N.D.	
96) Dibenz(a,h)anthracene	20.790	278	242		N.D.	
97) Benzo(g,h,i)perylene	0.000		0		N.D.	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
Data File : J09191917.D  
Acq On : 20 Sep 2019 12:49 am  
Operator : JK/ AMS/ DTH  
Sample : 9I19035-ICB1  
Misc : 1x, DCM + ISTD  
ALS Vial : 2 Sample Multiplier: 1  
DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 14:22:39 2019  
Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
Quant Title : EPA 8270D: Semivolatile Organics  
QLast Update : Fri Sep 20 10:41:03 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10

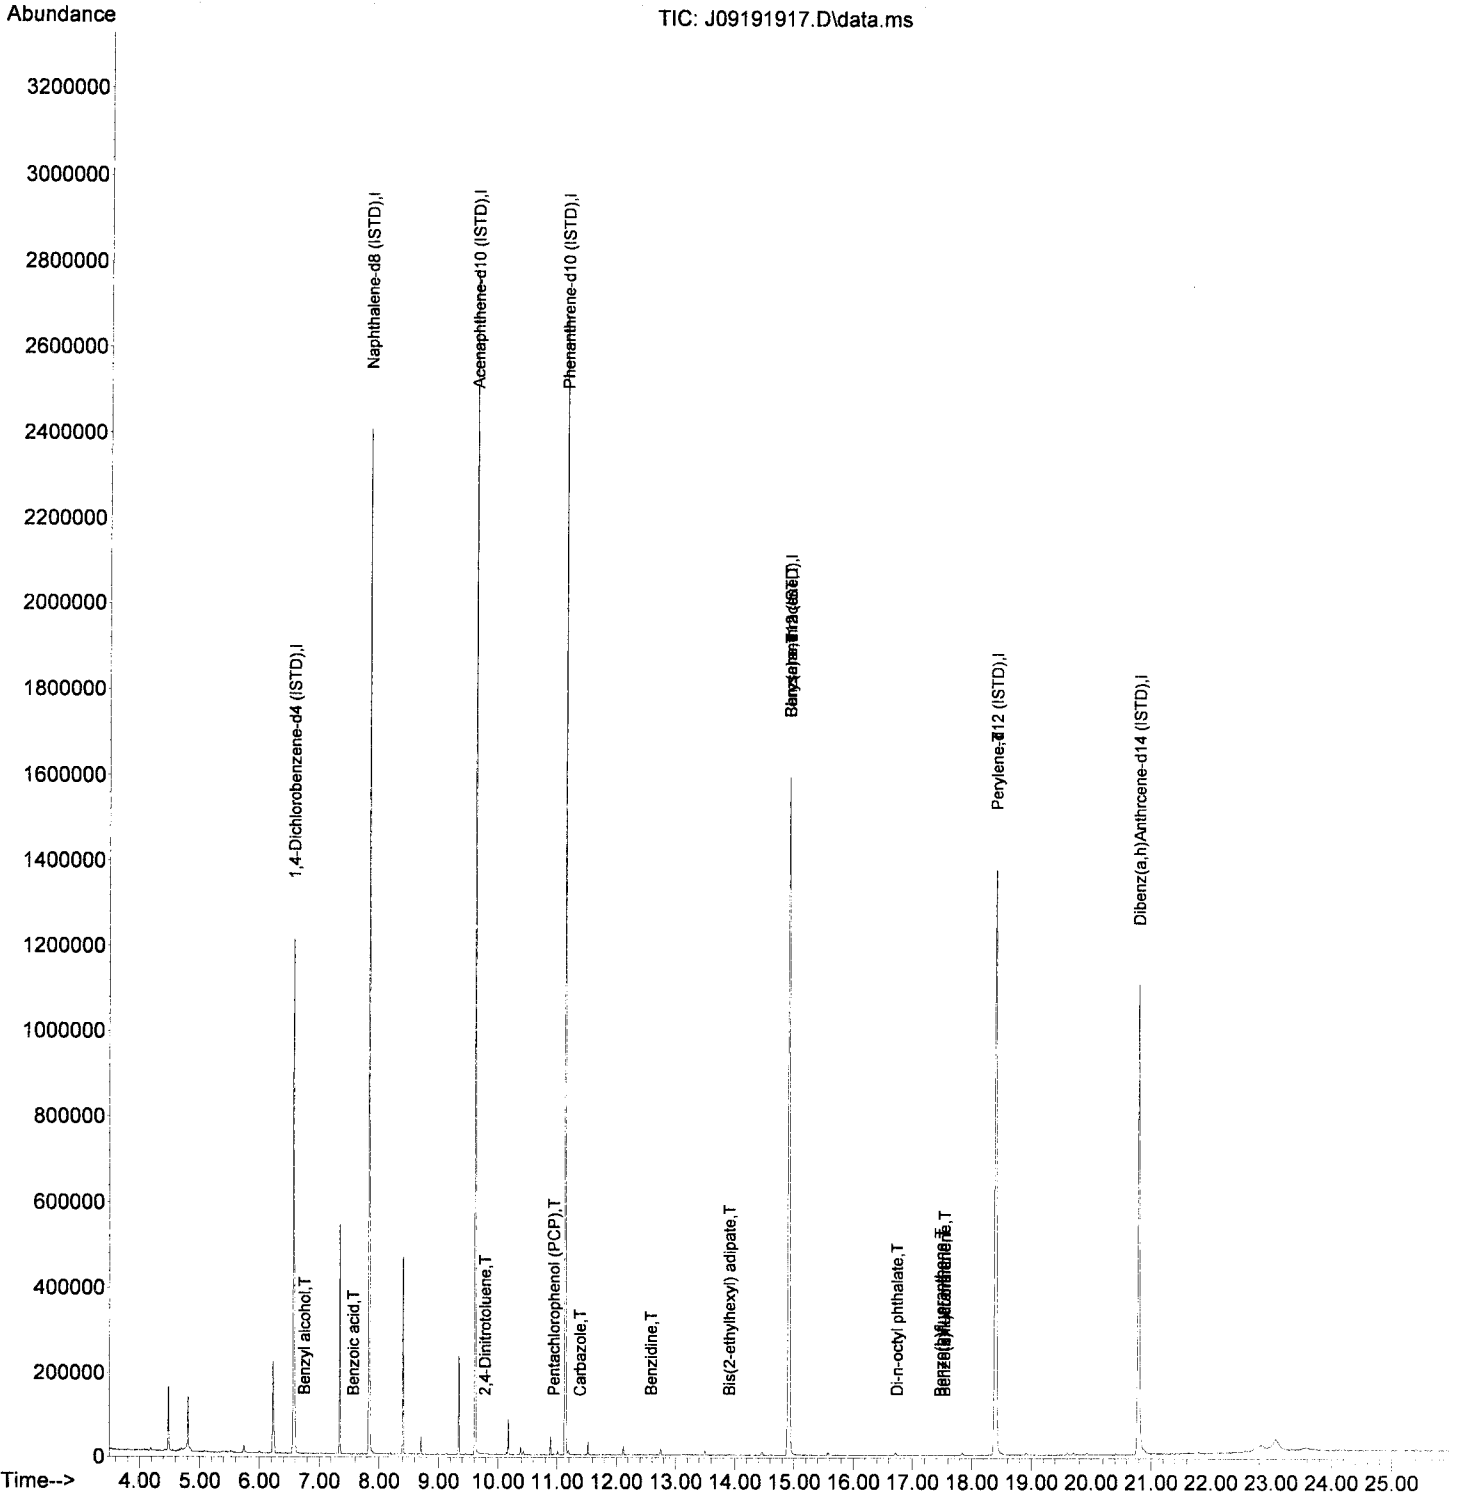

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:20 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*JK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev (Min)	Qvalue
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.573	152	291746	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.835	136	1221708	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.616	162	640527	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.130	188	1150535	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.912	240	1159268	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	18.394	264	1158997	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.795	292	913932	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.316	112	2742	13.86	ng/ml	0.03	
5) Phenol-d6 (Surr)	6.204	99	3493	13.74	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	7.113	82	2861	12.28	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.926	172	9460	20.11	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.413	330	762	14.12	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.922	244	9512	16.78	ng/ml	0.00	
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	<del>0.000</del>	<del>0</del>	<del>0</del>	<del>N.D.</del>			
3) Pyridine	<del>3.840</del>	<del>79</del>	<del>55</del>	<del>N.D.</del>			
6) Phenol	6.220	94	4498	15.57	ng/ml	89	
7) Aniline	6.252	93	2038	7.89	ng/ml	96	
8) Bis(2-chloroethyl) ether	6.311	93	4110	15.97	ng/ml	98	
9) 2-Chlorophenol	6.370	128	3591	17.25	ng/ml	95	
10) 1,3-Dichlorobenzene	6.520	146	4452	19.78	ng/ml	92	
11) 1,4-Dichlorobenzene	6.589	146	4492	20.57	ng/ml	93	
12) Benzyl alcohol	6.723	108	1506	11.09	ng/ml	96	
13) 1,2-Dichlorobenzene	6.744	146	4176	19.02	ng/ml	90	
14) 2-Methylphenol	6.808	107	2712	16.21	ng/ml	89	
15) 2,2'-Oxybis(1-Chloropr...	6.835	45	4376	13.18	ng/ml	93	
16) N-Nitrosodi-n-propylamine	6.964	70	2691	15.96	ng/ml	91	
17) 3+4-Methylphenol	6.958	107	3108	15.07	ng/ml	89	
18) Hexachloroethane	7.081	201	1267	21.07	ng/ml	89	
20) Nitrobenzene	7.135	77	3138	13.45	ng/ml	95	
22) Isophorone	7.370	82	6954	15.68	ng/ml	93	
23) 2-Nitrophenol	7.456	139	1053	38.03	ng/ml	91	
24) 2,4-Dimethylphenol	7.488	122	2375	14.05	ng/ml	83	
25) Bis(2-chloroethoxy) me...	7.579	93	4738	19.18	ng/ml	96	
26) Benzoic acid	7.552	105	229	305.92	ng/ml#	66	
27) 2,4-Dichlorophenol	7.691	162	1603	10.94	ng/ml	76	
28) 1,2,4-Trichlorobenzene	7.782	180	4361	24.59	ng/ml	82	
29) Naphthalene	7.857	128	14004	22.32	ng/ml	100	
30) 4-Chloroaniline	7.910	127	1531	18.26	ng/ml	90	
31) Hexachlorobutadiene	7.990	225	2247	23.76	ng/ml	84	
32) 4-Chloro-3-methylphenol	8.392	107	1917	10.87	ng/ml#	53	
33) 2-Methylnaphthalene	8.552	142	8620	20.12	ng/ml	94	
34) 1-Methylnaphthalene	8.654	142	9000	21.86	ng/ml	91	
36) Hexachlorocyclopentadiene	8.723	237	1303	12.86	ng/ml	74	
37) 2,4,6-Trichlorophenol	8.841	196	1119	20.94	ng/ml	79	
38) 2,4,5-Trichlorophenol	8.873	198	1218	11.18	ng/ml	91	
39) 1,1'-Biphenyl	9.028	154	10205	19.18	ng/ml	95	
41) 2-Chloronaphthalene	9.050	162	7646	19.58	ng/ml	99	
42) 2-Nitroaniline	9.146	138	939	7.22	ng/ml	82	
43) 2,6-Dimethylnaphthalene	9.189	156	7097	17.82	ng/ml	96	

*see MJ  
see MJ*

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:20 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev (Min)
44) 1,4-Dinitrobenzene	9.274	168	381	6.28	ng/ml#	63
45) Dimethyl phthalate	9.328	163	9190	20.06	ng/ml	91
46) 1,3-Dinitrobenzene	9.354	168	417	5.99	ng/ml	67
47) 2,6-Dinitrotoluene	9.386	165	1042	10.58	ng/ml	99
48) 1,2-Dinitrobenzene	9.440	168	304	6.59	ng/ml#	34
49) Acenaphthylene	9.472	152	12450	19.89	ng/ml	95
50) 3-Nitroaniline	9.563	138	592	27.61	ng/ml	93
51) Acenaphthene	9.649	153	8885	21.89	ng/ml	96
52) 2,4-Dinitrophenol	0.000		0	N.D.		
53) 4-Nitrophenol	9.723	139	120	34.89	ng/ml	85
54) 2,4-Dinitrotoluene	9.798	165	1027	8.10	ng/ml#	60
55) Dibenzofuran	9.825	168	11668	21.08	ng/ml	90
56) 2,3,5,6-Tetrachlorophenol	9.911	232	774	34.62	ng/ml	97
57) 2,3,4,6-Tetrachlorophenol	9.948	232	856	19.53	ng/ml	77
58) Diethyl phthalate	10.044	149	8035	18.39	ng/ml	97
59) 2,3,5-Trimethylnaphtha...	10.034	170	7629	21.57	ng/ml	95
60) Fluorene	10.173	166	9113	20.91	ng/ml	94
61) 4-Chlorophenyl phenyl ...	10.167	204	4548	22.45	ng/ml	95
62) 4-Nitroaniline	10.183	138	719	8.15	ng/ml	91
63) 4,6-Dinitro-2-methylph...	0.000		0	N.D.		
65) N-Nitrosodiphenylamine	10.285	169	5957	16.84	ng/ml	88
66) Azobenzene (1,2-DPH)	10.328	77	6853	14.60	ng/ml	95
68) 4-Bromophenyl phenyl e...	10.670	248	2390	20.18	ng/ml	86
69) Hexachlorobenzene	10.745	284	3454	25.35	ng/ml	83
70) Pentachlorophenol (PCP)	10.938	266	1000	46.06	ng/ml	93
71) Phenanthrene	11.157	178	13749	21.85	ng/ml	98
72) Anthracene	11.205	178	11450	18.50	ng/ml	96
73) Carbazole	11.365	167	9186	17.97	ng/ml	96
74) Di-n-butyl phthalate	11.718	149	11697	16.31	ng/ml	94
75) Fluoranthene	12.425	202	12248	18.61	ng/ml	96
76) Benzidine	12.580	184	3398	75.33	ng/ml	91
77) Pyrene	12.708	202	12641	19.23	ng/ml	93
80) Butyl benzyl phthalate	13.730	149	2535	6.98	ng/ml	75
81) Bis(2-ethylhexyl) adipate	13.906	129	2762	8.49	ng/ml	94
82) 3,3-Dichlorobenzidine	14.853	252	3617	Below	Cal	95
83) Benz(a)anthracene	14.890	228	13459	19.80	ng/ml	92
84) Chrysene	14.970	228	11530	18.39	ng/ml	96
85) Bis(2-ethylhexyl) phth...	15.077	149	2659	5.54	ng/ml	99
87) Di-n-octyl phthalate	16.741	149	3334	34.72	ng/ml	97
88) Benzo(b)fluoranthene	17.463	252	8297	11.82	ng/ml	98
89) Benzo(k)fluoranthene	17.538	252	8174	12.27	ng/ml	92
90) Benzo(b+k)fluoranthene	17.463	252	17019	24.40	ng/ml	98
91) Benzo(e)pyrene	18.126	252	8657	12.60	ng/ml	95
92) Benzo(a)pyrene	18.238	252	6648	10.53	ng/ml	84
93) Perylene	18.447	252	9278	15.50	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.774	276	10072	19.60	ng/ml	76
96) Dibenz(a,h)anthracene	20.854	278	8754	19.00	ng/ml	94
97) Benzo(g,h,i)perylene	21.319	276	7772	15.71	ng/ml	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:20 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(2) N-Nitrosodimethylamine (TG)

3.883min (-3.883) 0.00 ng/ml




response 0

Ion	Exp%	Act%
74.10	100.00	0.00
42.10	49.40	0.00#
43.10	22.20	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:20 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



(2) N-Nitrosodimethylamine (TG)

3.974min (+ 0.091) 16.33 ng/ml (m)

*JK* 9/20/19




response 2214

Ion	Exp%	Act%
74.10	100.00	100.00
42.10	49.40	66.21
43.10	22.20	47.47
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:20 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(3) Pyridine (TG)

3.840min (-0.064) 0.24 ng/ml

response




55

Ion	Exp%	Act%
79.10	100.00	100.00
52.10	50.80	81.20#
50.10	18.70	146.15#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:20 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191918.D\data.ms

(3) Pyridine (TG)

4.049min (+ 0.145) 9.55 ng/ml(m)


*Handwritten signature and date: 9/20/19*

response 2206

Ion	Exp%	Act%
79.10	100.00	100.00
52.10	50.80	96.24#
50.10	18.70	93.39#
0.00	0.00	0.00

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191918.D  
 Acq On : 20 Sep 2019 1:24 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL1  
 Misc : 1x, A19G238@20  
 ALS Vial : 3 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:20 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191919.D  
 Acq On : 20 Sep 2019 1:59 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL2  
 Misc : 1x, A19G239@50  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*Handwritten:* 9/20/19

Compound	R.T.	QIon	Response	Conc	Units	Dev (Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.573	152	291253	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.835	136	1195757	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.616	162	616226	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.130	188	1087898	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.906	240	1113286	2000.00	ng/ml	-0.01	
86) Perylene-d12 (ISTD)	18.393	264	1097209	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.790	292	855339	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.311	112	7611	38.53	ng/ml	0.02	
5) Phenol-d6 (Surr)	6.204	99	9501	37.44	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	7.113	82	7903	33.99	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.926	172	24802	54.81	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.419	330	1929	37.79	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.922	244	25113	46.14	ng/ml	0.00	
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	3.952	74	4569	33.76	ng/ml	93	Qvalue
3) Pyridine	4.000	79	7667m	33.23	ng/ml#		
6) Phenol	6.215	94	11373	39.43	ng/ml	93	
7) Aniline	6.252	93	10955	42.49	ng/ml	95	
8) Bis(2-chloroethyl) ether	6.306	93	10198	39.70	ng/ml	95	
9) 2-Chlorophenol	6.364	128	9461	45.54	ng/ml	88	
10) 1,3-Dichlorobenzene	6.519	146	11576	51.52	ng/ml	97	
11) 1,4-Dichlorobenzene	6.589	146	12059	55.30	ng/ml	94	
12) Benzyl alcohol	6.707	108	3460	25.97	ng/ml	94	
13) 1,2-Dichlorobenzene	6.739	146	12229	55.79	ng/ml	98	
14) 2-Methylphenol	6.808	107	6405	38.35	ng/ml	90	
15) 2,2'-Oxybis(1-Chloropr...	6.835	45	10585	31.94	ng/ml	90	
16) N-Nitrosodi-n-propylamine	6.963	70	6538	38.84	ng/ml	98	
17) 3+4-Methylphenol	6.958	107	8248	40.07	ng/ml	95	
18) Hexachloroethane	7.076	201	3313	55.18	ng/ml	93	
20) Nitrobenzene	7.135	77	8614	36.98	ng/ml	95	
22) Isophorone	7.370	82	18082	41.67	ng/ml	97	
23) 2-Nitrophenol	7.455	139	3400	54.77	ng/ml	93	
24) 2,4-Dimethylphenol	7.488	122	5922	35.79	ng/ml	97	
25) Bis(2-chloroethoxy) me...	7.579	93	11523	47.66	ng/ml	92	
26) Benzoic acid	7.573	105	200	305.64	ng/ml#	58	
27) 2,4-Dichlorophenol	7.691	162	5068	35.35	ng/ml	91	
28) 1,2,4-Trichlorobenzene	7.776	180	11103	63.97	ng/ml	92	
29) Naphthalene	7.857	128	34402	56.01	ng/ml	99	
30) 4-Chloroaniline	7.905	127	7306	53.73	ng/ml	92	
31) Hexachlorobutadiene	7.990	225	5972	64.52	ng/ml	97	
32) 4-Chloro-3-methylphenol	8.392	107	5211	30.18	ng/ml	82	
33) 2-Methylnaphthalene	8.557	142	23135	55.17	ng/ml	94	
34) 1-Methylnaphthalene	8.654	142	23006	57.09	ng/ml	92	
36) Hexachlorocyclopentadiene	8.723	237	3356	34.42	ng/ml	95	
37) 2,4,6-Trichlorophenol	8.835	196	3644	44.63	ng/ml	82	
38) 2,4,5-Trichlorophenol	8.873	198	3657	34.90	ng/ml	96	
39) 1,1'-Biphenyl	9.028	154	28683	56.03	ng/ml	96	
41) 2-Chloronaphthalene	9.049	162	19450	51.76	ng/ml	98	
42) 2-Nitroaniline	9.146	138	2728	21.81	ng/ml	70	
43) 2,6-Dimethylnaphthalene	9.188	156	20566	53.66	ng/ml	99	

*Handwritten:* See MJ

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191919.D  
 Acq On : 20 Sep 2019 1:59 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL2  
 Misc : 1x, A19G239@50  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10




Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.274	168	915	15.67	ng/ml#	75
45) Dimethyl phthalate	9.328	163	22486	51.02	ng/ml	99
46) 1,3-Dinitrobenzene	9.354	168	1390	20.76	ng/ml	79
47) 2,6-Dinitrotoluene	9.386	165	2915	30.75	ng/ml	88
48) 1,2-Dinitrobenzene	9.440	168	1349	30.38	ng/ml	98
49) Acenaphthylene	9.472	152	32192	53.45	ng/ml	98
50) 3-Nitroaniline	9.563	138	2106	41.58	ng/ml#	68
51) Acenaphthene	9.648	153	22572	57.81	ng/ml	99
52) 2,4-Dinitrophenol	0.000		0	N.D.		
53) 4-Nitrophenol	9.723	139	699	42.87	ng/ml	71
54) 2,4-Dinitrotoluene	9.798	165	2508	20.56	ng/ml	84
55) Dibenzofuran	9.825	168	29377	55.18	ng/ml	94
56) 2,3,5,6-Tetrachlorophenol	9.905	232	1678	45.25	ng/ml	83
57) 2,3,4,6-Tetrachlorophenol	9.948	232	2513	38.75	ng/ml	86
58) Diethyl phthalate	10.044	149	21378	50.87	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	10.034	170	19066	56.02	ng/ml	97
60) Fluorene	10.173	166	22247	53.06	ng/ml	99
61) 4-Chlorophenyl phenyl ...	10.167	204	11449	58.75	ng/ml	94
62) 4-Nitroaniline	10.178	138	2192	25.82	ng/ml	87
63) 4,6-Dinitro-2-methylph...	10.215	198	206	74.51	ng/ml#	65
65) N-Nitrosodiphenylamine	10.285	169	16461	49.20	ng/ml	97
66) Azobenzene (1,2-DPH)	10.328	77	17404	39.22	ng/ml	93
68) 4-Bromophenyl phenyl e...	10.665	248	6326	56.49	ng/ml	91
69) Hexachlorobenzene	10.745	284	7615	59.10	ng/ml	98
70) Pentachlorophenol (PCP)	10.937	266	1392	53.47	ng/ml#	61
71) Phenanthrene	11.157	178	32566	54.75	ng/ml	95
72) Anthracene	11.205	178	30636	52.34	ng/ml	98
73) Carbazole	11.365	167	24489	50.68	ng/ml	93
74) Di-n-butyl phthalate	11.718	149	29117	42.93	ng/ml	99
75) Fluoranthene	12.424	202	31166	50.09	ng/ml	93
76) Benzidine	12.579	184	5652	90.66	ng/ml	93
77) Pyrene	12.713	202	32717	52.64	ng/ml	98
80) Butyl benzyl phthalate	13.735	149	6765	19.40	ng/ml	97
81) Bis(2-ethylhexyl) adipate	13.911	129	6924	22.16	ng/ml	92
82) 3,3-Dichlorobenzidine	14.847	252	11318	Below Cal		86
83) Benz(a)anthracene	14.890	228	29779	45.62	ng/ml	97
84) Chrysene	14.960	228	29254	48.57	ng/ml	97
85) Bis(2-ethylhexyl) phth...	15.072	149	8694	18.85	ng/ml	93
87) Di-n-octyl phthalate	16.735	149	9861	43.05	ng/ml	94
88) Benzo(b)fluoranthene	17.468	252	21819	32.83	ng/ml	93
89) Benzo(k)fluoranthene	17.543	252	23687	37.57	ng/ml	95
90) Benzo(b+k)fluoranthene	17.468	252	47809	72.40	ng/ml	93
91) Benzo(e)pyrene	18.121	252	24570	37.78	ng/ml	95
92) Benzo(a)pyrene	18.238	252	18583	31.08	ng/ml	97
93) Perylene	18.447	252	24689	43.56	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.779	276	25006	52.00	ng/ml	88
96) Dibenz(a,h)anthracene	20.848	278	21791	50.52	ng/ml	94
97) Benzo(g,h,i)perylene	21.308	276	20181	43.59	ng/ml	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191919.D  
 Acq On : 20 Sep 2019 1:59 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL2  
 Misc : 1x, A19G239@50  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191919.D\data.ms

(2) N-Nitrosodimethylamine (TG)

3.952min (+ 0.070) 33.76 ng/ml

response 4569




Ion	Exp%	Act%
74.10	100.00	100.00
42.10	49.40	53.59
43.10	22.20	26.52
0.00	0.00	0.00



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191919.D  
 Acq On : 20 Sep 2019 1:59 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL2  
 Misc : 1x, A19G239@50  
 ALS Vial : 4 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191919.D\data.ms

(2) N-Nitrosodimethylamine (TG)

3.952min (+ 0.070) 40.76 ng/ml

response 5516


*Handwritten signature and date: 9/20/19*

Ion	Exp%	Act%
74.10	100.00	100.00
42.10	49.40	53.59
43.10	22.20	26.52
0.00	0.00	0.00

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
Data File : J09191919.D  
Acq On : 20 Sep 2019 1:59 am  
Operator : JK/ AMS/ DTH  
Sample : 9I19035-CAL2  
Misc : 1x, A19G239@50  
ALS Vial : 4 Sample Multiplier: 1  
DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:25 2019  
Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
Quant Title : EPA 8270D: Semivolatile Organics  
QLast Update : Fri Sep 20 09:45:16 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191920.D  
 Acq On : 20 Sep 2019 2:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL3  
 Misc : 1x, A19G240@100  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:30 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*JK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4...	6.573	152	290594	2000.00	ng/ml	0.00
21) Naphthalene-d8 (ISTD)	7.835	136	1186873	2000.00	ng/ml	0.00
35) Acenaphthene-d10 (ISTD)	9.616	162	615111	2000.00	ng/ml	0.00
64) Phenanthrene-d10 (ISTD)	11.130	188	1118597	2000.00	ng/ml	0.00
78) Chrysene-d12 (ISTD)	14.912	240	1122909	2000.00	ng/ml	0.00
86) Perylene-d12 (ISTD)	18.394	264	1127380	2000.00	ng/ml	0.00
94) Dibenz(a,h)Anthrcene-d...	20.790	292	892958	2000.00	ng/ml	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol (Surr)	5.311	112	13834	70.19	ng/ml	0.02
5) Phenol-d6 (Surr)	6.204	99	21003	82.96	ng/ml	0.00
19) Nitrobenzene-d5 (Surr)	7.113	82	16492	71.09	ng/ml	0.00
40) 2-Fluorobiphenyl (Surr)	8.926	172	53353	118.12	ng/ml	0.00
67) 2,4,6-Tribromophenol (...)	10.419	330	4809	91.63	ng/ml	0.00
79) Terphenyl-d14 (Surr)	12.922	244	54871	99.96	ng/ml	0.00
<b>Target Compounds</b>						
2) N-Nitrosodimethylamine	3.952	74	9178	67.97	ng/ml	91
3) Pyridine	3.990	79	18548m	80.58	ng/ml#	
6) Phenol	6.220	94	23364	81.19	ng/ml	97
7) Aniline	6.252	93	23125	89.89	ng/ml	94
8) Bis(2-chloroethyl) ether	6.311	93	21464	83.74	ng/ml	93
9) 2-Chlorophenol	6.370	128	19462	93.88	ng/ml	97
10) 1,3-Dichlorobenzene	6.520	146	23840	106.35	ng/ml	98
11) 1,4-Dichlorobenzene	6.589	146	23338	107.27	ng/ml	92
12) Benzyl alcohol	6.707	108	8907	67.02	ng/ml	96
13) 1,2-Dichlorobenzene	6.739	146	23746	108.58	ng/ml	95
14) 2-Methylphenol	6.808	107	14254	85.54	ng/ml	98
15) 2,2'-Oxybis(1-Chloropr...	6.835	45	21848	66.08	ng/ml	97
16) N-Nitrosodi-n-propylamine	6.963	70	13631	81.17	ng/ml	98
17) 3+4-Methylphenol	6.958	107	16854	82.07	ng/ml	89
18) Hexachloroethane	7.076	201	6562	109.55	ng/ml	86
20) Nitrobenzene	7.135	77	17280	74.35	ng/ml	100
22) Isophorone	7.370	82	37997	88.22	ng/ml	97
23) 2-Nitrophenol	7.450	139	7240	82.31	ng/ml	87
24) 2,4-Dimethylphenol	7.488	122	14806	90.15	ng/ml	90
25) Bis(2-chloroethoxy) me...	7.579	93	23395	97.49	ng/ml	95
26) Benzoic acid	7.605	105	129	304.84	ng/ml#	68
27) 2,4-Dichlorophenol	7.691	162	12689	89.17	ng/ml	98
28) 1,2,4-Trichlorobenzene	7.776	180	21292	123.58	ng/ml	98
29) Naphthalene	7.857	128	69263	113.61	ng/ml	96
30) 4-Chloroaniline	7.905	127	15139	102.27	ng/ml	96
31) Hexachlorobutadiene	7.990	225	11598	126.23	ng/ml	93
32) 4-Chloro-3-methylphenol	8.386	107	11698	68.25	ng/ml	89
33) 2-Methylnaphthalene	8.557	142	46039	110.62	ng/ml	99
34) 1-Methylnaphthalene	8.659	142	46134	115.33	ng/ml	98
36) Hexachlorocyclopentadiene	8.723	237	8031	82.51	ng/ml	94
37) 2,4,6-Trichlorophenol	8.841	196	7912	84.10	ng/ml	95
38) 2,4,5-Trichlorophenol	8.873	198	8310	79.46	ng/ml	93
39) 1,1'-Biphenyl	9.028	154	58168	113.83	ng/ml	98
41) 2-Chloronaphthalene	9.049	162	41705	111.19	ng/ml	97
42) 2-Nitroaniline	9.146	138	6877	55.07	ng/ml	89
43) 2,6-Dimethylnaphthalene	9.189	156	43362	113.35	ng/ml	96

*See M1*

*See M1*

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191920.D  
 Acq On : 20 Sep 2019 2:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL3  
 Misc : 1x, A19G240@100  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:30 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10




Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.274	168	2006	34.41	ng/ml	84
45) Dimethyl phthalate	9.328	163	49089	111.58	ng/ml	99
46) 1,3-Dinitrobenzene	9.354	168	3033	45.37	ng/ml	81
47) 2,6-Dinitrotoluene	9.386	165	6526	68.97	ng/ml	84
48) 1,2-Dinitrobenzene	9.445	168	2742	61.87	ng/ml	83
49) Acenaphthylene	9.472	152	68008	113.12	ng/ml	97
50) 3-Nitroaniline	9.558	138	6036	77.71	ng/ml	97
51) Acenaphthene	9.649	153	44425	113.99	ng/ml	98
52) 2,4-Dinitrophenol	9.670	184	169	146.81	ng/ml	80
53) 4-Nitrophenol	9.723	139	2106	62.15	ng/ml	64
54) 2,4-Dinitrotoluene	9.798	165	6812	55.94	ng/ml	98
55) Dibenzofuran	9.825	168	62656	117.90	ng/ml	96
56) 2,3,5,6-Tetrachlorophenol	9.905	232	5673	90.84	ng/ml	95
57) 2,3,4,6-Tetrachlorophenol	9.948	232	7263	92.88	ng/ml	95
58) Diethyl phthalate	10.044	149	47870	114.11	ng/ml	99
59) 2,3,5-Trimethylnaphtha...	10.034	170	38608	113.65	ng/ml	97
60) Fluorene	10.173	166	48968	116.99	ng/ml	96
61) 4-Chlorophenyl phenyl ...	10.167	204	23837	122.54	ng/ml	99
62) 4-Nitroaniline	10.178	138	5563	65.64	ng/ml	90
63) 4,6-Dinitro-2-methylph...	10.210	198	761	84.48	ng/ml	74
65) N-Nitrosodiphenylamine	10.285	169	36899	107.27	ng/ml	97
66) Azobenzene (1,2-DPH)	10.328	77	37821	82.88	ng/ml	96
68) 4-Bromophenyl phenyl e...	10.665	248	13242	115.00	ng/ml	94
69) Hexachlorobenzene	10.745	284	16314	123.13	ng/ml	97
70) Pentachlorophenol (PCP)	10.938	266	4341	100.38	ng/ml	92
71) Phenanthrene	11.151	178	68493	111.98	ng/ml	98
72) Anthracene	11.205	178	65192	108.32	ng/ml	98
73) Carbazole	11.365	167	54742	110.17	ng/ml	98
74) Di-n-butyl phthalate	11.718	149	70280	100.78	ng/ml	99
75) Fluoranthene	12.424	202	70234	109.79	ng/ml	96
76) Benzidine	12.580	184	12748	133.02	ng/ml	98
77) Pyrene	12.713	202	69474	108.72	ng/ml	98
80) Butyl benzyl phthalate	13.735	149	18774	53.39	ng/ml	97
81) Bis(2-ethylhexyl) adipate	13.911	129	18358	58.24	ng/ml	95
82) 3,3-Dichlorobenzidine	14.853	252	24584	98.99	ng/ml	93
83) Benz(a)anthracene	14.885	228	64818	98.44	ng/ml	99
84) Chrysene	14.965	228	61418	101.11	ng/ml	98
85) Bis(2-ethylhexyl) phth...	15.072	149	26668	57.33	ng/ml	98
87) Di-n-octyl phthalate	16.741	149	33665	71.49	ng/ml	95
88) Benzo(b)fluoranthene	17.468	252	57260	83.86	ng/ml	95
89) Benzo(k)fluoranthene	17.538	252	58523	90.33	ng/ml	99
90) Benzo(b+k)fluoranthene	17.538	252	120376	177.42	ng/ml	99
91) Benzo(e)pyrene	18.121	252	58165	87.04	ng/ml	93
92) Benzo(a)pyrene	18.244	252	50114	81.58	ng/ml	96
93) Perylene	18.447	252	50289	86.35	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.779	276	52504	104.59	ng/ml	97
96) Dibenz(a,h)anthracene	20.854	278	48705	108.17	ng/ml	97
97) Benzo(g,h,i)perylene	21.309	276	49447	102.31	ng/ml	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191920.D  
 Acq On : 20 Sep 2019 2:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL3  
 Misc : 1x, A19G240@100  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:30 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



(2) N-Nitrosodimethylamine (TG)

3.952min (+ 0.070) 67.97 ng/ml




response 9178

Ion	Exp%	Act%
74.10	100.00	100.00
42.10	49.40	55.00
43.10	22.20	27.95
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191920.D  
 Acq On : 20 Sep 2019 2:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL3  
 Misc : 1x, A19G240@100  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:30 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191920.D\data.ms

(2) N-Nitrosodimethylamine (TG)

3.952min (+ 0.070) 86.90 ng/ml (m)




*Handwritten signature and date: JK 9/20/19*

response	11734	
Ion	Exp%	Act%
74.10	100.00	100.00
42.10	49.40	55.00
43.10	22.20	27.95
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191920.D  
 Acq On : 20 Sep 2019 2:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL3  
 Misc : 1x, A19G240@100  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:30 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191920.D\data.ms

(26) Benzoic acid (T)

7.605min (+ 0.027) 304.84 ng/ml




response 129

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	108.48
77.00	72.00	113.33#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191920.D  
 Acq On : 20 Sep 2019 2:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL3  
 Misc : 1x, A19G240@100  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:30 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191920.D\data.ms

(26) Benzoic acid (T)

7.536min (-0.043) 327.42 ng/ml

*Handwritten signature and date: 9/20/19*


response 2086

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	99.19
77.00	72.00	54.47
0.00	0.00	0.00



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191920.D  
 Acq On : 20 Sep 2019 2:34 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL3  
 Misc : 1x, A19G240@100  
 ALS Vial : 5 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:30 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191921.D  
 Acq On : 20 Sep 2019 3:09 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL4  
 Misc : 1x, A19G241@200  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:34 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*JK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.568	152	286105	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.835	136	1204364	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.616	162	611745	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.130	188	1098102	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.912	240	1116848	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	18.399	264	1089238	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.795	292	868590	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.300	112	34817	179.42	ng/ml	0.01	
5) Phenol-d6 (Surr)	6.204	99	45844	183.93	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	7.113	82	34591	151.44	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.926	172	107137	238.50	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.419	330	10829	210.19	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.922	244	107135	196.23	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.915	74	19941	150.00	ng/ml		98
3) Pyridine	3.947	79	38499m	169.88	ng/ml#		
6) Phenol	6.215	94	51417	181.47	ng/ml		97
7) Aniline	6.247	93	49031	193.59	ng/ml		96
8) Bis(2-chloroethyl) ether	6.306	93	42595	168.79	ng/ml		93
9) 2-Chlorophenol	6.364	128	42160	206.57	ng/ml		96
10) 1,3-Dichlorobenzene	6.514	146	48050	217.71	ng/ml		98
11) 1,4-Dichlorobenzene	6.584	146	46724	218.13	ng/ml		96
12) Benzyl alcohol	6.701	108	18281	139.70	ng/ml		91
13) 1,2-Dichlorobenzene	6.739	146	47924	222.58	ng/ml		95
14) 2-Methylphenol	6.808	107	30801	187.74	ng/ml		98
15) 2,2'-Oxybis(1-Chloropr...	6.835	45	44401	136.40	ng/ml		97
16) N-Nitrosodi-n-propylamine	6.963	70	28365	171.56	ng/ml		98
17) 3+4-Methylphenol	6.958	107	38484	190.34	ng/ml		97
18) Hexachloroethane	7.076	201	13490	228.75	ng/ml		98
20) Nitrobenzene	7.129	77	37240	162.74	ng/ml		98
22) Isophorone	7.365	82	78525	179.67	ng/ml		96
23) 2-Nitrophenol	7.450	139	16298	145.34	ng/ml		96
24) 2,4-Dimethylphenol	7.488	122	31880	191.29	ng/ml		96
25) Bis(2-chloroethoxy) me...	7.579	93	49149	201.85	ng/ml		96
26) Benzoic acid	7.573	105	338	307.20	ng/ml		78
27) 2,4-Dichlorophenol	7.691	162	30346	210.14	ng/ml		97
28) 1,2,4-Trichlorobenzene	7.776	180	45007	257.44	ng/ml		95
29) Naphthalene	7.857	128	141239	228.31	ng/ml		99
30) 4-Chloroaniline	7.905	127	38526	242.70	ng/ml		98
31) Hexachlorobutadiene	7.990	225	24136	258.88	ng/ml		95
32) 4-Chloro-3-methylphenol	8.386	107	26469	152.19	ng/ml		98
33) 2-Methylnaphthalene	8.557	142	98607	233.48	ng/ml		98
34) 1-Methylnaphthalene	8.654	142	95459	235.18	ng/ml		99
36) Hexachlorocyclopentadiene	8.729	237	17504	180.83	ng/ml		95
37) 2,4,6-Trichlorophenol	8.841	196	18771	185.20	ng/ml		90
38) 2,4,5-Trichlorophenol	8.873	198	18422	177.11	ng/ml		88
39) 1,1'-Biphenyl	9.028	154	117826	231.84	ng/ml		99
41) 2-Chloronaphthalene	9.049	162	86117	230.86	ng/ml		100
42) 2-Nitroaniline	9.146	138	16161	130.13	ng/ml		94
43) 2,6-Dimethylnaphthalene	9.188	156	87215	229.24	ng/ml		96

*see MI*

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191921.D  
 Acq On : 20 Sep 2019 3:09 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL4  
 Misc : 1x, A19G241@200  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:34 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10




Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.274	168	5164	89.07	ng/ml	88
45) Dimethyl phthalate	9.328	163	96043	219.51	ng/ml	99
46) 1,3-Dinitrobenzene	9.354	168	7621	114.64	ng/ml	85
47) 2,6-Dinitrotoluene	9.386	165	16812	178.66	ng/ml	87
48) 1,2-Dinitrobenzene	9.440	168	7269	164.92	ng/ml	83
49) Acenaphthylene	9.472	152	136163	227.72	ng/ml	99
50) 3-Nitroaniline	9.558	138	15637	168.60	ng/ml	93
51) Acenaphthene	9.648	153	89211	230.16	ng/ml	98
52) 2,4-Dinitrophenol	9.665	184	796	162.82	ng/ml	85
53) 4-Nitrophenol	9.723	139	5790	112.91	ng/ml	91
54) 2,4-Dinitrotoluene	9.798	165	16915	139.67	ng/ml	99
55) Dibenzofuran	9.825	168	123476	233.62	ng/ml	99
56) 2,3,5,6-Tetrachlorophenol	9.905	232	13193	177.32	ng/ml	96
57) 2,3,4,6-Tetrachlorophenol	9.948	232	16040	193.66	ng/ml	99
58) Diethyl phthalate	10.044	149	92047	220.62	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	10.039	170	78195	231.45	ng/ml	96
60) Fluorene	10.173	166	95574	229.60	ng/ml	98
61) 4-Chlorophenyl phenyl ...	10.167	204	45790	236.70	ng/ml	98
62) 4-Nitroaniline	10.178	138	12832	152.25	ng/ml	96
63) 4,6-Dinitro-2-methylph...	10.215	198	2504	115.96	ng/ml	91
65) N-Nitrosodiphenylamine	10.285	169	77183	228.56	ng/ml	96
66) Azobenzene (1,2-DPH)	10.328	77	76676	171.16	ng/ml	99
68) 4-Bromophenyl phenyl e...	10.670	248	26212	231.88	ng/ml	97
69) Hexachlorobenzene	10.745	284	30519	234.65	ng/ml	96
70) Pentachlorophenol (PCP)	10.938	266	7638	155.67	ng/ml	93
71) Phenanthrene	11.151	178	134878	224.63	ng/ml	96
72) Anthracene	11.205	178	132343	224.01	ng/ml	97
73) Carbazole	11.365	167	110985	227.54	ng/ml	99
74) Di-n-butyl phthalate	11.718	149	138215	201.89	ng/ml	98
75) Fluoranthene	12.424	202	138551	220.63	ng/ml	99
76) Benzidine	12.580	184	43242	323.12	ng/ml	97
77) Pyrene	12.713	202	143586	228.88	ng/ml	99
80) Butyl benzyl phthalate	13.735	149	42397	121.22	ng/ml	99
81) Bis(2-ethylhexyl) adipate	13.911	129	37581	119.87	ng/ml	98
82) 3,3-Dichlorobenzidine	14.858	252	53778	529.15	ng/ml	97
83) Benz(a)anthracene	14.885	228	124472	190.07	ng/ml	97
84) Chrysene	14.965	228	120574	199.57	ng/ml	98
85) Bis(2-ethylhexyl) phth...	15.072	149	58143	125.67	ng/ml	100
87) Di-n-octyl phthalate	16.741	149	75567	125.21	ng/ml	98
88) Benzo(b)fluoranthene	17.479	252	113080	171.41	ng/ml	95
89) Benzo(k)fluoranthene	17.538	252	115987	185.29	ng/ml	97
90) Benzo(b+k)fluoranthene	17.479	252	234995	358.49	ng/ml	95
91) Benzo(e)pyrene	18.126	252	113143	175.23	ng/ml	91
92) Benzo(a)pyrene	18.244	252	99882	168.29	ng/ml	97
93) Perylene	18.447	252	100217	178.17	ng/ml	98
95) Indeno(1,2,3-cd)pyrene	20.784	276	100411	205.68	ng/ml	96
96) Dibenz(a,h)anthracene	20.854	278	95316	217.63	ng/ml	99
97) Benzo(g,h,i)perylene	21.319	276	101188	215.24	ng/ml	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191921.D  
 Acq On : 20 Sep 2019 3:09 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL4  
 Misc : 1x, A19G241@200  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:34 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191921.D\data.ms

~~(26) Benzoic acid (T)~~




~~7.573min (-0.005) 307.20 ng/ml~~

response	338
Ion	Exp% Act%
105.00	100.00 100.00
122.00	90.90 119.23
77.00	72.00 82.82
0.00	0.00 0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191921.D  
 Acq On : 20 Sep 2019 3:09 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL4  
 Misc : 1x, A19G241@200  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:34 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191921.D\data.ms

(26) Benzoic acid (T)

7.536min (-0.043) 341.24 ng/ml/m


response 3335

*JK 9/20/19*

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	83.48
77.00	72.00	58.50
0.00	0.00	0.00

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191921.D  
 Acq On : 20 Sep 2019 3:09 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL4  
 Misc : 1x, A19G241@200  
 ALS Vial : 6 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:34 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191922.D  
 Acq On : 20 Sep 2019 3:44 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL5  
 Misc : 1x, A19G242@500  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:39 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*OK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.573	152	299020	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.835	136	1217422	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.617	162	625555	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.130	188	1123094	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.917	240	1146727	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	18.399	264	1149483	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.795	292	954508	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.306	112	95687	471.80	ng/ml	0.02	
5) Phenol-d6 (Surr)	6.204	99	124621	478.38	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	7.113	82	98184	411.28	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.927	172	272047	592.23	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.419	330	33701	639.58	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.922	244	285146	508.67	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.931	74	52485m	377.75	ng/ml#		
3) Pyridine	3.958	79	83583	352.88	ng/ml		96
6) Phenol	6.215	94	136576	461.22	ng/ml		97
7) Aniline	6.247	93	124901	471.84	ng/ml		97
8) Bis(2-chloroethyl) ether	6.306	93	115667	438.55	ng/ml		97
9) 2-Chlorophenol	6.365	128	113634	532.72	ng/ml		95
10) 1,3-Dichlorobenzene	6.514	146	126152	546.89	ng/ml		98
11) 1,4-Dichlorobenzene	6.589	146	123497	551.64	ng/ml		99
12) Benzyl alcohol	6.702	108	59263	433.33	ng/ml		97
13) 1,2-Dichlorobenzene	6.739	146	124976	555.38	ng/ml		99
14) 2-Methylphenol	6.808	107	86329	503.48	ng/ml		99
15) 2,2'-Oxybis(1-Chloropr...	6.835	45	112933	331.95	ng/ml		97
16) N-Nitrosodi-n-propylamine	6.964	70	74700	432.29	ng/ml		99
17) 3+4-Methylphenol	6.958	107	107685	509.59	ng/ml		99
18) Hexachloroethane	7.076	201	36961	599.67	ng/ml		99
20) Nitrobenzene	7.129	77	100238	419.13	ng/ml		95
22) Isophorone	7.370	82	207804	470.36	ng/ml		99
23) 2-Nitrophenol	7.450	139	54694	414.23	ng/ml		98
24) 2,4-Dimethylphenol	7.488	122	86093	511.06	ng/ml		97
25) Bis(2-chloroethoxy) me...	7.579	93	131344	533.62	ng/ml		98
26) Benzoic acid	7.605	105	979	314.37	ng/ml#		66
27) 2,4-Dichlorophenol	7.691	162	89833	615.41	ng/ml		98
28) 1,2,4-Trichlorobenzene	7.777	180	113367	641.50	ng/ml		99
29) Naphthalene	7.857	128	361018	577.32	ng/ml		99
30) 4-Chloroaniline	7.905	127	106945	650.30	ng/ml		98
31) Hexachlorobutadiene	7.991	225	61063	647.92	ng/ml		98
32) 4-Chloro-3-methylphenol	8.386	107	84667	481.59	ng/ml	100	
33) 2-Methylnaphthalene	8.557	142	253485	593.76	ng/ml		98
34) 1-Methylnaphthalene	8.659	142	244797	596.63	ng/ml		99
36) Hexachlorocyclopentadiene	8.723	237	51180	517.04	ng/ml		98
37) 2,4,6-Trichlorophenol	8.841	196	59985	553.45	ng/ml		98
38) 2,4,5-Trichlorophenol	8.873	198	59608	560.44	ng/ml		98
39) 1,1'-Biphenyl	9.028	154	300735	578.68	ng/ml		99
41) 2-Chloronaphthalene	9.050	162	223930	587.06	ng/ml		97
42) 2-Nitroaniline	9.146	138	55795	439.35	ng/ml		98
43) 2,6-Dimethylnaphthalene	9.189	156	219677	564.67	ng/ml		99

*see MS*

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191922.D  
 Acq On : 20 Sep 2019 3:44 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL5  
 Misc : 1x, A19G242@500  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:39 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.274	168	19841	334.66	ng/ml	93
45) Dimethyl phthalate	9.328	163	250192	559.21	ng/ml	100
46) 1,3-Dinitrobenzene	9.354	168	28132	413.82	ng/ml	96
47) 2,6-Dinitrotoluene	9.387	165	51160	531.66	ng/ml	94
48) 1,2-Dinitrobenzene	9.445	168	22807	506.03	ng/ml	94
49) Acenaphthylene	9.472	152	361152	590.67	ng/ml	99
50) 3-Nitroaniline	9.558	138	44178	446.02	ng/ml	100
51) Acenaphthene	9.649	153	224540	566.51	ng/ml	99
52) 2,4-Dinitrophenol	9.665	184	4568	255.77	ng/ml	95
53) 4-Nitrophenol	9.723	139	25654	375.44	ng/ml	94
54) 2,4-Dinitrotoluene	9.798	165	57760	466.41	ng/ml	98
55) Dibenzofuran	9.825	168	310051	573.66	ng/ml	98
56) 2,3,5,6-Tetrachlorophenol	9.905	232	46260	542.89	ng/ml	99
57) 2,3,4,6-Tetrachlorophenol	9.948	232	50476	572.73	ng/ml	99
58) Diethyl phthalate	10.044	149	232776	545.61	ng/ml	99
59) 2,3,5-Trimethylnaphtha...	10.034	170	199252	576.75	ng/ml	99
60) Fluorene	10.173	166	244304	573.93	ng/ml	97
61) 4-Chlorophenyl phenyl ...	10.167	204	117369	593.31	ng/ml	99
62) 4-Nitroaniline	10.178	138	36541	423.99	ng/ml	96
63) 4,6-Dinitro-2-methylph...	10.216	198	14208	319.68	ng/ml	90
65) N-Nitrosodiphenylamine	10.285	169	197334	571.35	ng/ml	99
66) Azobenzene (1,2-DPH)	10.328	77	199437	435.30	ng/ml	99
68) 4-Bromophenyl phenyl e...	10.670	248	66857	578.28	ng/ml	97
69) Hexachlorobenzene	10.745	284	82813	622.55	ng/ml	99
70) Pentachlorophenol (PCP)	10.938	266	30348	512.59	ng/ml	94
71) Phenanthrene	11.157	178	343840	559.91	ng/ml	98
72) Anthracene	11.205	178	335865	555.84	ng/ml	99
73) Carbazole	11.366	167	281210	563.69	ng/ml	99
74) Di-n-butyl phthalate	11.719	149	369981	528.41	ng/ml	99
75) Fluoranthene	12.425	202	369455	575.22	ng/ml	98
76) Benzidine	12.580	184	152022	962.70	ng/ml	100
77) Pyrene	12.713	202	375136	584.68	ng/ml	99
80) Butyl benzyl phthalate	13.735	149	139695	388.99	ng/ml	98
81) Bis(2-ethylhexyl) adipate	13.911	129	126449	392.82	ng/ml	98
82) 3,3-Dichlorobenzidine	14.858	252	110907	1341.90	ng/ml	97
83) Benz(a)anthracene	14.890	228	327557	487.16	ng/ml	98
84) Chrysene	14.970	228	313539	505.43	ng/ml	99
85) Bis(2-ethylhexyl) phth...	15.077	149	202494	426.28	ng/ml	96
87) Di-n-octyl phthalate	16.746	149	281414	361.89	ng/ml	98
88) Benzo(b)fluoranthene	17.479	252	318669	457.74	ng/ml	99
89) Benzo(k)fluoranthene	17.543	252	321918	487.31	ng/ml	99
90) Benzo(b+k)fluoranthene	17.543	252	653019	943.99	ng/ml	99
91) Benzo(e)pyrene	18.132	252	316818	464.95	ng/ml	99
92) Benzo(a)pyrene	18.249	252	295305	471.49	ng/ml	97
93) Perylene	18.452	252	273199	460.10	ng/ml	100
95) Indeno(1,2,3-cd)pyrene	20.784	276	279363	520.62	ng/ml	99
96) Dibenz(a,h)anthracene	20.859	278	270778	562.60	ng/ml	97
97) Benzo(g,h,i)perylene	21.325	276	291609	564.45	ng/ml	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed



Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191922.D  
 Acq On : 20 Sep 2019 3:44 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL5  
 Misc : 1x, A19G242@500  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:39 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191922.D\data.ms

~~(26) Benzoic acid (T)~~

~~7.605min (+ 0.027) 314.37 ng/ml~~




~~response 979~~

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	66.67
77.00	72.00	109.78#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191922.D  
 Acq On : 20 Sep 2019 3:44 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL5  
 Misc : 1x, A19G242@500  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:39 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191922.D\data.ms

(26) Benzoic acid (T)

7.547min (-0.032) 552.34 ng/ml m


response 22389

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	83.94
77.00	72.00	66.43
0.00	0.00	0.00

*Handwritten signature and date: 9/20/19*

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191922.D  
 Acq On : 20 Sep 2019 3:44 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL5  
 Misc : 1x, A19G242@500  
 ALS Vial : 7 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:39 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191923.D  
 Acq On : 20 Sep 2019 4:19 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL6  
 Misc : 1x, A19G243@1000  
 ALS Vial : 8 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:43 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*Handwritten signature: JH 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.568	152	283511	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.835	136	1143968	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.616	162	583825	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.135	188	1065192	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.917	240	1048464	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	18.399	264	1042709	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.795	292	886236	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.289	112	179108	931.44	ng/ml	0.00	
5) Phenol-d6 (Surr)	6.204	99	238398	965.20	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	7.113	82	187377	827.84	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.926	172	482290	1124.97	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.419	330	65055	1301.74	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.922	244	507926	991.00	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.883	74	104763m	795.26	ng/ml		
3) Pyridine	3.904	79	182180	811.23	ng/ml	100	
6) Phenol	6.215	94	261231	930.43	ng/ml	100	
7) Aniline	6.241	93	189393	754.62	ng/ml	100	
8) Bis(2-chloroethyl) ether	6.306	93	237931	951.45	ng/ml	100	
9) 2-Chlorophenol	6.364	128	213396	1055.12	ng/ml	100	
10) 1,3-Dichlorobenzene	6.514	146	230358	1053.27	ng/ml	100	
11) 1,4-Dichlorobenzene	6.584	146	229877	1082.99	ng/ml	100	
12) Benzyl alcohol	6.701	108	124850	962.84	ng/ml	100	
13) 1,2-Dichlorobenzene	6.739	146	227139	1064.59	ng/ml	100	
14) 2-Methylphenol	6.808	107	162716	1000.89	ng/ml	100	
15) 2,2'-Oxybis(1-Chloropr...	6.835	45	204366	633.56	ng/ml	100	
16) N-Nitrosodi-n-propylamine	6.963	70	136460	832.90	ng/ml	100	
17) 3+4-Methylphenol	6.958	107	206745	1031.88	ng/ml	100	
18) Hexachloroethane	7.076	201	68545	1172.94	ng/ml	100	
20) Nitrobenzene	7.129	77	188065	829.39	ng/ml	100	
22) Isophorone	7.370	82	377941	910.39	ng/ml	100	
23) 2-Nitrophenol	7.450	139	114845	900.33	ng/ml	100	
24) 2,4-Dimethylphenol	7.488	122	164250	1037.61	ng/ml	100	
25) Bis(2-chloroethoxy) me...	7.579	93	236290	1021.63	ng/ml	100	
26) Benzoic acid	7.579	105	99342	1429.28	ng/ml	100	
27) 2,4-Dichlorophenol	7.691	162	173249	1263.07	ng/ml	100	
28) 1,2,4-Trichlorobenzene	7.782	180	206953	1246.26	ng/ml	100	
29) Naphthalene	7.857	128	638989	1087.45	ng/ml	100	
30) 4-Chloroaniline	7.905	127	199585	1281.62	ng/ml	100	
31) Hexachlorobutadiene	7.990	225	113762	1284.60	ng/ml	100	
32) 4-Chloro-3-methylphenol	8.386	107	162469	983.46	ng/ml	100	
33) 2-Methylnaphthalene	8.557	142	453493	1130.47	ng/ml	100	
34) 1-Methylnaphthalene	8.659	142	430139	1115.66	ng/ml	100	
36) Hexachlorocyclopentadiene	8.728	237	99801	1080.30	ng/ml	100	
37) 2,4,6-Trichlorophenol	8.841	196	117480	1142.89	ng/ml	100	
38) 2,4,5-Trichlorophenol	8.873	198	113799	1146.47	ng/ml	100	
39) 1,1'-Biphenyl	9.028	154	533233	1099.40	ng/ml	100	
41) 2-Chloronaphthalene	9.049	162	386877	1086.74	ng/ml	100	
42) 2-Nitroaniline	9.146	138	113482	957.47	ng/ml	100	
43) 2,6-Dimethylnaphthalene	9.188	156	389863	1073.75	ng/ml	100	

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191923.D  
 Acq On : 20 Sep 2019 4:19 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL6  
 Misc : 1x, A19G243@1000  
 ALS Vial : 8 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Sep 20 09:46:43 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.274	168	44207	798.94	ng/ml	100
45) Dimethyl phthalate	9.333	163	449574	1076.67	ng/ml	100
46) 1,3-Dinitrobenzene	9.354	168	57342	903.80	ng/ml	100
47) 2,6-Dinitrotoluene	9.392	165	97373	1084.24	ng/ml	100
48) 1,2-Dinitrobenzene	9.445	168	45222	1075.08	ng/ml	100
49) Acenaphthylene	9.472	152	637470	1117.11	ng/ml	100
50) 3-Nitroaniline	9.563	138	76212	868.39	ng/ml	100
51) Acenaphthene	9.648	153	399993	1081.31	ng/ml	100
52) 2,4-Dinitrophenol	9.664	184	18042	611.46	ng/ml	100
53) 4-Nitrophenol	9.723	139	58727	860.32	ng/ml	100
54) 2,4-Dinitrotoluene	9.798	165	116247	1005.79	ng/ml	100
55) Dibenzofuran	9.825	168	550893	1092.13	ng/ml	100
56) 2,3,5,6-Tetrachlorophenol	9.905	232	91879	1120.36	ng/ml	100
57) 2,3,4,6-Tetrachlorophenol	9.948	232	101167	1210.65	ng/ml	100
58) Diethyl phthalate	10.050	149	426259	1070.54	ng/ml	100
59) 2,3,5-Trimethylnaphtha...	10.039	170	355247	1101.79	ng/ml	100
60) Fluorene	10.173	166	426158	1072.71	ng/ml	100
61) 4-Chlorophenyl phenyl ...	10.167	204	209713	1135.90	ng/ml	100
62) 4-Nitroaniline	10.183	138	63138	784.97	ng/ml	100
63) 4,6-Dinitro-2-methylph...	10.215	198	38878	789.70	ng/ml	100
65) N-Nitrosodiphenylamine	10.285	169	350586	1070.25	ng/ml	100
66) Azobenzene (1,2-DPH)	10.328	77	355316	817.68	ng/ml	100
68) 4-Bromophenyl phenyl e...	10.670	248	125621	1145.62	ng/ml	100
69) Hexachlorobenzene	10.745	284	152211	1206.46	ng/ml	100
70) Pentachlorophenol (PCP)	10.943	266	65122	1104.57	ng/ml	100
71) Phenanthrene	11.157	178	610421	1048.04	ng/ml	100
72) Anthracene	11.210	178	608748	1062.21	ng/ml	100
73) Carbazole	11.365	167	458747	969.56	ng/ml	100
74) Di-n-butyl phthalate	11.718	149	683398	1029.09	ng/ml	100
75) Fluoranthene	12.424	202	669325	1098.75	ng/ml	100
76) Benzidine	12.579	184	302104	1915.60	ng/ml	100
77) Pyrene	12.713	202	683508	1123.21	ng/ml	100
80) Butyl benzyl phthalate	13.735	149	279356	850.79	ng/ml	100
81) Bis(2-ethylhexyl) adipate	13.911	129	247877	842.20	ng/ml	100
82) 3,3-Dichlorobenzidine	14.863	252	174855	2557.16	ng/ml	100
83) Benz(a)anthracene	14.890	228	577553	939.45	ng/ml	100
84) Chrysene	14.976	228	556735	981.58	ng/ml	100
85) Bis(2-ethylhexyl) phth...	15.072	149	389483	896.77	ng/ml	100
87) Di-n-octyl phthalate	16.746	149	592055	790.12	ng/ml	100
88) Benzo(b)fluoranthene	17.479	252	578435	915.95	ng/ml	100
89) Benzo(k)fluoranthene	17.548	252	582389	971.88	ng/ml	100
90) Benzo(b+k)fluoranthene	17.548	252	1182652	1884.67	ng/ml	100
91) Benzo(e)pyrene	18.137	252	576088	932.03	ng/ml	100
92) Benzo(a)pyrene	18.254	252	535317	942.21	ng/ml	100
93) Perylene	18.458	252	476752	885.12	ng/ml	100
95) Indeno(1,2,3-cd)pyrene	20.790	276	510691	1025.03	ng/ml	100
96) Dibenz(a,h)anthracene	20.865	278	489557	1095.51	ng/ml	100
97) Benzo(g,h,i)perylene	21.325	276	538150	1121.91	ng/ml	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
Data File : J09191923.D  
Acq On : 20 Sep 2019 4:19 am  
Operator : JK/ AMS/ DTH  
Sample : 9I19035-CAL6  
Misc : 1x, A19G243@1000  
ALS Vial : 8 Sample Multiplier: 1  
DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:43 2019  
Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
Quant Title : EPA 8270D: Semivolatile Organics  
QLast Update : Fri Sep 20 09:45:16 2019  
Response via : Initial Calibration  
InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191924.D  
 Acq On : 20 Sep 2019 4:54 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL7  
 Misc : 1x, A19G244@2000  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:48 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*JK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.573	152	285023	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.841	136	1095362	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.622	162	586466	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.135	188	1091855	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.922	240	1089712	2000.00	ng/ml	0.00	
86) Perylene-d12 (ISTD)	18.404	264	1076142	2000.00	ng/ml	0.00	
94) Dibenz(a,h)Anthrcene-d...	20.800	292	949148	2000.00	ng/ml	0.00	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.305	112	379802	1964.65	ng/ml	0.02	
5) Phenol-d6 (Surr)	6.209	99	477001	1920.99	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	7.113	82	365358	1605.60	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.926	172	917452	2130.37	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.424	330	142266	2777.20	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.927	244	1038865	1950.18	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.941	74	217151	1639.66	ng/ml		99
3) Pyridine	3.958	79	392152m	1736.94	ng/ml		
6) Phenol	6.220	94	506313	1793.78	ng/ml		98
7) Aniline	6.252	93	321662	1274.83	ng/ml		97
8) Bis(2-chloroethyl) ether	6.311	93	501220	1993.67	ng/ml		99
9) 2-Chlorophenol	6.370	128	423147	2081.13	ng/ml		99
10) 1,3-Dichlorobenzene	6.519	146	464902	2114.40	ng/ml		99
11) 1,4-Dichlorobenzene	6.589	146	453326	2124.37	ng/ml		99
12) Benzyl alcohol	6.707	108	261354	2004.87	ng/ml		98
13) 1,2-Dichlorobenzene	6.744	146	442316	2062.13	ng/ml		99
14) 2-Methylphenol	6.814	107	318341	1947.77	ng/ml		96
15) 2,2'-Oxybis(1-Chloropr...	6.840	45	366117	1128.98	ng/ml		97
16) N-Nitrosodi-n-propylamine	6.969	70	256713	1558.56	ng/ml		99
17) 3+4-Methylphenol	6.963	107	399183	1981.79	ng/ml		98
18) Hexachloroethane	7.076	201	143490	2442.36	ng/ml		97
20) Nitrobenzene	7.135	77	365107	1601.63	ng/ml		98
22) Isophorone	7.375	82	734609	1848.05	ng/ml		100
23) 2-Nitrophenol	7.456	139	207149	1710.18	ng/ml		94
24) 2,4-Dimethylphenol	7.493	122	333523	2200.44	ng/ml		97
25) Bis(2-chloroethoxy) me...	7.584	93	449978	2031.87	ng/ml		99
26) Benzoic acid	7.611	105	311714	3637.31	ng/ml		96
27) 2,4-Dichlorophenol	7.691	162	350635	2669.74	ng/ml		98
28) 1,2,4-Trichlorobenzene	7.782	180	388384	2442.61	ng/ml		100
29) Naphthalene	7.862	128	1178988	2095.46	ng/ml		99
30) 4-Chloroaniline	7.915	127	372183	2483.94	ng/ml		99
31) Hexachlorobutadiene	7.990	225	208693	2461.13	ng/ml		98
32) 4-Chloro-3-methylphenol	8.392	107	338452	2139.63	ng/ml		97
33) 2-Methylnaphthalene	8.557	142	857631	2232.77	ng/ml		98
34) 1-Methylnaphthalene	8.659	142	810434	2195.32	ng/ml		99
36) Hexachlorocyclopentadiene	8.723	237	213088	2296.19	ng/ml		97
37) 2,4,6-Trichlorophenol	8.841	196	248218	2364.26	ng/ml		100
38) 2,4,5-Trichlorophenol	8.873	198	245074	2457.78	ng/ml		99
39) 1,1'-Biphenyl	9.028	154	1010736	2074.51	ng/ml		98
41) 2-Chloronaphthalene	9.049	162	759926	2125.02	ng/ml		100
42) 2-Nitroaniline	9.151	138	248865	2090.27	ng/ml		95
43) 2,6-Dimethylnaphthalene	9.188	156	740663	2030.74	ng/ml		100

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191924.D  
 Acq On : 20 Sep 2019 4:54 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL7  
 Misc : 1x, A19G244@2000  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:48 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.279	168	108019	1943.39	ng/ml	94
45) Dimethyl phthalate	9.338	163	868820	2071.34	ng/ml	99
46) 1,3-Dinitrobenzene	9.360	168	128986	2023.86	ng/ml	95
47) 2,6-Dinitrotoluene	9.392	165	201552	2234.16	ng/ml	96
48) 1,2-Dinitrobenzene	9.451	168	94079	2226.50	ng/ml	97
49) Acenaphthylene	9.477	152	1211941	2114.25	ng/ml	99
50) 3-Nitroaniline	9.563	138	114743	1447.64	ng/ml	96
51) Acenaphthene	9.654	153	770675	2074.00	ng/ml	99
52) 2,4-Dinitrophenol	9.670	184	58400	1570.56	ng/ml	93
53) 4-Nitrophenol	9.729	139	141903	1959.29	ng/ml	98
54) 2,4-Dinitrotoluene	9.804	165	257547	2218.31	ng/ml	97
55) Dibenzofuran	9.825	168	1086183	2143.62	ng/ml	98
56) 2,3,5,6-Tetrachlorophenol	9.905	232	201504	2389.21	ng/ml	99
57) 2,3,4,6-Tetrachlorophenol	9.953	232	213539	2500.78	ng/ml	97
58) Diethyl phthalate	10.055	149	811497	2028.87	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	10.039	170	685050	2115.10	ng/ml	99
60) Fluorene	10.178	166	812478	2035.94	ng/ml	100
61) 4-Chlorophenyl phenyl ...	10.173	204	412942	2226.61	ng/ml	94
62) 4-Nitroaniline	10.189	138	129234	1599.47	ng/ml	95
63) 4,6-Dinitro-2-methylph...	10.221	198	101854	1883.45	ng/ml	99
65) N-Nitrosodiphenylamine	10.290	169	659355	1963.69	ng/ml	97
66) Azobenzene (1,2-DPH)	10.333	77	684303	1536.31	ng/ml	93
68) 4-Bromophenyl phenyl e...	10.670	248	256334	2280.59	ng/ml	96
69) Hexachlorobenzene	10.750	284	304969	2358.22	ng/ml	98
70) Pentachlorophenol (PCP)	10.943	266	154858	2438.76	ng/ml	99
71) Phenanthrene	11.157	178	1191270	1995.35	ng/ml	99
72) Anthracene	11.210	178	1187408	2021.33	ng/ml	98
73) Carbazole	11.365	167	646631	1333.27	ng/ml	99
74) Di-n-butyl phthalate	11.718	149	1348435	1980.94	ng/ml	100
75) Fluoranthene	12.430	202	1341415	2148.26	ng/ml	98
76) Benzidine	12.585	184	601547	3540.61	ng/ml	100
77) Pyrene	12.719	202	1337637	2144.45	ng/ml	98
80) Butyl benzyl phthalate	13.740	149	621242	1820.39	ng/ml	96
81) Bis(2-ethylhexyl) adipate	13.917	129	551677	1803.46	ng/ml	99
82) 3,3-Dichlorobenzidine	14.863	252	281736	4236.61	ng/ml	94
83) Benz(a)anthracene	14.895	228	1225586	1918.11	ng/ml	99
84) Chrysene	14.981	228	1148470	1948.23	ng/ml	99
85) Bis(2-ethylhexyl) phth...	15.077	149	846014	1874.18	ng/ml	98
87) Di-n-octyl phthalate	16.746	149	1439135	1774.42	ng/ml	99
88) Benzo(b)fluoranthene	17.490	252	1267321	1944.46	ng/ml	99
89) Benzo(k)fluoranthene	17.554	252	1256906	2032.34	ng/ml	98
90) Benzo(b+k)fluoranthene	17.554	252	2563432	3958.17	ng/ml	98
91) Benzo(e)pyrene	18.142	252	1218818	1910.61	ng/ml	98
92) Benzo(a)pyrene	18.260	252	1174506	2003.02	ng/ml	99
93) Perylene	18.468	252	1026574	1846.69	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.800	276	1143875	2143.74	ng/ml	99
96) Dibenz(a,h)anthracene	20.875	278	1087002	2271.22	ng/ml	97
97) Benzo(g,h,i)perylene	21.341	276	1186793	2310.13	ng/ml	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191924.D  
 Acq On : 20 Sep 2019 4:54 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL7  
 Misc : 1x, A19G244@2000  
 ALS Vial : 9 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:48 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191925.D  
 Acq On : 20 Sep 2019 5:29 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL8  
 Misc : 1x, A19G245@4000  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:52 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*JK* 9/20/19

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.573	152	305814	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.841	136	1197569	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.622	162	636039	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.135	188	1224924	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.938	240	1138264	2000.00	ng/ml	0.02	
86) Perylene-d12 (ISTD)	18.420	264	1185024	2000.00	ng/ml	0.02	
94) Dibenz(a,h)Anthrcene-d...	20.827	292	1037191	2000.00	ng/ml	0.03	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.305	112	844515	4071.54	ng/ml	0.02	
5) Phenol-d6 (Surr)	6.215	99	1043086	3915.14	ng/ml	0.01	
19) Nitrobenzene-d5 (Surr)	7.124	82	786633	3221.91	ng/ml	0.01	
40) 2-Fluorobiphenyl (Surr)	8.932	172	1718307	3679.02	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.429	330	305471	5315.35	ng/ml	0.01	
79) Terphenyl-d14 (Surr)	12.938	244	2102593	3778.67	ng/ml	0.02	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.925	74	480484	3381.37	ng/ml		99
3) Pyridine	3.942	79	866960	3578.93	ng/ml		99
6) Phenol	6.231	94	1097096	3622.58	ng/ml		98
7) Aniline	6.252	93	840844	3105.93	ng/ml		96
8) Bis(2-chloroethyl) ether	6.316	93	962255	3567.28	ng/ml		99
9) 2-Chlorophenol	6.370	128	902056	4134.88	ng/ml		98
10) 1,3-Dichlorobenzene	6.520	146	965051	4090.70	ng/ml		99
11) 1,4-Dichlorobenzene	6.589	146	926647	4047.22	ng/ml		99
12) Benzyl alcohol	6.712	108	581465	4157.22	ng/ml		99
13) 1,2-Dichlorobenzene	6.744	146	906070	3937.01	ng/ml		99
14) 2-Methylphenol	6.814	107	646688	3687.77	ng/ml		98
15) 2,2'-Oxybis(1-Chloropr...	6.840	45	739481	2125.28	ng/ml		94
16) N-Nitrosodi-n-propylamine	6.980	70	504346	2853.83	ng/ml		95
17) 3+4-Methylphenol	6.969	107	797964	3692.25	ng/ml		97
18) Hexachloroethane	7.076	201	311702	4944.82	ng/ml		98
20) Nitrobenzene	7.140	77	754990	3086.77	ng/ml		95
22) Isophorone	7.381	82	1524753	3508.45	ng/ml		100
23) 2-Nitrophenol	7.456	139	481353	3856.12	ng/ml		95
24) 2,4-Dimethylphenol	7.498	122	686286	4141.39	ng/ml		98
25) Bis(2-chloroethoxy) me...	7.589	93	900203	3717.94	ng/ml		99
26) Benzoic acid	7.498	105	22439	556.98	ng/ml#		1
27) 2,4-Dichlorophenol	7.702	162	731346	5093.24	ng/ml		98
28) 1,2,4-Trichlorobenzene	7.782	180	805154	4631.57	ng/ml		99
29) Naphthalene	7.862	128	2214900	3600.66	ng/ml		97
30) 4-Chloroaniline	7.926	127	663200	4035.49	ng/ml		99
31) Hexachlorobutadiene	7.990	225	442903	4777.41	ng/ml		97
32) 4-Chloro-3-methylphenol	8.392	107	698064	4036.41	ng/ml		97
33) 2-Methylnaphthalene	8.563	142	1625949	3871.75	ng/ml		97
34) 1-Methylnaphthalene	8.664	142	1521185	3768.94	ng/ml		99
36) Hexachlorocyclopentadiene	8.729	237	417829	4151.52	ng/ml		96
37) 2,4,6-Trichlorophenol	8.846	196	532499	4570.85	ng/ml		99
38) 2,4,5-Trichlorophenol	8.878	198	516958	4780.35	ng/ml		99
39) 1,1'-Biphenyl	9.033	154	1845876	3493.33	ng/ml		96
41) 2-Chloronaphthalene	9.055	162	1467799	3784.57	ng/ml		99
42) 2-Nitroaniline	9.156	138	528406	4092.28	ng/ml		94
43) 2,6-Dimethylnaphthalene	9.194	156	1385514	3502.70	ng/ml		97

See MS

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191925.D  
 Acq On : 20 Sep 2019 5:29 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL8  
 Misc : 1x, A19G245@4000  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:52 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.285	168	258106	4281.72	ng/ml	92
45) Dimethyl phthalate	9.349	163	1712764	3765.11	ng/ml	98
46) 1,3-Dinitrobenzene	9.370	168	289563	4189.29	ng/ml	93
47) 2,6-Dinitrotoluene	9.402	165	424265	4336.35	ng/ml	97
48) 1,2-Dinitrobenzene	9.467	168	202294	4414.41	ng/ml	92
49) Acenaphthylene	9.483	152	2224222	3577.77	ng/ml	97
50) 3-Nitroaniline	9.574	138	123216	1427.55	ng/ml	97
51) Acenaphthene	9.659	153	1433796	3557.81	ng/ml	99
52) 2,4-Dinitrophenol	9.675	184	174238	3652.38	ng/ml	99
53) 4-Nitrophenol	9.739	139	326661	3903.35	ng/ml	98
54) 2,4-Dinitrotoluene	9.814	165	555824	4414.31	ng/ml	93
55) Dibenzofuran	9.830	168	2040744	3713.59	ng/ml	95
56) 2,3,5,6-Tetrachlorophenol	9.911	232	434819	4639.23	ng/ml	97
57) 2,3,4,6-Tetrachlorophenol	9.959	232	451267	4758.24	ng/ml	95
58) Diethyl phthalate	10.060	149	1534521	3537.53	ng/ml	96
59) 2,3,5-Trimethylnaphtha...	10.044	170	1276533	3634.12	ng/ml	98
60) Fluorene	10.183	166	1464263	3383.22	ng/ml	99
61) 4-Chlorophenyl phenyl ...	10.173	204	786385	3909.75	ng/ml	95
62) 4-Nitroaniline	10.199	138	281600	3213.60	ng/ml	99
63) 4,6-Dinitro-2-methylph...	10.232	198	258196	4046.65	ng/ml	96
65) N-Nitrosodiphenylamine	10.296	169	1182676	3139.61	ng/ml	98
66) Azobenzene (1,2-DPH)	10.338	77	1316342	2634.24	ng/ml	87
68) 4-Bromophenyl phenyl e...	10.675	248	546207	4331.66	ng/ml	97
69) Hexachlorobenzene	10.750	284	617226	4254.30	ng/ml	98
70) Pentachlorophenol (PCP)	10.943	266	363768	4791.33	ng/ml	99
71) Phenanthrene	11.162	178	2302690	3437.96	ng/ml	97
72) Anthracene	11.216	178	2312152	3508.40	ng/ml	96
73) Carbazole	11.371	167	858655	1578.11	ng/ml	99
74) Di-n-butyl phthalate	11.724	149	2651399	3471.94	ng/ml	98
75) Fluoranthene	12.435	202	2665095	3804.46	ng/ml	97
76) Benzidine	12.596	184	1506619	7251.57	ng/ml	99
77) Pyrene	12.729	202	2681088	3831.29	ng/ml	95
80) Butyl benzyl phthalate	13.751	149	1344154	3770.70	ng/ml	94
81) Bis(2-ethylhexyl) adipate	13.922	129	1183408	3703.61	ng/ml	99
82) 3,3-Dichlorobenzidine	14.879	252	448650	6944.09	ng/ml	96
83) Benz(a)anthracene	14.912	228	2538581	3803.56	ng/ml	99
84) Chrysene	15.003	228	2370714	3850.07	ng/ml	96
85) Bis(2-ethylhexyl) phth...	15.088	149	1799096	3815.54	ng/ml	97
87) Di-n-octyl phthalate	16.762	149	3203842	3414.68	ng/ml	99
88) Benzo(b)fluoranthene	17.516	252	2803227	3905.83	ng/ml	98
89) Benzo(k)fluoranthene	17.586	252	2555733	3752.77	ng/ml	99
90) Benzo(b+k)fluoranthene	17.586	252	5439284	7627.06	ng/ml	99
91) Benzo(e)pyrene	18.174	252	2630004	3743.97	ng/ml	99
92) Benzo(a)pyrene	18.292	252	2485829	3849.85	ng/ml	99
93) Perylene	18.500	252	2164033	3535.17	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.838	276	2539375	4355.08	ng/ml	98
96) Dibenz(a,h)anthracene	20.902	278	2389624	4569.13	ng/ml	98
97) Benzo(g,h,i)perylene	21.378	276	2579448	4594.87	ng/ml	98




See m5

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191925.D  
 Acq On : 20 Sep 2019 5:29 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL8  
 Misc : 1x, A19G245@4000  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:52 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191925.D\data.ms

(26) Benzoic acid (T)

7.498min (-0.080) 556.98 ng/ml




response 22439

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	2944.12#
77.00	72.00	841.49#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191925.D  
 Acq On : 20 Sep 2019 5:29 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL8  
 Misc : 1x, A19G245@4000  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:52 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191925.D\data.ms

(26) Benzoic acid (T)




7.670min (+ 0.091) 7780.16 ng/ml m *md 9/20/19*

response	902544
Ion	Exp% Act%
105.00	100.00 100.00
122.00	90.90 85.67
77.00	72.00 68.01
0.00	0.00 0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191925.D  
 Acq On : 20 Sep 2019 5:29 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL8  
 Misc : 1x, A19G245@4000  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:52 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

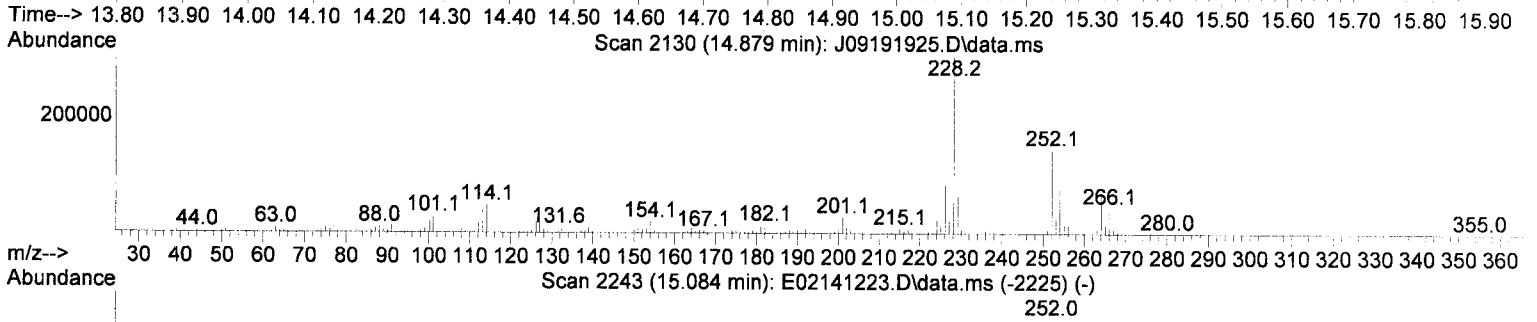




TIC: J09191925.D\data.ms

(82)	3,3-Dichlorobenzidine (T)	
14.879min (+ 0.016)	6944.09 ng/ml	
response	448650	
Ion	Exp%	Act%
252.00	100.00	100.00
254.00	66.30	63.38
126.00	12.00	13.81
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191925.D  
 Acq On : 20 Sep 2019 5:29 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL8  
 Misc : 1x, A19G245@4000  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:52 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191925.D\data.ms

(82) 3,3-Dichlorobenzidine (T)

14.879min (+ 0.016) 9026.86 ng/ml


*JK 9/20/19*

response 555604

Ion	Exp%	Act%
252.00	100.00	100.00
254.00	66.30	63.38
126.00	12.00	13.81
0.00	0.00	0.00

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191925.D  
 Acq On : 20 Sep 2019 5:29 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL8  
 Misc : 1x, A19G245@4000  
 ALS Vial : 10 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:52 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10





Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191926.D  
 Acq On : 20 Sep 2019 6:04 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL9  
 Misc : 1x, A19G246@6000  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*JK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.568	152	279602	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.841	136	1094080	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.622	162	593235	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.141	188	1148482	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.944	240	1022230	2000.00	ng/ml	0.03	
86) Perylene-d12 (ISTD)	18.426	264	1067597	2000.00	ng/ml	0.03	
94) Dibenz(a,h)Anthrcene-d...	20.838	292	945822	2000.00	ng/ml	0.04	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.295	112	1150405	6066.23	ng/ml	0.00	
5) Phenol-d6 (Surr)	6.215	99	1391310	5711.74	ng/ml	0.01	
19) Nitrobenzene-d5 (Surr)	7.124	82	1045001	4681.39	ng/ml	0.01	
40) 2-Fluorobiphenyl (Surr)	8.932	172	2148364	4931.70	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.429	330	407389	7560.59	ng/ml	0.01	
79) Terphenyl-d14 (Surr)	12.938	244	2699067	5401.22	ng/ml	0.02	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.883	74	674636m	5192.78	ng/ml		
3) Pyridine	3.893	79	1210013m	5463.38	ng/ml		
6) Phenol	6.231	94	1432862	5174.81	ng/ml		98
7) Aniline	6.252	93	1316393	5318.37	ng/ml		95
8) Bis(2-chloroethyl) ether	6.316	93	1158478	4697.35	ng/ml		99
9) 2-Chlorophenol	6.370	128	1211719	6075.04	ng/ml		99
10) 1,3-Dichlorobenzene	6.520	146	1260484	5843.89	ng/ml		100
11) 1,4-Dichlorobenzene	6.589	146	1202300	5743.45	ng/ml		99
12) Benzyl alcohol	6.712	108	768204	6007.21	ng/ml		98
13) 1,2-Dichlorobenzene	6.739	146	1159865	5512.26	ng/ml		99
14) 2-Methylphenol	6.819	107	839569	5236.51	ng/ml		98
15) 2,2'-Oxybis(1-Chloropr...	6.841	45	943818	2966.84	ng/ml		91
16) N-Nitrosodi-n-propylamine	6.985	70	644101	3986.31	ng/ml		94
17) 3+4-Methylphenol	6.974	107	997248	5046.94	ng/ml		99
18) Hexachloroethane	7.076	201	419784	7283.73	ng/ml		95
20) Nitrobenzene	7.145	77	977466	4371.02	ng/ml		92
22) Isophorone	7.386	82	2075603	5227.70	ng/ml		100
23) 2-Nitrophenol	7.461	139	659170	6267.15	ng/ml		93
24) 2,4-Dimethylphenol	7.504	122	932922	6162.23	ng/ml		98
25) Bis(2-chloroethoxy) me...	7.589	93	1142883	5166.72	ng/ml		98
26) Benzoic acid	7.579	105	96795	1449.32	ng/ml		96
27) 2,4-Dichlorophenol	7.702	162	943067	7188.94	ng/ml		98
28) 1,2,4-Trichlorobenzene	7.787	180	1041502	6557.84	ng/ml		100
29) Naphthalene	7.867	128	2711030	4824.07	ng/ml		95
30) 4-Chloroaniline	7.926	127	906180	6017.35	ng/ml		100
31) Hexachlorobutadiene	7.996	225	570722	6738.45	ng/ml		98
32) 4-Chloro-3-methylphenol	8.397	107	912303	5774.18	ng/ml		93
33) 2-Methylnaphthalene	8.563	142	2034929	5303.97	ng/ml		97
34) 1-Methylnaphthalene	8.664	142	1893325	5134.69	ng/ml		98
36) Hexachlorocyclopentadiene	8.729	237	601203	6404.52	ng/ml		95
37) 2,4,6-Trichlorophenol	8.846	196	713503	6449.67	ng/ml		99
38) 2,4,5-Trichlorophenol	8.884	198	699105	6931.12	ng/ml		99
39) 1,1'-Biphenyl	9.039	154	2268485	4602.89	ng/ml		95
41) 2-Chloronaphthalene	9.060	162	1860060	5142.02	ng/ml		98
42) 2-Nitroaniline	9.162	138	739914	6143.79	ng/ml		93
43) 2,6-Dimethylnaphthalene	9.199	156	1742370	4722.69	ng/ml		98

*See MI*

Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191926.D  
 Acq On : 20 Sep 2019 6:04 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL9  
 Misc : 1x, A19G246@6000  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.290	168	365105	6493.74	ng/ml	88
45) Dimethyl phthalate	9.354	163	2223667	5240.92	ng/ml	97
46) 1,3-Dinitrobenzene	9.381	168	407082	6314.46	ng/ml	91
47) 2,6-Dinitrotoluene	9.408	165	575872	6310.58	ng/ml	96
48) 1,2-Dinitrobenzene	9.472	168	266233	6228.85	ng/ml	93
49) Acenaphthylene	9.483	152	2704211	4663.72	ng/ml	95
50) 3-Nitroaniline	9.579	138	180797	Below Cal		97
51) Acenaphthene	9.659	153	1803278	4797.51	ng/ml	99
52) 2,4-Dinitrophenol	9.681	184	272053	5508.37	ng/ml	97
53) 4-Nitrophenol	9.745	139	467183	5690.24	ng/ml	97
54) 2,4-Dinitrotoluene	9.820	165	734363	6253.07	ng/ml	93
55) Dibenzofuran	9.836	168	2531005	4938.04	ng/ml	95
56) 2,3,5,6-Tetrachlorophenol	9.916	232	597064	6702.12	ng/ml	95
57) 2,3,4,6-Tetrachlorophenol	9.959	232	603345	6692.46	ng/ml	96
58) Diethyl phthalate	10.066	149	1916805	4737.64	ng/ml	94
59) 2,3,5-Trimethylnaphtha...	10.050	170	1592300	4860.15	ng/ml	97
60) Fluorene	10.189	166	1824399	4519.48	ng/ml	98
61) 4-Chlorophenyl phenyl ...	10.178	204	992417	5290.11	ng/ml	95
62) 4-Nitroaniline	10.205	138	385746	4719.73	ng/ml	97
63) 4,6-Dinitro-2-methylph...	10.237	198	377769	5981.86	ng/ml	95
65) N-Nitrosodiphenylamine	10.301	169	1569352	4443.39	ng/ml	97
66) Azobenzene (1,2-DPH)	10.339	77	1601806	3418.86	ng/ml	88
68) 4-Bromophenyl phenyl e...	10.681	248	726568	6145.51	ng/ml	92
69) Hexachlorobenzene	10.756	284	795928	5851.17	ng/ml	98
70) Pentachlorophenol (PCP)	10.948	266	500914	6716.78	ng/ml	99
71) Phenanthrene	11.168	178	2932288	4669.35	ng/ml	96
72) Anthracene	11.221	178	2907155	4704.86	ng/ml	96
73) Carbazole	11.371	167	1156567	2267.12	ng/ml	99
74) Di-n-butyl phthalate	11.729	149	3301933	4611.59	ng/ml	97
75) Fluoranthene	12.441	202	3417993	5203.99	ng/ml	96
76) Benzidine	12.601	184	2204013	10575.22	ng/ml	99
77) Pyrene	12.735	202	3436590	5237.78	ng/ml	95
80) Butyl benzyl phthalate	13.756	149	1779167	5557.56	ng/ml	93
81) Bis(2-ethylhexyl) adipate	13.933	129	1497303	5217.89	ng/ml	99
82) 3,3-Dichlorobenzidine	14.890	252	494238	8919.45	ng/ml	97
83) Benz(a)anthracene	14.917	228	3394067	5662.58	ng/ml	99
84) Chrysene	15.013	228	3095456	5597.68	ng/ml	97
85) Bis(2-ethylhexyl) phth...	15.093	149	2338505	5522.48	ng/ml	96
87) Di-n-octyl phthalate	16.773	149	4149203	4742.46	ng/ml	99
88) Benzo(b)fluoranthene	17.522	252	3768759	5828.72	ng/ml	99
89) Benzo(k)fluoranthene	17.602	252	3115398	5077.74	ng/ml	99
90) Benzo(b+k)fluoranthene	17.602	252	7129046	11096.00	ng/ml	99
91) Benzo(e)pyrene	18.185	252	3489142	5513.34	ng/ml	99
92) Benzo(a)pyrene	18.308	252	3235783	5562.53	ng/ml	100
93) Perylene	18.511	252	2908580	5274.09	ng/ml	99
95) Indeno(1,2,3-cd)pyrene	20.854	276	3489319	6562.35	ng/ml	97
96) Dibenz(a,h)anthracene	20.913	278	3129173	6561.19	ng/ml	99
97) Benzo(g,h,i)perylene	21.389	276	3417702	6676.22	ng/ml	97




*see MS*

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191926.D  
 Acq On : 20 Sep 2019 6:04 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL9  
 Misc : 1x, A19G246@6000  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191926.D\data.ms

(26) Benzoid acid (T)

7.579min (+ 0.000) 1449.32 ng/ml




response 96795

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	84.66
77.00	72.00	72.18
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191926.D  
 Acq On : 20 Sep 2019 6:04 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL9  
 Misc : 1x, A19G246@6000  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191926.D\data.ms

(26) Benzoic acid (T)




7.686min (+ 0.107) 10743.23 ng/ml *m* *JK 9/20/19*  
 response 1277463

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	87.13
77.00	72.00	68.78
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191926.D  
 Acq On : 20 Sep 2019 6:04 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL9  
 Misc : 1x, A19G246@6000  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191926.D\data.ms

(82) 3,3-Dichlorobenzidine (T)

14.890min (+ 0.027) 8919.45 ng/ml




response 494238

Ion	Exp%	Act%
252.00	100.00	100.00
254.00	66.30	63.96
126.00	12.00	13.33
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191926.D  
 Acq On : 20 Sep 2019 6:04 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL9  
 Misc : 1x, A19G246@6000  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191926.D\data.ms


(82) 3,3-Dichlorobenzidine (T)

14.890min (+ 0.027) 15215.95 ng/mL *OK 9/20/19*  
 response 730056

Ion	Exp%	Act%
252.00	100.00	100.00
254.00	66.30	63.96
126.00	12.00	13.33
0.00	0.00	0.00

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191926.D  
 Acq On : 20 Sep 2019 6:04 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CAL9  
 Misc : 1x, A19G246@6000  
 ALS Vial : 11 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:46:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*JK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.578	152	269345	2000.00	ng/ml	0.01	
21) Naphthalene-d8 (ISTD)	7.846	136	1074761	2000.00	ng/ml	0.01	
35) Acenaphthene-d10 (ISTD)	9.627	162	593771	2000.00	ng/ml	0.01	
64) Phenanthrene-d10 (ISTD)	11.135	188	1167219	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.933	240	1013392	2000.00	ng/ml	0.02	
86) Perylene-d12 (ISTD)	18.409	264	1108960	2000.00	ng/ml	0.01	
94) Dibenz(a,h)Anthrcene-d...	20.822	292	982889	2000.00	ng/ml	0.03	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.316	112	1458990	7986.41	ng/ml	0.03	
5) Phenol-d6 (Surr)	6.225	99	1721904	7338.12	ng/ml	0.02	
19) Nitrobenzene-d5 (Surr)	7.129	82	1284804	5974.84	ng/ml	0.02	
40) 2-Fluorobiphenyl (Surr)	8.937	172	2595271	5952.22	ng/ml	0.01	
67) 2,4,6-Tribromophenol (...)	10.435	330	524653	9580.55	ng/ml	0.02	
79) Terphenyl-d14 (Surr)	12.932	244	3392009	6847.09	ng/ml	0.01	
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	3.957	74	799031	6384.48	ng/ml	95	<i>See MS</i>
3) Pyridine	3.963	79	1480958m	6941.37	ng/ml#		
6) Phenol	6.247	94	1750392	6562.31	ng/ml	93	
7) Aniline	6.263	93	1480736	6210.15	ng/ml	95	
8) Bis(2-chloroethyl) ether	6.322	93	1435010	6040.20	ng/ml	98	
9) 2-Chlorophenol	6.375	128	1496104	7786.46	ng/ml	98	
10) 1,3-Dichlorobenzene	6.525	146	1570022	7556.17	ng/ml	99	
11) 1,4-Dichlorobenzene	6.594	146	1504749	7462.00	ng/ml	99	
12) Benzyl alcohol	6.723	108	932774	7571.89	ng/ml	99	
13) 1,2-Dichlorobenzene	6.744	146	1419977	7005.43	ng/ml	100	
14) 2-Methylphenol	6.824	107	1030806	6674.12	ng/ml	99	
15) 2,2'-Oxybis(1-Chloropr...	6.846	45	1103589	3601.18	ng/ml	87	
16) N-Nitrosodi-n-propylamine	6.995	70	803148	5159.93	ng/ml	94	
17) 3+4-Methylphenol	6.985	107	1205305	6332.18	ng/ml	99	
18) Hexachloroethane	7.081	201	541884	9760.36	ng/ml	92	
20) Nitrobenzene	7.151	77	1198679	5564.36	ng/ml	91	
22) Isophorone	7.397	82	2693969	6907.11	ng/ml	99	
23) 2-Nitrophenol	7.461	139	838038	8987.28	ng/ml	94	
24) 2,4-Dimethylphenol	7.509	122	1099526	7393.25	ng/ml	98	
25) Bis(2-chloroethoxy) me...	7.595	93	1380842	6354.69	ng/ml	98	
26) Benzoic acid	7.509	105	38011	776.83	ng/ml#	1	<i>See MS</i>
27) 2,4-Dichlorophenol	7.707	162	1167761	9061.78	ng/ml	97	
28) 1,2,4-Trichlorobenzene	7.787	180	1277566	8188.82	ng/ml	99	
29) Naphthalene	7.867	128	3240737	5870.30	ng/ml	95	
30) 4-Chloroaniline	7.931	127	1186251	7997.52	ng/ml	100	
31) Hexachlorobutadiene	7.996	225	701350	8429.61	ng/ml	98	
32) 4-Chloro-3-methylphenol	8.397	107	1141605	7355.36	ng/ml	93	
33) 2-Methylnaphthalene	8.563	142	2448839	6497.55	ng/ml	98	
34) 1-Methylnaphthalene	8.664	142	2286875	6313.48	ng/ml	98	
36) Hexachlorocyclopentadiene	8.728	237	759063	8078.87	ng/ml	96	
37) 2,4,6-Trichlorophenol	8.851	196	922776	8200.21	ng/ml	98	
38) 2,4,5-Trichlorophenol	8.884	198	870124	8618.86	ng/ml	98	
39) 1,1'-Biphenyl	9.039	154	2706900	5487.50	ng/ml	95	
41) 2-Chloronaphthalene	9.060	162	2240055	6186.91	ng/ml	98	
42) 2-Nitroaniline	9.167	138	944974	7839.40	ng/ml	90	
43) 2,6-Dimethylnaphthalene	9.199	156	2089018	5657.17	ng/ml	98	



Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.295	168	488295	8676.95	ng/ml	84
45) Dimethyl phthalate	9.360	163	2768841	6519.94	ng/ml	96
46) 1,3-Dinitrobenzene	9.386	168	525829	8149.05	ng/ml	91
47) 2,6-Dinitrotoluene	9.413	165	727325	7963.06	ng/ml	93
48) 1,2-Dinitrobenzene	9.477	168	322227	7532.10	ng/ml	94
49) Acenaphthylene	9.488	152	3146686	5421.92	ng/ml	95
50) 3-Nitroaniline	9.584	138	174843	Below Cal		96
51) Acenaphthene	9.664	153	2204696	5860.16	ng/ml	99
52) 2,4-Dinitrophenol	9.686	184	388560	7229.26	ng/ml	93
53) 4-Nitrophenol	9.755	139	610739	7150.14	ng/ml	97
54) 2,4-Dinitrotoluene	9.825	165	868405	7387.76	ng/ml	92
55) Dibenzofuran	9.836	168	3003141	5853.90	ng/ml	93
56) 2,3,5,6-Tetrachlorophenol	9.916	232	763806	8438.44	ng/ml	96
57) 2,3,4,6-Tetrachlorophenol	9.964	232	773723	8433.64	ng/ml	95
58) Diethyl phthalate	10.066	149	2319061	5726.69	ng/ml	94
59) 2,3,5-Trimethylnaphtha...	10.050	170	1931750	5890.92	ng/ml	99
60) Fluorene	10.189	166	2171368	5374.15	ng/ml	99
61) 4-Chlorophenyl phenyl ...	10.178	204	1192807	6352.55	ng/ml	94
62) 4-Nitroaniline	10.210	138	523369	6397.82	ng/ml	97
63) 4,6-Dinitro-2-methylph...	10.242	198	504056	7617.61	ng/ml	93
65) N-Nitrosodiphenylamine	10.306	169	1760214	4903.79	ng/ml	97
66) Azobenzene (1,2-DPH)	10.344	77	1950077	4095.39	ng/ml	78
68) 4-Bromophenyl phenyl e...	10.681	248	926306	7709.18	ng/ml	93
69) Hexachlorobenzene	10.756	284	1001688	7245.58	ng/ml	98
70) Pentachlorophenol (PCP)	10.948	266	646595	8238.97	ng/ml	98
71) Phenanthrene	11.167	178	3584429	5616.19	ng/ml	96
72) Anthracene	11.221	178	3477728	5537.91	ng/ml	95
73) Carbazole	11.371	167	1165062	2247.11	ng/ml	99
74) Di-n-butyl phthalate	11.724	149	4037361	5548.19	ng/ml	96
75) Fluoranthene	12.435	202	4158773	6230.20	ng/ml	95
76) Benzidine	12.595	184	3017555	13485.44	ng/ml	99
77) Pyrene	12.729	202	4271888	6406.36	ng/ml	95
80) Butyl benzyl phthalate	13.745	149	2308181	7272.91	ng/ml	91
81) Bis(2-ethylhexyl) adipate	13.917	129	1955106	6872.69	ng/ml	99
82) 3,3-Dichlorobenzidine	14.874	252	572542	10901.24	ng/ml	98
83) Benz(a)anthracene	14.906	228	4360504	7338.40	ng/ml	98
84) Chrysene	15.002	228	3992263	7282.39	ng/ml	96
85) Bis(2-ethylhexyl) phth...	15.083	149	2986931	7115.28	ng/ml	95
87) Di-n-octyl phthalate	16.751	149	5450180	5838.44	ng/ml	98
88) Benzo(b)fluoranthene	17.522	252	5003892	7450.31	ng/ml	98
89) Benzo(k)fluoranthene	17.591	252	3789489	5946.05	ng/ml	98
90) Benzo(b+k)fluoranthene	17.591	252	9407940	14096.81	ng/ml	98
91) Benzo(e)pyrene	18.174	252	4556103	6930.76	ng/ml	96
92) Benzo(a)pyrene	18.302	252	4292201	7103.37	ng/ml	100
93) Perylene	18.500	252	3844220	6710.58	ng/ml	98
95) Indeno(1,2,3-cd)pyrene	20.838	276	4879339	8830.49	ng/ml	97
96) Dibenz(a,h)anthracene	20.902	278	4143300	8359.97	ng/ml	98
97) Benzo(g,h,i)perylene	21.383	276	4554601	8561.53	ng/ml	98




*see MS*

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191927.D\data.ms

(2) N-Nitrosodimethylamine (TG)




3.957min (+ 0.075) 6384.48 ng/ml

response	799031
Ion	Exp% Act%
74.10	100.00 100.00
42.10	49.40 45.78
43.10	22.20 20.07
0.00	0.00 0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191927.D\data.ms

(2) N-Nitrosodimethylamine (TG)




3.957min (+ 0.075) 6923.78 ng/ml *MD 9/20/19*  
 response 866525

Ion	Exp%	Act%
74.10	100.00	100.00
42.10	49.40	45.78
43.10	22.20	20.07
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191927.D\data.ms

(26) Benzoic acid (T)

7.509min (-0.070) 776.83 ng/ml




response 38011

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	2797.37#
77.00	72.00	828.09#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191927.D\data.ms

(26) Benzoic acid (T)

7.728min (+ 0.150) 14150.47 ng/ml (m)

response 1853462




*JK 9/20/19*

Ion	Exp%	Act%
105.00	100.00	100.00
122.00	90.90	87.13
77.00	72.00	68.18
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191927.D\data.ms

(82) 3,3-Dichlorobenzidine (T)

14.874min (+ 0.011) 10901.24 ng/ml


response 572542

Ion	Exp%	Act%
252.00	100.00	100.00
254.00	66.30	64.83
126.00	12.00	13.82
0.00	0.00	0.00


Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Time--> 13.90 14.00 14.10 14.20 14.30 14.40 14.50 14.60 14.70 14.80 14.90 15.00 15.10 15.20 15.30 15.40 15.50 15.60 15.70 15.80 15.90 16.00  
 Abundance Scan 2129 (14.874 min): J09191927.D\data.ms



m/z--> 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170 180 190 200 210 220 230 240 250 260 270 280 290  
 Abundance Scan 2243 (15.084 min): E02141223.D\data.ms (-2225) (-)



TIC: J09191927.D\data.ms

(82) 3,3-Dichlorobenzidine (T)


14.874min (+ 0.011) -2000.00 ng/ml  
 response 945543

*Handwritten signature and date: JK 9/20/19*

Ion	Exp%	Act%
252.00	100.00	100.00
254.00	66.30	64.83
126.00	12.00	13.82
0.00	0.00	0.00

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191927.D  
 Acq On : 20 Sep 2019 6:39 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-CALA  
 Misc : 1x, A19G247@8000  
 ALS Vial : 12 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:02 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10





Quantitation Report (Not Reviewed)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

*OK 9/20/19*

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	Qvalue
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.573	152	299574	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.841	136	1168153	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.617	162	615222	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.130	188	1152828	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.906	240	1141161	2000.00	ng/ml	-0.01	
86) Perylene-d12 (ISTD)	18.388	264	1161309	2000.00	ng/ml	-0.01	
94) Dibenz(a,h)Anthrcene-d...	20.774	292	999067	2000.00	ng/ml	-0.02	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.316	112	178387	877.95	ng/ml	0.03	
5) Phenol-d6 (Surr)	6.209	99	236341	905.57	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	7.113	82	192375	804.35	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.927	172	511376	1131.94	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.419	330	72353	1337.71	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.917	244	557856	1000.00	ng/ml	0.00	
<b>Target Compounds</b>							
2) N-Nitrosodimethylamine	0.000		0	N.D.			See MS
3) Pyridine	4.000	79	174343m	734.70	ng/ml#		
6) Phenol	6.225	94	253216	853.53	ng/ml	99	
7) Aniline	6.258	93	184591	696.05	ng/ml	95	
8) Bis(2-chloroethyl) ether	6.311	93	252838	956.85	ng/ml	98	
9) 2-Chlorophenol	6.370	128	214007	1001.41	ng/ml	96	
10) 1,3-Dichlorobenzene	6.520	146	240742	1041.72	ng/ml	100	
11) 1,4-Dichlorobenzene	6.589	146	235033	1047.91	ng/ml	99	
12) Benzyl alcohol	6.707	108	114114	832.86	ng/ml	97	
13) 1,2-Dichlorobenzene	6.744	146	236669	1049.78	ng/ml	100	
14) 2-Methylphenol	6.814	107	162406	945.42	ng/ml	97	
15) 2,2'-Oxybis(1-Chloropr...	6.841	45	197724	580.10	ng/ml	98	
16) N-Nitrosodi-n-propylamine	6.969	70	139865	807.91	ng/ml	99	
17) 3+4-Methylphenol	6.964	107	204231	964.68	ng/ml	99	
18) Hexachloroethane	7.081	201	74950	1213.77	ng/ml	97	
20) Nitrobenzene	7.135	77	193505	807.62	ng/ml	99	
22) Isophorone	7.370	82	390447	921.04	ng/ml	96	
23) 2-Nitrophenol	7.456	139	106480	818.33	ng/ml	95	
24) 2,4-Dimethylphenol	7.488	122	151555	937.59	ng/ml	98	
25) Bis(2-chloroethoxy) me...	7.584	93	239341	1013.40	ng/ml	99	
26) Benzoic acid	7.579	105	114401	1564.85	ng/ml	97	
27) 2,4-Dichlorophenol	7.691	162	169468	1209.93	ng/ml	98	
28) 1,2,4-Trichlorobenzene	7.782	180	204325	1204.96	ng/ml	98	
29) Naphthalene	7.857	128	644117	1073.48	ng/ml	100	
30) 4-Chloroaniline	7.910	127	180562	1136.69	ng/ml	98	
31) Hexachlorobutadiene	7.991	225	114587	1267.13	ng/ml	98	
32) 4-Chloro-3-methylphenol	8.386	107	163749	970.69	ng/ml	98	
33) 2-Methylnaphthalene	8.557	142	471069	1149.97	ng/ml	99	
34) 1-Methylnaphthalene	8.659	142	446075	1133.04	ng/ml	100	
36) Hexachlorocyclopentadiene	8.723	237	102004	1047.80	ng/ml	99	
37) 2,4,6-Trichlorophenol	8.841	196	122991	1135.59	ng/ml	99	
38) 2,4,5-Trichlorophenol	8.873	198	123145	1177.26	ng/ml	99	
39) 1,1'-Biphenyl	9.028	154	545943	1068.16	ng/ml	99	
41) 2-Chloronaphthalene	9.050	162	403493	1075.57	ng/ml	98	
42) 2-Nitroaniline	9.146	138	126470	1012.60	ng/ml	98	
43) 2,6-Dimethylnaphthalene	9.189	156	401191	1048.56	ng/ml	98	

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10




Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.274	168	53357	915.09	ng/ml	94
45) Dimethyl phthalate	9.333	163	471576	1071.73	ng/ml	99
46) 1,3-Dinitrobenzene	9.354	168	66203	990.21	ng/ml	96
47) 2,6-Dinitrotoluene	9.392	165	104413	1103.30	ng/ml	94
48) 1,2-Dinitrobenzene	9.445	168	47869	1079.93	ng/ml	96
49) Acenaphthylene	9.472	152	662544	1101.80	ng/ml	98
50) 3-Nitroaniline	9.563	138	81403	882.15	ng/ml	95
51) Acenaphthene	9.649	153	411344	1055.24	ng/ml	99
52) 2,4-Dinitrophenol	9.665	184	21975	682.22	ng/ml	97
53) 4-Nitrophenol	9.723	139	67638	935.18	ng/ml	99
54) 2,4-Dinitrotoluene	9.798	165	130952	1075.20	ng/ml	96
55) Dibenzofuran	9.825	168	586441	1103.27	ng/ml	99
56) 2,3,5,6-Tetrachlorophenol	9.905	232	101694	1174.90	ng/ml	98
57) 2,3,4,6-Tetrachlorophenol	9.948	232	104694	1189.35	ng/ml	98
58) Diethyl phthalate	10.050	149	444740	1059.95	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	10.039	170	361627	1064.34	ng/ml	98
60) Fluorene	10.173	166	450597	1076.35	ng/ml	100
61) 4-Chlorophenyl phenyl ...	10.167	204	220862	1135.24	ng/ml	98
62) 4-Nitroaniline	10.183	138	71452	843.00	ng/ml	94
63) 4,6-Dinitro-2-methylph...	10.216	198	51879	975.85	ng/ml	99
65) N-Nitrosodiphenylamine	10.285	169	378338	1067.17	ng/ml	97
66) Azobenzene (1,2-DPH)	10.328	77	373113	793.36	ng/ml	97
68) 4-Bromophenyl phenyl e...	10.665	248	134322	1131.85	ng/ml	95
69) Hexachlorobenzene	10.745	284	157623	1154.38	ng/ml	96
70) Pentachlorophenol (PCP)	10.938	266	76022	1186.58	ng/ml	99
71) Phenanthrene	11.157	178	656765	1041.88	ng/ml	99
72) Anthracene	11.205	178	657889	1060.69	ng/ml	100
73) Carbazole	11.366	167	473433	924.53	ng/ml	100
74) Di-n-butyl phthalate	11.713	149	721001	1003.18	ng/ml	100
75) Fluoranthene	12.419	202	721487	1094.34	ng/ml	99
76) Benzidine	12.574	184	294532	1737.87	ng/ml	98
77) Pyrene	12.708	202	722196	1096.56	ng/ml	100
80) Butyl benzyl phthalate	13.724	149	293237	820.52	ng/ml	99
81) Bis(2-ethylhexyl) adipate	13.901	129	280177	874.62	ng/ml	98
82) 3,3-Dichlorobenzidine	14.853	252	184897	2473.10	ng/ml	97
83) Benz(a)anthracene	14.880	228	655689	979.93	ng/ml	98
84) Chrysene	14.965	228	602768	976.42	ng/ml	99
85) Bis(2-ethylhexyl) phth...	15.061	149	426572	902.38	ng/ml	98
87) Di-n-octyl phthalate	16.730	149	675629	808.44	ng/ml	100
88) Benzo(b)fluoranthene	17.463	252	645650	917.98	ng/ml	99
89) Benzo(k)fluoranthene	17.532	252	640735	960.05	ng/ml	99
90) Benzo(b+k)fluoranthene	17.532	252	1307403	1870.70	ng/ml	99
91) Benzo(e)pyrene	18.115	252	622430	904.16	ng/ml	100
92) Benzo(a)pyrene	18.238	252	564640	892.33	ng/ml	98
93) Perylene	18.442	252	636474	1060.98	ng/ml	100
95) Indeno(1,2,3-cd)pyrene	20.774	276	575136	1024.01	ng/ml	100
96) Dibenz(a,h)anthracene	20.843	278	552893	1097.51	ng/ml	99
97) Benzo(g,h,i)perylene	21.309	276	598608	1107.02	ng/ml	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191929.D\data.ms

(2) N-Nitrosodimethylamine (TG)




3.883min (-3.883) 0.00 ng/ml

Ion	Exp%	Act%
74.10	100.00	0.00
42.10	49.40	0.00#
43.10	22.20	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



TIC: J09191929.D\data.ms

(2) N-Nitrosodimethylamine (TG)

3.974min (+ 0.091) 856.94 ng/ml


response 119285

Ion	Exp%	Act%
74.10	100.00	100.00
42.10	49.40	49.08
43.10	22.20	22.06
0.00	0.00	0.00

*Handwritten signature and date: JK 9/20/19*

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 09:47:25 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 09:45:16 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10



Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

*Final Report*

*QA 9/23/19*

Quant Time: Sep 20 14:32:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev (Min)	
<b>Internal Standards</b>							
1) 1,4-Dichlorobenzene-d4...	6.573	152	299574	2000.00	ng/ml	0.00	
21) Naphthalene-d8 (ISTD)	7.841	136	1168153	2000.00	ng/ml	0.00	
35) Acenaphthene-d10 (ISTD)	9.617	162	615222	2000.00	ng/ml	0.00	
64) Phenanthrene-d10 (ISTD)	11.130	188	1152828	2000.00	ng/ml	0.00	
78) Chrysene-d12 (ISTD)	14.906	240	1141161	2000.00	ng/ml	-0.01	
86) Perylene-d12 (ISTD)	18.388	264	1161309	2000.00	ng/ml	-0.01	
94) Dibenz(a,h)Anthracene-d...	20.774	292	999067	2000.00	ng/ml	-0.02	
<b>System Monitoring Compounds</b>							
4) 2-Fluorophenol (Surr)	5.316	112	178387	981.27	ng/ml	0.03	
5) Phenol-d6 (Surr)	6.209	99	236341	1015.69	ng/ml	0.00	
19) Nitrobenzene-d5 (Surr)	7.113	82	192375	1065.68	ng/ml	0.00	
40) 2-Fluorobiphenyl (Surr)	8.927	172	511376	1062.10	ng/ml	0.00	
67) 2,4,6-Tribromophenol (...)	10.419	330	72353	1040.67	ng/ml	0.00	
79) Terphenyl-d14 (Surr)	12.917	244	557856	1060.78	ng/ml	0.00	
<b>Target Compounds</b>							
							Qvalue
2) N-Nitrosodimethylamine	3.974	74	119285m	1045.35	ng/ml		
3) Pyridine	4.000	79	174343m	896.19	ng/ml#		
6) Phenol	6.225	94	253216	989.66	ng/ml		99
7) Aniline	6.258	93	184591	836.20	ng/ml		95
8) Bis(2-chloroethyl) ether	6.311	93	252077	1091.65	ng/ml		98
9) 2-Chlorophenol	6.370	128	214007	1008.90	ng/ml		96
10) 1,3-Dichlorobenzene	6.520	146	240742	1009.72	ng/ml		100
11) 1,4-Dichlorobenzene	6.589	146	235033	1002.99	ng/ml		99
12) Benzyl alcohol	6.707	108	114114	910.79	ng/ml		97
13) 1,2-Dichlorobenzene	6.744	146	236669	1024.11	ng/ml		100
14) 2-Methylphenol	6.814	107	162406	1052.52	ng/ml		97
15) 2,2'-Oxybis(1-Chloropr...	6.841	45	197724	970.28	ng/ml		98
16) N-Nitrosodi-n-propylamine	6.969	70	139865	1043.26	ng/ml		99
17) 3+4-Methylphenol	6.964	107	204231	1067.42	ng/ml		99
18) Hexachloroethane	7.081	201	74950	1040.96	ng/ml		97
20) Nitrobenzene	7.135	77	193505	1058.01	ng/ml		99
22) Isophorone	7.370	82	390447	1048.41	ng/ml		96
23) 2-Nitrophenol	7.456	139	106480	968.55	ng/ml		95
24) 2,4-Dimethylphenol	7.488	122	151555	967.66	ng/ml		98
25) Bis(2-chloroethoxy) me...	7.584	93	239341	1057.13	ng/ml		99
26) Benzoic acid	7.579	105	114401	1974.82	ng/ml		97
27) 2,4-Dichlorophenol	7.691	162	169468	968.83	ng/ml		98
28) 1,2,4-Trichlorobenzene	7.782	180	204325	999.39	ng/ml		98
29) Naphthalene	7.857	128	644117	1048.17	ng/ml		100
30) 4-Chloroaniline	7.910	127	180562	939.27	ng/ml		98
31) Hexachlorobutadiene	7.991	225	114587	1037.18	ng/ml		98
32) 4-Chloro-3-methylphenol	8.386	107	163749	1056.42	ng/ml		98
33) 2-Methylnaphthalene	8.557	142	471069	1097.13	ng/ml		99
34) 1-Methylnaphthalene	8.659	142	446075	1073.20	ng/ml		100
36) Hexachlorocyclopentadiene	8.723	237	102004	1072.19	ng/ml		99
37) 2,4,6-Trichlorophenol	8.841	196	122991	1033.65	ng/ml		99
38) 2,4,5-Trichlorophenol	8.873	198	123145	1048.47	ng/ml		99
39) 1,1'-Biphenyl	9.028	154	545943	1032.43	ng/ml		99
41) 2-Chloronaphthalene	9.050	162	403493	1056.54	ng/ml		98
42) 2-Nitroaniline	9.146	138	126470	1106.58	ng/ml		98
43) 2,6-Dimethylnaphthalene	9.189	156	401191	1034.19	ng/ml		98

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M


Quant Time: Sep 20 14:32:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,4-Dinitrobenzene	9.274	168	53357	1114.51	ng/ml	94
45) Dimethyl phthalate	9.333	163	471576	1061.40	ng/ml	99
46) 1,3-Dinitrobenzene	9.354	168	66203	1081.70	ng/ml	96
47) 2,6-Dinitrotoluene	9.392	165	104413	1044.00	ng/ml	94
48) 1,2-Dinitrobenzene	9.445	168	47869	1063.48	ng/ml	96
49) Acenaphthylene	9.472	152	662544	1059.38	ng/ml	98
50) 3-Nitroaniline	9.563	138	81403	1060.77	ng/ml	95
51) Acenaphthene	9.649	153	411344	1001.62	ng/ml	99
52) 2,4-Dinitrophenol	9.665	184	21975	972.00	ng/ml	97
53) 4-Nitrophenol	9.723	139	67638	1106.89	ng/ml	99
54) 2,4-Dinitrotoluene	9.798	165	130952	1048.40	ng/ml	96
55) Dibenzofuran	9.825	168	586441	1071.22	ng/ml	99
56) 2,3,5,6-Tetrachlorophenol	9.905	232	101694	1077.31	ng/ml	98
57) 2,3,4,6-Tetrachlorophenol	9.948	232	104694	1014.00	ng/ml	98
58) Diethyl phthalate	10.050	149	444740	1087.44	ng/ml	98
59) 2,3,5-Trimethylnaphtha...	10.039	170	361627	1037.33	ng/ml	98
60) Fluorene	10.173	166	450597	1045.90	ng/ml	100
61) 4-Chlorophenyl phenyl ...	10.167	204	220862	1051.57	ng/ml	98
62) 4-Nitroaniline	10.183	138	71452	1080.74	ng/ml	94
63) 4,6-Dinitro-2-methylph...	10.216	198	51879	1157.72	ng/ml	99
65) N-Nitrosodiphenylamine	10.285	169	378338	1064.38	ng/ml	97
66) Azobenzene (1,2-DPH)	10.328	77	373113	1037.26	ng/ml	97
68) 4-Bromophenyl phenyl e...	10.665	248	134322	1032.58	ng/ml	95
69) Hexachlorobenzene	10.745	284	157623	1010.04	ng/ml	96
70) Pentachlorophenol (PCP)	10.938	266	76022	975.76	ng/ml	99
71) Phenanthrene	11.157	178	656765	1015.50	ng/ml	99
72) Anthracene	11.205	178	657889	1058.25	ng/ml	100
73) Carbazole	11.366	167	473433	964.91	ng/ml	100
74) Di-n-butyl phthalate	11.713	149	721001	1057.53	ng/ml	100
75) Fluoranthene	12.419	202	721487	1088.45	ng/ml	99
76) Benzidine	12.574	184	294175	1842.78	ng/ml	98
77) Pyrene	12.708	202	722196	1070.62	ng/ml	100
80) Butyl benzyl phthalate	13.724	149	293237	1004.00	ng/ml	99
81) Bis(2-ethylhexyl) adipate	13.901	129	280177	1058.58	ng/ml	98
82) 3,3-Dichlorobenzidine	14.853	252	184897	2062.77	ng/ml	97
83) Benz(a)anthracene	14.880	228	655689	1029.12	ng/ml	98
84) Chrysene	14.965	228	602768	1009.53	ng/ml	99
85) Bis(2-ethylhexyl) phth...	15.061	149	426572	1039.18	ng/ml	98
87) Di-n-octyl phthalate	16.730	149	675629	1013.80	ng/ml	100
88) Benzo(b)fluoranthene	17.463	252	645650	1008.51	ng/ml	99
89) Benzo(k)fluoranthene	17.532	252	640735	992.12	ng/ml	99
90) Benzo(b+k)fluoranthene	17.532	252	1307403	1987.64	ng/ml	99
91) Benzo(e)pyrene	18.115	252	622430	1042.80	ng/ml	100
92) Benzo(a)pyrene	18.238	252	564640	971.42	ng/ml	98
93) Perylene	18.442	252	636474	1215.26	ng/ml	100
95) Indeno(1,2,3-cd)pyrene	20.774	276	575136	973.51	ng/ml	100
96) Dibenz(a,h)anthracene	20.843	278	552893	1019.31	ng/ml	99
97) Benzo(g,h,i)perylene	21.309	276	598608	1054.88	ng/ml	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\msdchem\1\data\2019-09\9I19035\  
 Data File : J09191929.D  
 Acq On : 20 Sep 2019 7:50 am  
 Operator : JK/ AMS/ DTH  
 Sample : 9I19035-ICV1  
 Misc : 1x, A19I254@1000  
 ALS Vial : 13 Sample Multiplier: 1  
 DataAcq Meth:SV10\_AQUISITION.M

Quant Time: Sep 20 14:32:58 2019  
 Quant Method : C:\msdchem\1\methods\SV10\_091919.M  
 Quant Title : EPA 8270D: Semivolatile Organics  
 QLast Update : Fri Sep 20 10:41:03 2019  
 Response via : Initial Calibration  
 InstName : SV-GCMS10





**TCLP Metals by EPA 6020A (ICPMS)  
Benchsheet Data and Analysis (Including Calibration)**

Batch 9111213  
Sequence 9K26027



Ag (Silver) - 6020 - TCLP  
 As (Arsenic) - 6020 - TCLP  
 Ba (Barium) - 6020 - TCLP  
 Cd (Cadmium) - 6020 - TCLP  
 Cr (Chromium) - 6020 - TCLP  
 Hg (Mercury) - 6020 - TCLP  
 Pb (Lead) - 6020 - TCLP  
 Se (Selenium) - 6020 - TCLP

PREPARATION BENCH SHEET

9111213

DEC 10 2019

Apex Laboratories  
 BATCH #: 9111213 (Soil)  
 Prep Method: EPA 1311/3015

Lab Number	Due	Prepared	Initial (mL)	Final (mL)	Client	ClientID / Sample	Extraction Comments
9111213-BLK1		11/26/19 09:55	10	50	@C Sample		
9111213-BS1		11/26/19 09:55	10	50	@C Sample		
Spike 1: 250 uL of A19J064		Spike 2: 1000 uL of A19K228					
A9K0412-01	11/27/19	11/26/19 09:55	10	50	Anchor QEA, LLC	PDI#142RAB-C-00-3034-191	
<input type="checkbox"/> Ag (Silver) - 6020 - TCLP <input type="checkbox"/> As (Arsenic) - 6020 - TCLP <input type="checkbox"/> Ba (Barium) - 6020 - TCLP <input type="checkbox"/> Cd (Cadmium) - 6020 - TCLP <input type="checkbox"/> Cr (Chromium) - 6020 - TCLP <input type="checkbox"/> Hg (Mercury) - 6020 - TCLP <input type="checkbox"/> Pb (Lead) - 6020 - TCLP <input type="checkbox"/> Se (Selenium) - 6020 - TCLP							
9111213-MS1		11/26/19 09:55	10	50	@C Sample		
Source: A9K0412-01		Spike 1: 250 uL of A19J064		Spike 2: 1000 uL of A19K228			

Standards/Reagents

Reagent(s)	Std ID	Exp. Date	Description
	A13L213	11/30/23	Metals Prep Balance 2
	A17F264	06/23/23	Mars-6 Microwave
	A19I314	03/22/20	Conc. HCl - Omnitrace
	A19J492	04/28/20	Conc. HNO3 - Omnitrace

Analyte Spike(s)	Std ID	Exp. Date	Description
	A19J064	12/28/19	###TCLP 1 Spk
	A19K228	01/30/20	Hg Sb TCLP Spk Standard

CRL  
11/26/19

Fluid ID: ~~A19K296~~ A19K328    ESS 11/26/19  
 Extraction Batch: ~~9111049~~ 911146  
 Digestion time and temperature achieved? **YES**  
 Initials: **CRL**

Prepared By: CRL    Date: 11/26/19

Reviewed By: ESS    Date: 11/26/19

**Batch #: 9111213**

**If observed weight loss < 0.2g**

Digestion is within control limits

**If observed weight loss > 0.2g**

Enter data in to electronic VWW. Acceptance limit 1.0% sample loss.

Date: 11/26/19

Prepared by: CRL

#	Mars Tube ID	Sample ID	Pre-digestion Vessel + Sample Wt. (g)	Post-digestion Vessel + Sample Wt. (g)	Sample Wt. Loss (%)* <i>Formula only used if sample loss &gt; 0.2g</i>
1	S38	9111213-BLK1	208.23	208.22	n/a
2	S103	9111213-BS1	205.90	205.90	n/a
3	S96	A9K0412-01	207.32	207.32	n/a
4	S95	9111213-MS1	210.49	210.48	n/a
5					n/a
6					n/a
7					n/a
8					n/a
9					n/a
10					n/a
11					n/a
12					n/a
13					n/a
14					n/a
15					n/a
16					n/a
17					n/a
18					n/a
19					n/a
20					n/a
21					n/a
22					n/a
23					n/a
24					n/a
					n/a

\*Example Calculation:  $(\text{Pre(g)} - \text{Post(g)}) / (\text{Post(g)} - 159.32\text{g})$  This represents the mean weight of the empty digestion vessels. By factoring in the mean digestion vessel weight, we observe weight loss from only the sample, rather than as a percentage of the sample+vessel weight.



# ELEMENT SEQUENCE LOG

Apex Laboratories

Sequence:           **9K26027**  
Date:                   **11/26/19 09:48**

Instrument:           **ICPMS5**  
Calibration:           **UNASSIGNED**

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
1	9K26027-CAL1	Water	QC	QC			A19J130	A19K144
2	9K26027-CAL2	Water	QC	QC			A19J130	A19K145
3	9K26027-CAL3	Water	QC	QC			A19J130	A19K146
4	9K26027-CAL4	Water	QC	QC			A19J130	A19K147
5	9K26027-CAL5	Water	QC	QC			A19J130	A19K148
6	9K26027-CAL6	Water	QC	QC			A19J130	A19K149
7	9K26027-CAL7	Water	QC	QC			A19J130	A19K150
8	9K26027-CAL8	Water	QC	QC			A19J130	A19K151
9	9K26027-CAL9	Water	QC	QC			A19J130	A19K152
10	9K26027-ICV1	Water	QC	QC			A19J130	A19J138
11	9K26027-ICB1	Water	QC	QC			A19J130	
12	9K26027-CRL1	Water	QC	QC			A19J130	A19K144
13	9K26027-CRL2	Water	QC	QC			A19J130	A19K145
14	9K26027-CRL3	Water	QC	QC			A19J130	A19K146
15	9K26027-IFA1	Water	QC	QC			A19J130	A19K233
16	9K26027-IFB1	Water	QC	QC			A19J130	A19K234
17	9111212-BLK1	Solid	QC	QC		9111212	A19J130	
18	9111212-BS1	Solid	QC	QC		9111212	A19J130	
19	A9K0650-01	Solid	Ag (Silver) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
20	"	Solid	As (Arsenic) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
21	"	Solid	Ba (Barium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
22	"	Solid	Cd (Cadmium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
23	"	Solid	Cr (Chromium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
24	"	Solid	Hg (Mercury) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
25	"	Solid	Pb (Lead) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
26	"	Solid	Se (Selenium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
27	A9K0650-02	Solid	Ag (Silver) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
28	"	Solid	As (Arsenic) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
29	"	Solid	Ba (Barium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
30	"	Solid	Cd (Cadmium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
31	"	Solid	Cr (Chromium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
32	"	Solid	Hg (Mercury) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
33	"	Solid	Pb (Lead) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
34	"	Solid	Se (Selenium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
35	A9K0650-03	Solid	Ag (Silver) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
36	"	Solid	As (Arsenic) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
37	"	Solid	Ba (Barium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
38	"	Solid	Cd (Cadmium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
39	"	Solid	Cr (Chromium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
40	"	Solid	Hg (Mercury) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
41	"	Solid	Pb (Lead) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
42	"	Solid	Se (Selenium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
43	A9K0683-01	Solid	Ag (Silver) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
44	"	Solid	As (Arsenic) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
45	"	Solid	Ba (Barium) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
46	"	Solid	Cd (Cadmium) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
47	"	Solid	Cr (Chromium) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
48	"	Solid	Hg (Mercury) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
49	"	Solid	Pb (Lead) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
50	"	Solid	Se (Selenium) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
51	A9K0683-02	Solid	Ag (Silver) - 6020 - TCLP	"	11/27/19	9111212	A19J130	

Sequence:

9K26027

Instrument:

ICPMS5

Date:

11/26/19 09:48

Calibration:

UNASSIGNED

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
52	"	Solid	As (Arsenic) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
53	"	Solid	Ba (Barium) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
54	"	Solid	Cd (Cadmium) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
55	"	Solid	Cr (Chromium) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
56	"	Solid	Hg (Mercury) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
57	"	Solid	Pb (Lead) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
58	"	Solid	Se (Selenium) - 6020 - TCLP	"	11/27/19	9111212	A19J130	
59	A9K0725-01	Solid	Ag (Silver) - 6020 - TCLP	(QC Source)		9111212	A19J130	
60	"	Solid	As (Arsenic) - 6020 - TCLP	(QC Source)		9111212	A19J130	
61	"	Solid	Ba (Barium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
62	"	Solid	Cd (Cadmium) - 6020 - TCLP	(QC Source)		9111212	A19J130	
63	"	Solid	Cr (Chromium) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
64	"	Solid	Hg (Mercury) - 6020 - TCLP	(QC Source)		9111212	A19J130	
65	"	Solid	Pb (Lead) - 6020 - TCLP	(QC Source)		9111212	A19J130	
66	"	Solid	Se (Selenium) - 6020 - TCLP	(QC Source)		9111212	A19J130	
67	9111212-MS1	Solid	QC	QC		9111212	A19J130	
68	A9K0759-01	Solid	Ag (Silver) - 6020 - TCLP	(QC Source)		9111212	A19J130	
69	"	Solid	As (Arsenic) - 6020 - TCLP	(QC Source)		9111212	A19J130	
70	"	Solid	Ba (Barium) - 6020 - TCLP	(QC Source)		9111212	A19J130	
71	"	Solid	Cd (Cadmium) - 6020 - TCLP	(QC Source)		9111212	A19J130	
72	"	Solid	Cr (Chromium) - 6020 - TCLP	(QC Source)		9111212	A19J130	
73	"	Solid	Hg (Mercury) - 6020 - TCLP	(QC Source)		9111212	A19J130	
74	"	Solid	Pb (Lead) - 6020 - TCLP	"	11/26/19	9111212	A19J130	
75	"	Solid	Se (Selenium) - 6020 - TCLP	(QC Source)		9111212	A19J130	
76	9K26027-CCV1	Water	QC	QC			A19J130	A19J138
77	9K26027-CCB1	Water	QC	QC			A19J130	
78	9111212-MS2	Solid	QC	QC		9111212	A19J130	
79	9111213-BLK1	Soil	QC	QC		9111213	A19J130	
80	9111213-BS1	Soil	QC	QC		9111213	A19J130	
81	A9K0412-01	Soil	Ag (Silver) - 6020 - TCLP	Anchor QEA, LLC	11/27/19	9111213	A19J130	
82	"	Soil	As (Arsenic) - 6020 - TCLP	"	11/27/19	9111213	A19J130	
83	"	Soil	Ba (Barium) - 6020 - TCLP	"	11/27/19	9111213	A19J130	
84	"	Soil	Cd (Cadmium) - 6020 - TCLP	"	11/27/19	9111213	A19J130	
85	"	Soil	Cr (Chromium) - 6020 - TCLP	"	11/27/19	9111213	A19J130	
86	"	Soil	Hg (Mercury) - 6020 - TCLP	"	11/27/19	9111213	A19J130	
87	"	Soil	Pb (Lead) - 6020 - TCLP	"	11/27/19	9111213	A19J130	
88	"	Soil	Se (Selenium) - 6020 - TCLP	"	11/27/19	9111213	A19J130	
89	9111213-MS1	Soil	QC	QC		9111213	A19J130	
90	A9K0650-03RE1	Solid	Cr (Chromium) - 6020 - TCLP		11/26/19	9111212	A19J130	
91	A9K0458-03RE1	Water	Zn (Zinc) - 200.8 - Dissolved		12/02/19	9111168	A19J130	
92	9111147-BLK2	Water	QC	QC		9111147	A19J130	
93	A9K0713-01RE1	Water	Mg (Magnesium) - 200.8 - Total		12/02/19	9111147	A19J130	
94	A9K0713-02RE1	Water	Mg (Magnesium) - 200.8 - Total		12/02/19	9111147	A19J130	
95	9K26027-CCV2	Water	QC	QC			A19J130	A19J138
96	9K26027-CCB2	Water	QC	QC			A19J130	
97	9K26027-CRL4	Water	QC	QC			A19J130	A19K144
98	9K26027-CRL5	Water	QC	QC			A19J130	A19K145
99	9K26027-CRL6	Water	QC	QC			A19J130	A19K146
100	A9K0505-01RE1	Water	Ag (Silver) - 200.8 - Total		12/03/19	9111147	A19J130	
101	"	Water	As (Arsenic) - 200.8 - Total	"	12/03/19	9111147	A19J130	
102	"	Water	Cd (Cadmium) - 200.8 - Total	"	12/03/19	9111147	A19J130	
103	"	Water	Cr (Chromium) - 200.8 - Total	"	12/03/19	9111147	A19J130	
104	"	Water	Cu (Copper) - 200.8 - Total	"	12/03/19	9111147	A19J130	
105	"	Water	Mg (Magnesium) - 200.8 - Total	"	12/03/19	9111147	A19J130	
106	"	Water	Ni (Nickel) - 200.8 - Total	"	12/03/19	9111147	A19J130	

Sequence:

9K26027

Instrument:

ICPMS5

Date:

11/26/19 09:48

Calibration:

UNASSIGNED

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
107	"	Water	Pb (Lead) - 200.8 - Total	"	12/03/19	9111147	A19J130	
108	"	Water	Se (Selenium) - 200.8 - Total	"	12/03/19	9111147	A19J130	
109	"	Water	Zn (Zinc) - 200.8 - Total	"	12/03/19	9111147	A19J130	
110	A9K0714-01RE1	Water	Ca (Calcium) - 200.8 - Total	(QC Source)		9111147	A19J130	
111	"	Water	Cr (Chromium) - 6020 - Total	(QC Source)		9111147	A19J130	
112	9111147-MS3	Water	QC	QC		9111147	A19J130	
113	9111200-BLK1	Solid	QC	QC		9111200	A19J130	
114	9111200-BS1	Solid	QC	QC		9111200	A19J130	
115	A9K0776-01	Solid	Ag (Silver) - 6020 - Total		11/27/19	9111200	A19J130	
116	"	Solid	As (Arsenic) - 6020 - Total	"	11/27/19	9111200	A19J130	
117	"	Solid	Ba (Barium) - 6020 - Total	"	11/27/19	9111200	A19J130	
118	"	Solid	Cd (Cadmium) - 6020 - Total	"	11/27/19	9111200	A19J130	
119	"	Solid	Cr (Chromium) - 6020 - Total	"	11/27/19	9111200	A19J130	
120	"	Solid	Hg (Mercury) - 6020 - Total	"	11/27/19	9111200	A19J130	
121	"	Solid	Pb (Lead) - 6020 - Total	"	11/27/19	9111200	A19J130	
122	"	Solid	Se (Selenium) - 6020 - Total	"	11/27/19	9111200	A19J130	
123	9111200-DUP1	Solid	QC	QC		9111200	A19J130	
124	9111200-MS1	Solid	QC	QC		9111200	A19J130	
125	A9K0799-01	Solid	Pb (Lead) - 6020 - Total		11/27/19	9111200	A19J130	
126	A9K0807-01	Solid	Ag (Silver) - 6020 - Total		11/27/19	9111200	A19J130	
127	"	Solid	As (Arsenic) - 6020 - Total	"	11/27/19	9111200	A19J130	
128	"	Solid	Ba (Barium) - 6020 - Total	"	11/27/19	9111200	A19J130	
129	"	Solid	Cd (Cadmium) - 6020 - Total	"	11/27/19	9111200	A19J130	
130	"	Solid	Cr (Chromium) - 6020 - Total	"	11/27/19	9111200	A19J130	
131	"	Solid	Hg (Mercury) - 6020 - Total	"	11/27/19	9111200	A19J130	
132	"	Solid	Pb (Lead) - 6020 - Total	"	11/27/19	9111200	A19J130	
133	"	Solid	Se (Selenium) - 6020 - Total	"	11/27/19	9111200	A19J130	
134	9K26027-CCV3	Water	QC	QC			A19J130	A19J138
135	9K26027-CCB3	Water	QC	QC			A19J130	
136	9111204-BLK1	Water	QC	QC		9111204	A19J130	
137	9111204-BS1	Water	QC	QC		9111204	A19J130	
138	A9K0776-01RE1	Solid	Ag (Silver) - 6020 - Total		11/27/19	9111200	A19J130	
139	"	Solid	As (Arsenic) - 6020 - Total	"	11/27/19	9111200	A19J130	
140	"	Solid	Ba (Barium) - 6020 - Total	"	11/27/19	9111200	A19J130	
141	"	Solid	Cd (Cadmium) - 6020 - Total	"	11/27/19	9111200	A19J130	
142	"	Solid	Cr (Chromium) - 6020 - Total	"	11/27/19	9111200	A19J130	
143	"	Solid	Hg (Mercury) - 6020 - Total	"	11/27/19	9111200	A19J130	
144	"	Solid	Pb (Lead) - 6020 - Total	"	11/27/19	9111200	A19J130	
145	"	Solid	Se (Selenium) - 6020 - Total	"	11/27/19	9111200	A19J130	
146	9111200-DUP2	Solid	QC	QC		9111200	A19J130	
147	9111200-MS2	Solid	QC	QC		9111200	A19J130	
148	A9K0807-01RE1	Solid	Ag (Silver) - 6020 - Total		11/27/19	9111200	A19J130	
149	"	Solid	As (Arsenic) - 6020 - Total	"	11/27/19	9111200	A19J130	
150	"	Solid	Ba (Barium) - 6020 - Total	"	11/27/19	9111200	A19J130	
151	"	Solid	Cd (Cadmium) - 6020 - Total	"	11/27/19	9111200	A19J130	
152	"	Solid	Hg (Mercury) - 6020 - Total	"	11/27/19	9111200	A19J130	
153	"	Solid	Pb (Lead) - 6020 - Total	"	11/27/19	9111200	A19J130	
154	"	Solid	Se (Selenium) - 6020 - Total	"	11/27/19	9111200	A19J130	
155	A9K0752-01	Water	Cu (Copper) - 6020 - Total		12/03/19	9111204	A19J130	
156	"	Water	Fe (Iron) - 6020 - Total	"	12/03/19	9111204	A19J130	
157	"	Water	Hg (Mercury) - 6020 - Total	"	12/03/19	9111204	A19J130	
158	"	Water	Pb (Lead) - 6020 - Total	"	12/03/19	9111204	A19J130	
159	A9K0764-01	Water	Cd (Cadmium) - 200.8 - Total		12/03/19	9111204	A19J130	
160	"	Water	Cr (Chromium) - 200.8 - Total		12/03/19	9111204	A19J130	
161	"	Water	Pb (Lead) - 200.8 - Total	"	12/03/19	9111204	A19J130	

Sequence:

9K26027

Instrument:

ICPMS5

Date:

11/26/19 09:48

Calibration:

UNASSIGNED

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
162	A9K0764-02	Water	Cd (Cadmium) - 200.8 - Total		12/03/19	9111204	A19J130	
163	"	Water	Cr (Chromium) - 200.8 - Total	"	12/03/19	9111204	A19J130	
164	"	Water	Pb (Lead) - 200.8 - Total	"	12/03/19	9111204	A19J130	
165	A9K0765-01	Water	As (Arsenic) - 200.8 - Total	(QC Source)		9111204	A19J130	
166	"	Water	Cd (Cadmium) - 200.8 - Total	"	12/03/19	9111204	A19J130	
167	"	Water	Cr (Chromium) - 200.8 - Total	"	12/03/19	9111204	A19J130	
168	"	Water	Cu (Copper) - 6020 - Total	(QC Source)		9111204	A19J130	
169	"	Water	Cu (Copper) - 200.8 - Total	(QC Source)		9111204	A19J130	
170	"	Water	Fe (Iron) - 6020 - Total	(QC Source)		9111204	A19J130	
171	"	Water	Hg (Mercury) - 6020 - Total	(QC Source)		9111204	A19J130	
172	"	Water	Pb (Lead) - 6020 - Total	(QC Source)		9111204	A19J130	
173	"	Water	Pb (Lead) - 200.8 - Total	"	12/03/19	9111204	A19J130	
174	"	Water	Zn (Zinc) - 200.8 - Total	(QC Source)		9111204	A19J130	
175	9K26027-CCV4	Water	QC	QC			A19J130	A19J138
176	9K26027-CCB4	Water	QC	QC			A19J130	
177	9111204-DUP1	Water	QC	QC		9111204	A19J130	
178	9111204-MS1	Water	QC	QC		9111204	A19J130	
179	A9K0771-01	Water	As (Arsenic) - 200.8 - Total		11/27/19	9111204	A19J130	
180	A9K0771-02	Water	As (Arsenic) - 200.8 - Total		11/27/19	9111204	A19J130	
181	A9K0771-03	Water	As (Arsenic) - 200.8 - Total		11/27/19	9111204	A19J130	
182	A9K0771-04	Water	As (Arsenic) - 200.8 - Total		11/27/19	9111204	A19J130	
183	"	Water	Cd (Cadmium) - 200.8 - Total	(QC Source)		9111204	A19J130	
184	"	Water	Cr (Chromium) - 200.8 - Total	(QC Source)		9111204	A19J130	
185	"	Water	Cu (Copper) - 6020 - Total	(QC Source)		9111204	A19J130	
186	"	Water	Cu (Copper) - 200.8 - Total	(QC Source)		9111204	A19J130	
187	"	Water	Fe (Iron) - 6020 - Total	(QC Source)		9111204	A19J130	
188	"	Water	Hg (Mercury) - 6020 - Total	(QC Source)		9111204	A19J130	
189	"	Water	Pb (Lead) - 6020 - Total	(QC Source)		9111204	A19J130	
190	"	Water	Pb (Lead) - 200.8 - Total	(QC Source)		9111204	A19J130	
191	"	Water	Zn (Zinc) - 200.8 - Total	(QC Source)		9111204	A19J130	
192	9111204-MS2	Water	QC	QC		9111204	A19J130	
193	9111114-MS3	Solid	QC	QC		9111114	A19J130	
194	9111114-MSD3	Solid	QC	QC		9111114	A19J130	
195	A9K0767-01	Water	Cd (Cadmium) - 200.8 - Total		12/03/19	9111204	A19J130	
196	"	Water	Cr (Chromium) - 200.8 - Total	"	12/03/19	9111204	A19J130	
197	"	Water	Pb (Lead) - 200.8 - Total	"	12/03/19	9111204	A19J130	
198	9K26027-CCV5	Water	QC	QC			A19J130	A19J138
199	9K26027-CCB5	Water	QC	QC			A19J130	
200	9K26027-CRL7	Water	QC	QC			A19J130	A19K144
201	9K26027-CRL8	Water	QC	QC			A19J130	A19K145
202	9K26027-CRL9	Water	QC	QC			A19J130	A19K146
203	9K26027-CRLA	Water	QC	QC			A19J130	A19K147
204	A9K0768-01	Water	Cd (Cadmium) - 200.8 - Total		12/03/19	9111204	A19J130	
205	"	Water	Cr (Chromium) - 200.8 - Total	"	12/03/19	9111204	A19J130	
206	"	Water	Pb (Lead) - 200.8 - Total	"	12/03/19	9111204	A19J130	
207	"	Water	Zn (Zinc) - 200.8 - Total	"	12/03/19	9111204	A19J130	
208	A9K0769-01	Water	Cd (Cadmium) - 200.8 - Total		12/03/19	9111204	A19J130	
209	"	Water	Cr (Chromium) - 200.8 - Total	"	12/03/19	9111204	A19J130	
210	"	Water	Cu (Copper) - 200.8 - Total	"	12/03/19	9111204	A19J130	
211	"	Water	Pb (Lead) - 200.8 - Total	"	12/03/19	9111204	A19J130	
212	"	Water	Zn (Zinc) - 200.8 - Total	"	12/03/19	9111204	A19J130	
213	9111172-BLK1	Solid	QC	QC		9111172	A19J130	
214	9111172-BS1	Solid	QC	QC		9111172	A19J130	
215	A9K0686-01	Solid	Cr (Chromium) - 6020 - Total	PreRD	12/03/19	9111172	A19J130	
216	9111172-DUP1	Solid	QC	QC		9111172	A19J130	

Sequence:

9K26027

Instrument:

ICPMS5

Date:

11/26/19 09:48

Calibration:

UNASSIGNED

#	Lab Number	Matrix	Analysis	Client	Due	Batch	ISTD ID	STD ID
217	9111172-MS1	Solid	QC	QC		9111172	A19J130	
218	9111119-BLK1	Water	QC	QC		9111119	A19J130	
219	9111119-BS1	Water	QC	QC		9111119	A19J130	
220	9K26027-CCV6	Water	QC	QC			A19J130	A19J138
221	9K26027-CCB6	Water	QC	QC			A19J130	
222	A9K0513-01	Water	Cu (Copper) - 200.8 - Dissolved		12/03/19	9111119	A19J130	
223	A9K0576-01	Water	Cu (Copper) - 200.8 - Dissolved		12/04/19	9111119	A19J130	
224	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/04/19	9111119	A19J130	
225	A9K0576-02	Water	Cu (Copper) - 200.8 - Dissolved		12/04/19	9111119	A19J130	
226	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/04/19	9111119	A19J130	
227	A9K0599-01	Water	Cu (Copper) - 200.8 - Dissolved		12/04/19	9111119	A19J130	
228	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/04/19	9111119	A19J130	
229	A9K0669-02	Water	Cu (Copper) - 200.8 - Dissolved	(QC Source)		9111119	A19J130	
230	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/06/19	9111119	A19J130	
231	9111119-DUP1	Water	QC	QC		9111119	A19J130	
232	9111119-MS1	Water	QC	QC		9111119	A19J130	
233	9111115-BLK1	Water	QC	QC		9111115	A19J130	
234	9111115-BS1	Water	QC	QC		9111115	A19J130	
235	A9K0473-01	Water	Cu (Copper) - 200.8 - Dissolved		12/02/19	9111115	A19J130	
236	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/02/19	9111115	A19J130	
237	9K26027-CCV7	Water	QC	QC			A19J130	A19J138
238	9K26027-CCB7	Water	QC	QC			A19J130	
239	A9K0500-01	Water	Cu (Copper) - 200.8 - Dissolved		12/03/19	9111115	A19J130	
240	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/03/19	9111115	A19J130	
241	A9K0613-01	Water	Cu (Copper) - 200.8 - Dissolved		12/05/19	9111115	A19J130	
242	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/05/19	9111115	A19J130	
243	"	Water	Zn (Zinc) - 200.8 - Dissolved	"	12/05/19	9111115	A19J130	
244	A9K0669-01	Water	Ag (Silver) - 200.8 - Dissolved	(QC Source)		9111115	A19J130	
245	"	Water	Cd (Cadmium) - 200.8 - Dissolved	(QC Source)		9111115	A19J130	
246	"	Water	Cu (Copper) - 200.8 - Dissolved	(QC Source)		9111115	A19J130	
247	"	Water	Ni (Nickel) - 200.8 - Dissolved	(QC Source)		9111115	A19J130	
248	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/06/19	9111115	A19J130	
249	"	Water	Zn (Zinc) - 200.8 - Dissolved	(QC Source)		9111115	A19J130	
250	9111115-DUP1	Water	QC	QC		9111115	A19J130	
251	9111115-MS1	Water	QC	QC		9111115	A19J130	
252	A9K0669-03	Water	Pb (Lead) - 200.8 - Dissolved		12/06/19	9111115	A19J130	
253	A9K0694-01	Water	Ag (Silver) - 200.8 - Dissolved		12/06/19	9111115	A19J130	
254	"	Water	Cd (Cadmium) - 200.8 - Dissolved	"	12/06/19	9111115	A19J130	
255	"	Water	Ni (Nickel) - 200.8 - Dissolved	"	12/06/19	9111115	A19J130	
256	"	Water	Pb (Lead) - 200.8 - Dissolved	"	12/06/19	9111115	A19J130	
257	"	Water	Zn (Zinc) - 200.8 - Dissolved	"	12/06/19	9111115	A19J130	
258	A9K0702-01	Water	Cu (Copper) - 200.8 - Dissolved		12/06/19	9111115	A19J130	
259	9K26027-CCV8	Water	QC	QC			A19J130	A19J138
260	9K26027-CCB8	Water	QC	QC			A19J130	
261	9K26027-CRLB	Water	QC	QC			A19J130	A19K144
262	9K26027-CRLC	Water	QC	QC			A19J130	A19K145
263	9K26027-CRLD	Water	QC	QC			A19J130	A19K146
264	9K26027-CRLE	Water	QC	QC			A19J130	A19K147

Data Entered By: ESS 11/27/19

Comments:

Data Reviewed By: [Signature] 11/27/19



# Tune Report

**Batch Folder** C:\Agilent\ICPMH\1\DATA\9K26027.b  
**Acq. Date-Time** 11/26/2019 10:21  
**Report Comment** 9K26027 EPA Multi-mode Tune Report A19I052  
**Instrument Name** 7700x JP09240003

[H2]

Mass	Range	Count (Actual)	Response (Actual) [cps/ug/l]	Response (Required) [cps/ug/l]	Response (Flag)
59		3358	33580.32	1000.00	
89		15481	154812.17	1000.00	
78		12			


Mass	Resp Ratio (Actual)	Resp Ratio (Required)	Resp Ratio (Flag)
59		-	
89		-	
78		-	

Mass	RSD% (Actual)	RSD% (Required)	RSD% (Flag)
59	2.44	5.00	
89	1.31	5.00	
78	18.28		

Mass	Background (Actual)	Background (Required)	Background (Flag)
59			
89			
78			

Mass	Rep. 1 Count	Rep. 2 Count	Rep. 3 Count	Rep. 4 Count	Rep. 5 Count
59	3414	3418	3318	3409	3232
89	15623	15514	15615	15524	15130
78	13	15	10	11	11

Integration Time [sec] 0.1



Mass	Peak Height	Axis (Actual)	Axis (Required)	Axis (Flag)	W-50% (Actual)	W-50% (Required)	W-50% (Flag)
59	552.05	59.05	58.9 - 59.1		0.64	0.788	0.900

# Tune Report

89      2626.60      89.00      88.9 - 89.1      0.62      0.790      0.900  
78

**Integration Time [sec]**                      0.1 **Acquisition Time [sec]**                      100.35 **Y Axis**    Linear

**Tune Parameters**

**## Plasma Paramters ##**

RF Power	1550 W	Nebulizer Pump	0.10 rps
RF Matching	1.94 V	S/C Temp	2 °C
Smpl Depth	8.0 mm	Gas Switch	Makeup Gas
Carrier Gas	1.08 L/min	Makeup/Dilution Gas	0.00 L/min
Option Gas	0.0 %		

**## Lenses Parameters ##**

Extract 1	0.0 V	Cell Entrance	-40 V
Extract 2	-160.0 V	Cell Exit	-60 V
Omega Bias	-90 V	Deflect	2.0 V
Omega Lens	6.0 V	Plate Bias	-40 V

**## Cell Parameters ##**

Use Gas	true	OctP Bias	-18.0 V
He Flow	0.0 mL/min	OctP RF	180 V
H2 Flow	3.3 mL/min	Energy Discrimination	5.0 V
3rd Gas Flow	0 %		

**[He]**

Mass	Range	Count (Actual)	Response (Actual) [cps/ug/l]	Response (Required) [cps/ug/l]	Response (Flag)
59		4207	42072.09	1000.00	
89		4424	44241.25	1000.00	
205		5511	55114.87	1000.00	
75		20			

Mass	Resp Ratio (Actual)	Resp Ratio (Required)	Resp Ratio (Flag)
59		-	
89		-	
205		-	
75		-	

Mass	RSD% (Actual)	RSD% (Required)	RSD% (Flag)
59	1.97	5.00	
89	2.01	5.00	
205	1.45	5.00	
75	19.90		

Mass	Background (Actual)	Background (Required)	Background (Flag)
59			
89			



# Tune Report

205  
75

Mass	Rep. 1 Count	Rep. 2 Count	Rep. 3 Count	Rep. 4 Count	Rep. 5 Count
59	4161	4104	4275	4307	4189
89	4281	4402	4486	4446	4504
205	5455	5419	5615	5567	5502
75	20	17	25	24	17

Integration Time [sec] 0.1

Mass	Peak Height	Axis (Actual)	Axis (Required)	Axis (Flag)	W-50%	W-5% (Actual)	W-5% (Required)	W-5% (Flag)
59	690.80	59.00	58.9 - 59.1		0.64	0.787	0.900	
89	763.68	89.05	88.9 - 89.1		0.61	0.780	0.900	
205	968.52	205.00	204.9 - 205.1		0.57	0.747	0.900	
75	3.05	75.00	-		0.69	0.789		

Integration Time [sec] 0.1 Acquisition Time [sec] 134.8 Y Axis Linear

### Tune Parameters

#### ## Plasma Parameters ##

RF Power	1550 W	Nebulizer Pump	0.10 rps
RF Matching	1.94 V	S/C Temp	2 °C
Smpl Depth	8.0 mm	Gas Switch	Makeup Gas
Carrier Gas	1.08 L/min	Makeup/Dilution Gas	0.00 L/min
Option Gas	0.0 %		

#### ## Lenses Parameters ##

Extract 1	0.0 V	Cell Entrance	-40 V
Extract 2	-160.0 V	Cell Exit	-60 V
Omega Bias	-90 V	Deflect	1.0 V
Omega Lens	6.0 V	Plate Bias	-40 V

#### ## Cell Parameters ##

Use Gas	true	OctP Bias	-18.0 V
He Flow	3.3 mL/min	OctP RF	180 V
H2 Flow	0.0 mL/min	Energy Discrimination	5.0 V
3rd Gas Flow	0 %		

#### [NoGas]

Mass	Range	Count (Actual)	Response (Actual) [cps/ug/l]	Response (Required) [cps/ug/l]	Response (Flag)
7		8986	89862.36	1000.00	
89		19770	197695.63	1000.00	
205		12078	120782.86	1000.00	
102		3			

Mass	Resp Ratio (Actual)	Resp Ratio (Required)	Resp Ratio (Flag)
7			

# Tune Report

89 -  
 205 -  
 102 -

Mass	RSD% (Actual)	RSD% (Required)	RSD% (Flag)
7	0.45	5.00	
89	2.02	5.00	
205	2.22	5.00	
102	44.60		

Mass	Background (Actual)	Background (Required)	Background (Flag)
7			
89			
205			
102			

Mass	Rep. 1 Count	Rep. 2 Count	Rep. 3 Count	Rep. 4 Count	Rep. 5 Count
7	8932	9005	8977	9042	8976
89	19112	19820	19748	20028	20140
205	11627	12153	12164	12102	12345
102	2	1	4	4	3

Integration Time [sec] 0.1

Mass	Peak Height	Axis (Actual)	Axis (Required)	Axis (Flag)	W-50%	W-5% (Actual)	W-5% (Required)	W-5% (Flag)
7	1398.80	7.05	6.9 - 7.1		0.66	0.813	0.900	
89	3299.95	89.05	88.9 - 89.1		0.63	0.785	0.900	
205	2124.17	205.00	204.9 - 205.1		0.58	0.749	0.900	
102								

Integration Time [sec] 0.1 Acquisition Time [sec] 135.3 Y Axis Linear

### Tune Parameters

#### ## Plasma Parameters ##

RF Power	1550 W	Nebulizer Pump	0.10 rps
RF Matching	1.94 V	S/C Temp	2 °C
SmpI Depth	8.0 mm	Gas Switch	Makeup Gas
Carrier Gas	1.08 L/min	Makeup/Dilution Gas	0.00 L/min
Option Gas	0.0 %		

#### ## Lenses Parameters ##

Extract 1	0.0 V	Cell Entrance	-40 V
Extract 2	-160.0 V	Cell Exit	-60 V
Omega Bias	-90 V	Deflect	16.0 V
Omega Lens	6.0 V	Plate Bias	-40 V

#### ## Cell Parameters ##

Use Gas	false	OctP Bias	-8.0 V
---------	-------	-----------	--------



# Tune Report


He Flow	0.0 mL/min	OctP RF	180 V
H2 Flow	0.0 mL/min	Energy Discrimination	5.0 V
3rd Gas Flow	0 %		



# Tune Report

**Batch Folder** C:\Agilent\ICPMH\1\DATA\9K26027.b  
**Acq. Date-Time** 11/26/2019 10:10  
**Report Comment** 9K26027 Std Multi-mode Tune Report A19I052  
**Instrument Name** 7700x JP09240003

[H2]



Mass	Range	Count (Actual)	Response (Actual) [cps/ug/l]	Response (Required) [cps/ug/l]	Response (Flag)
59	1000	598	5975.60	1000.00	
89	5000	2706	27059.84	1000.00	
78	20	0			

Mass	Resp Ratio (Actual)	Resp Ratio (Required)	Resp Ratio (Flag)
59			-
89			-
78			-

Mass	RSD% (Actual)	RSD% (Required)	RSD% (Flag)
59	5.59	5.00	(F)
89	2.96	5.00	
78	261.78		

*see EPA tune for RSDs*  
*11/27/19*

Mass	Background (Actual)	Background (Required)	Background (Flag)
59			
89			
78			

**Integration Time [sec]** 0.1      **Sampling Period [sec]** 0.306

**Tune Parameters**  
**## Plasma Parameters ##**

RF Power	1550 W	Nebulizer Pump	0.10 rps
RF Matching	1.94 V	S/C Temp	2 °C
Smpl Depth	8.0 mm	Gas Switch	Makeup Gas
Carrier Gas	1.08 L/min	Makeup/Dilution Gas	0.00 L/min

# Tune Report

Option Gas                      0.0 %

**## Lenses Parameters ##**

Extract 1	0.0 V	Cell Entrance	-40 V
Extract 2	-160.0 V	Cell Exit	-60 V
Omega Bias	-90 V	Deflect	2.0 V
Omega Lens	6.0 V	Plate Bias	-40 V

**## Cell Parameters ##**

Use Gas	true	OctP Bias	-18.0 V
He Flow	0.0 mL/min	OctP RF	180 V
H2 Flow	3.3 mL/min	Energy Discrimination	5.0 V
3rd Gas Flow	0 %		

[He]

Mass	Range	Count (Actual)	Response (Actual) [cps/ug/l]	Response (Required) [cps/ug/l]	Response (Flag)
59	1000	710	7095.41	1000.00	
89	1000	788	7875.19	1000.00	
205	2000	999	9989.14	1000.00	
75	20	3			

Mass	Resp Ratio (Actual)	Resp Ratio (Required)	Resp Ratio (Flag)
59			-
89			-
205			-
75			-

Mass	RSD% (Actual)	RSD% (Required)	RSD% (Flag)
59	4.36	5.00	
89	4.69	5.00	
205	3.49	5.00	
75	68.64		

Mass	Background (Actual)	Background (Required)	Background (Flag)
59			
89			
205			
75			

Integration Time [sec]                      0.1      Sampling Period [sec]                      0.412

**Tune Parameters**

**## Plasma Parameters ##**

RF Power	1550 W	Nebulizer Pump	0.10 rps
RF Matching	1.94 V	S/C Temp	2 °C

# Tune Report

Smpl Depth	8.0 mm	Gas Switch	Makeup Gas
Carrier Gas	1.08 L/min	Makeup/Dilution Gas	0.00 L/min
Option Gas	0.0 %		

## ## Lenses Parameters ##

Extract 1	0.0 V	Cell Entrance	-40 V
Extract 2	-160.0 V	Cell Exit	-60 V
Omega Bias	-90 V	Deflect	1.0 V
Omega Lens	6.0 V	Plate Bias	-40 V

## ## Cell Parameters ##

Use Gas	true	OctP Bias	-18.0 V
He Flow	3.3 mL/min	OctP RF	180 V
H2 Flow	0.0 mL/min	Energy Discrimination	5.0 V
3rd Gas Flow	0 %		

## [NoGas]

Mass	Range	Count (Actual)	Response (Actual) [cps/ug/l]	Response (Required) [cps/ug/l]	Response (Flag)
7	2000	1415	14149.78	1000.00	
89	5000	3187	31872.38	1000.00	
205	5000	2022	20215.84	1000.00	
102	20	0			

Mass	Resp Ratio (Actual)	Resp Ratio (Required)	Resp Ratio (Flag)
7			-
89			-
205			-
102			-

Mass	RSD% (Actual)	RSD% (Required)	RSD% (Flag)
7	4.19	5.00	
89	2.23	5.00	
205	3.39	5.00	
102	264.41		

Mass	Background (Actual)	Background (Required)	Background (Flag)
7			
89			
205			
102			

Ratio (oxide)	156/140	1.359 %
Ratio (2+)	69/138	2.081 %

Integration Time [sec]	0.1	Sampling Period [sec]	0.413
------------------------	-----	-----------------------	-------



# Tune Report

## Tune Parameters

### ## Plasma Parameters ##

RF Power	1550 W	Nebulizer Pump	0.10 rps
RF Matching	1.94 V	S/C Temp	2 °C
Smpl Depth	8.0 mm	Gas Switch	Makeup Gas
Carrier Gas	1.08 L/min	Makeup/Dilution Gas	0.00 L/min
Option Gas	0.0 %		

### ## Lenses Parameters ##

Extract 1	0.0 V	Cell Entrance	-40 V
Extract 2	-160.0 V	Cell Exit	-60 V
Omega Bias	-90 V	Deflect	16.0 V
Omega Lens	6.0 V	Plate Bias	-40 V

### ## Cell Parameters ##

Use Gas	false	OctP Bias	-8.0 V
He Flow	0.0 mL/min	OctP RF	180 V
H2 Flow	0.0 mL/min	Energy Discrimination	5.0 V
3rd Gas Flow	0 %		

P/A Factor Tuning Report

=====  
Current Sample  
=====

Sample Name: 9K26027-ICV1  
Data File: 013\_ICV.d  
Acquired: 11/26/2019 12:03:29

=====  
Detector Parameters and P/A Factors  
=====

Discriminator: 4.5 mV  
AnalogHV: 1861 V  
PulseHV: 1720 V

Acquired: 11/25/2019 11:53:44

Mass[u]	Element	P/A Factor
6	Li	0.090004
7	Li	0.094505
11	B	0.102443
28	Si	0.098675
31	P	0.124270
45	Sc	0.126554
74	Ge	0.139907
88	Sr	0.140736
90	Zr	0.138257
103	Rh	0.144407
118	Sn	0.146234
159	Tb	0.148391
209	Bi	0.152692
197	Au	Signal too low
238	U	Signal too low

==== Independent Detector Parameters and P/A Factors ===

Tune Mode Name: H2  
Discriminator: 4.5 mV  
AnalogHV: 1861 V  
PulseHV: 1720 V

Acquired: 11/26/2019 11:40:43

Mass[u]	Element	P/A Factor
23	Na	0.111941
44	Ca	0.125957
45	Sc	0.123724
56	Fe	0.130227
57	Fe	0.129450
74	Ge	Signal too low
78	Se	Signal too low

-----  
Tune Mode Name: He  
Discriminator: 4.5 mV  
AnalogHV: 1861 V  
PulseHV: 1720 V

Acquired: 11/26/2019 11:51:10

Mass[u]	Element	P/A Factor
23	Na	0.111204
24	Mg	0.116145
27	Al	0.120438
39	K	0.122623
44	Ca	0.123577
51	V	0.125586
52	Cr	0.127390
55	Mn	0.128418
59	Co	0.131250
60	Ni	0.132213
65	Cu	0.135395
66	Zn	0.134172
138	Ba	0.138312

PAFactor.txt

205	Tl	0.143102	
45	Sc	Signal too low	
74	Ge	Signal too low	
75	As	Signal too low	
95	Mo	Signal too low	
103	Rh	Signal too low	
107	Ag	Signal too low	
111	Cd	Signal too low	
121	Sb	Signal too low	
159	Tb	Signal too low	
209	Bi	Signal too low	

-----

Tune Mode Name: NoGas  
 Discriminator: 4.5 mV  
 AnalogHV: 1861 V  
 PulseHV: 1720 V

Acquired: 11/26/2019 11:52:33

Mass[u]	Element	P/A Factor	
6	Li	0.089021	
45	Sc	0.123419	
47	Ti	0.122230	
65	Cu	0.133398	
74	Ge	0.136072	
103	Rh	0.137530	
111	Cd	0.138251	
159	Tb	0.140441	
182	W	0.140055	
206	Pb	0.142038	
207	Pb	0.143147	
208	Pb	0.144534	
209	Bi	0.146336	
7	Li	Signal too low	
9	Be	Signal too low	
106	[Cd]	Signal too low	
108	[Cd]	Signal too low	
201	Hg	Signal too low	

Created: 11/27/2019 10:22:31

### Quantitation Report - ICPMS5

Sample Name:	Rinse	Total Dilution:	1.0000
File Name:	001RINS.d	Vial:	3
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	Rinse
Acq Time:	11/26/2019 10:56:48	I.S. Reference File:	---
Comment:	rinse	Last Calibration:	N/A

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	LDR	QC Flag
Be	9	6	NoGas		ppb		838	0.18	
Na	23	45	He		ppb		3,911	90	
Mg	24	45	He		ppb		416	90	
Al	27	45	He		ppb		359	45	
K	39	45	He		ppb		22,442	90	
Ca	44	45	H2		ppb		410	90	
[Ca]	44	45	He		ppb		160		
Ti	47	45	NoGas		ppb		128	0.9	
V	51	74	He		ppb		2,095	0.9	
Cr	52	74	He		ppb		1,308	0.9	
Mn	55	74	He		ppb		223	0.9	
Fe	56	74	H2		ppb		41,348	45	
Co	59	74	He		ppb		816	0.18	
Ni	60	74	He		ppb		506	0.9	
Cu	65	74	He		ppb		73	0.9	
Zn	66	74	He		ppb		64	3.6	
As	75	74	He		ppb		20	0.9	
Se	78	74	H2		ppb		2	0.9	
Mo	95	103	He		ppb		50	0.9	
Ag	107	103	He		ppb		1	0.18	
Cd	111	103	He		ppb		1		
[Cd]	111	103	NoGas		ppb		3	0.18	
Sb	121	103	He		ppb		38	0.9	
Ba	138	159	He		ppb		1,787	0.9	
W	182	159	NoGas		ppb		52		
Hg	201	159	NoGas		ppt		3	72	
Tl	205	159	He		ppb		1,272	0.18	
Pb	208	159	NoGas		ppb		306	0.18	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	4,521	3.6	0	Pulse		
Sc	45	H2	822	13.4	0	Pulse		
Sc	45	He	42	46.3	0	Pulse		Note RSD; OK < 20%
Sc	45	NoGas	923	12.8	0	Pulse		
Ge	74	H2	163	8.0	0	Pulse		
Ge	74	He	45	27.0	0	Pulse		Note RSD; OK < 20%
Ge	74	NoGas	247	12.4	0	Pulse		
Rh	103	He	180	8.5	0	Pulse		
Rh	103	NoGas	371	8.8	0	Pulse		
Tb	159	He	20	44.1	0	Pulse		Note RSD; OK < 20%
Tb	159	NoGas	62	16.4	0	Pulse		Note RSD; OK < 20%
Bi	209	He	101	10.1	0	Pulse		
Bi	209	NoGas	247	11.1	0	Pulse		

### Quantitation Report - ICPMS5

Sample Name:	Rinse	Total Dilution:	1.0000
File Name:	002RINS.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	Rinse
Acq Time:	11/26/2019 11:01:32	I.S. Reference File:	---
Comment:	Cal Bik check	Last Calibration:	N/A

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	LDR	QC Flag
Be	9	6	NoGas		ppb		33	0.18	
Na	23	45	He		ppb		3,107	90	
Mg	24	45	He		ppb		331	90	
Al	27	45	He		ppb		111	45	
K	39	45	He		ppb		24,257	90	
Ca	44	45	H2		ppb		512	90	
[Ca]	44	45	He		ppb		187		
Ti	47	45	NoGas		ppb		23	0.9	
V	51	74	He		ppb		2,105	0.9	
Cr	52	74	He		ppb		200	0.9	
Mn	55	74	He		ppb		60	0.9	
Fe	56	74	H2		ppb		8,828	45	
Co	59	74	He		ppb		8	0.18	
Ni	60	74	He		ppb		120	0.9	
Cu	65	74	He		ppb		26	0.9	
Zn	66	74	He		ppb		51	3.6	
As	75	74	He		ppb		26	0.9	
Se	78	74	H2		ppb		2	0.9	
Mo	95	103	He		ppb		0	0.9	
Ag	107	103	He		ppb		2	0.18	
Cd	111	103	He		ppb		2		
[Cd]	111	103	NoGas		ppb		3	0.18	
Sb	121	103	He		ppb		28	0.9	
Ba	138	159	He		ppb		80	0.9	
W	182	159	NoGas		ppb		27		
Hg	201	159	NoGas		ppt		2	72	
Tl	205	159	He		ppb		39	0.18	
Pb	208	159	NoGas		ppb		612	0.18	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	952,664	0.8	0	Analog		
Sc	45	H2	1,756,878	1.4	0	Analog		
Sc	45	He	267,451	1.5	0	Pulse		
Sc	45	NoGas	2,693,888	1.2	0	Analog		
Ge	74	H2	550,903	0.4	0	Pulse		
Ge	74	He	162,181	0.8	0	Pulse		
Ge	74	NoGas	711,053	1.0	0	Pulse		
Rh	103	He	370,150	0.9	0	Pulse		
Rh	103	NoGas	758,142	0.6	0	Pulse		
Tb	159	He	522,110	1.0	0	Pulse		
Tb	159	NoGas	1,259,465	0.4	0	Pulse		
Bi	209	He	309,535	1.2	0	Pulse		
Bi	209	NoGas	741,991	0.7	0	Pulse		

### Calibration Standard Report - ICPMS5

Sample Name: **9K26027-CAL0** Total Dilution: **1.0000**  
 File Name: 003CALB.d Vial: 1  
 File Path: C:\Agilent\ICPMH\1\DATA\9K26027.b Sample Type: CalBlk  
 Acq Time: 11/26/2019 11:06:14 I.S. Reference File: 003CALB.d  
 Comment: **Cal Blk (3.5% HNO3 + 0.4% HCl)** Last Calibration: 11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	0	ppb	N/A	31	40.6	
Na	23	45	He	0	ppb	N/A	3,064	1.7	
Mg	24	45	He	0	ppb	N/A	373	15.5	
Al	27	45	He	0	ppb	N/A	86	6.0	
K	39	45	He	0	ppb	N/A	23,727	1.9	
Ca	44	45	H2	0	ppb	N/A	427	15.3	
[Ca]	44	45	He	0	ppb	N/A	151	37.7	
Ti	47	45	NoGas	0	ppb	N/A	28	71.3	
V	51	74	He	0	ppb	N/A	2,051	2.1	
Cr	52	74	He	0	ppb	N/A	224	23.1	
Mn	55	74	He	0	ppb	N/A	40	54.6	
Fe	56	74	H2	0	ppb	N/A	9,147	1.0	
Co	59	74	He	0	ppb	N/A	11	34.6	
Ni	60	74	He	0	ppb	N/A	96	13.2	
Cu	65	74	He	0	ppb	N/A	36	39.0	
Zn	66	74	He	0	ppb	N/A	30	22.2	
As	75	74	He	0	ppb	N/A	25	19.9	
Se	78	74	H2	0	ppb	N/A	3	34.6	
Mo	95	103	He	0	ppb	N/A	2	86.6	
Ag	107	103	He	0	ppb	N/A	4	86.6	
Cd	111	103	He	0	ppb	N/A	2	86.6	
[Cd]	111	103	NoGas	0	ppb	N/A	8	208.1	
Sb	121	103	He	0	ppb	N/A	36	42.3	
Ba	138	159	He	0	ppb	N/A	80	28.9	
W	182	159	NoGas	0	ppb	N/A	9	114.5	
Hg	201	159	NoGas	0.273	ppt	559.3	3	50.0	
Tl	205	159	He	0	ppb	N/A	27	43.3	
Pb	208	159	NoGas	0	ppb	N/A	576	6.9	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	943,670	0.7	943670.243333333	Analog	100.0	
Sc	45	H2	1,761,204	1.0	1761203.933333333	Analog	100.0	
Sc	45	He	270,213	1.3	270213.02	Pulse	100.0	
Sc	45	NoGas	2,719,053	1.9	2719052.54	Analog	100.0	
Ge	74	H2	547,888	0.2	547887.95	Pulse	100.0	
Ge	74	He	161,578	0.7	161577.683333333	Pulse	100.0	
Ge	74	NoGas	710,934	0.8	710934.333333333	Pulse	100.0	
Rh	103	He	367,686	0.1	367685.51	Pulse	100.0	
Rh	103	NoGas	751,394	0.4	751394.163333333	Pulse	100.0	
Tb	159	He	522,975	0.9	522974.92	Pulse	100.0	
Tb	159	NoGas	1,255,415	0.3	1255414.6	Pulse	100.0	
Bi	209	He	308,813	1.0	308812.996666667	Pulse	100.0	
Bi	209	NoGas	737,867	0.7	737867.09	Pulse	100.0	

### Calibration Standard Report - ICPMS5

Sample Name:	9K26027-CAL1	Total Dilution:	1.0000
File Name:	004CAL5.d	Vial:	1102
File Path:	C:\Agilent\ICPMH1\DATA\9K26027.b	Sample Type:	CalStd
Acq Time:	11/26/2019 11:10:56	I.S. Reference File:	003CALB.d
Comment:	A19K144 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

FullQuant Table:

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	0.181	ppb	9.6	511	7.7	
Na	23	45	He	8.948	ppb	2.2	11,722	1.1	
Mg	24	45	He	9.407	ppb	0.9	5,470	0.8	
Al	27	45	He	9.328	ppb	6.0	2,834	5.2	
K	39	45	He	8.829	ppb	8.3	28,147	1.0	
Ca	44	45	H2	8.363	ppb	3.2	2,090	2.4	
[Ca]	44	45	He	10.252	ppb	16.2	400	10.4	
Ti	47	45	NoGas	0.174	ppb	18.2	213	15.6	
V	51	74	He	0.179	ppb	14.4	2,659	2.8	
Cr	52	74	He	0.167	ppb	13.3	859	10.8	
Mn	55	74	He	0.17	ppb	12.0	503	11.3	
Fe	56	74	H2	8.853	ppb	0.7	98,433	0.6	
Co	59	74	He	0.195	ppb	3.2	1,020	2.1	
Ni	60	74	He	0.166	ppb	28.0	303	20.0	
Cu	65	74	He	0.211	ppb	15.1	360	12.5	
Zn	66	74	He	0.205	ppb	17.6	154	14.7	
As	75	74	He	0.21	ppb	3.1	106	3.3	
Se	78	74	H2	0.173	ppb	11.6	50	11.0	
Mo	95	103	He	0.201	ppb	20.3	324	20.0	
Ag	107	103	He	0.174	ppb	7.2	811	6.8	
Cd	111	103	He	0.189	ppb	1.1	150	1.4	
[Cd]	111	103	NoGas	0.177	ppb	8.9	388	9.2	
Sb	121	103	He	0.136	ppb	12.4	321	11.4	
Ba	138	159	He	0.191	ppb	19.8	917	17.5	
W	182	159	NoGas	0.001	ppb	109.1	20	60.1	
Hg	201	159	NoGas	9.611	ppt	7.9	12	6.3	
Tl	205	159	He	0.175	ppb	2.9	1,356	3.0	
Pb	208	159	NoGas	0.182	ppb	0.3	4,729	0.6	

ISTD Table:

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	942,450	1.3	943670.243333333	Analog	99.9	
Sc	45	H2	1,731,271	0.7	1761203.93333333	Analog	98.3	
Sc	45	He	271,890	0.6	270213.02	Pulse	100.6	
Sc	45	NoGas	2,674,421	1.2	2719052.54	Analog	98.4	
Ge	74	H2	551,773	0.2	547887.95	Pulse	100.7	
Ge	74	He	163,788	1.1	161577.683333333	Pulse	101.4	
Ge	74	NoGas	715,490	0.8	710934.333333333	Pulse	100.6	
Rh	103	He	371,304	0.4	367685.51	Pulse	101.0	
Rh	103	NoGas	757,512	0.5	751394.163333333	Pulse	100.8	
Tb	159	He	524,217	0.9	522974.92	Pulse	100.2	
Tb	159	NoGas	1,261,973	0.3	1255414.6	Pulse	100.5	
Bi	209	He	311,205	0.7	308812.996666667	Pulse	100.8	
Bi	209	NoGas	737,079	0.3	737867.09	Pulse	99.9	

### Calibration Standard Report - ICPMS5

Sample Name:	9K26027-CAL2	Total Dilution:	1.0000
File Name:	005CAL5.d	Vial:	1103
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CalStd
Acq Time:	11/26/2019 11:15:57	I.S. Reference File:	003CALB.d
Comment:	A19K145 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	0.891	ppb	3.4	2,334	5.3	
Na	23	45	He	44.804	ppb	0.5	46,127	0.5	
Mg	24	45	He	44.653	ppb	1.2	24,440	1.2	
Al	27	45	He	44.281	ppb	0.7	13,071	0.9	
K	39	45	He	46.721	ppb	1.9	46,273	0.3	
Ca	44	45	H2	44.51	ppb	4.9	9,168	3.9	
[Ca]	44	45	He	46.478	ppb	7.2	1,271	6.3	
Ti	47	45	NoGas	0.96	ppb	8.1	1,046	7.0	
V	51	74	He	0.854	ppb	3.0	4,840	2.3	
Cr	52	74	He	0.886	ppb	5.1	3,564	5.3	
Mn	55	74	He	0.882	ppb	5.3	2,427	5.0	
Fe	56	74	H2	44.543	ppb	0.4	453,968	0.6	
Co	59	74	He	0.919	ppb	3.7	4,742	3.4	
Ni	60	74	He	1.037	ppb	1.9	1,377	2.2	
Cu	65	74	He	1	ppb	9.2	1,566	8.9	
Zn	66	74	He	0.952	ppb	4.3	604	4.1	
As	75	74	He	0.9	ppb	2.7	369	2.6	
Se	78	74	H2	0.903	ppb	7.7	246	7.8	
Mo	95	103	He	0.895	ppb	9.0	1,427	9.1	
Ag	107	103	He	0.857	ppb	2.1	3,952	2.8	
Cd	111	103	He	0.856	ppb	4.1	668	4.9	
[Cd]	111	103	NoGas	0.821	ppb	9.2	1,751	9.0	
Sb	121	103	He	0.864	ppb	1.4	1,828	1.0	
Ba	138	159	He	0.95	ppb	2.8	4,233	2.6	
W	182	159	NoGas	0.002	ppb	50.4	26	32.8	
Hg	201	159	NoGas	39.474	ppt	13.8	41	13.1	
Tl	205	159	He	0.886	ppb	4.0	6,723	3.8	
Pb	208	159	NoGas	0.851	ppb	1.1	19,879	0.8	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref,CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	918,618	2.0	943670.243333333	Analog	97.3	
Sc	45	H2	1,704,637	0.7	1761203.933333333	Analog	96.8	
Sc	45	He	270,624	0.7	270213.02	Pulse	100.2	
Sc	45	NoGas	2,665,556	1.5	2719052.54	Analog	98.0	
Ge	74	H2	546,785	0.3	547887.95	Pulse	99.8	
Ge	74	He	163,222	0.6	161577.683333333	Pulse	101.0	
Ge	74	NoGas	711,395	0.6	710934.333333333	Pulse	100.1	
Rh	103	He	368,466	0.8	367685.51	Pulse	100.2	
Rh	103	NoGas	748,509	0.2	751394.163333333	Pulse	99.6	
Tb	159	He	523,346	0.2	522974.92	Pulse	100.1	
Tb	159	NoGas	1,253,491	0.3	1255414.6	Pulse	99.8	
Bi	209	He	307,178	0.8	308812.996666667	Pulse	99.5	
Bi	209	NoGas	730,460	0.2	737867.09	Pulse	99.0	



### Calibration Standard Report - ICPMS5

Sample Name:	9K26027-CAL3	Total Dilution:	1.0000
File Name:	006CAL5.d	Vial:	1104
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CalStd
Acq Time:	11/26/2019 11:20:55	I.S. Reference File:	003CALB.d
Comment:	A19K146 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	1.693	ppb	1.5	4,506	1.3	
Na	23	45	He	91.491	ppb	0.3	91,004	0.9	
Mg	24	45	He	91.67	ppb	0.3	49,785	0.8	
Al	27	45	He	91.932	ppb	0.7	27,045	0.2	
K	39	45	He	94.823	ppb	2.3	69,462	2.0	
Ca	44	45	H2	90.303	ppb	3.4	18,274	3.4	
[Ca]	44	45	He	92.666	ppb	6.8	2,385	6.2	
Ti	47	45	NoGas	1.91	ppb	3.9	2,061	4.0	
V	51	74	He	1.758	ppb	1.8	7,766	0.9	
Cr	52	74	He	1.822	ppb	1.4	7,087	2.1	
Mn	55	74	He	1.784	ppb	4.5	4,867	4.0	
Fe	56	74	H2	90.703	ppb	0.6	916,340	0.3	
Co	59	74	He	1.845	ppb	3.0	9,511	3.1	
Ni	60	74	He	1.92	ppb	1.7	2,466	2.3	
Cu	65	74	He	1.957	ppb	2.2	3,028	2.8	
Zn	66	74	He	1.835	ppb	6.0	1,137	5.2	
As	75	74	He	1.898	ppb	2.9	750	2.3	
Se	78	74	H2	1.846	ppb	10.0	500	10.3	
Mo	95	103	He	1.784	ppb	8.0	2,846	7.1	
Ag	107	103	He	1.813	ppb	1.4	8,369	2.1	
Cd	111	103	He	1.769	ppb	2.2	1,382	2.9	
[Cd]	111	103	NoGas	1.751	ppb	3.0	3,727	2.8	
Sb	121	103	He	1.775	ppb	2.3	3,725	2.6	
Ba	138	159	He	1.893	ppb	3.8	8,368	4.6	
W	182	159	NoGas	0.001	ppb	75.8	16	32.7	
Hg	201	159	NoGas	71.612	ppt	9.9	73	9.1	
Tl	205	159	He	1.798	ppb	1.8	13,639	2.0	
Pb	208	159	NoGas	1.781	ppb	0.9	41,125	0.4	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD.Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	939,550	0.3	943670.243333333	Analog	99.6	
Sc	45	H2	1,713,432	0.4	1761203.93333333	Analog	97.3	
Sc	45	He	270,645	0.6	270213.02	Pulse	100.2	
Sc	45	NoGas	2,673,152	1.3	2719052.54	Analog	98.3	
Ge	74	H2	547,618	0.4	547887.95	Pulse	100.0	
Ge	74	He	163,179	0.9	161577.683333333	Pulse	101.0	
Ge	74	NoGas	712,946	0.6	710934.333333333	Pulse	100.3	
Rh	103	He	369,118	1.0	367685.51	Pulse	100.4	
Rh	103	NoGas	749,245	0.2	751394.163333333	Pulse	99.7	
Tb	159	He	524,146	1.3	522974.92	Pulse	100.2	
Tb	159	NoGas	1,257,566	0.5	1255414.6	Pulse	100.2	
Bi	209	He	309,215	1.4	308812.996666667	Pulse	100.1	
Bi	209	NoGas	734,327	0.3	737867.09	Pulse	99.5	

### Calibration Standard Report - ICPMS5

Sample Name:	9K26027-CAL4	Total Dilution:	1.0000
File Name:	007CAL5.d	Vial:	1105
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CalStd
Acq Time:	11/26/2019 11:25:53	I.S. Reference File:	003CALB.d
Comment:	A19K147 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	3.431	ppb	1.9	9,062	0.9	
Na	23	45	He	184.503	ppb	0.8	178,617	0.3	
Mg	24	45	He	185.937	ppb	0.4	99,605	0.8	
Al	27	45	He	183.126	ppb	1.3	53,261	1.7	
K	39	45	He	187.286	ppb	1.2	112,895	1.3	
Ca	44	45	H2	179.796	ppb	1.2	35,987	1.1	
[Ca]	44	45	He	185.341	ppb	7.3	4,572	6.3	
Ti	47	45	NoGas	3.719	ppb	1.9	3,978	1.6	
V	51	74	He	3.504	ppb	1.7	13,395	1.3	
Cr	52	74	He	3.609	ppb	1.2	13,788	1.5	
Mn	55	74	He	3.585	ppb	0.3	9,723	0.7	
Fe	56	74	H2	184.631	ppb	0.6	1,843,313	0.9	
Co	59	74	He	3.633	ppb	1.4	18,682	1.8	
Ni	60	74	He	3.764	ppb	1.7	4,732	1.1	
Cu	65	74	He	4.066	ppb	1.9	6,242	2.1	
Zn	66	74	He	3.869	ppb	1.3	2,359	0.9	
As	75	74	He	3.603	ppb	4.2	1,399	4.0	
Se	78	74	H2	3.764	ppb	1.0	1,009	1.0	
Mo	95	103	He	3.497	ppb	1.5	5,533	1.3	
Ag	107	103	He	3.598	ppb	0.5	16,469	0.4	
Cd	111	103	He	3.602	ppb	1.8	2,788	2.6	
[Cd]	111	103	NoGas	3.425	ppb	4.1	7,204	3.9	
Sb	121	103	He	3.582	ppb	2.3	7,418	1.4	
Ba	138	159	He	3.826	ppb	0.7	16,821	0.3	
W	182	159	NoGas	0.002	ppb	40.8	23	24.7	
Hg	201	159	NoGas	138.183	ppt	5.5	138	4.6	
Tl	205	159	He	3.518	ppb	0.7	26,660	1.0	
Pb	208	159	NoGas	3.522	ppb	0.6	80,751	0.2	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref/CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	935,847	1.4	943670.243333333	Analog	99.2	
Sc	45	H2	1,714,180	1.1	1761203.933333333	Analog	97.3	
Sc	45	He	267,982	0.8	270213.02	Pulse	99.2	
Sc	45	NoGas	2,667,366	0.4	2719052.54	Analog	98.1	
Ge	74	H2	543,928	0.4	547887.95	Pulse	99.3	
Ge	74	He	162,874	0.5	161577.683333333	Pulse	100.8	
Ge	74	NoGas	710,219	0.5	710934.333333333	Pulse	99.9	
Rh	103	He	366,056	0.9	367685.51	Pulse	99.6	
Rh	103	NoGas	741,146	0.9	751394.163333333	Pulse	98.6	
Tb	159	He	523,981	0.7	522974.92	Pulse	100.2	
Tb	159	NoGas	1,257,397	0.8	1255414.6	Pulse	100.2	
Bi	209	He	305,985	0.7	308812.996666667	Pulse	99.1	
Bi	209	NoGas	732,928	0.6	737867.09	Pulse	99.3	

### Calibration Standard Report - ICPMS5

Sample Name:	9K26027-CAL5	Total Dilution:	1.0000
File Name:	008CAL5.d	Vial:	1106
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CalStd
Acq Time:	11/26/2019 11:30:51	I.S. Reference File:	003CALB.d
Comment:	A19K148 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

FullQuant Table:

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	9.513	ppb	2.8	24,256	2.0	
Na	23	45	He	404.816	ppb	0.4	385,065	0.2	
Mg	24	45	He	407.395	ppb	0.9	215,987	0.5	
Al	27	45	He	403.103	ppb	0.6	116,163	0.6	
K	39	45	He	412.281	ppb	0.9	218,423	0.7	
Ca	44	45	H2	393.767	ppb	0.5	78,402	1.2	
[Ca]	44	45	He	424.405	ppb	2.7	10,194	2.5	
Ti	47	45	NoGas	20.069	ppb	0.6	20,832	1.0	
V	51	74	He	19.745	ppb	0.8	64,351	1.0	
Cr	52	74	He	19.988	ppb	1.2	73,564	0.6	
Mn	55	74	He	20.116	ppb	1.7	53,102	1.8	
Fe	56	74	H2	409.638	ppb	1.1	4,059,566	1.2	
Co	59	74	He	20.278	ppb	0.8	101,776	1.0	
Ni	60	74	He	21.552	ppb	2.5	26,015	3.1	
Cu	65	74	He	22.321	ppb	0.8	33,304	1.5	
Zn	66	74	He	21.214	ppb	0.9	12,499	0.9	
As	75	74	He	20.134	ppb	1.5	7,519	1.9	
Se	78	74	H2	10.07	ppb	4.1	2,681	4.3	
Mo	95	103	He	9.91	ppb	2.8	15,417	3.1	
Ag	107	103	He	9.867	ppb	1.2	44,406	0.9	
Cd	111	103	He	19.866	ppb	1.2	15,106	1.4	
[Cd]	111	103	NoGas	19.281	ppb	1.0	39,704	0.6	
Sb	121	103	He	9.59	ppb	1.5	19,472	1.7	
Ba	138	159	He	21.274	ppb	1.0	91,939	0.7	
W	182	159	NoGas	0.004	ppb	35.2	39	27.5	
Hg	201	159	NoGas	394.322	ppt	5.8	381	5.9	
Tl	205	159	He	9.817	ppb	0.8	73,363	1.1	
Pb	208	159	NoGas	19.576	ppb	0.3	437,907	0.0	

ISTD Table:

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	905,543	0.8	943670.243333333	Analog	96.0	
Sc	45	H2	1,715,986	1.7	1761203.933333333	Analog	97.4	
Sc	45	He	265,761	0.4	270213.02	Pulse	98.4	
Sc	45	NoGas	2,603,447	0.6	2719052.54	Analog	95.7	
Ge	74	H2	541,382	0.2	547887.95	Pulse	98.8	
Ge	74	He	159,054	0.7	161577.683333333	Pulse	98.4	
Ge	74	NoGas	696,856	1.0	710934.333333333	Pulse	98.0	
Rh	103	He	359,942	0.3	367685.51	Pulse	97.9	
Rh	103	NoGas	726,133	0.4	751394.163333333	Pulse	96.6	
Tb	159	He	517,103	0.6	522974.92	Pulse	98.9	
Tb	159	NoGas	1,233,952	0.3	1255414.6	Pulse	98.3	
Bi	209	He	305,301	0.9	308812.996666667	Pulse	98.9	
Bi	209	NoGas	725,594	0.2	737867.09	Pulse	98.3	

### Calibration Standard Report - ICPMS5

Sample Name:	9K26027-CAL6	Total Dilution:	1.0000
File Name:	009CAL5.d	Vial:	1107
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CalStd
Acq Time:	11/26/2019 11:35:47	I.S. Reference File:	003CALB.d
Comment:	A19K149	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	49.185	ppb	2.0	117,522	0.9	
Na	23	45	He	2529.167	ppb	0.4	2,293,971	0.2	
Mg	24	45	He	2558.81	ppb	0.5	1,300,308	1.1	
Al	27	45	He	2501.244	ppb	0.4	691,422	0.3	
K	39	45	He	2564.293	ppb	0.5	1,187,082	0.6	
Ca	44	45	H2	2476.737	ppb	0.6	470,081	0.4	
[Ca]	44	45	He	2536.074	ppb	1.1	57,762	0.8	
Ti	47	45	NoGas	49.652	ppb	0.4	49,457	0.6	
V	51	74	He	49.179	ppb	0.3	151,674	0.2	
Cr	52	74	He	49.609	ppb	0.6	175,782	0.5	
Mn	55	74	He	50.06	ppb	0.5	127,387	0.6	
Fe	56	74	H2	2540.112	ppb	0.4	24,179,961	0.5	
Co	59	74	He	50.287	ppb	0.5	243,400	0.4	
Ni	60	74	He	52.401	ppb	0.2	60,866	0.1	
Cu	65	74	He	53.562	ppb	0.3	77,024	0.4	
Zn	66	74	He	51.671	ppb	3.0	29,320	3.1	
As	75	74	He	49.593	ppb	0.8	17,826	0.8	
Se	78	74	H2	50.03	ppb	1.5	12,807	1.0	
Mo	95	103	He	49.417	ppb	1.1	73,463	1.2	
Ag	107	103	He	49.708	ppb	0.5	213,771	0.2	
Cd	111	103	He	49.578	ppb	1.5	36,021	1.0	
[Cd]	111	103	NoGas	48.034	ppb	0.7	93,715	0.7	
Sb	121	103	He	49.23	ppb	0.4	95,390	0.7	
Ba	138	159	He	52.397	ppb	0.5	222,280	1.1	
W	182	159	NoGas	0.012	ppb	14.2	97	12.4	
Hg	201	159	NoGas	2014.764	ppt	1.1	1,894	1.6	
Tl	205	159	He	49.321	ppb	0.5	361,876	0.4	
Pb	208	159	NoGas	48.615	ppb	0.3	1,063,990	0.2	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	849,418	1.7	943670.243333333	Mix	90.0	
Sc	45	H2	1,643,004	0.2	1761203.933333333	Analog	93.3	
Sc	45	He	255,090	0.6	270213.02	Pulse	94.4	
Sc	45	NoGas	2,500,152	0.6	2719052.54	Analog	91.9	
Ge	74	H2	521,005	0.4	547887.95	Pulse	95.1	
Ge	74	He	153,393	0.1	161577.683333333	Pulse	94.9	
Ge	74	NoGas	663,570	0.5	710934.333333333	Pulse	93.3	
Rh	103	He	343,992	0.6	367685.51	Pulse	93.6	
Rh	103	NoGas	688,055	0.4	751394.163333333	Pulse	91.6	
Tb	159	He	507,833	0.7	522974.92	Pulse	97.1	
Tb	159	NoGas	1,208,227	0.6	1255414.6	Pulse	96.2	
Bi	209	He	297,643	1.0	308812.996666667	Pulse	96.4	
Bi	209	NoGas	706,882	0.2	737867.09	Pulse	95.8	

### Calibration Standard Report - ICPMS5

Sample Name: <b>9K26027-CAL7</b>	Total Dilution: <b>1.0000</b>
File Name: <b>010CAL5.d</b>	Vial: <b>1108</b>
File Path: <b>C:\Agilent\ICPMH\1\DATA\9K26027.b</b>	Sample Type: <b>CalStd</b>
Acq Time: <b>11/26/2019 11:40:41</b>	I.S. Reference File: <b>003CALB.d</b>
Comment: <b>A19K150</b>	Last Calibration: <b>11/26/2019 11:53:02</b>

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	100.464	ppb	0.4	220,377	0.3	
Na	23	45	He	4104.089	ppb	1.1	3,421,070	0.9	
Mg	24	45	He	4189.702	ppb	1.2	1,957,376	0.8	
Al	27	45	He	4028.629	ppb	0.4	1,023,947	0.4	
K	39	45	He	4179.59	ppb	1.4	1,766,156	1.6	
Ca	44	45	H2	3937.429	ppb	0.8	709,383	0.6	
[Ca]	44	45	He	4120.13	ppb	1.2	86,205	0.8	
Ti	47	45	NoGas	200.38	ppb	1.2	181,370	0.3	
V	51	74	He	197.289	ppb	0.3	560,368	0.4	
Cr	52	74	He	198.05	ppb	0.2	651,991	0.8	
Mn	55	74	He	199.772	ppb	0.6	472,627	0.7	
Fe	56	74	H2	4014.394	ppb	0.1	36,326,958	0.5	
Co	59	74	He	200.202	ppb	0.3	901,072	0.4	
Ni	60	74	He	210.727	ppb	0.5	227,357	0.1	
Cu	65	74	He	212.194	ppb	0.5	283,660	0.2	
Zn	66	74	He	209.49	ppb	0.2	110,461	0.8	
As	75	74	He	200.368	ppb	0.3	66,905	0.8	
Se	78	74	H2	99.971	ppb	1.3	24,328	0.8	
Mo	95	103	He	100.305	ppb	0.8	139,478	0.0	
Ag	107	103	He	100.159	ppb	0.8	402,928	1.0	
Cd	111	103	He	201.511	ppb	1.4	136,951	0.7	
[Cd]	111	103	NoGas	196.149	ppb	0.9	353,397	0.3	
Sb	121	103	He	100.427	ppb	0.5	181,996	0.9	
Ba	138	159	He	207.046	ppb	0.5	845,081	0.5	
W	182	159	NoGas	0.026	ppb	4.4	186	3.7	
Hg	201	159	NoGas	3993.371	ppt	0.6	3,580	0.7	
Tl	205	159	He	100.361	ppb	0.7	708,660	0.6	
Pb	208	159	NoGas	200.87	ppb	0.2	4,194,653	0.4	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref.CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	779,769	0.7	943670.243333333	Pulse	82.6	
Sc	45	H2	1,560,147	1.0	1761203.933333333	Analog	88.6	
Sc	45	He	234,553	0.4	270213.02	Pulse	86.8	
Sc	45	NoGas	2,272,935	0.9	2719052.54	Analog	83.6	
Ge	74	H2	495,343	0.6	547887.95	Pulse	90.4	
Ge	74	He	142,644	0.6	161577.683333333	Pulse	88.3	
Ge	74	NoGas	613,859	0.2	710934.333333333	Pulse	86.3	
Rh	103	He	321,782	0.8	367685.51	Pulse	87.5	
Rh	103	NoGas	635,449	0.7	751394.163333333	Pulse	84.6	
Tb	159	He	488,752	0.9	522974.92	Pulse	93.5	
Tb	159	NoGas	1,153,261	0.5	1255414.6	Pulse	91.9	
Bi	209	He	288,302	0.6	308812.996666667	Pulse	93.4	
Bi	209	NoGas	670,136	0.6	737867.09	Pulse	90.8	

### Calibration Standard Report - ICPMS5

Sample Name:	9K26027-CAL8	Total Dilution:	1.0000
File Name:	011CAL5.d	Vial:	1109
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CalStd
Acq Time:	11/26/2019 11:45:32	I.S. Reference File:	003CALB.d
Comment:	A19K151	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	0.02	ppb	8.1	67	5.0	
Na	23	45	He	10000.624	ppb	0.4	7,900,824	0.6	
Mg	24	45	He	10160.138	ppb	0.8	4,500,320	0.7	
Al	27	45	He	10068.675	ppb	0.3	2,426,399	0.4	
K	39	45	He	10140.3	ppb	0.6	4,034,962	0.8	
Ca	44	45	H2	10314.21	ppb	0.3	1,717,809	0.5	
[Ca]	44	45	He	10069.515	ppb	0.1	199,590	0.1	
Ti	47	45	NoGas	503.879	ppb	1.0	433,626	0.5	
V	51	74	He	501.178	ppb	1.4	1,340,700	1.5	
Cr	52	74	He	502.566	ppb	0.9	1,560,979	1.2	
Mn	55	74	He	495.722	ppb	0.6	1,106,660	0.4	
Fe	56	74	H2	9958.818	ppb	0.2	83,165,573	0.6	
Co	59	74	He	499.879	ppb	1.2	2,123,040	0.8	
Ni	60	74	He	512.555	ppb	0.5	521,740	0.3	
Cu	65	74	He	516.606	ppb	0.5	651,651	0.1	
Zn	66	74	He	518.376	ppb	0.9	257,888	0.4	
As	75	74	He	499.888	ppb	0.3	157,481	0.3	
Se	78	74	H2	0.114	ppb	22.4	28	20.7	
Mo	95	103	He	0.109	ppb	15.9	144	15.7	
Ag	107	103	He	0.014	ppb	75.2	56	70.3	
Cd	111	103	He	503.548	ppb	0.2	322,218	0.2	
[Cd]	111	103	NoGas	496.94	ppb	0.3	838,189	0.1	
Sb	121	103	He	0.138	ppb	11.5	264	10.3	
Ba	138	159	He	521.853	ppb	1.3	2,038,178	0.7	
W	182	159	NoGas	100	ppb	0.5	653,955	0.1	
Hg	201	159	NoGas	82.876	ppt	8.7	74	9.1	
Tl	205	159	He	0.038	ppb	23.0	278	20.4	
Pb	208	159	NoGas	499.808	ppb	0.4	10,058,905	0.3	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref.CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	741,357	0.3	943670.243333333	Pulse	78.6	
Sc	45	H2	1,442,643	0.2	1761203.933333333	Analog	81.9	
Sc	45	He	222,397	0.2	270213.02	Pulse	82.3	
Sc	45	NoGas	2,161,191	0.9	2719052.54	Analog	79.5	
Ge	74	H2	457,182	0.4	547887.95	Pulse	83.4	
Ge	74	He	134,607	0.4	161577.683333333	Pulse	83.3	
Ge	74	NoGas	576,611	0.4	710934.333333333	Pulse	81.1	
Rh	103	He	302,958	0.1	367685.51	Pulse	82.4	
Rh	103	NoGas	594,884	0.3	751394.163333333	Pulse	79.2	
Tb	159	He	467,721	0.7	522974.92	Pulse	89.4	
Tb	159	NoGas	1,111,559	0.7	1255414.6	Pulse	88.5	
Bi	209	He	276,676	0.8	308812.996666667	Pulse	89.6	
Bi	209	NoGas	632,858	0.3	737867.09	Pulse	85.8	

### Calibration Standard Report - ICPMS5

Sample Name: **9K26027-CAL9** Total Dilution: **1.0000**  
 File Name: **012CAL5.d** Vial: **1110**  
 File Path: **C:\Agilent\ICPMH\1\DATA\9K26027.b** Sample Type: **CalStd**  
 Acq Time: **11/26/2019 11:50:12** I.S. Reference File: **003CALB.d**  
 Comment: **A19K152** Last Calibration: **11/26/2019 11:53:02**

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	CPS RSD	QC Flag
Be	9	6	NoGas	0.017	ppb	56.4	60	33.3	
Na	23	45	He	49990.032	ppb	0.4	38,284,802	0.8	
Mg	24	45	He	49949.773	ppb	0.2	21,451,674	0.4	
Al	27	45	He	49983.874	ppb	0.4	11,679,392	0.8	
K	39	45	He	49954.224	ppb	0.8	19,199,392	1.0	
Ca	44	45	H2	49943.377	ppb	1.4	7,852,074	1.1	
[Ca]	44	45	He	49974.462	ppb	0.5	959,993	0.5	
Ti	47	45	NoGas	2499.2	ppb	1.2	2,143,694	1.0	
V	51	74	He	-0.295	ppb	N/A	864	0.5	
Cr	52	74	He	999.127	ppb	0.6	2,914,268	1.1	
Mn	55	74	He	2500.872	ppb	0.7	5,243,254	1.2	
Fe	56	74	H2	50004.985	ppb	0.1	378,458,412	0.5	
Co	59	74	He	0.192	ppb	1.2	776	1.8	
Ni	60	74	He	991.425	ppb	0.5	947,694	0.3	
Cu	65	74	He	989.032	ppb	0.3	1,171,617	0.3	
Zn	66	74	He	2495.522	ppb	0.5	1,165,856	0.2	
As	75	74	He	0.108	ppb	8.8	52	5.9	
Se	78	74	H2	0.081	ppb	26.9	19	22.9	
Mo	95	103	He	0.124	ppb	8.9	150	9.7	
Ag	107	103	He	0.021	ppb	28.5	74	26.2	
Cd	111	103	He	997.948	ppb	0.6	585,230	0.3	
[Cd]	111	103	NoGas	1002.414	ppb	1.6	1,575,102	1.0	
Sb	121	103	He	0.066	ppb	12.9	130	9.2	
Ba	138	159	He	2495.007	ppb	0.4	9,224,719	0.7	
W	182	159	NoGas	0.309	ppb	2.5	1,965	3.3	
Hg	201	159	NoGas	31.842	ppt	26.1	29	25.0	
Tl	205	159	He	0.003	ppb	53.7	41	24.8	
Pb	208	159	NoGas	0.148	ppb	2.5	3,371	3.0	

**ISTD Table:**


Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	746,834	0.2	943670.243333333	Pulse	79.1	
Sc	45	H2	1,362,370	2.5	1761203.93333333	Analog	77.4	
Sc	45	He	215,642	0.4	270213.02	Pulse	79.8	
Sc	45	NoGas	2,154,158	0.9	2719052.54	Analog	79.2	
Ge	74	H2	414,374	0.5	547887.95	Pulse	75.6	
Ge	74	He	126,414	0.6	161577.683333333	Pulse	78.2	
Ge	74	NoGas	546,673	1.0	710934.333333333	Pulse	76.9	
Rh	103	He	277,658	1.0	367685.51	Pulse	75.5	
Rh	103	NoGas	554,226	0.9	751394.163333333	Pulse	73.8	
Tb	159	He	442,754	0.6	522974.92	Pulse	84.7	
Tb	159	NoGas	1,075,936	1.1	1255414.6	Pulse	85.7	
Bi	209	He	248,268	0.7	308812.996666667	Pulse	80.4	
Bi	209	NoGas	592,880	0.8	737867.09	Pulse	80.4	

Calibration for 013\_ICV.d

Batch Folder: C:\Agilent\ICPMH\1\DATA\9K26027.b\  
 Analysis File: 9K26027.batch.bin  
 DA Date-Time: 11/26/2019 12:06:14  
 Calibration Title:  
 Calibration Method: External Calibration  
 VIS Interpolation Fit:

Level	Standard Data File	Sample Name	Acq. Date-Time
1	003CALB.d	9K26027-CAL0	11/26/2019 11:06:14
2	004CALS.d	9K26027-CAL1	11/26/2019 11:10:56
3	005CALS.d	9K26027-CAL2	11/26/2019 11:15:57
4	006CALS.d	9K26027-CAL3	11/26/2019 11:20:55
5	007CALS.d	9K26027-CAL4	11/26/2019 11:25:53
6	008CALS.d	9K26027-CAL5	11/26/2019 11:30:51
7	009CALS.d	9K26027-CAL6	11/26/2019 11:35:47
8	010CALS.d	9K26027-CAL7	11/26/2019 11:40:41
9	011CALS.d	9K26027-CAL8	11/26/2019 11:45:32
10	012CALS.d	9K26027-CAL9	11/26/2019 11:50:12





	Rjct	Conc	Calc Conc	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	31	0.000	P	40.8
2	<input type="checkbox"/>	0.180	0.181	511	0.001	P	9.0
3	<input type="checkbox"/>	0.900	0.891	2,334	0.003	P	3.4
4	<input type="checkbox"/>	1.800	1.693	4,506	0.005	P	1.5
5	<input type="checkbox"/>	3.600	3.431	9,062	0.010	P	1.9
6	<input type="checkbox"/>	10.000	9.513	24,256	0.027	P	2.8
7	<input type="checkbox"/>	50.000	49.185	117,522	0.138	P	2.0
8	<input type="checkbox"/>	100.000	100.464	220,377	0.283	P	0.4
9	<input type="checkbox"/>			67	0.000	P	5.2
10	<input type="checkbox"/>			60	0.000	P	33.2

$y = 0.0028 * x + 3.2990E-005$


R = 0.9999

DL = 0.01434

BEC = 0.01173

Weight: <None>

Min Conc: <None>



	Rjct	Conc	Calc Conc	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	3,064	0.011	P	2.3
2	<input type="checkbox"/>			11,722	0.043	P	1.6
3	<input type="checkbox"/>	45.000	44.804	46,127	0.170	P	0.5
4	<input type="checkbox"/>	90.000	91.491	91,004	0.336	P	0.3
5	<input type="checkbox"/>	180.000	184.503	178,617	0.667	P	0.8
6	<input type="checkbox"/>	400.000	404.816	385,065	1.449	P	0.4
7	<input type="checkbox"/>	2500.000	2529.167	2,293,971	8.993	A	0.4
8	<input type="checkbox"/>	4000.000	4104.089	3,421,070	14.586	A	1.1
9	<input type="checkbox"/>	10000.000	10000.624	7,900,824	35.526	A	0.4
10	<input type="checkbox"/>	50000.000	49990.032	38,284,802	177.537	A	0.4

$y = 0.0036 * x + 0.0113$


R = 1.0000

DL = 0.2186

BEC = 3.193

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	373	0.001	P	16.5
2	<input type="checkbox"/>			5,470	0.020	P	0.9
3	<input type="checkbox"/>	45.000	44.653	24,440	0.090	P	1.2
4	<input type="checkbox"/>	90.000	91.670	49,785	0.184	P	0.3
5	<input type="checkbox"/>	180.000	185.937	99,605	0.372	P	0.4
6	<input type="checkbox"/>	400.000	407.395	215,987	0.813	P	0.9
7	<input type="checkbox"/>	2500.000	2558.810	1,300,308	5.097	A	0.5
8	<input type="checkbox"/>	4000.000	4189.702	1,957,376	8.345	A	1.2
9	<input type="checkbox"/>	10000.000	10160.138	4,500,320	20.236	A	0.8
10	<input type="checkbox"/>	50000.000	49949.773	21,451,674	99.478	A	0.2

$y = 0.0020 * x + 0.0014$


R = 1.0000

DL = 0.3442

BEC = 0.6947

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	86	0.000	P	7.2
2	<input type="checkbox"/>			2,834	0.010	P	5.8
3	<input type="checkbox"/>	45.000	44.281	13,071	0.048	P	0.7
4	<input type="checkbox"/>	90.000	91.932	27,045	0.100	P	0.7
5	<input type="checkbox"/>	180.000	183.126	53,261	0.199	P	1.3
6	<input type="checkbox"/>	400.000	403.103	116,163	0.437	P	0.6
7	<input type="checkbox"/>	2500.000	2501.244	691,422	2.711	P	0.4
8	<input type="checkbox"/>	4000.000	4028.629	1,023,947	4.366	P	0.4
9	<input type="checkbox"/>	10000.000	10068.675	2,426,399	10.910	A	0.3
10	<input type="checkbox"/>	50000.000	49983.874	11,679,392	54.160	A	0.4

$y = 0.0011 * x + 3.1682E-004$

R = 1.0000


DL = 0.06335

BEC = 0.2924

Weight: <None>

Min Conc: <None>

Calibration for 013\_ICV.d



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	23,727	0.088	P	1.0
2	<input type="checkbox"/>			28,147	0.104	P	1.3
3	<input type="checkbox"/>	45.000	46.721	46,273	0.171	P	0.9
4	<input type="checkbox"/>	90.000	94.823	69,462	0.257	P	1.5
5	<input type="checkbox"/>	180.000	187.286	112,895	0.421	P	0.9
6	<input type="checkbox"/>	400.000	412.281	218,423	0.822	P	0.8
7	<input type="checkbox"/>	2500.000	2564.293	1,187,082	4.654	P	0.4
8	<input type="checkbox"/>	4000.000	4179.590	1,766,156	7.530	A	1.4
9	<input type="checkbox"/>	10000.000	10140.300	4,034,962	18.143	A	0.6
10	<input type="checkbox"/>	50000.000	49954.224	19,199,392	89.033	A	0.8

$y = 0.0018 * x + 0.0878$


R = 1.0000

DL = 1.406

BEC = 49.31

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	427	0.000	P	14.2
2	<input type="checkbox"/>			2,090	0.001	P	2.5
3	<input type="checkbox"/>	45.000	44.510	9,168	0.005	P	4.6
4	<input type="checkbox"/>	90.000	90.303	18,274	0.011	P	3.4
5	<input type="checkbox"/>	180.000	179.796	35,987	0.021	P	1.1
6	<input type="checkbox"/>	400.000	393.767	78,402	0.046	P	0.5
7	<input type="checkbox"/>	2500.000	2476.737	470,081	0.286	P	0.6
8	<input type="checkbox"/>	4000.000	3937.429	709,383	0.455	P	0.8
9	<input type="checkbox"/>	10000.000	10314.210	1,717,809	1.191	A	0.3
10	<input type="checkbox"/>	50000.000	49943.377	7,852,074	5.765	A	1.4

$y = 1.1542E-004 * x + 2.4203E-004$

R = 1.0000


DL = 0.894

BEC = 2.097

Weight: <None>

Min Conc: <None>

Calibration for 013\_ICV.d



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	151	0.001	P	36.4
2	<input type="checkbox"/>			400	0.001	P	10.0
3	<input type="checkbox"/>	45.000	46.478	1,271	0.005	P	6.3
4	<input type="checkbox"/>	90.000	92.666	2,385	0.009	P	6.3
5	<input type="checkbox"/>	180.000	185.341	4,572	0.017	P	7.1
6	<input type="checkbox"/>	400.000	424.405	10,194	0.038	P	2.7
7	<input type="checkbox"/>	2500.000	2536.074	57,762	0.226	P	1.1
8	<input type="checkbox"/>	4000.000	4120.130	86,205	0.368	P	1.2
9	<input type="checkbox"/>	10000.000	10069.515	199,590	0.897	P	0.1
10	<input type="checkbox"/>	50000.000	49974.462	959,993	4.452	P	0.5

$y = 8.9070E-005 * x + 5.5774E-004$


R = 1.0000

DL = 6.843

BEC = 6.262

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	28	0.000	P	71.2
2	<input type="checkbox"/>	0.180	0.174	213	0.000	P	15.8
3	<input type="checkbox"/>	0.900	0.960	1,046	0.000	P	7.9
4	<input type="checkbox"/>	1.800	1.910	2,061	0.001	P	3.8
5	<input type="checkbox"/>	3.600	3.719	3,978	0.001	P	1.9
6	<input type="checkbox"/>	20.000	20.069	20,832	0.008	P	0.6
7	<input type="checkbox"/>	50.000	49.652	49,457	0.020	P	0.4
8	<input type="checkbox"/>	200.000	200.380	181,370	0.080	P	1.2
9	<input type="checkbox"/>	500.000	503.879	433,626	0.201	P	1.0
10	<input type="checkbox"/>	2500.000	2499.200	2,143,694	0.995	A	1.2

$y = 3.9820E-004 * x + 1.0382E-005$

R = 1.0000


DL = 0.05567

BEC = 0.02607

Weight: <None>

Min Conc: <None>

Calibration for 013\_ICV.d



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	2,051	0.013	P	2.7
2	<input type="checkbox"/>	0.180	0.179	2,659	0.016	P	3.1
3	<input type="checkbox"/>	0.900	0.854	4,840	0.030	P	1.7
4	<input type="checkbox"/>	1.800	1.758	7,766	0.048	P	1.3
5	<input type="checkbox"/>	3.600	3.504	13,395	0.082	P	1.4
6	<input type="checkbox"/>	20.000	19.745	64,351	0.405	P	0.7
7	<input type="checkbox"/>	50.000	49.179	151,674	0.989	P	0.3
8	<input type="checkbox"/>	200.000	197.289	560,368	3.928	P	0.3
9	<input type="checkbox"/>	500.000	501.178	1,340,700	9.960	A	1.4
10	<input type="checkbox"/>			864	0.007	P	0.9

$y = 0.0198 * x + 0.0127$


R = 1.0000

DL = 0.05203

BEC = 0.6395

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	224	0.001	P	23.1
2	<input type="checkbox"/>	0.180	0.167	859	0.005	P	9.8
3	<input type="checkbox"/>	0.900	0.886	3,564	0.022	P	4.8
4	<input type="checkbox"/>	1.800	1.822	7,087	0.043	P	1.4
5	<input type="checkbox"/>	3.600	3.609	13,788	0.085	P	1.2
6	<input type="checkbox"/>	20.000	19.988	73,564	0.463	P	1.2
7	<input type="checkbox"/>	50.000	49.609	175,782	1.146	P	0.6
8	<input type="checkbox"/>	200.000	198.050	651,991	4.571	P	0.2
9	<input type="checkbox"/>	500.000	502.566	1,560,979	11.596	A	0.9
10	<input type="checkbox"/>	1000.000	999.127	2,914,268	23.053	A	0.6

$y = 0.0231 * x + 0.0014$


R = 1.0000

DL = 0.04163

BEC = 0.0602

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	40	0.000	P	55.0
2	<input type="checkbox"/>	0.180	0.170	503	0.003	P	11.0
3	<input type="checkbox"/>	0.900	0.882	2,427	0.015	P	5.2
4	<input type="checkbox"/>	1.800	1.784	4,867	0.030	P	4.5
5	<input type="checkbox"/>	3.600	3.585	9,723	0.060	P	0.3
6	<input type="checkbox"/>	20.000	20.116	53,102	0.334	P	1.6
7	<input type="checkbox"/>	50.000	50.060	127,387	0.830	P	0.5
8	<input type="checkbox"/>	200.000	199.772	472,627	3.313	P	0.6
9	<input type="checkbox"/>	500.000	495.722	1,106,660	8.222	P	0.6
10	<input type="checkbox"/>	2500.000	2500.872	5,243,254	41.476	A	0.7

$y = 0.0166 * x + 2.4816E-004$


R = 1.0000

DL = 0.02471

BEC = 0.01496

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	9,147	0.017	P	1.1
2	<input type="checkbox"/>			98,433	0.178	P	0.6
3	<input type="checkbox"/>	45.000	44.543	453,968	0.830	P	0.4
4	<input type="checkbox"/>	90.000	90.703	916,340	1.673	P	0.6
5	<input type="checkbox"/>	180.000	184.631	1,843,313	3.389	A	0.6
6	<input type="checkbox"/>	400.000	409.638	4,059,566	7.498	A	1.1
7	<input type="checkbox"/>	2500.000	2540.112	24,179,961	46.410	A	0.4
8	<input type="checkbox"/>	4000.000	4014.394	36,326,958	73.337	A	0.1
9	<input type="checkbox"/>	10000.000	9958.818	83,165,573	181.908	A	0.2
10	<input type="checkbox"/>	50000.000	50004.985	378,458,412	913.327	A	0.1

$y = 0.0183 * x + 0.0167$


R = 1.0000

DL = 0.03021

BEC = 0.9141

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	11	0.000	P	34.4
2	<input type="checkbox"/>	0.180	0.195	1,020	0.006	P	3.1
3	<input type="checkbox"/>	0.900	0.919	4,742	0.029	P	3.7
4	<input type="checkbox"/>	1.800	1.845	9,511	0.058	P	3.0
5	<input type="checkbox"/>	3.600	3.633	18,682	0.115	P	1.4
6	<input type="checkbox"/>	20.000	20.278	101,776	0.640	P	0.8
7	<input type="checkbox"/>	50.000	50.287	243,400	1.587	P	0.5
8	<input type="checkbox"/>	200.000	200.202	901,072	6.317	P	0.3
9	<input type="checkbox"/>	500.000	499.879	2,123,040	15.773	A	1.2
10	<input type="checkbox"/>			776	0.006	P	1.2

$y = 0.0316 * x + 6.8724E-005$


R = 1.0000

DL = 0.002251

BEC = 0.002178

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	96	0.001	P	13.6
2	<input type="checkbox"/>	0.180	0.166	303	0.002	P	19.1
3	<input type="checkbox"/>	0.900	1.037	1,377	0.008	P	1.7
4	<input type="checkbox"/>	1.800	1.920	2,466	0.015	P	1.7
5	<input type="checkbox"/>	3.600	3.764	4,732	0.029	P	1.6
6	<input type="checkbox"/>	20.000	21.552	26,015	0.164	P	2.5
7	<input type="checkbox"/>	50.000	52.401	60,866	0.397	P	0.2
8	<input type="checkbox"/>	200.000	210.727	227,357	1.594	P	0.5
9	<input type="checkbox"/>	500.000	512.555	521,740	3.876	P	0.5
10	<input type="checkbox"/>	1000.000	991.425	947,694	7.497	P	0.5

$y = 0.0076 * x + 5.9160E-004$


R = 0.9998

DL = 0.03195

BEC = 0.07824

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	36	0.000	P	39.4
2	<input type="checkbox"/>	0.180	0.211	360	0.002	P	13.6
3	<input type="checkbox"/>	0.900	1.000	1,566	0.010	P	9.0
4	<input type="checkbox"/>	1.800	1.957	3,028	0.019	P	2.1
5	<input type="checkbox"/>	3.600	4.066	6,242	0.038	P	1.9
6	<input type="checkbox"/>	20.000	22.321	33,304	0.209	P	0.8
7	<input type="checkbox"/>	50.000	53.562	77,024	0.502	P	0.3
8	<input type="checkbox"/>	200.000	212.194	283,660	1.989	P	0.5
9	<input type="checkbox"/>	500.000	516.606	651,651	4.841	P	0.5
10	<input type="checkbox"/>	1000.000	989.032	1,171,617	9.268	P	0.3

$y = 0.0094 * x + 2.2042E-004$


R = 0.9998

DL = 0.02784

BEC = 0.02352

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	30	0.000	P	22.4
2	<input type="checkbox"/>	0.180	0.205	154	0.001	P	14.1
3	<input type="checkbox"/>	0.900	0.952	604	0.004	P	4.0
4	<input type="checkbox"/>	1.800	1.835	1,137	0.007	P	5.8
5	<input type="checkbox"/>	3.600	3.869	2,359	0.014	P	1.3
6	<input type="checkbox"/>	20.000	21.214	12,499	0.079	P	0.9
7	<input type="checkbox"/>	50.000	51.671	29,320	0.191	P	3.0
8	<input type="checkbox"/>	200.000	209.490	110,461	0.774	P	0.2
9	<input type="checkbox"/>	500.000	518.376	257,888	1.916	P	0.9
10	<input type="checkbox"/>	2500.000	2495.522	1,165,856	9.223	P	0.5

$y = 0.0037 * x + 1.8571E-004$

R = 1.0000


DL = 0.03382

BEC = 0.05025

Weight: <None>

Min Conc: <None>






	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	25	0.000	P	19.3
2	<input type="checkbox"/>	0.180	0.210	106	0.001	P	2.4
3	<input type="checkbox"/>	0.900	0.900	369	0.002	P	2.5
4	<input type="checkbox"/>	1.800	1.898	750	0.005	P	2.8
5	<input type="checkbox"/>	3.600	3.603	1,399	0.009	P	4.2
6	<input type="checkbox"/>	20.000	20.134	7,519	0.047	P	1.5
7	<input type="checkbox"/>	50.000	49.593	17,826	0.116	P	0.8
8	<input type="checkbox"/>	200.000	200.368	66,905	0.469	P	0.3
9	<input type="checkbox"/>	500.000	499.888	157,481	1.170	P	0.3
10	<input type="checkbox"/>			52	0.000	P	5.4

$y = 0.0023 * x + 1.5667E-004$   
 $R = 1.0000$   
 $DL = 0.03871$   
 $BEC = 0.06695$

Weight: <None>  
 Min Conc: <None>




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	3	0.000	P	34.8
2	<input type="checkbox"/>	0.180	0.173	50	0.000	P	10.8
3	<input type="checkbox"/>	0.900	0.903	246	0.000	P	7.6
4	<input type="checkbox"/>	1.800	1.846	500	0.001	P	9.9
5	<input type="checkbox"/>	3.600	3.764	1,009	0.002	P	1.0
6	<input type="checkbox"/>	10.000	10.070	2,681	0.005	P	4.1
7	<input type="checkbox"/>	50.000	50.030	12,807	0.025	P	1.5
8	<input type="checkbox"/>	100.000	99.971	24,328	0.049	P	1.3
9	<input type="checkbox"/>			28	0.000	P	20.2
10	<input type="checkbox"/>			19	0.000	P	23.4

$y = 4.9124E-004 * x + 6.0873E-006$   
 $R = 1.0000$   
 $DL = 0.01294$   
 $BEC = 0.01239$

Weight: <None>  
 Min Conc: <None>

Calibration for 013\_ICV.d



	Rjct	Conc	Calc Conc	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	2	0.000	P	86.6
2	<input type="checkbox"/>	0.180	0.201	324	0.001	P	20.2
3	<input type="checkbox"/>	0.900	0.895	1,427	0.004	P	9.0
4	<input type="checkbox"/>	1.800	1.784	2,846	0.008	P	8.0
5	<input type="checkbox"/>	3.600	3.497	5,533	0.015	P	1.5
6	<input type="checkbox"/>	10.000	9.910	15,417	0.043	P	2.8
7	<input type="checkbox"/>	50.000	49.417	73,463	0.214	P	1.1
8	<input type="checkbox"/>	100.000	100.305	139,478	0.433	P	0.8
9	<input type="checkbox"/>			144	0.000	P	15.7
10	<input type="checkbox"/>			150	0.001	P	8.8

$y = 0.0043 * x + 6.0363E-006$


R = 1.0000

DL = 0.003629

BEC = 0.001397

Weight: <None>

Min Conc: <None>



	Rjct	Conc	Calc Conc	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	4	0.000	P	86.6
2	<input type="checkbox"/>	0.180	0.174	811	0.002	P	7.1
3	<input type="checkbox"/>	0.900	0.857	3,952	0.011	P	2.1
4	<input type="checkbox"/>	1.800	1.813	8,369	0.023	P	1.4
5	<input type="checkbox"/>	3.600	3.598	16,469	0.045	P	0.5
6	<input type="checkbox"/>	10.000	9.867	44,406	0.123	P	1.2
7	<input type="checkbox"/>	50.000	49.708	213,771	0.621	P	0.5
8	<input type="checkbox"/>	100.000	100.159	402,928	1.252	P	0.8
9	<input type="checkbox"/>			56	0.000	P	70.2
10	<input type="checkbox"/>			74	0.000	P	27.2

$y = 0.0125 * x + 1.2099E-005$


R = 1.0000

DL = 0.002514

BEC = 0.0009678

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	2	0.000	P	86.5
2	<input type="checkbox"/>	0.180	0.189	150	0.000	P	1.1
3	<input type="checkbox"/>	0.900	0.856	668	0.002	P	4.1
4	<input type="checkbox"/>	1.800	1.769	1,382	0.004	P	2.2
5	<input type="checkbox"/>	3.600	3.602	2,788	0.008	P	1.8
6	<input type="checkbox"/>	20.000	19.866	15,106	0.042	P	1.2
7	<input type="checkbox"/>	50.000	49.578	36,021	0.105	P	1.5
8	<input type="checkbox"/>	200.000	201.511	136,951	0.426	P	1.4
9	<input type="checkbox"/>	500.000	503.548	322,218	1.064	P	0.2
10	<input type="checkbox"/>	1000.000	997.948	585,230	2.108	P	0.6

$y = 0.0021 * x + 5.4371E-006$


R = 1.0000

DL = 0.006682

BEC = 0.002574

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	8	0.000	P	208.0
2	<input type="checkbox"/>	0.180	0.177	388	0.001	P	8.7
3	<input type="checkbox"/>	0.900	0.821	1,751	0.002	P	9.1
4	<input type="checkbox"/>	1.800	1.751	3,727	0.005	P	3.0
5	<input type="checkbox"/>	3.600	3.425	7,204	0.010	P	4.1
6	<input type="checkbox"/>	20.000	19.281	39,704	0.055	P	1.0
7	<input type="checkbox"/>	50.000	48.034	93,715	0.136	P	0.7
8	<input type="checkbox"/>	200.000	196.149	353,397	0.556	P	0.9
9	<input type="checkbox"/>	500.000	496.940	838,189	1.409	P	0.3
10	<input type="checkbox"/>	1000.000	1002.414	1,575,102	2.842	A	1.6

$y = 0.0028 * x + 1.0083E-005$


R = 1.0000

DL = 0.02218

BEC = 0.003556

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	36	0.000	P	42.3
2	<input type="checkbox"/>	0.180	0.136	321	0.001	P	11.0
3	<input type="checkbox"/>	0.900	0.864	1,828	0.005	P	1.4
4	<input type="checkbox"/>	1.800	1.775	3,725	0.010	P	2.3
5	<input type="checkbox"/>	3.600	3.582	7,418	0.020	P	2.3
6	<input type="checkbox"/>	10.000	9.590	19,472	0.054	P	1.5
7	<input type="checkbox"/>	50.000	49.230	95,390	0.277	P	0.4
8	<input type="checkbox"/>	100.000	100.427	181,996	0.566	P	0.5
9	<input type="checkbox"/>			264	0.001	P	10.2
10	<input type="checkbox"/>			130	0.000	P	10.2

$y = 0.0056 * x + 9.6704E-005$


R = 1.0000

DL = 0.02179

BEC = 0.01717

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	80	0.000	P	28.4
2	<input type="checkbox"/>	0.180	0.191	917	0.002	P	18.0
3	<input type="checkbox"/>	0.900	0.950	4,233	0.008	P	2.8
4	<input type="checkbox"/>	1.800	1.893	8,368	0.016	P	3.8
5	<input type="checkbox"/>	3.600	3.826	16,821	0.032	P	0.7
6	<input type="checkbox"/>	20.000	21.274	91,939	0.178	P	1.0
7	<input type="checkbox"/>	50.000	52.397	222,280	0.438	P	0.5
8	<input type="checkbox"/>	200.000	207.046	845,081	1.729	P	0.5
9	<input type="checkbox"/>	500.000	521.853	2,038,178	4.358	A	1.3
10	<input type="checkbox"/>	2500.000	2495.007	9,224,719	20.835	A	0.4

$y = 0.0084 * x + 1.5279E-004$

R = 1.0000


DL = 0.01557

BEC = 0.0183

Weight: <None>

Min Conc: <None>

Calibration for 013\_ICV.d



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.000	9	0.000	P	114.7
2	<input type="checkbox"/>			20	0.000	P	60.4
3	<input type="checkbox"/>			26	0.000	P	32.9
4	<input type="checkbox"/>			16	0.000	P	32.3
5	<input type="checkbox"/>			23	0.000	P	25.2
6	<input type="checkbox"/>			39	0.000	P	27.3
7	<input type="checkbox"/>			97	0.000	P	13.0
8	<input type="checkbox"/>			186	0.000	P	4.2
9	<input type="checkbox"/>	100.000	100.000	653.955	0.588	P	0.5
10	<input type="checkbox"/>			1.965	0.002	P	2.5

$y = 0.0059 * x + 7.0827E-006$


R = 1.0000

DL = 0.004143

BEC = 0.001204

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	0.000	0.273	3	0.000	P	49.7
2	<input type="checkbox"/>			12	0.000	P	6.1
3	<input type="checkbox"/>	36.000	39.474	41	0.000	P	12.9
4	<input type="checkbox"/>	72.000	71.612	73	0.000	P	9.5
5	<input type="checkbox"/>	144.000	138.183	138	0.000	P	5.4
6	<input type="checkbox"/>	400.000	394.322	381	0.000	P	5.7
7	<input type="checkbox"/>	2000.000	2014.764	1,894	0.002	P	1.1
8	<input type="checkbox"/>	4000.000	3993.371	3,580	0.003	P	0.6
9	<input type="checkbox"/>			74	0.000	P	8.4
10	<input type="checkbox"/>			29	0.000	P	24.0

$y = 7.767459E-007 * x + 2.175191E-006$

R = 1.0000


DL = 4.586

BEC = 2.8

Weight: <None>

Min Conc: <None>

Calibration for 013\_ICV.d



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	27	0.000	P	43.2
2	<input type="checkbox"/>	0.180	0.175	1,356	0.003	P	2.8
3	<input type="checkbox"/>	0.900	0.886	6,723	0.013	P	4.0
4	<input type="checkbox"/>	1.800	1.798	13,639	0.026	P	1.8
5	<input type="checkbox"/>	3.600	3.518	26,660	0.051	P	0.7
6	<input type="checkbox"/>	10.000	9.817	73,363	0.142	P	0.8
7	<input type="checkbox"/>	50.000	49.321	361,876	0.713	P	0.5
8	<input type="checkbox"/>	100.000	100.361	708,660	1.450	P	0.7
9	<input type="checkbox"/>			278	0.001	P	21.0
10	<input type="checkbox"/>			41	0.000	P	24.2

$y = 0.0144 * x + 5.0966E-005$


R = 1.0000

DL = 0.004575

BEC = 0.003528

Weight: <None>

Min Conc: <None>



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det	RSD
1	<input type="checkbox"/>	0.000	0.000	576	0.000	P	6.7
2	<input type="checkbox"/>	0.180	0.182	4,729	0.004	P	0.3
3	<input type="checkbox"/>	0.900	0.851	19,879	0.016	P	1.1
4	<input type="checkbox"/>	1.800	1.781	41,125	0.033	P	0.9
5	<input type="checkbox"/>	3.600	3.522	80,751	0.064	P	0.6
6	<input type="checkbox"/>	20.000	19.576	437,907	0.355	P	0.3
7	<input type="checkbox"/>	50.000	48.615	1,063,990	0.881	P	0.3
8	<input type="checkbox"/>	200.000	200.870	4,194,653	3.637	A	0.2
9	<input type="checkbox"/>	500.000	499.808	10,058,905	9.050	A	0.4
10	<input type="checkbox"/>			3,371	0.003	P	2.2

$y = 0.0181 * x + 4.5844E-004$

R = 1.0000


DL = 0.005096

BEC = 0.02532


Weight: <None>

Min Conc: <None>

Calibration for 013\_ICV.d




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		943,670		A	0.7
2	<input type="checkbox"/>	1.000		942,450		A	1.3
3	<input type="checkbox"/>	1.000		918,618		A	2.0
4	<input type="checkbox"/>	1.000		939,550		A	0.3
5	<input type="checkbox"/>	1.000		935,847		A	1.4
6	<input type="checkbox"/>	1.000		905,543		A	0.8
7	<input type="checkbox"/>	1.000		849,418		M	1.7
8	<input type="checkbox"/>	1.000		779,769		P	0.7
9	<input type="checkbox"/>	1.000		741,357		P	0.3
10	<input type="checkbox"/>	1.000		746,834		P	0.2




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		1,761,204		A	1.0
2	<input type="checkbox"/>	1.000		1,731,271		A	0.7
3	<input type="checkbox"/>	1.000		1,704,637		A	0.7
4	<input type="checkbox"/>	1.000		1,713,432		A	0.4
5	<input type="checkbox"/>	1.000		1,714,180		A	1.1
6	<input type="checkbox"/>	1.000		1,715,986		A	1.7
7	<input type="checkbox"/>	1.000		1,643,004		A	0.2
8	<input type="checkbox"/>	1.000		1,560,147		A	1.0
9	<input type="checkbox"/>	1.000		1,442,643		A	0.2
10	<input type="checkbox"/>	1.000		1,362,370		A	2.5

Calibration for 013\_ICV.d




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		270,213		P	1.3
2	<input type="checkbox"/>	1.000		271,890		P	0.6
3	<input type="checkbox"/>	1.000		270,624		P	0.7
4	<input type="checkbox"/>	1.000		270,645		P	0.6
5	<input type="checkbox"/>	1.000		267,982		P	0.8
6	<input type="checkbox"/>	1.000		265,761		P	0.4
7	<input type="checkbox"/>	1.000		255,090		P	0.6
8	<input type="checkbox"/>	1.000		234,553		P	0.4
9	<input type="checkbox"/>	1.000		222,397		P	0.2
10	<input type="checkbox"/>	1.000		215,642		P	0.4




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		2,719,053		A	1.9
2	<input type="checkbox"/>	1.000		2,674,421		A	1.2
3	<input type="checkbox"/>	1.000		2,665,556		A	1.5
4	<input type="checkbox"/>	1.000		2,673,152		A	1.3
5	<input type="checkbox"/>	1.000		2,667,366		A	0.4
6	<input type="checkbox"/>	1.000		2,603,447		A	0.6
7	<input type="checkbox"/>	1.000		2,500,152		A	0.6
8	<input type="checkbox"/>	1.000		2,272,935		A	0.9
9	<input type="checkbox"/>	1.000		2,161,191		A	0.9
10	<input type="checkbox"/>	1.000		2,154,158		A	0.9







	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		547,888		P	0.2
2	<input type="checkbox"/>	1.000		551,773		P	0.2
3	<input type="checkbox"/>	1.000		546,785		P	0.3
4	<input type="checkbox"/>	1.000		547,618		P	0.4
5	<input type="checkbox"/>	1.000		543,928		P	0.4
6	<input type="checkbox"/>	1.000		541,382		P	0.2
7	<input type="checkbox"/>	1.000		521,005		P	0.4
8	<input type="checkbox"/>	1.000		495,343		P	0.6
9	<input type="checkbox"/>	1.000		457,182		P	0.4
10	<input type="checkbox"/>	1.000		414,374		P	0.5




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		161,578		P	0.7
2	<input type="checkbox"/>	1.000		163,788		P	1.1
3	<input type="checkbox"/>	1.000		163,222		P	0.6
4	<input type="checkbox"/>	1.000		163,179		P	0.9
5	<input type="checkbox"/>	1.000		162,874		P	0.5
6	<input type="checkbox"/>	1.000		159,054		P	0.7
7	<input type="checkbox"/>	1.000		153,393		P	0.1
8	<input type="checkbox"/>	1.000		142,644		P	0.6
9	<input type="checkbox"/>	1.000		134,607		P	0.4
10	<input type="checkbox"/>	1.000		126,414		P	0.6




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		710,934		P	0.8
2	<input type="checkbox"/>	1.000		715,490		P	0.8
3	<input type="checkbox"/>	1.000		711,395		P	0.6
4	<input type="checkbox"/>	1.000		712,946		P	0.6
5	<input type="checkbox"/>	1.000		710,219		P	0.5
6	<input type="checkbox"/>	1.000		696,856		P	1.0
7	<input type="checkbox"/>	1.000		663,570		P	0.5
8	<input type="checkbox"/>	1.000		613,859		P	0.2
9	<input type="checkbox"/>	1.000		576,611		P	0.4
10	<input type="checkbox"/>	1.000		546,673		P	1.0



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		367,686		P	0.1
2	<input type="checkbox"/>	1.000		371,304		P	0.4
3	<input type="checkbox"/>	1.000		368,466		P	0.8
4	<input type="checkbox"/>	1.000		369,118		P	1.0
5	<input type="checkbox"/>	1.000		366,056		P	0.9
6	<input type="checkbox"/>	1.000		359,942		P	0.3
7	<input type="checkbox"/>	1.000		343,992		P	0.6
8	<input type="checkbox"/>	1.000		321,782		P	0.8
9	<input type="checkbox"/>	1.000		302,958		P	0.1
10	<input type="checkbox"/>	1.000		277,658		P	1.0




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		751,394		P	0.4
2	<input type="checkbox"/>	1.000		757,512		P	0.5
3	<input type="checkbox"/>	1.000		748,509		P	0.2
4	<input type="checkbox"/>	1.000		749,245		P	0.2
5	<input type="checkbox"/>	1.000		741,146		P	0.9
6	<input type="checkbox"/>	1.000		726,133		P	0.4
7	<input type="checkbox"/>	1.000		688,055		P	0.4
8	<input type="checkbox"/>	1.000		635,449		P	0.7
9	<input type="checkbox"/>	1.000		594,884		P	0.3
10	<input type="checkbox"/>	1.000		554,226		P	0.9




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		522,975		P	0.9
2	<input type="checkbox"/>	1.000		524,217		P	0.9
3	<input type="checkbox"/>	1.000		523,346		P	0.2
4	<input type="checkbox"/>	1.000		524,146		P	1.3
5	<input type="checkbox"/>	1.000		523,981		P	0.7
6	<input type="checkbox"/>	1.000		517,103		P	0.6
7	<input type="checkbox"/>	1.000		507,833		P	0.7
8	<input type="checkbox"/>	1.000		488,752		P	0.9
9	<input type="checkbox"/>	1.000		467,721		P	0.7
10	<input type="checkbox"/>	1.000		442,754		P	0.6

Calibration for 013\_ICV.d




	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		1,255,415		P	0.3
2	<input type="checkbox"/>	1.000		1,261,973		P	0.3
3	<input type="checkbox"/>	1.000		1,253,491		P	0.3
4	<input type="checkbox"/>	1.000		1,257,566		P	0.5
5	<input type="checkbox"/>	1.000		1,257,397		P	0.8
6	<input type="checkbox"/>	1.000		1,233,952		P	0.3
7	<input type="checkbox"/>	1.000		1,208,227		P	0.6
8	<input type="checkbox"/>	1.000		1,153,261		P	0.5
9	<input type="checkbox"/>	1.000		1,111,559		P	0.7
10	<input type="checkbox"/>	1.000		1,075,936		P	1.1



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		308,813		P	1.0
2	<input type="checkbox"/>	1.000		311,205		P	0.7
3	<input type="checkbox"/>	1.000		307,178		P	0.8
4	<input type="checkbox"/>	1.000		309,215		P	1.4
5	<input type="checkbox"/>	1.000		305,985		P	0.7
6	<input type="checkbox"/>	1.000		305,301		P	0.9
7	<input type="checkbox"/>	1.000		297,643		P	1.0
8	<input type="checkbox"/>	1.000		288,302		P	0.6
9	<input type="checkbox"/>	1.000		276,676		P	0.8
10	<input type="checkbox"/>	1.000		248,268		P	0.7

Calibration for 013\_ICV.d



	Rjct	Conc.	Calc Conc.	CPS	Ratio	Det.	RSD
1	<input type="checkbox"/>	1.000		737,867		P	0.7
2	<input type="checkbox"/>	1.000		737,079		P	0.3
3	<input type="checkbox"/>	1.000		730,460		P	0.2
4	<input type="checkbox"/>	1.000		734,327		P	0.3
5	<input type="checkbox"/>	1.000		732,928		P	0.6
6	<input type="checkbox"/>	1.000		725,594		P	0.2
7	<input type="checkbox"/>	1.000		706,882		P	0.2
8	<input type="checkbox"/>	1.000		670,136		P	0.6
9	<input type="checkbox"/>	1.000		632,858		P	0.3
10	<input type="checkbox"/>	1.000		592,880		P	0.8

### Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name: <b>9K26027-ICV1</b>	Total Dilution: <b>1.0000</b>
File Name: 013_ICV.d	Vial: 2
File Path: C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type: ICV
Acq Time: 11/26/2019 12:03:29	I.S. Reference File: 003CALB.d
Comment: <b>A19J138 - ESS 11/26</b>	Last Calibration: 11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	40.100	ppb	0.8	86,665	40	100.25	
Na	23	45	He	3902.818	ppb	0.3	3,276,971	4000	97.57	
Mg	24	45	He	4146.007	ppb	0.6	1,951,000	4000	103.65	
Al	27	45	He	3916.804	ppb	0.2	1,002,717	4000	97.92	
K	39	45	He	4088.169	ppb	1.8	1,740,394	4000	102.2	
Ca	44	45	H2	3999.418	ppb	1.4	692,886	4000	99.99	
[Ca]	44	45	He	4076.875	ppb	0.2	85,919	4000	101.92	
Ti	47	45	NoGas	96.462	ppb	2.7	87,577	100	96.46	
V	51	74	He	94.193	ppb	0.5	271,354	100	94.19	
Cr	52	74	He	96.091	ppb	0.4	319,814	100	96.09	
Mn	55	74	He	99.773	ppb	0.5	238,582	100	99.77	
Fe	56	74	H2	3993.211	ppb	0.3	35,427,302	4000	99.83	
Co	59	74	He	99.231	ppb	0.5	451,399	100	99.23	
Ni	60	74	He	103.626	ppb	1.0	113,041	100	103.63	
Cu	65	74	He	103.019	ppb	0.4	139,206	100	103.02	
Zn	66	74	He	101.921	ppb	1.0	54,330	100	101.92	
As	75	74	He	96.845	ppb	0.6	32,695	100	96.84	
Se	78	74	H2	40.346	ppb	0.5	9,628	40	100.86	
Mo	95	103	He	39.736	ppb	1.0	55,118	40	99.34	
Ag	107	103	He	40.231	ppb	0.9	161,431	40	100.58	
Cd	111	103	He	98.090	ppb	1.1	66,493	100	98.09	
[Cd]	111	103	NoGas	95.008	ppb	0.4	167,862	100	95.01	
Sb	121	103	He	40.383	ppb	0.9	73,009	40	100.96	
Ba	138	159	He	102.185	ppb	0.6	420,936	100	102.18	
Hg	201	159	NoGas	816.137	ppt	1.7	728	800	102.02	
Tl	205	159	He	39.913	ppb	0.9	284,426	40	99.78	
Pb	208	159	NoGas	97.468	ppb	0.8	2,021,432	100	97.47	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.3	768,129	943670.243333333	81.4	
Sc	45	H2	Analog	1.6	1,500,422	1761203.933333333	85.2	
Sc	45	He	Pulse	0.4	236,246	270213.02	87.4	
Sc	45	NoGas	Analog	0.8	2,279,711	2719052.54	83.8	
Ge	74	H2	Pulse	0.4	485,636	547887.95	88.6	
Ge	74	He	Pulse	0.5	144,168	161577.683333333	89.2	
Ge	74	NoGas	Pulse	0.5	603,509	710934.333333333	84.9	
Rh	103	He	Pulse	0.7	320,952	367685.51	87.3	
Rh	103	NoGas	Pulse	0.2	623,116	751394.163333333	82.9	
Tb	159	He	Pulse	0.6	493,220	522974.92	94.3	
Tb	159	NoGas	Pulse	0.7	1,145,250	1255414.6	91.2	
Bi	209	He	Pulse	0.5	290,334	308812.996666667	94.0	
Bi	209	NoGas	Pulse	0.1	675,530	737867.09	91.6	

### Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name:	9K26027-ICB1	Total Dilution:	1.0000
File Name:	014_ICB.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	ICB
Acq Time:	11/26/2019 12:08:07	I.S. Reference File:	003CALB.d
Comment:	CCB	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.009	ppb	32.3	47	
Na	23	45	He	1.658	ppb	11.6	4,059	
Mg	24	45	He	0.841	ppb	9.6	721	
Al	27	45	He	0.817	ppb	27.4	283	
K	39	45	He	2.689	ppb	34.7	21,823	
Ca	44	45	H2	1.388	ppb	25.5	603	
[Ca]	44	45	He	0.197	ppb	807.1	136	
Ti	47	45	NoGas	0.057	ppb	62.1	77	
V	51	74	He	-0.314	ppb	N/A	939	
Cr	52	74	He	0.011	ppb	46.9	240	
Mn	55	74	He	0.027	ppb	32.8	102	
Fe	56	74	H2	1.017	ppb	8.5	17,021	
Co	59	74	He	0.011	ppb	31.4	60	
Ni	60	74	He	0.009	ppb	256.6	96	
Cu	65	74	He	0.038	ppb	47.5	83	
Zn	66	74	He	0.109	ppb	23.3	86	
As	75	74	He	0.010	ppb	138.0	26	
Se	78	74	H2	0.025	ppb	91.3	9	
Mo	95	103	He	0.029	ppb	29.1	43	
Ag	107	103	He	0.005	ppb	113.6	23	
Cd	111	103	He	0.038	ppb	8.2	29	
[Cd]	111	103	NoGas	0.030	ppb	74.3	62	
Sb	121	103	He	0.251	ppb	15.2	500	
Ba	138	159	He	0.015	ppb	86.2	138	
Hg	201	159	NoGas	5.102	ppt	60.3	7	
Tl	205	159	He	0.002	ppb	45.7	42	
Pb	208	159	NoGas	0.046	ppb	13.7	1,511	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.3	796,853	943670.243333333	84.4	
Sc	45	H2	Analog	1.3	1,501,107	1761203.93333333	85.2	
Sc	45	He	Pulse	0.9	235,695	270213.02	87.2	
Sc	45	NoGas	Analog	0.9	2,332,499	2719052.54	85.8	
Ge	74	H2	Pulse	0.7	482,642	547887.95	88.1	
Ge	74	He	Pulse	1.0	145,173	161577.683333333	89.8	
Ge	74	NoGas	Pulse	1.1	626,829	710934.333333333	88.2	
Rh	103	He	Pulse	0.8	331,736	367685.51	90.2	
Rh	103	NoGas	Pulse	0.8	659,265	751394.163333333	87.7	
Tb	159	He	Pulse	0.7	493,072	522974.92	94.3	
Tb	159	NoGas	Pulse	0.5	1,168,962	1255414.6	93.1	
Bi	209	He	Pulse	0.5	295,038	308812.996666667	95.5	
Bi	209	NoGas	Pulse	0.4	696,572	737867.09	94.4	

### CRL Verification Report - ICPMS5

Sample Name: <b>9K26027-CRL1</b>	Total Dilution: <b>1.0000</b>
File Name: 015CRL.d	Vial: 1102
File Path: C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type: CRL1
Acq Time: 11/26/2019 12:12:50	I.S. Reference File: 003CALB.d
Comment: <b>A19K144 - ESS 11/26</b>	Last Calibration: 11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	0.175	ppb	14.0	428	97.22	
Na	23	45	He	9.963	ppb	0.2	11,275	110.7	
Mg	24	45	He	9.397	ppb	1.8	4,851	104.41	
Al	27	45	He	9.256	ppb	3.9	2,497	102.84	
K	39	45	He	11.455	ppb	5.4	26,112	127.28	
Ca	44	45	H2	8.982	ppb	5.1	1,947	99.8	
[Ca]	44	45	He	8.578	ppb	10.4	319	95.31	
Ti	47	45	NoGas	0.228	ppb	8.3	242	126.67	
V	51	74	He	-0.096	ppb	N/A	1,590	-53.33	R-11
Cr	52	74	He	0.185	ppb	8.3	834	102.78	
Mn	55	74	He	0.202	ppb	3.3	530	112.22	
Fe	56	74	H2	8.753	ppb	0.6	86,633	97.26	
Co	59	74	He	0.182	ppb	6.4	857	101.11	
Ni	60	74	He	0.134	ppb	6.1	237	74.44	
Cu	65	74	He	0.229	ppb	11.5	349	127.22	
Zn	66	74	He	0.213	ppb	13.5	143	118.33	
As	75	74	He	0.189	ppb	8.6	88	105	
Se	78	74	H2	0.185	ppb	29.0	48	102.78	
Mo	95	103	He	0.182	ppb	7.9	266	101.11	
Ag	107	103	He	0.188	ppb	11.7	793	104.44	
Cd	111	103	He	0.200	ppb	13.2	144	111.11	
[Cd]	111	103	NoGas	0.182	ppb	23.8	353	101.11	
Sb	121	103	He	0.214	ppb	3.0	437	118.89	
Ba	138	159	He	0.193	ppb	4.5	873	107.22	
Hg	201	159	NoGas	10.477	ppt.	24.2	12	145.51	R-11
Tl	205	159	He	0.182	ppb	4.3	1,329	101.11	
Pb	208	159	NoGas	0.215	ppb	5.0	5,129	119.44	

*L.M.R.L*

*L.M.R.L*

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.4	816,186	943670.243333333	86.5	
Sc	45	H2	Analog	1.3	1,522,610	1761203.933333333	86.5	
Sc	45	He	Pulse	0.7	241,331	270213.02	89.3	
Sc	45	NoGas	Analog	1.2	2,382,837	2719052.54	87.6	
Ge	74	H2	Pulse	0.2	490,669	547887.95	89.6	
Ge	74	He	Pulse	0.8	147,517	161577.683333333	91.3	
Ge	74	NoGas	Pulse	0.5	638,978	710934.333333333	89.9	
Rh	103	He	Pulse	0.5	335,527	367685.51	91.3	
Rh	103	NoGas	Pulse	1.0	671,378	751394.163333333	89.4	
Tb	159	He	Pulse	0.6	495,200	522974.92	94.7	
Tb	159	NoGas	Pulse	1.2	1,178,082	1255414.6	93.8	
Bi	209	He	Pulse	0.7	295,698	308812.996666667	95.8	
Bi	209	NoGas	Pulse	0.6	699,515	737867.09	94.8	



### CRL Verification Report - ICPMS5

Sample Name:	9K26027-CRL2	Total Dilution:	1.0000
File Name:	016_CRL.d	Vial:	1103
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL2
Acq Time:	11/26/2019 12:17:31	I.S. Reference File:	003CALB.d
Comment:	A19K145 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	0.910	ppb	7.6	2,180	101.11	
Na	23	45	He	46.777	ppb	0.4	43,577	103.95	
Mg	24	45	He	46.266	ppb	2.3	22,967	102.81	
Al	27	45	He	46.473	ppb	1.3	12,443	103.27	
K	39	45	He	49.724	ppb	2.9	43,302	110.5	
Ca	44	45	H2	45.080	ppb	1.4	8,432	100.18	
[Ca]	44	45	He	48.471	ppb	7.8	1,197	107.71	
Ti	47	45	NoGas	0.854	ppb	8.9	846	94.89	
V	51	74	He	0.663	ppb	6.1	3,862	73.67	
Cr	52	74	He	0.953	ppb	6.1	3,490	105.89	
Mn	55	74	He	0.953	ppb	1.6	2,396	105.89	
Fe	56	74	H2	44.865	ppb	0.7	416,263	99.7	
Co	59	74	He	0.880	ppb	0.9	4,155	97.78	
Ni	60	74	He	0.903	ppb	11.8	1,109	100.33	
Cu	65	74	He	0.976	ppb	4.1	1,398	108.44	
Zn	66	74	He	0.922	ppb	13.4	537	102.44	
As	75	74	He	0.909	ppb	10.7	341	101	
Se	78	74	H2	0.876	ppb	9.8	217	97.33	
Mo	95	103	He	0.891	ppb	5.4	1,311	99	
Ag	107	103	He	0.923	ppb	3.7	3,925	102.56	
Cd	111	103	He	0.911	ppb	3.6	656	101.22	
[Cd]	111	103	NoGas	0.856	ppb	4.4	1,658	95.11	
Sb	121	103	He	0.922	ppb	4.4	1,797	102.44	
Ba	138	159	He	0.925	ppb	1.3	3,954	102.78	
Hg	201	159	NoGas	40.119	ppt.	2.6	40	111.44	
Tl	205	159	He	0.914	ppb	1.5	6,652	101.56	
Pb	208	159	NoGas	0.932	ppb	1.4	20,705	103.56	

**ISTD Table:**

Name	Mass	Tune Mode	Def.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Mix	2.5	840,964	943670.243333333	89.1	
Sc	45	H2	Analog	1.0	1,548,482	1761203.933333333	87.9	
Sc	45	He	Pulse	0.8	245,572	270213.02	90.9	
Sc	45	NoGas	Analog	0.7	2,414,758	2719052.54	88.8	
Ge	74	H2	Pulse	0.4	497,848	547887.95	90.9	
Ge	74	He	Pulse	0.9	149,328	161577.683333333	92.4	
Ge	74	NoGas	Pulse	0.6	651,713	710934.333333333	91.7	
Rh	103	He	Pulse	1.4	339,976	367685.51	92.5	
Rh	103	NoGas	Pulse	0.4	680,354	751394.163333333	90.5	
Tb	159	He	Pulse	1.4	501,688	522974.92	95.9	
Tb	159	NoGas	Pulse	0.5	1,194,951	1255414.6	95.2	
Bi	209	He	Pulse	1.5	298,330	308812.996666667	96.6	
Bi	209	NoGas	Pulse	0.4	708,130	737867.09	96.0	

### CRL Verification Report - ICPMS5

Sample Name:	9K26027-CRL3	Total Dilution:	1.0000
File Name:	017CRL_d	Vial:	1104
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL3
Acq Time:	11/26/2019 12:22:12	I.S. Reference File:	003CALB.d
Comment:	A19K146 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	1.712	ppb	5.2	4,083	95.11	
Na	23	45	He	91.426	ppb	0.9	83,032	101.58	
Mg	24	45	He	92.617	ppb	1.0	45,922	102.91	
Al	27	45	He	92.169	ppb	3.1	24,758	102.41	
K	39	45	He	95.257	ppb	1.6	63,610	105.84	
Ca	44	45	H2	89.033	ppb	2.1	16,498	98.93	
[Ca]	44	45	He	97.226	ppb	6.3	2,278	108.03	
Ti	47	45	NoGas	1.931	ppb	4.2	1,896	107.28	
V	51	74	He	1.590	ppb	0.3	6,683	88.33	
Cr	52	74	He	1.794	ppb	3.4	6,464	99.67	
Mn	55	74	He	1.769	ppb	3.2	4,470	98.28	
Fe	56	74	H2	89.697	ppb	0.5	835,520	99.66	
Co	59	74	He	1.823	ppb	2.3	8,698	101.28	
Ni	60	74	He	1.870	ppb	4.0	2,226	103.89	
Cu	65	74	He	1.864	ppb	3.1	2,671	103.56	
Zn	66	74	He	1.900	ppb	3.3	1,089	105.56	
As	75	74	He	1.889	ppb	4.1	691	104.94	
Se	78	74	H2	1.757	ppb	3.8	439	97.61	
Mo	95	103	He	1.764	ppb	6.8	2,614	98	
Ag	107	103	He	1.818	ppb	0.6	7,786	101	
Cd	111	103	He	1.889	ppb	6.3	1,368	104.94	
[Cd]	111	103	NoGas	1.768	ppb	4.8	3,439	98.22	
Sb	121	103	He	1.868	ppb	2.4	3,634	103.78	
Ba	138	159	He	1.892	ppb	2.4	7,982	105.11	
Hg	201	159	NoGas	75.739	ppt	11.7	73	105.19	
Tl	205	159	He	1.808	ppb	2.5	13,096	100.44	
Pb	208	159	NoGas	1.800	ppb	0.9	39,544	100	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Mix	1.1	842,612	843670.243333333	89.3	
Sc	45	H2	Analog	0.7	1,568,561	1761203.933333333	89.1	
Sc	45	He	Pulse	0.2	247,112	270213.02	91.5	
Sc	45	NoGas	Analog	1.1	2,433,087	2719052.54	89.5	
Ge	74	H2	Pulse	0.3	504,856	547887.95	92.1	
Ge	74	He	Pulse	0.5	151,055	161577.683333333	93.5	
Ge	74	NoGas	Pulse	1.2	655,306	710934.333333333	92.2	
Rh	103	He	Pulse	0.6	342,392	367685.51	93.1	
Rh	103	NoGas	Pulse	0.2	684,470	751394.163333333	91.1	
Tb	159	He	Pulse	0.6	500,328	522974.92	95.7	
Tb	159	NoGas	Pulse	0.3	1,196,469	1255414.6	95.3	
Bi	209	He	Pulse	1.0	300,528	308812.996666667	97.3	
Bi	209	NoGas	Pulse	0.9	708,176	737867.09	96.0	

Quantitation Report ICPMS5

File Name 018ICSA.d  
 File Path C:\Agilent\ICPMH\1\DATA\9K26027.b  
 Acq Time 11/26/2019 12:26:56 Sample Type  
 Sample Name **9K26027-IFA1**  
 Comment **A19K340** ICSA  
 Last Calib 11/26/2019 11:53:02  
 Prep Dilution 1.0000 Vial: 1111  
 Total Dilution **1.0000** Operator Name ICPMS Analyst

FullQuant Table

Element	Mass	ISTD	Tune Mode	Raw Conc	Corrected Conc.	Units	RSD(%)	ExpectedValue	QC Flag
Be	9	6	NoGas	0.004	0.004	ppb	129.3		
Na	23	45	He	255357.63	255357.630	ppb	0.3		
Mg	24	45	He	102213.54	102213.540	ppb	0.5	100000	
Al	27	45	He	101984.96	101984.960	ppb	0.3	100000	
K	39	45	He	100069.207	100069.207	ppb	0.7	100000	
Ca	44	45	H2	297760.082	297760.082	ppb	4.2		
[Ca]	44	45	He	304384.484	304384.484	ppb	0.3		
Ti	47	45	NoGas	2097.64	2097.640	ppb	1.3		
V	51	74	He	-0.047	-0.047	ppb	N/A	2	
Cr	52	74	He	1.775	1.775	ppb	0.6	2	
Mn	55	74	He	3.469	3.469	ppb	2.4	2	> CRI
Fe	56	74	H2	248497.298	248497.298	ppb	1.6		
Co	59	74	He	0.851	0.851	ppb	6.7		
Ni	60	74	He	0.826	0.826	ppb	4.2	2	
Cu	65	74	He	0.795	0.795	ppb	4.3	2	
Zn	66	74	He	2.528	2.528	ppb	4.3	2	> CRI
As	75	74	He	0.199	0.199	ppb	25.8	0.9	
Se	78	74	H2	0.24	0.240	ppb	26.2	0.9	
Mo	95	103	He	2264.884	2264.884	ppb	0.5	2000	
Ag	107	103	He	0.31	0.310	ppb	4.1		
Cd	111	103	He	5.976	5.976	ppb	2.4		
[Cd]	111	103	NoGas	0.439	0.439	ppb	57.0		
Sb	121	103	He	0.182	0.182	ppb	11.9	0.9	
Ba	138	159	He	1.607	1.607	ppb	3.1	2	
W	182	159	NoGas	68.049	68.049	ppb	0.5		
Hg	201	159	NoGas	59.448	59.448	ppt	9.3		
Tl	205	159	He	0.001	0.001	ppb	56.7	0.9	
Pb	208	159	NoGas	0.762	0.762	ppb	2.5		

ISTD Table:

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD Recovery %	QC Flag
Li	6	NoGas	783,684	0.3	943670.243333333	Pulse	83.0	
Sc	45	H2	1,209,704	5.3	1761203.933333333	Mix	68.7	IS Q-06
Sc	45	He	205,060	0.9	270213.02	Pulse	75.9	
Sc	45	NoGas	2,181,382	2.0	2719052.54	Analog	80.2	
Ge	74	H2	356,482	1.2	547887.95	Pulse	65.1	IS Q-06
Ge	74	He	116,692	1.2	161577.683333333	Pulse	72.2	
Ge	74	NoGas	531,058	0.7	710934.333333333	Pulse	74.7	
Rh	103	He	240,305	1.0	367685.51	Pulse	65.4	IS Q-06
Rh	103	NoGas	512,246	0.3	751394.163333333	Pulse	68.2	IS Q-06
Tb	159	He	400,834	1.2	522974.92	Pulse	76.6	
Tb	159	NoGas	1,017,291	0.7	1255414.6	Pulse	81.0	
Bi	209	He	209,230	1.1	308812.996666667	Pulse	67.8	IS Q-06
Bi	209	NoGas	530,044	0.1	737867.09	Pulse	71.8	

Quantitation Report ICPMS5

File Name 019ICSB.d  
 File Path C:\Agilent\ICPMH\1\DATA\9K26027.b  
 Acq Time 11/26/2019 12:31:28 Sample Type  
 Sample Name **9K26027-IFB1**  
 Comment **A19K341** ICSB  
 Last Calib 11/26/2019 11:53:02  
 Prep Dilution 1.0000 Vial: 1112  
 Total Dilution **1.0000** Operator Name ICPMS Analyst

FullQuant Table

Element	Mass	ISTD	Tune Mode	Raw Conc	Corrected Conc.	Units	RSD(%)	ExpectedValue	QC Flag
Be	9	6	NoGas	0.008	0.008	ppb	72.1		
Na	23	45	He	258287.269	258287.269	ppb	0.9		
Mg	24	45	He	102382.081	102382.081	ppb	0.9	100000	
Al	27	45	He	101949.329	101949.329	ppb	1.1	100000	
K	39	45	He	98215.543	98215.543	ppb	1.1	100000	
Ca	44	45	H2	284022.194	284022.194	ppb	0.6		
[Ca]	44	45	He	303070.26	303070.260	ppb	0.6		
Ti	47	45	NoGas	2101.717	2101.717	ppb	0.3		
V	51	74	He	211.164	211.164	ppb	0.4	200	
Cr	52	74	He	204.159	204.159	ppb	0.3	200	
Mn	55	74	He	209.713	209.713	ppb	0.7	200	
Fe	56	74	H2	250045.595	250045.595	ppb	0.7		
Co	59	74	He	197.901	197.901	ppb	0.2		
Ni	60	74	He	196.786	196.786	ppb	0.3	200	
Cu	65	74	He	195.654	195.654	ppb	0.7	200	
Zn	66	74	He	95.922	95.922	ppb	0.7	100	
As	75	74	He	99.195	99.195	ppb	0.8	100	
Se	78	74	H2	99.835	99.835	ppb	0.6	100	
Mo	95	103	He	2263.526	2263.526	ppb	1.3	2000	
Ag	107	103	He	50.707	50.707	ppb	0.8	50	
Cd	111	103	He	103.903	103.903	ppb	0.6		
[Cd]	111	103	NoGas	100.531	100.531	ppb	1.9		
Sb	121	103	He	0.171	0.171	ppb	16.7	0.9	
Ba	138	159	He	1.721	1.721	ppb	3.2	2	> +/- 10%
W	182	159	NoGas	68.051	68.051	ppb	1.7		
Hg	201	159	NoGas	1943.39	1943.390	ppt	1.7		
Tl	205	159	He	0.004	0.004	ppb	99.4	0.9	
Pb	208	159	NoGas	0.78	0.780	ppb	2.8		

ISTD Table:

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD Recovery %	QC Flag
Li	6	NoGas	780,044	0.5	943670.243333333	Pulse	82.7	
Sc	45	H2	1,331,093	0.6	1761203.933333333	Analog	75.6	
Sc	45	He	207,070	0.9	270213.02	Pulse	76.6	
Sc	45	NoGas	2,195,002	1.4	2719052.54	Analog	80.7	
Ge	74	H2	372,301	0.5	547887.95	Pulse	68.0	IS Q-06
Ge	74	He	115,313	1.0	161577.683333333	Pulse	71.4	
Ge	74	NoGas	527,120	2.0	710934.333333333	Pulse	74.1	
Rh	103	He	237,541	0.4	367685.51	Pulse	64.6	IS Q-06
Rh	103	NoGas	501,985	1.3	751394.163333333	Pulse	66.8	IS Q-06
Tb	159	He	390,126	0.6	522974.92	Pulse	74.6	
Tb	159	NoGas	1,000,084	1.5	1255414.6	Pulse	79.7	
Bi	209	He	205,171	0.2	308812.996666667	Pulse	66.4	IS Q-06
Bi	209	NoGas	519,476	1.1	737867.09	Pulse	70.4	

### Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name: <b>9K26027-CCV1</b>	Total Dilution: <b>1.0000</b>
File Name: 031_CCV.d	Vial: 2
File Path: C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type: CCV
Acq Time: 11/26/2019 13:42:12	I.S. Reference File: 003CALB.d
Comment: <b>A19J138 - ESS 11/26</b>	Last Calibration: 11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	40.024	ppb	0.2	80,569	40	100.06	
Na	23	45	He	3962.373	ppb	0.8	3,049,215	4000	99.06	
Mg	24	45	He	4196.601	ppb	2.1	1,809,941	4000	104.92	
Al	27	45	He	3956.300	ppb	0.5	928,286	4000	98.91	
K	39	45	He	4180.579	ppb	0.7	1,630,773	4000	104.51	
Ca	44	45	H2	3993.997	ppb	2.1	620,177	4000	99.85	
[Ca]	44	45	He	4117.001	ppb	0.3	79,523	4000	102.93	
Ti	47	45	NoGas	95.835	ppb	2.4	81,656	100	95.84	
V	51	74	He	93.175	ppb	0.2	248,952	100	93.18	
Cr	52	74	He	94.255	ppb	0.6	290,929	100	94.26	
Mn	55	74	He	99.439	ppb	0.3	220,520	100	99.44	
Fe	56	74	H2	4019.051	ppb	0.6	32,162,091	4000	100.48	
Co	59	74	He	98.647	ppb	0.6	416,160	100	98.65	
Ni	60	74	He	102.577	ppb	0.8	103,776	100	102.58	
Cu	65	74	He	101.955	ppb	0.8	127,767	100	101.96	
Zn	66	74	He	100.932	ppb	0.5	49,894	100	100.93	
As	75	74	He	96.577	ppb	0.9	30,236	100	96.58	
Se	78	74	H2	41.287	ppb	1.6	8,887	40	103.22	
Mo	95	103	He	39.724	ppb	0.7	51,495	40	99.31	
Ag	107	103	He	40.738	ppb	0.6	152,773	40	101.85	
Cd	111	103	He	98.588	ppb	0.4	62,465	100	98.59	
[Cd]	111	103	NoGas	95.008	ppb	0.3	158,917	100	95.01	
Sb	121	103	He	40.918	ppb	0.8	69,144	40	102.3	
Ba	138	159	He	101.612	ppb	0.4	399,406	100	101.61	
Hg	201	159	NoGas	820.996	ppt	3.5	709	800	102.62	
Tl	205	159	He	40.108	ppb	0.4	272,726	40	100.27	
Pb	208	159	NoGas	97.365	ppb	0.4	1,955,125	100	97.36	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.4	715,444	943670.243333333	75.8	
Sc	45	H2	Analog	1.9	1,344,918	1761203.933333333	76.4	
Sc	45	He	Pulse	0.5	216,529	270213.02	80.1	
Sc	45	NoGas	Analog	0.7	2,139,411	2719052.54	78.7	
Ge	74	H2	Pulse	0.6	438,049	547887.95	80.0	
Ge	74	He	Pulse	0.5	133,699	161577.683333333	82.7	
Ge	74	NoGas	Pulse	0.0	570,411	710934.333333333	80.2	
Rh	103	He	Pulse	0.7	299,967	367685.51	81.6	
Rh	103	NoGas	Pulse	0.2	589,916	751394.163333333	78.5	
Tb	159	He	Pulse	0.9	470,638	522974.92	90.0	
Tb	159	NoGas	Pulse	0.2	1,108,821	1255414.6	88.3	
Bi	209	He	Pulse	1.2	278,786	308812.996666667	90.3	
Bi	209	NoGas	Pulse	0.2	654,407	737867.09	88.7	

### Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name:	9K26027-CCB1	Total Dilution:	1.0000
File Name:	032_CCB.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCB
Acq Time:	11/26/2019 13:46:51	I.S. Reference File:	003CALB.d
Comment:	CCB	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.003	ppb	179.8	30	
Na	23	45	He	5.490	ppb	3.9	6,647	
Mg	24	45	He	0.716	ppb	8.3	606	
Al	27	45	He	0.527	ppb	34.1	191	
K	39	45	He	1.881	ppb	59.8	19,651	
Ca	44	45	H2	0.968	ppb	17.0	491	
[Ca]	44	45	He	0.455	ppb	301.6	129	
Ti	47	45	NoGas	0.026	ppb	69.2	43	
V	51	74	He	-0.302	ppb	N/A	900	
Cr	52	74	He	0.006	ppb	331.2	204	
Mn	55	74	He	0.004	ppb	199.7	41	
Fe	56	74	H2	0.882	ppb	9.8	14,666	
Co	59	74	He	0.010	ppb	40.1	51	
Ni	60	74	He	-0.034	ppb	N/A	44	
Cu	65	74	He	0.007	ppb	133.5	39	
Zn	66	74	He	0.006	ppb	473.3	28	
As	75	74	He	0.005	ppb	406.8	23	
Se	78	74	H2	0.045	ppb	14.9	13	
Mo	95	103	He	0.045	ppb	17.9	62	
Ag	107	103	He	0.006	ppb	9.0	26	
Cd	111	103	He	0.026	ppb	33.8	19	
[Cd]	111	103	NoGas	0.020	ppb	34.6	41	
Sb	121	103	He	0.250	ppb	3.4	462	
Ba	138	159	He	0.012	ppb	80.1	119	
Hg	201	159	NoGas	5.553	ppt	17.8	7	
Tl	205	159	He	0.000	ppb	3944.6	24	
Pb	208	159	NoGas	0.032	ppb	6.3	1,153	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.3	714,896	943670.243333333	75.8	
Sc	45	H2	Analog	1.0	1,388,868	1761203.933333333	78.9	
Sc	45	He	Pulse	1.6	215,617	270213.02	79.8	
Sc	45	NoGas	Analog	0.8	2,090,512	2719052.54	76.9	
Ge	74	H2	Pulse	0.5	447,164	547887.95	81.6	
Ge	74	He	Pulse	0.8	134,415	161577.683333333	83.2	
Ge	74	NoGas	Pulse	0.8	571,115	710934.333333333	80.3	
Rh	103	He	Pulse	0.3	307,475	367685.51	83.6	
Rh	103	NoGas	Pulse	0.9	602,032	751394.163333333	80.1	
Tb	159	He	Pulse	0.8	471,503	522974.92	90.2	
Tb	159	NoGas	Pulse	1.2	1,105,605	1255414.6	88.1	
Bi	209	He	Pulse	0.3	285,417	308812.996666667	92.4	
Bi	209	NoGas	Pulse	0.8	665,496	737867.09	90.2	

### Quantitation Report - ICPMS5

Sample Name:	9111213-BLK1	Total Dilution:	10.0000
File Name:	034SMPL.d	Vial:	3112
File Path:	C:\Agilent\ICPMH1\DATA\9K26027.b	Sample Type:	Sample
Acq Time:	11/26/2019 13:56:13	I.S. Reference File:	003CALB.d
Comment:	9111213 TCLP RCRA	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	LDR	QC Flag
Be	9	6	NoGas	0.017	ppb	68.2	56	100	
Na	23	45	He	28488.45	ppb	1.3	21,298,708	50000	
Mg	24	45	He	2.902	ppb	6.0	1,508	50000	
Al	27	45	He	1.703	ppb	33.2	454	50000	
K	39	45	He	6.196	ppb	3.0	20,808	50000	
Ca	44	45	H2	22.651	ppb	2.7	3,789	50000	
[Ca]	44	45	He	24.042	ppb	17.0	568	50000	
Ti	47	45	NoGas	0.087	ppb	26.8	92	2500	
V	51	74	He	-0.358	ppb	N/A	720	500	
Cr	52	74	He	0.105	ppb	15.3	493	1000	
Mn	55	74	He	0.037	ppb	36.7	112	2500	
Fe	56	74	H2	1.582	ppb	2.0	19,626	50000	
Co	59	74	He	0.004	ppb	110.0	26	500	
Ni	60	74	He	0.508	ppb	2.2	572	1000	
Cu	65	74	He	0.131	ppb	19.5	187	1000	
Zn	66	74	He	0.606	ppb	7.5	313	2500	
As	75	74	He	-0.003	ppb	N/A	19	500	
Se	78	74	H2	0.008	ppb	235.9	4	100	
Mo	95	103	He	0.018	ppb	66.3	24	100	
Ag	107	103	He	0.004	ppb	35.0	18	100	
Cd	111	103	He	0.011	ppb	47.7	8	1000	
[Cd]	111	103	NoGas	0.01	ppb	98.3	22	1000	
Sb	121	103	He	0.043	ppb	25.9	99	100	
Ba	138	159	He	1.468	ppb	3.5	5,732	2500	
W	182	159	NoGas	0.004	ppb	34.2	33	40	
Hg	201	159	NoGas	4.775	ppt	52.4	6	4000	
Tl	205	159	He	0.012	ppb	18.3	107	100	
Pb	208	159	NoGas	0.115	ppb	2.8	2,728	500	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref. CPS	Det.	ISTD, %	QC Flag
Li	6	NoGas	694,508	0.2	943670.243333333	Pulse	73.6	
Sc	45	H2	1,326,610	1.0	1761203.933333333	Analog	75.3	
Sc	45	He	210,518	0.9	270213.02	Pulse	77.9	
Sc	45	NoGas	2,034,848	1.4	2719052.54	Analog	74.8	
Ge	74	H2	430,555	0.4	547887.95	Pulse	78.6	
Ge	74	He	129,143	0.7	161577.683333333	Pulse	79.9	
Ge	74	NoGas	549,235	1.0	710934.333333333	Pulse	77.3	
Rh	103	He	292,457	0.6	367685.51	Pulse	79.5	
Rh	103	NoGas	568,443	0.7	751394.163333333	Pulse	75.7	
Tb	159	He	461,968	0.8	522974.92	Pulse	88.3	
Tb	159	NoGas	1,076,920	0.2	1255414.6	Pulse	85.8	
Bi	209	He	273,213	1.0	308812.996666667	Pulse	88.5	
Bi	209	NoGas	637,288	0.9	737867.09	Pulse	86.4	

### Quantitation Report - ICPMS5

Sample Name:	9111213-BS1	Total Dilution:	10.0000
File Name:	035SMPL.d	Vial:	3113
File Path:	C:\Agilent\ICPMH1\DATA\9K26027.b	Sample Type:	Sample
Acq Time:	11/26/2019 14:01:07	I.S. Reference File:	003CALB.d
Comment:	9111213 TCLP RCRA	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	LDR	QC Flag
Be	9	6	NoGas	50.136	ppb	1.1	97,706	100	
Na	23	45	He	29185.116	ppb	0.5	21,668,615	50000	
Mg	24	45	He	2.172	ppb	7.9	1,193	50000	
Al	27	45	He	0.345	ppb	23.6	144	50000	
K	39	45	He	7.917	ppb	9.3	21,303	50000	
Ca	44	45	H2	18.653	ppb	6.1	3,207	50000	
[Ca]	44	45	He	19.575	ppb	13.2	481	50000	
Ti	47	45	NoGas	0.058	ppb	54.9	68	2500	
V	51	74	He	48.085	ppb	0.8	124,073	500	
Cr	52	74	He	98.463	ppb	0.6	291,637	1000	
Mn	55	74	He	51.095	ppb	1.0	108,749	2500	
Fe	56	74	H2	-0.225	ppb	N/A	5,385	50000	
Co	59	74	He	49.729	ppb	1.0	201,322	500	
Ni	60	74	He	52.385	ppb	0.9	50,892	1000	
Cu	65	74	He	52.805	ppb	1.6	63,508	1000	
Zn	66	74	He	107.495	ppb	1.0	50,990	2500	
As	75	74	He	101.777	ppb	0.9	30,580	500	
Se	78	74	H2	20.089	ppb	1.1	4,223	100	
Mo	95	103	He	0.005	ppb	84.9	8	100	
Ag	107	103	He	21.179	ppb	0.4	76,755	100	
Cd	111	103	He	20.72	ppb	1.0	12,687	1000	
[Cd]	111	103	NoGas	20.545	ppb	0.4	32,989	1000	
Sb	121	103	He	22.161	ppb	1.7	36,197	100	
Ba	138	159	He	211.281	ppb	0.7	812,745	2500	
W	182	159	NoGas	0.004	ppb	35.2	31	40	
Hg	201	159	NoGas	2133.392	ppt	2.5	1,779	4000	
Tl	205	159	He	51.271	ppb	0.7	341,214	100	
Pb	208	159	NoGas	102.663	ppb	0.1	1,992,811	500	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref/CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	692,659	0.4	943670.243333333	Pulse	73.4	
Sc	45	H2	1,339,927	1.8	1761203.933333333	Analog	76.1	
Sc	45	He	209,047	0.2	270213.02	Pulse	77.4	
Sc	45	NoGas	2,049,201	1.1	2719052.54	Analog	75.4	
Ge	74	H2	427,634	0.4	547887.95	Pulse	78.1	
Ge	74	He	128,303	1.2	161577.683333333	Pulse	79.4	
Ge	74	NoGas	549,044	0.6	710934.333333333	Pulse	77.2	
Rh	103	He	289,876	0.9	367685.51	Pulse	78.8	
Rh	103	NoGas	566,216	0.3	751394.163333333	Pulse	75.4	
Tb	159	He	460,614	0.3	522974.92	Pulse	88.1	
Tb	159	NoGas	1,071,880	0.5	1255414.6	Pulse	85.4	
Bi	209	He	272,854	1.5	308812.996666667	Pulse	88.4	
Bi	209	NoGas	637,748	0.6	737867.09	Pulse	86.4	



### Quantitation Report - ICPMS5

Sample Name:	A9K0412-01	Total Dilution:	10.0000
File Name:	036SMPL.d	Vial:	3114
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	Sample
Acq Time:	11/26/2019 14:05:46	I.S. Reference File:	003CALB.d
Comment:	9111213 TCLP RCRA	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	LDR	QC Flag
Be	9	6	NoGas	0.024	ppb	39.9	70	100	
Na	23	45	He	27911.889	ppb	0.9	20,741,527	50000	
Mg	24	45	He	164.663	ppb	0.2	68,903	50000	
Al	27	45	He	8.76	ppb	10.9	2,052	50000	
K	39	45	He	92.062	ppb	1.2	52,669	50000	
Ca	44	45	H2	629.191	ppb	0.8	96,830	50000	
[Ca]	44	45	He	662.034	ppb	1.9	12,455	50000	
Ti	47	45	NoGas	0.244	ppb	18.9	218	2500	
V	51	74	He	-0.357	ppb	N/A	723	500	
Cr	52	74	He	0.045	ppb	49.3	312	1000	
Mn	55	74	He	19.283	ppb	2.0	41,305	2500	
Fe	56	74	H2	6.572	ppb	1.4	58,650	50000	
Co	59	74	He	0.356	ppb	5.4	1,460	500	
Ni	60	74	He	0.749	ppb	3.4	807	1000	
Cu	65	74	He	0.276	ppb	9.2	362	1000	
Zn	66	74	He	2.496	ppb	4.3	1,215	2500	
As	75	74	He	0.03	ppb	22.2	29	500	
Se	78	74	H2	0.008	ppb	204.5	4	100	
Mo	95	103	He	0.009	ppb	51.0	13	100	
Ag	107	103	He	0.002	ppb	89.4	10	100	
Cd	111	103	He	0.015	ppb	46.8	11	1000	
[Cd]	111	103	NoGas	0.013	ppb	20.5	27	1000	
Sb	121	103	He	0.027	ppb	63.3	72	100	
Ba	138	159	He	5.835	ppb	0.8	22,462	2500	
W	182	159	NoGas	0.005	ppb	17.2	38	40	
Hg	201	159	NoGas	10.823	ppt	16.5	11	4000	
Tl	205	159	He	0.014	ppb	11.9	113	100	
Pb	208	159	NoGas	0.038	ppb	19.6	1,231	500	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	689,031	0.5	943670.243333333	Pulse	73.0	
Sc	45	H2	1,328,914	0.7	1761203.933333333	Analog	75.5	
Sc	45	He	209,231	0.0	270213.02	Pulse	77.4	
Sc	45	NoGas	2,029,926	0.4	2719052.54	Analog	74.7	
Ge	74	H2	428,949	0.5	547887.95	Pulse	78.3	
Ge	74	He	129,061	0.7	161577.683333333	Pulse	79.9	
Ge	74	NoGas	544,403	0.7	710934.333333333	Pulse	76.6	
Rh	103	He	292,203	0.9	367685.51	Pulse	79.5	
Rh	103	NoGas	562,548	0.7	751394.163333333	Pulse	74.9	
Tb	159	He	459,527	0.9	522974.92	Pulse	87.9	
Tb	159	NoGas	1,071,305	0.5	1255414.6	Pulse	85.3	
Bi	209	He	274,110	0.9	308812.996666667	Pulse	88.8	
Bi	209	NoGas	633,754	0.6	737867.09	Pulse	85.9	

### Quantitation Report - ICPMS5

Sample Name:	9111213-MS1	Total Dilution:	10.0000
File Name:	037SMPL.d	Vial:	3115
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	Sample
Acq Time:	11/26/2019 14:10:25	I.S. Reference File:	003CALB.d
Comment:	9111213 TCLP RCRA	Last Calibration:	11/26/2019 11:53:02

**FullQuant Table:**

Element	Mass	ISTD	Tune Mode	Raw Conc	Units	RSD(%)	CPS	LDR	QC Flag
Be	9	6	NoGas	48.671	ppb	1.1	94,870	100	
Na	23	45	He	27546.903	ppb	1.1	20,387,467	50000	
Mg	24	45	He	161.861	ppb	0.3	67,463	50000	
Al	27	45	He	8	ppb	7.9	1,872	50000	
K	39	45	He	90.194	ppb	0.8	51,764	50000	
Ca	44	45	H2	619.987	ppb	1.7	94,860	50000	
[Ca]	44	45	He	636.55	ppb	1.8	11,931	50000	
Ti	47	45	NoGas	0.389	ppb	26.2	337	2500	
V	51	74	He	46.569	ppb	0.2	120,458	500	
Cr	52	74	He	95.343	ppb	0.6	282,969	1000	
Mn	55	74	He	68.634	ppb	0.7	146,362	2500	
Fe	56	74	H2	5.819	ppb	0.6	52,609	50000	
Co	59	74	He	48.801	ppb	0.5	197,964	500	
Ni	60	74	He	50.619	ppb	0.8	49,281	1000	
Cu	65	74	He	51.207	ppb	1.3	61,714	1000	
Zn	66	74	He	105.472	ppb	0.7	50,134	2500	
As	75	74	He	99.077	ppb	0.7	29,826	500	
Se	78	74	H2	19.556	ppb	4.1	4,112	100	
Mo	95	103	He	0.006	ppb	97.7	9	100	
Ag	107	103	He	20.53	ppb	0.7	74,662	100	
Cd	111	103	He	20.229	ppb	0.6	12,430	1000	
[Cd]	111	103	NoGas	19.566	ppb	1.0	31,313	1000	
Sb	121	103	He	21.053	ppb	1.1	34,509	100	
Ba	138	159	He	209.731	ppb	0.8	807,982	2500	
W	182	159	NoGas	0.007	ppb	51.0	49	40	
Hg	201	159	NoGas	2041.113	ppt	1.9	1,705	4000	
Tl	205	159	He	50.072	ppb	1.2	333,729	100	
Pb	208	159	NoGas	99.176	ppb	0.4	1,928,478	500	

**ISTD Table:**

Element	Mass	Tune Mode	CPS	RSD(%)	ISTD Ref CPS	Det.	ISTD %	QC Flag
Li	6	NoGas	692,812	0.2	943670.243333333	Pulse	73.4	
Sc	45	H2	1,321,296	1.2	1761203.933333333	Analog	75.0	
Sc	45	He	208,390	0.5	270213.02	Pulse	77.1	
Sc	45	NoGas	2,032,865	0.5	2719052.54	Analog	74.8	
Ge	74	H2	427,803	0.7	547887.95	Pulse	78.1	
Ge	74	He	128,560	0.6	161577.683333333	Pulse	79.6	
Ge	74	NoGas	546,366	1.0	710934.333333333	Pulse	76.9	
Rh	103	He	290,879	0.6	367685.51	Pulse	79.1	
Rh	103	NoGas	564,359	0.8	751394.163333333	Pulse	75.1	
Tb	159	He	461,330	1.2	522974.92	Pulse	88.2	
Tb	159	NoGas	1,073,758	0.9	1255414.6	Pulse	85.5	
Bi	209	He	274,644	1.0	308812.996666667	Pulse	88.9	
Bi	209	NoGas	636,218	0.5	737867.09	Pulse	86.2	

### Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name: <b>9K26027-CCV2</b>	Total Dilution: <b>1.0000</b>
File Name: <b>043_CCV.d</b>	Vial: <b>2</b>
File Path: <b>C:\Agilent\ICPMH\1\DATA\9K26027.b</b>	Sample Type: <b>CCV</b>
Acq Time: <b>11/26/2019 14:40:03</b>	I.S. Reference File: <b>003CALB.d</b>
Comment: <b>A19J138 - ESS 11/26</b>	Last Calibration: <b>11/26/2019 11:53:02</b>

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	39.731	ppb	0.7	81,457	40	99.33	
Na	23	45	He	3950.785	ppb	0.8	3,115,792	4000	98.77	
Mg	24	45	He	4243.731	ppb	1.4	1,875,661	4000	106.09	
Al	27	45	He	3941.024	ppb	0.4	947,624	4000	98.53	
K	39	45	He	4143.091	ppb	0.7	1,656,365	4000	103.58	
Ca	44	45	H2	3964.961	ppb	0.8	664,578	4000	99.12	
[Ca]	44	45	He	4156.829	ppb	1.1	82,281	4000	103.92	
Ti	47	45	NoGas	97.008	ppb	1.4	82,875	100	97.01	
V	51	74	He	92.965	ppb	0.1	254,493	100	92.96	
Cr	52	74	He	94.717	ppb	0.5	299,530	100	94.72	
Mn	55	74	He	99.845	ppb	0.3	226,859	100	99.84	
Fe	56	74	H2	4048.947	ppb	0.4	34,334,783	4000	101.22	
Co	59	74	He	98.793	ppb	0.5	427,007	100	98.79	
Ni	60	74	He	102.849	ppb	1.6	106,605	100	102.85	
Cu	65	74	He	101.694	ppb	0.3	130,567	100	101.69	
Zn	66	74	He	101.178	ppb	1.4	51,245	100	101.18	
As	75	74	He	96.611	ppb	0.2	30,990	100	96.61	
Se	78	74	H2	40.723	ppb	1.6	9,289	40	101.81	
Mo	95	103	He	39.221	ppb	1.2	52,125	40	98.05	
Ag	107	103	He	40.288	ppb	0.7	154,896	40	100.72	
Cd	111	103	He	98.034	ppb	1.3	63,676	100	98.03	
[Cd]	111	103	NoGas	95.191	ppb	1.3	162,143	100	95.19	
Sb	121	103	He	40.494	ppb	0.8	70,150	40	101.24	
Ba	138	159	He	102.699	ppb	0.7	408,294	100	102.7	
Hg	201	159	NoGas	795.939	ppt	4.7	696	800	99.49	
Tl	205	159	He	40.403	ppb	0.4	277,869	40	101.01	
Pb	208	159	NoGas	97.502	ppb	0.3	1,979,917	100	97.5	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.6	728,653	943670.243333333	77.2	
Sc	45	H2	Analog	1.1	1,451,492	1761203.933333333	82.4	
Sc	45	He	Pulse	0.4	221,896	270213.02	82.1	
Sc	45	NoGas	Analog	1.6	2,145,132	2719052.54	78.9	
Ge	74	H2	Pulse	0.1	464,182	547887.95	84.7	
Ge	74	He	Pulse	0.2	136,982	161577.683333333	84.8	
Ge	74	NoGas	Pulse	0.8	578,742	710934.333333333	81.4	
Rh	103	He	Pulse	0.9	307,537	367685.51	83.6	
Rh	103	NoGas	Pulse	0.1	600,735	751394.163333333	79.9	
Tb	159	He	Pulse	0.3	476,006	522974.92	91.0	
Tb	159	NoGas	Pulse	0.1	1,121,294	1255414.6	89.3	
Bi	209	He	Pulse	0.5	282,511	308812.996666667	91.5	
Bi	209	NoGas	Pulse	0.4	662,659	737867.09	89.8	

### Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name:	9K26027-CCB2	Total Dilution:	1.0000
File Name:	044_CCB.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCB
Acq Time:	11/26/2019 14:44:42	I.S. Reference File:	003CALB.d
Comment:	CCB	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.009	ppb	27.5	42	
Na	23	45	He	5.720	ppb	3.0	6,816	
Mg	24	45	He	0.430	ppb	22.4	482	
Al	27	45	He	0.427	ppb	56.2	168	
K	39	45	He	2.111	ppb	40.0	19,717	
Ca	44	45	H2	0.881	ppb	47.4	474	
[Ca]	44	45	He	0.226	ppb	892.4	124	
Ti	47	45	NoGas	0.021	ppb	48.9	40	
V	51	74	He	-0.288	ppb	N/A	936	
Cr	52	74	He	0.007	ppb	164.7	207	
Mn	55	74	He	0.013	ppb	83.4	62	
Fe	56	74	H2	0.678	ppb	7.1	13,036	
Co	59	74	He	0.007	ppb	32.1	39	
Ni	60	74	He	-0.045	ppb	N/A	33	
Cu	65	74	He	0.014	ppb	90.2	47	
Zn	66	74	He	0.028	ppb	13.0	39	
As	75	74	He	-0.008	ppb	N/A	19	
Se	78	74	H2	0.019	ppb	70.3	7	
Mo	95	103	He	0.036	ppb	27.6	50	
Ag	107	103	He	0.006	ppb	58.2	26	
Cd	111	103	He	0.019	ppb	87.6	14	
[Cd]	111	103	NoGas	0.011	ppb	87.5	25	
Sb	121	103	He	0.260	ppb	9.2	483	
Ba	138	159	He	0.010	ppb	77.8	113	
Hg	201	159	NoGas	4.399	ppt	40.2	6	
Tl	205	159	He	0.003	ppb	148.0	43	
Pb	208	159	NoGas	0.026	ppb	6.2	1,033	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.4	716,842	943670.243333333	76.0	
Sc	45	H2	Analog	1.1	1,381,647	1761203.933333333	78.4	
Sc	45	He	Pulse	0.5	215,338	270213.02	79.7	
Sc	45	NoGas	Analog	1.3	2,113,667	2719052.54	77.7	
Ge	74	H2	Pulse	0.1	448,459	547887.95	81.9	
Ge	74	He	Pulse	0.3	134,240	161577.683333333	83.1	
Ge	74	NoGas	Pulse	0.6	570,073	710934.333333333	80.2	
Rh	103	He	Pulse	1.1	309,562	367685.51	84.2	
Rh	103	NoGas	Pulse	0.5	601,448	751394.163333333	80.0	
Tb	159	He	Pulse	0.7	471,768	522974.92	90.2	
Tb	159	NoGas	Pulse	0.5	1,102,133	1255414.6	87.8	
Bi	209	He	Pulse	0.5	284,635	308812.996666667	92.2	
Bi	209	NoGas	Pulse	0.4	662,689	737867.09	89.8	

### CRL Verification Report - ICPMS5

Sample Name: <b>9K26027-CRL4</b>	Total Dilution: <b>1.0000</b>
File Name: <b>.045CRL.d</b>	Vial: <b>1102</b>
File Path: <b>C:\Agilent\ICPMH\1\DATA\9K26027.b</b>	Sample Type: <b>CRL1</b>
Acq Time: <b>11/26/2019 14:49:25</b>	I.S. Reference File: <b>003CALB.d</b>
Comment: <b>A19K144 - ESS 11/26</b>	Last Calibration: <b>11/26/2019 11:53:02</b>

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	0.183	ppb	15.9	392	101.67	
Na	23	45	He	12.979	ppb	3.6	12,392	144.21	R-11
Mg	24	45	He	9.021	ppb	3.1	4,175	100.23	
Al	27	45	He	8.740	ppb	5.9	2,111	97.11	
K	39	45	He	11.455	ppb	6.0	23,345	127.28	
Ca	44	45	H2	8.915	ppb	1.6	1,740	99.06	
[Ca]	44	45	He	7.954	ppb	34.3	273	88.38	
Ti	47	45	NoGas	0.158	ppb	10.3	155	87.78	
V	51	74	He	-0.094	ppb	N/A	1,442	-52.22	R-11
Cr	52	74	He	0.164	ppb	20.3	689	91.11	
Mn	55	74	He	0.177	ppb	7.4	424	98.33	
Fe	56	74	H2	8.474	ppb	1.1	76,082	94.16	
Co	59	74	He	0.162	ppb	9.5	689	90	
Ni	60	74	He	0.118	ppb	17.1	198	65.56	R-11
Cu	65	74	He	0.209	ppb	18.8	290	116.11	
Zn	66	74	He	0.168	ppb	35.4	108	93.33	
As	75	74	He	0.161	ppb	39.1	71	89.44	
Se	78	74	H2	0.162	ppb	19.7	38	90	
Mo	95	103	He	0.200	ppb	8.4	266	111.11	
Ag	107	103	He	0.160	ppb	11.3	612	88.89	
Cd	111	103	He	0.213	ppb	7.6	139	118.33	
[Cd]	111	103	NoGas	0.205	ppb	14.1	354	113.89	
Sb	121	103	He	0.254	ppb	7.6	464	141.11	R-11
Ba	138	159	He	0.173	ppb	7.8	748	96.11	
Hg	201	159	NoGas	10.603	ppt	38.2	12	147.26	R-11
Tl	205	159	He	0.177	ppb	5.9	1,221	98.33	
Pb	208	159	NoGas	0.193	ppb	3.0	4,366	107.22	

< MRL

< MRL

< MRL

< MRL

< MRL

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.4	714,998	943670.243333333	75.8	
Sc	45	H2	Analog	0.6	1,369,135	1761203.933333333	77.7	
Sc	45	He	Pulse	0.5	215,755	270213.02	79.8	
Sc	45	NoGas	Analog	0.7	2,119,245	2719052.54	77.9	
Ge	74	H2	Pulse	0.2	443,691	547887.95	81.0	
Ge	74	He	Pulse	1.0	133,230	161577.683333333	82.5	
Ge	74	NoGas	Pulse	1.1	567,918	710934.333333333	79.9	
Rh	103	He	Pulse	0.5	304,672	367685.51	82.9	
Rh	103	NoGas	Pulse	0.2	597,865	751394.163333333	79.6	
Tb	159	He	Pulse	0.7	468,863	522974.92	89.7	
Tb	159	NoGas	Pulse	0.6	1,103,816	1255414.6	87.9	
Bi	209	He	Pulse	0.7	283,711	308812.996666667	91.9	
Bi	209	NoGas	Pulse	0.7	662,721	737867.09	89.8	

**CRL Verification Report - ICPMS5**

Sample Name:	9K26027-CRL5	Total Dilution:	1.0000
File Name:	046_CRL.d	Vial:	1103
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL2
Acq Time:	11/26/2019 14:54:06	I.S. Reference File:	003CALB.d
Comment:	A19K145 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

Analyte Table:

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	0.888	ppb	1.5	1,806	98.67	
Na	23	45	He	48.878	ppb	0.3	39,813	108.62	
Mg	24	45	He	46.772	ppb	1.0	20,354	103.94	
Al	27	45	He	45.748	ppb	0.7	10,741	101.66	
K	39	45	He	49.285	ppb	0.2	37,799	109.52	
Ca	44	45	H2	45.134	ppb	0.6	7,421	100.3	
[Ca]	44	45	He	45.183	ppb	4.0	987	100.41	
Ti	47	45	NoGas	1.007	ppb	8.3	860	111.89	
V	51	74	He	0.608	ppb	10.5	3,301	67.56	R-11
Cr	52	74	He	0.842	ppb	5.7	2,774	93.56	
Mn	55	74	He	0.893	ppb	4.7	2,007	99.22	
Fe	56	74	H2	44.241	ppb	0.2	365,453	98.31	
Co	59	74	He	0.882	ppb	2.6	3,718	98	
Ni	60	74	He	0.857	ppb	3.2	942	95.22	
Cu	65	74	He	0.945	ppb	6.4	1,210	105	
Zn	66	74	He	0.962	ppb	8.8	499	106.89	
As	75	74	He	0.836	ppb	13.8	281	92.89	
Se	78	74	H2	0.893	ppb	3.5	197	99.22	
Mo	95	103	He	0.879	ppb	9.6	1,162	97.67	
Ag	107	103	He	0.899	ppb	1.8	3,439	99.89	
Cd	111	103	He	0.927	ppb	4.3	600	103	
[Cd]	111	103	NoGas	0.817	ppb	6.4	1,392	90.78	
Sb	121	103	He	0.998	ppb	3.4	1,747	110.89	
Ba	138	159	He	0.960	ppb	1.1	3,829	106.67	
Hg	201	159	NoGas	34.587	ppt	7.5	32	96.08	
Tl	205	159	He	0.883	ppb	2.0	6,007	98.11	
Pb	208	159	NoGas	0.909	ppb	1.3	18,538	101	

V MPL ↑ 2 ppb  
ESS 11/27/19

ISTD Table:

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.4	713,372	943670.243333333	75.6	
Sc	45	H2	Analog	0.8	1,361,225	1761203.933333333	77.3	
Sc	45	He	Pulse	0.7	215,305	270213.02	79.7	
Sc	45	NoGas	Analog	0.7	2,088,177	2719052.54	76.8	
Ge	74	H2	Pulse	0.2	443,113	547887.95	80.9	
Ge	74	He	Pulse	0.8	133,294	161577.683333333	82.5	
Ge	74	NoGas	Pulse	1.3	566,786	710934.333333333	79.7	
Rh	103	He	Pulse	0.6	305,657	367685.51	83.1	
Rh	103	NoGas	Pulse	0.3	598,420	751394.163333333	79.6	
Tb	159	He	Pulse	0.6	468,946	522974.92	89.7	
Tb	159	NoGas	Pulse	0.6	1,095,944	1255414.6	87.3	
Bi	209	He	Pulse	1.2	282,910	308812.996666667	91.6	
Bi	209	NoGas	Pulse	0.4	661,042	737867.09	89.6	

### CRL Verification Report - ICPMS5

Sample Name:	9K26027-CRL6	Total Dilution:	1.0000
File Name:	047CRL_d	Vial:	1104
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL3
Acq Time:	11/26/2019 14:58:47	I.S. Reference File:	003CALB.d
Comment:	A19K146 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	1.850	ppb	3.2	3,767	102.78	
Na	23	45	He	94.964	ppb	0.1	74,579	105.52	
Mg	24	45	He	93.002	ppb	1.0	39,923	103.34	
Al	27	45	He	92.632	ppb	2.0	21,543	102.92	
K	39	45	He	96.865	ppb	0.8	55,688	107.63	
Ca	44	45	H2	90.149	ppb	2.0	14,615	100.17	
[Ca]	44	45	He	93.898	ppb	8.9	1,909	104.33	
Ti	47	45	NoGas	1.990	ppb	9.7	1,683	110.56	
V	51	74	He	1.475	ppb	1.6	5,599	81.94	
Cr	52	74	He	1.737	ppb	3.2	5,534	96.5	
Mn	55	74	He	1.766	ppb	4.3	3,942	98.11	
Fe	56	74	H2	88.333	ppb	0.6	725,019	98.15	
Co	59	74	He	1.714	ppb	3.7	7,226	95.22	
Ni	60	74	He	1.769	ppb	2.4	1,863	98.28	
Cu	65	74	He	1.975	ppb	5.7	2,500	109.72	
Zn	66	74	He	1.928	ppb	4.8	976	107.11	
As	75	74	He	1.816	ppb	4.5	588	100.89	
Se	78	74	H2	1.846	ppb	4.8	406	102.56	
Mo	95	103	He	1.799	ppb	4.2	2,378	99.94	
Ag	107	103	He	1.841	ppb	3.7	7,039	102.28	
Cd	111	103	He	1.819	ppb	1.6	1,176	101.06	
[Cd]	111	103	NoGas	1.760	ppb	5.9	3,008	97.78	
Sb	121	103	He	1.870	ppb	5.8	3,247	103.89	
Ba	138	159	He	1.858	ppb	3.2	7,365	103.22	
Hg	201	159	NoGas	85.069	ppt	10.9	75	118.15	
Tl	205	159	He	1.852	ppb	2.8	12,606	102.89	
Pb	208	159	NoGas	1.844	ppb	0.4	37,373	102.44	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.2	719,440	943670.243333333	76.2	
Sc	45	H2	Analog	1.1	1,372,780	1761203.933333333	77.9	
Sc	45	He	Pulse	0.3	213,954	270213.02	79.2	
Sc	45	NoGas	Analog	0.8	2,095,713	2719052.54	77.1	
Ge	74	H2	Pulse	0.1	444,788	547887.95	81.2	
Ge	74	He	Pulse	0.7	133,442	161577.683333333	82.6	
Ge	74	NoGas	Pulse	0.8	572,320	710934.333333333	80.5	
Rh	103	He	Pulse	1.2	305,677	367685.51	83.1	
Rh	103	NoGas	Pulse	0.2	601,731	751394.163333333	80.1	
Tb	159	He	Pulse	1.4	470,283	522974.92	89.9	
Tb	159	NoGas	Pulse	0.6	1,104,111	1255414.6	87.9	
Bi	209	He	Pulse	0.8	283,582	308812.996666667	91.8	
Bi	209	NoGas	Pulse	0.7	662,755	737867.09	89.8	

### Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name:	9K26027-CCV3	Total Dilution:	1.0000
File Name:	058_CCV.d	Vial:	2
File Path:	C:\Agilent\ICPMH1\DATA\9K26027.b	Sample Type:	CCV
Acq Time:	11/26/2019 15:50:17	I.S. Reference File:	003CALB.d
Comment:	A19J138 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	39.919	ppb	1.0	82,244	40	99.8	
Na	23	45	He	3974.362	ppb	0.6	3,112,967	4000	99.36	
Mg	24	45	He	4285.883	ppb	1.5	1,881,383	4000	107.15	
Al	27	45	He	3945.811	ppb	0.7	942,324	4000	98.65	
K	39	45	He	4243.712	ppb	0.9	1,684,600	4000	106.09	
Ca	44	45	H2	3963.815	ppb	1.5	649,881	4000	99.1	
[Ca]	44	45	He	4151.250	ppb	0.2	81,611	4000	103.78	
Ti	47	45	NoGas	96.227	ppb	1.8	83,406	100	96.23	
V	51	74	He	94.136	ppb	0.1	254,961	100	94.14	
Cr	52	74	He	95.543	ppb	0.1	298,959	100	95.54	
Mn	55	74	He	100.360	ppb	0.3	225,627	100	100.36	
Fe	56	74	H2	4049.073	ppb	0.3	33,579,022	4000	101.23	
Co	59	74	He	99.223	ppb	0.3	424,346	100	99.22	
Ni	60	74	He	103.765	ppb	0.7	106,422	100	103.76	
Cu	65	74	He	102.819	ppb	0.6	130,623	100	102.82	
Zn	66	74	He	101.902	ppb	1.3	51,067	100	101.9	
As	75	74	He	97.046	ppb	0.9	30,801	100	97.05	
Se	78	74	H2	40.781	ppb	0.9	9,097	40	101.95	
Mo	95	103	He	39.832	ppb	1.4	52,521	40	99.58	
Ag	107	103	He	40.332	ppb	0.1	153,854	40	100.83	
Cd	111	103	He	97.416	ppb	0.7	62,781	100	97.42	
[Cd]	111	103	NoGas	94.626	ppb	0.3	160,944	100	94.63	
Sb	121	103	He	40.531	ppb	0.7	69,665	40	101.33	
Ba	138	159	He	102.761	ppb	0.6	405,363	100	102.76	
Hg	201	159	NoGas	823.977	ppt	2.6	710	800	103.	
Tl	205	159	He	40.166	ppb	0.6	274,096	40	100.42	
Pb	208	159	NoGas	97.761	ppb	1.0	1,957,120	100	97.76	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD/Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.5	732,265	943670.243333333	77.6	
Sc	45	H2	Analog	1.1	1,419,875	1761203.933333333	80.6	
Sc	45	He	Pulse	0.2	220,386	270213.02	81.6	
Sc	45	NoGas	Analog	1.3	2,176,471	2719052.54	80.0	
Ge	74	H2	Pulse	0.1	453,951	547887.95	82.9	
Ge	74	He	Pulse	0.5	135,539	161577.683333333	83.9	
Ge	74	NoGas	Pulse	0.4	579,844	710934.333333333	81.6	
Rh	103	He	Pulse	0.6	305,123	367685.51	83.0	
Rh	103	NoGas	Pulse	0.7	599,856	751394.163333333	79.8	
Tb	159	He	Pulse	0.6	472,313	522974.92	90.3	
Tb	159	NoGas	Pulse	0.9	1,105,507	1255414.6	88.1	
Bi	209	He	Pulse	0.1	277,734	308812.996666667	89.9	
Bi	209	NoGas	Pulse	0.4	653,906	737867.09	88.6	



### Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name:	9K26027-CCB3	Total Dilution:	1.0000
File Name:	059_CCB.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCB
Acq Time:	11/26/2019 15:54:57	I.S. Reference File:	003CALB.d
Comment:	CCB	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.009	ppb	51.4	44	
Na	23	45	He	2.496	ppb	11.9	4,540	
Mg	24	45	He	0.448	ppb	7.3	511	
Al	27	45	He	0.502	ppb	9.5	193	
K	39	45	He	2.938	ppb	15.9	20,904	
Ca	44	45	H2	0.865	ppb	61.3	492	
[Ca]	44	45	He	0.233	ppb	464.4	130	
Ti	47	45	NoGas	0.036	ppb	95.2	55	
V	51	74	He	-0.214	ppb	N/A	1,169	
Cr	52	74	He	0.002	ppb	167.3	199	
Mn	55	74	He	0.018	ppb	55.7	77	
Fe	56	74	H2	0.739	ppb	7.7	13,927	
Co	59	74	He	0.008	ppb	8.5	47	
Ni	60	74	He	-0.049	ppb	N/A	31	
Cu	65	74	He	0.018	ppb	92.1	53	
Zn	66	74	He	0.015	ppb	192.1	33	
As	75	74	He	-0.005	ppb	N/A	20	
Se	78	74	H2	0.024	ppb	73.5	8	
Mo	95	103	He	0.035	ppb	12.6	50	
Ag	107	103	He	0.004	ppb	49.5	18	
Cd	111	103	He	0.018	ppb	38.0	14	
[Cd]	111	103	NoGas	0.011	ppb	32.2	26	
Sb	121	103	He	0.273	ppb	17.9	516	
Ba	138	159	He	0.005	ppb	7.7	94	
Hg	201	159	NoGas	3.106	ppt	73.9	5	
Tl	205	159	He	0.002	ppb	203.6	40	
Pb	208	159	NoGas	0.023	ppb	22.6	983	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.4	754,323	943670.243333333	79.9	
Sc	45	H2	Analog	1.1	1,438,060	1761203.933333333	81.7	
Sc	45	He	Pulse	0.5	224,676	270213.02	83.1	
Sc	45	NoGas	Analog	0.9	2,231,690	2719052.54	82.1	
Ge	74	H2	Pulse	0.5	461,329	547887.95	84.2	
Ge	74	He	Pulse	0.4	138,546	161577.683333333	85.7	
Ge	74	NoGas	Pulse	0.6	600,031	710934.333333333	84.4	
Rh	103	He	Pulse	0.6	316,182	367685.51	86.0	
Rh	103	NoGas	Pulse	0.6	625,038	751394.163333333	83.2	
Tb	159	He	Pulse	0.7	477,462	522974.92	91.3	
Tb	159	NoGas	Pulse	0.7	1,125,615	1255414.6	89.7	
Bi	209	He	Pulse	1.2	285,001	308812.996666667	92.3	
Bi	209	NoGas	Pulse	0.9	671,366	737867.09	91.0	

### Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name:	9K26027-CCV4	Total Dilution:	1.0000
File Name:	070_CCV.d	Vial:	2
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCV
Acq Time:	11/26/2019 16:46:03	I.S. Reference File:	003CALB.d
Comment:	A19J138 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	40.735	ppb	0.8	79,290	40	101.84	
Na	23	45	He	4073.554	ppb	0.9	3,041,393	4000	101.84	
Mg	24	45	He	4283.045	ppb	1.2	1,792,261	4000	107.08	
Al	27	45	He	3967.923	ppb	0.9	903,300	4000	99.2	
K	39	45	He	4234.828	ppb	2.5	1,602,439	4000	105.87	
Ca	44	45	H2	3948.663	ppb	1.8	629,687	4000	98.72	
[Ca]	44	45	He	4154.529	ppb	0.8	77,862	4000	103.86	
Ti	47	45	NoGas	95.696	ppb	0.7	77,581	100	95.7	
V	51	74	He	94.035	ppb	0.2	241,577	100	94.04	
Cr	52	74	He	95.901	ppb	0.1	284,631	100	95.9	
Mn	55	74	He	100.625	ppb	0.6	214,578	100	100.63	
Fe	56	74	H2	4088.647	ppb	0.7	32,824,362	4000	102.22	
Co	59	74	He	99.348	ppb	0.4	403,005	100	99.35	
Ni	60	74	He	103.874	ppb	0.6	101,047	100	103.87	
Cu	65	74	He	102.890	ppb	1.1	123,981	100	102.89	
Zn	66	74	He	102.657	ppb	0.9	48,796	100	102.66	
As	75	74	He	96.554	ppb	0.5	29,068	100	96.55	
Se	78	74	H2	40.966	ppb	1.5	8,847	40	102.42	
Mo	95	103	He	39.921	ppb	0.3	50,249	40	99.8	
Ag	107	103	He	40.760	ppb	0.2	148,421	40	101.9	
Cd	111	103	He	99.552	ppb	0.5	61,245	100	99.55	
[Cd]	111	103	NoGas	97.213	ppb	1.3	154,988	100	97.21	
Sb	121	103	He	40.782	ppb	1.4	66,913	40	101.96	
Ba	138	159	He	101.491	ppb	0.9	389,002	100	101.49	
Hg	201	159	NoGas	829.740	ppt.	4.8	690	800	103.72	
Tl	205	159	He	40.790	ppb	1.1	270,454	40	101.98	
Pb	208	159	NoGas	99.009	ppb	0.3	1,913,295	100	99.01	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.3	691,820	943670.243333333	73.3	
Sc	45	H2	Analog	1.5	1,381,118	1761203.93333333	78.4	
Sc	45	He	Pulse	0.7	210,087	270213.02	77.7	
Sc	45	NoGas	Analog	0.8	2,035,381	2719052.54	74.9	
Ge	74	H2	Pulse	0.4	439,459	547887.95	80.2	
Ge	74	He	Pulse	0.4	128,561	161577.683333333	79.6	
Ge	74	NoGas	Pulse	0.9	543,172	710934.333333333	76.4	
Rh	103	He	Pulse	0.6	291,258	367685.51	79.2	
Rh	103	NoGas	Pulse	1.1	562,335	751394.163333333	74.8	
Tb	159	He	Pulse	0.9	458,935	522974.92	87.8	
Tb	159	NoGas	Pulse	0.7	1,067,090	1255414.6	85.0	
Bi	209	He	Pulse	0.2	271,754	308812.996666667	88.0	
Bi	209	NoGas	Pulse	0.6	631,309	737867.09	85.6	

### Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name:	9K26027-CCB4	Total Dilution:	1.0000
File Name:	071_CCB.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCB
Acq Time:	11/26/2019 16:50:42	I.S. Reference File:	003CALB.d
Comment:	CCB	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.004	ppb	46.3	30	
Na	23	45	He	7.462	ppb	6.4	7,815	
Mg	24	45	He	0.418	ppb	25.0	458	
Al	27	45	He	0.636	ppb	21.1	208	
K	39	45	He	2.050	ppb	41.1	18,891	
Ca	44	45	H2	1.381	ppb	6.5	532	
[Ca]	44	45	He	0.198	ppb	930.5	119	
Ti	47	45	NoGas	0.115	ppb	104.2	113	
V	51	74	He	-0.240	ppb	N/A	1,016	
Cr	52	74	He	0.000	ppb	N/A	177	
Mn	55	74	He	0.013	ppb	32.0	59	
Fe	56	74	H2	0.955	ppb	11.9	14,641	
Co	59	74	He	0.008	ppb	86.3	41	
Ni	60	74	He	-0.050	ppb	N/A	28	
Cu	65	74	He	0.002	ppb	684.7	31	
Zn	66	74	He	0.032	ppb	181.0	39	
As	75	74	He	0.006	ppb	316.0	22	
Se	78	74	H2	0.011	ppb	42.5	5	
Mo	95	103	He	0.039	ppb	38.9	51	
Ag	107	103	He	0.006	ppb	52.2	27	
Cd	111	103	He	0.024	ppb	23.7	16	
[Cd]	111	103	NoGas	0.008	ppb	148.1	18	
Sb	121	103	He	0.262	ppb	2.7	464	
Ba	138	159	He	0.008	ppb	14.2	102	
Hg	201	159	NoGas	3.663	ppt	9.1	5	
Tl	205	159	He	0.004	ppb	94.9	47	
Pb	208	159	NoGas	0.026	ppb	20.1	989	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.1	692,380	943670.243333333	73.4	
Sc	45	H2	Analog	2.4	1,326,274	1761203.933333333	75.3	
Sc	45	He	Pulse	0.3	206,558	270213.02	76.4	
Sc	45	NoGas	Analog	0.9	2,011,761	2719052.54	74.0	
Ge	74	H2	Pulse	0.3	428,915	547887.95	78.3	
Ge	74	He	Pulse	0.7	128,255	161577.683333333	79.4	
Ge	74	NoGas	Pulse	0.5	540,754	710934.333333333	76.1	
Rh	103	He	Pulse	0.2	295,945	367685.51	80.5	
Rh	103	NoGas	Pulse	0.5	570,836	751394.163333333	76.0	
Tb	159	He	Pulse	1.3	458,471	522974.92	87.7	
Tb	159	NoGas	Pulse	0.2	1,062,294	1255414.6	84.6	
Bi	209	He	Pulse	1.0	276,234	308812.996666667	89.5	
Bi	209	NoGas	Pulse	0.2	640,953	737867.09	86.9	

### Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name:	9K26027-CCV5	Total Dilution:	1.0000
File Name:	082_CCV.d	Vial:	2
File Path:	C:\Agilent\ICPMH1\DATA\9K26027.b	Sample Type:	CCV
Acq Time:	11/26/2019 17:44:37	I.S. Reference File:	003CALB.d
Comment:	A19J138 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	40.427	ppb	0.5	76,814	40	101.07	
Na	23	45	He	4023.080	ppb	0.7	2,905,786	4000	100.58	
Mg	24	45	He	4285.355	ppb	1.3	1,734,729	4000	107.13	
Al	27	45	He	3972.527	ppb	0.6	874,844	4000	99.31	
K	39	45	He	4276.866	ppb	1.2	1,565,455	4000	106.92	
Ca	44	45	H2	3975.783	ppb	0.4	596,598	4000	99.39	
[Ca]	44	45	He	4159.081	ppb	1.2	75,400	4000	103.98	
Ti	47	45	NoGas	96.625	ppb	0.9	77,033	100	96.62	
V	51	74	He	93.223	ppb	0.4	235,858	100	93.22	
Cr	52	74	He	94.319	ppb	0.5	275,672	100	94.32	
Mn	55	74	He	100.111	ppb	0.6	210,229	100	100.11	
Fe	56	74	H2	4058.566	ppb	0.2	31,247,834	4000	101.46	
Co	59	74	He	98.613	ppb	0.7	393,941	100	98.61	
Ni	60	74	He	102.651	ppb	0.5	98,340	100	102.65	
Cu	65	74	He	101.593	ppb	1.1	120,551	100	101.59	
Zn	66	74	He	102.545	ppb	0.8	48,000	100	102.54	
As	75	74	He	96.821	ppb	1.1	28,704	100	96.82	
Se	78	74	H2	40.568	ppb	1.5	8,402	40	101.42	
Mo	95	103	He	39.680	ppb	1.4	49,153	40	99.2	
Ag	107	103	He	40.878	ppb	0.7	146,492	40	102.2	
Cd	111	103	He	99.608	ppb	0.6	60,305	100	99.61	
[Cd]	111	103	NoGas	96.568	ppb	1.2	151,580	100	96.57	
Sb	121	103	He	40.899	ppb	1.8	66,040	40	102.25	
Ba	138	159	He	101.871	ppb	0.2	386,588	100	101.87	
Hg	201	159	NoGas	849.491	ppt.	1.9	700	800	106.19	
Tl	205	159	He	40.738	ppb	0.5	267,435	40	101.85	
Pb	208	159	NoGas	99.308	ppb	0.4	1,902,131	100	99.31	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.3	675,299	943670.243333333	71.6	
Sc	45	H2	Analog	0.3	1,299,401	1761203.933333333	73.8	
Sc	45	He	Pulse	0.2	203,226	270213.02	75.2	
Sc	45	NoGas	Analog	1.3	2,001,510	2719052.54	73.6	
Ge	74	H2	Pulse	0.2	421,448	547887.95	76.9	
Ge	74	He	Pulse	0.4	126,602	161577.683333333	78.4	
Ge	74	NoGas	Pulse	0.8	535,283	710934.333333333	75.3	
Rh	103	He	Pulse	0.5	286,635	367685.51	78.0	
Rh	103	NoGas	Pulse	0.1	553,587	751394.163333333	73.7	
Tb	159	He	Pulse	0.6	454,363	522974.92	86.9	
Tb	159	NoGas	Pulse	0.6	1,057,675	1255414.6	84.2	
Bi	209	He	Pulse	0.1	272,491	308812.996666667	88.2	
Bi	209	NoGas	Pulse	0.7	628,439	737867.09	85.2	

## Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name: **9K26027-CCB5**  
 File Name: **083\_CCB.d**  
 File Path: **C:\Agilent\ICPMH\1\DATA\9K26027.b**  
 Acq Time: **11/26/2019 17:49:17**  
 Comment: **CCB**

Total Dilution: **1.0000**  
 Vial: **1**  
 Sample Type: **CCB**  
 I.S. Reference File: **003CALB.d**  
 Last Calibration: **11/26/2019 11:53:02**

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.002	ppb	79.5	27	
Na	23	45	He	4.774	ppb	3.3	5,760	
Mg	24	45	He	0.344	ppb	7.7	421	
Al	27	45	He	0.638	ppb	13.9	206	
K	39	45	He	1.990	ppb	60.1	18,598	
Ca	44	45	H2	1.225	ppb	16.6	506	
[Ca]	44	45	He	-1.488	ppb	N/A	87	
Ti	47	45	NoGas	0.024	ppb	128.8	40	
V	51	74	He	-0.192	ppb	N/A	1,129	
Cr	52	74	He	0.005	ppb	347.3	192	
Mn	55	74	He	0.011	ppb	80.0	56	
Fe	56	74	H2	0.985	ppb	8.3	14,828	
Co	59	74	He	0.006	ppb	12.5	33	
Ni	60	74	He	-0.037	ppb	N/A	40	
Cu	65	74	He	0.026	ppb	118.7	59	
Zn	66	74	He	0.049	ppb	39.5	47	
As	75	74	He	0.010	ppb	230.0	23	
Se	78	74	H2	0.016	ppb	106.1	6	
Mo	95	103	He	0.037	ppb	22.3	49	
Ag	107	103	He	0.004	ppb	14.1	18	
Cd	111	103	He	0.018	ppb	69.9	13	
[Cd]	111	103	NoGas	0.008	ppb	187.1	19	
Sb	121	103	He	0.280	ppb	8.5	492	
Ba	138	159	He	0.010	ppb	135.7	108	
Hg	201	159	NoGas	2.657	ppt	127.7	5	
Tl	205	159	He	0.005	ppb	15.6	59	
Pb	208	159	NoGas	0.066	ppb	2.5	1,760	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.3	679,966	943670.243333333	72.1	
Sc	45	H2	Analog	0.5	1,318,194	1761203.93333333	74.8	
Sc	45	He	Pulse	1.4	203,628	270213.02	75.4	
Sc	45	NoGas	Analog	0.5	1,989,828	2719052.54	73.2	
Ge	74	H2	Pulse	0.2	427,407	547887.95	78.0	
Ge	74	He	Pulse	0.9	127,153	161577.683333333	78.7	
Ge	74	NoGas	Pulse	0.5	539,967	710934.333333333	76.0	
Rh	103	He	Pulse	0.6	294,271	367685.51	80.0	
Rh	103	NoGas	Pulse	0.5	570,518	751394.163333333	75.9	
Tb	159	He	Pulse	0.8	457,971	522974.92	87.6	
Tb	159	NoGas	Pulse	0.6	1,062,864	1255414.6	84.7	
Bi	209	He	Pulse	0.1	276,503	308812.996666667	89.5	
Bi	209	NoGas	Pulse	0.2	642,200	737867.09	87.0	

### CRL Verification Report - ICPMS5

Sample Name: <b>9K26027-CRL7</b>	Total Dilution: <b>1.0000</b>
File Name: 084CRL.d	Vial: 1102
File Path: C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type: CRL1
Acq Time: 11/26/2019 17:54:00	I.S. Reference File: 003CALB.d
Comment: <b>A19K144 - ESS 11/26</b>	Last Calibration: 11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	0.195	ppb	14.5	393	108.33	
Na	23	45	He	12.998	ppb	2.7	11,668	144.42	R-11
Mg	24	45	He	9.234	ppb	7.0	4,013	102.6	
Al	27	45	He	9.011	ppb	2.1	2,046	100.12	
K	39	45	He	11.574	ppb	4.2	22,003	128.6	
Ca	44	45	H2	9.015	ppb	15.7	1,693	100.17	
[Ca]	44	45	He	8.747	ppb	32.8	271	97.19	
Ti	47	45	NoGas	0.175	ppb	35.1	158	97.22	
V	51	74	He	-0.033	ppb	N/A	1,529	-18.33	R-11
Cr	52	74	He	0.142	ppb	10.0	593	78.89	
Mn	55	74	He	0.201	ppb	0.9	456	111.67	
Fe	56	74	H2	8.619	ppb	0.4	74,155	95.77	
Co	59	74	He	0.192	ppb	10.3	780	106.67	
Ni	60	74	He	0.123	ppb	21.8	193	68.33	R-11
Cu	65	74	He	0.187	ppb	13.6	251	103.89	
Zn	66	74	He	0.153	ppb	29.0	96	85	
As	75	74	He	0.164	ppb	28.2	69	91.11	
Se	78	74	H2	0.192	ppb	17.8	43	106.67	
Mo	95	103	He	0.177	ppb	26.6	226	98.33	
Ag	107	103	He	0.182	ppb	13.0	669	101.11	
Cd	111	103	He	0.194	ppb	8.8	122	107.78	
[Cd]	111	103	NoGas	0.197	ppb	7.7	323	109.44	
Sb	121	103	He	0.253	ppb	9.5	446	140.56	R-11
Ba	138	159	He	0.180	ppb	4.3	757	100	
Hg	201	159	NoGas	8.736	ppt.	36.2	10	121.33	
Tl	205	159	He	0.175	ppb	9.6	1,181	97.22	
Pb	208	159	NoGas	0.228	ppb	2.0	4,864	126.67	

*L MRL*

*L MRL*

*L MRL*

*L MRL*

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.4	677,775	943670.243333333	71.8	
Sc	45	H2	Analog	1.0	1,321,350	1761203.933333333	75.0	
Sc	45	He	Pulse	0.7	202,954	270213.02	75.1	
Sc	45	NoGas	Analog	0.2	1,978,251	2719052.54	72.8	
Ge	74	H2	Pulse	0.4	425,905	547887.95	77.7	
Ge	74	He	Pulse	0.6	127,042	161577.683333333	78.6	
Ge	74	NoGas	Pulse	1.1	534,672	710934.333333333	75.2	
Rh	103	He	Pulse	0.4	292,371	367685.51	79.5	
Rh	103	NoGas	Pulse	0.6	566,062	751394.163333333	75.3	
Tb	159	He	Pulse	0.6	457,702	522974.92	87.5	
Tb	159	NoGas	Pulse	0.6	1,059,517	1255414.6	84.4	
Bi	209	He	Pulse	0.6	276,341	308812.996666667	89.5	
Bi	209	NoGas	Pulse	0.4	636,769	737867.09	86.3	

### CRL Verification Report - ICPMS5

Sample Name:	9K26027-CRL8	Total Dilution:	1.0000
File Name:	085_CRL.d	Vial:	1103
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL2
Acq Time:	11/26/2019 17:58:41	I.S. Reference File:	003CALB.d
Comment:	A19K145 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	0.901	ppb	3.3	1,745	100.11	
Na	23	45	He	49.389	ppb	2.2	38,019	109.75	
Mg	24	45	He	46.604	ppb	0.5	19,179	103.56	
Al	27	45	He	46.831	ppb	3.0	10,394	104.07	
K	39	45	He	49.173	ppb	2.8	35,705	109.27	
Ca	44	45	H2	45.107	ppb	1.2	7,246	100.24	
[Ca]	44	45	He	45.847	ppb	9.1	946	101.88	
Ti	47	45	NoGas	0.988	ppb	11.1	790	109.78	
V	51	74	He	0.673	ppb	1.7	3,307	74.78	
Cr	52	74	He	0.846	ppb	2.5	2,656	94	
Mn	55	74	He	0.898	ppb	7.3	1,922	99.78	
Fe	56	74	H2	44.377	ppb	0.4	351,079	98.62	
Co	59	74	He	0.906	ppb	3.2	3,640	100.67	
Ni	60	74	He	0.872	ppb	13.0	912	96.89	
Cu	65	74	He	0.942	ppb	9.2	1,149	104.67	
Zn	66	74	He	0.951	ppb	3.8	470	105.67	
As	75	74	He	0.877	ppb	9.0	280	97.44	
Se	78	74	H2	0.965	ppb	6.5	204	107.22	
Mo	95	103	He	0.869	ppb	10.7	1,102	96.56	
Ag	107	103	He	0.895	ppb	1.6	3,283	99.44	
Cd	111	103	He	0.908	ppb	3.8	563	100.89	
[Cd]	111	103	NoGas	0.879	ppb	6.6	1,410	97.67	
Sb	121	103	He	0.946	ppb	5.6	1,589	105.11	
Ba	138	159	He	0.901	ppb	4.2	3,507	100.11	
Hg	201	159	NoGas	39.650	ppt	17.5	35	110.14	
Tl	205	159	He	0.909	ppb	0.9	6,022	101	
Pb	208	159	NoGas	0.962	ppb	0.9	18,869	106.89	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.3	679,334	943670.243333333	72.0	
Sc	45	H2	Analog	2.4	1,330,169	1761203.933333333	75.5	
Sc	45	He	Pulse	1.2	203,614	270213.02	75.4	
Sc	45	NoGas	Analog	1.0	1,956,329	2719052.54	71.9	
Ge	74	H2	Pulse	0.2	424,411	547887.95	77.5	
Ge	74	He	Pulse	0.7	126,990	161577.683333333	78.6	
Ge	74	NoGas	Pulse	0.9	536,379	710934.333333333	75.4	
Rh	103	He	Pulse	0.6	292,926	367685.51	79.7	
Rh	103	NoGas	Pulse	0.4	563,575	751394.163333333	75.0	
Tb	159	He	Pulse	0.5	456,808	522974.92	87.3	
Tb	159	NoGas	Pulse	0.8	1,055,917	1255414.6	84.1	
Bi	209	He	Pulse	0.4	275,706	308812.996666667	89.3	
Bi	209	NoGas	Pulse	1.0	638,667	737867.09	86.6	

### CRL Verification Report - ICPMS5

Sample Name:	9K26027-CRL9	Total Dilution:	1.0000
File Name:	086CRL_d	Vial:	1104
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL3
Acq Time:	11/26/2019 18:03:22	I.S. Reference File:	003CALB.d
Comment:	A19K146 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	1.784	ppb	1.1	3,433	99.11	
Na	23	45	He	95.083	ppb	1.1	71,099	105.65	
Mg	24	45	He	91.617	ppb	0.6	37,453	101.8	
Al	27	45	He	94.354	ppb	0.7	20,895	104.84	
K	39	45	He	94.994	ppb	2.1	52,344	105.55	
Ca	44	45	H2	89.036	ppb	1.1	13,909	98.93	
[Ca]	44	45	He	101.253	ppb	5.1	1,951	112.5	
Ti	47	45	NoGas	1.785	ppb	11.6	1,433	99.17	
V	51	74	He	1.513	ppb	2.4	5,413	84.06	
Cr	52	74	He	1.728	ppb	3.0	5,226	96	
Mn	55	74	He	1.816	ppb	4.5	3,847	100.89	
Fe	56	74	H2	88.675	ppb	0.1	695,229	98.53	
Co	59	74	He	1.773	ppb	3.2	7,097	98.5	
Ni	60	74	He	1.803	ppb	5.9	1,802	100.17	
Cu	65	74	He	1.951	ppb	3.6	2,345	108.39	
Zn	66	74	He	1.886	ppb	7.7	907	104.78	
As	75	74	He	1.805	ppb	3.2	555	100.28	
Se	78	74	H2	1.810	ppb	5.1	380	100.56	
Mo	95	103	He	1.696	ppb	5.7	2,136	94.22	
Ag	107	103	He	1.804	ppb	2.9	6,568	100.22	
Cd	111	103	He	1.782	ppb	4.6	1,097	99	
[Cd]	111	103	NoGas	1.821	ppb	6.9	2,916	101.17	
Sb	121	103	He	1.880	ppb	0.8	3,109	104.44	
Ba	138	159	He	1.846	ppb	3.9	7,103	102.56	
Hg	201	159	NoGas	76.975	ppt	12.2	66	106.91	
Tl	205	159	He	1.839	ppb	1.2	12,143	102.17	
Pb	208	159	NoGas	1.872	ppb	0.9	36,334	104	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.2	679,441	943670.243333333	72.0	
Sc	45	H2	Analog	1.0	1,322,235	1761203.933333333	75.1	
Sc	45	He	Pulse	0.9	203,733	270213.02	75.4	
Sc	45	NoGas	Analog	1.0	1,988,010	2719052.54	73.1	
Ge	74	H2	Pulse	0.5	424,881	547887.95	77.5	
Ge	74	He	Pulse	0.5	126,718	161577.683333333	78.4	
Ge	74	NoGas	Pulse	0.7	535,603	710934.333333333	75.3	
Rh	103	He	Pulse	0.8	291,077	367685.51	79.2	
Rh	103	NoGas	Pulse	0.4	563,674	751394.163333333	75.0	
Tb	159	He	Pulse	0.4	456,207	522974.92	87.2	
Tb	159	NoGas	Pulse	0.8	1,057,689	1255414.6	84.3	
Bi	209	He	Pulse	0.9	276,799	308812.996666667	89.6	
Bi	209	NoGas	Pulse	0.4	640,842	737867.09	86.9	



### CRL Verification Report - ICPMS5

Sample Name:	9K26027-CRLA	Total Dilution:	1.0000
File Name:	087CRL4.d	Vial:	1105
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL4
Acq Time:	11/26/2019 18:08:03	I.S. Reference File:	003CALB.d
Comment:	A19K147 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	3.582	ppb	3.6	6,898	99.5	
Na	23	45	He	186.732	ppb	0.4	137,630	103.74	
Mg	24	45	He	185.627	ppb	0.3	75,720	103.13	
Al	27	45	He	181.925	ppb	0.9	40,290	101.07	
K	39	45	He	191.288	ppb	1.9	87,416	106.27	
Ca	44	45	H2	183.327	ppb	1.6	28,026	101.85	
[Ca]	44	45	He	186.164	ppb	2.0	3,498	103.42	
Ti	47	45	NoGas	3.610	ppb	9.4	2,861	100.28	
V	51	74	He	3.185	ppb	1.8	9,645	88.47	
Cr	52	74	He	3.451	ppb	2.9	10,293	95.86	
Mn	55	74	He	3.706	ppb	1.1	7,842	102.94	
Fe	56	74	H2	185.056	ppb	1.9	1,440,174	102.81	
Co	59	74	He	3.477	ppb	0.7	13,950	96.58	
Ni	60	74	He	3.709	ppb	1.5	3,638	103.03	
Cu	65	74	He	3.766	ppb	4.6	4,513	104.61	
Zn	66	74	He	3.856	ppb	6.6	1,835	107.11	
As	75	74	He	3.616	ppb	3.3	1,095	100.44	
Se	78	74	H2	3.573	ppb	2.1	747	99.25	
Mo	95	103	He	3.462	ppb	3.6	4,396	96.17	
Ag	107	103	He	3.613	ppb	1.1	13,271	100.36	
Cd	111	103	He	3.759	ppb	0.6	2,334	104.42	
[Cd]	111	103	NoGas	3.673	ppb	2.5	5,905	102.03	
Sb	121	103	He	3.560	ppb	0.8	5,917	98.89	
Ba	138	159	He	3.740	ppb	0.1	14,356	103.89	
Hg	201	159	NoGas	149.299	ppt	2.8	126	103.68	
Tl	205	159	He	3.679	ppb	0.1	24,334	102.19	
Pb	208	159	NoGas	3.699	ppb	1.9	71,695	102.75	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.3	682,395	943670.243333333	72.3	
Sc	45	H2	Analog	2.0	1,309,701	1761203.933333333	74.4	
Sc	45	He	Pulse	0.6	204,061	270213.02	75.5	
Sc	45	NoGas	Analog	0.4	1,975,448	2719052.54	72.7	
Ge	74	H2	Pulse	0.3	424,015	547887.95	77.4	
Ge	74	He	Pulse	0.4	127,069	161577.683333333	78.6	
Ge	74	NoGas	Pulse	0.6	539,629	710934.333333333	75.9	
Rh	103	He	Pulse	0.5	293,725	367685.51	79.9	
Rh	103	NoGas	Pulse	0.4	566,558	751394.163333333	75.4	
Tb	159	He	Pulse	0.3	457,396	522974.92	87.5	
Tb	159	NoGas	Pulse	0.7	1,063,484	1255414.6	84.7	
Bi	209	He	Pulse	0.8	276,756	308812.996666667	89.6	
Bi	209	NoGas	Pulse	0.4	643,958	737867.09	87.3	

## Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name:	9K26027-CCV6	Total Dilution:	1.0000
File Name:	098_CCV.d	Vial:	2
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCV
Acq Time:	11/26/2019 18:59:36	I.S. Reference File:	003CALB.d
Comment:	A19J138 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	39.491	ppb	0.2	78,850	40	98.73	
Na	23	45	He	4022.401	ppb	1.1	3,016,479	4000	100.56	
Mg	24	45	He	4284.488	ppb	1.6	1,800,785	4000	107.11	
Al	27	45	He	3974.108	ppb	0.2	908,706	4000	99.35	
K	39	45	He	4335.955	ppb	1.7	1,647,703	4000	108.4	
Ca	44	45	H2	3977.680	ppb	1.4	631,244	4000	99.44	
[Ca]	44	45	He	4153.217	ppb	0.9	78,174	4000	103.83	
Ti	47	45	NoGas	96.325	ppb	0.3	80,014	100	96.32	
V	51	74	He	93.717	ppb	0.6	244,232	100	93.72	
Cr	52	74	He	94.830	ppb	0.3	285,511	100	94.83	
Mn	55	74	He	100.610	ppb	0.5	217,632	100	100.61	
Fe	56	74	H2	4089.844	ppb	0.3	32,924,230	4000	102.25	
Co	59	74	He	99.620	ppb	0.1	409,936	100	99.62	
Ni	60	74	He	104.184	ppb	0.3	102,810	100	104.18	
Cu	65	74	He	102.911	ppb	0.4	125,792	100	102.91	
Zn	66	74	He	100.324	ppb	1.0	48,375	100	100.32	
As	75	74	He	97.080	ppb	0.5	29,647	100	97.08	
Se	78	74	H2	41.186	ppb	3.9	8,918	40	102.96	
Mo	95	103	He	39.935	ppb	0.7	50,901	40	99.84	
Ag	107	103	He	40.718	ppb	0.9	150,140	40	101.8	
Cd	111	103	He	99.316	ppb	0.3	61,872	100	99.32	
[Cd]	111	103	NoGas	95.230	ppb	0.6	155,368	100	95.23	
Sb	121	103	He	40.529	ppb	1.6	67,338	40	101.32	
Ba	138	159	He	101.636	ppb	0.6	393,362	100	101.64	
Hg	201	159	NoGas	821.888	ppt	1.1	692	800	102.74	
Tl	205	159	He	40.207	ppb	0.6	269,198	40	100.52	
Pb	208	159	NoGas	98.041	ppb	0.6	1,918,027	100	98.04	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.2	709,623	943670.243333333	75.2	
Sc	45	H2	Analog	1.2	1,374,346	1761203.933333333	78.0	
Sc	45	He	Pulse	0.6	211,011	270213.02	78.1	
Sc	45	NoGas	Analog	0.4	2,085,508	2719052.54	76.7	
Ge	74	H2	Pulse	0.7	440,670	547887.95	80.4	
Ge	74	He	Pulse	0.6	130,414	161577.683333333	80.7	
Ge	74	NoGas	Pulse	0.5	558,445	710934.333333333	78.6	
Rh	103	He	Pulse	0.4	294,939	367685.51	80.2	
Rh	103	NoGas	Pulse	0.6	575,388	751394.163333333	76.6	
Tb	159	He	Pulse	0.5	463,399	522974.92	88.6	
Tb	159	NoGas	Pulse	0.7	1,080,304	1255414.6	86.1	
Bi	209	He	Pulse	0.6	274,582	308812.996666667	88.9	
Bi	209	NoGas	Pulse	0.4	643,234	737867.09	87.2	

### Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name:	9K26027-CCB6	Total Dilution:	1.0000
File Name:	099_CCB.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCB
Acq Time:	11/26/2019 19:04:16	I.S. Reference File:	003CALB.d
Comment:	CCB	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.010	ppb	62.3	43	
Na	23	45	He	2.388	ppb	1.6	4,249	
Mg	24	45	He	0.440	ppb	10.3	484	
Al	27	45	He	0.632	ppb	33.0	214	
K	39	45	He	3.482	ppb	14.2	20,155	
Ca	44	45	H2	1.009	ppb	42.5	497	
[Ca]	44	45	He	-1.025	ppb	N/A	100	
Ti	47	45	NoGas	0.011	ppb	253.8	32	
V	51	74	He	-0.206	ppb	N/A	1,143	
Cr	52	74	He	-0.001	ppb	N/A	180	
Mn	55	74	He	0.018	ppb	33.7	72	
Fe	56	74	H2	0.984	ppb	6.2	15,428	
Co	59	74	He	0.007	ppb	40.6	39	
Ni	60	74	He	-0.034	ppb	N/A	44	
Cu	65	74	He	0.034	ppb	31.3	71	
Zn	66	74	He	0.050	ppb	79.1	49	
As	75	74	He	0.001	ppb	2914.7	21	
Se	78	74	H2	0.024	ppb	49.7	8	
Mo	95	103	He	0.046	ppb	15.9	62	
Ag	107	103	He	0.009	ppb	14.2	38	
Cd	111	103	He	0.021	ppb	23.6	15	
[Cd]	111	103	NoGas	0.021	ppb	52.5	42	
Sb	121	103	He	0.259	ppb	12.6	471	
Ba	138	159	He	0.007	ppb	62.2	97	
Hg	201	159	NoGas	4.451	ppt	62.3	6	
Tl	205	159	He	0.005	ppb	65.4	59	
Pb	208	159	NoGas	0.039	ppb	19.7	1,281	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.4	723,219	943670.243333333	76.6	
Sc	45	H2	Analog	0.6	1,384,698	1761203.933333333	78.6	
Sc	45	He	Pulse	0.8	214,407	270213.02	79.3	
Sc	45	NoGas	Analog	1.3	2,112,270	2719052.54	77.7	
Ge	74	H2	Pulse	0.3	445,124	547887.95	81.2	
Ge	74	He	Pulse	1.2	132,798	161577.683333333	82.2	
Ge	74	NoGas	Pulse	0.4	566,754	710934.333333333	79.7	
Rh	103	He	Pulse	1.0	303,680	367685.51	82.6	
Rh	103	NoGas	Pulse	0.8	597,117	751394.163333333	79.5	
Tb	159	He	Pulse	1.5	464,294	522974.92	88.8	
Tb	159	NoGas	Pulse	0.4	1,094,332	1255414.6	87.2	
Bi	209	He	Pulse	1.6	278,455	308812.996666667	90.2	
Bi	209	NoGas	Pulse	0.9	656,046	737867.09	88.9	

## Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name: <b>9K26027-CCV7</b>	Total Dilution: <b>1.0000</b>
File Name: 110_CCV.d	Vial: 2
File Path: C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type: CCV
Acq Time: 11/26/2019 19:55:40	I.S. Reference File: 003CALB.d
Comment: <b>A19J138 - ESS 11/26</b>	Last Calibration: 11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	40.492	ppb	0.4	77,089	40	101.23	
Na	23	45	He	4048.160	ppb	0.8	2,910,516	4000	101.2	
Mg	24	45	He	4339.331	ppb	0.5	1,748,542	4000	108.48	
Al	27	45	He	3970.831	ppb	0.9	870,468	4000	99.27	
K	39	45	He	4330.455	ppb	1.0	1,577,719	4000	108.26	
Ca	44	45	H2	3970.860	ppb	1.4	607,294	4000	99.27	
[Ca]	44	45	He	4140.293	ppb	0.6	74,716	4000	103.51	
Ti	47	45	NoGas	95.609	ppb	0.7	75,726	100	95.61	
V	51	74	He	93.207	ppb	0.4	233,534	100	93.21	
Cr	52	74	He	95.552	ppb	0.3	276,572	100	95.55	
Mn	55	74	He	101.392	ppb	0.3	210,856	100	101.39	
Fe	56	74	H2	4094.657	ppb	0.4	31,668,017	4000	102.37	
Co	59	74	He	99.348	ppb	0.6	393,023	100	99.35	
Ni	60	74	He	102.964	ppb	0.7	97,682	100	102.96	
Cu	65	74	He	102.497	ppb	1.0	120,450	100	102.5	
Zn	66	74	He	102.486	ppb	1.7	47,508	100	102.49	
As	75	74	He	96.900	ppb	0.6	28,449	100	96.9	
Se	78	74	H2	41.066	ppb	0.5	8,543	40	102.66	
Mo	95	103	He	39.389	ppb	0.3	48,489	40	98.47	
Ag	107	103	He	40.772	ppb	0.6	145,198	40	101.93	
Cd	111	103	He	99.269	ppb	0.5	59,727	100	99.27	
[Cd]	111	103	NoGas	96.725	ppb	0.5	150,805	100	96.72	
Sb	121	103	He	41.033	ppb	0.6	65,842	40	102.58	
Ba	138	159	He	100.778	ppb	0.4	382,472	100	100.78	
Hg	201	159	NoGas	828.646	ppt	3.5	680	800	103.58	
Tl	205	159	He	40.790	ppb	0.6	267,799	40	101.98	
Pb	208	159	NoGas	99.311	ppb	0.6	1,893,053	100	99.31	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.1	676,630	943670.243333333	71.7	
Sc	45	H2	Analog	1.5	1,324,497	1761203.933333333	75.2	
Sc	45	He	Pulse	0.8	202,305	270213.02	74.9	
Sc	45	NoGas	Analog	0.4	1,988,505	2719052.54	73.1	
Ge	74	H2	Pulse	0.4	423,351	547887.95	77.3	
Ge	74	He	Pulse	0.5	125,378	161577.683333333	77.6	
Ge	74	NoGas	Pulse	0.6	531,170	710934.333333333	74.7	
Rh	103	He	Pulse	0.8	284,858	367685.51	77.5	
Rh	103	NoGas	Pulse	0.1	549,864	751394.163333333	73.2	
Tb	159	He	Pulse	0.4	454,399	522974.92	86.9	
Tb	159	NoGas	Pulse	0.4	1,052,592	1255414.6	83.8	
Bi	209	He	Pulse	0.8	269,953	308812.996666667	87.4	
Bi	209	NoGas	Pulse	0.3	628,579	737867.09	85.2	

### Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name:	9K26027-CCB7	Total Dilution:	1.0000
File Name:	111_CCB.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCB
Acq Time:	11/26/2019 20:00:21	I.S. Reference File:	003CALB.d
Comment:	CCB	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.015	ppb	100.9	51	
Na	23	45	He	2.453	ppb	7.9	4,053	
Mg	24	45	He	0.391	ppb	34.8	437	
Al	27	45	He	0.565	ppb	32.1	188	
K	39	45	He	2.738	ppb	16.8	18,732	
Ca	44	45	H2	1.557	ppb	19.3	562	
[Ca]	44	45	He	0.581	ppb	297.9	123	
Ti	47	45	NoGas	0.031	ppb	60.9	45	
V	51	74	He	-0.185	ppb	N/A	1,132	
Cr	52	74	He	-0.005	ppb	N/A	161	
Mn	55	74	He	0.068	ppb	9.6	173	
Fe	56	74	H2	0.939	ppb	10.8	14,305	
Co	59	74	He	0.010	ppb	54.5	48	
Ni	60	74	He	-0.042	ppb	N/A	34	
Cu	65	74	He	0.024	ppb	31.9	56	
Zn	66	74	He	0.033	ppb	177.0	39	
As	75	74	He	0.034	ppb	102.6	30	
Se	78	74	H2	0.039	ppb	49.3	11	
Mo	95	103	He	0.031	ppb	13.4	41	
Ag	107	103	He	0.004	ppb	66.7	17	
Cd	111	103	He	0.026	ppb	21.4	17	
[Cd]	111	103	NoGas	0.021	ppb	34.5	39	
Sb	121	103	He	0.239	ppb	4.8	420	
Ba	138	159	He	0.009	ppb	75.9	103	
Hg	201	159	NoGas	5.777	ppt	37.6	7	
Tl	205	159	He	0.002	ppb	44.0	39	
Pb	208	159	NoGas	0.036	ppb	0.8	1,161	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.7	678,537	943670.243333333	71.9	
Sc	45	H2	Analog	1.5	1,333,157	1761203.93333333	75.7	
Sc	45	He	Pulse	0.7	202,105	270213.02	74.8	
Sc	45	NoGas	Analog	0.3	1,977,152	2719052.54	72.7	
Ge	74	H2	Pulse	0.5	422,630	547887.95	77.1	
Ge	74	He	Pulse	1.0	125,490	161577.683333333	77.7	
Ge	74	NoGas	Pulse	0.4	529,155	710934.333333333	74.4	
Rh	103	He	Pulse	1.1	290,965	367685.51	79.1	
Rh	103	NoGas	Pulse	0.6	558,156	751394.163333333	74.3	
Tb	159	He	Pulse	0.6	454,463	522974.92	86.9	
Tb	159	NoGas	Pulse	0.6	1,049,749	1255414.6	83.6	
Bi	209	He	Pulse	1.2	275,094	308812.996666667	89.1	
Bi	209	NoGas	Pulse	0.6	634,133	737867.09	85.9	

### Continuing Calibration Verification (CCV) Report - ICPMS5

Sample Name: <b>9K26027-CCV8</b>	Total Dilution: <b>1.0000</b>
File Name: 120_CCV.d	Vial: 2
File Path: C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type: CCV
Acq Time: 11/26/2019 20:42:25	I.S. Reference File: 003CALB.d
Comment: <b>A19J138 - ESS 11/26</b>	Last Calibration: 11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	Conc. RSD	CPS	ExpValue	% Rec	Flag
Be	9	6	NoGas	40.157	ppb	0.7	77,262	40	100.39	
Na	23	45	He	4064.668	ppb	1.6	2,959,270	4000	101.62	
Mg	24	45	He	4335.213	ppb	0.9	1,768,955	4000	108.38	
Al	27	45	He	4009.909	ppb	0.6	890,159	4000	100.25	
K	39	45	He	4297.115	ppb	2.2	1,585,339	4000	107.43	
Ca	44	45	H2	3932.782	ppb	0.8	615,326	4000	98.32	
[Ca]	44	45	He	4160.071	ppb	0.7	76,022	4000	104	
Ti	47	45	NoGas	96.257	ppb	2.6	76,653	100	96.26	
V	51	74	He	93.754	ppb	0.8	236,499	100	93.75	
Cr	52	74	He	95.248	ppb	0.4	277,585	100	95.25	
Mn	55	74	He	101.210	ppb	0.3	211,920	100	101.21	
Fe	56	74	H2	4143.426	ppb	0.3	32,457,995	4000	103.59	
Co	59	74	He	98.860	ppb	1.1	393,769	100	98.86	
Ni	60	74	He	103.078	ppb	0.2	98,463	100	103.08	
Cu	65	74	He	101.809	ppb	0.3	120,462	100	101.81	
Zn	66	74	He	101.466	ppb	0.8	47,361	100	101.47	
As	75	74	He	96.615	ppb	1.3	28,559	100	96.62	
Se	78	74	H2	40.963	ppb	1.6	8,631	40	102.41	
Mo	95	103	He	40.016	ppb	1.1	49,235	40	100.04	
Ag	107	103	He	41.075	ppb	0.8	146,205	40	102.69	
Cd	111	103	He	99.521	ppb	0.3	59,849	100	99.52	
[Cd]	111	103	NoGas	97.643	ppb	0.4	152,692	100	97.64	
Sb	121	103	He	41.355	ppb	0.3	66,326	40	103.39	
Ba	138	159	He	101.058	ppb	0.6	384,274	100	101.06	
Hg	201	159	NoGas	812.905	ppt	0.1	675	800	101.61	
Tl	205	159	He	40.926	ppb	0.8	269,208	40	102.32	
Pb	208	159	NoGas	99.649	ppb	0.0	1,921,518	100	99.65	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.2	683,806	943670.243333333	72.5	
Sc	45	H2	Analog	0.8	1,354,866	1761203.933333333	76.9	
Sc	45	He	Pulse	0.5	204,862	270213.02	75.8	
Sc	45	NoGas	Analog	1.6	1,999,637	2719052.54	73.5	
Ge	74	H2	Pulse	0.3	428,806	547887.95	78.3	
Ge	74	He	Pulse	0.8	126,237	161577.683333333	78.1	
Ge	74	NoGas	Pulse	1.3	532,475	710934.333333333	74.9	
Rh	103	He	Pulse	0.5	284,711	367685.51	77.4	
Rh	103	NoGas	Pulse	0.5	551,515	751394.163333333	73.4	
Tb	159	He	Pulse	0.3	455,274	522974.92	87.1	
Tb	159	NoGas	Pulse	0.5	1,064,786	1255414.6	84.8	
Bi	209	He	Pulse	1.0	271,633	308812.996666667	88.0	
Bi	209	NoGas	Pulse	0.5	633,700	737867.09	85.9	

### Continuing Calibration Blank (CCB) Report ICPMS5

Sample Name:	9K26027-CCB8	Total Dilution:	1.0000
File Name:	121_CCB.d	Vial:	1
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CCB
Acq Time:	11/26/2019 20:47:04	I.S. Reference File:	003CALB.d
Comment:	CCB	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune Mode	Conc.	Units	Conc. RSD	CPS	QC Flag
Be	9	6	NoGas	0.009	ppb	9.4	41	
Na	23	45	He	3.626	ppb	3.8	4,951	
Mg	24	45	He	0.913	ppb	6.1	654	
Al	27	45	He	0.979	ppb	38.5	282	
K	39	45	He	3.134	ppb	69.3	19,090	
Ca	44	45	H2	2.490	ppb	32.7	707	
[Ca]	44	45	He	0.264	ppb	368.5	119	
Ti	47	45	NoGas	0.028	ppb	90.3	43	
V	51	74	He	-0.092	ppb	N/A	1,383	
Cr	52	74	He	0.011	ppb	107.8	209	
Mn	55	74	He	0.070	ppb	72.3	180	
Fe	56	74	H2	1.320	ppb	4.3	17,364	
Co	59	74	He	0.016	ppb	23.5	72	
Ni	60	74	He	-0.051	ppb	N/A	27	
Cu	65	74	He	0.033	ppb	17.5	68	
Zn	66	74	He	0.058	ppb	27.7	51	
As	75	74	He	0.061	ppb	11.2	38	
Se	78	74	H2	0.053	ppb	51.3	14	
Mo	95	103	He	0.051	ppb	9.3	67	
Ag	107	103	He	0.007	ppb	37.1	30	
Cd	111	103	He	0.035	ppb	29.6	23	
[Cd]	111	103	NoGas	0.020	ppb	54.4	37	
Sb	121	103	He	0.290	ppb	6.7	508	
Ba	138	159	He	0.010	ppb	33.5	109	
Hg	201	159	NoGas	6.547	ppt	20.1	8	
Tl	205	159	He	0.007	ppb	38.4	71	
Pb	208	159	NoGas	0.037	ppb	7.5	1,184	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC flag
Li	6	NoGas	Pulse	0.6	692,394	943670.243333333	73.4	
Sc	45	H2	Analog	1.1	1,335,752	1761203.933333333	75.8	
Sc	45	He	Pulse	1.0	204,448	270213.02	75.7	
Sc	45	NoGas	Analog	1.4	2,014,285	2719052.54	74.1	
Ge	74	H2	Pulse	0.3	425,520	547887.95	77.7	
Ge	74	He	Pulse	0.2	127,173	161577.683333333	78.7	
Ge	74	NoGas	Pulse	0.7	536,983	710934.333333333	75.5	
Rh	103	He	Pulse	0.9	293,195	367685.51	79.7	
Rh	103	NoGas	Pulse	0.8	563,431	751394.163333333	75.0	
Tb	159	He	Pulse	1.2	457,057	522974.92	87.4	
Tb	159	NoGas	Pulse	0.7	1,056,423	1255414.6	84.1	
Bi	209	He	Pulse	1.2	277,143	308812.996666667	89.7	
Bi	209	NoGas	Pulse	0.1	637,391	737867.09	86.4	

### CRL Verification Report - ICPMS5

Sample Name: <b>9K26027-CRLB</b>	Total Dilution: <b>1.0000</b>
File Name: 122CRL.d	Vial: 1102
File Path: C:\Agilent\ICPMH1\DATA\9K26027.b	Sample Type: CRL1
Acq Time: 11/26/2019 20:51:47	I.S. Reference File: 003CALB.d
Comment: <b>A19K144 - ESS 11/26</b>	Last Calibration: 11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	0.184	ppb	1.1	381	102.22	
Na	23	45	He	12.625	ppb	0.3	11,545	140.28	R-11
Mg	24	45	He	9.579	ppb	3.9	4,205	106.43	
Al	27	45	He	9.323	ppb	1.1	2,141	103.59	
K	39	45	He	12.191	ppb	10.2	22,508	135.46	R-11
Ca	44	45	H2	9.390	ppb	0.9	1,781	104.33	
[Ca]	44	45	He	9.094	ppb	5.9	281	101.04	
Ti	47	45	NoGas	0.192	ppb	32.6	175	106.67	
V	51	74	He	0.147	ppb	22.4	1,997	81.67	
Cr	52	74	He	0.152	ppb	14.0	627	84.44	
Mn	55	74	He	0.217	ppb	4.8	492	120.56	
Fe	56	74	H2	8.697	ppb	1.2	75,175	96.63	
Co	59	74	He	0.189	ppb	6.8	772	105	
Ni	60	74	He	0.101	ppb	25.5	173	56.11	R-11
Cu	65	74	He	0.206	ppb	11.8	276	114.44	
Zn	66	74	He	0.131	ppb	50.4	86	72.78	
As	75	74	He	0.200	ppb	12.0	80	111.11	
Se	78	74	H2	0.140	ppb	29.9	32	77.78	
Mo	95	103	He	0.177	ppb	9.4	227	98.33	
Ag	107	103	He	0.172	ppb	1.5	633	95.56	
Cd	111	103	He	0.209	ppb	12.3	131	116.11	
[Cd]	111	103	NoGas	0.203	ppb	12.4	330	112.78	
Sb	121	103	He	0.262	ppb	13.0	462	145.56	R-11
Ba	138	159	He	0.188	ppb	1.6	789	104.44	
Hg	201	159	NoGas	8.779	ppt	56.2	10	121.93	
Tl	205	159	He	0.188	ppb	4.3	1,268	104.44	
Pb	208	159	NoGas	0.199	ppb	5.1	4,293	110.56	

*L.M.R.L.*

*L.M.R.L.*

*L.M.R.L.*

*L.M.R.L.*

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.8	692,181	943670.243333333	73.3	
Sc	45	H2	Analog	1.5	1,343,511	1761203.933333333	76.3	
Sc	45	He	Pulse	0.1	205,523	270213.02	76.1	
Sc	45	NoGas	Analog	0.5	2,012,677	2719052.54	74.0	
Ge	74	H2	Pulse	0.4	428,242	547887.95	78.2	
Ge	74	He	Pulse	1.0	127,884	161577.683333333	79.1	
Ge	74	NoGas	Pulse	0.5	535,631	710934.333333333	75.3	
Rh	103	He	Pulse	0.7	293,543	367685.51	79.8	
Rh	103	NoGas	Pulse	0.4	562,274	751394.163333333	74.8	
Tb	159	He	Pulse	0.8	457,371	522974.92	87.5	
Tb	159	NoGas	Pulse	0.8	1,058,531	1255414.6	84.3	
Bi	209	He	Pulse	0.6	276,146	308812.996666667	89.4	
Bi	209	NoGas	Pulse	0.1	637,761	737867.09	86.4	



### CRL Verification Report - ICPMS5

Sample Name:	9K26027-CRLC	Total Dilution:	1.0000
File Name:	123_CRL.d	Vial:	1103
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL2
Acq Time:	11/26/2019 20:56:29	I.S. Reference File:	003CALB.d
Comment:	A19K145 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	0.973	ppb	5.3	1,927	108.11	
Na	23	45	He	48.766	ppb	1.2	37,868	108.37	
Mg	24	45	He	46.090	ppb	0.7	19,121	102.42	
Al	27	45	He	46.288	ppb	2.7	10,356	102.86	
K	39	45	He	50.814	ppb	1.4	36,587	112.92	
Ca	44	45	H2	45.737	ppb	0.9	7,467	101.64	
[Ca]	44	45	He	43.873	ppb	15.7	917	97.5	
Ti	47	45	NoGas	0.908	ppb	8.3	748	100.89	
V	51	74	He	0.837	ppb	4.8	3,753	93	
Cr	52	74	He	0.881	ppb	3.2	2,781	97.89	
Mn	55	74	He	0.940	ppb	3.0	2,028	104.44	
Fe	56	74	H2	44.349	ppb	0.6	354,968	98.55	
Co	59	74	He	0.867	ppb	3.6	3,514	96.33	
Ni	60	74	He	0.796	ppb	9.8	847	88.44	
Cu	65	74	He	0.921	ppb	12.9	1,135	102.33	
Zn	66	74	He	1.064	ppb	11.3	528	118.22	
As	75	74	He	0.948	ppb	8.1	304	105.33	
Se	78	74	H2	0.903	ppb	13.1	193	100.33	
Mo	95	103	He	0.926	ppb	2.8	1,173	102.89	
Ag	107	103	He	0.897	ppb	1.7	3,288	99.67	
Cd	111	103	He	0.946	ppb	2.7	587	105.11	
[Cd]	111	103	NoGas	0.923	ppb	6.1	1,489	102.56	
Sb	121	103	He	0.955	ppb	4.7	1,603	106.11	
Ba	138	159	He	0.949	ppb	4.4	3,676	105.44	
Hg	201	159	NoGas	40.035	ppt	16.4	35	111.21	
Tl	205	159	He	0.913	ppb	1.3	6,027	101.44	
Pb	208	159	NoGas	0.933	ppb	0.5	18,349	103.67	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.3	695,579	943670.243333333	73.7	
Sc	45	H2	Analog	0.8	1,352,524	1761203.933333333	76.8	
Sc	45	He	Pulse	0.7	205,219	270213.02	75.9	
Sc	45	NoGas	Analog	0.6	2,010,943	2719052.54	74.0	
Ge	74	H2	Pulse	0.6	429,386	547887.95	78.4	
Ge	74	He	Pulse	0.6	128,090	161577.683333333	79.3	
Ge	74	NoGas	Pulse	1.1	540,358	710934.333333333	76.0	
Rh	103	He	Pulse	0.9	292,951	367685.51	79.7	
Rh	103	NoGas	Pulse	0.1	566,850	751394.163333333	75.4	
Tb	159	He	Pulse	1.3	455,310	522974.92	87.1	
Tb	159	NoGas	Pulse	1.0	1,057,826	1255414.6	84.3	
Bi	209	He	Pulse	0.8	276,819	308812.996666667	89.6	
Bi	209	NoGas	Pulse	0.6	637,864	737867.09	86.4	

### CRL Verification Report - ICPMS5

Sample Name:	9K26027-CRLD	Total Dilution:	1.0000
File Name:	124CRL_d	Vial:	1104
File Path:	C:\Agilent\ICPMH\1\DATA\9K26027.b	Sample Type:	CRL3
Acq Time:	11/26/2019 21:01:11	I.S. Reference File:	003CALB.d
Comment:	A19K146 - ESS 11/26	Last Calibration:	11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	1.760	ppb	3.8	3,472	97.78	
Na	23	45	He	95.741	ppb	1.7	72,233	106.38	
Mg	24	45	He	93.438	ppb	1.1	38,545	103.82	
Al	27	45	He	93.043	ppb	2.7	20,791	103.38	
K	39	45	He	97.424	ppb	2.0	53,719	108.25	
Ca	44	45	H2	91.378	ppb	2.8	14,462	101.53	
[Ca]	44	45	He	89.565	ppb	4.5	1,755	99.52	
Ti	47	45	NoGas	1.765	ppb	3.5	1,434	98.06	
V	51	74	He	1.776	ppb	4.3	6,098	98.67	
Cr	52	74	He	1.770	ppb	2.3	5,371	98.33	
Mn	55	74	He	1.776	ppb	4.8	3,777	98.67	
Fe	56	74	H2	89.102	ppb	0.3	705,870	99	
Co	59	74	He	1.747	ppb	1.5	7,019	97.06	
Ni	60	74	He	1.752	ppb	3.1	1,760	97.33	
Cu	65	74	He	1.858	ppb	3.3	2,242	103.22	
Zn	66	74	He	1.957	ppb	1.4	943	108.72	
As	75	74	He	1.827	ppb	4.4	564	101.5	
Se	78	74	H2	1.760	ppb	5.5	374	97.78	
Mo	95	103	He	1.755	ppb	6.9	2,234	97.5	
Ag	107	103	He	1.814	ppb	3.8	6,676	100.78	
Cd	111	103	He	1.916	ppb	1.4	1,193	106.44	
[Cd]	111	103	NoGas	1.899	ppb	7.1	3,052	105.5	
Sb	121	103	He	1.891	ppb	2.7	3,161	105.06	
Ba	138	159	He	1.868	ppb	3.9	7,181	103.78	
Hg	201	159	NoGas	76.460	ppt.	5.2	65	106.19	
Tl	205	159	He	1.851	ppb	2.2	12,212	102.83	
Pb	208	159	NoGas	1.875	ppb	1.5	36,335	104.17	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.5	696,524	943670.243333333	73.8	
Sc	45	H2	Analog	1.5	1,340,604	1761203.933333333	76.1	
Sc	45	He	Pulse	1.2	205,624	270213.02	76.1	
Sc	45	NoGas	Analog	1.7	2,011,581	2719052.54	74.0	
Ge	74	H2	Pulse	0.5	429,335	547887.95	78.4	
Ge	74	He	Pulse	0.6	127,202	161577.683333333	78.7	
Ge	74	NoGas	Pulse	0.8	539,103	710934.333333333	75.8	
Rh	103	He	Pulse	0.6	294,219	367685.51	80.0	
Rh	103	NoGas	Pulse	0.7	565,874	751394.163333333	75.3	
Tb	159	He	Pulse	0.7	455,757	522974.92	87.1	
Tb	159	NoGas	Pulse	0.8	1,055,915	1255414.6	84.1	
Bi	209	He	Pulse	0.8	275,855	308812.996666667	89.3	
Bi	209	NoGas	Pulse	0.2	640,496	737867.09	86.8	

### CRL Verification Report - ICPMS5

Sample Name: <b>9K26027-CRLE</b>	Total Dilution: <b>1.0000</b>
File Name: 125CRL4.d	Vial: 1105
File Path: C:\Agilent\ICPMH1\DATA\9K26027.b	Sample Type: CRL4
Acq Time: 11/26/2019 21:05:53	I.S. Reference File: 003CALB.d
Comment: <b>A19K147 - ESS 11/26</b>	Last Calibration: 11/26/2019 11:53:02

**Analyte Table:**

Name	Mass	ISTD	Tune	Conc.	Units	RSD	CPS	% Rec	Flag
Be	9	6	NoGas	3.490	ppb	3.2	6,848	96.94	
Na	23	45	He	186.855	ppb	0.2	138,736	103.81	
Mg	24	45	He	185.867	ppb	0.4	76,377	103.26	
Al	27	45	He	187.531	ppb	0.5	41,836	104.18	
K	39	45	He	191.474	ppb	1.0	88,133	106.37	
Ca	44	45	H2	179.881	ppb	4.0	28,445	99.93	
[Ca]	44	45	He	186.074	ppb	2.4	3,522	103.37	
Ti	47	45	NoGas	3.418	ppb	3.0	2,754	94.94	
V	51	74	He	3.480	ppb	1.5	10,405	96.67	
Cr	52	74	He	3.475	ppb	1.3	10,379	96.53	
Mn	55	74	He	3.556	ppb	1.3	7,535	98.78	
Fe	56	74	H2	187.627	ppb	0.6	1,476,973	104.24	
Co	59	74	He	3.547	ppb	1.5	14,250	98.53	
Ni	60	74	He	3.553	ppb	2.7	3,495	98.69	
Cu	65	74	He	3.746	ppb	2.8	4,494	104.06	
Zn	66	74	He	4.124	ppb	2.2	1,963	114.56	
As	75	74	He	3.685	ppb	5.9	1,117	102.36	
Se	78	74	H2	3.810	ppb	0.8	805	105.83	
Mo	95	103	He	3.443	ppb	3.0	4,353	95.64	
Ag	107	103	He	3.595	ppb	1.2	13,146	99.86	
Cd	111	103	He	3.739	ppb	1.2	2,311	103.86	
[Cd]	111	103	NoGas	3.587	ppb	0.9	5,760	99.64	
Sb	121	103	He	3.646	ppb	2.1	6,033	101.28	
Ba	138	159	He	3.716	ppb	1.3	14,232	103.22	
Hg	201	159	NoGas	146.833	ppt	8.6	123	101.97	
Tl	205	159	He	3.721	ppb	2.4	24,554	103.36	
Pb	208	159	NoGas	3.688	ppb	0.5	71,047	102.44	

**ISTD Table:**

Name	Mass	Tune Mode	Det.	CPS RSD	CPS	ISTD Ref CPS	ISTD Recovery %	QC Flag
Li	6	NoGas	Pulse	0.3	695,222	943670.243333333	73.7	
Sc	45	H2	Analog	1.9	1,354,897	1761203.933333333	76.9	
Sc	45	He	Pulse	0.4	205,567	270213.02	76.1	
Sc	45	NoGas	Analog	0.7	2,008,141	2719052.54	73.9	
Ge	74	H2	Pulse	0.4	428,911	547887.95	78.3	
Ge	74	He	Pulse	1.0	127,256	161577.683333333	78.8	
Ge	74	NoGas	Pulse	0.3	539,103	710934.333333333	75.8	
Rh	103	He	Pulse	0.4	292,452	367685.51	79.5	
Rh	103	NoGas	Pulse	0.9	565,649	751394.163333333	75.3	
Tb	159	He	Pulse	1.0	456,329	522974.92	87.3	
Tb	159	NoGas	Pulse	0.5	1,056,911	1255414.6	84.2	
Bi	209	He	Pulse	1.2	276,366	308812.996666667	89.5	
Bi	209	NoGas	Pulse	0.3	641,161	737867.09	86.9	

## **Metals IFA/IFB Metals Internal Standards Recovery Summary**

A19K340 IFA  
A19K341 IFB  
A9K0412 (I.S Tables)

# Analytical Standard Record

**A19K340**

Description:	ICSA working std	Expires:	12/03/2019
Standard Type:	Calibration Standard	Prepared:	11/25/2019
Solvent:	3.5% HNO3 + 0.4% HCl	Prepared By:	Emily S. Stefansson
Final Volume (mls):	50	Department:	Metals
Vials:	1	Last Edit:	12/02/2019 14:38 by jsj

Analyte	Parent	CAS Number	Concentration	Units
Aluminum	A18L138	7429-90-5	100	ug/mL
Calcium	A18L138	7440-70-2	300	ug/mL
Carbon	A18L138	7440-44-0	200	ug/mL
Chlorine	A18L138	7782-50-5	2000	ug/mL
Iron	A18L138	7439-89-6	250	ug/mL
Magnesium	A18L138	7439-95-4	100	ug/mL
Molybdenum	A18L138	7439-98-7	2	ug/mL
Phosphorus	A18L138	7723-14-0	100	ug/mL
Potassium	A18L138	7440-09-7	100	ug/mL
Sodium	A18L138	7440-23-5	250	ug/mL
Sulfur	A18L138	7704-34-9	100	ug/mL
Titanium	A18L138	7440-32-6	2	ug/mL
Tungsten	A19J281	7440-33-7	0.1	ug/mL

Parent Standards used:									
Standard	Description	Prepared	Prepared By	Lot Nbr	Expires	Last Edit	(mls)		
A18L138	6020A ICS Interferents A	12/11/2018	LGC	150520-8	12/03/2019	07/23/2019 16:48	by arf	5	
A19H398	Conc. HCl - Omnitrace	08/23/2019	Omni Trace	56208	08/23/2021	08/29/2019 11:38	by jsj	0.2	
A19J277	Conc. HNO3 - Omnitrace	10/18/2019	Omni Trace	59162	04/15/2020	10/28/2019 13:30	by jsj	1.75	
A19J281	1 W 10 ppm	10/18/2019	Dilution	n/a	04/15/2020	10/28/2019 12:35	by jsj	0.5	

# Analytical Standard Record

**A19K341**

Description:	ICSA+B working std	Expires:	12/03/2019
Standard Type:	Calibration Standard	Prepared:	11/25/2019
Solvent:	3.5% HNO3 + 0.4% HCl	Prepared By:	Emily S. Stefansson
Final Volume (mls):	50	Department:	Metals
Vials:	1	Last Edit:	12/02/2019 14:39 by jsj

Analyte	Parent	CAS Number	Concentration	Units
Aluminum	A18L138	7429-90-5	100	ug/mL
Calcium	A18L138	7440-70-2	300	ug/mL
Carbon	A18L138	7440-44-0	200	ug/mL
Chlorine	A18L138	7782-50-5	2000	ug/mL
Iron	A18L138	7439-89-6	250	ug/mL
Magnesium	A18L138	7439-95-4	100	ug/mL
Molybdenum	A18L138	7439-98-7	2	ug/mL
Phosphorus	A18L138	7723-14-0	100	ug/mL
Potassium	A18L138	7440-09-7	100	ug/mL
Sodium	A18L138	7440-23-5	250	ug/mL
Sulfur	A18L138	7704-34-9	100	ug/mL
Titanium	A18L138	7440-32-6	2	ug/mL
Arsenic	A18L139	7440-38-2	0.1	ug/mL
Cadmium	A18L139	7440-43-9	0.1	ug/mL
Chromium	A18L139	7440-47-3	0.2	ug/mL
Cobalt	A18L139	7440-48-4	0.2	ug/mL
Copper	A18L139	7440-50-8	0.2	ug/mL
Manganese	A18L139	7439-96-5	0.2	ug/mL
Nickel	A18L139	7440-02-0	0.2	ug/mL
Selenium	A18L139	7782-49-2	0.1	ug/mL
Silver	A18L139	7440-22-4	0.05	ug/mL
Vanadium	A18L139	7440-62-2	0.2	ug/mL
Zinc	A18L139	7440-66-6	0.1	ug/mL
Mercury	A19J028	7439-97-6	0.002	ug/mL
Tungsten	A19J281	7440-33-7	0.1	ug/mL

**Parent Standards used:**

Standard	Description	Prepared	Prepared By	Lot Nbr	Expires	Last Edit	(mls)
A18L138	6020A ICS Interferents A	12/11/2018	LGC	150520-8	12/03/2019	07/23/2019 16:48	by arf 5
A18L139	6020A & CLP-M ICS Analytes B	12/11/2018	LGC	983307-1	12/03/2019	12/18/2018 13:34	by jsj 0.5
A19H398	Conc. HCl - Omnitrace	08/23/2019	Omni Trace	56208	08/23/2021	08/29/2019 11:38	by jsj 0.2
A19J028	Hg Stock 1.00ppm Std Primary	10/02/2019	n/a	n/a	03/30/2020	10/23/2019 17:40	by jsj 0.1
A19J277	Conc. HNO3 - Omnitrace	10/18/2019	Omni Trace	59162	04/15/2020	10/28/2019 13:30	by jsj 1.75
A19J281	1 W 10 ppm	10/18/2019	Dilution	n/a	04/15/2020	10/28/2019 12:35	by jsj 0.5



**Total Solids by SM 2540G  
Benchsheet Data**

Batch 9110857 (A9K0412-01)





Apex Laboratories  
PREPARATION BENCH SHEET

NOV 20 2019

Percent Solids + Dry Weight Worksheet

BATCH #: 9110857 (Matrix: Sediment)

Lab Number	Analysis	QC Source ID	Prepared (Time In)	Weighed (Time Out)	Tare Wt. (g)	Wet Weight (+Tare) (g)	Dry Weight (+Tare) (g)	% Solids (Calc)	LogComments
A9K0412-01	Solids, Total (SM 254		11/15/19 11:24		1.272	27.136	25.199	92.5	
9110857-DUP1	QC	A9K0412-01	11/15/19 11:24		1.272	27.857	25.81	92.3	
A9K0412-02	Solids, Total (SM 254		11/15/19 11:24		1.256	29.132		-4.5	cancelled per client 11/15

NRP  
Prepared By: \_\_\_\_\_ Date: 11/16/19

James S. Johnson  
Reviewed By: \_\_\_\_\_ Date: 11/18/19

Batch #: 9110857

# Total Solids Worksheet

Date: 11/15/2019

Analyst: nrp

Method: SM 2540 G

Sample ID	Tare Wt. (g)	Vessel ID	Initial (wet) Wt. (g)	Final Weight (g)			Comments
				1 <sup>st</sup> weighing	2nd Weighing	3rd Weighing	
A9K0412-01	1.272	412-01	27.136	25.199	25.213		
9110857-DUP1	1.272	412-01DUP	27.857	25.810	25.820		source: A9K0412-01
A9K0412-02	1.256	412-02	29.132				Analysis canceled
Date/time first in oven: 11/15/19@13:39		Oven temp. (°C; in/out):		103.7/103.7	103.2/104.7	/	
		Time of weighing:		11/16@9:47	11/16@11:36		

**TCLP Extraction by EPA 1311  
Benchsheet Data**

Batch 9111146 (A9K0412-01)  
Batch 9110920 (A9K0412-01) (ZHE)

DEC 10 2019

Apex Laboratories  
 BATCH #: 9111146 (Matrix: Soil)  
 TCLP Leachate Bench Sheet

#	Lab Number	Analysis	Initial (g)	Final (mL)	Start Time	Stop Time	Sample pH	TCLP Fluid	Client / Sample
	9111146-BLK1	QC	50	1000	11/25/19 16:40	11/26/19 0845	4.96	#1	
	A9K0412-01	TCLP Extraction - Metals	100	2000	11/25/19 16:40	11/26/19 0845	4.5	#1	Anchor QEA, LLC / PDI-142RAB-C-00-30.4-191112
	A9K0412-01	TCLP Extraction - Organics	100	2000	11/25/19 16:40	11/26/19 0845	4.5	#1	Anchor QEA, LLC / PDI-142RAB-C-00-30.4-191112

Fluid ID: A19K328  
 Syringe Filter Lot: A19J375  
 % Solids Filter Lot: A19C193

CRL                      11/26/19  
 Prepared By:                      Date

ESS                      11/26/19  
 Reviewed By:                      Date

**TCLP \ SPLP\*** (circle one)

Batch.# 911146

Prepared By: CRL

\*For SPLP, the FD pre-test is not performed. If the sample is water or waste (not soil) then use fluid #1. If the sample is soil, FD is based on sample origination: east of the Mississippi R. - use fluid #1, west of the Mississippi R. - use fluid #2.

**Fluid Determination (FD)**

Sample ID	Weight 5 g	+DI H2O 96.5 mL (19.3 mL/g)	pH after 5 min stir	If pH >5, add 3.5 mL 1N HCl** (0.7mL/g)	Heat to 50° for 10 min.	pH @ room temp	Fluid #	% Solids	Size Reduction
	(g)	(mL)	(s.u.)	(mL or "NA")	("✓" or "NA")	(s.u. or "NA")	("1" or "2")	(%)	("Y" or "N")
A9K0412-01	5	96.5	4.5				1	100	N

**Extraction**

Sample ID	Tare Weight	Weight 100±0.1	Fluid 2000±1%	Fluid #	Fluid ID	Extract pH (to nearest 0.5)
	(g)	(g)	(g)	("1" or "2")		(s.u.)
9111146-BLK1		50	1000	1	A9K328	4.96
A9K0412-01	1143	100	2000	1	↓	4.5

Extraction Start/Stop

	Date	Time	Intl.
START	11/25/19	1640	CRL
STOP	11/26/19	845	CRL

Stop time window:

RPM 31

Reset Min/Max Temp	Min Temp	Max Temp
<input checked="" type="checkbox"/>	As read: 21.4	22.8
	Corr factor: 0	0
	Actual: 21.4	22.8

Thermometer ID: S/N RC-5-001

**PREPARATION BENCH SHEET**

**Apex Laboratories**

NOV 21 2019



**BATCH #: 9110920 (Solid)**

**Prep Method: EPA 1311 TCLP/ZHE**

Lab Number	Cont.	Analysis	Prepared	Initial (g)	Final (mL)	Spike ID	Source ID	ul Spike	ul Surr.	ClientID / Sample	Extraction Comments	pH*
A9K0403-01	A	TCLP/ZHE Extraction	11/18/19 15:55	25	500					FC-111319-1219		
A9K0412-01	B	TCLP/ZHE Extraction	11/18/19 15:55	25	500					PDI-142RAB-C-00-30.4-191112		

\*pH <2 verified 1/A

**Standards/Reagents**

Reagent(s)			Analyte Spike(s)			Surrogate(s)		
Std ID	Exp. Date	Description	Std ID	Exp. Date	Description	Std ID	Exp. Date	Description

TCLP Fluid #1  
 Fluid ID: A19K247  
 Start: 11/18/19 1555  
 Stop: 11/19/19 1020  
 Temp: 21.7 to 23 C  
 A19F218 Metals Balance

Prepared By: [Signature] Date: 11/19/19

Reviewed By: [Signature] Date: 11/20/19

**APEX LABS ZHE WORKSHEET**

Batch # 9110920

Analyst 

Sample ID	ZHE #	Matrix	Weight of Sample in Pan (g)	Weight of Sample Remaining in Pan (g)	Weight of Sample Added (g)	TCLP Fluid #1 (g)	Initial PSI (5-10)	Final PSI *	Comments
AAK0403-01	1	Soil	NA	NA	25.0	500	10	10	
AAK04112-01	2	↓	↓	↓	25.0	500	10	11	

\*Re-extract if pressure reads 0 PSI

Start 11/18/19 Stop 11/19/19  
 Date/Initials JS Date/Initials JB

Time (18+/- 2h) 1555 Time 1020

RPM (30) 30

Temp (23+/- 2°C) Min: 21.7 Max: 23 (For thermometer SN EU6200919) C.F. 0

Comments: TCLP Fluid # 1 Lot # A19K247 Temp before C.F. NA

## **Balance Checksheets**

Extractions November 2019  
Extractions November 2019  
Dry Weight November 2019  
Wet Chem November 2019  
Metals November 2019  
Sample Rec. November 2019



Balance Challenge Log

Extractions  
AND FX-2000  
ID# 5210177

Weight ID	weight (g)	acceptance range (g)	
	$\leq 1g$	$\pm 0.02g$	
	$> 1g$	$\pm 2%$	
10077	0.5g	0.48	0.52
1000143395	300g	294.00	306.00

If other than as listed above, the weight and tracking ID of the mass used to challenge the balance must be recorded.

Alternate Weight/ID used:

Date Range:

Month: November  
Year: 2019

Day/Time	Initials
1 07:40	JAG
2	
3	
4 07:25	JAG
5 07:25	JAG
6 07:55	JAG
7 07:20	JAG
8 07:34	AJJ
9	
10	
11 07:15	JAG
12 10:20	Curt
13	
14 07:20	JAG
15 07:10	AJJ
16	
17	
18 07:20	AJJ
19 9/5	X
20 07:18	AJJ
21 07:24	AJJ
22 07:33	AJJ
23	
24	
25 07:20	JAG
26 08:05	JAG
27 07:05	JAG
28	
29	
30	
31	

Weight One	Observed
	.48
	.51
	.50
	.51
	.49
	0.51
	.50
	0.49
	.50
	0.50
0.50g	
	0.49
	0.50
	0.50
	0.51
	0.50
	<del>JAG 11/25/19</del> <del>0.49</del>
	0.49
	0.49

Weight Two	Observed
	299.98
	300.00
	299.98
	299.99
	299.95
	299.98
	299.98
	299.99
	299.97
	299.97
300.00g	
	299.95
	299.96
	299.98
	299.96
	299.97
	299.95
	299.97
	300.00

Balance Challenge Log

Dredd  
Intelli-lab PC-6001  
ID# 190408014

Weight ID      weight (g)      acceptance range (g)  
 =/ $<1g$        $\pm 0.02g$   
 $>1g$        $\pm 2%$

03-J68814-10      10.0      9.8      10.2  
 15477      200.0      196.0      204.0  
 15477 + 1000139353      1 kg + 2kg      2940.0      3060.0

If other than as listed above, the weight and tracking ID of the mass used to challenge the balance must be recorded.

Month: November  
 Year: 2019

Alternate Weight/ID used:

Date Range:

*at 11/4/19*

Day/Time	Initials
1 750	KT
2 800	KT
3	
4 800	KT
5 807	MJG
6 750	MJG
7 759	MJG
8 806	MJG
9	
10	
11 750	MJG
12 815	MJG
13 750	KT
14 815	MJG
15 720	KT
16	
17	
18 800	KT
19 845	MJG
20 812	MJG
21 800	KT
22 817	MJG
23	
24	
25 800	KT
26 740	MJG
27 835	MJG
28	
29	
30	
31	

Weight 1	Observed
	9.9
	9.9
	10.0
	10.0
	10.0
	10.0
	10.0
	10.0
	10.0
	10.0
	10.0
	10.0
	9.9
	9.9
	9.9
	10.0
	10.0
	10.0
	9.9
	9.9

10.0 g

Weight 2	Observed
	200.0
	200.1
	200.1
	200.1
	200.0
	200.1
	200.1
	200.1
	200.1
	200.1
	200.1
	200.1
	200.1
	200.1
	200.1
	200.2
	199.9

200.0 g

Weight 3	Observed
	3002.1
	<del>3002.3</del>
	3002.3
	3002.1
	3002.2
	3002.2
	3002.1
	3002.2
	3002.3
	3002.3
	3002.2
	3002.3
	3002.5
	3002.4
	3002.3
	3002.3
	3002.1
	3002.3
	3002.2
	2999.9

*MJG 11/19/19*

*3002.4*

Balance Challenge Log

Metals Prep Balance 2  
Sartorius LC 620 P  
40020073

Weight ID	weight (g)	acceptance range (g)	
	=/<1g	± 0.02g	
	>1g	± 2%	
03-J68049-19	0.100g	0.080	0.120
03-J68814-10	10g	9.800	10.200
15477 (100g + 500g)	600g	588.000	612.000

If other than as listed above, the weight and tracking ID of the mass used to challenge the balance must be recorded.

Month: November  
Year: 2019

Alternate Weight/ID used: \_\_\_\_\_ Date Range: \_\_\_\_\_

~~11/11/19~~ let 11/14/19

Day/Time	Initials	Weight 1	Observed	Weight 2	Observed	Weight 3	Observed
1 750	KT		599.990		9.998		0.097
2 8							
3							
4 800	KT		599.985		10.000		0.099
5 805	MSG		599.980		9.999		0.100
6 748	MSG		599.985		9.998		0.099
7 757	MSG		599.985		10.000		0.100
8 805	MSG		599.980		9.997		0.098
9							
10							
11 748	MSG		599.990		9.999		0.099
12 813	MSG		599.990		10.004		0.103
13 750	KT		599.995		10.001		0.100
14 813	MSG		599.990		9.999		0.099
15 720	KT		599.990		10.000		0.099
16		600.000g		10.000g		0.100g	
17							
18 800	KT		600.000		9.999		0.098
19 942	MSG		600.000		10.000		0.101
20 810	MSG		600.000		10.001		0.101
21 800	KT		599.995		10.001		0.101
22 815	MSG		599.990		9.999		0.100
23							
24							
25 800	KT		599.990		10.000		0.100
26 737	MSG		599.990		10.001		0.101
27 834	MSG		599.985		10.000		0.100
28							
29							
30							
31							

Balance Challenge Log

Wet Chem Balance 3

Mettler AE160  
ID# C82939

Weight ID	weight (g)	acceptance range (g)	
	<0.5000g	± 0.5mg	
	>/=0.5000g	± 0.1%	
1000015949	0.005g	0.0045	0.0055
66067	0.100g	0.0995	0.1005
66067	100g	99.9000	100.1000

If other than as listed above, the weight and tracking ID of the mass used to challenge the balance must be recorded.

Month: November  
Year: 2019

Alternate Weight/ID used: \_\_\_\_\_  
Date Range: \_\_\_\_\_

Day/Time	Initials	Weight 1	Observed	Weight 2	Observed	Weight 3	Observed
1							
2							
3							
4							
5							
6							
7							
8	12:35 MKK		99.9992		0.1000		0.0050
9							
10							
11	1044 MKK		99.9988		0.1000		0.0050
12	0935 CMZ		100.0003		0.1001		0.0051
13	0626 JLP		100.0003		0.1001		0.0050
14	0821 CMZ		100.0004		0.1001		0.0051
15	0415 JLP		100.0004		0.1001		0.0050
16		100.0000g		0.1000g		0.0050g	
17							
18							
19	0653 JLP		100.0009		0.1002		0.0051
20							
21							
22							
23							
24							
25							
26							
27							
28							
29							
30							
31							

Balance Challenge Log

Wet Chem Balance 1  
 Ohaus Adventurer Pro  
 ID# 8C30461093

Weight ID	weight (g)	acceptance range (g)	
	<0.5000g	± 0.5mg	
	>/=0.5000g	± 0.1%	
1000015949	0.005g	0.0045	0.0055
66067	0.100g	0.0995	0.1005
66067	100g	99.9000	100.1000

If other than as listed above, the weight and tracking ID of the mass used to challenge the balance must be recorded.

Month: NOV  
 Year: 2019

Alternate Weight/ID used: \_\_\_\_\_  
 Date Range: \_\_\_\_\_

Day/Time	Initials	Weight 1	Observed	Weight 2	Observed	Weight 3	Observed
1							
2							
3							
4	9:59 MRE		99.9986		0.1001		0.0050
5	10:20 MRF		99.9989		0.1000		0.0050
6	10:10 WVD		99.9986		0.0999		0.0050
7	10:49 MRE		99.9981		0.1000		0.0051
8	10:45 WVD		99.9987		0.1000		0.0051
9							
10							
11	7:55 MRF		99.9994		0.1001		0.0050
12	8:00 MRF		99.9993		0.1000		0.0051
13	9:46 MRE		99.9997		0.1002		0.0051
14	0827 CMA		99.9995		0.0998		0.0048
15	0613 JEP		100.0002		0.1001		0.0050
16		100.0000g		0.1000g		0.0050g	
17					0.1000		
18	9:25 MRF		100.0011		0.1000		0.0050
19	7:42 MRF		100.0014		0.0999		0.0049
20	10:30 MRF		100.0012		0.1000		0.0050
21	11:00 MRF		100.0011		0.1001		0.0049
22							
23							
24	12						
25	14:22 MRF		100.0017		0.1000		0.0051
26	7:35 MRE		100.0002		0.1000		0.0050
27	8:58 MRE		99.9997		0.1000		0.0050
28							
29							
30							
31							

**Balance Challenge Log**

**Wet Chem Balance 4**  
 Ohaus Pioneer PA124C  
 ID# B549799185

Weight ID	weight (g)	acceptance range (g)	
		± 0.5mg	
		± 0.1%	
1000015949	0.005g	0.0045	0.0055
66067	0.100g	0.0995	0.1005
66067	100g	99.9000	100.1000

If other than as listed above, the weight and tracking ID of the mass used to challenge the balance must be recorded.

Month: November  
 Year: 2019

Alternate Weight/ID used: \_\_\_\_\_ Date Range: \_\_\_\_\_

Day/Time	Initials	Weight 1	Observed	Weight 2	Observed	Weight 3	Observed
1 0319	CMB		99.9999		0.0998		0.0078
2 0950	CMB		100.0005		0.1001		0.0051
3							
4 0824	CMB		100.0004		0.1000		0.0051
5 0804	CMB		100.0003		0.0998		0.0050
6 0915	CMB		100.0002		0.0998		0.0050
7 1024	WVD		100.0002		0.1000		0.0049
8 0933	CMB		100.0001		0.1000		0.0051
9 1405	CMB		100.0000		0.0999		0.0050
10 15:53	CMB		100.0007		0.1000		0.0050
11 1246	CMB		100.0006		0.1000		0.0050
12 0777	CMB		100.0002		0.1000		0.0051
13 0747	CMB		100.0002		0.1001		0.0051
14 0826	CMB		100.0003		0.1000		0.0049
15 0616	JKP		99.9996		0.1000		0.0050
16		100.0000g		0.1000g		.0050g	
17							
18 0840	CMB		100.0001		0.1000		0.0049
19 1053	WVD		100.0008		0.1000		0.0050
20 0636	JKP		100.0012		0.1000		0.0050
21 0641	JKP		100.0023		0.0998		0.0048
22 0635	JKP		99.9998		0.0999		0.0050
23 1059	CMB		100.0000		0.0999		0.0051
24 1027	CMB		100.0000		0.1001		0.0052
25 0707	JKP		99.9998		0.1000		0.0050
26 0627	JKP		100.0003		0.1000		0.0051
27 0605	JKP		100.0005		0.1000		0.0050
28							
29							
30							
31							

Balance Challenge Log

BalanceName  
Lady Justice  
S/N 593312

Weight ID	weight (g)	acceptance range (g)	
		$\pm < 1g$	$\pm 2%$
10660	0.10g	0.08	0.12
10581	50.00g	49.00	51.00
15477	500.00g	490.00	510.00

If other than as listed above, the weight and tracking ID of the mass used to challenge the balance must be recorded.

Month: ~~October~~ November  
Year: 2019

Alternate Weight/ID used: \_\_\_\_\_ Date Range: \_\_\_\_\_

Day/Time	Initials	Weight 1	Observed	Weight 2	Observed	Weight 3	Observed
1 8:20	WS		0.10		49.99	ONLY	
2						NEEDED	
3						WHEN	
4 7:35	WS		0.10		49.99	WEIGHING	
5 8:25	WS		0.08		49.97	OVER	
6 8:05	WS		0.10		49.99	50 g	499.76
7 9:25	WS		0.09		49.99	KEPT	
8 7:45	WS		49.98		0.10	IN METALS	
9 9:00	PK		0.10		49.98	DEPT.	
10						500.00g	
11 13:40	WS		0.09		49.97		
12 8:42	WS		0.09		49.97		
13 7:40	WS		0.09		49.97		
14 7:45	WS		0.10		49.98		
15 8:00	WS		0.09		49.97		
16 10:30	PK	0.10g	0.09	50.00g	49.98		1199.70
17							
18 7:43	WS		0.09		49.98		
19 7:46	WS		0.10		49.97		499.70
20 8:45	WS		0.09		49.97		
21 7:40	WS		0.09		49.98		
22 7:35	WS		0.09		49.97		499.72
23 10:59	WS		0.09		49.97		
24							
25 7:45	WS		0.10		49.97		
26 7:40	WS		0.09		49.97		
27 9:40	WS		0.09		49.99		
28							
29							
30							
31							

WS 11/8  
↔

14:13  
WS 11/8/19

+49.99  
549.77

WS 11/20/19  
12:53

WS 11/25  
7:45