


STERICYCLE...YOUR PARTNER FOR SUCCESS.



MARKET LEADER IN HEALTHCARE COMPLIANCE SERVICES



**Stericycle®**

## YOU NEEDED TO...

- Responsibly manage your medical waste.*
- Comply with current OSHA regulations.*
- Protect your business against potential liability.*
- Guarantee your employees health and safety.*
- Ensure your success.*

THAT'S WHY YOU CHOSE STERICYCLE, THE LARGEST PROVIDER OF COMPLIANCE SERVICES FOR THE HEALTHCARE INDUSTRY IN THE UNITED STATES. YOU CHOSE THE ONLY NATIONWIDE COMPANY THAT OFFERS INTEGRATED SERVICES AND PROGRAMS — SAFE AND COST-EFFECTIVE MANAGEMENT OF REGULATED MEDICAL WASTE COLLECTION, TRANSPORTATION, TREATMENT AND DISPOSAL, ALONG WITH COMPREHENSIVE OSHA COMPLIANCE PROGRAMS AND PRODUCT SALES. TOTAL CUSTOMER SATISFACTION IS OUR NUMBER ONE PRIORITY, YOU WILL RECEIVE BEST-IN-CLASS SERVICE FROM DEDICATED PROFESSIONALS WHO CARE.



### USE STERICYCLE TO...

- TAKE THE GUESSWORK OUT OF OSHA COMPLIANCE (STERI•SAFE<sup>SM</sup>).
- PROVIDE TRAINING, WASTE MINIMIZATION AND MOCK OSHA AUDITS.
- PROVIDE LEGAL DOCUMENTATION FOR STATE REPORTING.
- SUPPLY COMPLIANCE TRAINING, SHARPS CONTAINERS, SAFETY PRODUCTS, ETC.



SINCE 1989, STERICYCLE HAS PROVIDED INTEGRATED SERVICES TO HEALTHCARE COMPANIES NATIONWIDE, INCLUDING HOSPITALS, PHYSICIAN AND DENTAL OFFICES, LABORATORIES AND CLINICS. OVER 275,000\* CUSTOMERS HAVE CHOSEN STERICYCLE AS THEIR COMPLIANCE PARTNER.

\*CUSTOMERS AS OF 9/02

Cs
Bp
Pr
Pa
Cp
Tr

## STERICYCLE...YOUR PARTNER FOR SUCCESS.



Pa



Bp

INSIDE, YOU MAY FIND INFORMATION ON THE FOLLOWING TOPICS, INCLUDING:

	CALENDAR - SERVICE SCHEDULE
SAMPLE INVOICE STATEMENT	
	WASTE ACCEPTANCE PROTOCOL
REGULATORY ALERTS	

### MISSION STATEMENT

TO BE THE LEADING COMPANY DEDICATED TO THE ENVIRONMENTALLY RESPONSIBLE MANAGEMENT OF INFECTION CONTROL AND COMPLIANCE SERVICES FOR THE HEALTHCARE COMMUNITY.


Experts in Infection Control and Healthcare Compliance Services



**Laura Batte**  
Inside Sales Coordinator

20320 80th Avenue South  
Kent, WA 98032  
www.stericycle.com

Tel: 425.291.9322  
Fax: 425.291.9329  
lbatte@stericycle.com



**Stericycle®**

Experts in infection control and healthcare compliance services.

## Company Overview

**P**roducts that protect and programs that comply. That's Stericycle – a leading full-service provider of infection control management and compliance services for the healthcare community. Our medical, personal protection, and infectious waste disposal products and services include comprehensive programs that help our customers comply with evolving regulations. It is our mission to improve safety by reducing risk exposure for both patients and professionals, while making healthcare more efficient for everyone.

Since it began in 1989, Stericycle has become the leading provider of regulated medical waste management services in North America. As strict medical waste management regulations were adopted to protect the public, we saw the opportunity to manage medical waste for a wide variety of healthcare customers far more efficiently than they could on their own – and in compliance with regulatory conditions. Moreover, we developed a patented treatment process that is safe, clean and reduces the volume of medical waste in landfills.

### Sterifacts: The Basics

- Stericycle was founded in 1989 and became a publicly traded company (NASDAQ:SRCL) in 1996
- Corporate headquarters is in Lake Forest, Illinois, near Chicago

Today, we're a national full-service medical waste management provider, and we have a growing global presence. We serve more than 300,000 customers including hospitals, blood banks and pharmaceutical manufacturers, as well as medical and dental offices, outpatient clinics, laboratories and more.

For Stericycle, medical waste management was just the beginning. We're constantly seeking to advance the industry by developing new technologies and improved products that expand the frontiers of medical waste management and compliance services.


For example, in addition to our industry-leading medical waste management services:

- We offer **BioSystems sharps management** services that reduce cost, free up valuable personnel time, and reduce the risk of needle sticks in hospital settings.
- Our **Steri-Safe<sup>SM</sup> OSHA and HIPAA Compliance programs** help healthcare employers manage current OSHA and HIPAA requirements with state-of-the-art training tools and services for a predictable flat monthly fee.
- Our new **Stericycle JRepository<sup>TM</sup>** is a dynamic, web-based tool designed to improve the total quality of healthcare and provide continual readiness for JCAHO compliance.
- Our **Stericycle Infection Control Management Software** lets professionals spend less time managing data and more time preventing infections.
- Our **Steri-Safe<sup>SM</sup> disinfectant** is the only hospital-grade disinfectant cleaner with a human safety profile (dermal, oral and ocular) that is EPA Toxicity category IV\*.
- Our **Stericycle Direct Return** program removes the guesswork and effort from returning expired pharmaceuticals.

\* Support on file

In addition to our diverse customer base and broad range of high-quality services, our advantages include:

- **Industry leadership.** We are the industry's most efficient, fully integrated operator, the leading market innovator, and the industry's environmental and safety leader.
- **Global reach.** We combine our technological expertise with the know-how of local partners to offer total solutions that address local and national requirements. Since 1996,

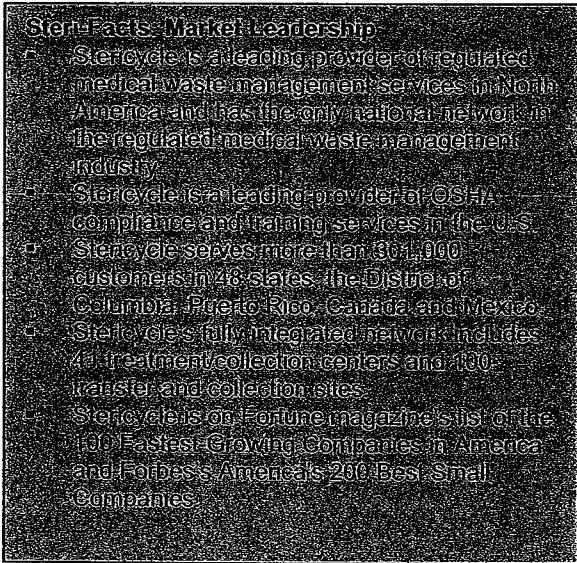

we have entered into agreements with companies in Brazil, Mexico, Argentina, South Africa, Japan and Australia to either form joint ventures or license our patented treatment technology. Through our Canadian subsidiary, we operate in six provinces.


- **An established national network.** Our 41 treatment/collection centers and 100 transfer and collection sites operate as an integrated network throughout North America.
- **Efficient operations.** Our vertically integrated network and broad geographic presence means we are able to increase our route densities, so our

drivers make more stops per shift and keep the distance traveled to treatment facilities to a minimum.

## Medical Waste Management

Every day, throughout North America and across the globe, Stericycle is collecting, treating and disposing of medical waste in the most responsible methods. We have more than 300,000 customers in 48 states, the District of Columbia, Puerto Rico, Canada and Mexico.

Collect it. Treat it. Dispose of it. Document it. Simply put, that's the process. Yet Stericycle's full-service medical waste management program goes further. We not only champion the need for safe, secure and environmentally responsible management of medical waste, we combine our services with training and education, consulting services, and product sales. We help protect customers and their employees against potential liabilities and injuries associated with the handling, transportation, and disposal of regulated medical waste. For example:

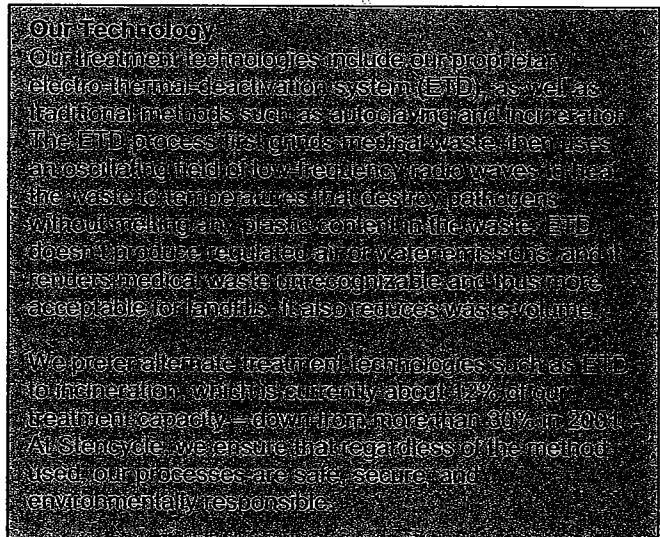

- Our programs help customers identify, handle and segregate their regulated medical waste, reducing the amount of medical waste they pay to manage.
- We advise and assist healthcare customers with the proper methods of recording and documenting their medical waste management to comply with all regulations. Our Bio-Track bar-coding system tracks the container from the point of generation to treatment.
- We offer training and consulting to help customers reduce the amount of medical waste they generate and improve safety and OSHA regulatory compliance in their workplace.

Stericycle also provides assured destruction of expired pharmaceuticals, recycling of mercury in dental amalgam, and mail-back programs for disposing small or infrequently generated quantities of regulated medical waste, including sharps.

### **BioSystems Sharps Management Program**

BioSystems is the expert in providing safe, environmentally-friendly, and cost effective full-service sharps management solutions to hundreds of major hospitals throughout the U.S. We're much more than collection and safe disposal – our unique sharps containers are easy to use and re-useable, reducing waste in landfills. Our technicians manage the process of container monitoring and disposal, mitigating the risk of sharps injuries due to overfull containers, freeing up valuable time by relieving sharps container handling and disposal responsibility from health professionals. This results in lowered risk and cost.


### **Steri-Safe<sup>SM</sup> OSHA Compliance Program**

With our Steri-Safe<sup>SM</sup> OSHA Compliance Program, we take the guesswork out of getting into compliance and staying there. It is the worry-free way to keep in compliance, enhance employee safety, keep your waste under control and keep your costs down. A flat monthly fee includes a comprehensive package of services, including waste pickup and disposal, training manuals and interactive CD-ROMs, on-site training and mock inspections, safety product discounts and more.

In addition, our Steri-Safe<sup>SM</sup> HIPAA Compliance Program gives you all the online web-based tools you need for a low flat monthly fee. It's the easy way to track and manage all the changes in your practice mandated by HIPAA.

### **Stericycle JRepository<sup>TM</sup>**

The Stericycle JRepository<sup>TM</sup> is a comprehensive, web-based compliance tool that helps hospital organizations constantly monitor JCAHO compliance, thereby ensuring continual readiness for unannounced surveys. With its customizable assessments, tracer methodology, automated corrective action plans, event reporting and tracking, and more, the Stericycle JRepository<sup>TM</sup> moves complex manual tasks to an automated quality process – reducing the time and costs usually needed to keep organizations in a state of continuous readiness. Moreover, it allows collaborative communication and accountability among hospital professionals, thereby including everyone in creating total quality improvement.

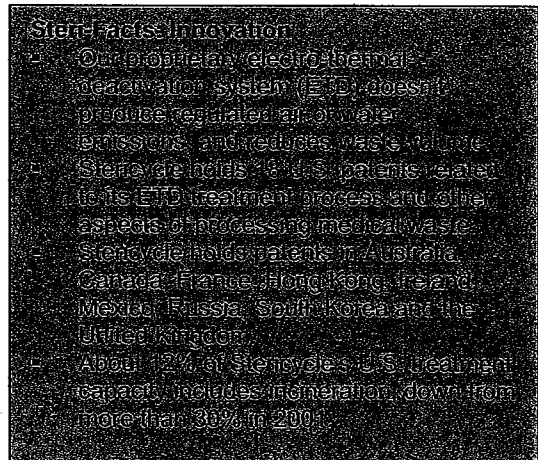

## **Infection Control and Safety Solutions Products**

From infection control to personal protection, from patient care to waste containment, the Steri-Safe Infection Control & Safety Solutions guide offers a wide range of products that are carefully evaluated to meet the highest standards. Included in our catalog are infection control products, needle stick safety syringes, patient care products, our special waste disposal program for mercury and dental amalgams, and more.

## **Stericycle Infection Control Management Software**

Giving professionals more time to prevent and control infections rather than spend time collecting and reporting data is the objective of Stericycle Infection Control Management Software. It is an infection surveillance and outbreak management tool that helps infection control professionals save lives by attacking the root causes of infection, while also reducing the excessive time demands of infection monitoring and analysis. Every year, infections lead to more than an estimated 30,000 preventable deaths and billions of dollars in healthcare costs\*\*. Our easy-to-learn software standardizes the infection-tracking process, monitors for potential outbreaks, and gives advance warning of possible outbreaks.

## **Steri-Safe<sup>SM</sup> Disinfectant Cleaner**

Steri-Safe<sup>SM</sup> Disinfectant Cleaner is a breakthrough disinfectant cleaner for infection control in any setting – including patient care areas, laboratories, food preparation areas, health club facilities, daycare centers, schools and households. It's revolutionary because it offers hospital grade, broad spectrum disinfection without the disadvantages -- Steri-Safe<sup>SM</sup> is a safe, ready-to-use, non-flammable single product that disinfects multiple surfaces with no special disposal needed. It's the only hospital-grade disinfectant cleaner of its kind that is non-toxic, non-irritating and non-corrosive. In addition, it is the only hospital-grade disinfectant cleaner with a human safety profile (dermal, oral and ocular) that is EPA Toxicity category IV, and it's registered by the EPA for use on food contact surfaces.

## **Stericycle -- Direct Return<sup>TM</sup>**

Stericycle -- Direct Return<sup>TM</sup> takes the guesswork, the labor, the risk, and a lot of hassle out of managing expired medications, while reducing pharmaceutical costs. Hospital pharmacies annually lose thousands of dollars in manufacturer credits for outdated, damaged, and unsalable pharmaceutical products due to inefficient, costly and often confusing return processes. Stericycle -- Direct Return<sup>TM</sup> delivers a double-digit percentage increase in average annual manufacturer returns credits. Our technicians will manage expired medications on site, or we'll provide a kit that allows hospitals to easily handle the process themselves. We offer internet-based technology that provides 24/7 online availability of current returns data and reports, on-site packing and shipping service, and a single location to which all expired medications are shipped. It's easy to use, generates increased revenues for the hospital, and reduces the risk to patient health from expired medications.

\*\*U.S. Agency for Healthcare Research and Quality and Johns Hopkins University.

# Steri-Safe™

## Breakthrough Nanoemulsion Technology – Breaks the “Efficacy-Safety” Paradox

Finally there's a broad spectrum, hospital-grade disinfectant cleaner without the harmful effects to humans, materials or the environment!

### Introducing Steri-Safe™ Disinfectant Cleaner

Steri-Safe™ is the only hospital-grade disinfectant cleaner with broad bactericidal, virucidal, fungicidal and tuberculocidal efficacy that does not require special handling or disposal, is non-flammable and is safe to use (non-staining, non-corrosive) on a wide variety of surfaces.

## EFFICACY

### Bactericidal – *Campylobacter jejuni*,\*\*\*

*Escherichia coli* OH157,\*\* *Legionella pneumophila*  
*Listeria monocytogenes*,\*\* Methicillin resistant  
*Staphylococcus aureus* (MRSA),\*\*\*  
*Pseudomonas aeruginosa*,\* *Salmonella choleraesuis*  
*Salmonella typhimurium*,\*\* *Staphylococcus aureus*  
*Streptococcus pyogenes*,\*\* Vancomycin resistant  
*Enterococcus faecium* (VRE)\*\*\*

### Virucidal – Hepatitis B,\*\* Hepatitis C,\*

Herpes simplex Type I,\*\* Herpes simplex Type II,\*  
HIV-1,\*\* Influenza A2,\*\*\* Rhinovirus 39\*\*\*

### Fungicidal – *Candida albicans*,\*\*

*Trichophyton mentagrophytes*\*\*

### Tuberculocidal – *Mycobacterium bovis* (TB)

\* 2 minutes contact time. In California,

*Staphylococcus aureus* contact time is 10 minutes

\*\* 5 minutes contact time

\*\*\* 10 minutes contact time

**Kills TB, HIV and HBV in five minutes\*\***



## SAFETY

- No eye & lung irritation
- No odor or dermal toxicity
- No use around children or asthmatics
- Non-flammable
- No personal protective equipment required
- Non-corrosive and non-staining on any surface
- Registered by EPA for use on food contact surfaces

Steri-Safe™ is the only formula on the market today that meets the CDC Guidelines of an ideal disinfectant.\*

See properties on back. \*Reference – CDC Guideline for Disinfection and Sterilization in Healthcare Facilities, 2008, June 2003.

## BENEFITS



- One product for a broad range of disinfectant uses
- Value for money – lasts longer due to material safety
- Employee safety and satisfaction – hypo-allergenic, no contact dermatitis or skin irritation
- Environmental safety – no waste treatment or special disposal required

**Powerful, Non-Corrosive  
and Ready To Use**

For use in:  
Hospitals (Surgical & Non-Surgical)  
Rehab • Mental Health • Long Term Care  
Health Care Corporations • State Health Services

Available in:  
8 oz., 22 oz., 1 gal., 5 gal., 55 gal.  
See back for ordering information.



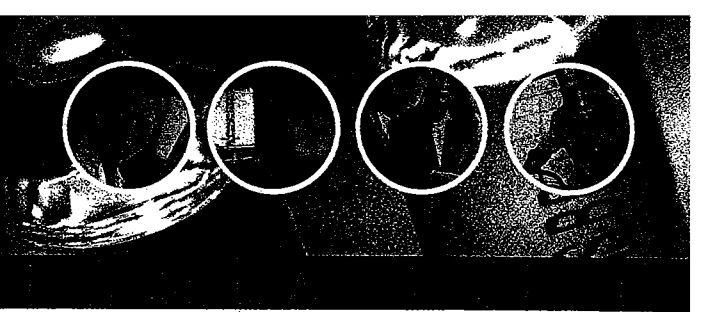

## **W A S T E   A C C E P T A N C E   P R O T O C O L**

Stericycle policy requires compliance with all applicable regulations regarding the collection, transportation and treatment of regulated medical waste. Federal Department of Transportation (DOT) Regulations require the generator of regulated medical waste to certify that the packaging and documentation of transported regulated medical waste complies with DOT regulations regarding waste classification, packaging, labeling and shipping documentation. To ensure that neither Stericycle nor the generator of regulated medical waste violates applicable regulations, it is imperative that all parties understand the rules regarding proper identification, classification, segregation and packaging of regulated medical waste. The purpose of this policy is to summarize the minimum requirements for preparing your medical waste for collection, transportation and treatment. Additional facility or state-specific waste acceptance policies may apply based on permit specifications. Please contact your local representative.



### **REGULATED MEDICAL WASTE**

Stericycle accepts medical waste generated in a broad range of medical diagnostic, therapeutic and research activities. The term "medical waste" includes biohazardous, biomedical, infectious or regulated medical waste as defined under federal, state or local laws, rules, regulations and guidelines. Except as defined by specific state regulations, this excludes pharmaceuticals, waste containing mercury or other heavy metals, chemicals such as solvents, reagents, corrosives or ignitable materials classified as hazardous waste under Federal EPA Regulations. Stericycle cannot accept these excluded materials. In addition, Stericycle cannot accept bulk liquids or chemotherapy waste, radioactive materials, fetal remains or human torsos. Separate protocol and packaging requirements apply for the disposal of non-hazardous pharmaceuticals.

Please contact your local representative for details and packaging specifications. Before accepting pharmaceutical waste from your facility, we must have on file a signed Pharmaceutical Waste Acceptance Protocol. This protocol outlines the bags and labeling that are required. It also gives some guidelines as to what can be considered a hazardous pharmaceutical. If you would like us to pick up your expired pharmaceuticals, please contact our customer service department.

### **WASTE SEGREGATION AND PACKAGING**

The generator is solely responsible for properly segregating, packaging and labeling of regulated medical waste. Proper segregation and packaging reduces the potential for accidental release of the contents and exposure to employees and the general public. All Stericycle customers are provided with packaging instructions which describe the packaging, maximum weights, proper sealing/closure of inner bags and outer containers and proper packaging of sharps. These instructions are designed to comply with the packaging requirements of 49 CFR 173.197, which require that waste be packaged in a container that is 1) rigid; 2) leak resistant; 3) impervious to moisture; 4) of sufficient strength to prevent tearing or bursting under normal conditions.

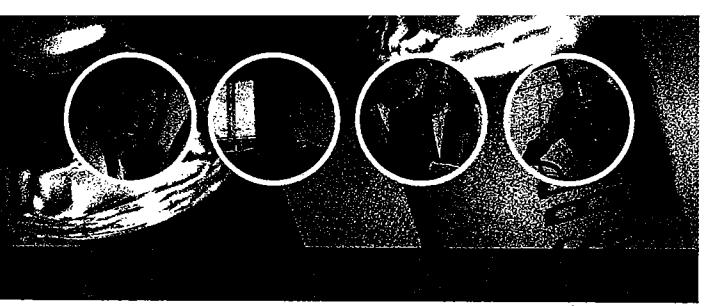

## P A C K A G I N G   G U I D E L I N E S

All medical waste collected for disposal, must be placed in a corrugated box or reusable container which is lined. (Massachusetts requires two liners per box.) The bag used for this purpose must be of sufficient strength to prevent ripping or tearing per applicable standards. In addition, the bag must be marked according to federal, state and local regulations (i.e., red in color and/or biohazard symbol).

Place all "red bags" into the reusable shipping containers or corrugated boxes.

Sharp materials ("sharps") must be placed in special puncture-resistant containers. Sharps include needles and syringes, scalpel blades, broken glass, culture slides, culture dishes, broken capillary tubes, broken rigid plastic and exposed ends of dental wire. As with other medical waste, sealed containers filled with sharps may be placed in the shipping container. No loose sharps permitted in corrugated boxes or non-approved reusable containers.

Each bag must be sealed/tied. The reusable containers/corrugated boxes must be securely closed.

The outside of each container must bear a label showing your facility's name and address or a specially provided bar code label.

*Medical waste **does not** include chemicals, mercury, solvents, pharmaceuticals (see Waste Acceptance Protocol) or other hazardous wastes. For pathological waste, the preservative agent must be decanted prior to placement in the container.*

### WHAT STERICYCLE CAN PROVIDE TO YOU:

- Plastic bags which meet the requirements of federal, state and local regulations
- Reusable containers with lids or corrugated boxes which are marked to meet state standards
- Tape
- Special containers for sharps
- Bar code labels (not available in all areas)
- Expertise on Medical Waste Regulations and Management

*The above items may be subject to additional charges.*

### PLEASE FOLLOW THESE ADDITIONAL REGULATIONS AND PROCEDURES:

- **Generators are responsible for packaging their wastes. Only properly packaged containers will be accepted.**
- Each container will be tested for radiation. Materials with unacceptable radioactive readings will be rejected and should be disposed of at a properly licensed facility.

This information is based on laws and regulations as of August 2002. However, laws and regulations change. We advise you to stay abreast of all laws and regulations pertaining to the handling and disposal of medical waste. For more complete information, write to the U.S. Department of Transportation (DOT) Research and Special Program Administration Department (see address below) or the appropriate agency in your state.

U.S. Department of Transportation (DOT)  
Research and Special Program  
Administration Department  
400 7th Street Southwest  
Washington DC 20590

or call: (800) 467-4922

[www.DOT.gov](http://www.DOT.gov)

# 5

## Five Questions To Ask Yourself Before OSHA Does !

1. Does our facility have an up-to-date written safety plan?
2. Have our employees received their annual bloodborne pathogens training?
3. Are we conducting and documenting safety meetings?
4. How would my staff react to an OSHA inspection?
5. Does our facility have site-specific material safety data sheets for all of our chemicals?

If you answered "No" to any of these questions, the Steri-Safe<sup>SM</sup> Compliance Program can help you achieve total compliance with current OSHA regulations. If you answered "Yes" to any of these questions, the Steri-Safe<sup>SM</sup> Compliance Program will complement or help you maintain your current OSHA program, plus provide computer-based training tools and regular updates to keep your facility in compliance long-term. **Guaranteed.**

M O R E   T H A N   J U S T   S A F E . . . B E   S T E R I - S A F E <sup>SM</sup>

How  
Little  
Can Staying  
in  
Compliance  
Really Cost?

*You'll be Amazed!*

Selecting The Perfect Steri-Safe<sup>SM</sup> Level For You  
There's no easier way to handle your essential OSHA Compliance and Medical Waste Management needs than Steri-Safe<sup>SM</sup>. When choosing the level that's ideal for your facility, remember that the Preferred level gives you the best value. Start benefiting from the most comprehensive solution on the market, Steri-Safe<sup>SM</sup>, by calling Stericycle<sup>®</sup> Customer Service today.

**Steri-Safe<sup>SM</sup> OSHA COMPLIANCE PROGRAM**

S T E R I - S A F E <sup>SM</sup> • P R O G R A M   L E V E L S

**Preferred**  
ANNUAL ON-SITE OSHA TRAINING FOR ALL EMPLOYEES  
PRODUCT DISCOUNTS  
Savings on OSHA Compliance, Safety Products, etc.

**Select**  
MSDS SYSTEM CDS  
Over 260,000 Materials Updated Annually

**Standard**  
OSHA COMPLIANCE MANUAL  
Including Updated Federal Regulations, Forms, Posters, and Labels


**GUARANTEE**  
If, by following our program, you are found to be in non-compliance with OSHA regulations, Stericycle will pay your fine.



www.stericycle.com



For further information on how you can obtain One-Stop-OSHA-Compliance and Medical Waste Management for One Low Monthly Fee, contact one of our Compliance Professionals at **(866) STERI-CALL or (866) 783-7422**



Stericycle®



SAMPLE TRANSACTION INVOICE

\* REPRINT \*

ABC Dental Group  
Dr. A. Anybody  
1234 Any Street  
Anytown, AZ 12345-1234

Page: 1 of 1

FOR CUSTOMER SERVICE CALL 800-953-9324	FOR PICK-UP INFORMATION CALL 800-953-9324	INVOICE DATE 04/30/2002	INVOICE NUMBER 0123456789
		CUSTOMER NUMBER 0123456	TERMS Net 30 Days

DATE	QUANTITY	DESCRIPTION	UNIT	PRICE PER UNIT	TOTAL
<p>Site: 001 ABC Dental Group 1234 Any Street, Anytown, AZ 12345</p> <p><small>WARRANTY CERTIFICATE: This is to certify that the following described commodity was weighed, measured or counted by a weighmaster, whose signature is on this certificate, who is a recognized authority of accuracy, as prescribed by Chapter 7 (commencing with Section 17700) of Division 6 of the California Business and Professions Code, administered by the Director of Consumer Standards of the California Department of Food and Agriculture.</small></p> <p><small>Community Medical Waste Weighted at: Stericycle, Inc. 2715 G. 28th St., Venice, CA 90291    <b>100% Sharp, Empty Weighted at:</b></small></p>					
04/02/2002	1.00	Monthly Fee		9.88	9.88
04/02/2002	1.00	20 Gal Tub(Bio), CT 5.7 LB		38.47	38.47
04/02/2002	1.00	Environmental Processing Fee		5.36	5.36
04/02/2002	1.00	Milium Pick-up Fee		29.43	29.43
				SITE-SUBTOTAL-AMT:	\$83.34
				SITE-TOTAL-DISC:	\$0.00
				SITE-TOTAL-AMT:	\$83.34

Client	1-30 Days	31-60 Days	61-90 Days
\$3.34	0.00	0.00	0.00

**INVOICE TOTAL: \$83.34**

**NOTE**

If your account is invoiced per pickup or by weight, and you would prefer to be billed a flat monthly fee, your account may be eligible for the Steri-Safe<sup>SM</sup> OSHA Compliance Program. Simply choose desired service frequency and program level. See Steri-Safe<sup>SM</sup> Program details in your welcome packet. Please contact Stericycle's Customer Service Department at (866) STERI•CALL [(866) 783-7422] for further information or to enroll.

**CERTIFICATION:** THE MATERIAL LISTED ON THE MANIFEST # IS BEING TREATED IN ACCORDANCE WITH THE REQUIREMENTS OF FEDERAL, STATE, AND LOCAL REGULATIONS, APPLICABLE MANIFESTS, AND THE APPROPRIATE LOGS.

**DIRECTIONS:** MEDICAL WASTE HAS BEEN TREATED IN ACCORDANCE WITH THE REQUIREMENTS OF FEDERAL, STATE, AND LOCAL REGULATIONS GOVERNING THE TREATMENT OF SUCH WASTE. A COPY OF THIS CERTIFICATE, APPLICABLE MANIFESTS, AND THE APPROPRIATE LOGS WILL BE FURNISHED TO YOU WITH YOUR PAYMENT.

DETACH AT PERFORMANCE AND RETURN TO STERICYCLE WITH YOUR PAYMENT

<input type="checkbox"/> Check Enclosed	<input type="checkbox"/> VISA	<input type="checkbox"/> MasterCard	<input type="checkbox"/> Discover
Credit Card Account Number		Expiration Date	
Signature			


0006003690 0001609151 0000008334 3.030008

**REMITTANCE**      Please write Amount Paid below


<p>ABC Dental Group Dr. A. Anybody 1234 Any Street Anytown, AZ 12345-1234</p>	<p>STERICYCLE INC PO BOX 79145 PHOENIX AZ 85062-9145</p>
-------------------------------------------------------------------------------------------	------------------------------------------------------------------

Invoice Number: 0123456789	Customer Number: 0123456	Date: 04/30/2002	Invoice Amount: \$83.34
		Amount Paid: \$	

1	5
Toll free (866) STERI•CALL [(866) 783-7422]	This is the current period charges.
2	6
Your account number. Please have this available when calling customer service.	Payable aging status of invoice.
3	7
Please include this number on your payment.	This area is reserved for messages or special offers.
4	8
Date of service, manifest number, quantity, description of what was picked up, weight — if applicable, unit price and total.	You can select check or credit card payment. If you choose to pay via credit card, your account number, expiration date and signature are required.



**Stericycle®**

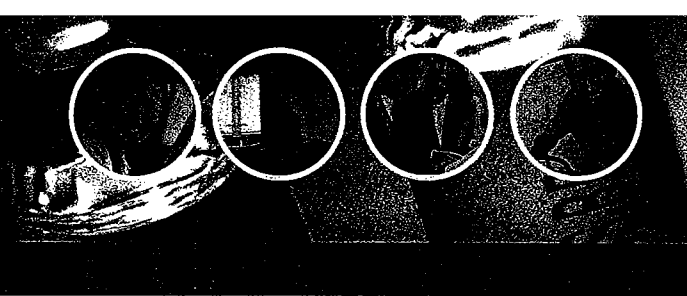


## F A C I L I T Y   I N F O R M A T I O N

	Mission	To be the leading company dedicated to the environmentally responsible management of infection control and compliance services for the healthcare community.
	Technology	Electro-Thermal Deactivation
	Capacity	Maximum: 6,000 lbs/hour Average: 3,400 lbs/hr
	Facility Contact	830 Westlake Boulevard PO Box 1229 Morton, Washington 98356
	Operating Hours	Two 10-hour shifts, Monday through Friday.

Stericycle is the nation's number one provider of Medical Waste collection and disposal services, with a network of over 30 processing facilities and 100 collection operations in the United States and Canada. Stericycle's Morton Medical Waste Facility is located south of Seattle metropolitan area. It services the Washington and Oregon geographic area. The facility was established in 1992 and is one of the most technologically advanced medical waste

treatment facilities in the United States. The 15,000 sq. ft. ETD facility is capable of treating and disposing of medical wastes, safely and effectively, both now and far into the future. Currently, the Morton facility processes approximately 18 million pounds of medical waste per year.

The Morton facility applies a patented Stericycle technology called Electro-Thermal Deactivation (ETD). Waste is first reduced in size and rendered




**Corporate**  
28161 North Keith Drive  
Lake Forest, Illinois 60045

■ **East Region**  
3 Expressway Plaza Suite 114  
Roslyn Heights, New York 11577

■ **Central Region**  
13975 Polo Trail Drive Suite 201  
Lake Forest, Illinois 60045

■ **West Region**  
9188 Glenoaks Boulevard Suite 300  
Sun Valley, California 91352

■ **Canada Region**  
79 Vulcan Street  
Toronto, Ontario M9W1L4



**Stericycle®**

W.U.T.C. NO. 1

SECOND REVISED TITLE PAGE  
CANCELS  
FIRST REVISED TITLE PAGE

TARIFF NO. 1  
OF  
STERICYCLE OF WASHINGTON, INC.  
d/b/a  
STERICYCLE  
CERTIFICATE NO. G-244

(C) Naming Rates for the Collection, Transportation and Disposal of Solid Waste  
Consisting of Biohazardous or Biomedical Wastes in the State of Washington

ISSUED BY:

Michael S. Philpott, District Manager  
STERICYCLE OF WASHINGTON, INC.  
20320 80<sup>th</sup> Avneue S.  
Kent, WA 98032  
Telephone: (425) 291-9322  
Fax: (425) 291-9329

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_ By: \_\_\_\_\_

**CHECK SHEET**

All of the pages contained in this tariff are listed consecutively by number. The pages to the tariff and/or any supplements to the tariff listed on this page have issue dates which are the same as, or are prior to, the issue date of this page. "0" in the revision column indicates an original page.

<u>Page Number</u>	<u>Current Revision</u>	<u>Page Number</u>	<u>Current Revision</u>
Title Page	2		
1	6		
2	3		
3	2		
4	2		
5	2		
5A	1		
5B	1		
5C	0		
6	3		
7	0		
8	1		
9	0		

**SUPPLEMENTS IN EFFECT, including tax supplements:**

- Supplement No. 6
- Supplement No. 7
- Supplement No. 8
- Supplement No. 9
- Supplement No. 10
- Supplement No. 11

Issued By: Michael S. Philpott, District Manager

Issue Date: June 25, 2004

Effective Date: June 29, 2004

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_ By: \_\_\_\_\_



Item 10

Application of rates:

The rates contained in this tariff cover the utilization by a medical waste generator of Stericycle of Washington's transportation service and medical waste management program.

(C)Unless otherwise specified, the rates include the following:

1. Use of Stericycle's unique containers
2. Medical waste tracking and documentation
3. Transportation; and
4. Treatment and disposal

Unless otherwise provided herein, rates contained in this tariff apply to the transportation of biohazardous or biomedical waste, as defined in (C)WAC 480-70-041, in Steritubs or other containers provided by Stericycle of Washington.

Item 14

Customers will be charged for lost containers. The charge per container will be: (C) \*\*\* for a small container; (A)\$30.00 for a small tub; \$5.00 for a small box; \$30.00 for a small/medium container; \$30.00 for a medium tub; (C) \*\*\* for a medium container; \$30.00 for a med/large tub; \$30.00 for a 32 gal. Medium/large container; (C) \*\*\* for a medium/large container; \$5.00 for a med/large box; \$30.00 for a large tub; (C) \*\*\* for a large box; and \$30.00 for a large container. (\*\*\*) indicates container no longer available)

Item 15

Maximum weights:

The maximum weight allowed per container is:

<u>Container Size</u>	<u>Maximum Weight</u>
(C)Small (9 gal.)	***
Small Tub (10 gal.)	(C)35 pounds
(C)Small Box (15 gal.)	40 pounds
Small/Medium (21 gal.)	(C)50 pounds
Medium Tub (20 gal.)	(C)50 pounds
Medium (24 gal.)	***
Medium/Large Tub (28 gal.)	60 pounds
(C)Medium/Large (32 gal.)	60 pounds
(C)Med/Large Box (33 gal.)	40 pounds
Large Tub (40 gal.)	60 pounds
Large (48 gal.)	60 pounds
(C)Large Box (66 gal.)	***

(\*\*\*) indicates container no longer available)

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_

LSN: \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Item 20

Limitations of Service:

1. Stericycle will not (C)knowingly accept shipments including containers which are not properly packaged or identified.
2. (C)Stericycle may refuse to accept shipments not immediately available for pickup at designated pickup areas adjacent to a loading dock or otherwise immediately accessible to Stericycle vehicles.
3. All manifesting paperwork must be properly completed by the generator, verified, appropriately signed and available at the time of pickup.
4. Stericycle may refuse to pick up materials from points where the designated pickup area is obstructed at the time of pickup.
5. Rates include normal wear and tear on reusable containers. Reusable containers provided to the generator for the storage of biomedical waste shall remain the property of Stericycle of Washington. Charges for replacement of reusable containers lost by the generator are shown in Item 14.
6. Stericycle reserves the right to modify its container sizes in the future provided the rate per gallon equivalent remains the same and unless and until rate changes per gallon are approved by the Washington Utilities and Transportation Commission.
7. Stericycle will not (C)knowingly accept containers for shipment unless they have sealed bag liners.
8. The generator shall not tender and Stericycle shall not (C)knowingly accept for transportation any container which:
  - a. is not sealed and properly labeled;
  - b. is punctured or materially damaged;
  - c. is overfilled or overweight;
  - d. contains anything other than biomedical waste; or
  - e. (C)contains radioactive materials as defined by the U.S. Nuclear Regulatory Commission.

(C)In the event Stericycle inadvertently accepts a container described in this paragraph 8, Item 70 shall apply.

9. Stericycle shall not (C)knowingly accept for transportation any shipment which does not meet packing, labeling and handling requirements imposed or required by law.

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_

LSN: \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Tariff No. 1

2<sup>nd</sup> Revised Page No. 4

Company Name: Stericycle of Washington, Inc.

Cancels

1<sup>st</sup> Revised Page No. 4

**(C)Item 30 Rate Schedule (Biomedical Waste except Pathological, Chemotherapy and Pharmaceutical Wastes) – Price per Container**

Container Quantity	Small (9 gallon) Container	Small/Medium (21 gallon) Container	Medium (24 gallon) Container	Medium/Large (32 gallon) Container	Medium/Large (35 gallon) Container	Large (48 gallon) Container
1	(C)***	35.16	(C)***	51.52	(C)***	75.67
2		33.66		47.36		58.32
3		28.94		39.04		48.20
4		26.16		34.24		41.45
5		22.73		30.72		38.08
6		20.80		27.84		35.19
7		19.30		26.56		32.78
8		18.44		25.28		31.33
9		17.37		23.36		29.88
10		16.51		22.72		28.44
11		16.08		21.76		26.99
12		15.44		21.12		25.55
13		15.01		20.48		24.58
14		14.36		19.84		23.14
15		14.15		19.20		22.17
16		13.72		18.88		18.32
17		13.29		17.92		17.83
18		13.08		17.60		17.35
19		12.86		16.96		16.39
20		12.44		16.64		15.91
21		12.01		16.00		15.91
22		11.79		15.68		15.91
23		11.58		15.01		15.91
24		11.36		13.76		15.91
25		10.93		13.28		15.91
26		10.72		13.12		15.91
27		10.51		12.80		15.91
28		10.08		12.32		15.91
29		9.86		12.00		15.91
30		9.86		10.88		15.91

Note 1: Rates to be charged shall be based upon the total number of containers per pickup, (C)including containers rated under Item 90. Rates stated in this Item are in addition to charges specified in Items 60, 70 and 80.

Note 2: A minimum of \$20.00 will be charged per scheduled pickup.

Note 3: (C)Tariff matter previously contained in Note 3 has been deleted.

(A)Note 4: A minimum of \$10.00 per month will be charged for on-call or less-than-monthly service per Item 80.

(A)Note 5: A Reinstatement Charge will be assessed in accordance with Item 85, when applicable.

(C)(\*\*\* indicates container size no longer available)

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_

LSN: \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Tariff No. 1

2<sup>nd</sup> Revised Page No. 5  
Cancels

Company Name: Stericycle of Washington, Inc.

1<sup>st</sup> Revised Page No. 5

(C)Item 30 Rate Schedule (Biomedical Waste except Pathological, Chemotherapy and Pharmaceutical Wastes) -- Price per Container

Container Quantity	Small (9 gallon) Container	Small/Medium (21 gallon) Container	Medium (24 gallon) Container	Medium/Large (32 gallon) Container	Med/Large (35 gallon) Container	Large (48 gallon) Container
31	***	9.86	***	10.56	***	15.91
32		9.86		10.56		13.75
33		9.86		10.56		13.75
34		9.86		10.56		13.75
35		9.86		10.56		13.75
36		9.86		10.56		13.75
37		9.86		10.56		13.75
38		9.86		10.56		13.75
39		9.00		10.56		13.75
40		9.00		10.56		13.75
41		9.00		10.56		13.75
42		9.00		10.56		13.75
43		9.00		10.56		13.75
44		9.00		10.56		13.75
45		9.00		10.56		13.75
46		9.00		10.56		13.75
47		9.00		10.56		13.75
48		9.00		10.56		13.75
49		9.00		10.56		13.75
50		9.00		10.56		13.75
51		9.00		10.56		13.75
52		9.00		9.12		13.75
53		9.00		9.12		13.75
54		9.00		9.12		13.75
55		9.00		9.12		13.75
56		9.00		9.12		13.75
57		9.00		9.12		13.75
58		9.00		9.12		13.75
59		8.58		9.12		13.75
60+		8.58		9.12		13.75

Note 1: Rates to be charged shall be based upon the total number of containers per pickup, (C)including containers rated under Item 90. Rates stated in this Item are in addition to charges specified in Items 60, 70 and 80.

Note 2: A minimum of \$20.00 will be charged per scheduled pickup.

Note 3: (C)Tariff matter previously contained in Note 3 has been deleted.

(A)Note 4: A minimum of \$10.00 per month will be charged for on-call or less-than-monthly service per Item 80.

(A)Note 5: A Reinstatement Charge will be assessed in accordance with Item 85, when applicable.

(C)(\*\*\* indicates container size no longer available)

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_

LSN: \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Tariff No. 1

1<sup>st</sup> Revised Page No. 5A

Company Name: Stericycle of Washington, Inc.

Cancels

Original Page No. 5A

**Item 30 Rate Schedule (C)(Biomedical Waste except Pathological, Chemotherapy and Pharmaceutical Wastes) – Price per Container**

Container Quantity	Small Tub (10 gallon)	Small Box 12"x12"x24" (C)(Approx. 15 gallon)	Medium Tub (20 gallon)	Medium/Large Tub (28 gallon)	Medium/Large Box 18"x18"x24" (C)(Approx. 33 gallon)	Large Tub (40 gallon)
1	22.20	31.20	33.40	45.34	51.52	64.24
2	16.38	23.03	31.98	41.68	47.36	59.05
3	15.88	22.32	27.49	34.36	39.04	48.68
4	15.68	22.04	24.85	30.13	34.24	42.69
5	14.79	20.78	21.59	27.03	30.72	38.30
6	13.49	18.95	19.76	24.50	27.84	34.71
7	12.79	17.97	18.34	23.37	26.56	33.12
8	12.19	17.13	17.52	22.25	25.28	31.52
9	11.19	15.72	16.50	20.56	23.36	29.13
10	10.59	14.88	15.68	19.99	22.72	28.33
11	10.39	14.60	15.28	19.15	21.76	27.13
12	9.69	13.62	14.67	18.59	21.12	26.33
13	9.49	13.34	14.26	18.02	20.48	25.54
14	8.99	12.64	13.64	17.46	19.84	24.74
15	8.79	12.36	13.44	16.90	19.20	23.94
16	8.59	12.07	13.03	16.61	18.88	23.54
17	8.29	11.65	12.63	15.77	17.92	22.34
18	7.99	11.23	12.43	15.49	17.60	21.95
19	7.69	10.81	12.22	14.92	16.96	21.15
20	7.59	10.67	11.82	14.64	16.64	20.75
21	7.49	10.53	11.41	14.08	16.00	19.95
22	7.39	10.39	11.20	13.80	15.68	19.55
23	7.29	10.25	11.00	13.21	15.01	18.72
24	7.19	10.11	10.79	12.11	13.76	17.16
25	7.09	9.97	10.38	11.69	13.28	16.56
26	6.99	9.83	10.18	11.55	13.12	16.36
27	6.89	9.69	9.98	11.26	12.80	15.96
28	6.79	9.55	9.58	10.84	12.32	15.37
29	6.69	9.41	9.37	10.56	12.00	14.97
30	6.59	9.27	9.37	9.57	10.88	13.57

Note 1: Rates to be charged shall be based upon the total number of containers per pickup, (C)including containers rated under Item 90.

Rates stated in this Item are in addition to charges specified in Items 60, 70 and 80.

Note 2: A minimum of \$20.00 will be charged per scheduled pickup.

Note 3: (C)Tariff matter previously contained in Note 3 has been deleted.

(A)Note 4: A minimum of \$10.00 per month will be charged for on-call or less-than-monthly service per Item 80.

(A)Note 5: A Reinstatement Charge will be assessed in accordance with Item 85, when applicable.

(C)(\*\*\* indicates container size no longer available)

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(FOR OFFICIAL USE ONLY)

Effective: \_\_\_\_\_ Docket TG- \_\_\_\_\_ Other \_\_\_\_\_

LSN \_\_\_\_\_ IAA \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Company Name: Stericycle of Washington, Inc.

Cancels  
Original Page No. 5B

(C)Item 30 Rate Schedule (Biomedical Waste except Pathological, Chemotherapy and Pharmaceutical Wastes) – Price per Container

Container Quantity	Small Tub (10 gallon)	Small Box 12"x12"x24" (C)(Approx. 15 gallon)	Medium Tub (20 gallon)	Medium/Large Tub (28 gallon)	Medium/Large Box 18"x18"x24" (C)(Approx. 33 gallon)	Large Tub (40 gallon)
31	6.16	8.66	9.37	9.29	10.56	13.17
32	6.39	8.99	9.37	9.29	10.56	13.17
33	6.29	8.85	9.37	9.29	10.56	13.17
34	6.19	8.70	9.37	9.29	10.56	13.17
35	6.09	8.56	9.37	9.29	10.56	13.17
36	5.99	8.42	9.37	9.29	10.56	13.17
37	5.89	8.28	9.37	9.29	10.56	13.17
38	5.89	8.28	9.37	9.29	10.56	13.17
39	5.87	8.25	8.55	9.29	10.56	13.17
40	5.85	8.22	8.55	9.29	10.56	13.17
41	5.79	8.14	8.55	9.29	10.56	13.17
42	5.69	8.00	8.55	9.29	10.56	13.17
43	5.65	7.94	8.55	9.29	10.56	13.17
44	5.59	7.86	8.55	9.29	10.56	13.17
45	5.49	7.72	8.55	9.29	10.56	13.17
46	5.45	7.66	8.55	9.29	10.56	13.17
47	5.39	7.58	8.55	9.29	10.56	13.17
48	5.35	7.52	8.55	9.29	10.56	13.17
49	5.29	7.44	8.55	9.29	10.56	13.17
50	5.19	7.30	8.55	9.29	10.56	13.17
51	5.09	7.16	8.55	8.03	9.12	11.38
52	5.00	7.02	8.55	8.03	9.12	11.38
53	4.95	6.96	8.55	8.03	9.12	11.38
54	4.90	6.88	8.55	8.03	9.12	11.38
55	4.80	6.74	8.55	8.03	9.12	11.38
56	4.75	6.68	8.55	8.03	9.12	11.38
57	4.70	6.60	8.55	8.03	9.12	11.38
58	4.60	6.46	8.55	8.03	9.12	11.38
59	4.10	5.76	8.15	8.03	9.12	11.38
60	4.10	5.76	8.15	8.03	9.12	11.38

Note 1: Rates to be charged shall be based upon the total number of containers per pickup, (C)including containers rated under Item 90. Rates stated in this Item are in addition to charges specified in Items 60, 70 and 80.

Note 2: A minimum of \$20.00 will be charged per scheduled pickup.

Note 3: (C)Tariff matter previously contained in Note 3 has been deleted.

~~(A)Note 4: A minimum of \$10.00 per month will be charged for on-call or less than monthly service per Item 80.~~

(A)Note 5: A Reinstatement Charge will be assessed in accordance with Item 85, when applicable.

(C)(\*\*\* indicates container size no longer available)

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(FOR OFFICIAL USE ONLY)

Effective: \_\_\_\_\_ Docket TG- \_\_\_\_\_ Other \_\_\_\_\_

LSN \_\_\_\_\_ 1AA \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Company Name: Stericycle of Washington, Inc.

(C)Item 30 Rate Schedule (Biomedical Waste except Pathological, Chemotherapy and Pharmaceutical Wastes)

Container Quantity	Small Tub (10 gallon)	Small Box 15"x15"x14" (C)(Approx. 15 gallon)	Medium Tub (20 gallon)	Medium/Large Tub (28 gallon)	Medium/Large Box 18"x18"x24" (C)(Approx. 33 gallon)	Large Tub (40 gallon)
61	4.10	5.76	8.15	8.03	9.12	11.38
62	4.00	5.62	8.15	8.03	9.12	11.38
63	3.80	5.34	8.15	8.03	9.12	11.38
64	3.80	5.34	8.15	8.03	9.12	11.38
65	3.80	5.34	8.15	8.03	9.12	11.38
66	3.80	5.34	8.15	8.03	9.12	11.38
67	3.70	5.19	8.15	8.03	9.12	11.38
68	3.60	5.05	8.15	8.03	9.12	11.38
69	3.60	5.05	8.15	8.03	9.12	11.38
70	3.60	5.05	8.15	8.03	9.12	11.38
71	3.60	5.05	8.15	8.03	9.12	11.38
72	3.60	5.05	8.15	8.03	9.12	11.38
73	3.50	4.91	8.15	8.03	9.12	11.38
74	3.30	4.63	8.15	8.03	9.12	11.38
75+	2.85	4.01	8.15	8.03	9.12	11.38

[This space intentionally left blank]

Note 1: Rates to be charged shall be based upon the total number of containers per pickup, (C)including containers rated under Item 90. Rates stated in this Item are in addition to charges specified in Items 60, 70 and 80.

Note 2: A minimum of \$20.00 will be charged per scheduled pickup.

Note 3: (C)Tariff matter previously contained in Note 3 has been deleted.

~~(A)Note 4: A minimum of \$10.00 per month will be charged for on-call or less-than-monthly service per Item 80.~~

(A)Note 5: A Reinstatement Charge will be assessed in accordance with Item 85, when applicable.

(C)(\*\* indicates container size no longer available)

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(FOR OFFICIAL USE ONLY)

Effective: \_\_\_\_\_ Docket TG- \_\_\_\_\_ Other \_\_\_\_\_

LSN \_\_\_\_\_ 1AA \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Tariff No. 1

3<sup>rd</sup> Revised Page No. 6

Company Name: Stericycle of Washington, Inc.

Cancels  
2<sup>nd</sup> Revised Page No. 6

Item 40	(C)Tariff matter previously published in this item has been deleted.
Item 50	Tariff matter previously published in this item has been deleted.
Item 60	<u>Delinquent Fees:</u>  In addition to the rates and charges shown herein, a late charge in the amount of one percent (1%) will be added to any account which remains unpaid at the time of the next regular billing.
Item 70	<u>Special Handling or Packaging Charges:</u>  The following charges will be assessed when the carrier is required to provide special handling or packaging because of the improper packaging of the material shipped by the generator, the shipment of improper waste materials, (C)overweight containers or the generator's special loading requirements:  \$2.00 per gallon in addition to all other rates and charges shown herein.
(A)Item 80	<u>On-Call or Less-Than-Monthly Service:</u> Stericycle offers on-call or less-than-monthly service for a minimum charge of \$10.00 per month. This minimum charge applies in any calendar month in which no pickup is scheduled. Stericycle provides a container or containers for the generator's use. Where on-call service is provided, Stericycle will schedule a pickup within a reasonable time after a request for pickup is received from the generator.

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_

LSN: \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_



Company Name: Stericycle of Washington, Inc.

(A)Item  
85

Reinstatement Charge:

In addition to the other rates and charges shown herein, a Reinstatement Charge of \$120.00 will be charged to any generator that has cancelled service within the preceding 12 months and wishes to reinstate service. The Reinstatement Charge includes re-delivery of a container or containers to the generator.

*[The remainder of this page intentionally left blank]*

Issued By: Michael S. Philpott, District Manager

Issue Date: October 8, 2001

Effective Date: December 1, 2001

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_

LSN: \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Company Name: Stericycle of Washington, Inc.

Item 90

Rates for Pathological Waste, Chemotherapy Waste and Pharmaceutical Waste

Medium/Large Tub (28 gal.): \$30  
 Small box (12x12x24 – 15 gallon) \$20/box  
 Medium/large box (18x18x26 – 33 gallon) \$30/box

The rates stated in this Item 90 are flat rates per container and do not vary with the number of containers tendered for pickup. Stericycle will require all Pathological Waste, Chemotherapy Waste and Pharmaceutical Waste to be packaged by the generator in reusable plastic Medium/Large Tubs (28 gal.) provided by Stericycle to the extent available. The other containers indicated may be used only to the extent that Medium/Large Tubs are not available from Stericycle or the alternative containers are required to be used, at Stericycle’s direction. Charges will also be assessed under Items 60, 70, 80 and 85, when applicable.

For purposes of this Item 90:

“Pathological Waste” means “Pathological waste,” as defined in the definition of “Biomedical waste” found at WAC 480-70-041.

“Chemotherapy Waste” means sharps, syringes, IV tubing/bags/bottles, vials, and other discarded contaminated items generated in the preparation and administration of cytotoxic/antineoplastic drugs. Only *empty* containers/bags are acceptable with residue not to exceed 3% of total volume.

“Pharmaceutical Waste” means pharmaceutical waste which has been properly characterized as not hazardous under the Resource Conservation and Recovery Act (RCRA) regulations and criteria (or more stringent state regulations, where applicable) and which has been packaged and labeled by the generator and approved and accepted by Stericycle of Washington in accordance with a Pharmaceutical Waste Acceptance Agreement executed by Stericycle and the generator. Only properly packaged and labeled Pharmaceutical Waste covered by a Pharmaceutical Waste Acceptance Agreement may be tendered to Stericycle by the generator.

(C) Note 1: The April 30, 2003 expiration date previously found in Item 90 has been deleted.

Issued By: Michael S. Philpott, District Manager

Issue Date: March 14, 2003

Effective Date: April 30, 2003

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_

LSN: \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_

Company Name: Stericycle of Washington, Inc. (G-244)

(A) All rates on this page are new rates

(A) Item  
95

Rates for Collection and Transportation of Biomedical Waste in, and Processing of, Re-Usable Sharps Containers – Prices per rack (240 gallon maximum)

<u>Quantity</u>	<u>Collection and Disposal</u>	<u>Container Processing</u>	<u>Total Charge Per Rack</u>
1	\$190.40	\$90.00	\$280.40
2	142.20	90.00	232.20
3	110.85	90.00	200.85
4 or more	79.55	90.00	169.55

*[This space intentionally left blank]*

Note 1: Stericycle will provide wheeled racks, with a maximum capacity of 240 gallons per rack, for the collection, transportation and disposal of sharps waste in Stericycle's standard re-usable sharps containers. The rates specified in this Item 95 apply only to a combined service including the collection, transportation and disposal of sharps waste using Stericycle racks and sharps containers and the processing of such containers for re-use by the customer.

Note 2: Sharps containers are classified by the United States Food and Drug Administration ("FDA") as Class II medical devices. The "container processing" charge specified in this Item 95 includes processing of Stericycle's re-usable sharps containers for re-use in accordance with FDA requirements.

Issued By: Michael S. Philpott, District Manager

Issue Date: June 25, 2004

Effective Date: June 29, 2004

(This box for official use only)

Effective: \_\_\_\_\_ Docket No. \_\_\_\_\_

LSN: \_\_\_\_\_ Hearing \_\_\_\_\_ By \_\_\_\_\_



**Stericycle Medical Waste Systems**  
**Service Schedule for 2004**

---

Customer and Site No: 6060945-001  
Frequency: Every 4 Weeks

To Schedule a Pickup, or for Service Related Questions  
Please Call: 1-800-Med-Waste

For Information on Steri-Safe, or to Order Sharps Containers  
Please Call : 1-800-355-8773

Contact Name: Julie-A/P

For Any Other Questions

Please Call : 800-633-9278

Acme Assisted Living  
2317 W 5th  
Walla Walla, WA, 99362

---

**Pickup Day and Date:**

**July**

1-Thu                      29-Thu

**August**

26-Thu

**September**

23-Thu

**October**

21-Thu

**November**


18-Thu

**December**

16-Thu

---









**Stericycle**®

Introducing

**Steri-Safe**<sup>SM</sup>  
**OSHA**  
COMPLIANCE  
program

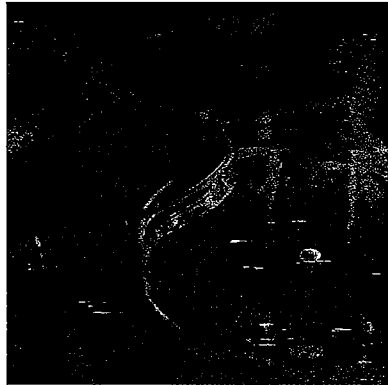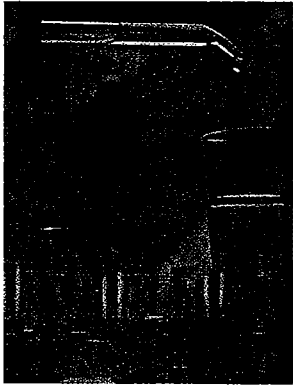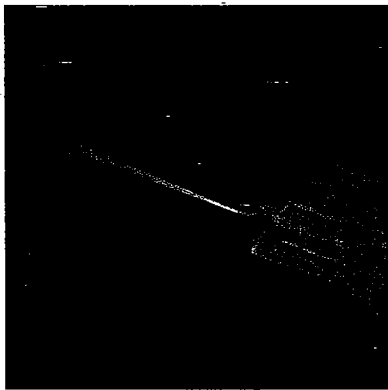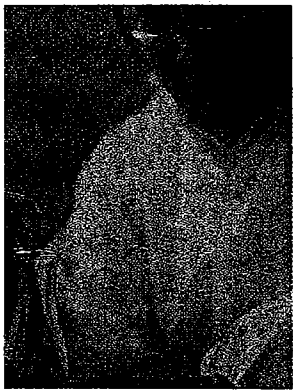

A Simple,  
Comprehensive  
OSHA Compliance  
Program.



# Now You Can Meet OSHA Requirements

## Steri-Safe<sup>SM</sup> OSHA Compliance Program Manual


### IT'S THE LAW

#### **Public Law 91-596, Section 5(A1) General Duty Clause**

Provide employees with a safe work environment based on a **written exposure control plan**.

#### **Title 29, Section 1910.1030 & Applicable State Requirements**

Ensure proper removal of on-site medical waste.

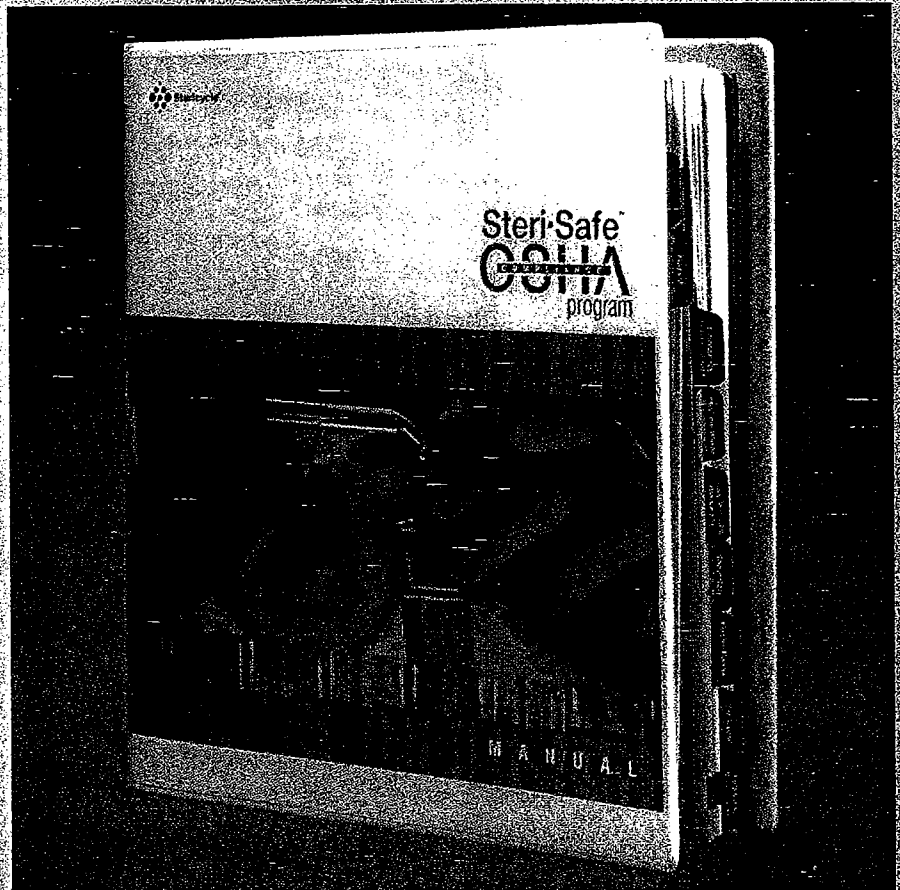


Steri-Safe<sup>SM</sup>  
**OSHA**  
program

MANUAL

OSHA Compliance Program Manual includes:  
• Complete Training Materials  
• Comprehensive Training Lessons  
• OSHA Mandated Plans and Forms

## Employee Safety Meeting CD

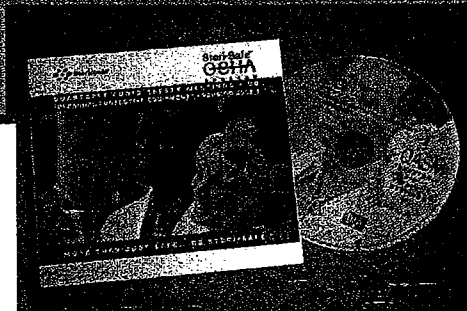


### IT'S THE LAW

#### **Public Law 91-596, Section 5(A1) General Duty Clause**

Conduct regular communications with employees regarding safety issues, including documentation.

## Material Safety Data Sheets CD

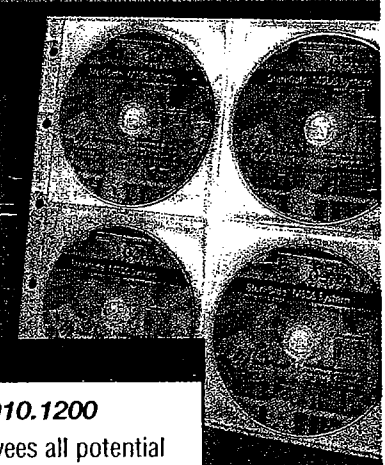

### IT'S THE LAW

#### **Title 29, Section 1910.1200**

Communicate to employees all potential and existing hazards in the workplace. Material Safety Data Sheets (MSDS) and necessary documentation are required.

# MORE THAN JUST SAFE

# s – With One Flat Monthly Fee.




## Bloodborne Pathogens Training CD

The Bloodborne Pathogens interactive training program teaches the BBP standard using an interactive motion video presented by Robert MacMillan, M.D., M.P.H., Chief Medical Officer, Stericycle, Inc.


- Meets OSHA requirements using a quiz at the end of each segment
- Prints a record of training
- In-house training with full motion video

**IT'S THE LAW**  
**Title 29, Section 1910.1030**  
 Provide Bloodborne Pathogens Training for all employees who may be exposed to bloodborne pathogens. Training is required prior to their assignment and at least annually thereafter.

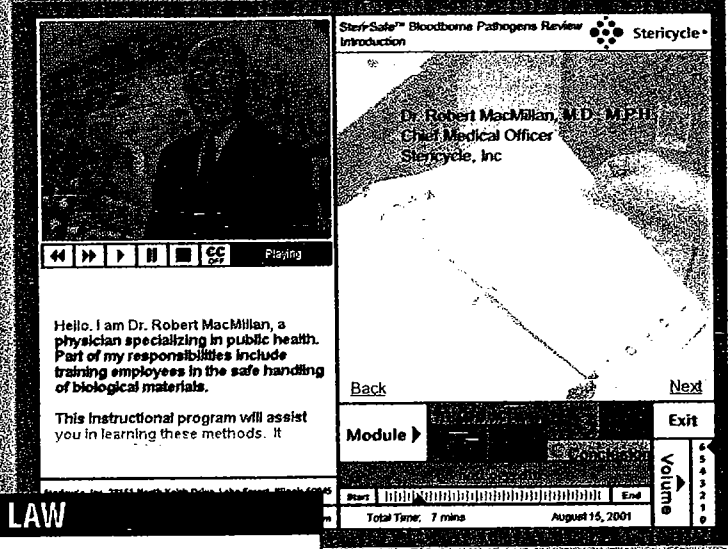

Minimum system requirements for Steri-Safe™ Program Components are as follows:  
 BBP CD-ROM: Windows 9X, ME, 2K, XP, Pentium II 333MHz, 64 MB RAM, 12x CD-ROM, 50 MB hard disk space, sound card/speakers  
 MSDS CD-ROM: Windows 3.1 or higher, X86 or higher, 5 MB hard disk space, 2GB if whole database is copied on hard drive, 16 MB RAM, 1x CD-ROM  
 OASIS CD-ROM: Windows 9X, ME, 2K, XP, Pentium Base 3 processor, 2x CD-ROM, Sound Card/speakers, Acrobat Adobe Reader (included on CD-ROM)

### Hazard/Personal Protective Equipment ID Poster and Labels

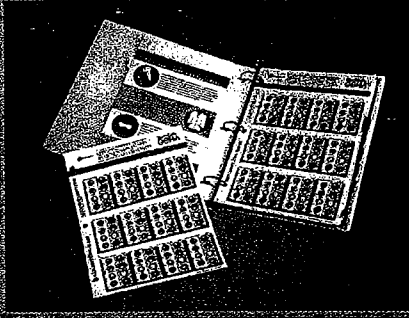

## Steri-Safe<sup>SM</sup> Preferred Level Includes All Program Components plus -

Annual On-Site OSHA Training with a Steri-Safe<sup>SM</sup> Consultant.



On-Site Mock OSHA Inspection with written recommendations

## Risk-Free Guarantee

Guaranteed OSHA Compliance Or We Pay Your Fine

# ... BE STERI-SAFE<sup>SM</sup>



## Selecting The Perfect Steri-Safe<sup>SM</sup> Level For You

There's no easier way to handle your essential OSHA Compliance needs than Steri-Safe<sup>SM</sup>. When choosing the level that's ideal for your facility, remember that the Preferred level gives you the best value. Start benefiting from the most comprehensive solution on the market, Steri-Safe<sup>SM</sup>, by calling Stericycle Customer Service today.

**Steri-Safe<sup>SM</sup>**  
**OSHA**  
COMPLIANCE  
program


### Products and Benefits

Select

Preferred

#### Flat Monthly Fee

Determined by Program Level and Number of Employees.



#### OSHA Compliance Program Manual

Including Updated Federal Regulations, Forms, etc.



#### Bloodborne Pathogens Training CD

Teaches BBP Standard with Interactive, Full-Motion Video



#### Quarterly Audio Safety Meeting (QASM) CD

On Critical and Timely Safety Topics.



#### Material Safety Data Sheets (MSDS) System CD

Over 300,000 Materials Updated Annually.



#### Hazard/Personal Protective Equipment ID Poster

with Hazard/Personal Protective Equipment (PPE) ID Labels.




#### Product Discounts

Savings on Sharps Containers, Safety Products, etc.

#### On-Site Mock OSHA Inspection

Conducted By Your Steri-Safe<sup>SM</sup> Consultant



#### Annual On-Site OSHA Training

with a Steri-Safe<sup>SM</sup> Consultant. May qualify for CE Units.

### GUARANTEE

Guaranteed OSHA Compliance or We Pay You Fine

\*As it pertains to Bloodborne Pathogens and Medical Waste Management practices

**Medical Waste Management Services Available - Sold Separately**  
"Removal, Disposal & Complete Documentation with Flexible Service Frequencies"

### Enroll Today

Call Stericycle Customer Service at:

**800-755-3291**

to initiate your Steri-Safe<sup>SM</sup> OSHA Compliance Program or to upgrade your current service level.

Pacific Northwest District Office

20320 80th Ave S • Kent, WA 98032

Regulated Medical Waste



5028-6060945-001-00A000P

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle  
Regulated Medical Waste



5028-6060945-001-00A000S

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle  
Regulated Medical Waste



5028-6060945-001-00A000V

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle

Regulated Medical Waste



5028-6060945-001-00A000Q

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle  
Regulated Medical Waste



5028-6060945-001-00A000T

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle  
Regulated Medical Waste



5028-6060945-001-00A000W

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle  
Regulated Medical Waste



5028-6060945-001-00A000Z

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle

Regulated Medical Waste



5028-6060945-001-00A000R

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle  
Regulated Medical Waste



5028-6060945-001-00A000U

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle  
Regulated Medical Waste



5028-6060945-001-00A000X

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle  
Regulated Medical Waste



5028-6060945-001-00A0010

Generator  
Acme Assisted Living  
2317 W 5th  
Walla Walla, WA 99362  
Ph: (509)555-1212

Transporter

Stericycle  
20320 80th Ave S  
Kent, WA 98032  
(800) 633-9278

Date

Thank You for Choosing Stericycle